

[54] **ELECTRODE FOR BIOMEDICAL SIGNALS**

[76] Inventors: **Robert D. Stone**, 23641 Cremona St., Laguna Hills, Calif. 92653; **Kenneth L. Dufour**, 440 Desola Ter., Corona Del Mar, Calif. 92625

[\*\*] Term: **14 Years**

[21] Appl. No.: **275,808**

[22] Filed: **Jun. 22, 1981**

[51] Int. Cl. .... **D24—02**

[52] U.S. Cl. .... **D24/29; D24/36**

[58] Field of Search ..... 128/639, 641, 803; **D24/36, 29**

[56] **References Cited**

**U.S. PATENT DOCUMENTS**

D. 231,497	4/1974	Hinnenkamp	.....	D24/29
D. 232,589	8/1974	Hinnenkamp	.....	D24/29
D. 232,590	8/1974	Moore et al.	.....	D24/29
D. 243,476	2/1977	Avery	.....	D24/36
3,961,623	6/1976	Milani et al.	.....	128/639
4,319,579	3/1982	Cartmell	.....	128/803 X

4,354,509	10/1982	Strahwald et al.	.....	128/639 X
4,370,984	2/1983	Cartmell	.....	128/641 X
4,375,219	3/1983	Schmid	.....	128/639



*Primary Examiner*—Bernard Ansher  
*Attorney, Agent, or Firm*—Charles H. Thomas

[57] **CLAIM**


The ornamental design for a electrode for biomedical signals, substantially as shown and described.

**DESCRIPTION**


FIG. 1 is a perspective view from above of an electrode for biomedical signals showing our new design; FIG. 2 is a perspective view of our biomedical electrode from beneath showing our new design; FIG. 3 is an end elevational view of the biomedical electrode of FIGS. 1 and 2; FIG. 4 is a top plan view of the biomedical electrode of FIGS. 1 and 2; FIG. 5 is a bottom plan view of the biomedical electrode of FIGS. 1 and 2; FIG. 6 is a left side elevational view of the biomedical electrode of FIGS. 1 and 2; and FIG. 7 is a right side elevational view of the biomedical electrode of FIGS. 1 and 2.

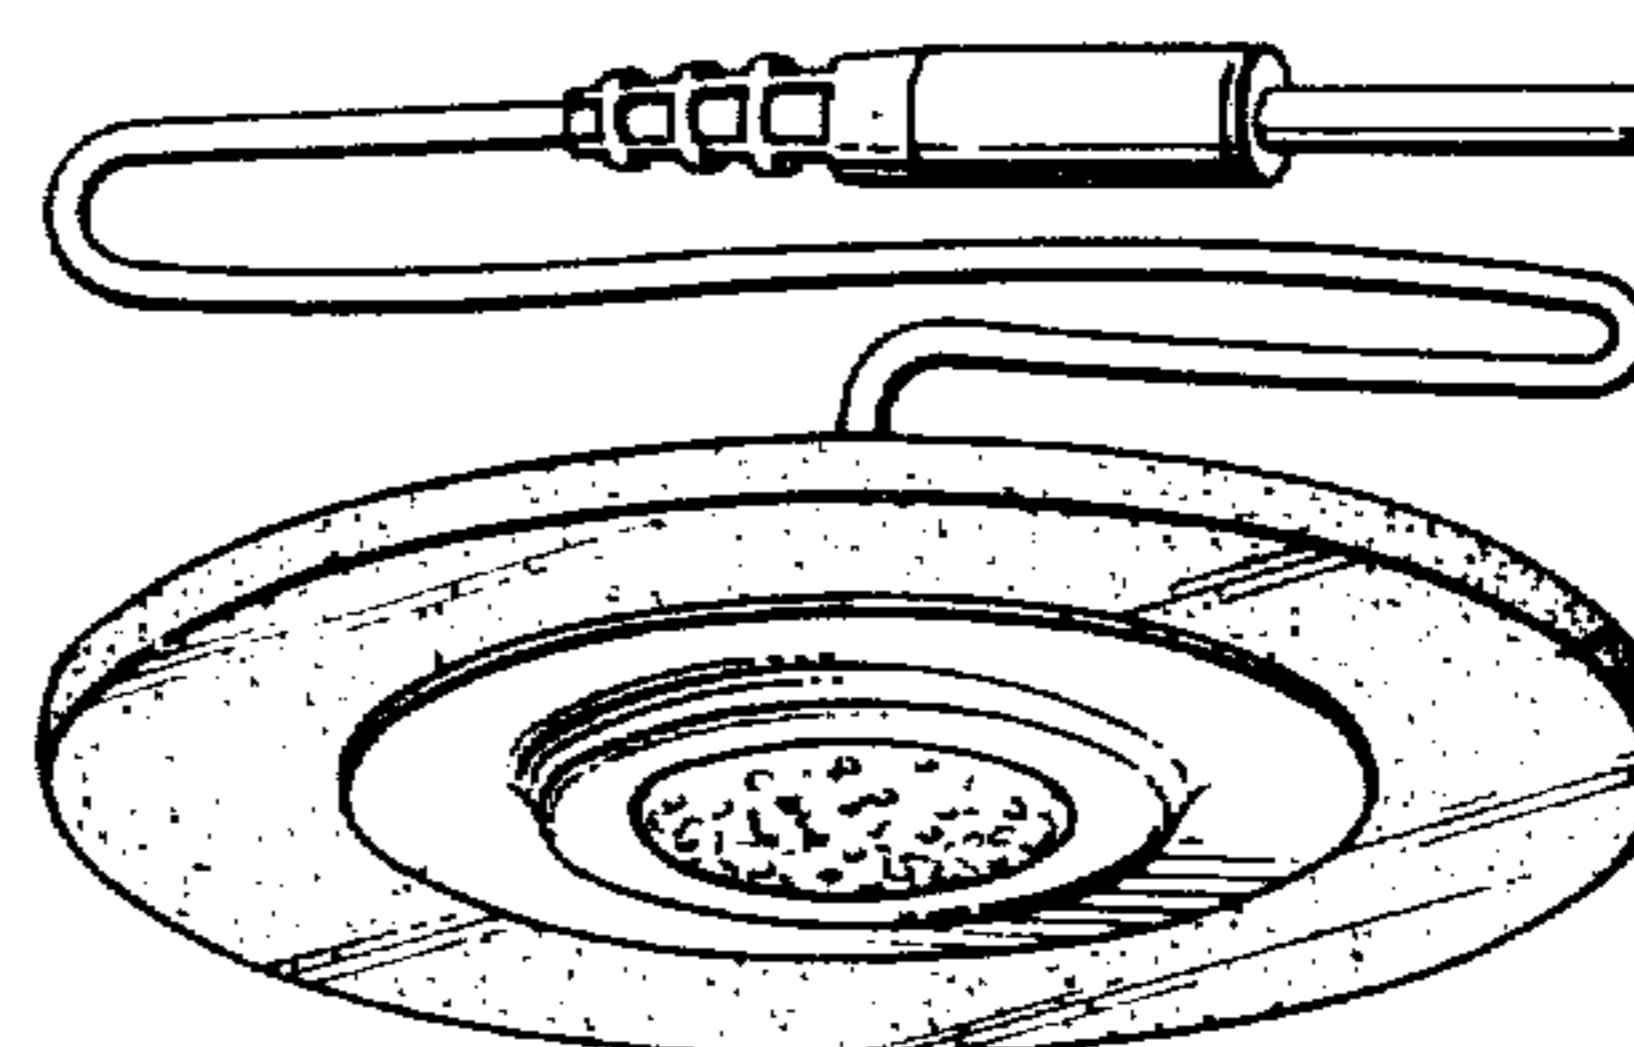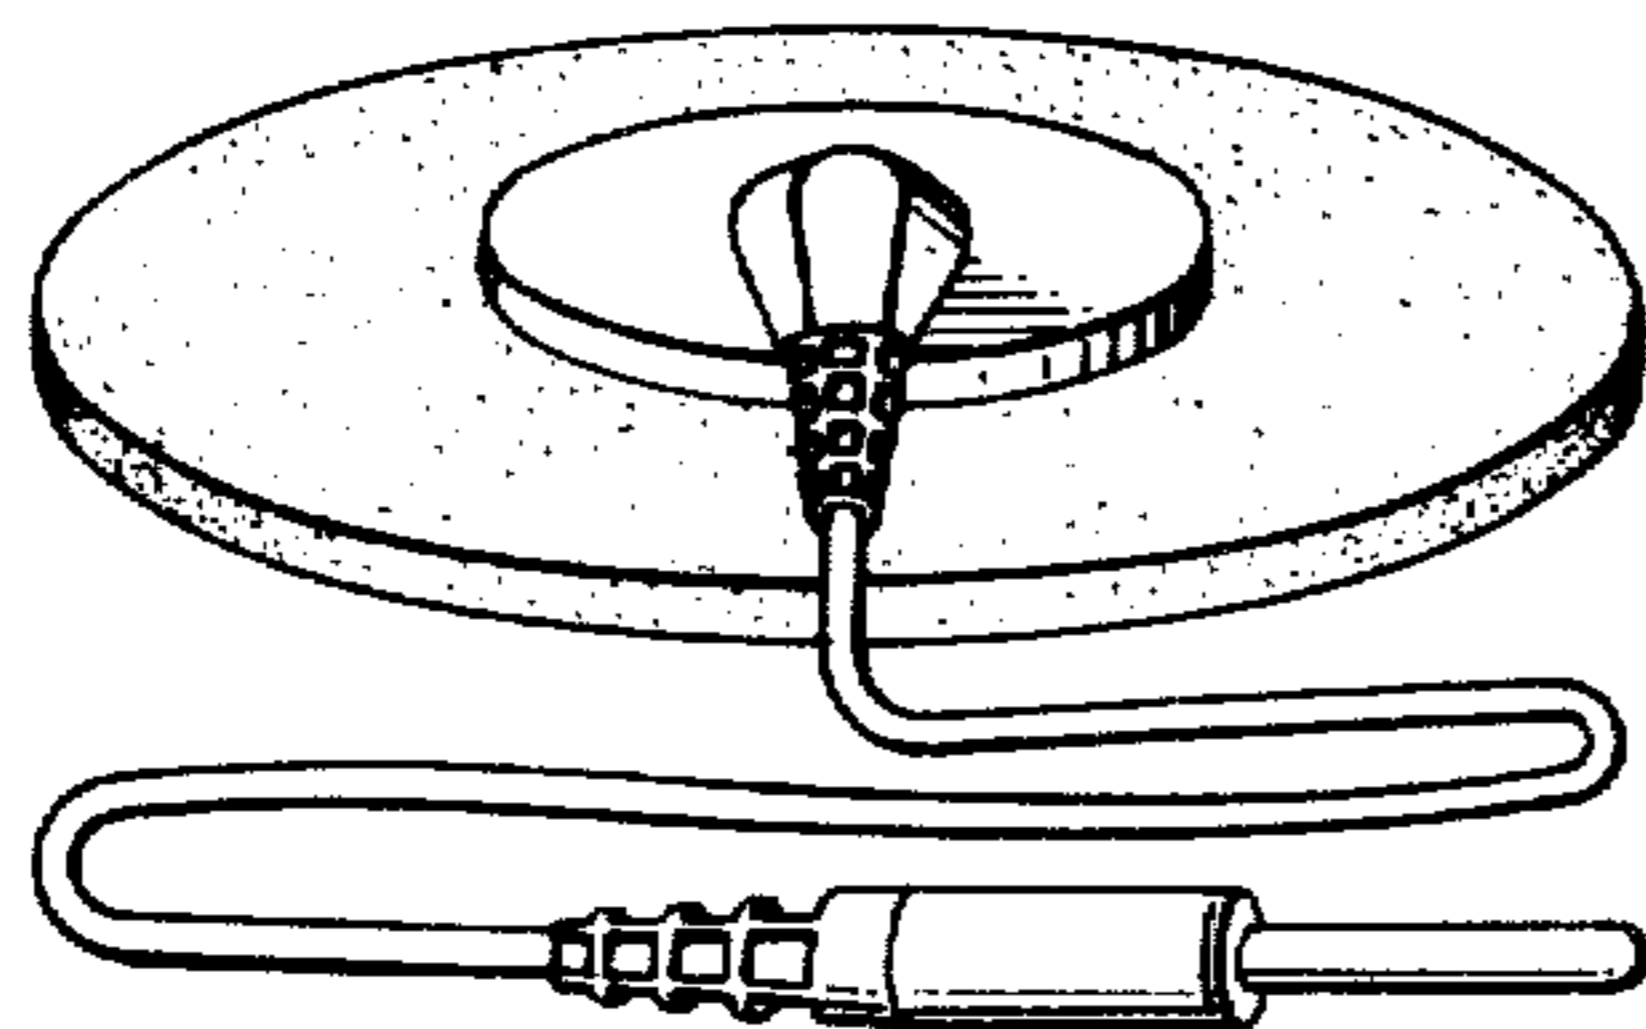


*Fig. 1.*

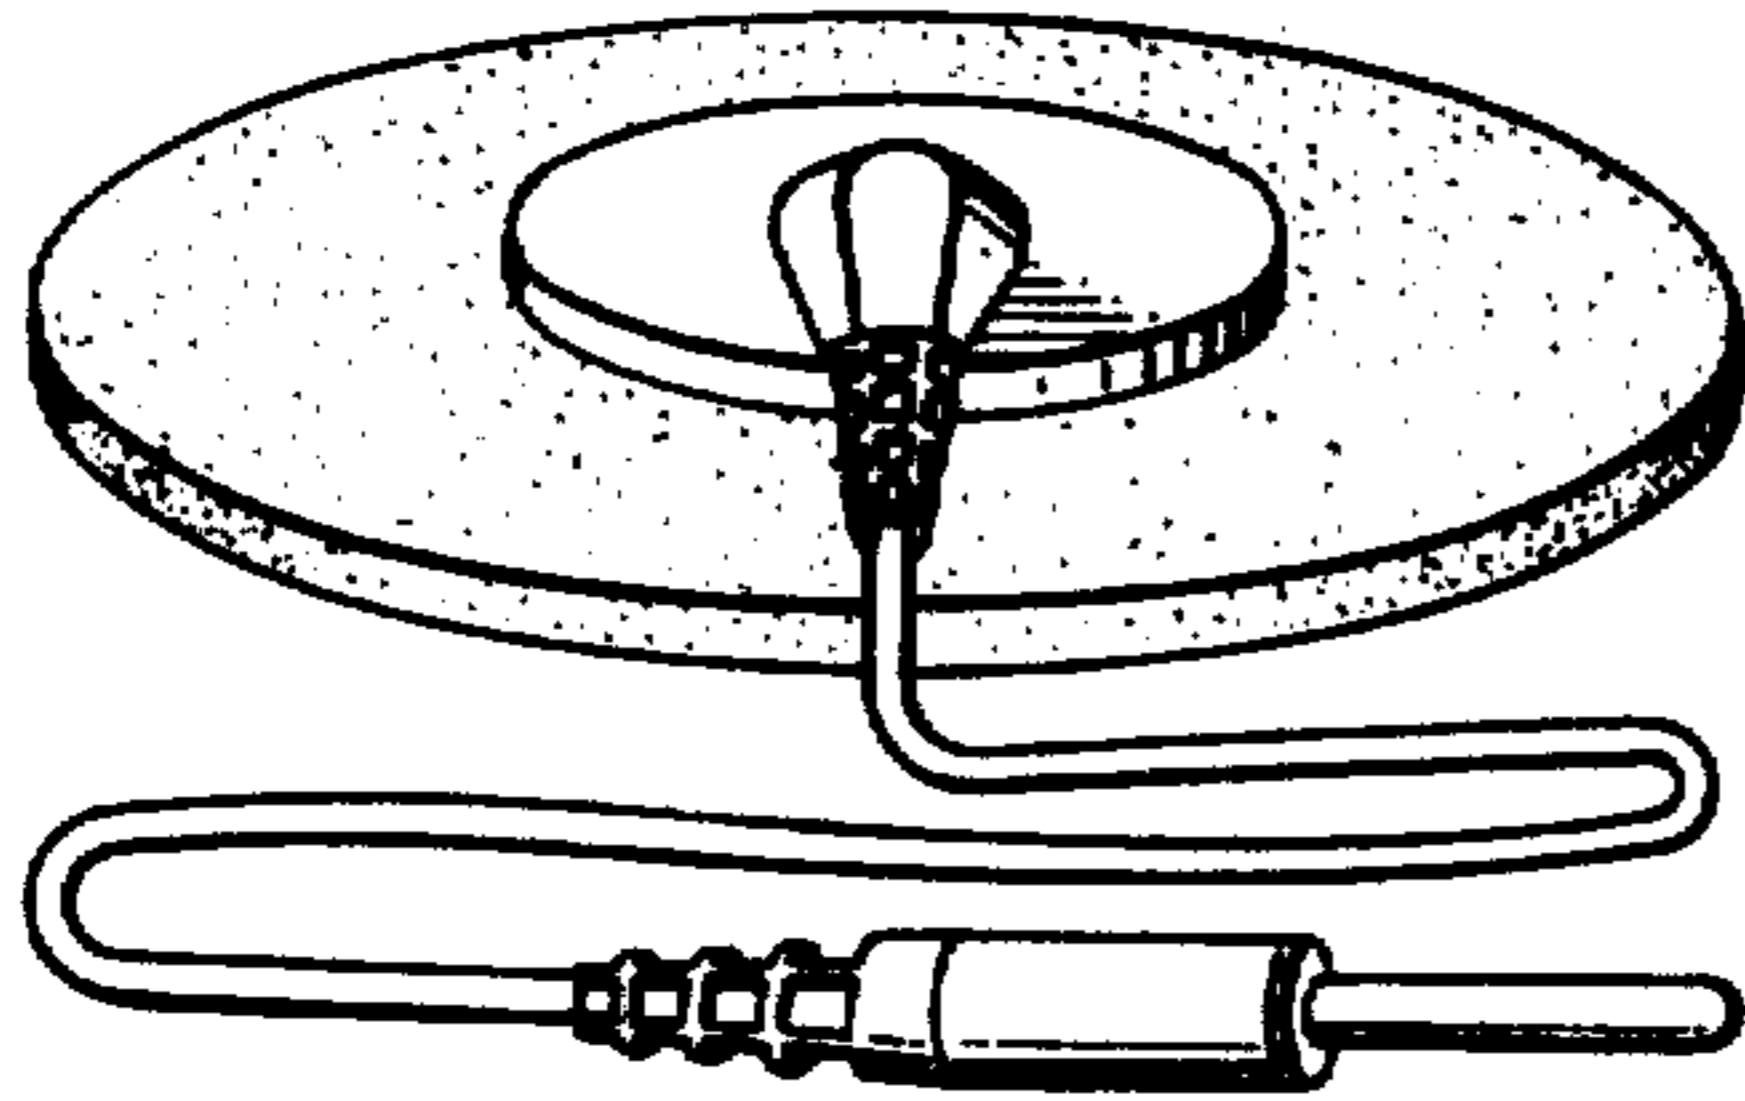


*Fig. 2.*

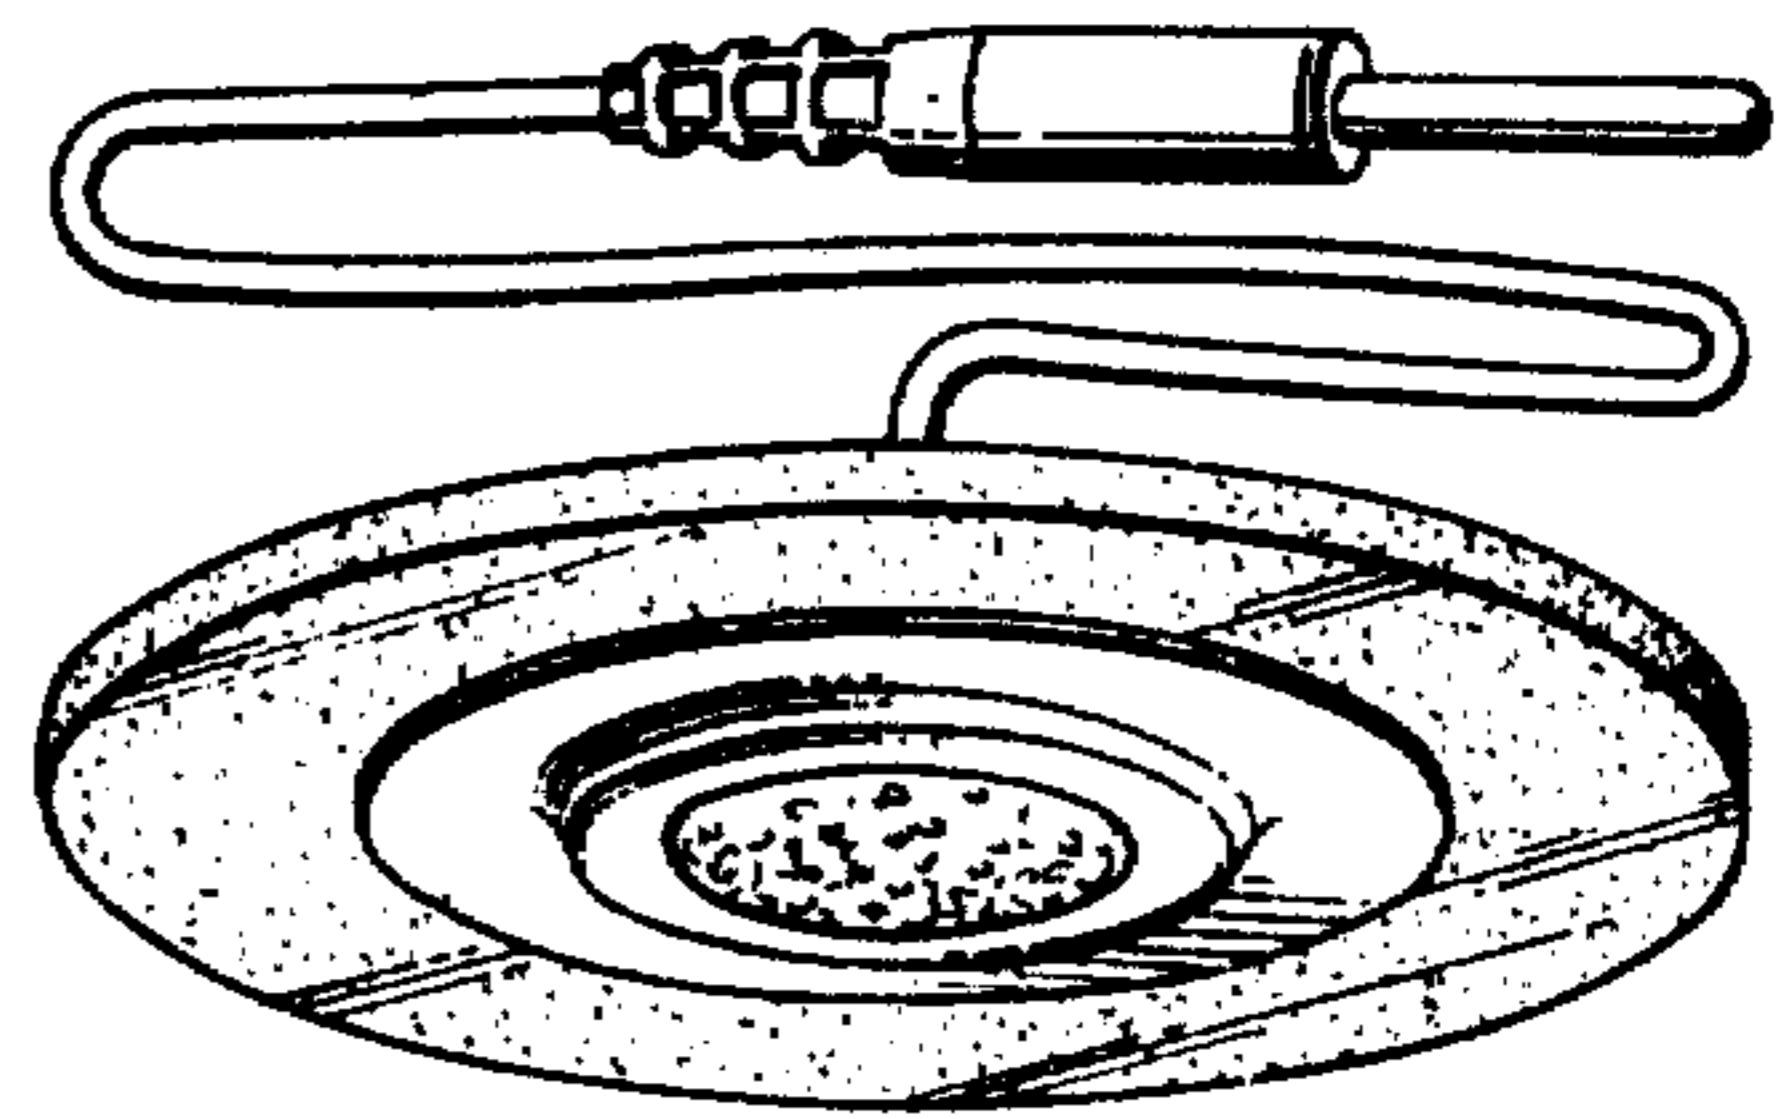


*Fig. 3.*

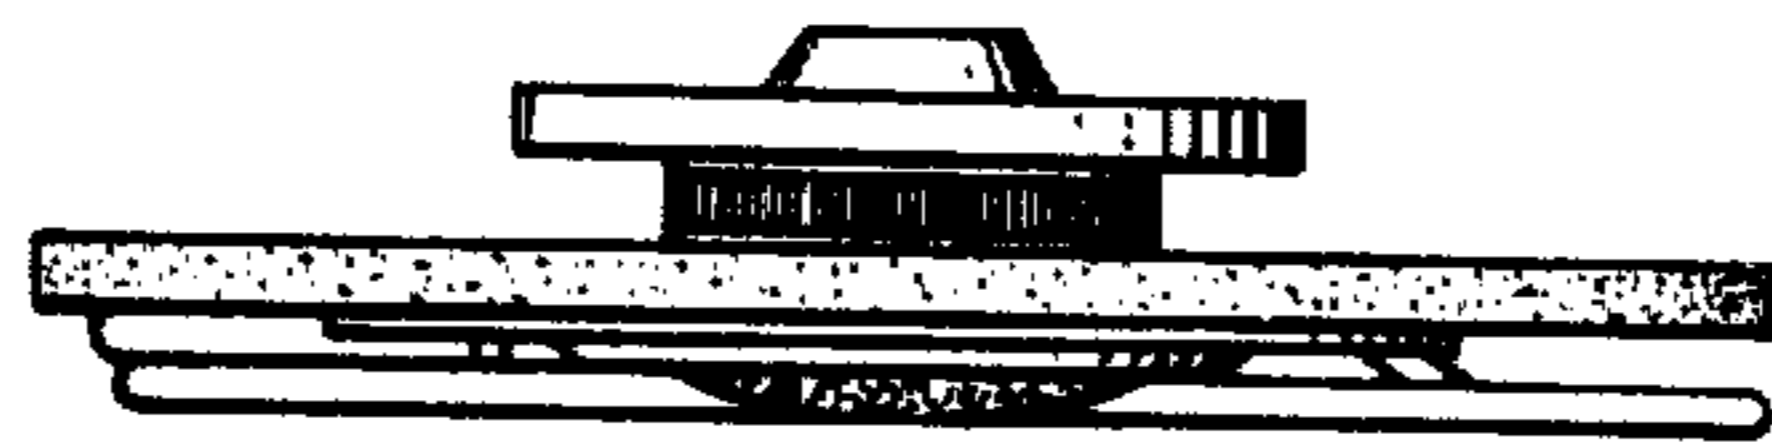


*Fig. 4.*

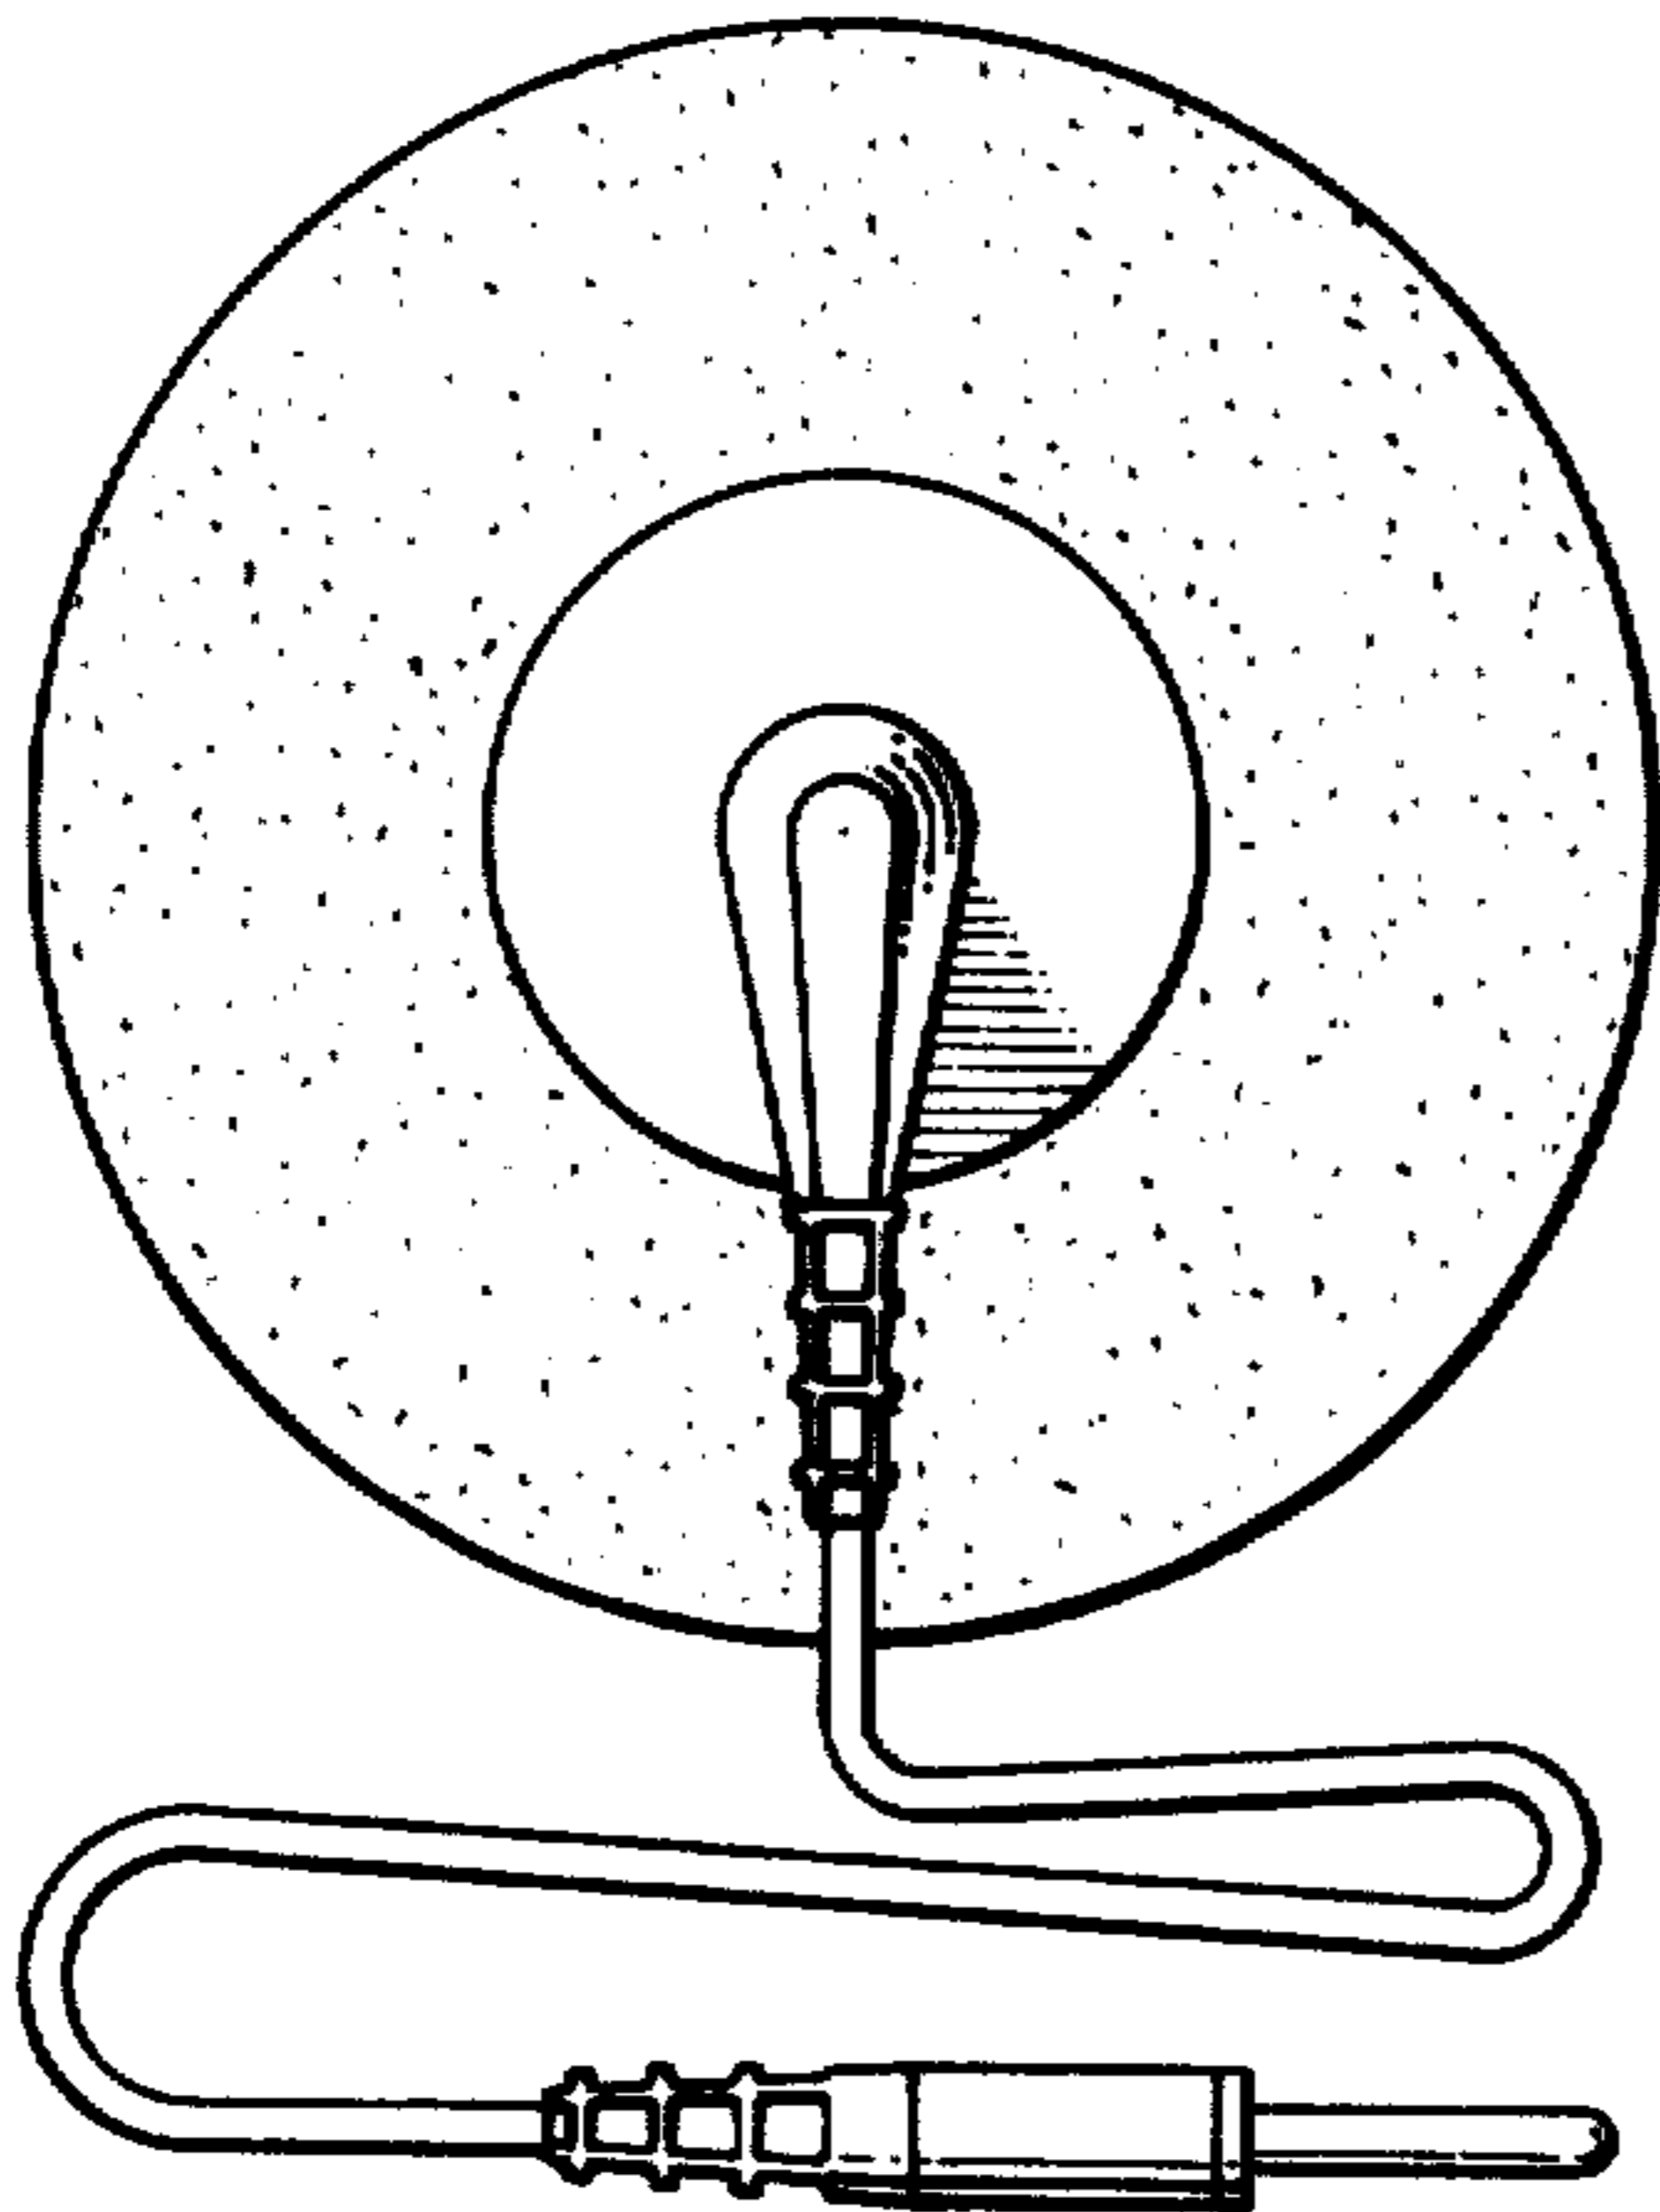

*Fig. 5.*

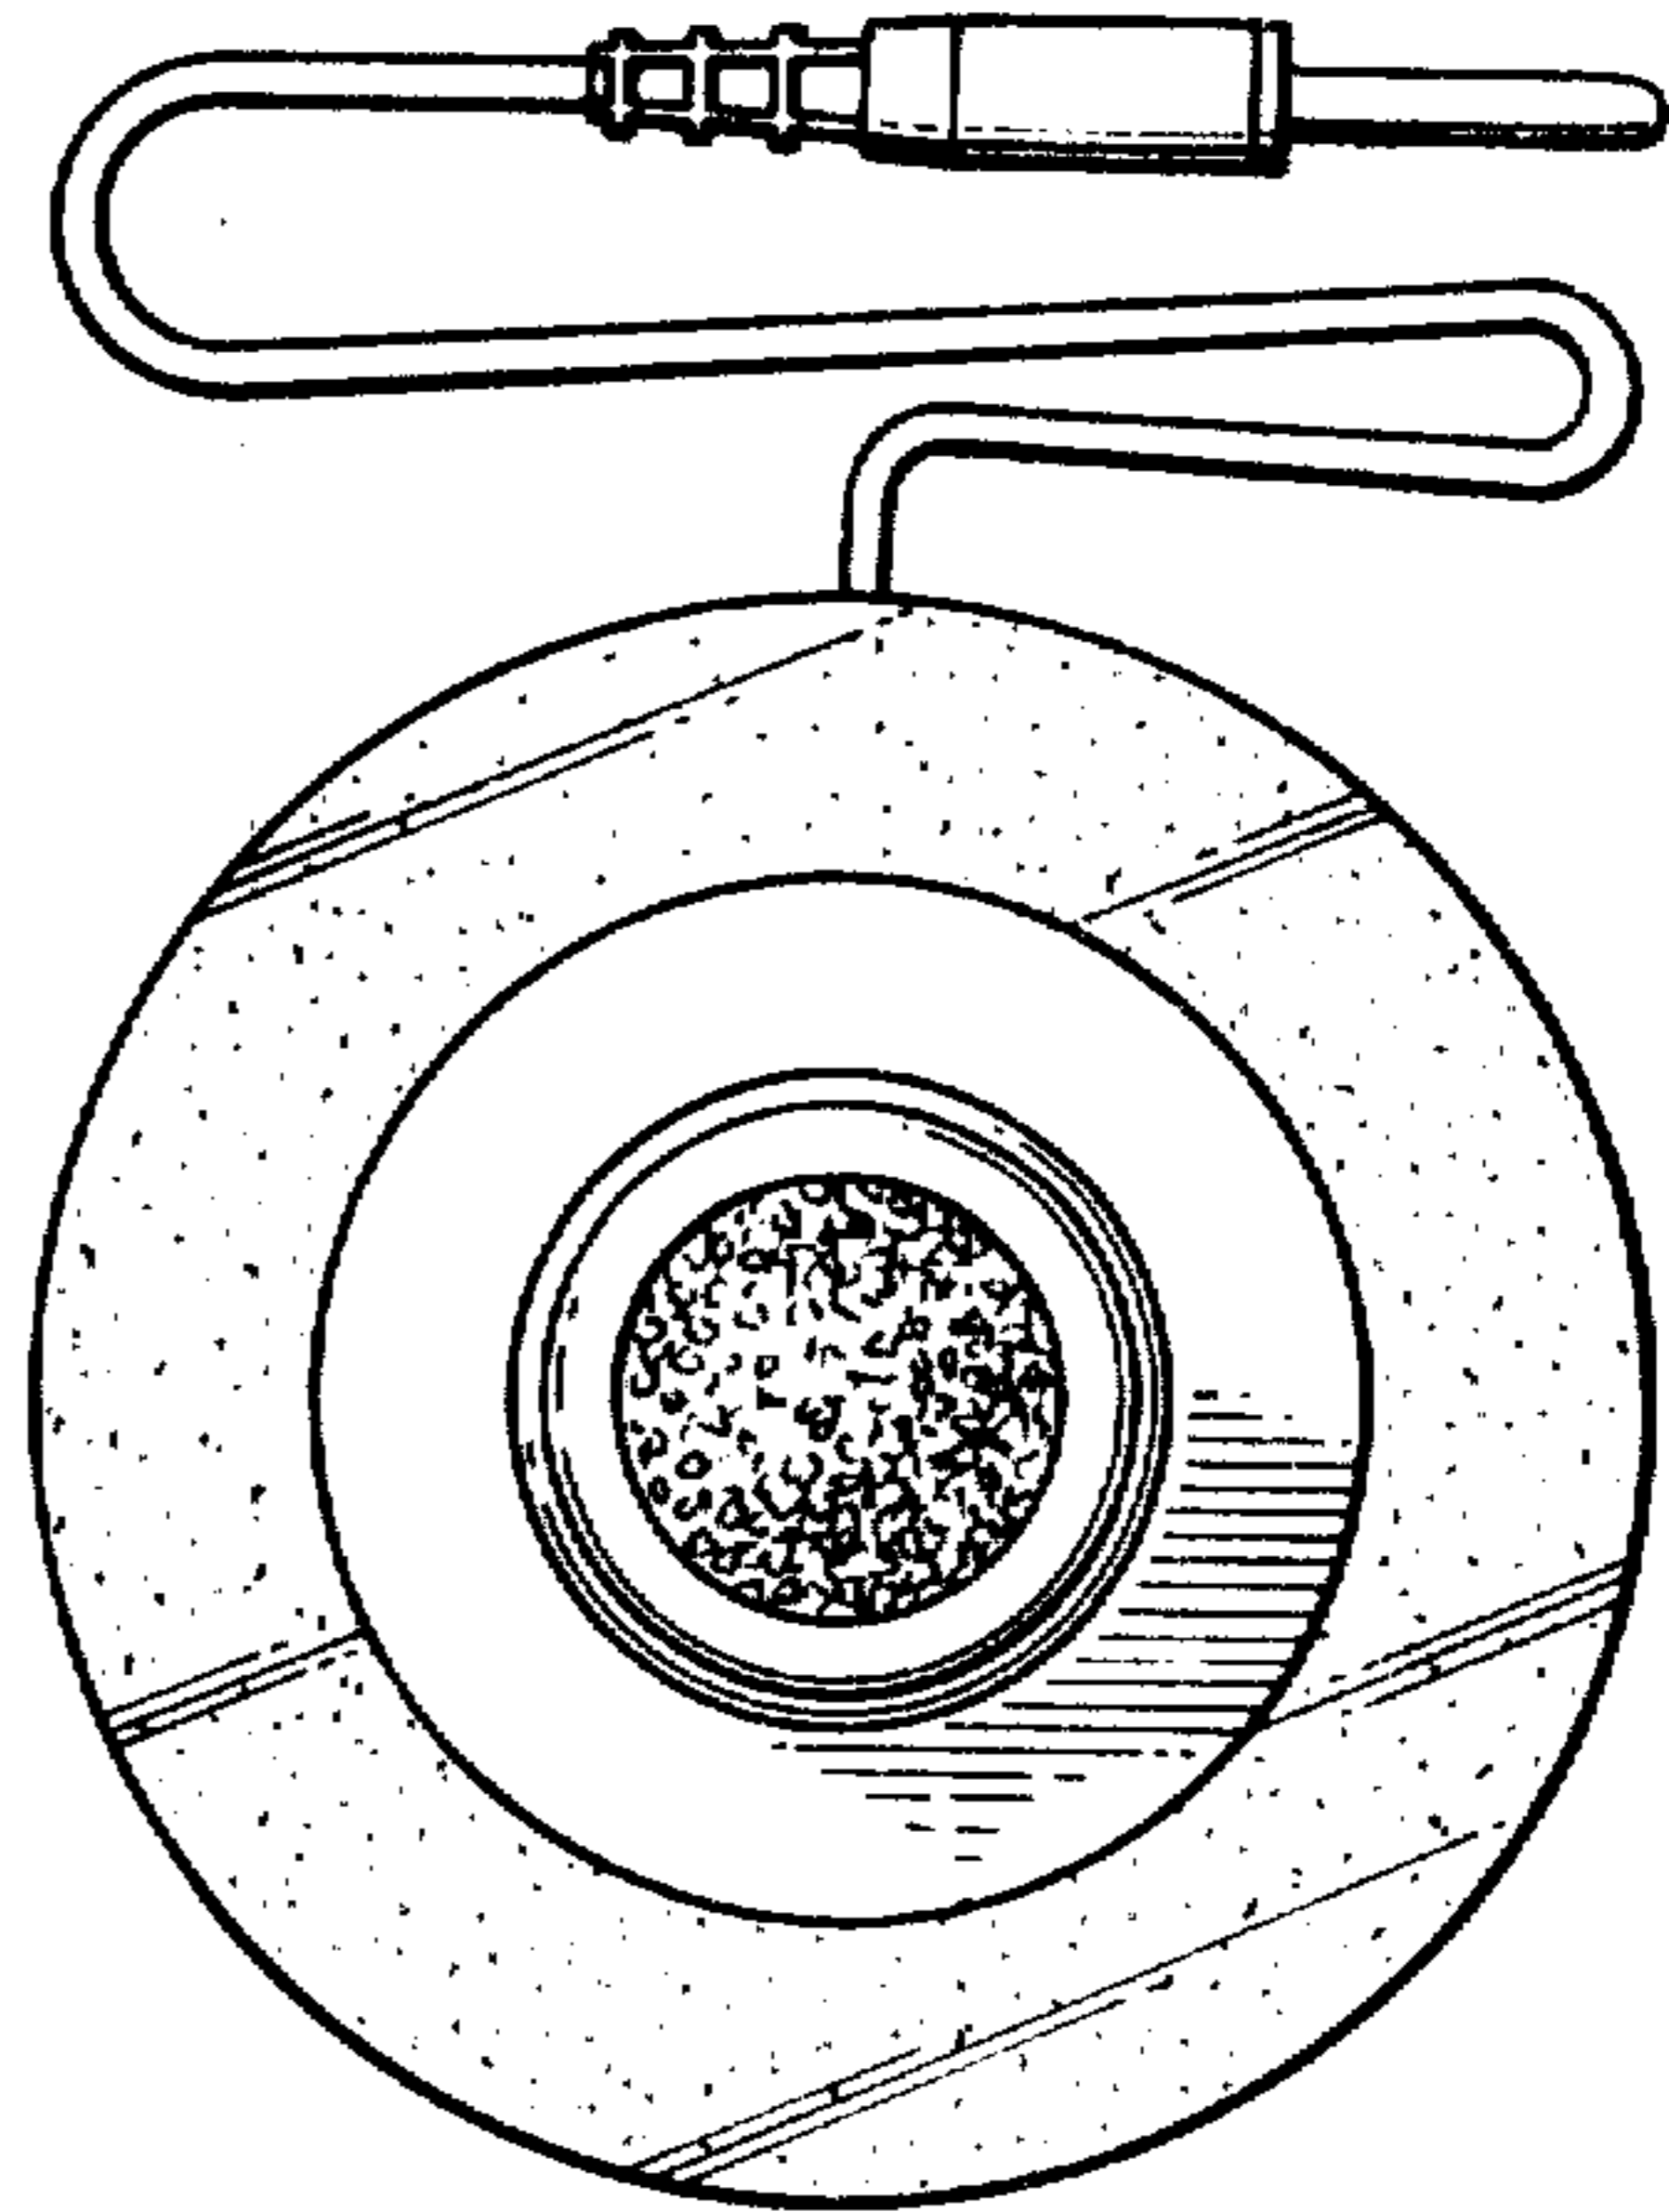

*Fig. 6.*

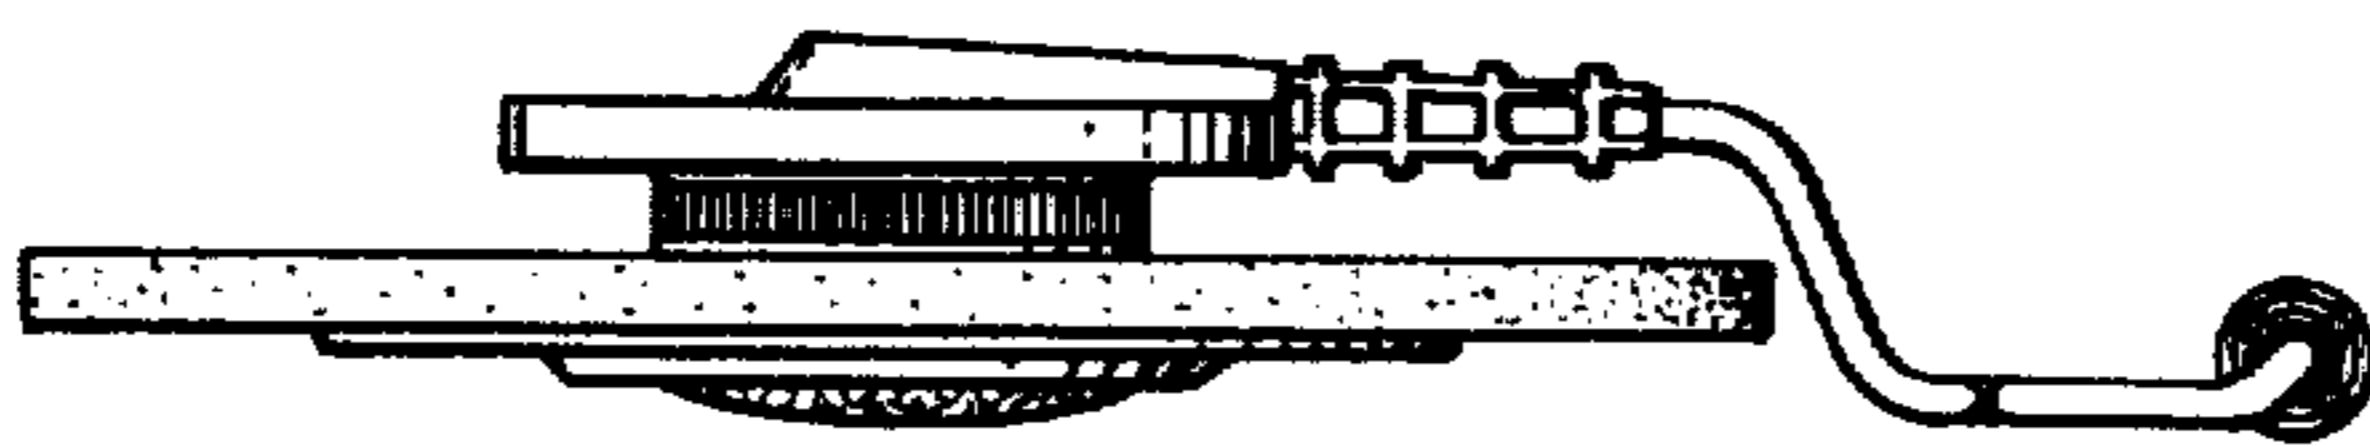

*Fig. 7.*

