

[54] DESIGN FOR A BLOOD CLOT DETECTION INSTRUMENT

3,969,079 7/1976 Catarious et al. 422/73

[75] Inventor: Edward J. Johnson, Furlong, Pa.

[73] Assignee: Warner Lambert Technologies, Inc., Southbridge, Mass.

[**] Term: 14 Years

[21] Appl. No.: 281,440

[22] Filed: Jul. 8, 1981

Related U.S. Application Data

[62] Division of Ser. No. 39,085, May 14, 1979.

[52] U.S. Cl. D24/17; D24/8

[58] Field of Search D24/8, 17, 21, 24; 123/253 R; 422/73; 73/64.1

[56] References Cited

U.S. PATENT DOCUMENTS

- D. 202,466 10/1965 Hayes D24/8
- D. 256,726 9/1980 Meuli D24/8
- D. 262,994 2/1982 Holler, Jr. et al. D24/8
- D. 263,422 3/1982 Koshino D24/8

OTHER PUBLICATIONS

Video Review, Dec. 1981, vol. 2 No. 9, ©1981 Viaro Pub. Co. pp. 52, 56, copy available at USPFO. Lafayette 1975, Electronics Catalog No. 750 p. 237 Lafayette Monitorscan.


Primary Examiner—Bernard Ansher
Assistant Examiner—Horace B. Fay
Attorney, Agent, or Firm—Alan H. Spencer

[57] CLAIM

The ornamental design of a blood clot detection instrument, as shown and described.

DESCRIPTION

FIG. 1 is a front left top perspective view of a blood clot detection instrument showing my new design; FIG. 2 is a top plan view thereof; FIG. 3 is a front elevational view thereof; FIG. 4 is a left side elevational view thereof, the right side elevational view being a mirror image of FIG. 4; FIG. 5 is a rear elevational view in which the details shown upon the upper horizontal surfaces in FIGS. 3 and 4 are omitted for ease of illustration.

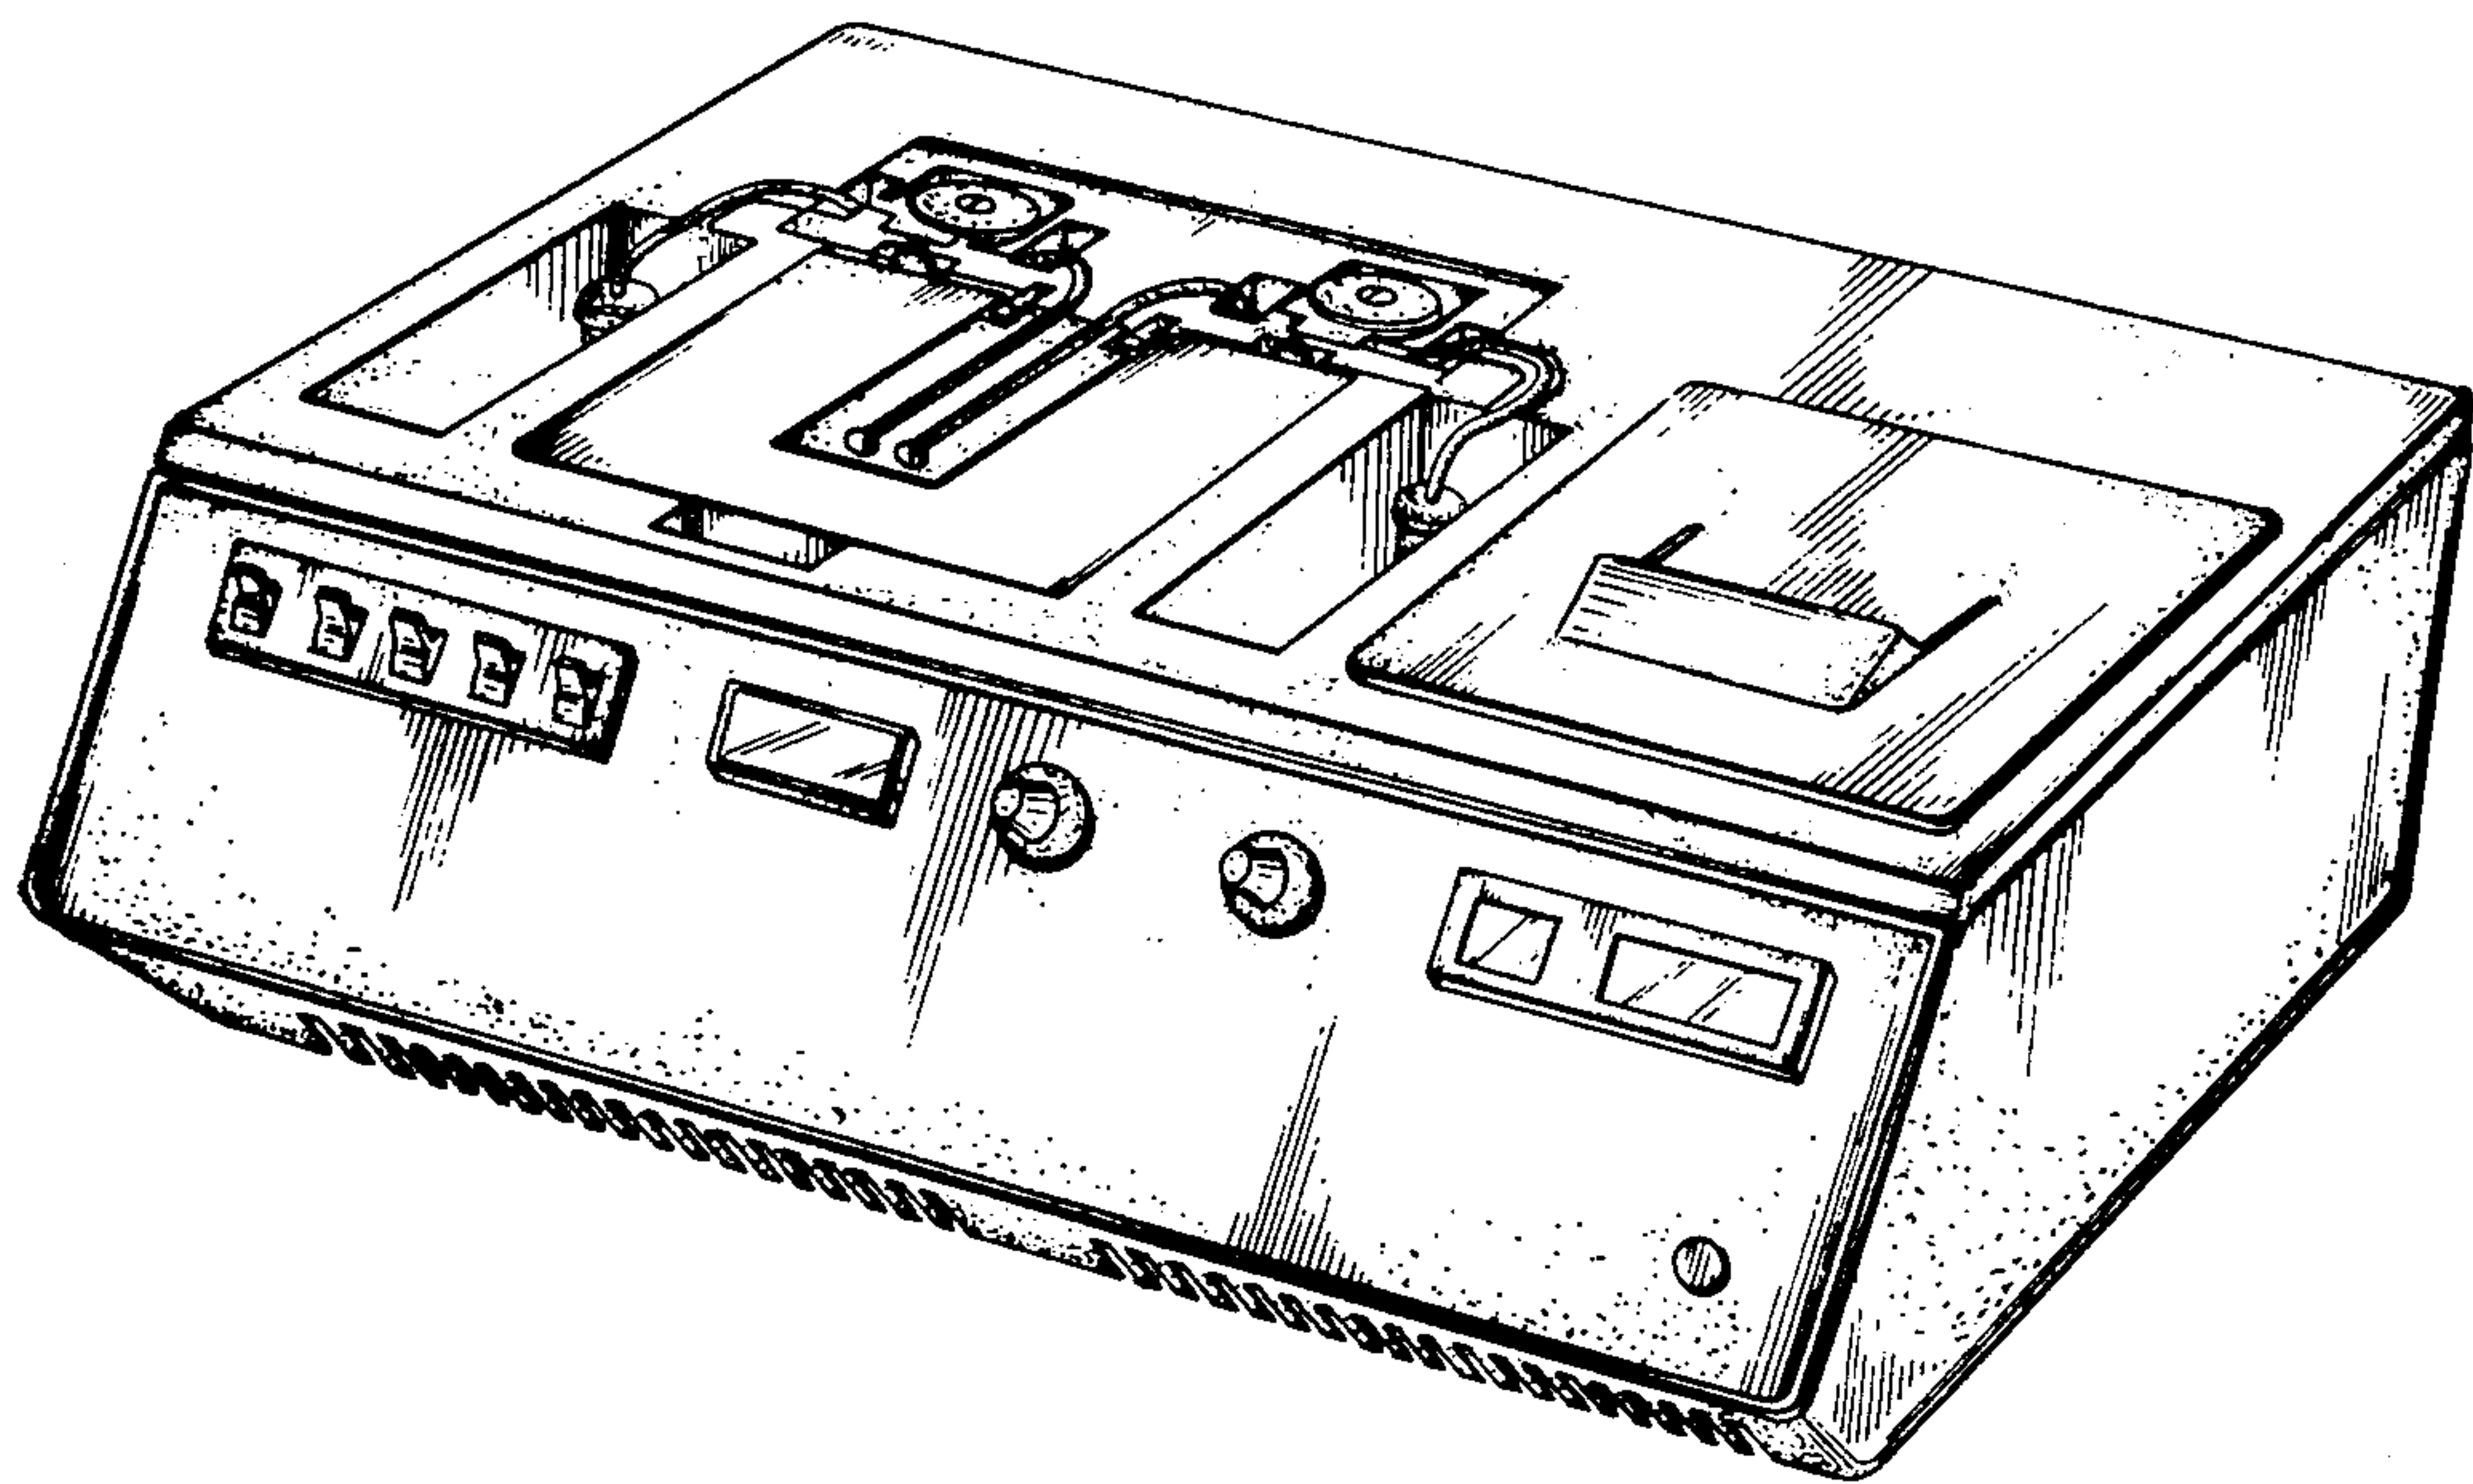

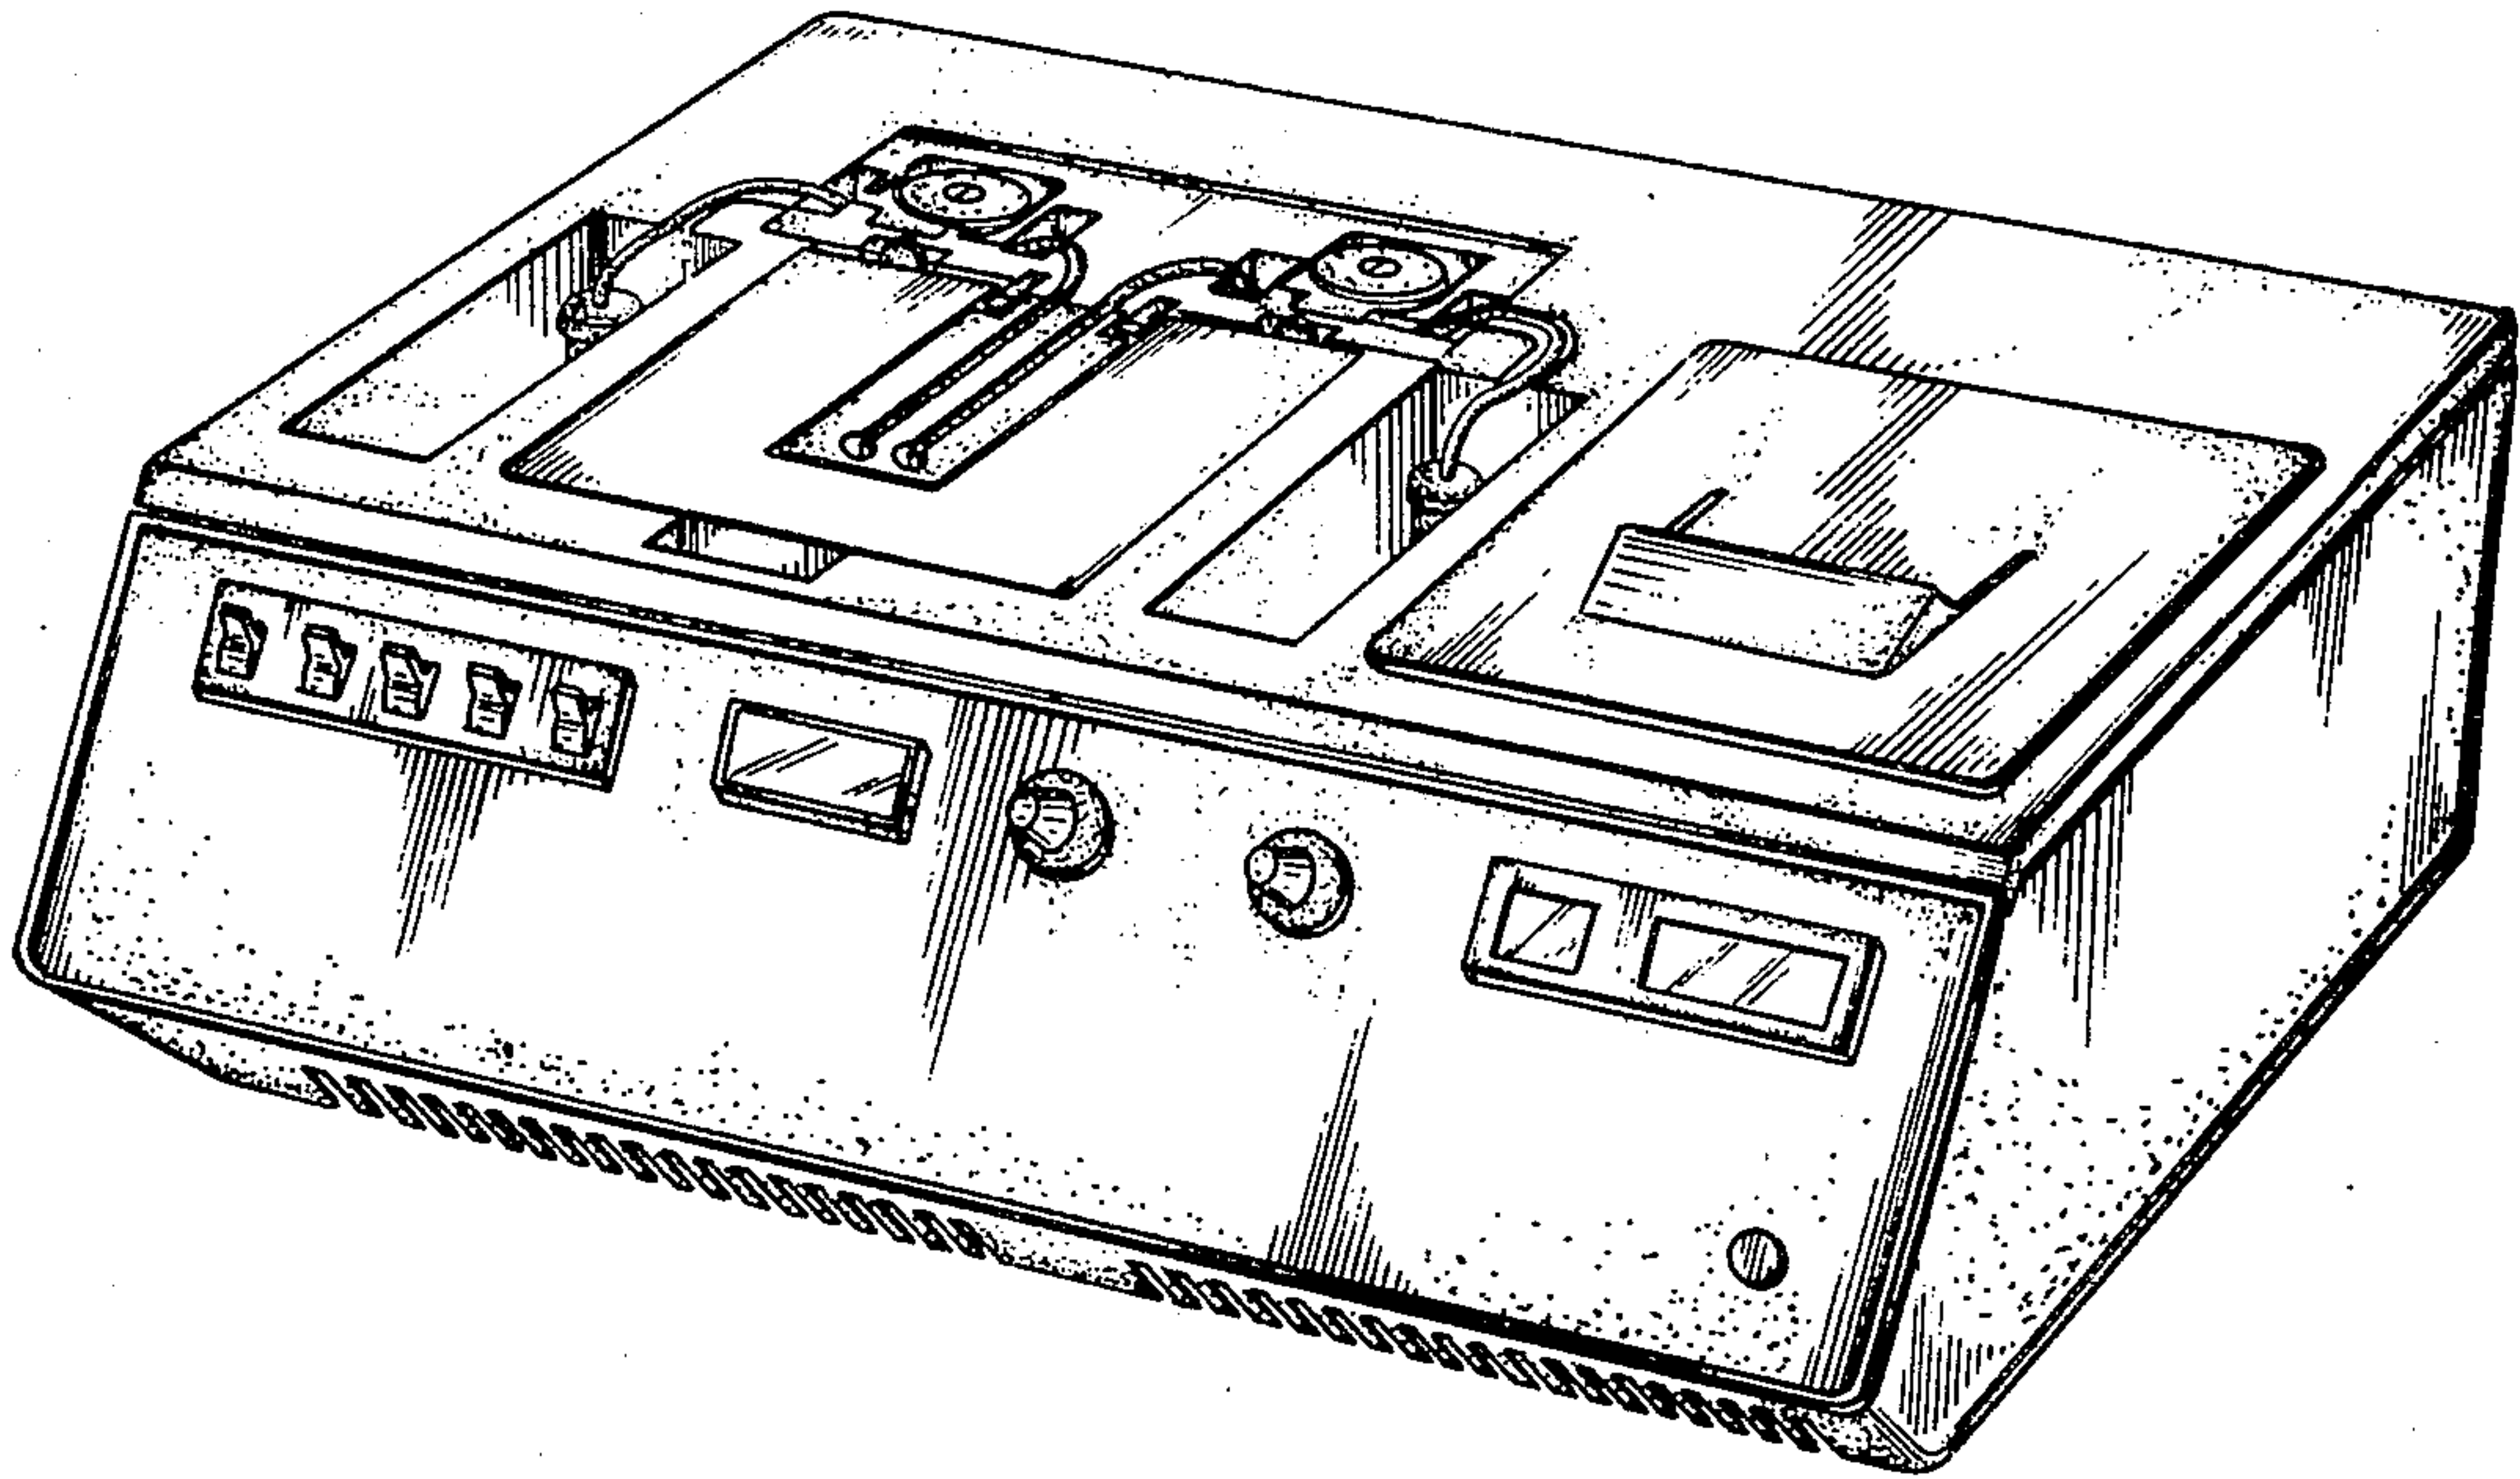


FIG. 1

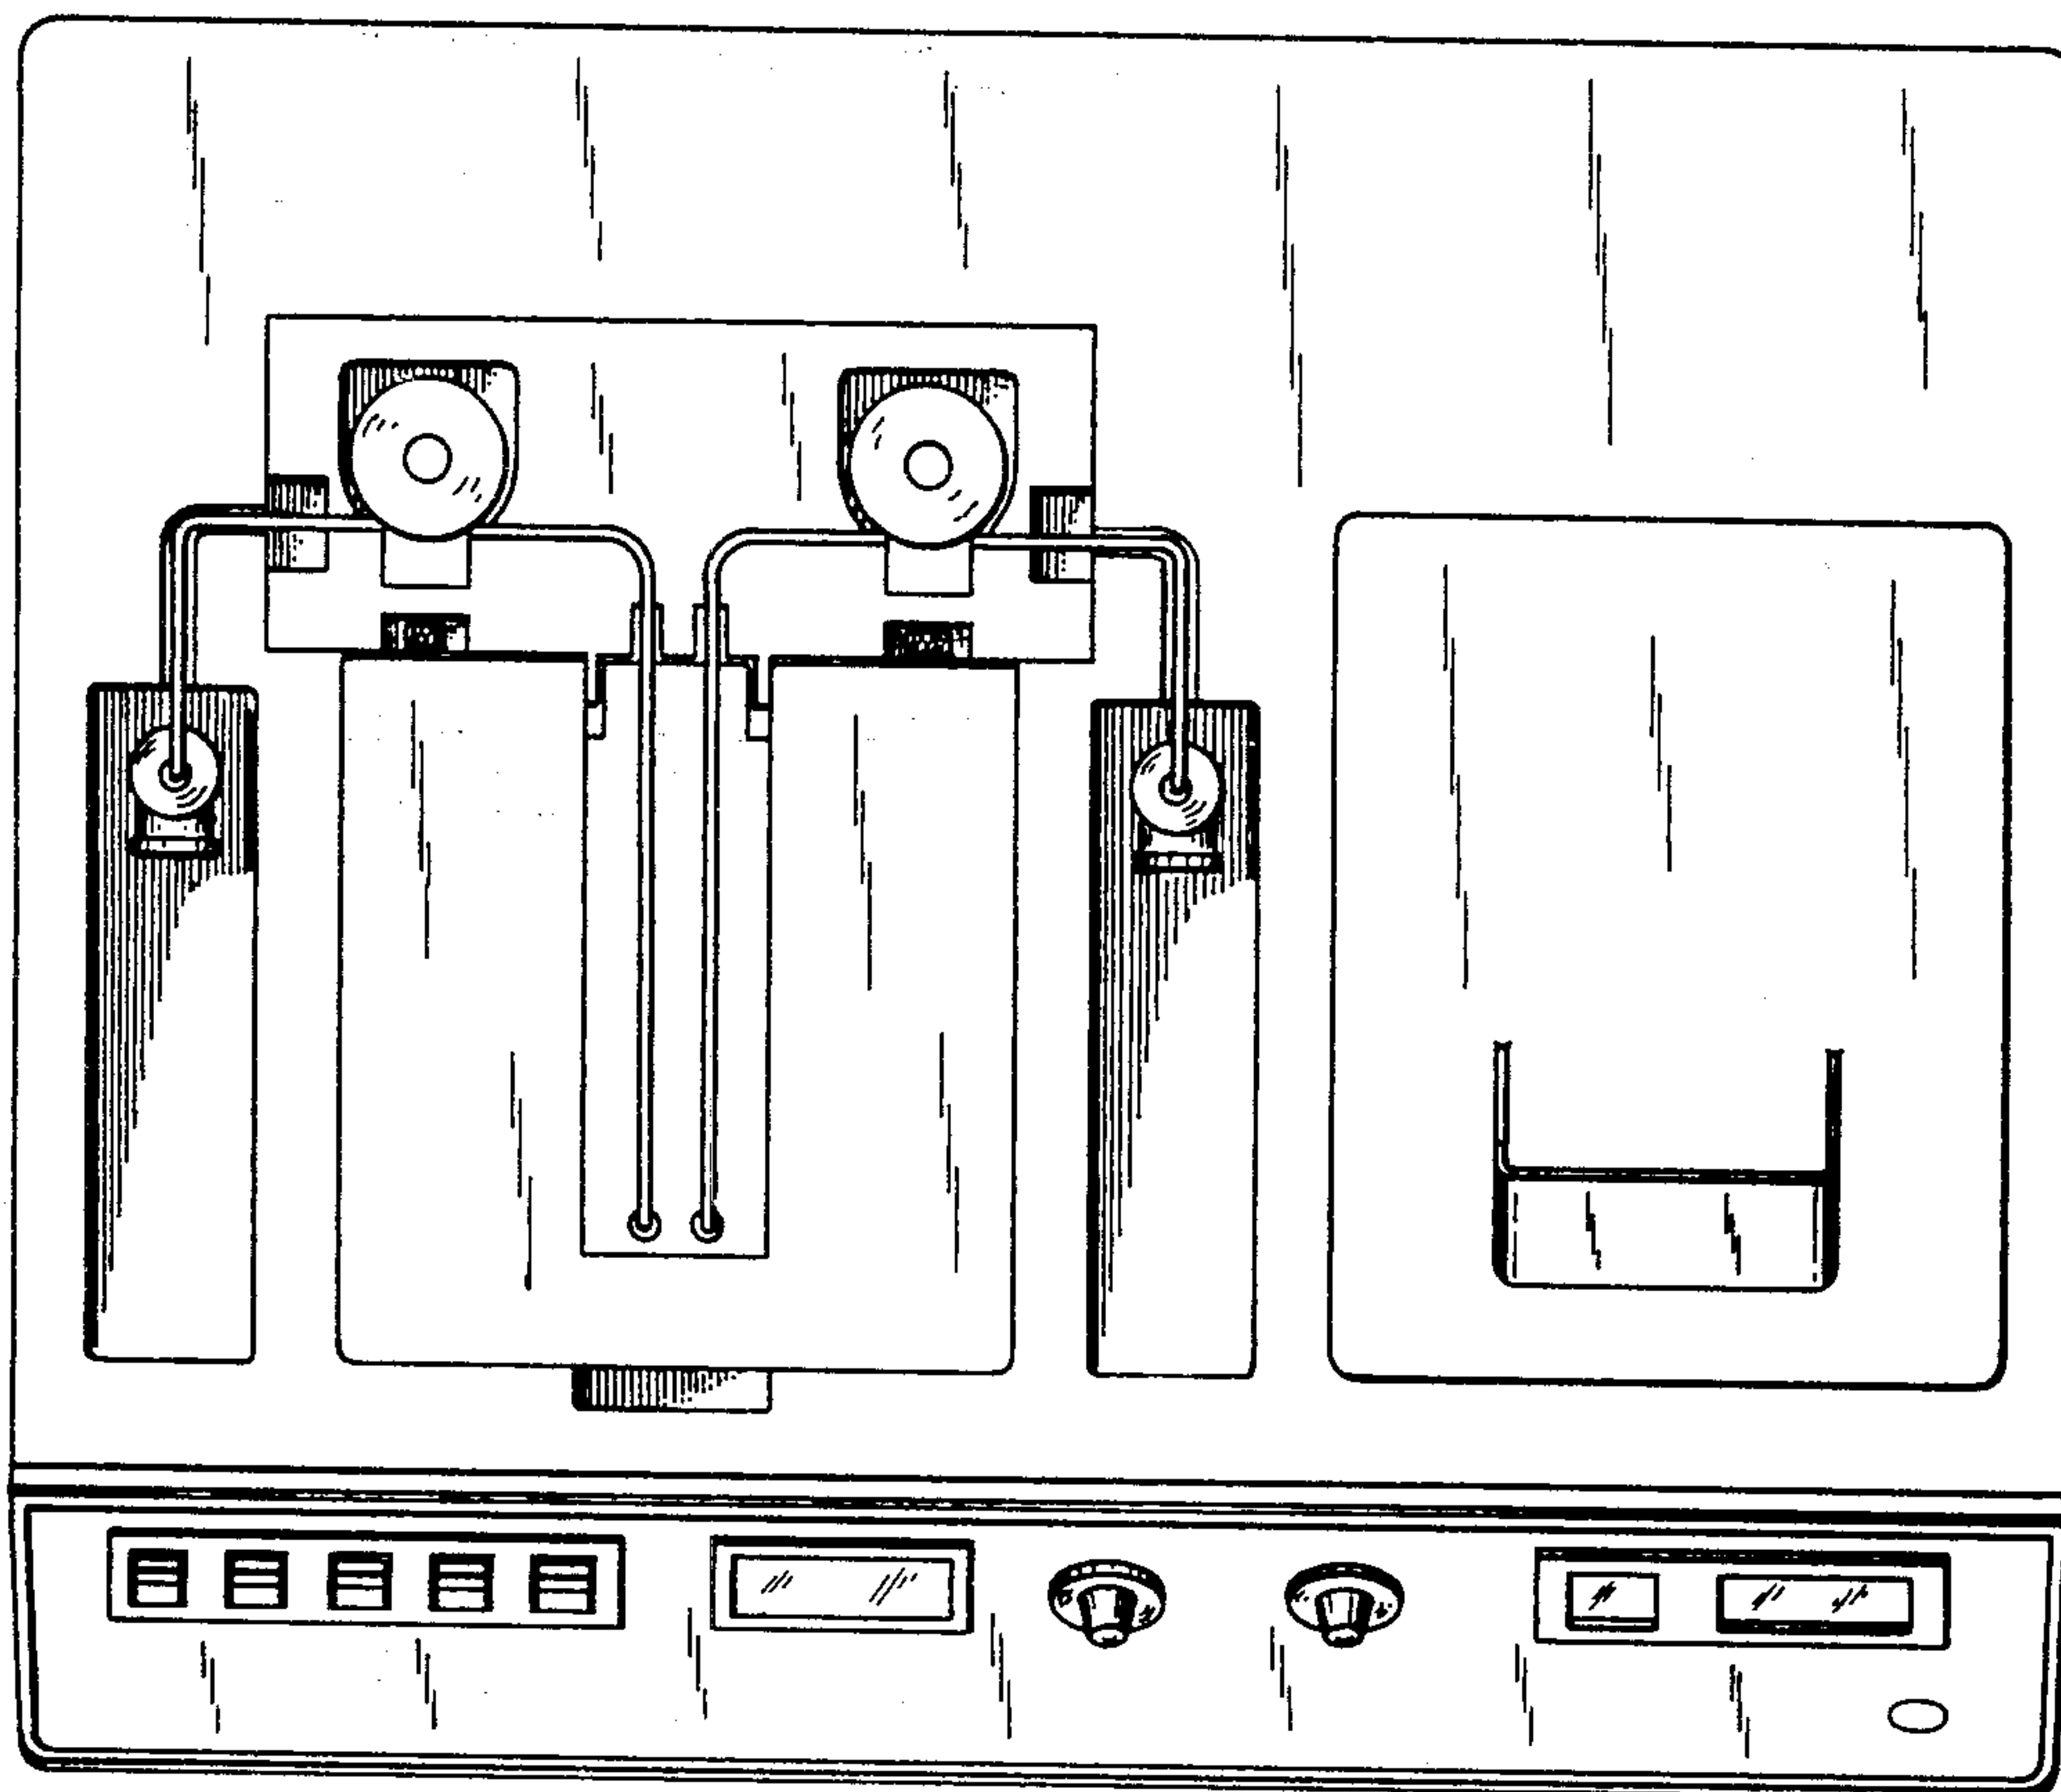


FIG. 2

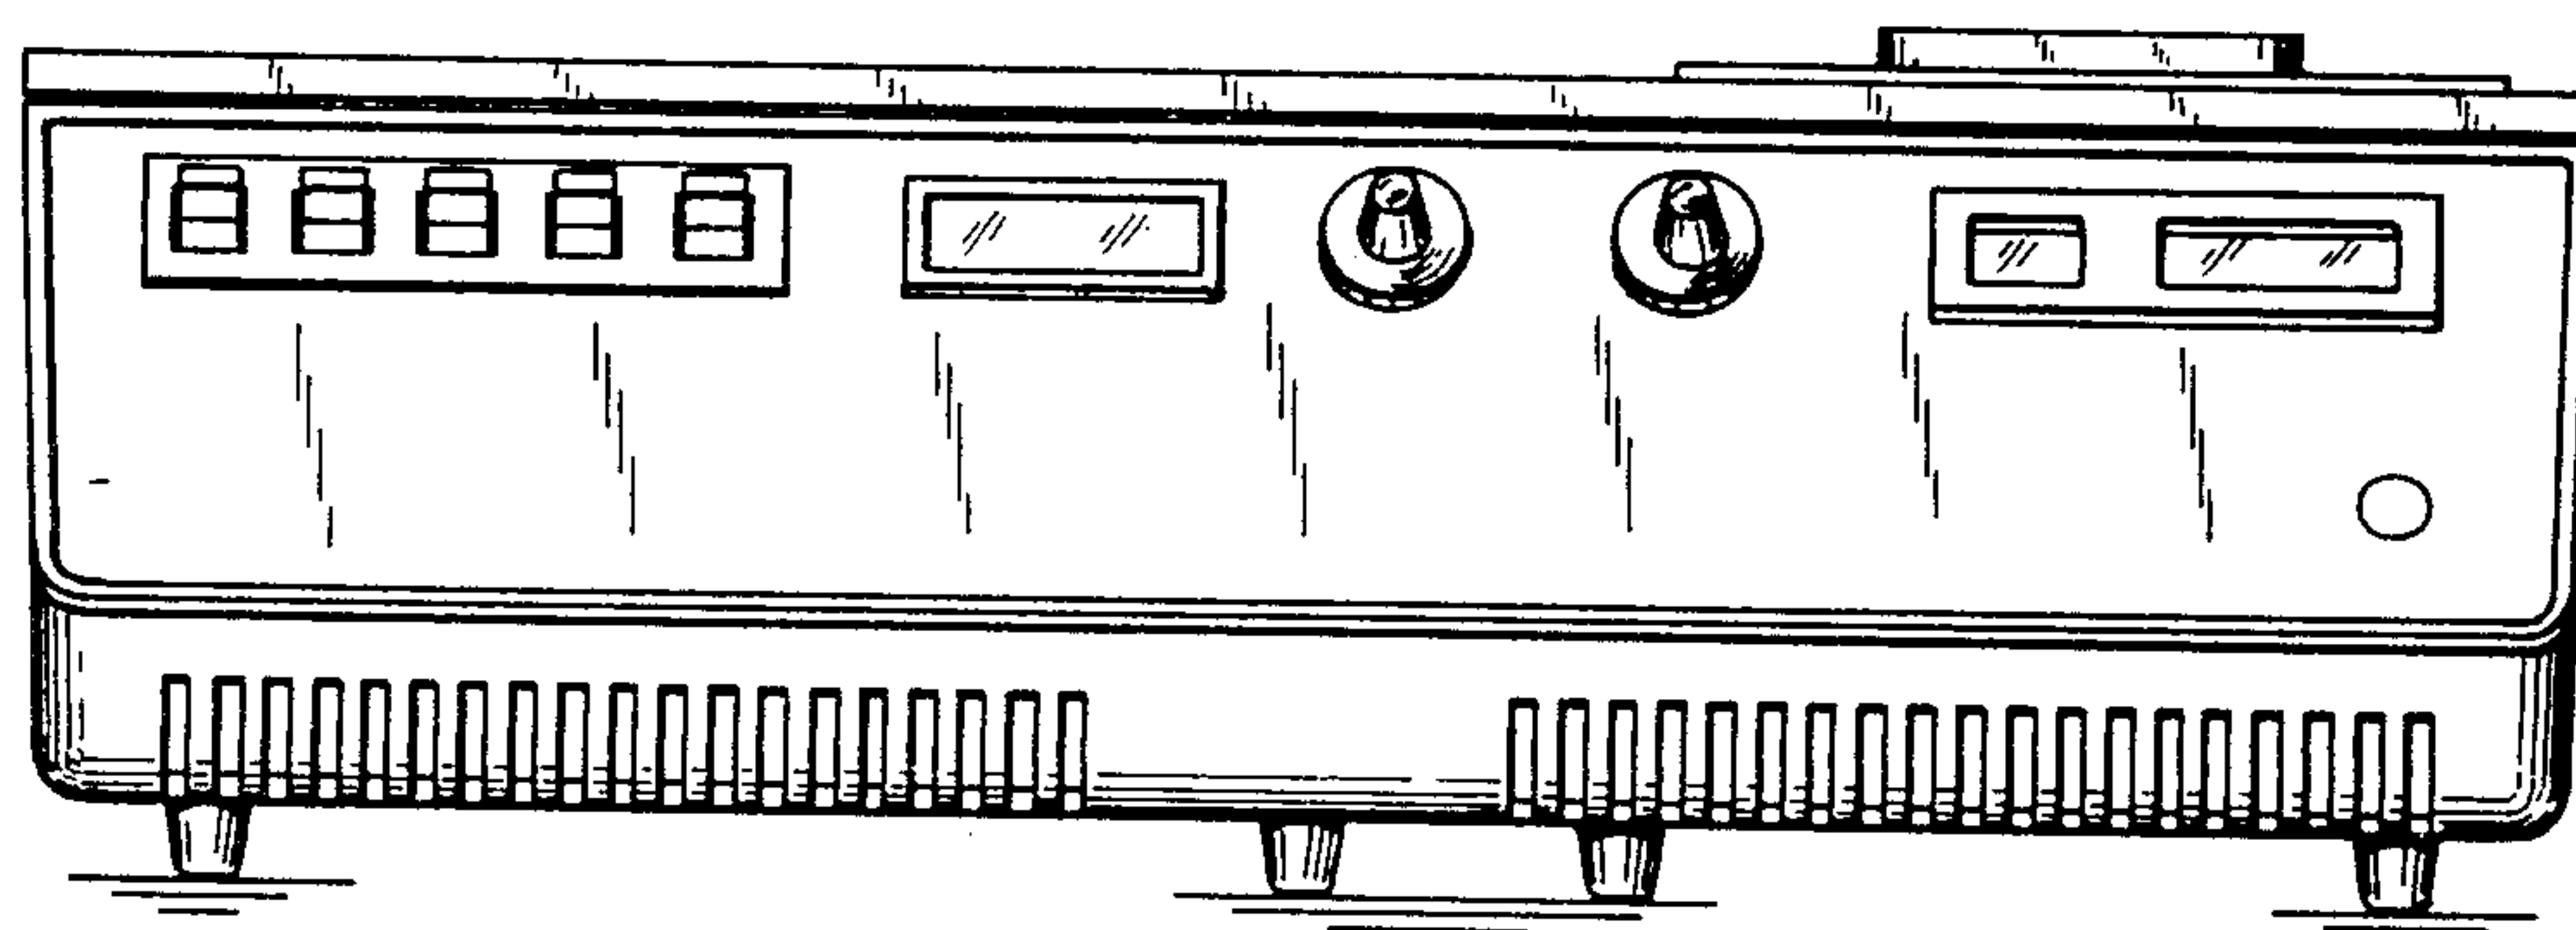


FIG. 3

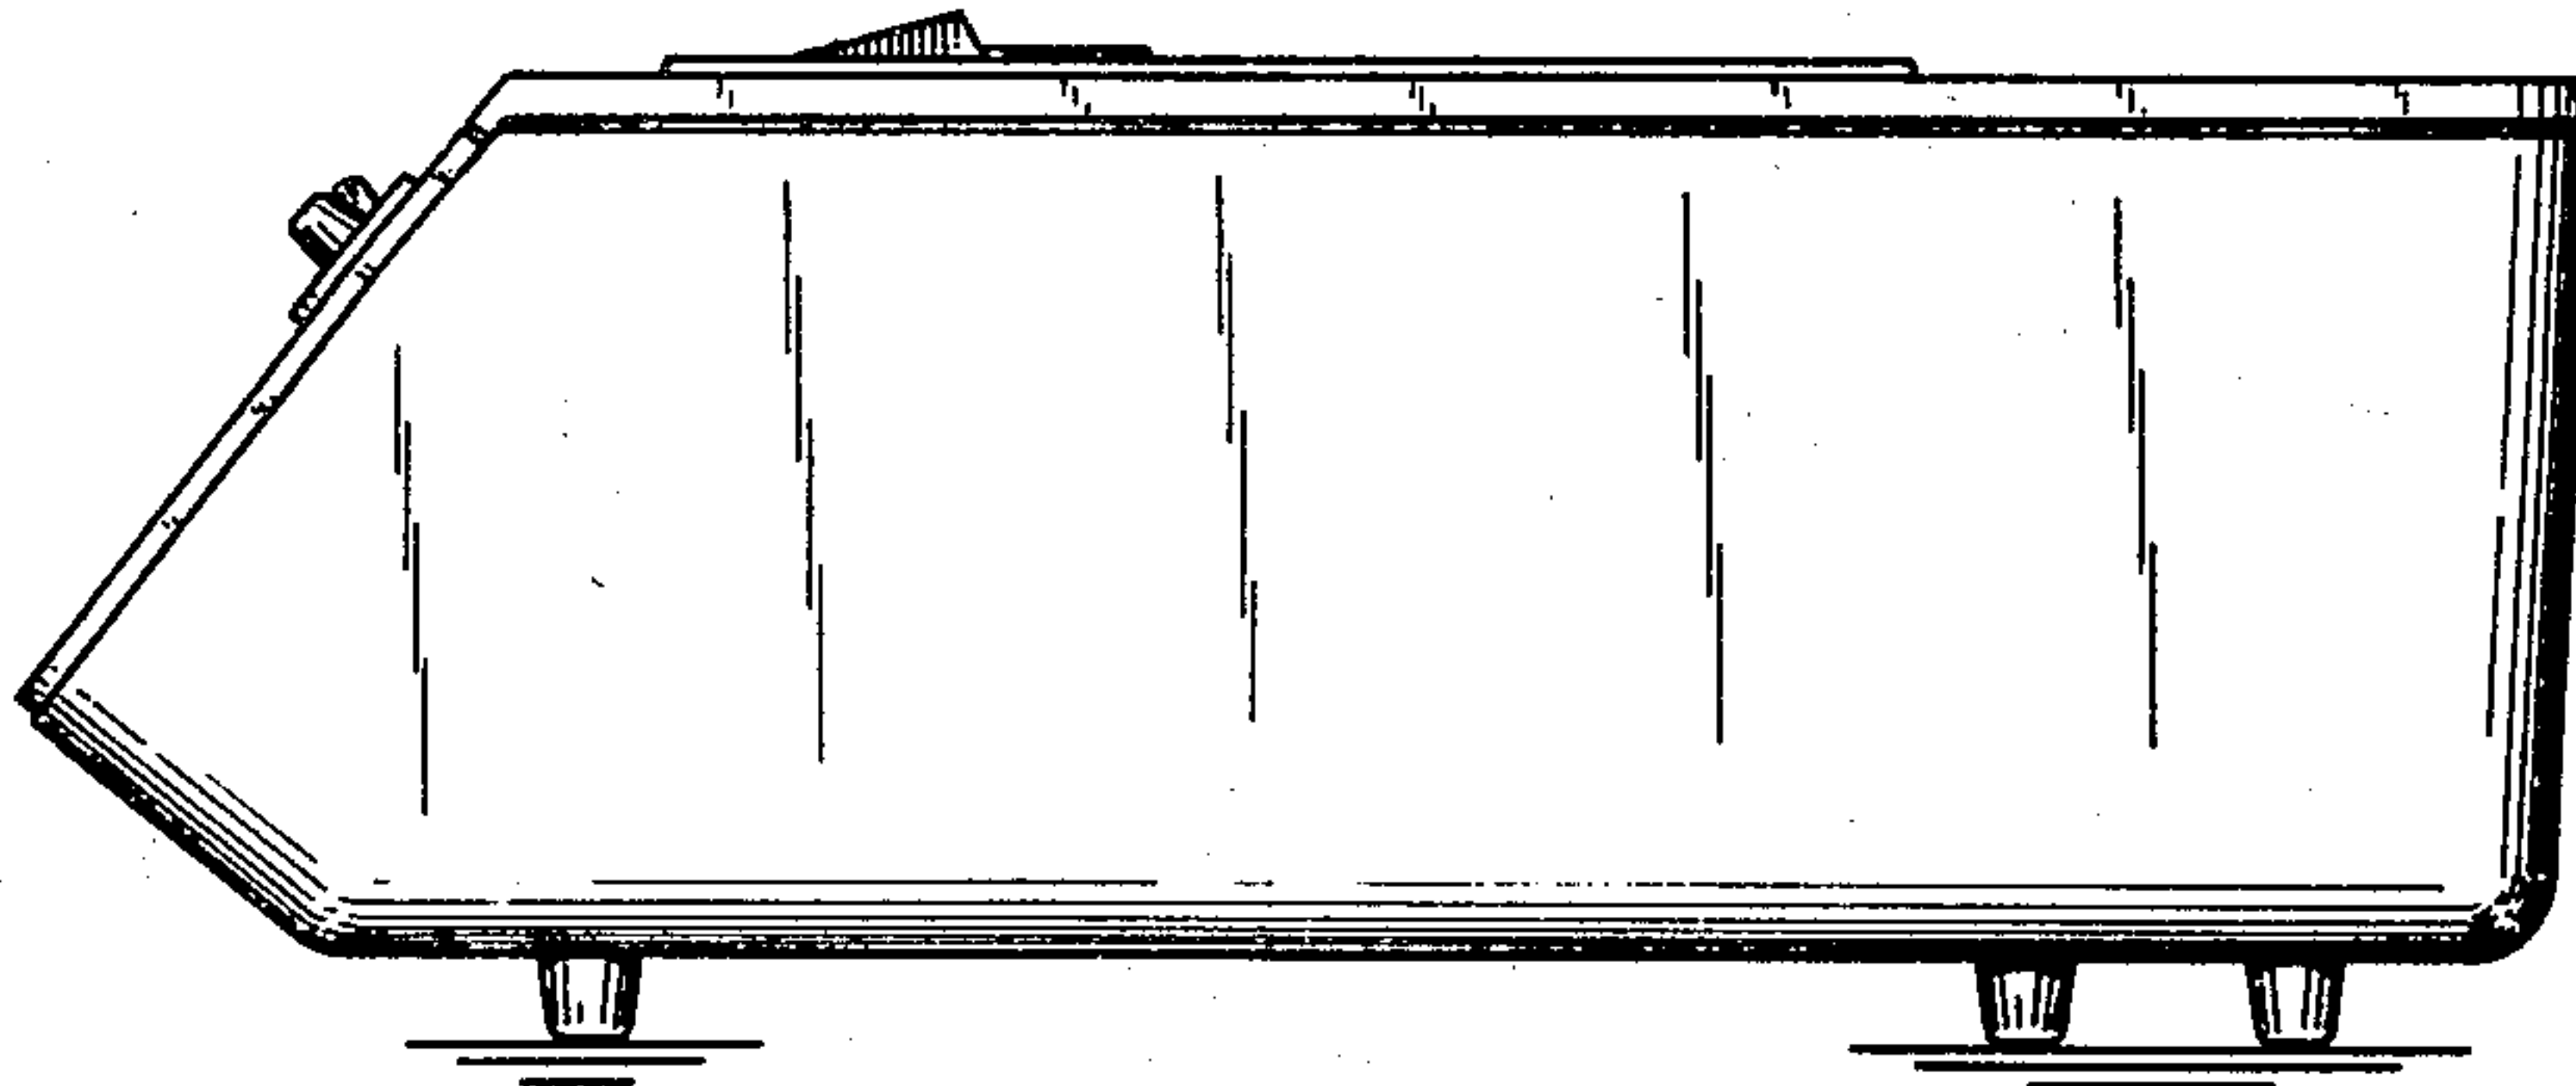


FIG. 4

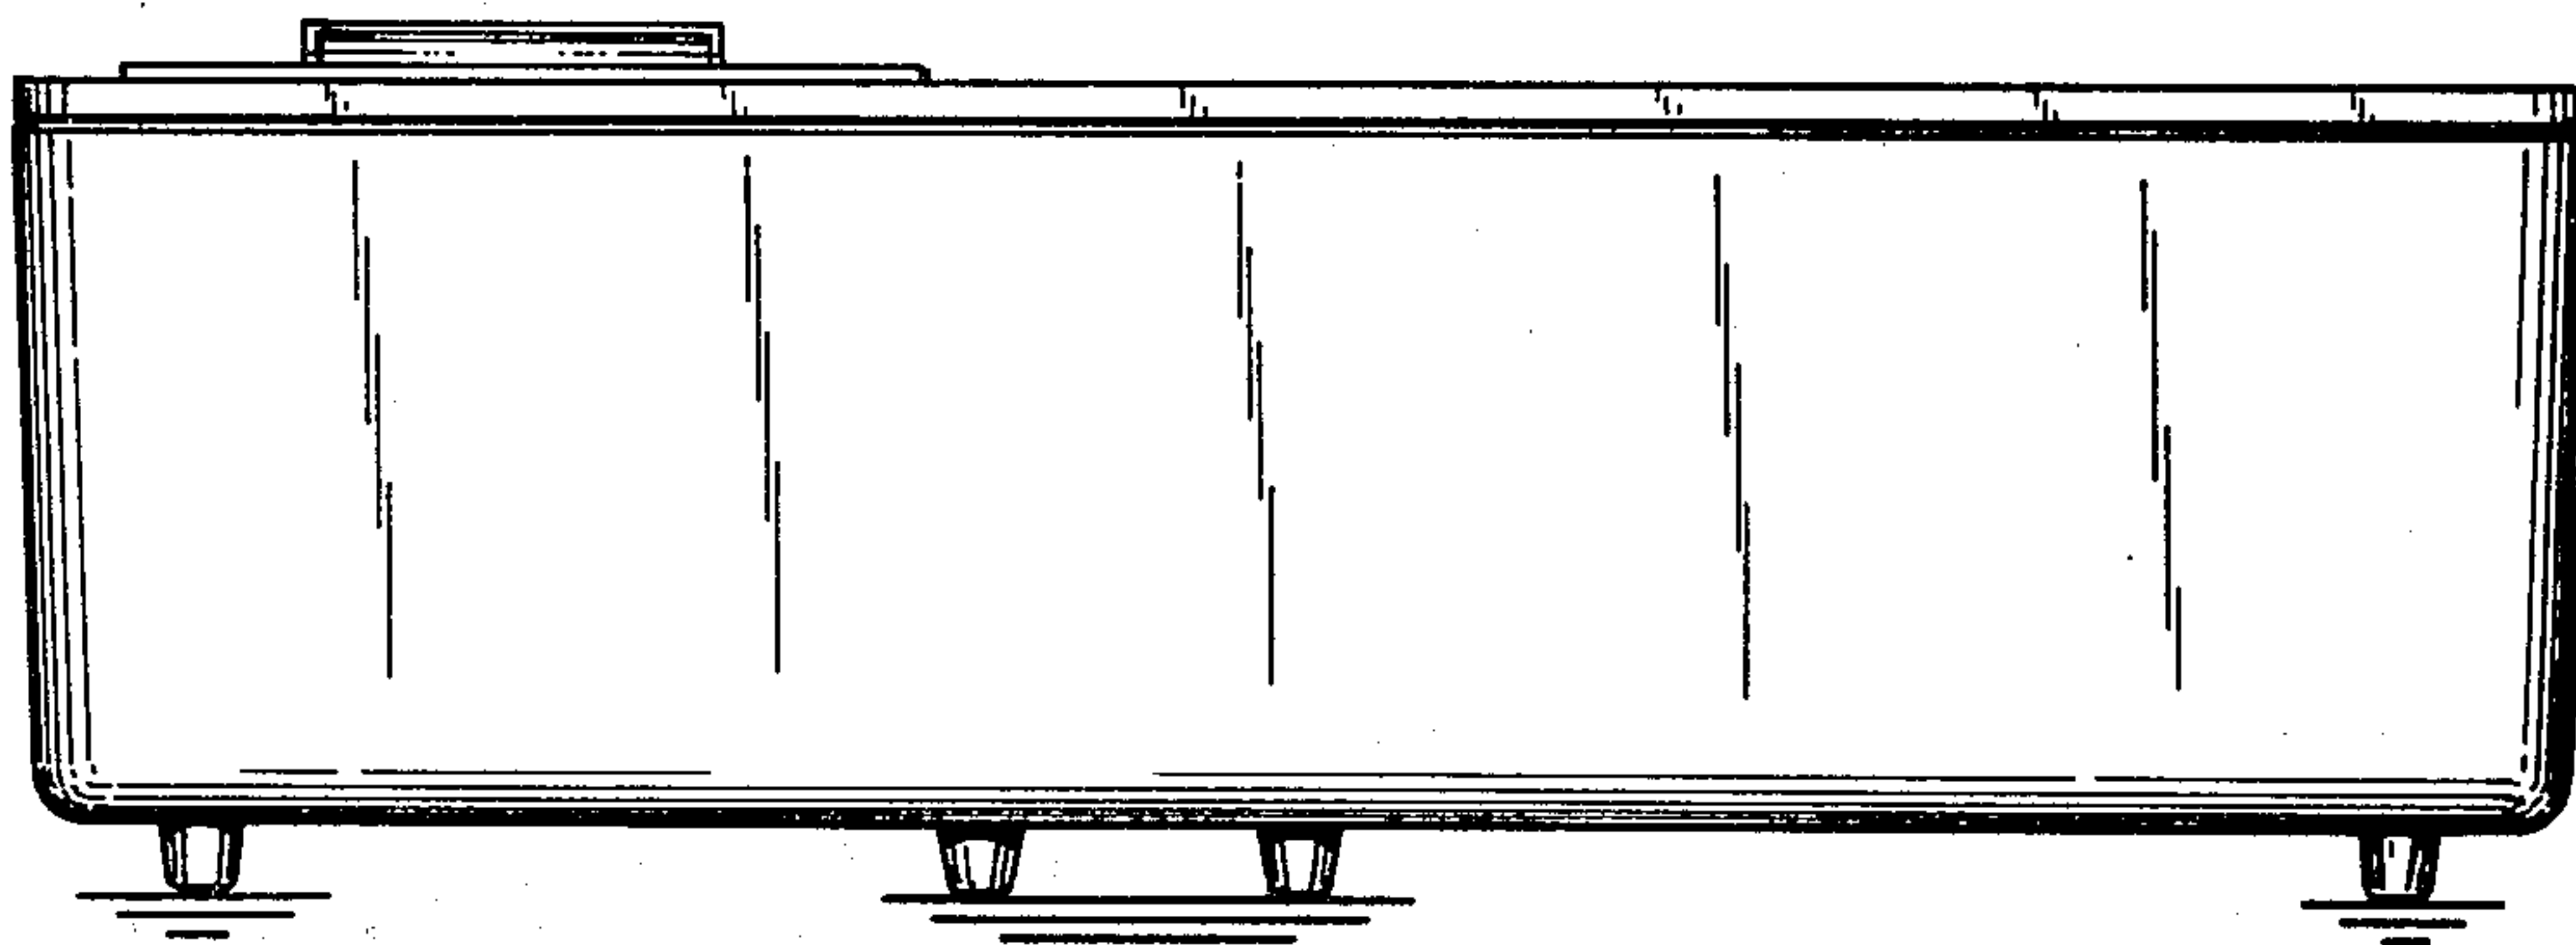


FIG. 5