

[54] CLOT DETECTION APPARATUS

[75] Inventor: Warren J. Bonney, Yardley, Pa.

[73] Assignee: Warner-Lambert Co., Morris Plains, N.J.

[\*\*] Term: 14 Years

[21] Appl. No.: 315,078

[22] Filed: Oct. 26, 1981

[52] U.S. Cl. .... D24/17; D10/46; D24/22

[58] Field of Search ..... 128/637, 638, 770; D24/8, 17, 21, 22; D10/46

[56] References Cited

U.S. PATENT DOCUMENTS

- D. 211,466 6/1968 Gulotta ..... D24/22
- D. 230,355 2/1974 van den Broek et al. .... D10/46
- D. 248,044 5/1978 Odom et al. .... D24/22
- D. 248,407 7/1978 Bassett et al. .... D24/22

- D. 254,806 4/1980 Kitai et al. .... D24/17
- D. 264,991 6/1982 Quandt ..... D24/17
- 3,626,929 12/1971 Sanz et al. .... 128/770
- 4,167,038 9/1979 Hennessy ..... 128/637 X

Primary Examiner—Bernard Ansher  
Attorney, Agent, or Firm—Gary M. Nath; Daniel A. Scola, Jr.


[57] CLAIM

The ornamental design for a clot detection apparatus, as shown and described.

DESCRIPTION

FIG. 1 is a top plan view of the clot detection apparatus holder embodying my new design; FIG. 2 is an elevational view of one side of the clot detection apparatus; and FIG. 3 is a perspective view of the clot detection apparatus thereof.

The undisclosed rear portions of the clot detection apparatus are plane and unornamented.

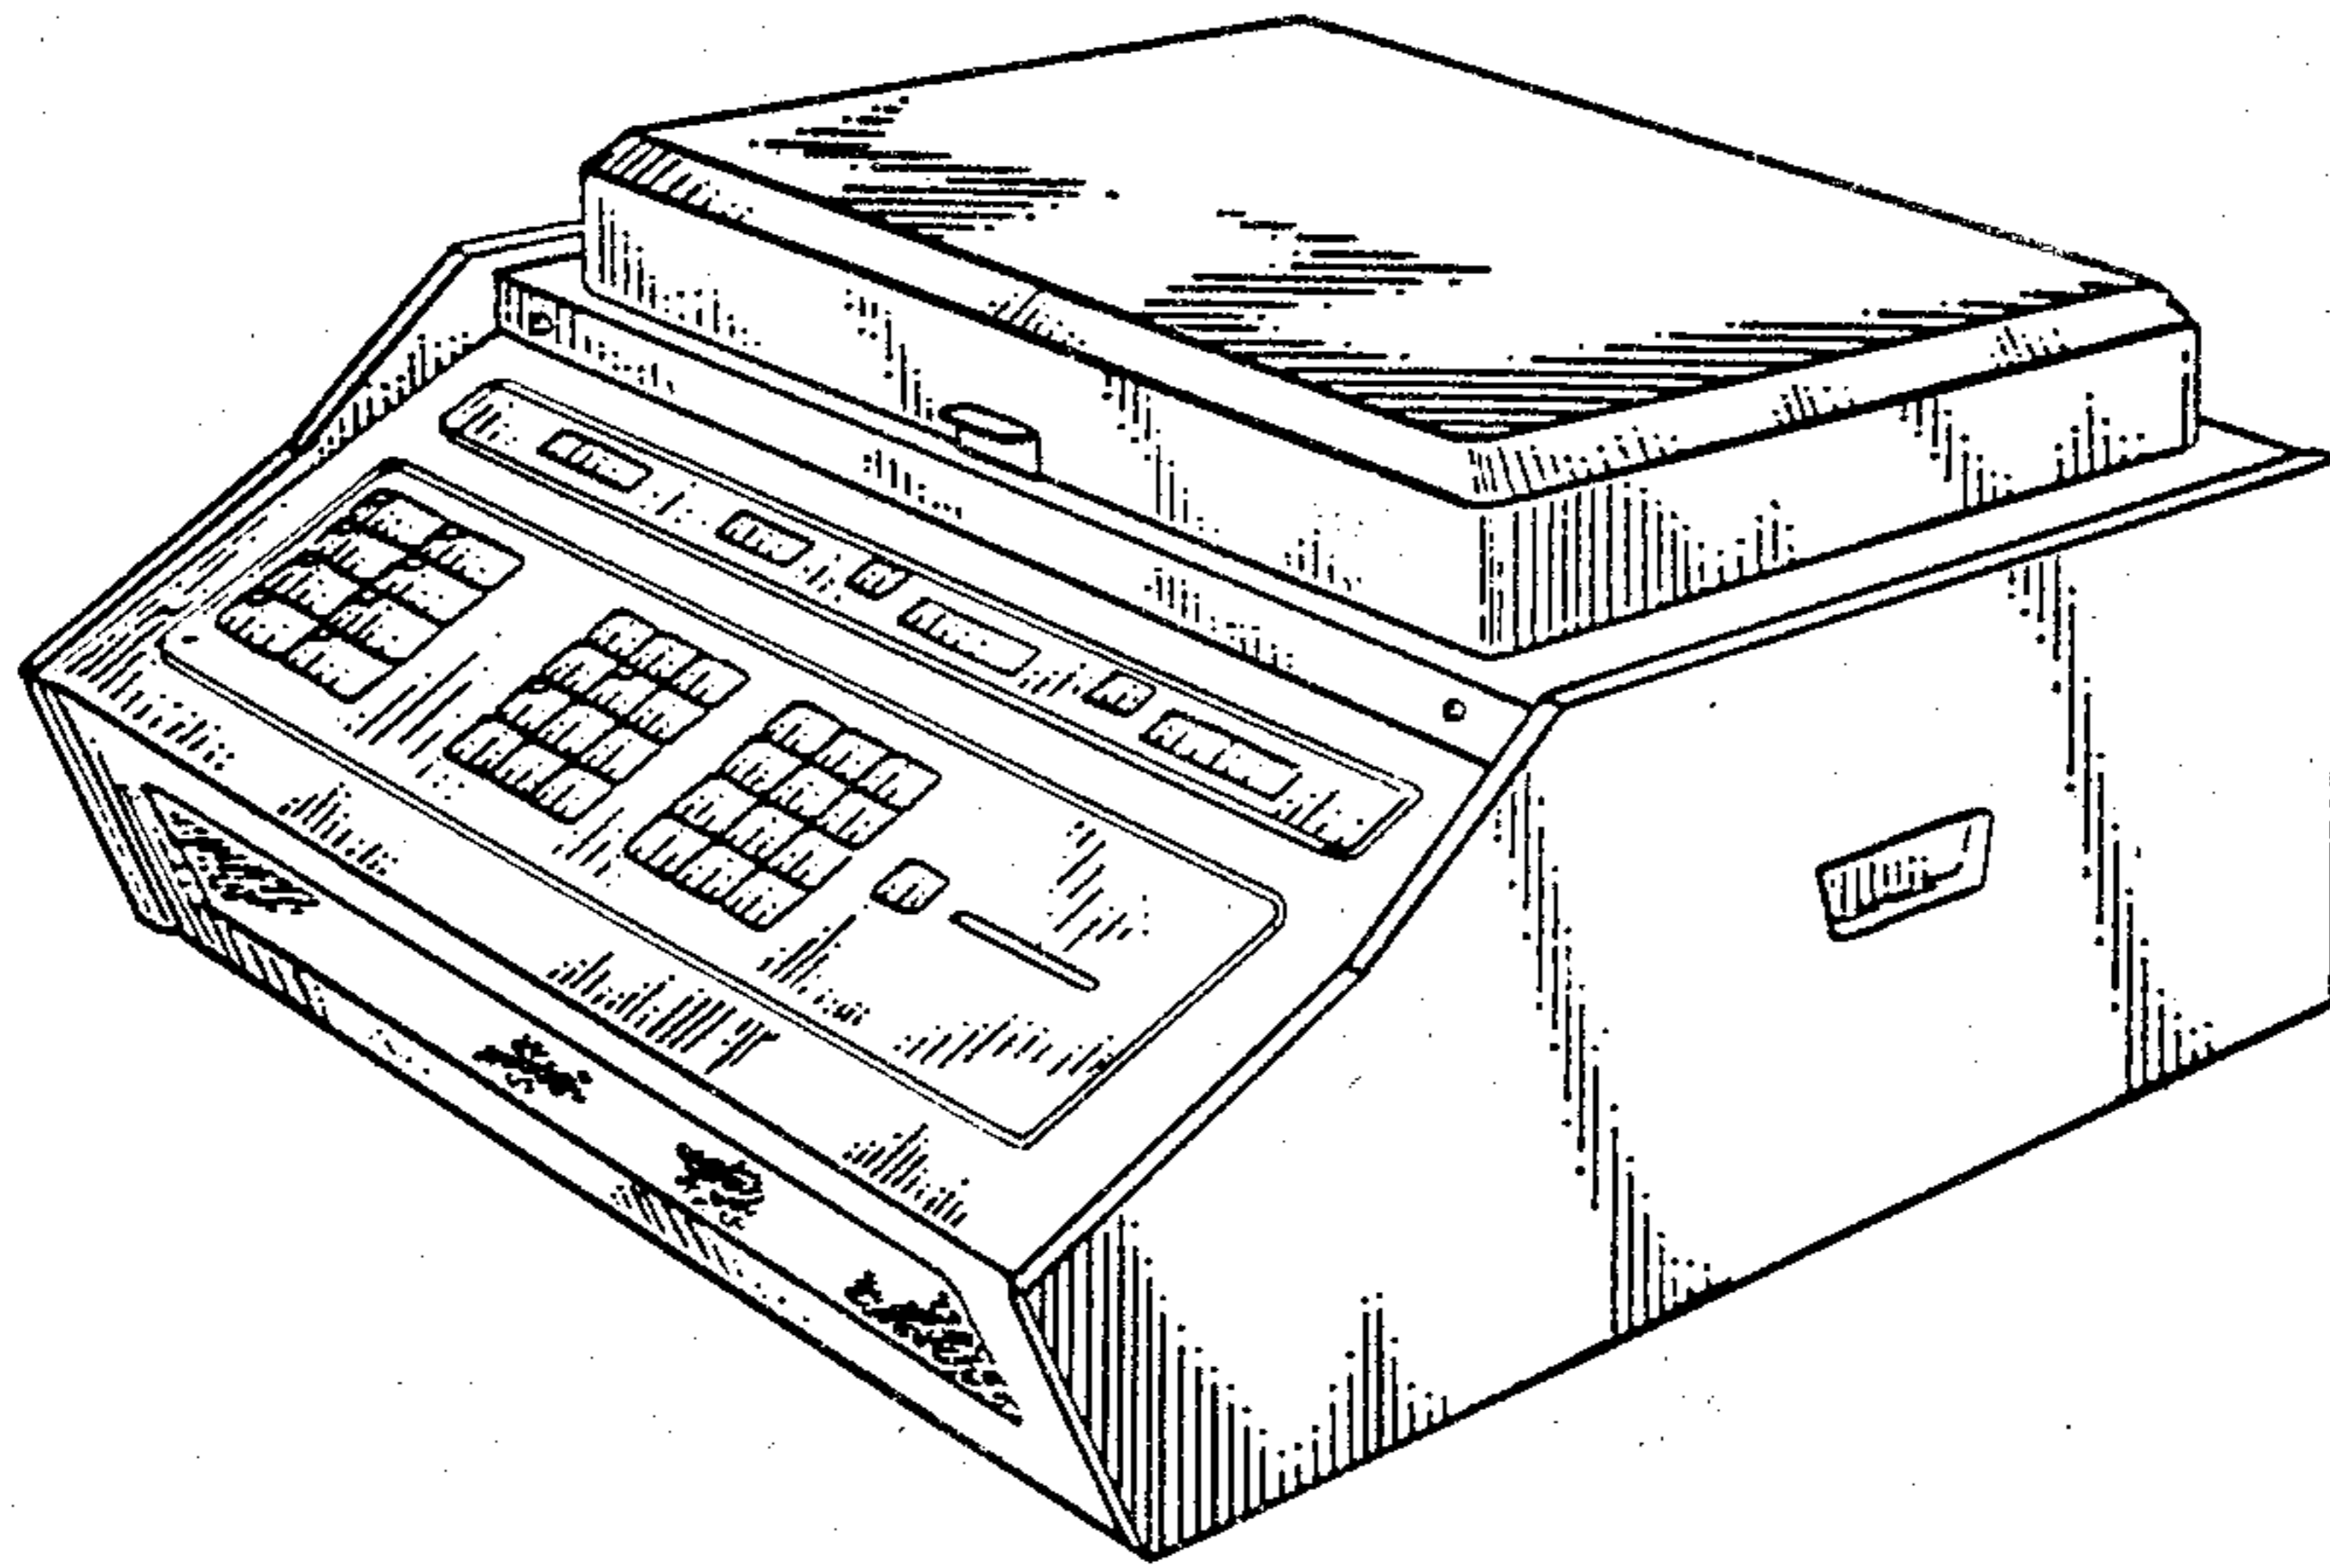

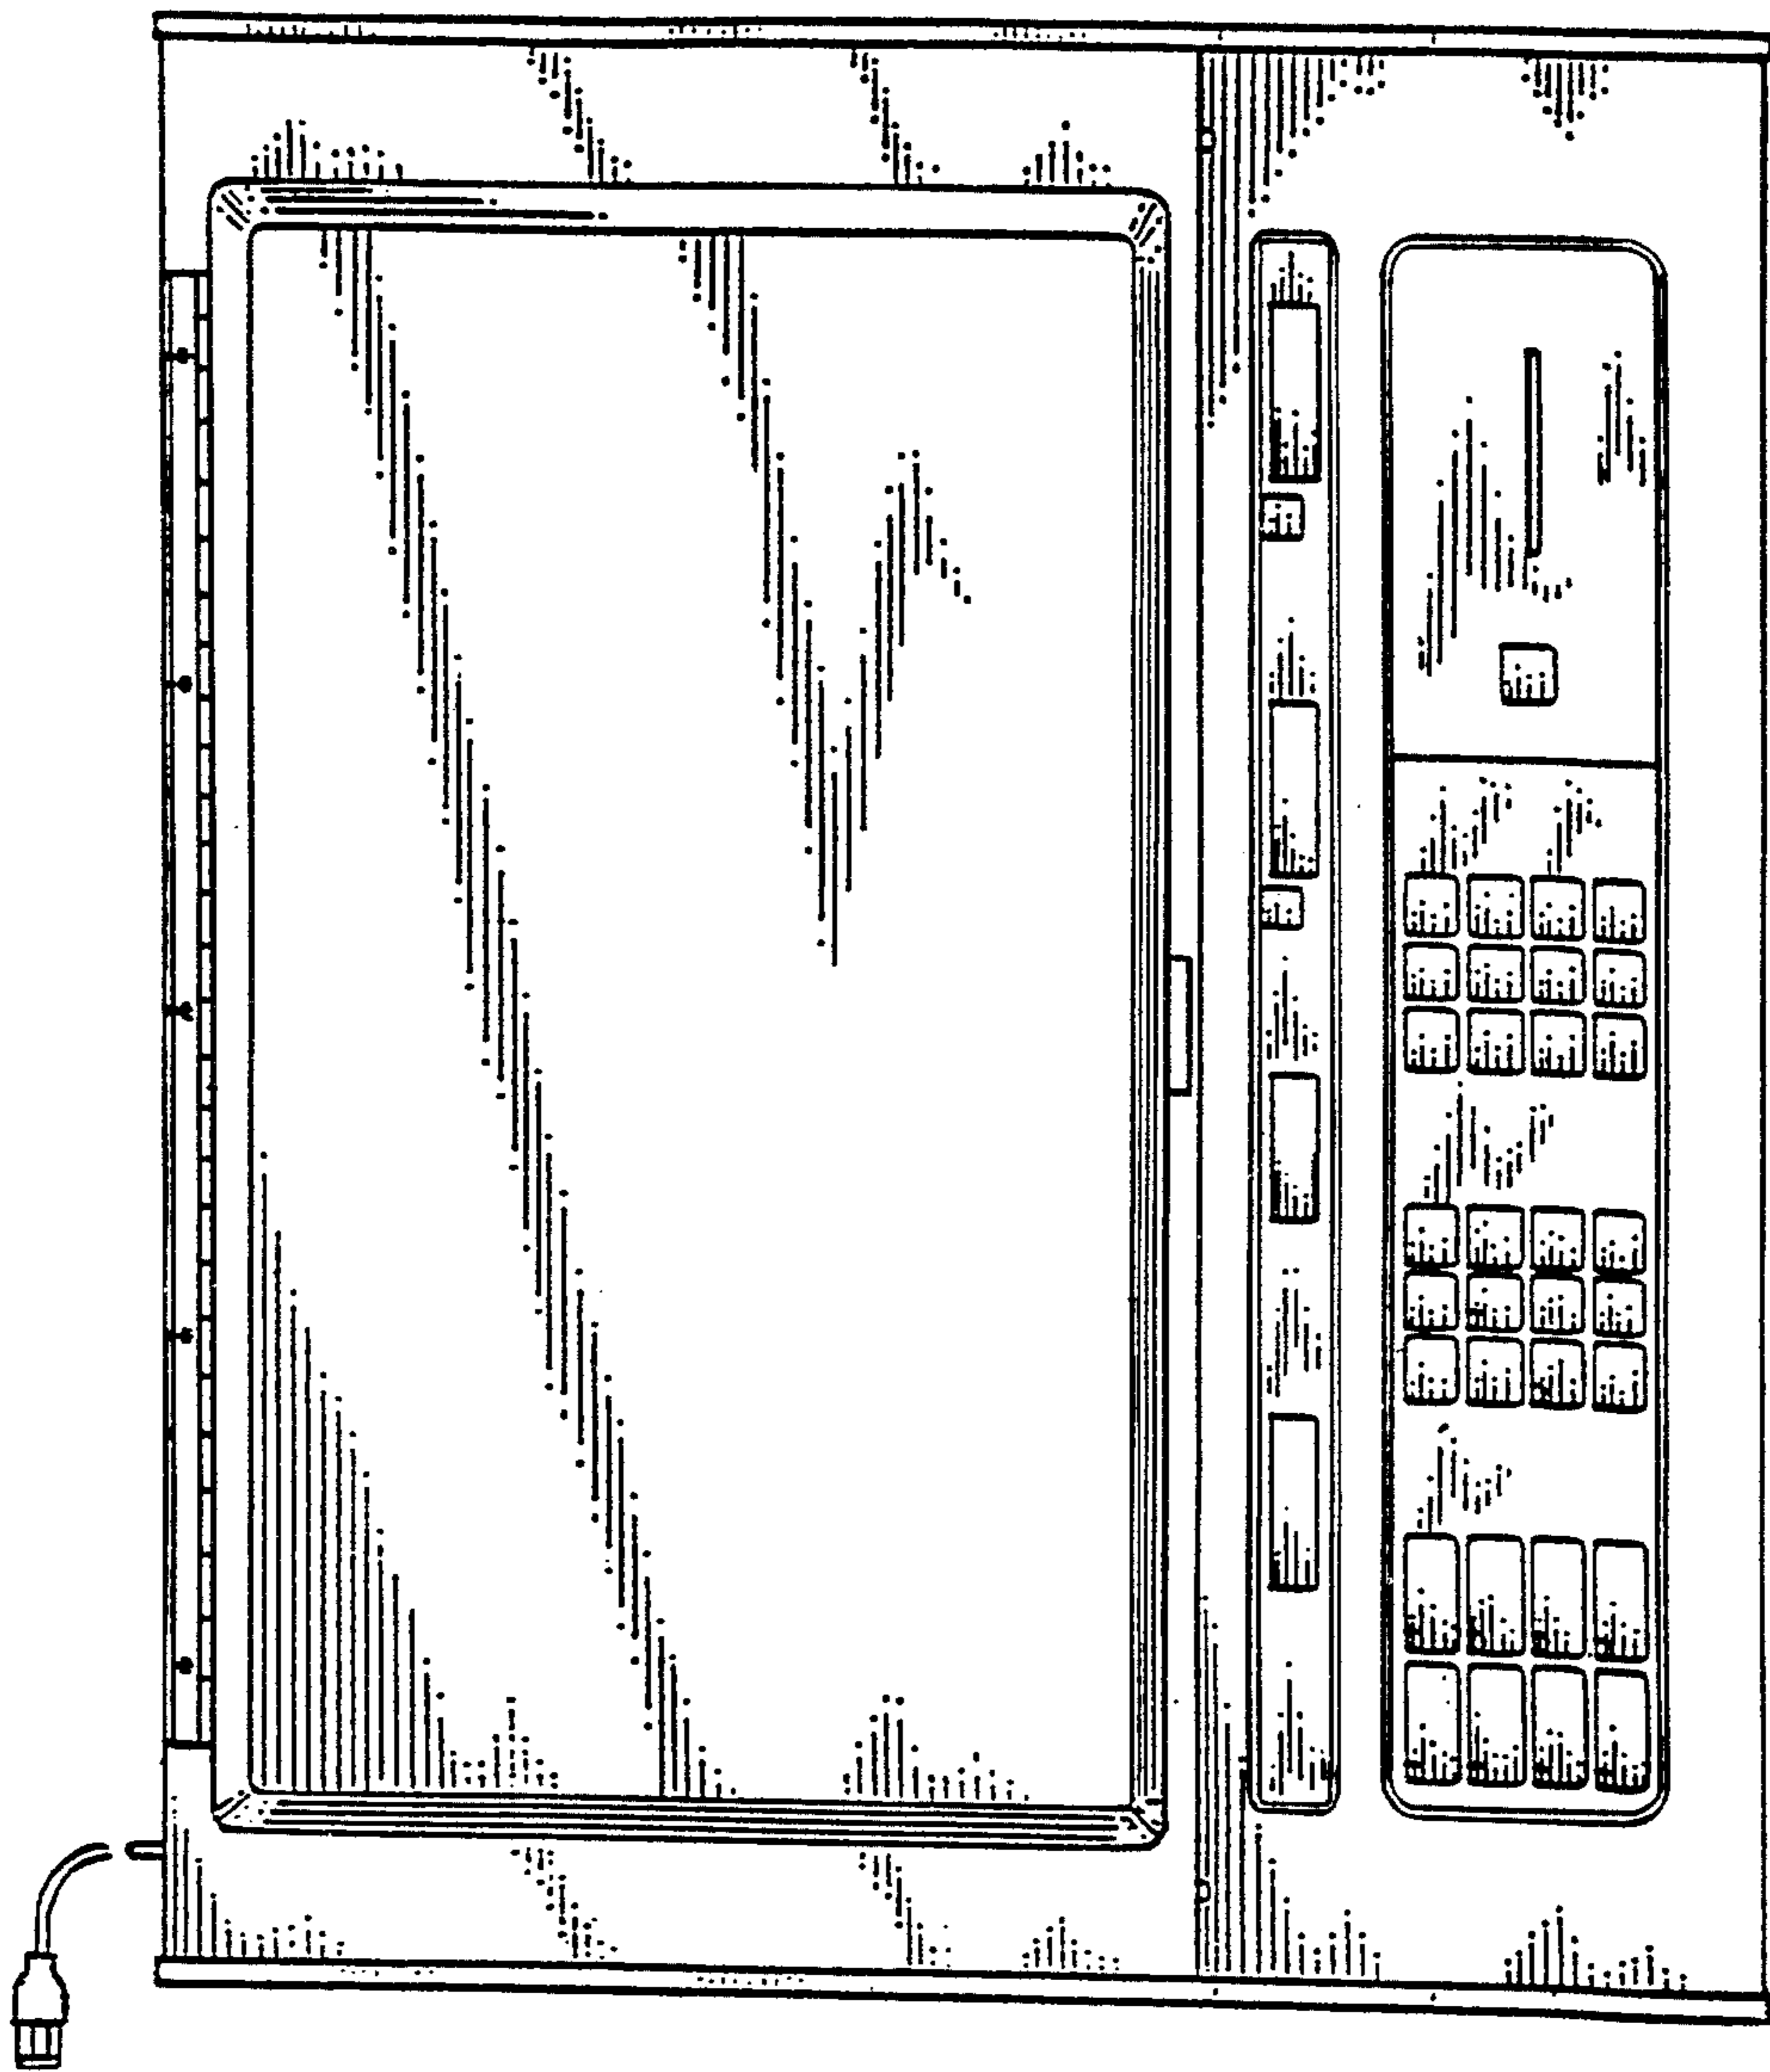


FIG. 1

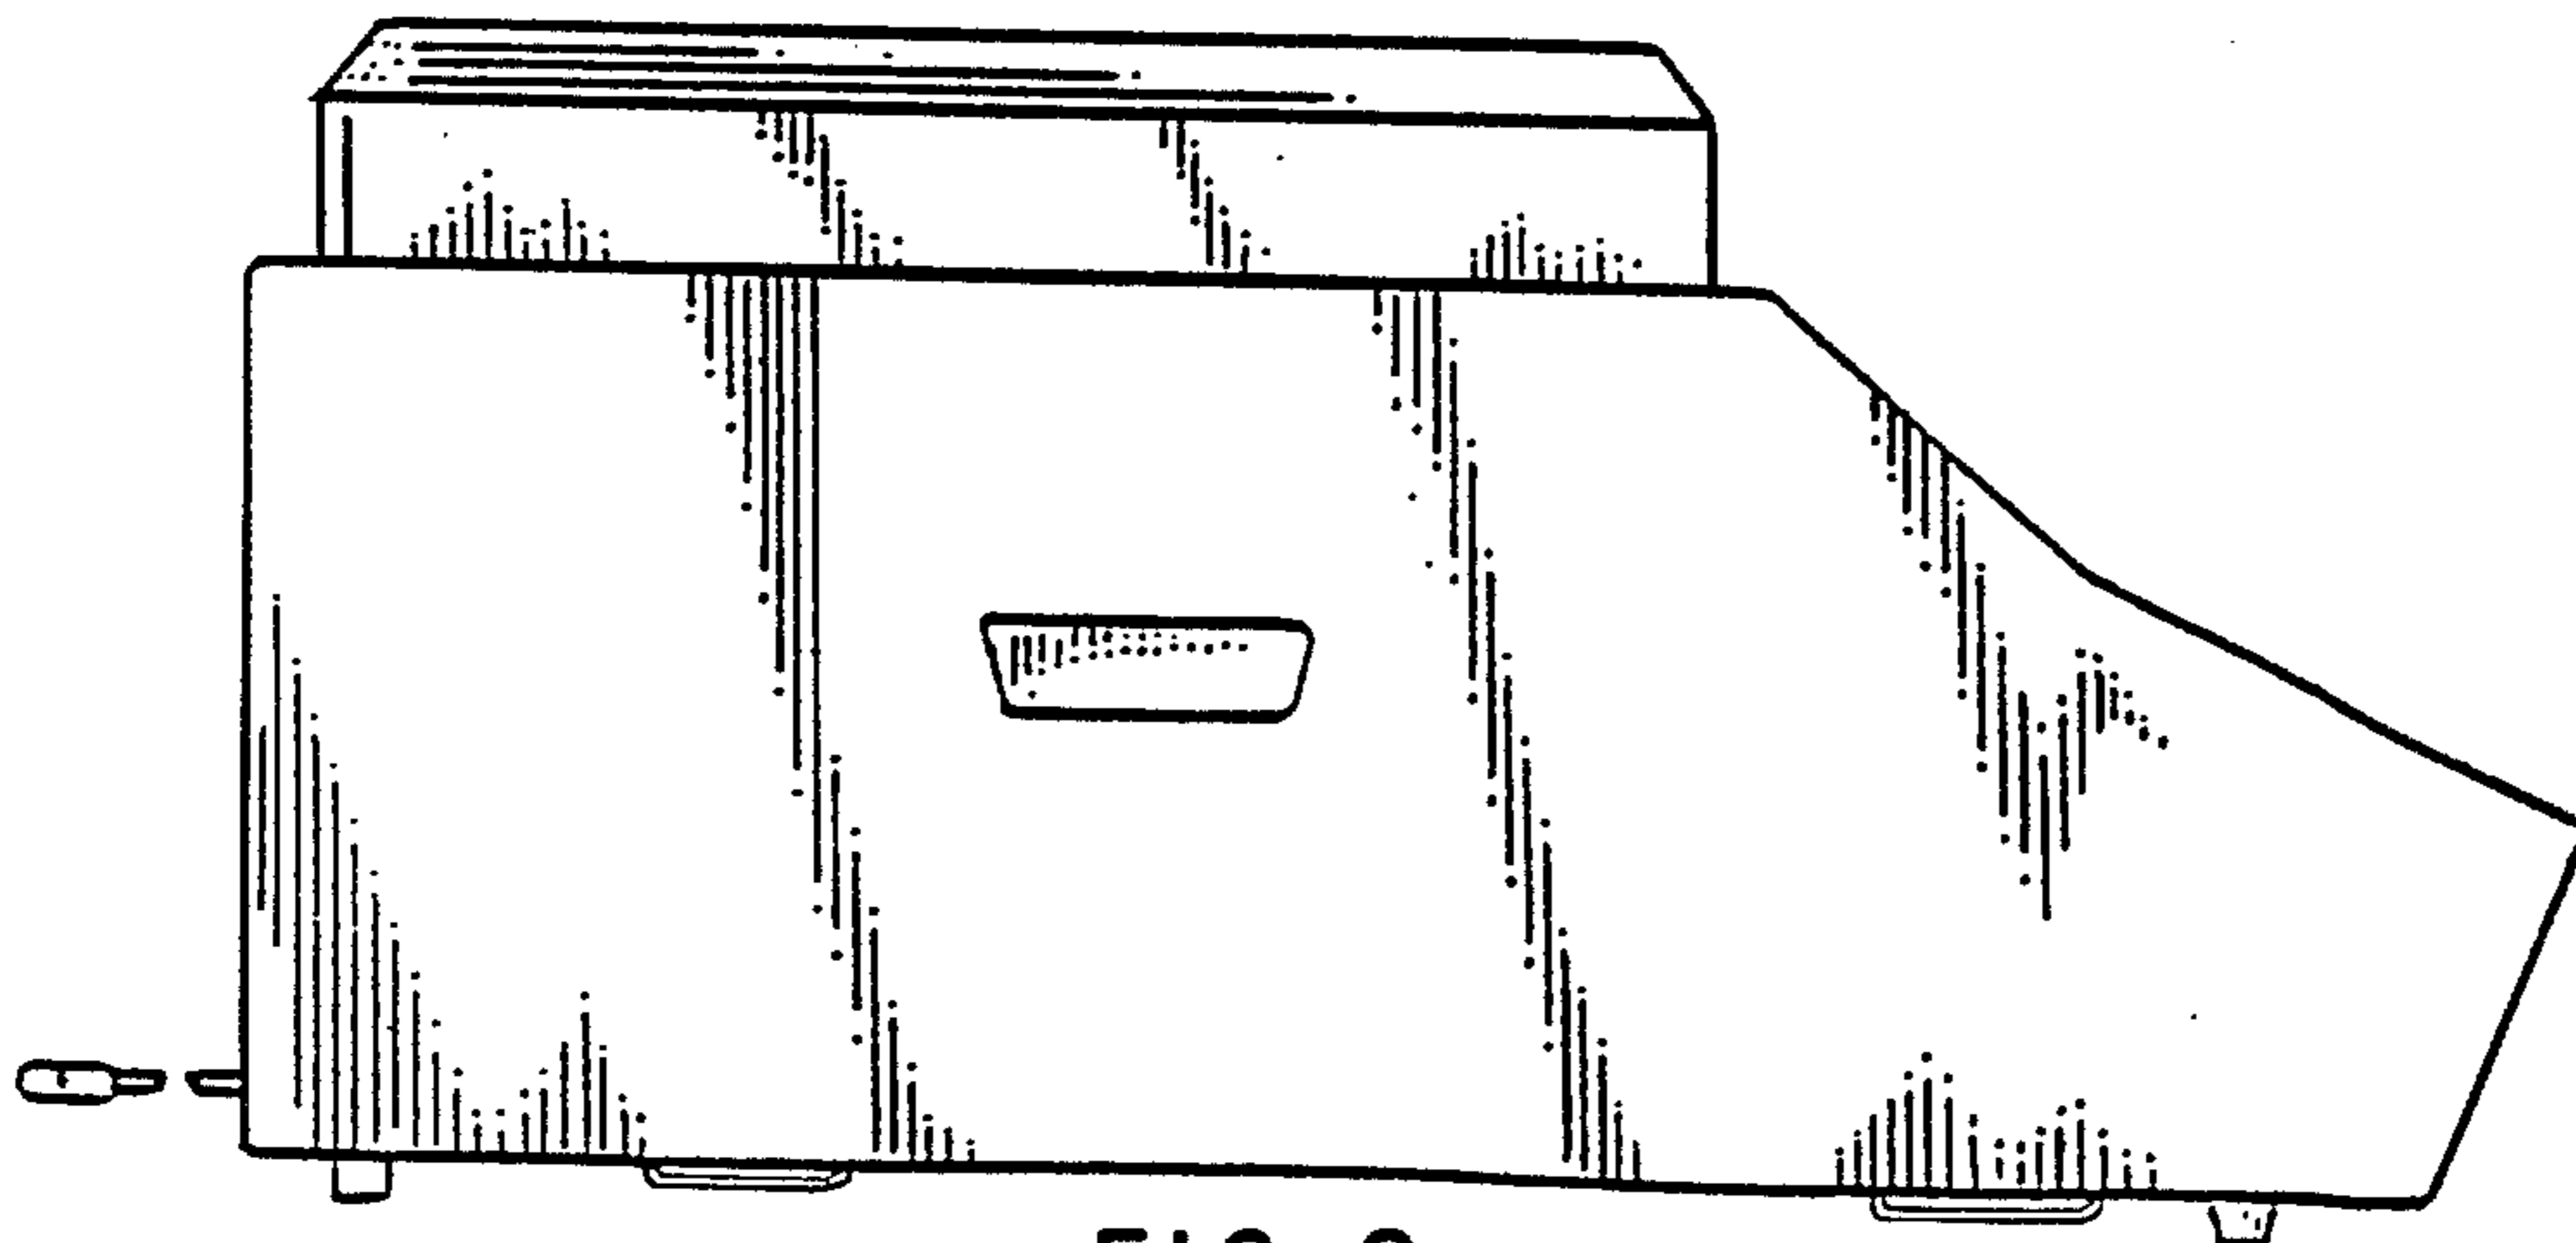


FIG. 2

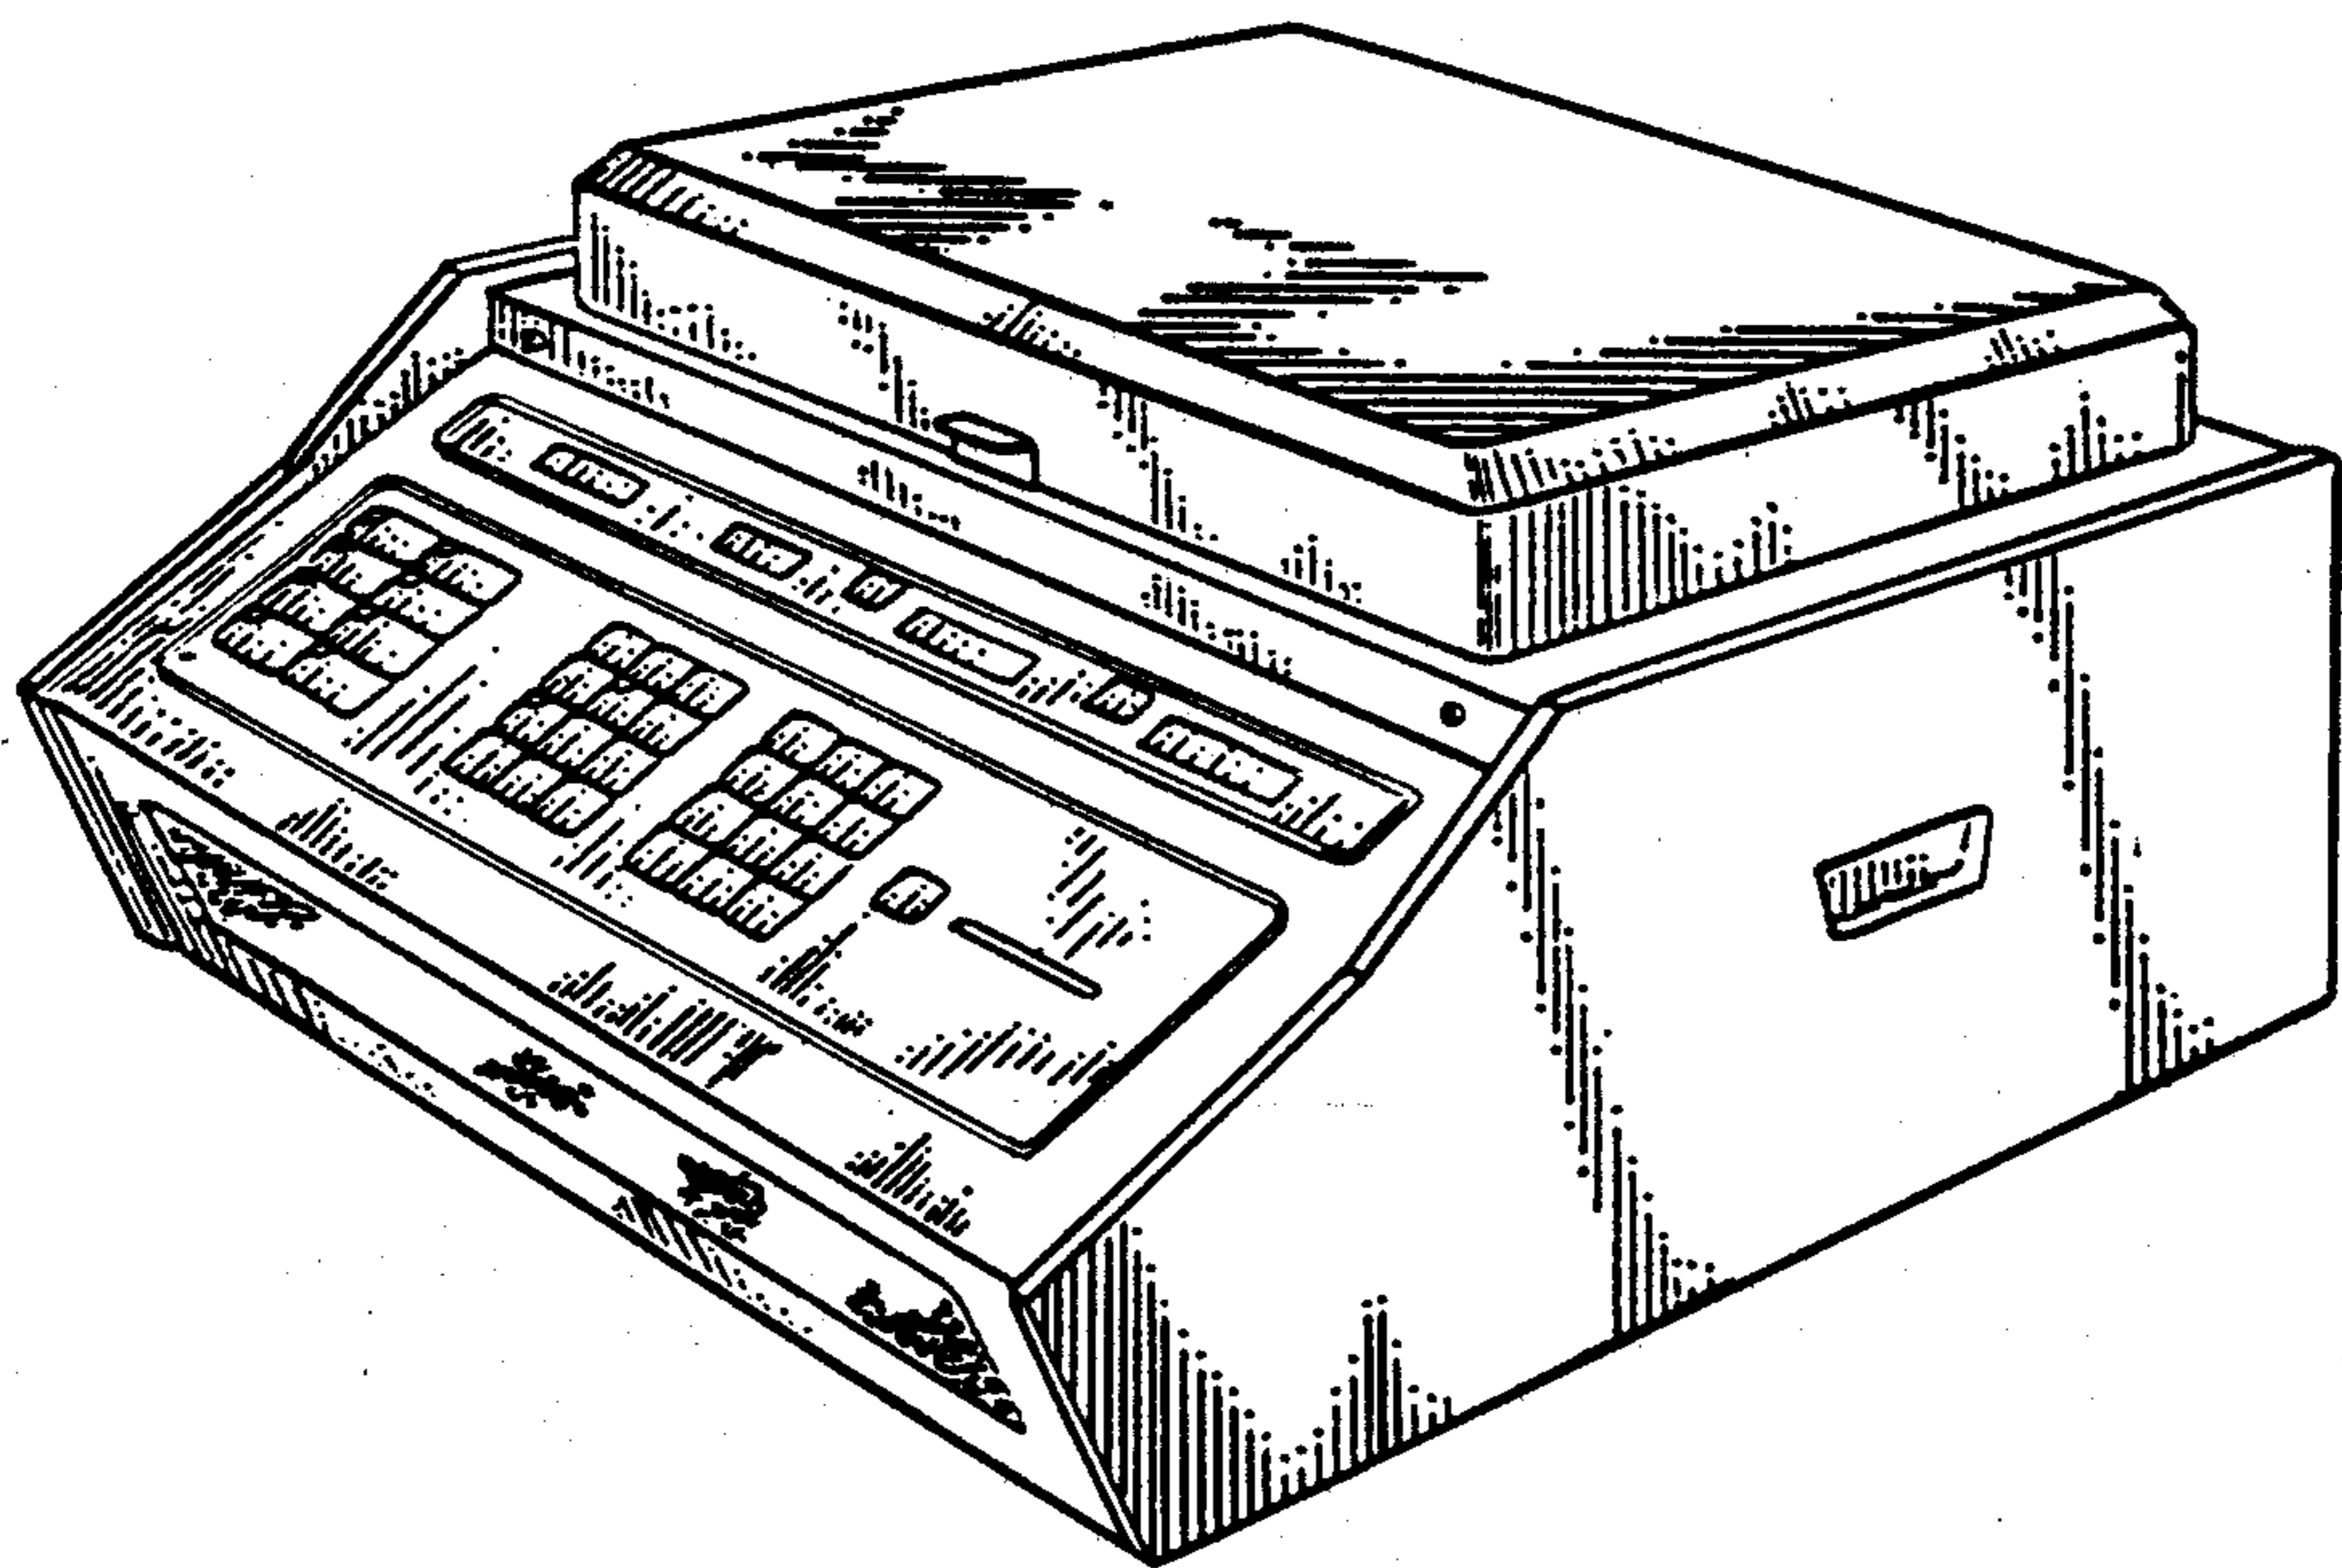


FIG. 3