

[54] ELECTROOPTIC DISPLAY FOR BLOOD PRESSURE DEVICE

[75] Inventor: David W. Eaton, Canton, Conn.

[73] Assignee: Timex Medical Products Corporation, Waterbury, Conn.

[\*\*] Term: 14 Years

[21] Appl. No.: 369,705

[22] Filed: Apr. 19, 1982

[52] U.S. Cl. .... D24/21; D10/57; D10/125; D24/17

[58] Field of Search ..... D24/17, 21; D10/15, D10/30, 33, 37, 57, 96, 52, 60, 123, 125; 128/303.1, 303.19, 900, 672, 667, 689, 721, 680, 672; D18/6, 11, 14, 16, 27, 29, 33; 340/765; 368/72, 82, 239, 10

[56] References Cited

U.S. PATENT DOCUMENTS

- D. 259,408 6/1981 Wright et al. .... D10/125
- 4,026,103 5/1977 Ichikawa et al. .... 368/239
- 4,188,776 2/1980 Scherrer ..... 368/70

OTHER PUBLICATIONS

Henry Dreyfus Symbol Sourcebook, An Authoritative Guide to International Graphic Symbols ©1972 by Henry Dreyfuss, McGraw-Hill.

Primary Examiner—A. Hugo Word  
Assistant Examiner—Ruth C. Anderson  
Attorney, Agent, or Firm—William C. Crutcher

[57] CLAIM

The ornamental design for an electrooptic display for blood pressure device, as shown and described.

DESCRIPTION


FIG. 1 is a top plan view of an electrooptic display for blood pressure device showing my new design in an unenergized condition.

FIG. 2 is a front elevational view thereof;

FIG. 3 is a right side elevation view thereof, the left side being a substantially mirror image thereof;

FIG. 4 is a bottom plan view thereof; and

FIG. 5 is a top plan view thereof, in a representative energized condition displaying blood pressure as 120/80 and displaying a "cuff deflate" symbol.

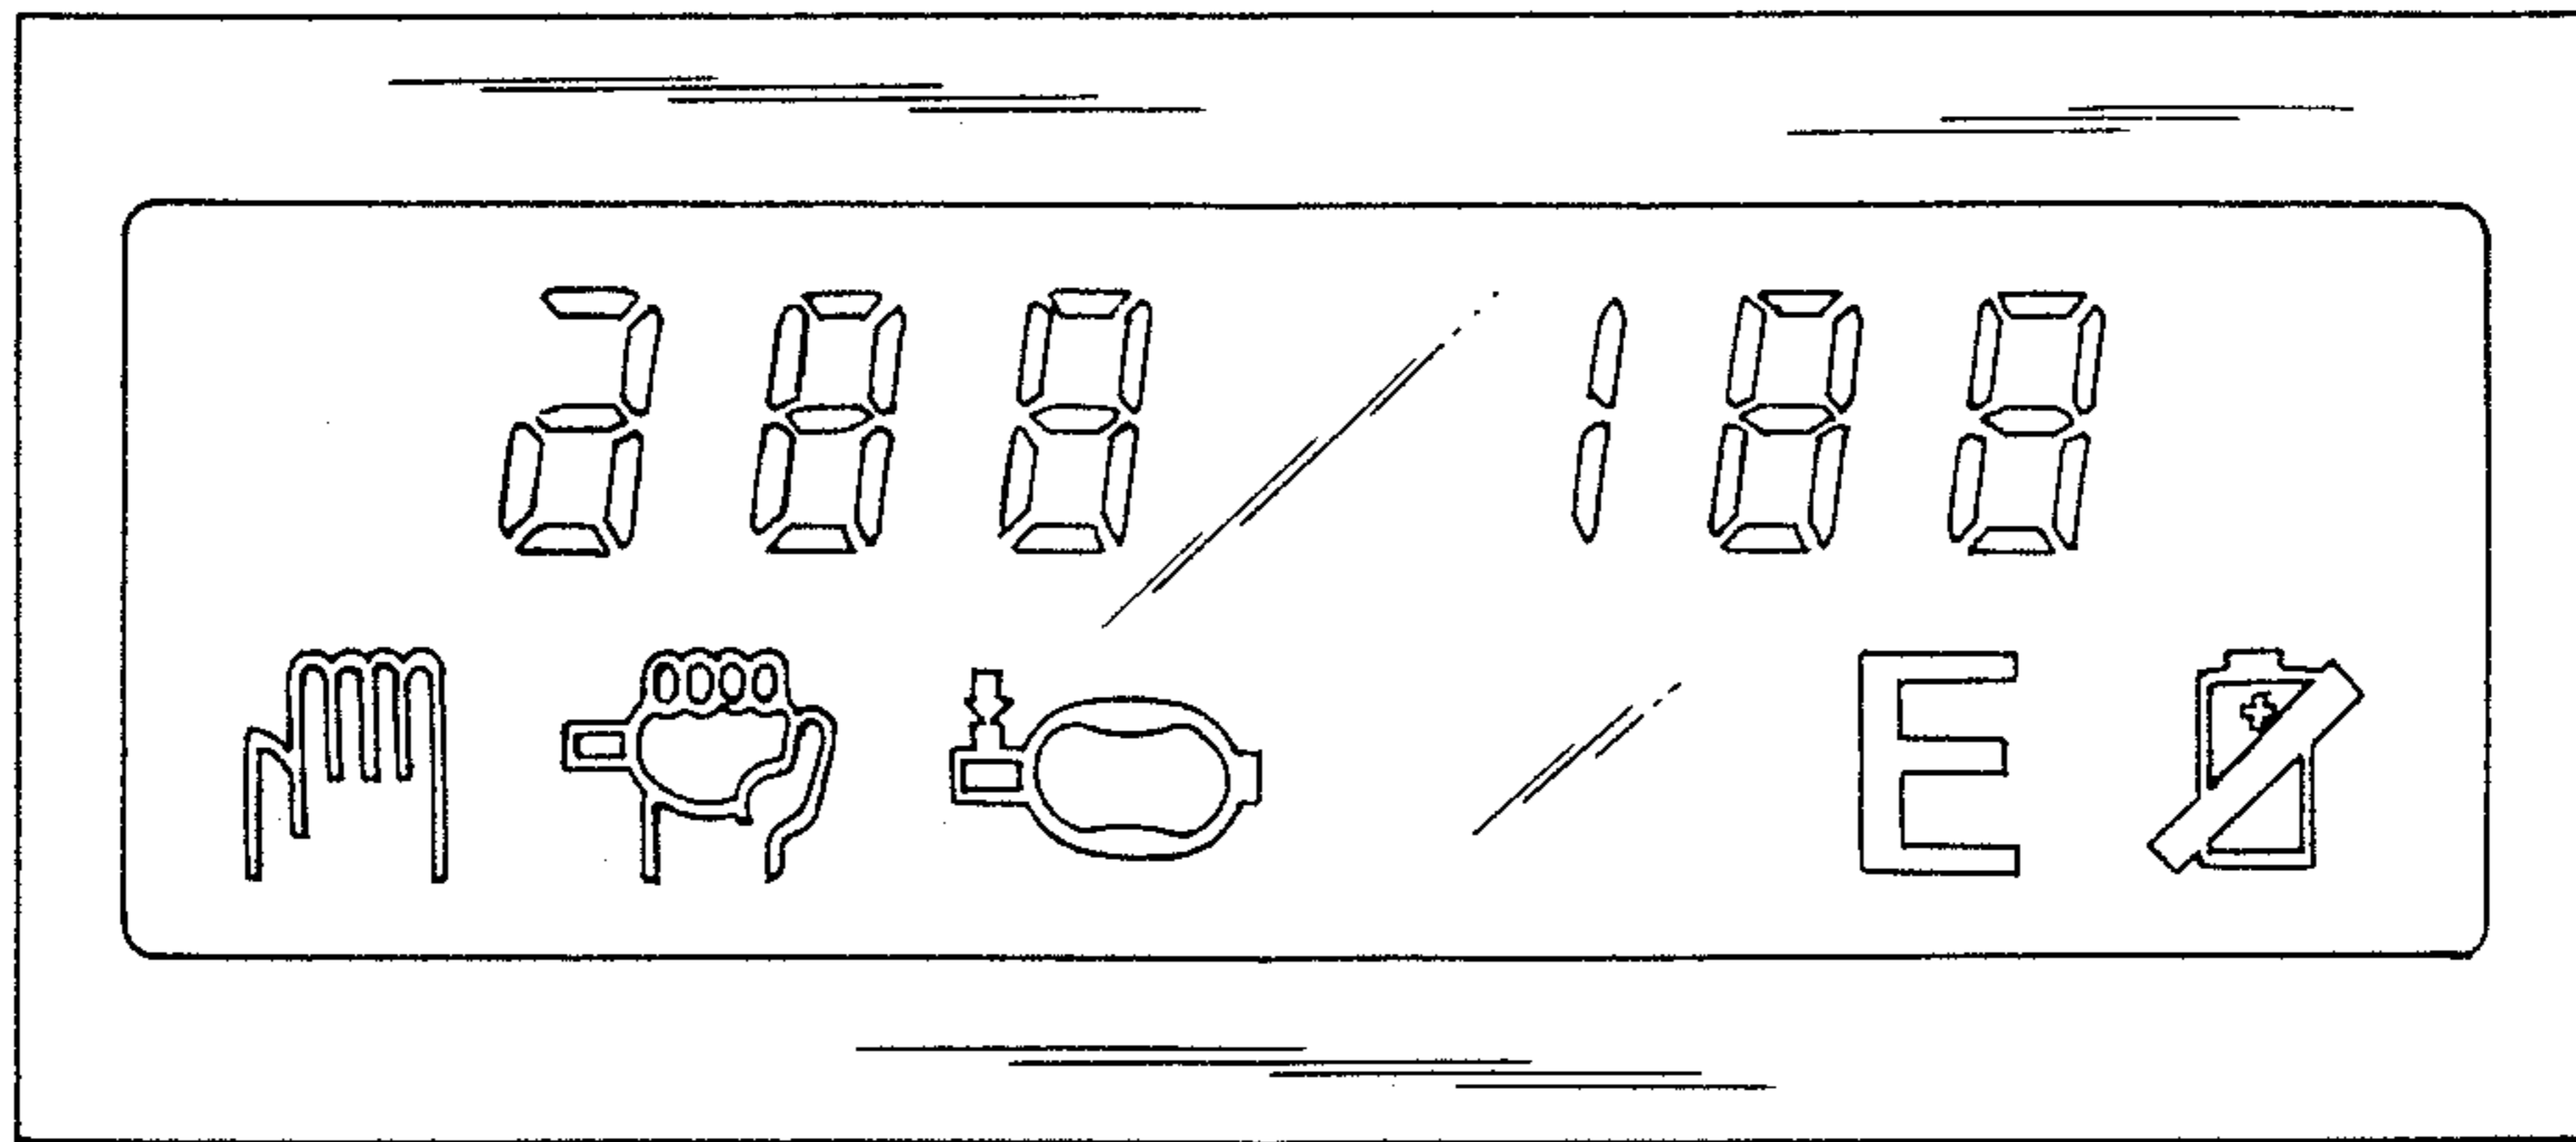

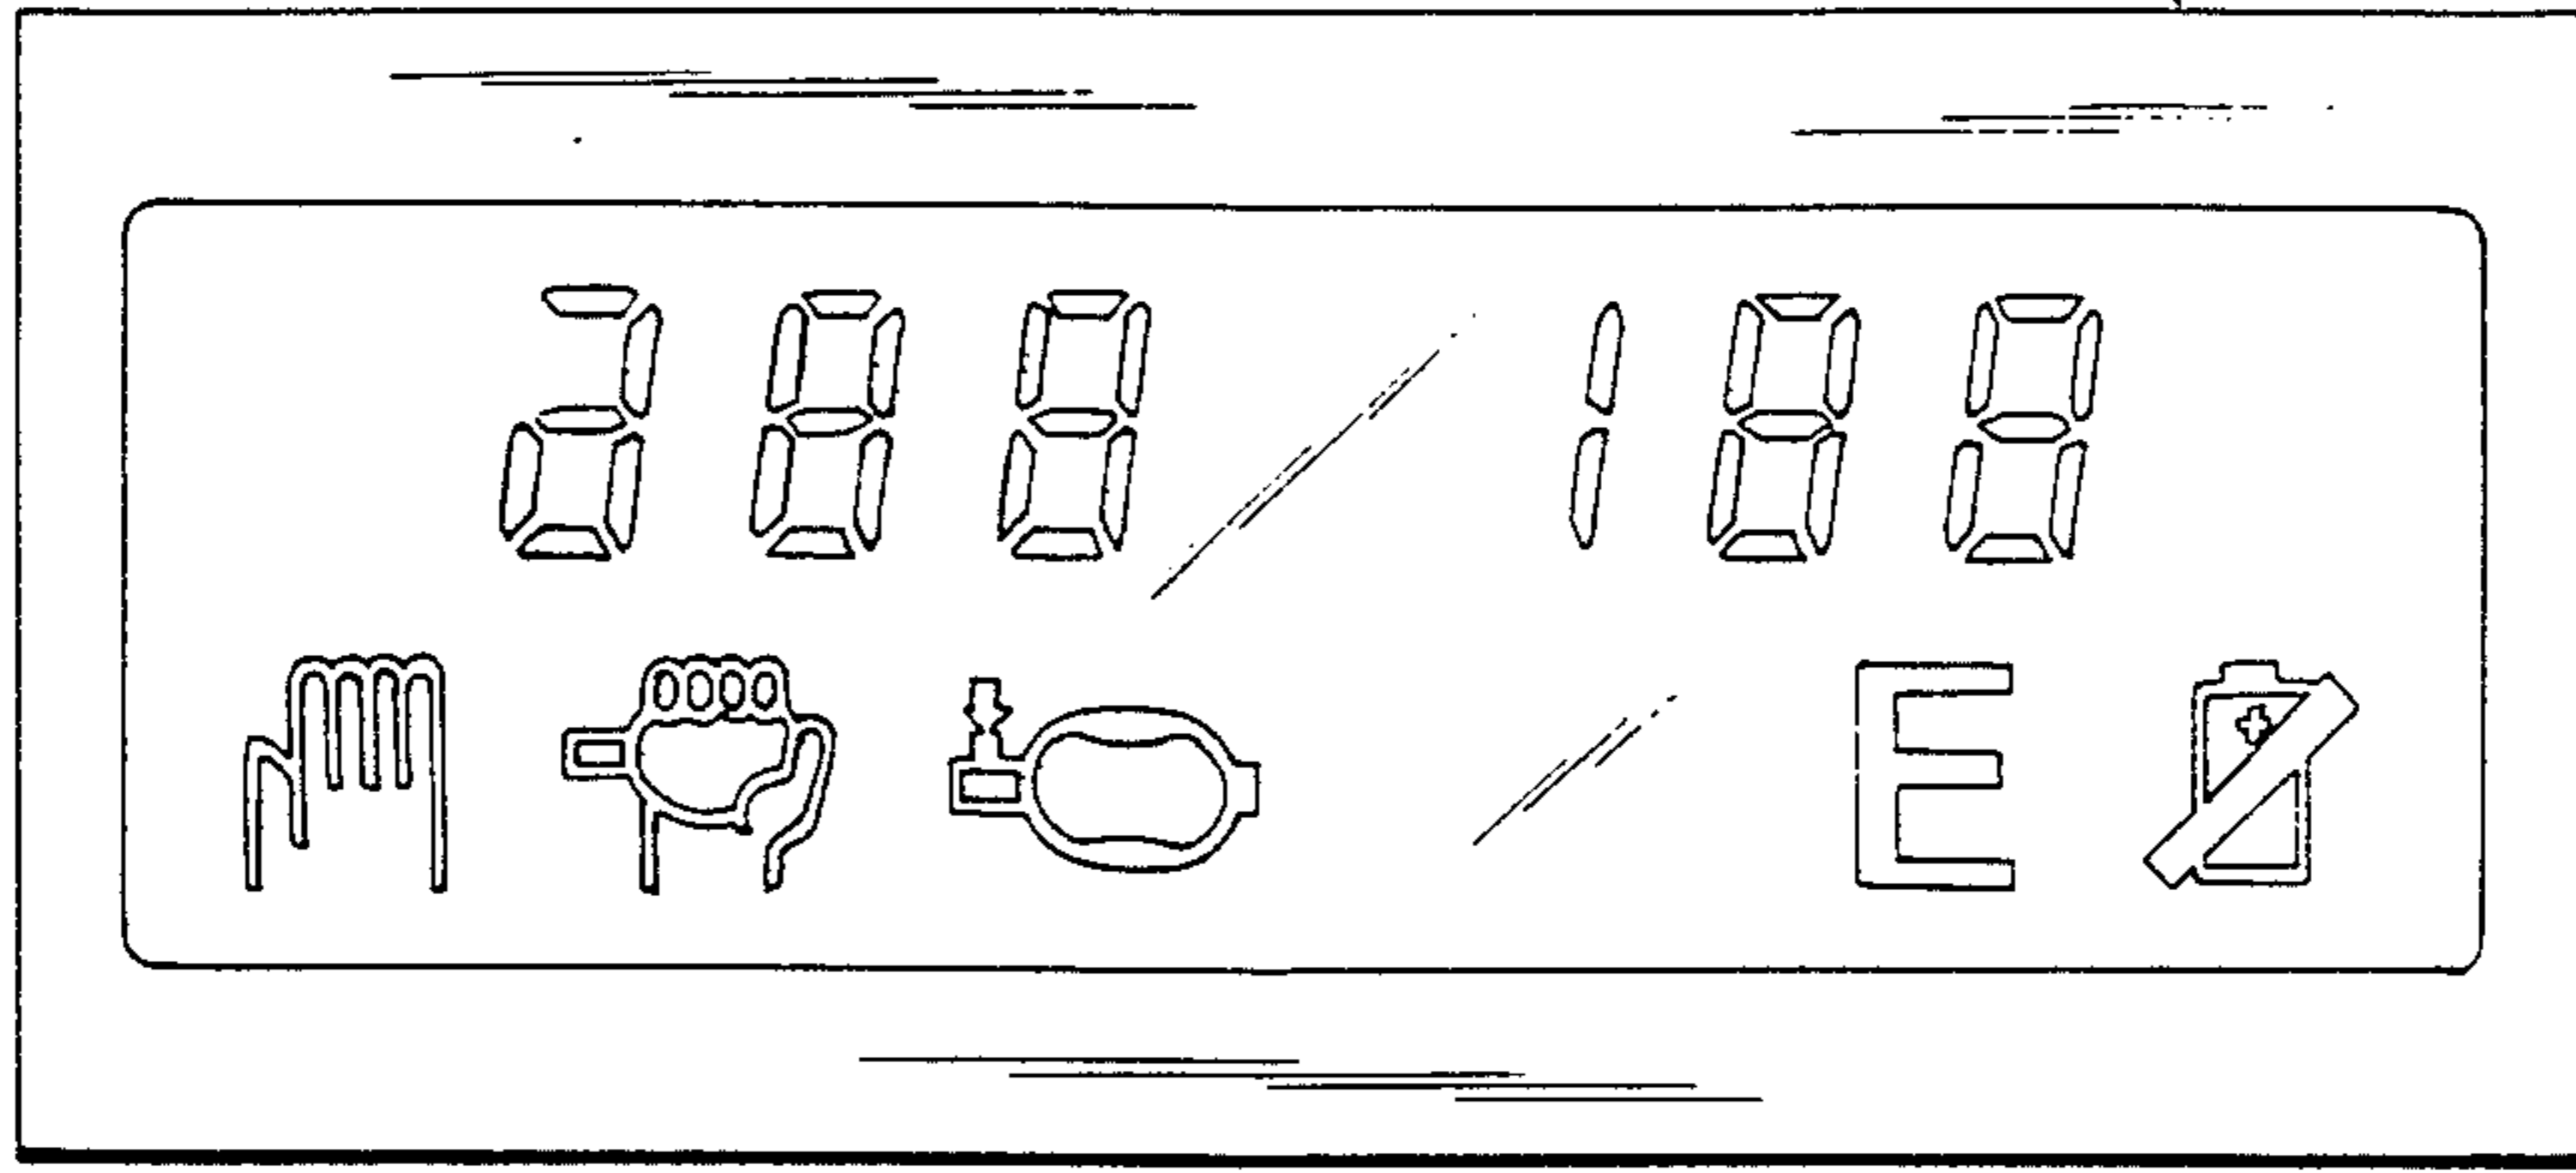


FIG. 1

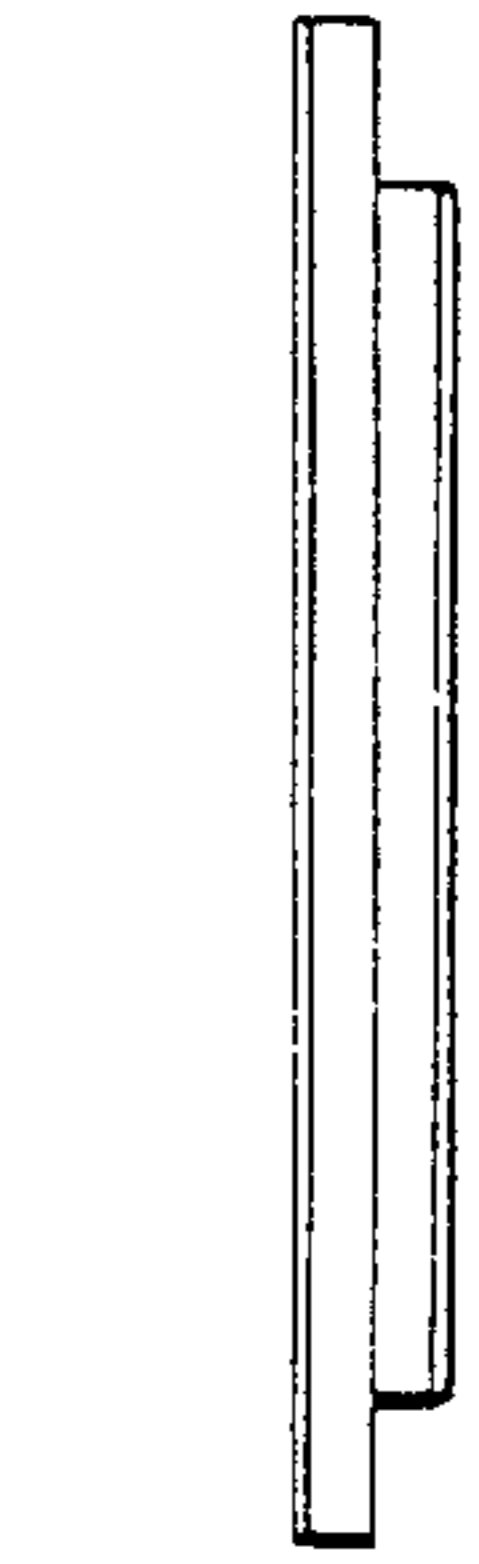


FIG. 3

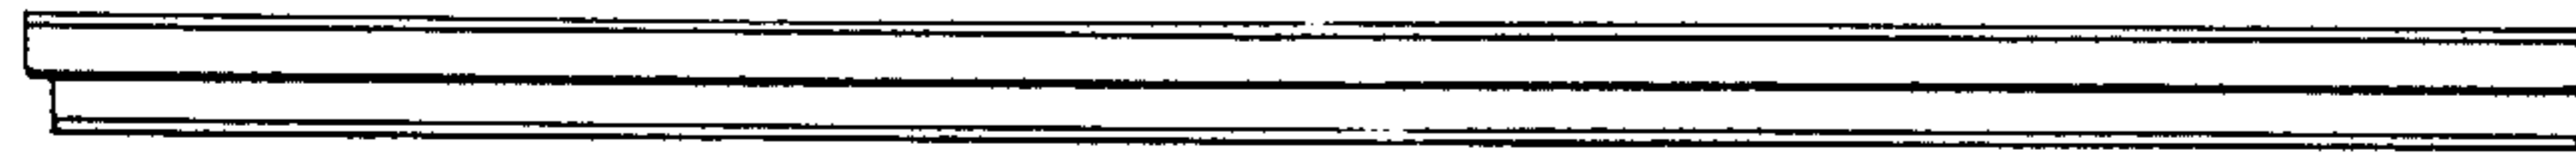


FIG. 2

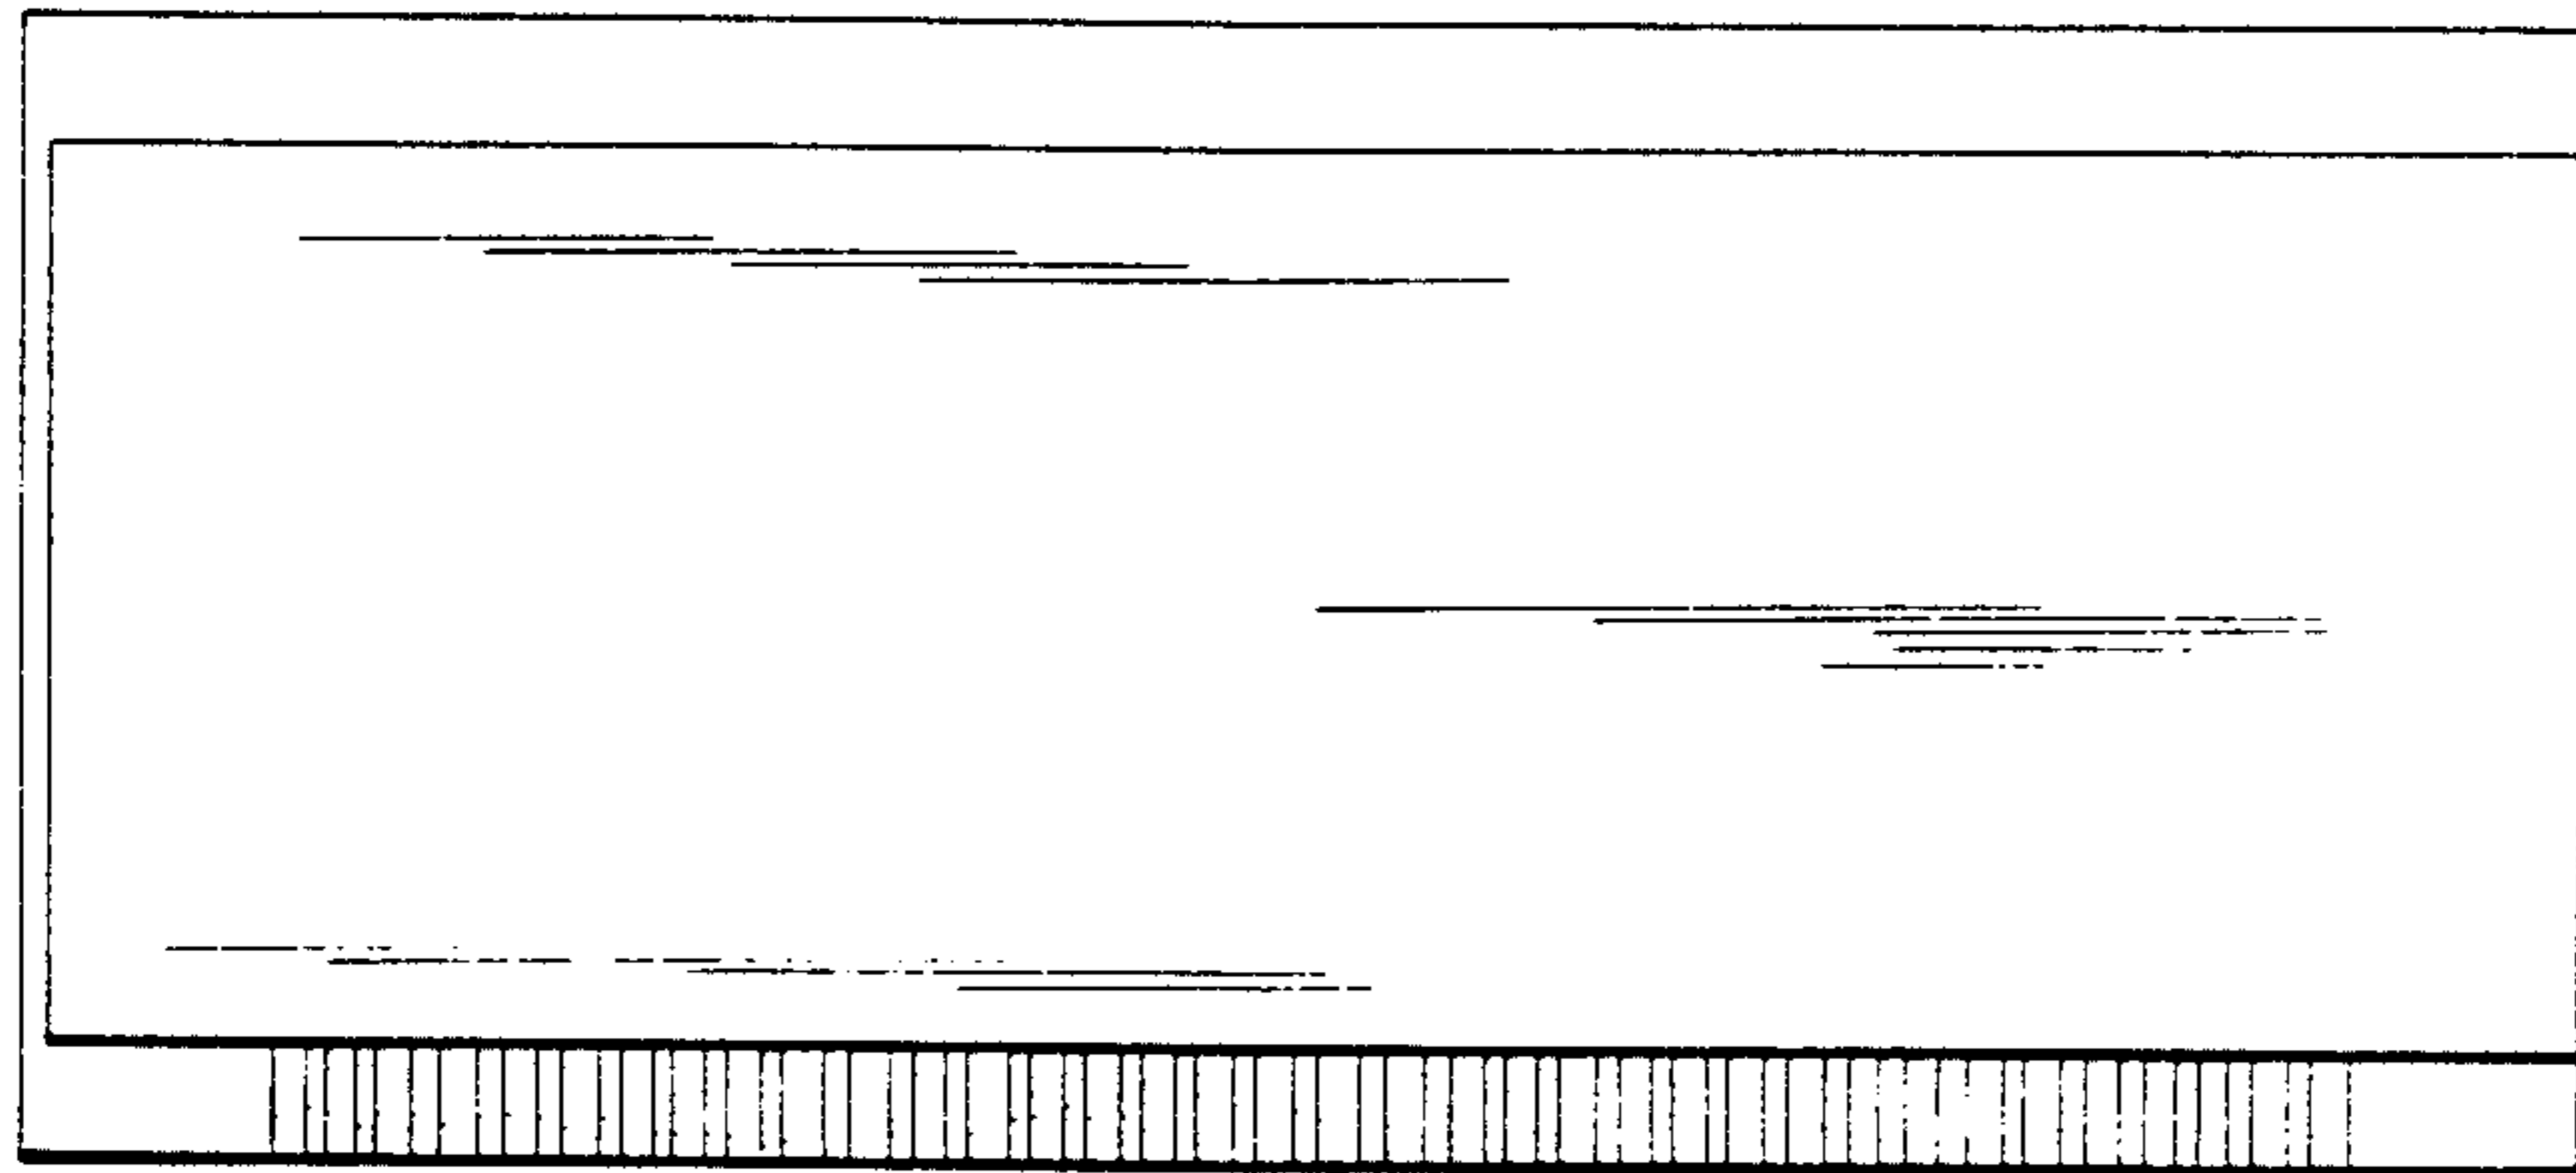


FIG. 4

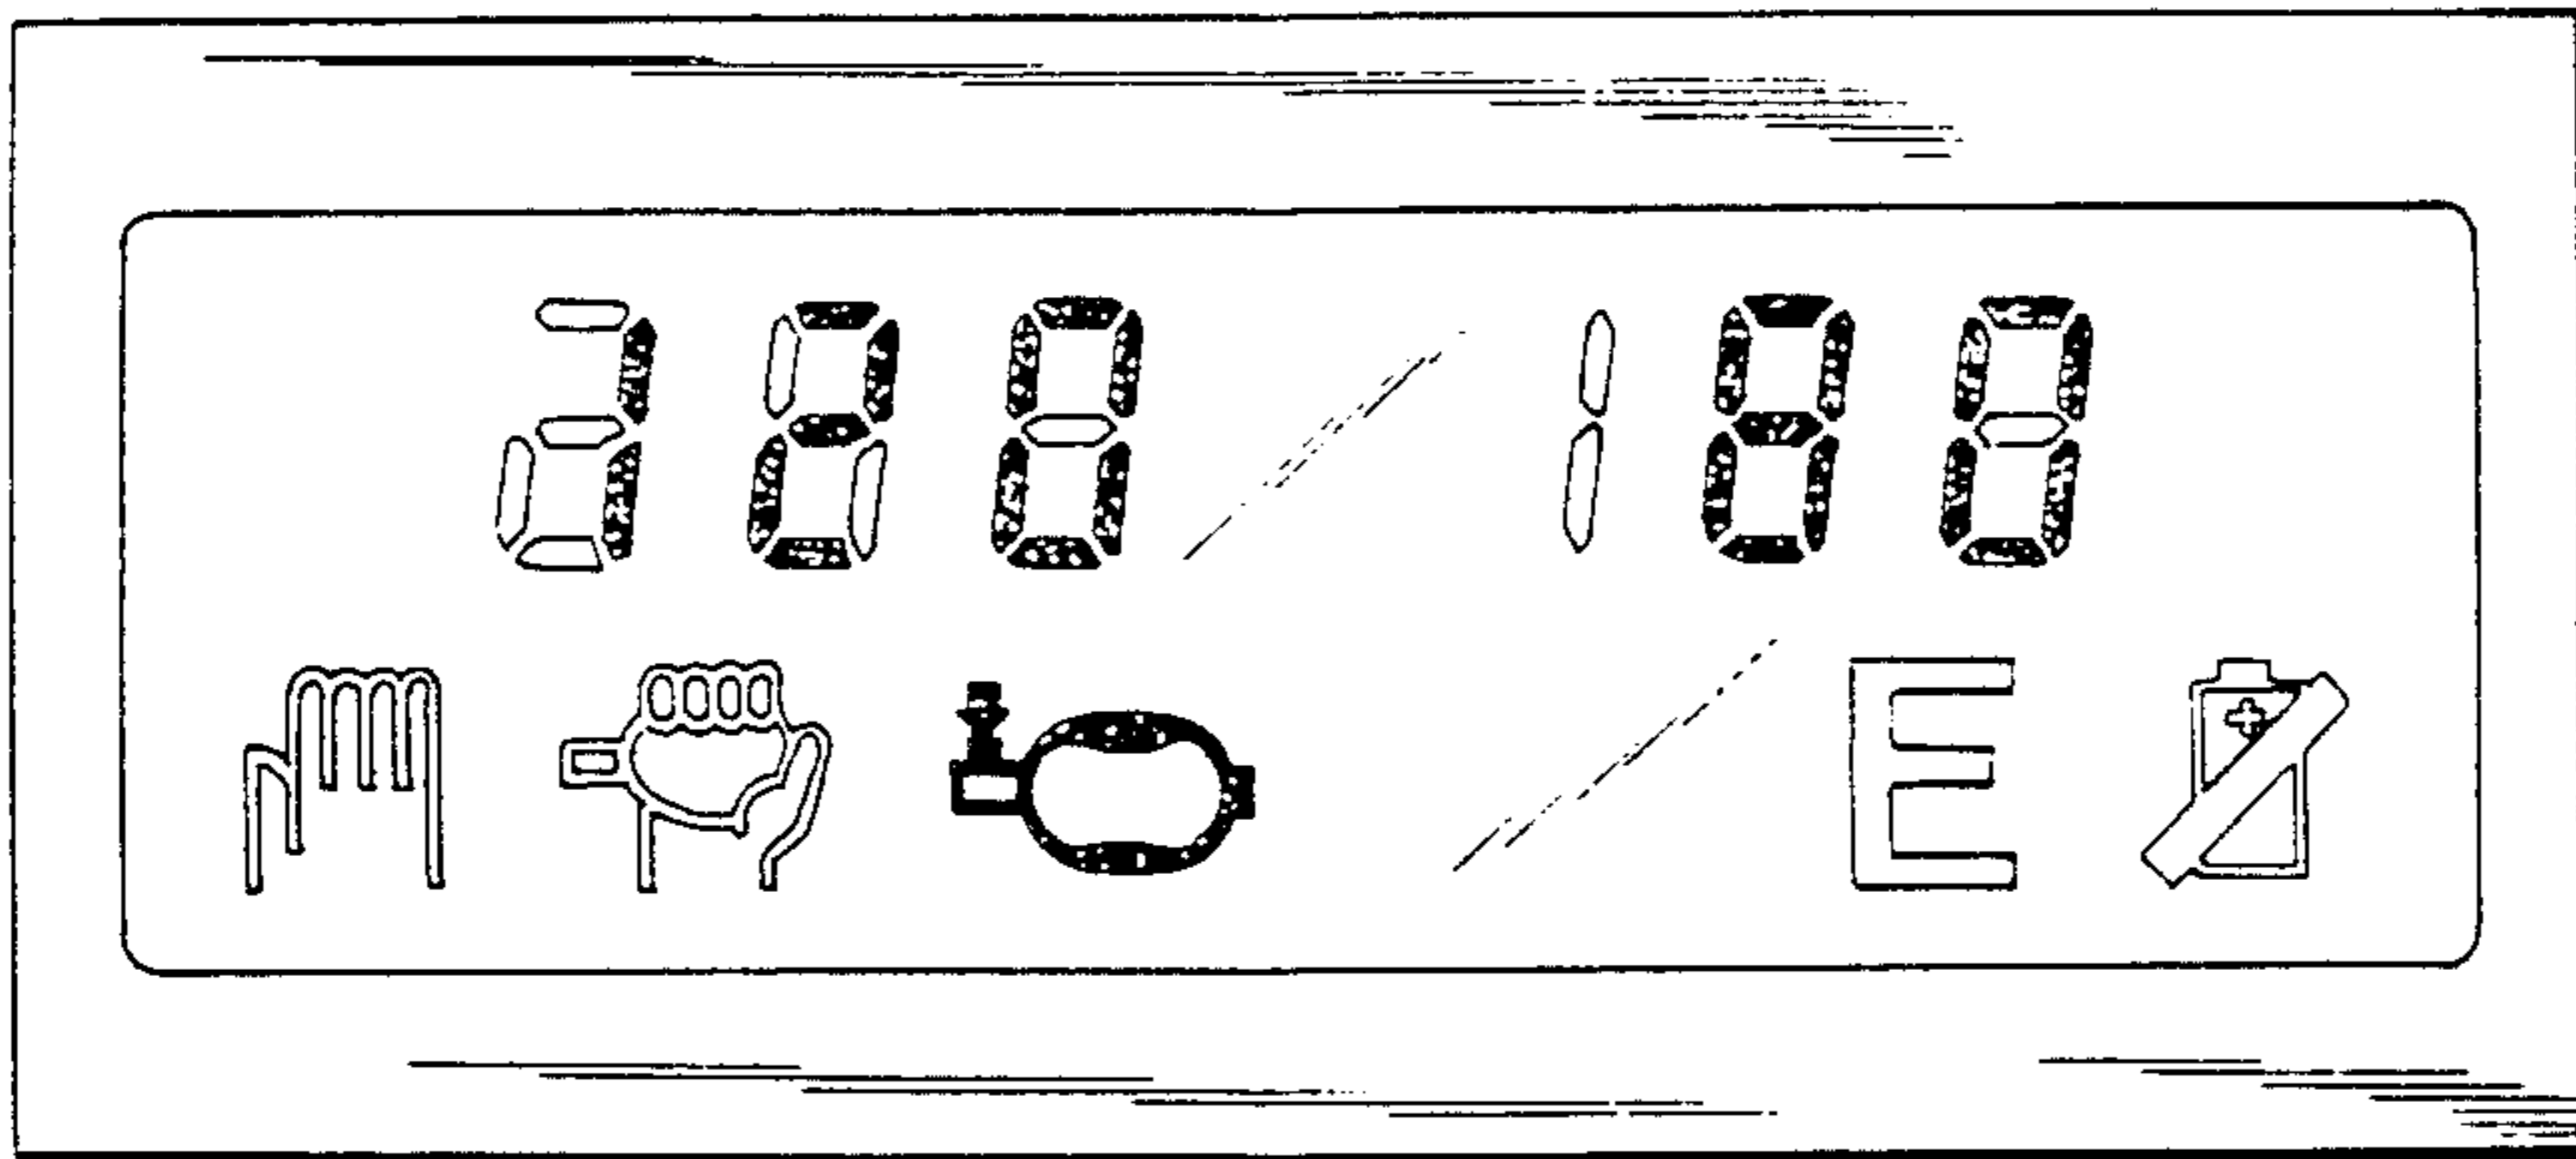


FIG. 5