

[54] SURGICAL TEMPERATURE MONITOR AND ALARM SYSTEM

[75] Inventors: Allen L. Van Beek, Minneapolis; Alfred L. Iversen, Minnetonka, both of Minn.

[73] Assignee: PMT Inc., Hopkins, Minn.

[\*\*] Term: 14 Years

[21] Appl. No.: 418,805

[22] Filed: Sep. 16, 1982

[52] U.S. Cl. .... D10/53; D10/57 X; D24/17 X

[58] Field of Search ..... D10/52, 53, 57, 60, D10/102, 103, 75, 78, 81; D24/8, 17, 21; 128/736; 374/163, 170, 183, 185

[56] References Cited

U.S. PATENT DOCUMENTS

- D. 251,370 3/1979 Katzman ..... D10/78 X
- D. 269,372 6/1983 Reis ..... D24/17
- 3,187,576 6/1965 Beeston ..... D24/17 X

- 3,289,671 12/1966 Troutman ..... D24/17 X
- 3,531,642 9/1970 Barnes ..... 128/736 X
- 3,651,694 3/1972 Lamb ..... 374/170 X
- 4,276,888 7/1981 Smith ..... 128/736 X
- 4,321,933 3/1982 Baessler ..... 128/736

OTHER PUBLICATIONS

*Electronic Design Gold Book*—Sec. 4200—vol. 3, p. 624—Multipoints With Unit For Dibitac Therm.


Primary Examiner—Nelson C. Holtje  
Attorney, Agent, or Firm—Hugh D. Jaeger

[57] CLAIM

The ornamental design for a surgical temperature monitor and alarm system, as shown.

DESCRIPTION

FIG. 1 is a front elevational view of a surgical temperature monitor and alarm system showing our new design; FIG. 2 is a top plan view thereof; FIG. 3 is a rear elevational view thereof; FIG. 4 is a bottom plan view thereof; FIG. 5 is a left side elevational view thereof; FIG. 6 is a right side elevational view thereof.

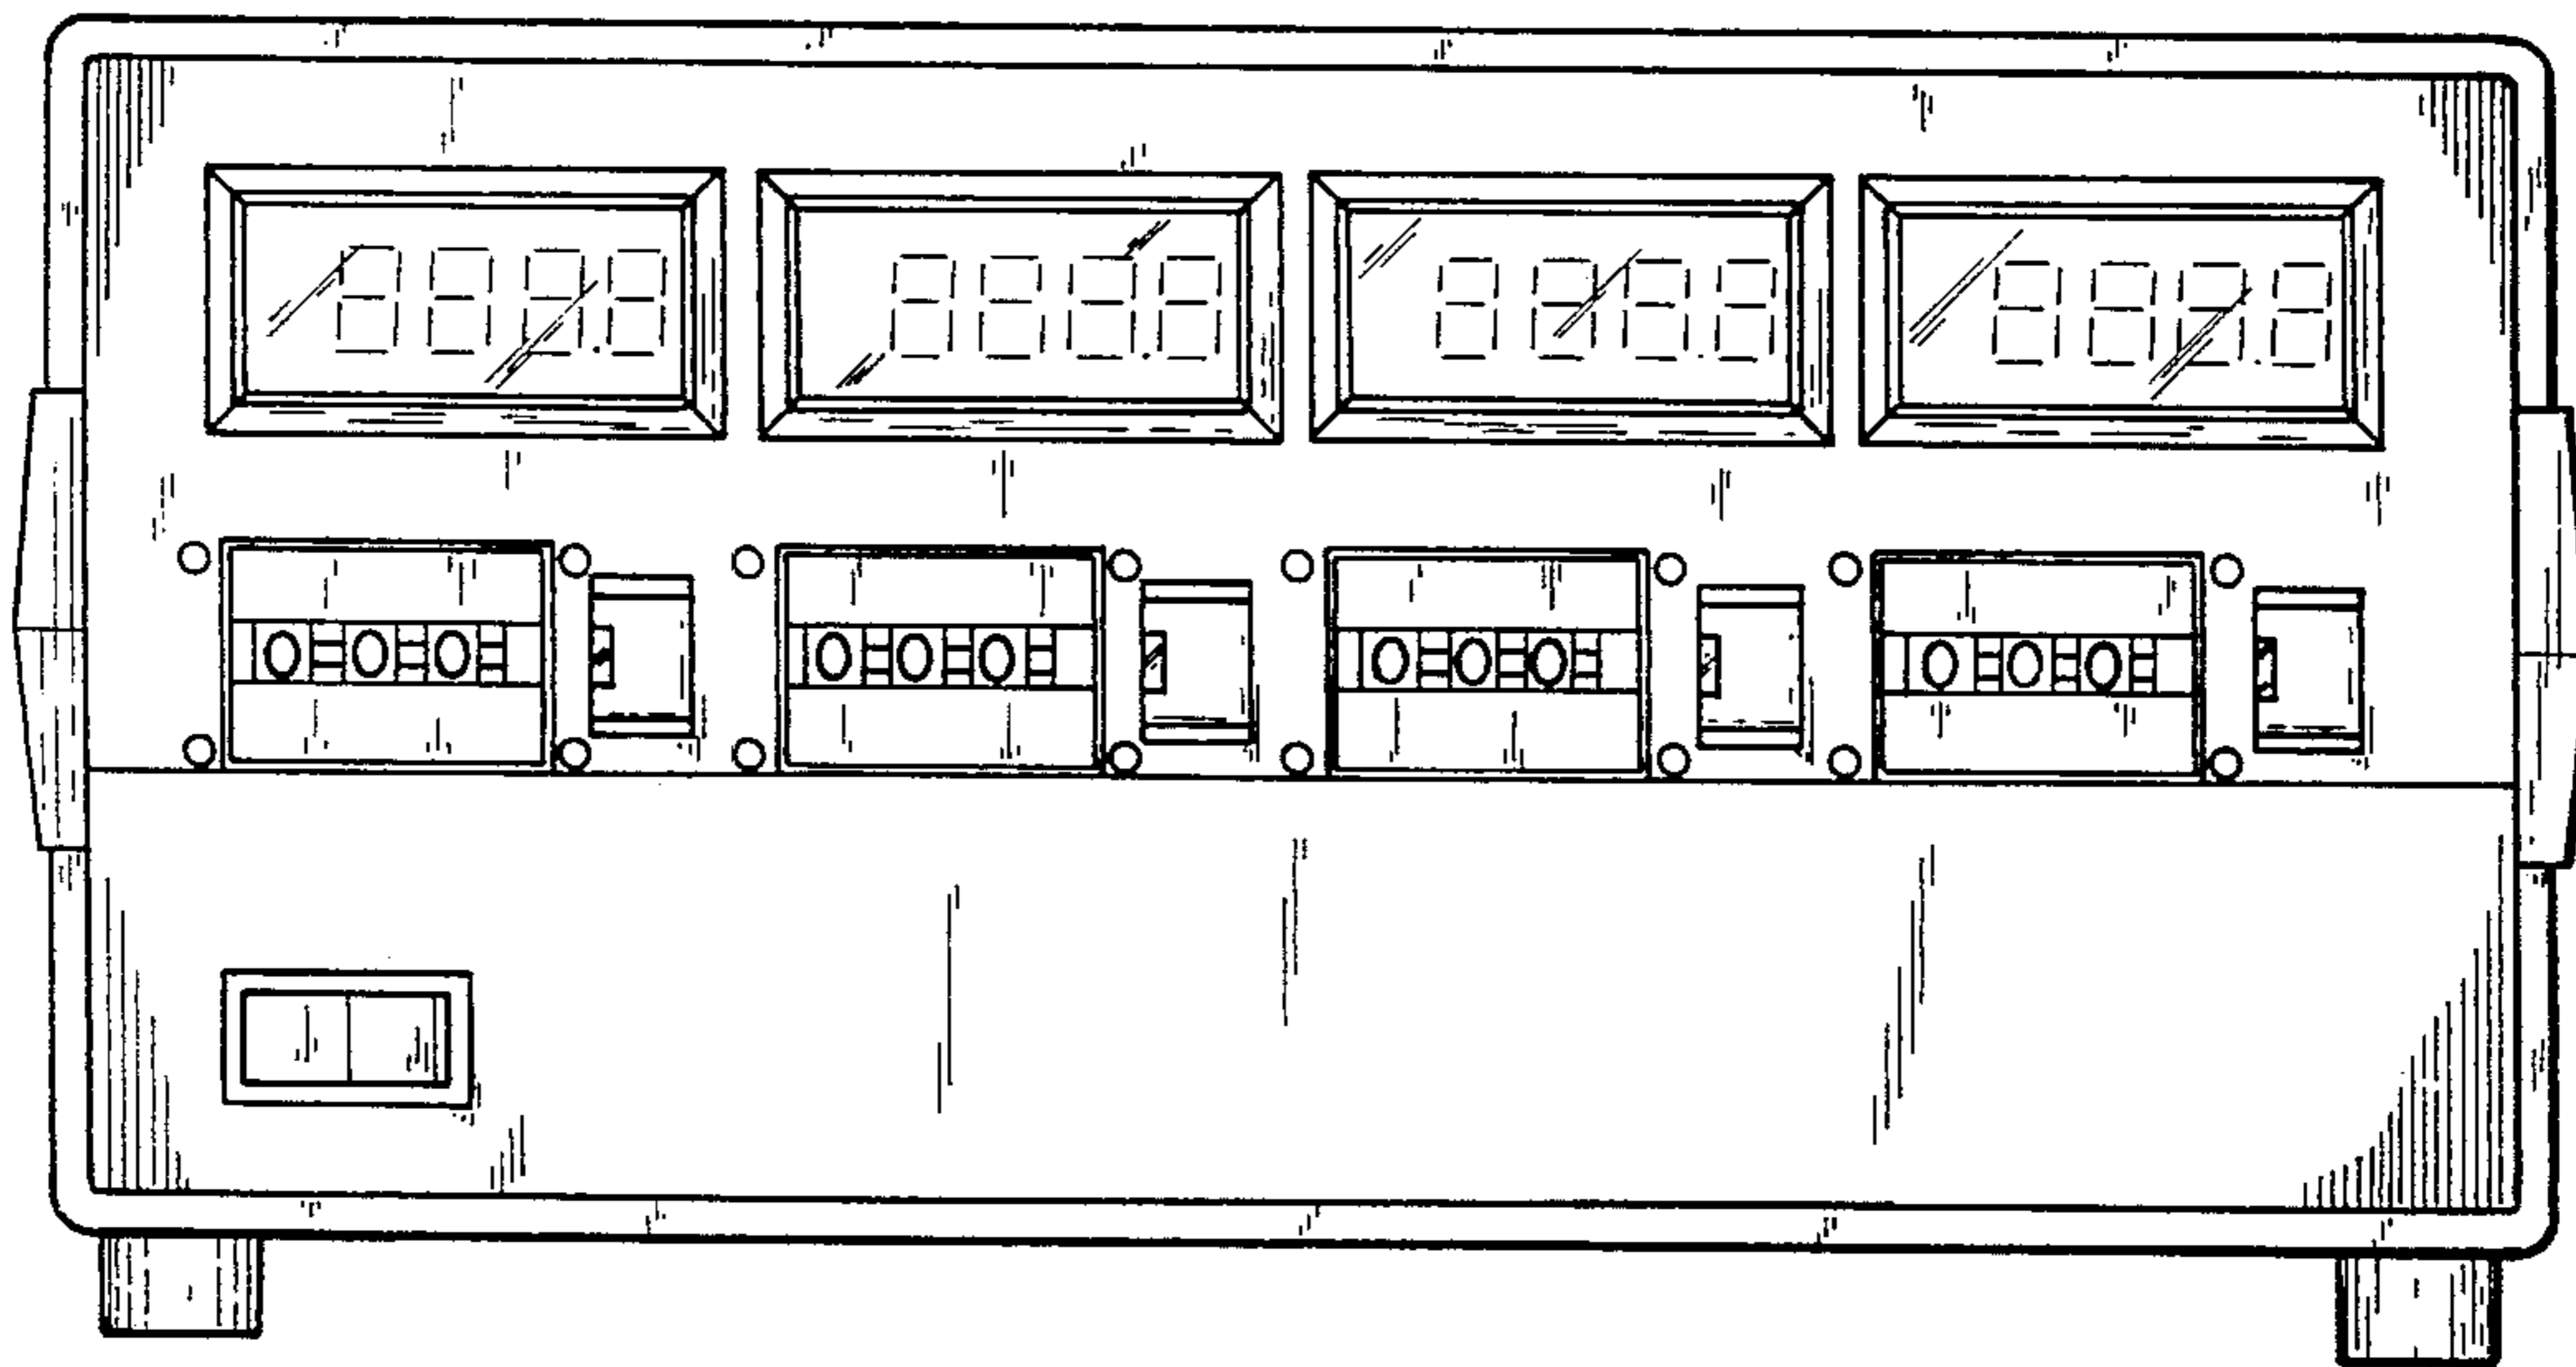

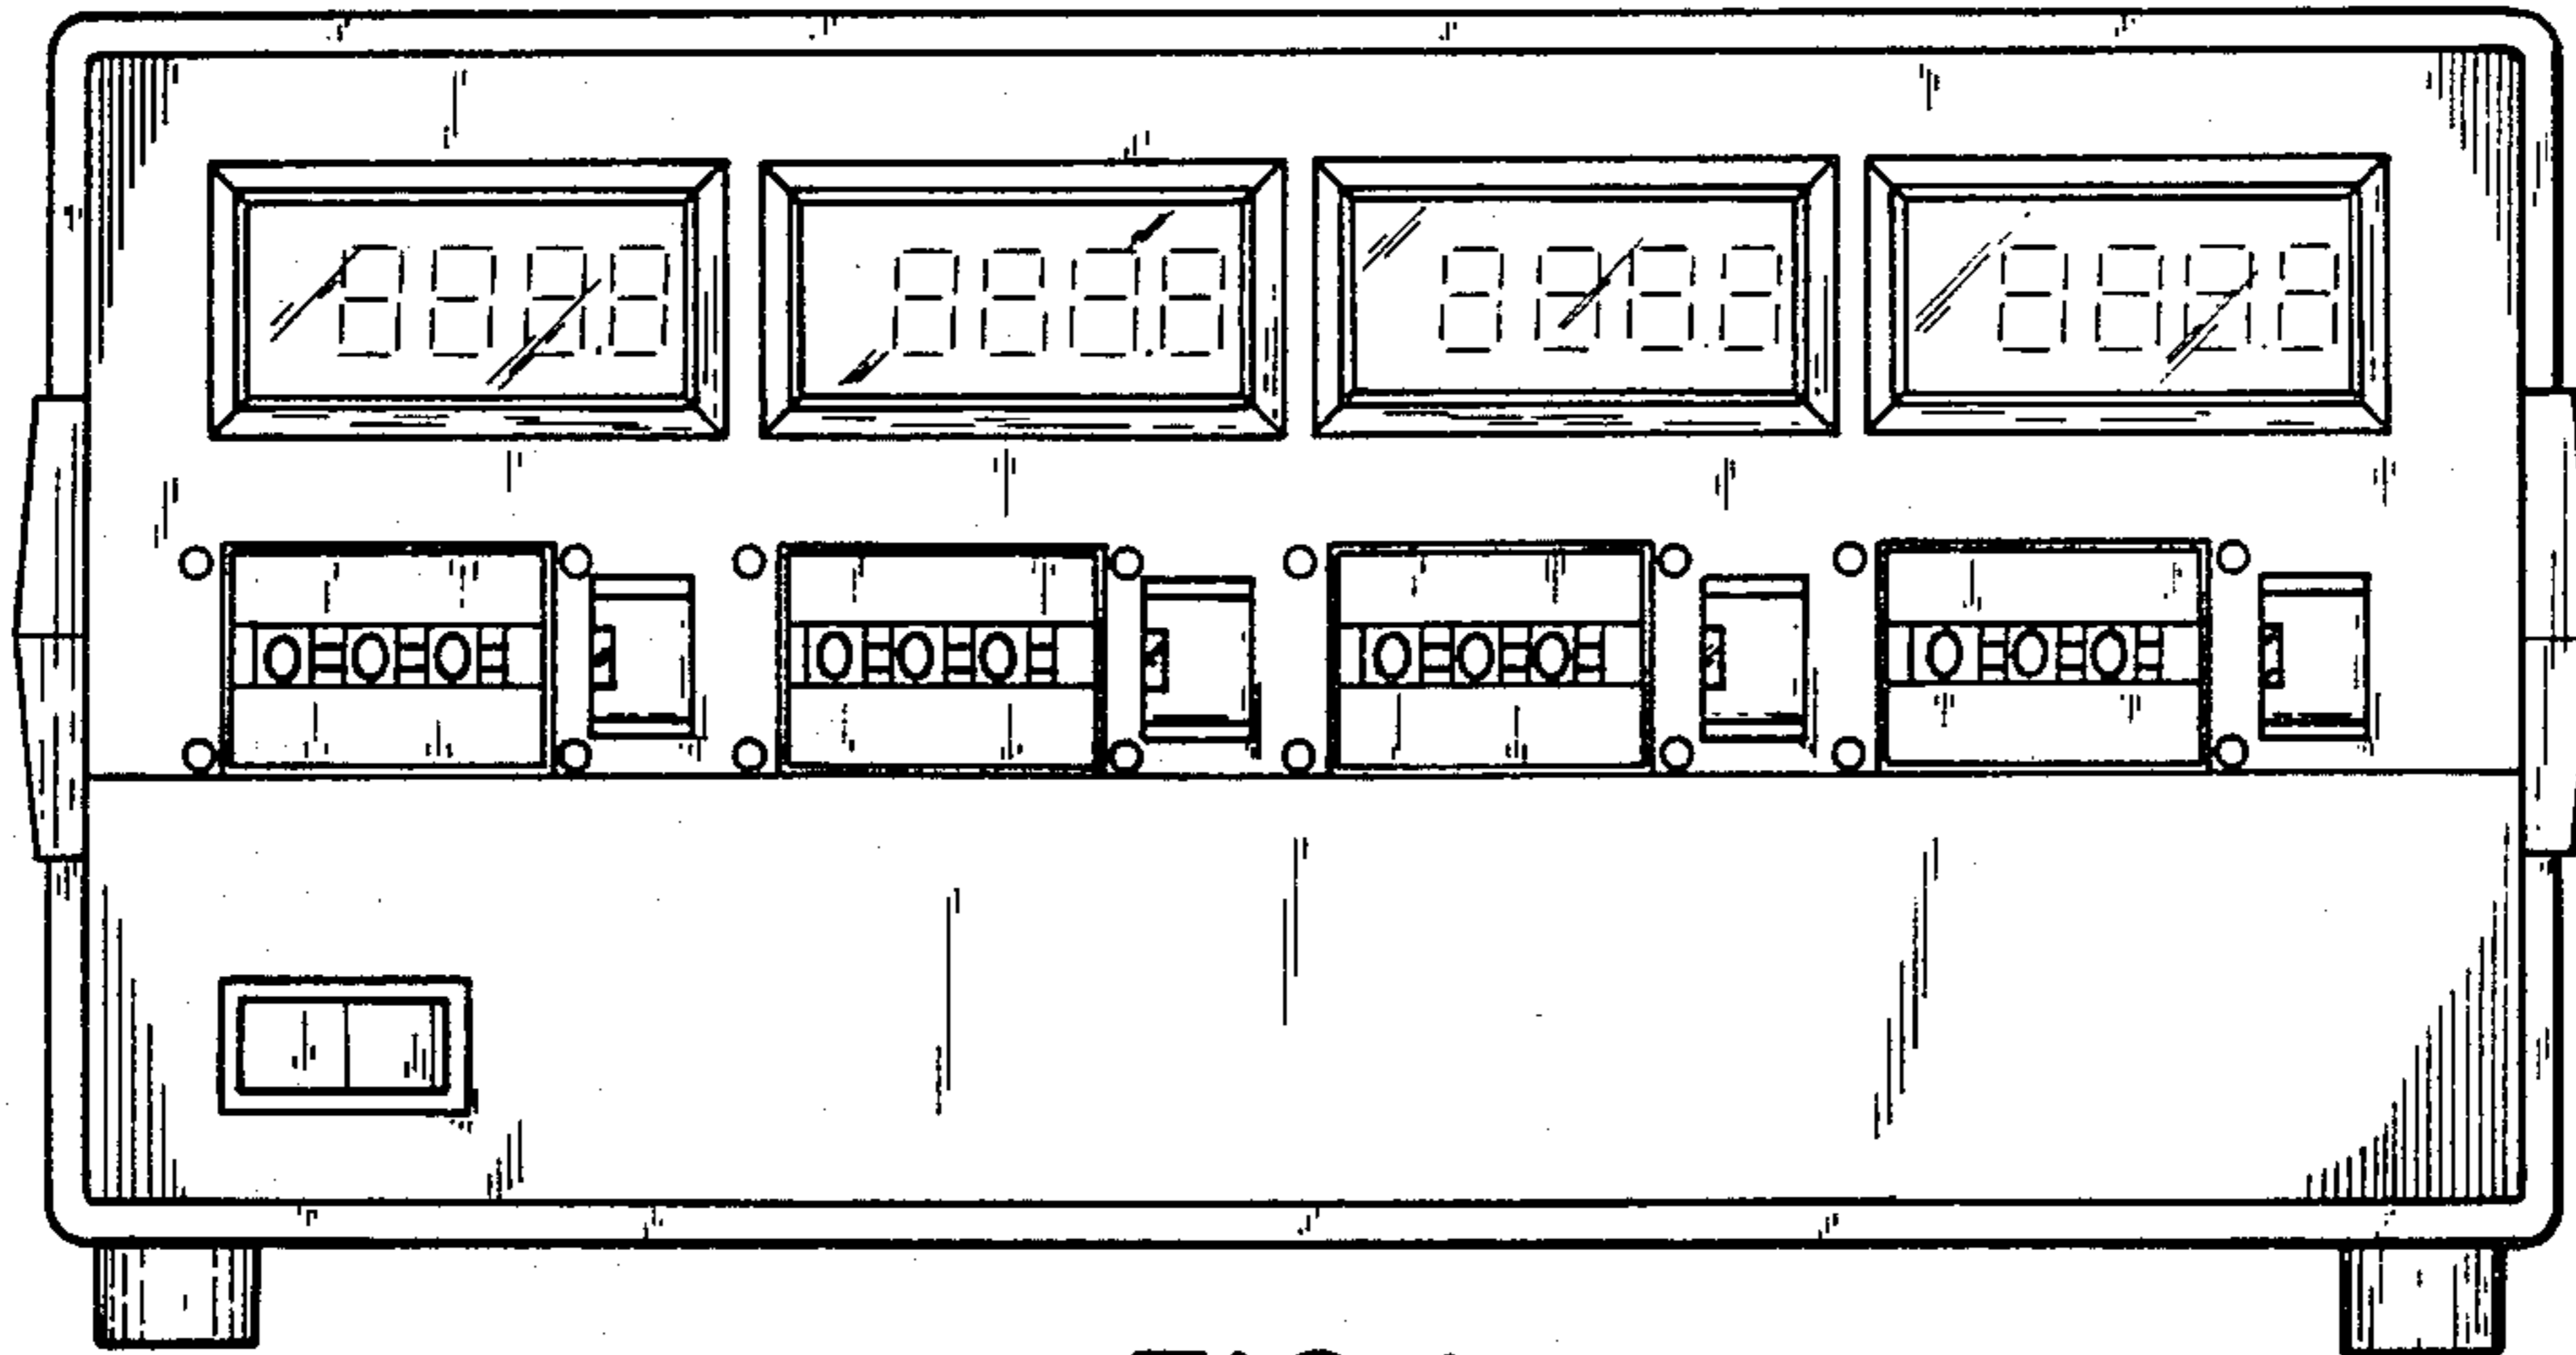


FIG. 1

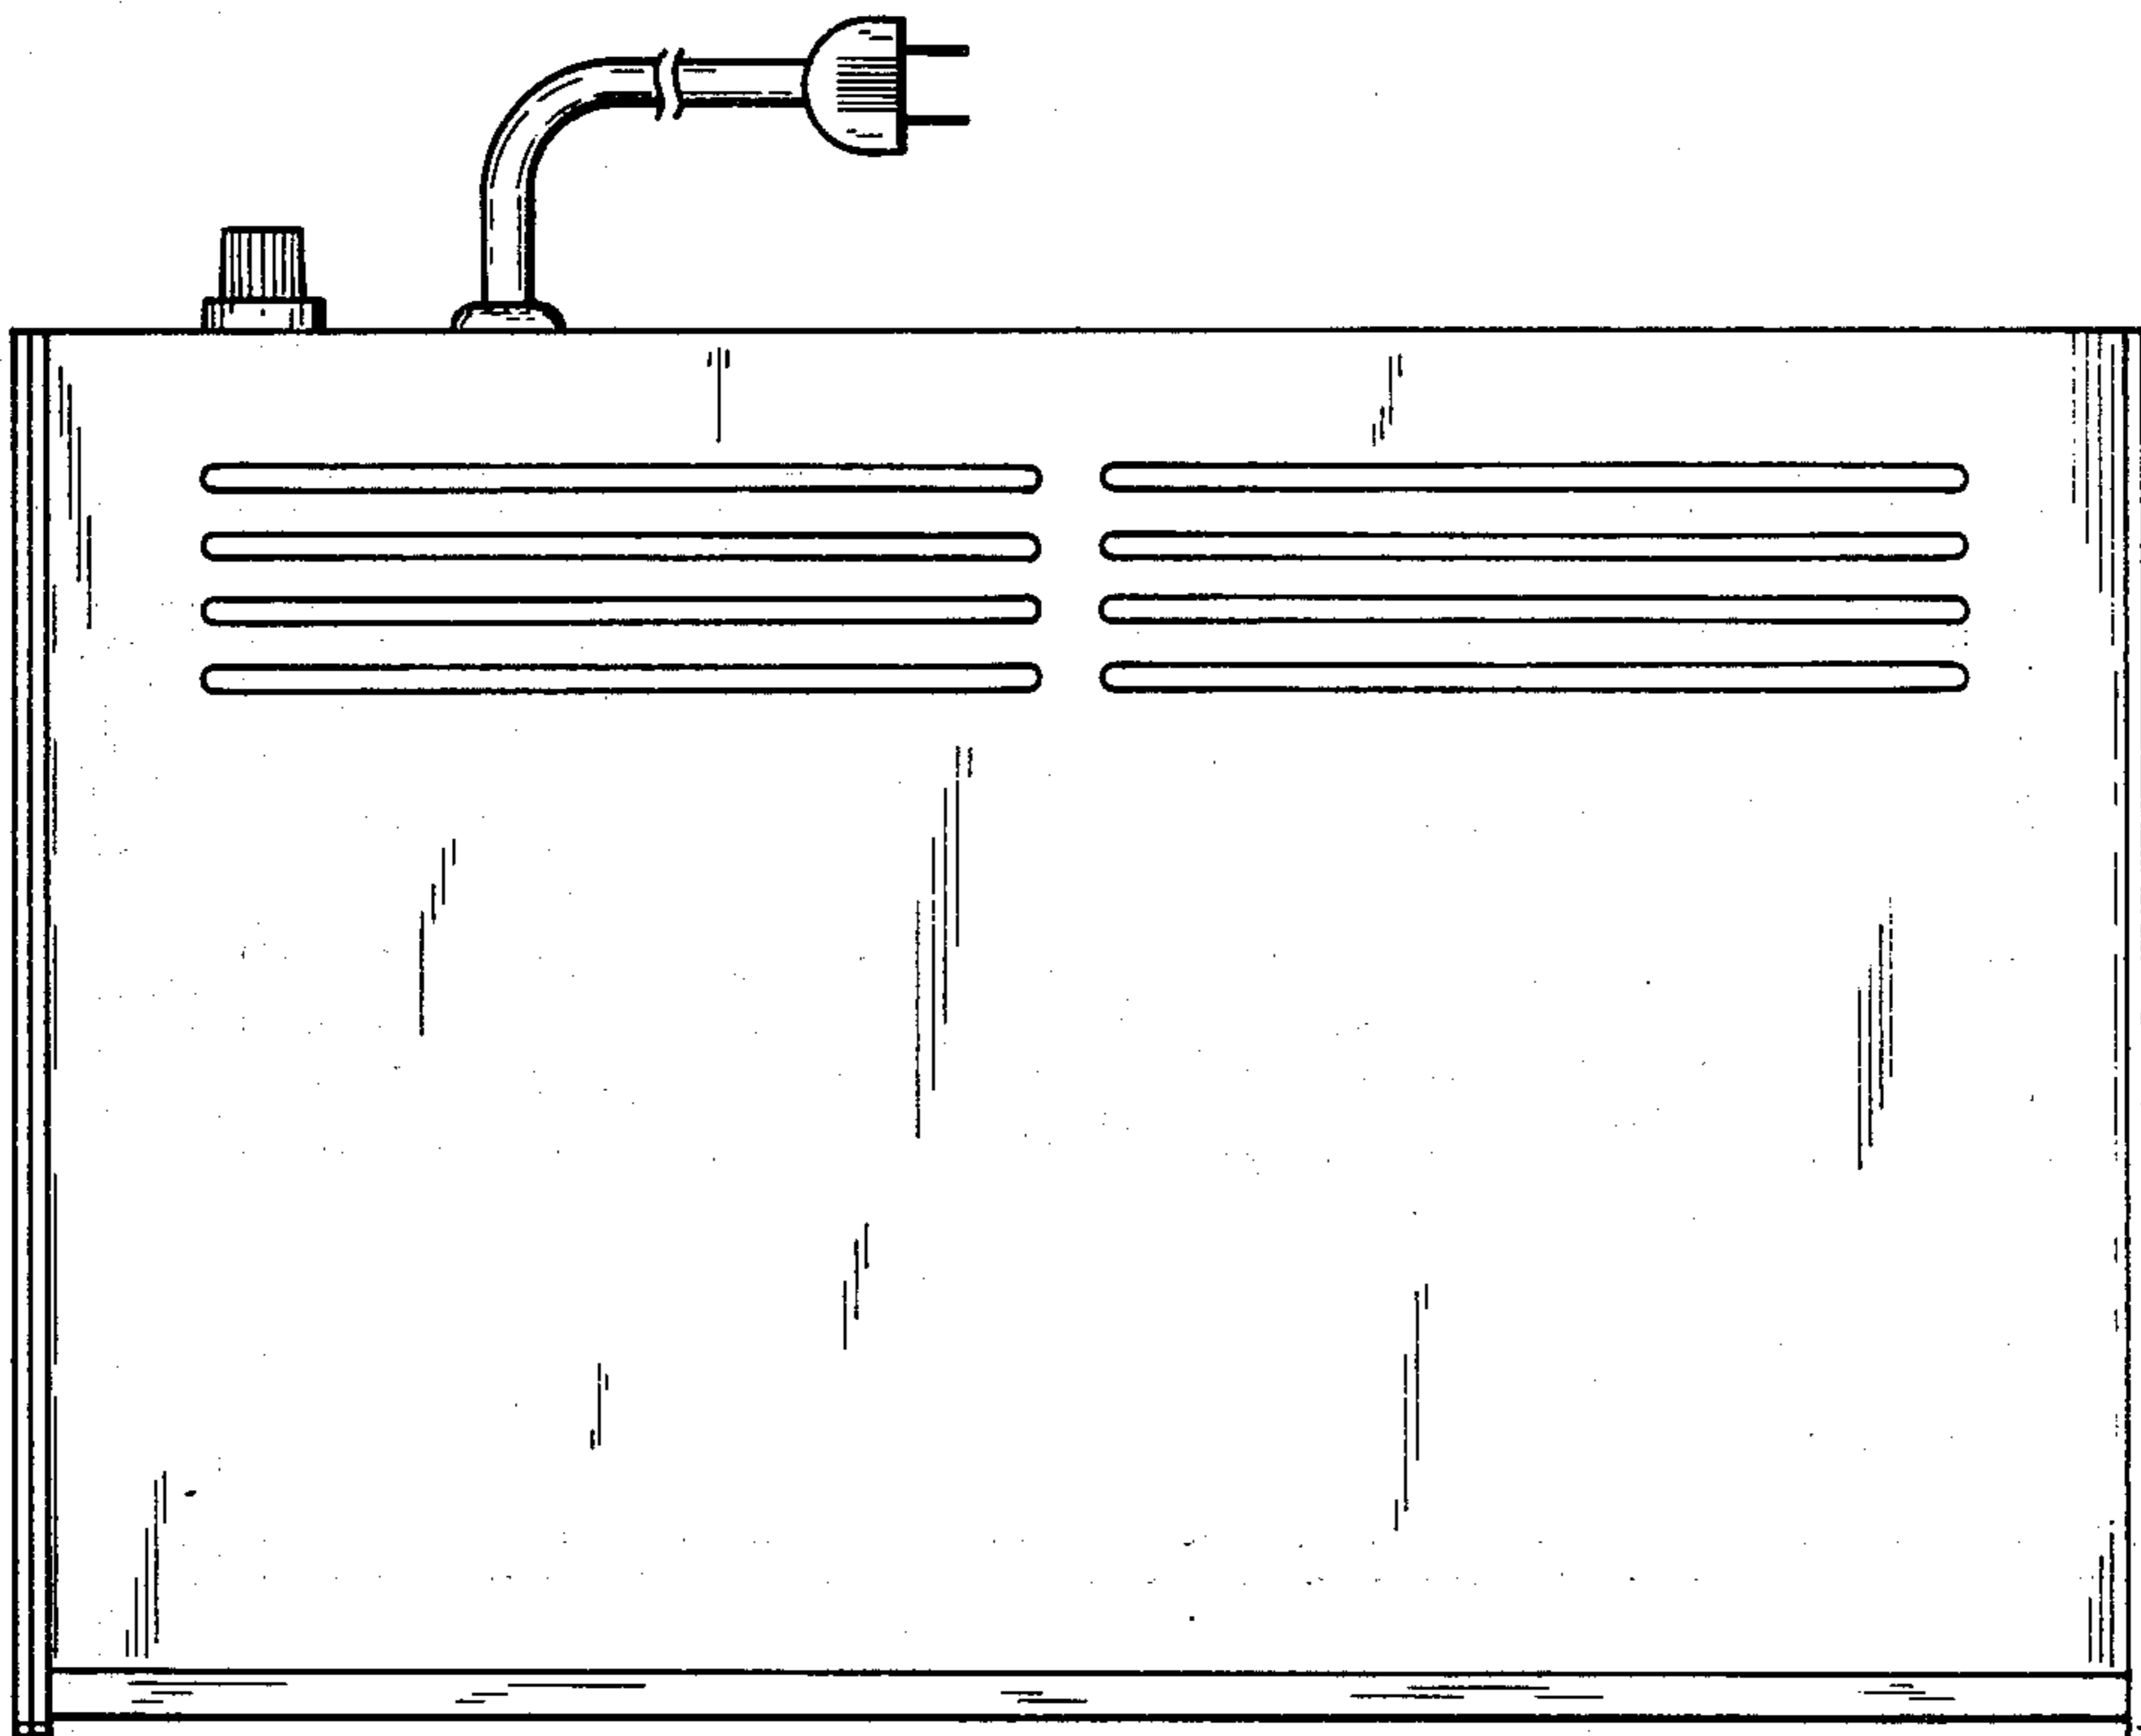


FIG. 2

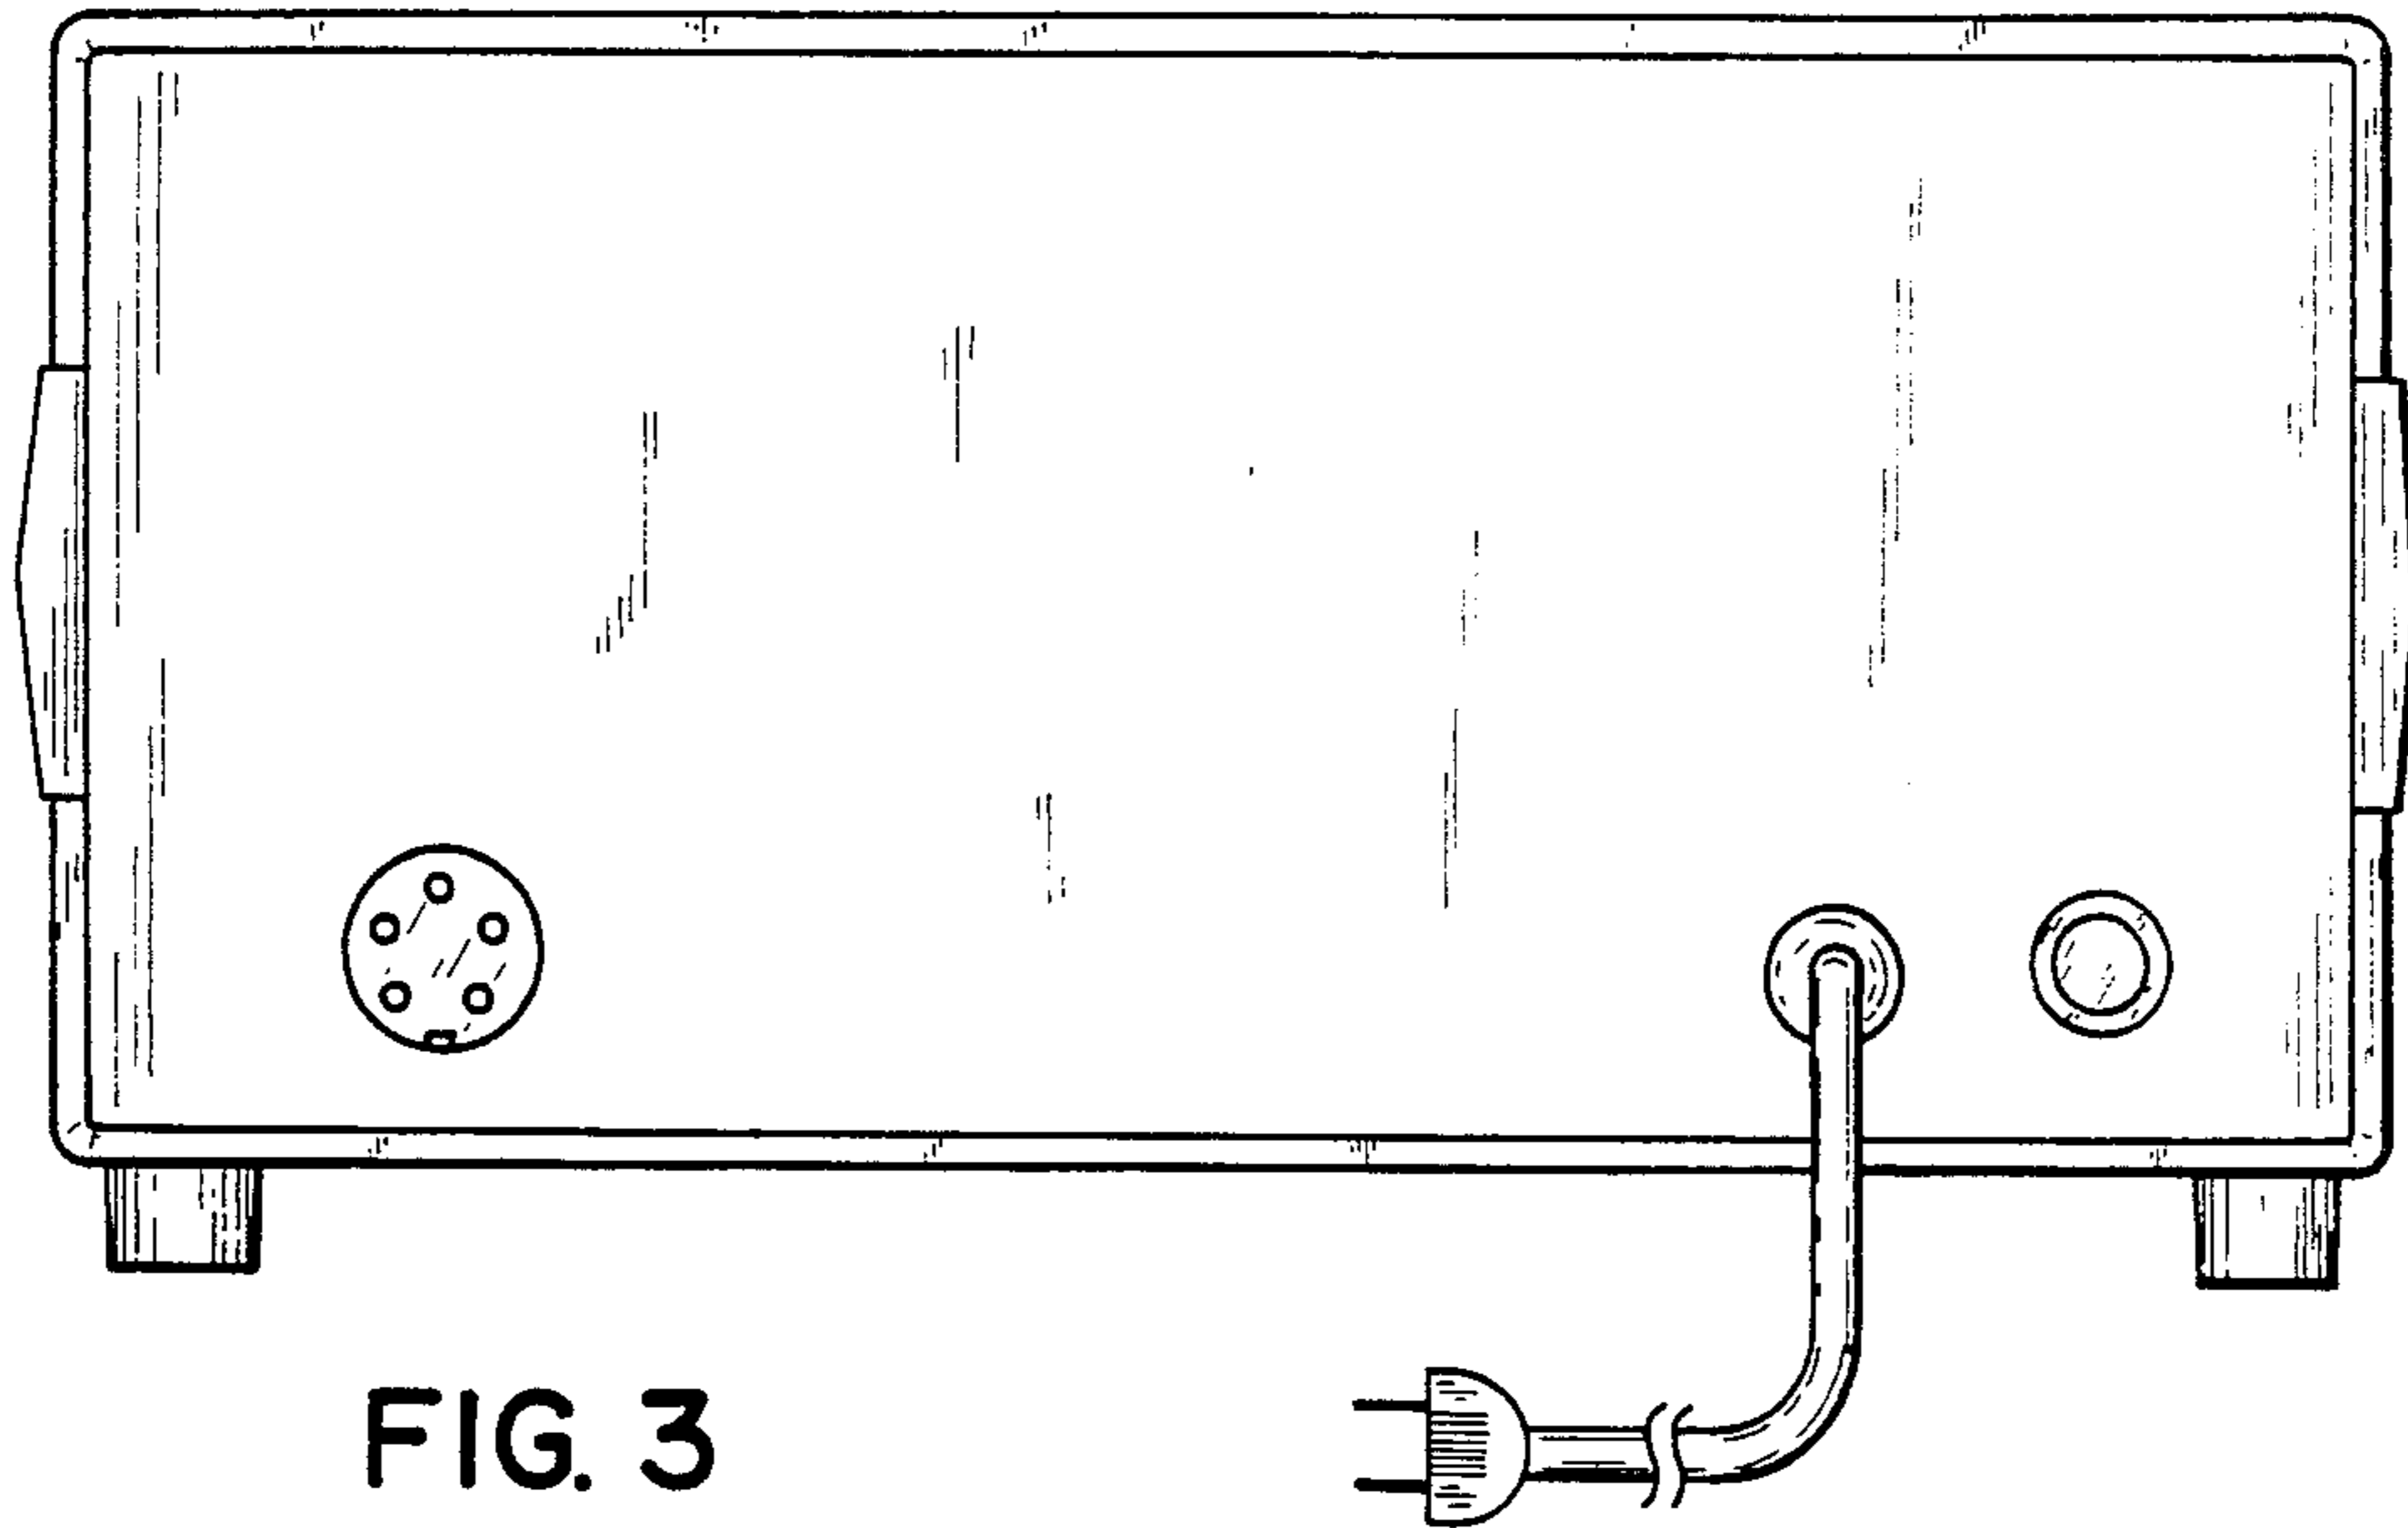


FIG. 3

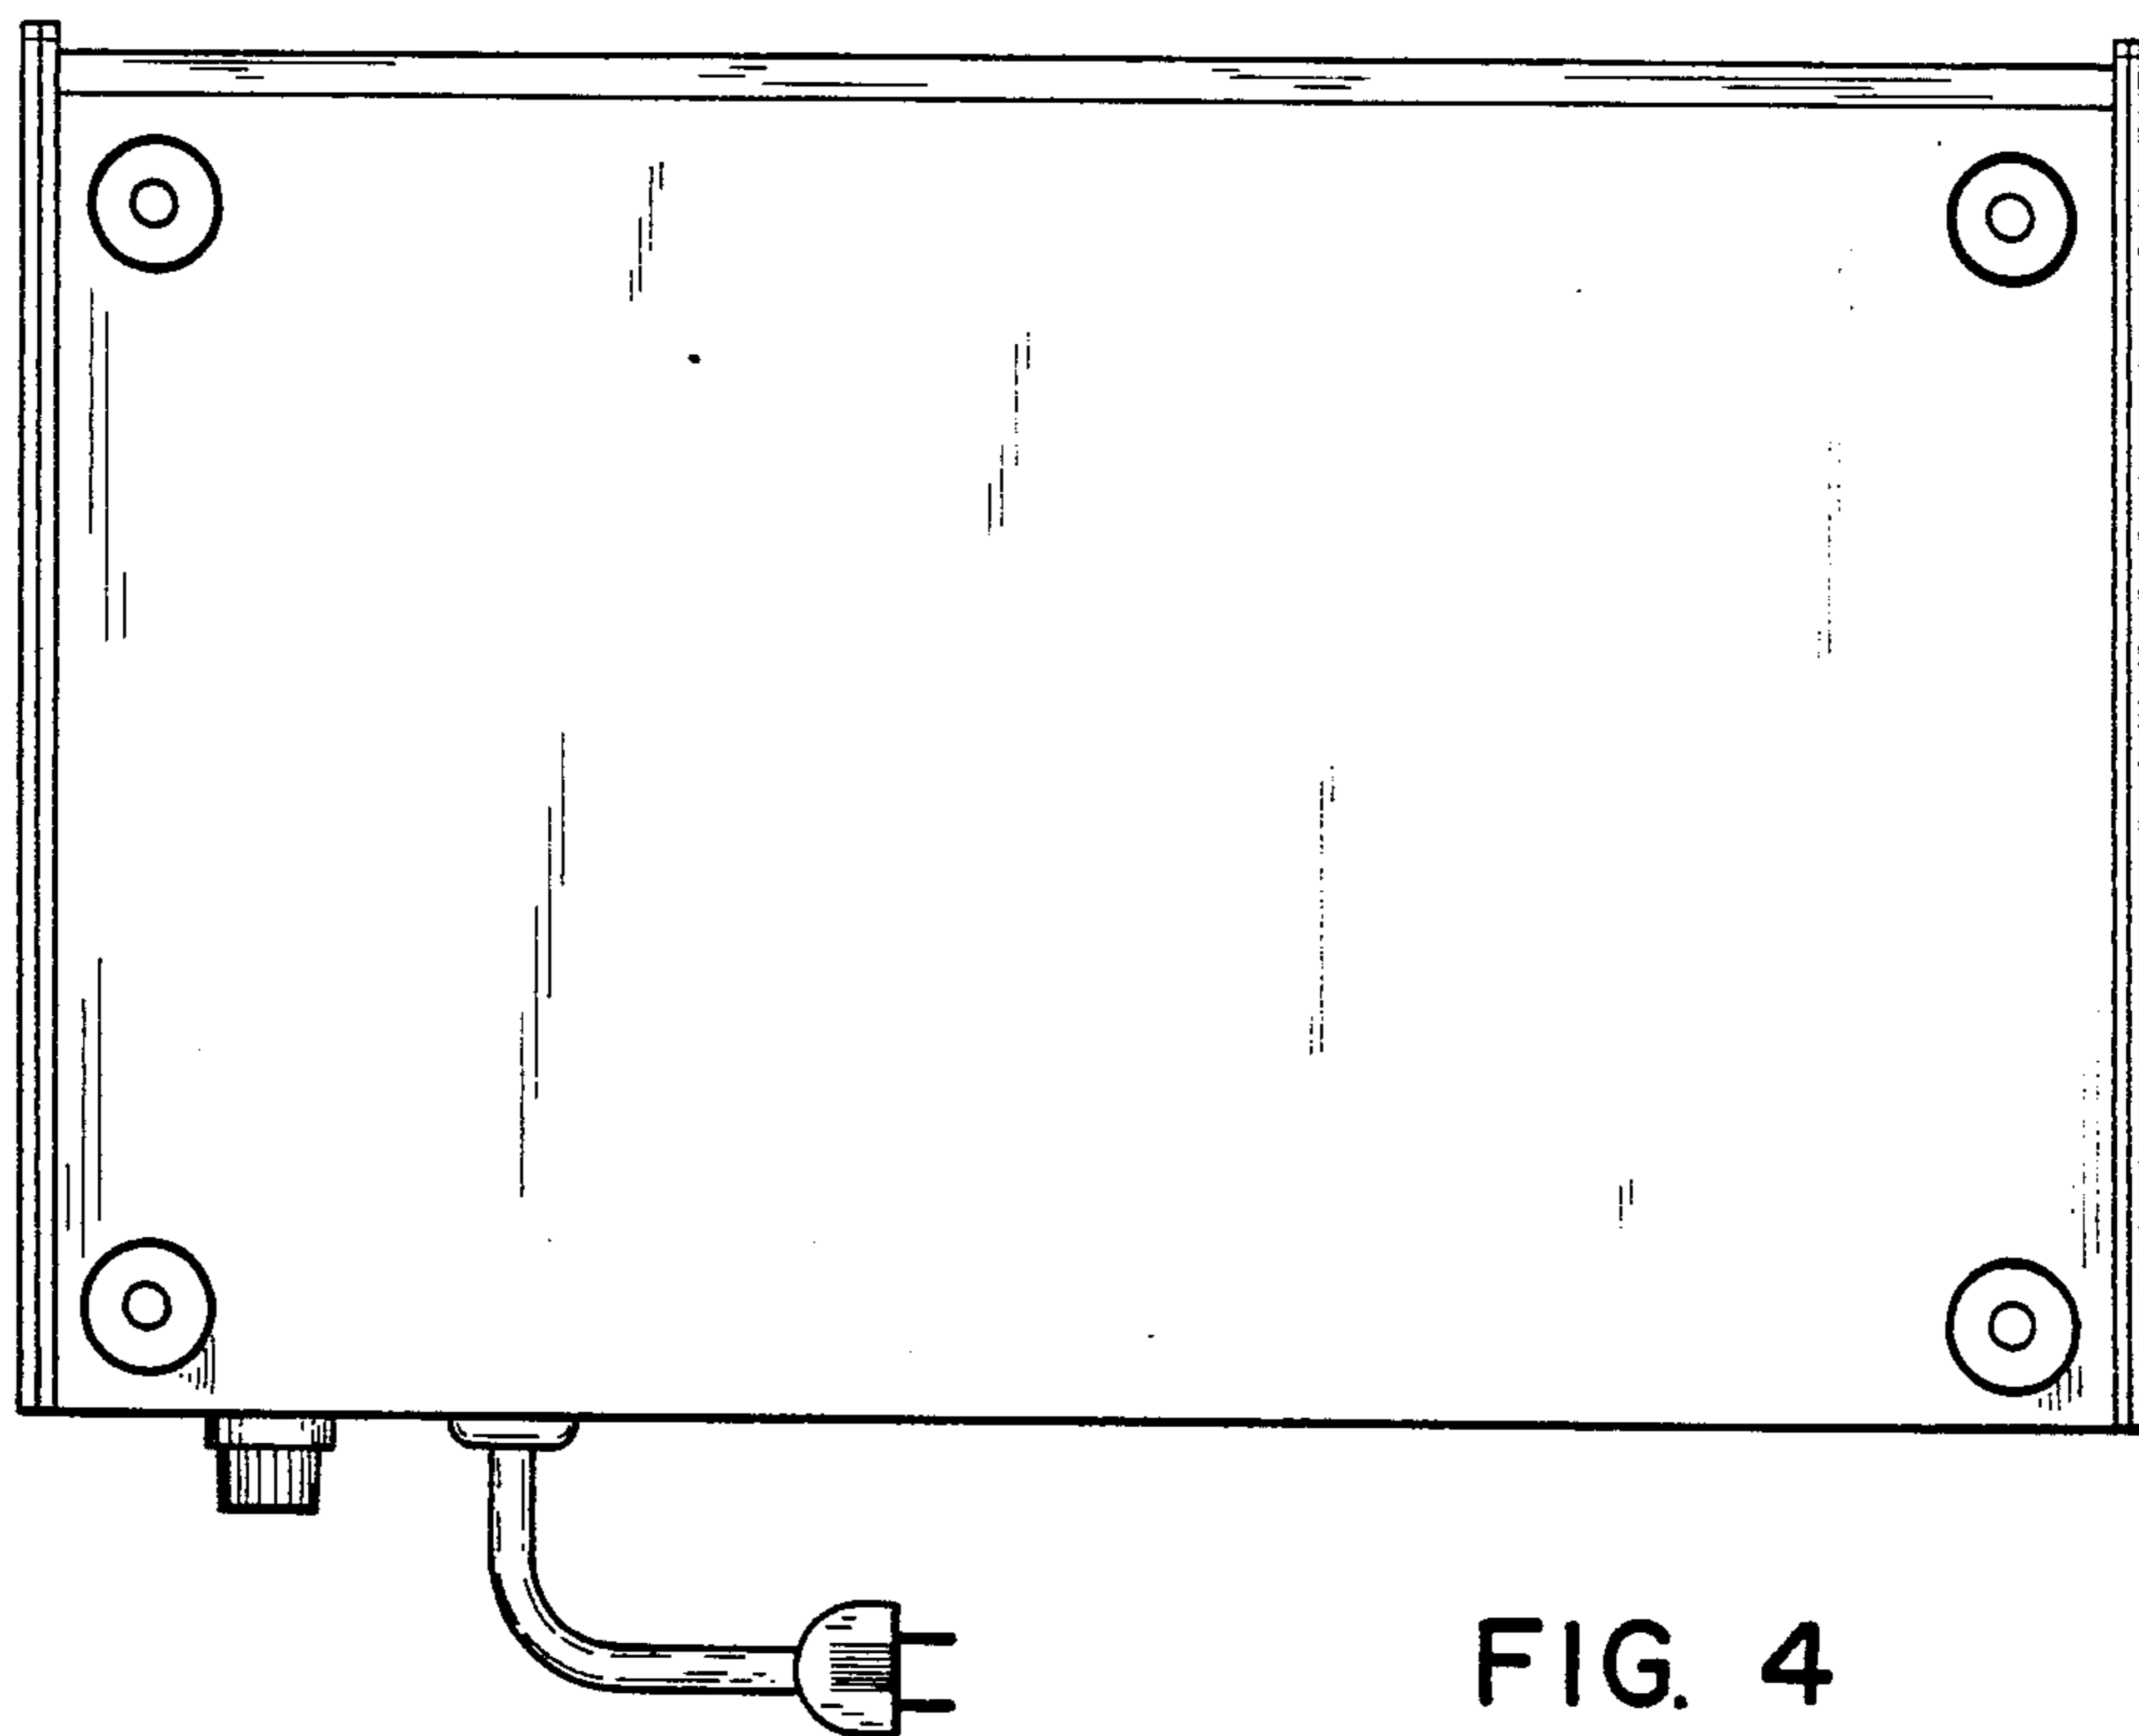


FIG. 4

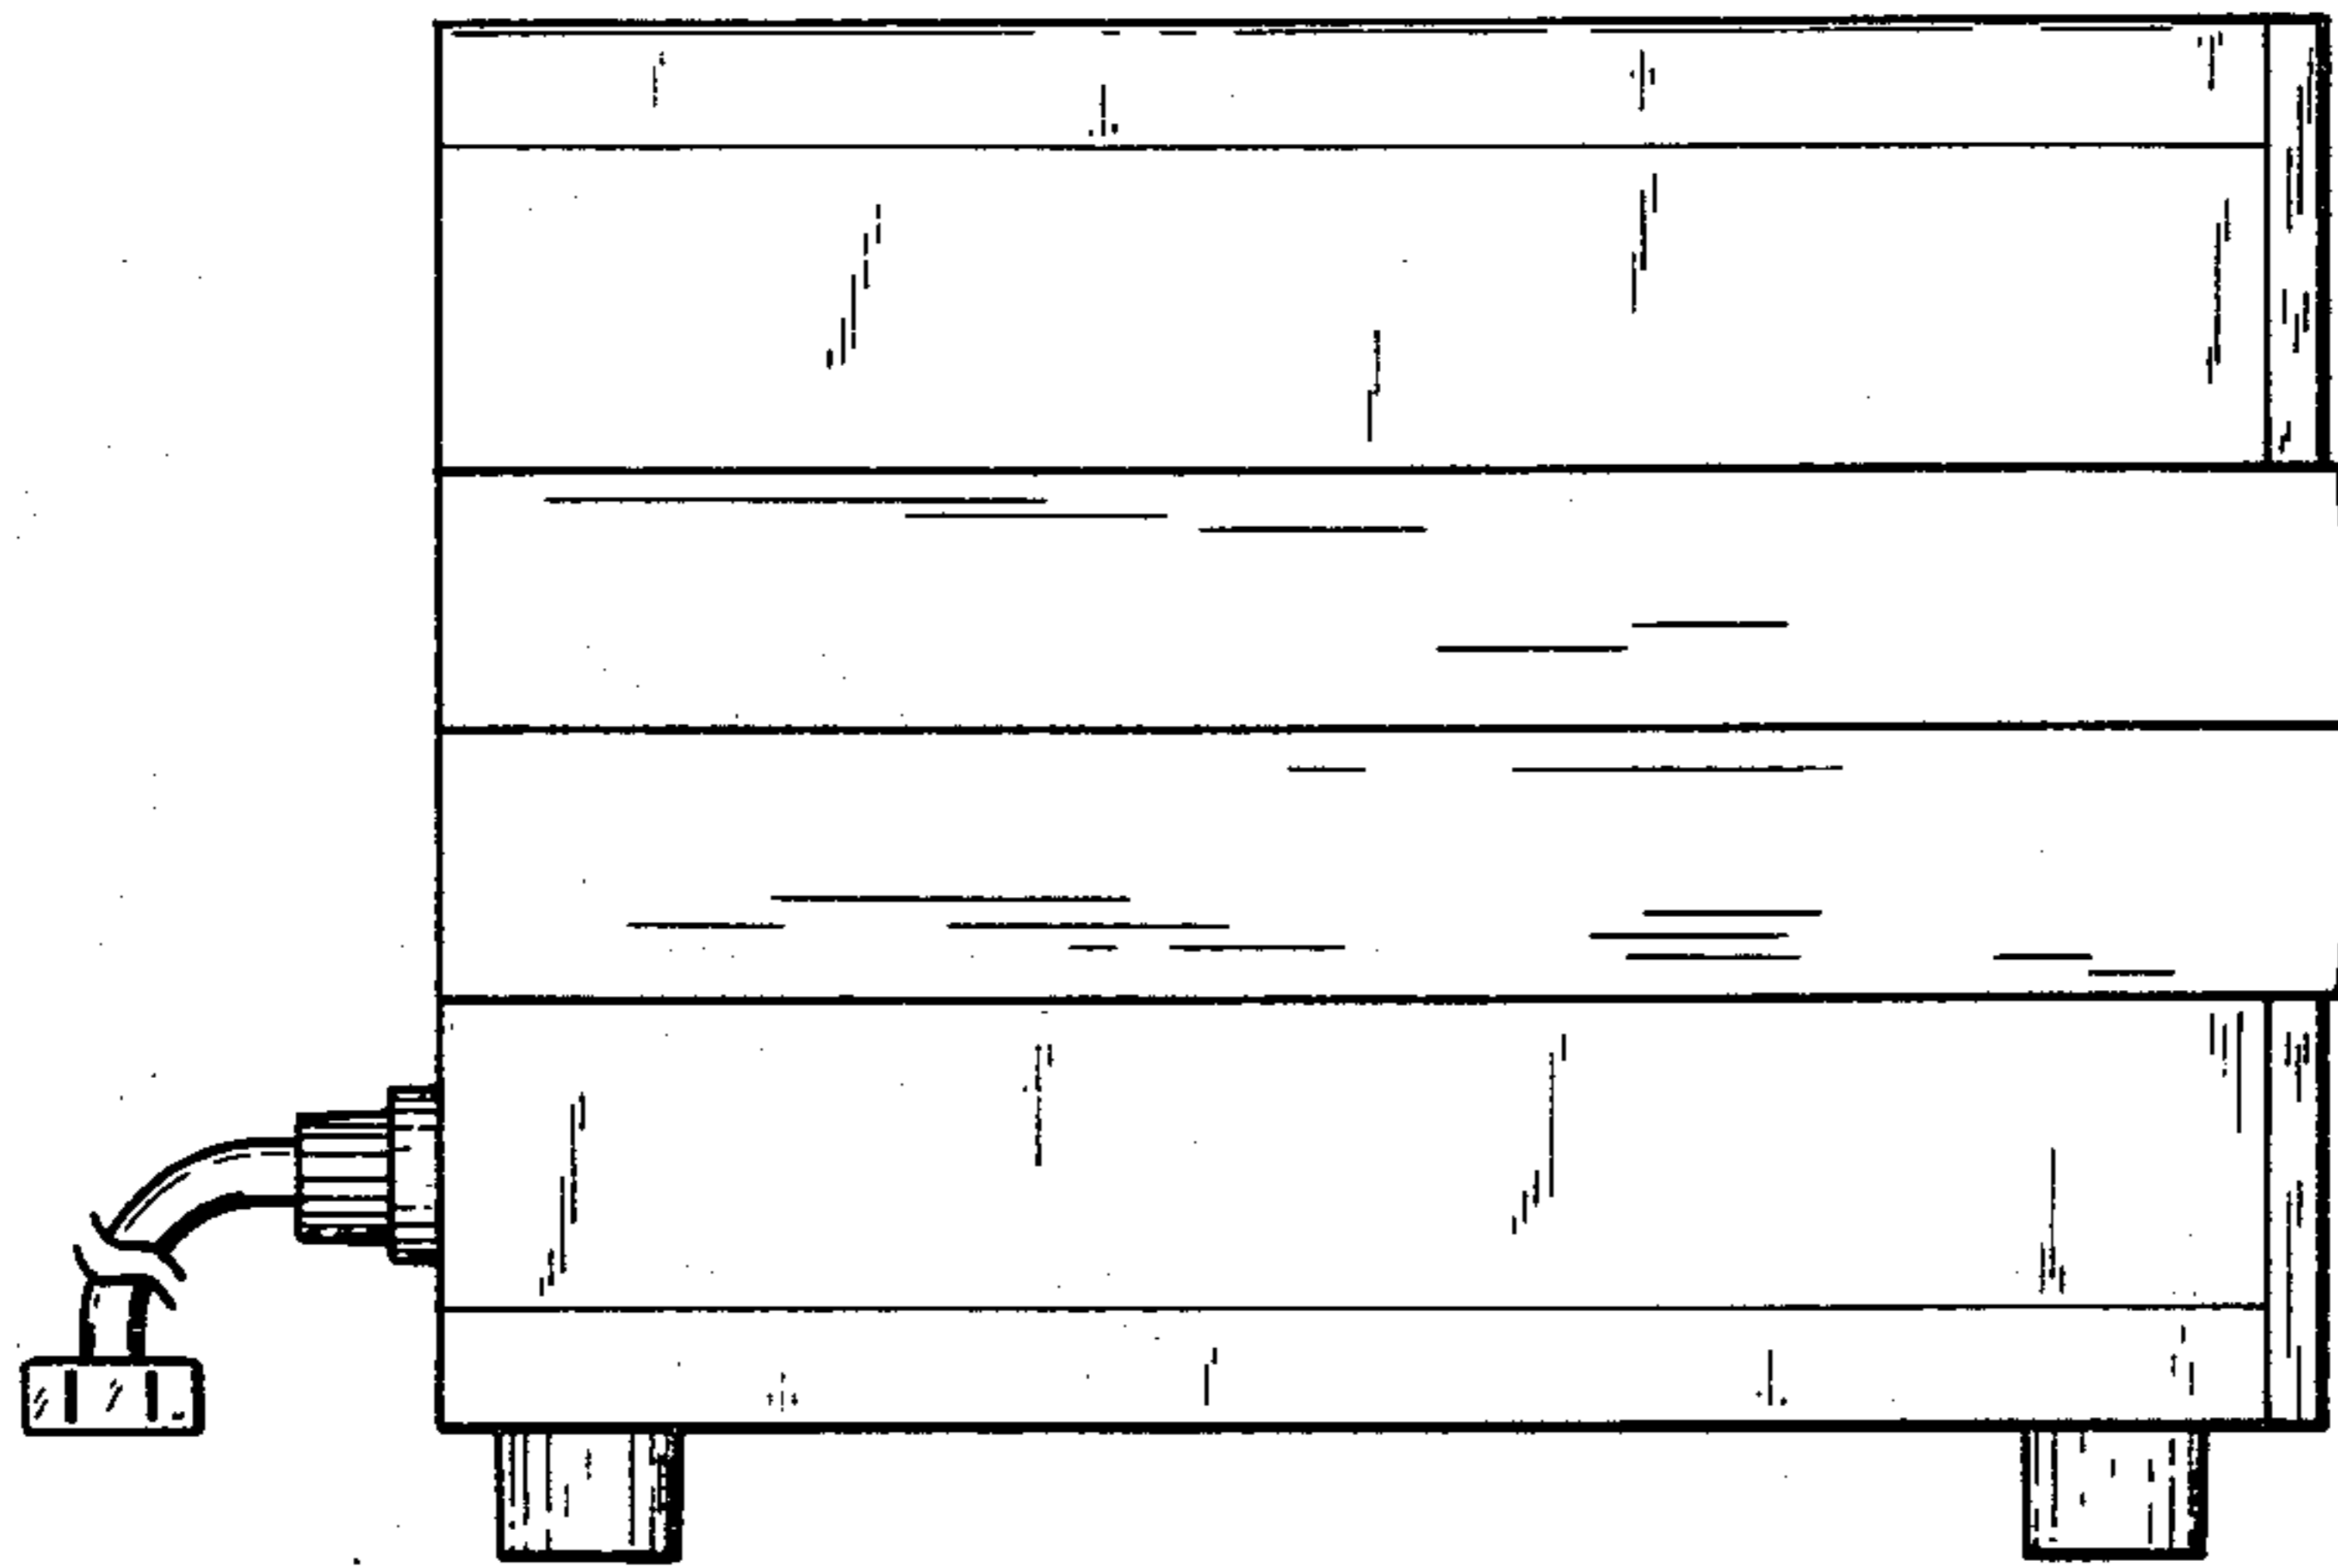


FIG. 5

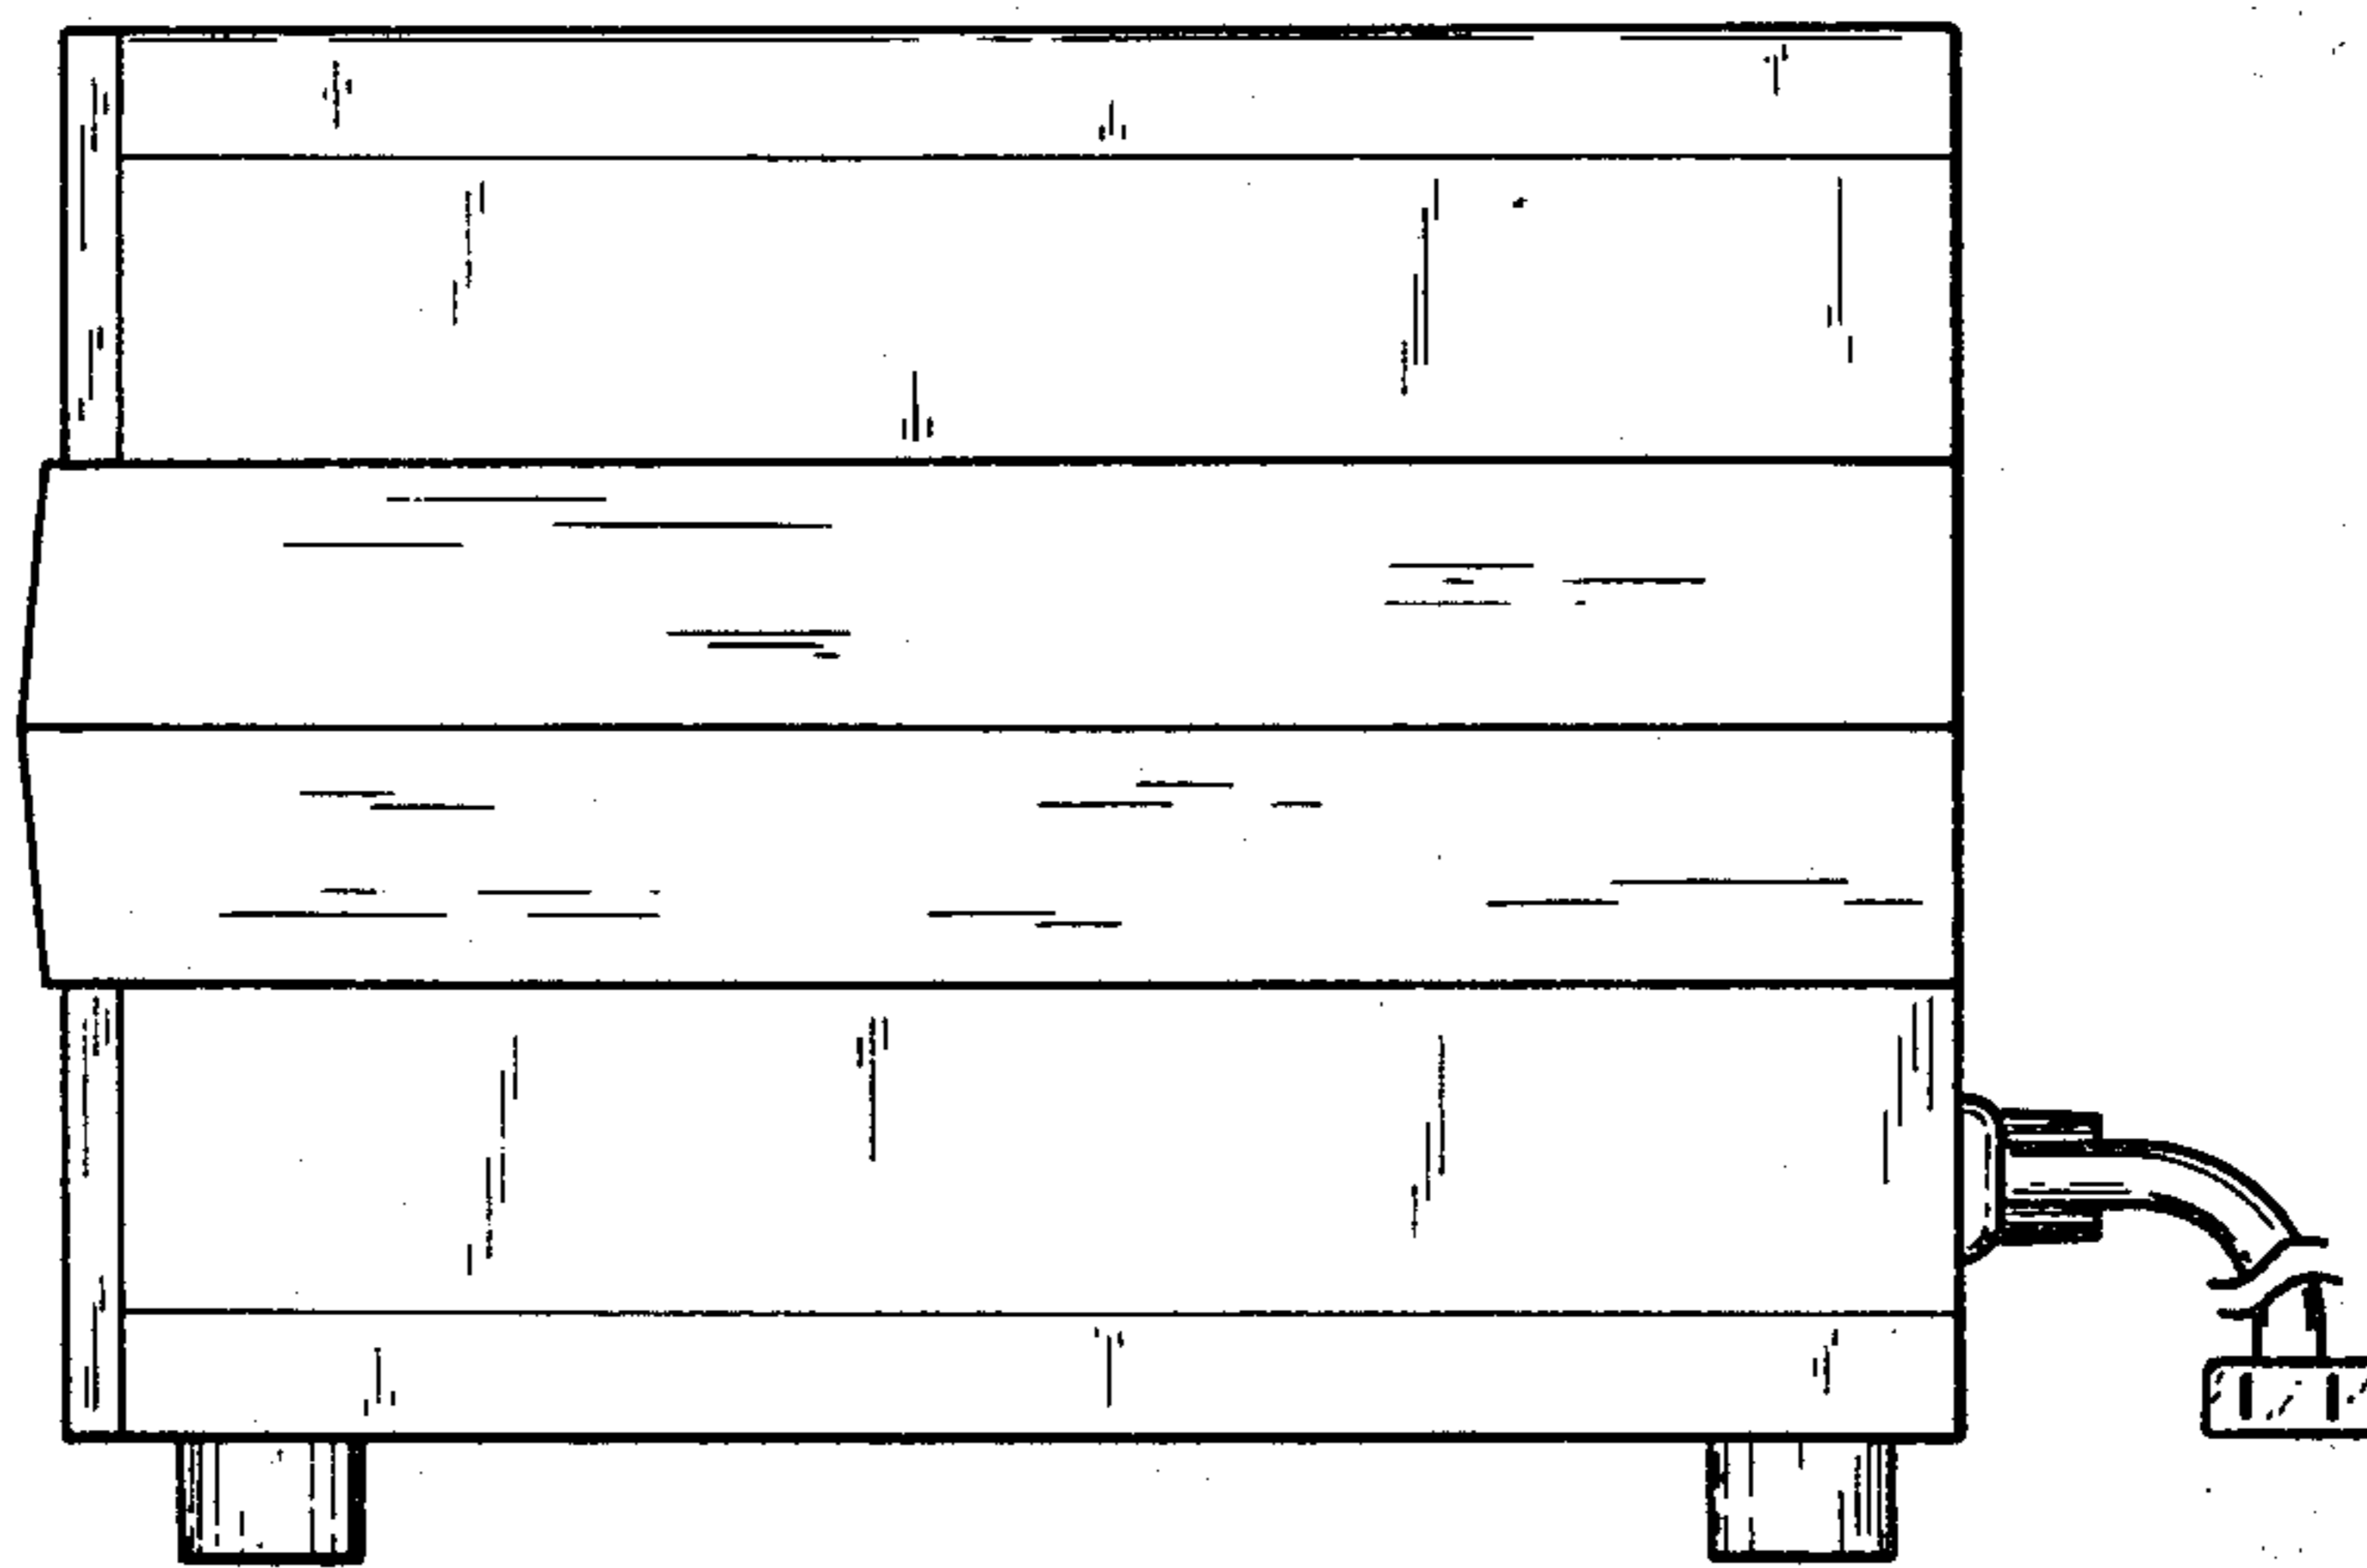


FIG. 6