

[54] FLOW DETECTOR FOR AN INTRAVENOUS ADMINISTRATION SET

[75] Inventors: Herbert F. D'Alo, Crystal Lake; Joseph N. Genese; Ronald W. Smith, both of Waukegan, all of Ill.

[73] Assignee: Abbott Laboratories, North Chicago, Ill.

[\*] Notice: The portion of the term of this patent subsequent to Apr. 10, 1998 has been disclaimed.

[\*\*] Term: 14 Years

[21] Appl. No.: 360,505

[22] Filed: Mar. 22, 1982

[52] U.S. Cl. .... D24/8; D24/52; D24/99

[58] Field of Search ..... D24/8, 52, 99, 17, 51; 128/DIG. 13; 604/253, 65, 73; 73/861.41

[56] References Cited

U.S. PATENT DOCUMENTS

D. 273,419 4/1984 D'Alo et al. .... D24/8

Primary Examiner—B. J. Bullock

Assistant Examiner—Suzanne N. Gitlin

Attorney, Agent, or Firm—Neil E. Hamilton; Alan R. Thiele

[57] CLAIM

The ornamental design for a flow detector for an intravenous administration set, substantially as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a flow detector for an intravenous administration set, showing our new design;

FIG. 2 is an end view thereof;

FIG. 3 is an end view from the opposing end thereof;


FIG. 4 is a front elevational view thereof;

FIG. 5 is a back elevational view thereof;


FIG. 6 is a top plan view thereof; and

FIG. 7 is a bottom plan view thereof.


The broken line showing of a vented piercing pin and drip chamber with tubing in FIGS. 2-7 is for illustrative purposes only.

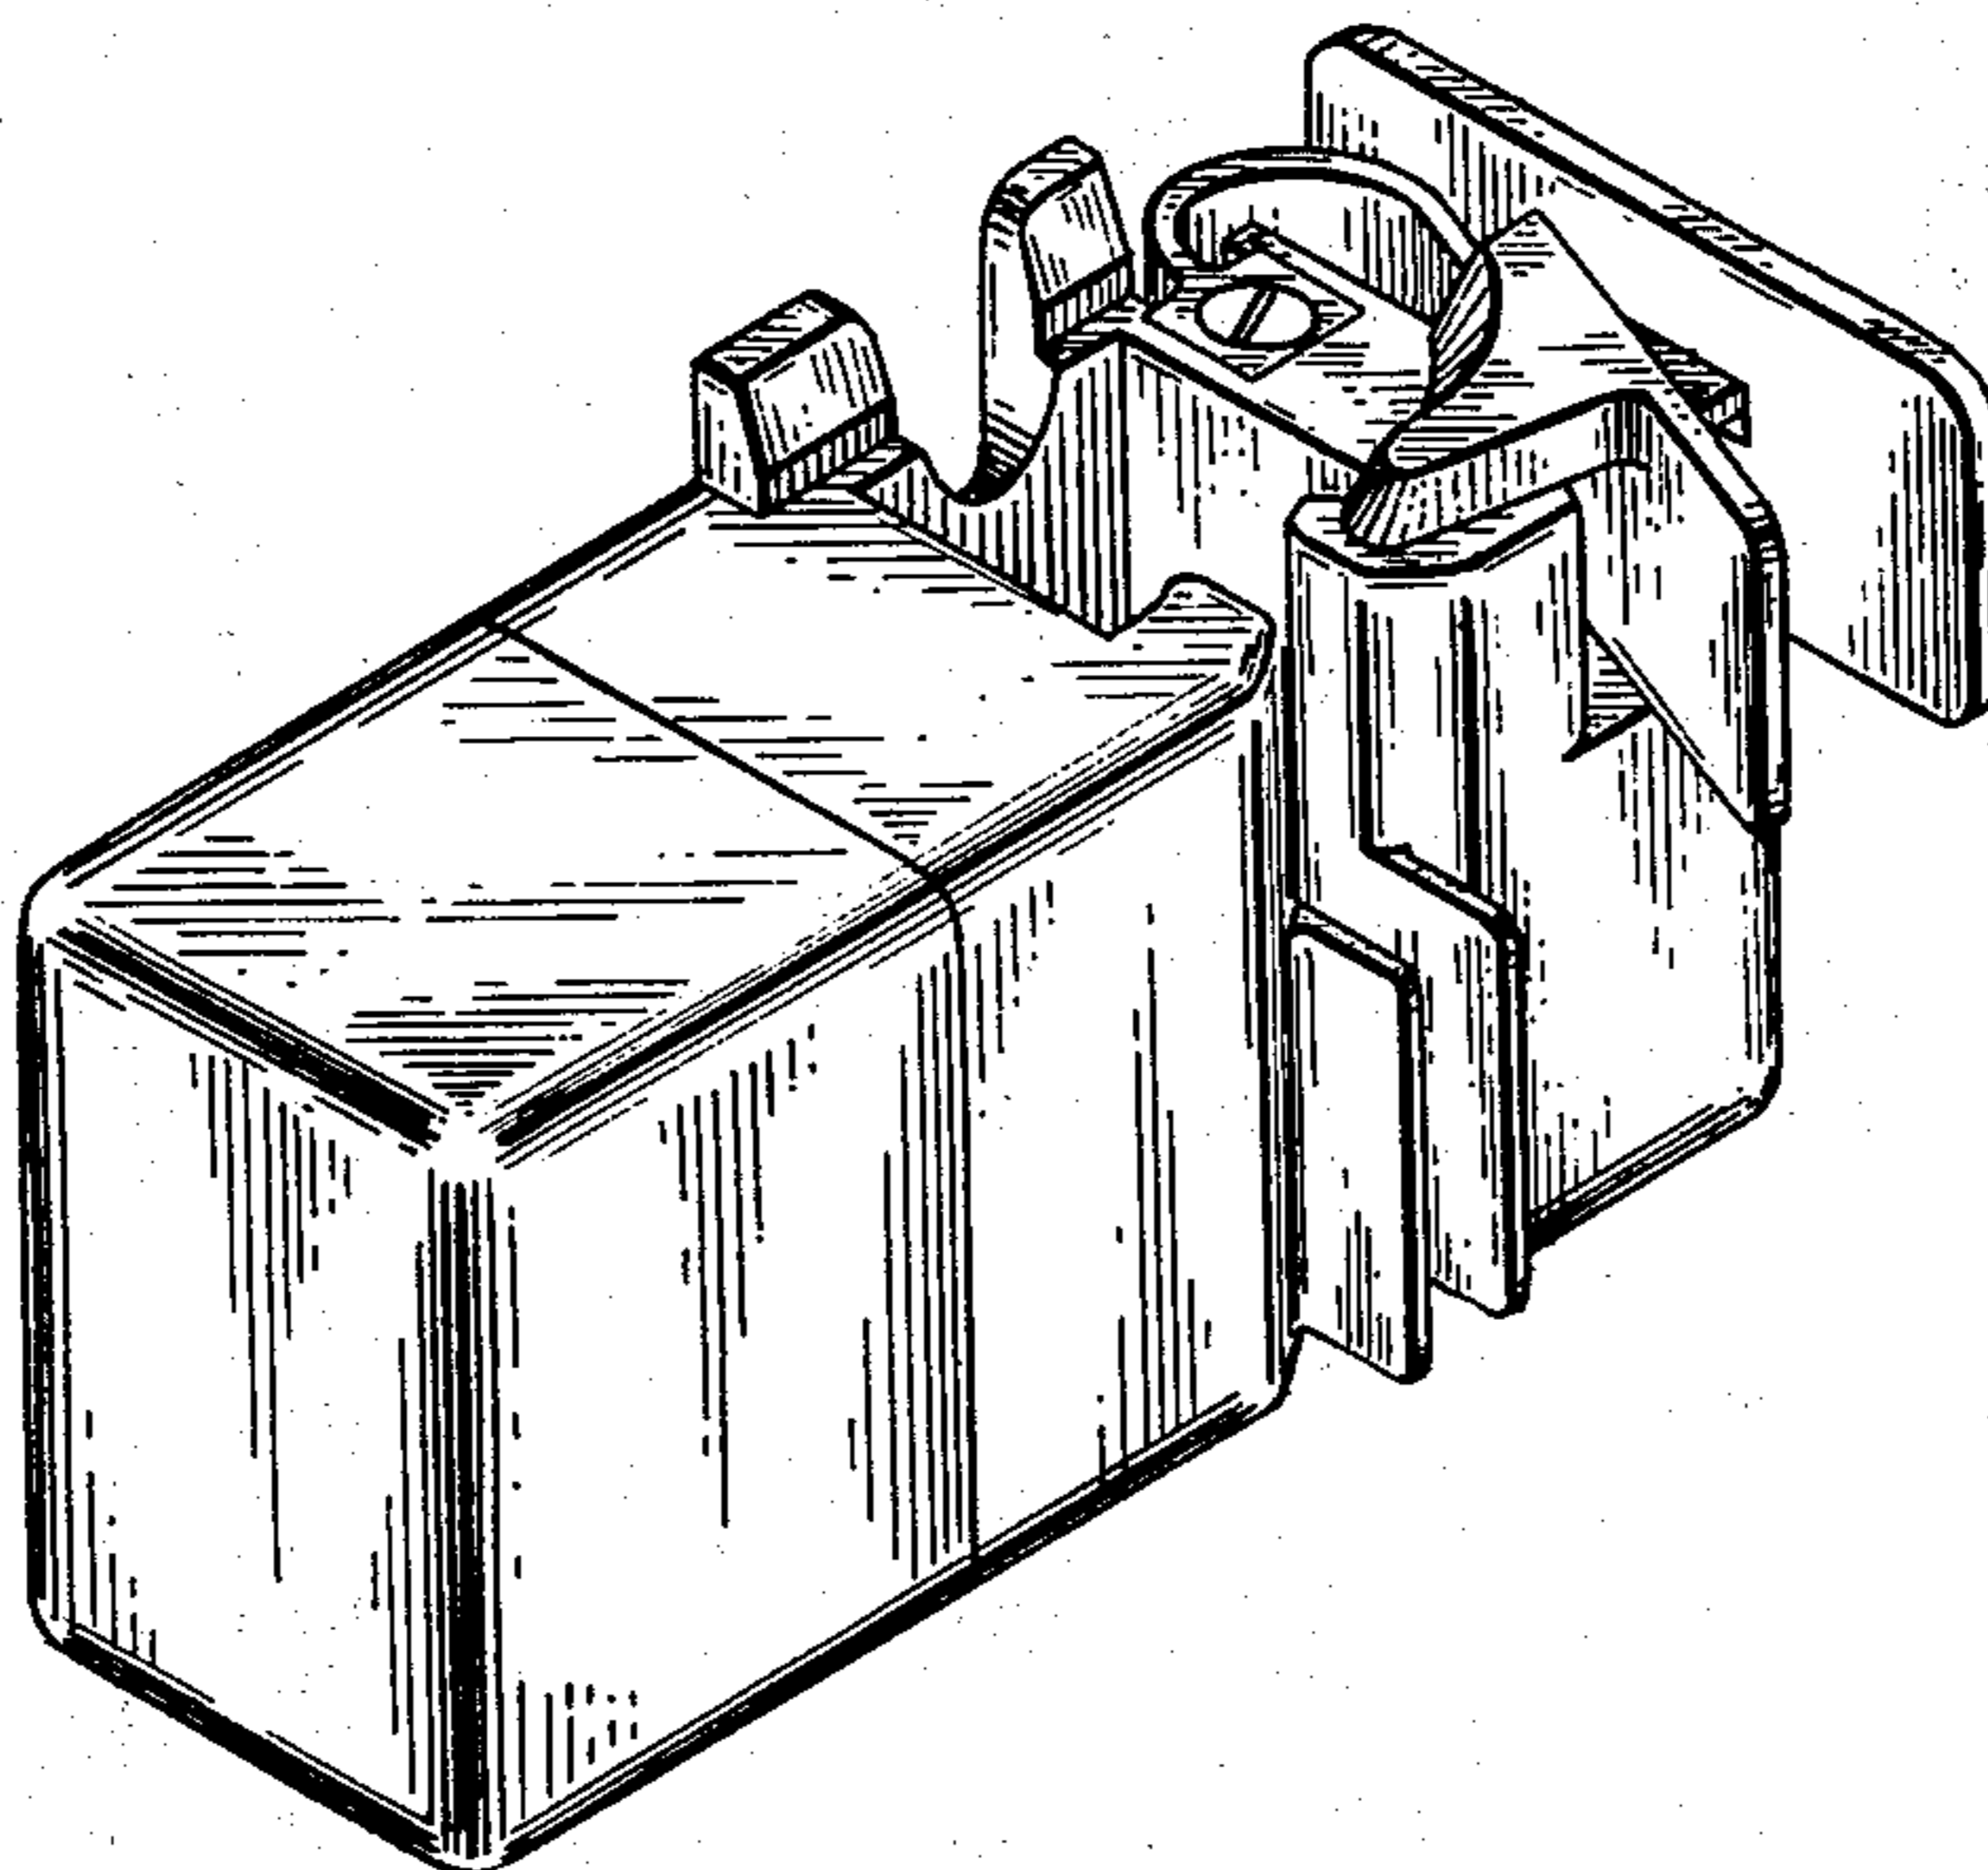


*Fig. 1.*

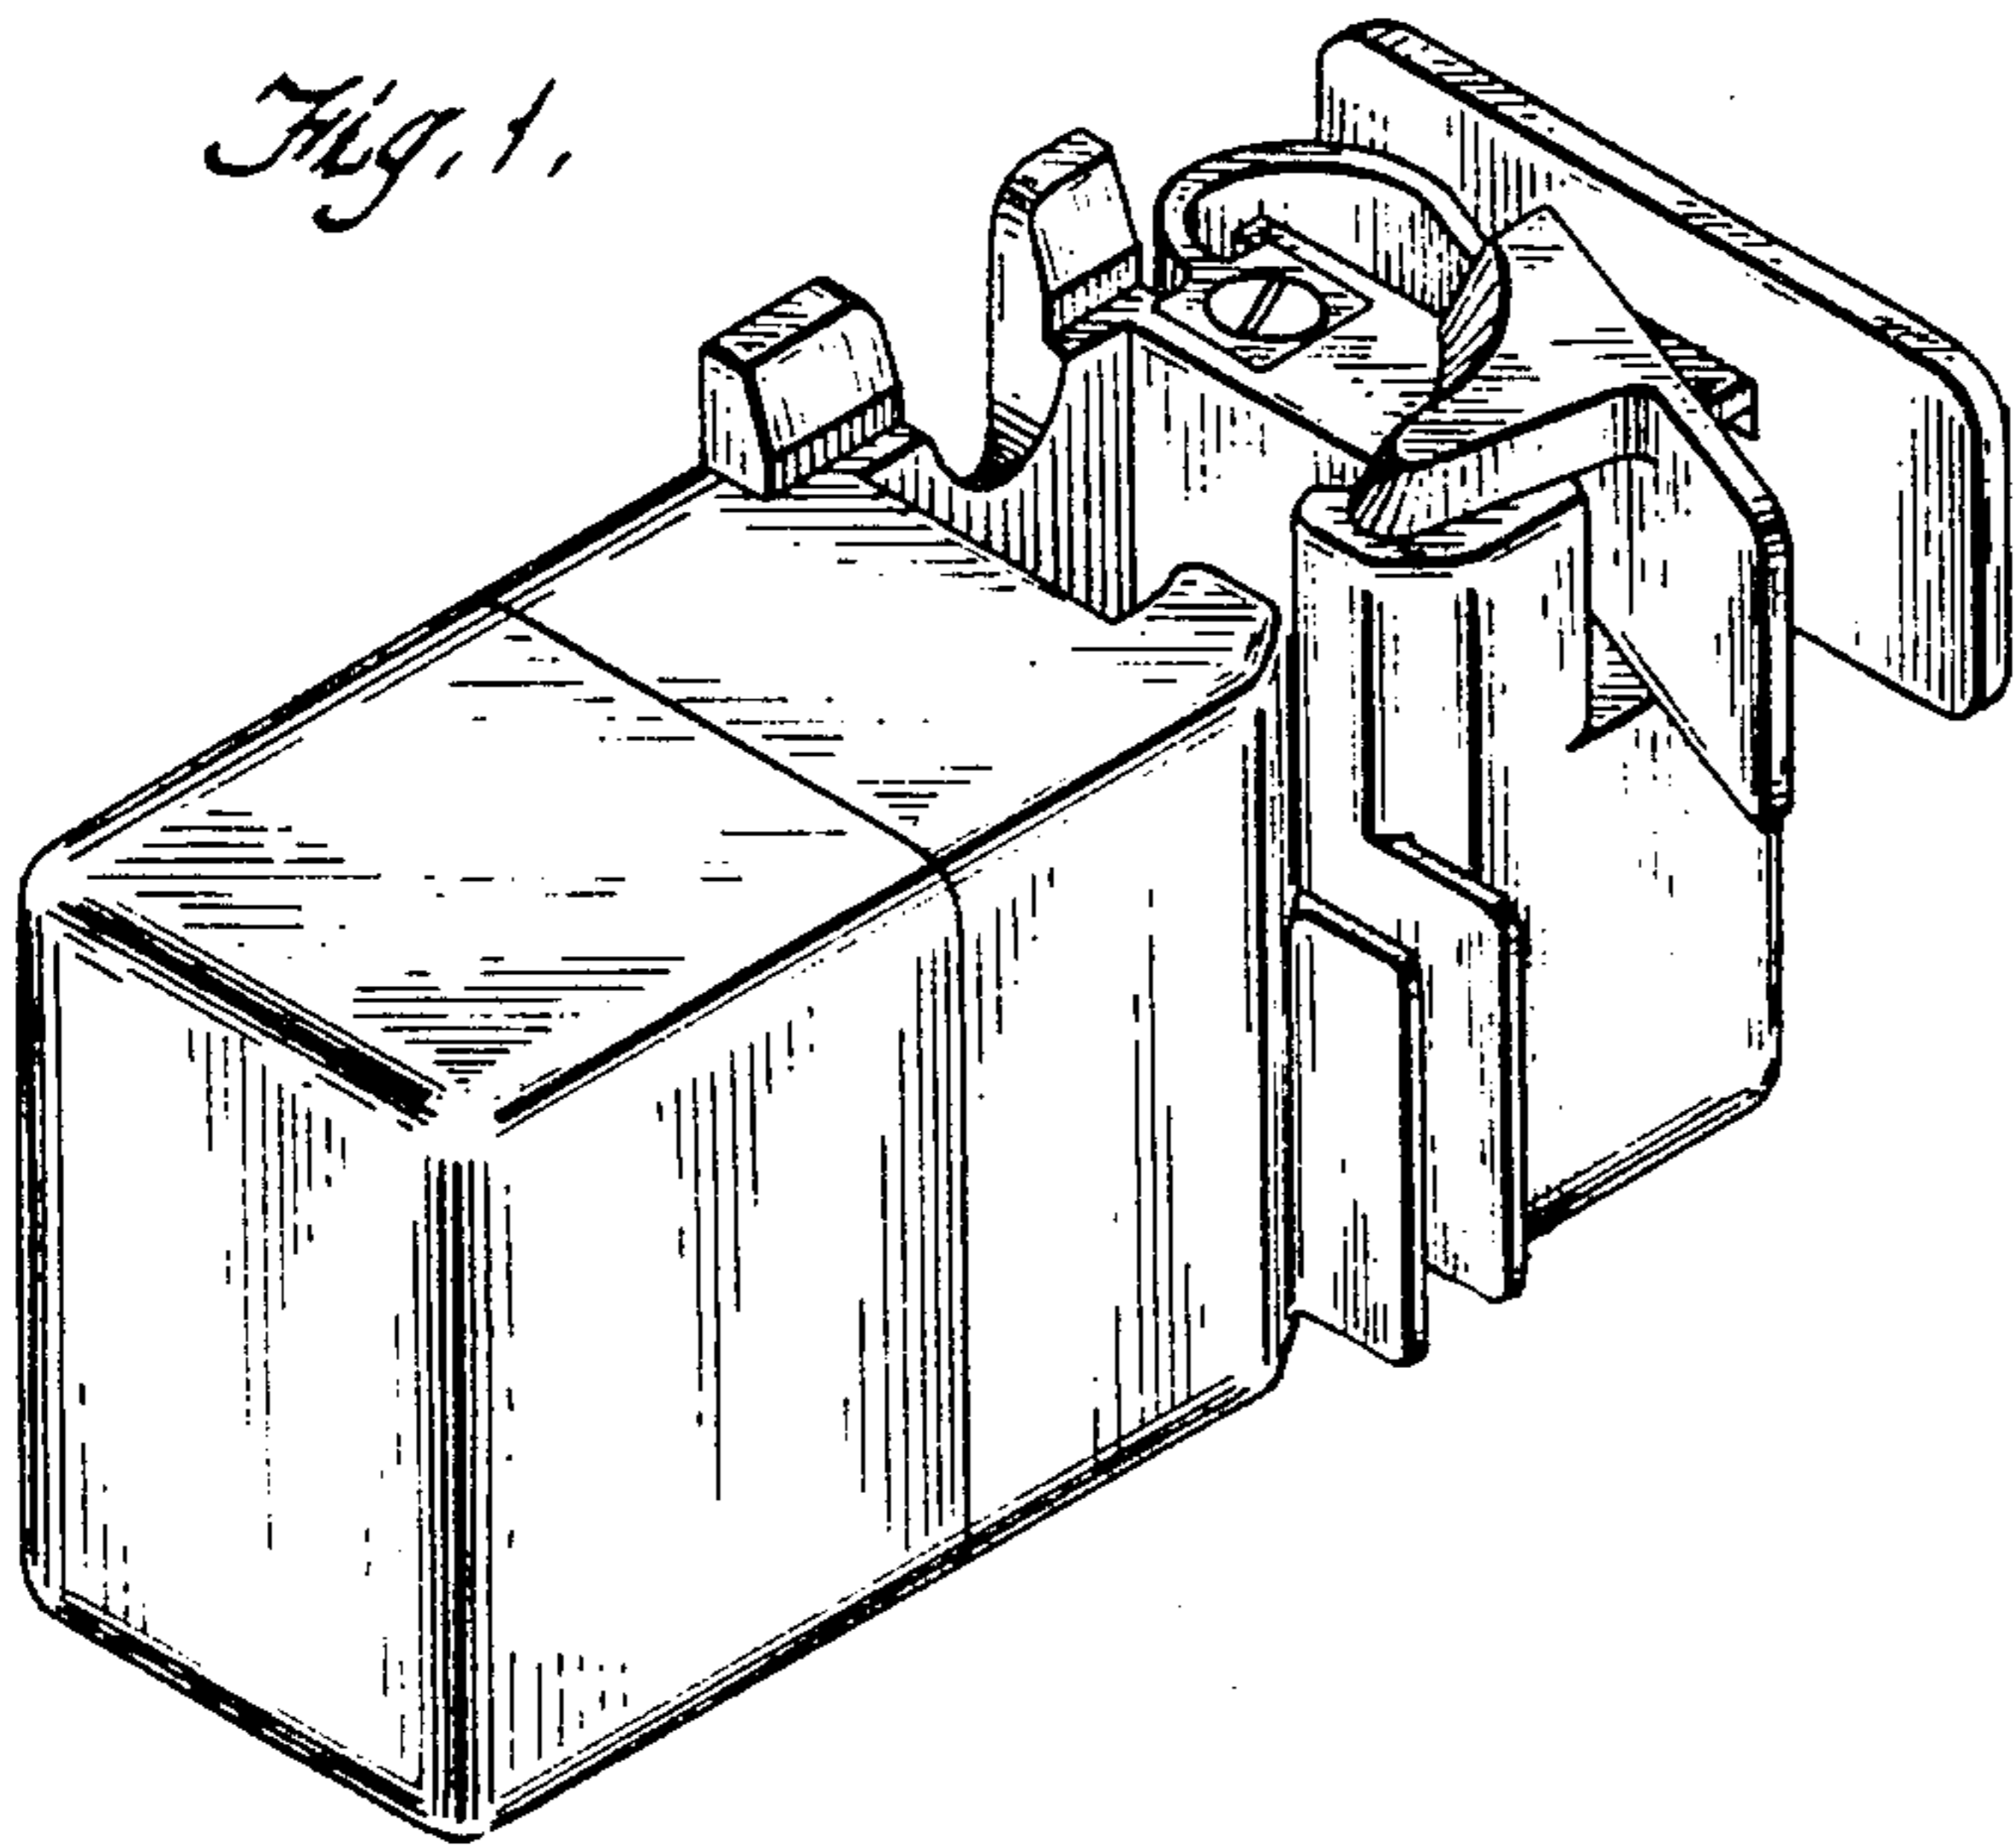

*Fig. 2.*

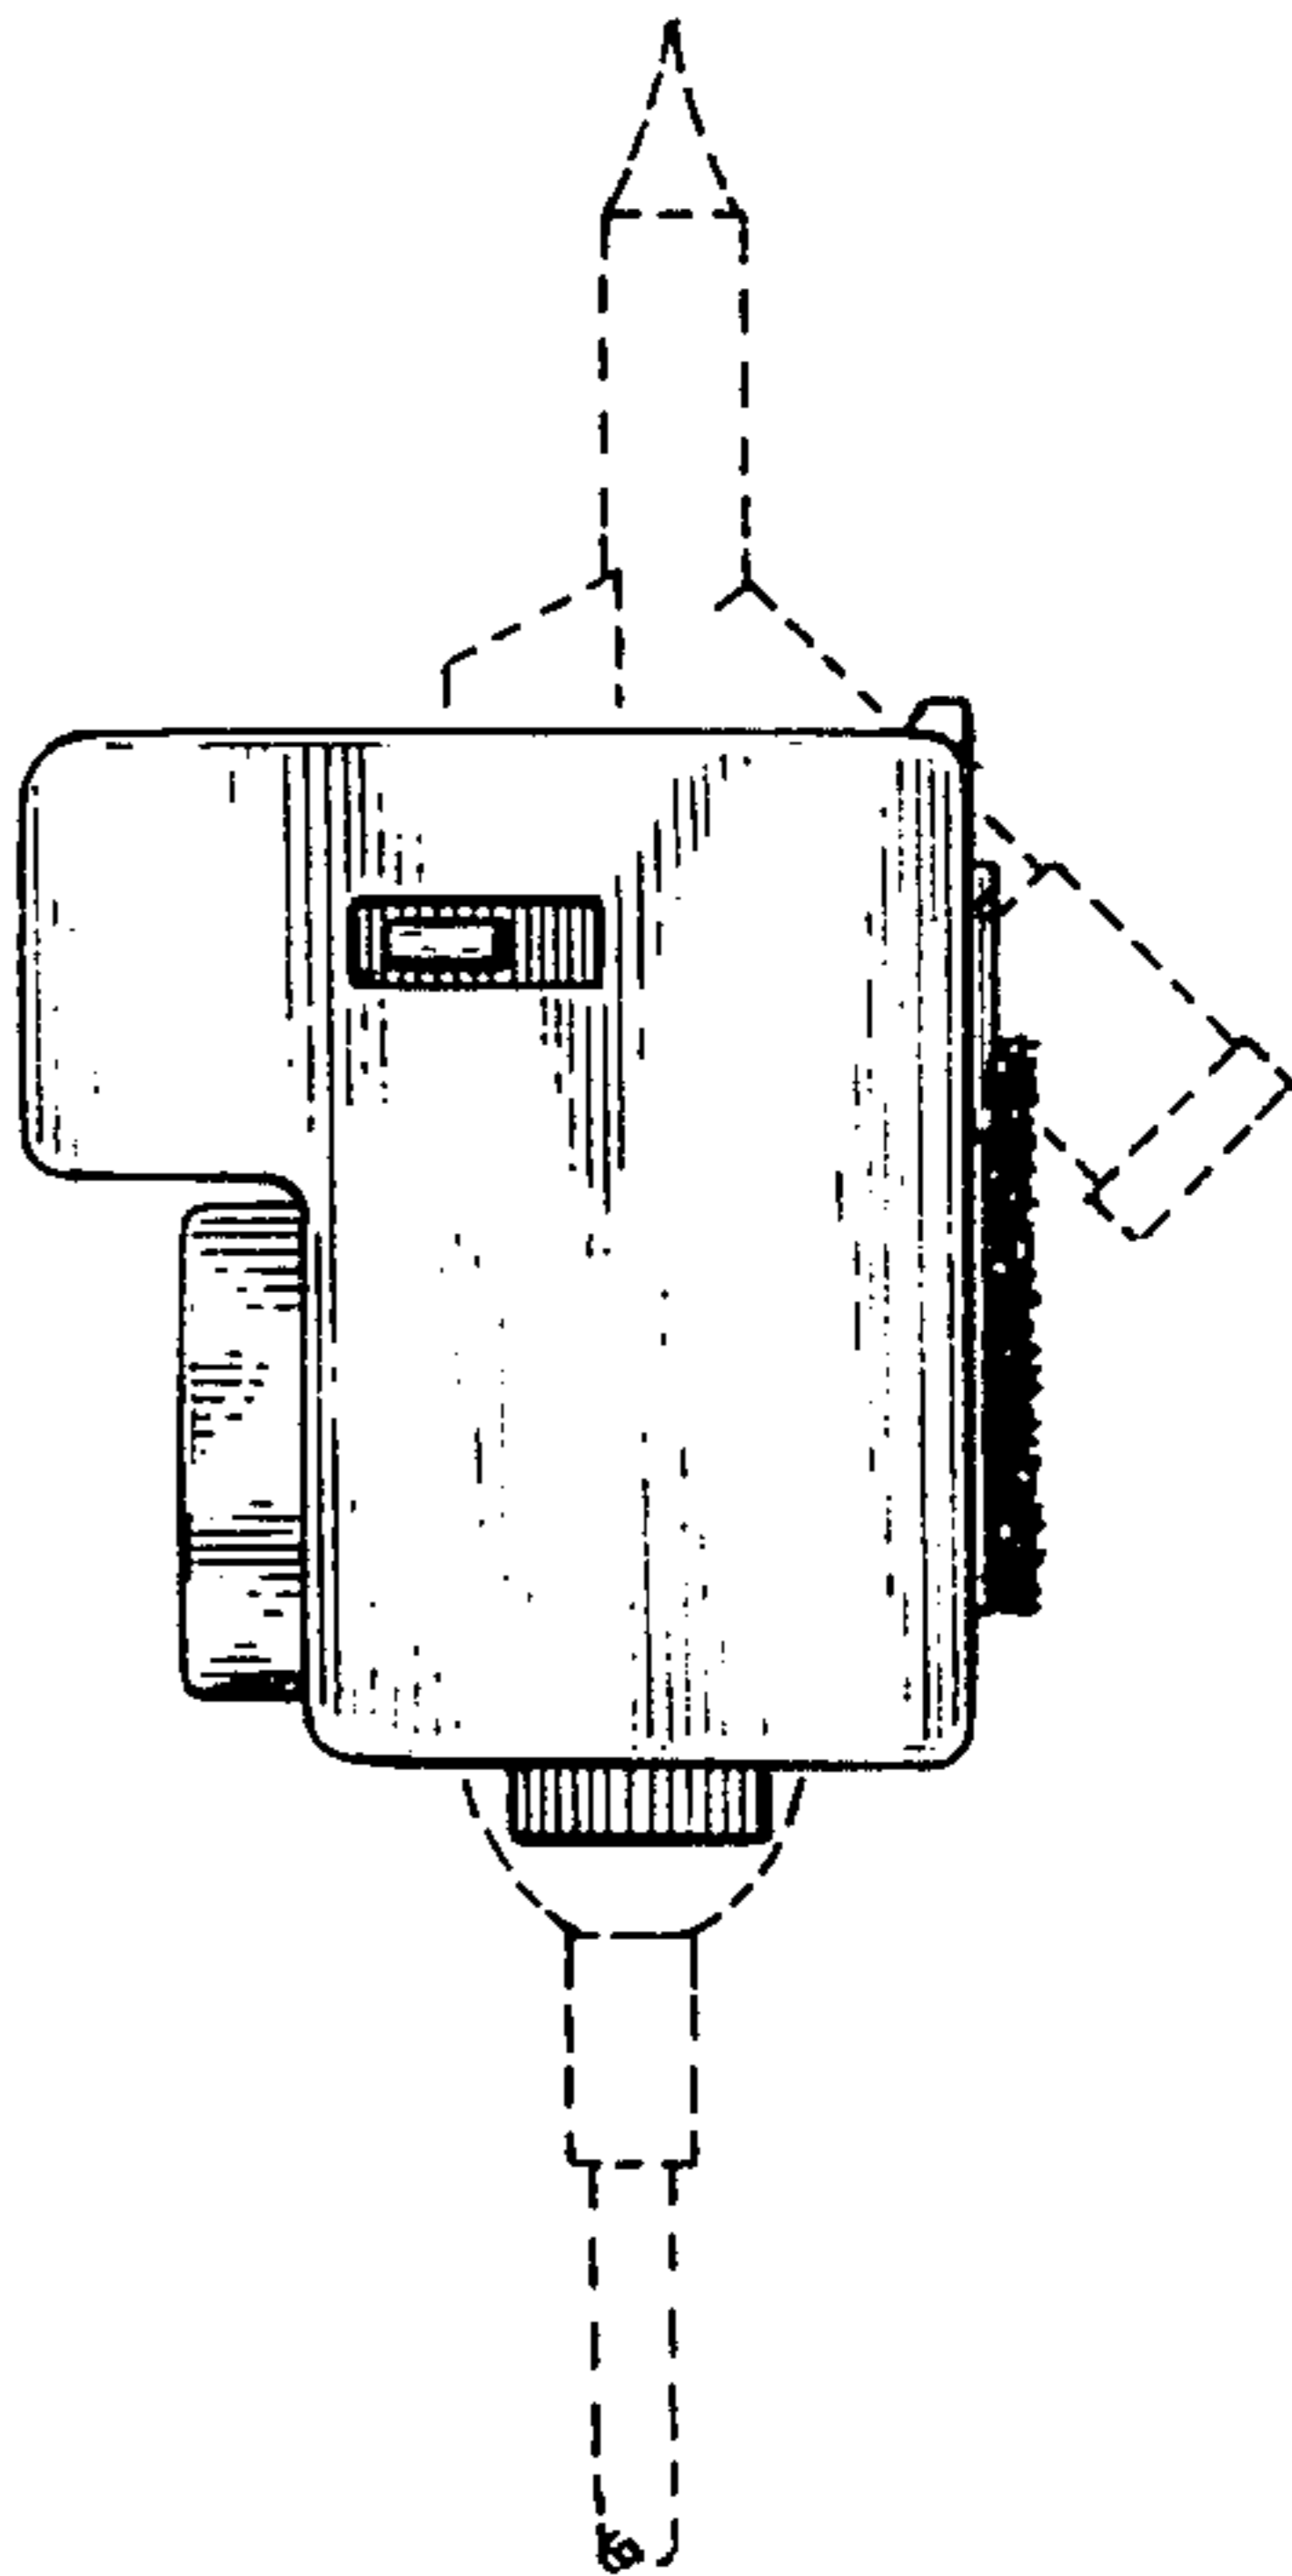

*Fig. 3.*

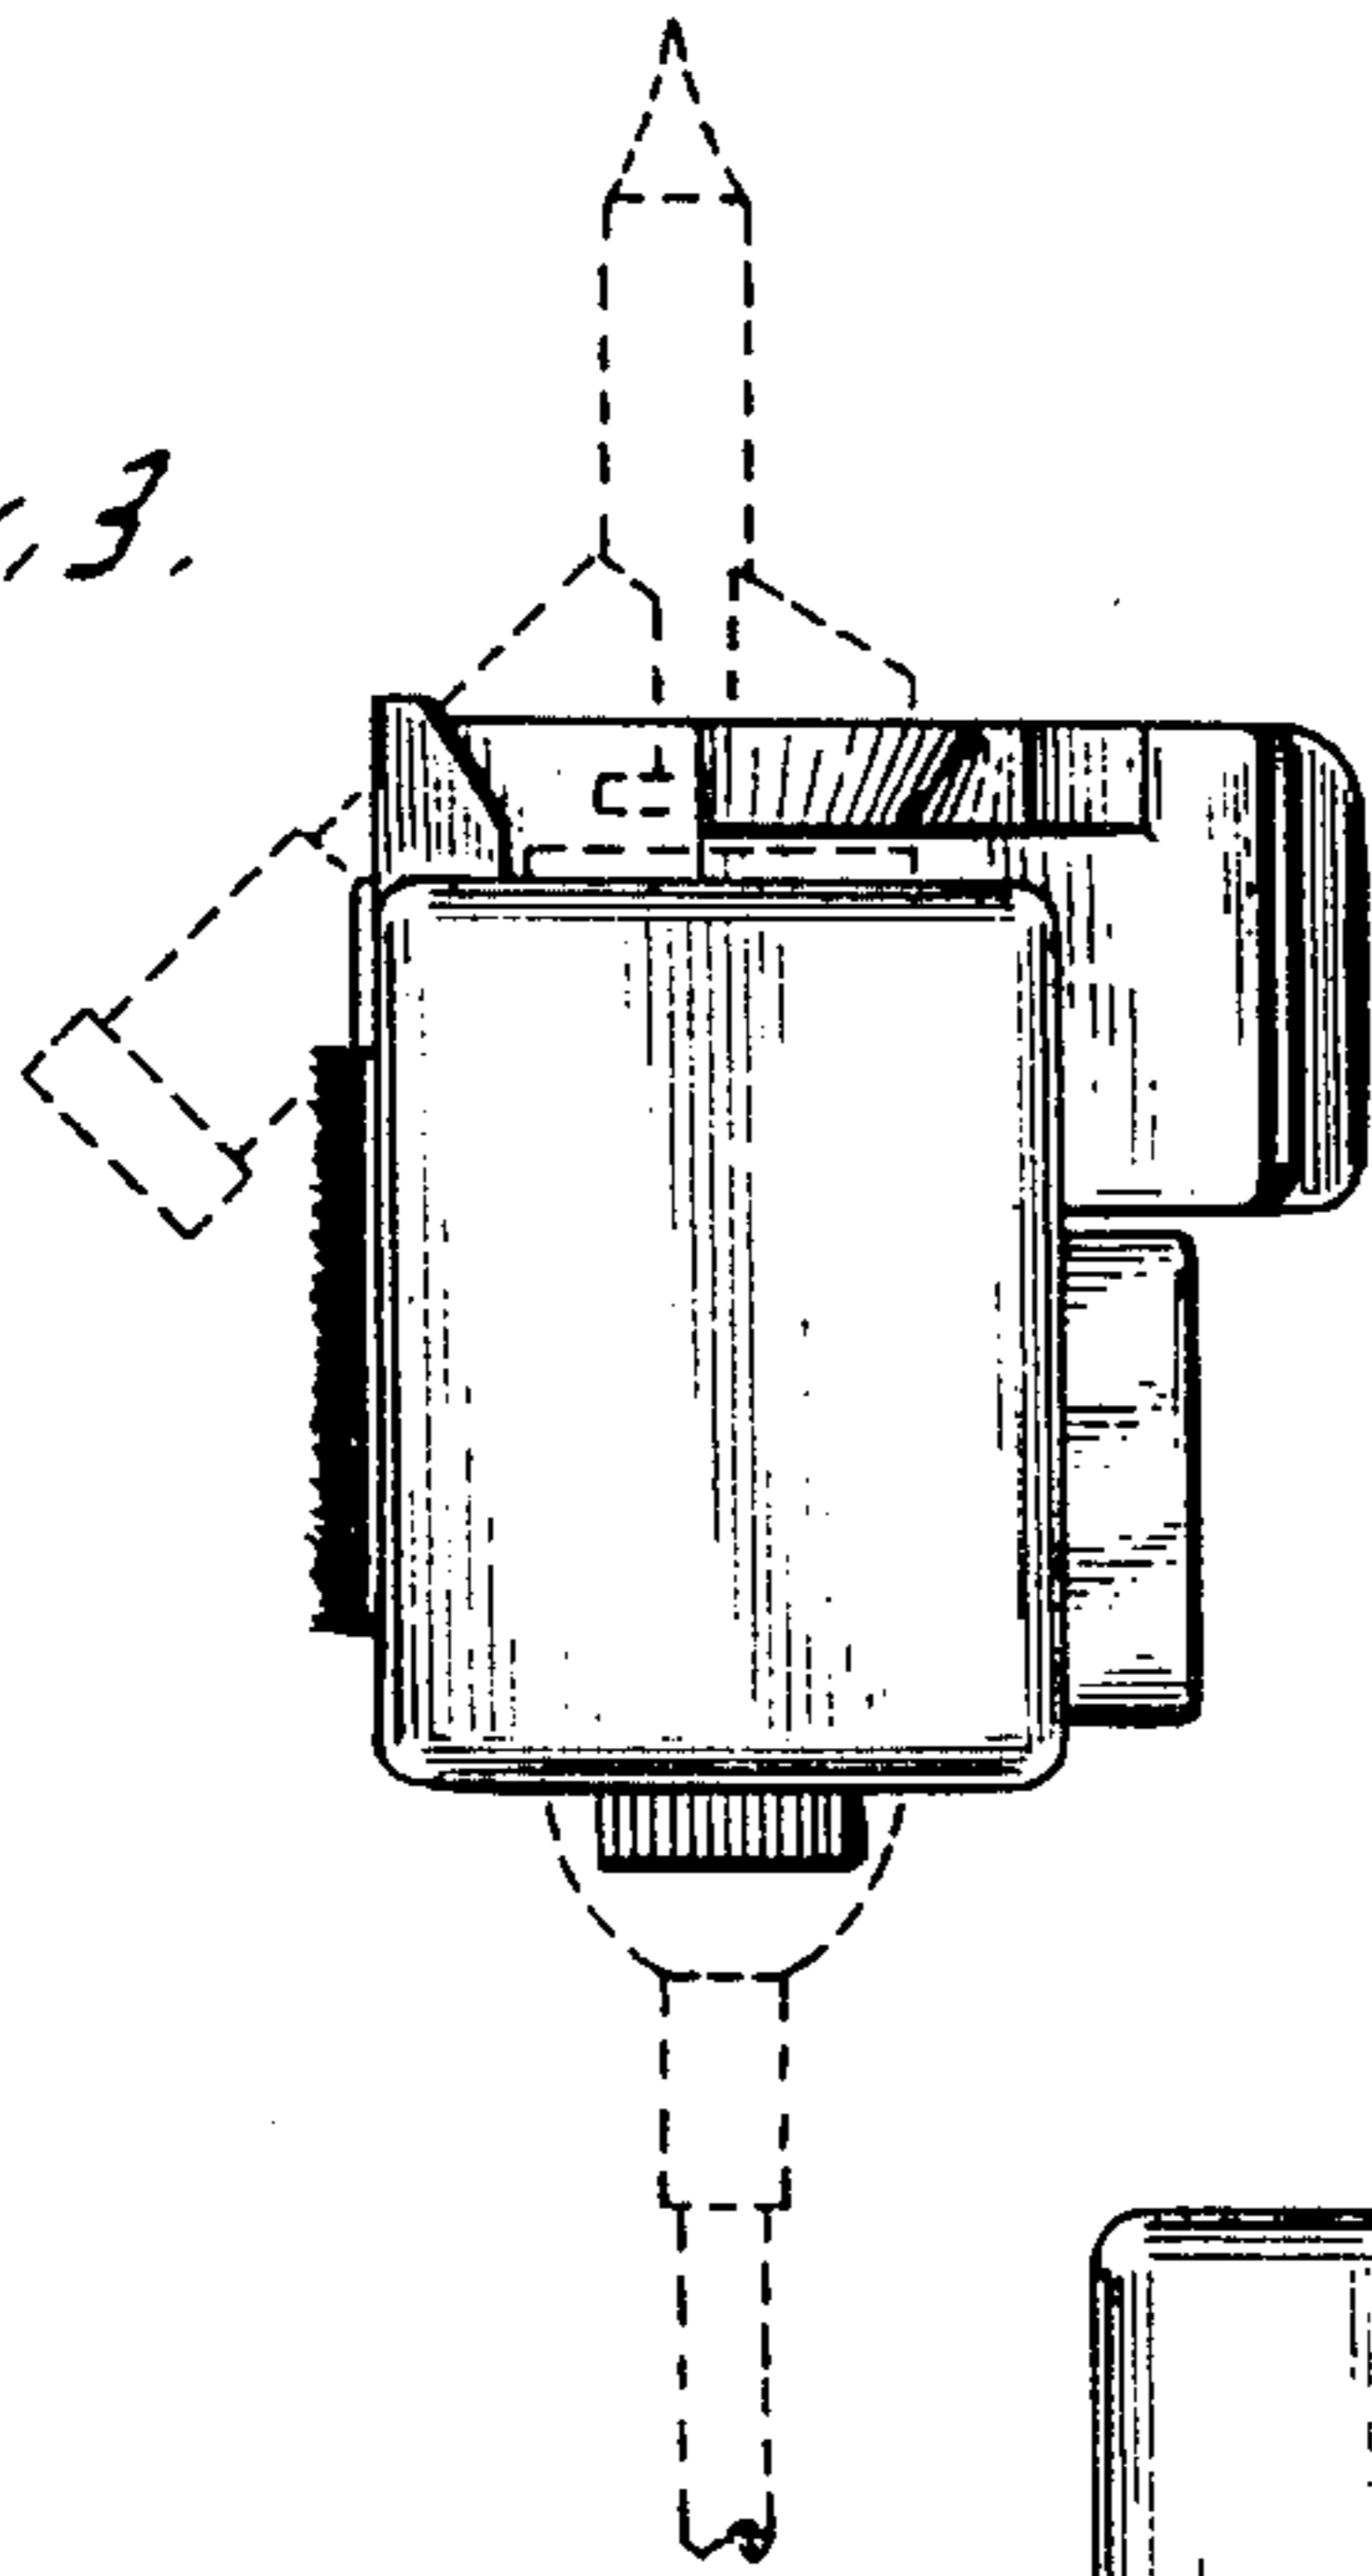

*Fig. 4.*

