

[54] AUTOMATIC CHEMICAL ANALYZER

[75] Inventors: Yasuo Hattori, Hachioji; Masaharu Kame, Sagamihara; Masahiko Sakurada, Machida, all of Japan

[73] Assignee: Olympus Optical Company Ltd., Japan

[**] Term: 14 Years

[21] Appl. No.: 483,112

[22] Filed: Apr. 8, 1983

[30] Foreign Application Priority Data

Oct. 19, 1982 [JP] Japan SHO/57-47731

[52] U.S. Cl. D10/81; D24/1.1

[58] Field of Search D10/81; D24/1.1, 8, D24/17; 422/63-67; 356/39-41

[56] References Cited

U.S. PATENT DOCUMENTS

D. 228,454 9/1973 Amar et al. D24/1.1
D. 248,488 7/1978 Ashcraft et al. D24/1.1
D. 264,873 6/1982 Olson et al. D10/81 X

4,039,287 8/1977 Moran 422/65

FOREIGN PATENT DOCUMENTS

1417852 12/1975 United Kingdom 356/39

Primary Examiner—Bernard Ansher

Assistant Examiner—Terry Pfeffer

Attorney, Agent, or Firm—Ostrolenk, Faber, Gerb & Soffen

[57] CLAIM

The ornamental design for an automatic chemical analyzer, as shown and described.

DESCRIPTION

FIG. 1 is a front, top, and right side perspective view of an automatic chemical analyzer, showing our new design;

FIG. 2 is a rear, bottom, and left side perspective view thereof;

FIG. 3 is a front view thereof;

FIG. 4 is a rear view thereof;

FIG. 5 is a left side view thereof;

FIG. 6 is a right side view thereof;

FIG. 7 is a top view thereof; and

FIG. 8 is a bottom view thereof.

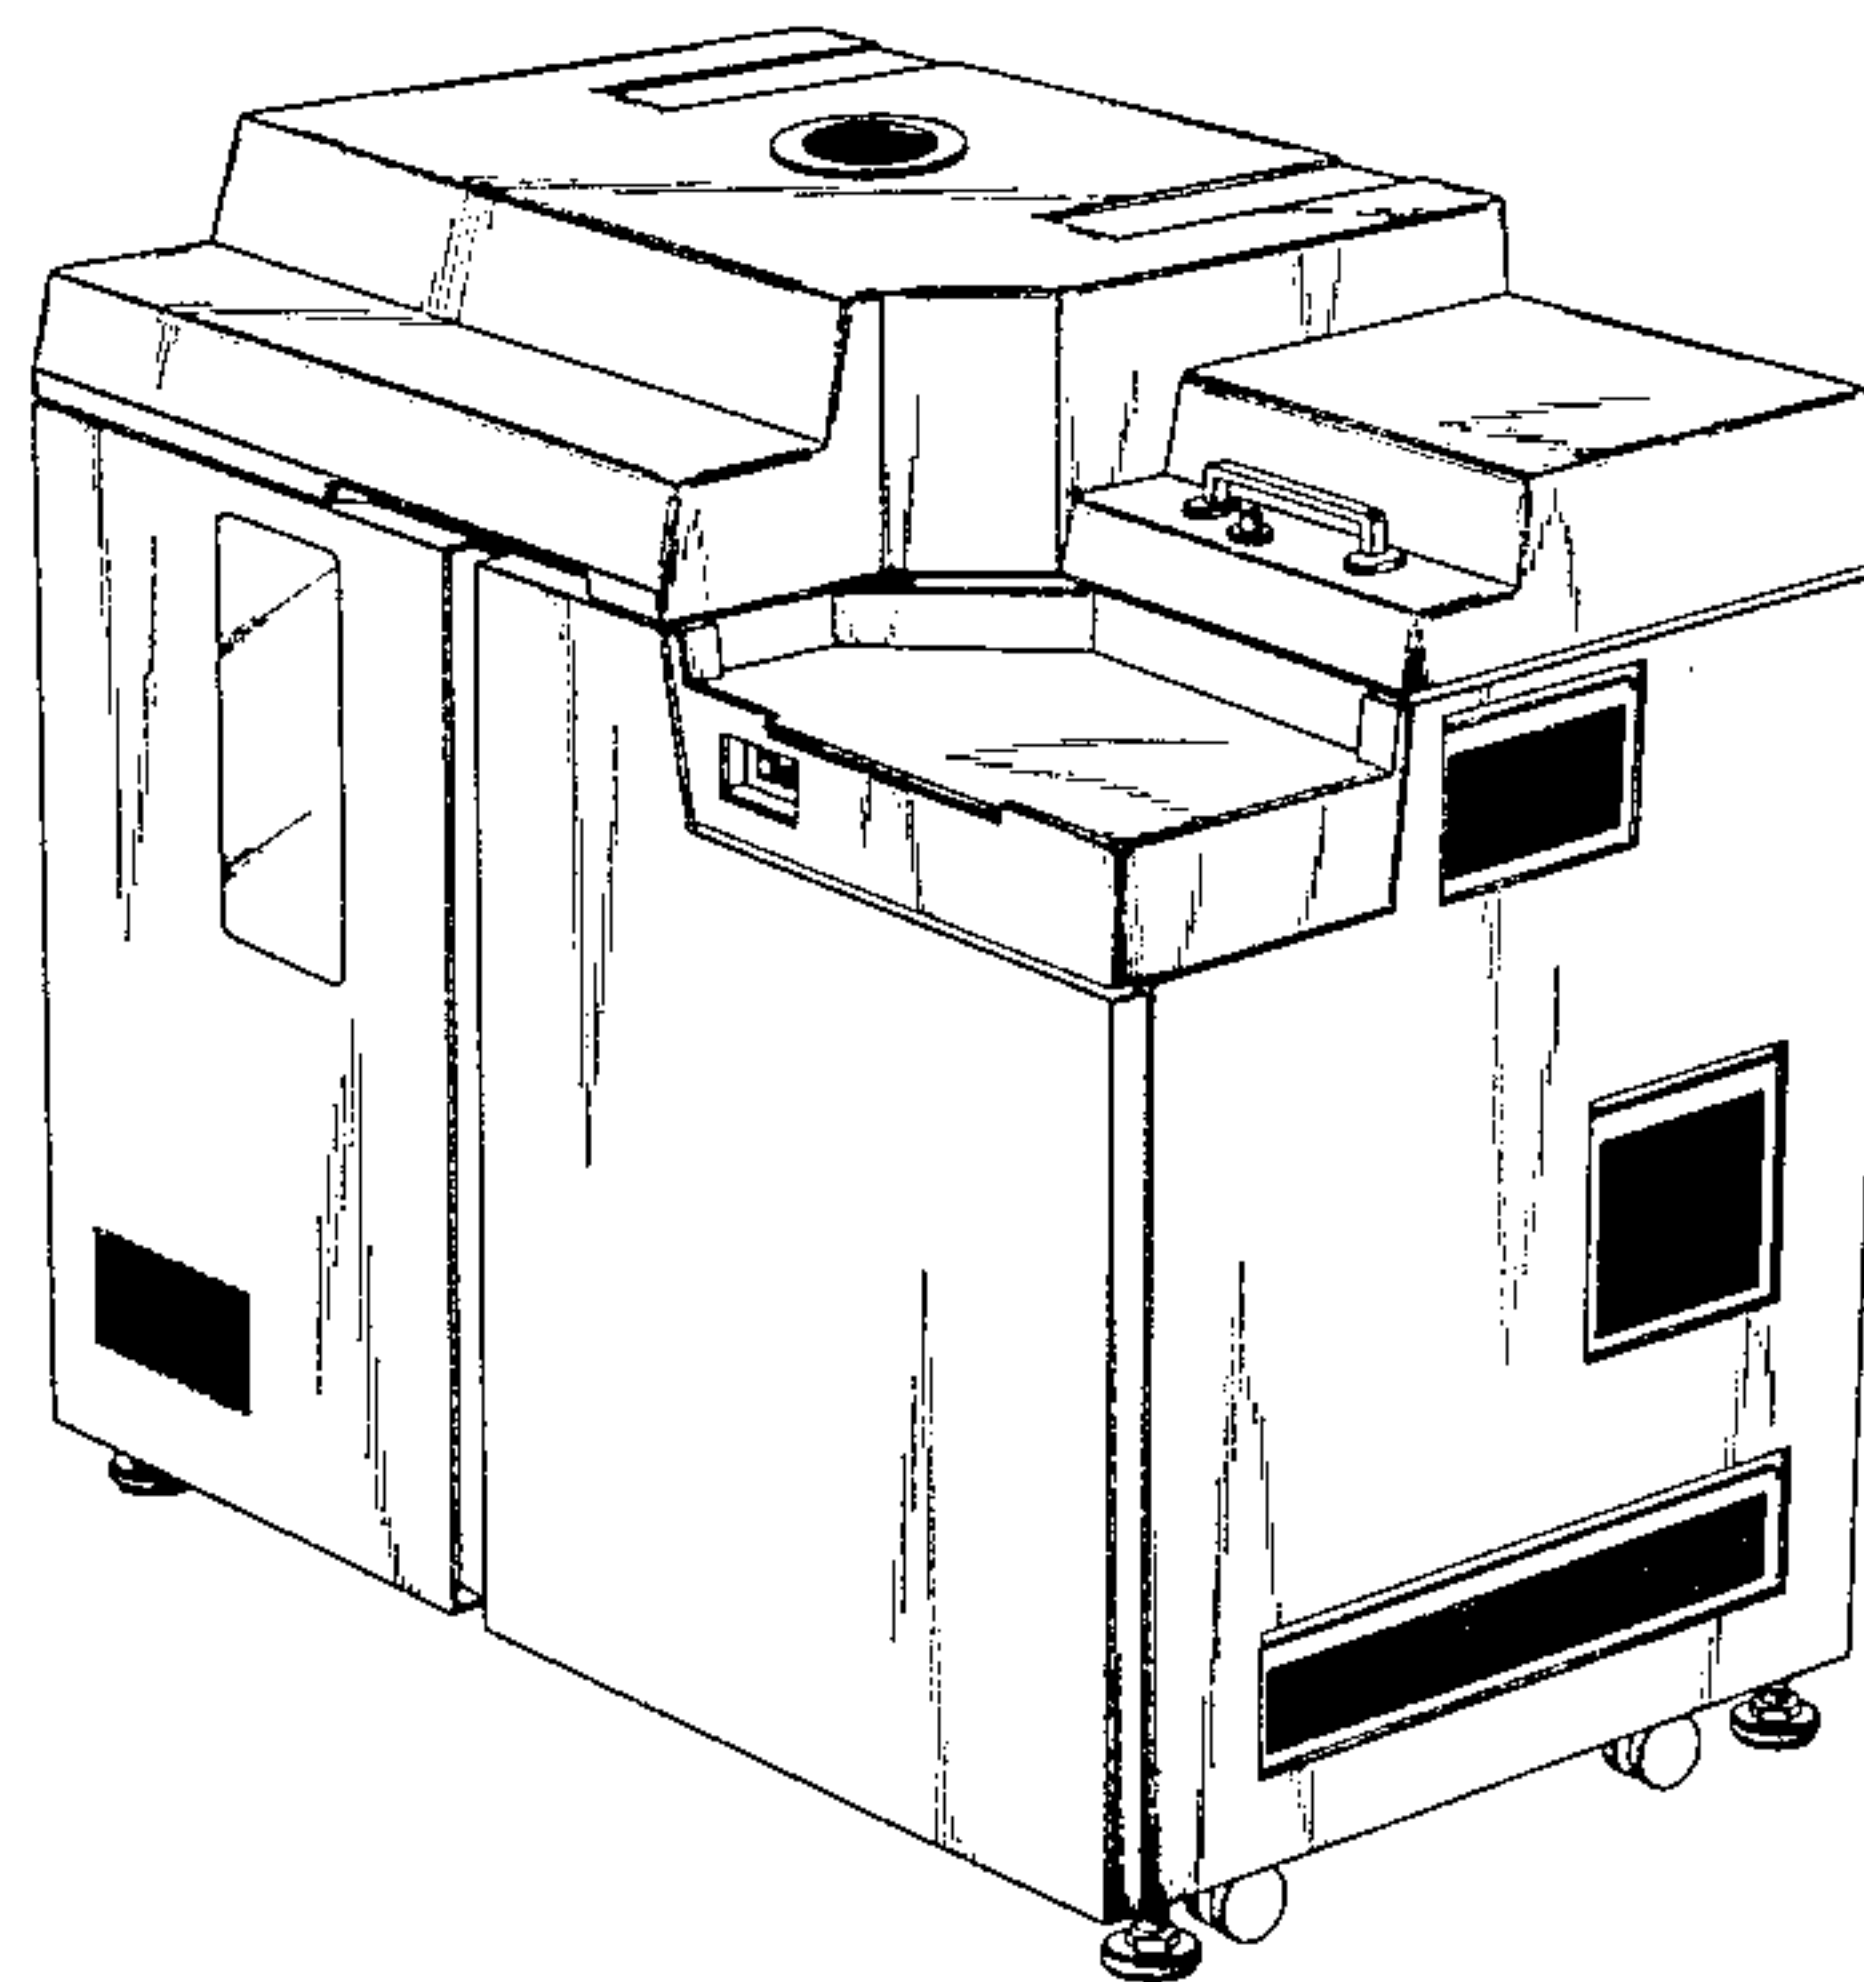


FIG. 1

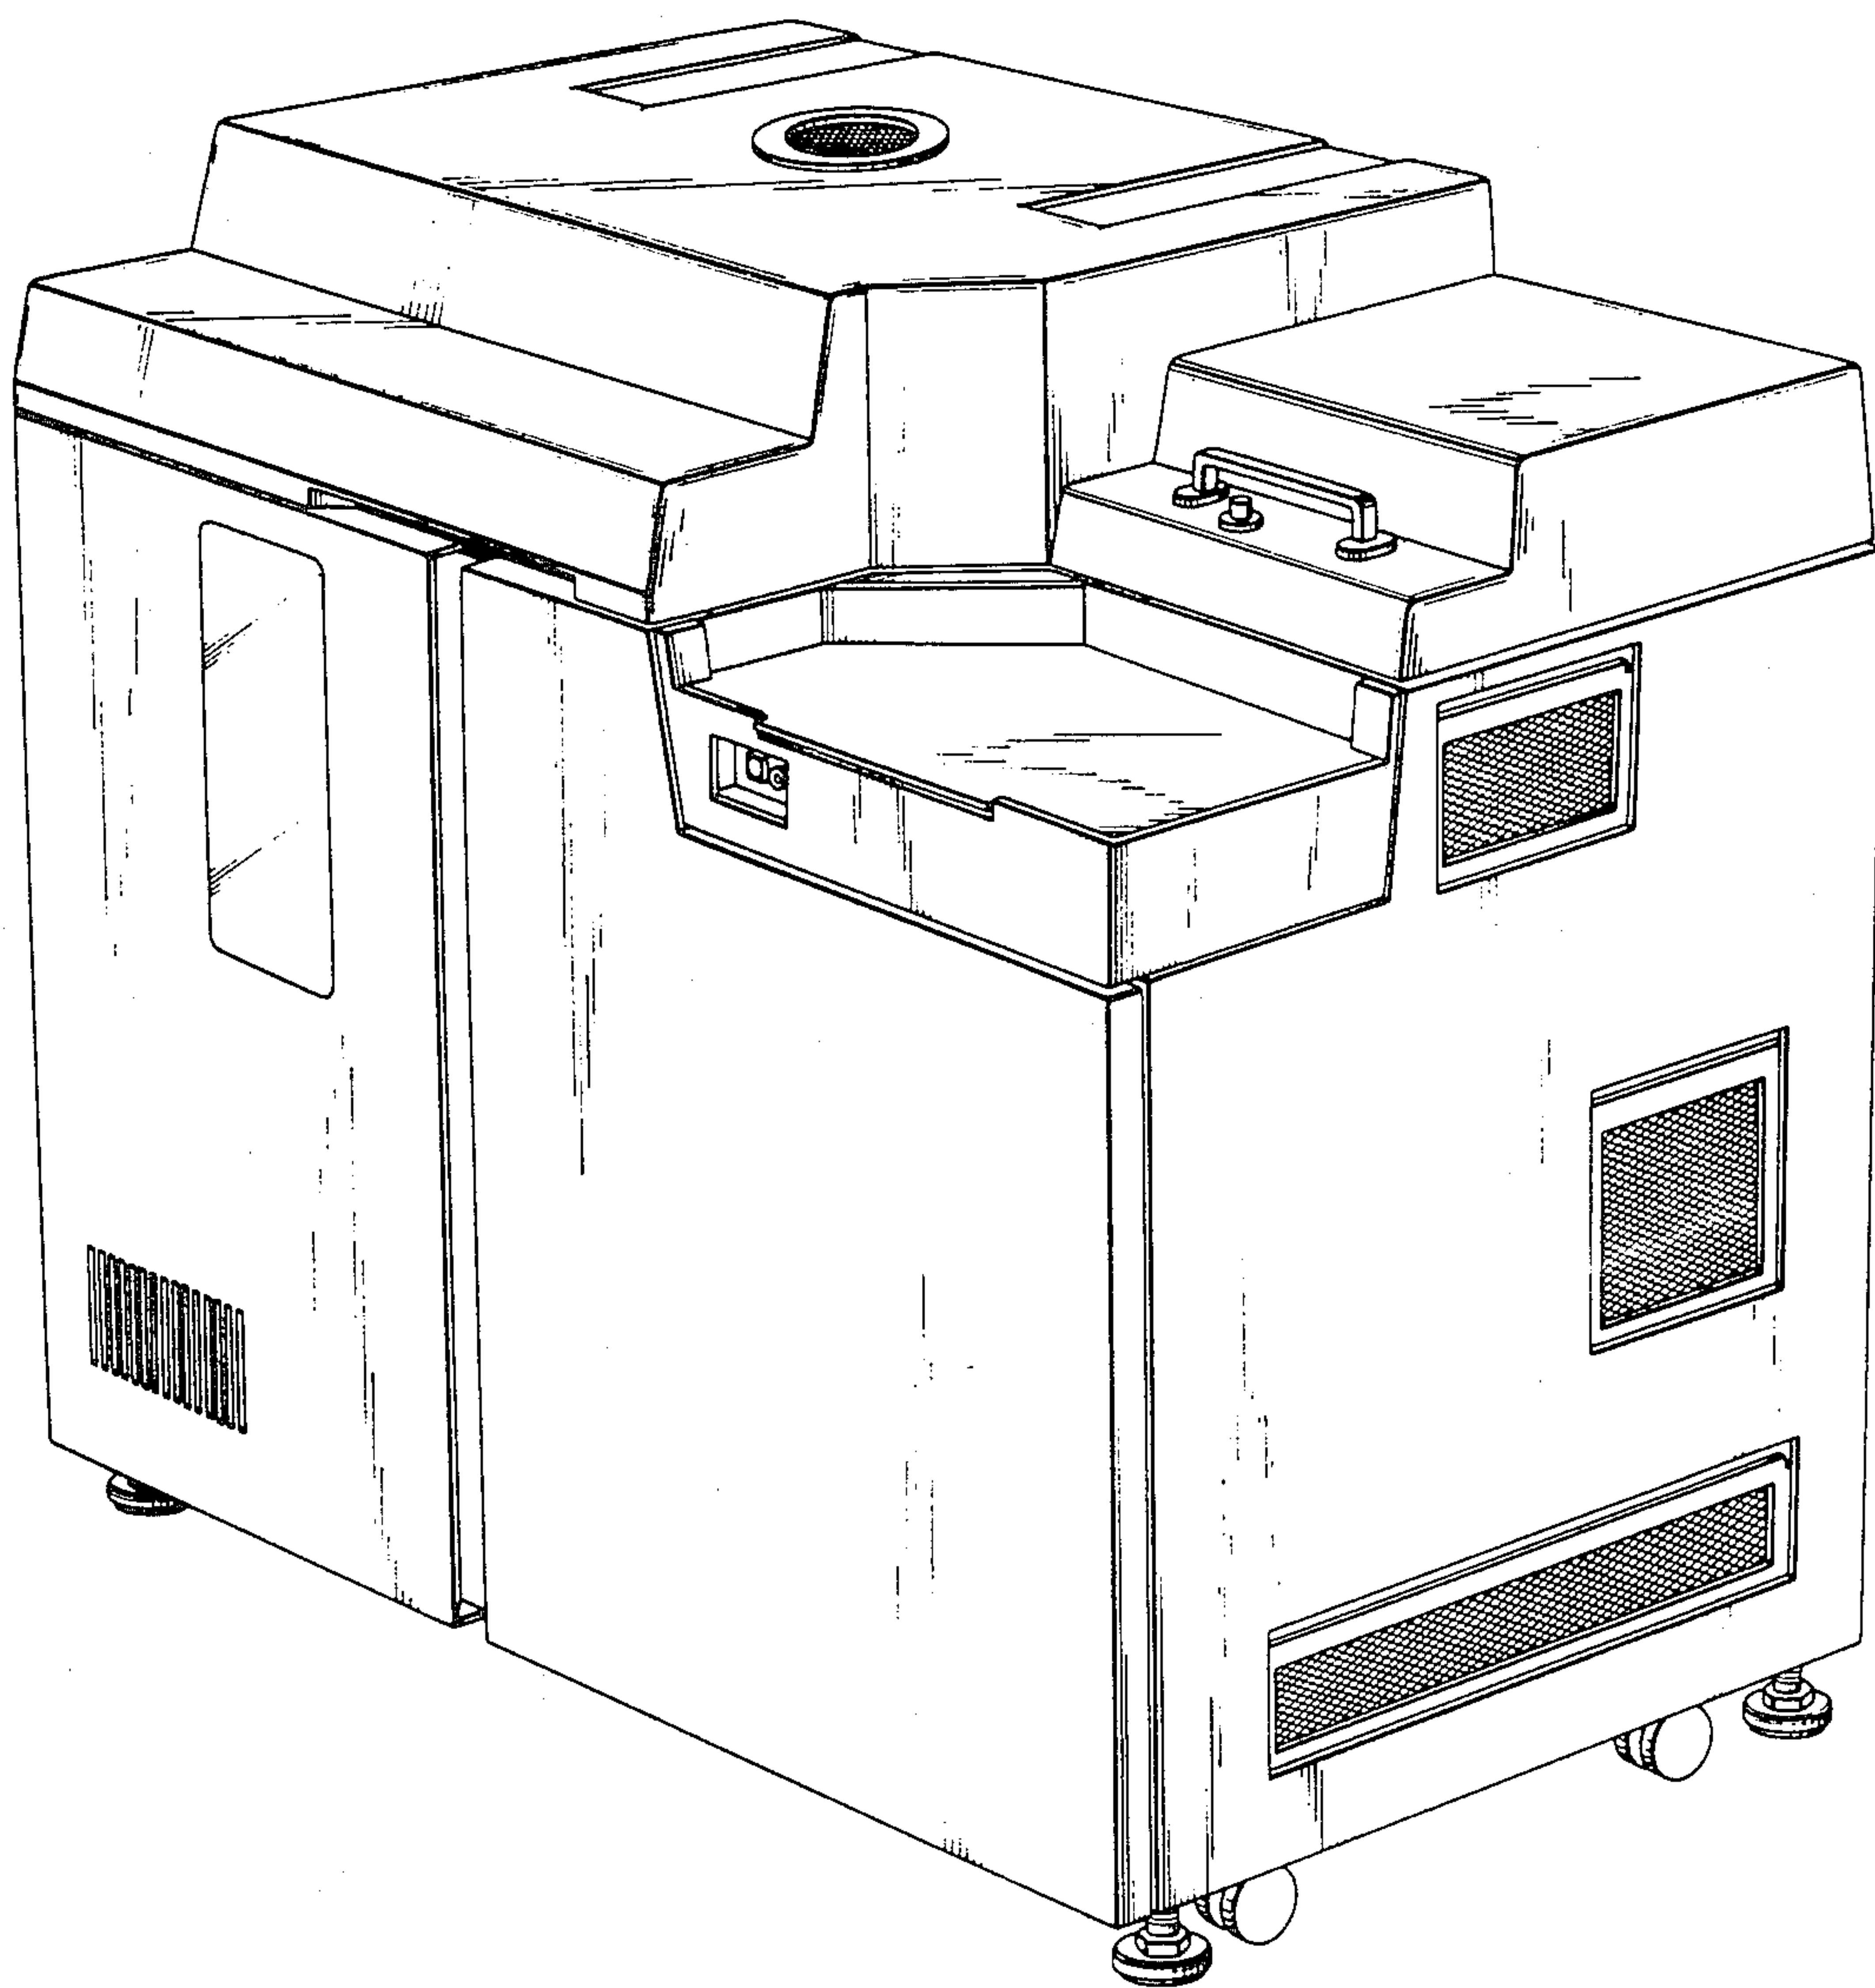


FIG. 2

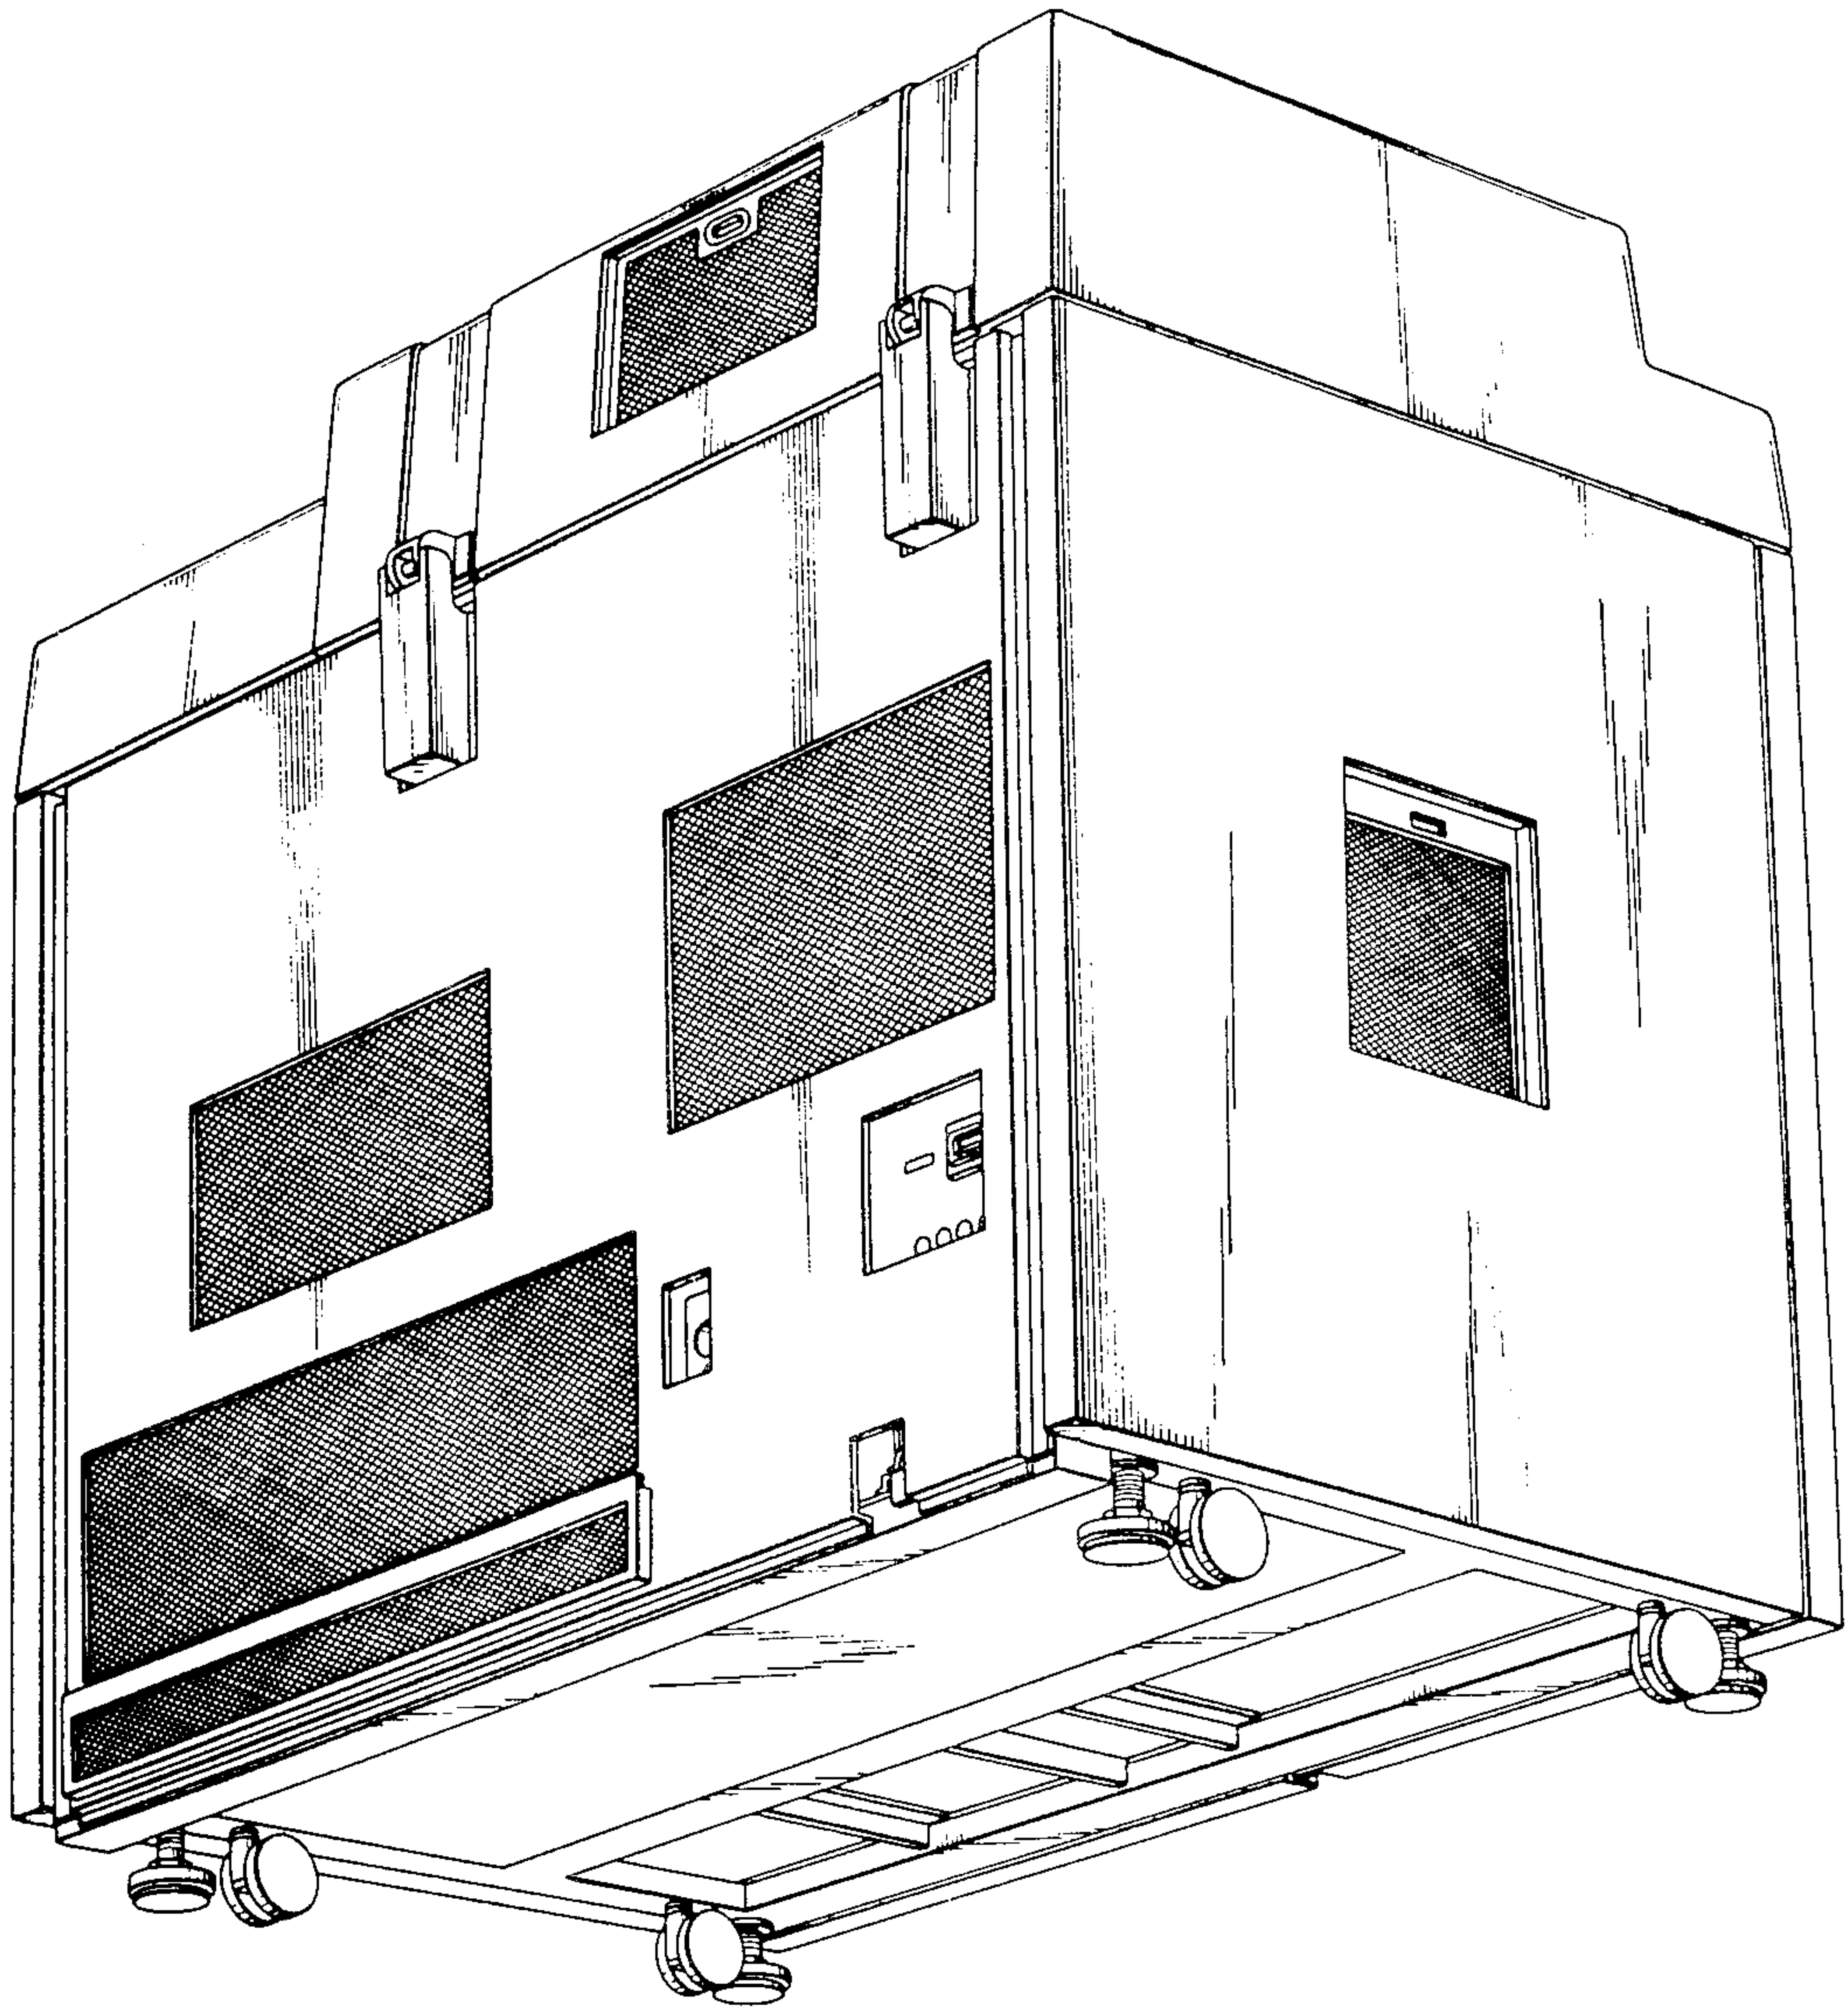


FIG. 3

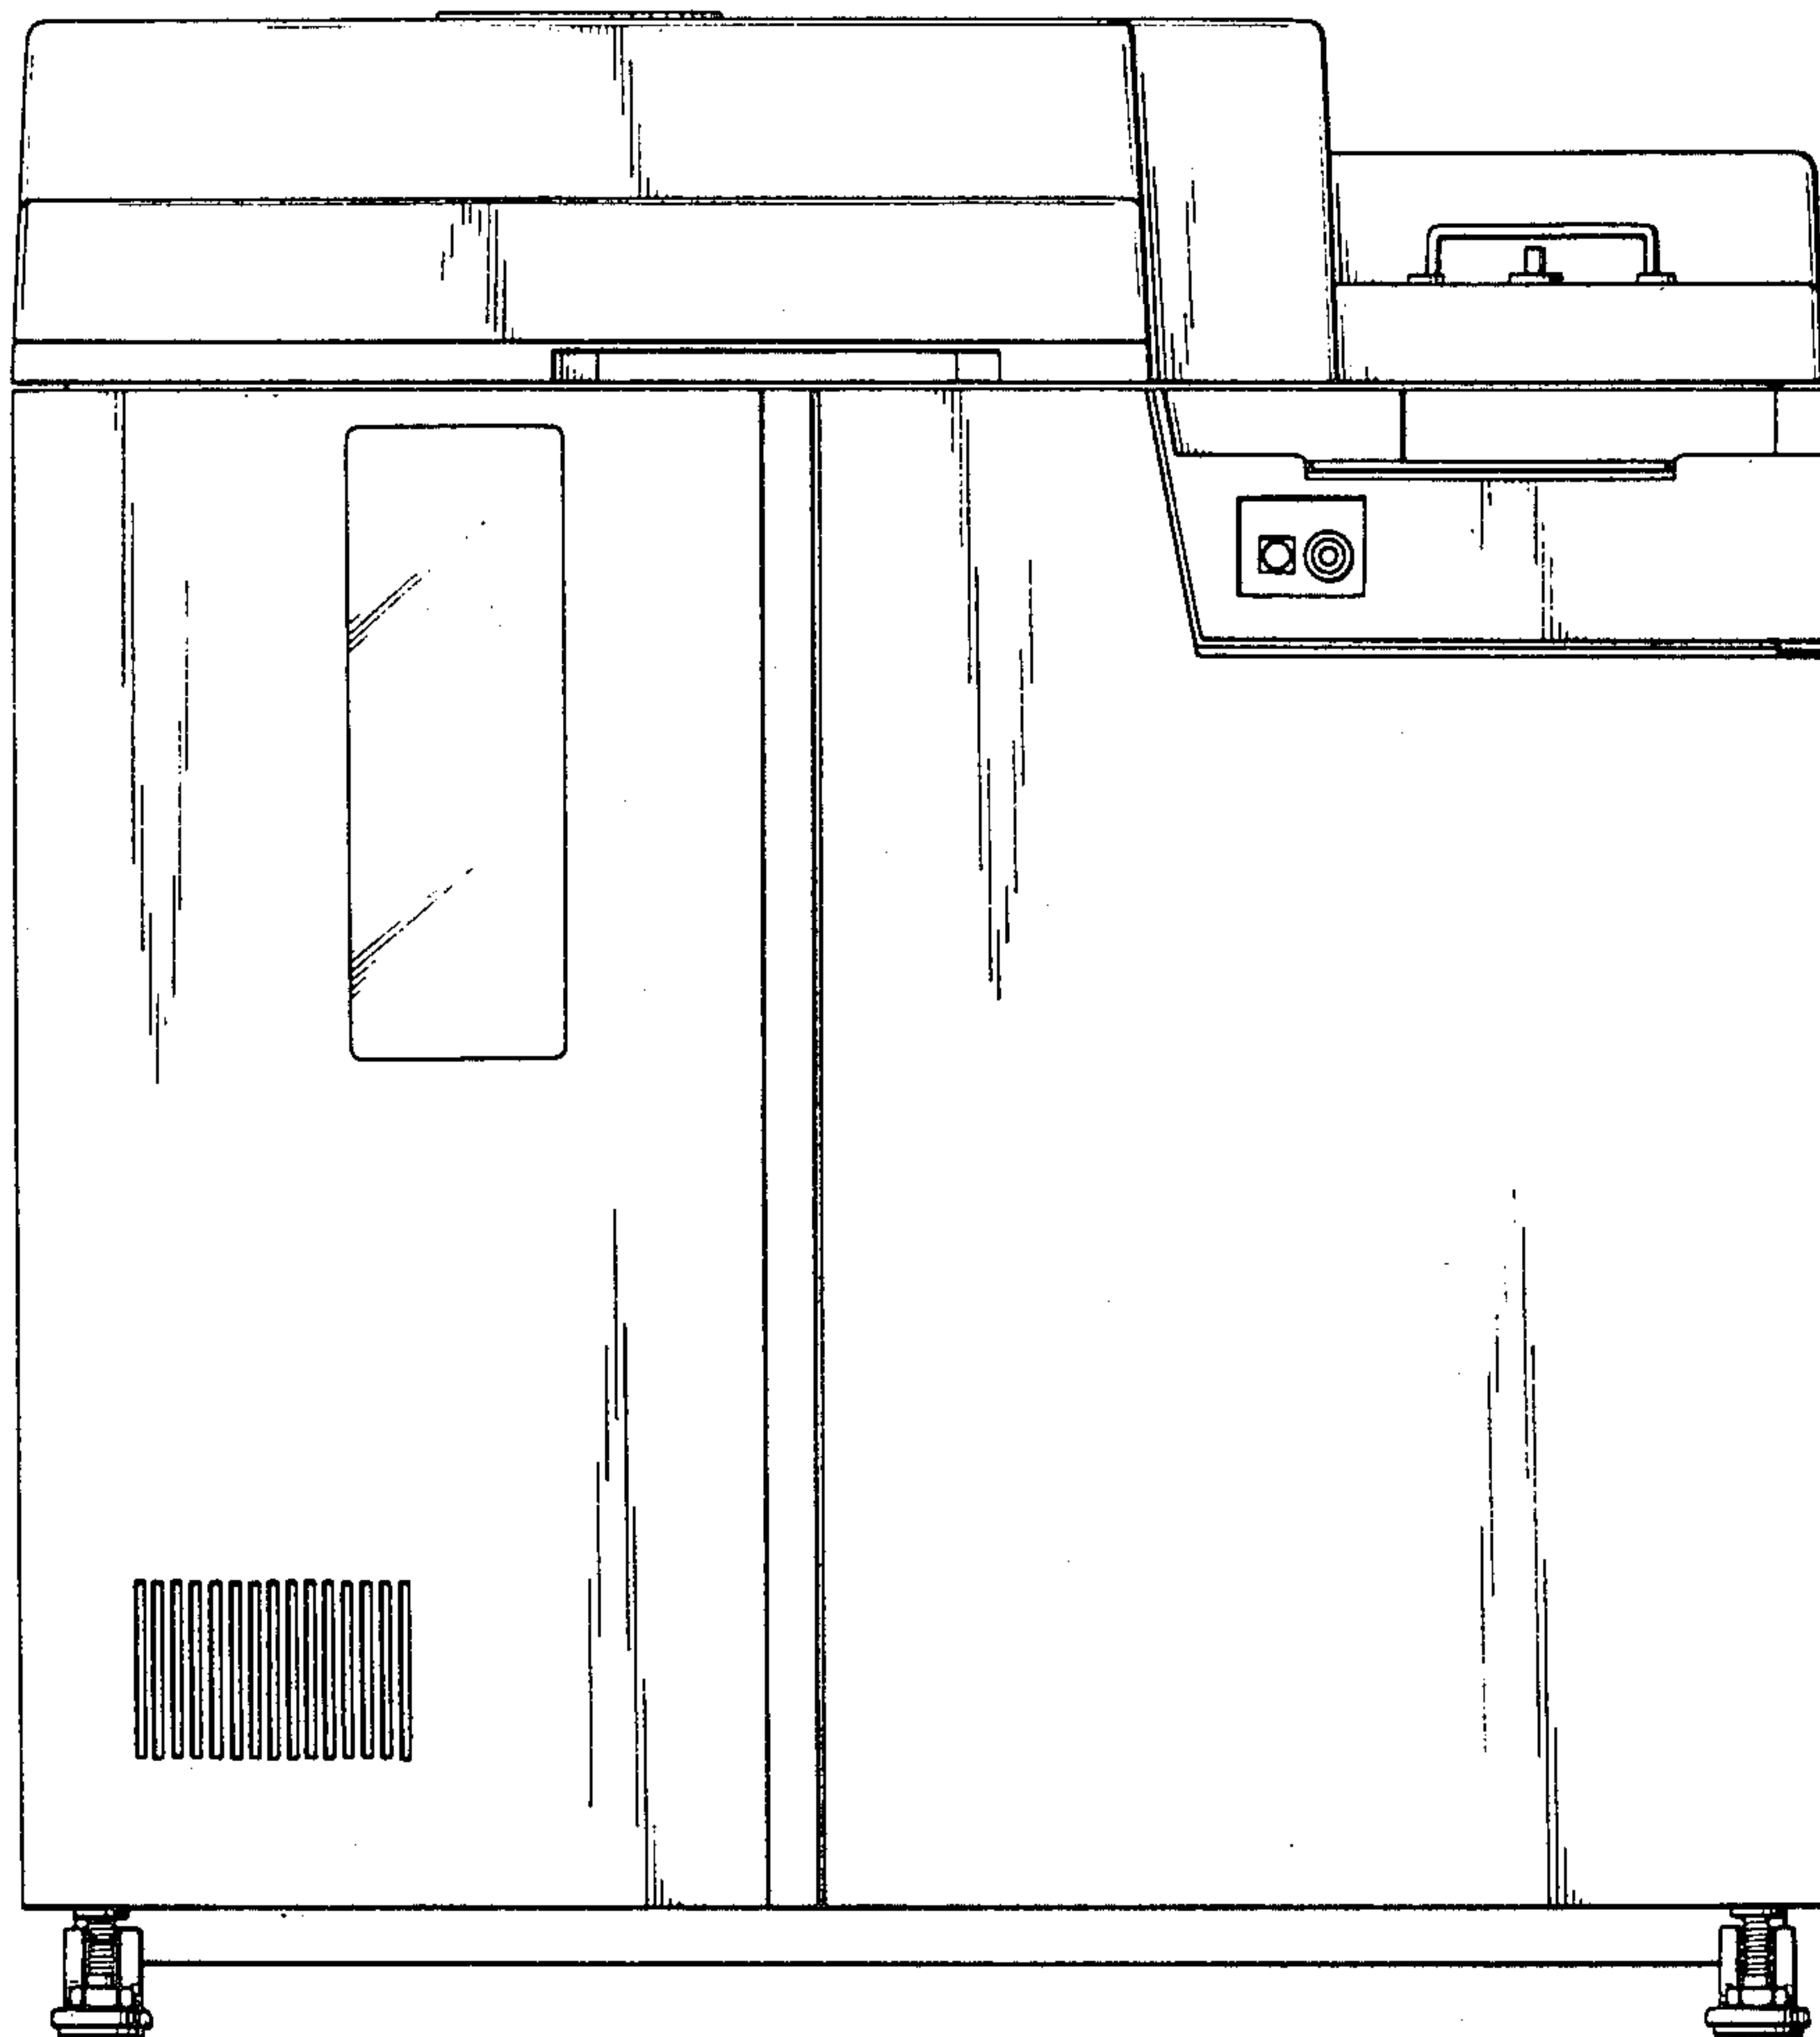


FIG. 4

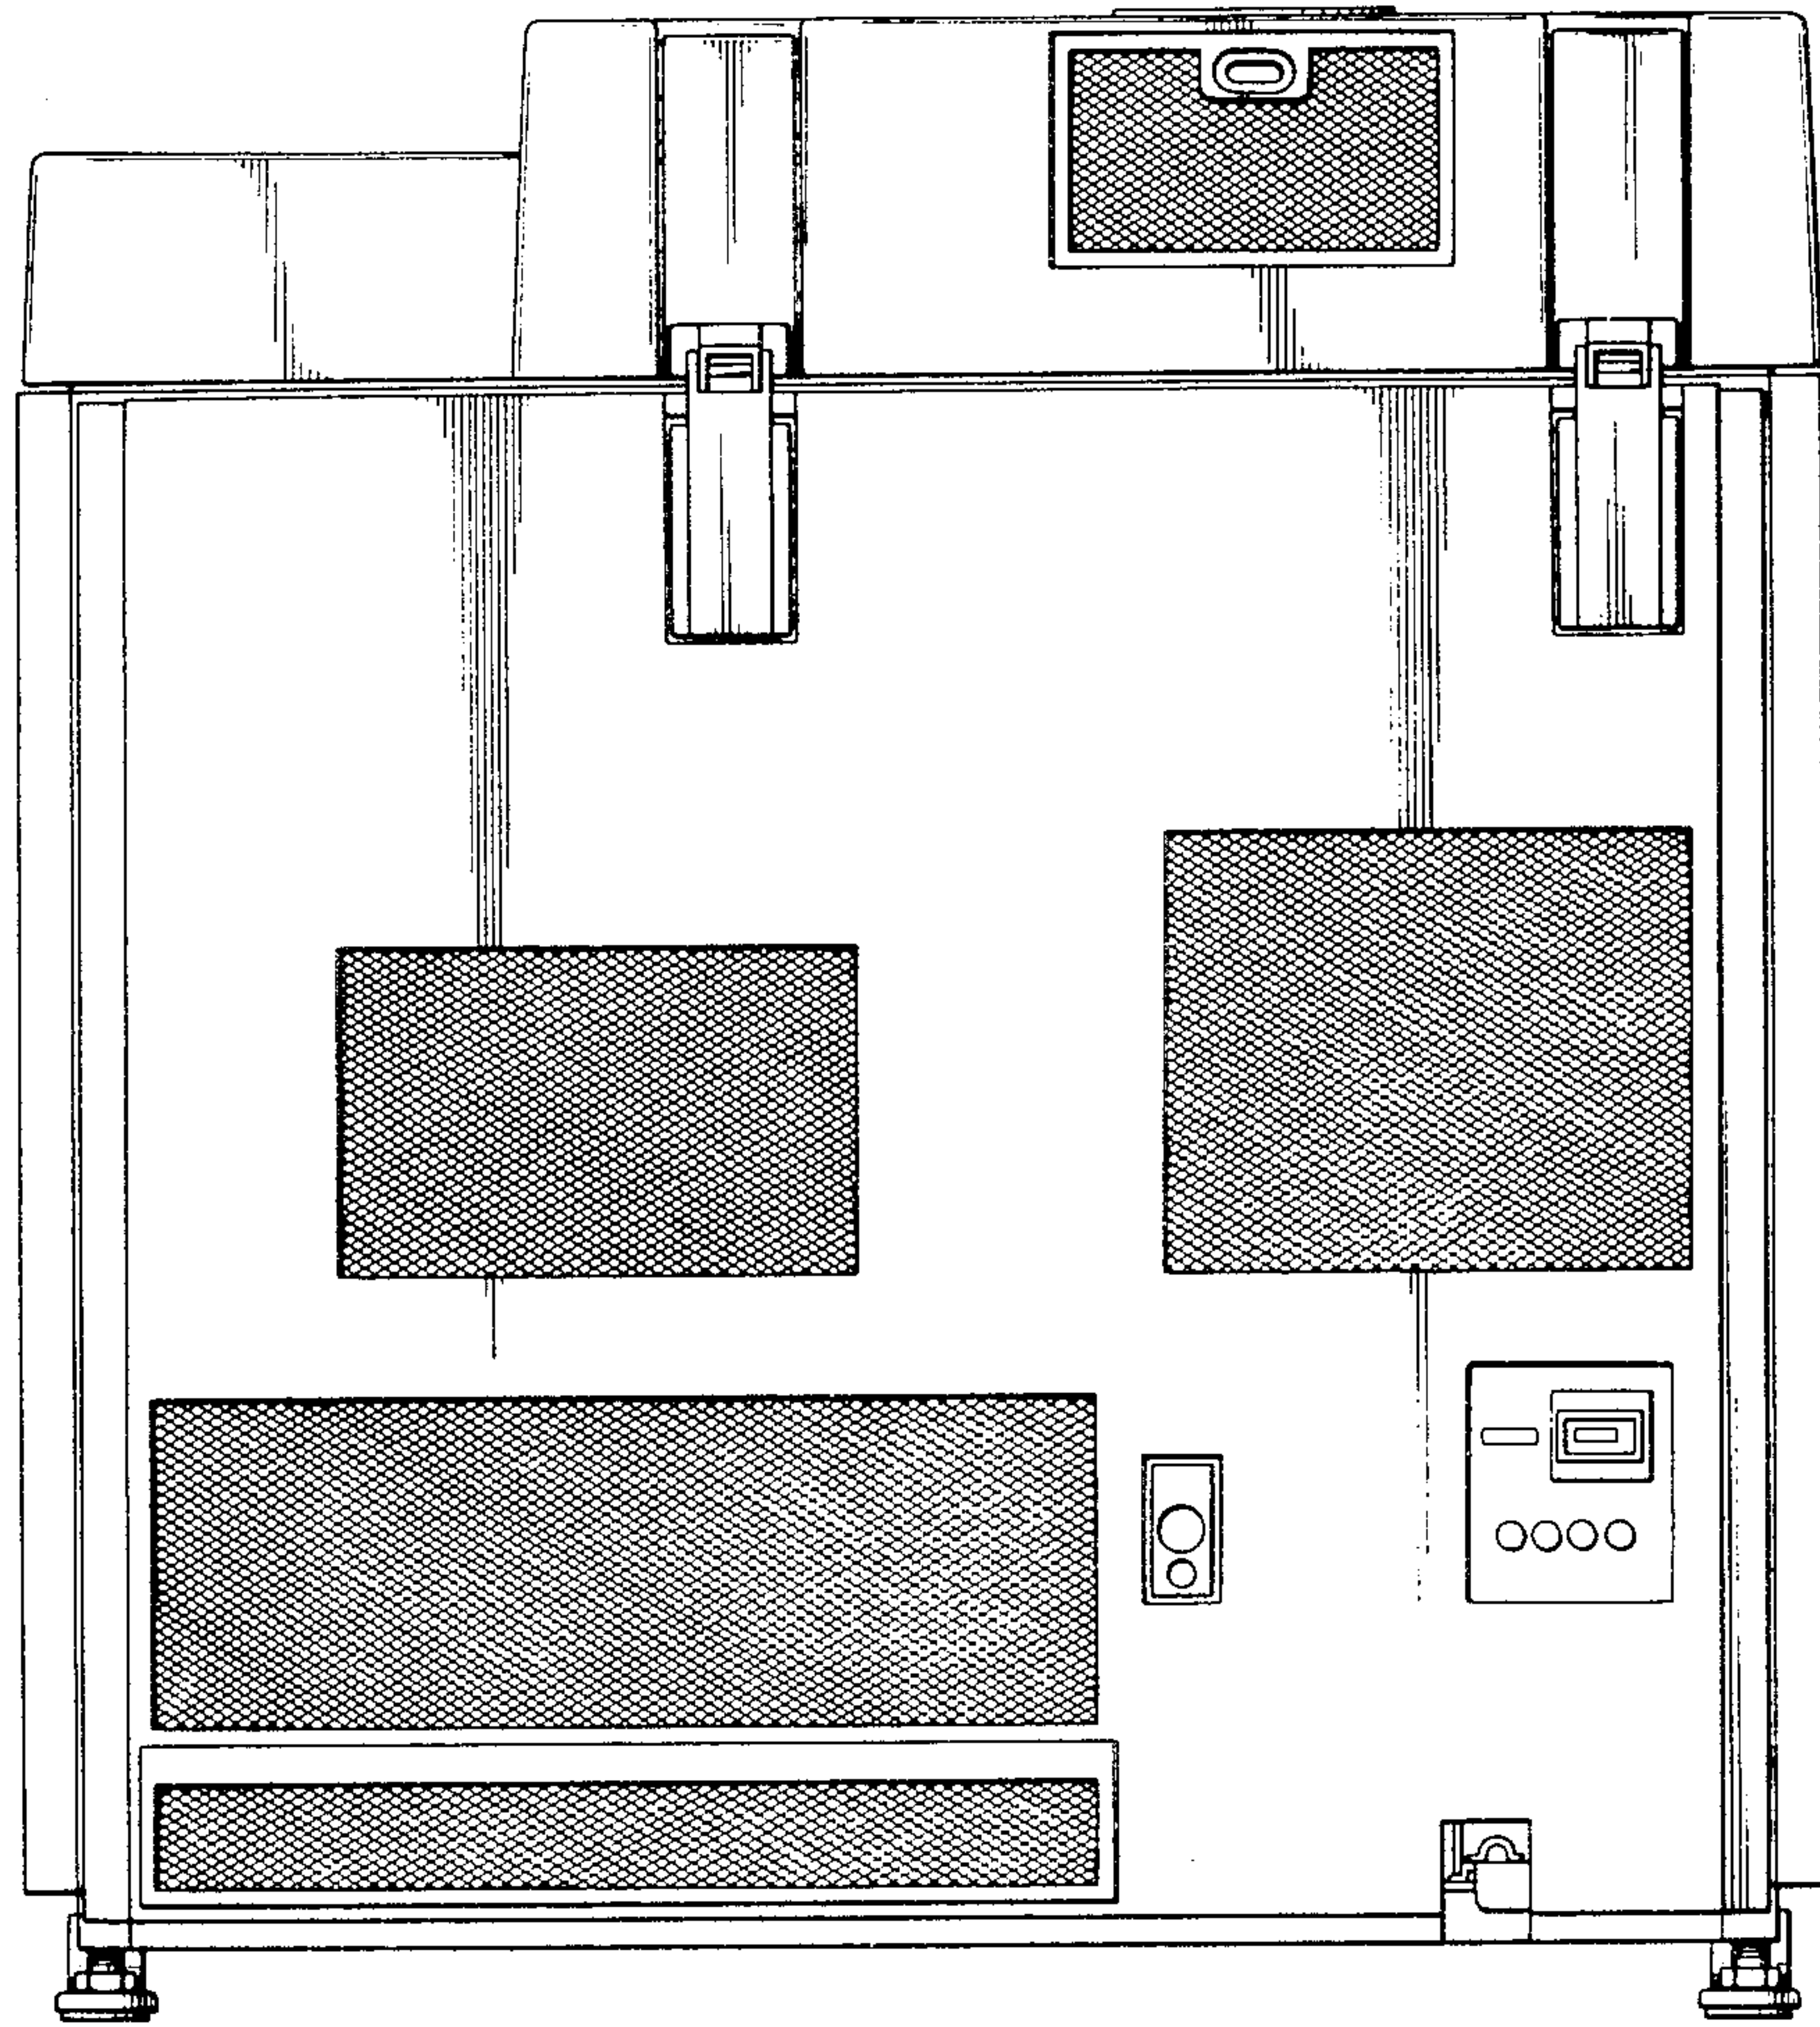


FIG. 6

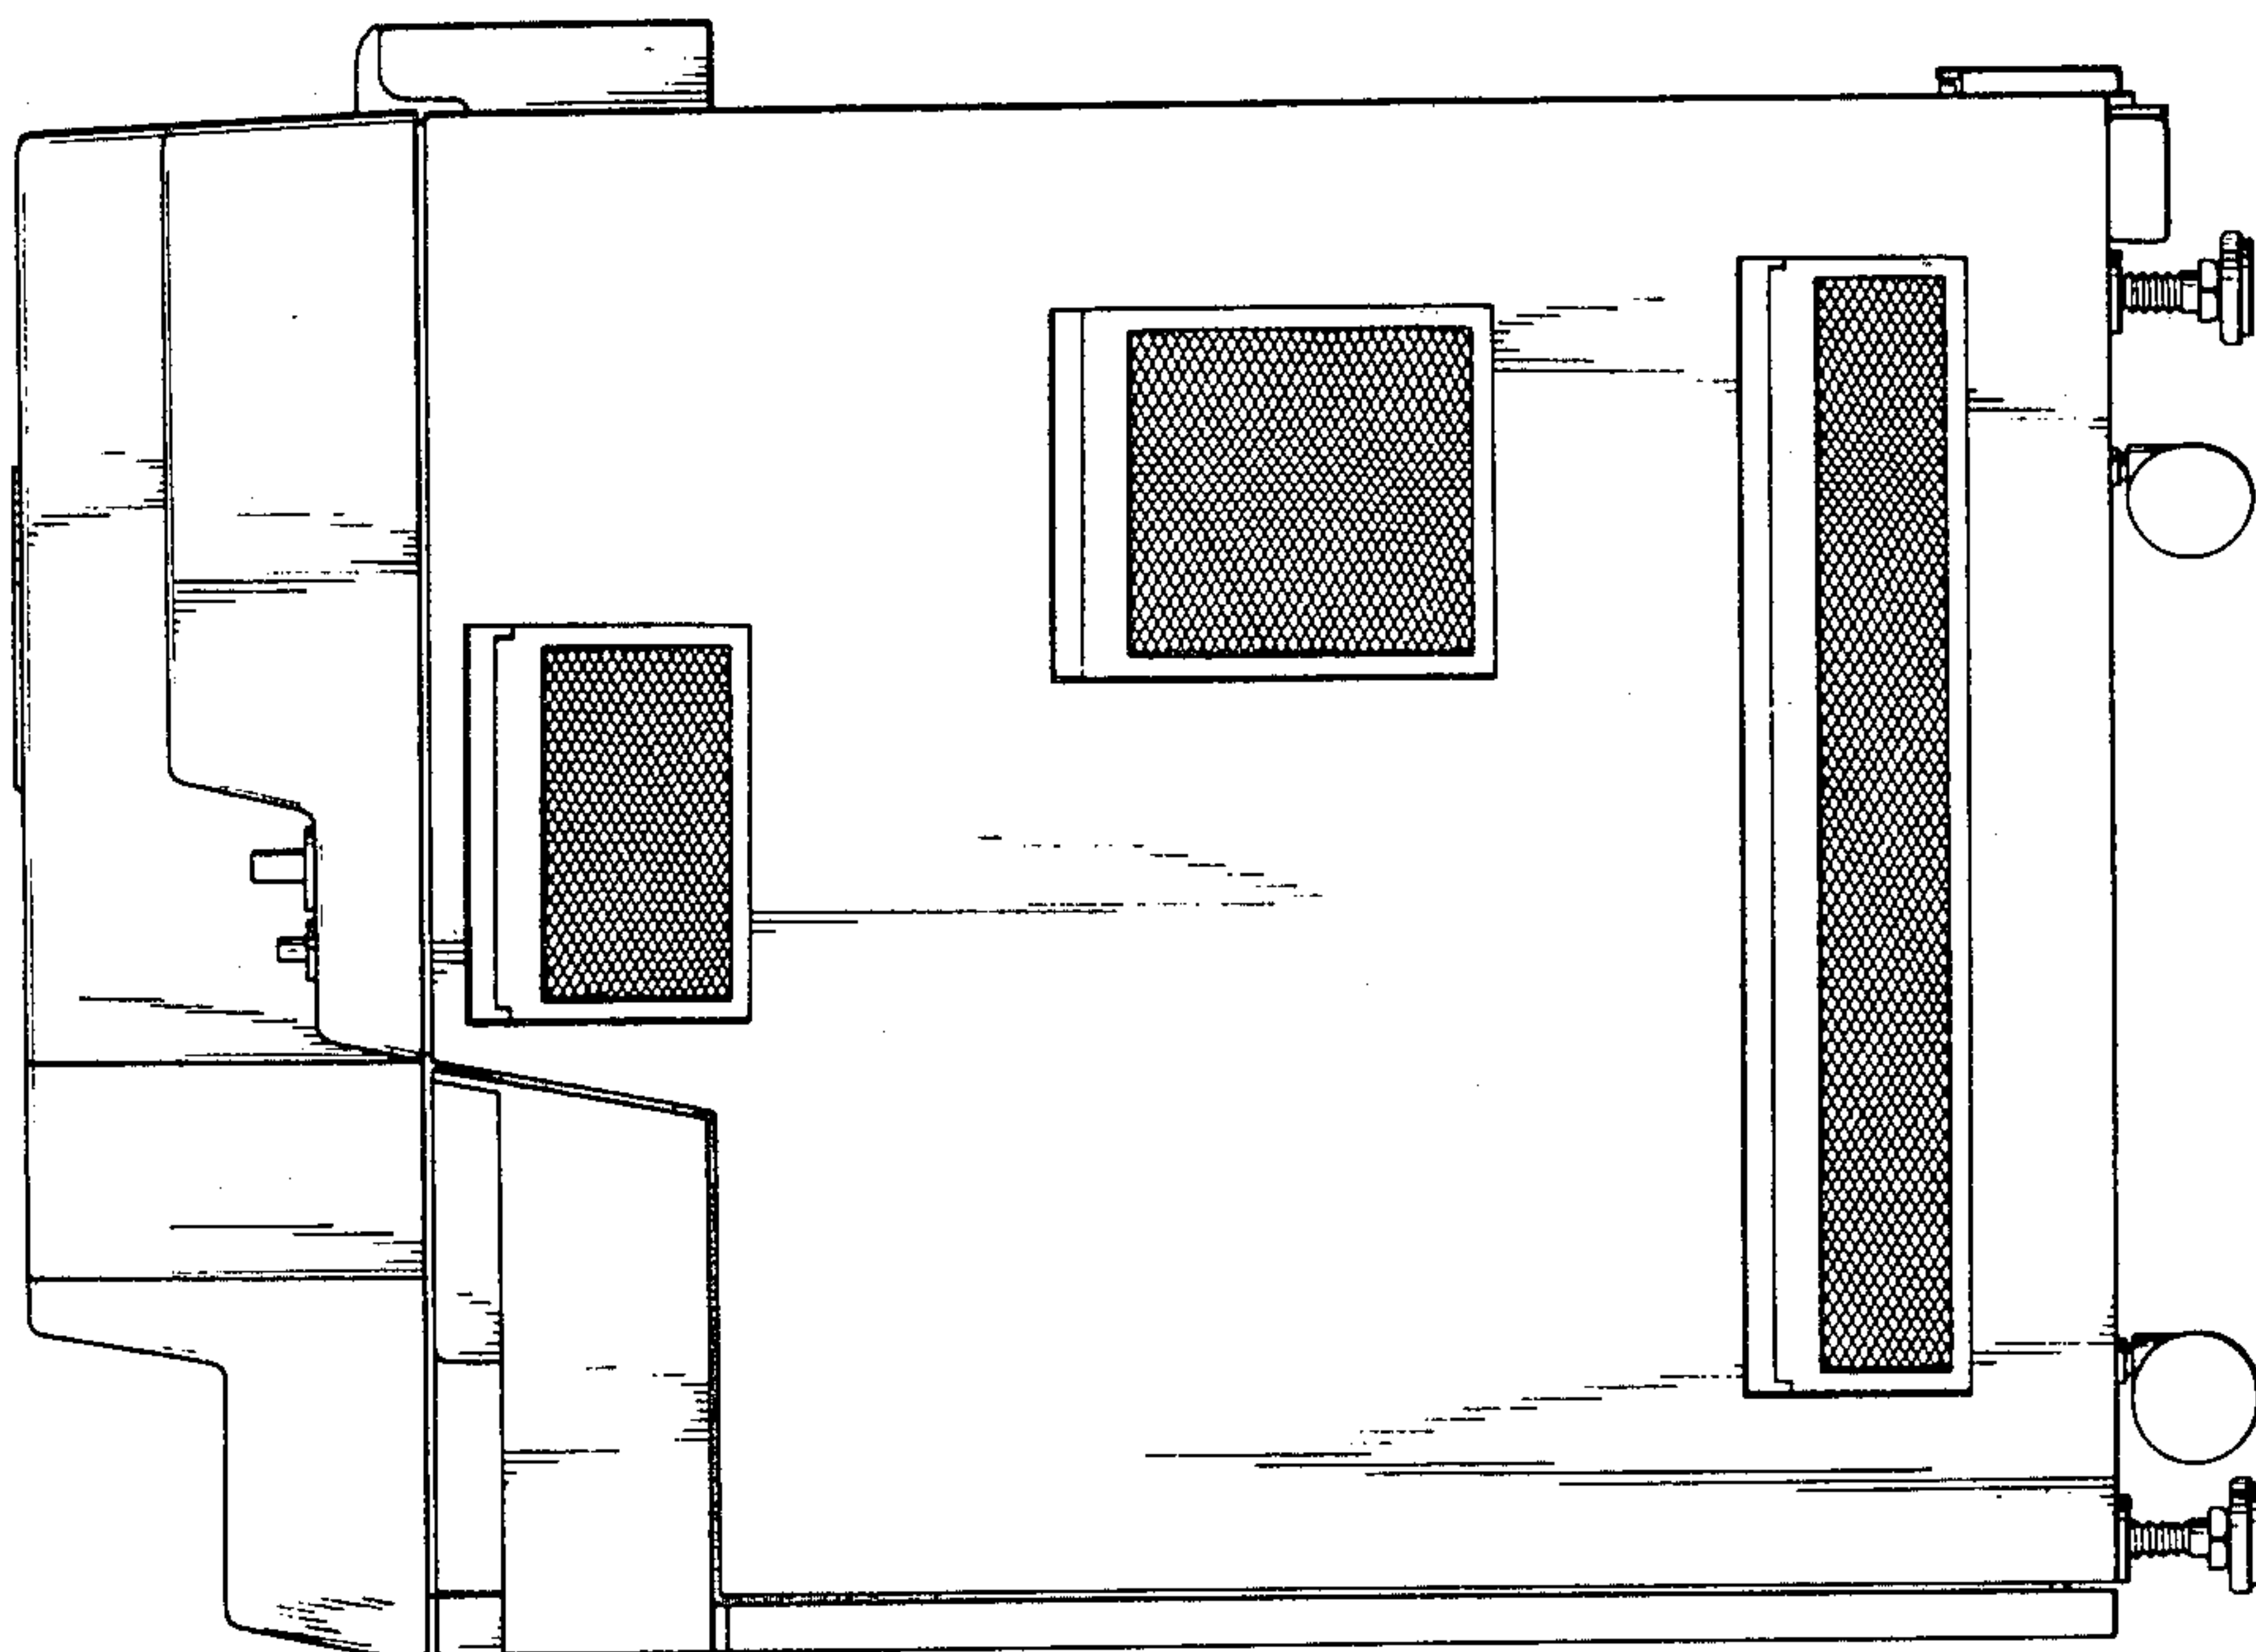


FIG. 5

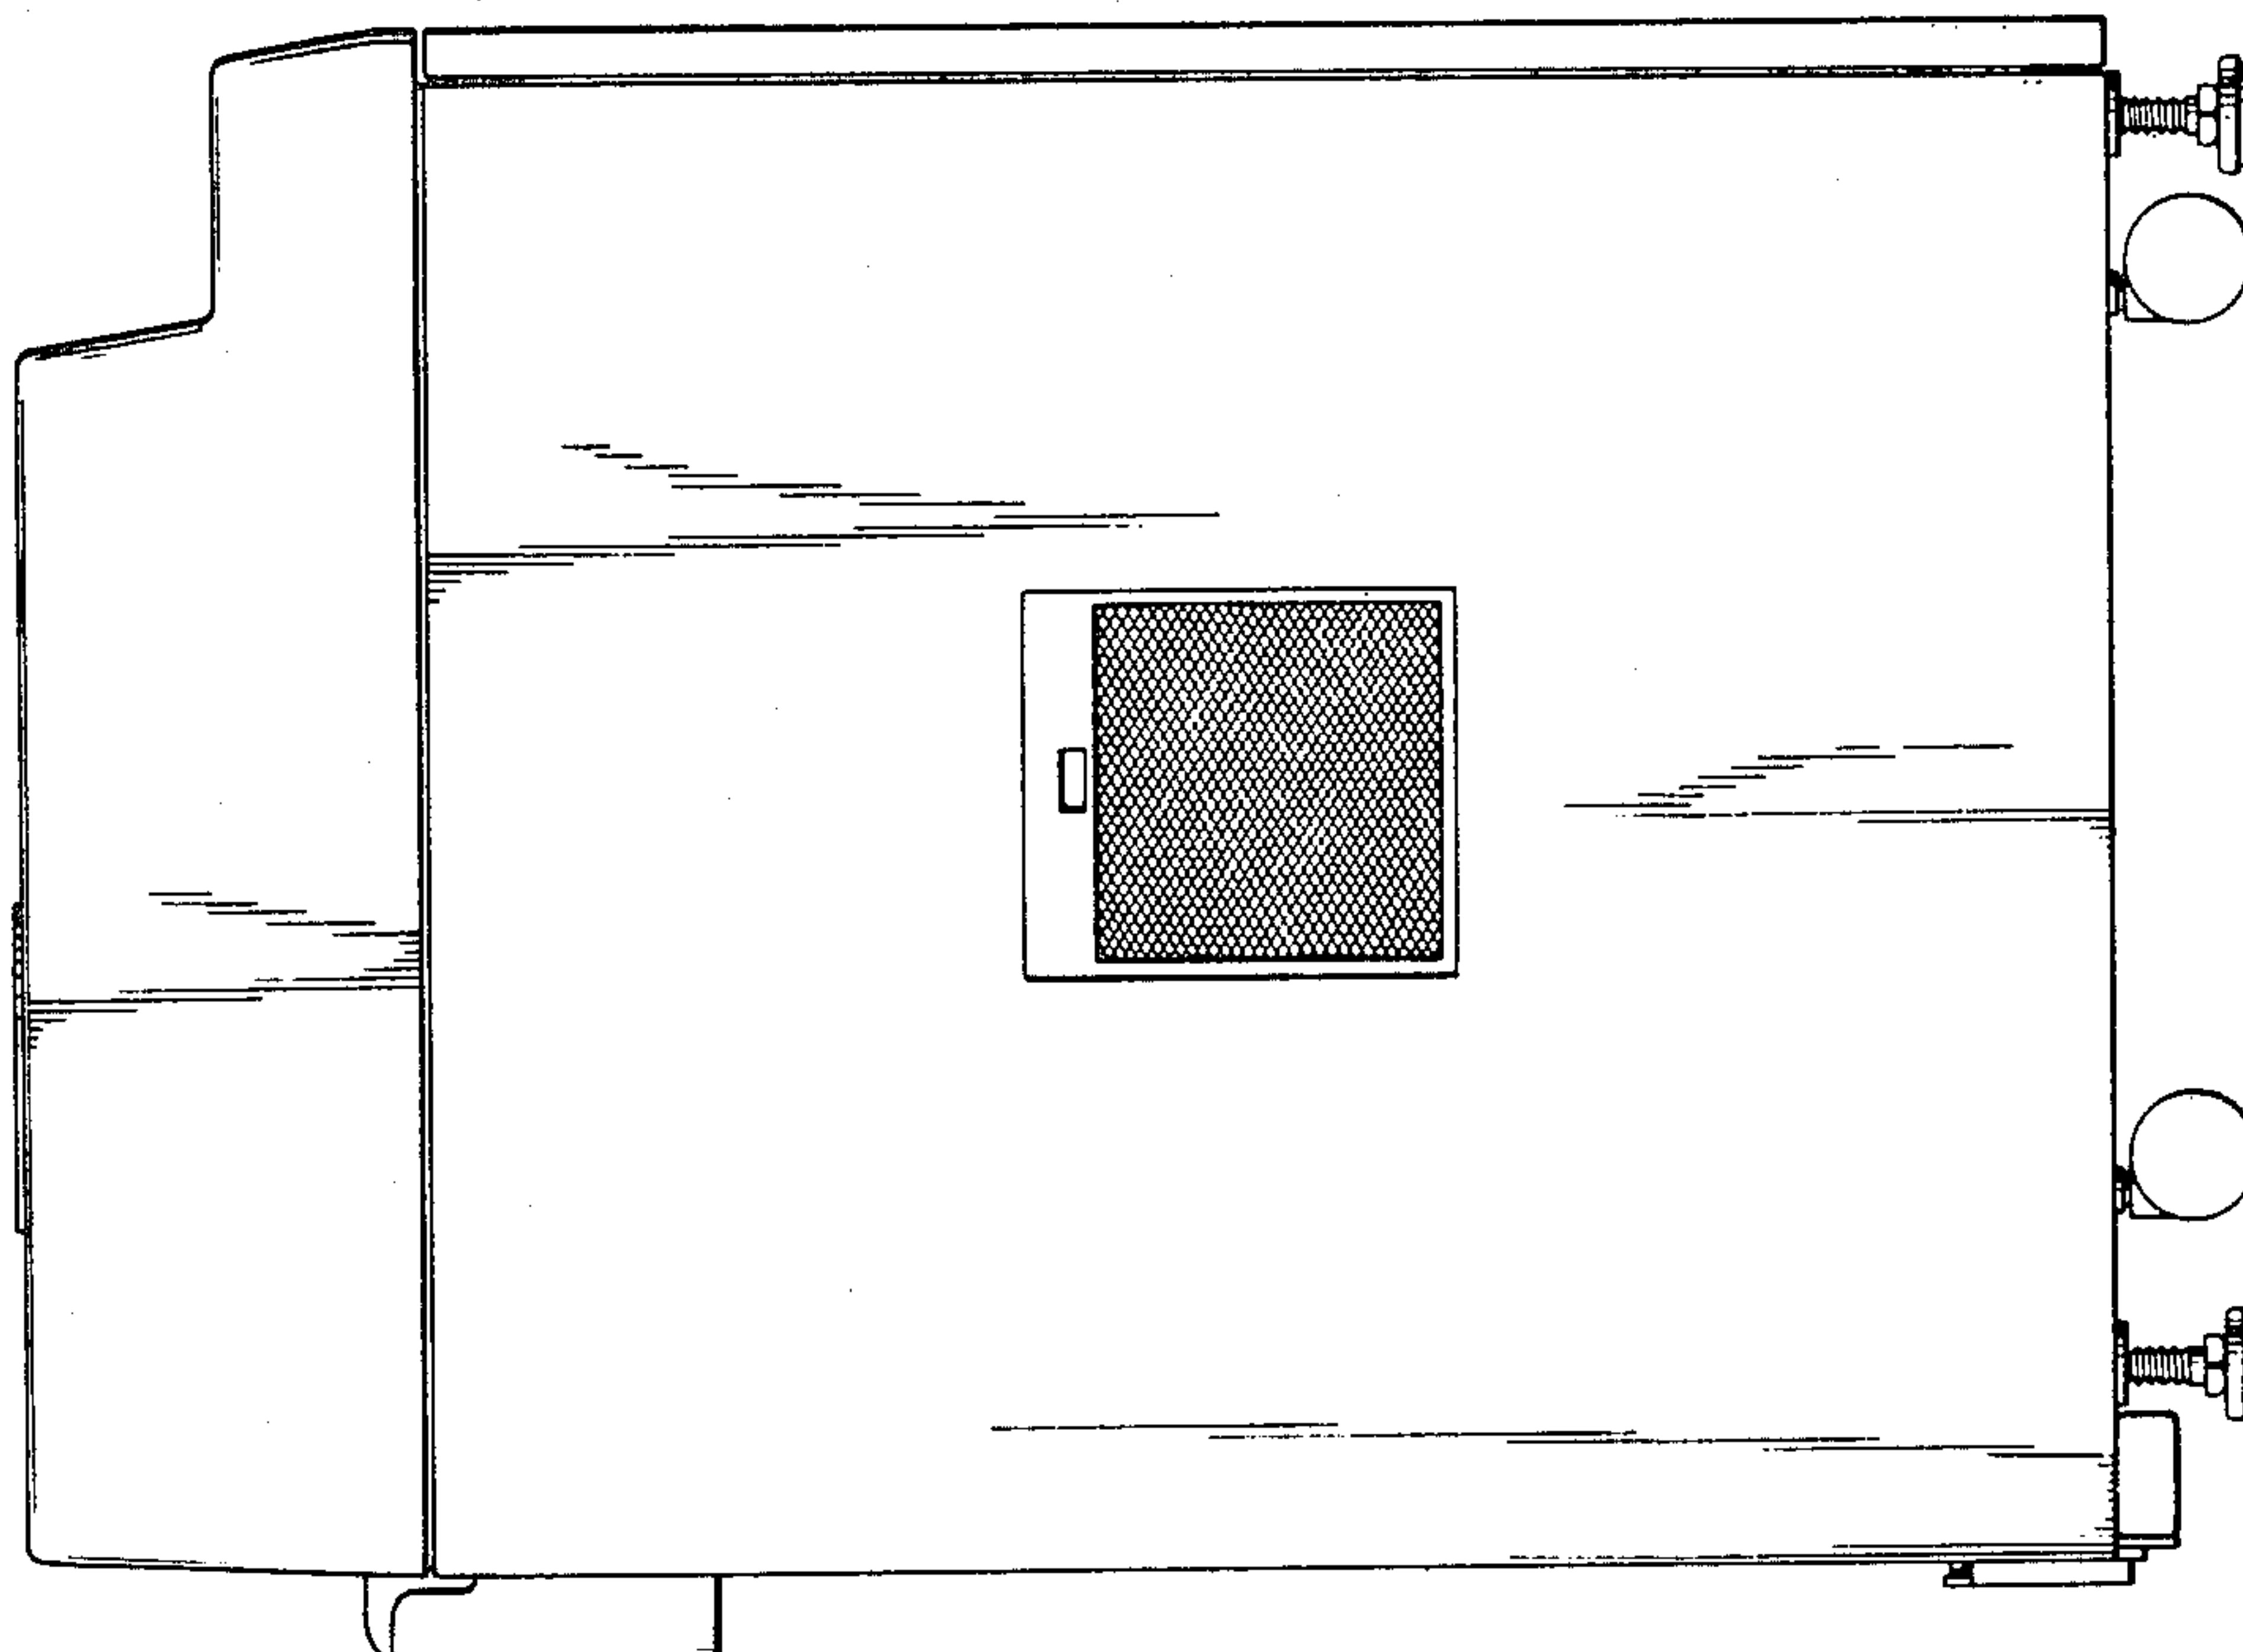


FIG. 7

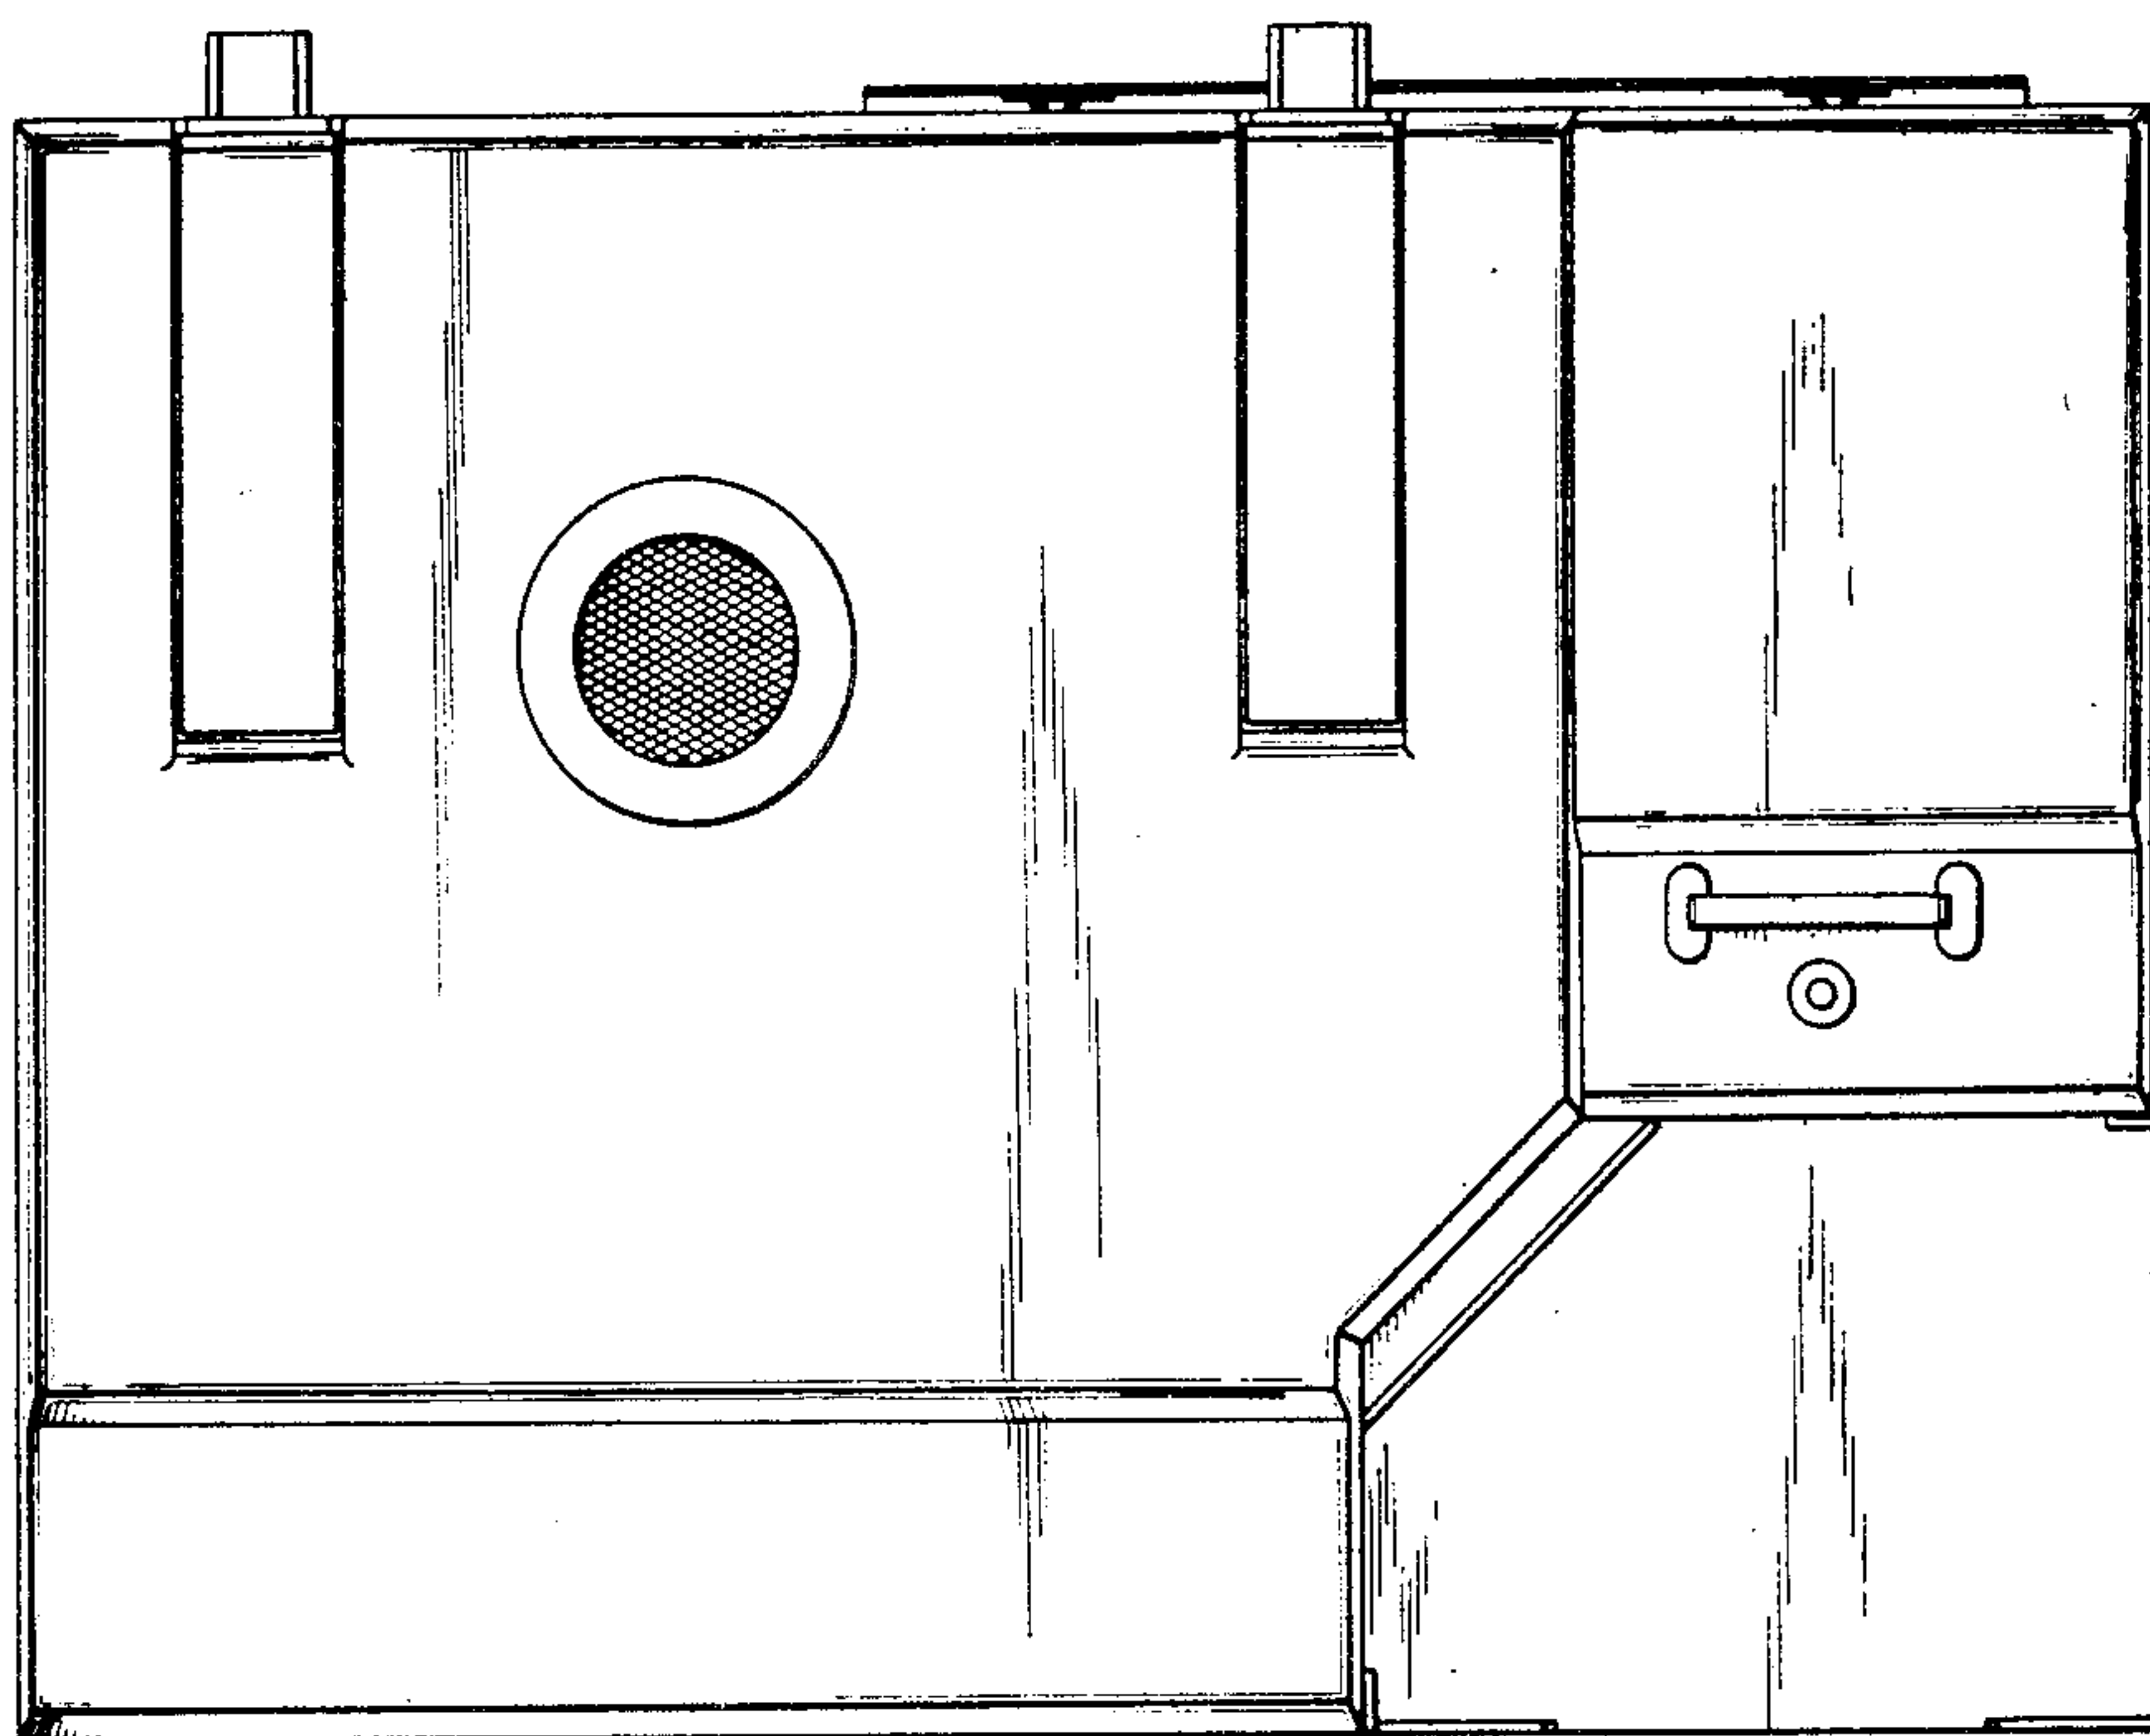


FIG. 8

