

[54] THERMAL MYRINGOTOMY SYSTEM

[75] Inventor: John K. Lynn, Jacksonville, Fla.

[73] Assignee: Xomed Inc., Jacksonville, Fla.

[**] Term: 14 Years

[21] Appl. No.: 483,065

[22] Filed: Apr. 7, 1983

[52] U.S. Cl. D24/8; D24/26; D24/28; D8/30

[58] Field of Search D24/8, 23, 26, 28, 29; 128/303.14, 303 R, 303.13, 303.15-303.19; D8/30, 71

[56] References Cited

U.S. PATENT DOCUMENTS

D. 224,070	6/1972	Lopez et al.	D24/8
3,234,356	2/1966	Babb	128/303.14 X
3,526,750	9/1970	Siegel	128/303.14 X
3,807,404	4/1974	Weissman et al.	128/303.14
4,112,950	9/1978	Pike	128/303.14
4,202,337	5/1980	Hren et al.	128/303.14

Primary Examiner—Catherine E. Kemper
Attorney, Agent, or Firm—Stuart E. Krieger; Richard H. Brink; Isaac Jarkovsky


[57] CLAIM

The ornamental design for a thermal myringotomy system, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view taken from the upper right

of a thermal myringotomy system handpiece charger stand showing my new design;
 FIG. 2 is a top plan view of the charger illustrated in FIG. 1;
 FIG. 3 is a left side elevational view of the charger of FIG. 2;
 FIG. 4 is a back side elevational view of the charger of FIG. 1;
 FIG. 5 is a bottom plan view of the charger of FIG. 1;
 FIG. 6 is a perspective view taken from the upper right of a thermal myringotomy system handpiece showing my new design;
 FIG. 7 is a top plan view of the handpiece illustrated in FIG. 6;
 FIG. 8 is a front elevational view of the handpiece of FIG. 7;
 FIG. 9 is a left side elevational view of the handpiece of FIG. 7;
 FIG. 10 is a bottom plan view of the handpiece of FIG. 7;
 FIG. 11 is a perspective view taken from the upper right of a thermal myringotomy system handpiece as shown in FIG. 6 with a probe tip, showing my new design;
 FIG. 12 is a top plan view of the handpiece illustrated in FIG. 11;
 FIG. 13 is a front elevational view of the handpiece of FIG. 12;
 FIG. 14 is a left side elevational view of the handpiece of FIG. 12;
 FIG. 15 is a bottom plan view of the handpiece of FIG. 12; and
 FIG. 16 is a perspective view taken from the upper right of the thermal myringotomy system showing my new design, comprising the charger and handpiece shown engaged.

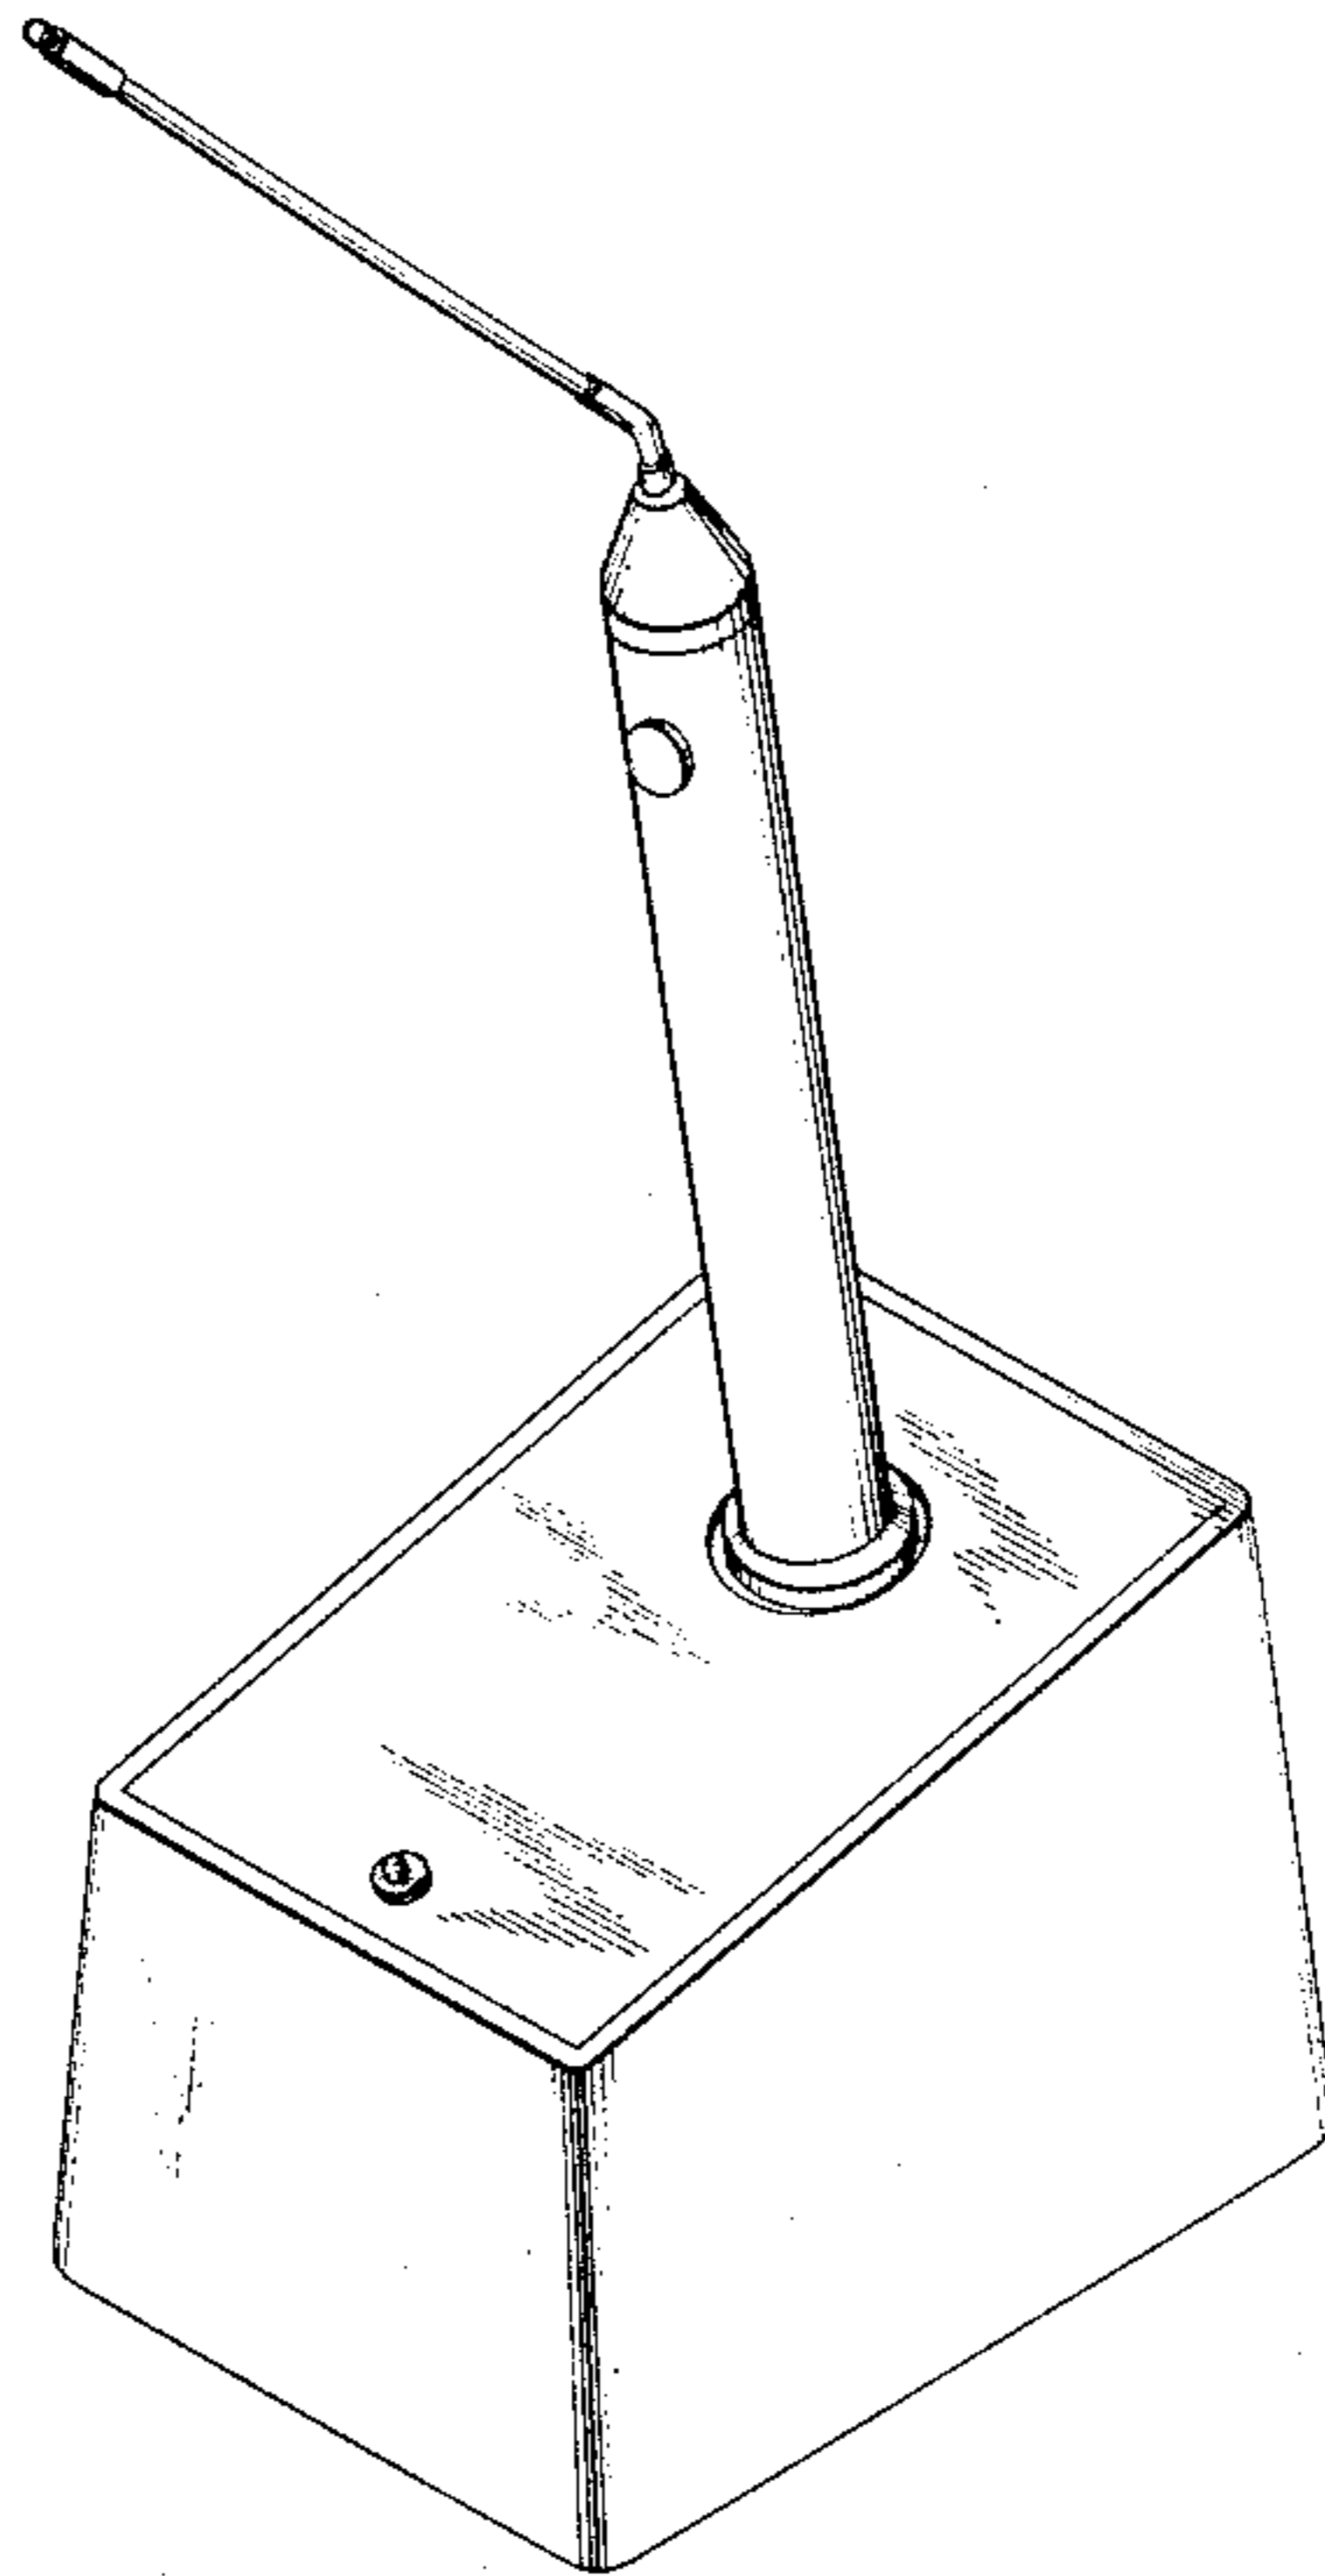

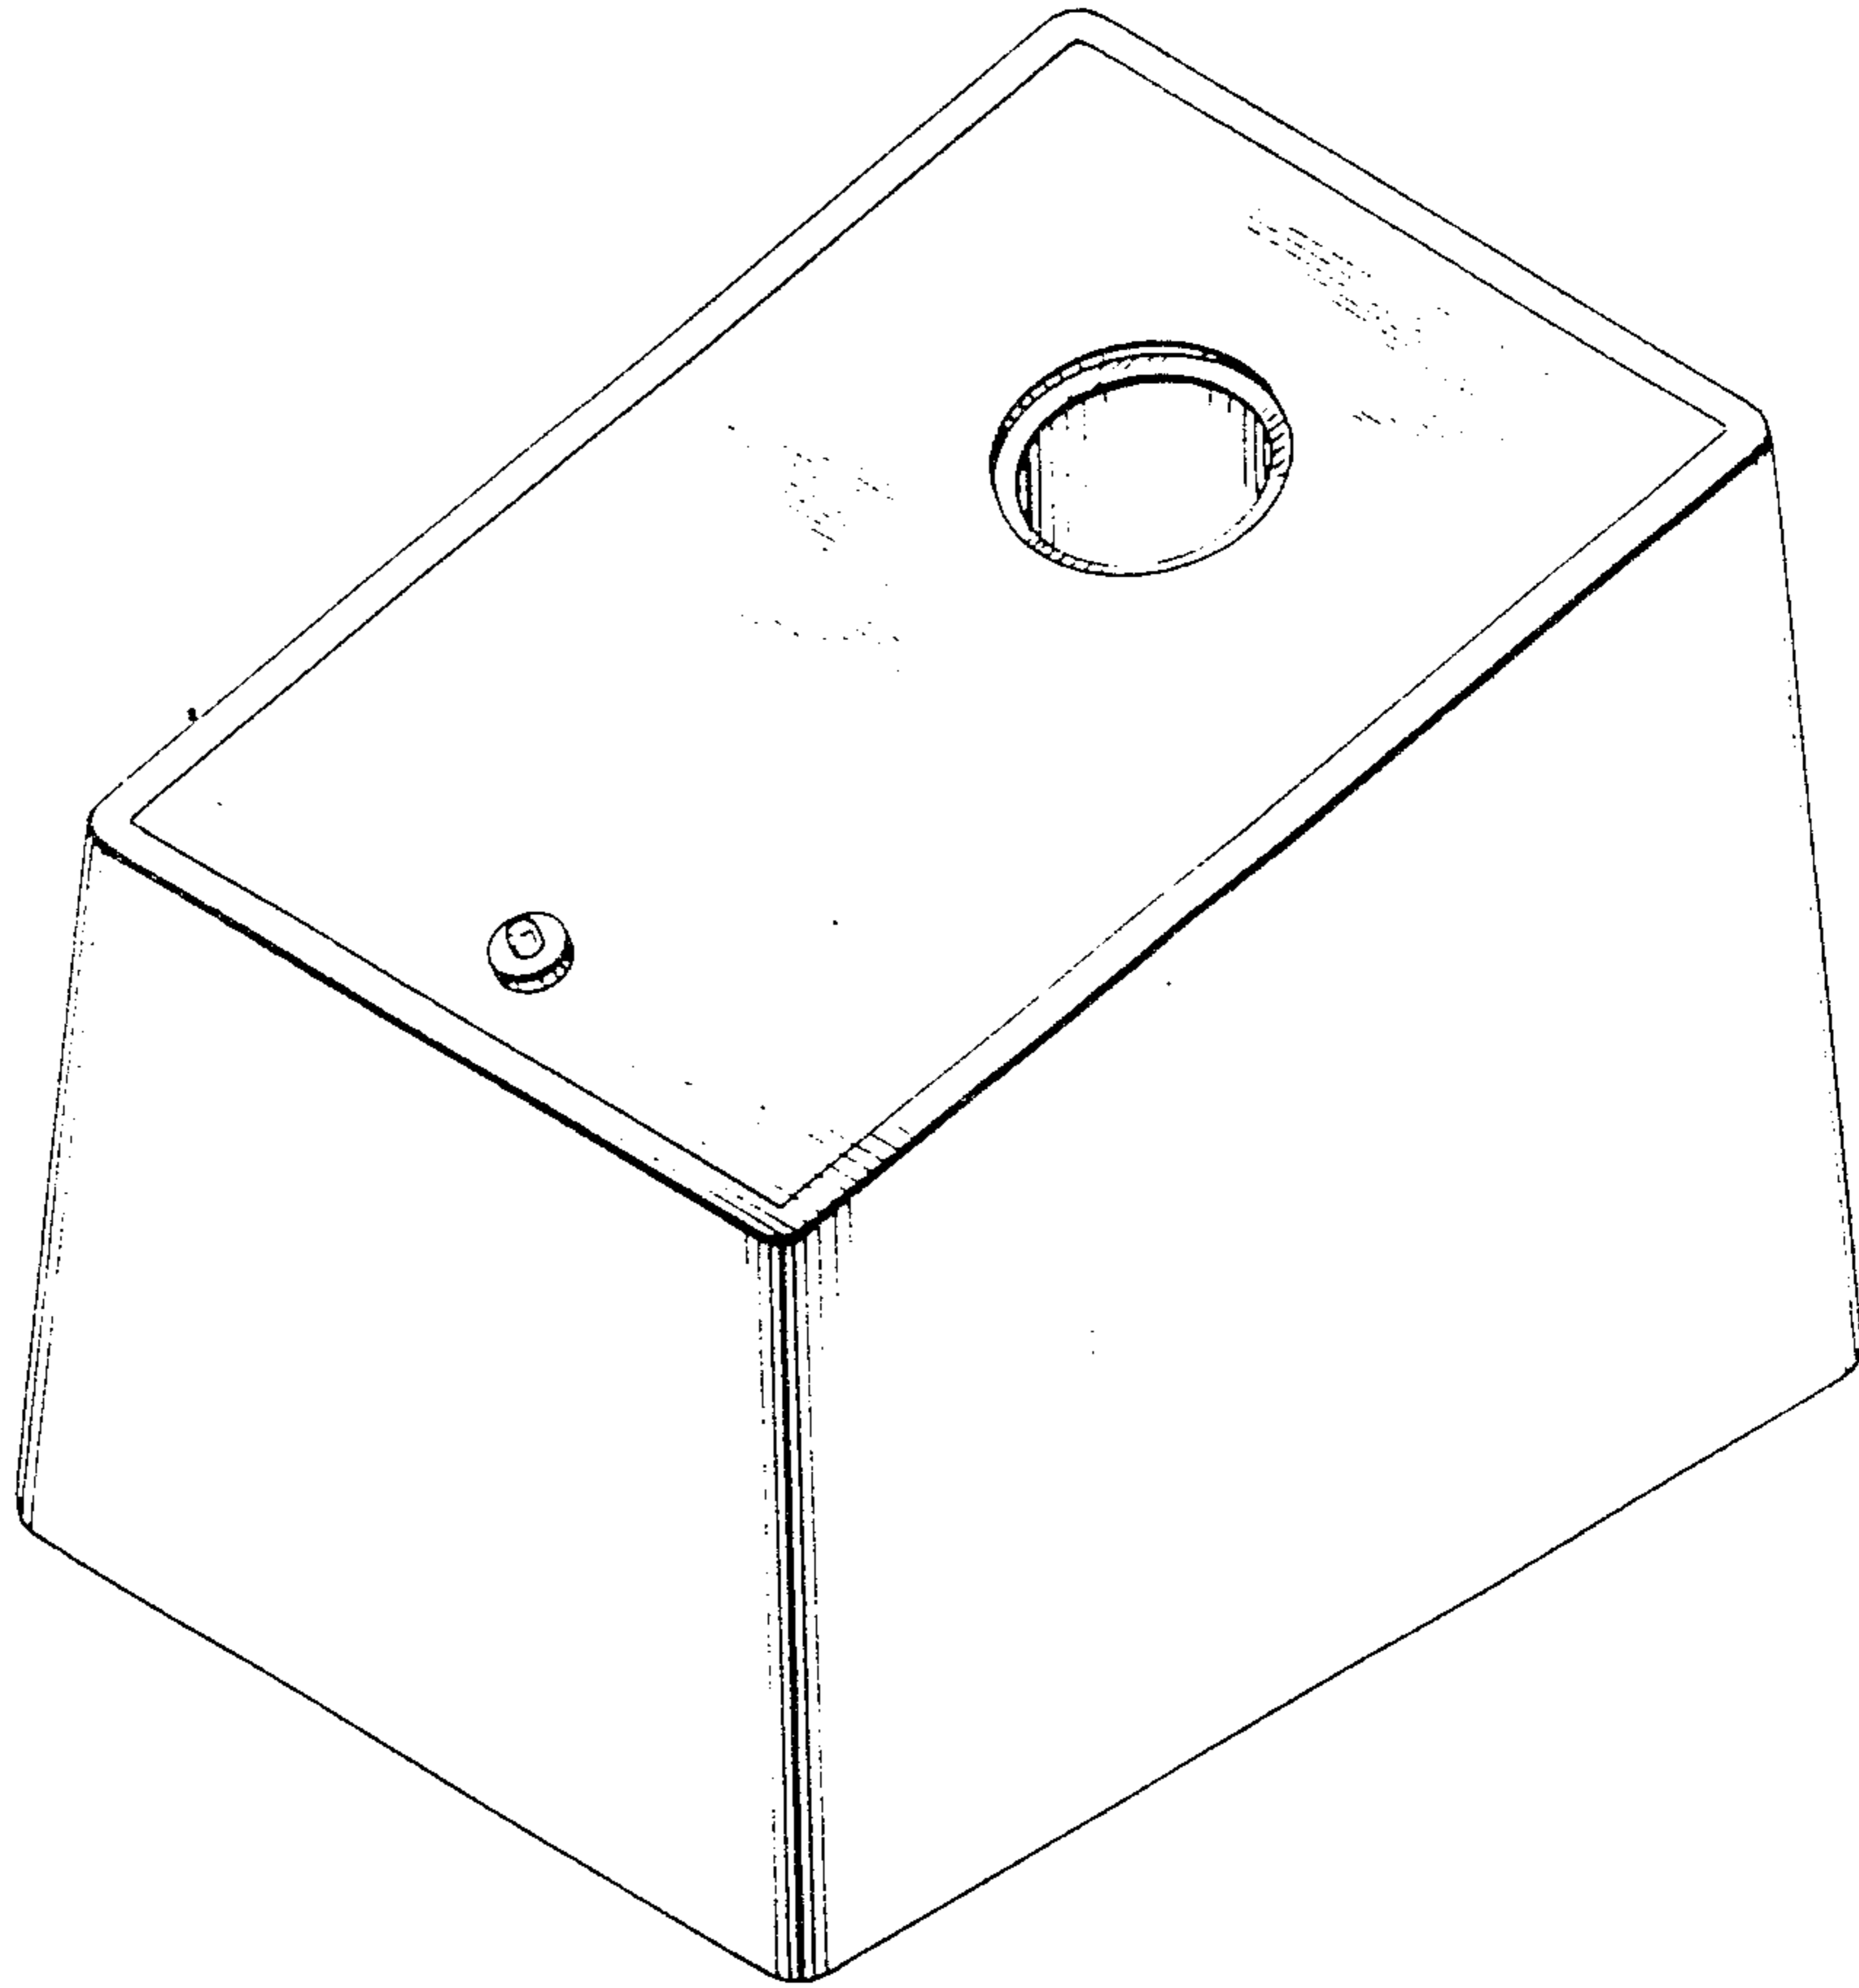


FIG. 1

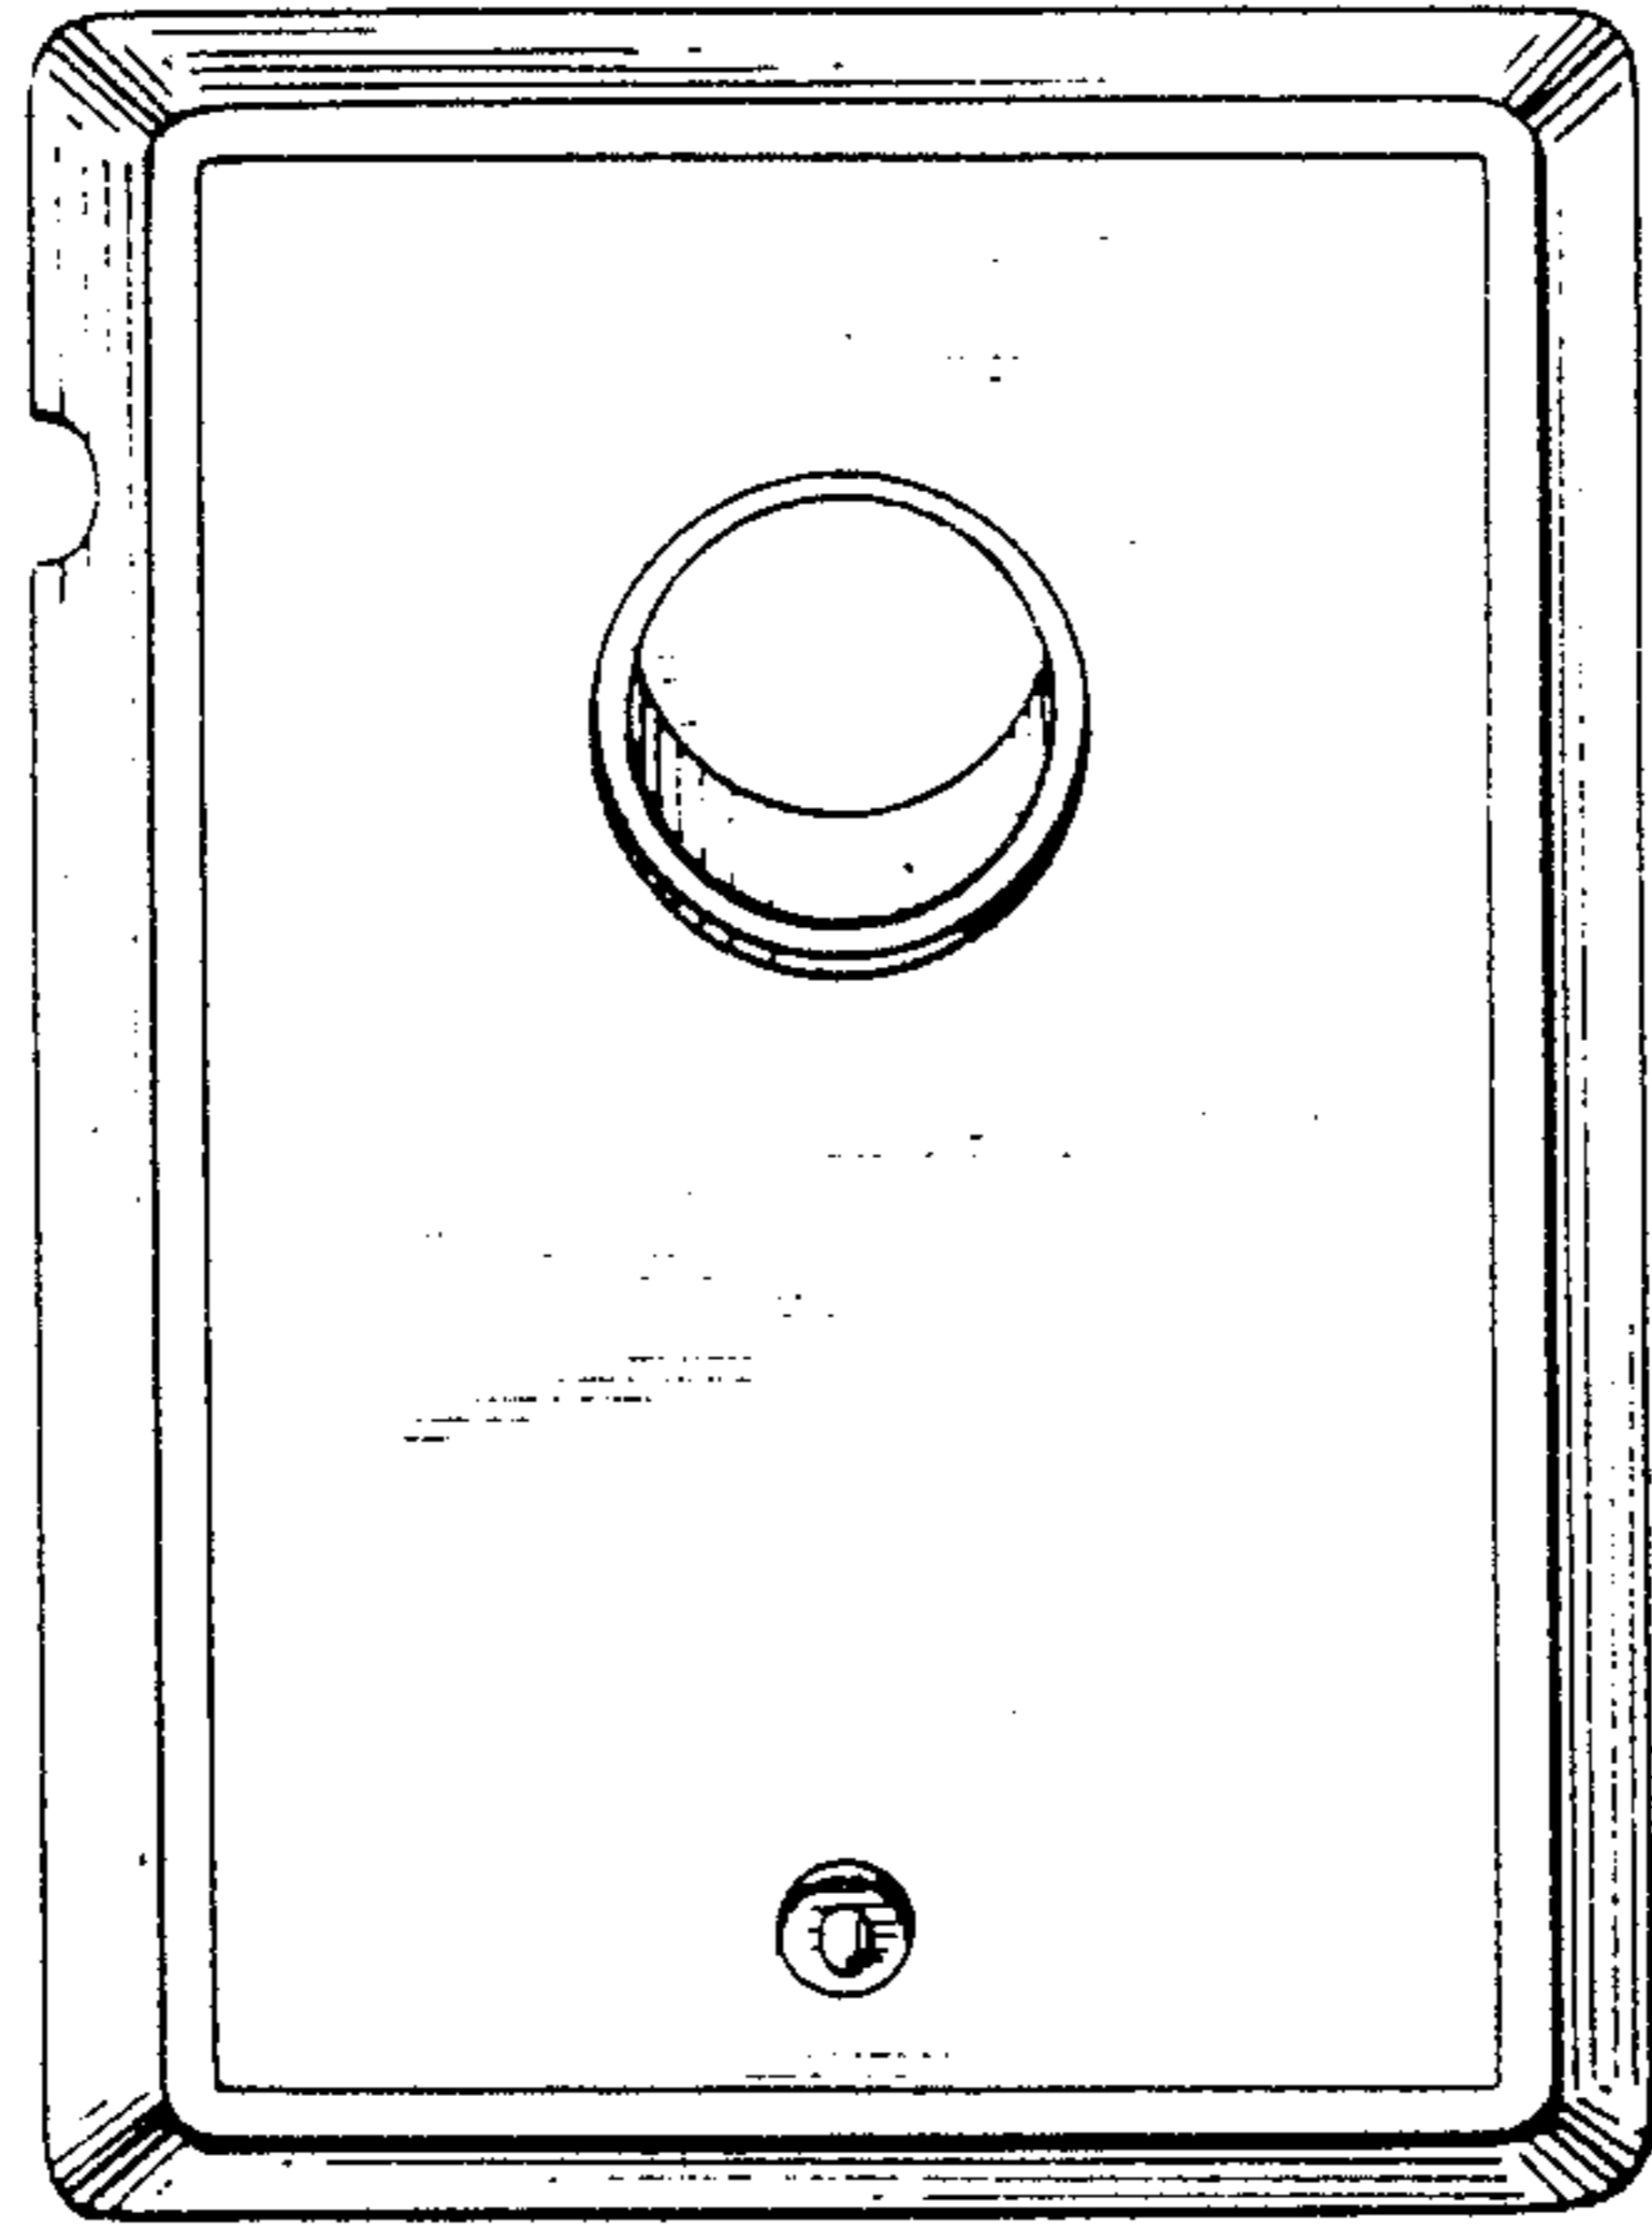


FIG. 2

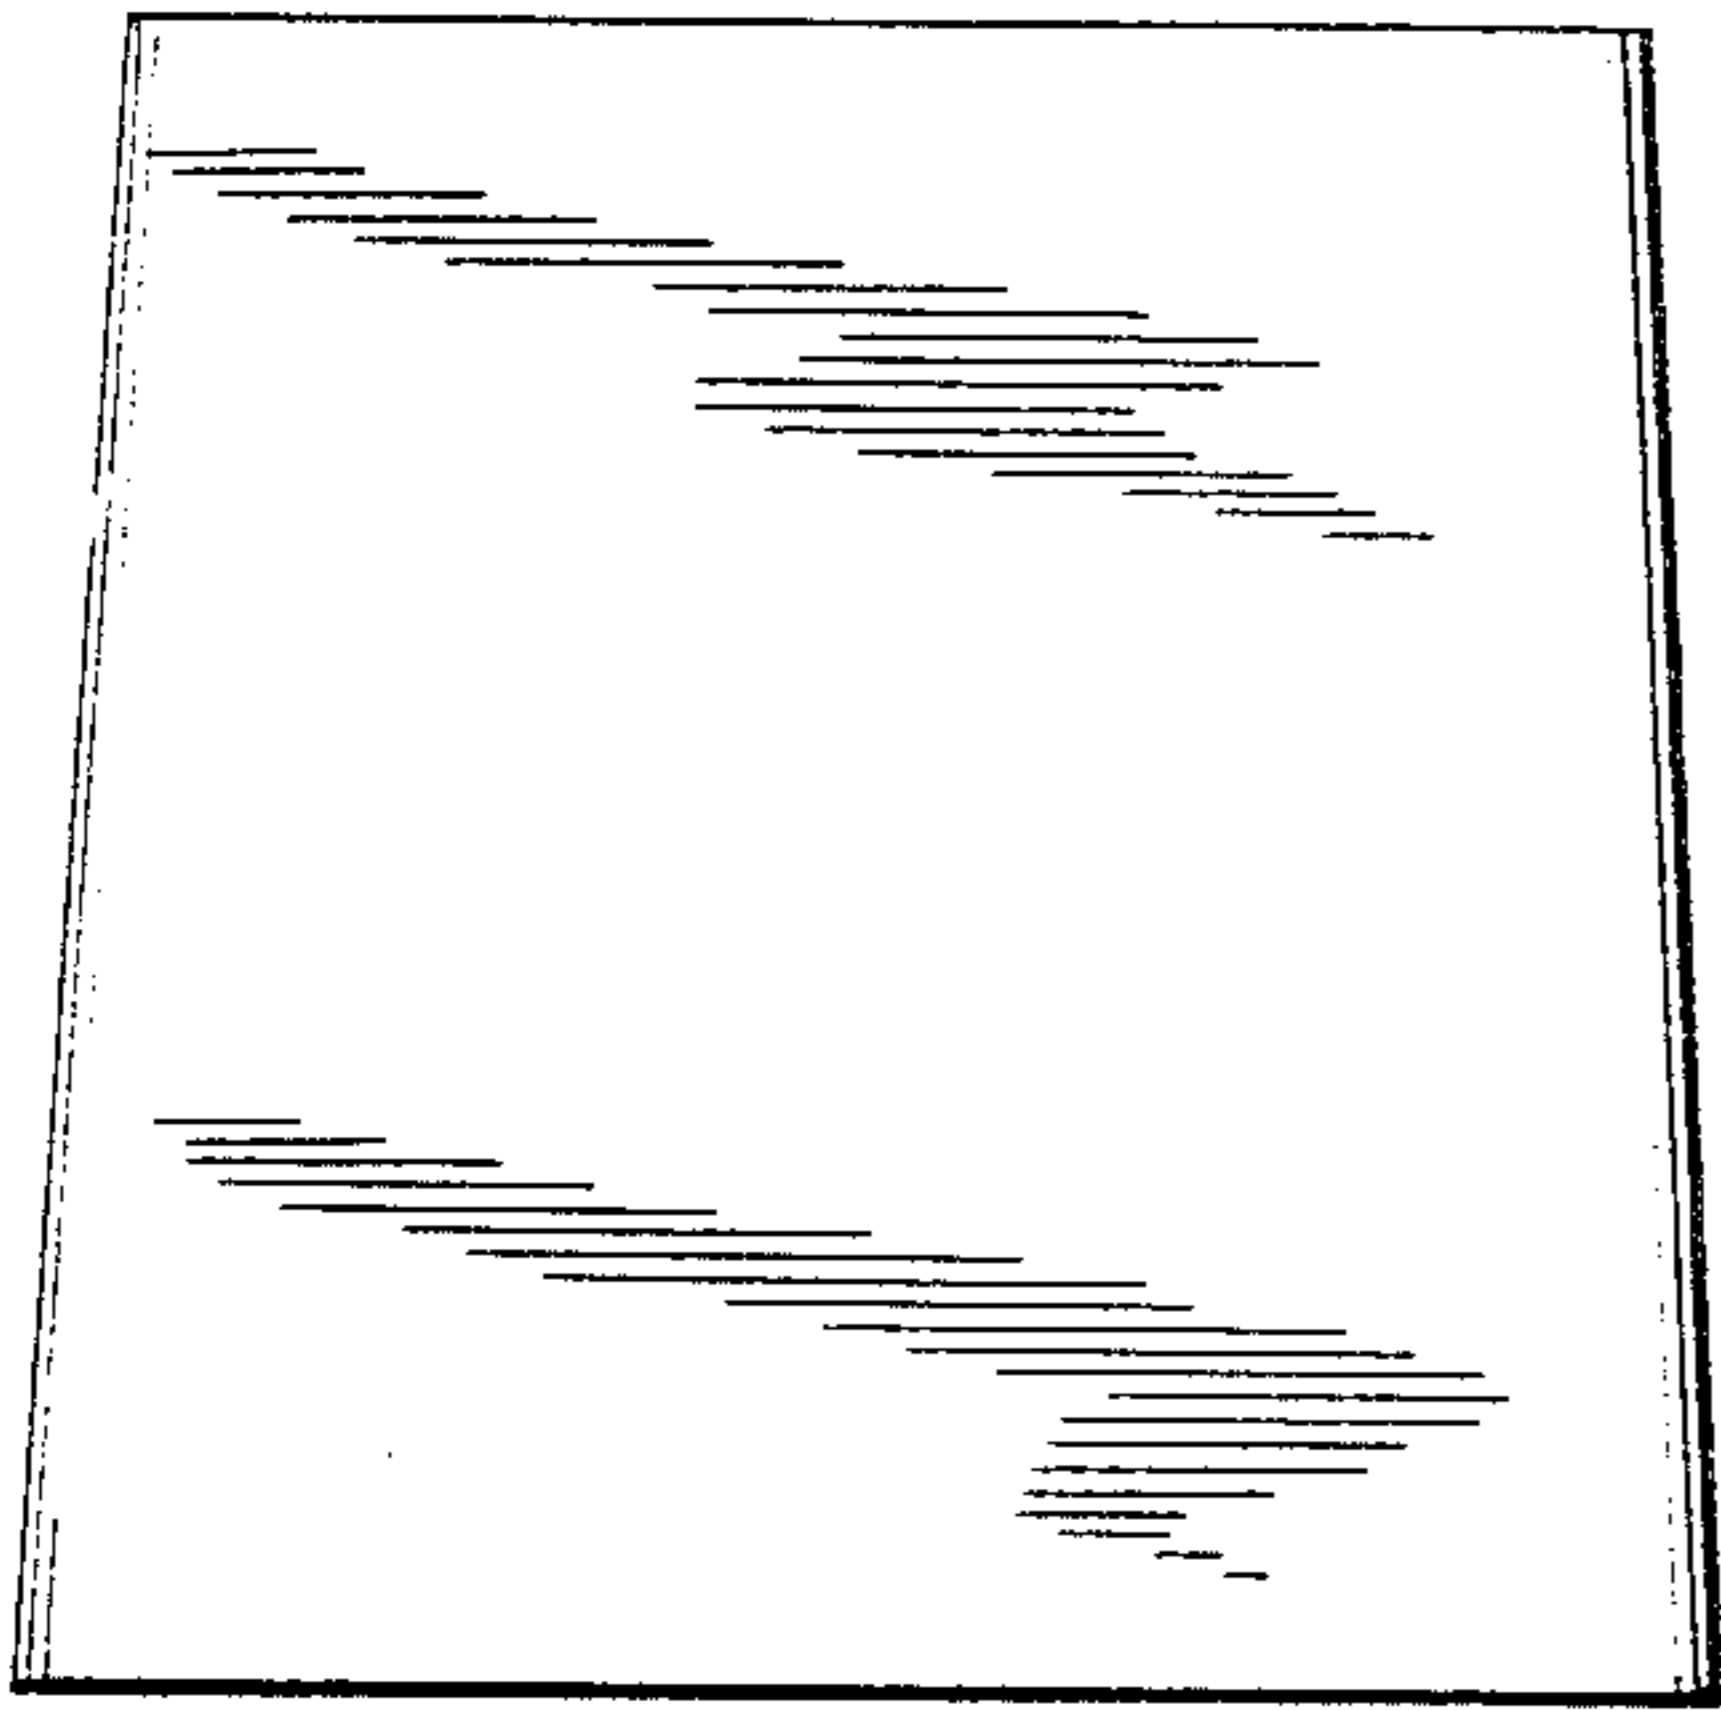


FIG. 4

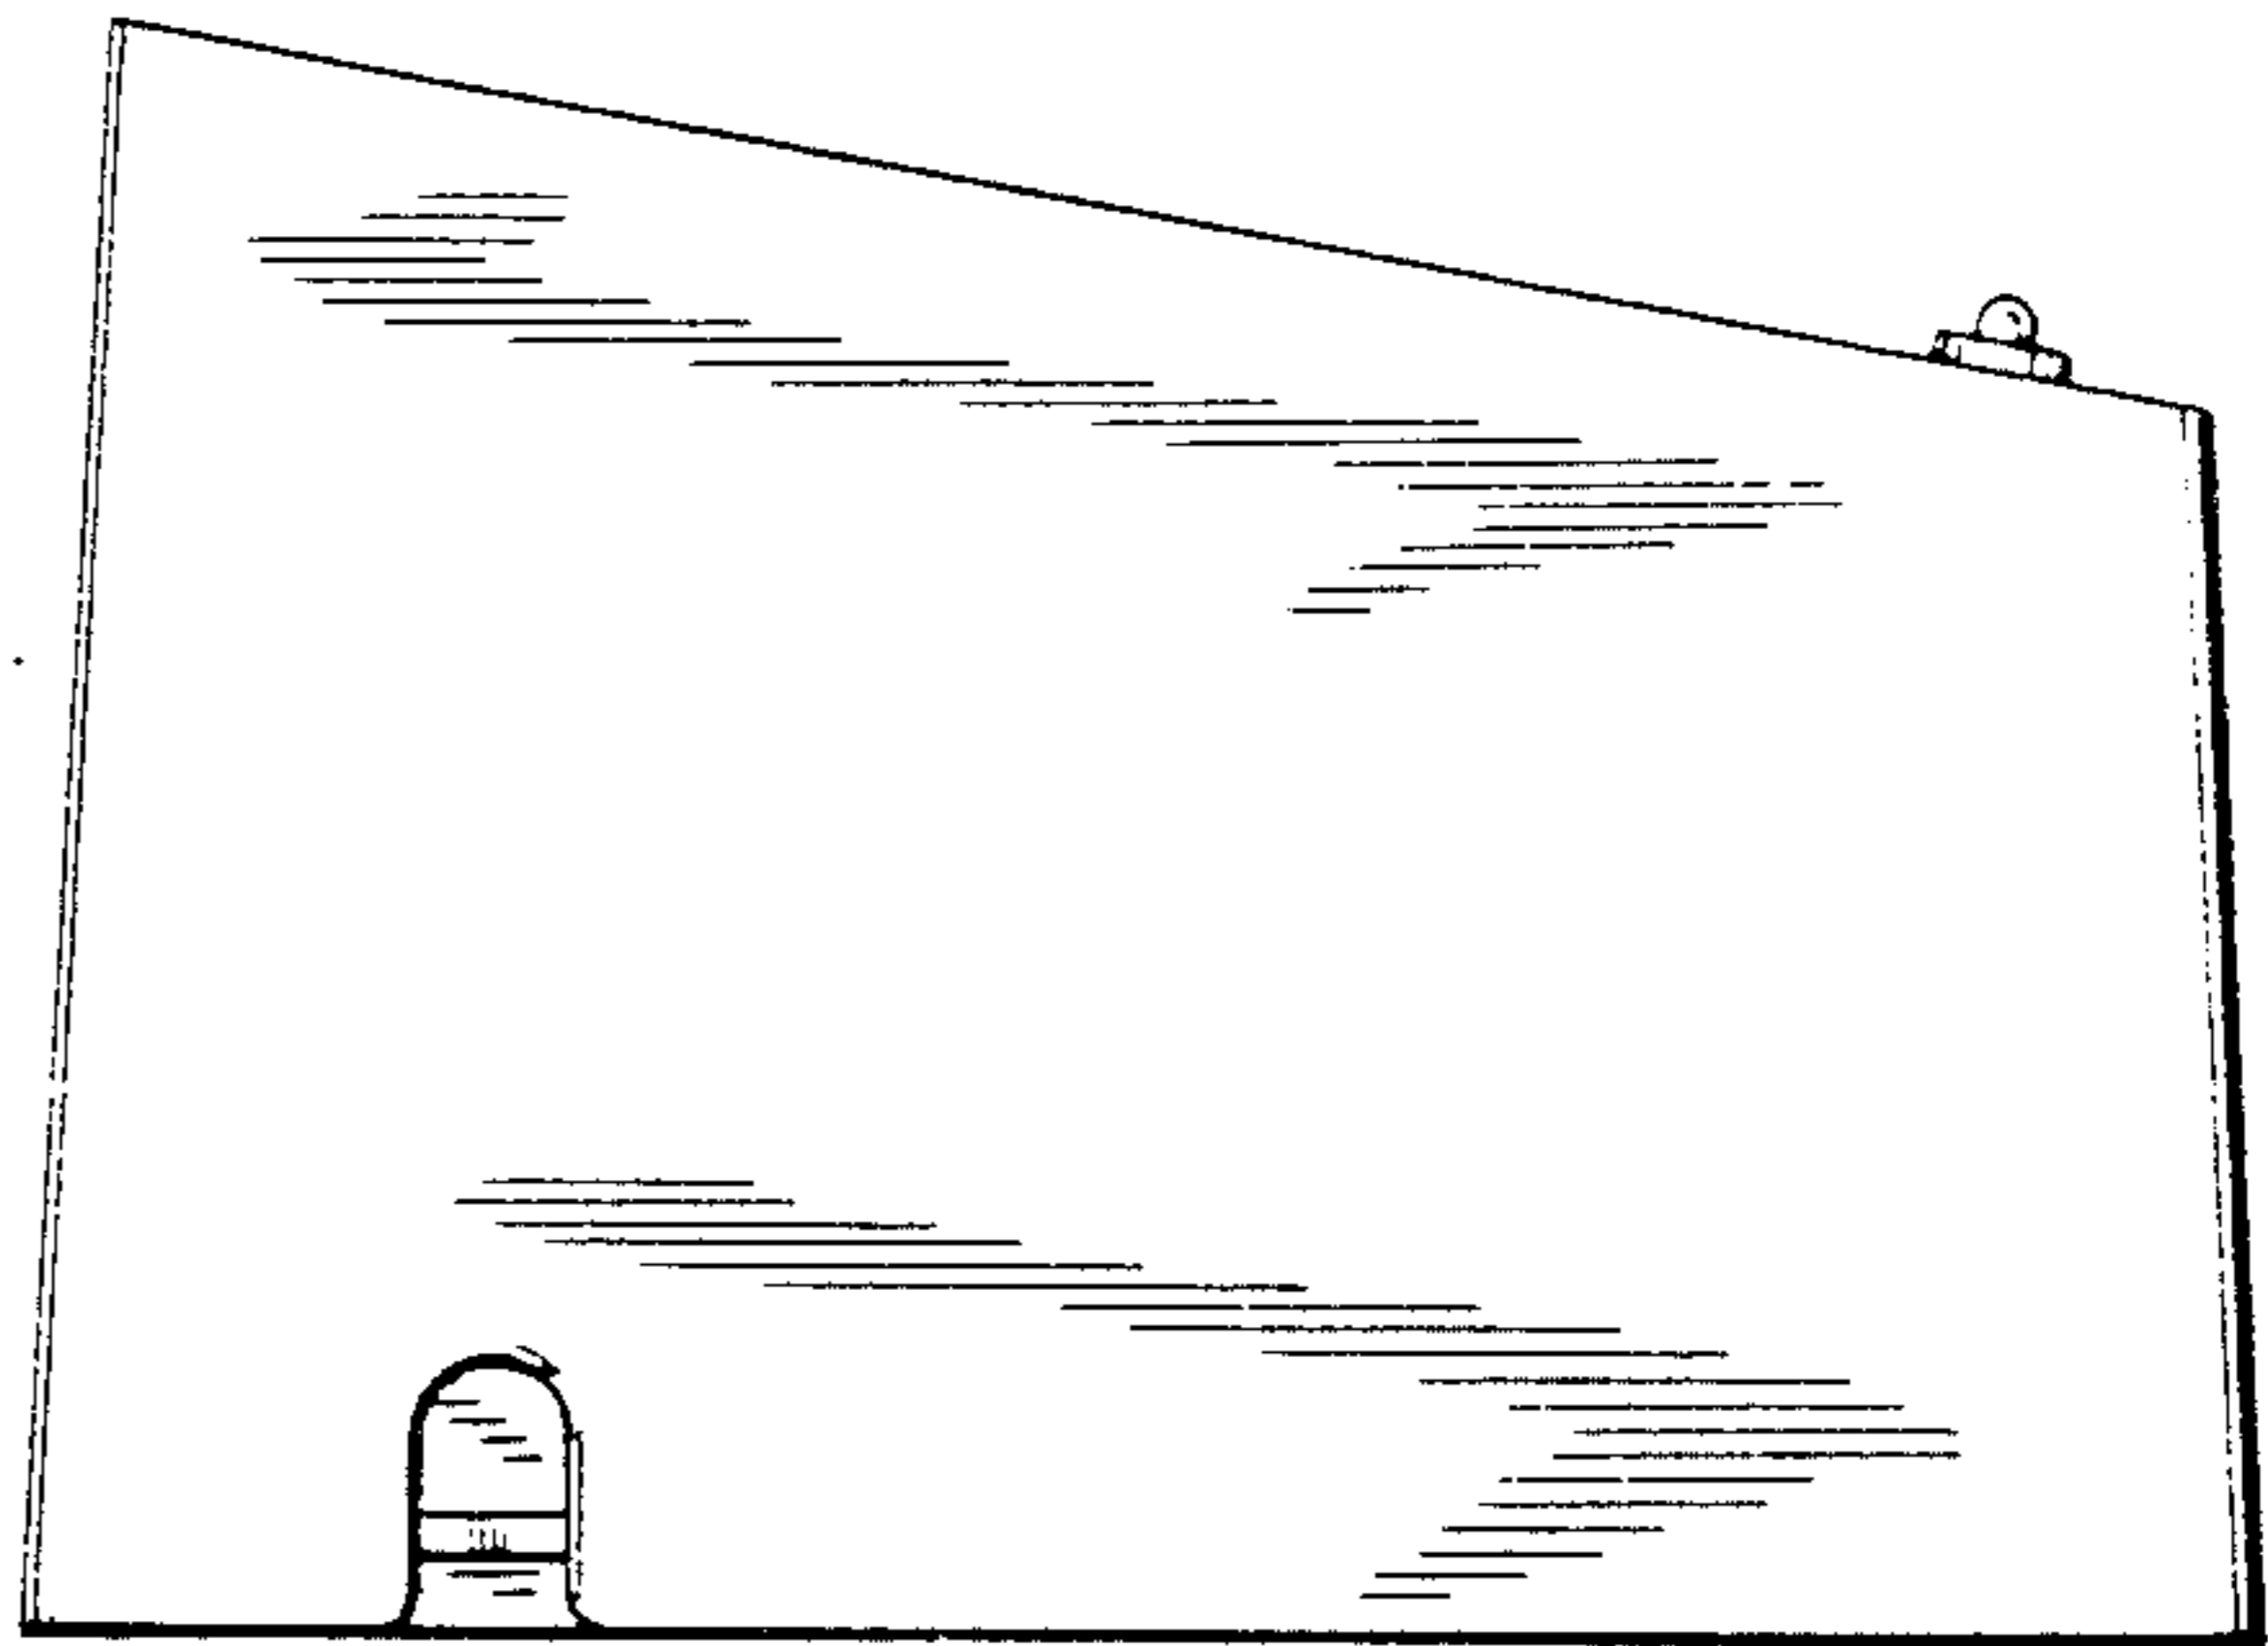


FIG. 3

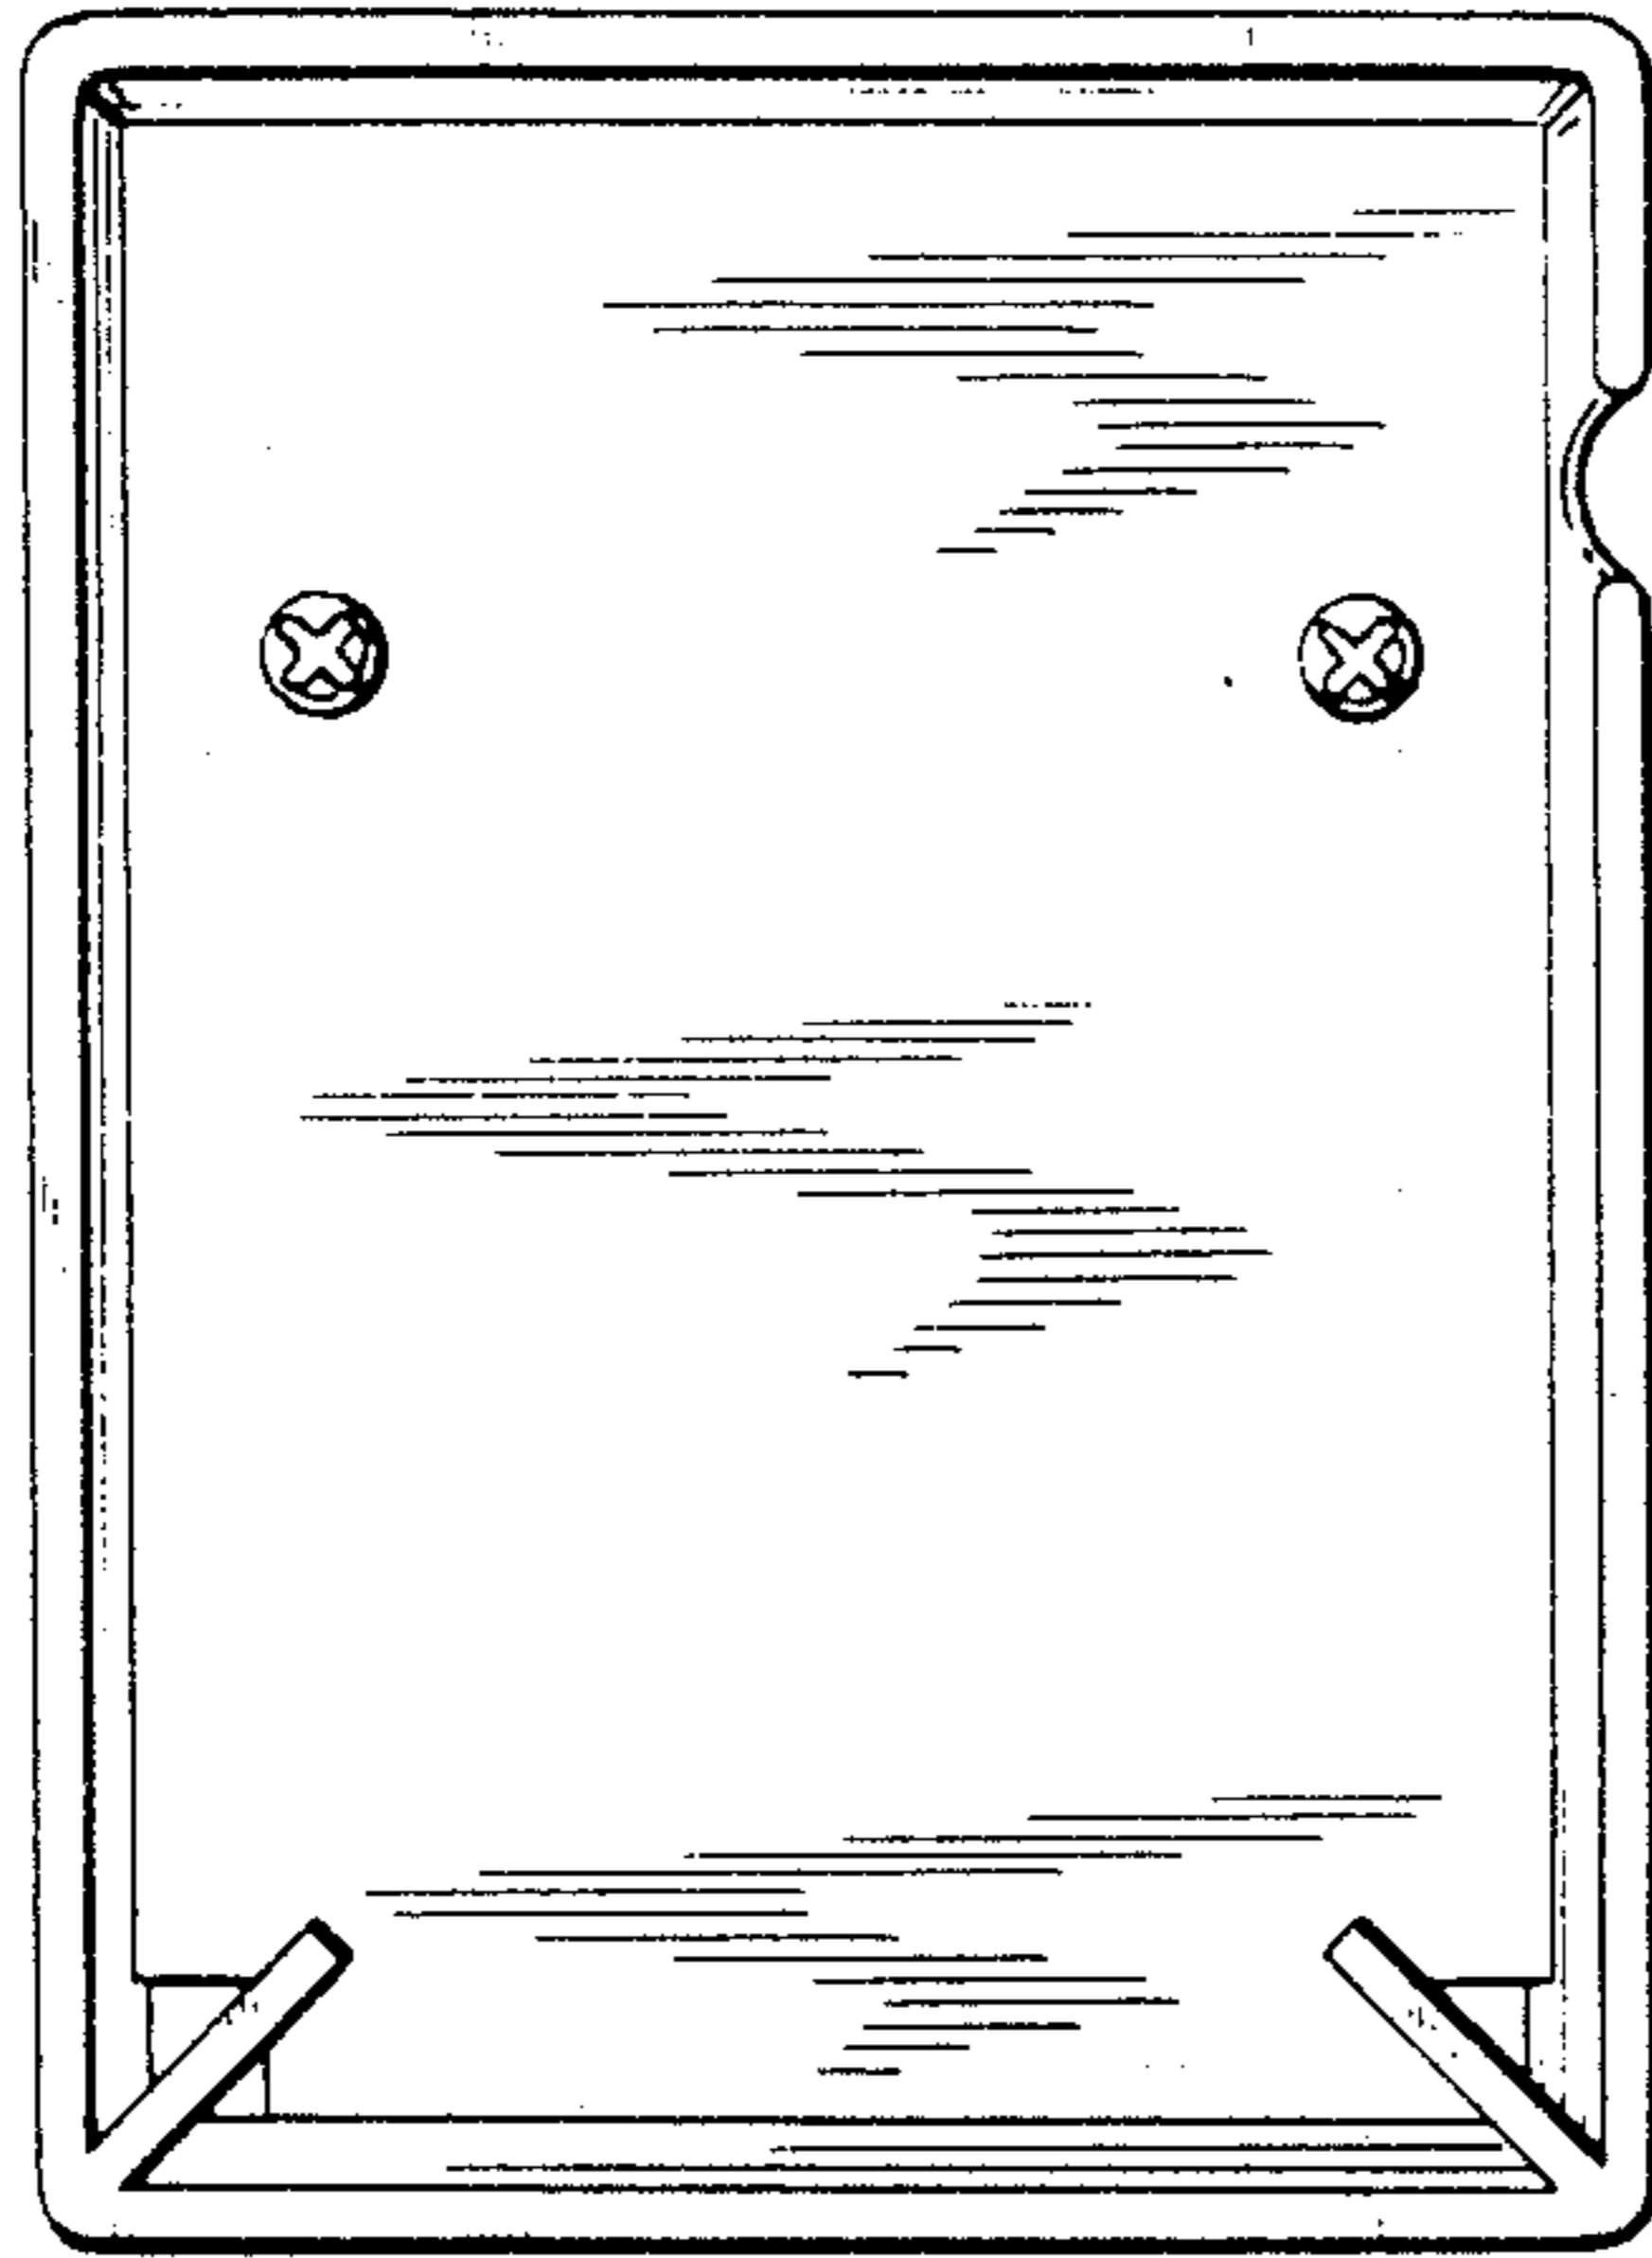


FIG. 5

FIG. 6

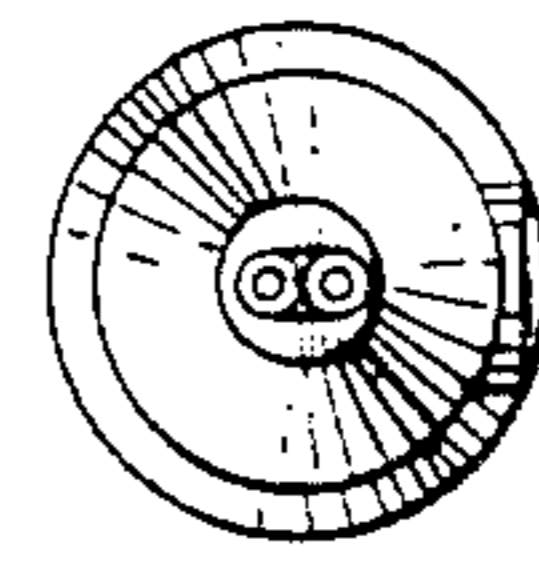
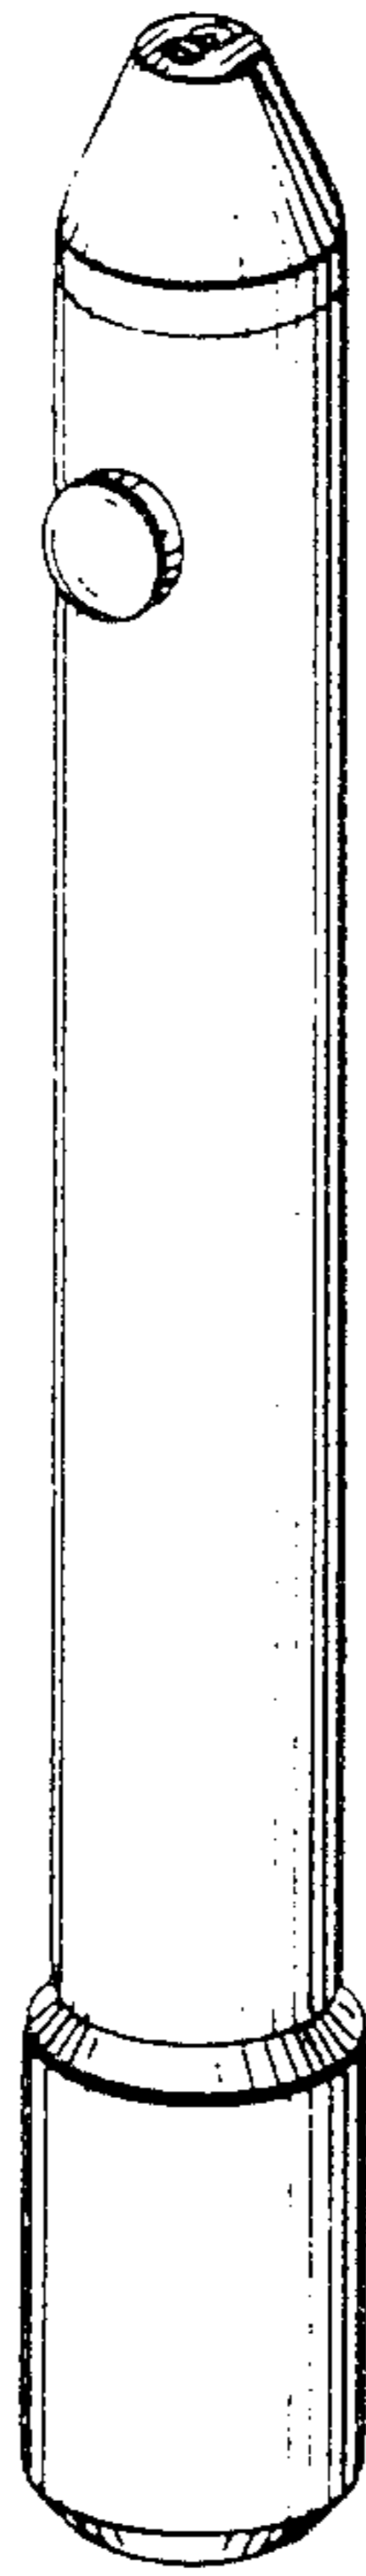


FIG. 7

FIG. 8

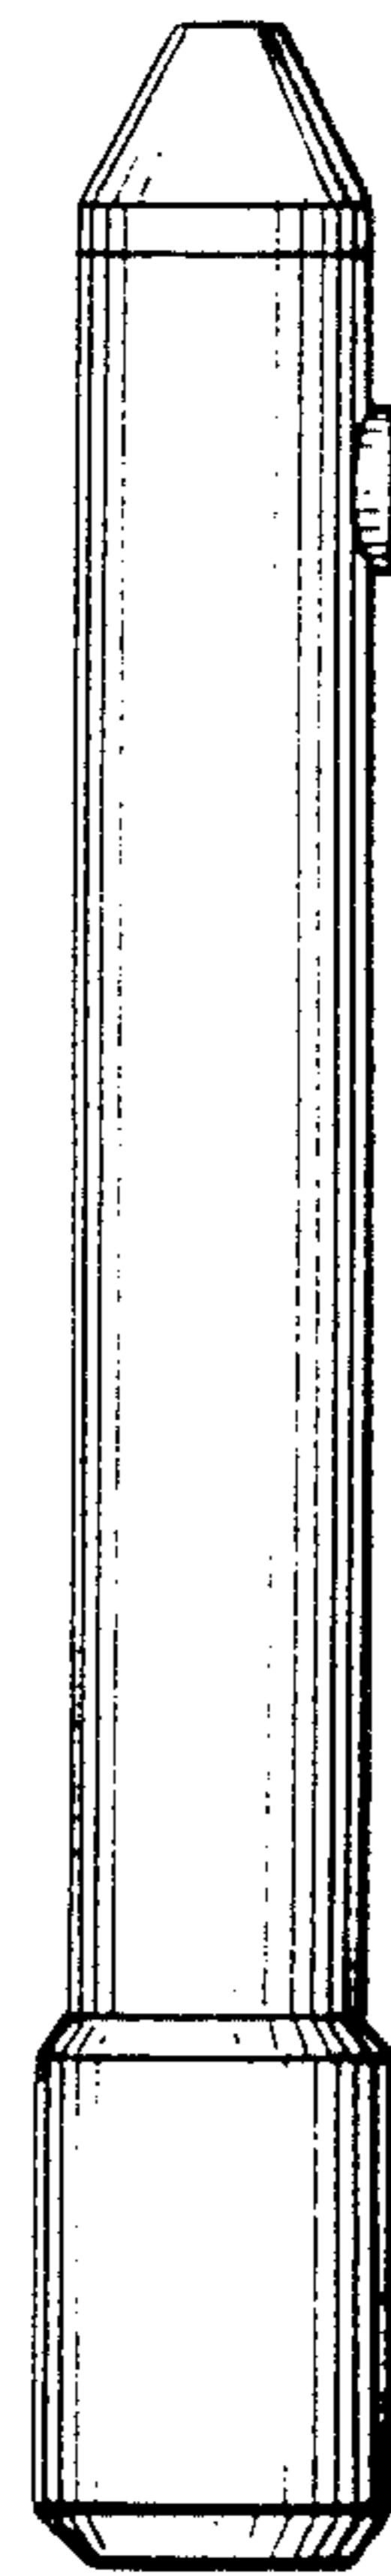


FIG. 9

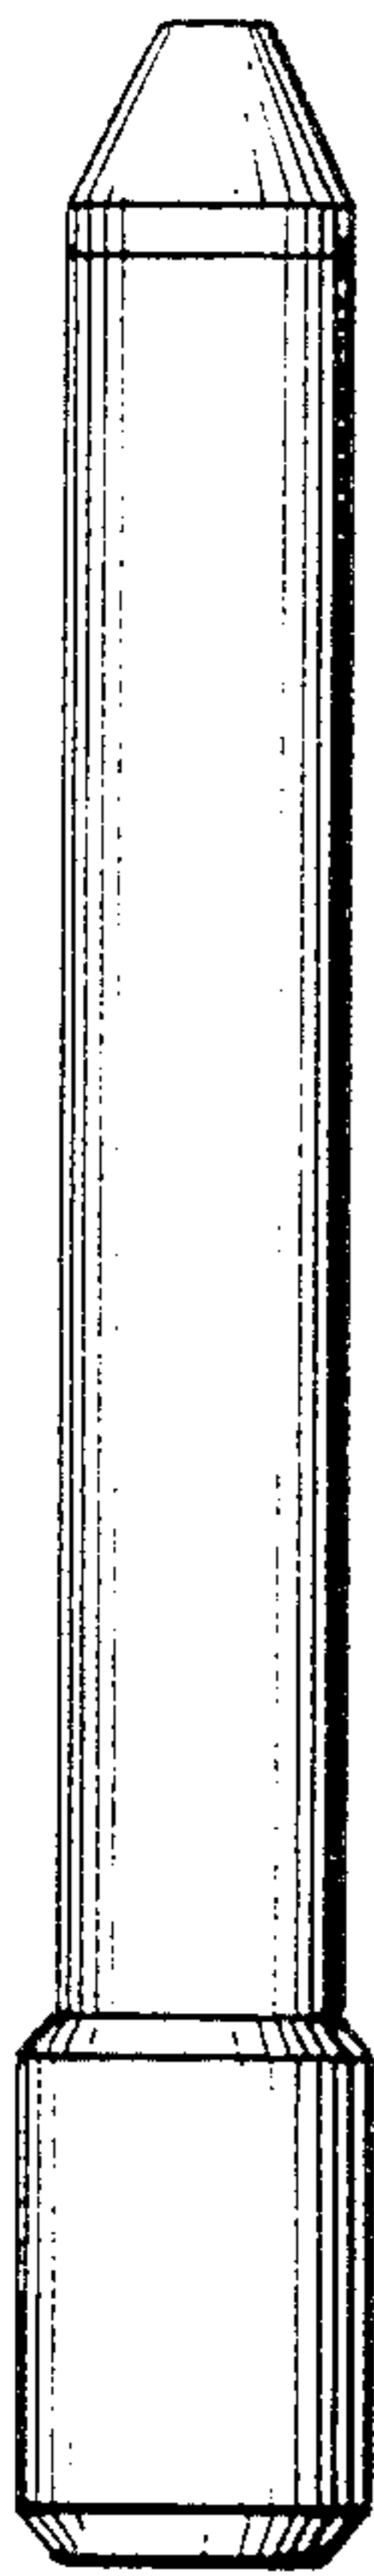
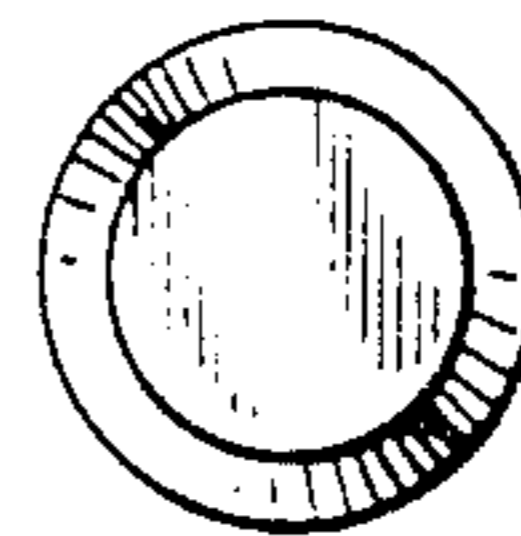


FIG. 10



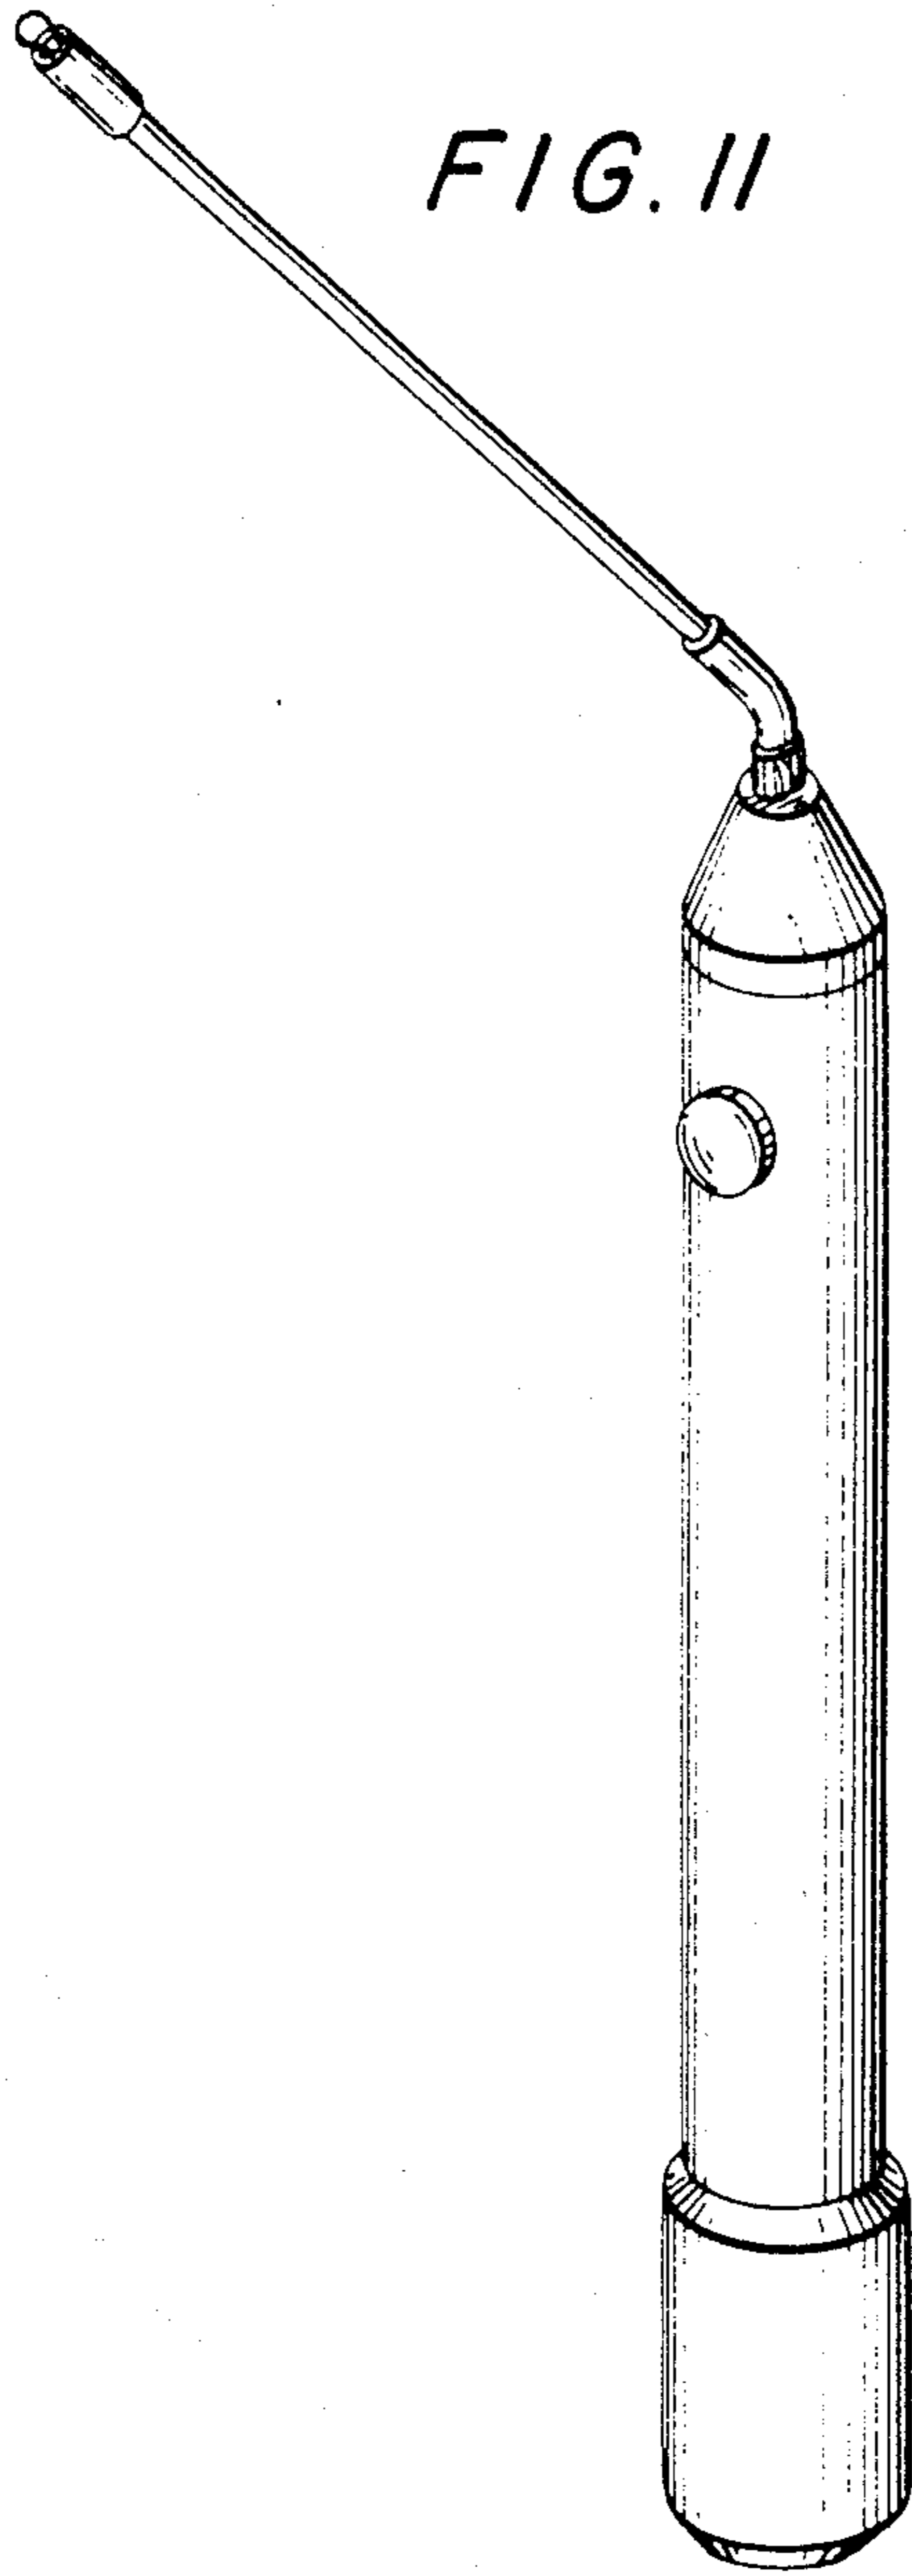


FIG. 11

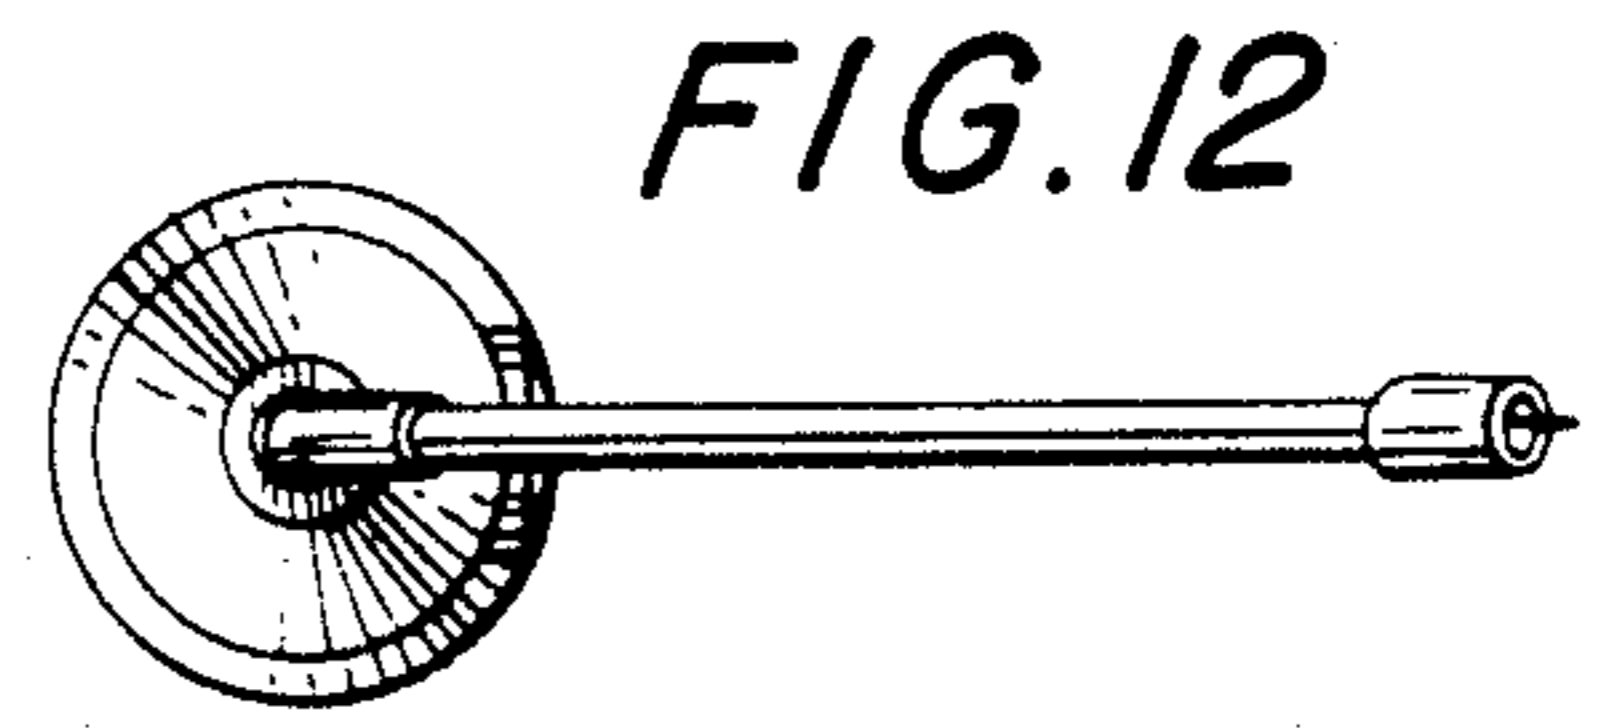


FIG. 12

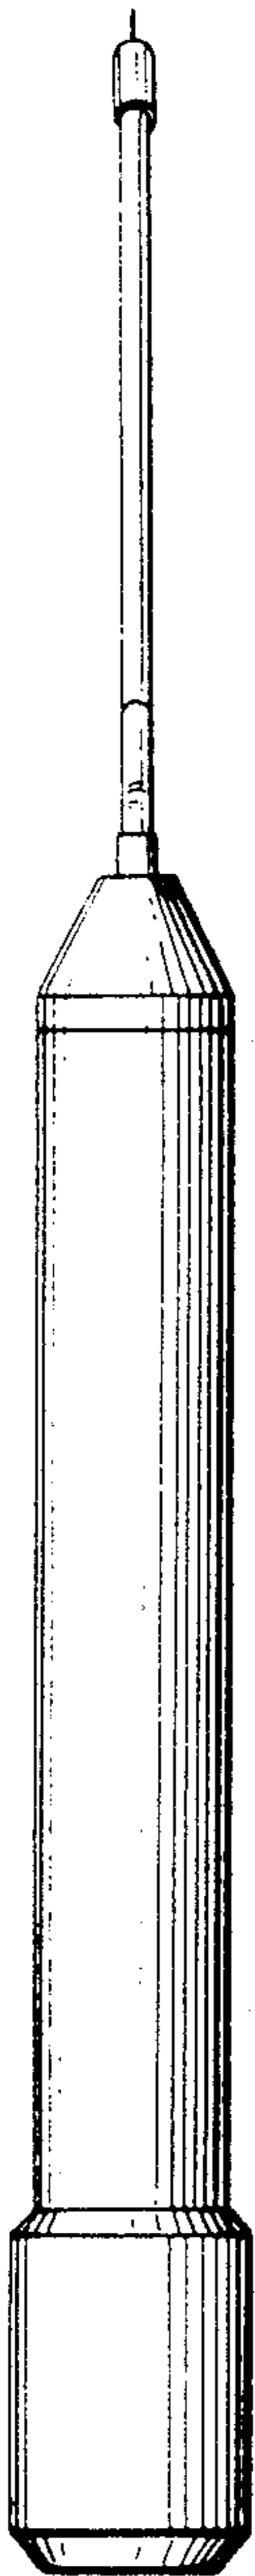


FIG. 14

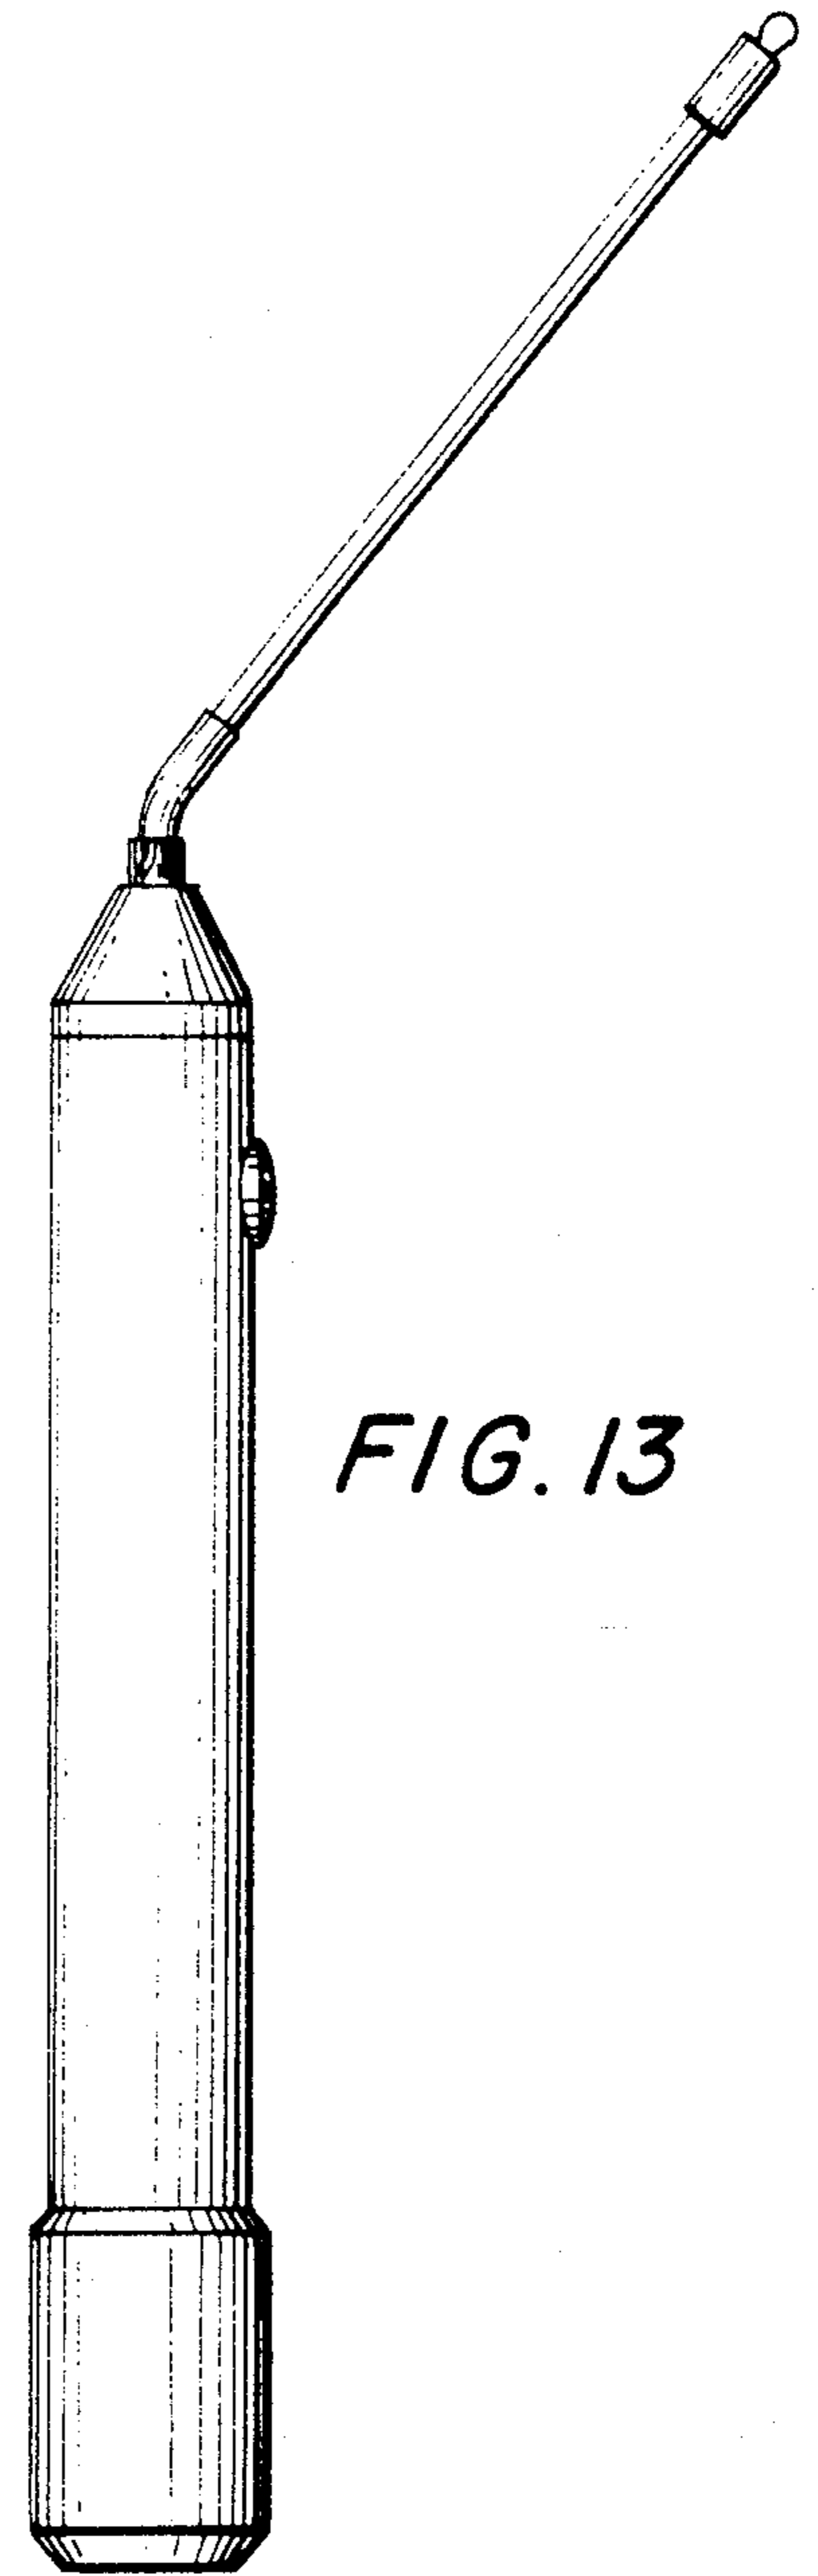


FIG. 13

FIG. 15

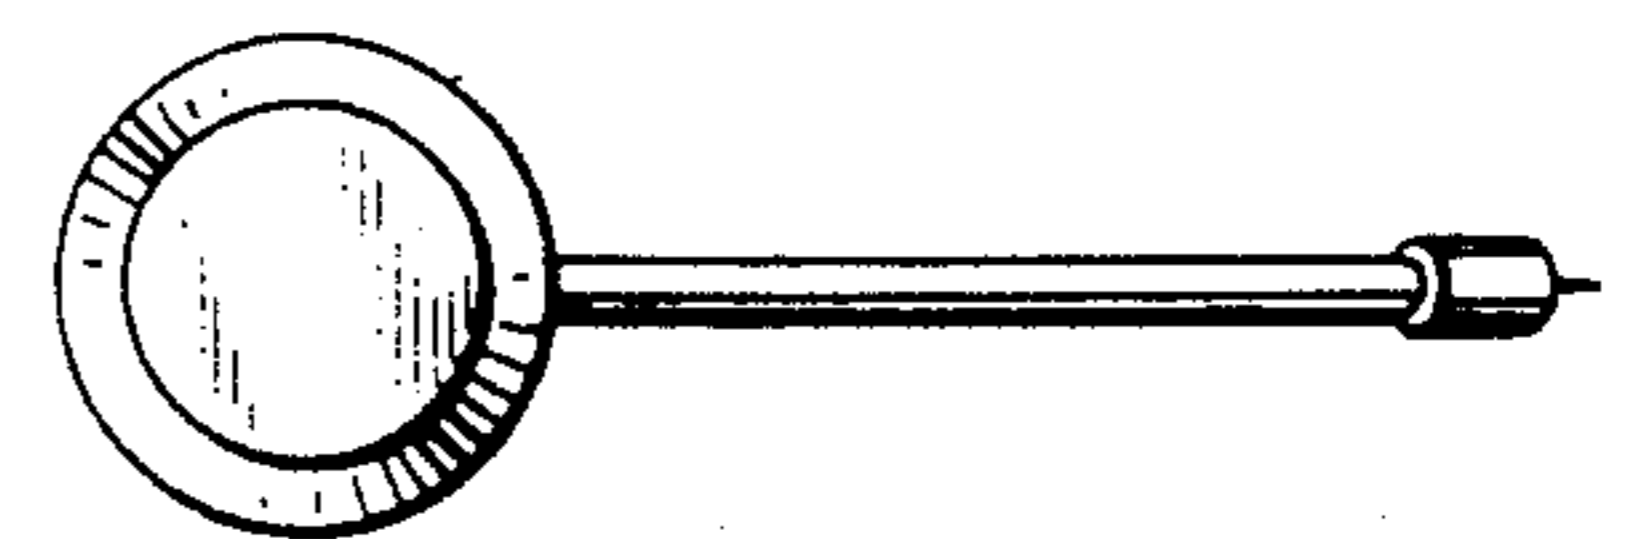


FIG. 16

