

- [54] ENTERAL ADMINISTRATION SET ADAPTER FOR CONNECTION WITH AN ENTERAL FEEDING TUBE
- [75] Inventor: Frank M. Richmond, Harvard, Ill.
- [73] Assignee: Baxter Travenol Laboratories, Inc., Deerfield, Ill.
- [**] Term: 14 Years
- [21] Appl. No.: 474,385
- [22] Filed: Mar. 11, 1983
- [52] U.S. Cl. D24/53
- [58] Field of Search D24/53, 51; 604/175, 604/174, 283, 408, 905, 65, 67, 245, 246, 253, 249; D13/24, 28, 29

[56] References Cited

U.S. PATENT DOCUMENTS

D. 252,470	7/1979	Pawlak	D24/54
D. 257,062	9/1980	Swartz et al.	D24/53
4,294,250	10/1981	Dennehey	604/408
4,296,949	10/1981	Muetterties et al.	604/174 X
4,335,770	6/1982	Kulle et al.	.	
4,397,442	8/1983	Larkin	604/249

FOREIGN PATENT DOCUMENTS

2486803	1/1982	France	604/905
---------	--------	--------	-------	---------

OTHER PUBLICATIONS

- U.S. Ser. No. 434,646 filed Oct. 15, 1982, Gerald J. Sukel, "Roller Pump Set".
- U.S. Ser. No. 399,395 filed July 19, 1982, Robert A.

Miller, et al., "Enteral" Administration Set Adapter For Connection With An Enteral Feeding Tube. Vivonex™ Tungsten Tip Nasogastric Nasointestinal Feeding Tube, distributed by Norwich-Eaton Pharmaceuticals.

Primary Examiner—A. Hugo Word
Assistant Examiner—Stella M. Reid
Attorney, Agent, or Firm—Bradford R. L. Price; Paul C. Flattery; Robert M. Barrett

[57] CLAIM

The ornamental design for an enteral administration set adapter for connection with an enteral feeding tube, substantially as shown and described.

DESCRIPTION

FIG. 1 is a top perspective view of an enteral administration set adapter for connection with an enteral feeding tube showing my new design; the enteral administration set tubing shown in phantom line is for illustrative purposes only and forms no part of the claimed design.

FIG. 2 is a bottom perspective view of the adapter shown in FIG. 1;

FIG. 3 is a side elevational view of the adapter shown in FIG. 1;

FIG. 4 is an end elevational view of the adapter shown in FIG. 1;

FIG. 5 is a top plan view of the adapter shown in FIG. 1; and

FIG. 6 is a bottom plan view of the adapter shown in FIG. 1.

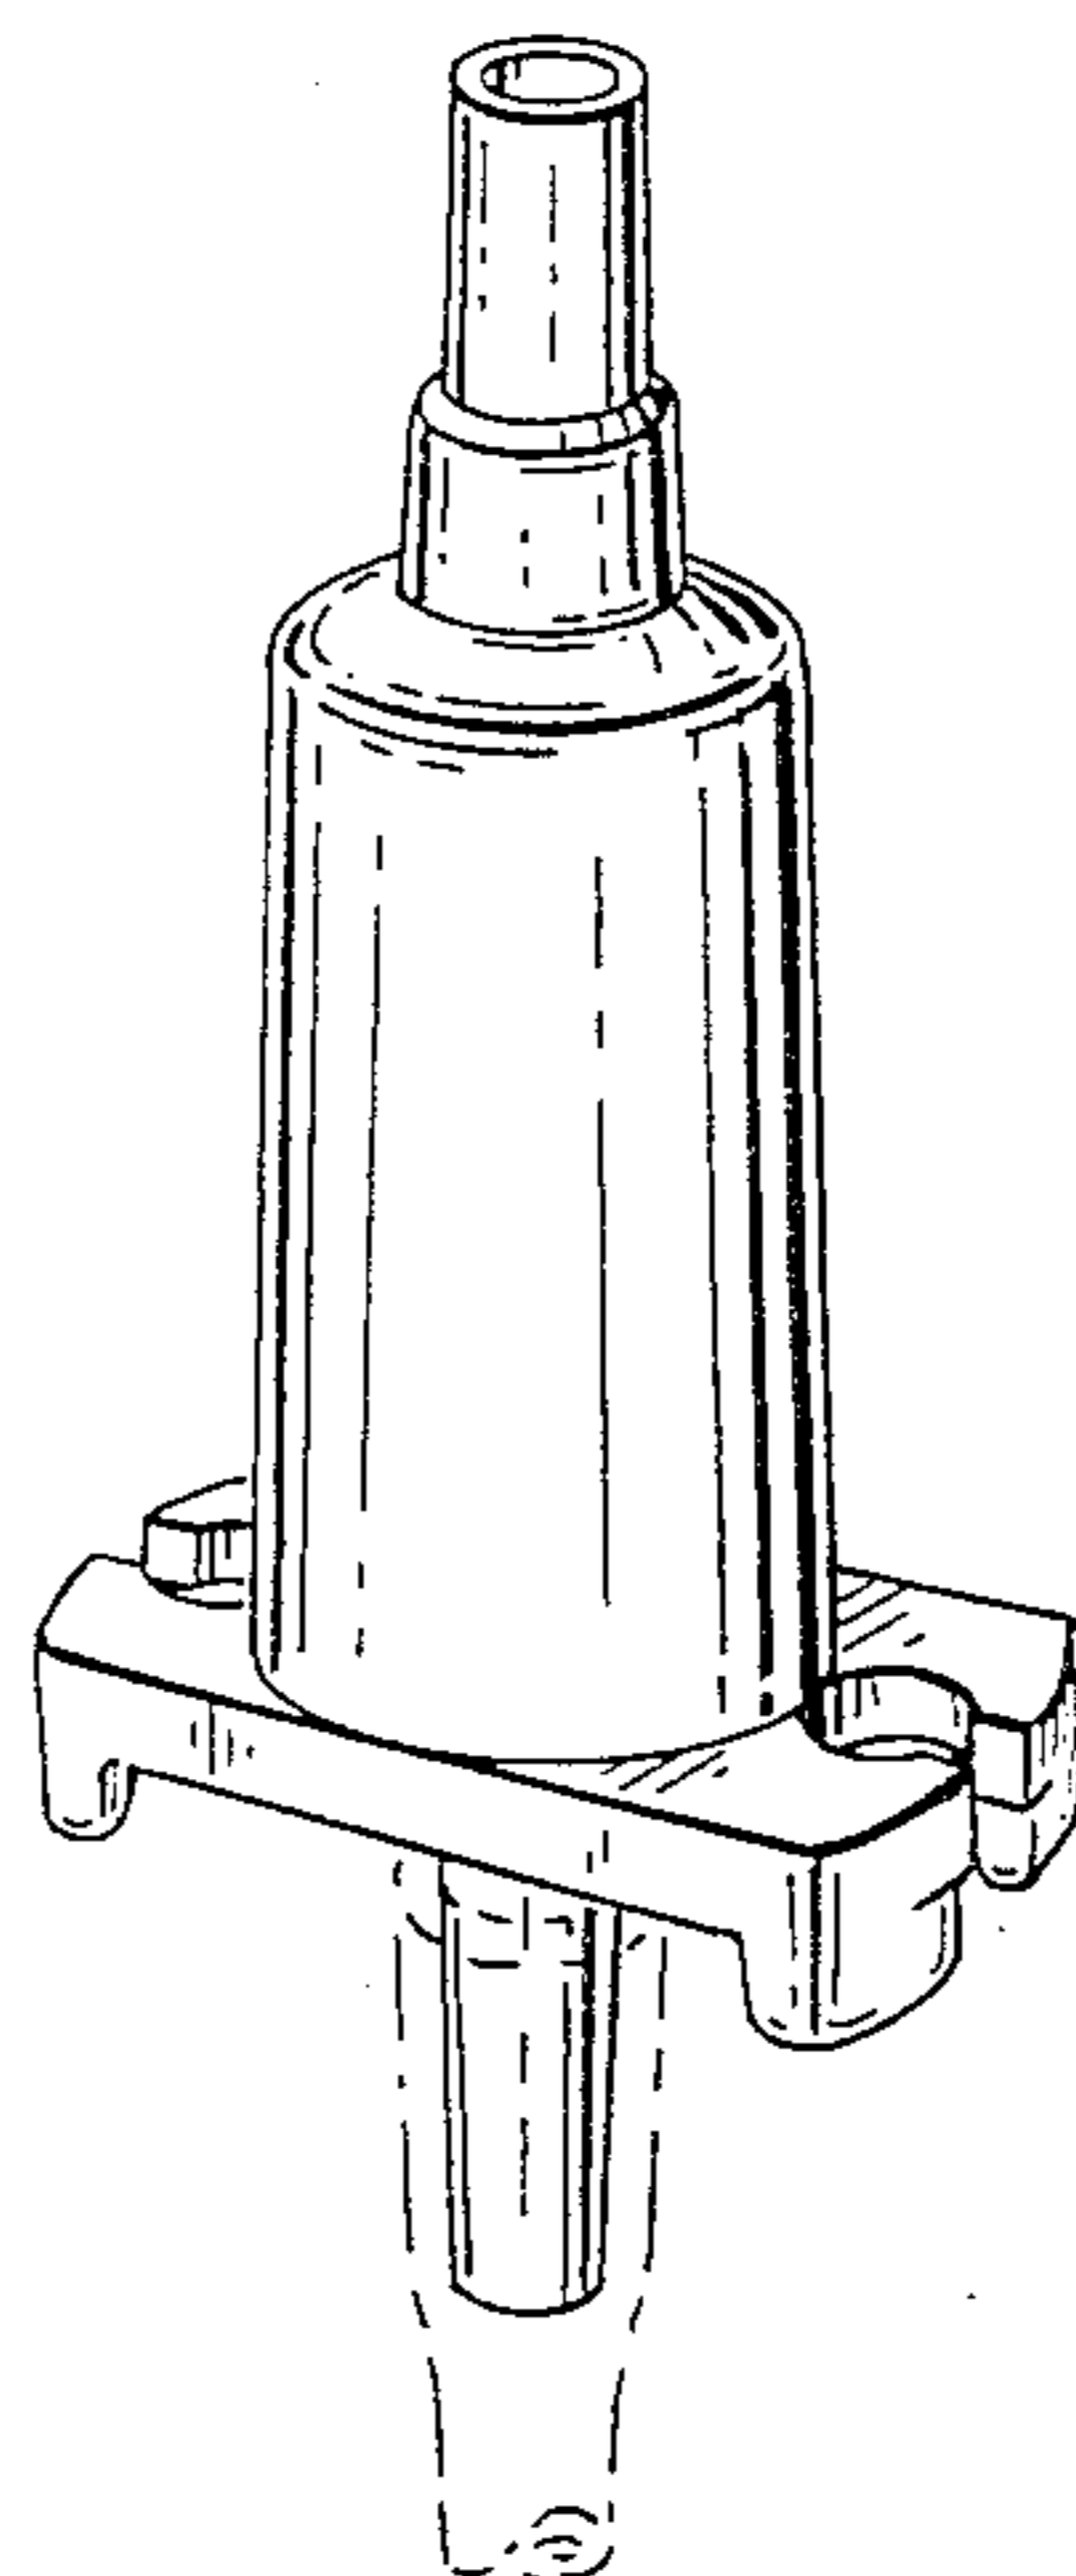


FIG. 1

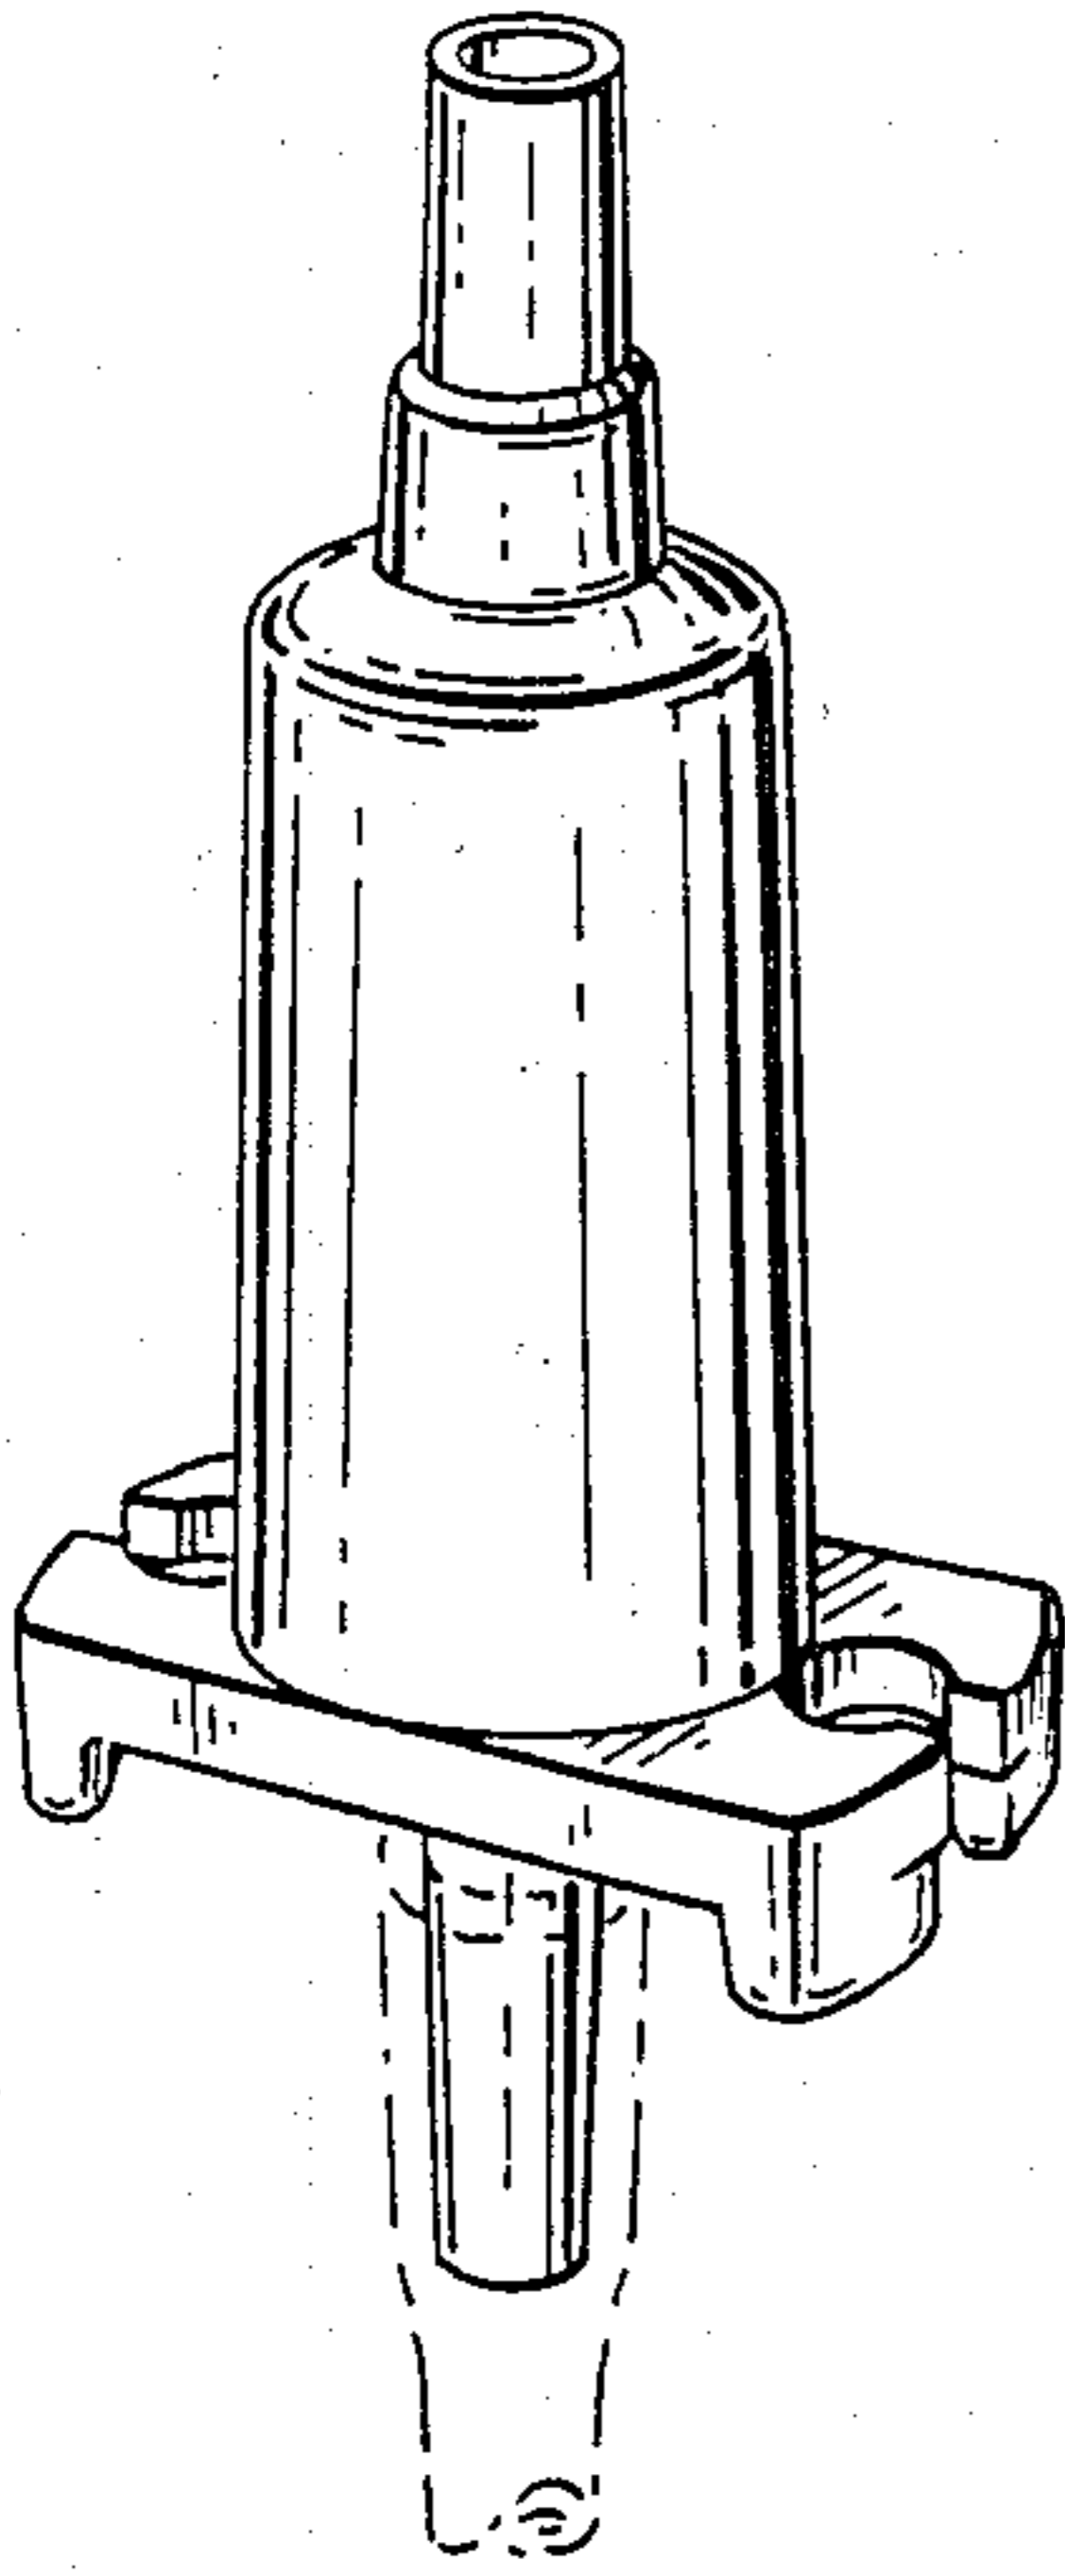


FIG. 2

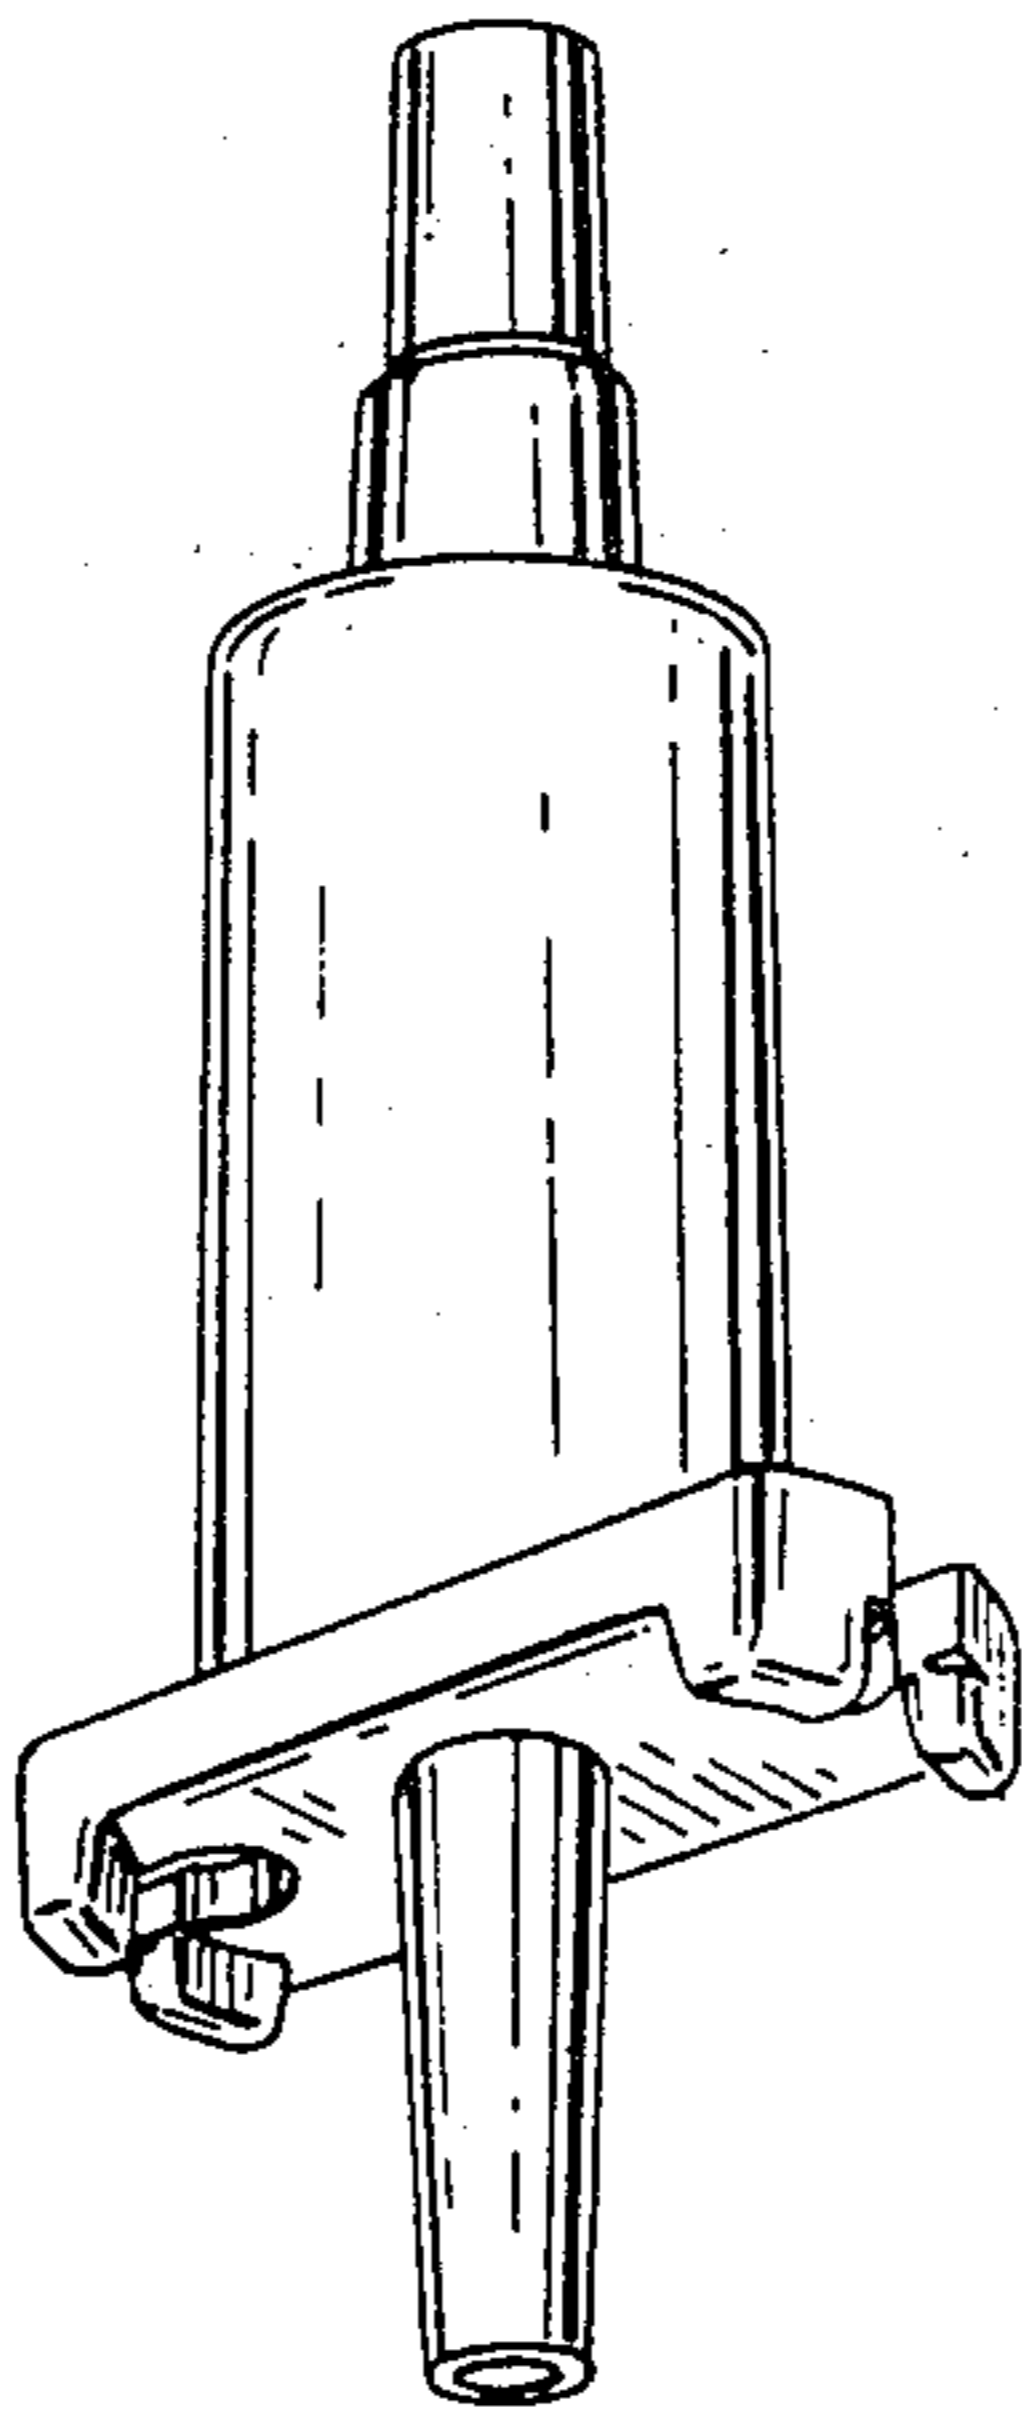


FIG. 3

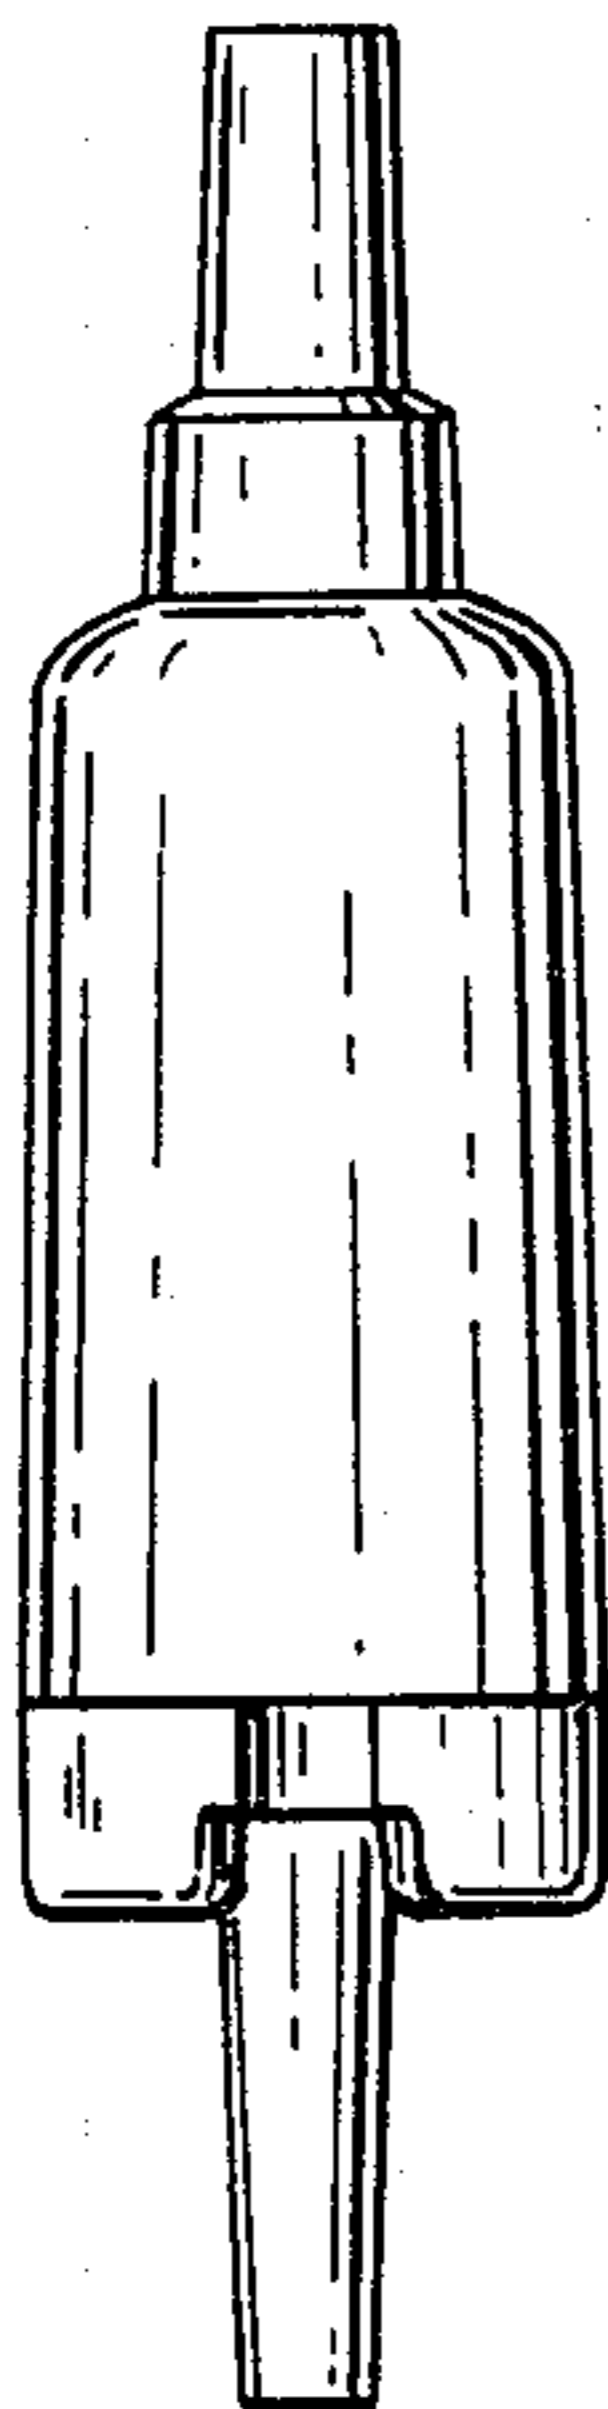
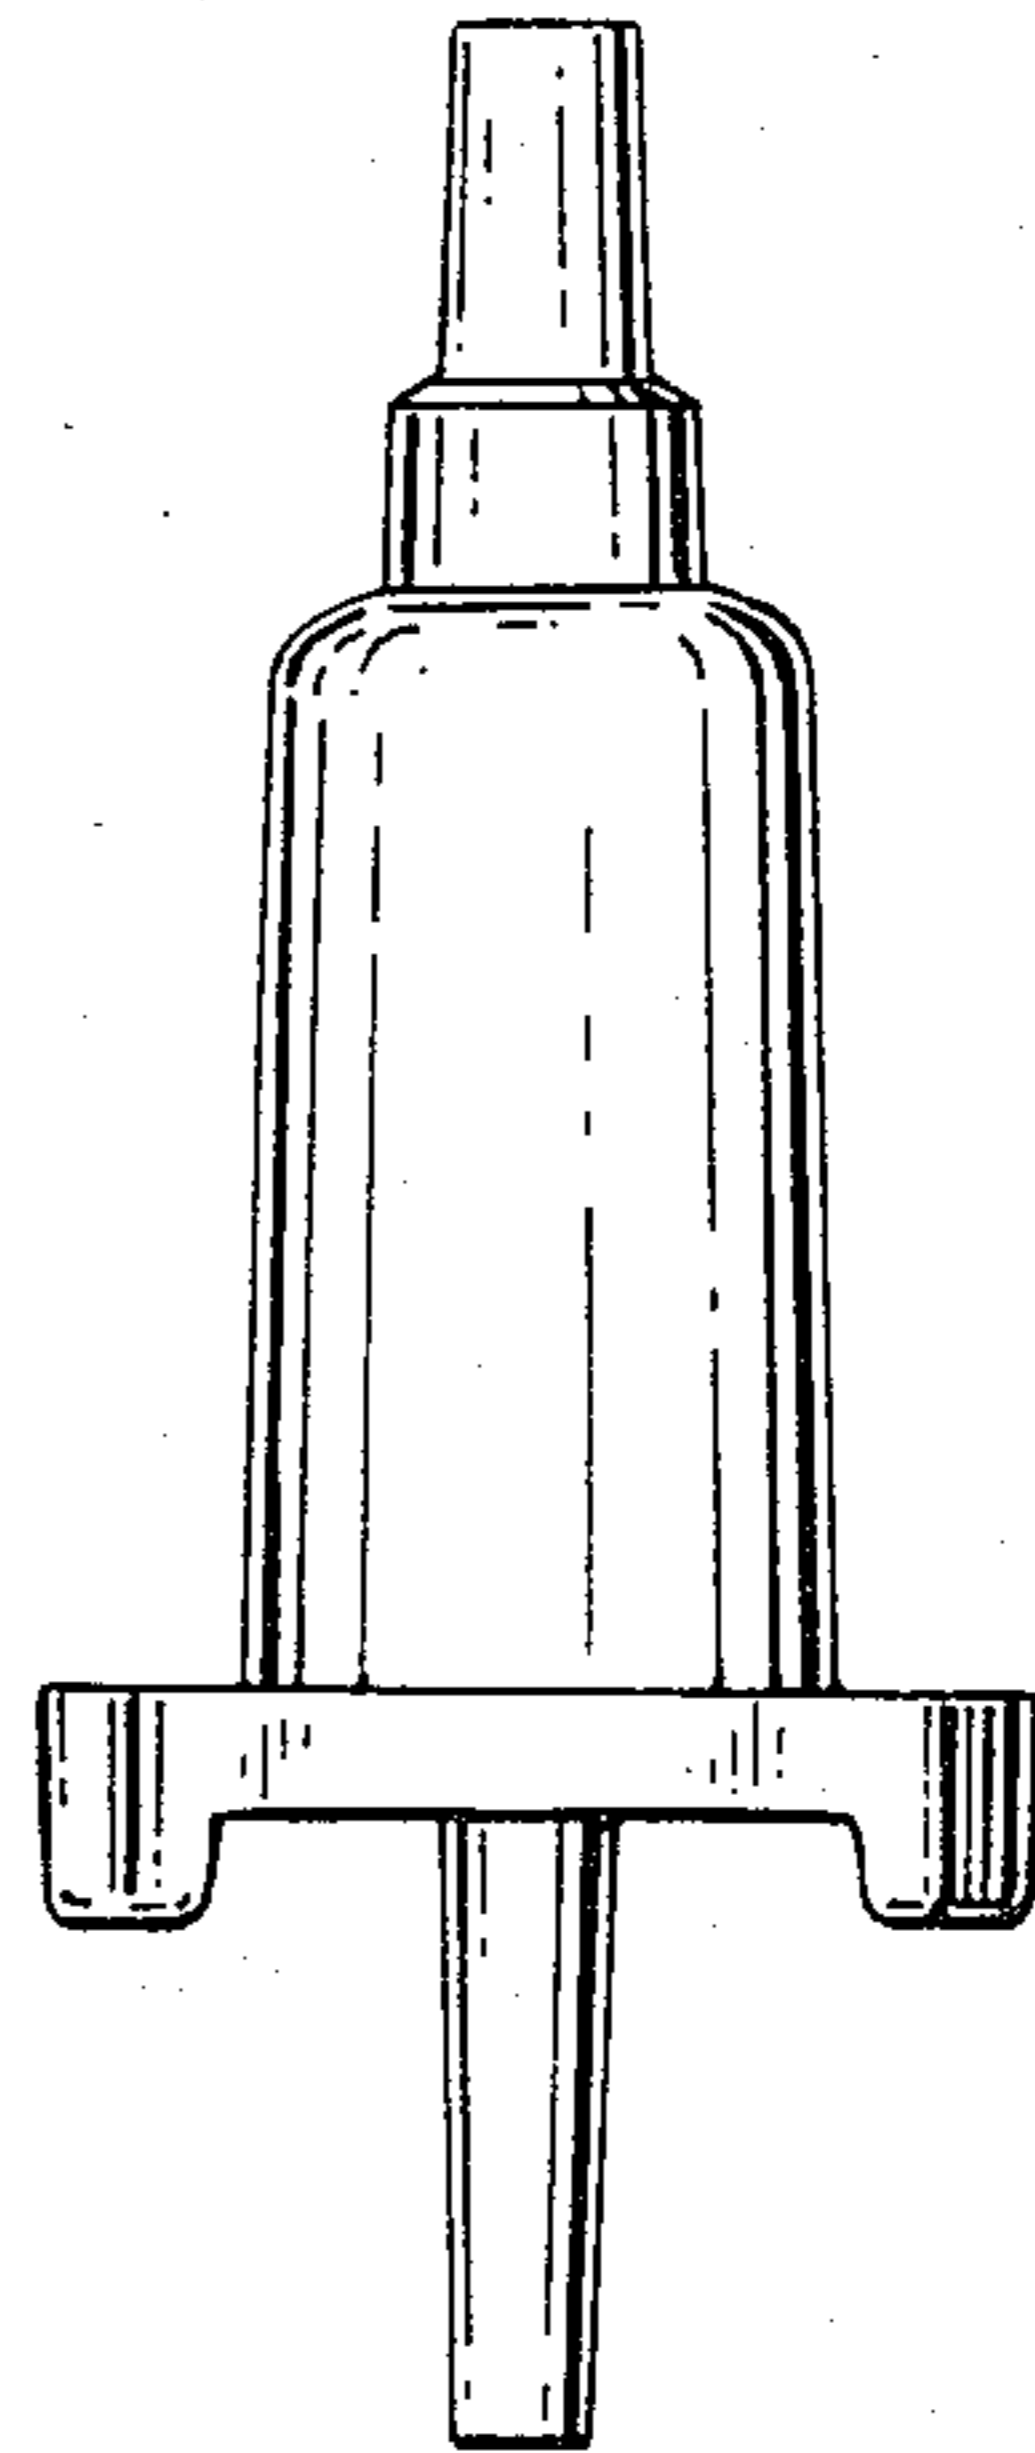


FIG. 4

FIG. 5

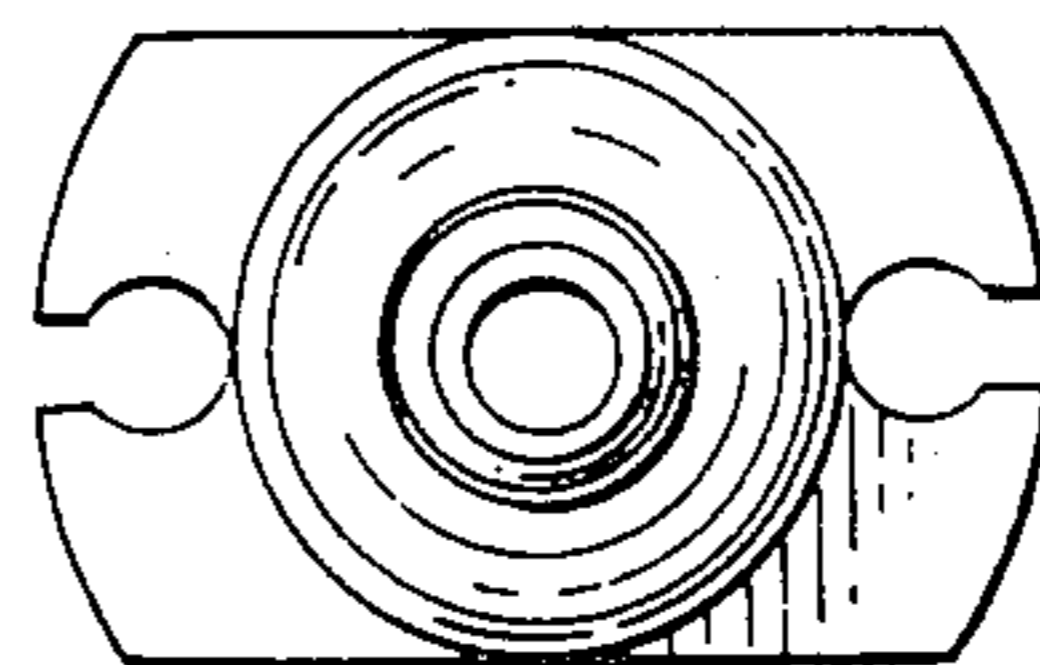


FIG. 6

