

[54] **DOSIMETER FOR MONITORING RADIATION EXPOSURE**

[75] Inventors: **Robert Pollock, Aurora, Ill.; Douglas Patton; David Sharbaugh, both of Irvine, Calif.; John Goodin, Long Beach, Calif.**

[73] Assignee: **Siemens Gammasonics, Inc., Des Plaines, Ill.**

[**] Term: **14 Years**

[21] Appl. No.: **468,117**

[22] Filed: **Feb. 28, 1983**

[52] U.S. Cl. **D10/47**

[58] Field of Search **D10/47, 81, 96; 250/472.1, 475.2, 482.1; D11/95**

[56] **References Cited**

U.S. PATENT DOCUMENTS

- D. 188,251 6/1960 Leone D20/27
- D. 217,257 4/1970 Baker et al. D11/95

- 2,496,218 1/1950 Kieffer 250/482.1
- 2,659,013 11/1953 Davis et al. 250/482.1
- 2,706,939 4/1955 Fairbank 250/475.2 X
- 2,753,460 7/1956 Reed et al. 250/482.1

Primary Examiner—Bernard Ansher
Assistant Examiner—Terry Pfeffer
Attorney, Agent, or Firm—Mark H. Jay



[57] **CLAIM**

The ornamental design for a dosimeter for monitoring radiation exposure, as shown and described.

DESCRIPTION

FIG. 1 is a front elevational view of the dosimeter for monitoring radiation exposure showing our new design; FIG. 2 is a rear elevation view thereof; FIG. 3 is a top plan view thereof; FIG. 4 is a left side elevational view thereof; and FIG. 5 is a bottom front right side perspective view thereof.

The broken lines in FIG. 5 are a wire clamp that is shown for illustrative purposes only.

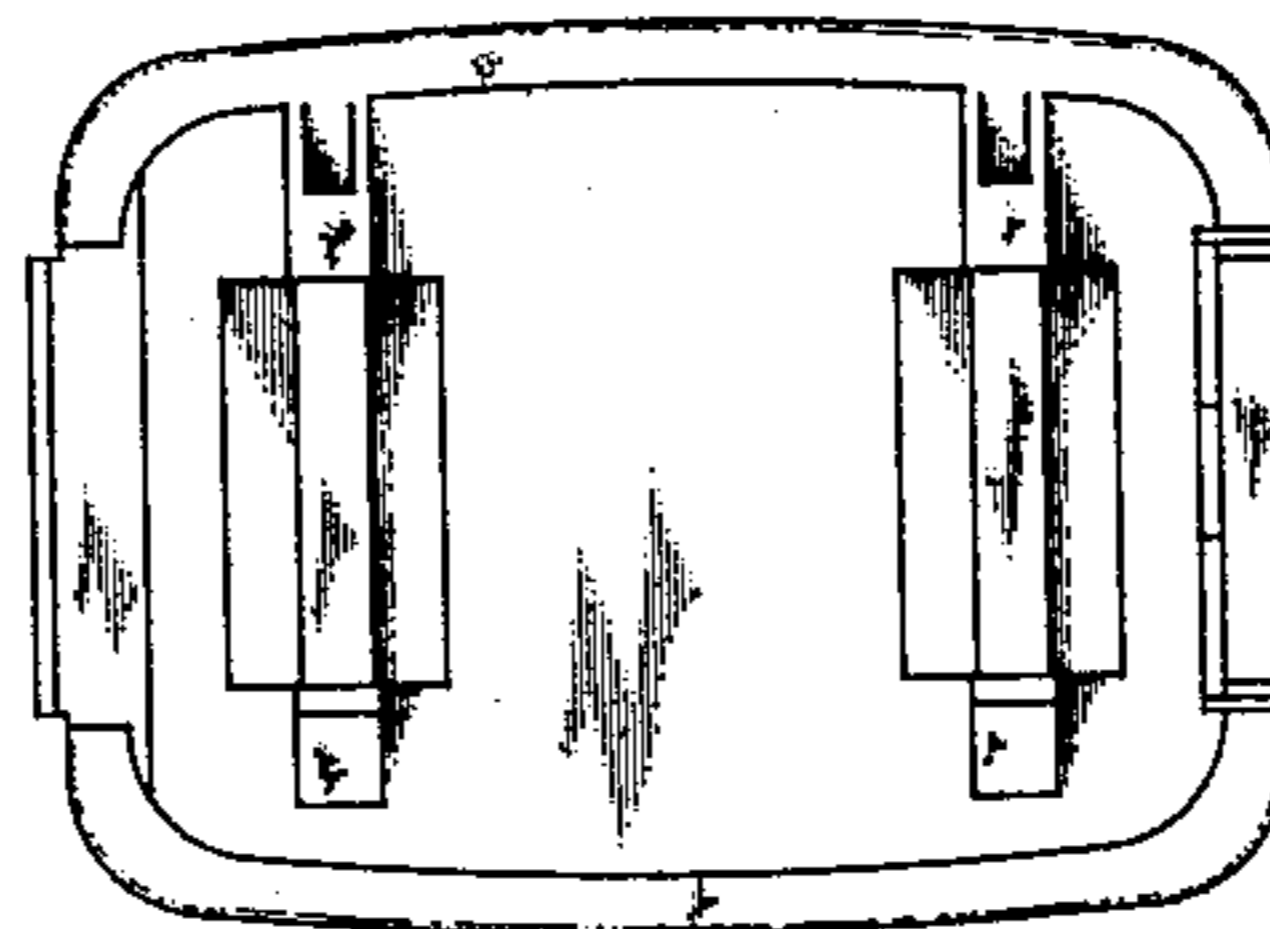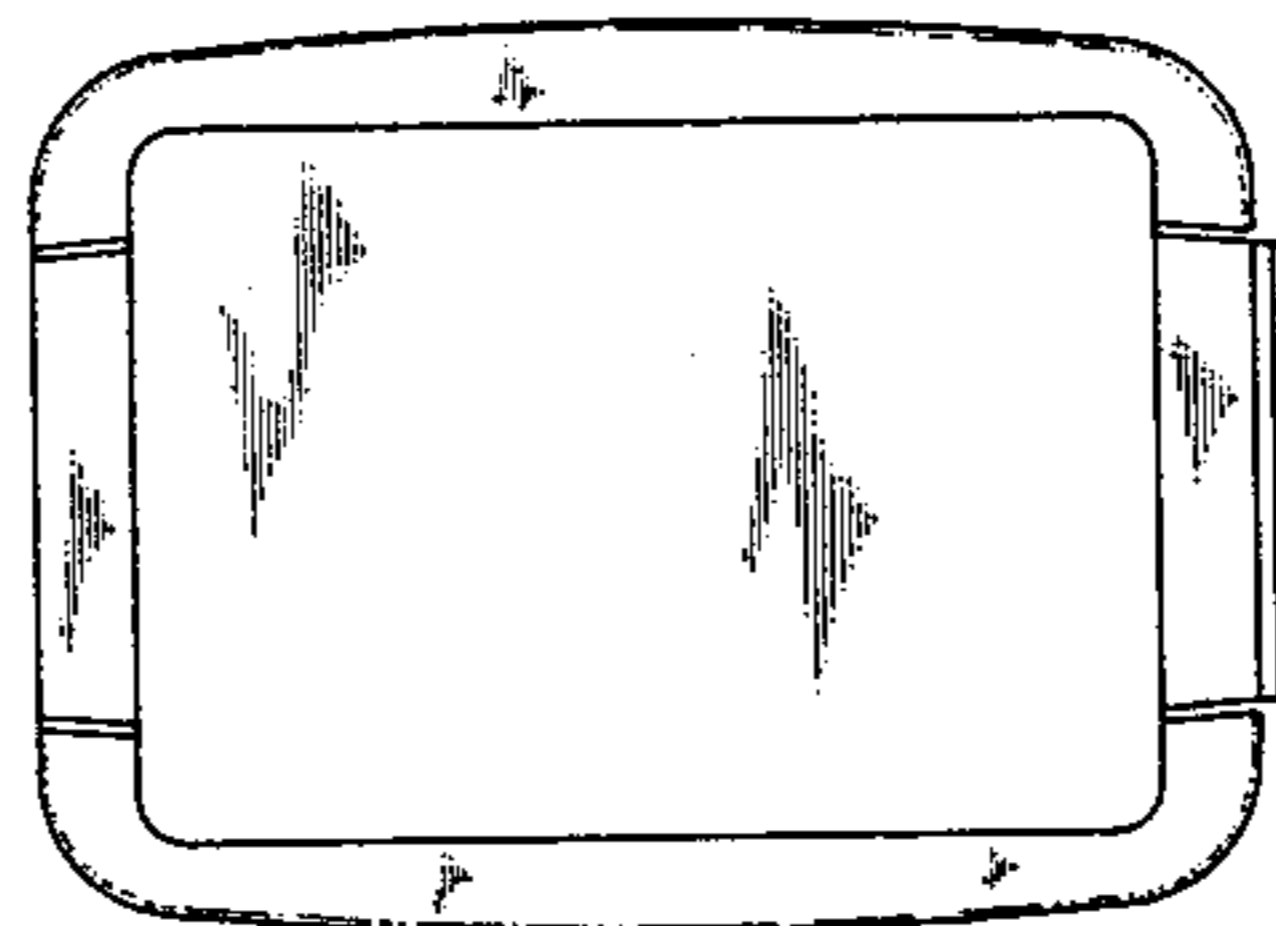

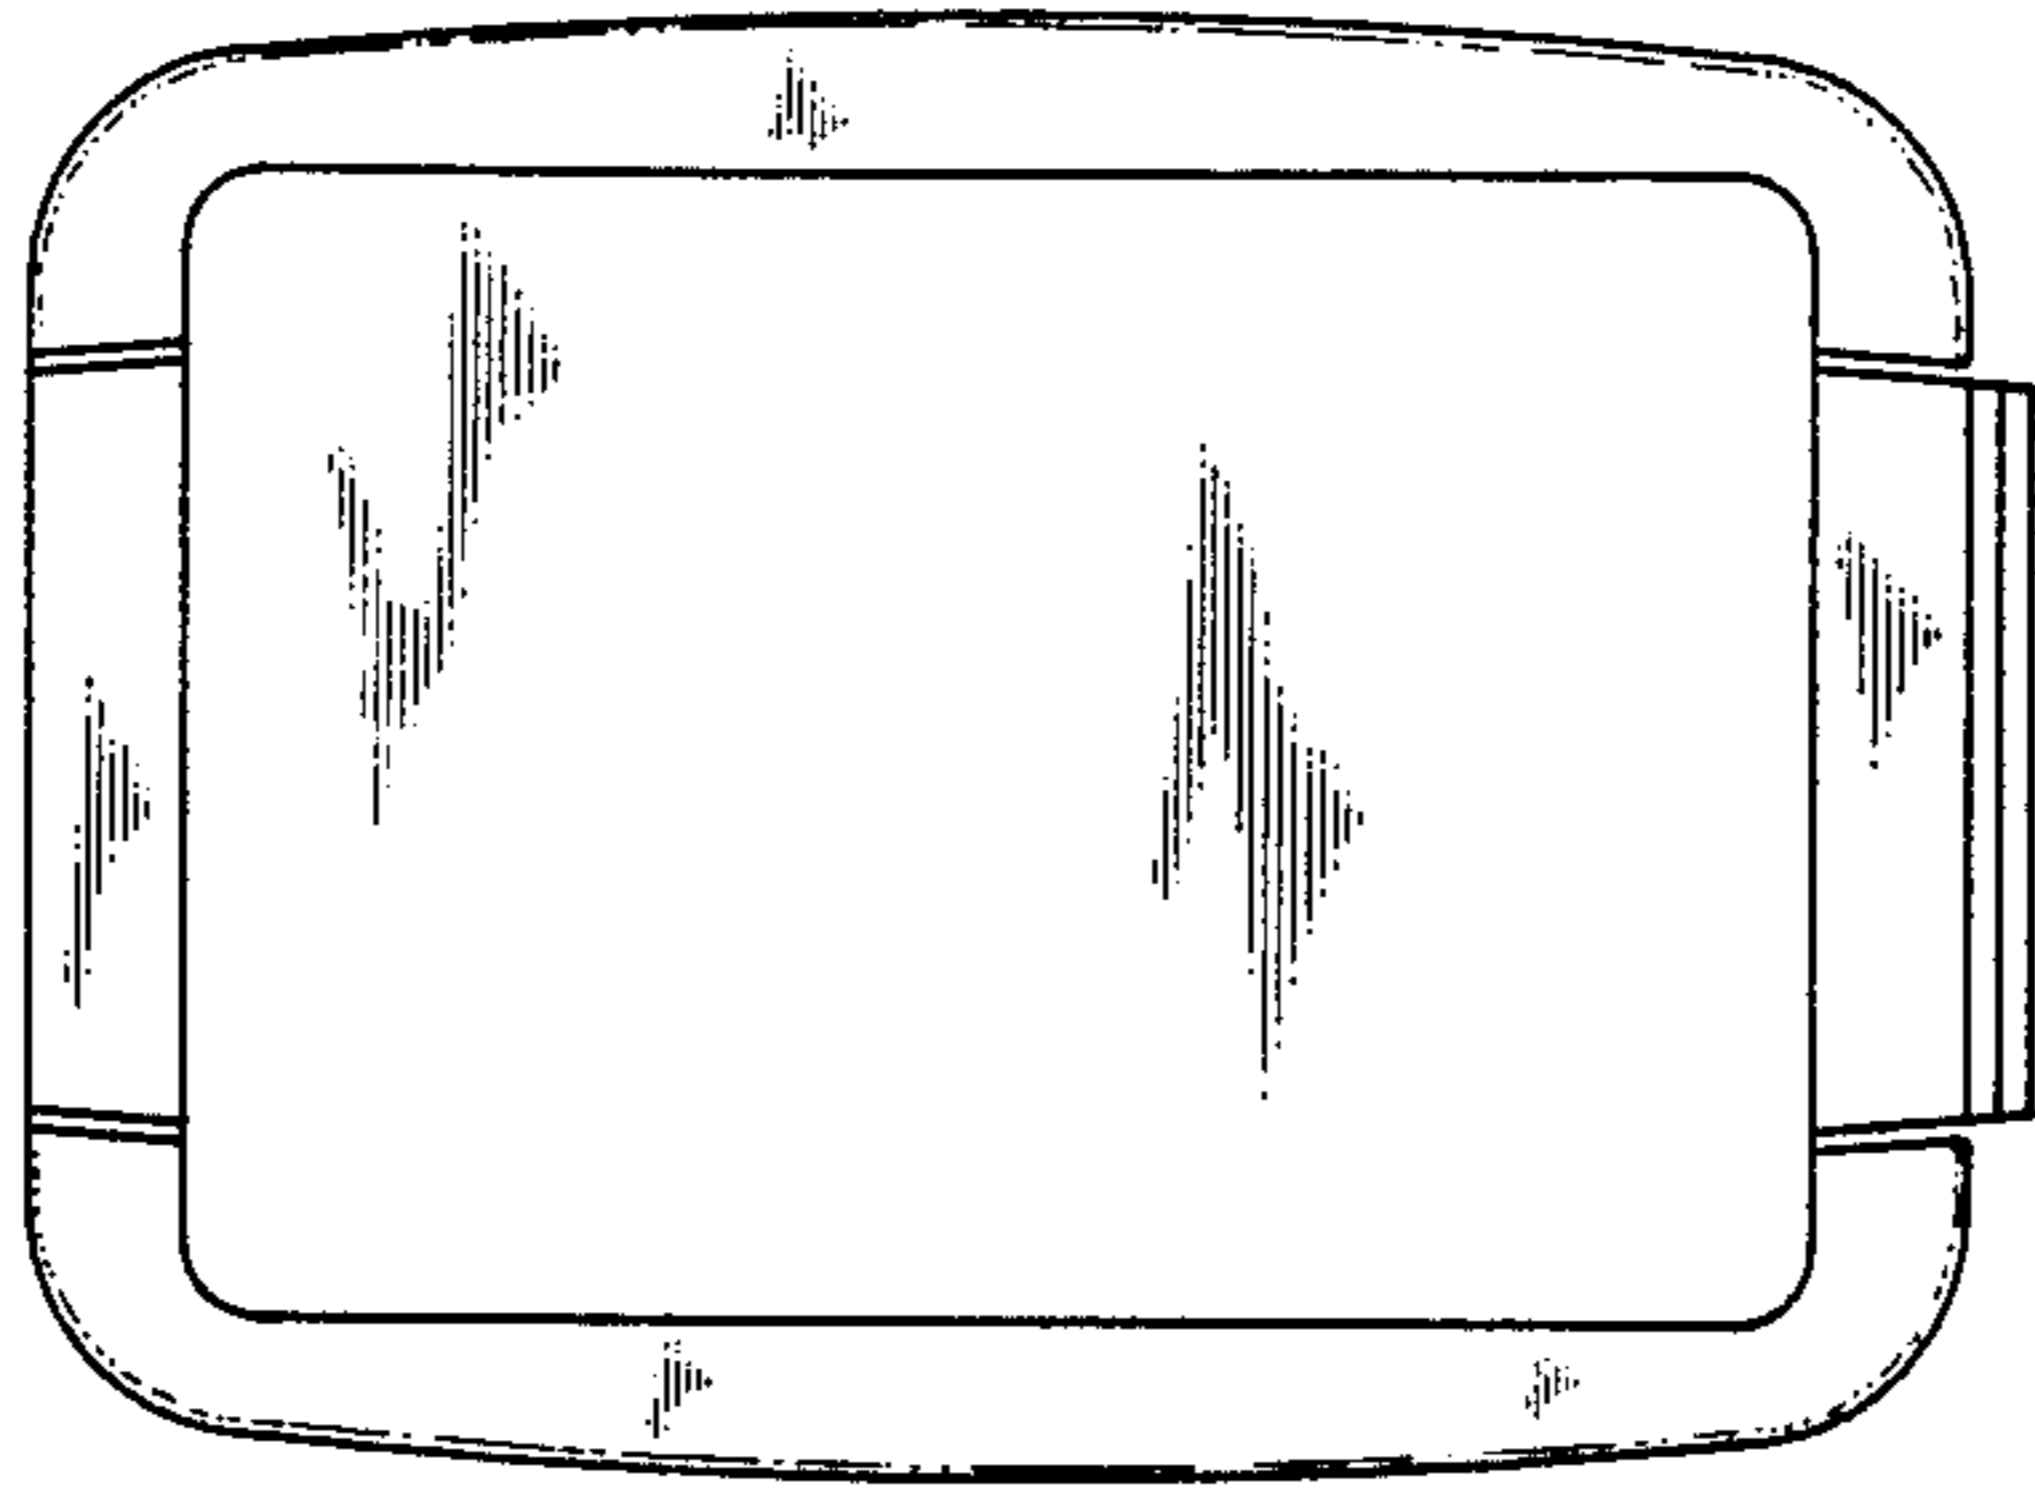


FIG. 1

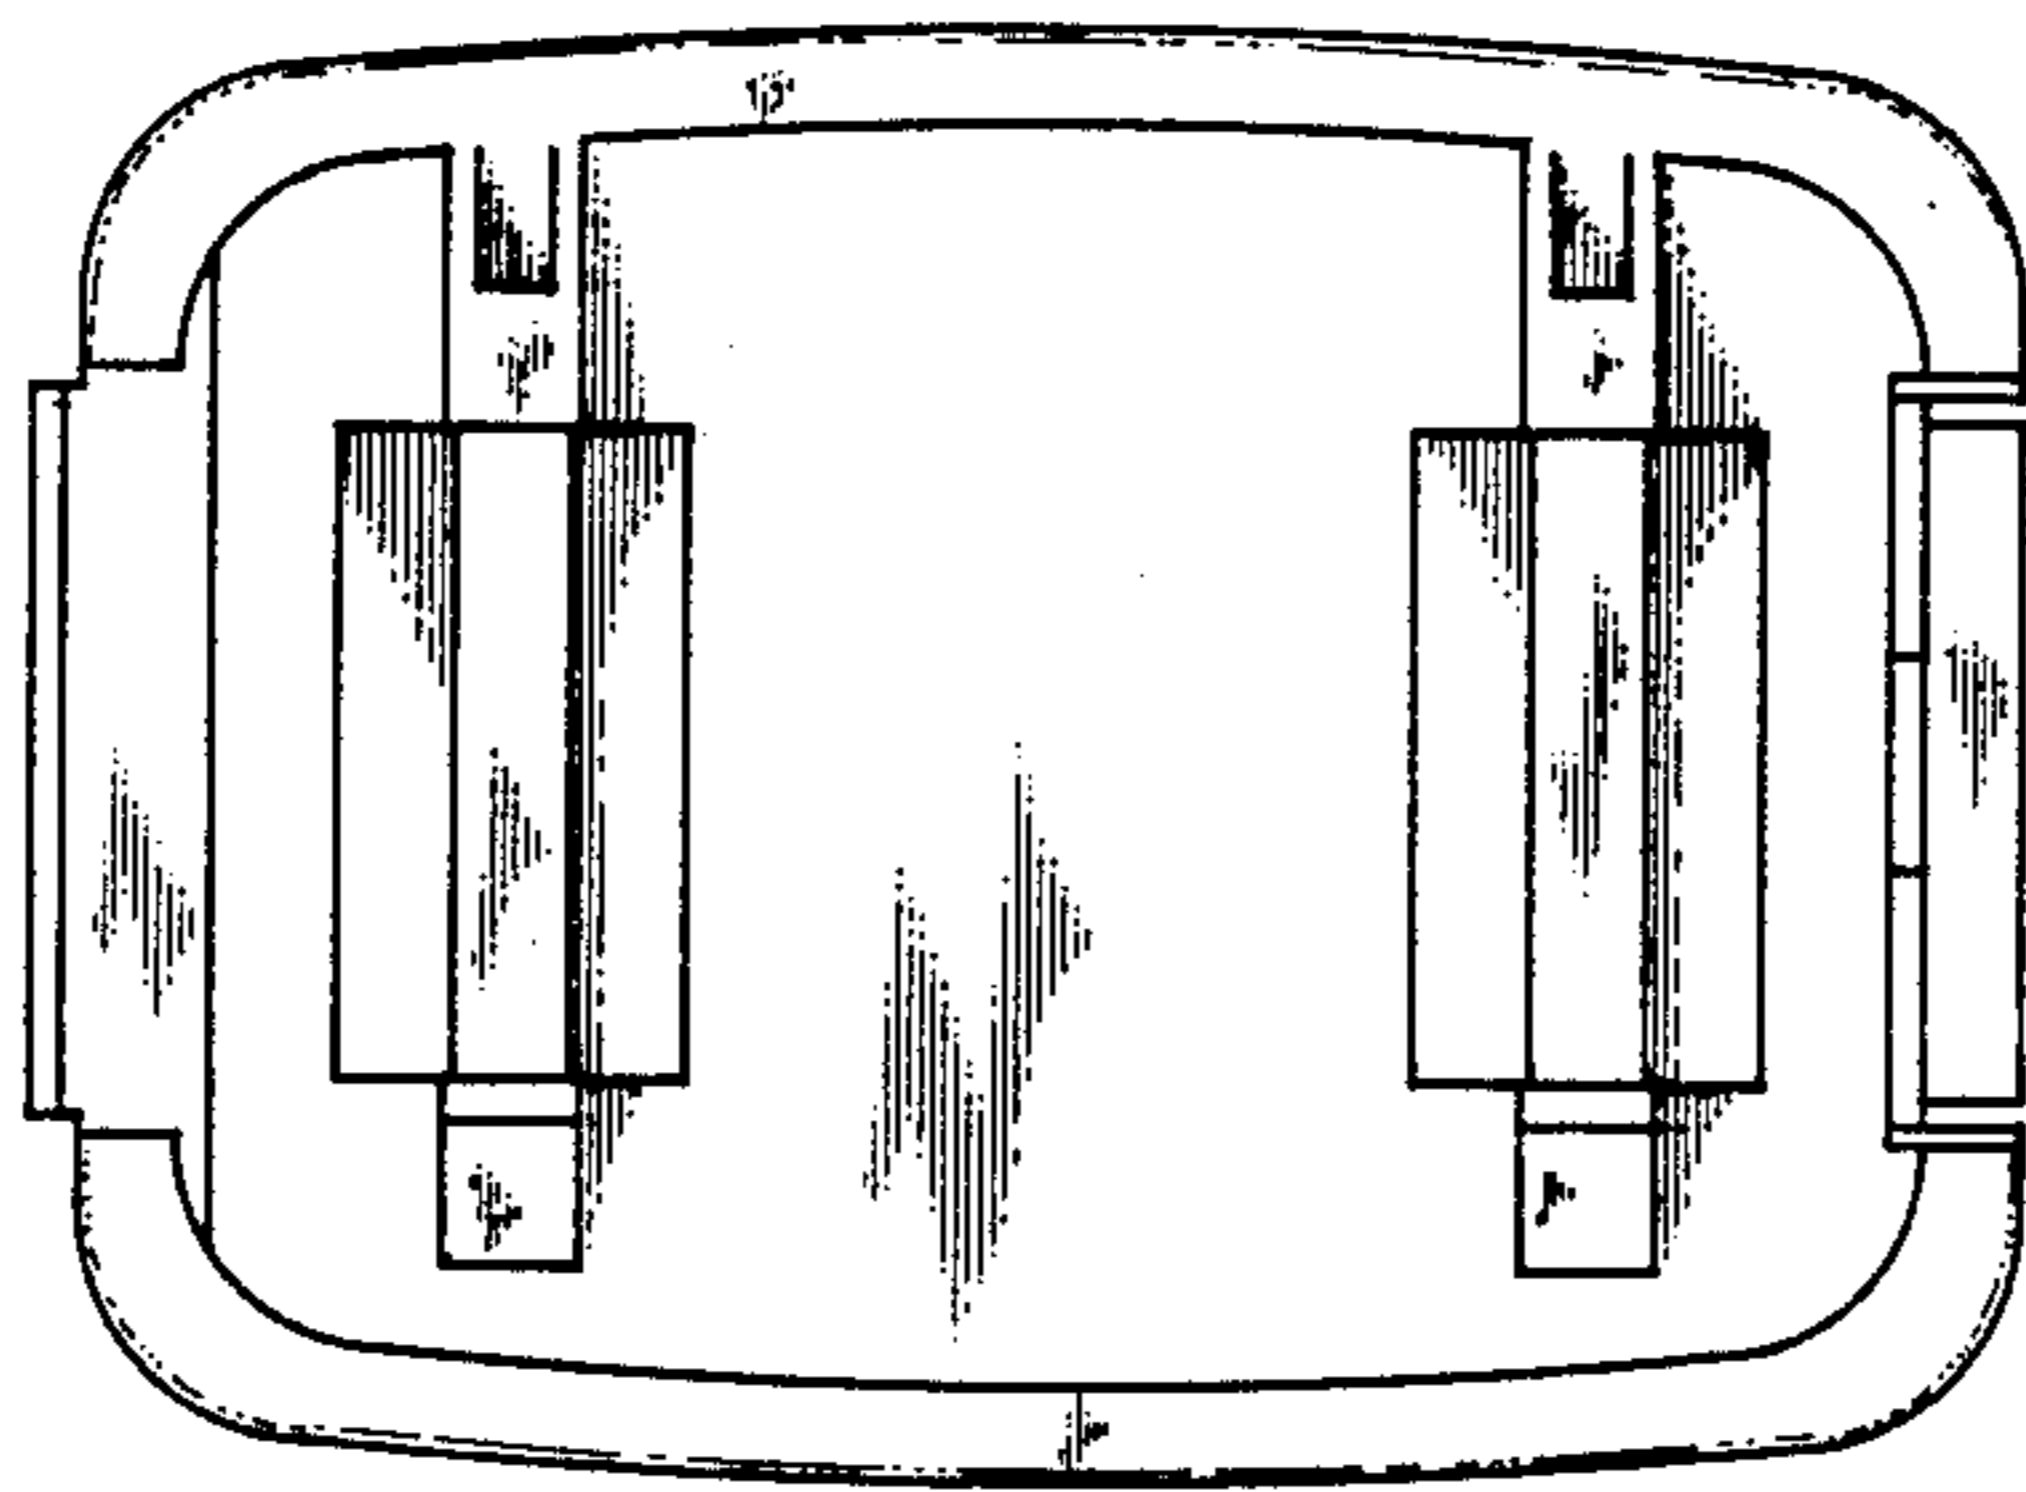


FIG. 2

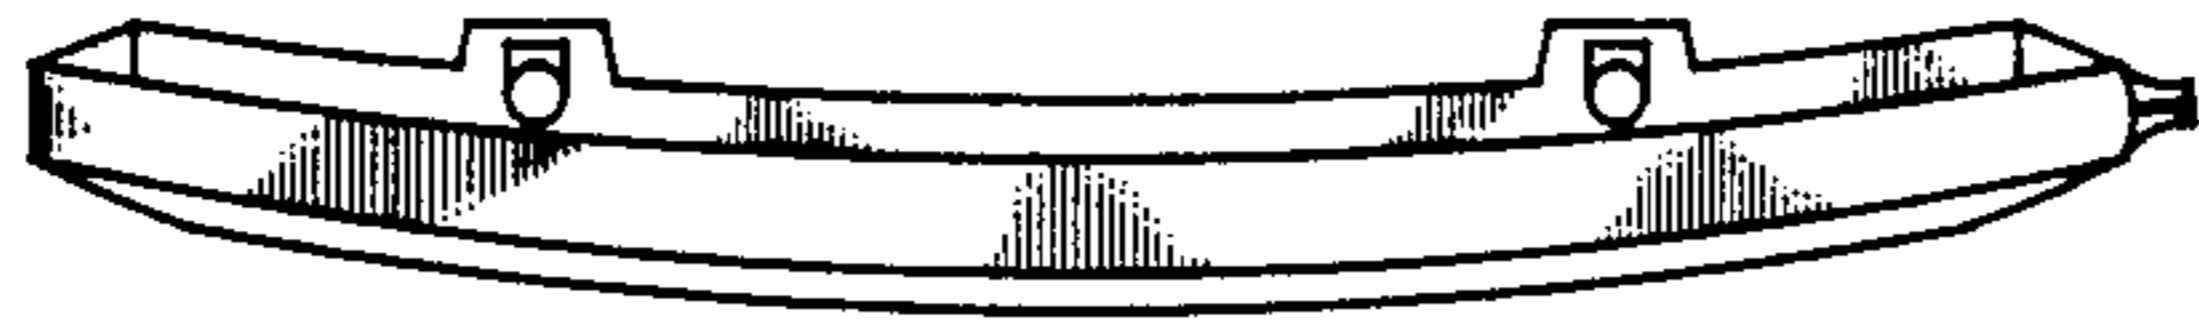


FIG. 3



FIG. 4

FIG. 5

