

[54] DIAGNOSTIC TEST KIT

[75] Inventors: Edward F. Covell, Glen Cove, N.Y.; Lovick E. Cannon, III, Wayland, Mass.

[73] Assignee: Tambrands Inc., Lake Success, N.Y.

[\*\*] Term: 14 Years

[21] Appl. No.: 638,729

[22] Filed: Aug. 8, 1984

[52] U.S. Cl. .... D24/17

[58] Field of Search ..... D24/17, 8, 99; 128/738; 206/569, 45.34; D9/337, 436, 341, 455

[56] References Cited

U.S. PATENT DOCUMENTS

D. 215,774	10/1969	Crane	.....	D24/17
D. 241,173	8/1976	Corneille	.....	D24/17
D. 241,174	8/1976	Corneille	.....	D24/17
D. 274,752	7/1984	Byrne	.....	D24/8
D. 275,789	10/1984	Byrne	.....	D24/8
3,234,107	2/1966	Kaufman et al.	.....	206/569
3,615,222	10/1971	Mead	.....	23/230

OTHER PUBLICATIONS

Carter-Wallace, Inc. Answer At-Home Early Pregnancy Test Kit instruction sheet, Jul. 1981.

Ortho Pharmaceutical Corporation FACT Pregnancy Test Kit instruction sheet, 1982.

Warner-Lambert Company E.P.T. Early In-Home Pregnancy Test instruction sheet, undated.

Warner-Lambert Company E.P.T. Plus Early Pregnancy Test instruction sheet, undated.

Whitehall Laboratories, Inc. PREDICTOR In-Home Early Pregnancy Test instruction sheet, undated.

J. B. Williams Company, Inc. ACU-TEST In-Home Pregnancy Test instruction sheet, Nov. 1980.

Primary Examiner—A. Hugo Word

Assistant Examiner—Stella M. Reid

Attorney, Agent, or Firm—John E. Nathan; Jeffrey H. Ingerman

[57] CLAIM

The ornamental design for a diagnostic test kit, as shown and described.

DESCRIPTION

FIG. 1 is an isometric view of a diagnostic test kit showing our new design;

FIG. 2 is a top plan view of the diagnostic test kit;

FIG. 3 is a right side elevational view of the diagnostic test kit;

FIG. 4 is a rear elevational view of the diagnostic test kit;

FIG. 5 is a bottom plan view of the diagnostic test kit;

FIG. 6 is an exploded isometric view of the diagnostic test kit, with its cover removed;

FIG. 7 is a top plan view of the diagnostic test kit without its cover;

FIG. 8 is an exploded isometric view of the diagnostic test kit without its cover, with its utensils removed; and

FIG. 9 is a top plan view of the diagnostic test kit without its cover or utensils.

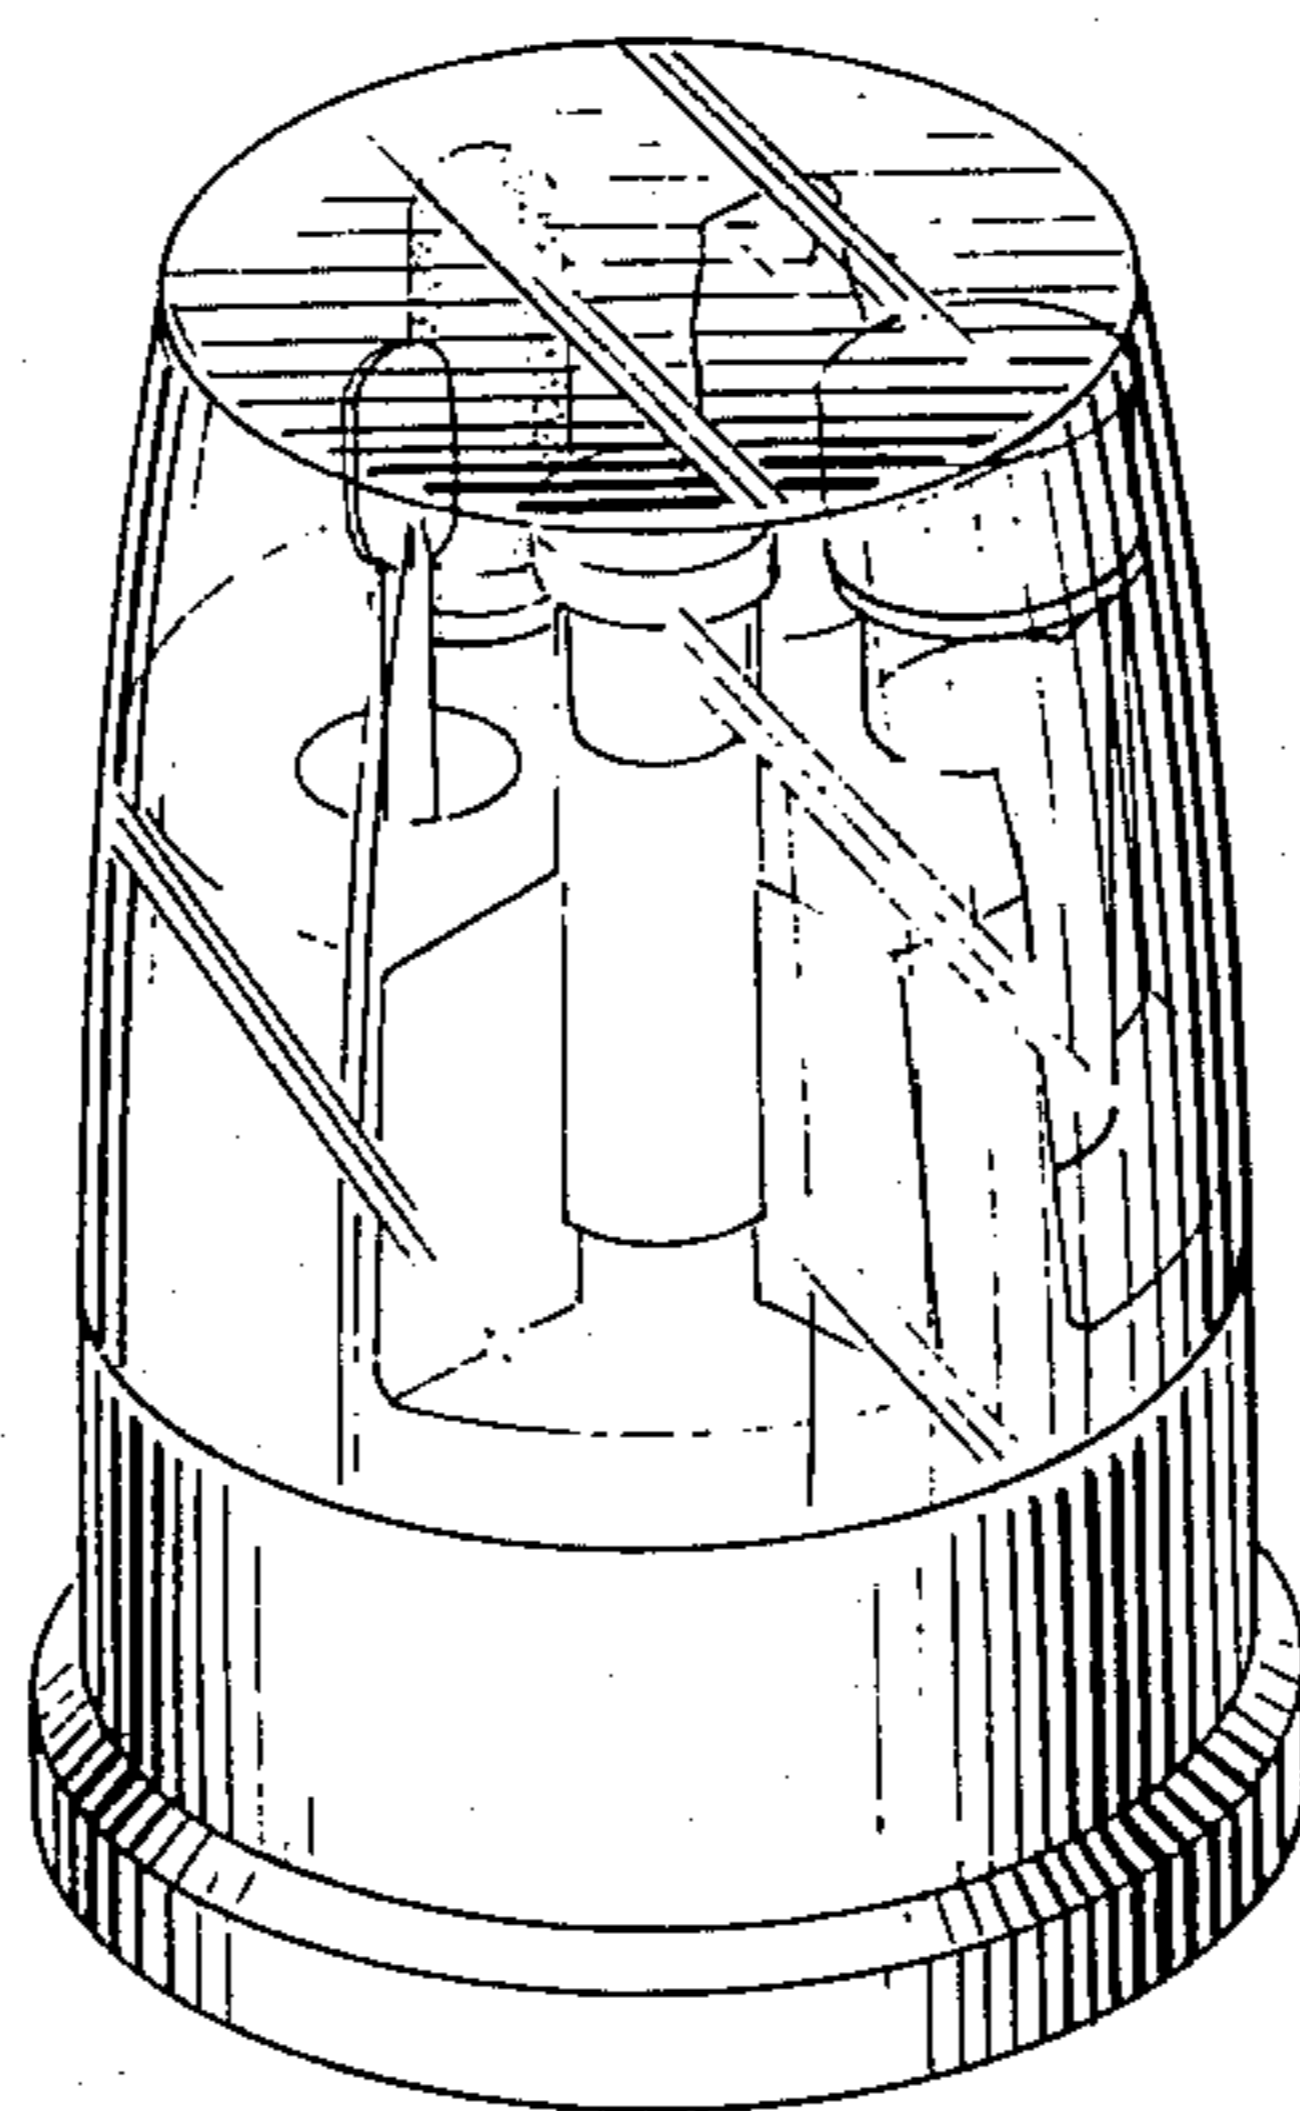


Fig. 1.

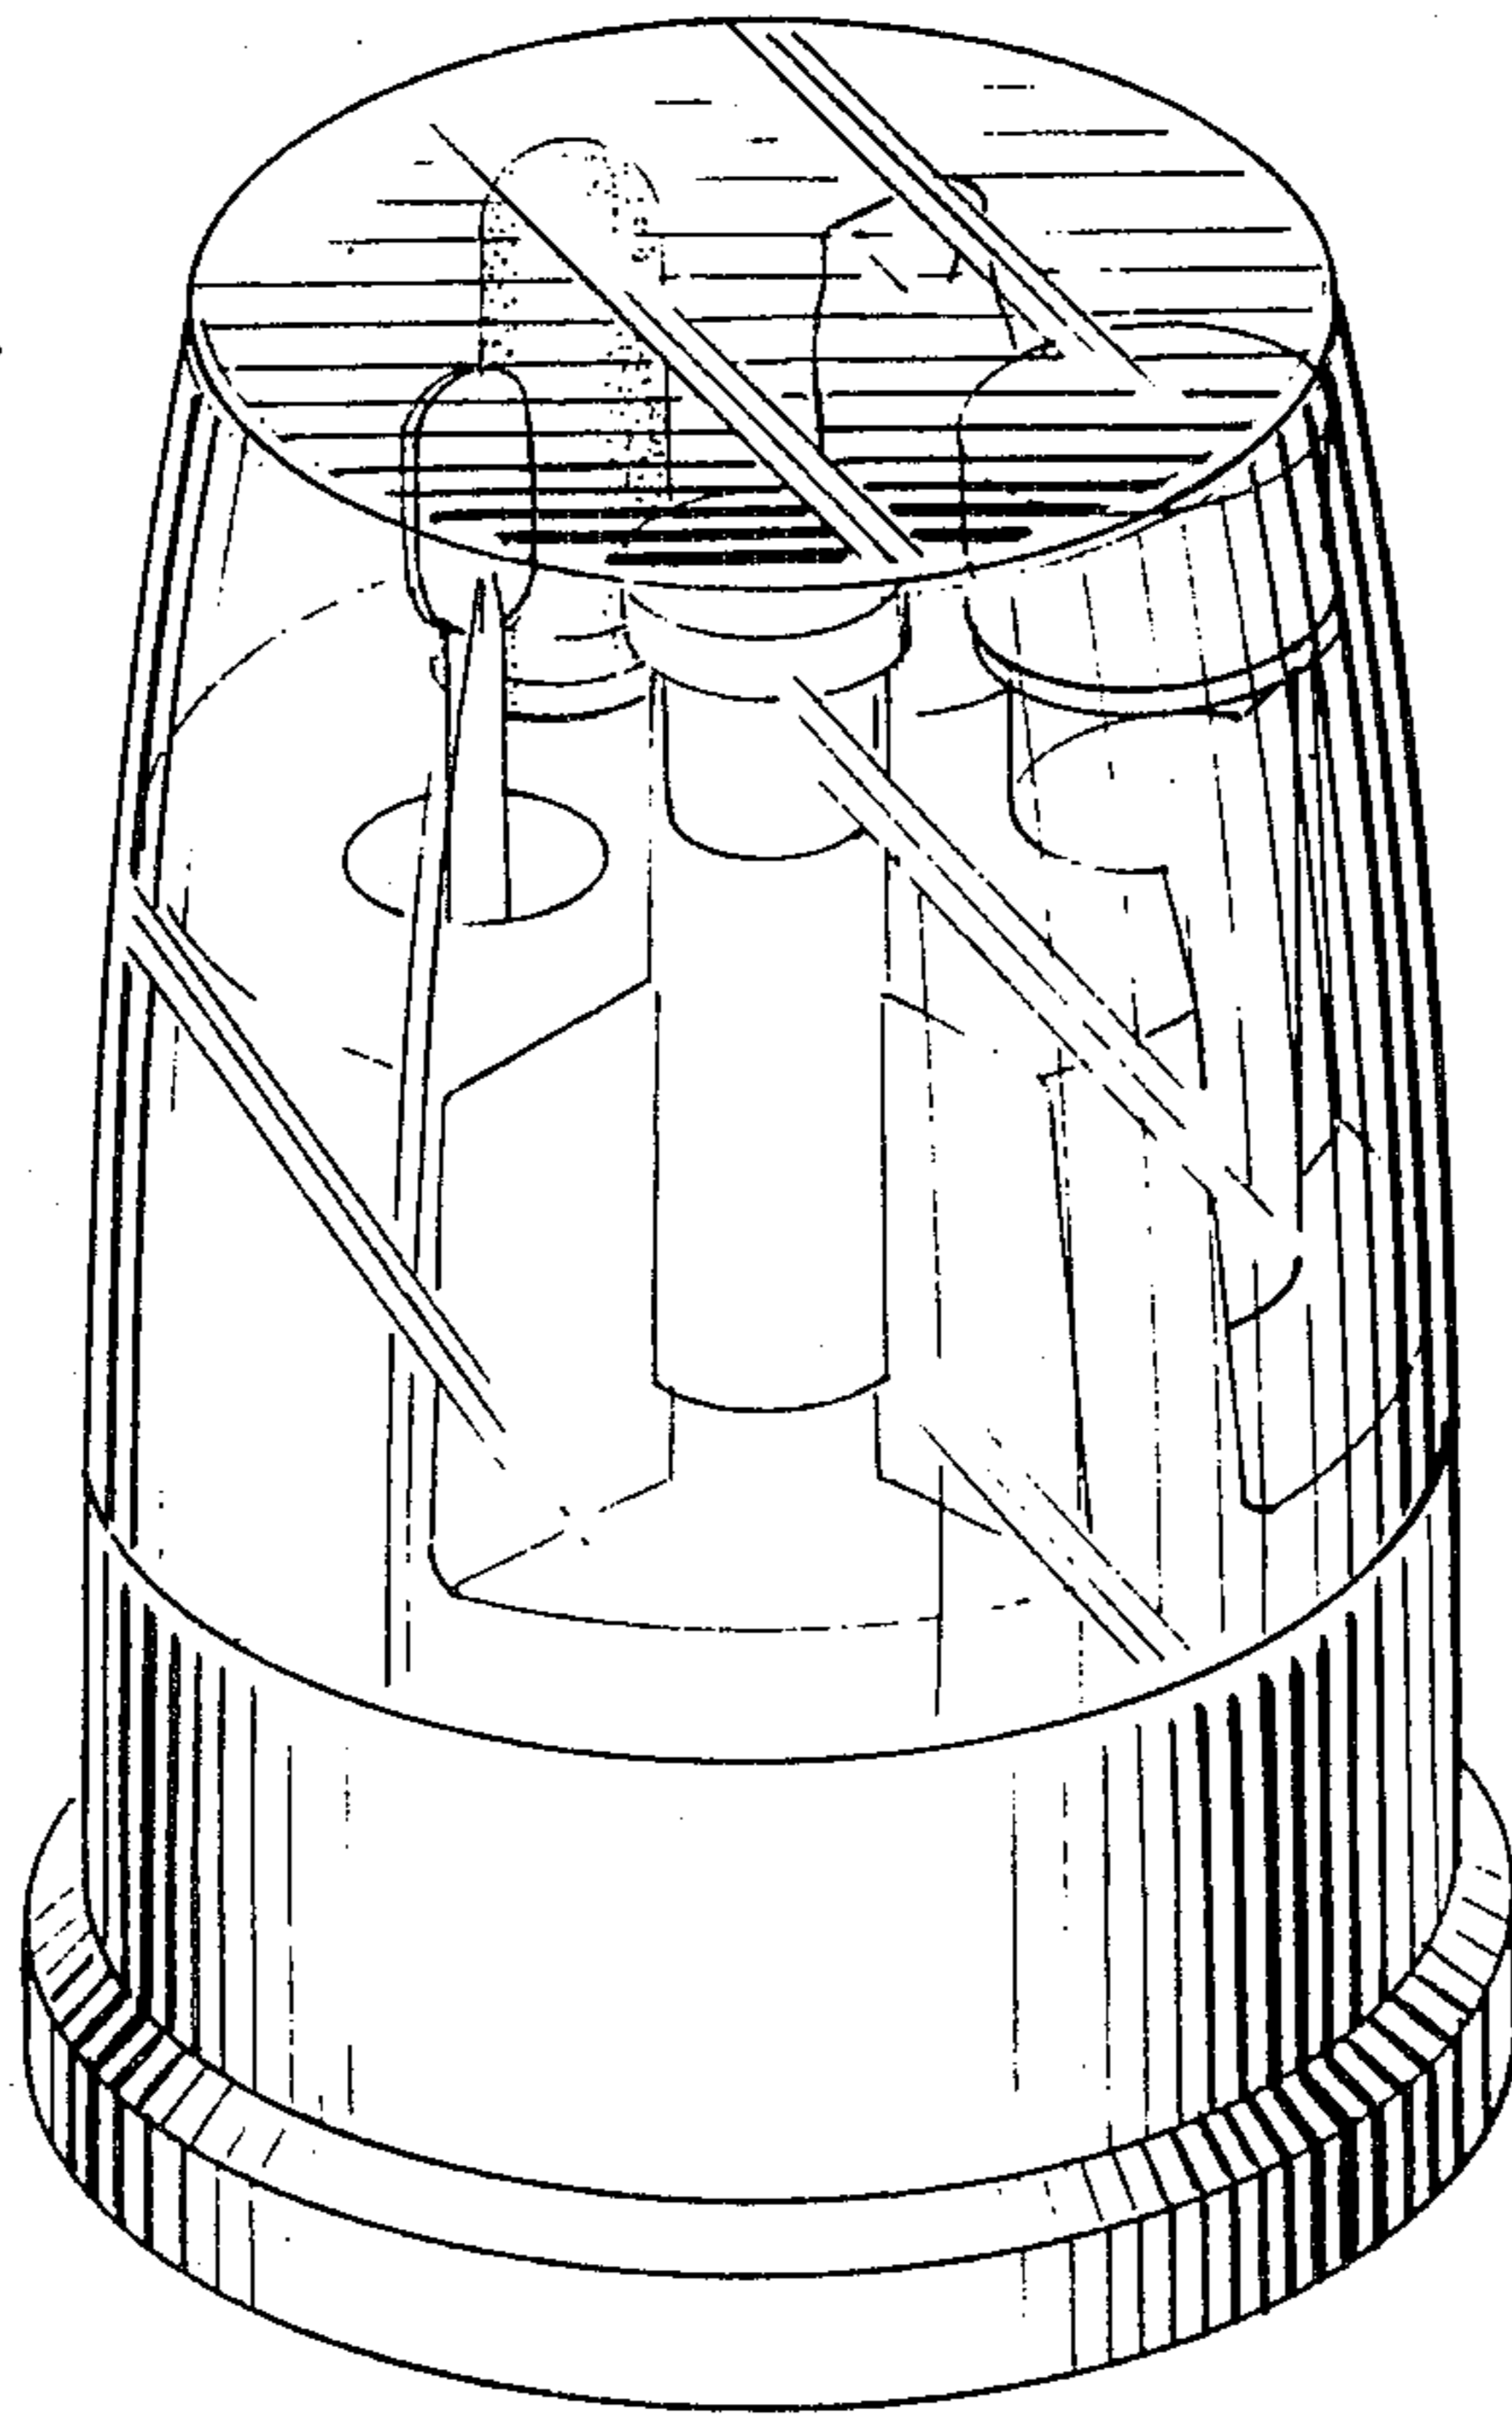


Fig. 3.

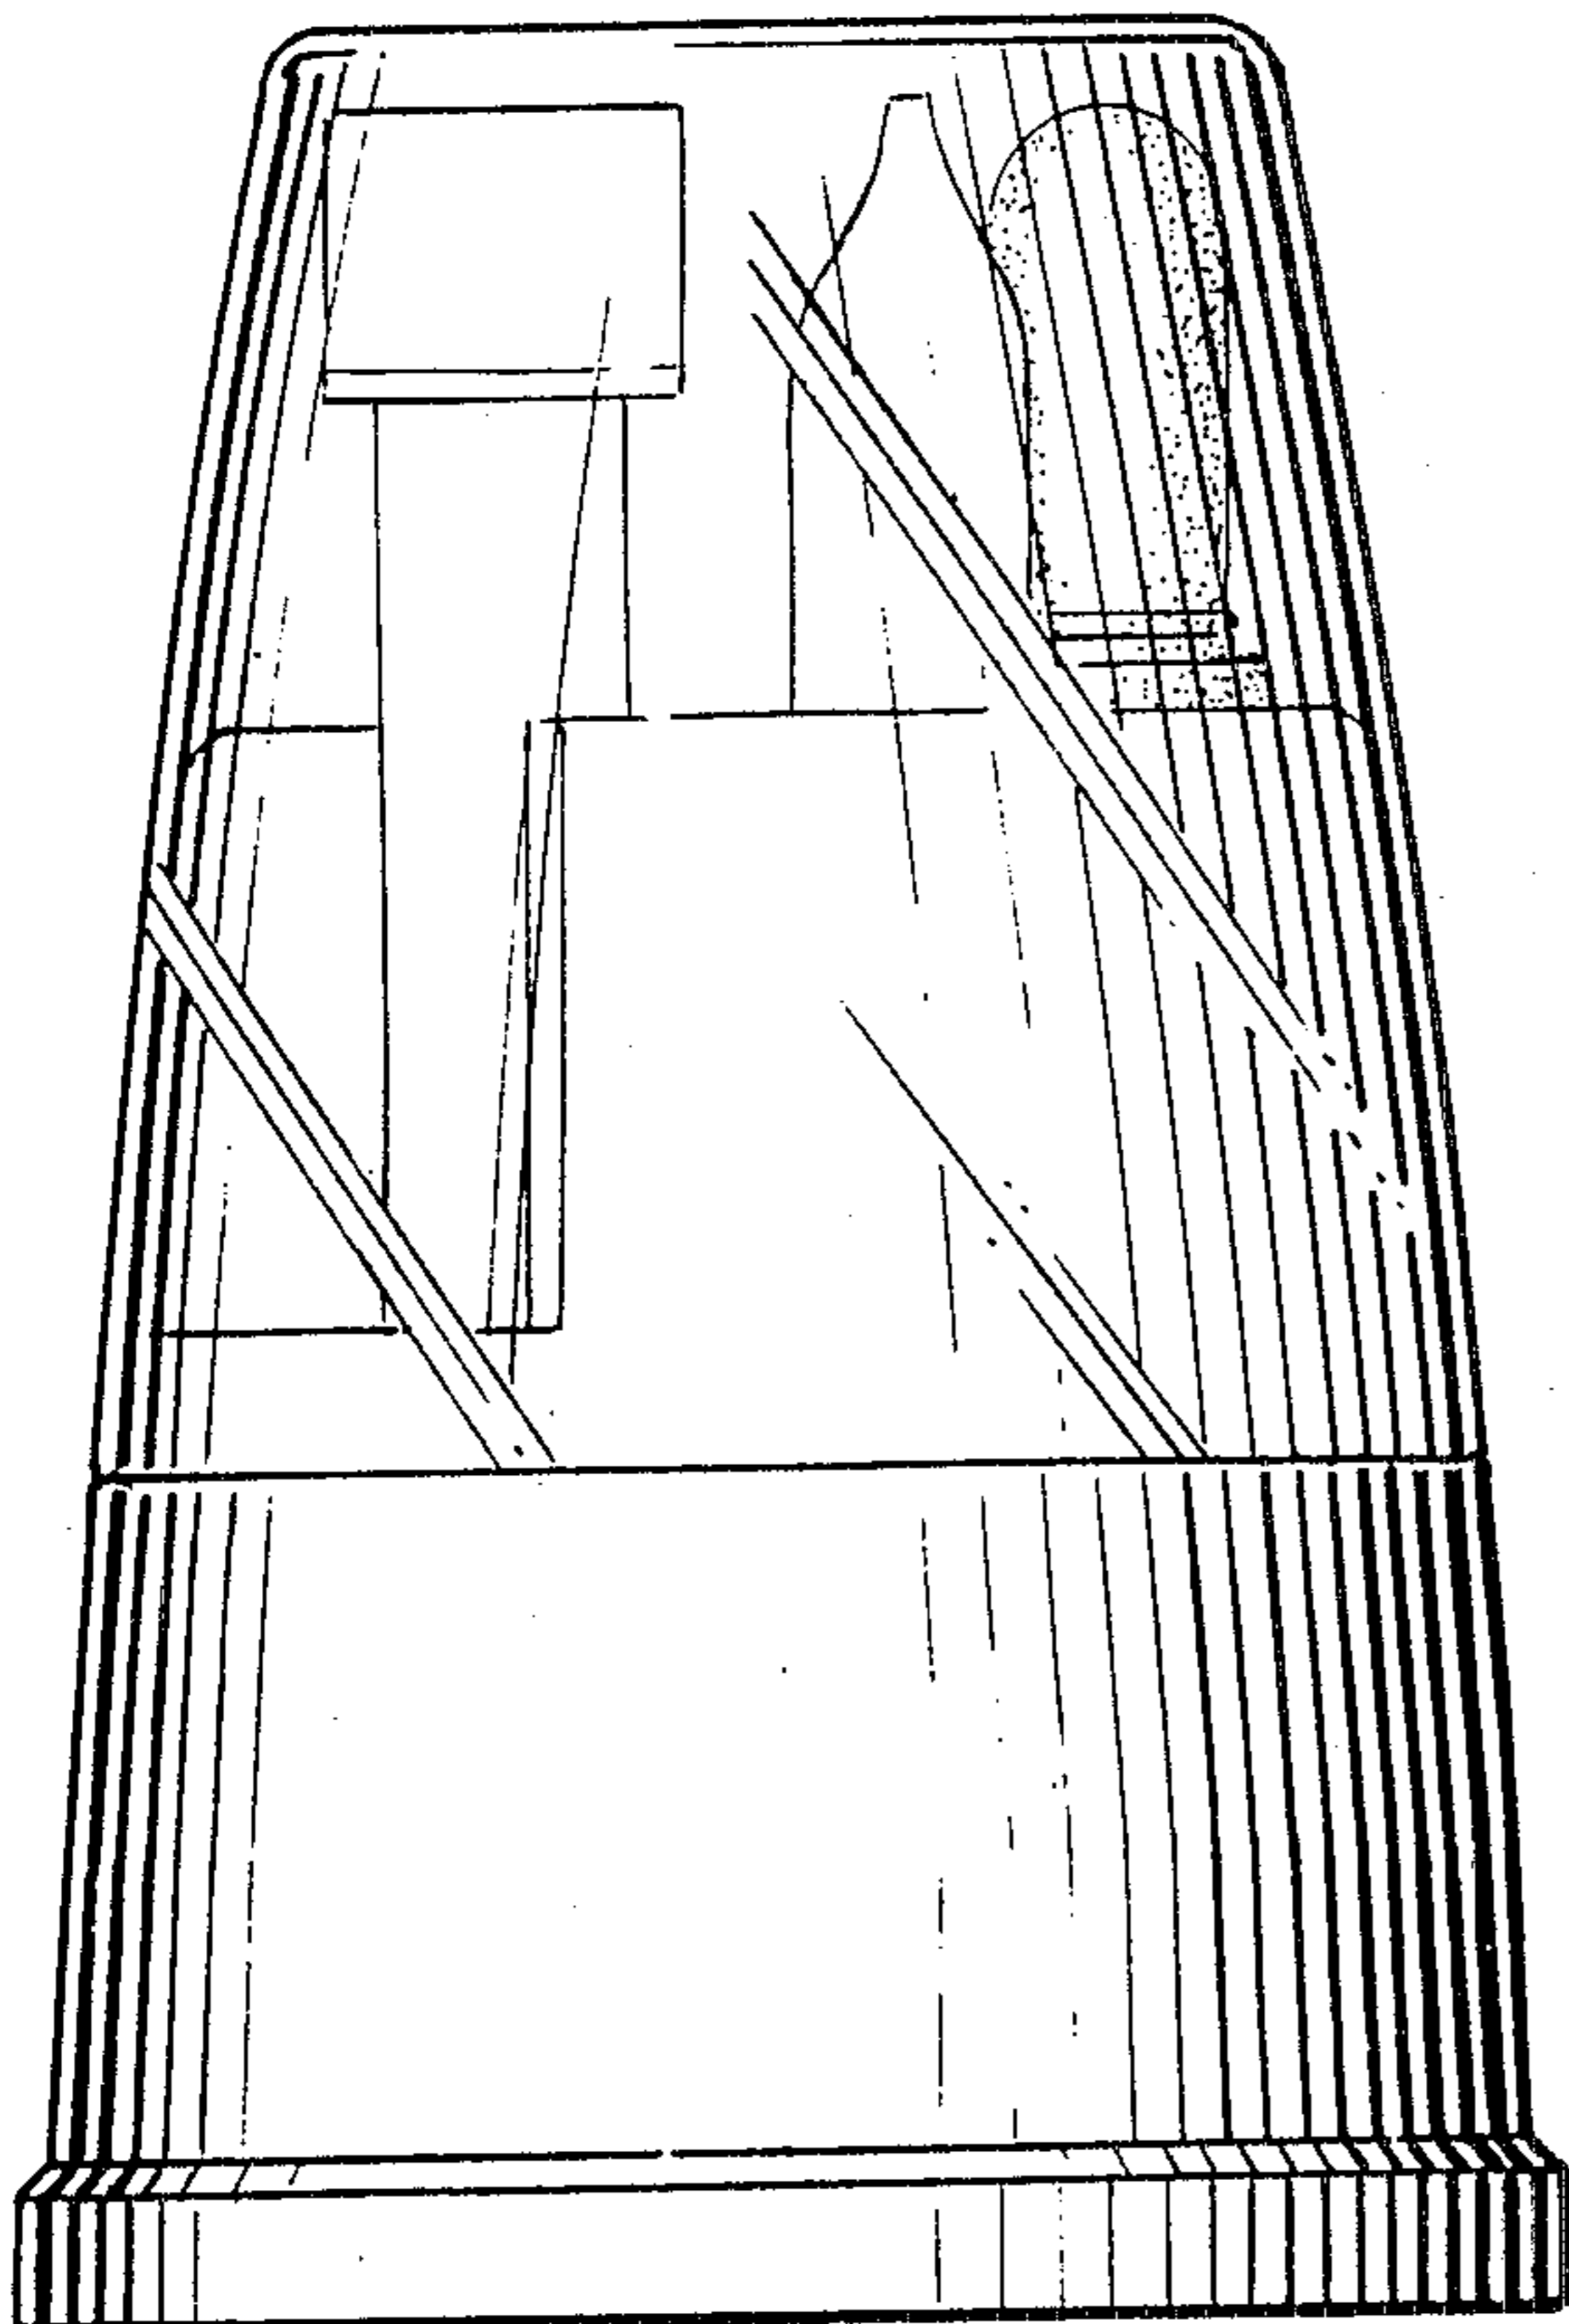


Fig. 2.

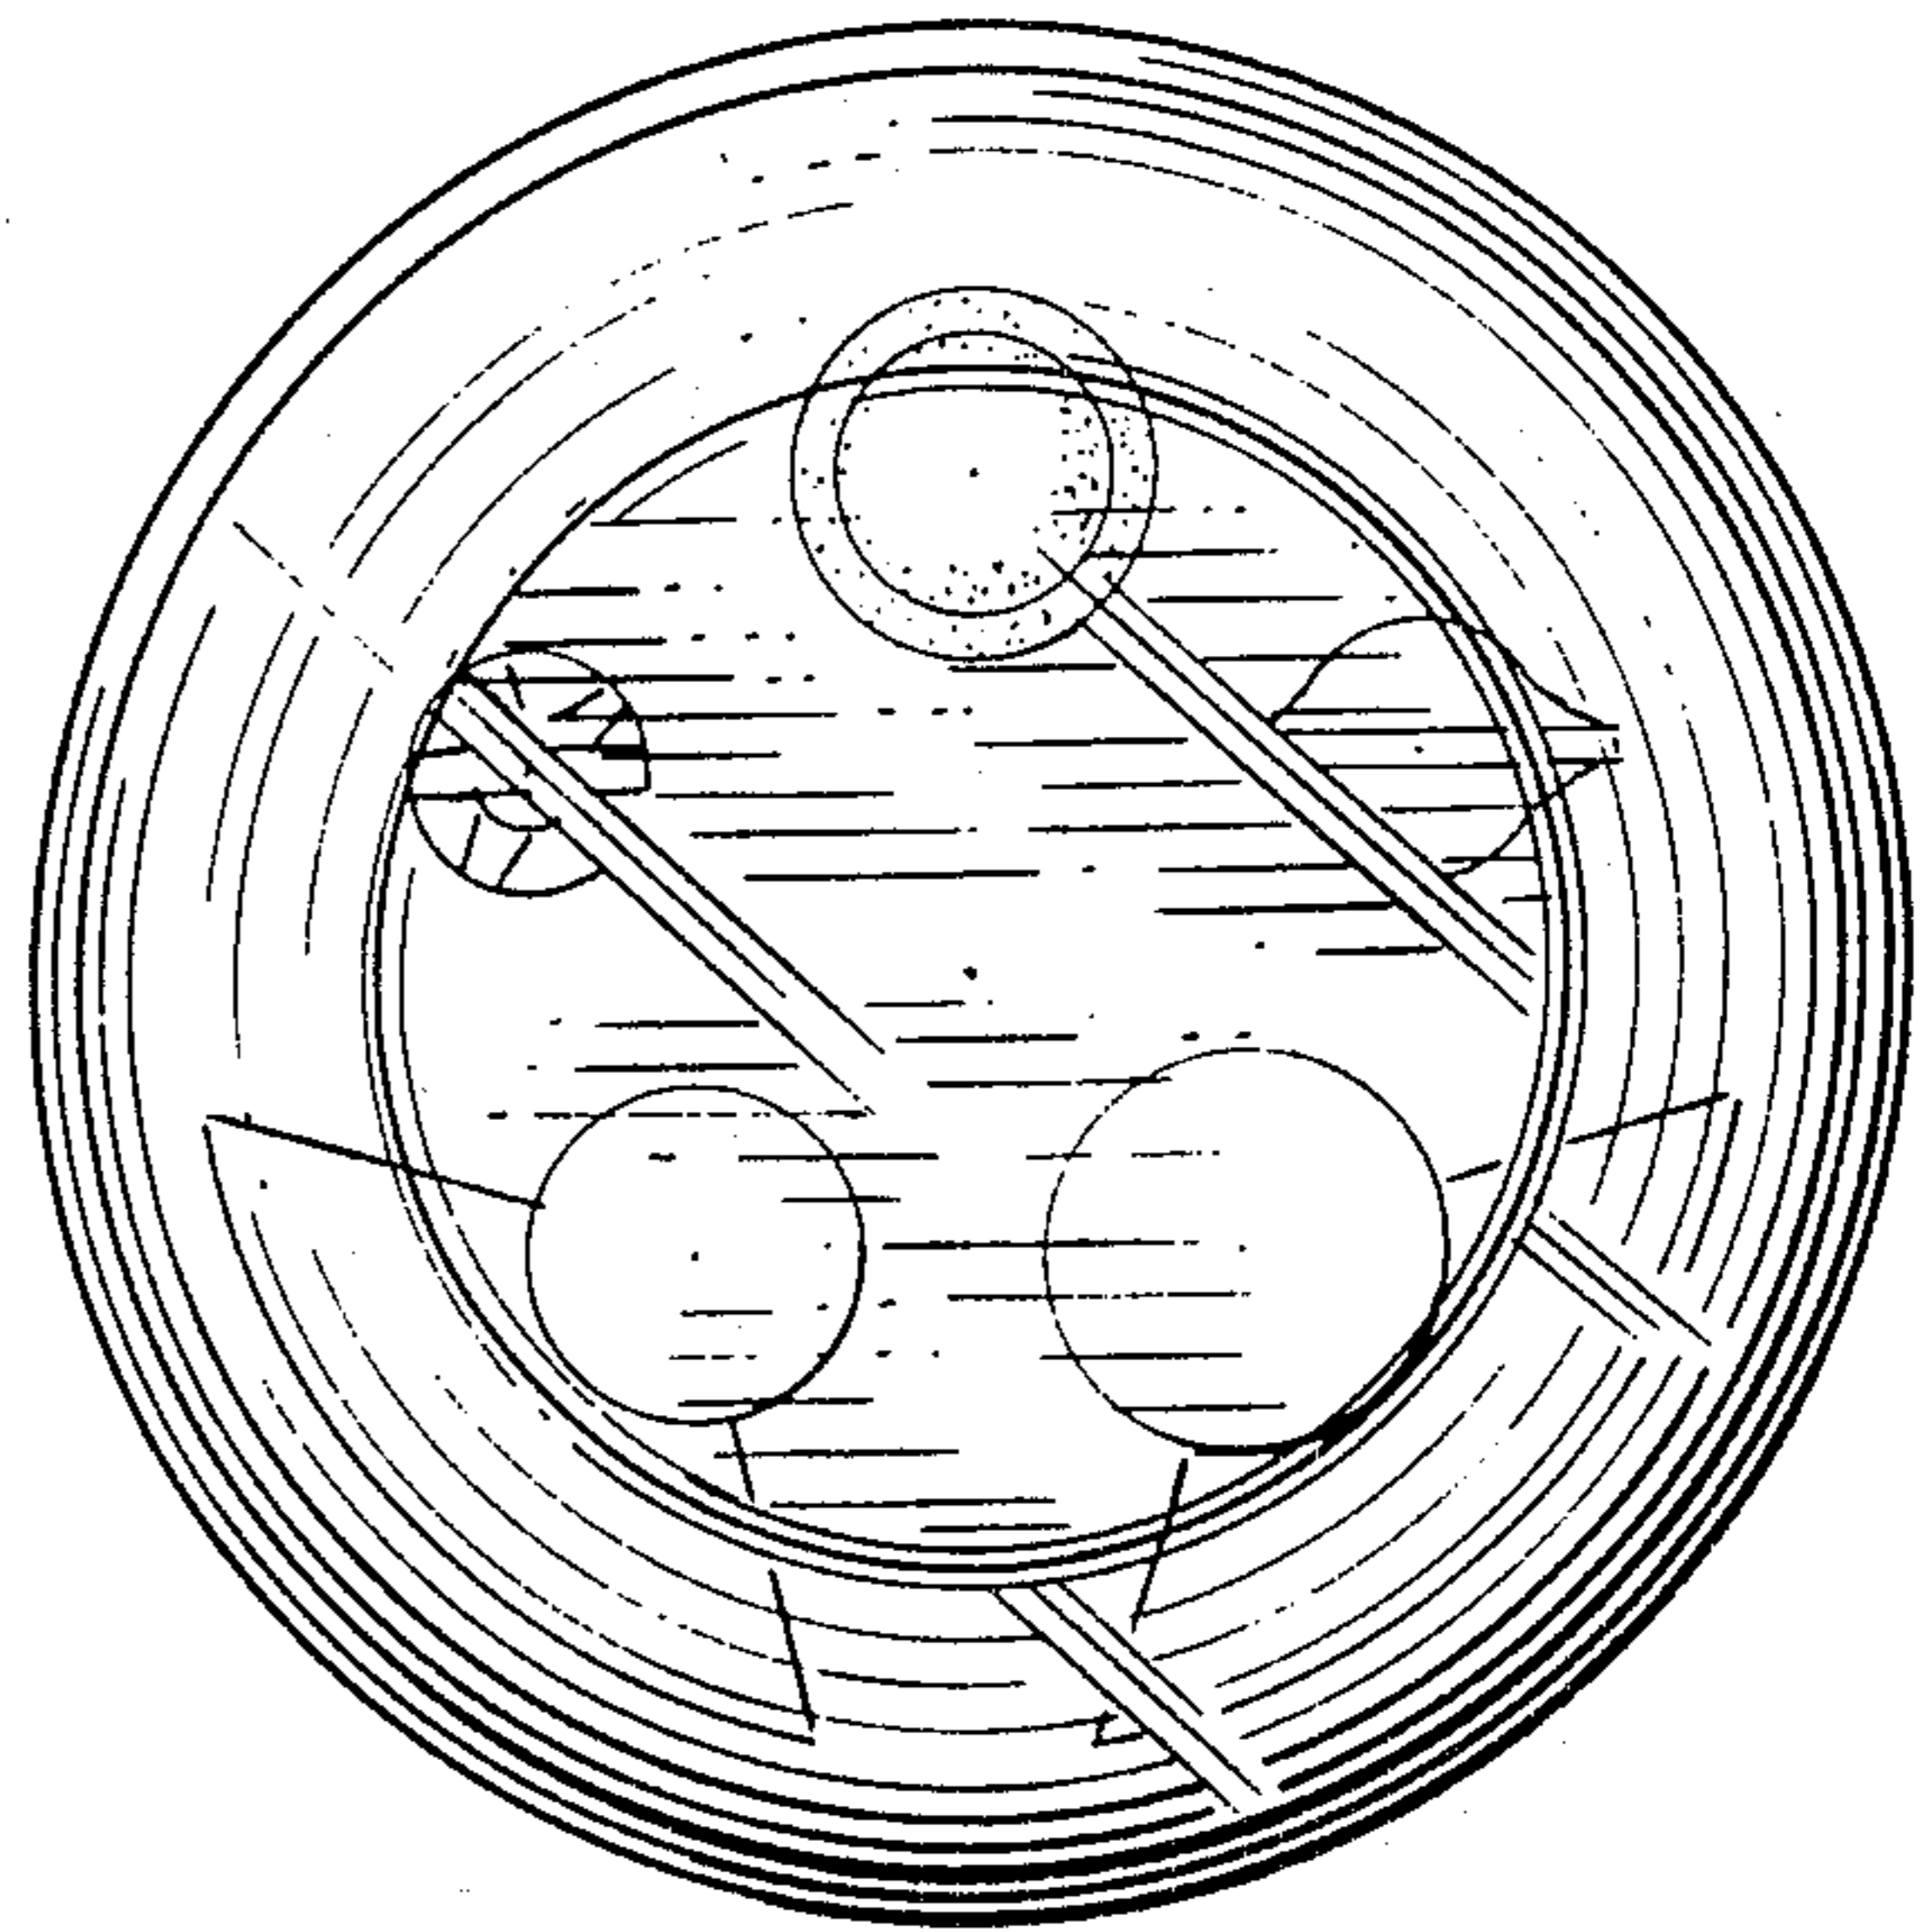


Fig. 4.

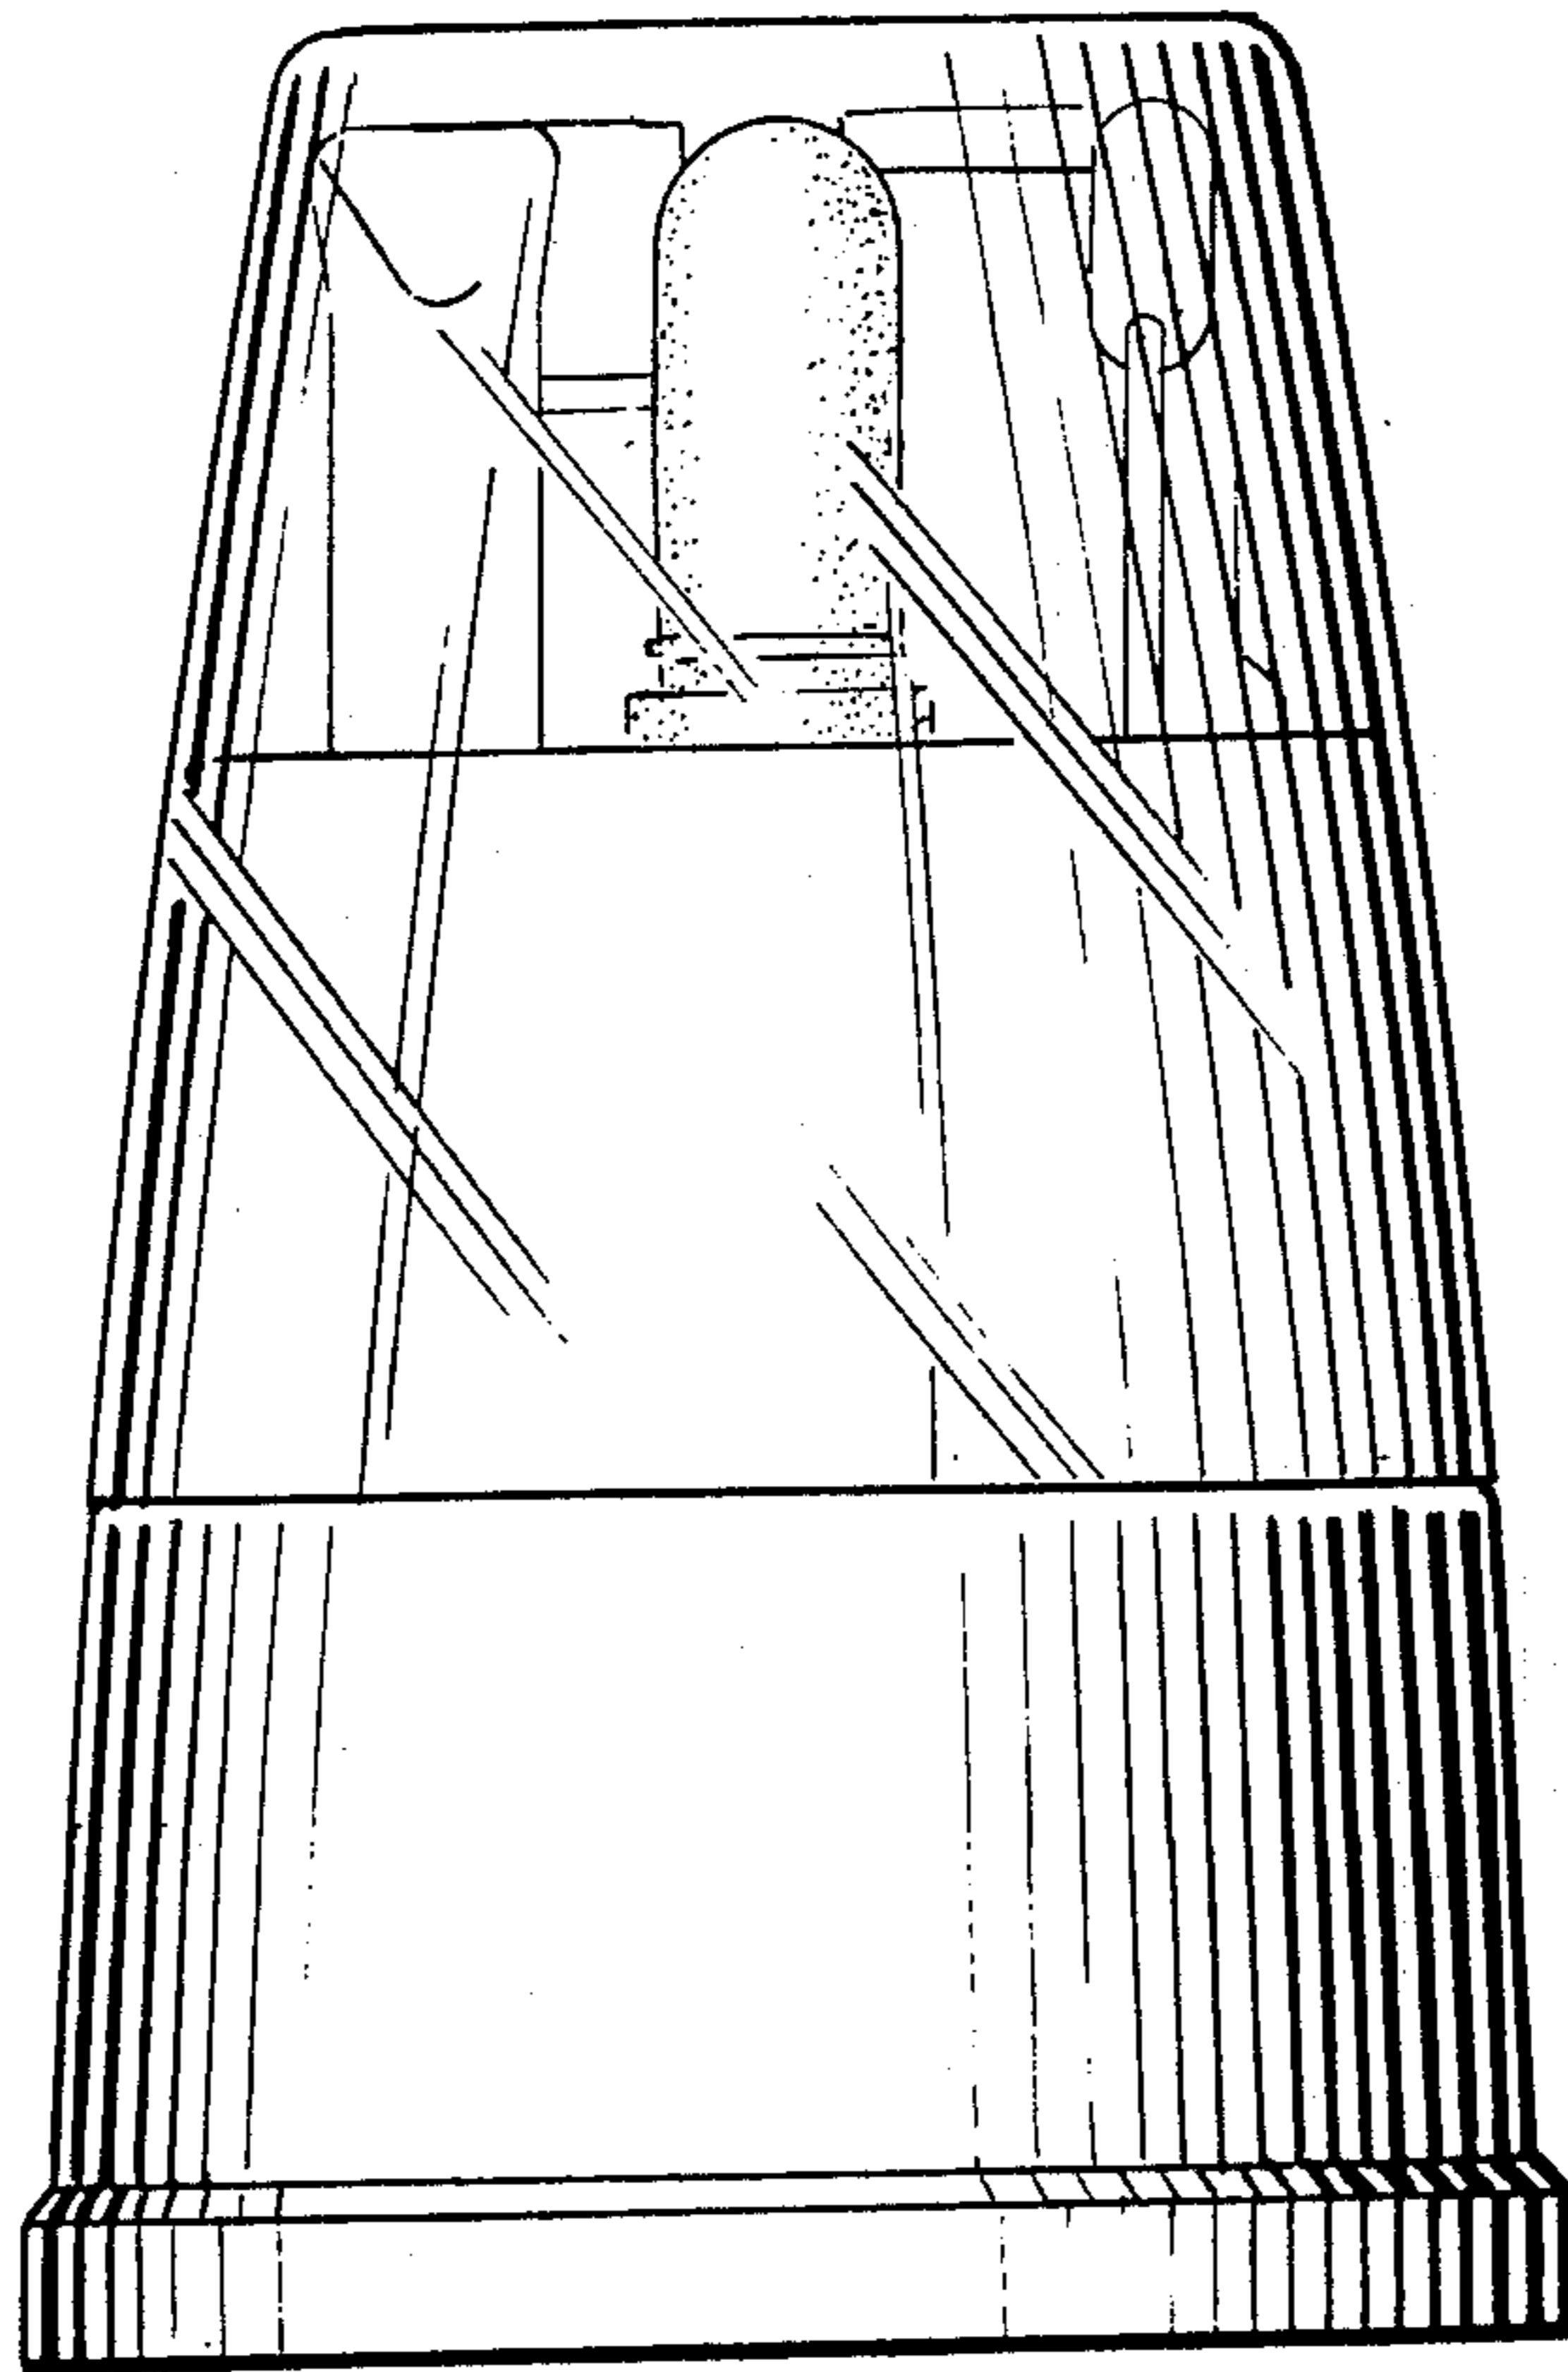
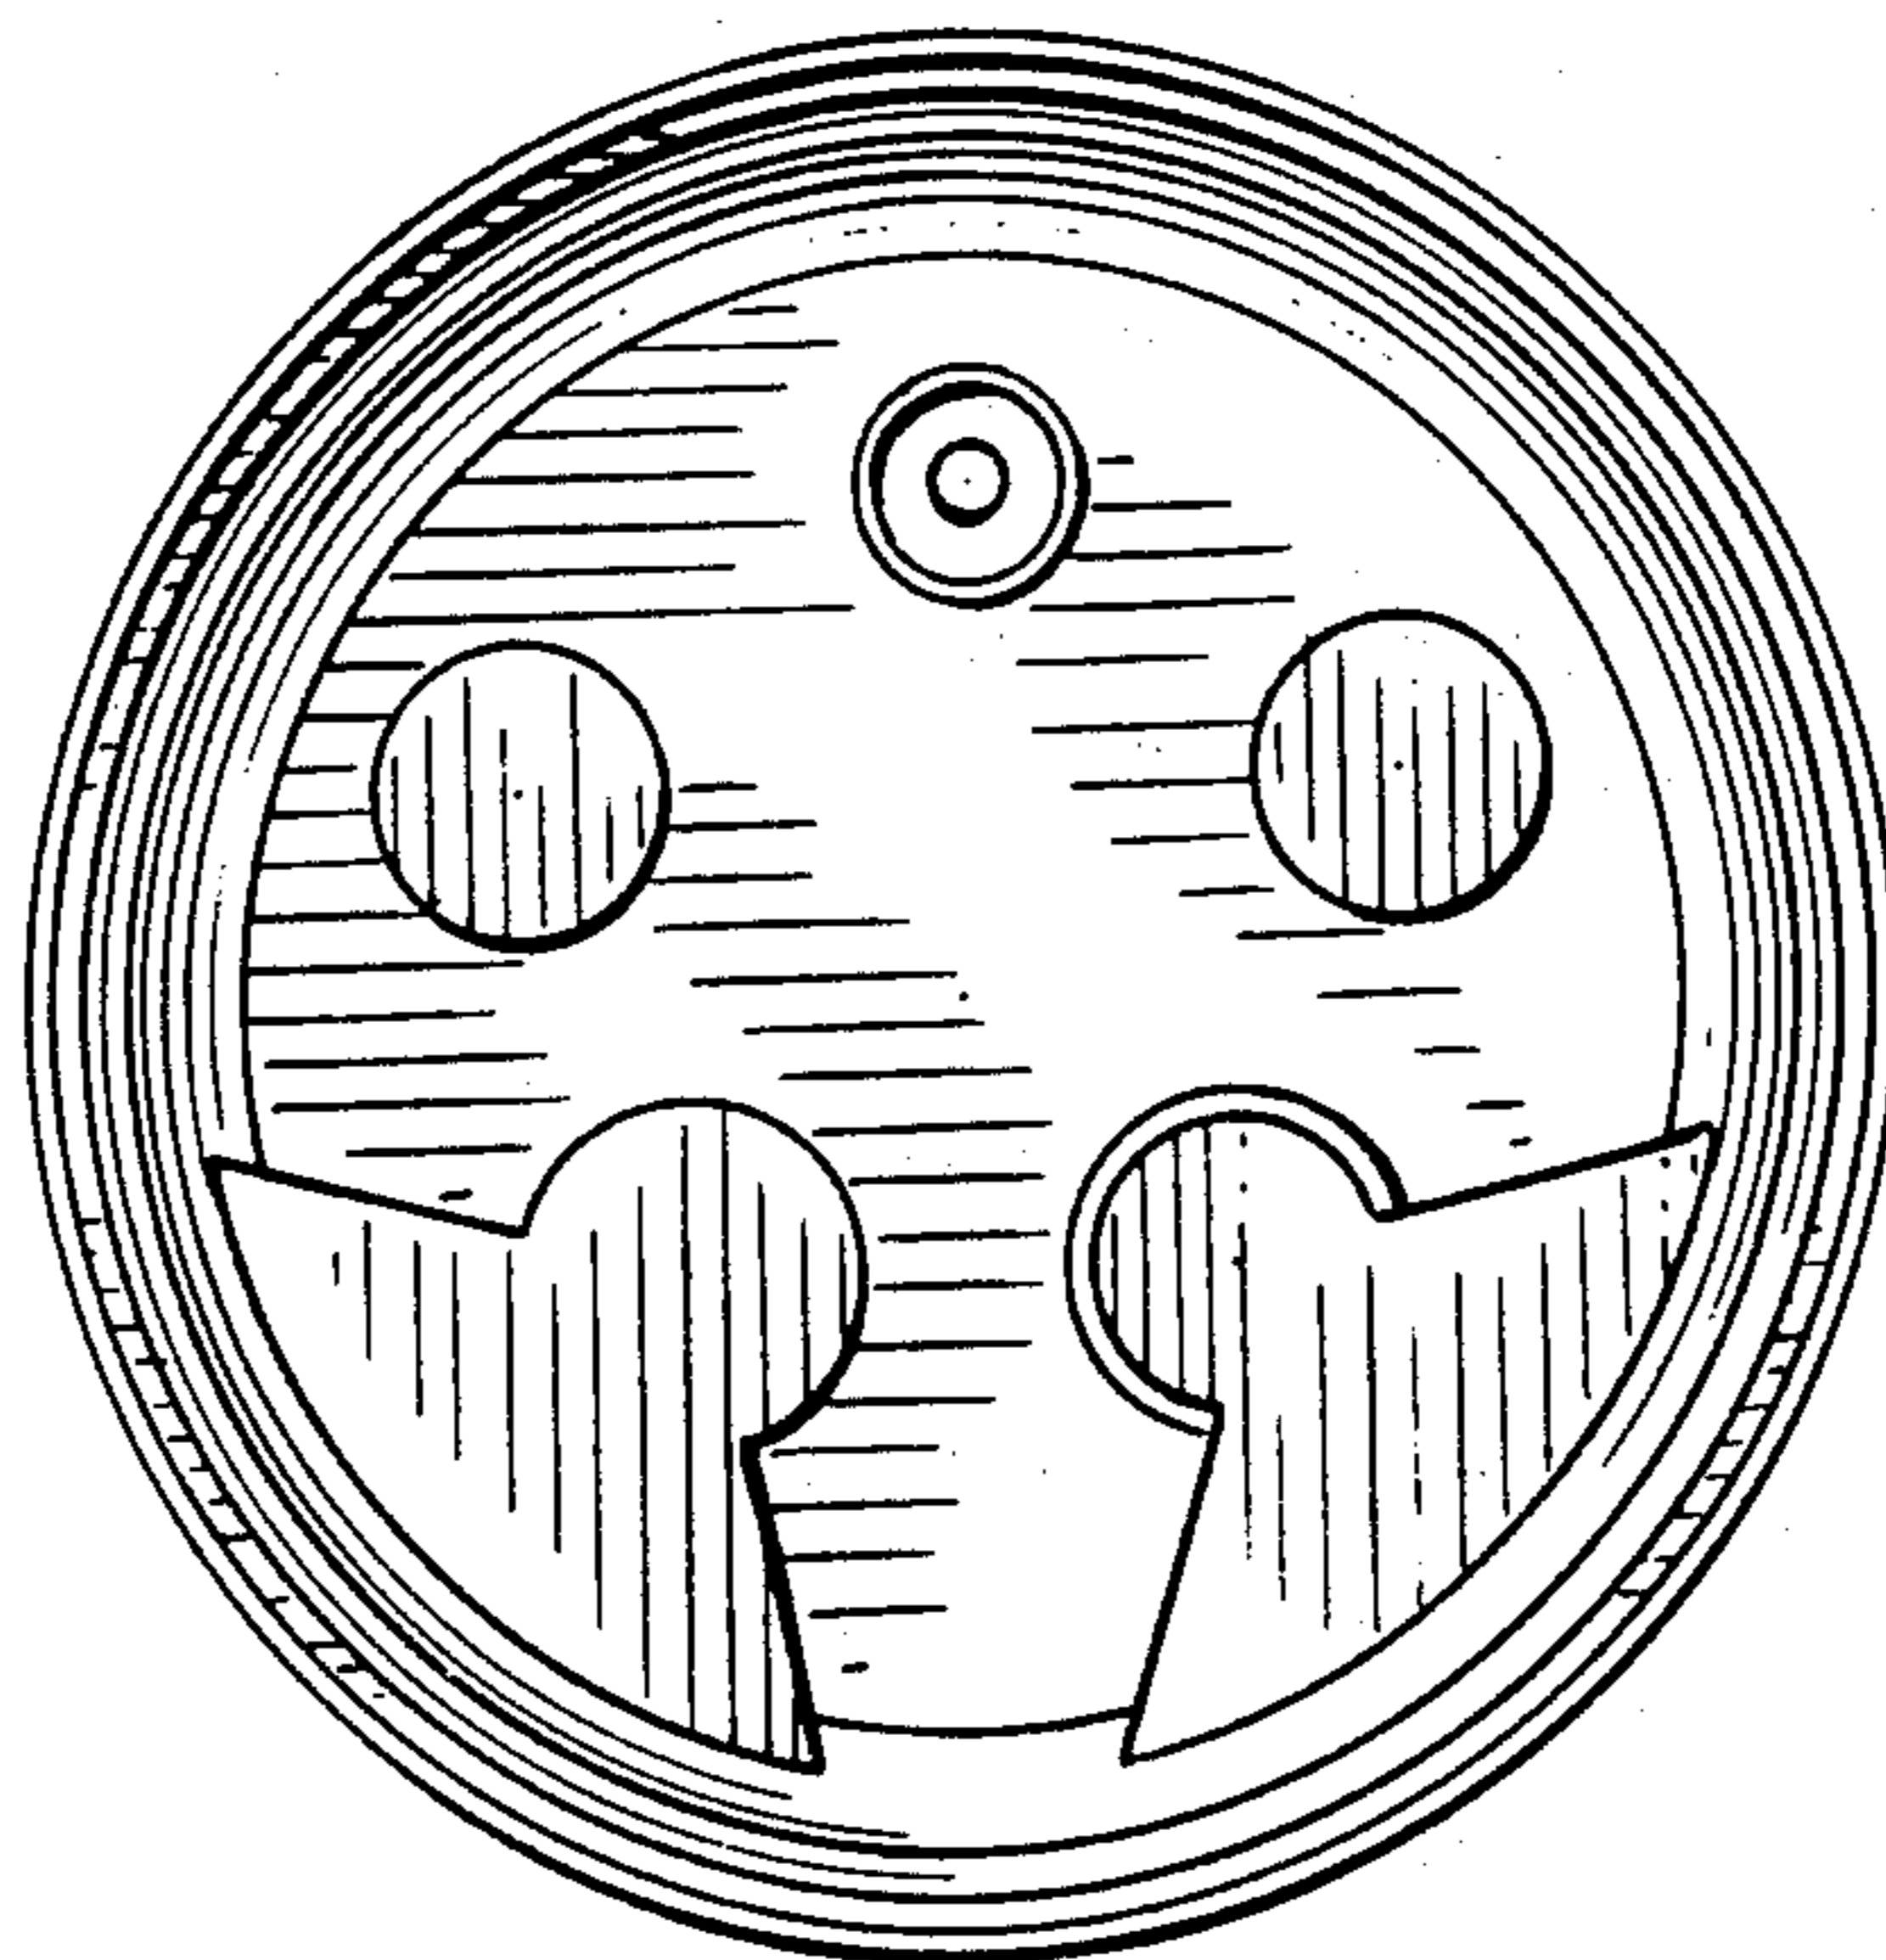


Fig. 5.





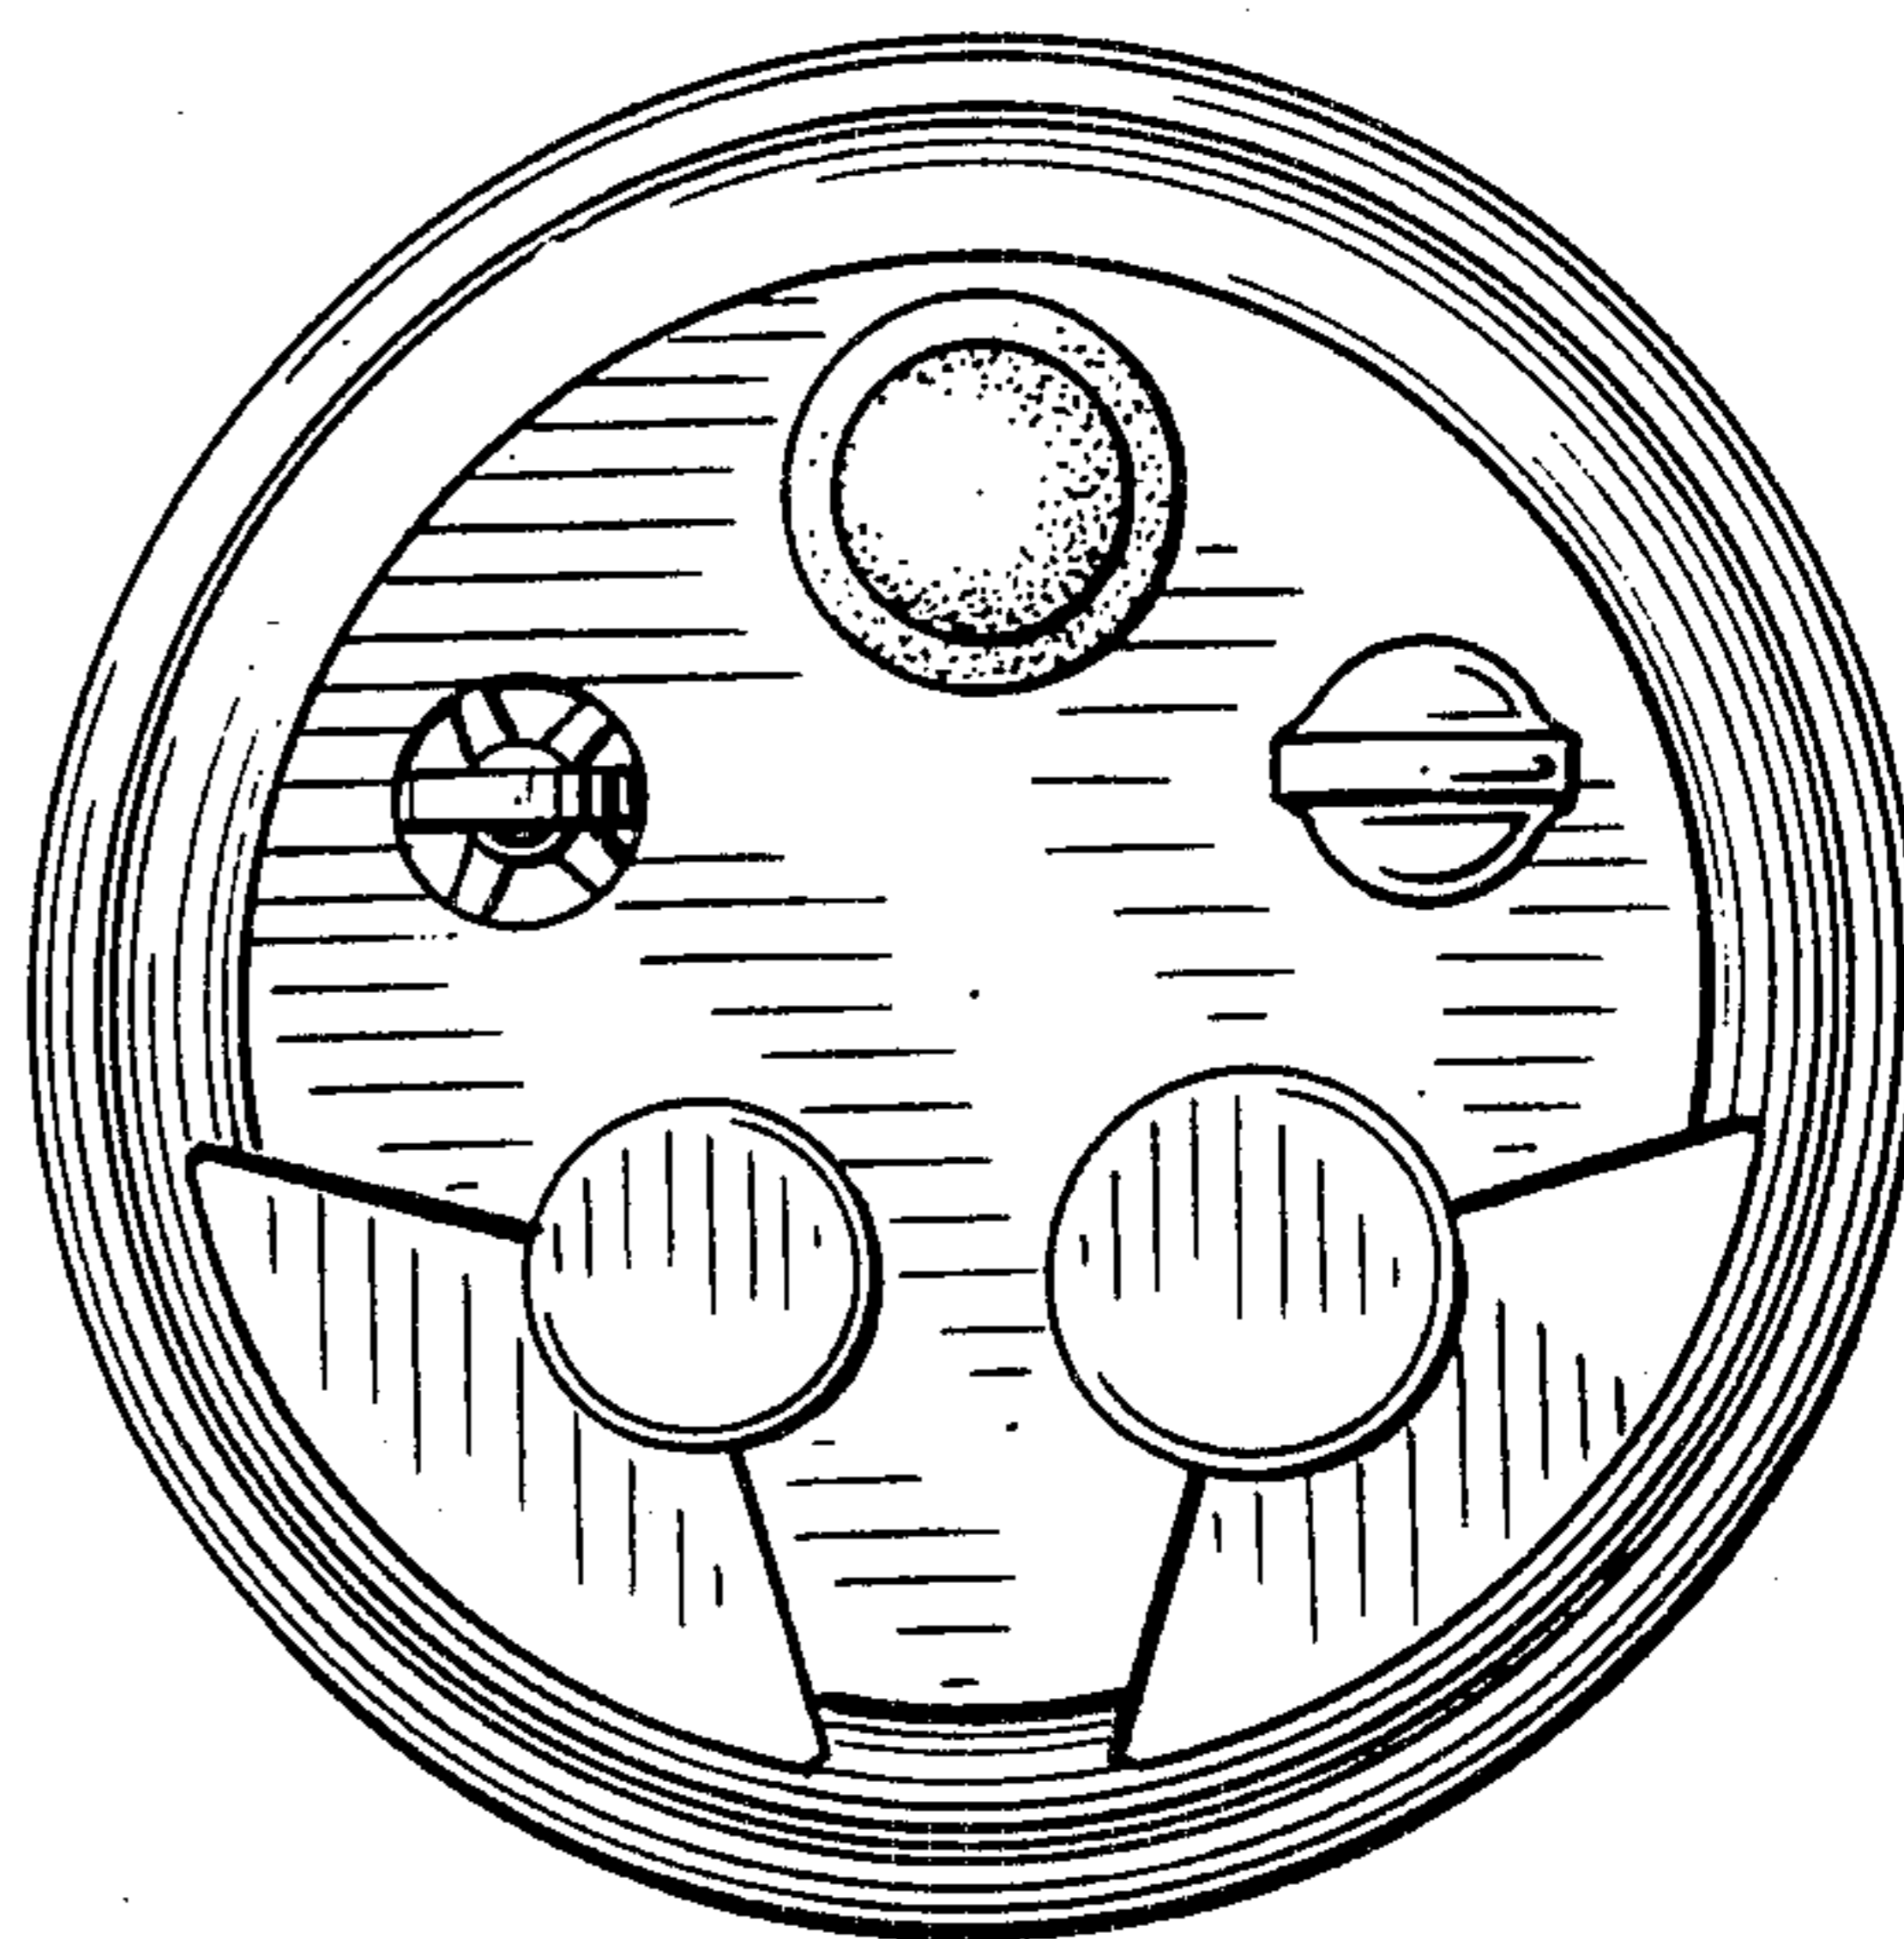
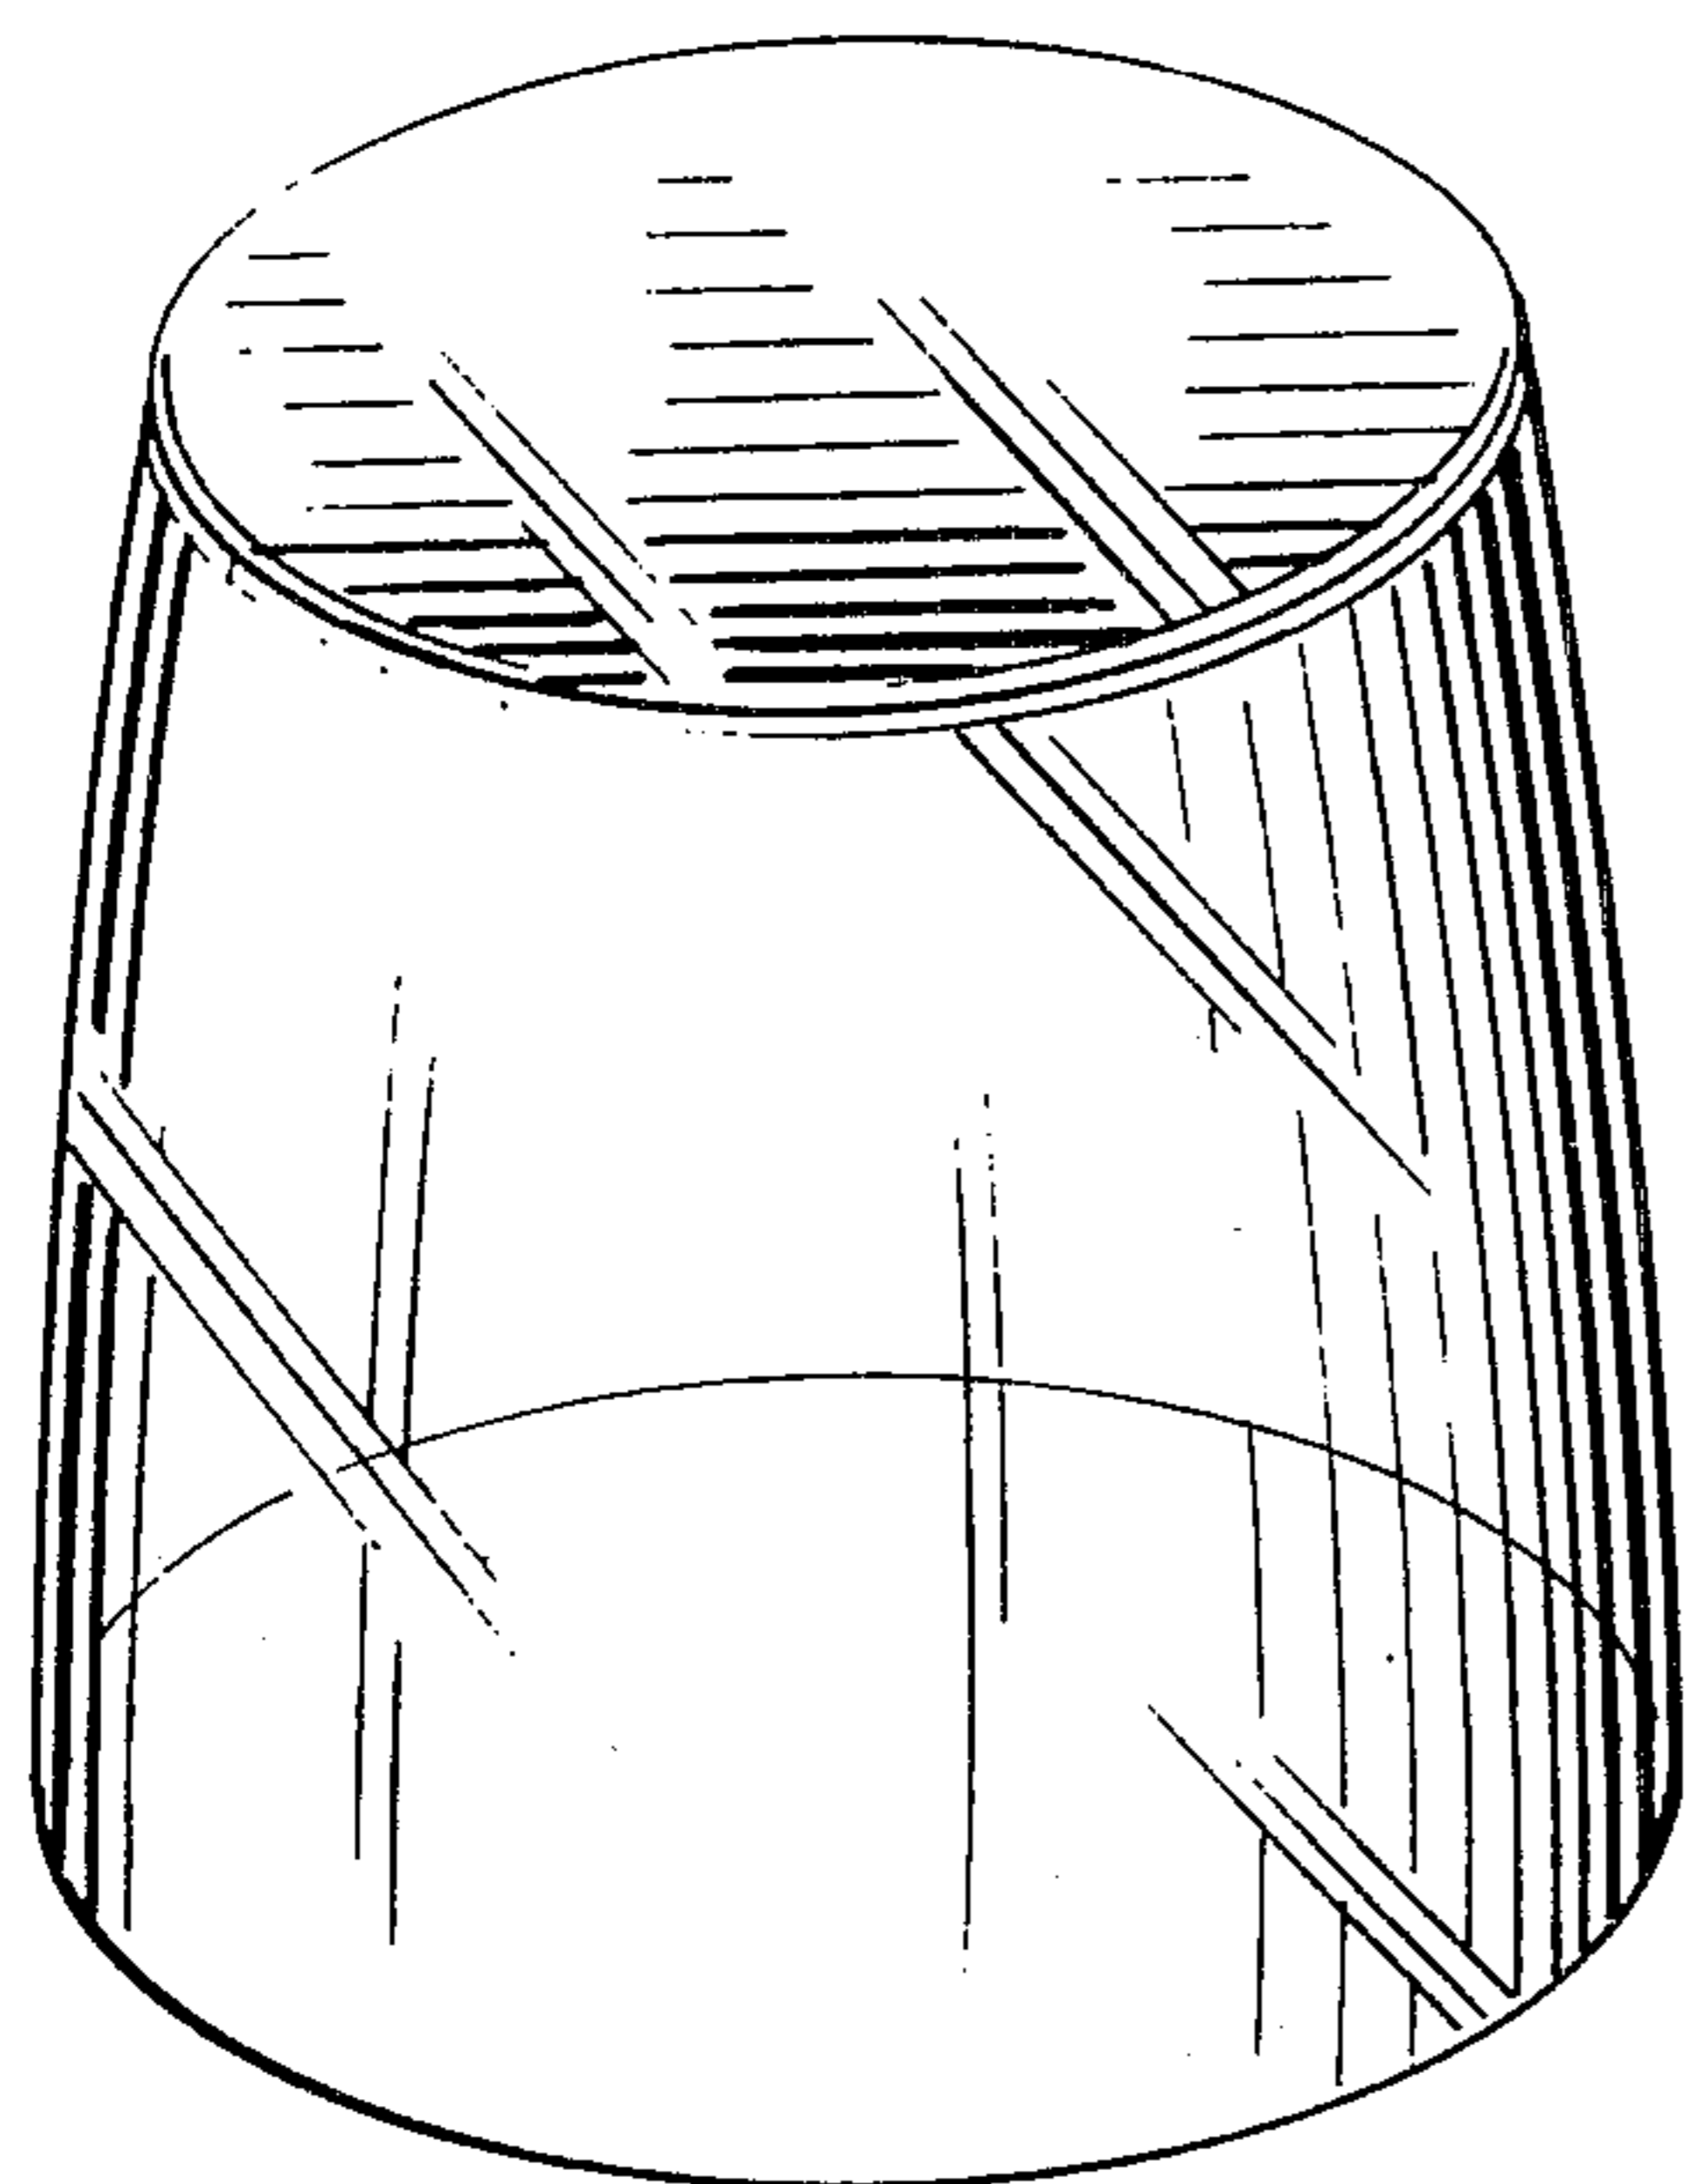


Fig. 7.

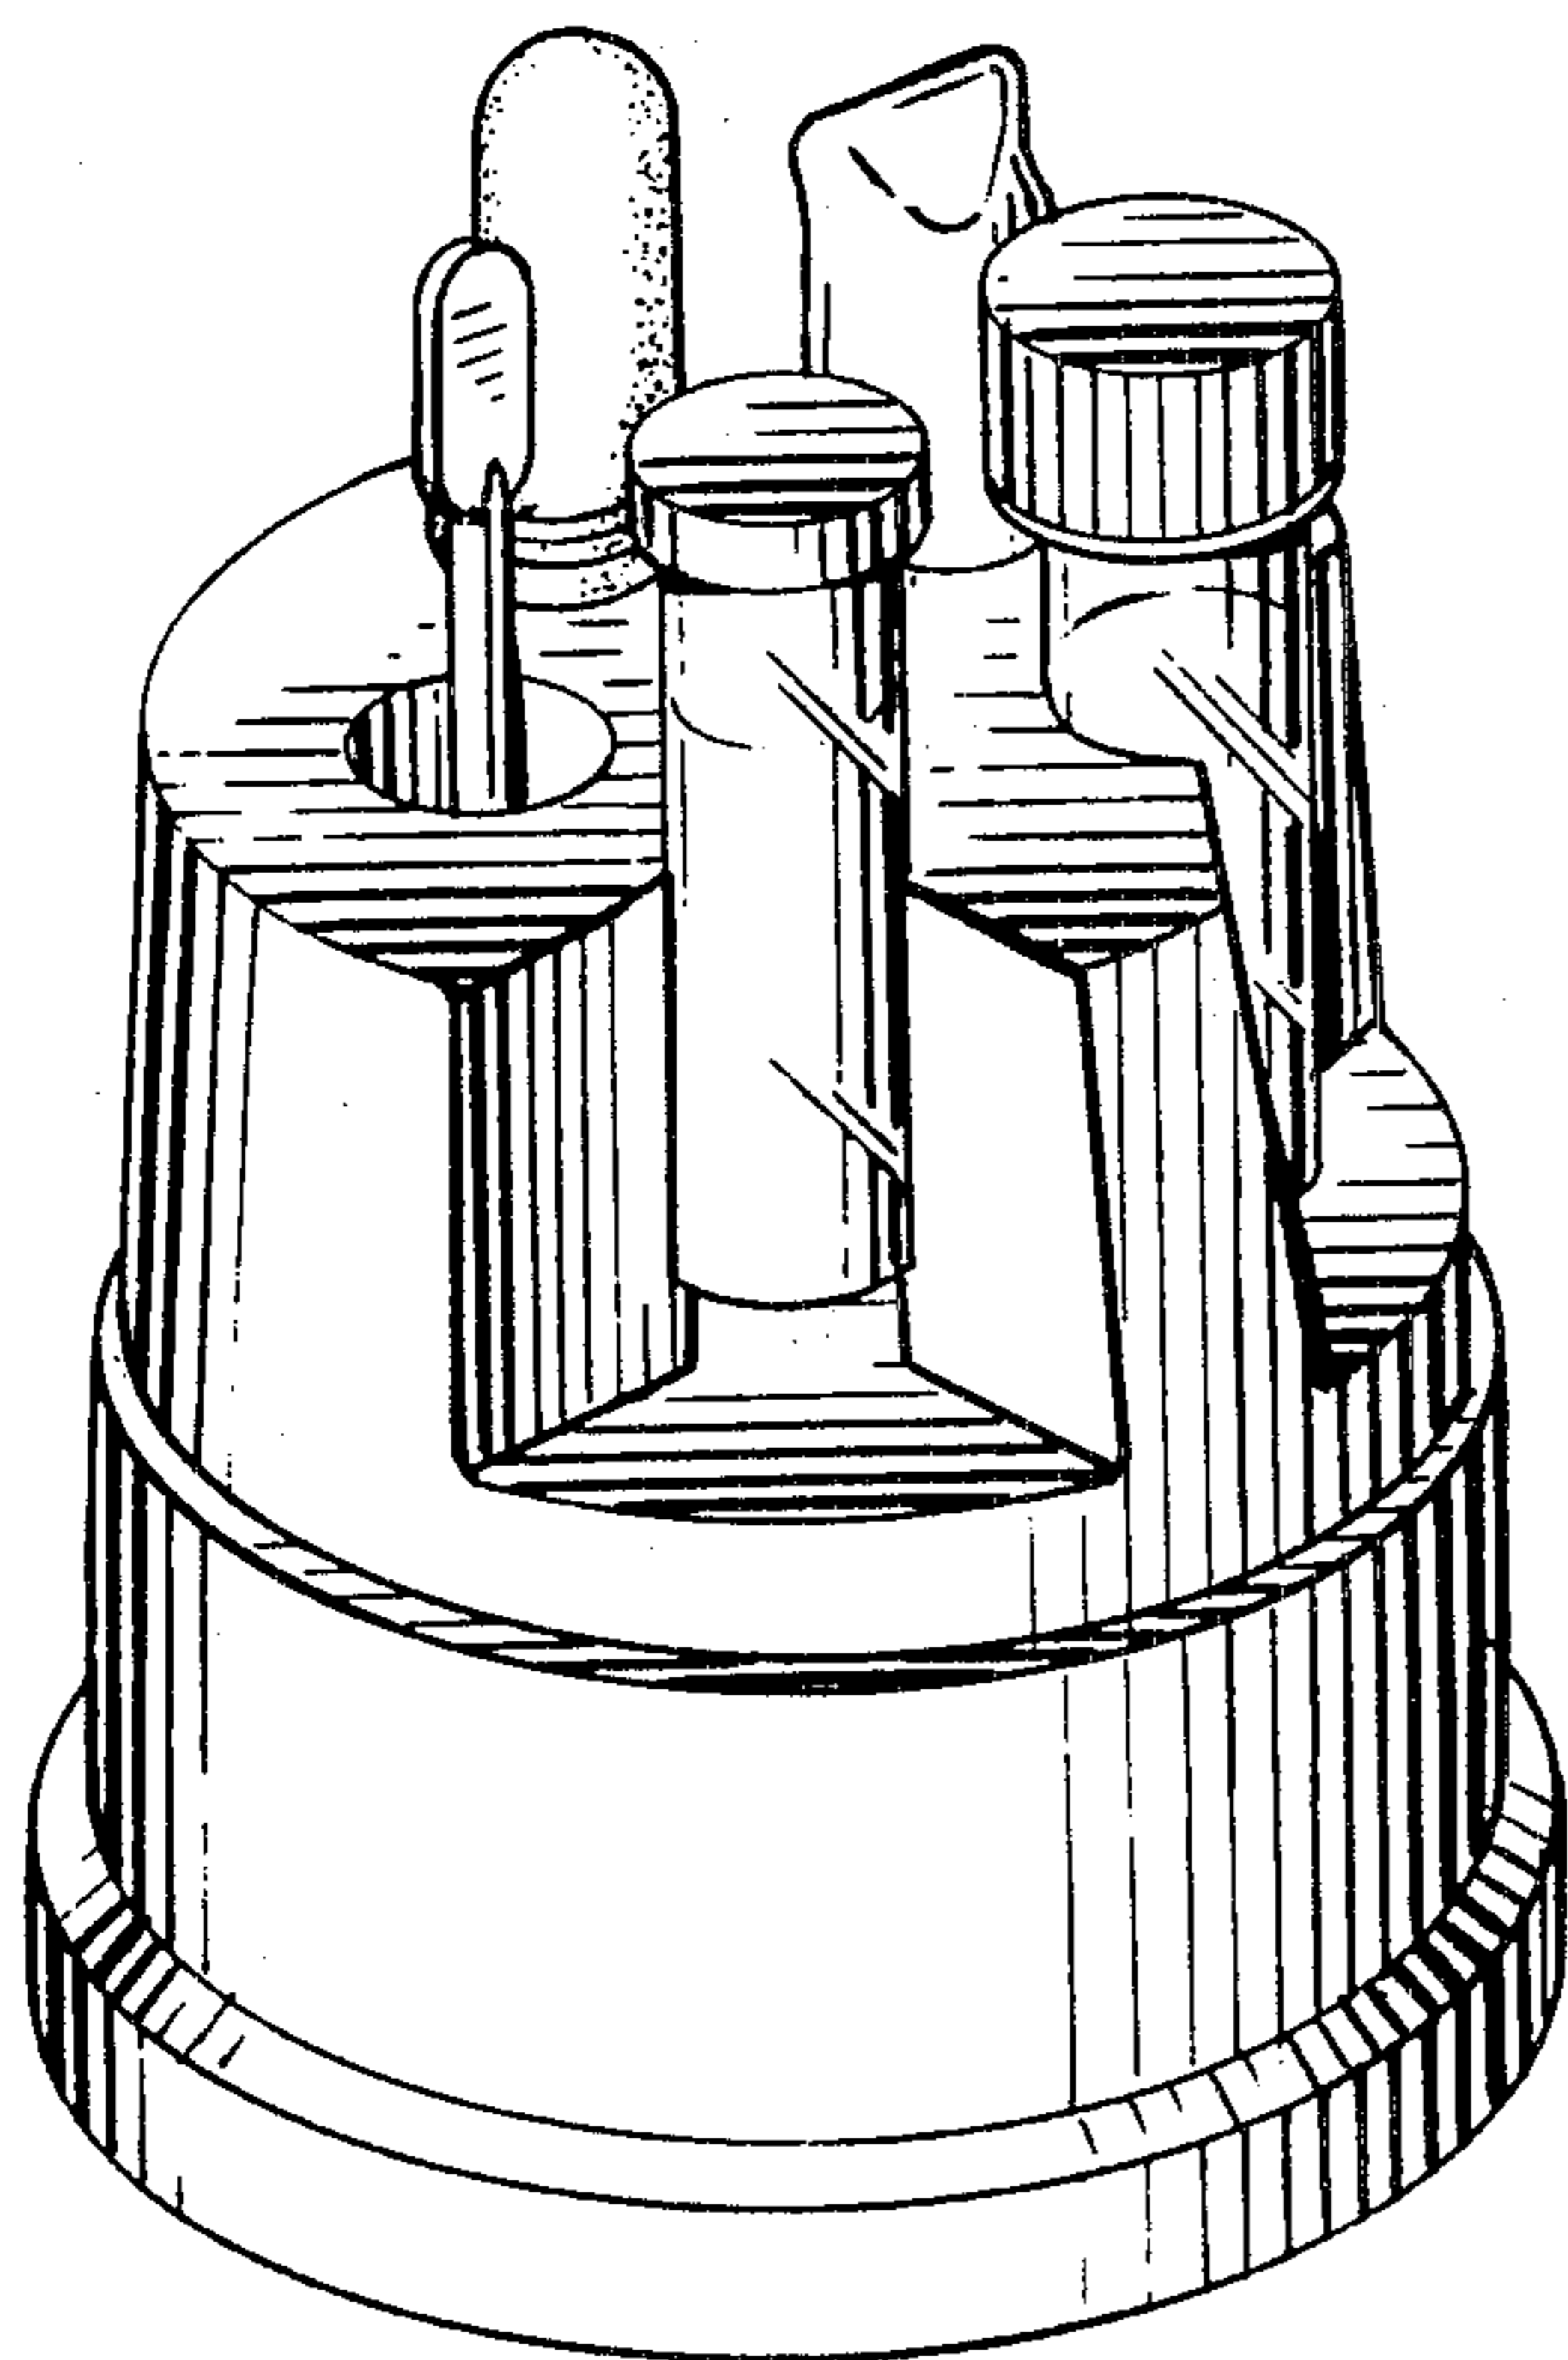


Fig. 6.

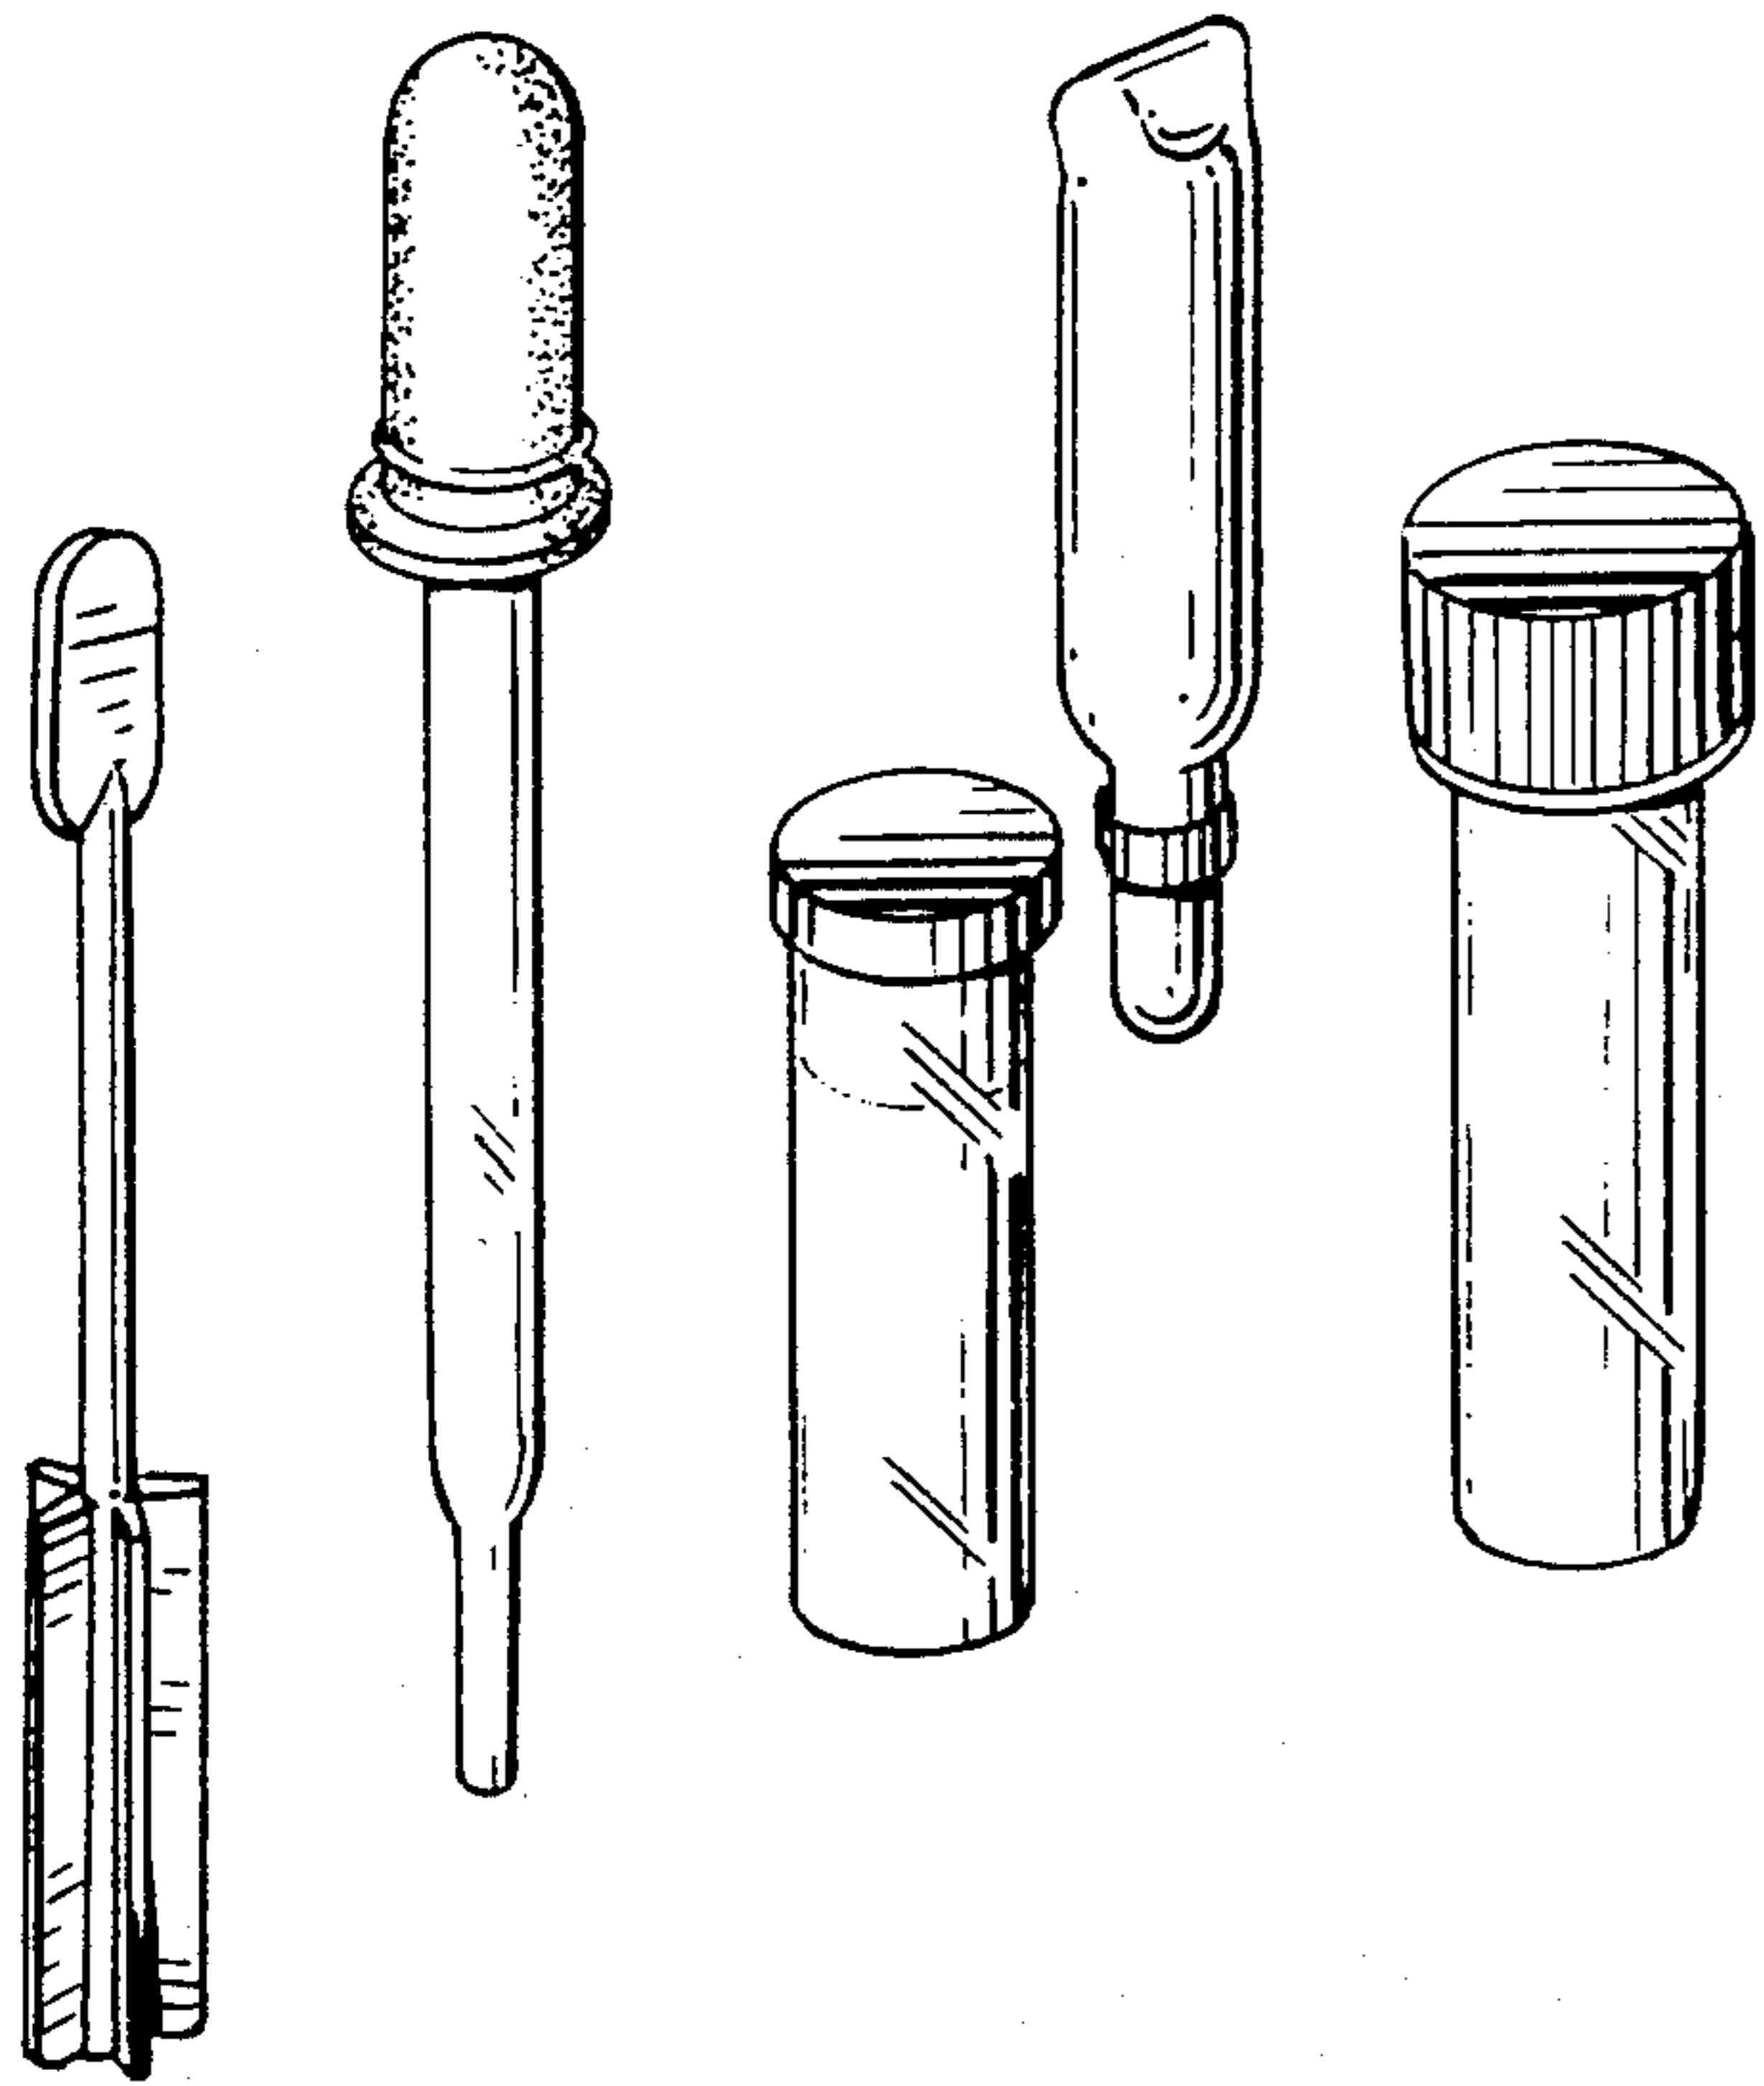


Fig. 8.

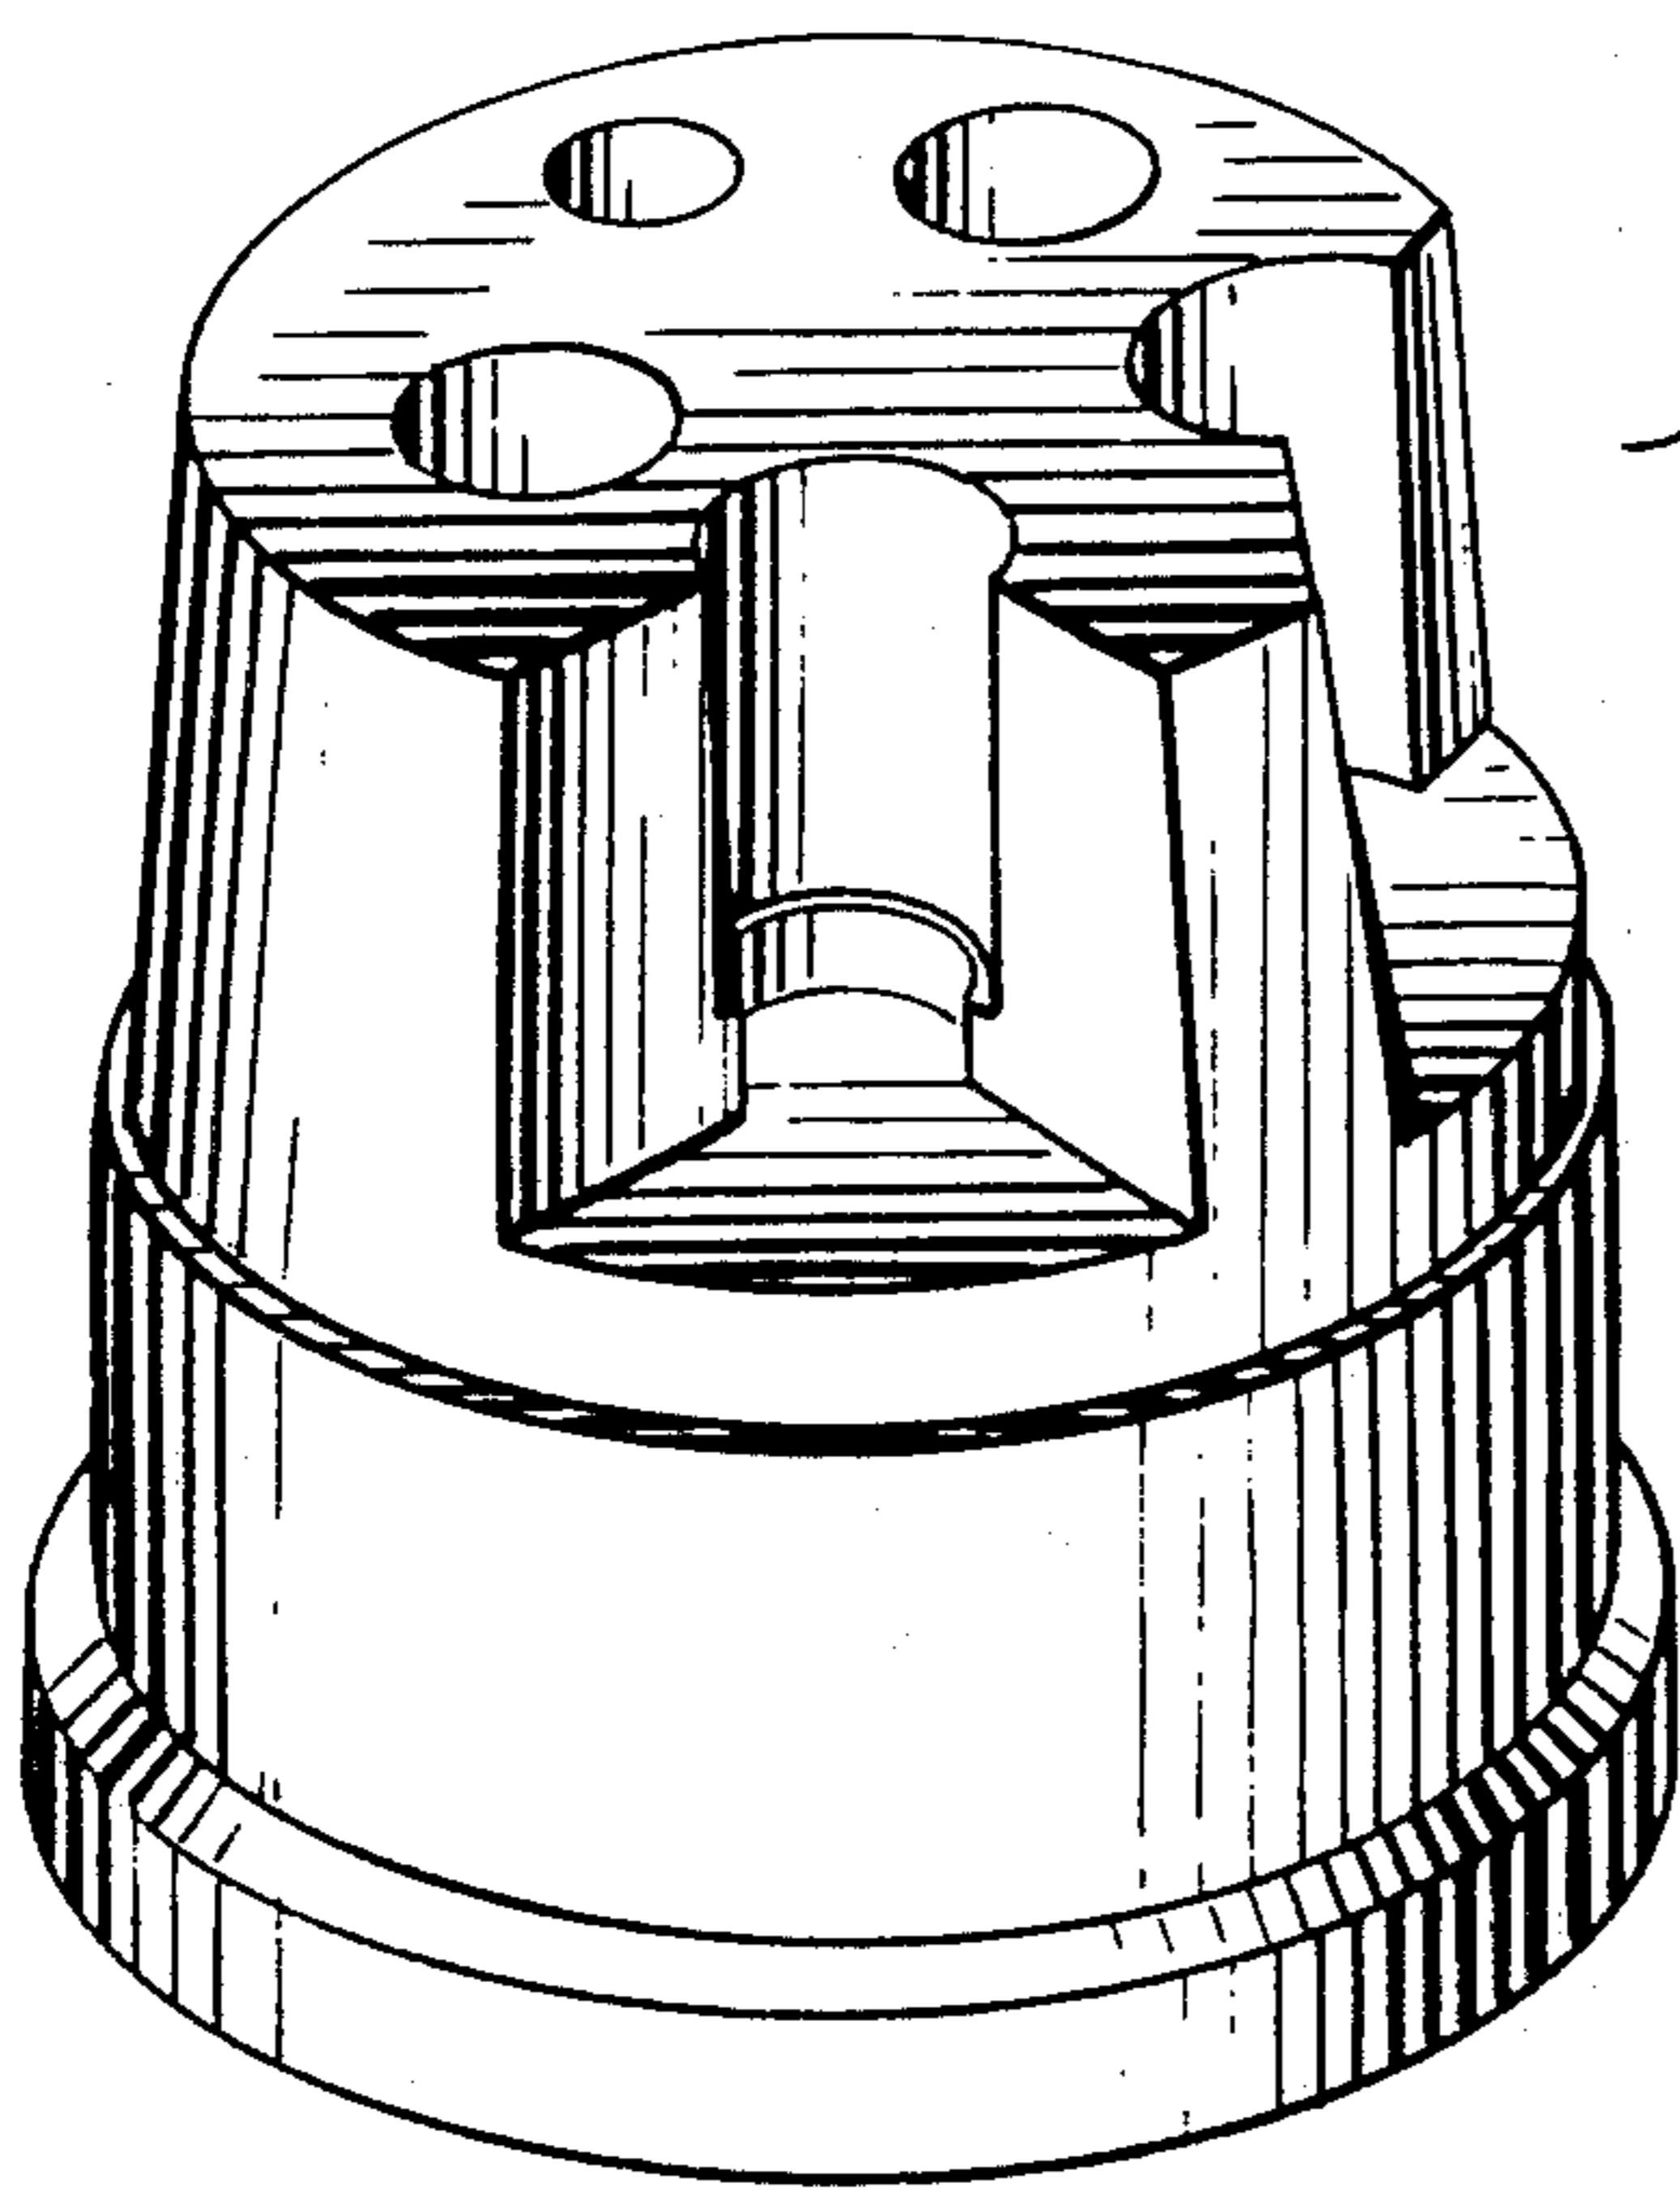


Fig. 9.

