

[54] **NOMOGRAM FOR CALCULATING THE
MAXIMUM TOLERABLE BLOOD LOSS OF
A PATIENT**

[75] **Inventor: Henrik Zetterström, Frösön, Sweden**

[73] **Assignee: Pharmacia AB, Uppsala, Sweden**

[**] **Term: 14 Years**

[21] **Appl. No.: 790,934**

[22] **Filed: Oct. 24, 1985**

[30] **Foreign Application Priority Data**

May 10, 1985 [SE] Sweden 85-1262

[52] **U.S. Cl.** D24/21; D10/61;
D24/8; D24/17

[58] **Field of Search** D24/8, 99, 17, 21;
D10/61, 62, 64; D19/1, 2; 33/1 C, 1 B, 571,
177, 563; 128/668, 670, 706

[56] **References Cited**

U.S. PATENT DOCUMENTS

D. 254,125 2/1980 Powell D10/61
D. 288,786 3/1987 Olsson D10/61
3,377,707 4/1968 Breese 33/1 B X
4,550,502 11/1985 Grayzel 128/706 X

Primary Examiner—Wallace R. Burke
Assistant Examiner—Stella M. Reid
Attorney, Agent, or Firm—Bacon & Thomas

[57] **CLAIM**

The ornamental design for a nomogram for calculating the maximum tolerable blood loss of a patient, as shown and described.

DESCRIPTION

FIG. 1 is a top plan view of a nomogram for calculating the maximum tolerable blood loss of a patient, embodying my new design;

FIG. 2 is a side elevational view thereof; and

FIG. 3 is an end elevational view thereof.

The undisclosed bottom is plain and unornamented.

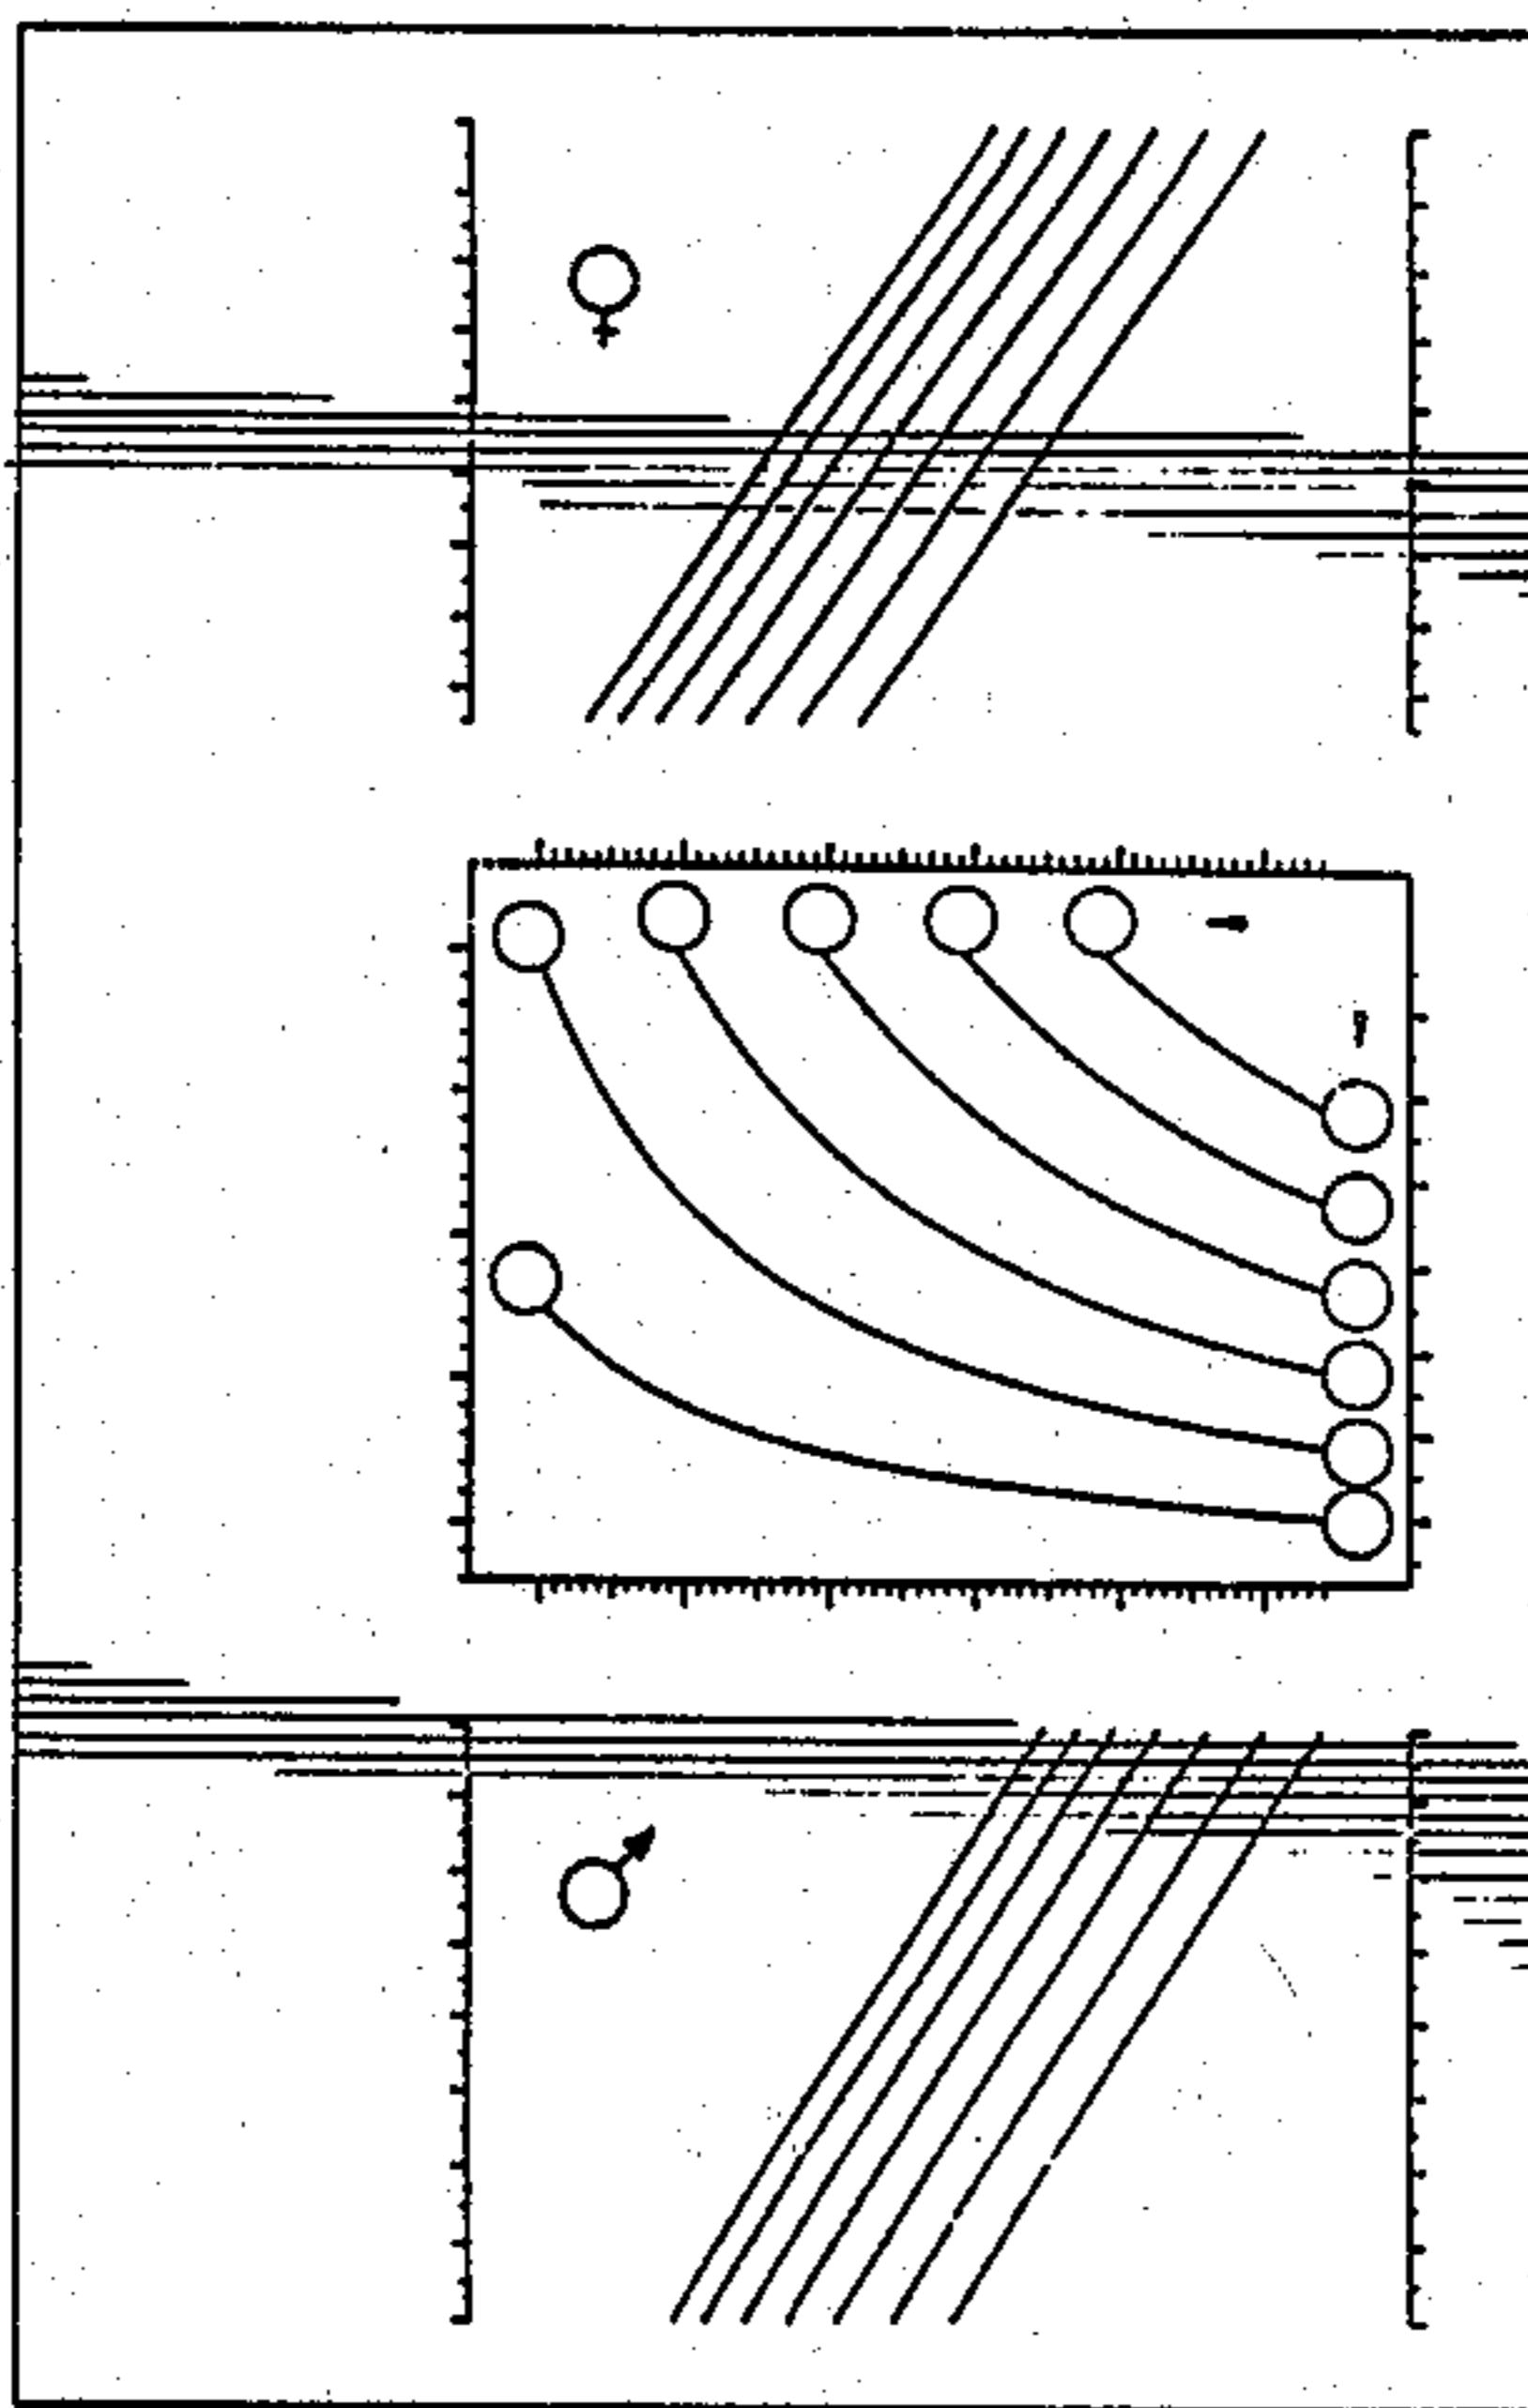


Fig. 1

Fig. 2

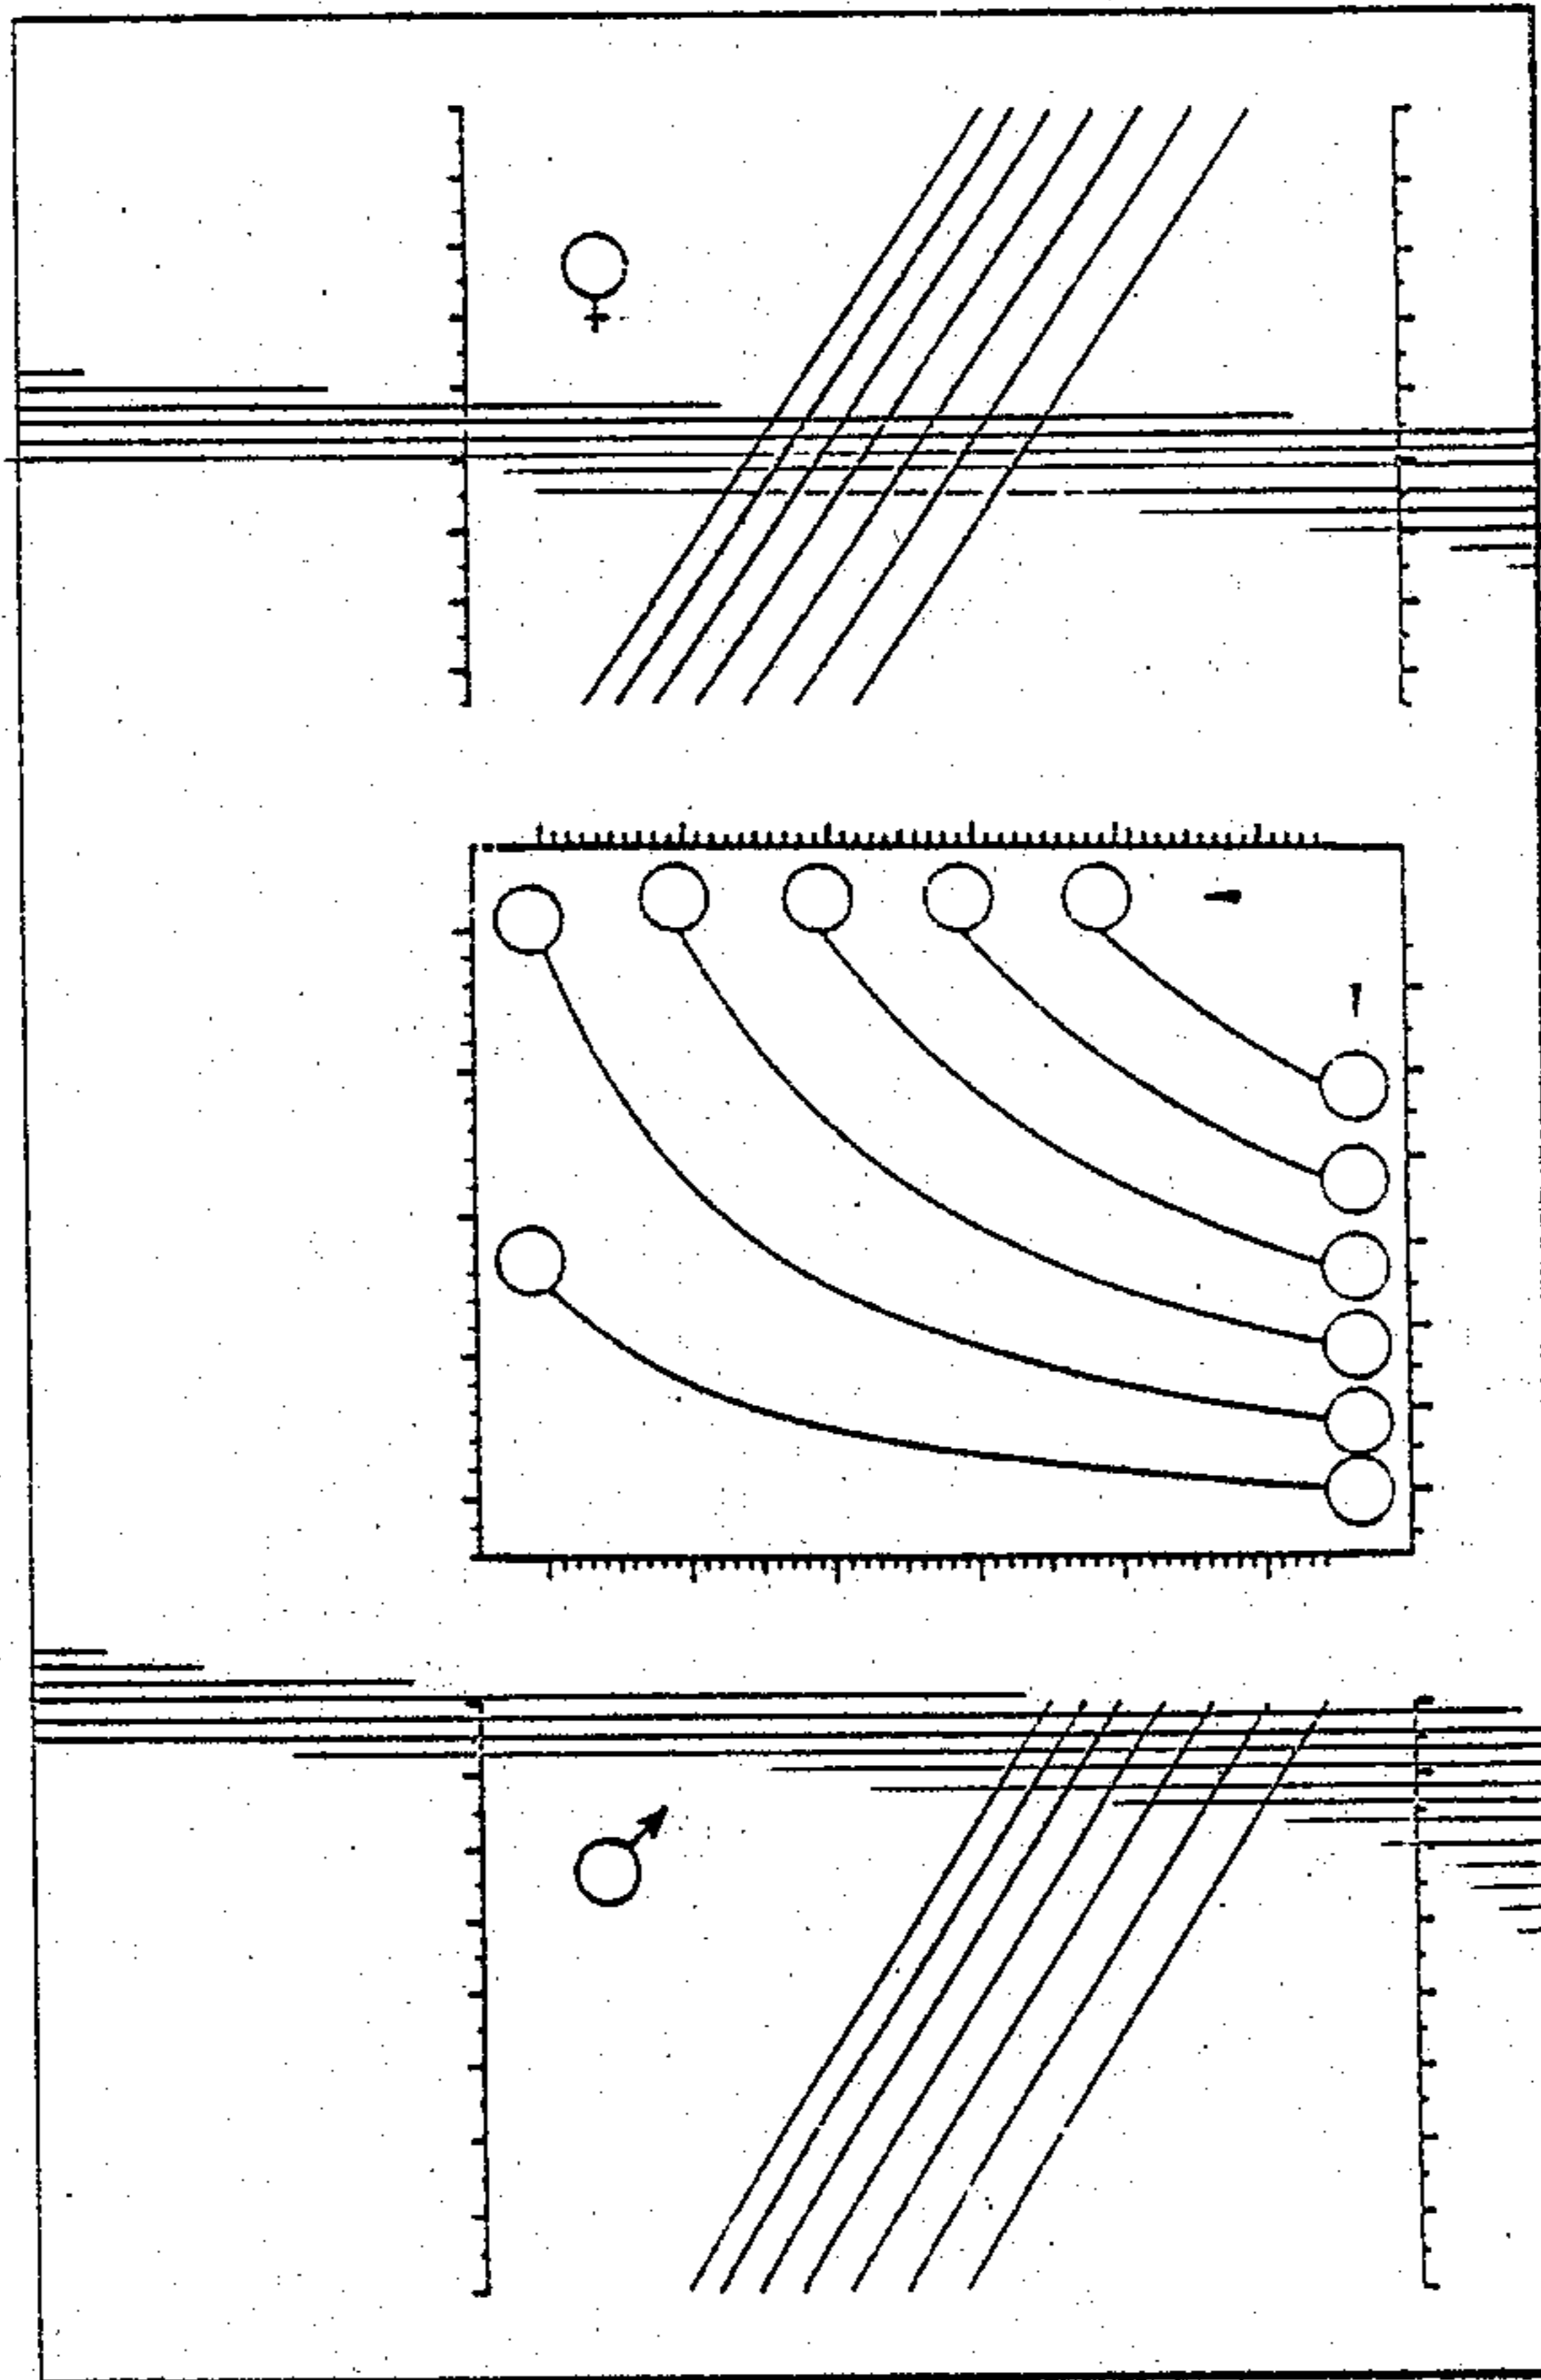


Fig. 3

