

[54] AUTOMATIC ENZYME IMMUNOLOGICAL ANALYZER

4,078,895 3/1978 Moran 422/66
4,483,823 11/1984 Umetsu et al. 422/64 X

[75] Inventors: Masaharu Kame, Sagamihara;
Kenichi Abe, Hachioji, both of Japan

Primary Examiner—Wallace R. Burke
Assistant Examiner—Stella M. Reid
Attorney, Agent, or Firm—Ostrolenk, Faber, Gerb &
Soffen

[73] Assignee: Olympus Optical Company, Inc.,
Japan

[57] CLAIM

[**] Term: 14 Years

The ornamental design for an automatic enzyme immu-
nological analyzer, as shown and described.

[21] Appl. No.: 858,298

DESCRIPTION

[22] Filed: Apr. 30, 1986

[52] U.S. Cl. D24/1.1

[58] Field of Search D24/8, 1.1, 17;
422/63-68, 50; 356/39, 40, 41; 436/43, 48;
D10/81

FIG. 1 is a front, top, and right side perspective view of
an automatic enzyme immunological analyzer, showing
our new design;

FIG. 2 is a rear, bottom, and left side perspective view
thereof;

FIG. 3 is a front elevational view thereof;

FIG. 4 is a rear elevational view thereof;

FIG. 5 is a right side elevational view thereof;

FIG. 6 is a left side elevational view thereof;

FIG. 7 is a top plan view thereof; and

FIG. 8 is a bottom plan view thereof.

[56] References Cited

U.S. PATENT DOCUMENTS

- D. 264,873 6/1982 Olson et al. D24/1.1
- D. 281,310 11/1985 Hattori et al. D24/1.1 X
- D. 282,203 1/1986 Leonard et al. D24/1.1

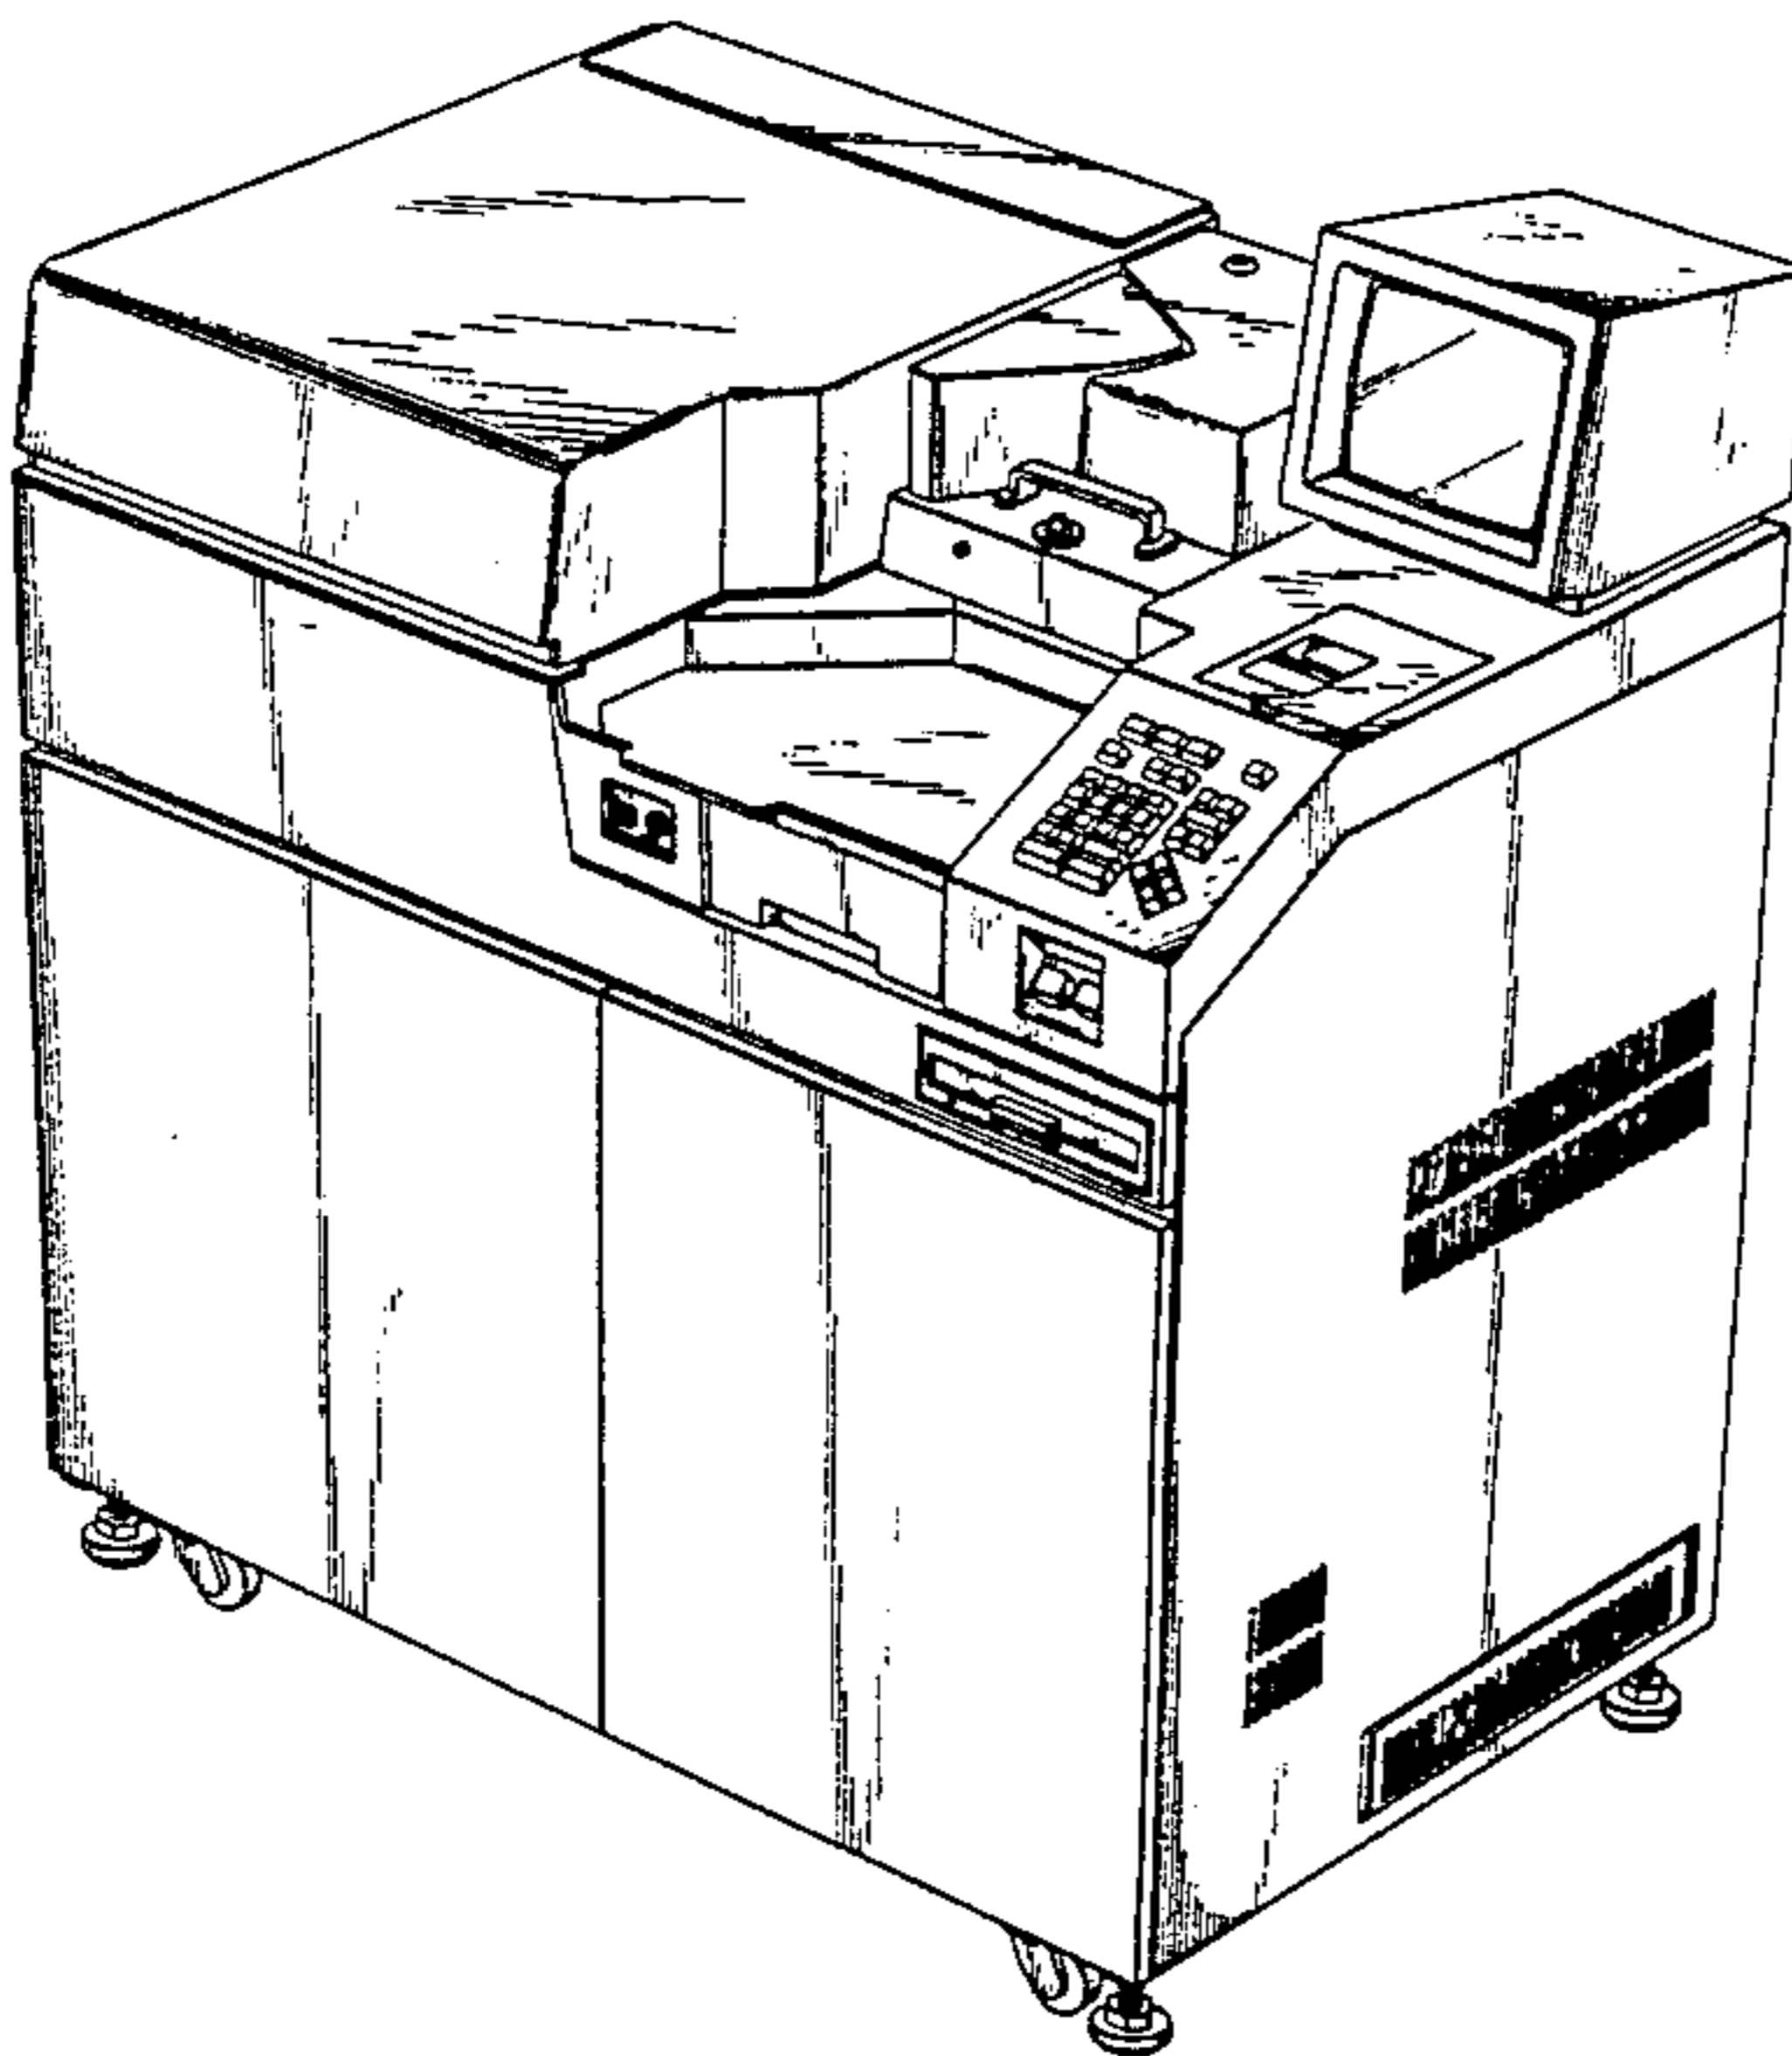


FIG. 1

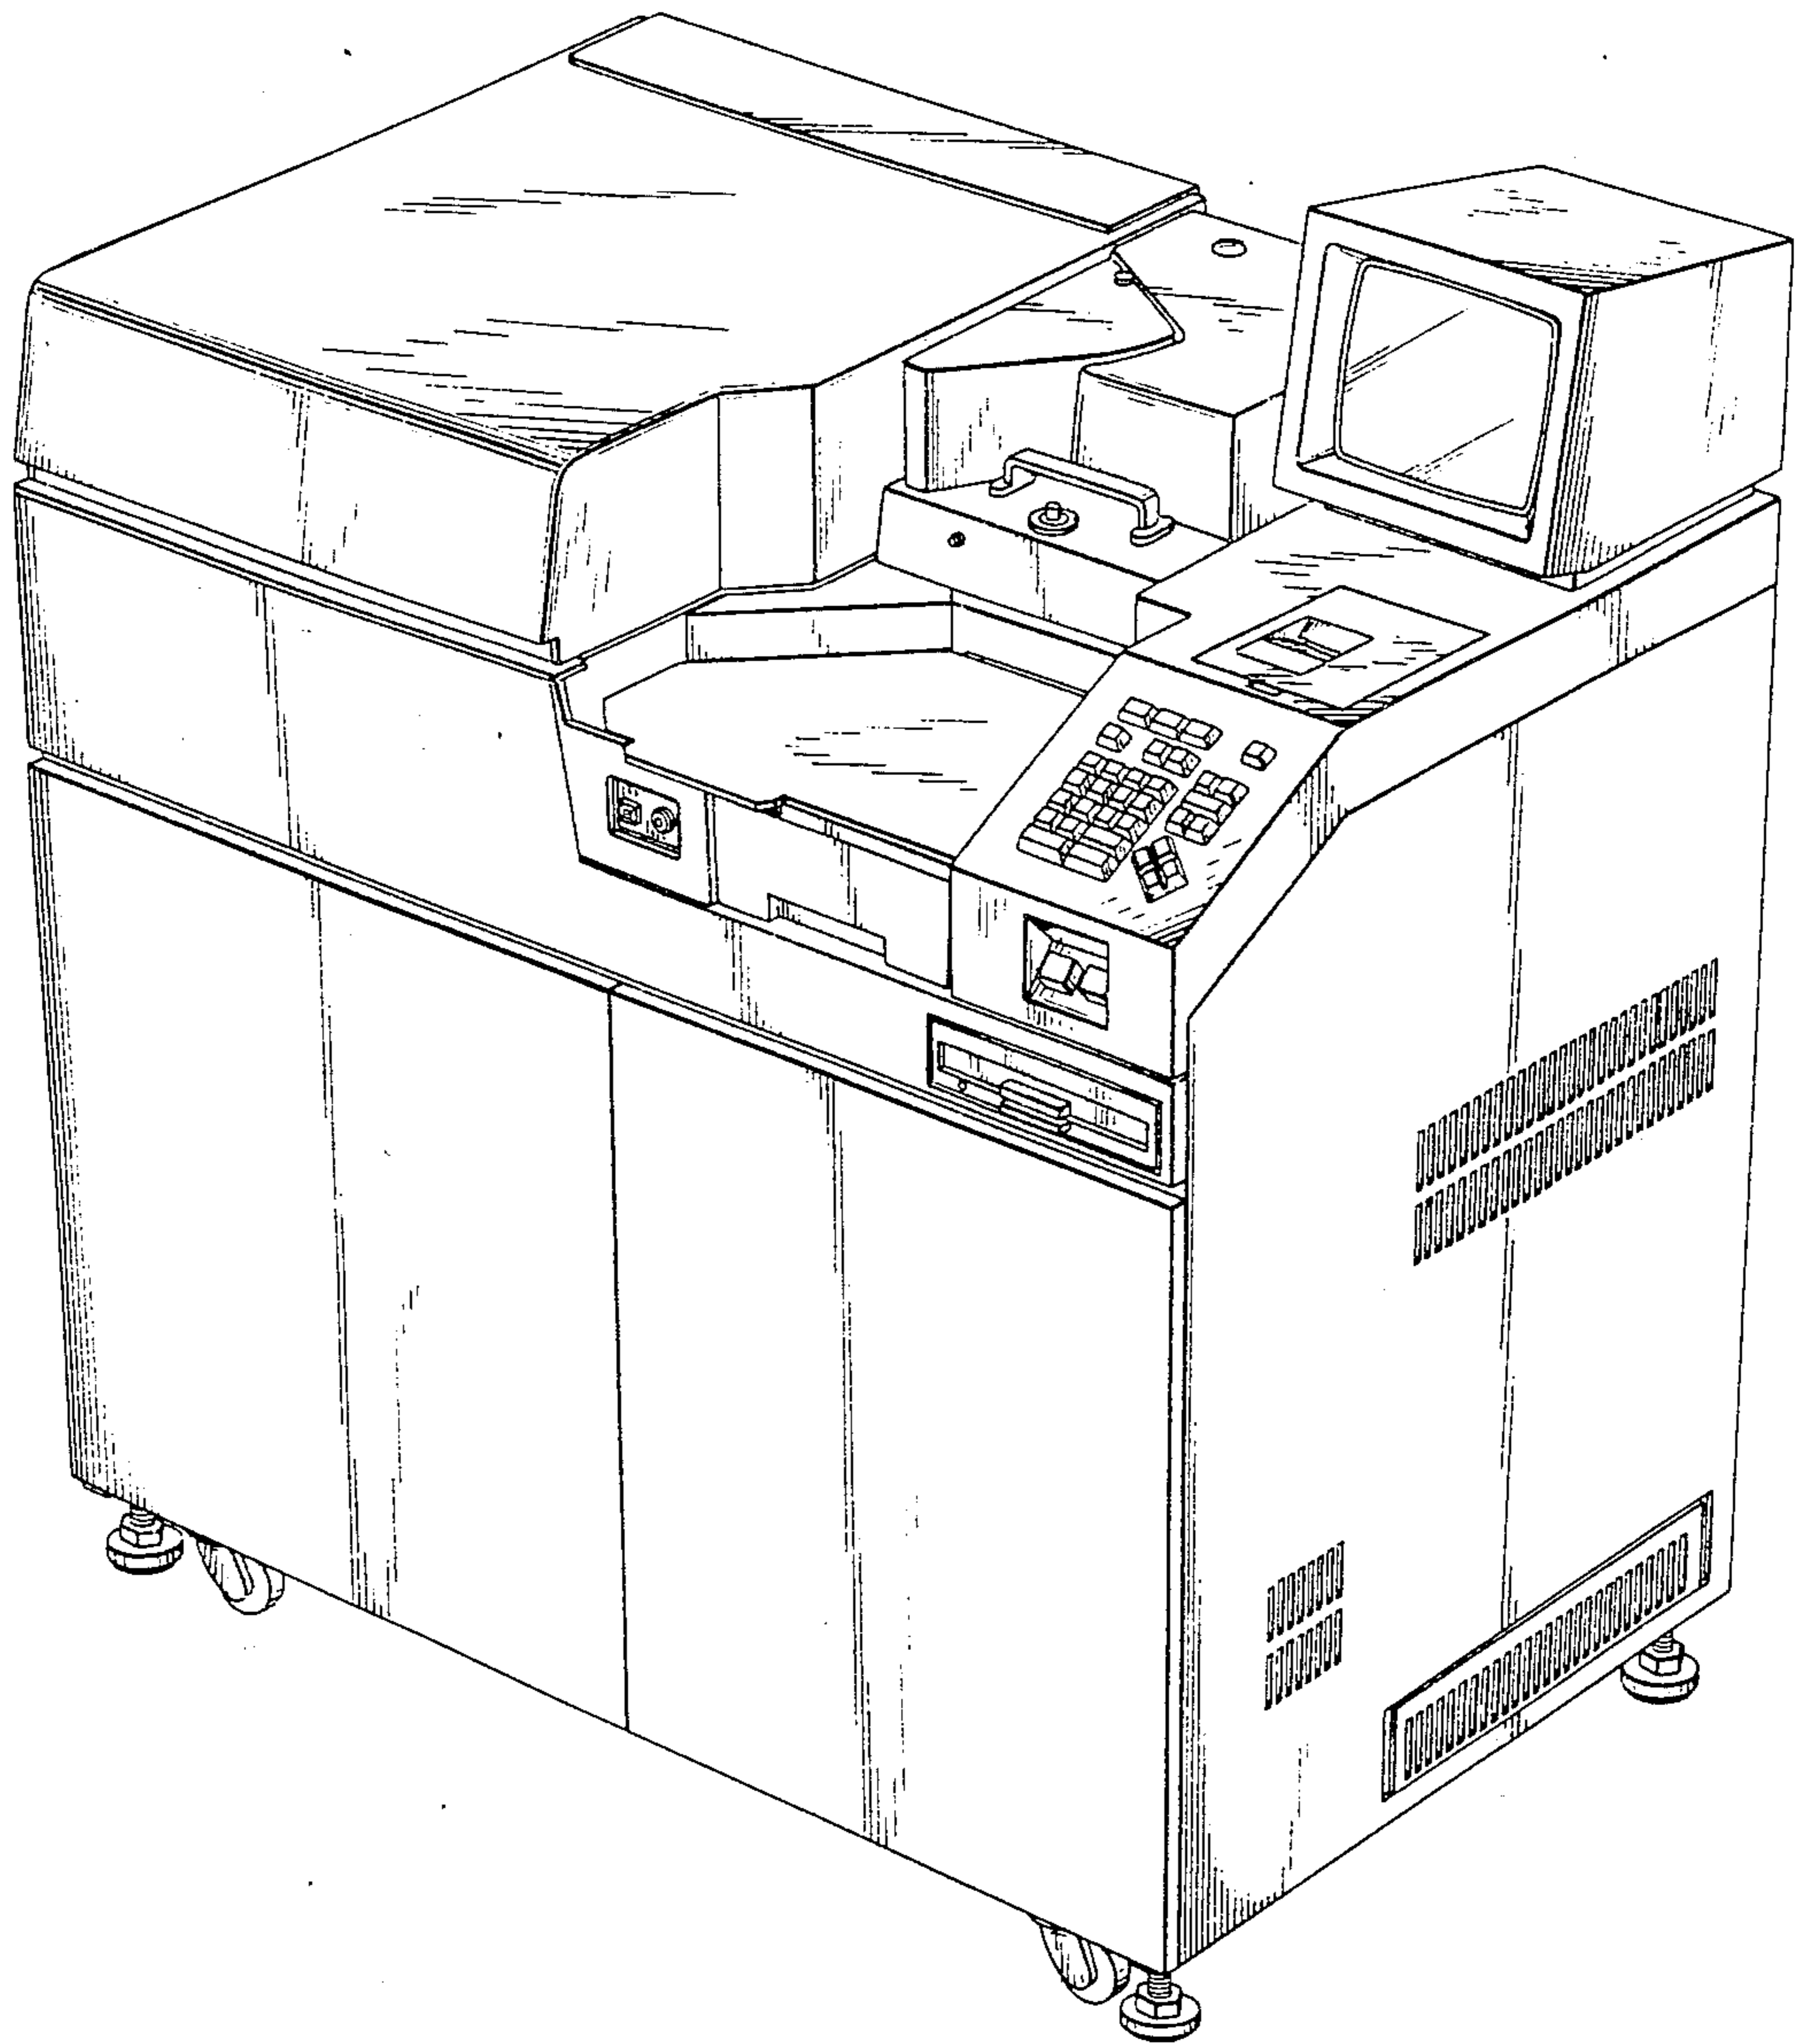


FIG. 2

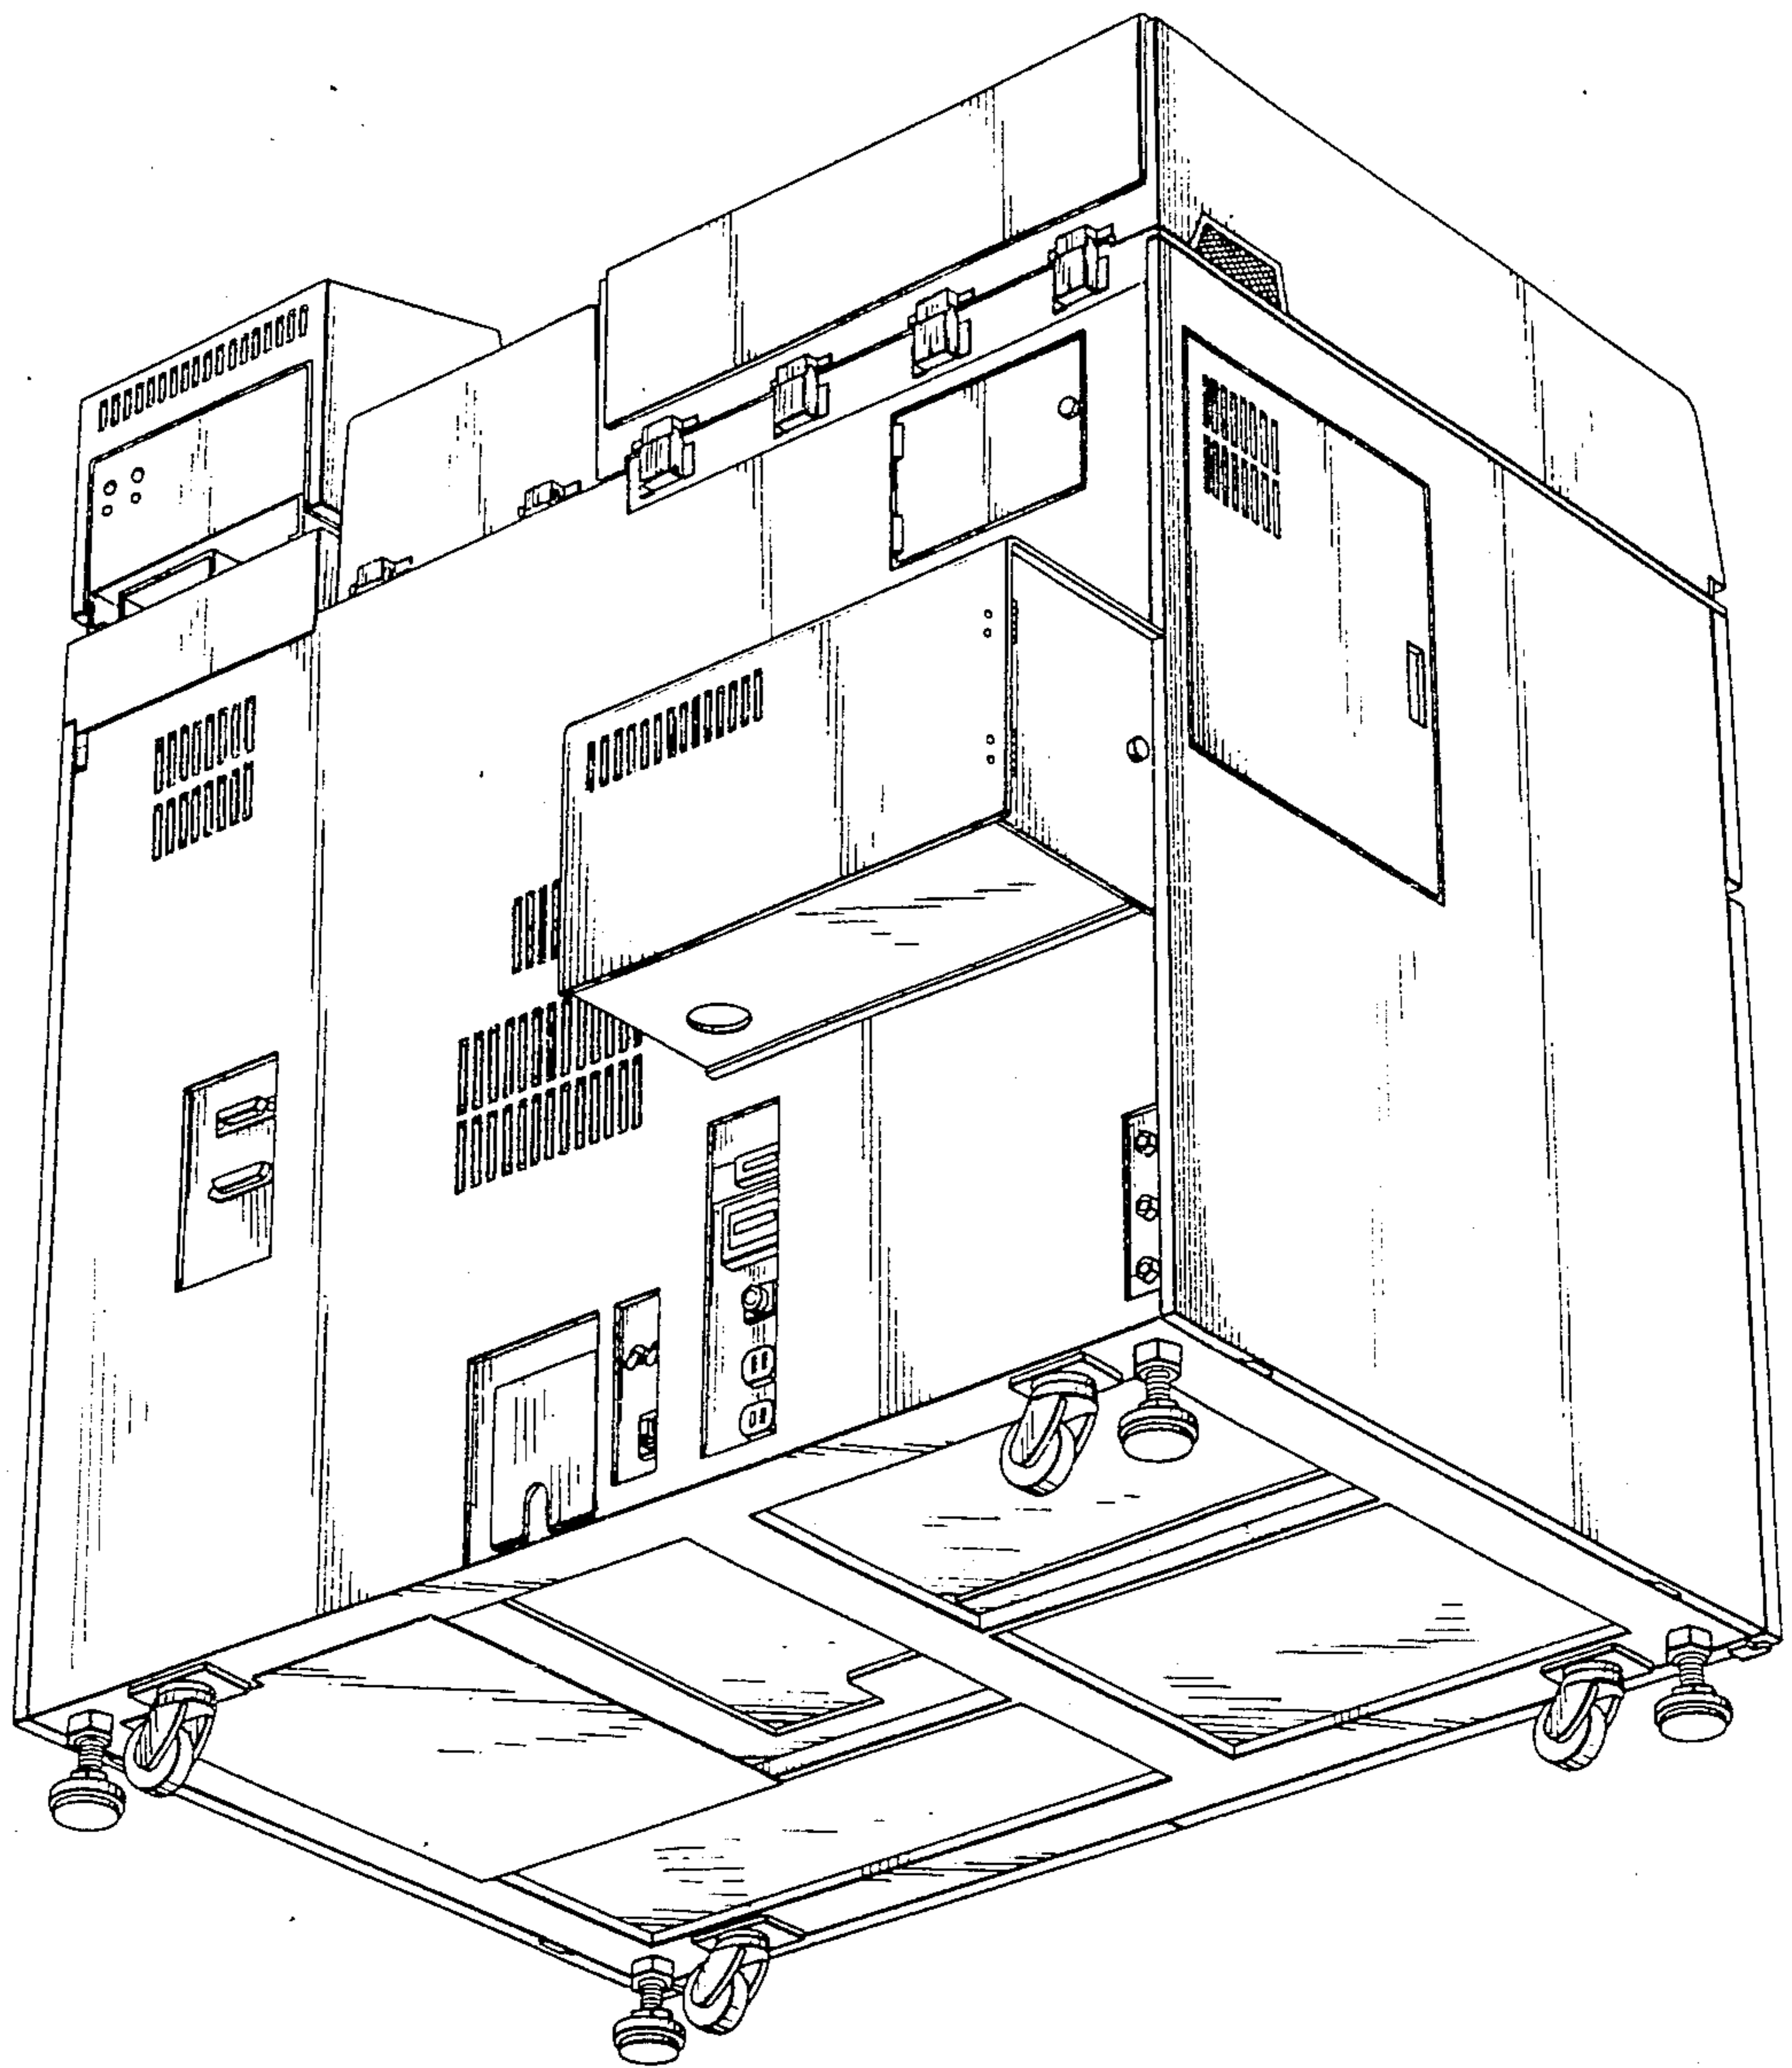


FIG. 3

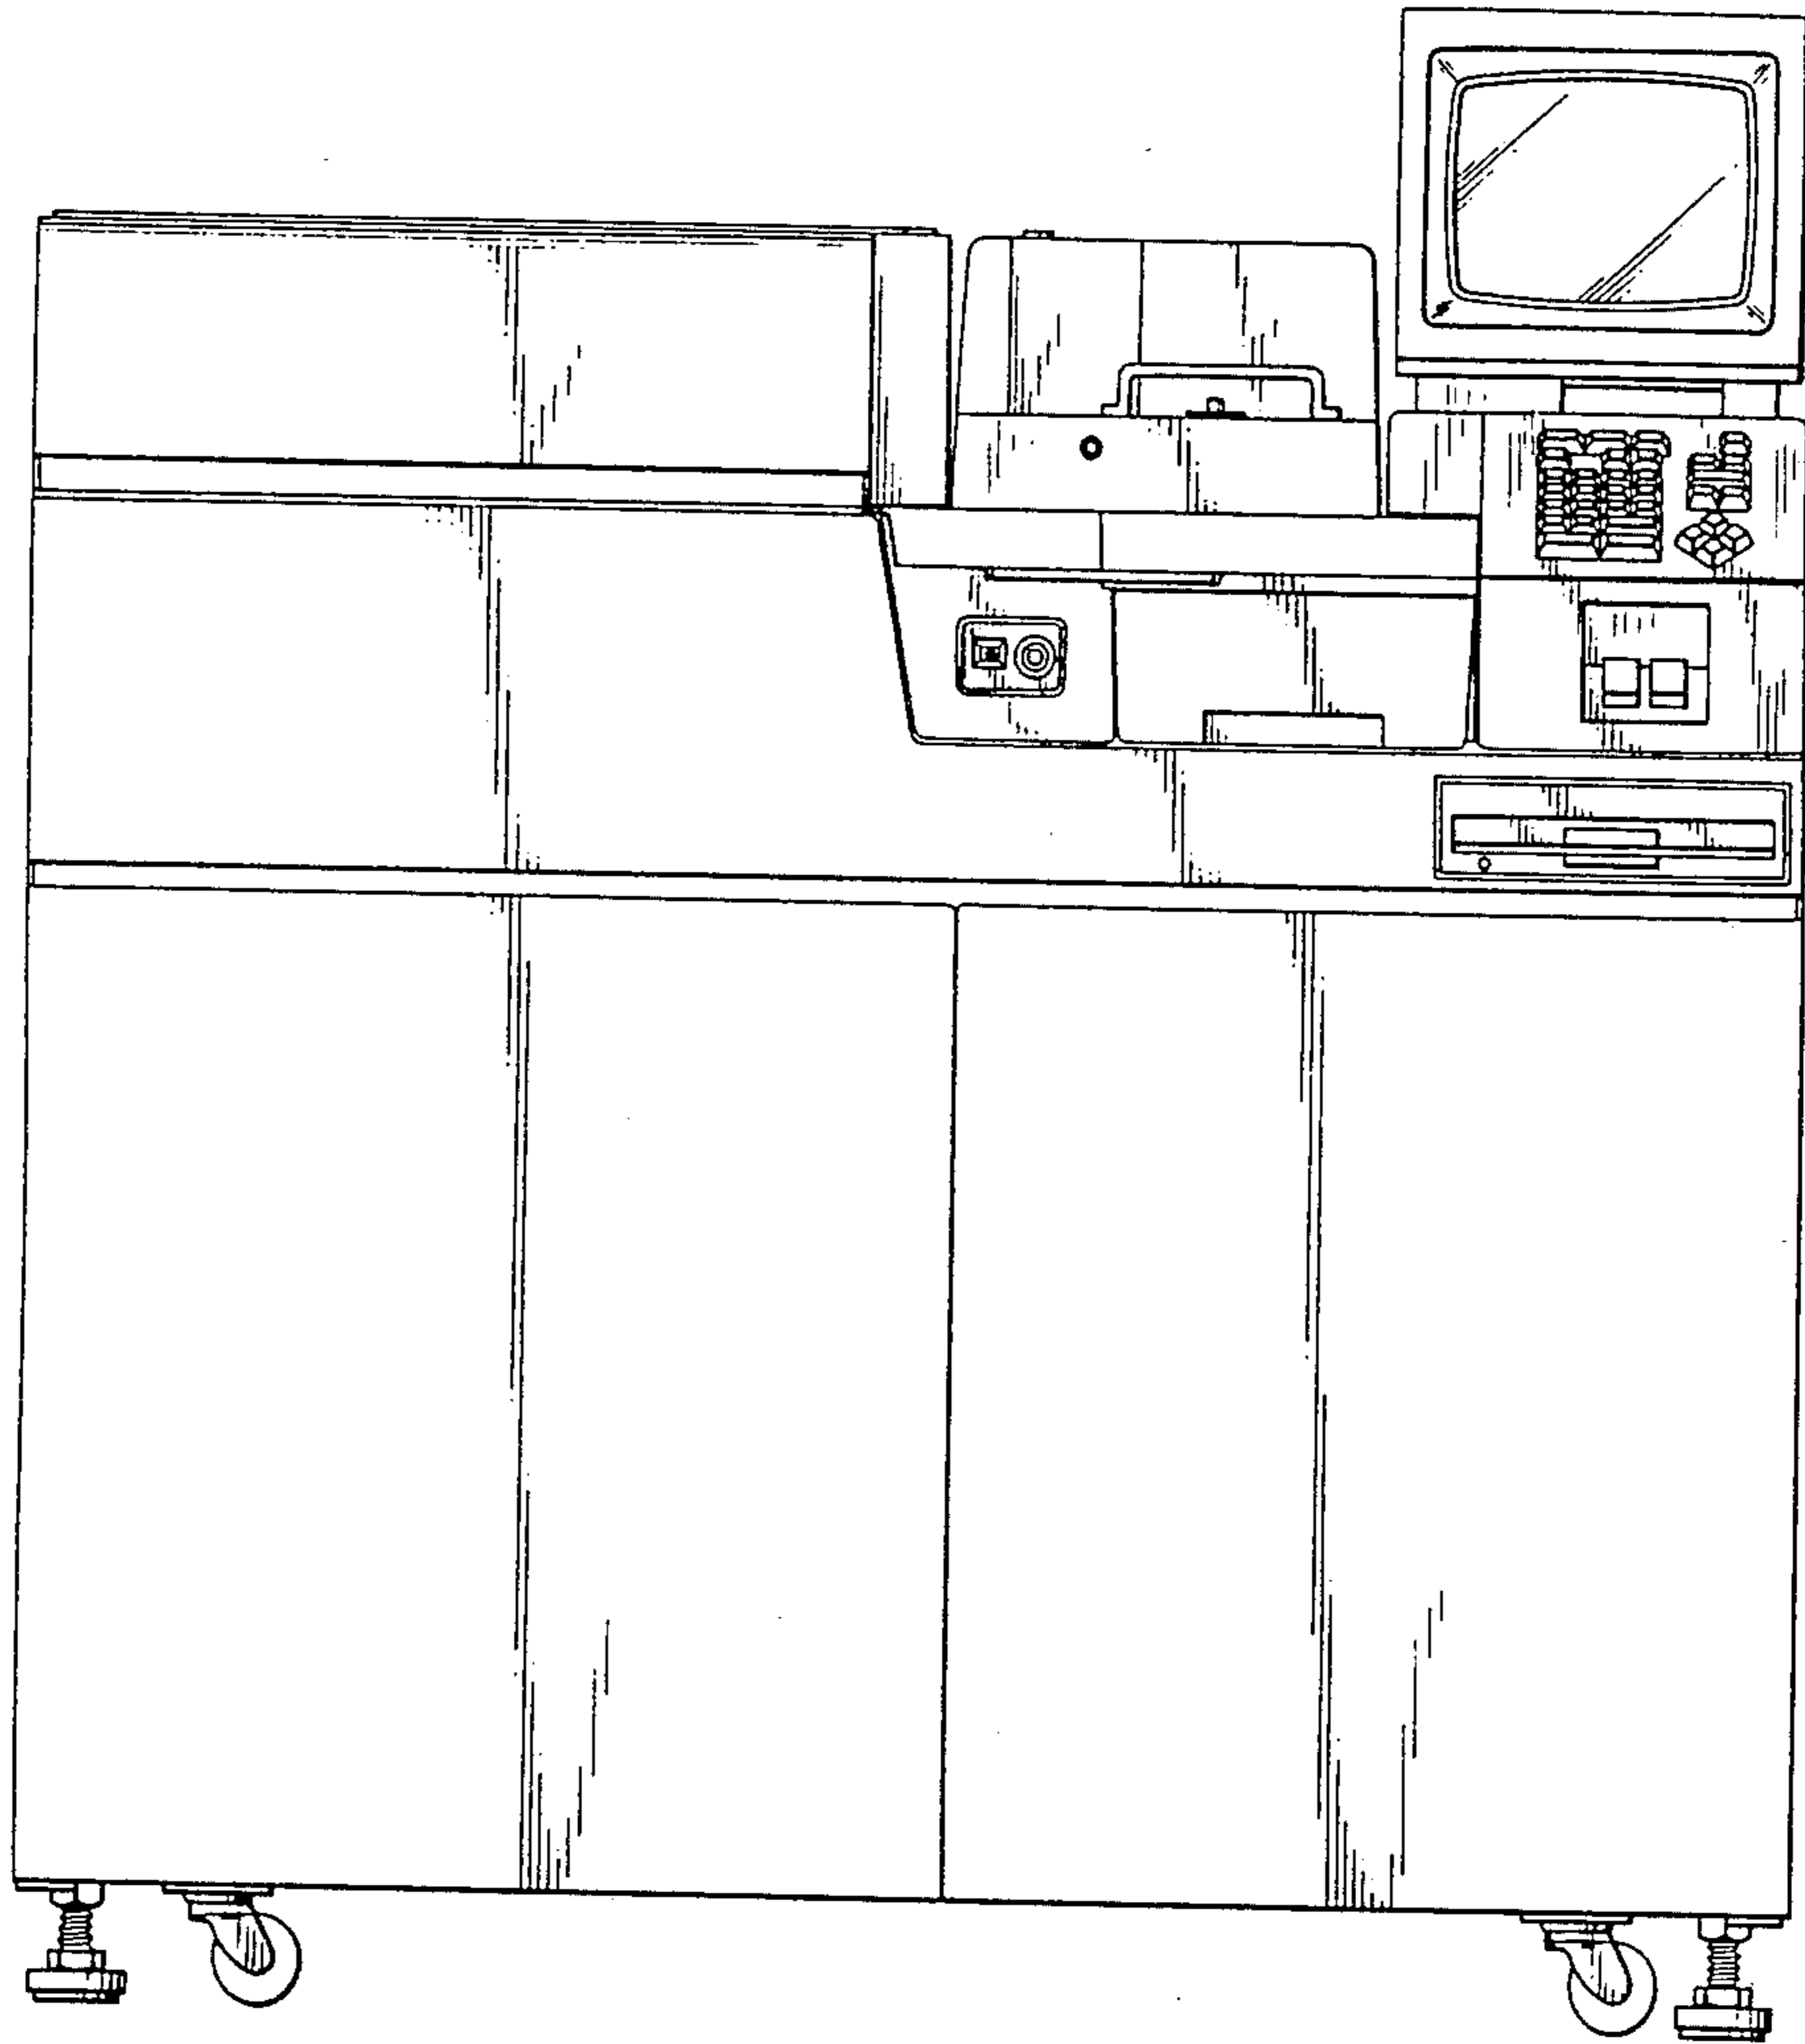


FIG. 4

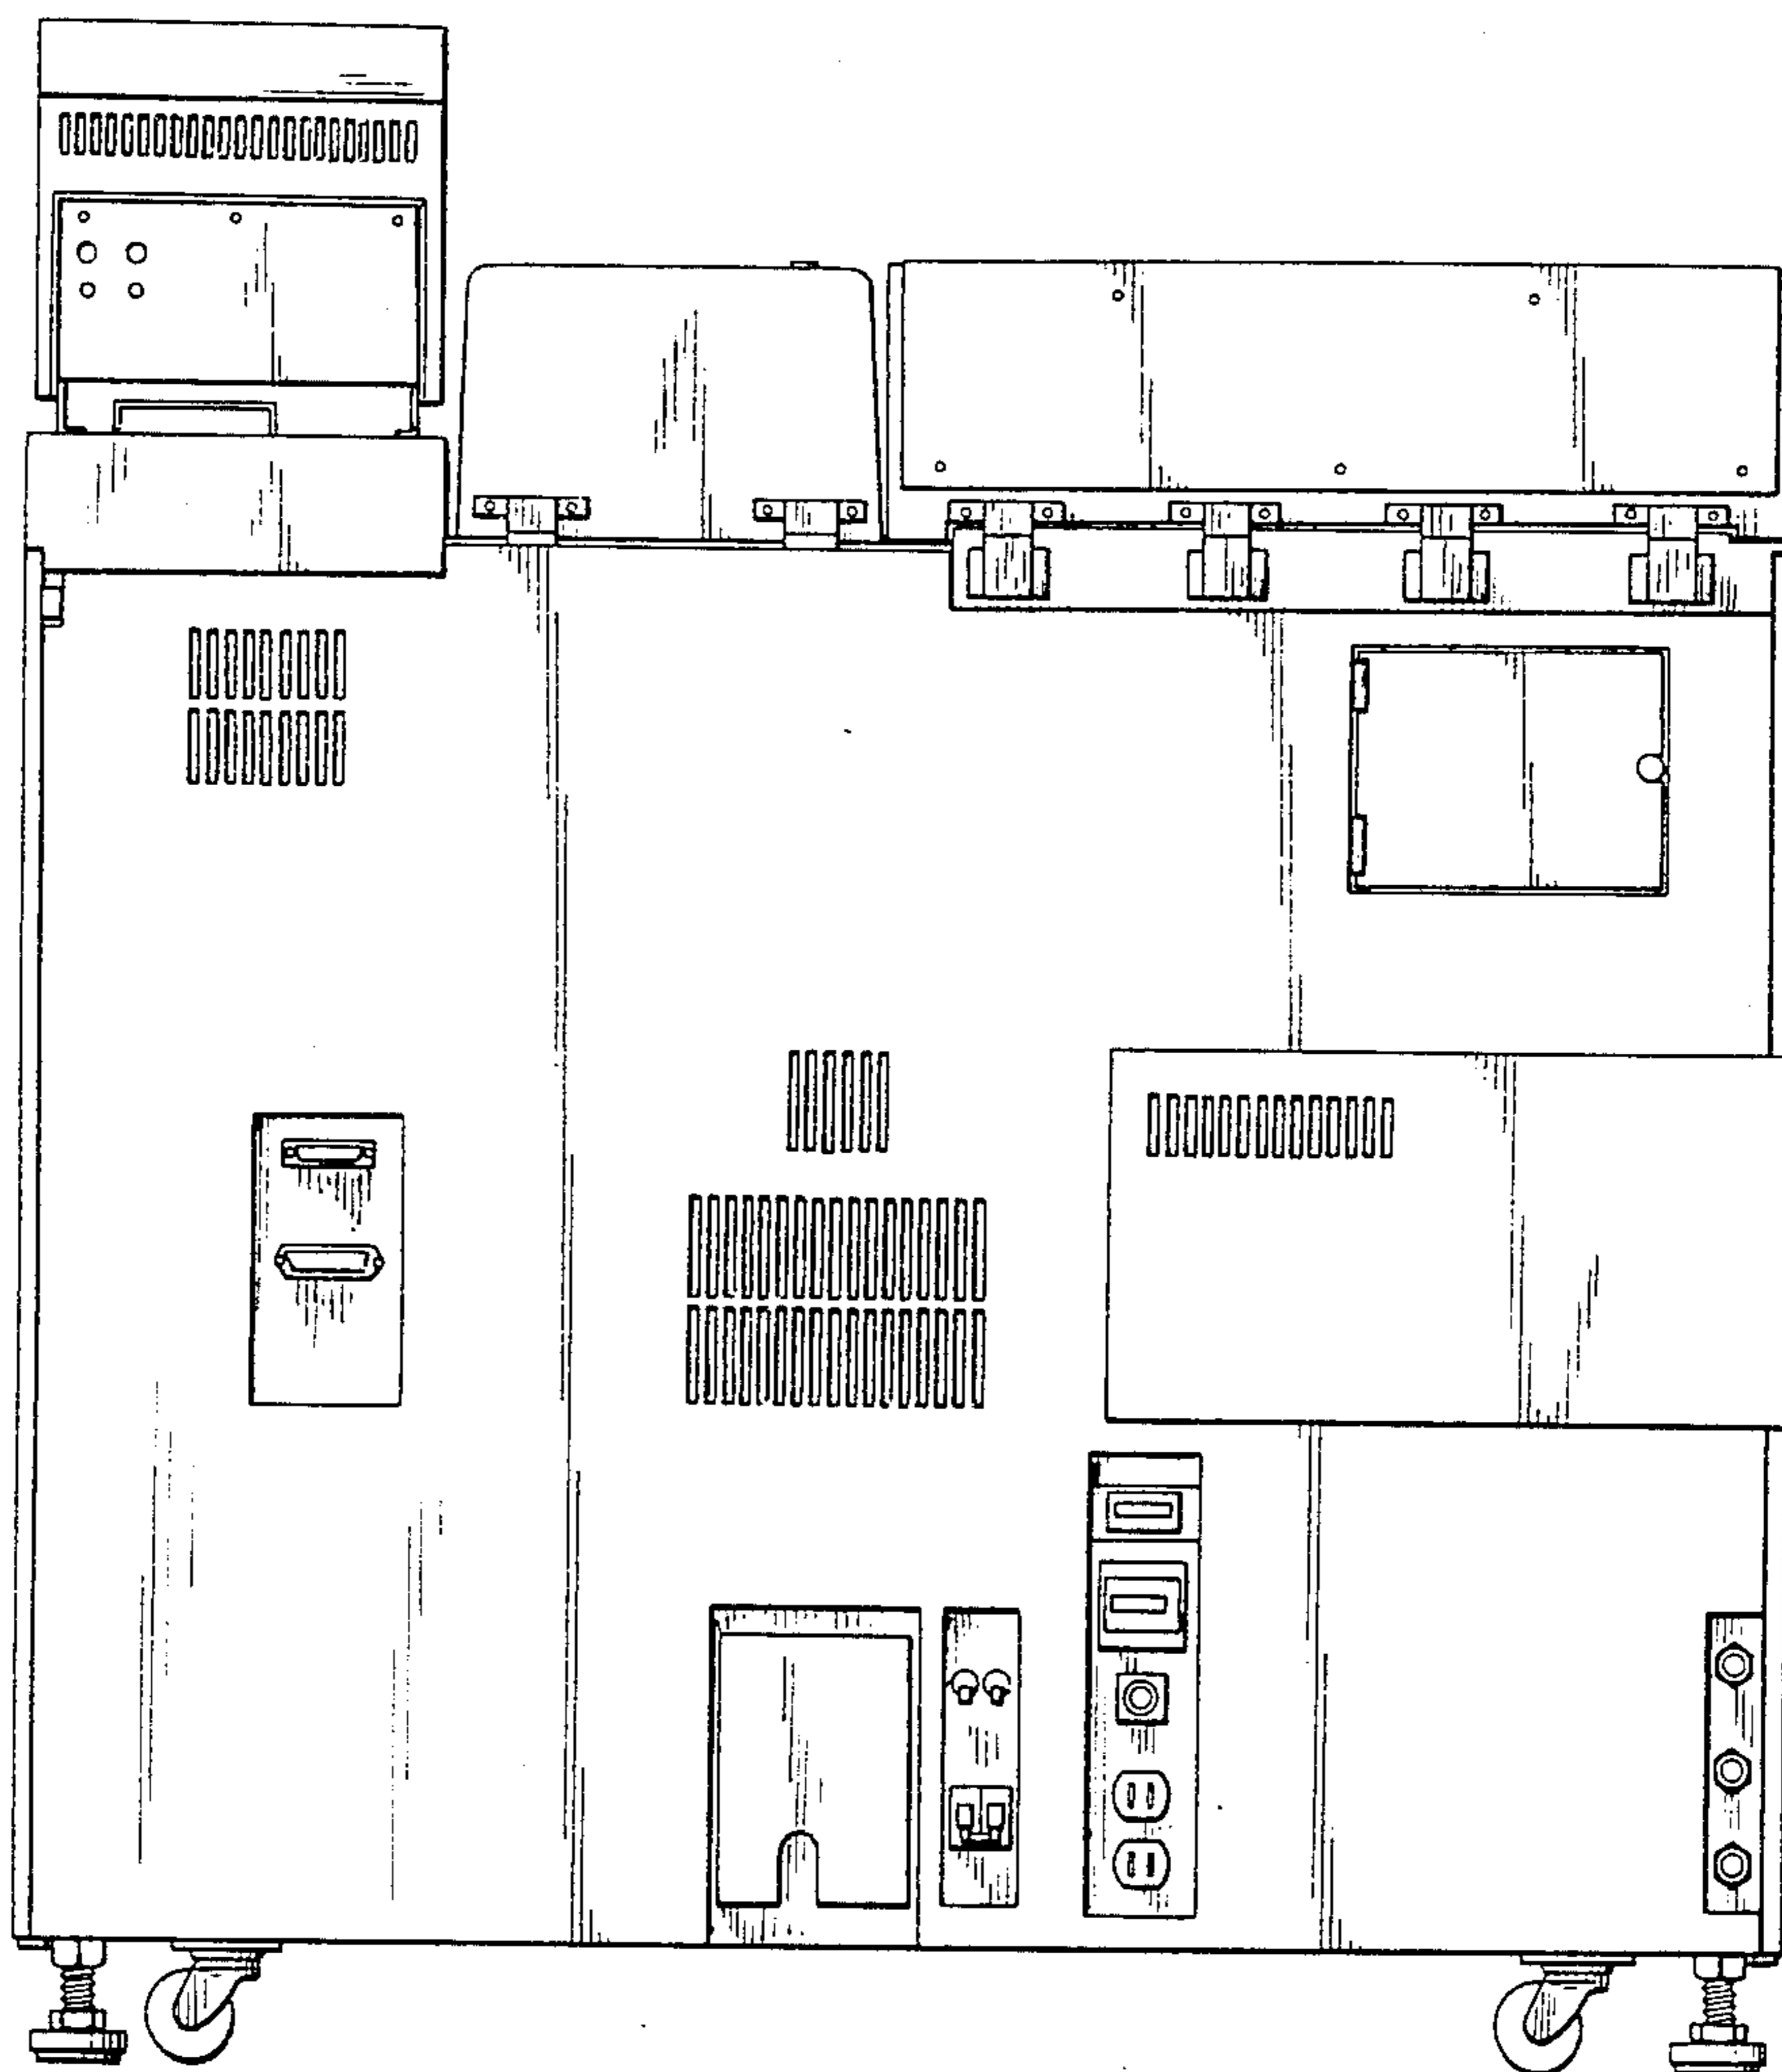


FIG. 5

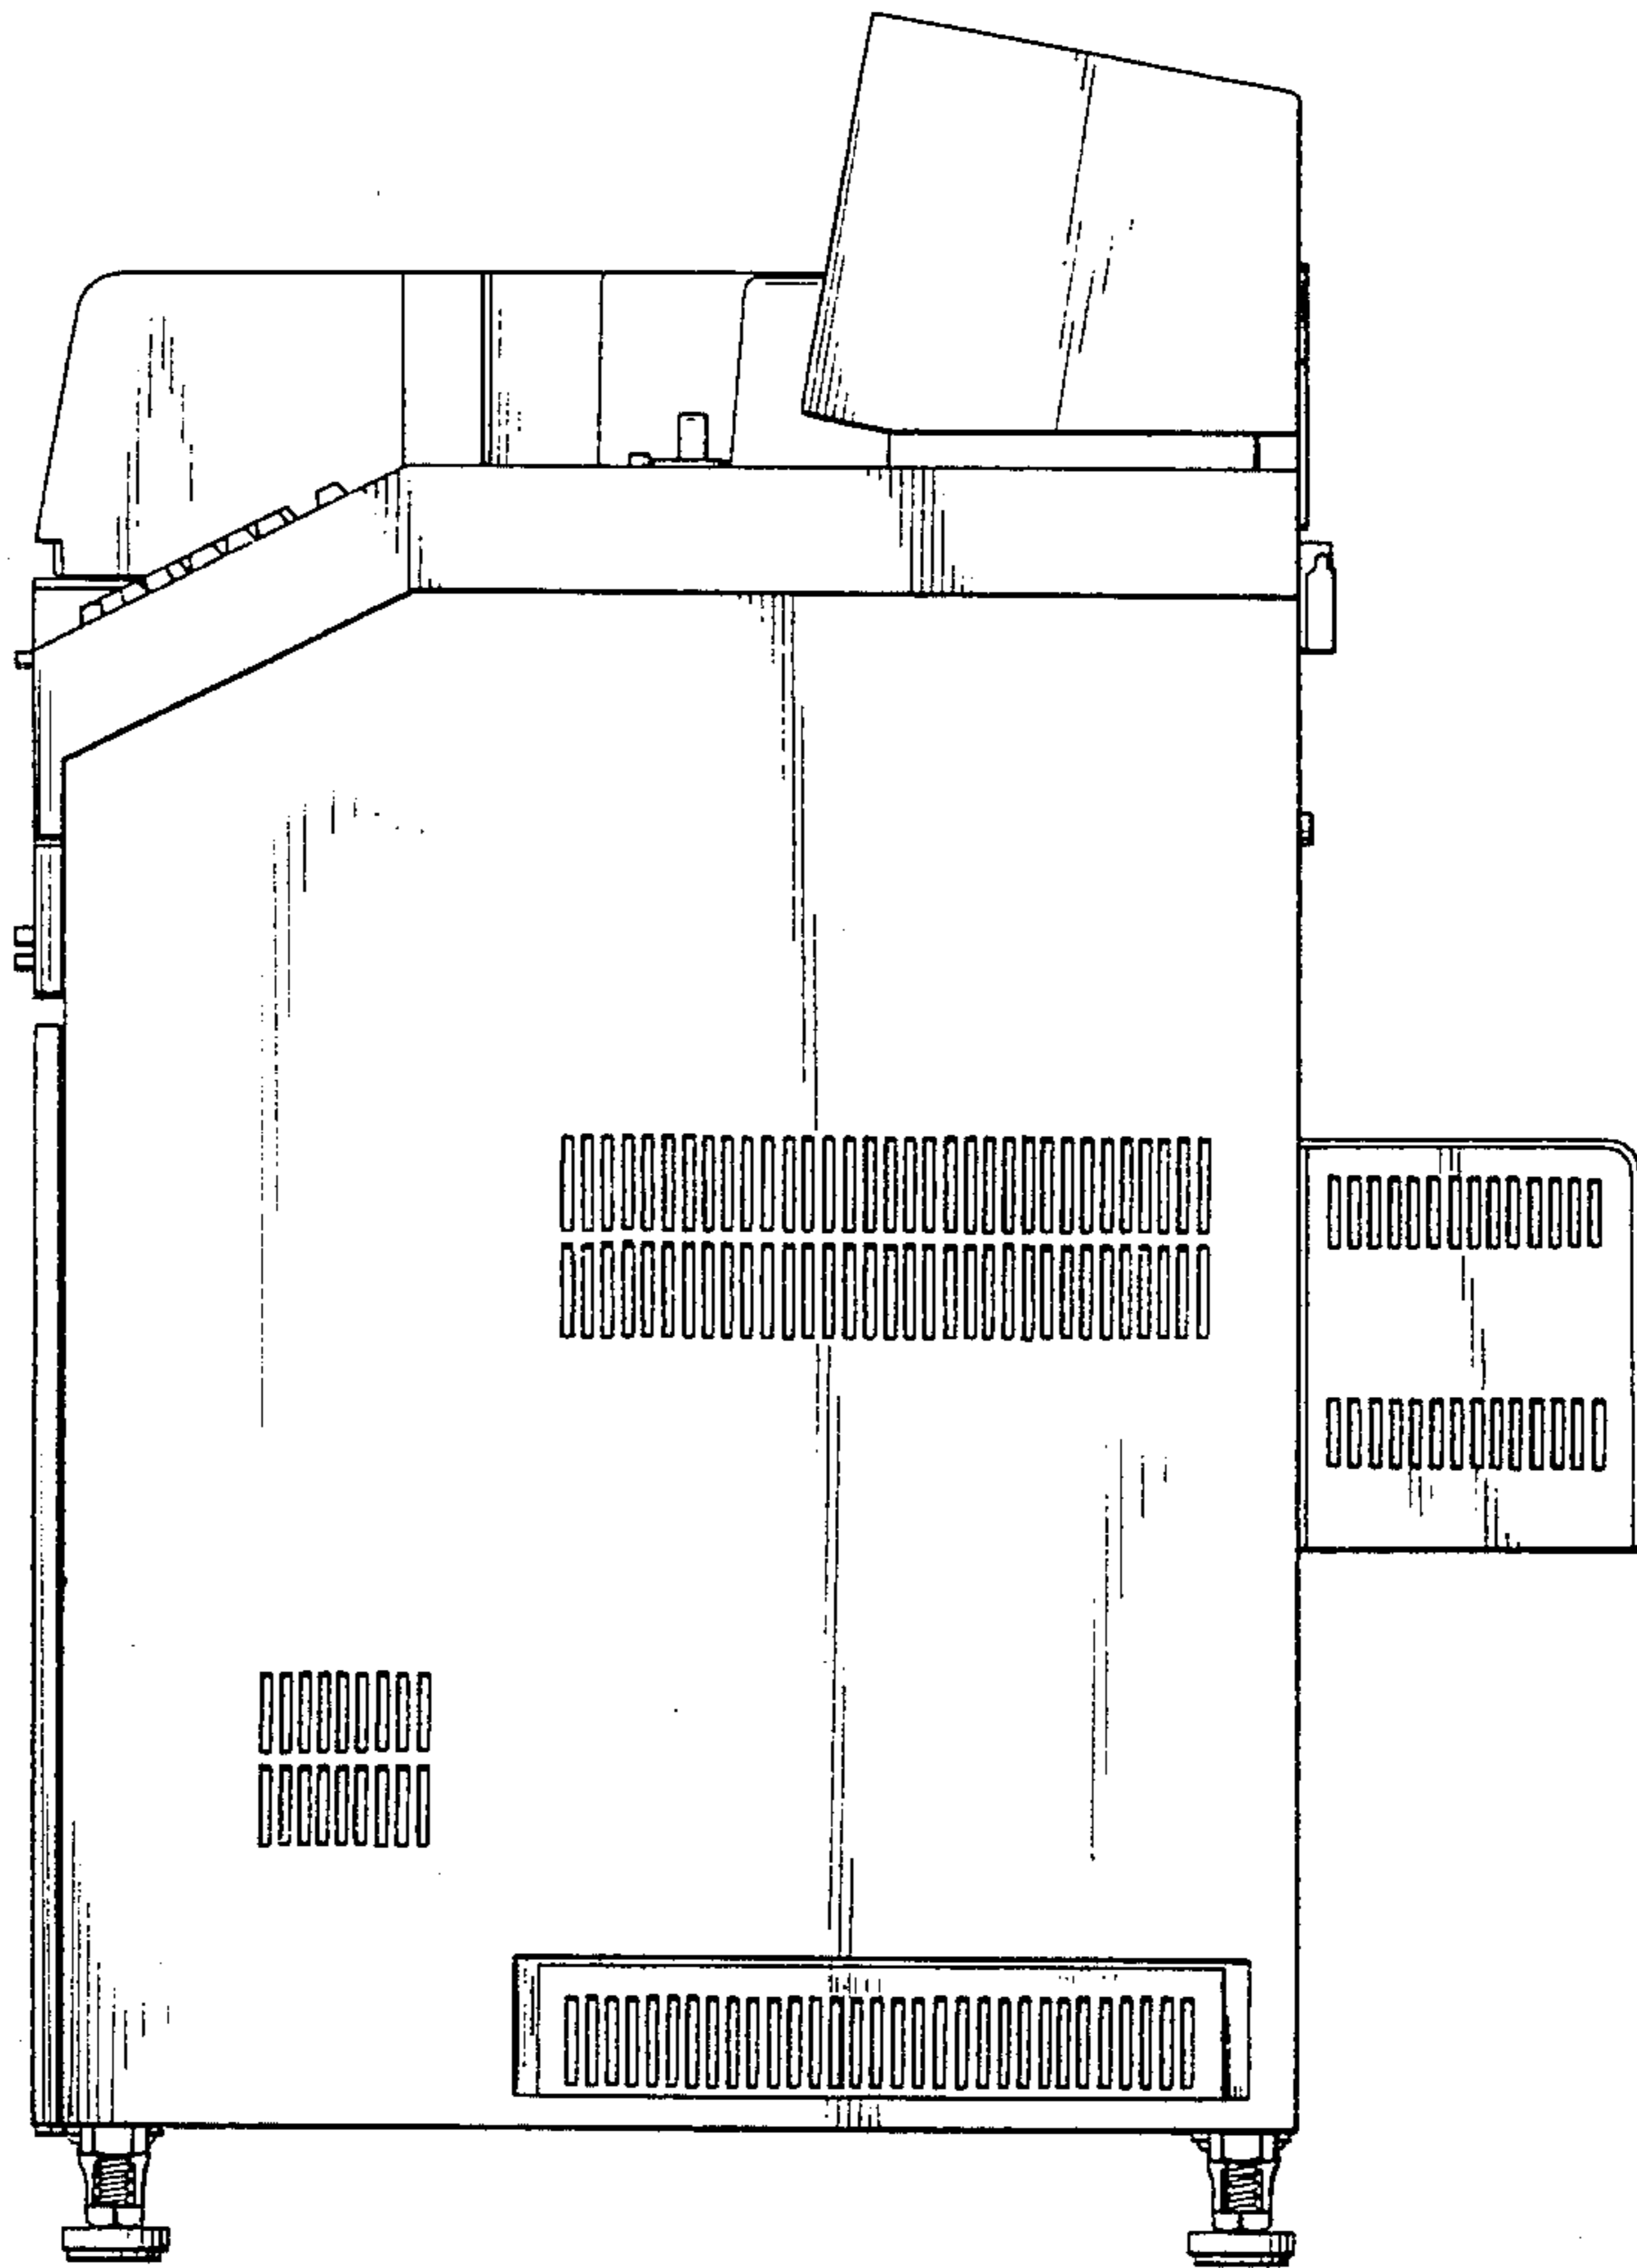


FIG. 6

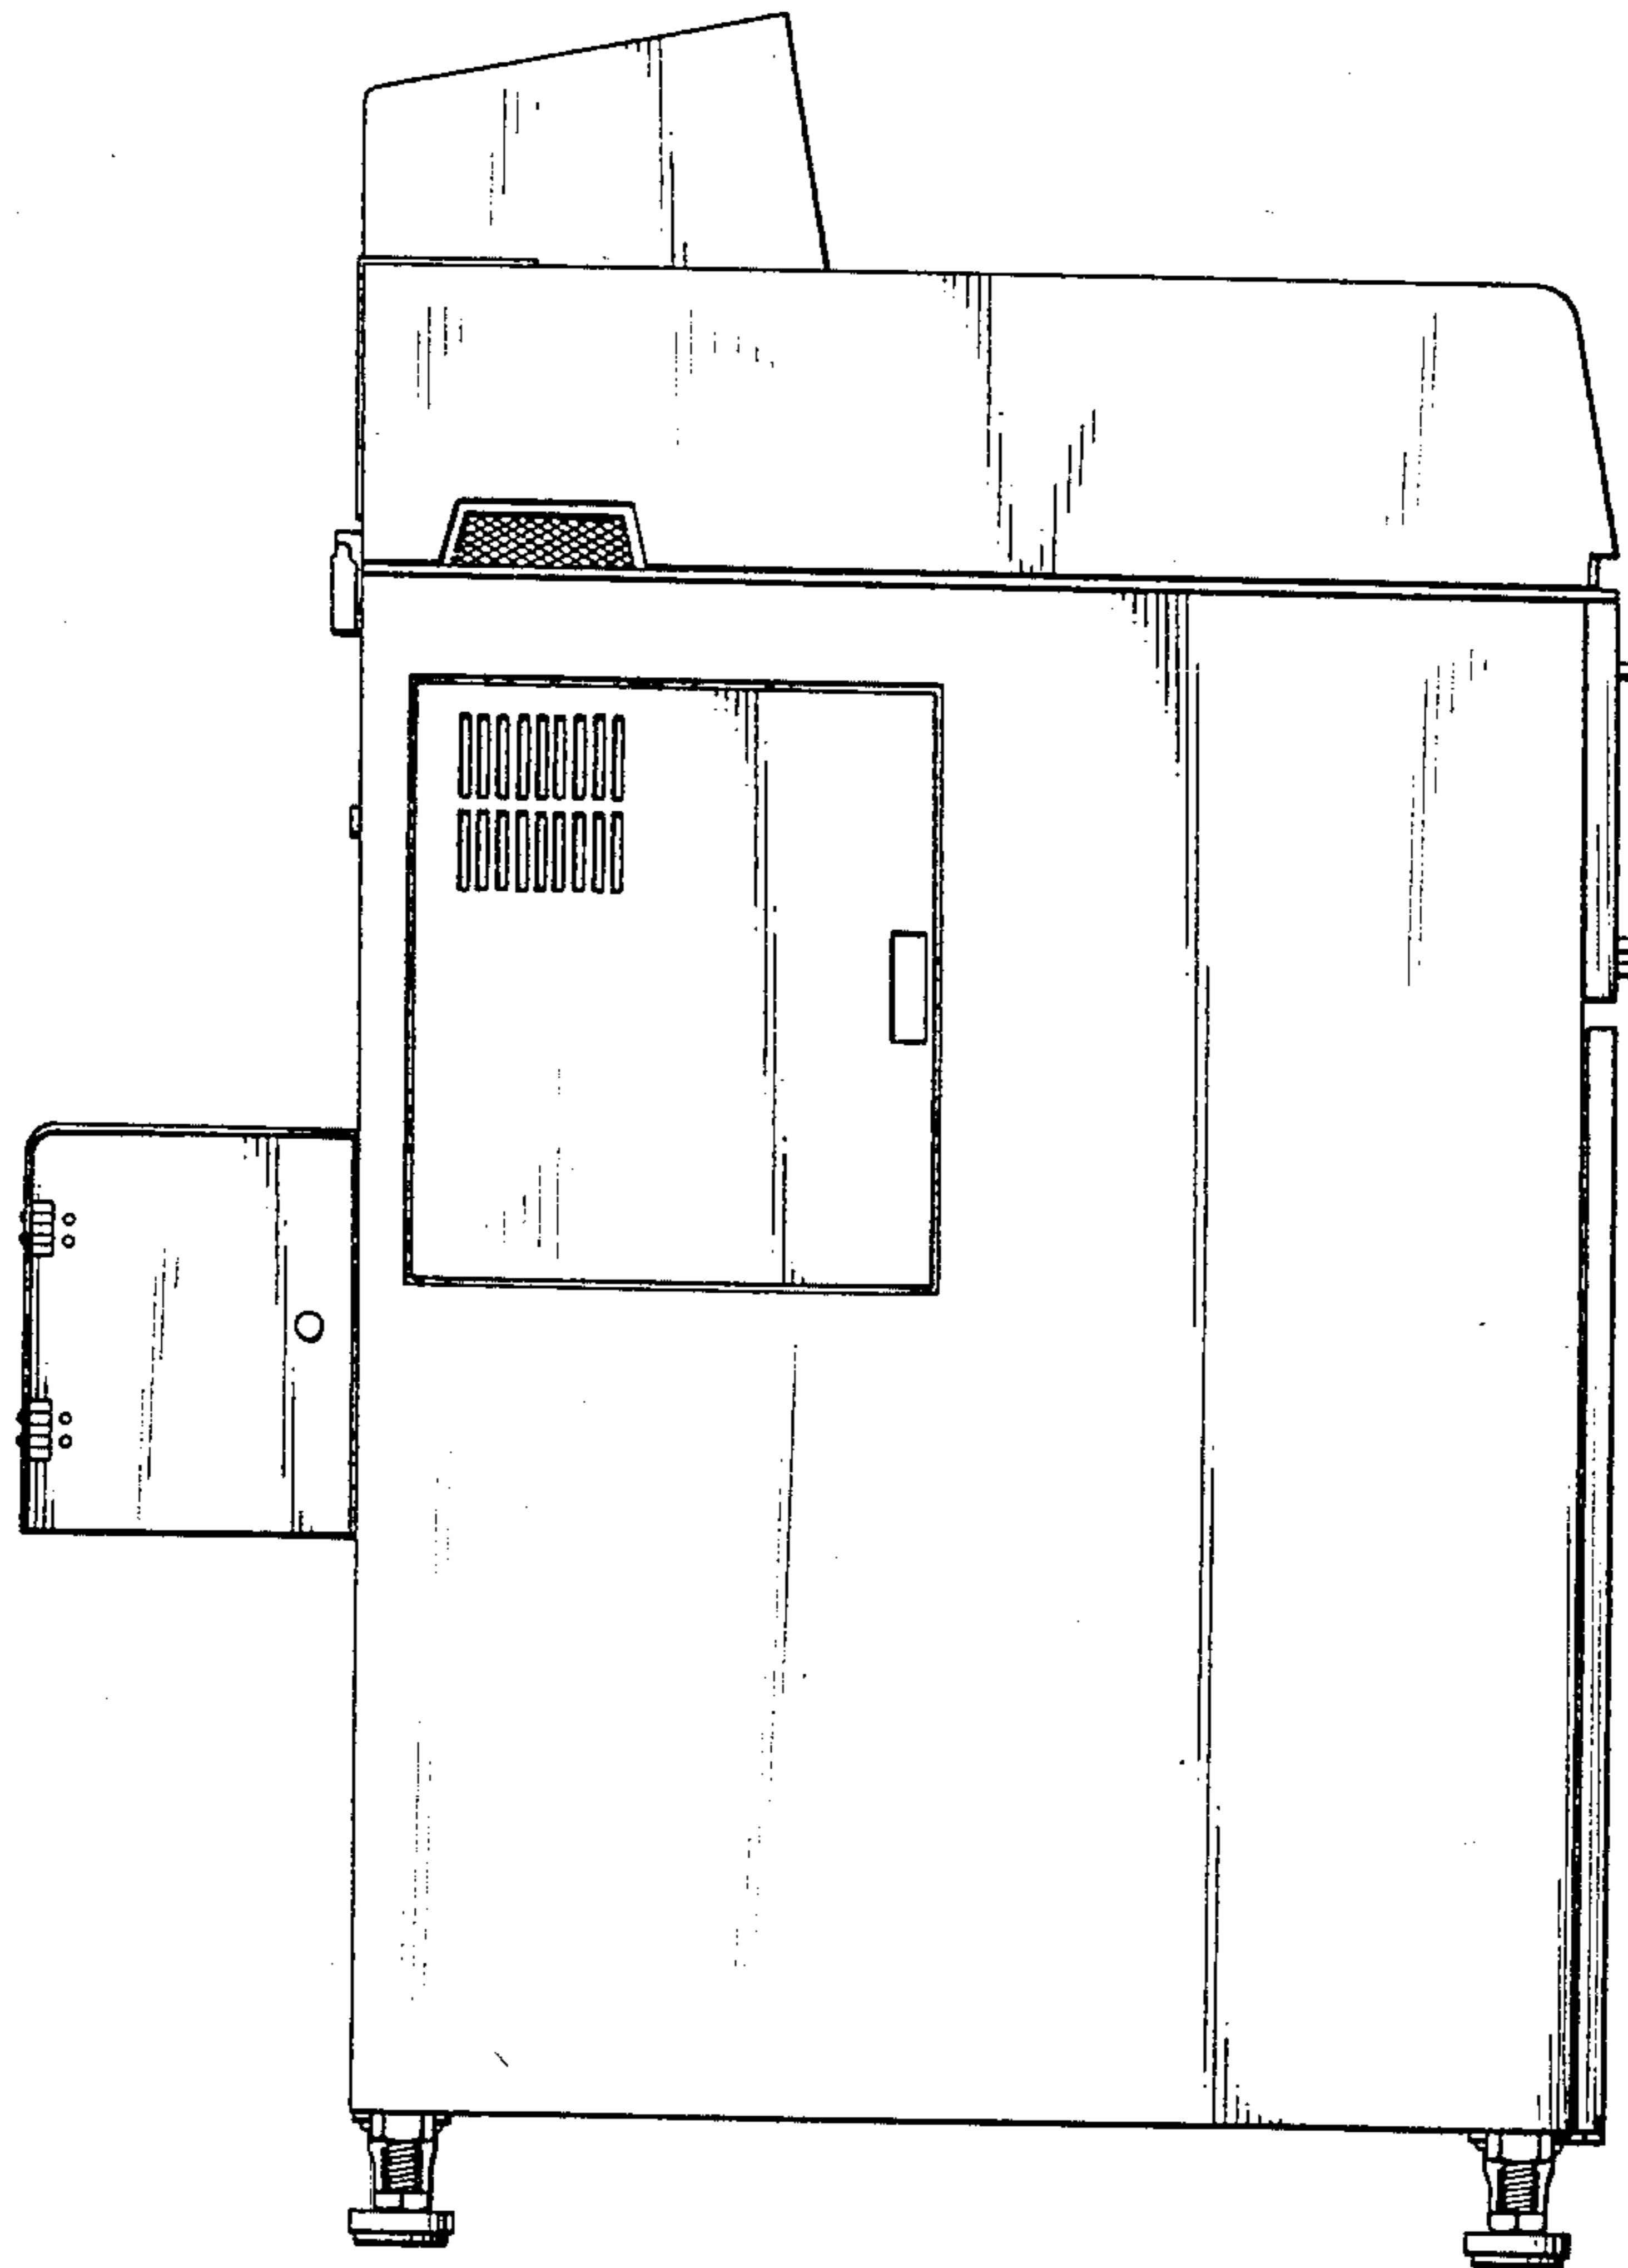


FIG. 7

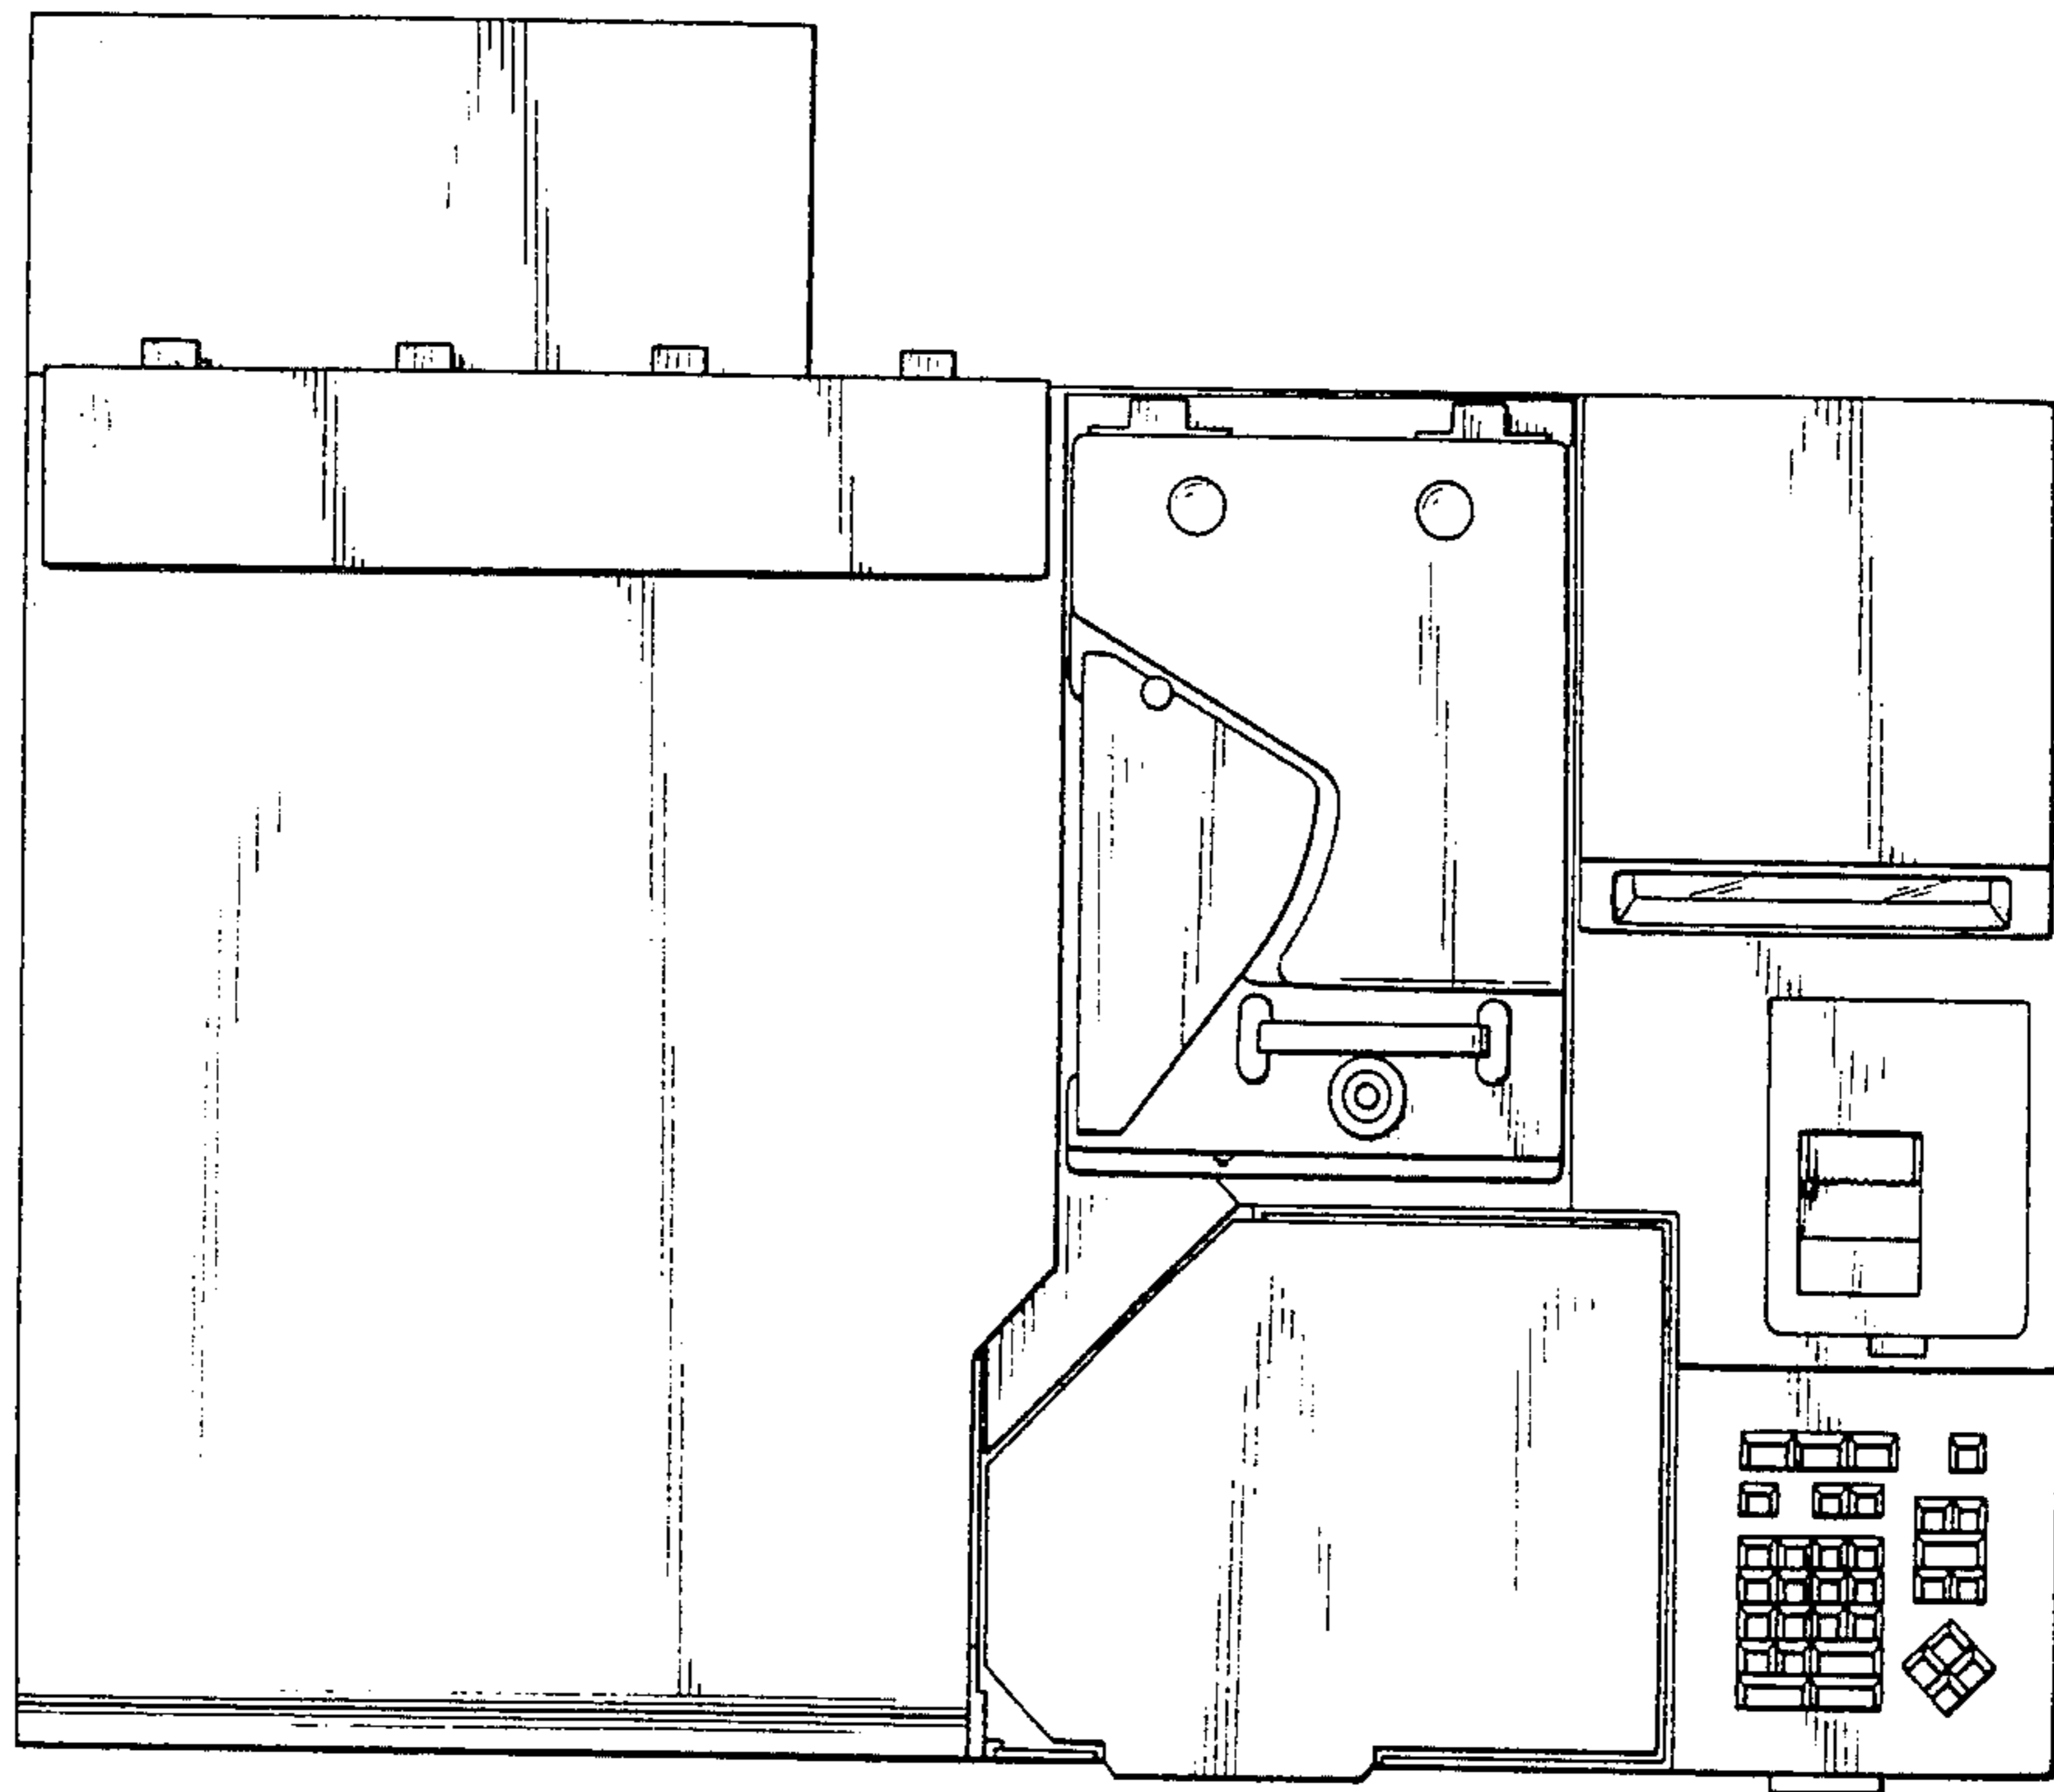


FIG. 8

