

[54] THERMAL INDICATOR FOR VACUUM
STERILIZER TEST PACKS

D. 253,492 11/1979 Augurt D10/57 X
D. 286,622 11/1986 deOliveira D10/57

[75] Inventor: John R. Scoville, Jr., Henrietta, N.Y.

Primary Examiner—Nelson C. Holtje
Attorney, Agent, or Firm—Trask, Britt & Rossa

[73] Assignee: Castle Company, Rochester, N.Y.

[57] CLAIM

[**] Term: 14 Years

The ornamental design for a thermal indicator for vacuum sterilizer test packs, as shown and described.

[21] Appl. No.: 875,354

DESCRIPTION

[22] Filed: Jun. 16, 1986

[52] U.S. Cl. D10/57; D24/99


[58] Field of Search D10/57, 60; D24/99;
116/216, 217, 219; 422/55-60; 374/161, 162

FIG. 1 is a top plan view of a thermal indicator for vacuum sterilizer test packs showing my new design; FIG. 2 is a typical side elevational view thereof; FIG. 3 is an enlarged cross-sectional view thereof as taken from line 3—3 of FIG. 1; FIG. 4 is a top plan view thereof after exposure in a vacuum sterilizer; FIG. 5 is another embodiment of my new design of FIGS. 1-4.

[56] References Cited

U.S. PATENT DOCUMENTS

D. 222,516 10/1971 Kelson D24/99
D. 235,279 6/1975 Schuman D24/99

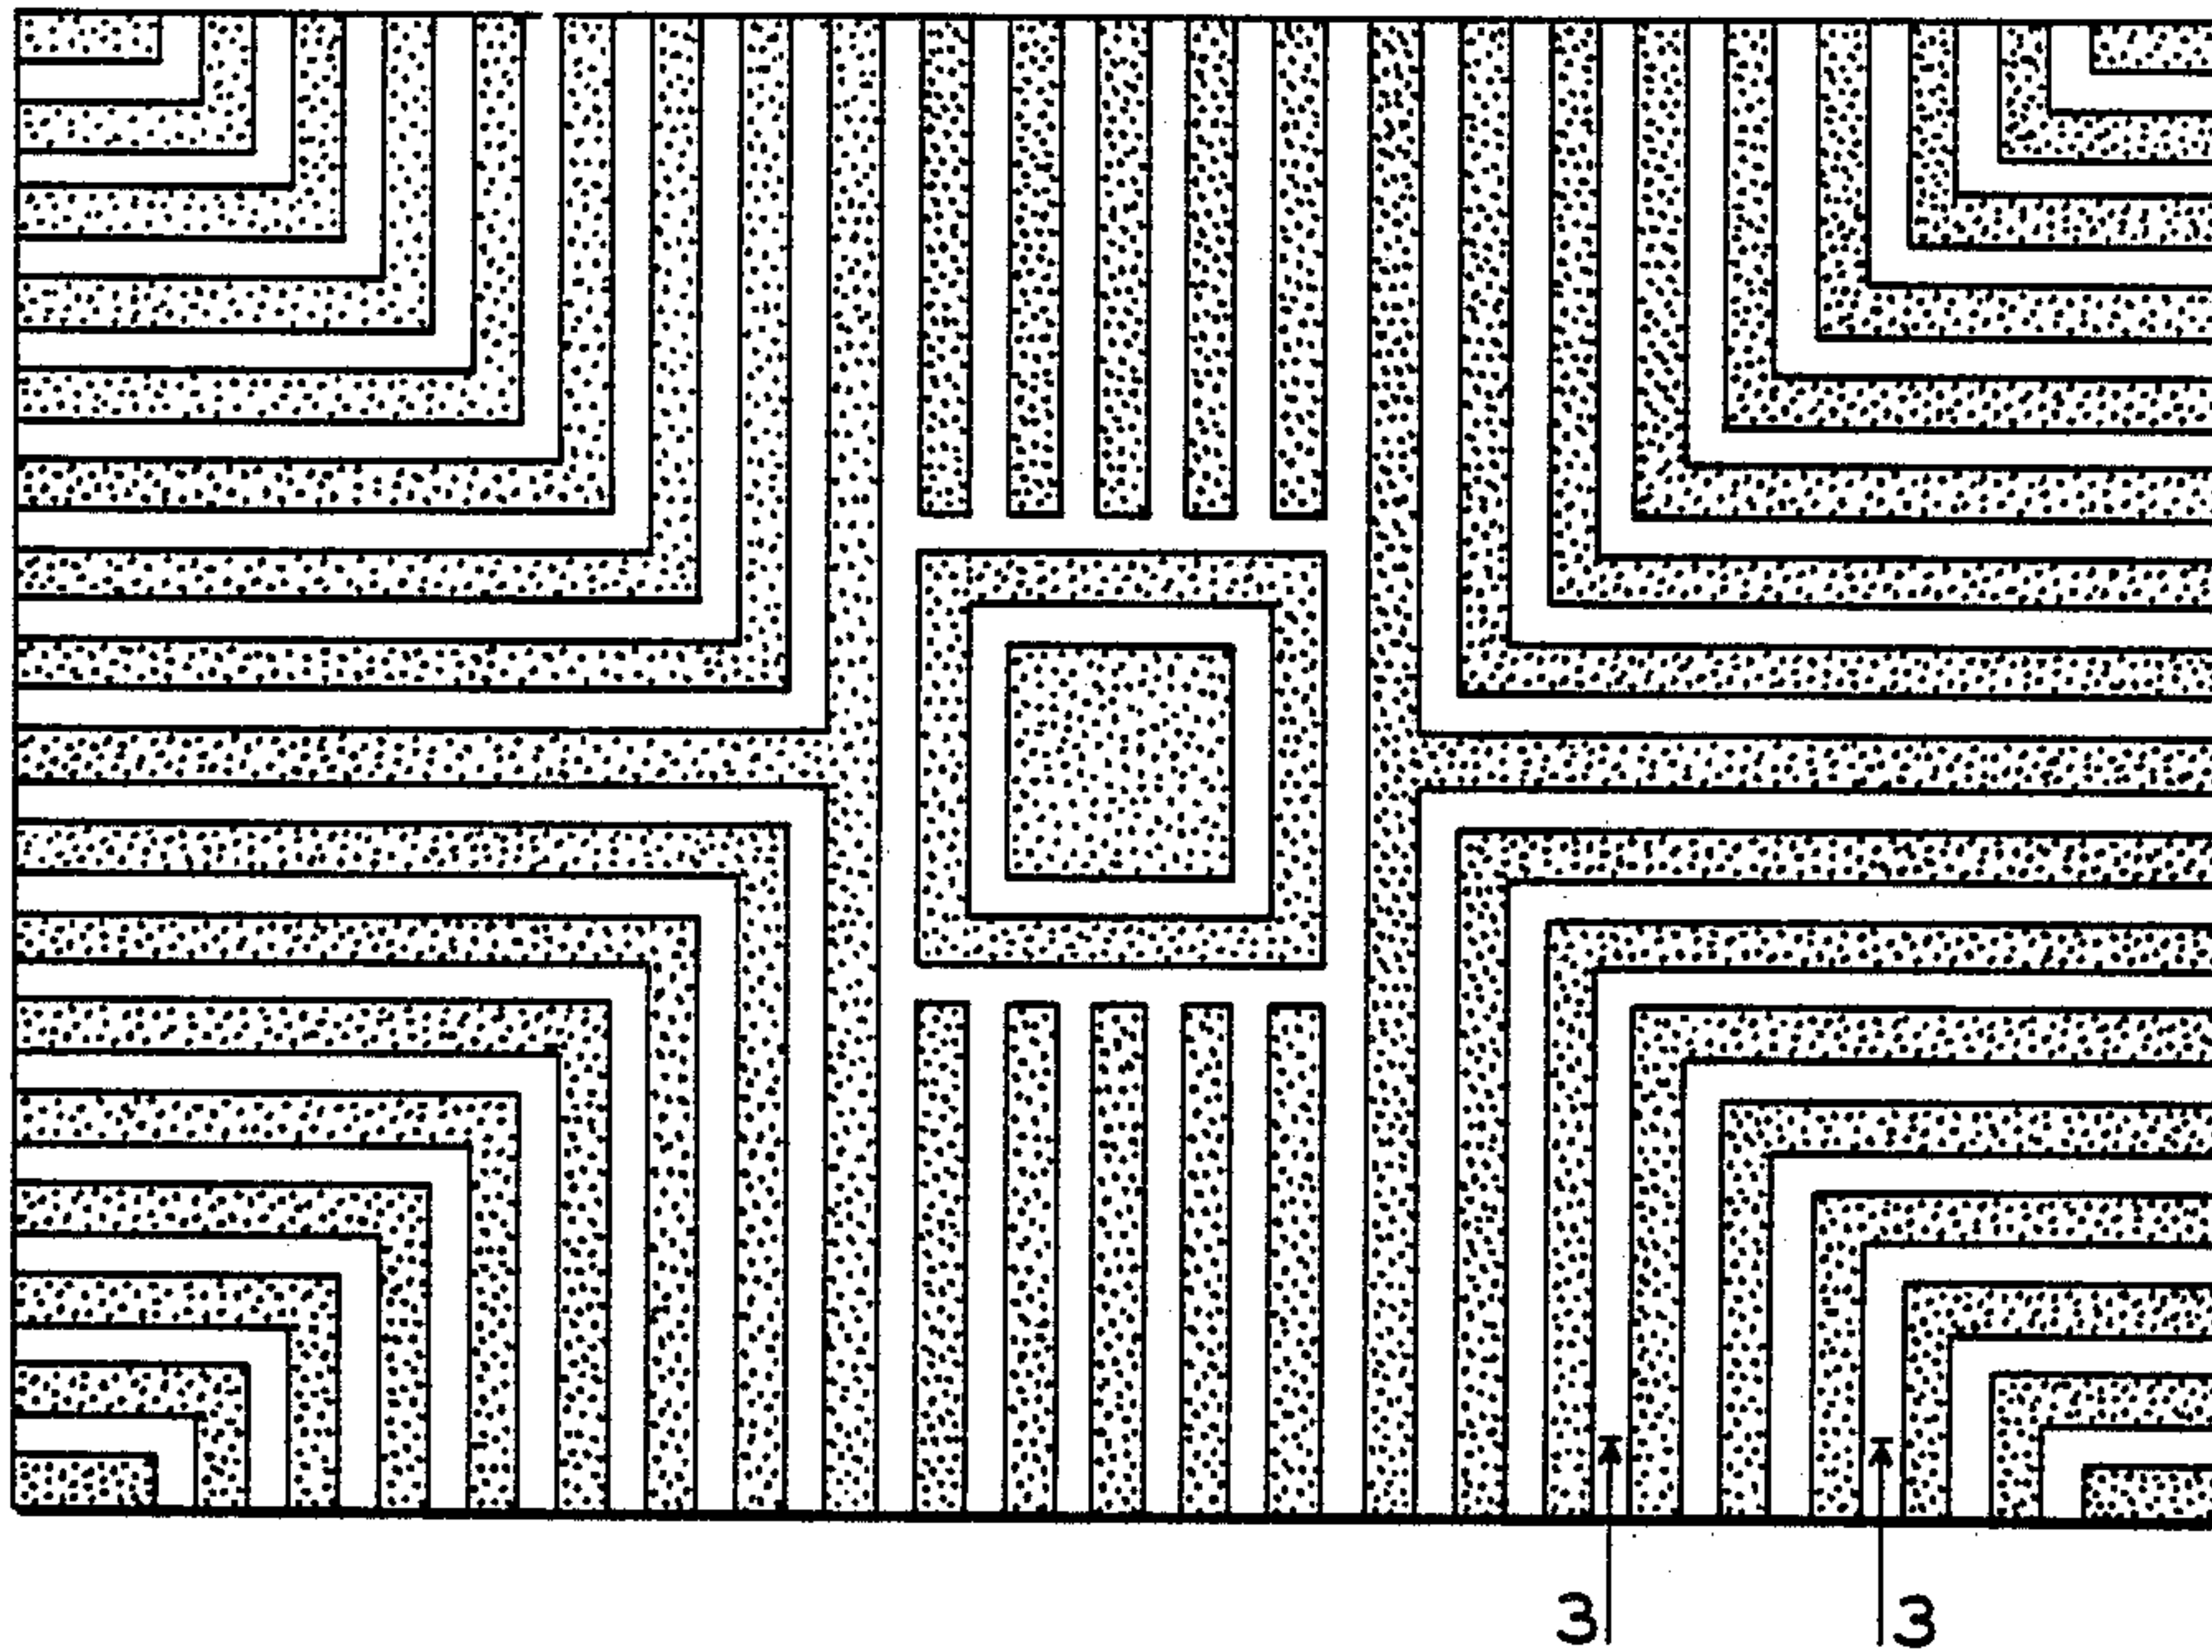

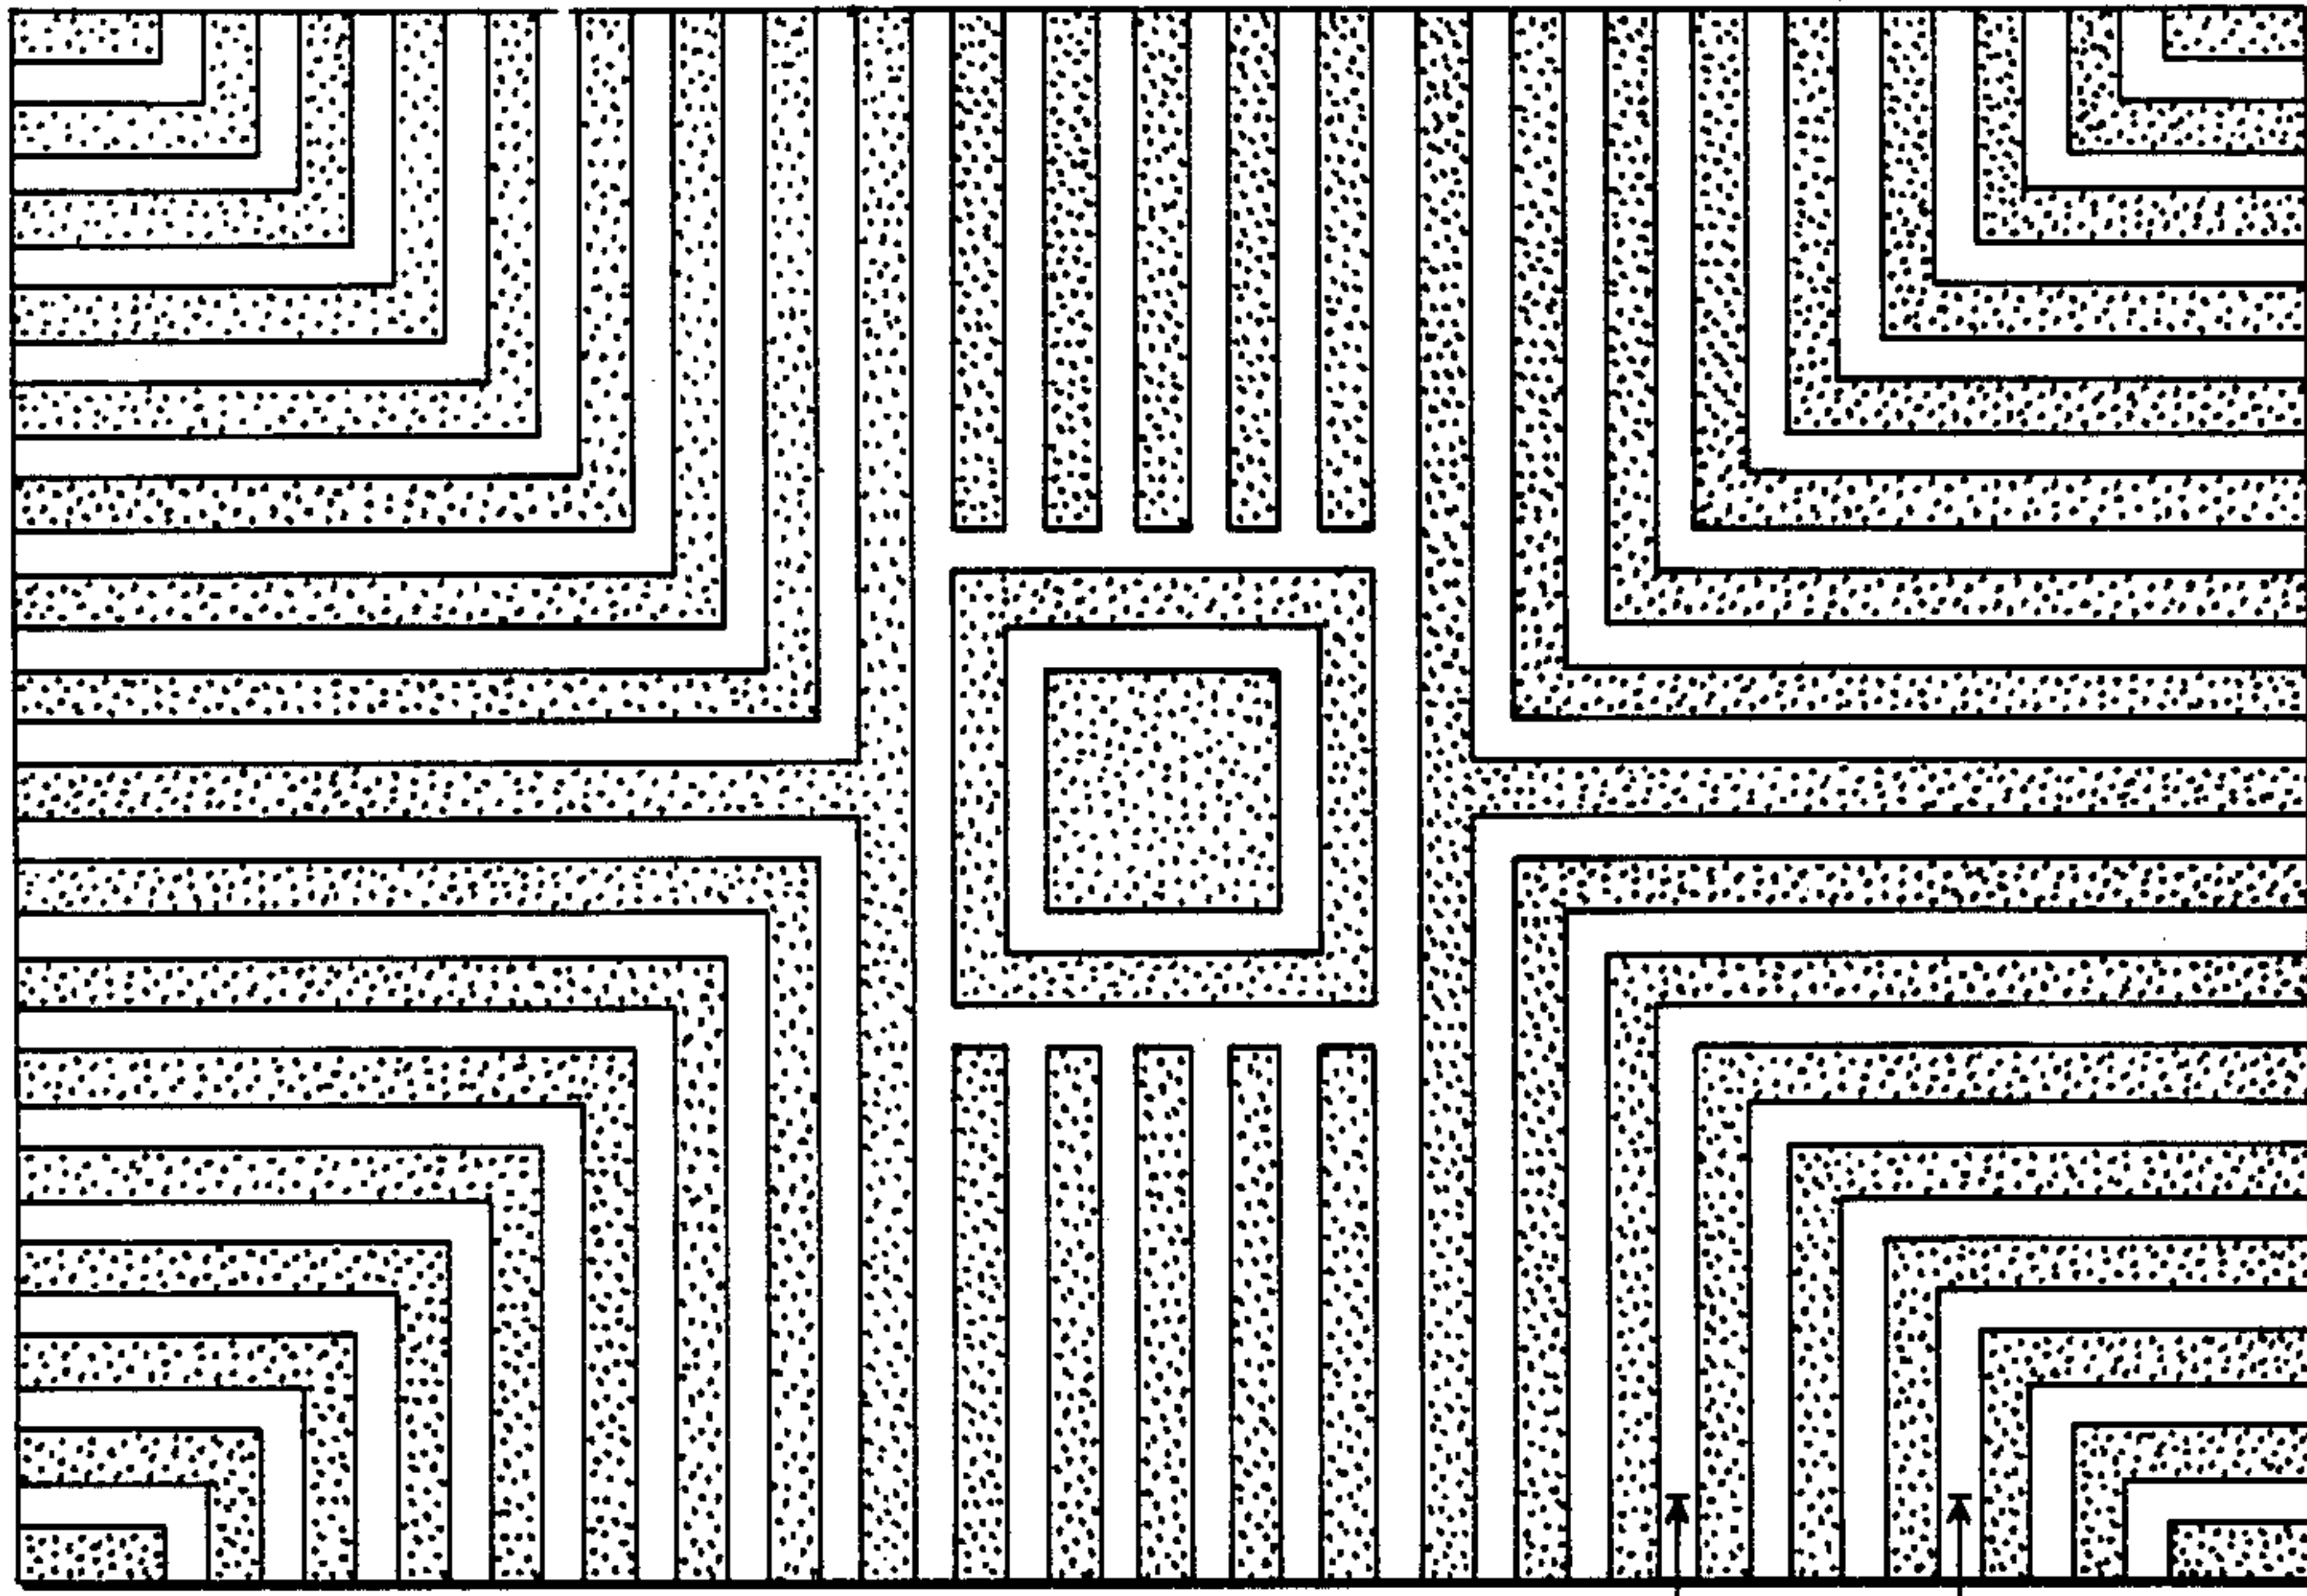


FIG. 1

3

3



FIG. 2



FIG. 3

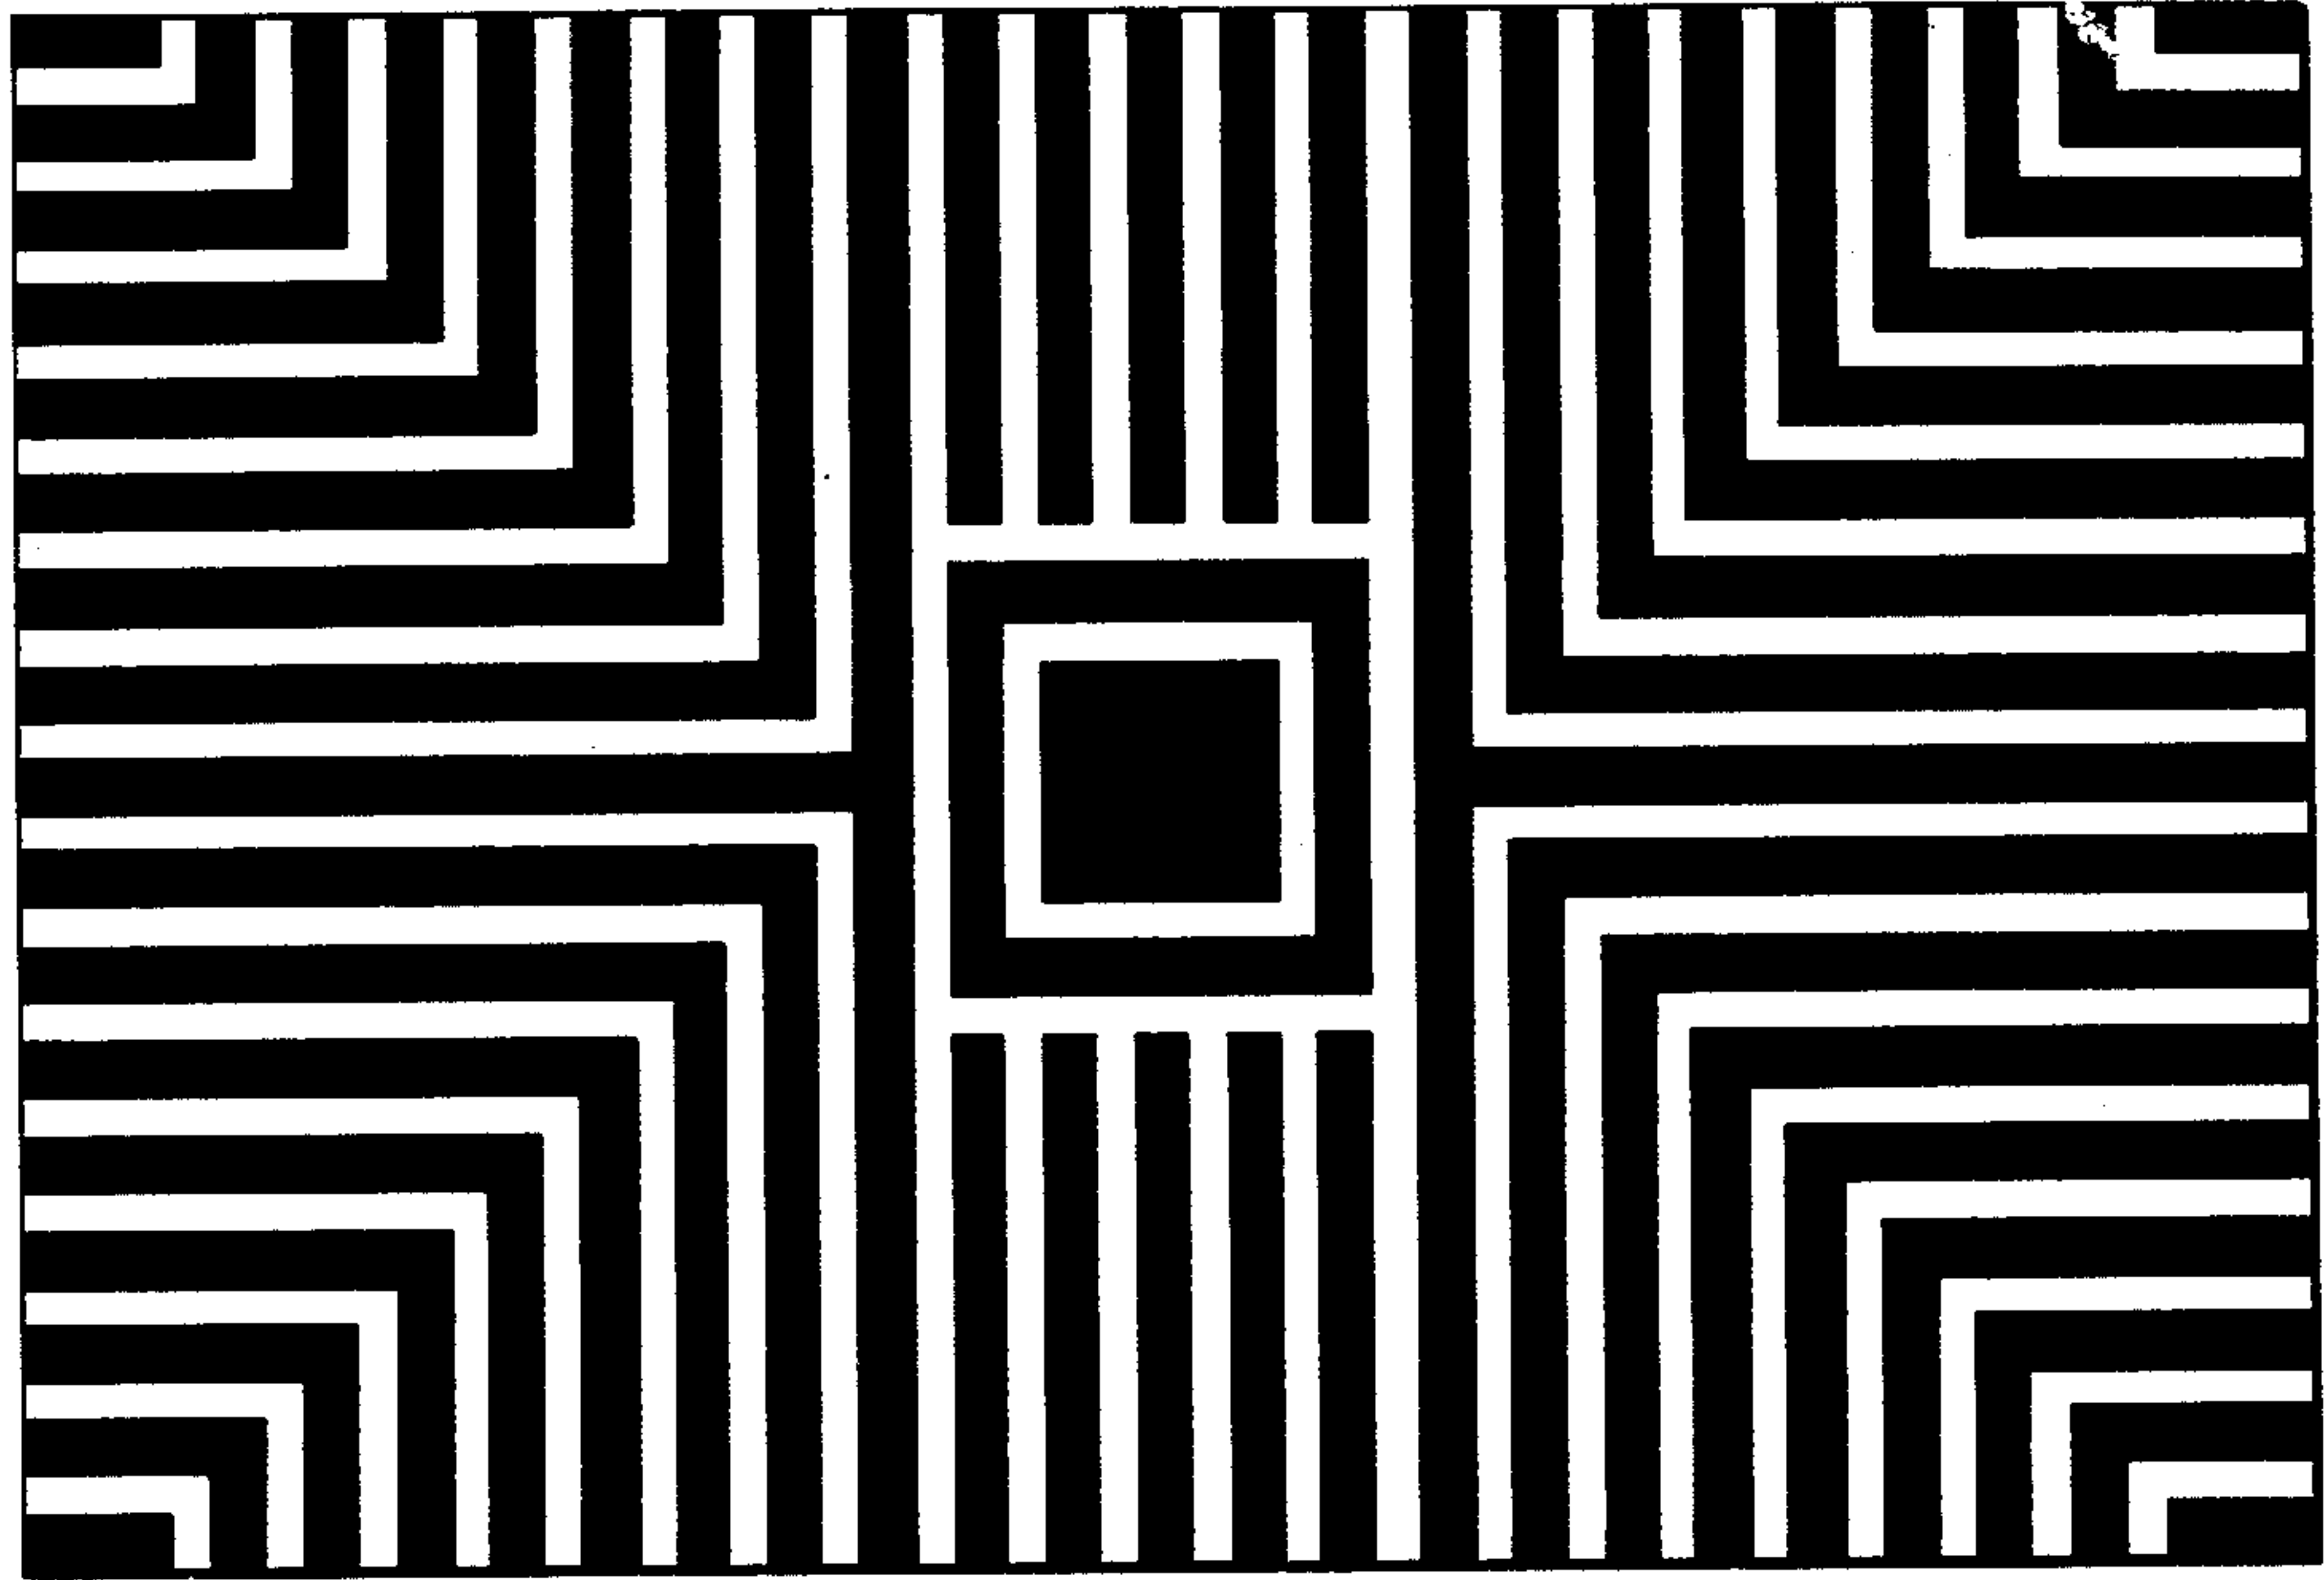


FIG. 4

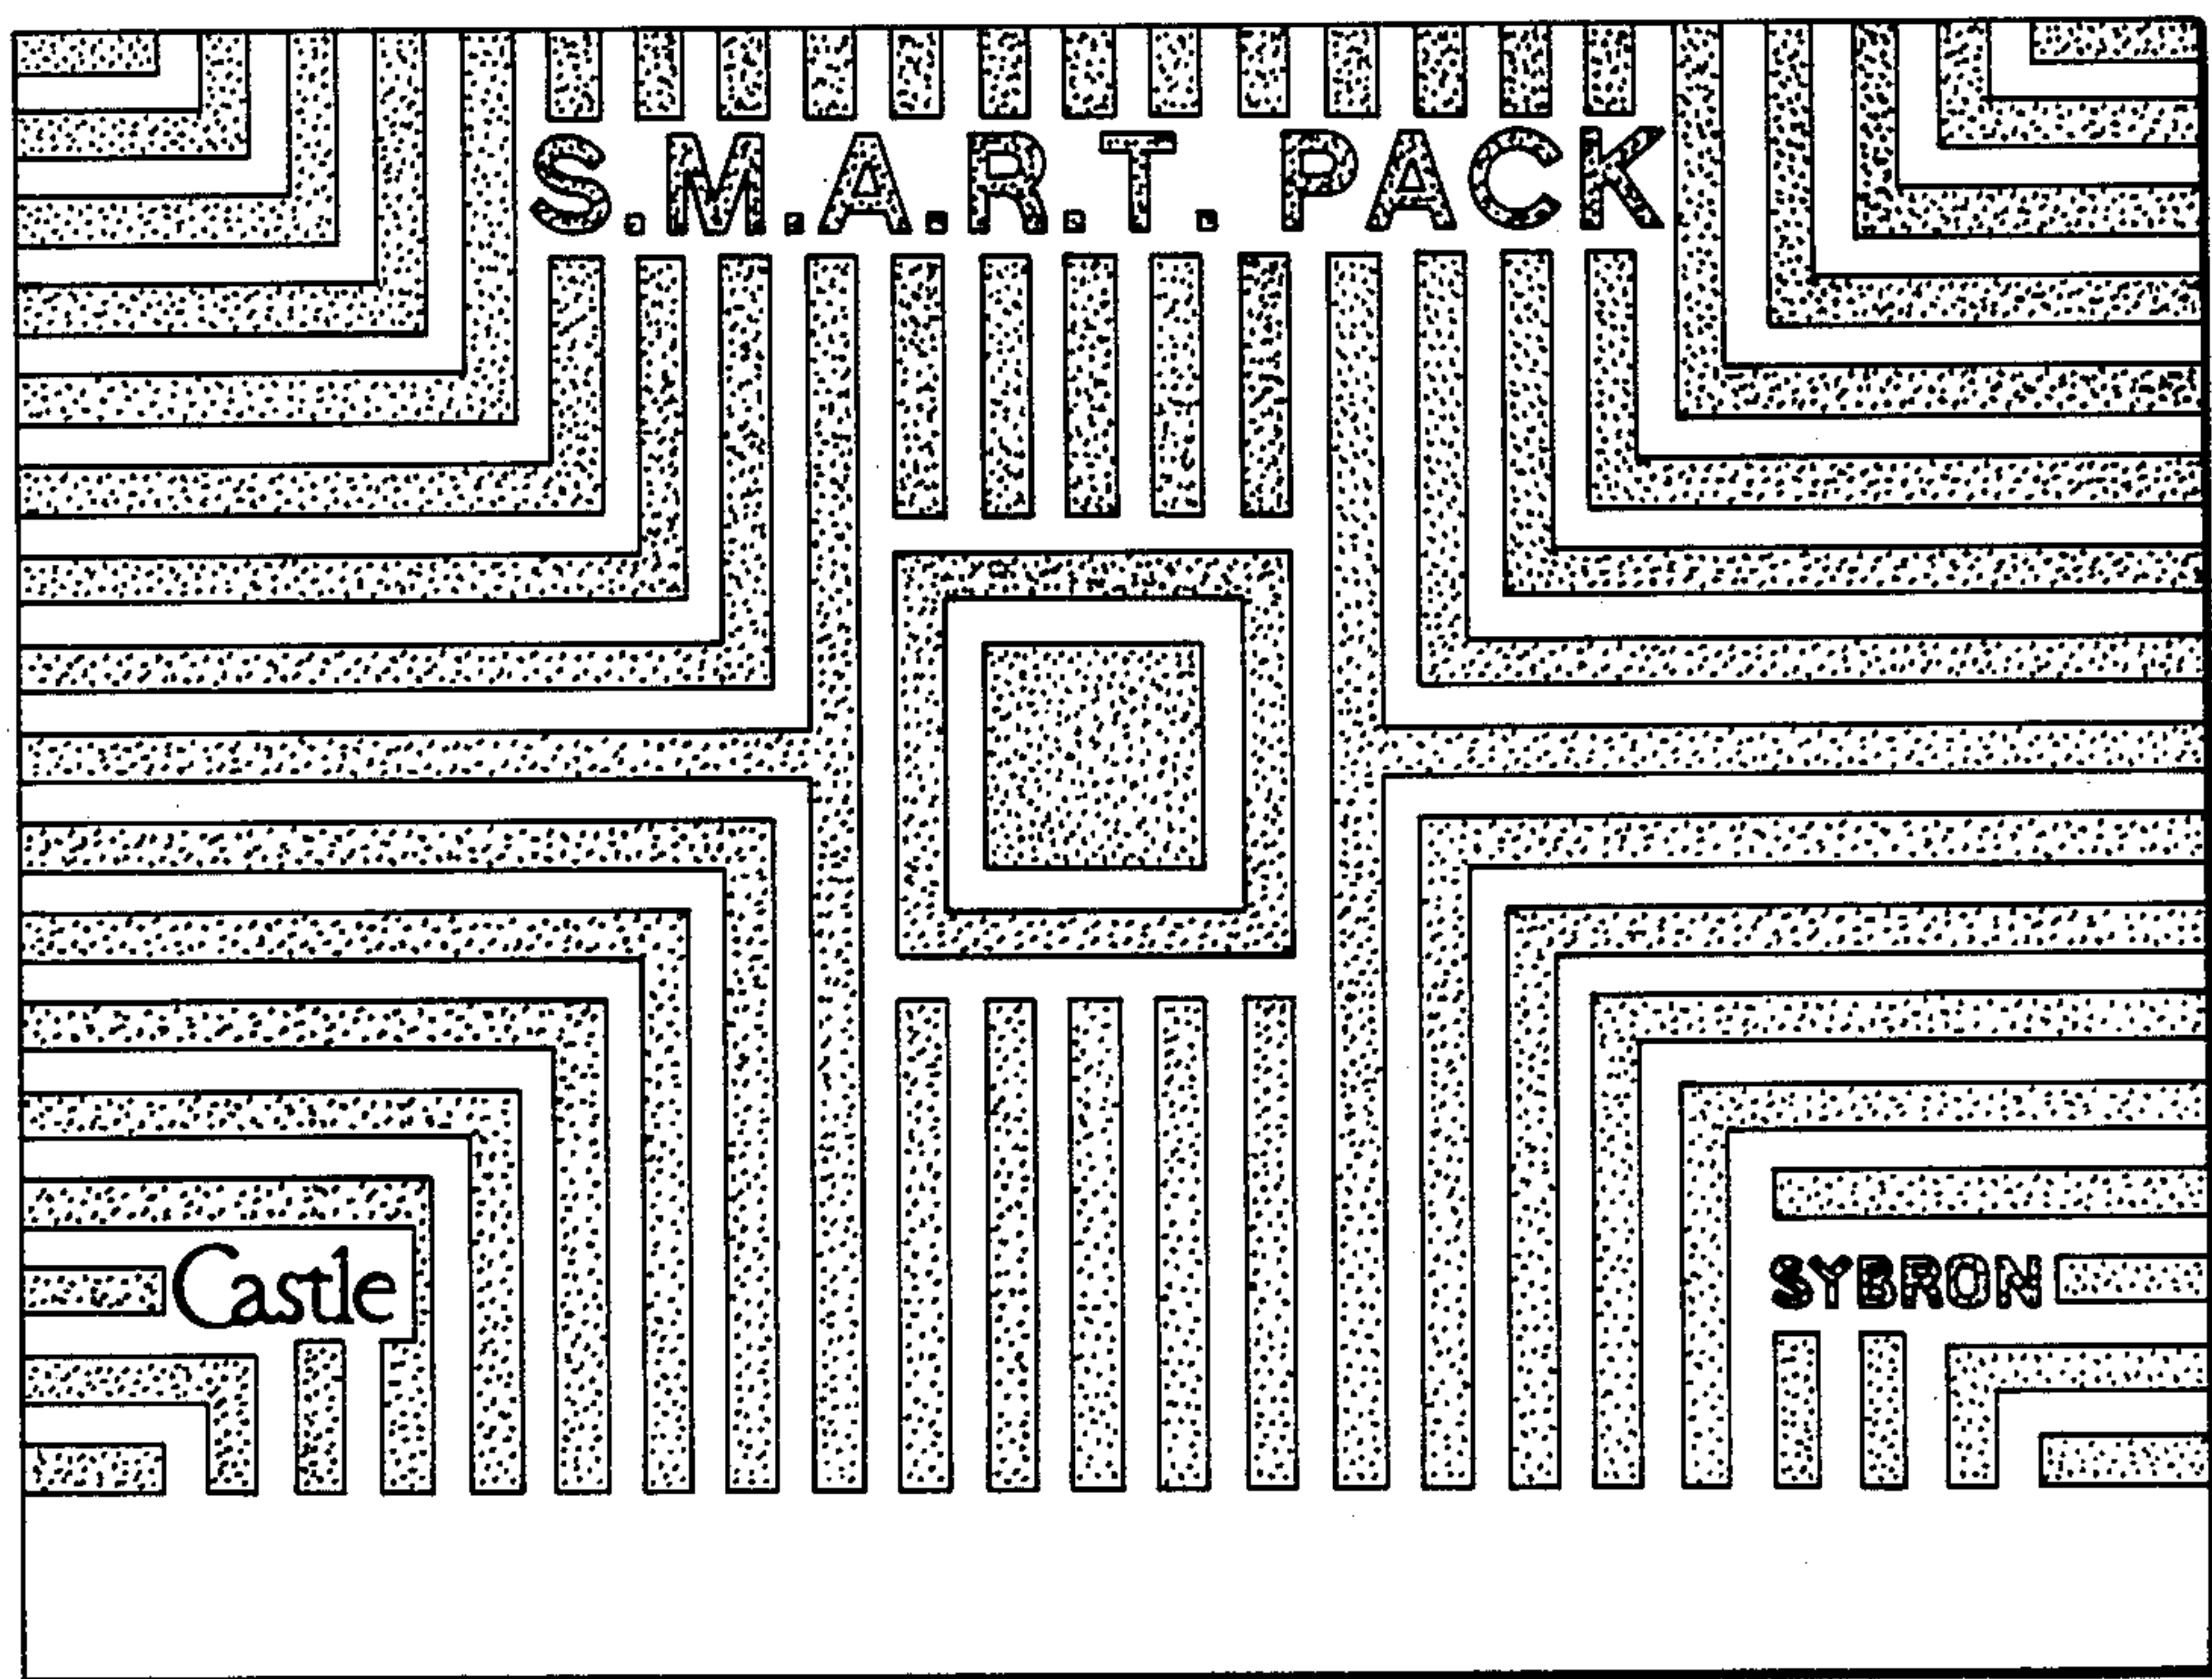


FIG. 5