

[54] AUTOMATIC CHEMICAL ANALYZER

[75] Inventors: Yawara Nagai, Hachioji; Shigeru Yoshinari; Masao Ushikubo, both of Tokyo, all of Japan

[73] Assignee: Olympus Optical Co., Ltd., Japan

[**] Term: 14 Years

[21] Appl. No.: 852,918

[22] Filed: Apr. 16, 1986

[52] U.S. Cl. D10/81; D24/1.1

[58] Field of Search D10/46, 81; D24/1.1, D24/8, 17, 21; 422/63-67; 356/39-41

[56] References Cited

U.S. PATENT DOCUMENTS

D. 206,767	1/1967	MacMillan	D10/81	X
D. 235,356	6/1975	Faraco	D24/1.1	
D. 264,873	6/1982	Olson	D10/81	X
D. 269,544	6/1983	Jarmell	D10/81	X
D. 277,979	3/1985	Brown	D10/81	X
D. 283,203	1/1986	Leonard	D24/1.1	
2,334,776	11/1943	King	D24/1.1	X
3,533,744	10/1970	Unger	356/39	X
4,000,976	1/1977	Kramer	422/65	

4,078,895	3/1978	Moran	422/66	
4,692,308	9/1987	Riley	422/63	X

FOREIGN PATENT DOCUMENTS

1417852	12/1975	United Kingdom	356/39	
---------	---------	----------------	-------	--------	--

Primary Examiner—Nelson C. Holtje
Attorney, Agent, or Firm—Ostrolenk, Faber, Gerb & Soffen

[57] CLAIM

The ornamental design for an automatic chemical analyzer, as shown and described.

DESCRIPTION

FIG. 1 is a front, top, and left side perspective view of an automatic chemical analyzer, showing our new design;

FIG. 2 is a rear, bottom, and right side perspective view thereof;

FIG. 3 is a front elevational view thereof;


FIG. 4 is a rear elevational view thereof;

FIG. 5 is a top plan view thereof;

FIG. 6 is a bottom plan view thereof;

FIG. 7 is a left side elevational view thereof;

FIG. 8 is a right side elevational view thereof.

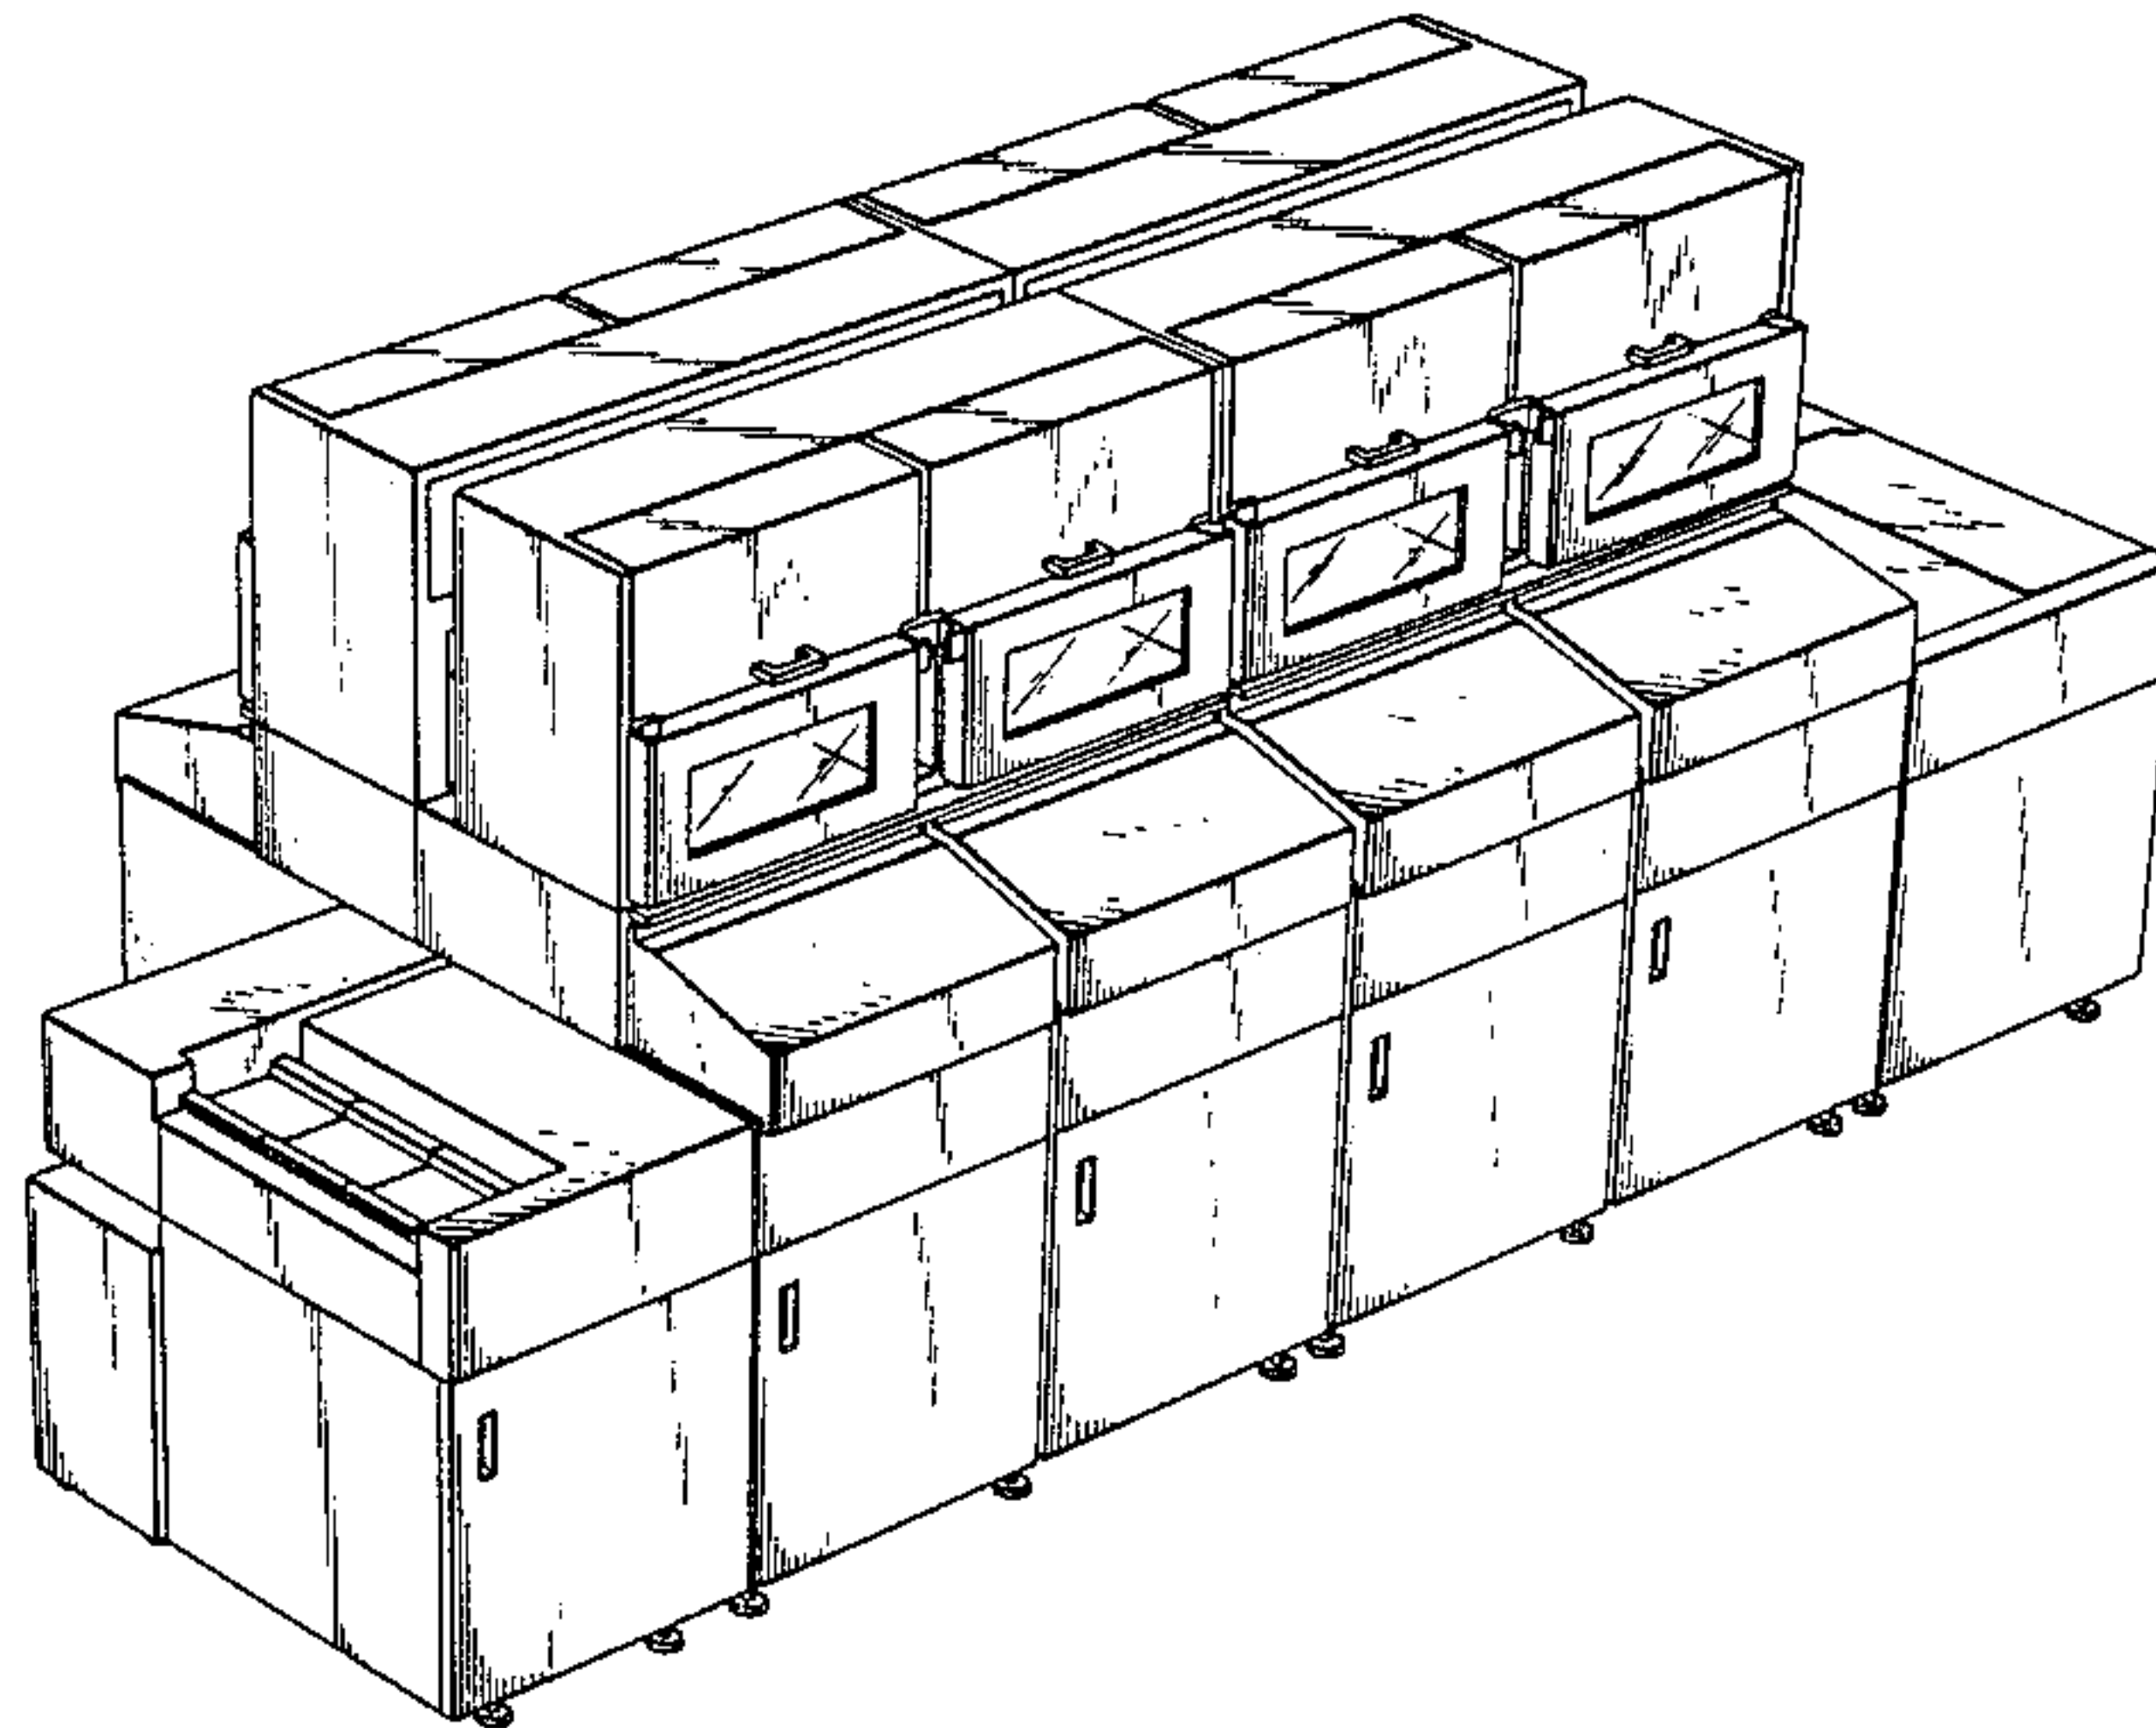

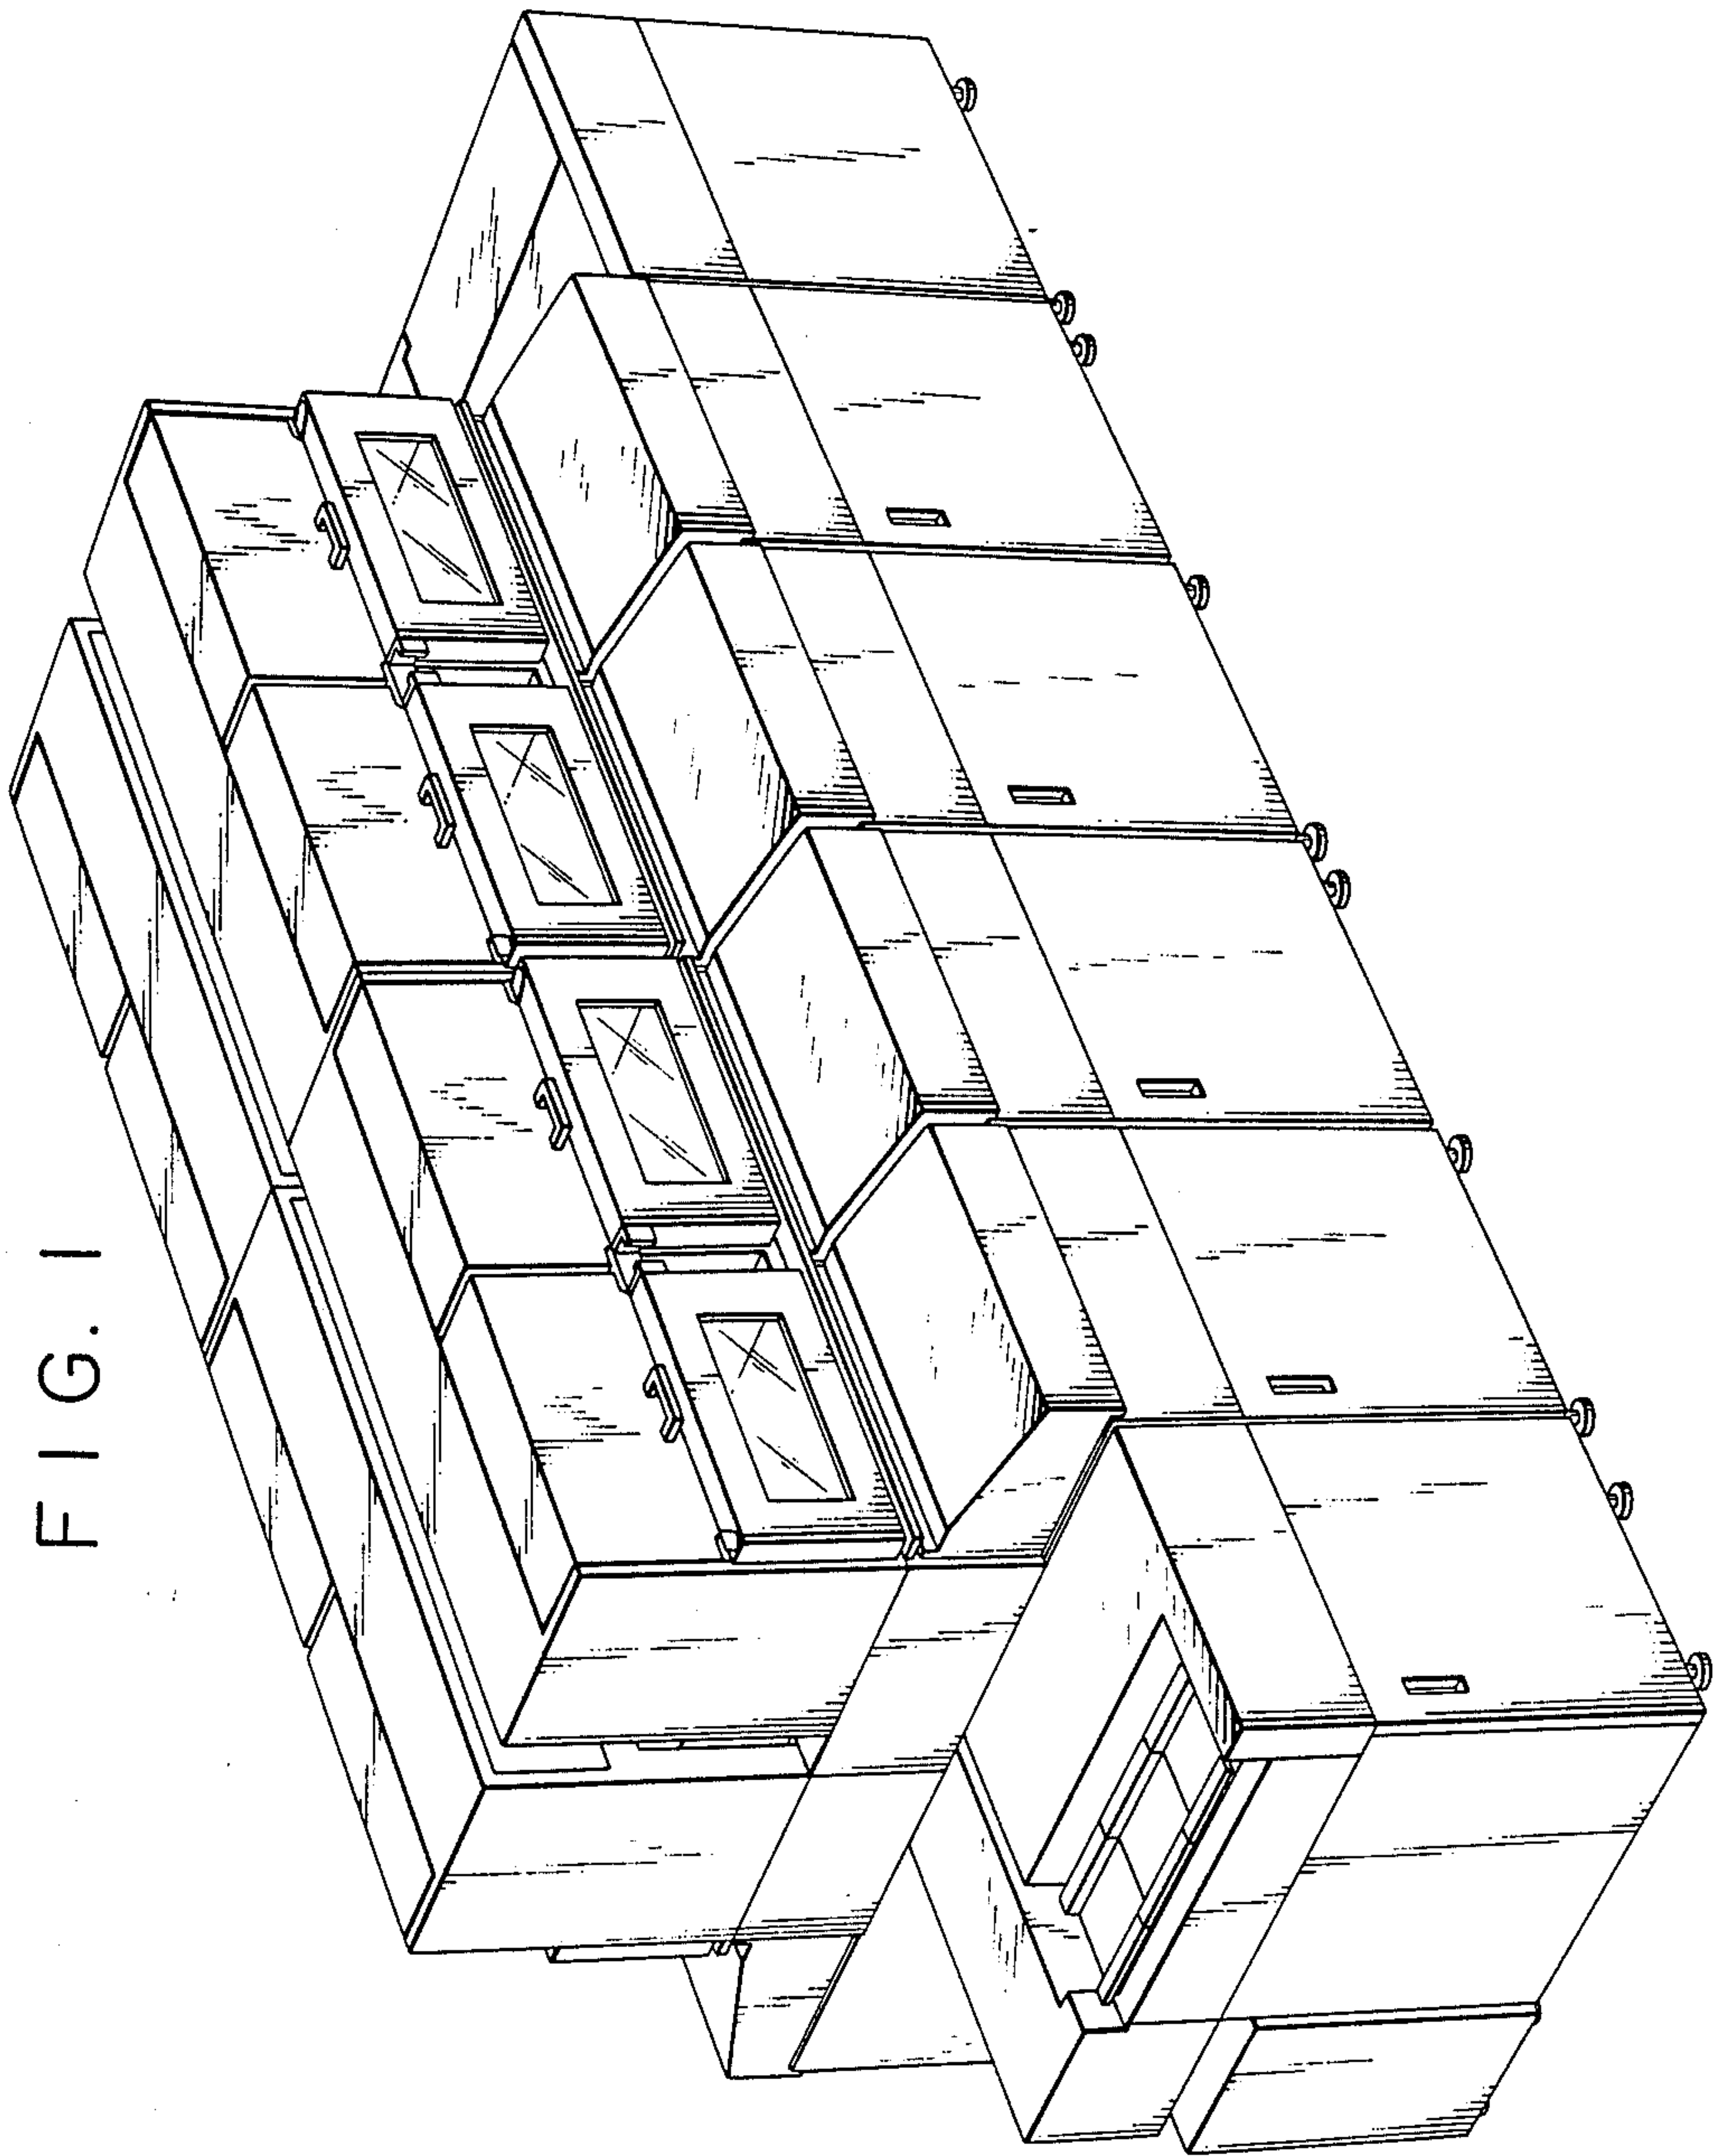


FIG. 1

FIG. 2

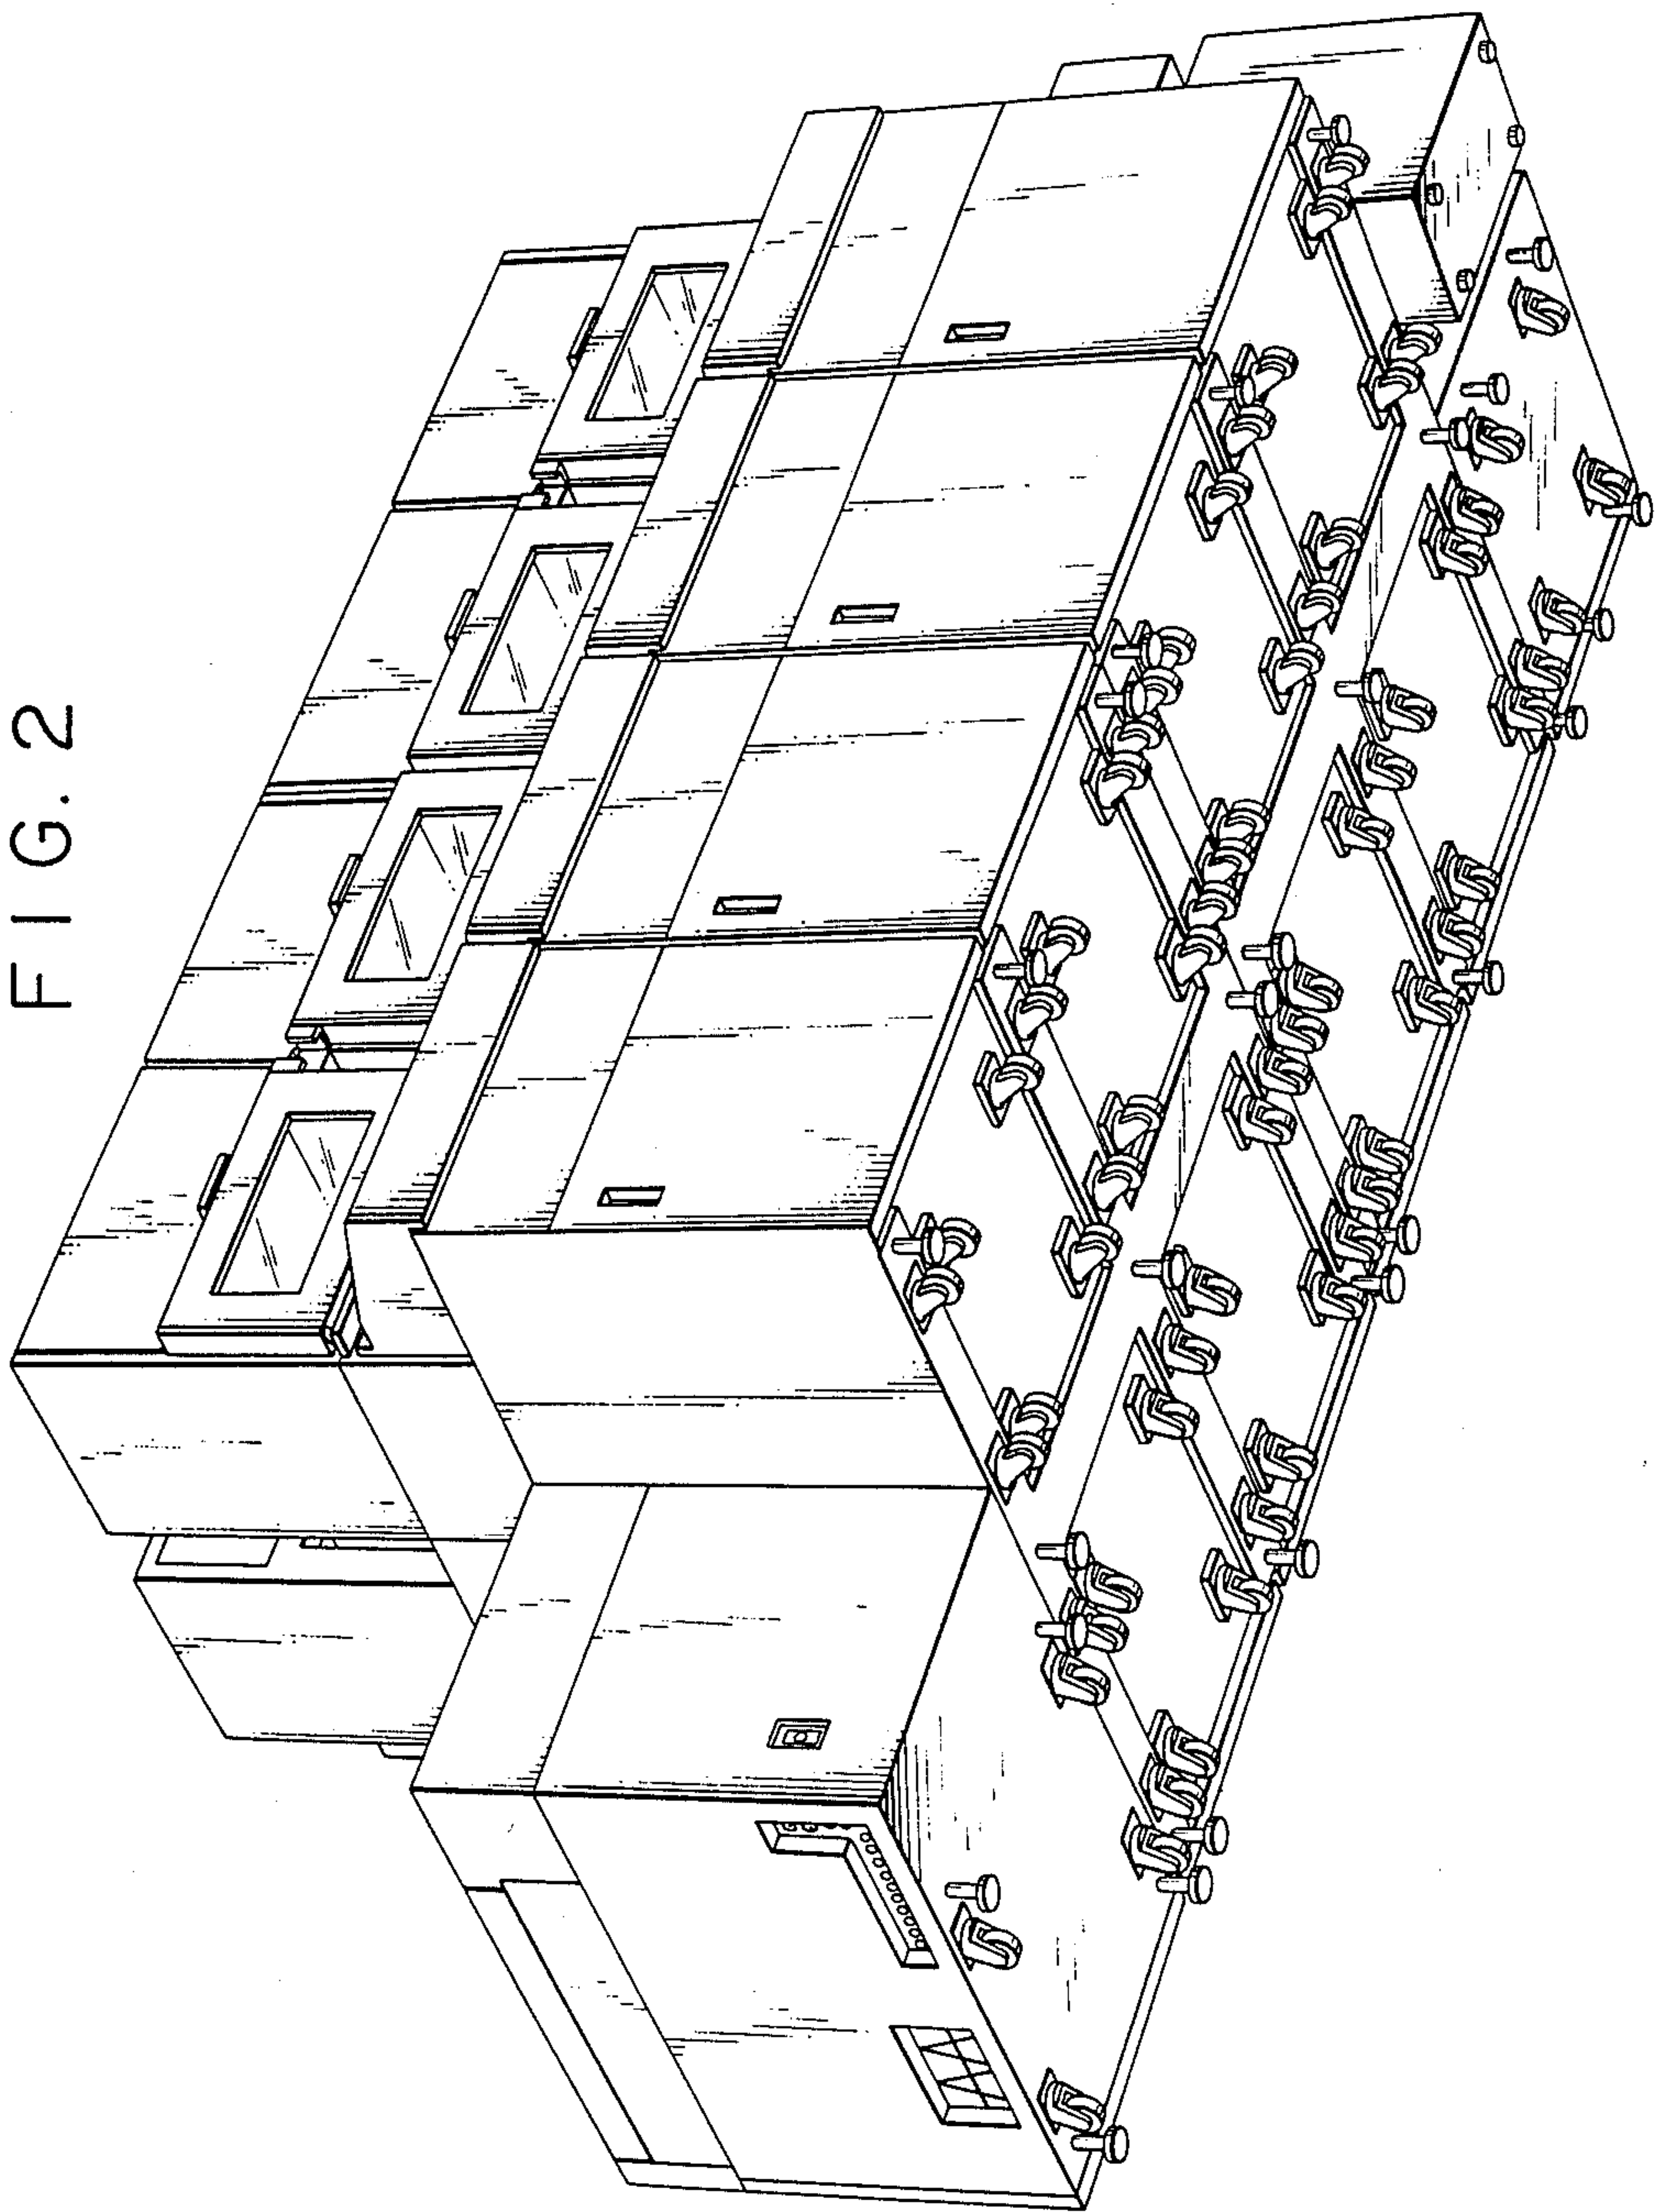


FIG. 3

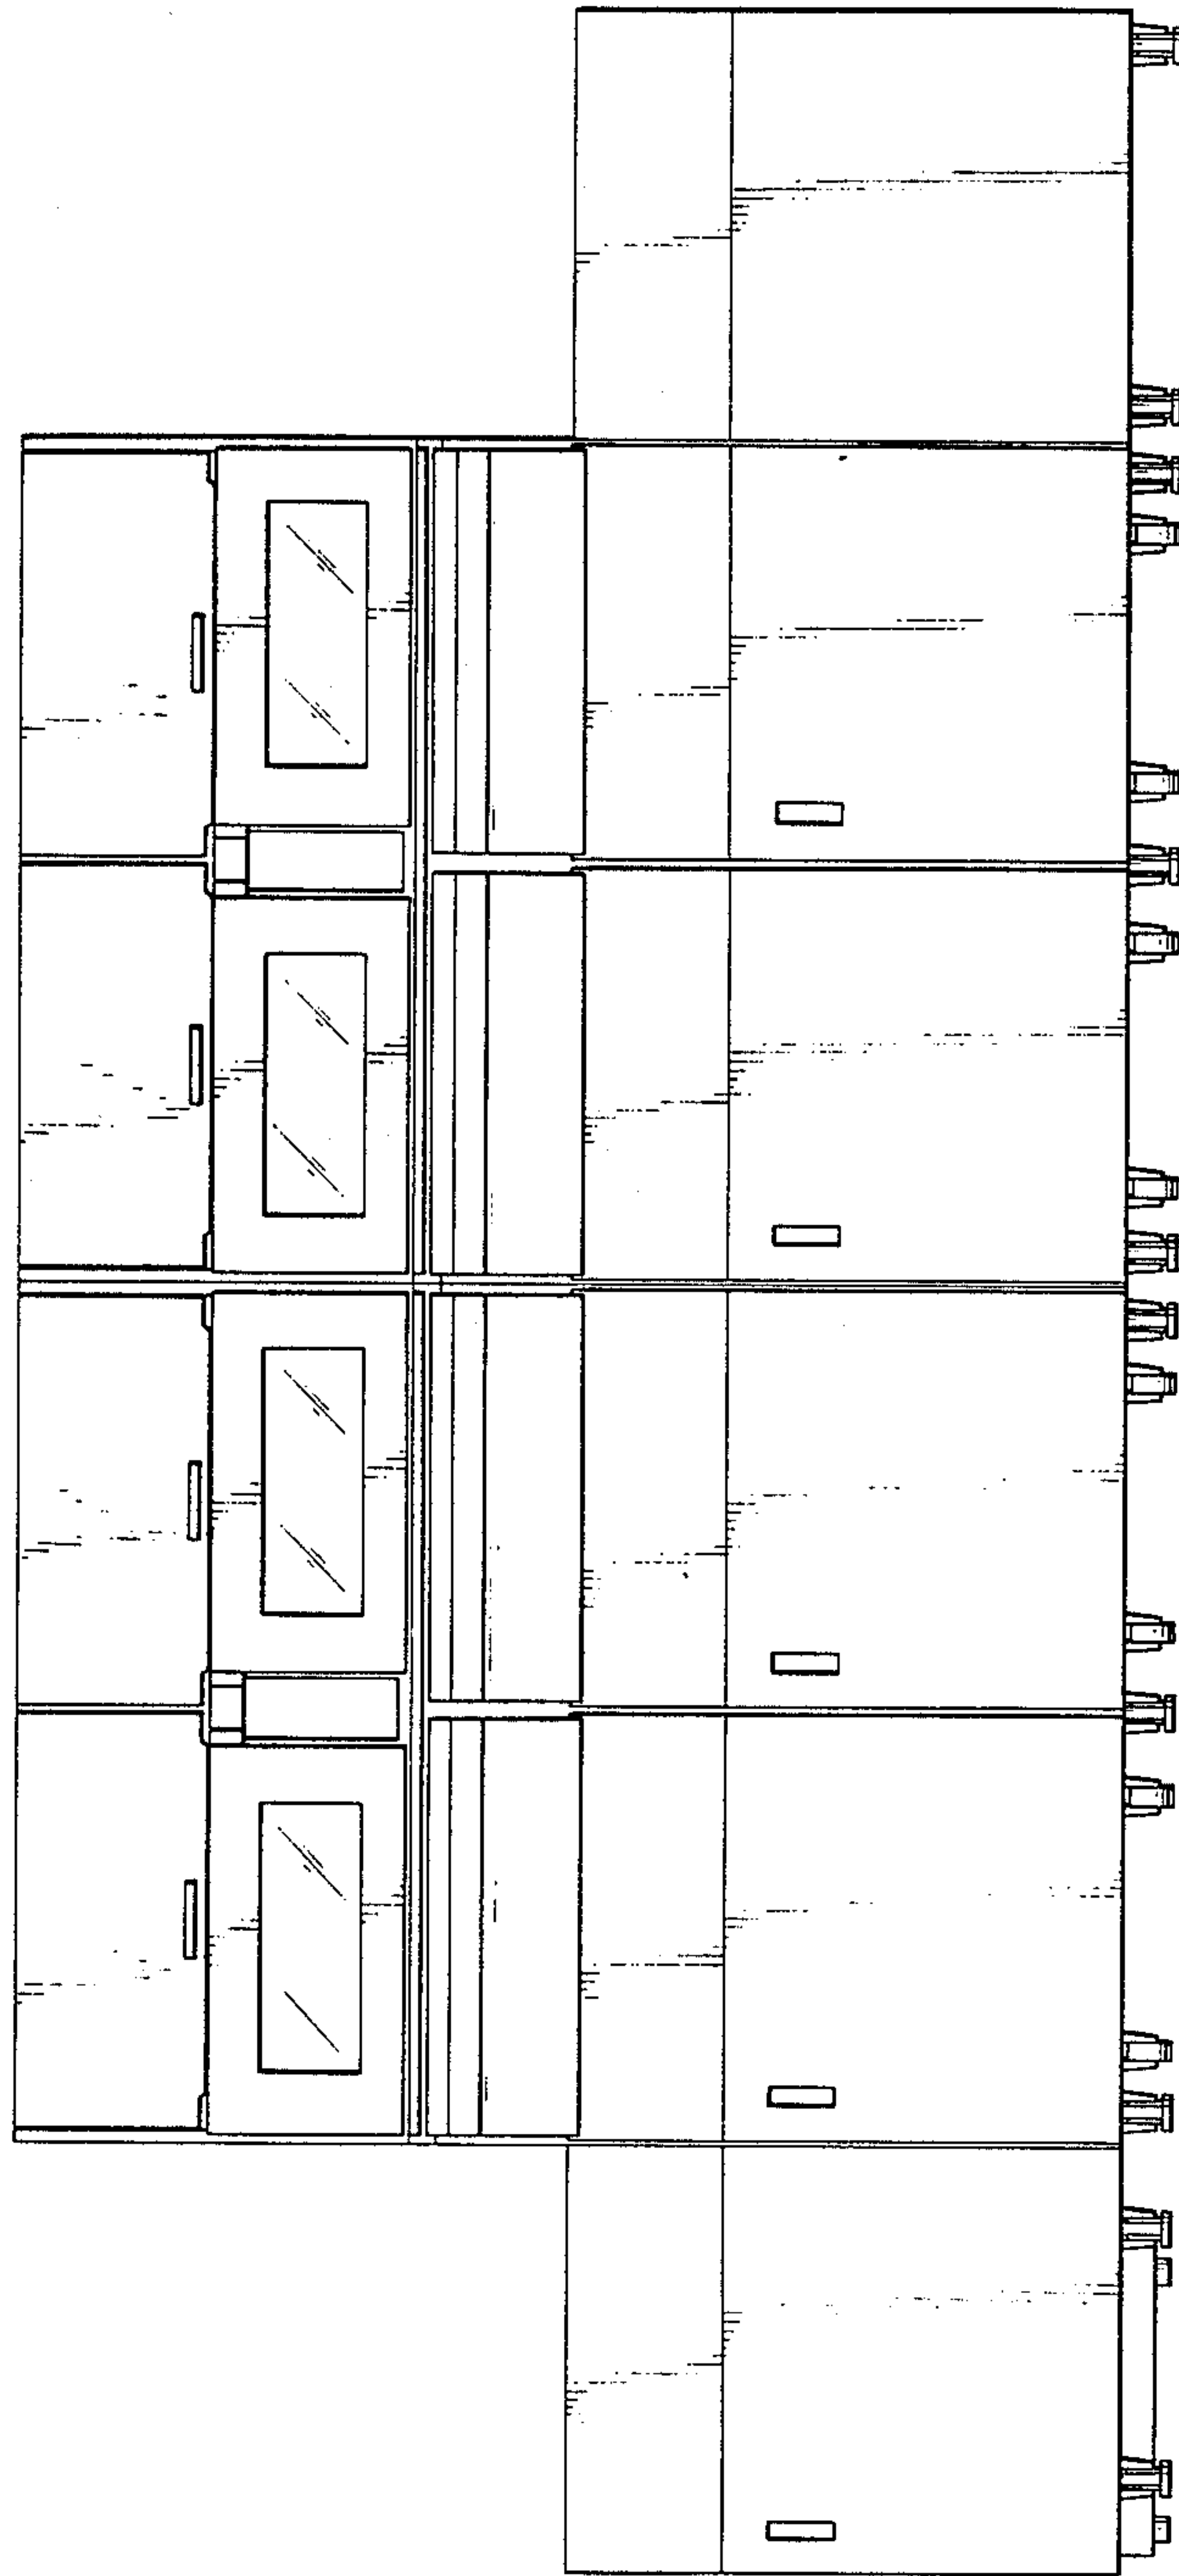


FIG. 4

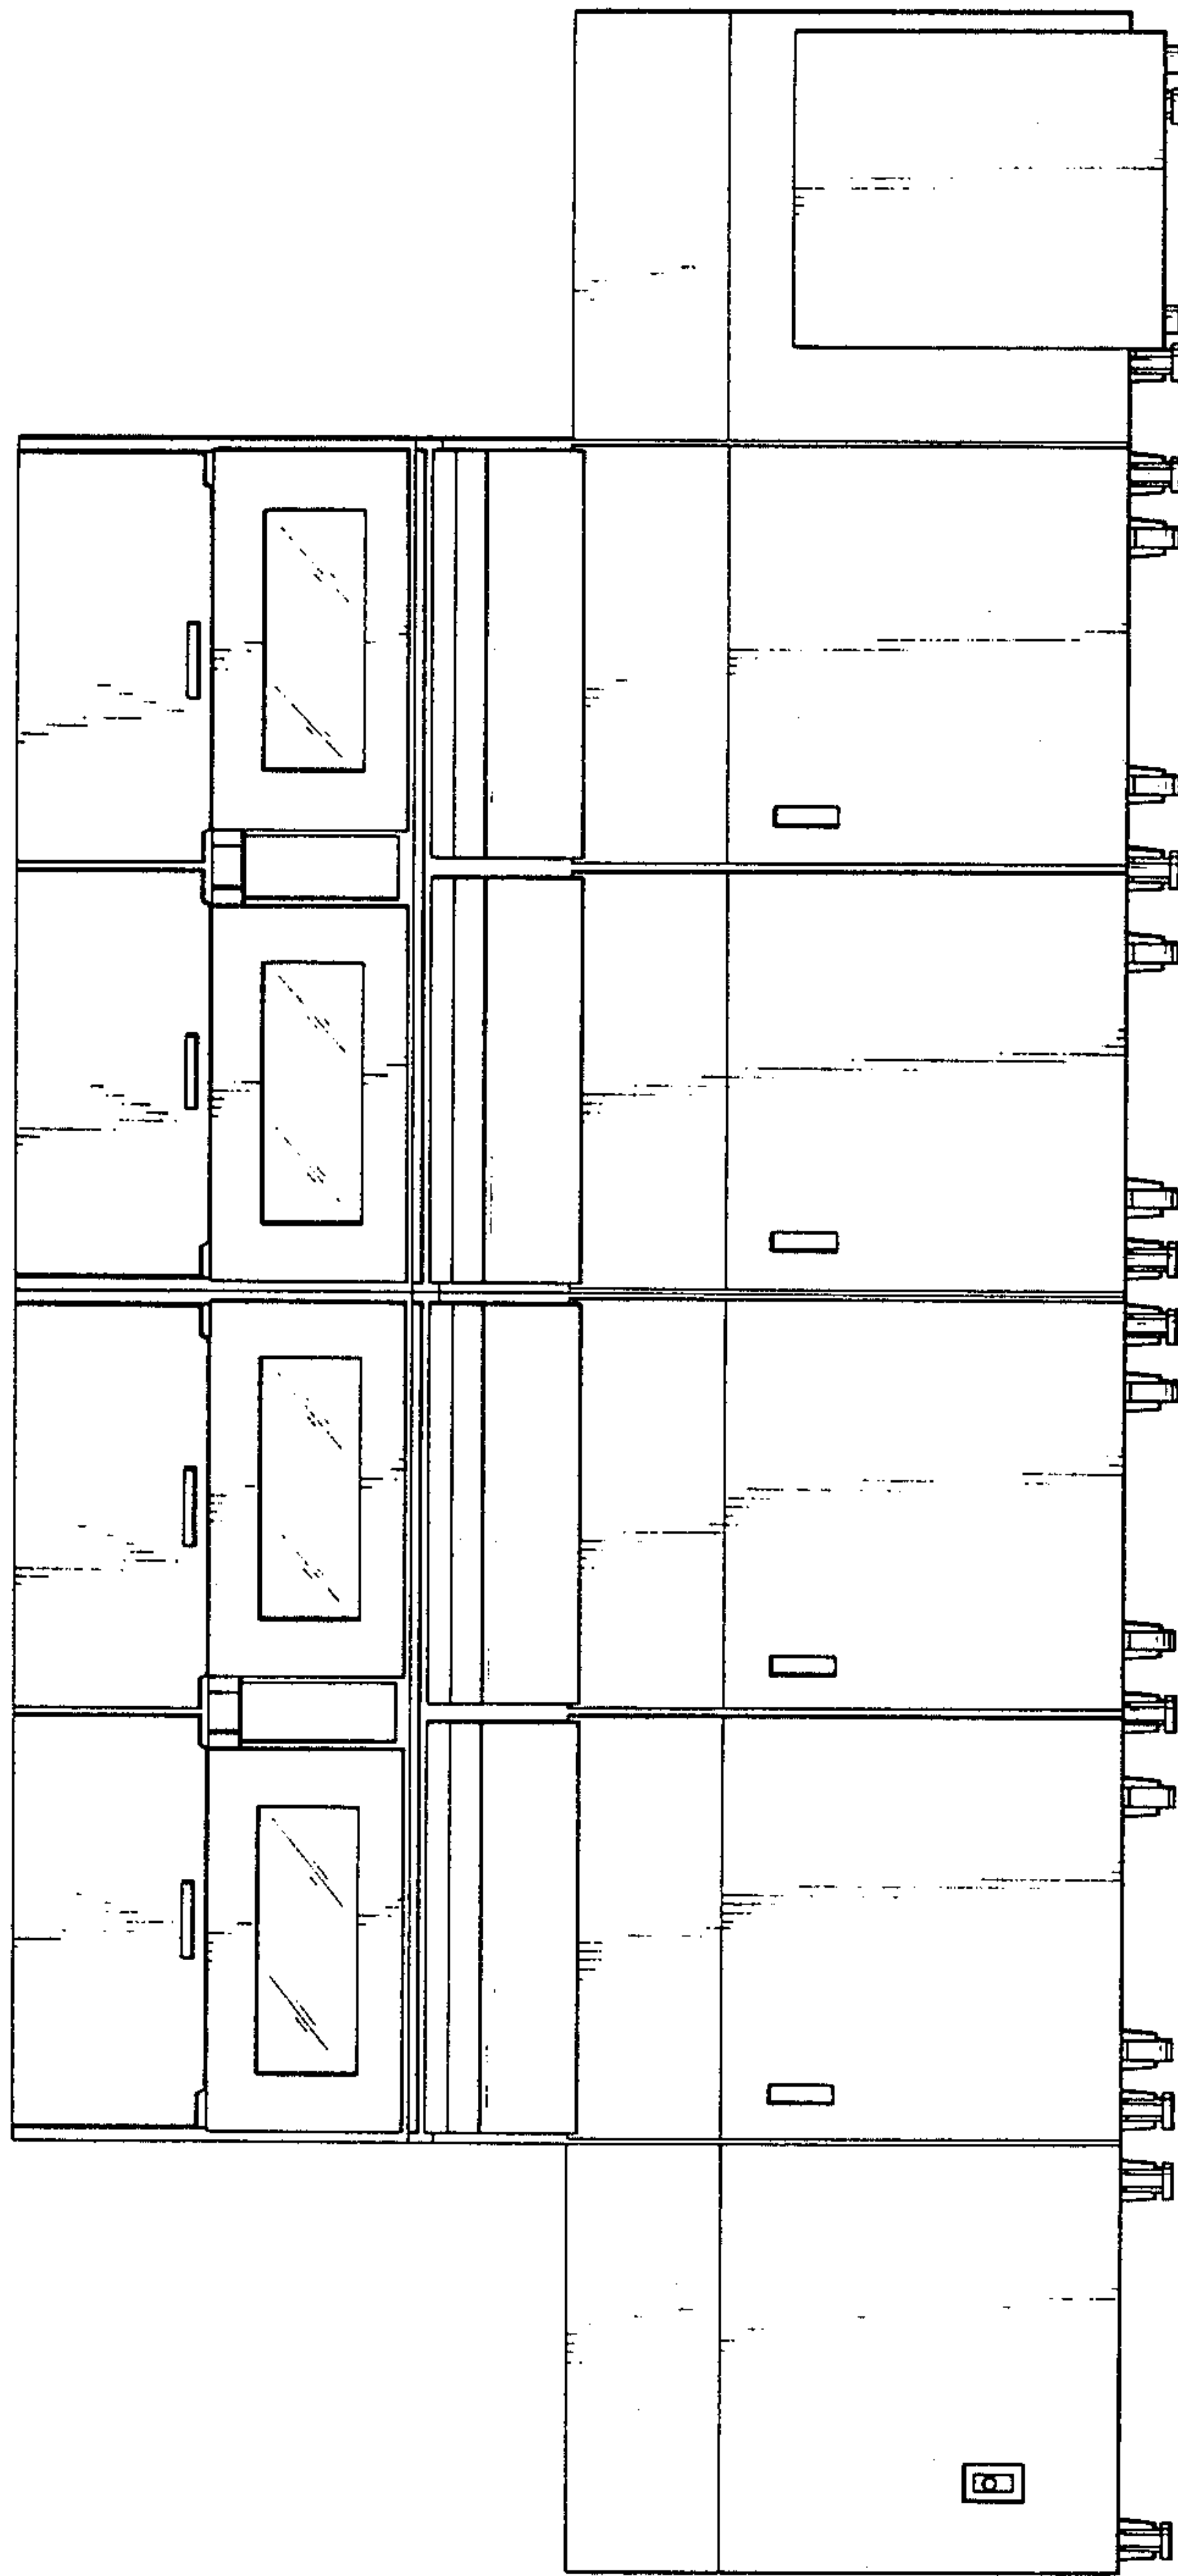


FIG. 5

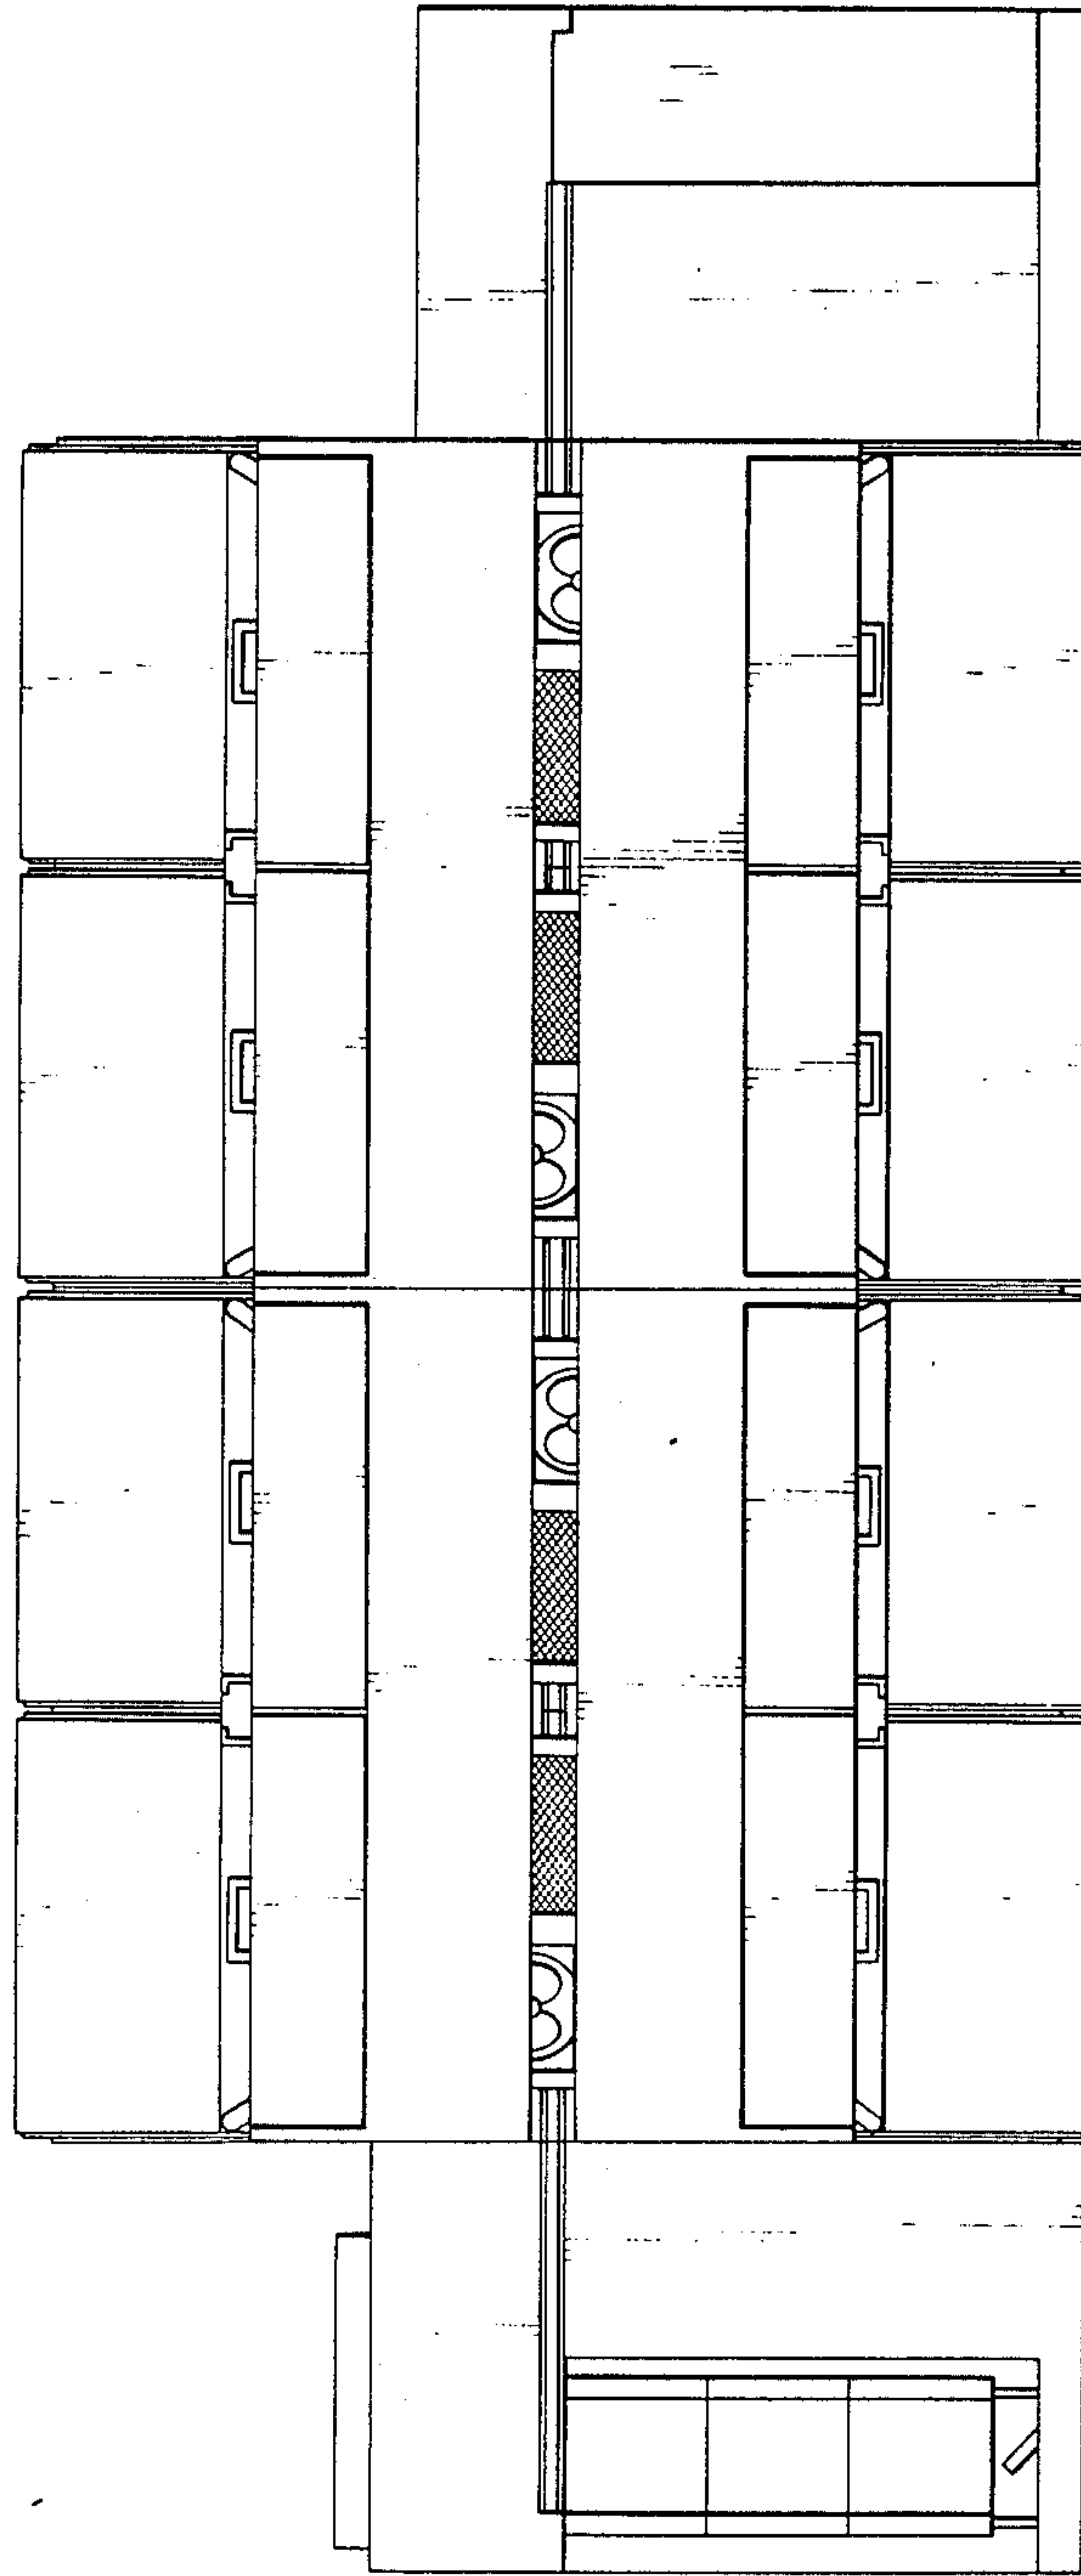


FIG. 6

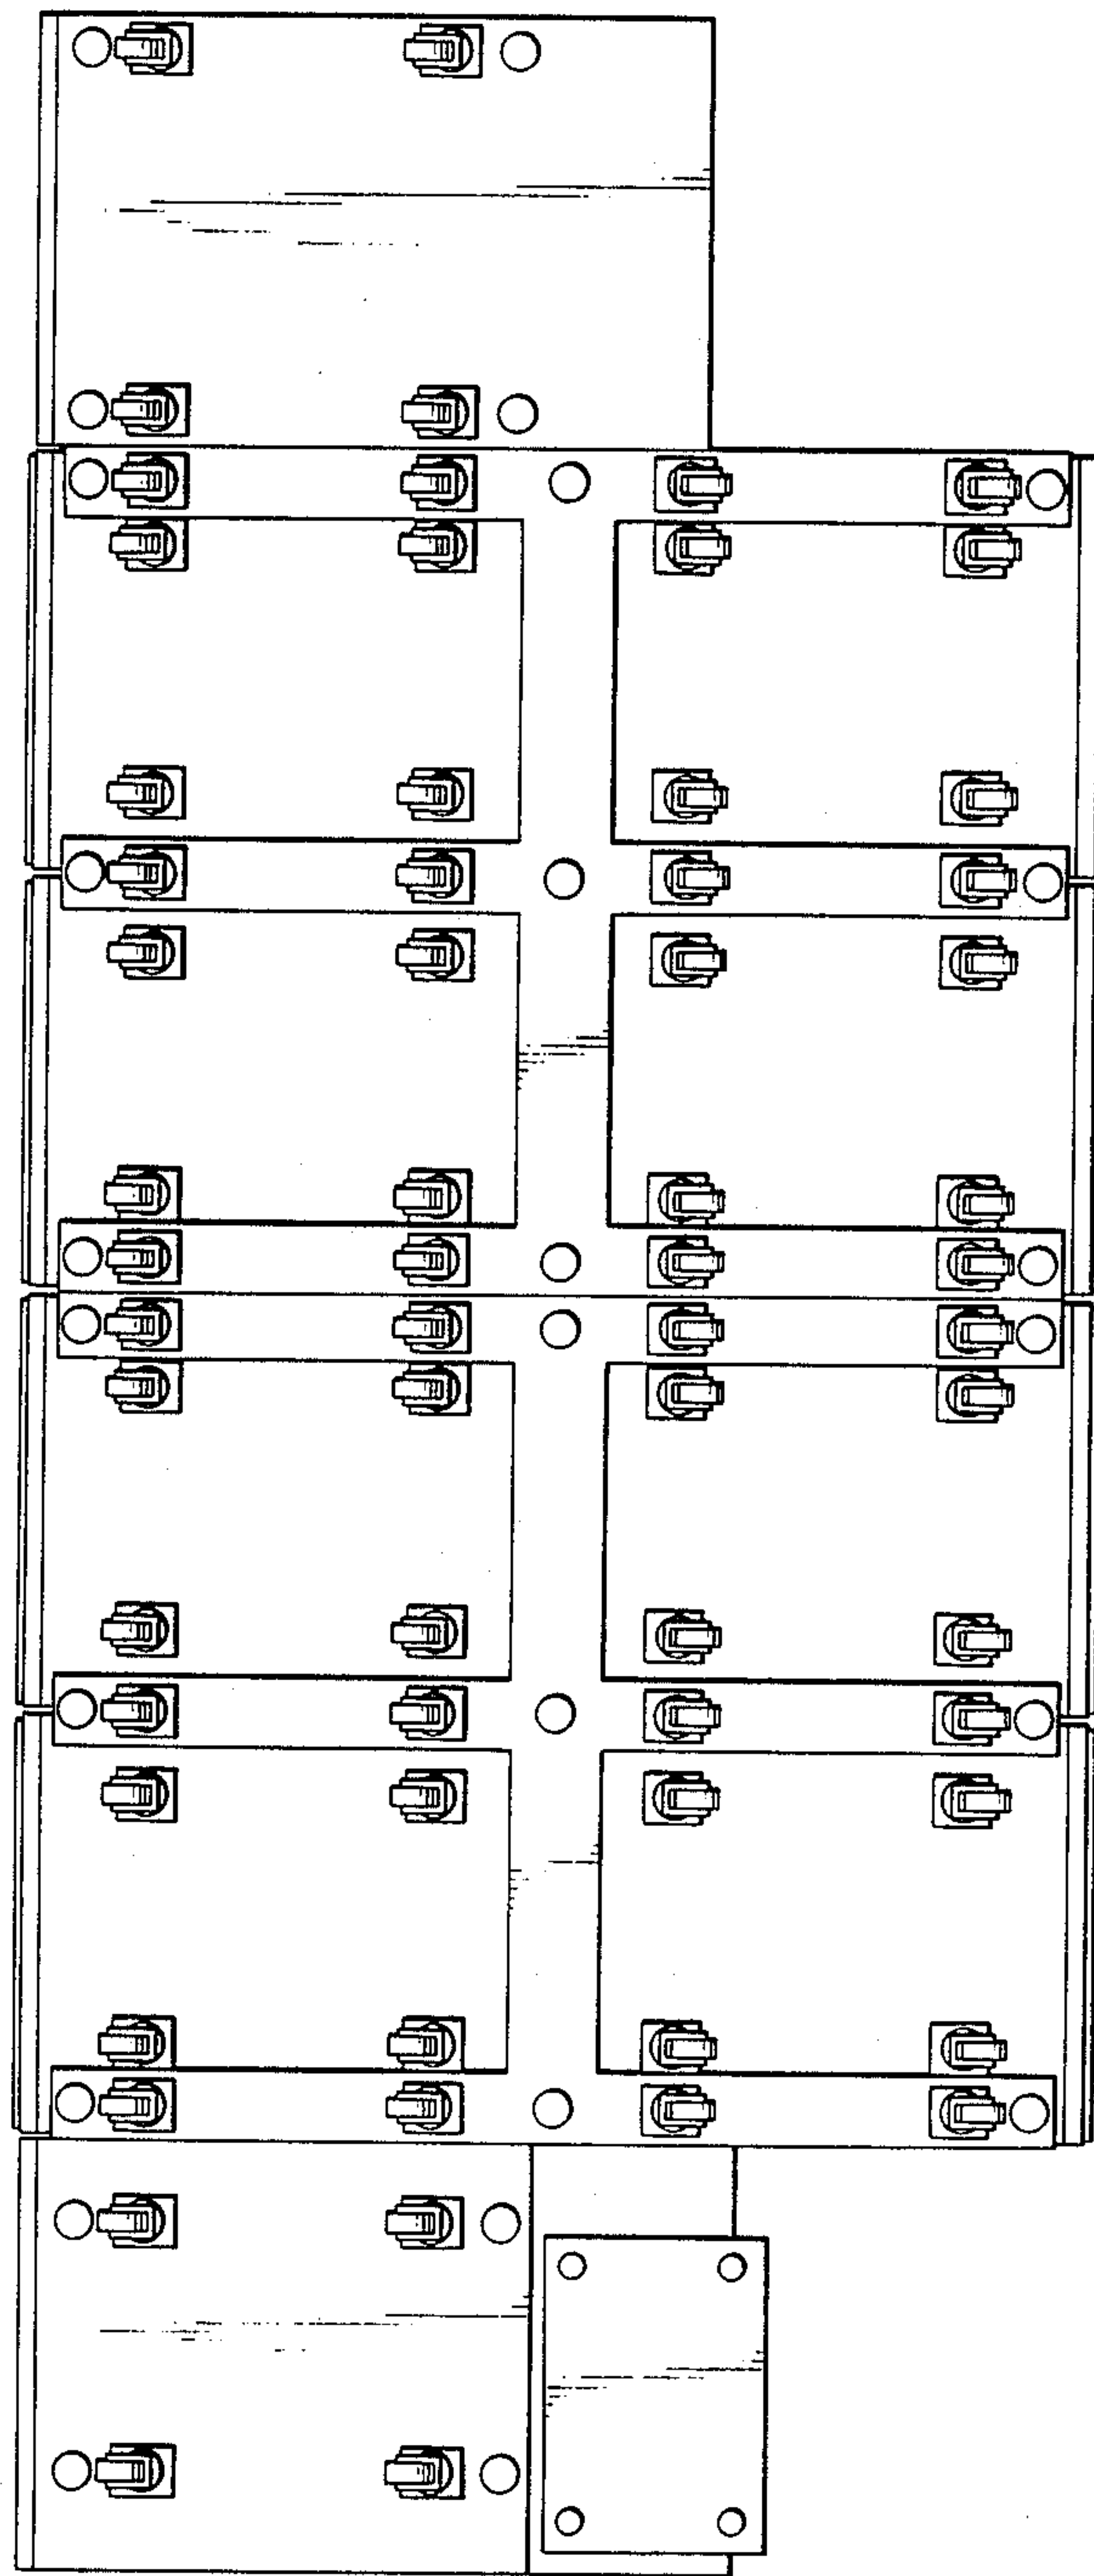


FIG. 8

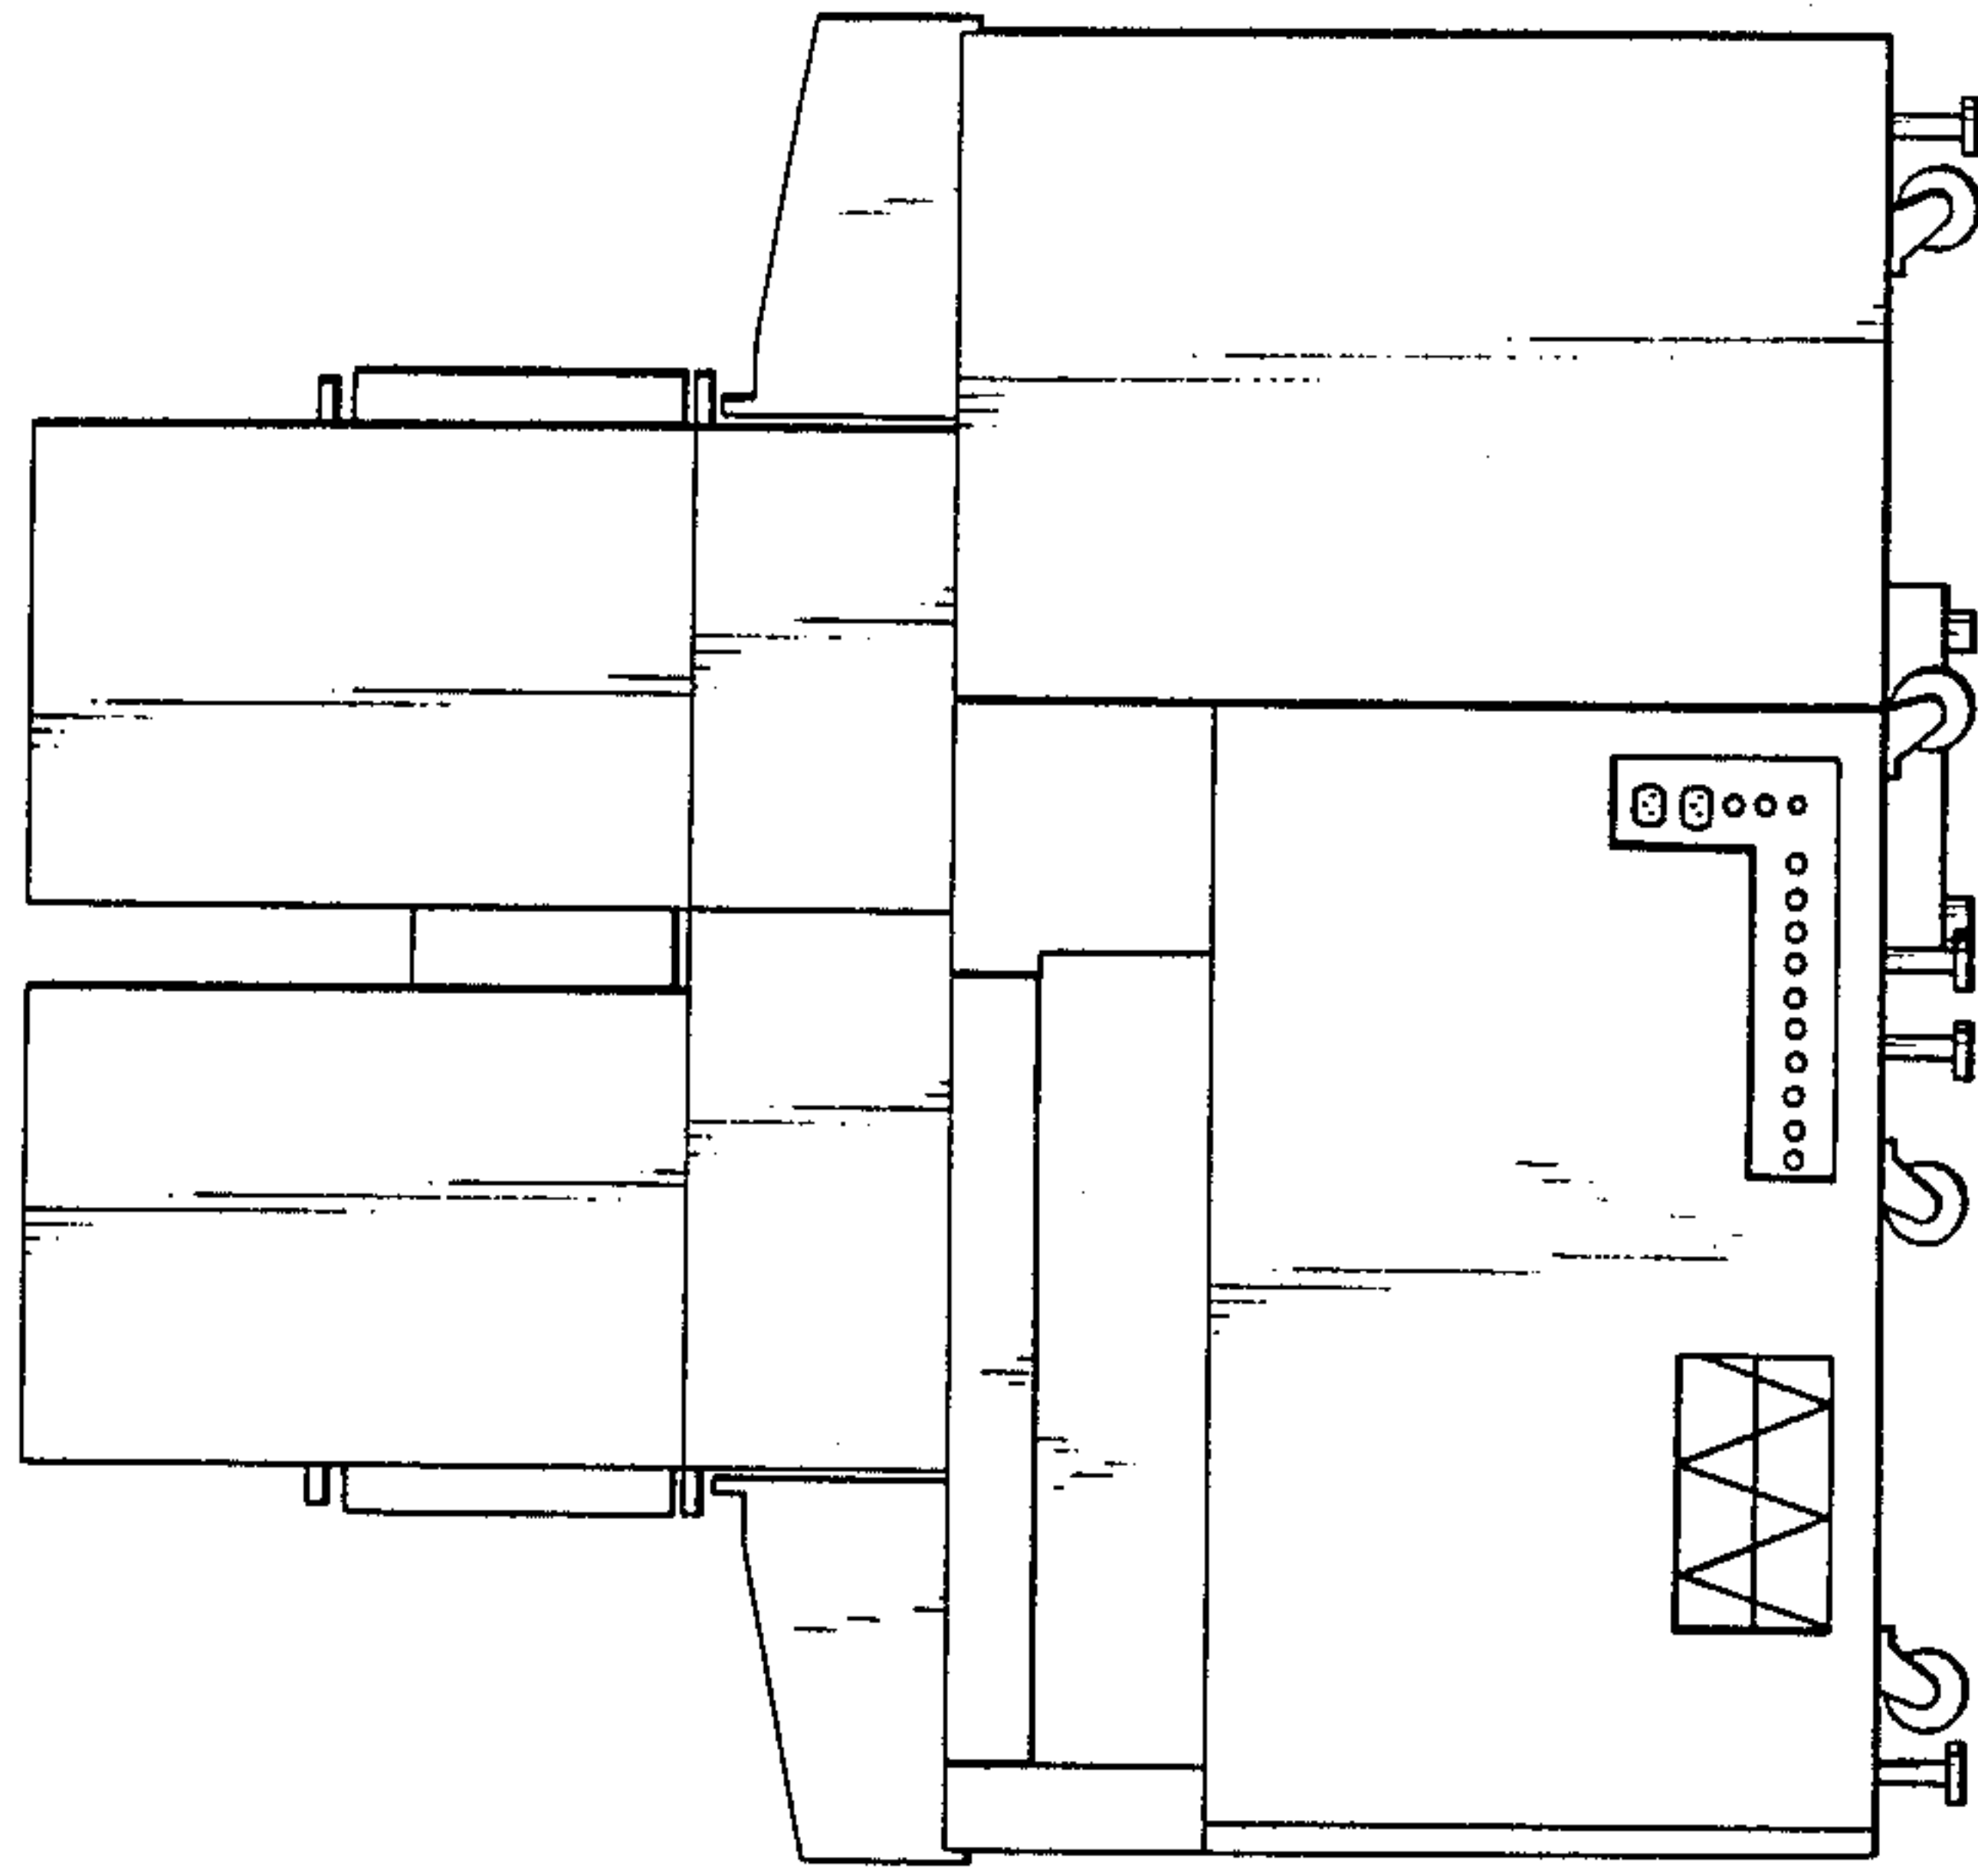


FIG. 7

