

[54] IMMUNOASSAY TEST KIT

[75] Inventors: Dennis M. Mochnal, Clinton; Henry A. Graham, Jr., Annandale; Walter J. Yarrow, Jr., Lambertville, all of N.J.; C. Minot Dole, Purdy's, N.Y.; Joseph R. Paradis, Hilton Head Island, S.C.

[73] Assignee: Ortho Diagnostic Systems Inc., Raritan, N.J.

[**] Term: 14 Years

[21] Appl. No.: 99,842

[22] Filed: Sep. 21, 1987

[52] U.S. Cl. D24/17

[58] Field of Search D24/17, 8, 21; 436/65, 436/178, 814, 906; 422/102, 100, 99, 55-58, 61; 435/7.5

[56] References Cited

U.S. PATENT DOCUMENTS

D. 216,306 12/1969 Dutch D24/17
D. 292,229 10/1987 Knudson et al. D24/21
3,219,421 11/1965 Schwarz, Jr. et al. 422/102
4,181,500 1/1980 Cowsar et al. D24/17 X

4,230,664 10/1980 Cais 422/61
4,495,151 1/1985 Ohyama et al. 422/102
4,628,036 12/1986 Scheepens et al. 436/520
4,681,782 7/1987 Ozkan 435/7 X

FOREIGN PATENT DOCUMENTS

0203443 3/1986 European Pat. Off. .

Primary Examiner—A. Hugo Word
Assistant Examiner—Stella M. Reid

[57] CLAIM

The ornamental design for an immunoassay test kit, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of an immunoassay test kit, showing our new design;
FIG. 2 is a right end elevational view thereof;
FIG. 3 is a left end elevational view thereof;
FIG. 4 is a top plan view thereof;
FIG. 5 is a side elevational view thereof, the opposite side elevational view being identical thereto;
FIG. 6 is a bottom plan view thereof; and
FIG. 7 is an exploded perspective view thereof, with parts removed.

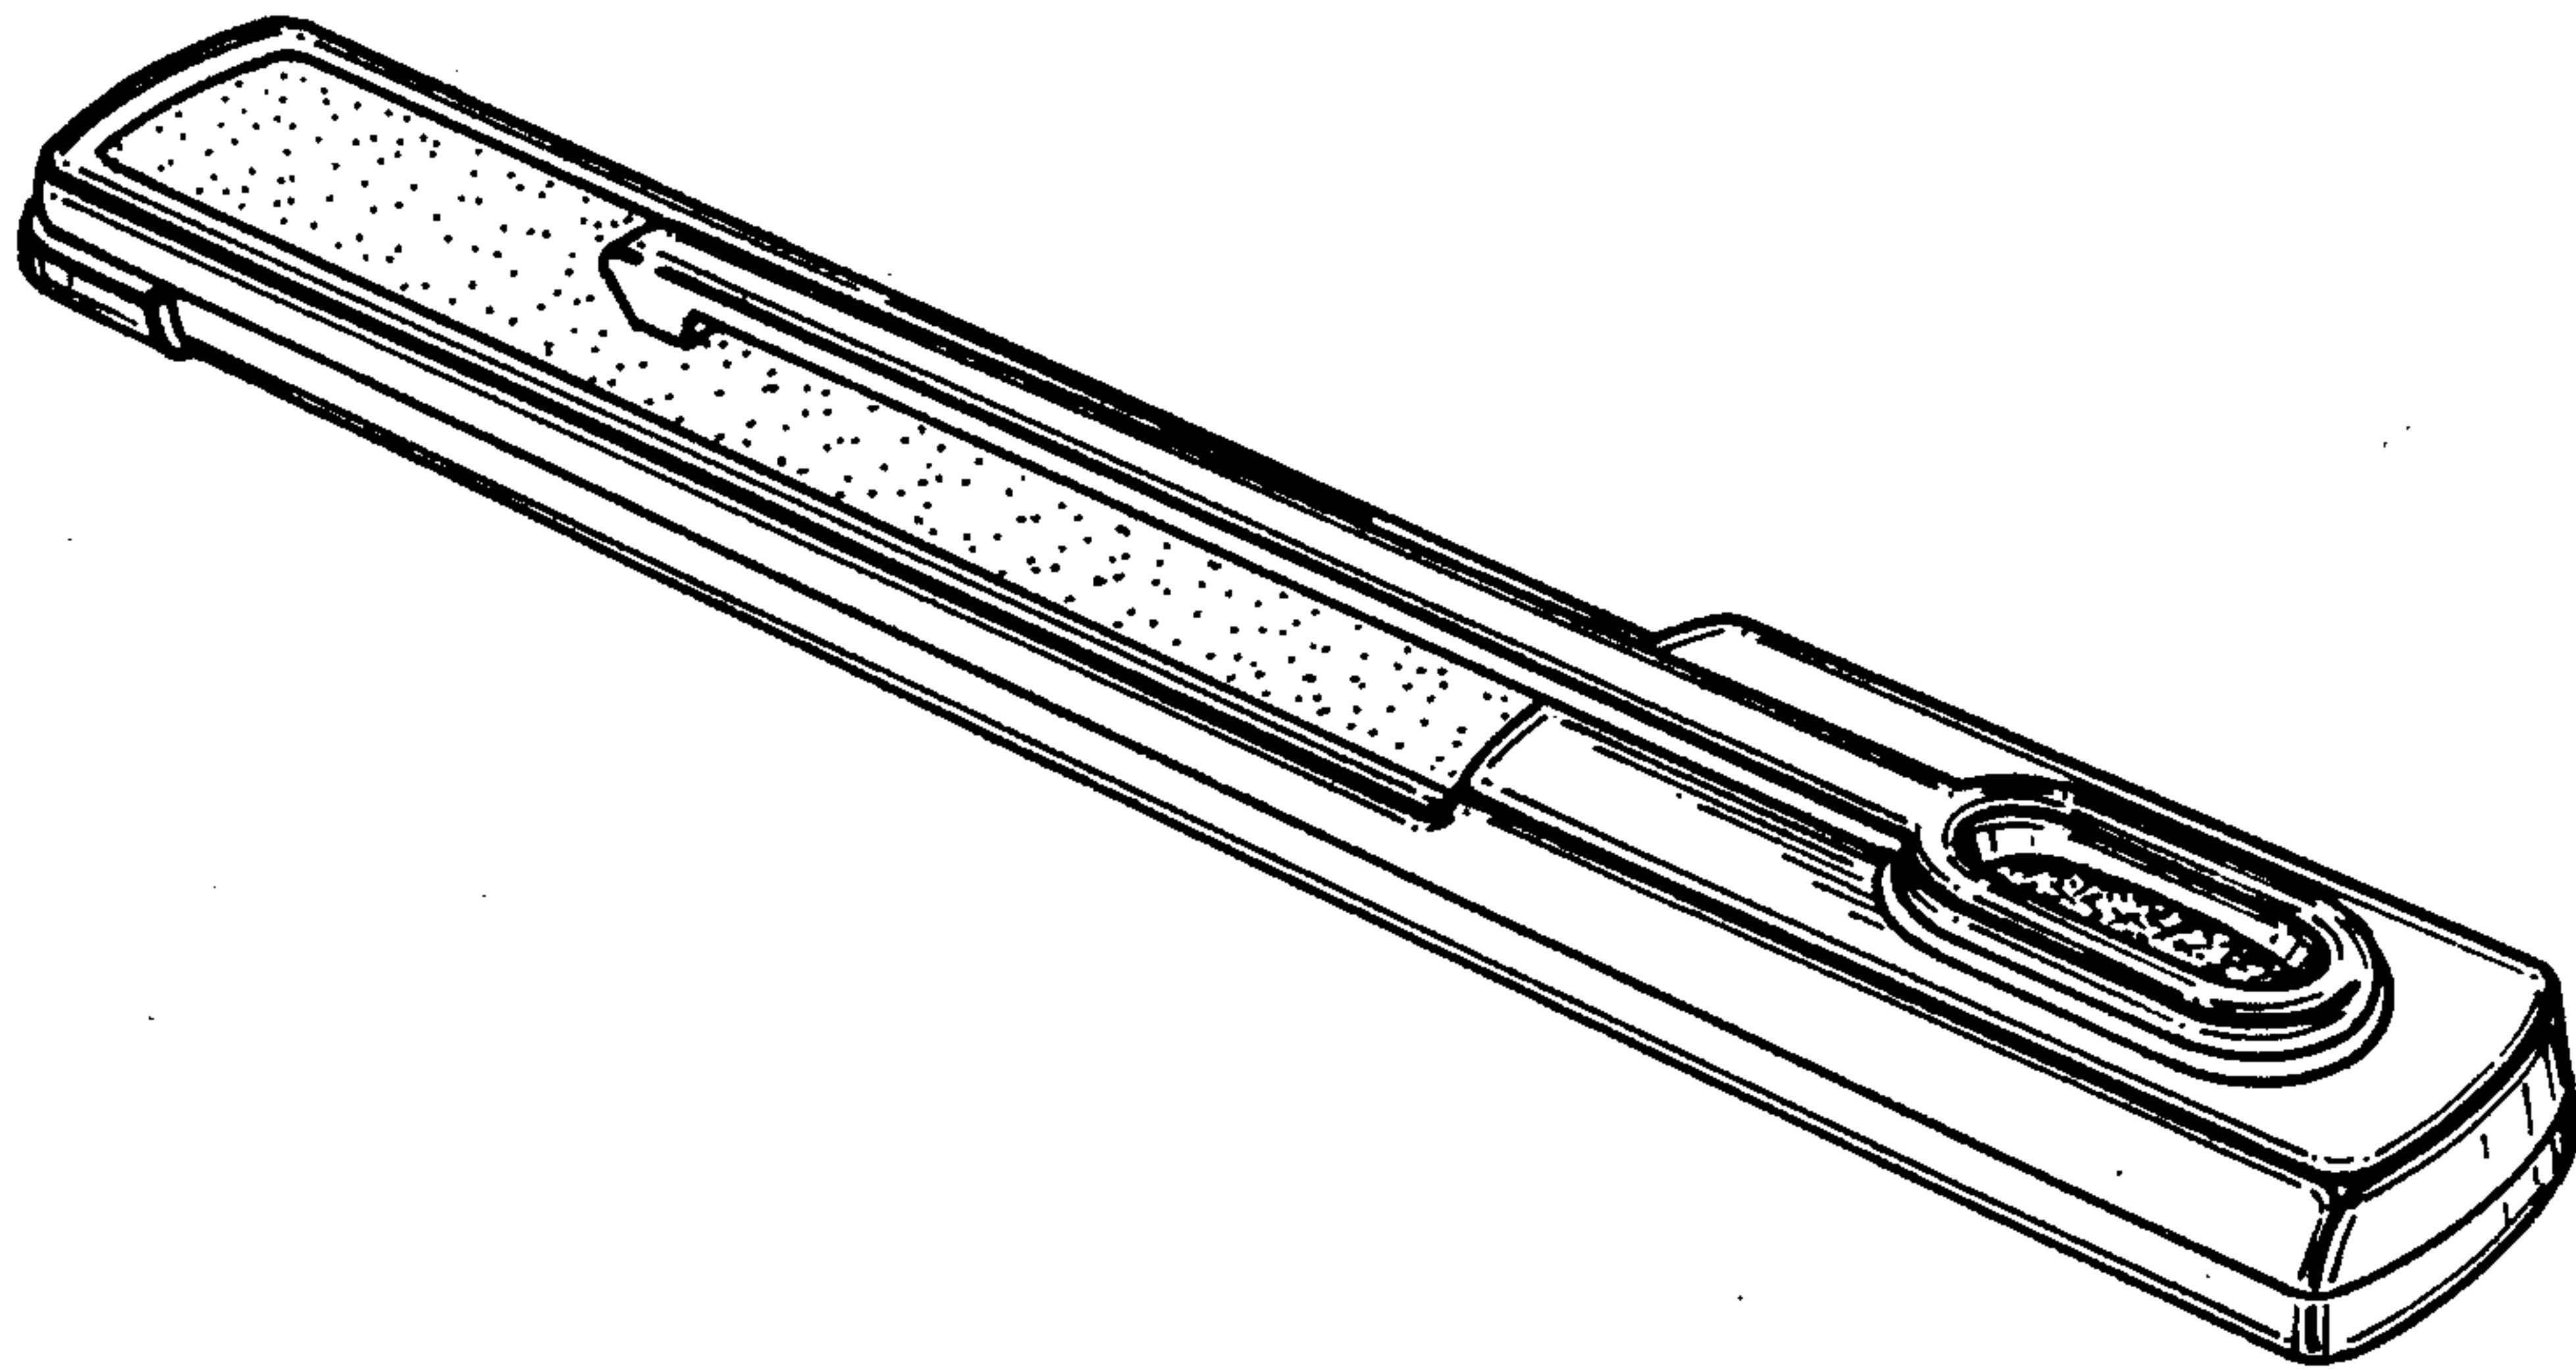


FIG-1

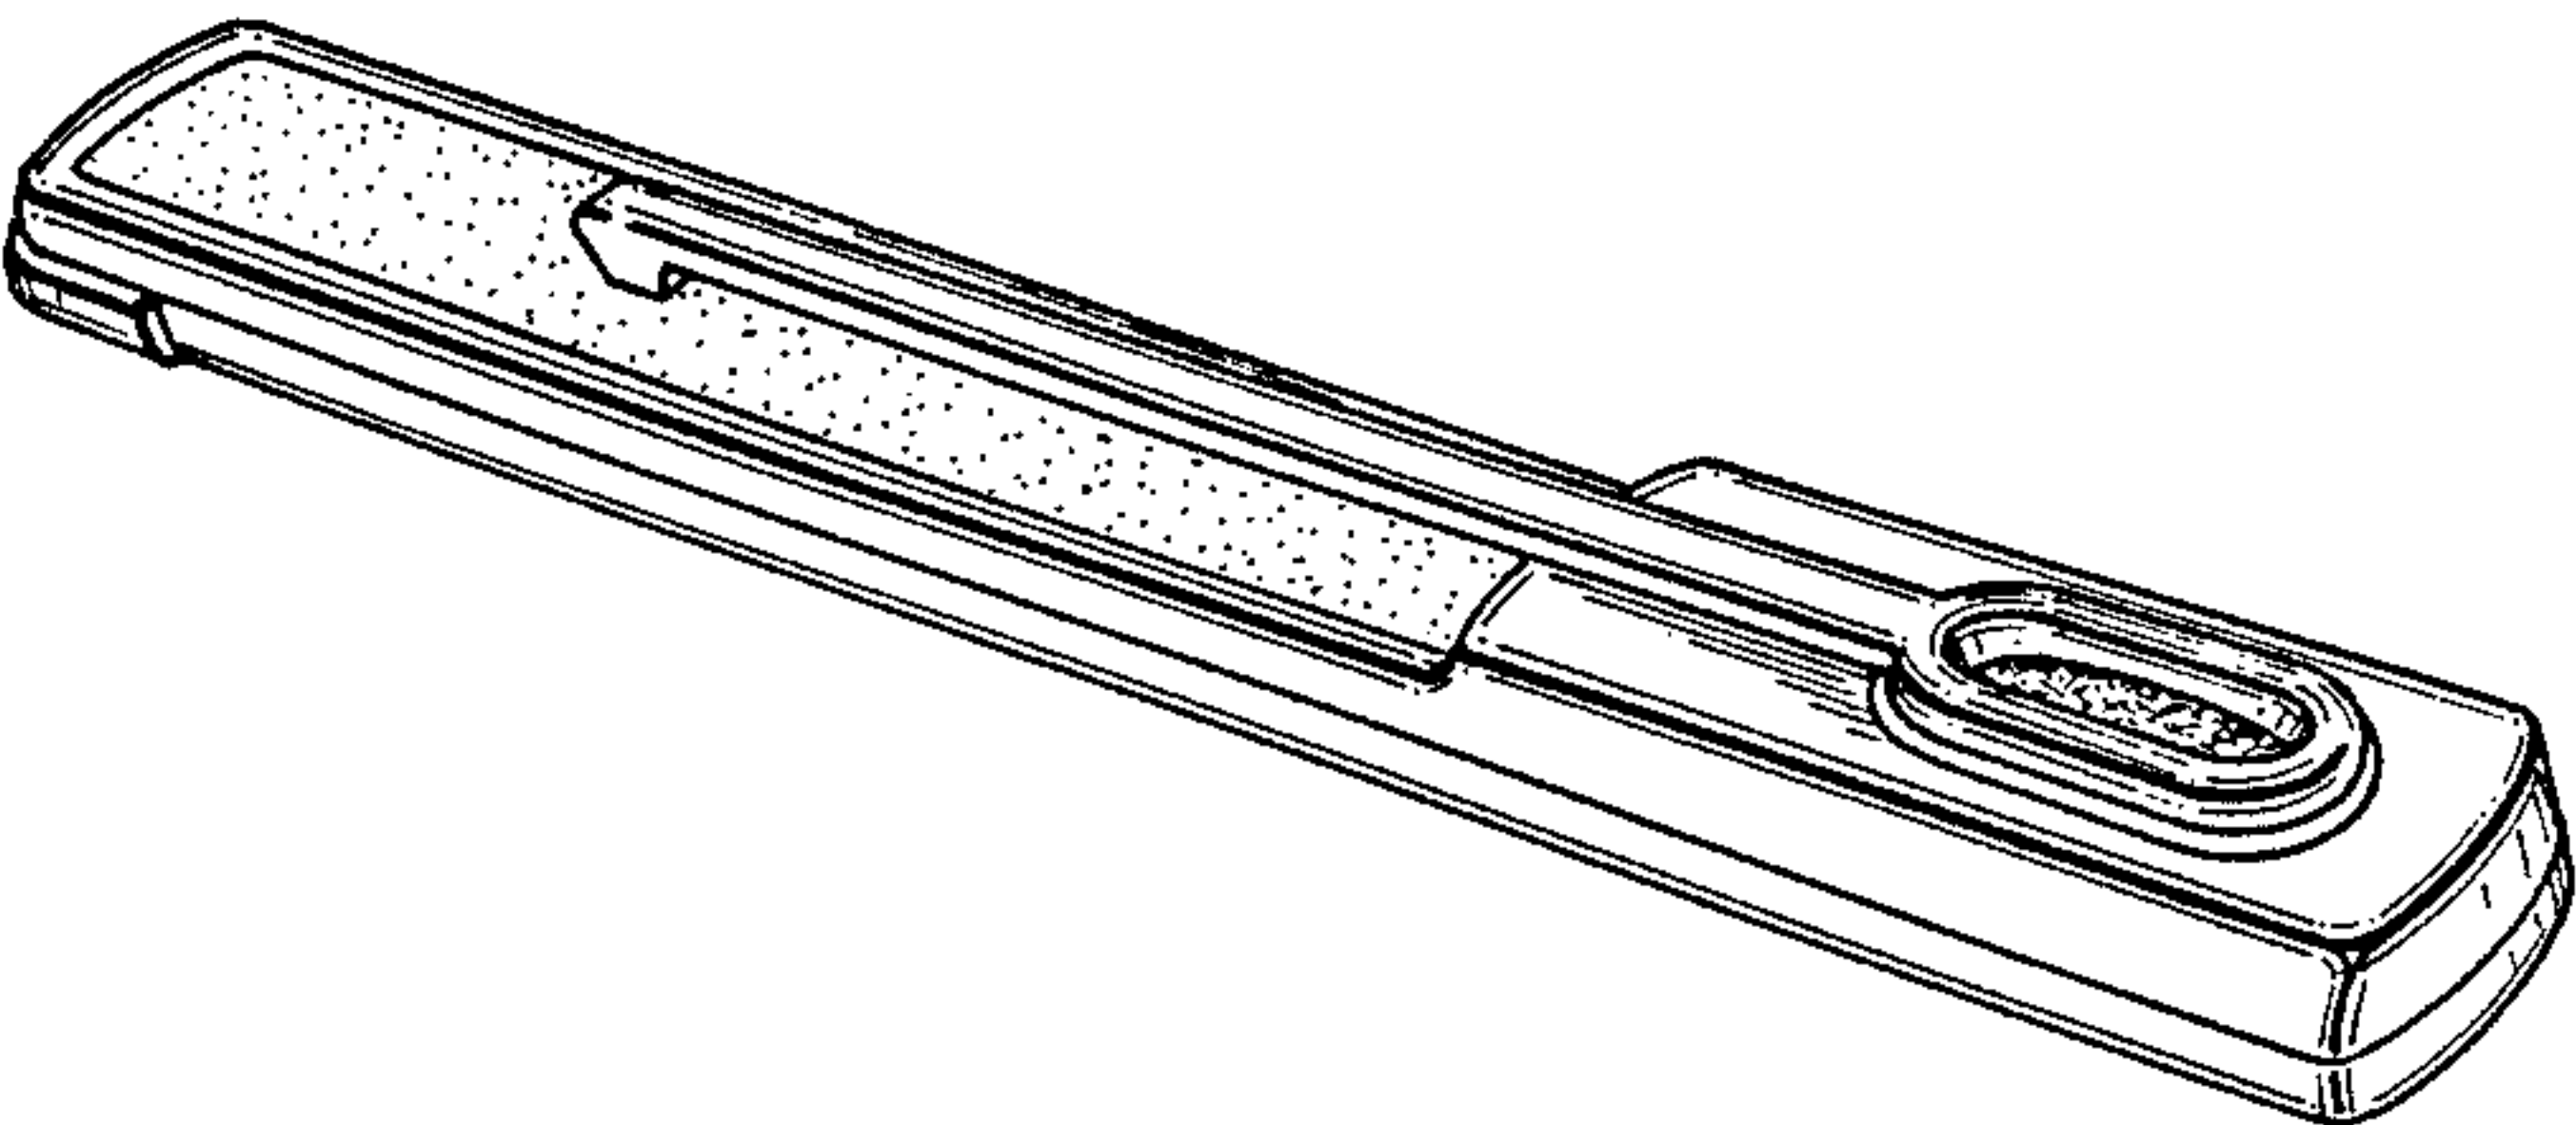


FIG-2



FIG-3



FIG-4

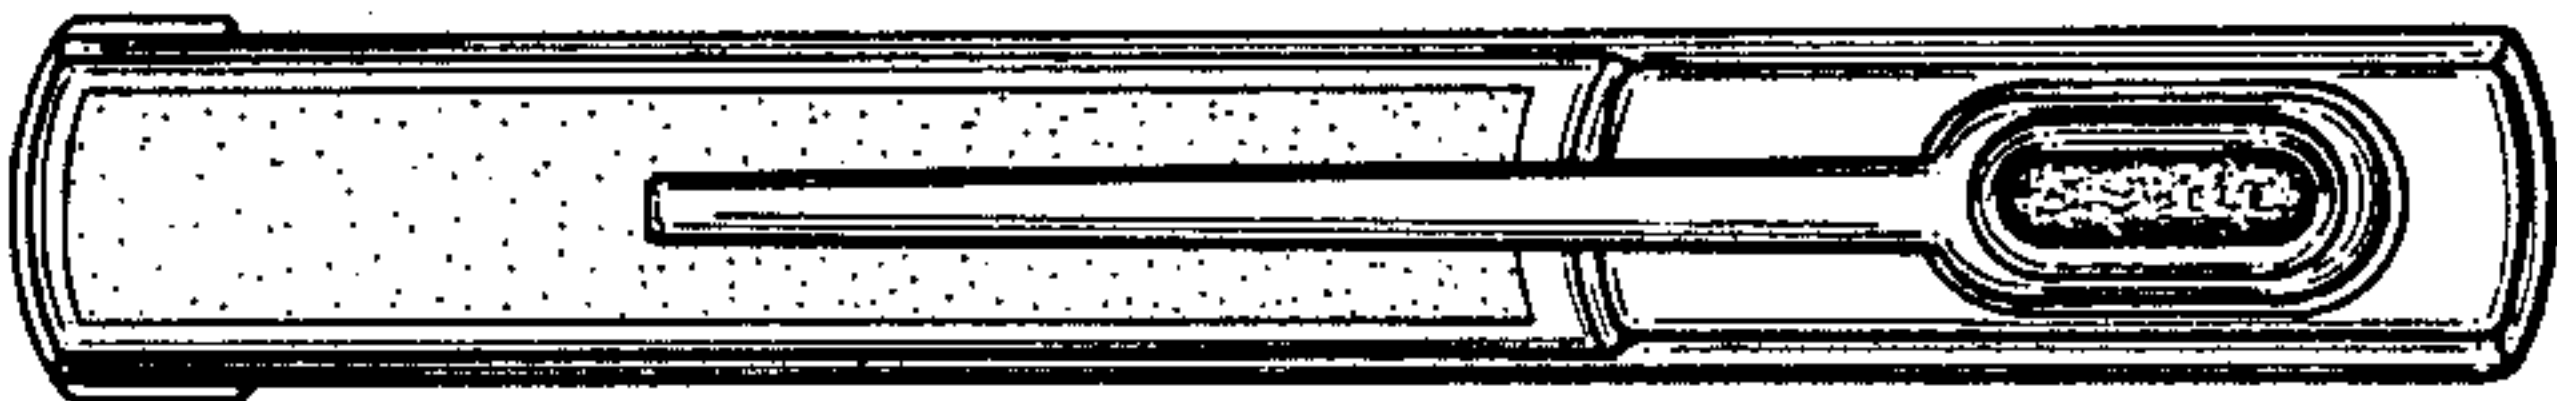


FIG-5

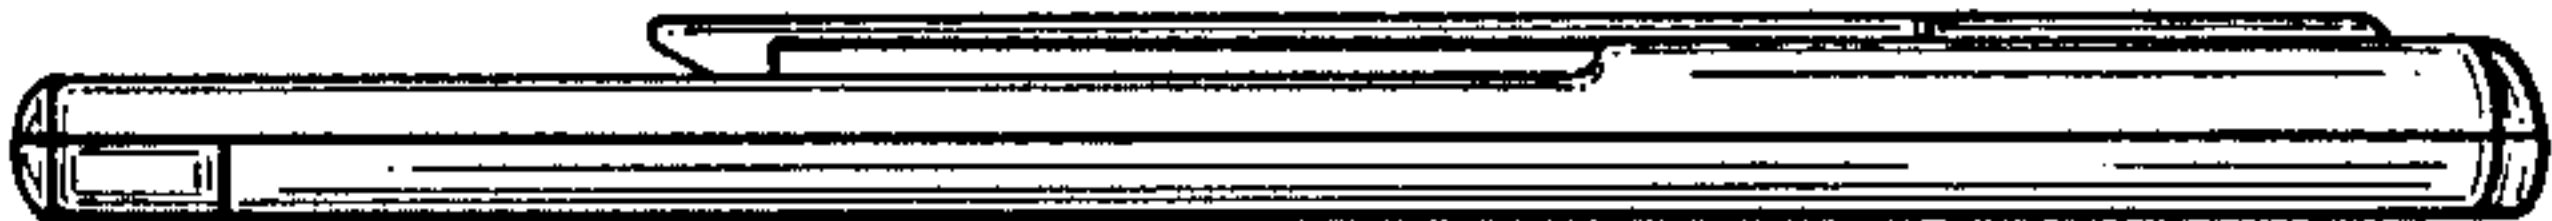


FIG-6

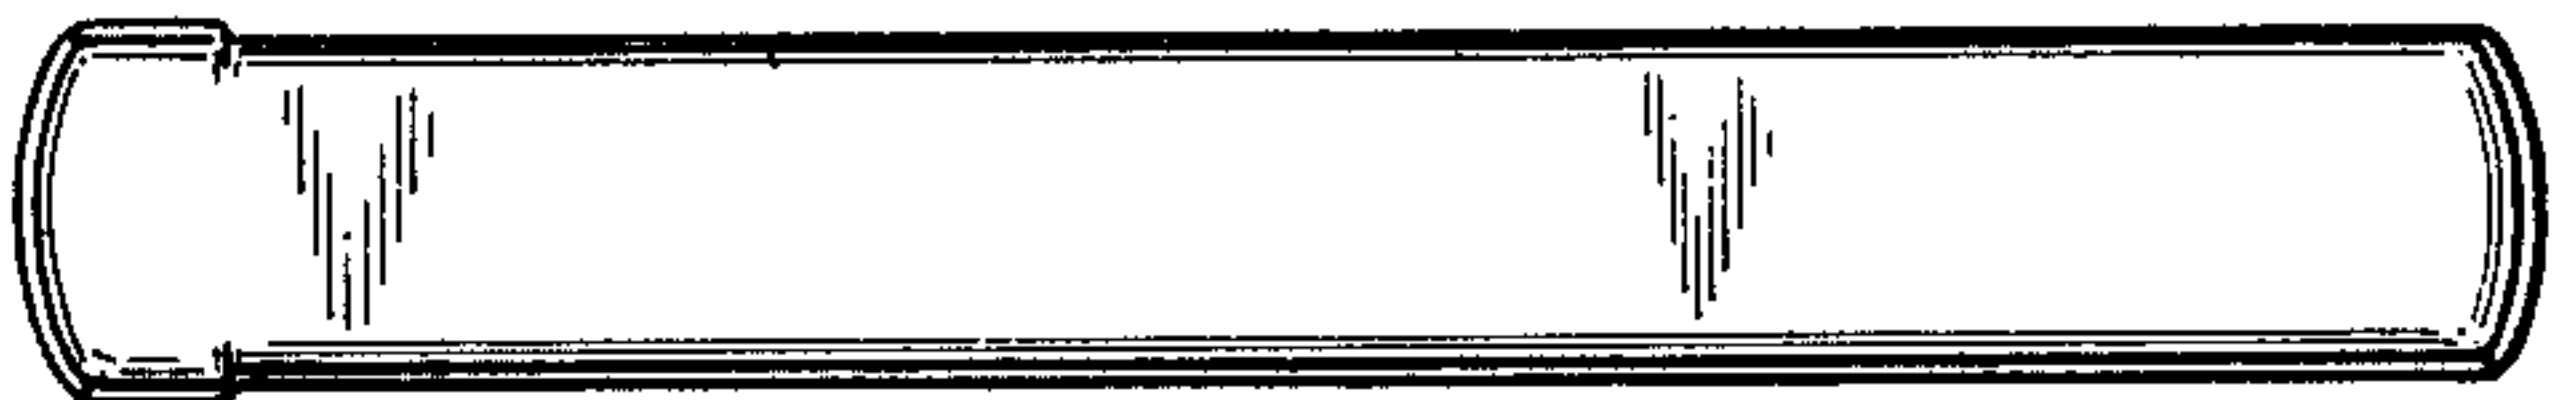


FIG-7

