

[54] BIOCHEMICAL ANALYZER

[75] Inventor: Masaharu Katayama, Tokyo, Japan

[73] Assignee: Kabushiki Kaisha Toshiba, Kawasaki, Japan

[\*\*] Term: 14 Years

[21] Appl. No.: 94,432

[22] Filed: Sep. 8, 1987

[30] Foreign Application Priority Data

Mar. 25, 1987 [JP] Japan ..... 62-10841

[52] U.S. Cl. .... D24/1.1

[58] Field of Search ..... D24/8, 1.1, 17;  
422/63-68; 436/43, 48

[56] References Cited

U.S. PATENT DOCUMENTS

- D. 264,873 6/1982 Olsen et al. .... D24/1.1
- D. 281,310 11/1985 Hattori et al. .... D24/1.1 X
- D. 282,203 1/1986 Leonard et al. .... D24/1.1
- 4,043,756 8/1977 Sommervold ..... 422/64 X
- 4,459,265 7/1984 Berglund ..... 422/64
- 4,483,823 11/1984 Umetsu et al. .... 422/64 X

OTHER PUBLICATIONS

Japanese Design Registration No. 573591, published

Mar. 27, 1982, "Biochemical Analyzer", Tokyo Shibaura Denki Kabushiki Kaisha.

Catalog of Hitachi Automatic Analyzer 7050.

Catalog of Olympus Automatic Analyzer AU 500.

Catalog of JEOL Biochemical Automatic Analyzer JCA-VX 1000.

Primary Examiner—A. Hugo Word

Assistant Examiner—Stella M. Reid

Attorney, Agent, or Firm—Oblon, Spivak, McClelland, Maier & Neustadt

[57] CLAIM

The ornamental design for a biochemical analyzer, as shown and described.

DESCRIPTION

FIG. 1 is a top, front and right side perspective view of a biochemical analyzer showing my new design, with the cover shown open;


FIG. 2 is a front elevational view thereof;

FIG. 3 is a right side elevational view thereof with the cover shown closed, the left side being a mirror image of the right;

FIG. 4 is a top plan view thereof;

FIG. 5 is a rear elevational view thereof; and

FIG. 6 is a bottom plan view thereof.

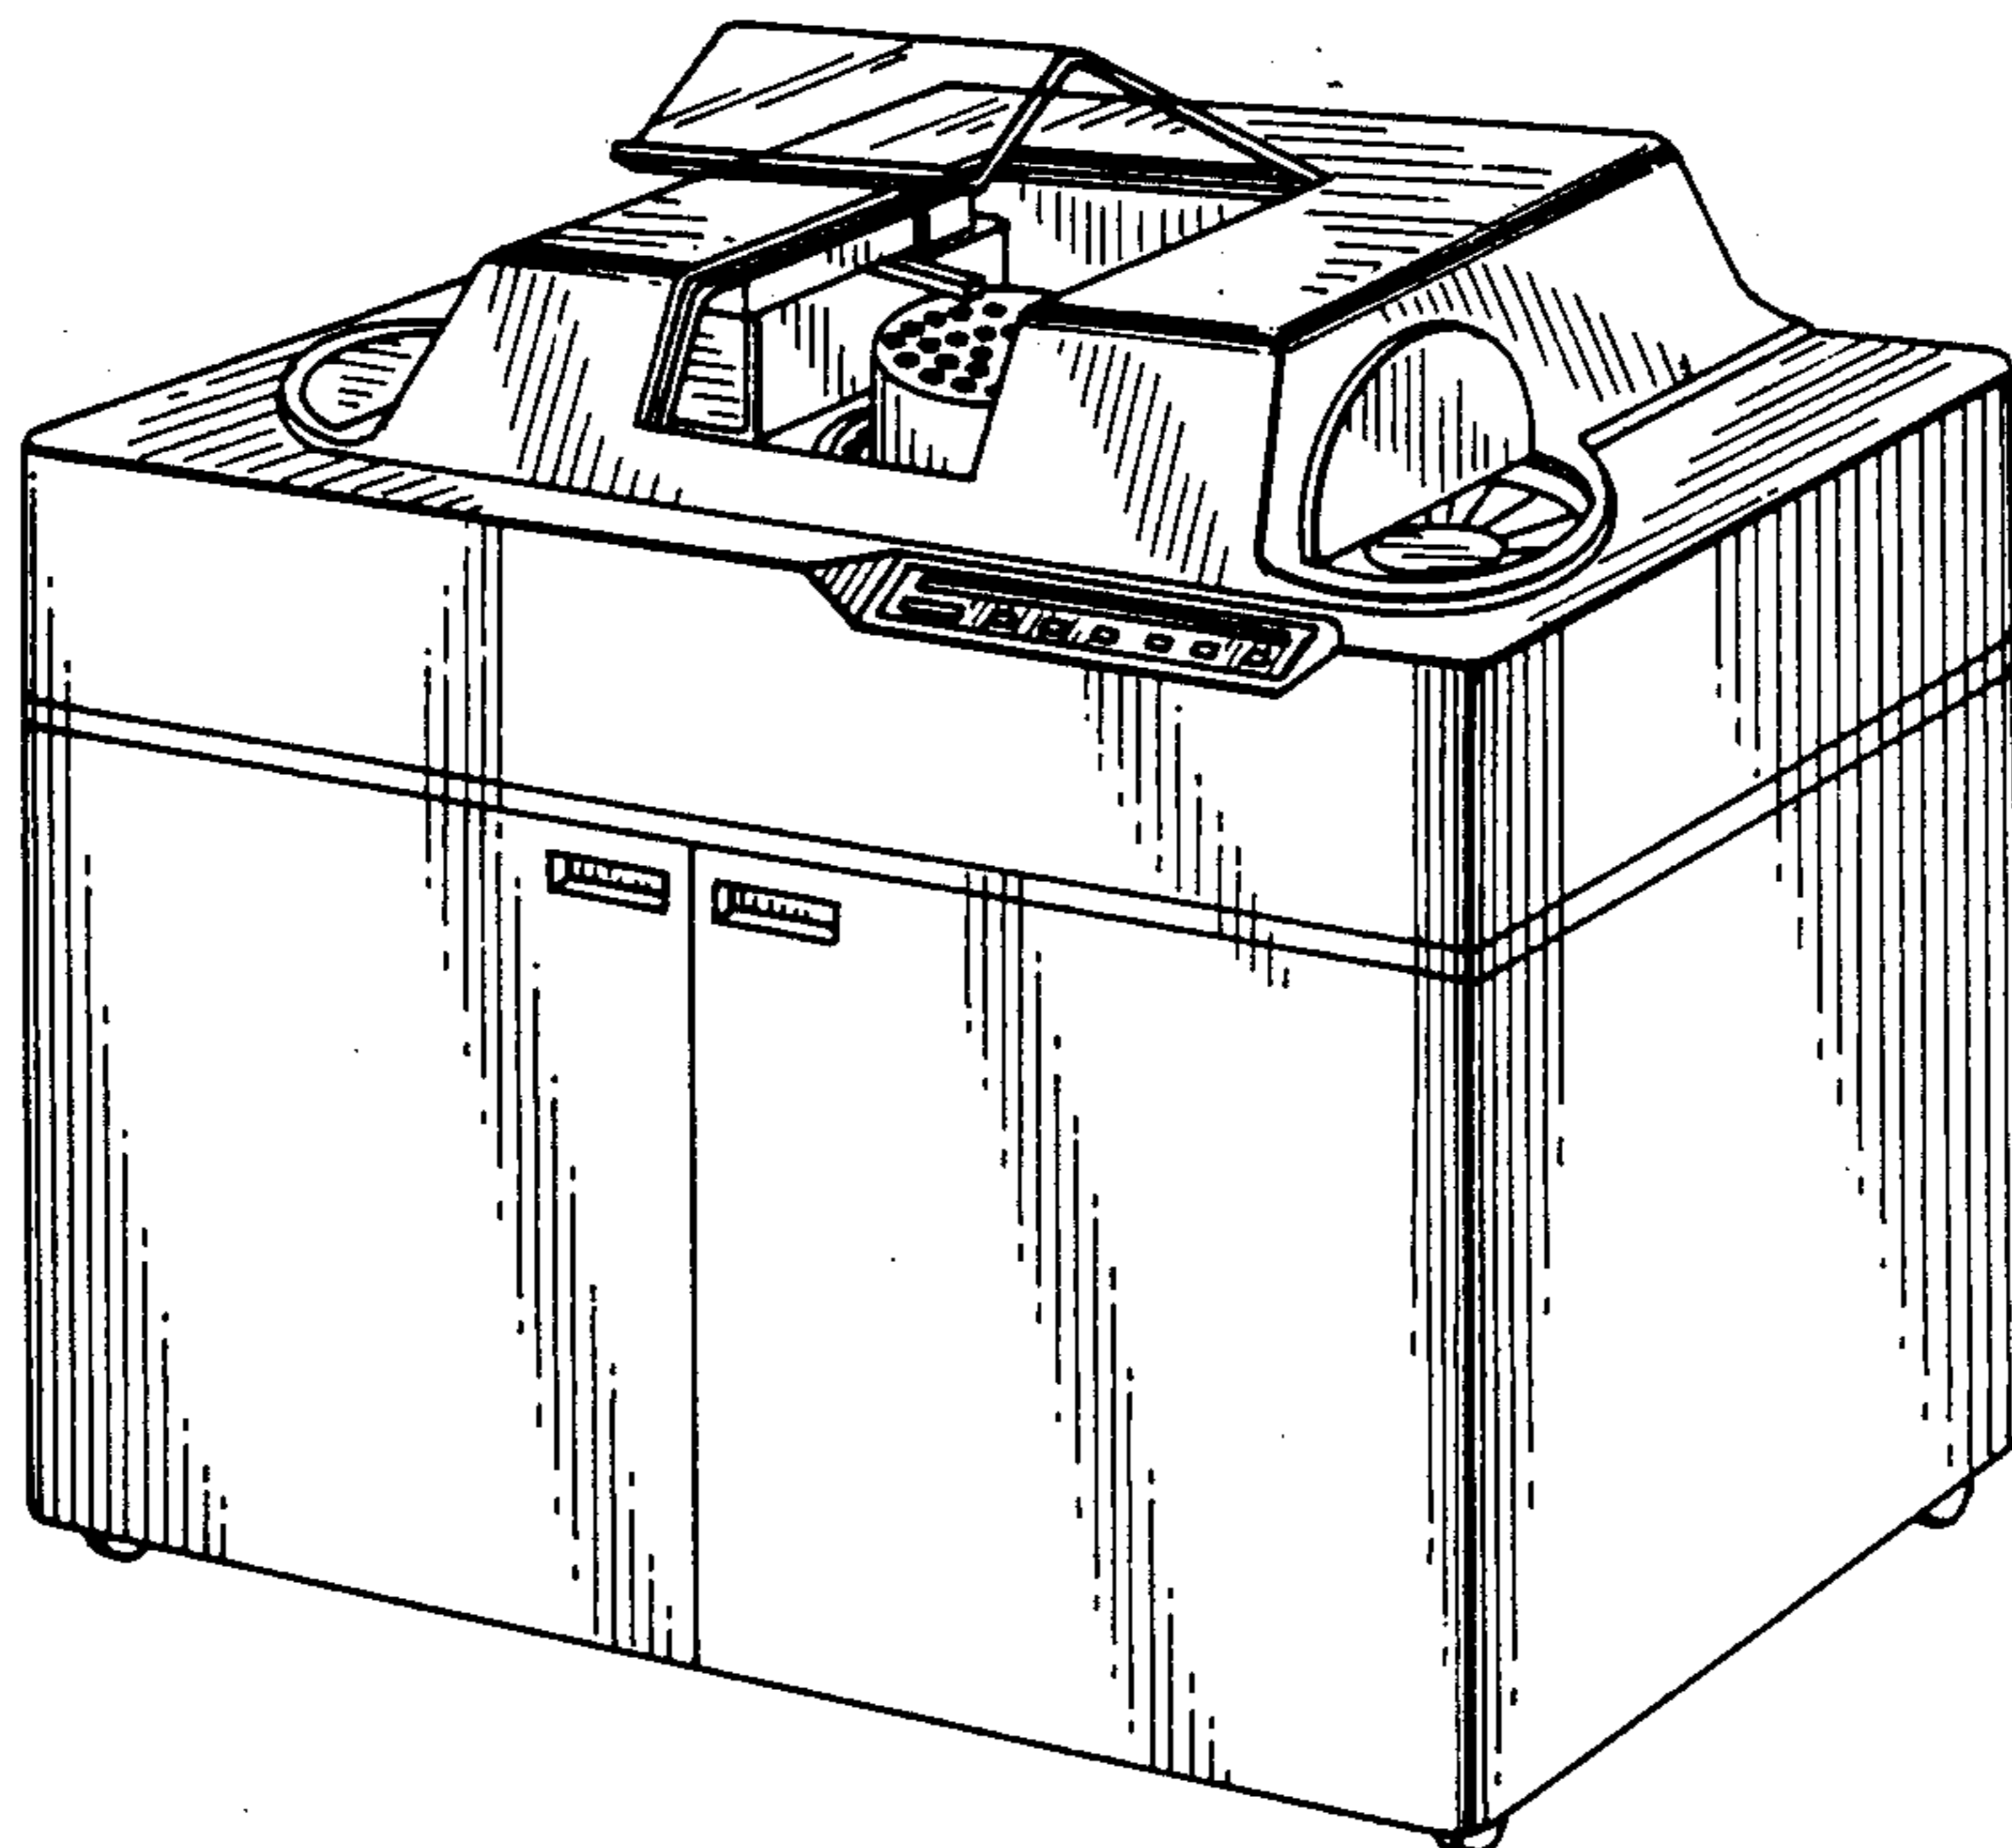

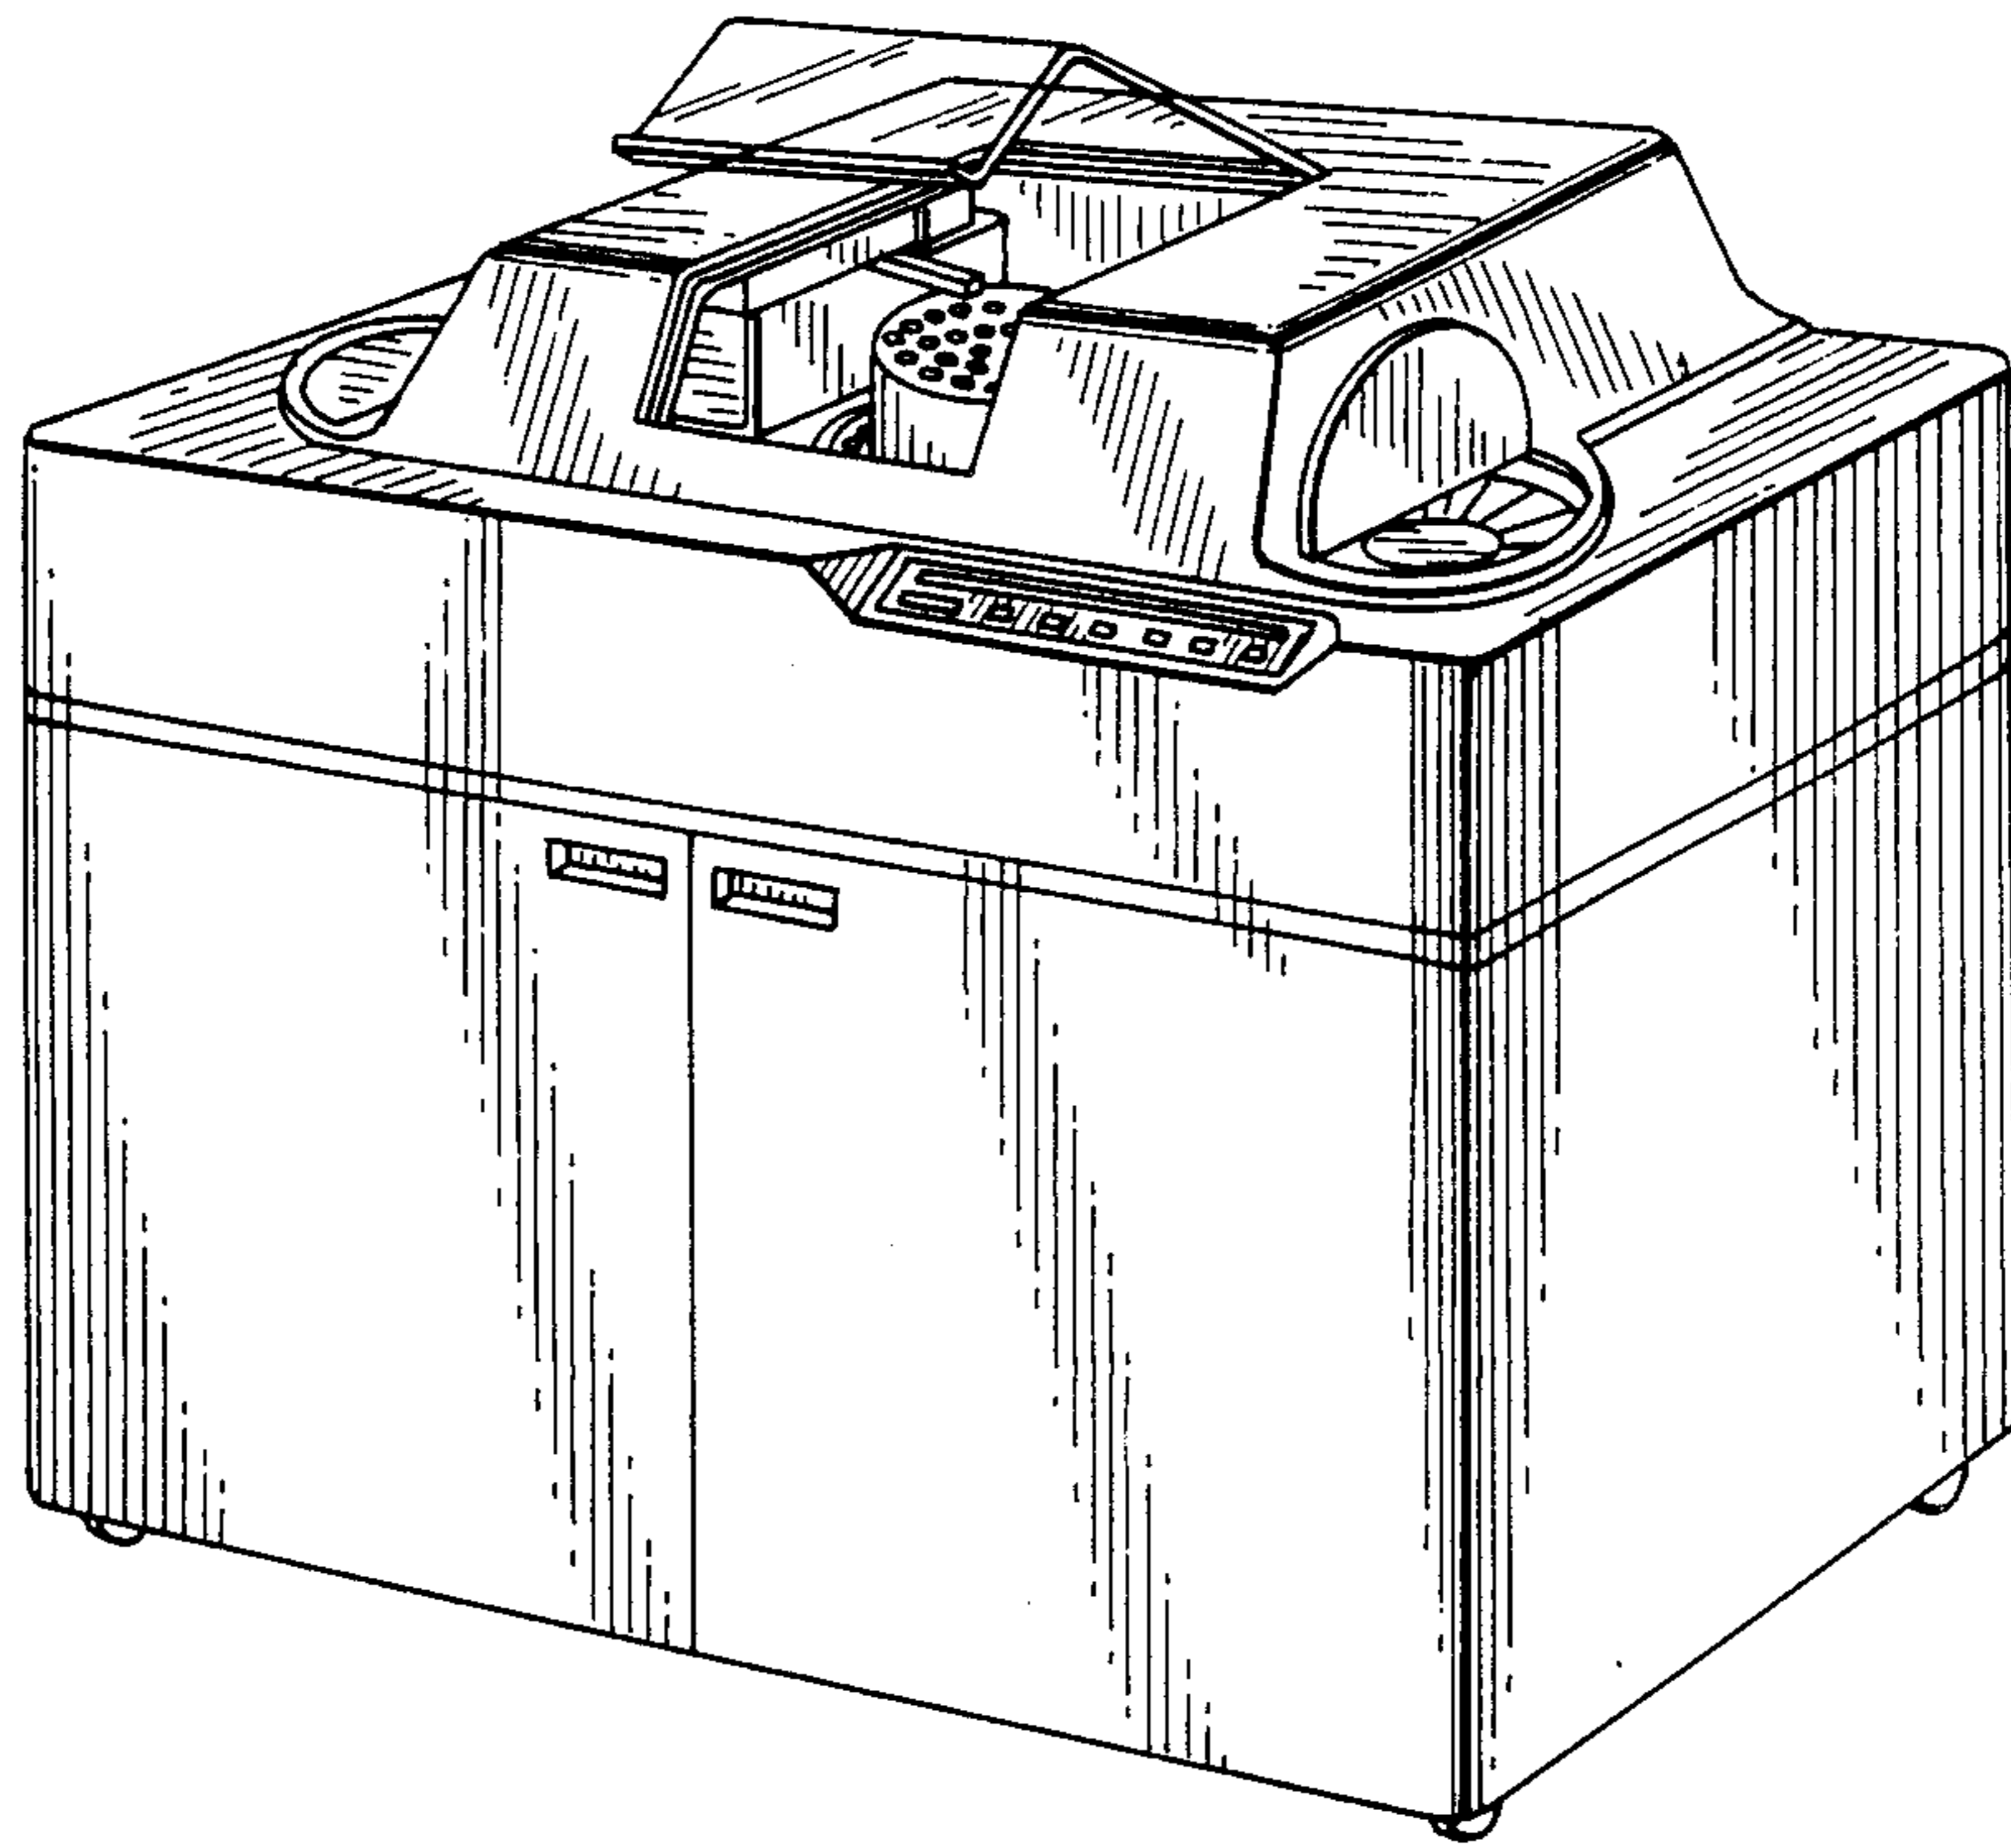


FIG. 1

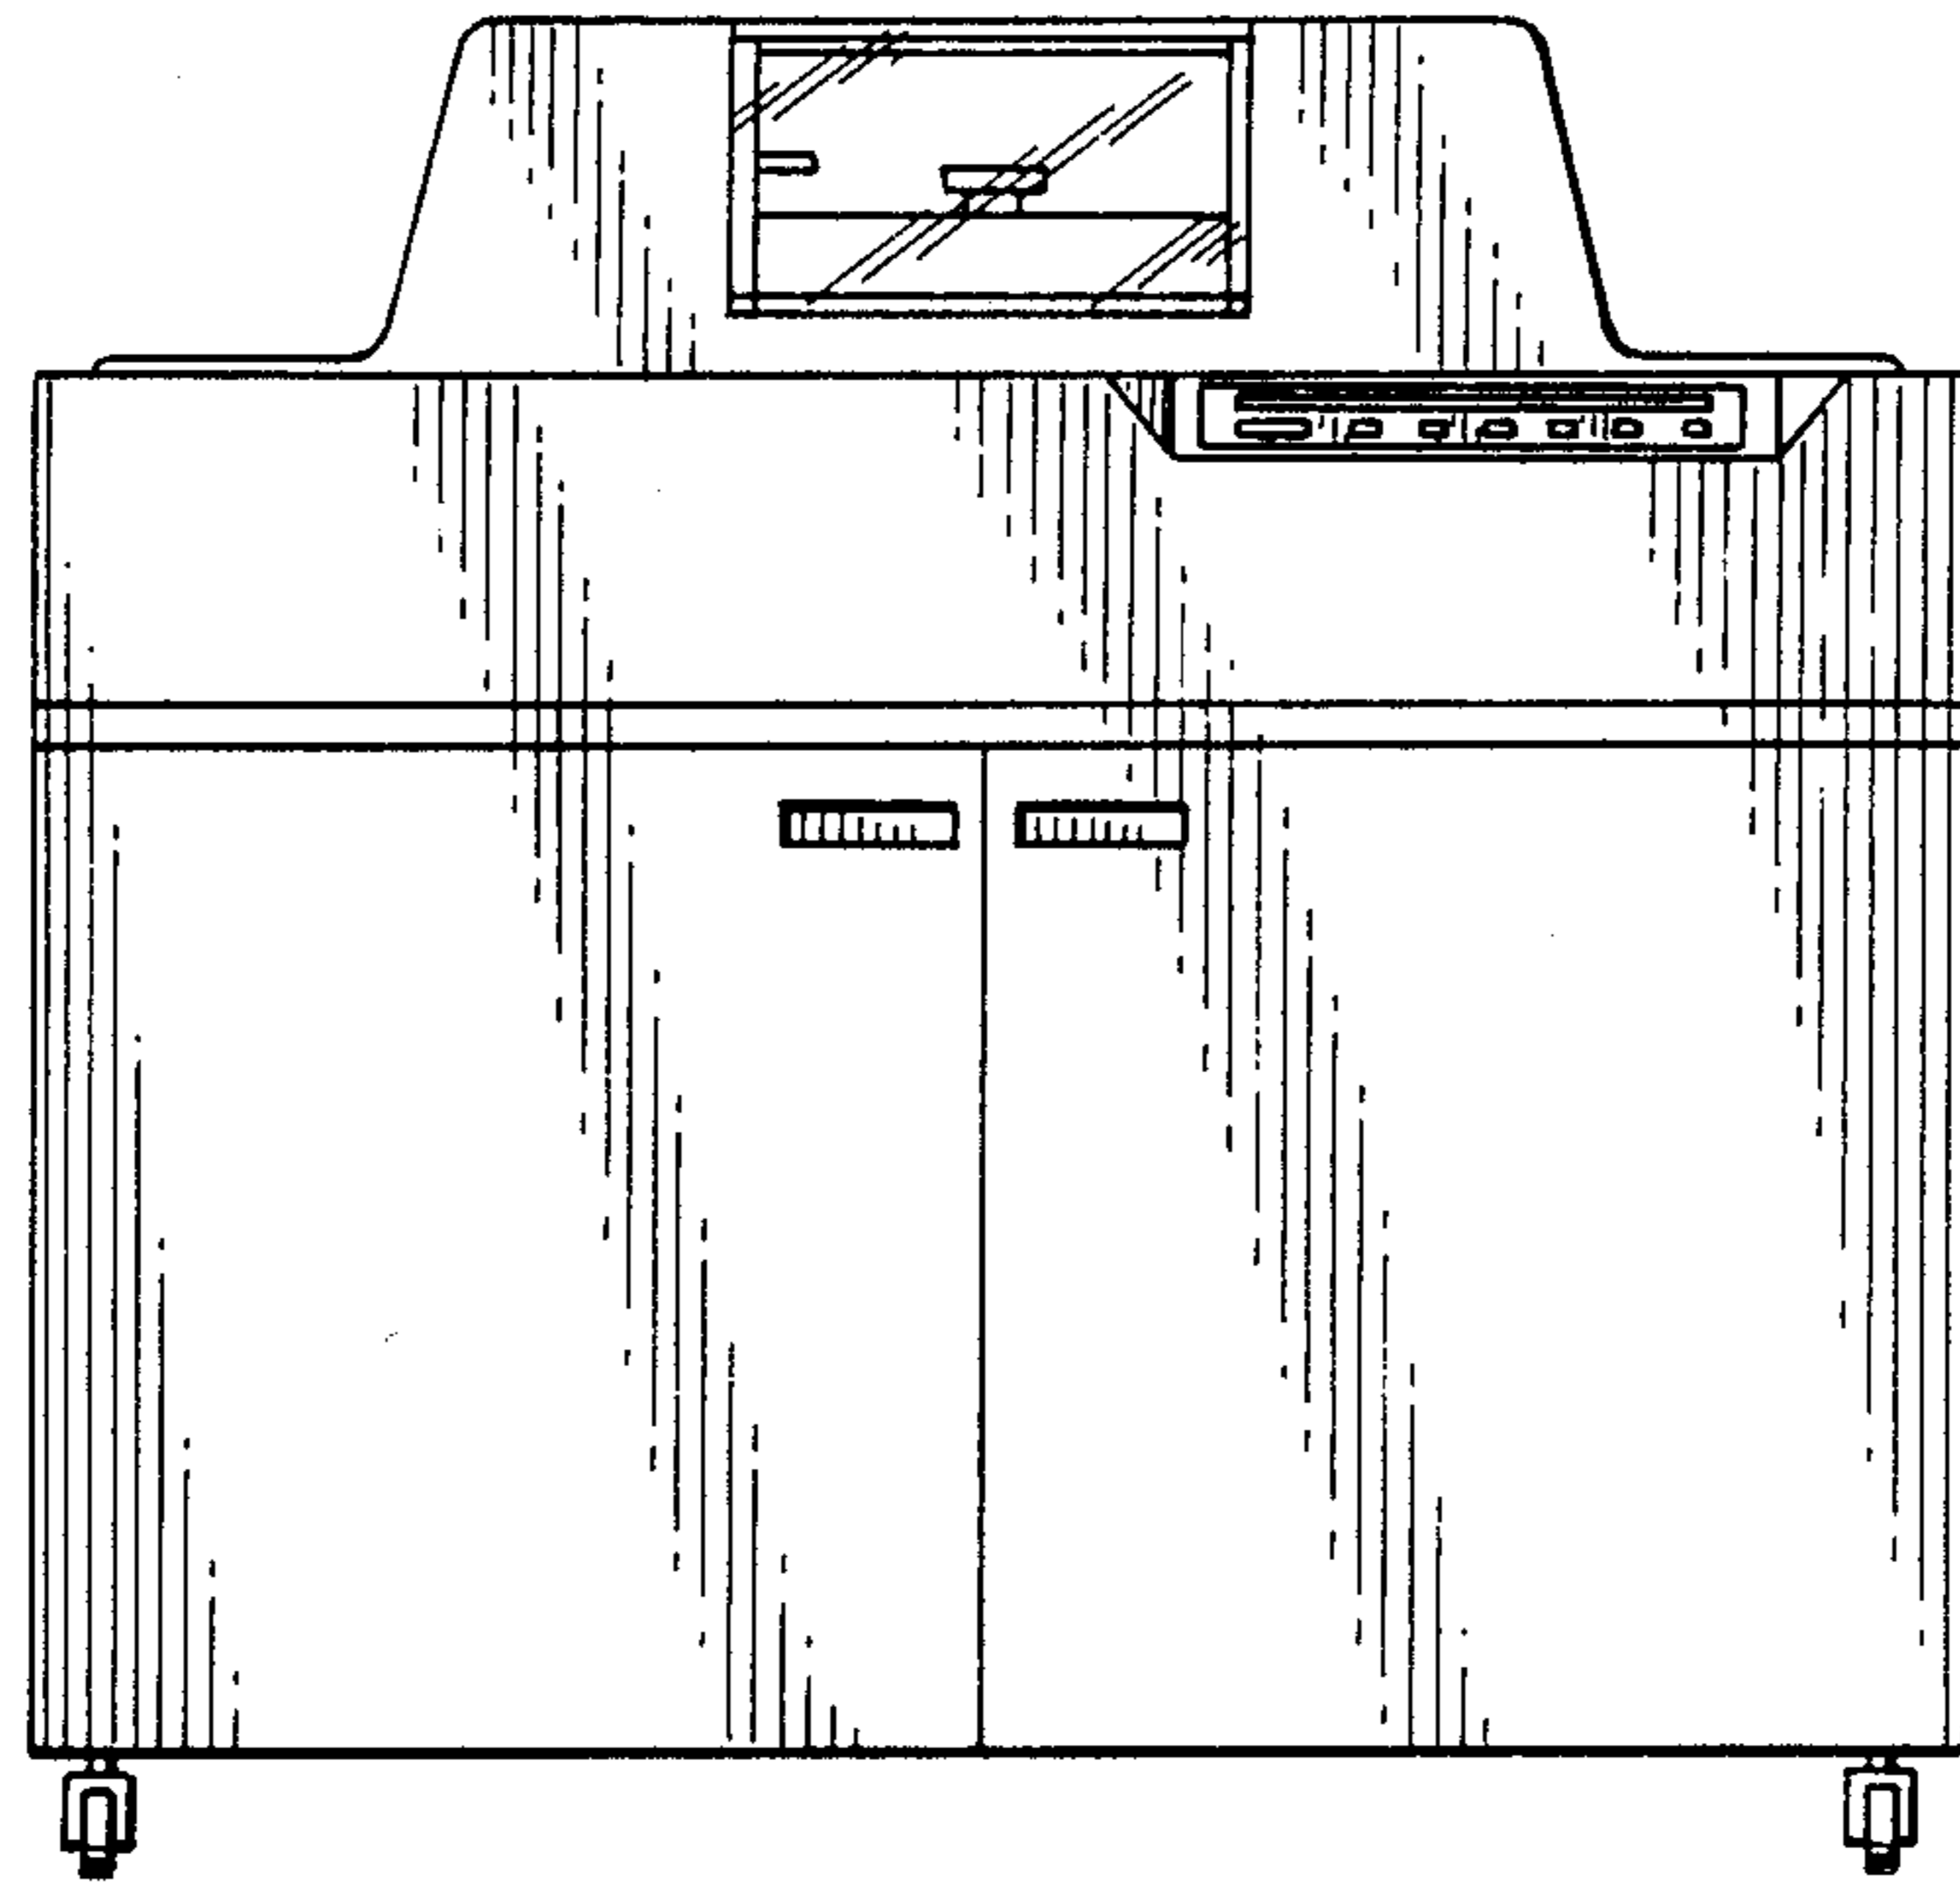
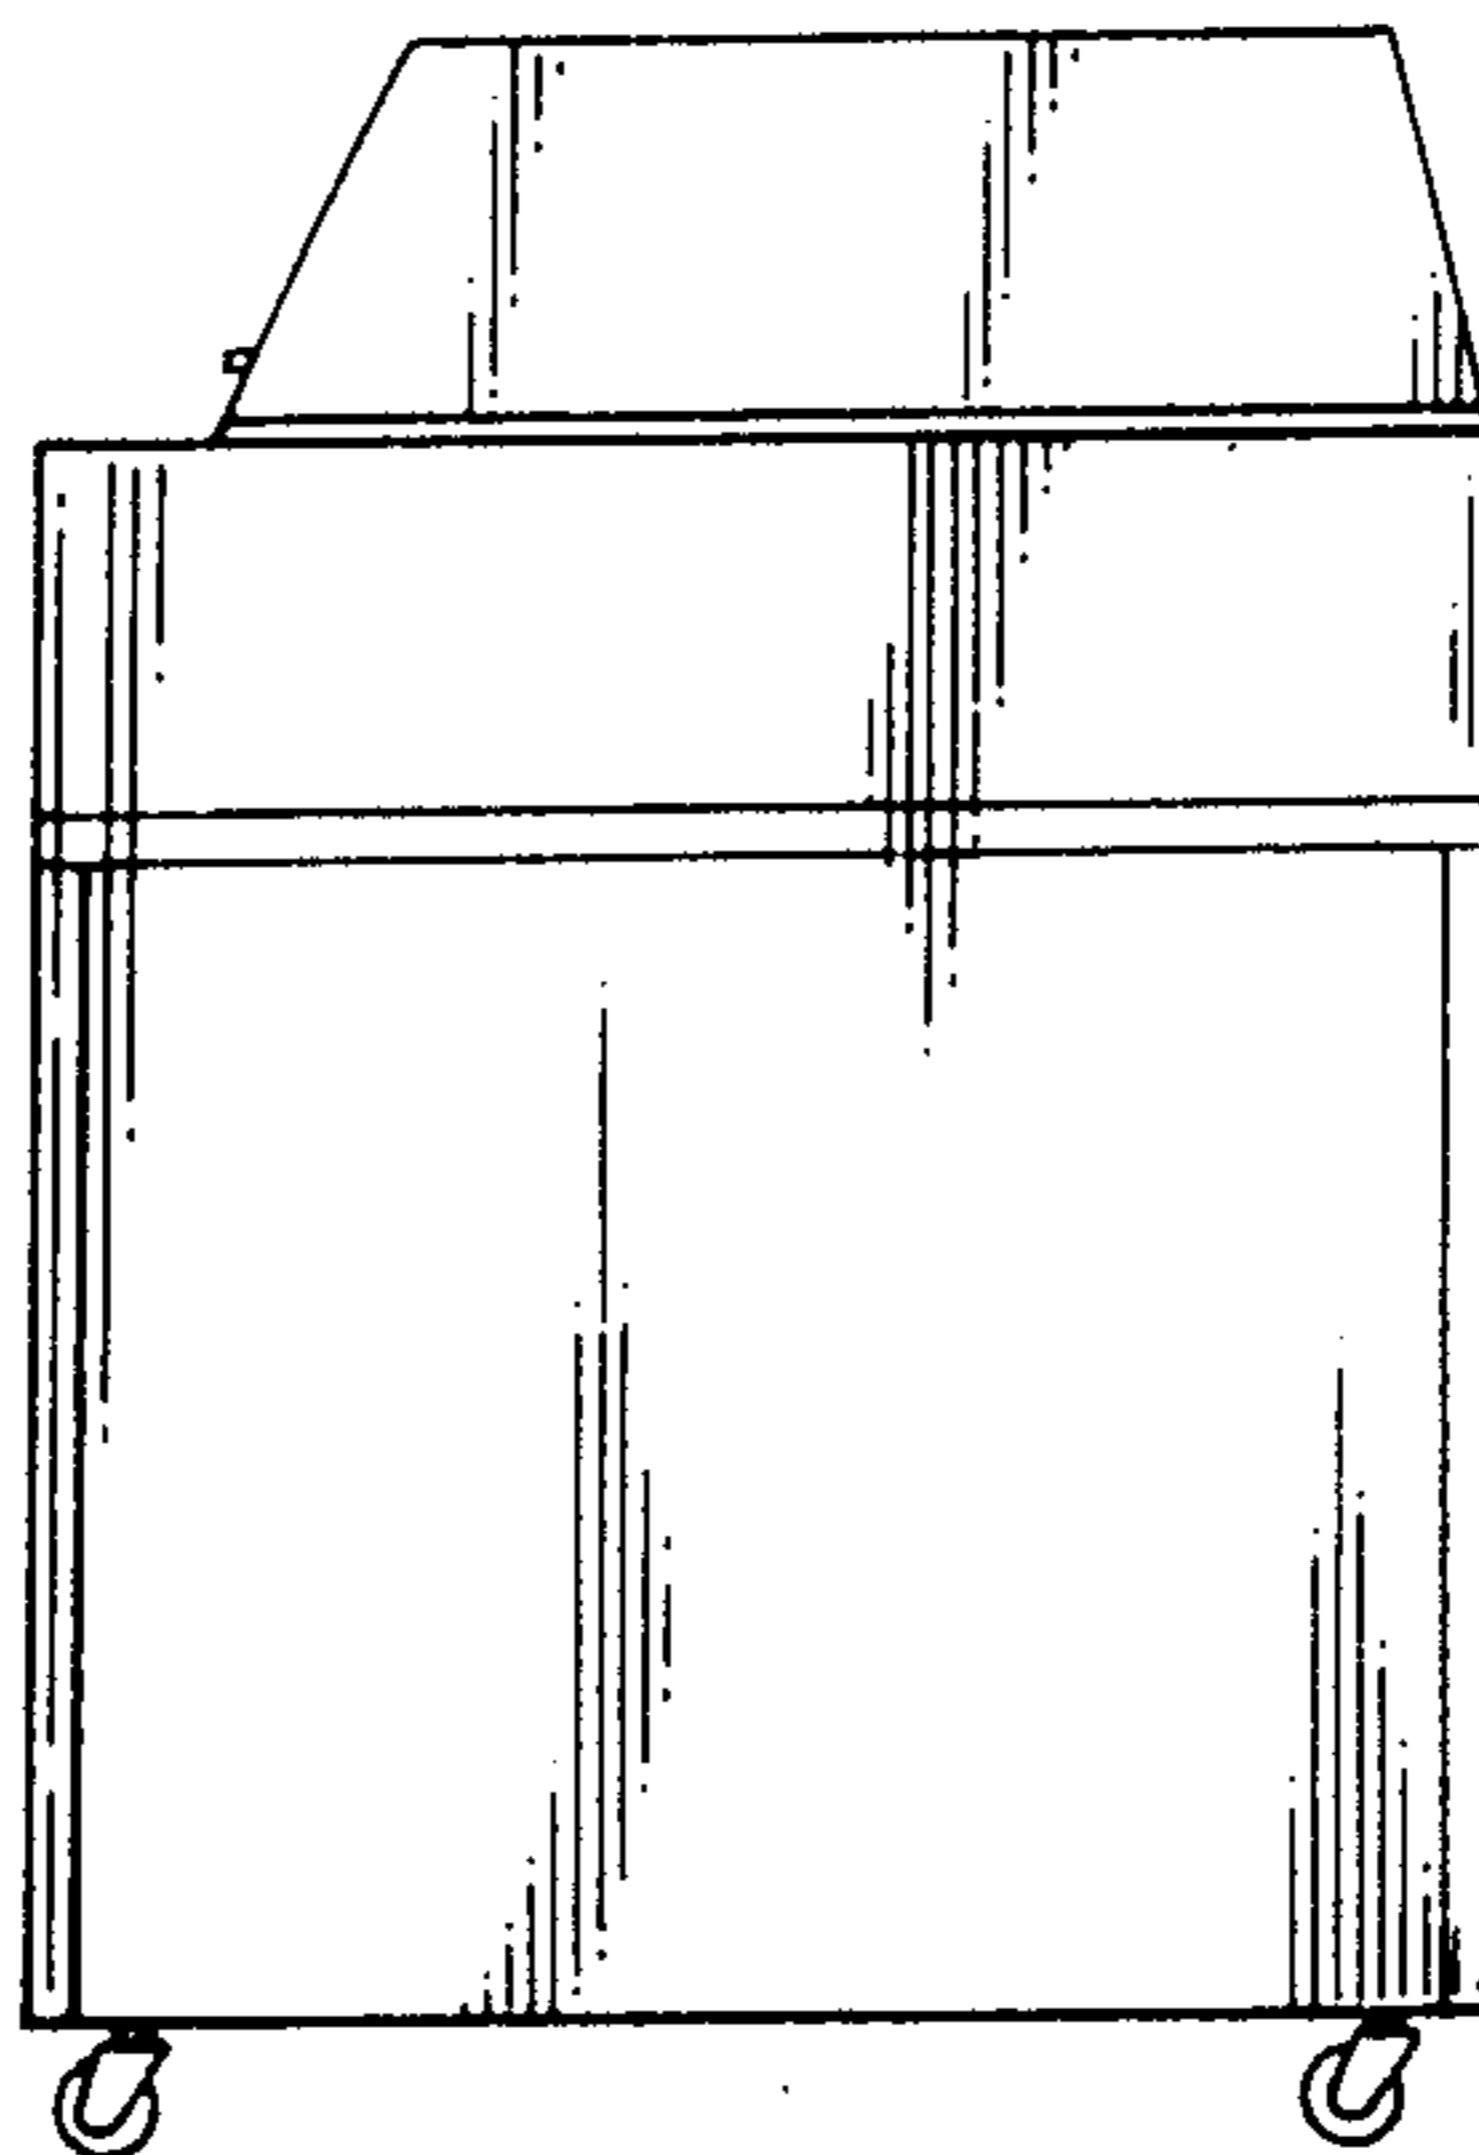


FIG. 2

FIG. 3



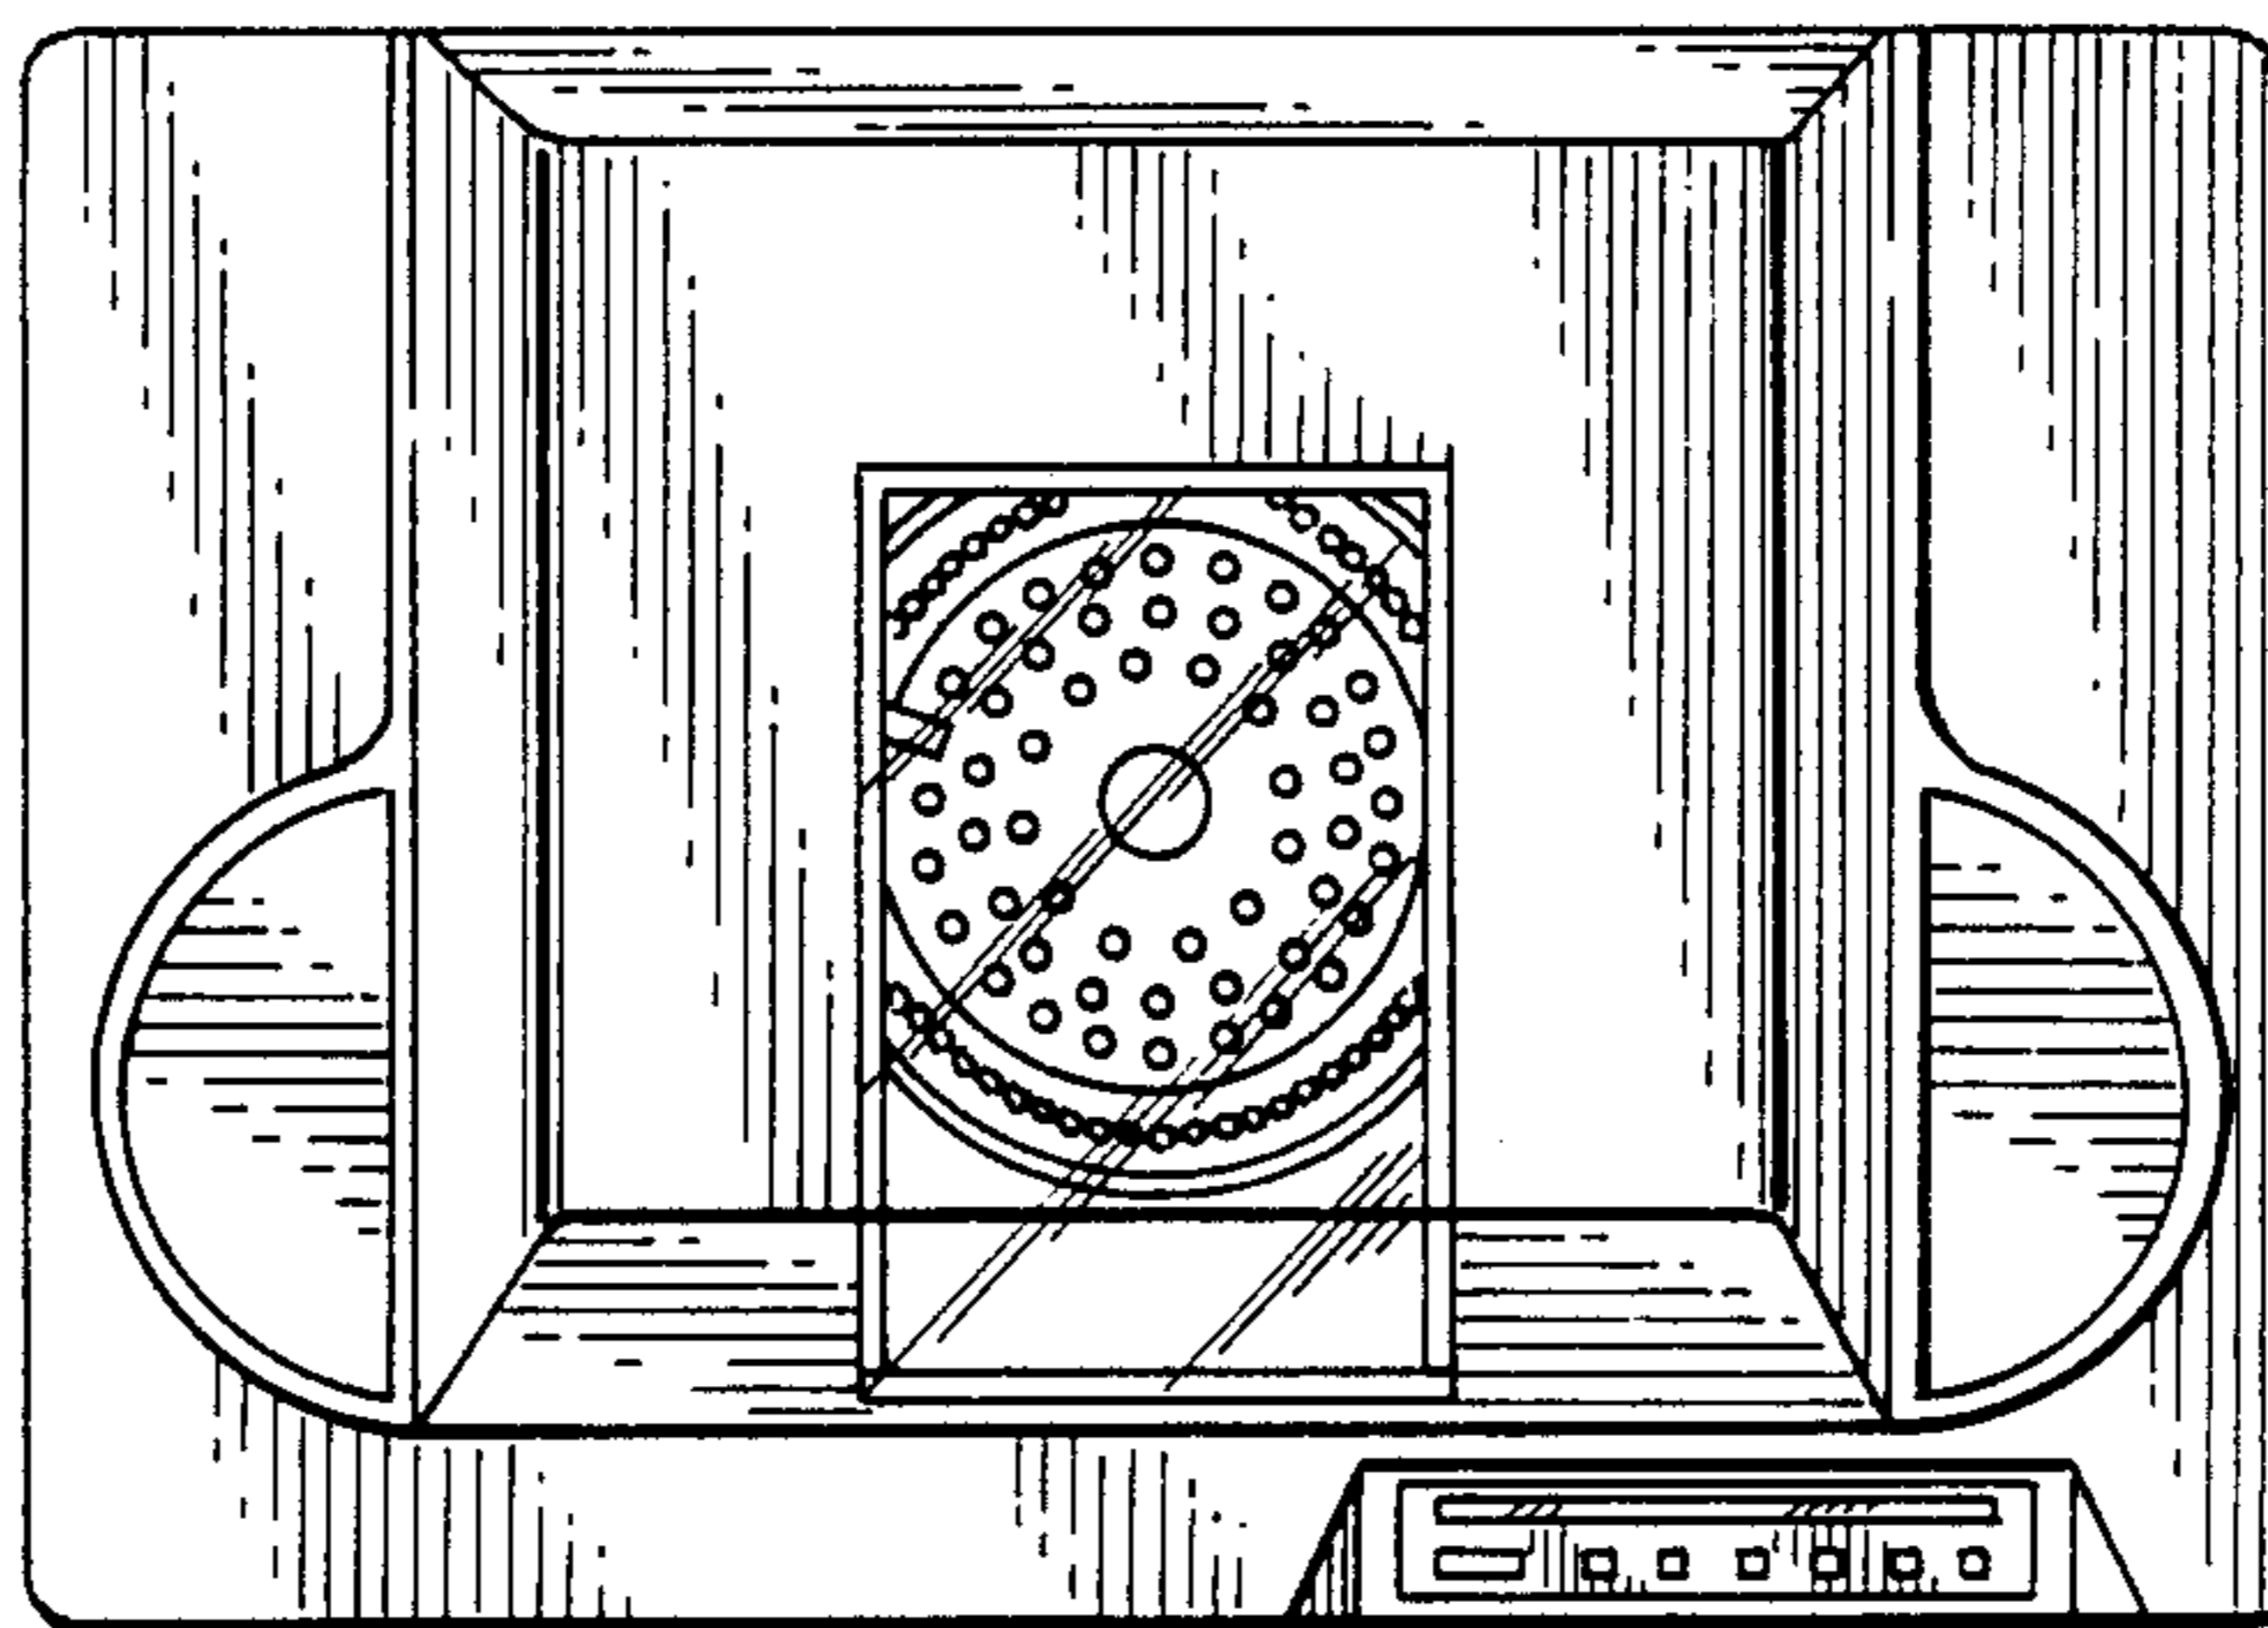


FIG. 4

FIG. 5

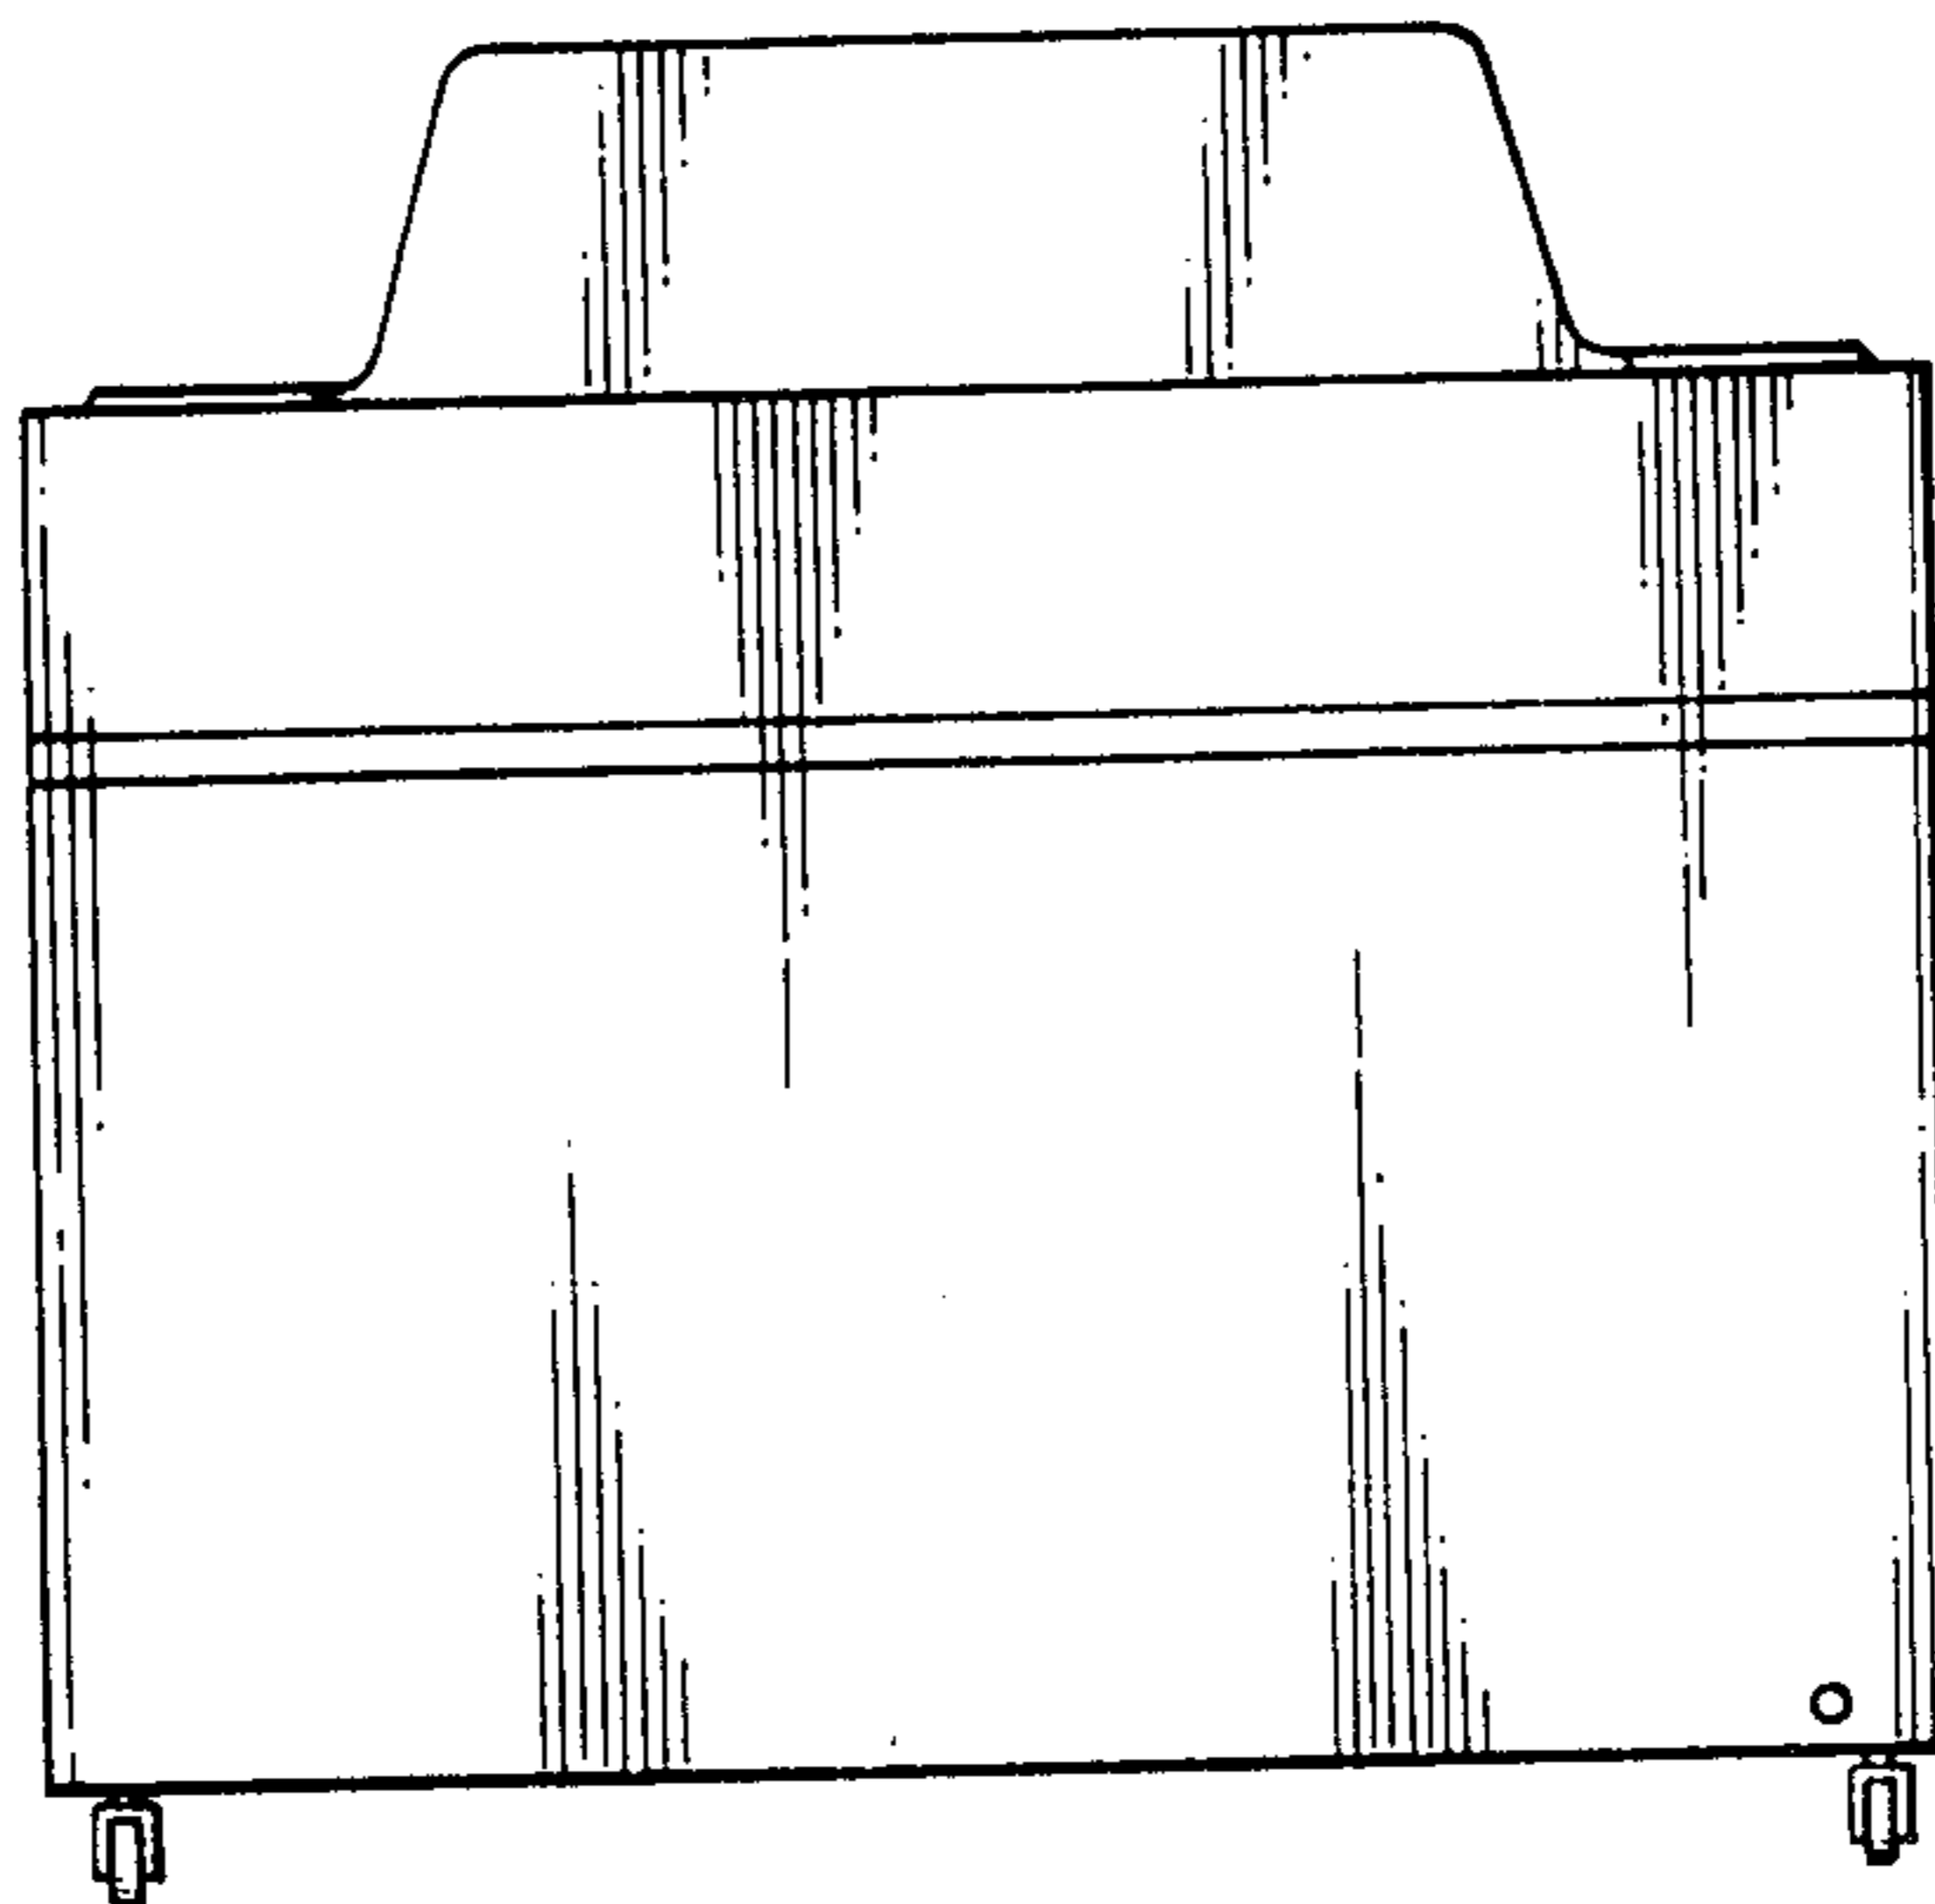


FIG. 6

