

[54] DETECTOR FOR USE IN MONITORING  
EMPTY INTRAVENOUS INFUSION  
CONTAINERS

4,759,756 7/1988 Forman et al. .... D24/53  
4,922,226 5/1990 Hsieh et al. .... 340/612

[75] Inventor: Michael R. Aten, San Diego, Calif.

Primary Examiner—Wallace R. Burke  
Assistant Examiner—Marcus Jackson  
Attorney, Agent, or Firm—Nydegger & Associates

[73] Assignee: Imed Corporation, San Diego, Calif.

[\*\*] Term: 14 Years

[57] CLAIM

[21] Appl. No.: 299,743

The ornamental design for detector for use in monitoring empty intravenous infusion containers, as shown and described.

[22] Filed: Jan. 19, 1989

[52] U.S. Cl. .... D24/51

[58] Field of Search ..... D10/104, 106, 121, 109;  
340/612, 618, 621, 689, 242, 244, 6212;  
367/908; D24/51, 52, 53; 285/114, 405, 420;  
604/253, 251

DESCRIPTION

FIG. 1 is a front elevational view of a detector for use in monitoring empty intravenous infusion container showing my new design;

FIG. 2 is a right side elevational view with the left side being a mirror image thereof;

FIG. 3 is a top plan view thereof;

FIG. 4 is a bottom plan view thereof;

FIG. 5 is a rear elevational view thereof;


FIG. 6 is a front perspective view thereof; and

FIG. 7 is a rear perspective view thereof.

[56] References Cited

U.S. PATENT DOCUMENTS

D. 283,441 4/1986 Vcelka et al. .... D24/53  
2,706,755 4/1955 Krasno ..... 340/613  
3,838,691 10/1974 Paludan et al. .... D24/53

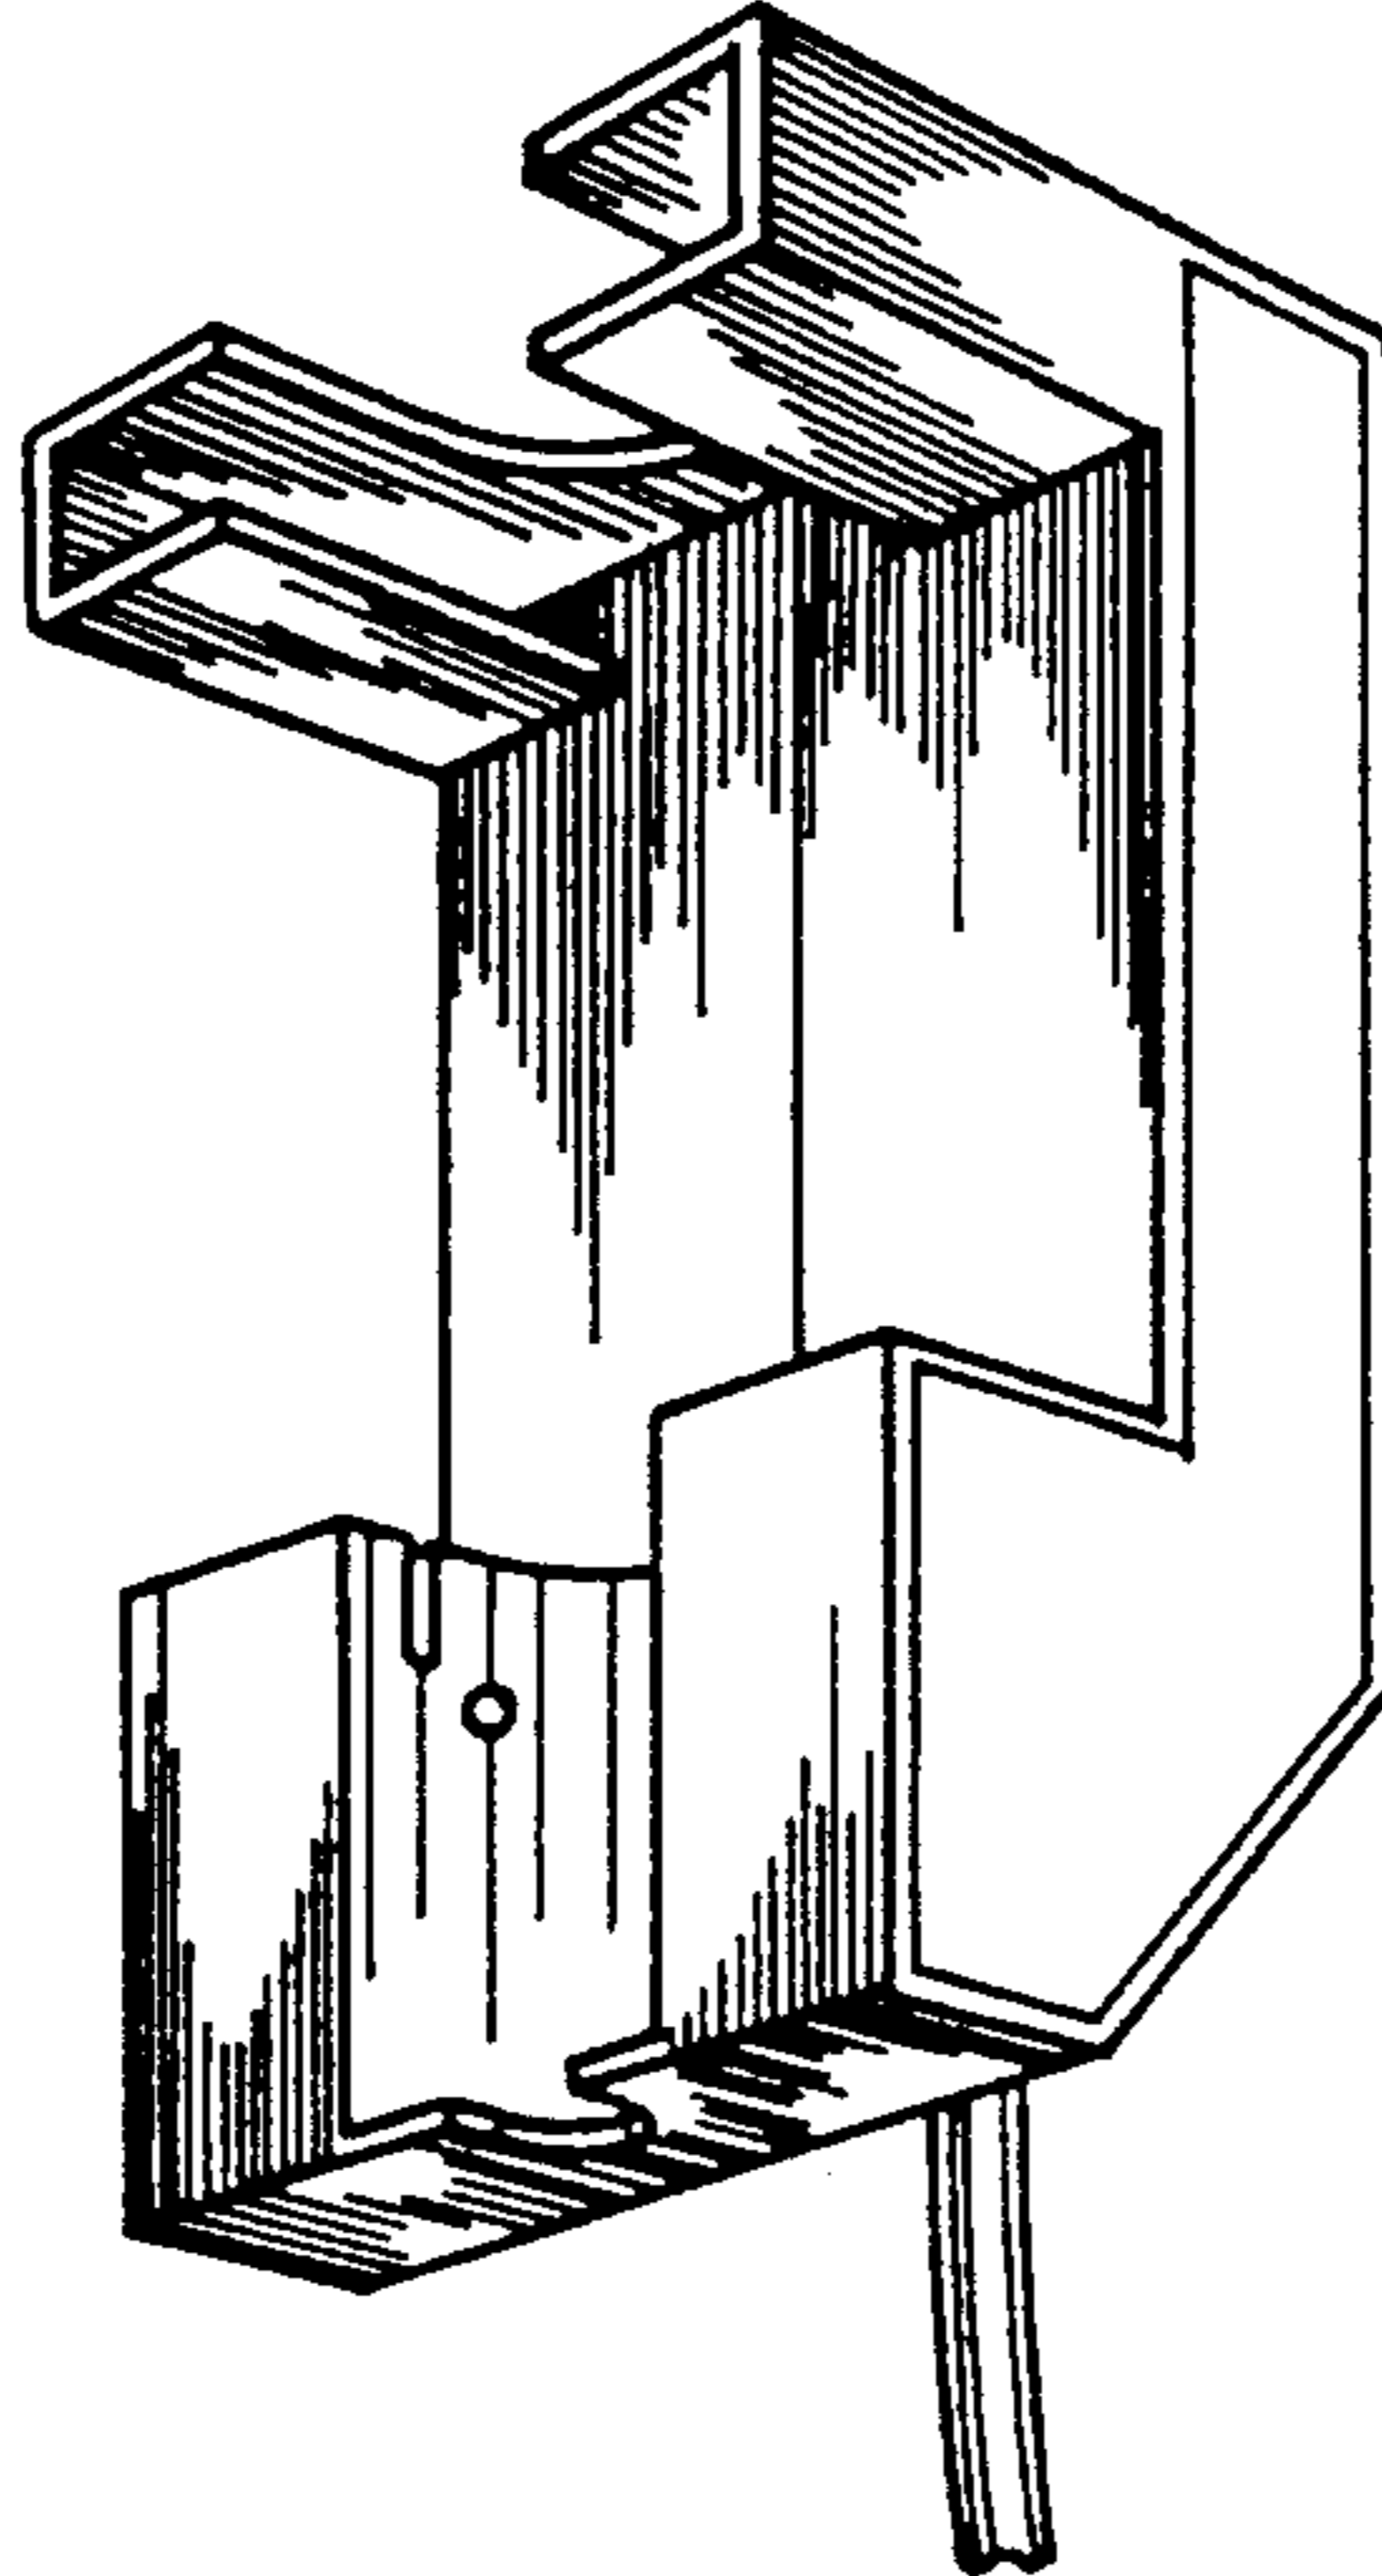

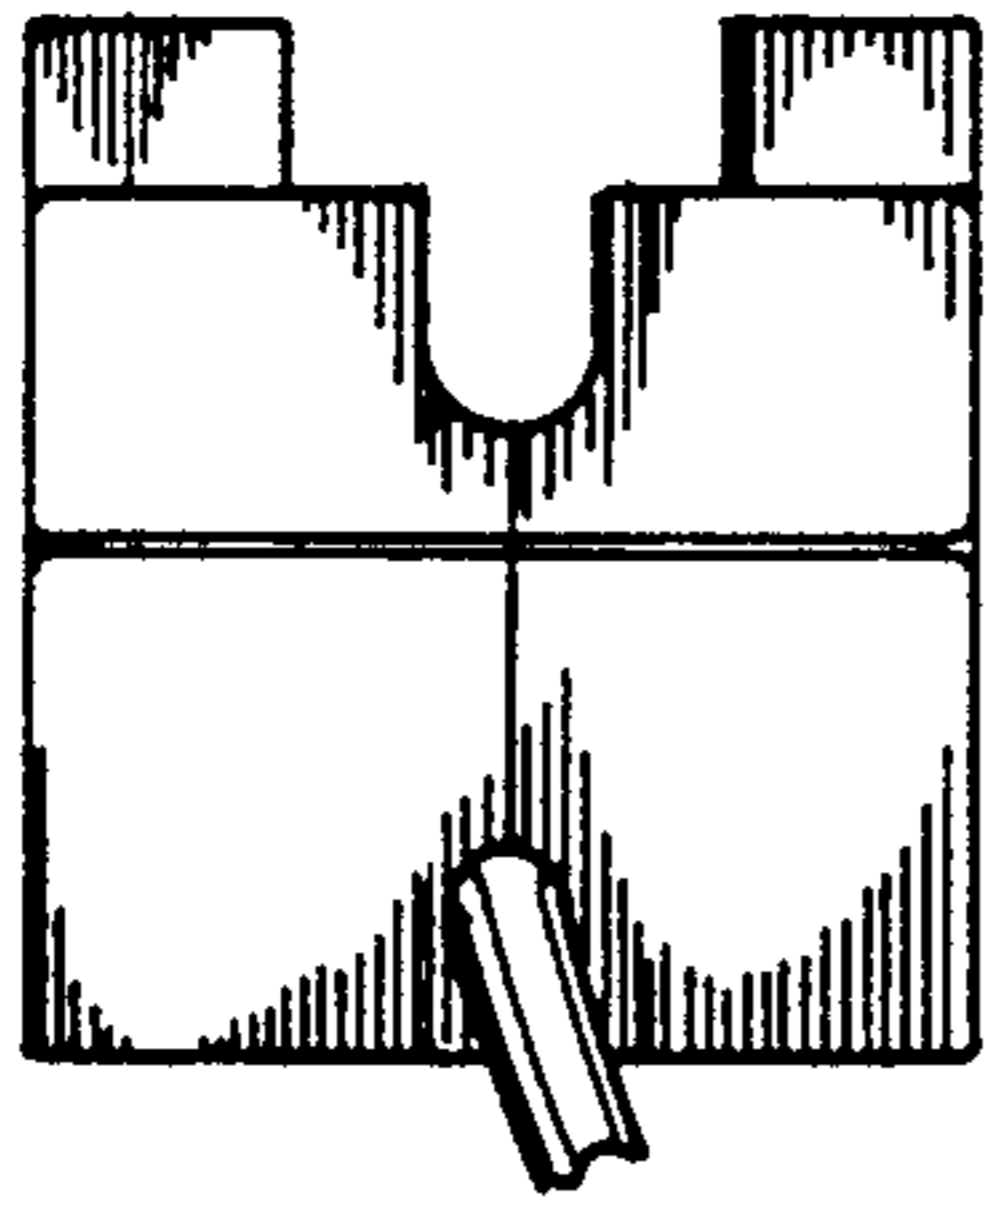


FIG. 4

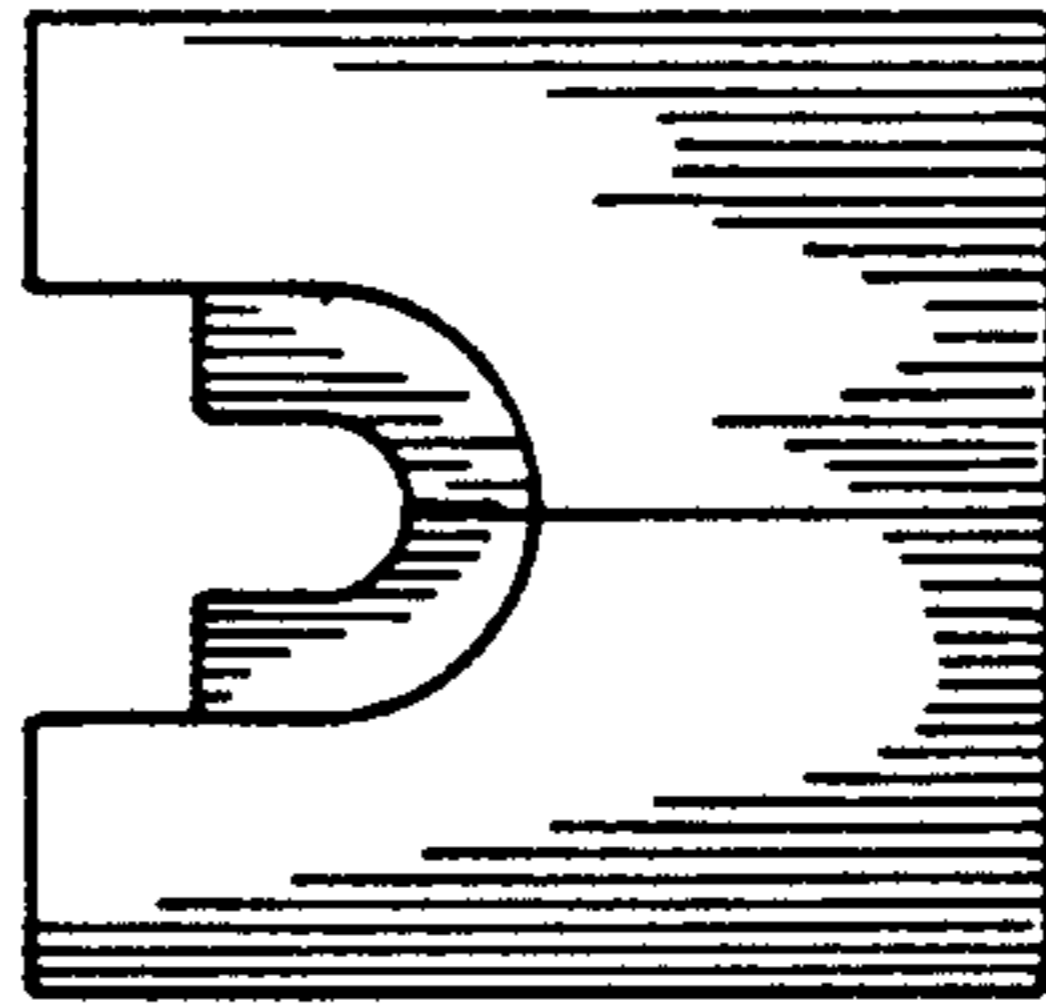


FIG. 3

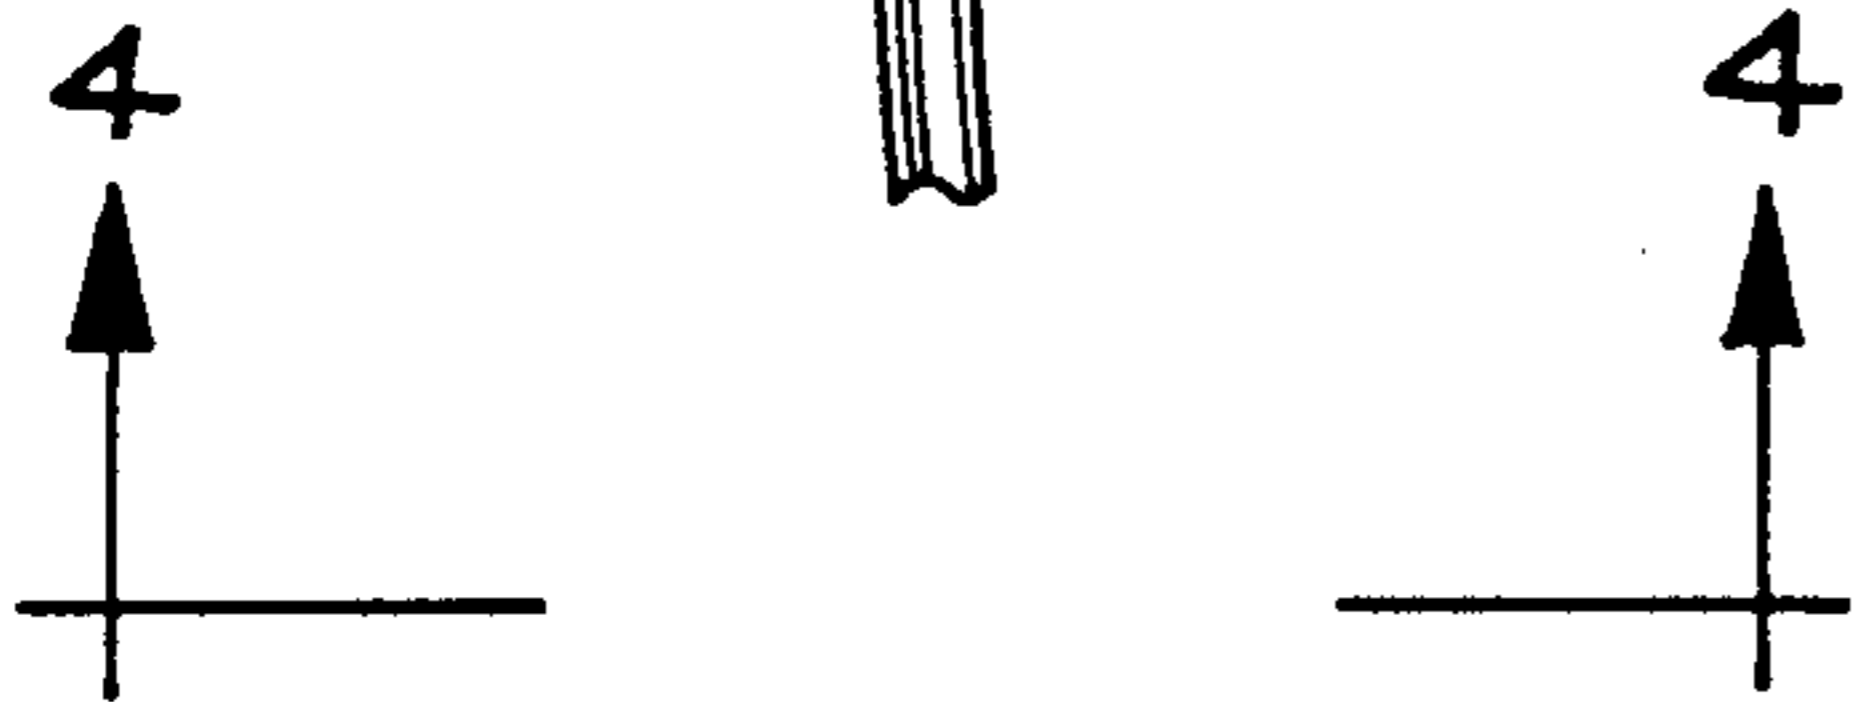
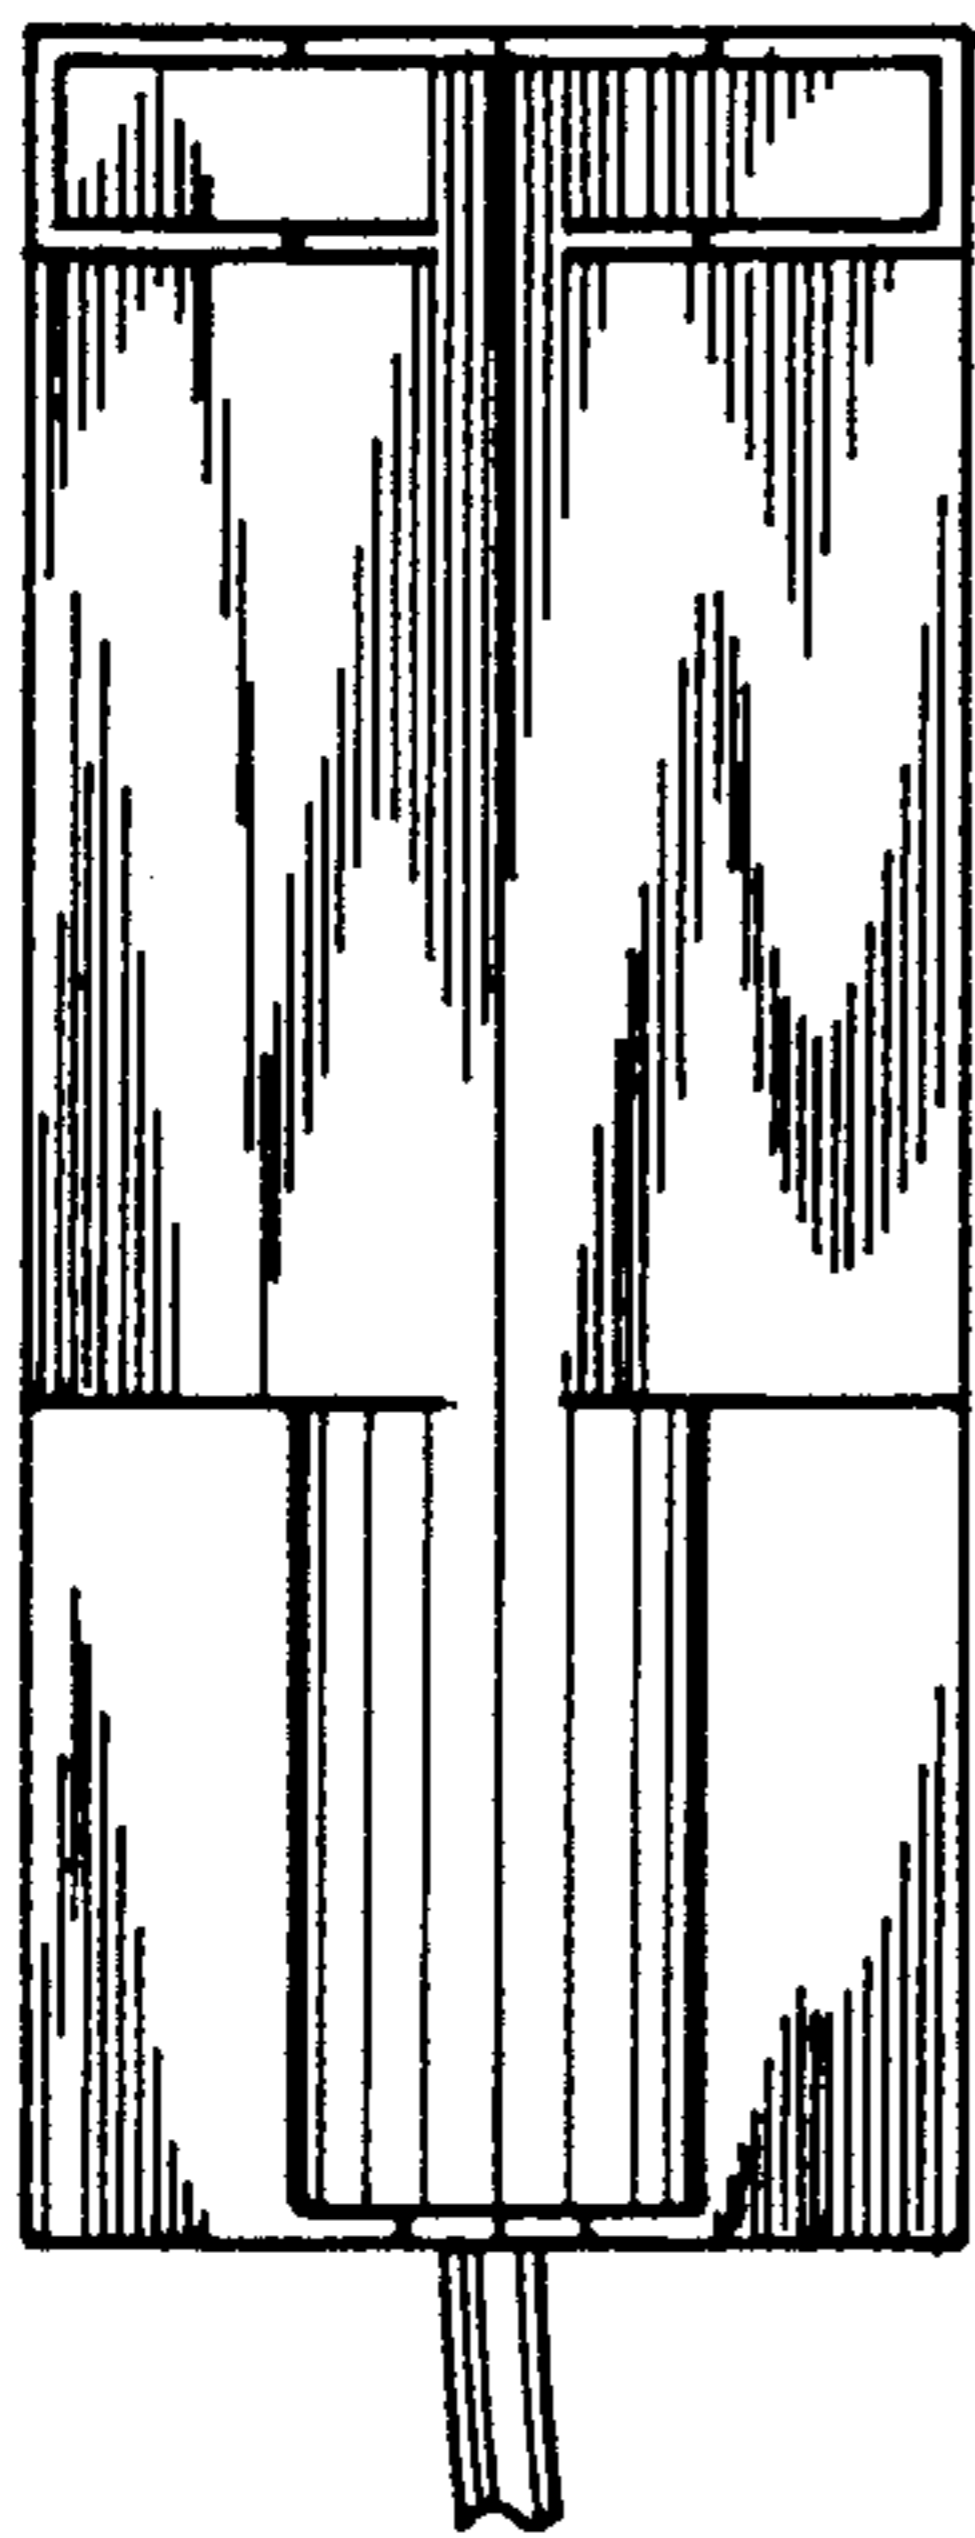


FIG. 1

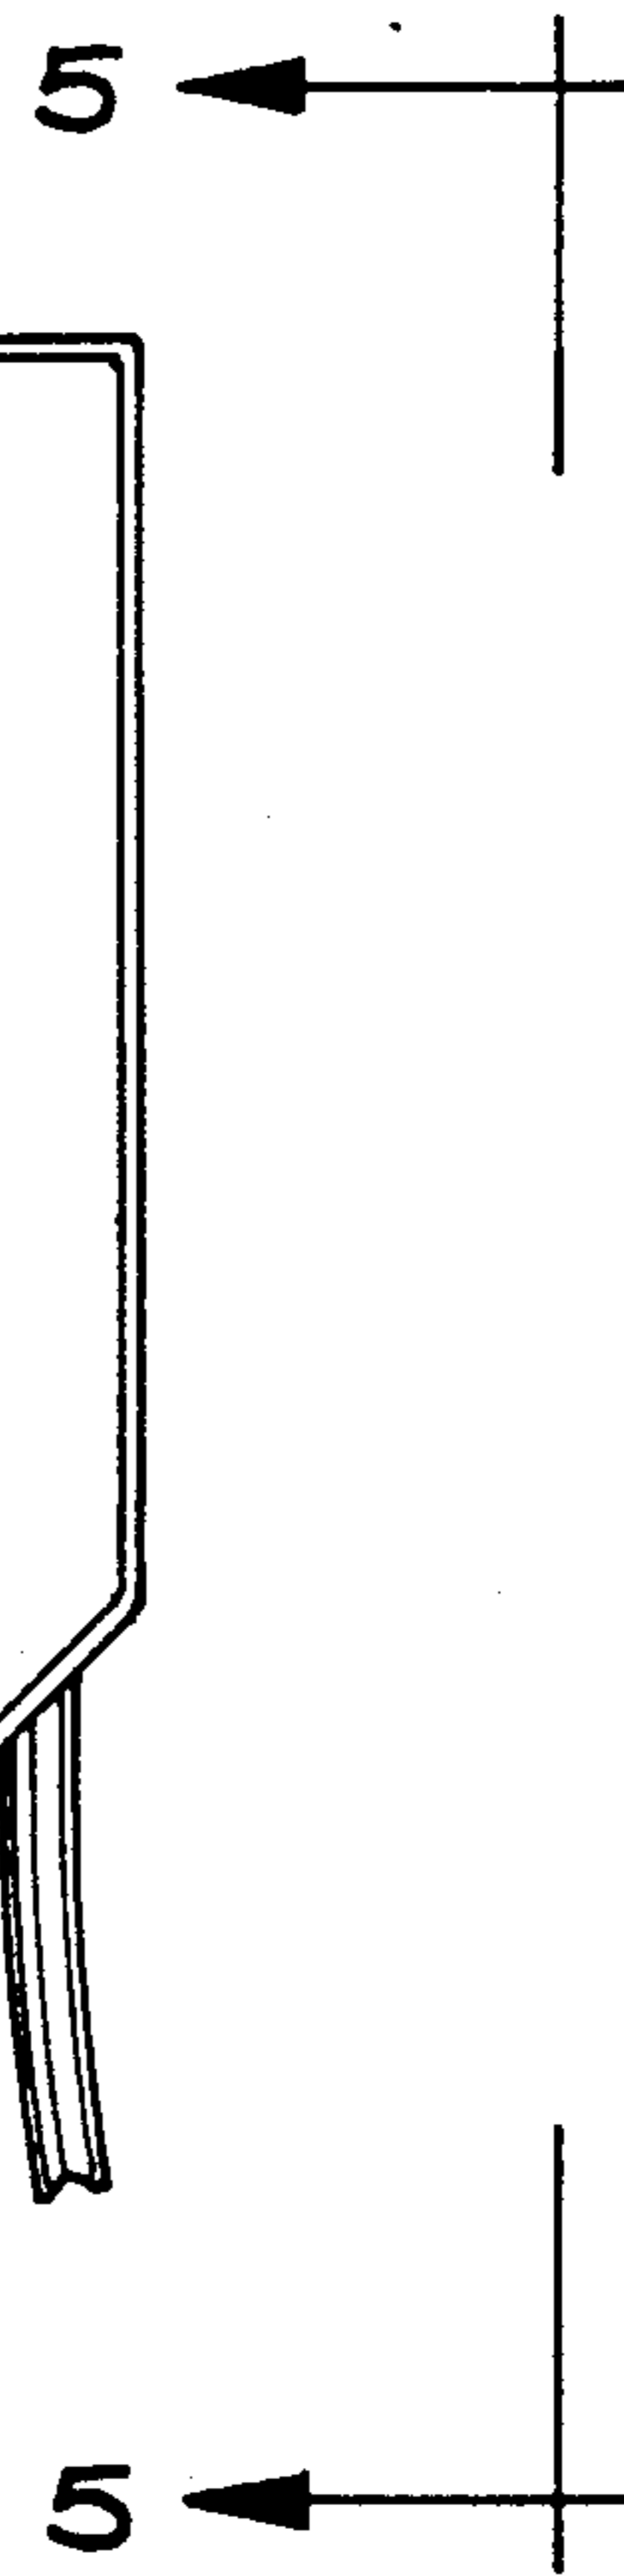
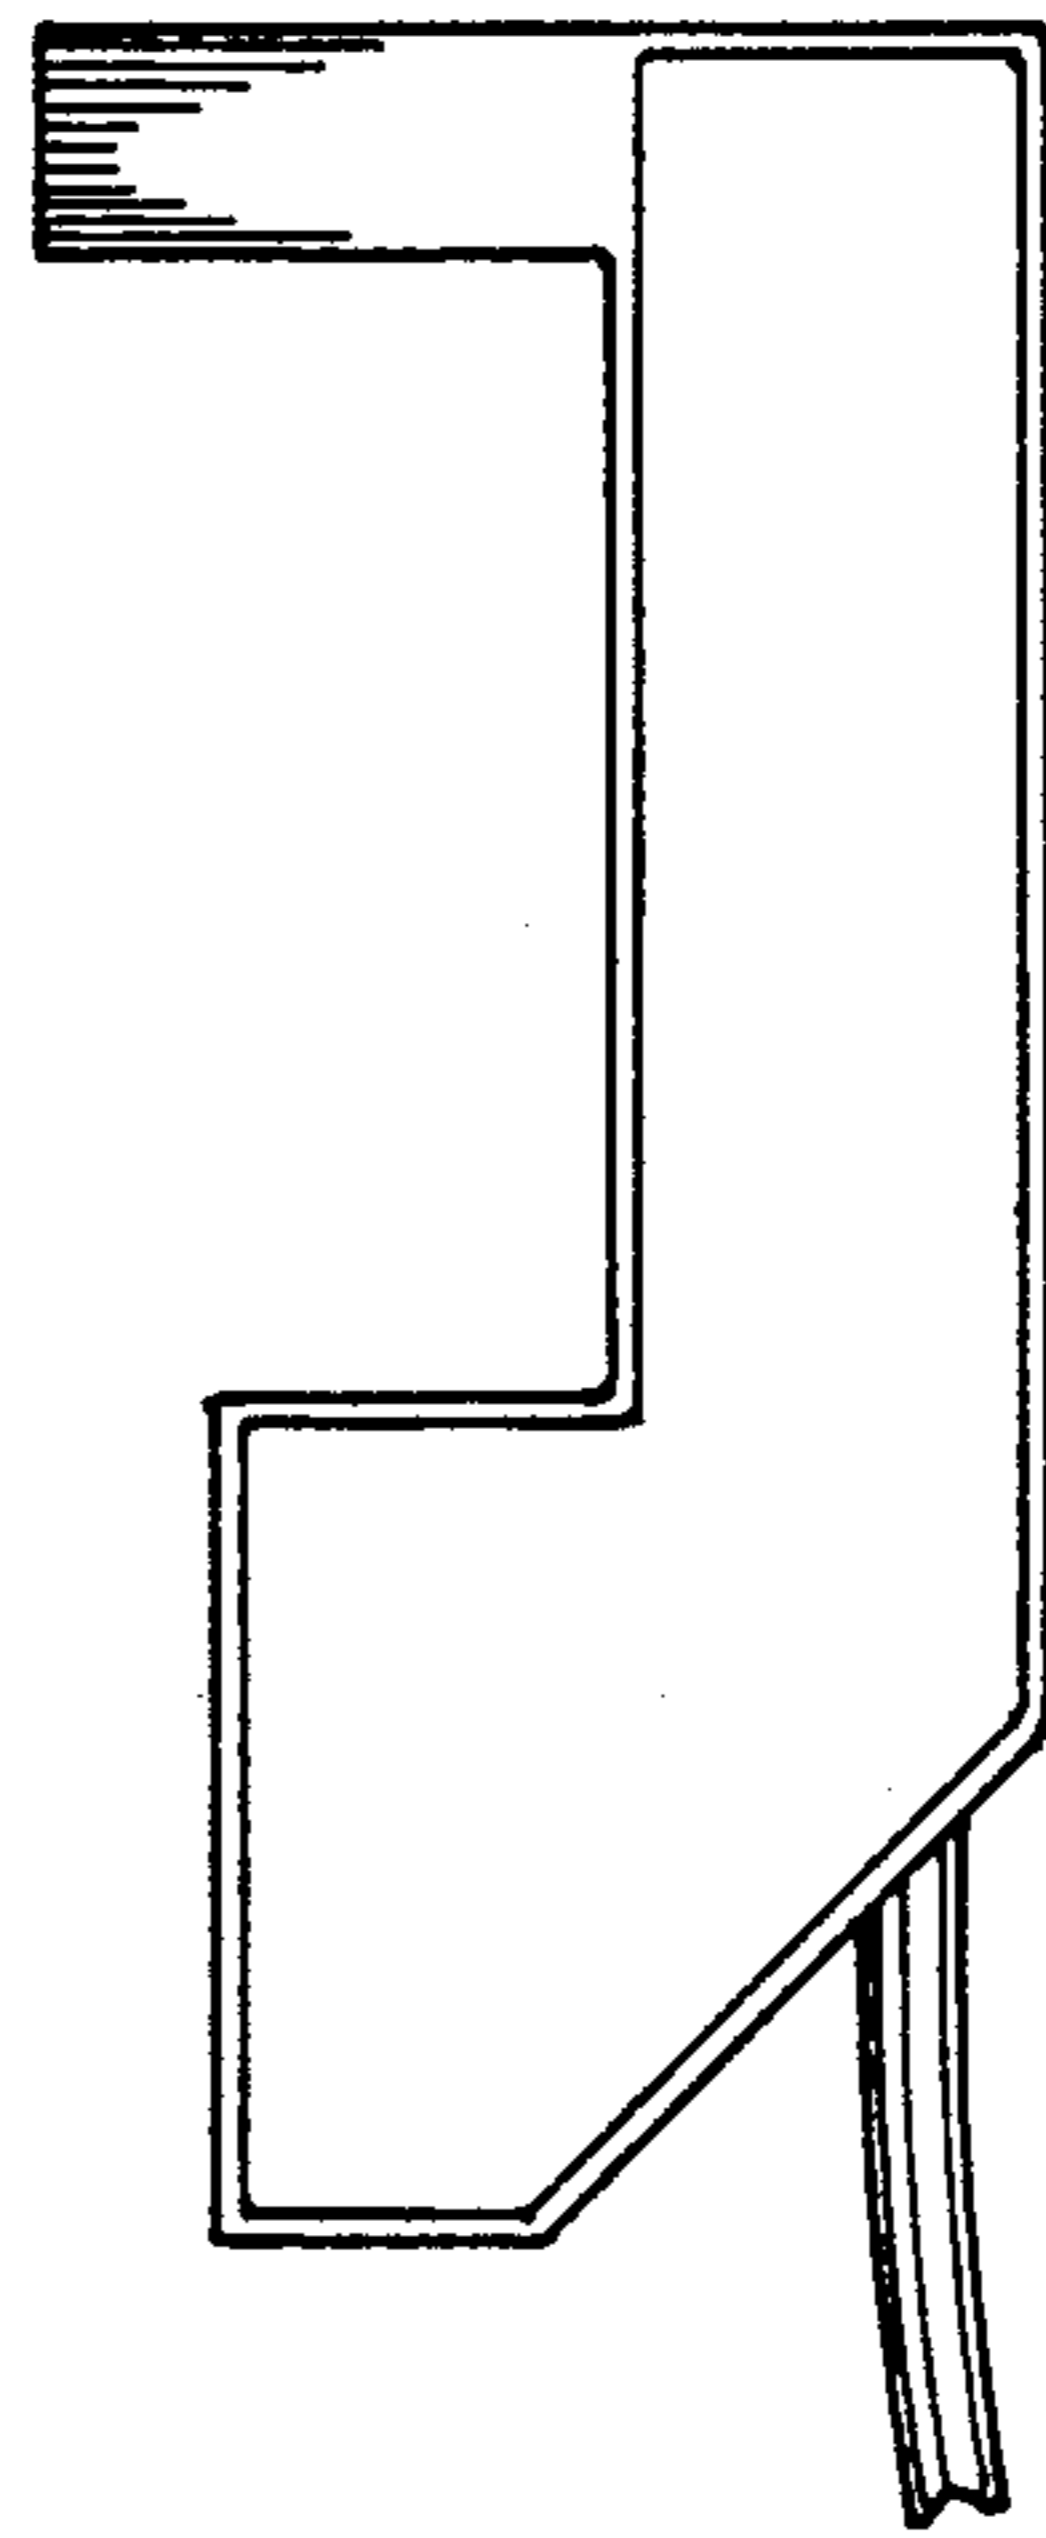


FIG. 2

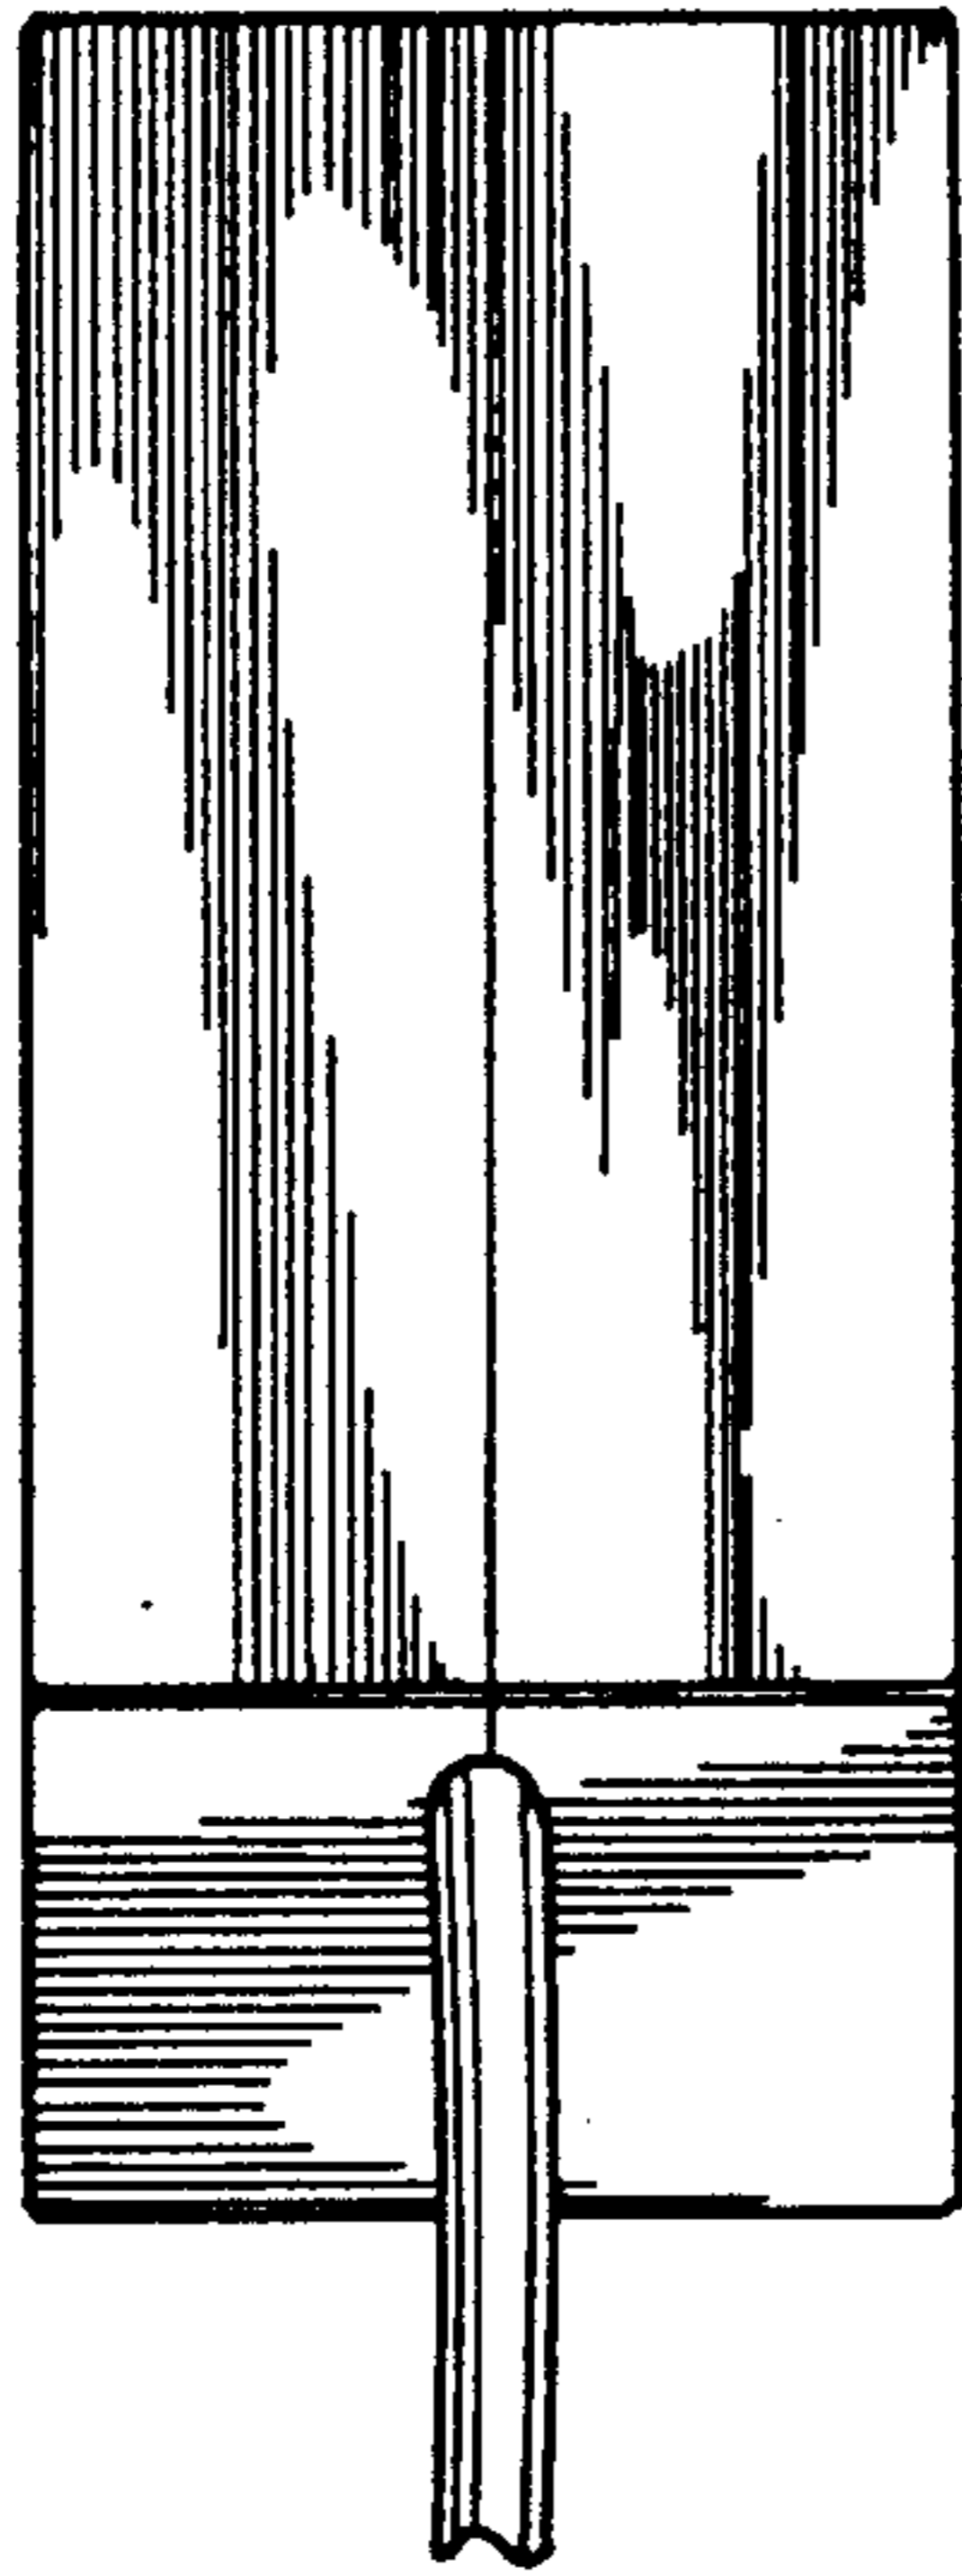


Fig. 5

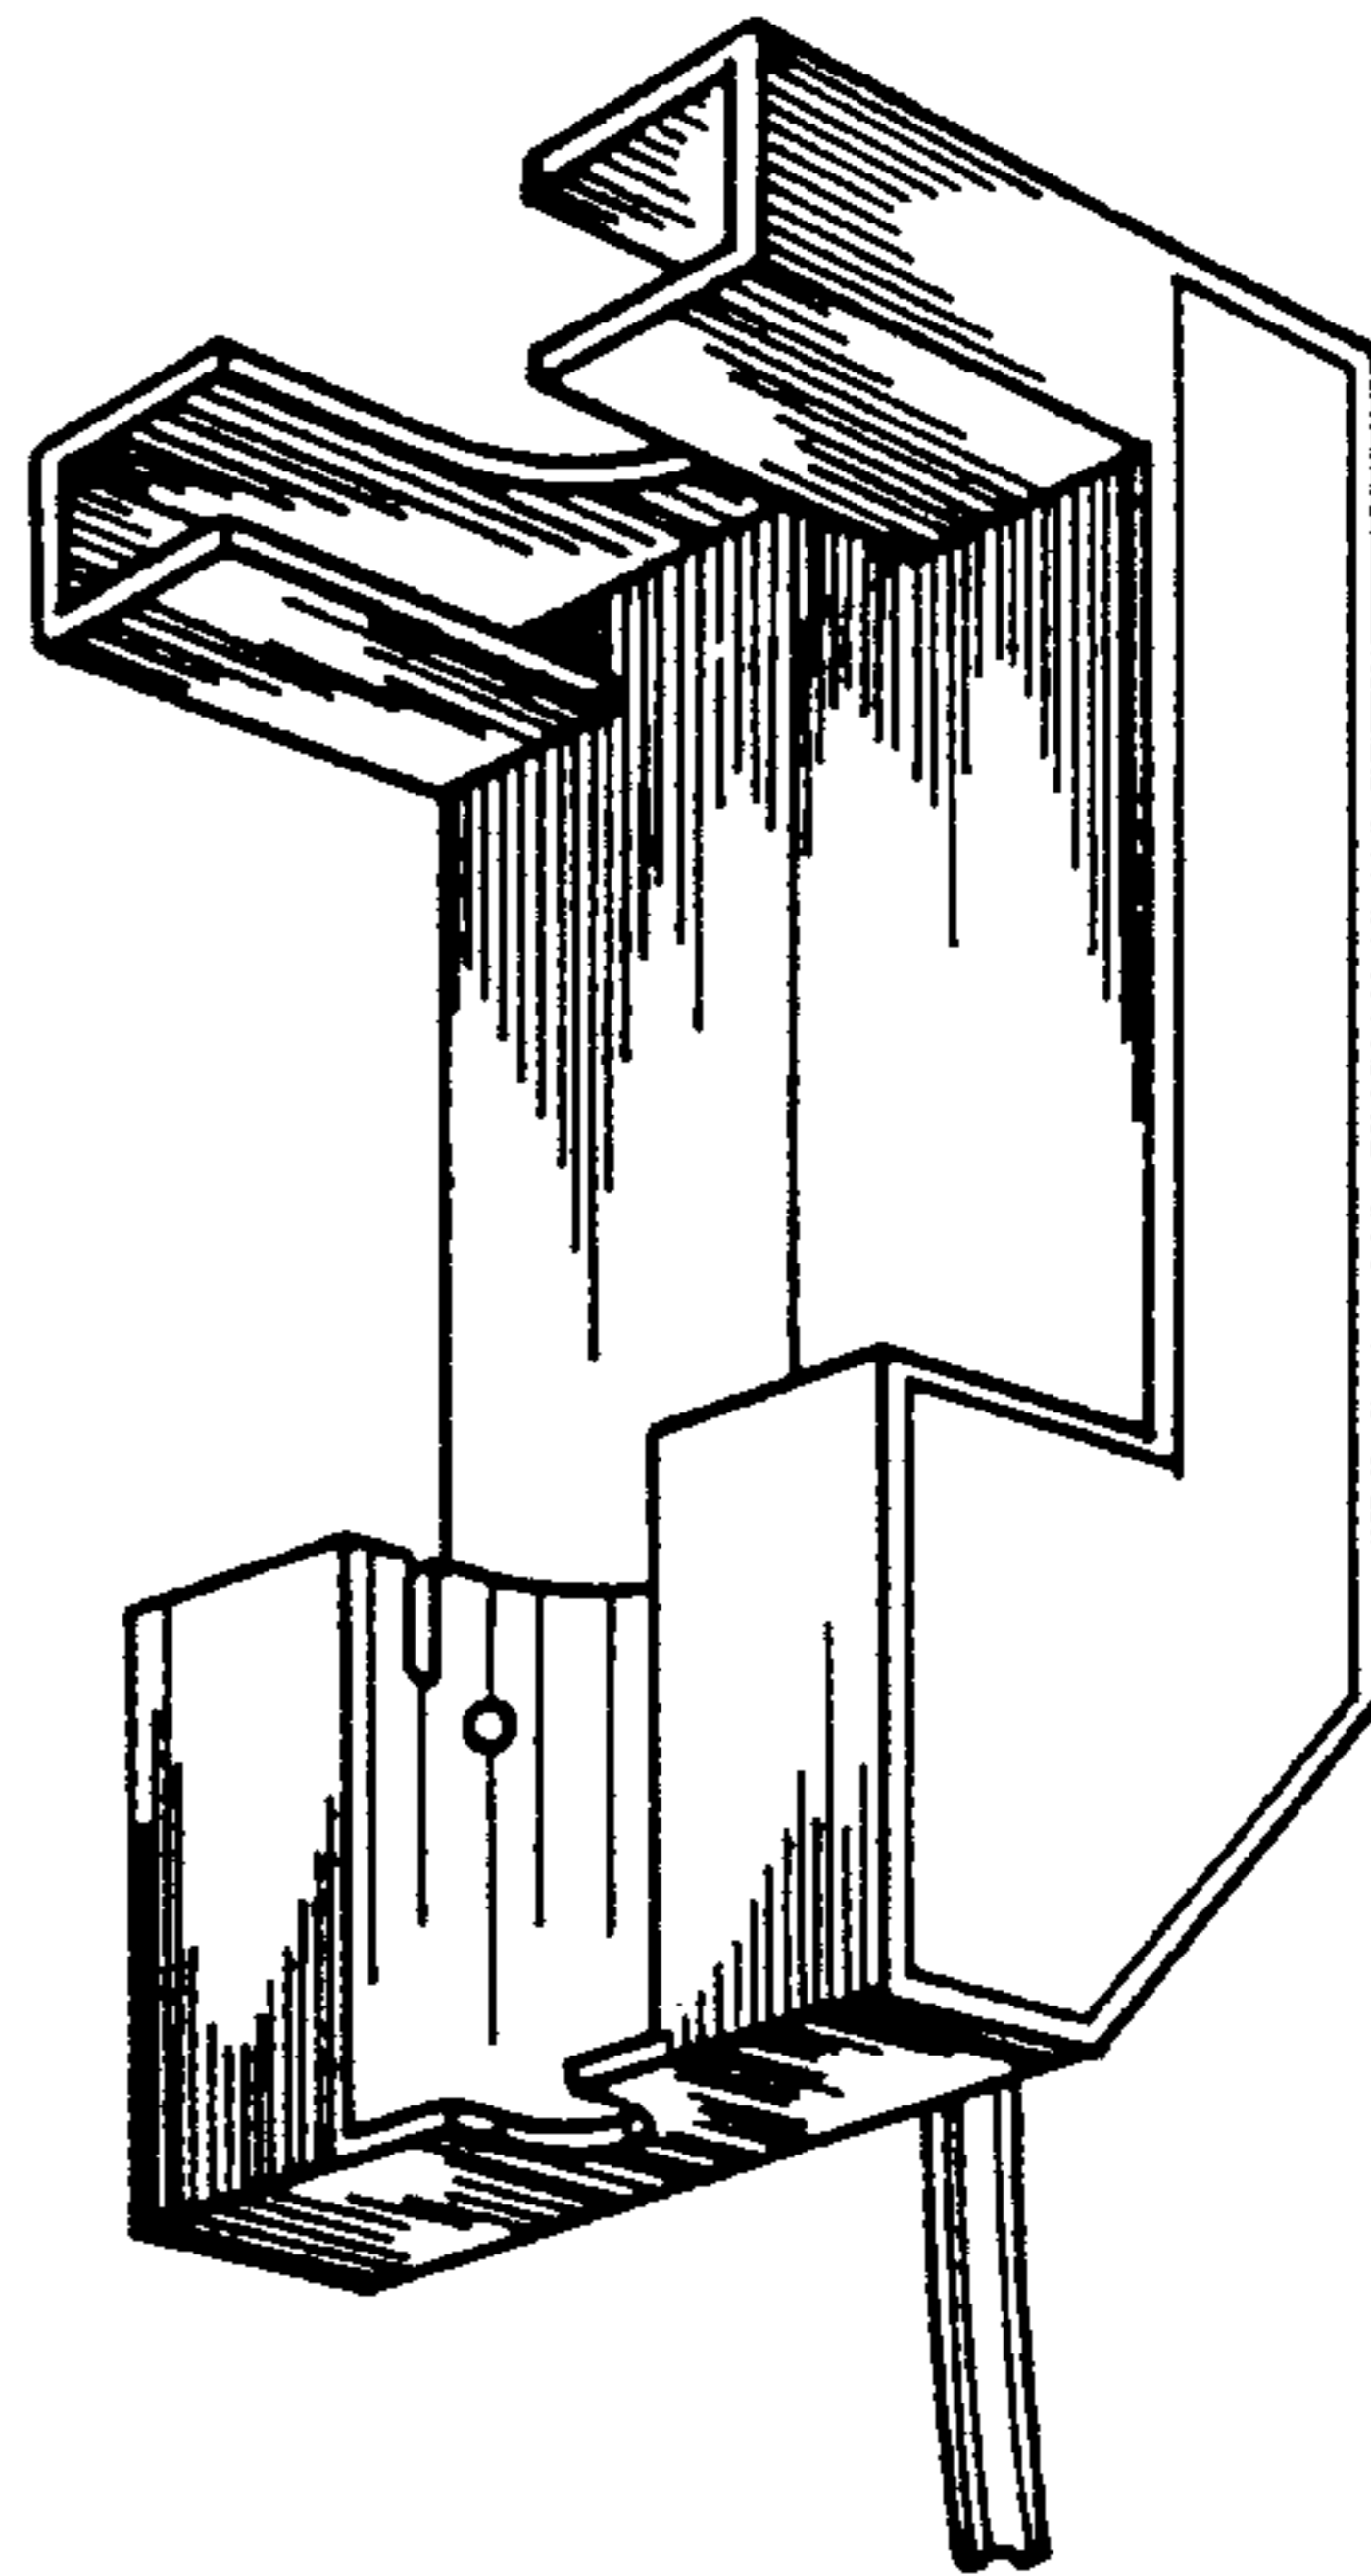


Fig. 6

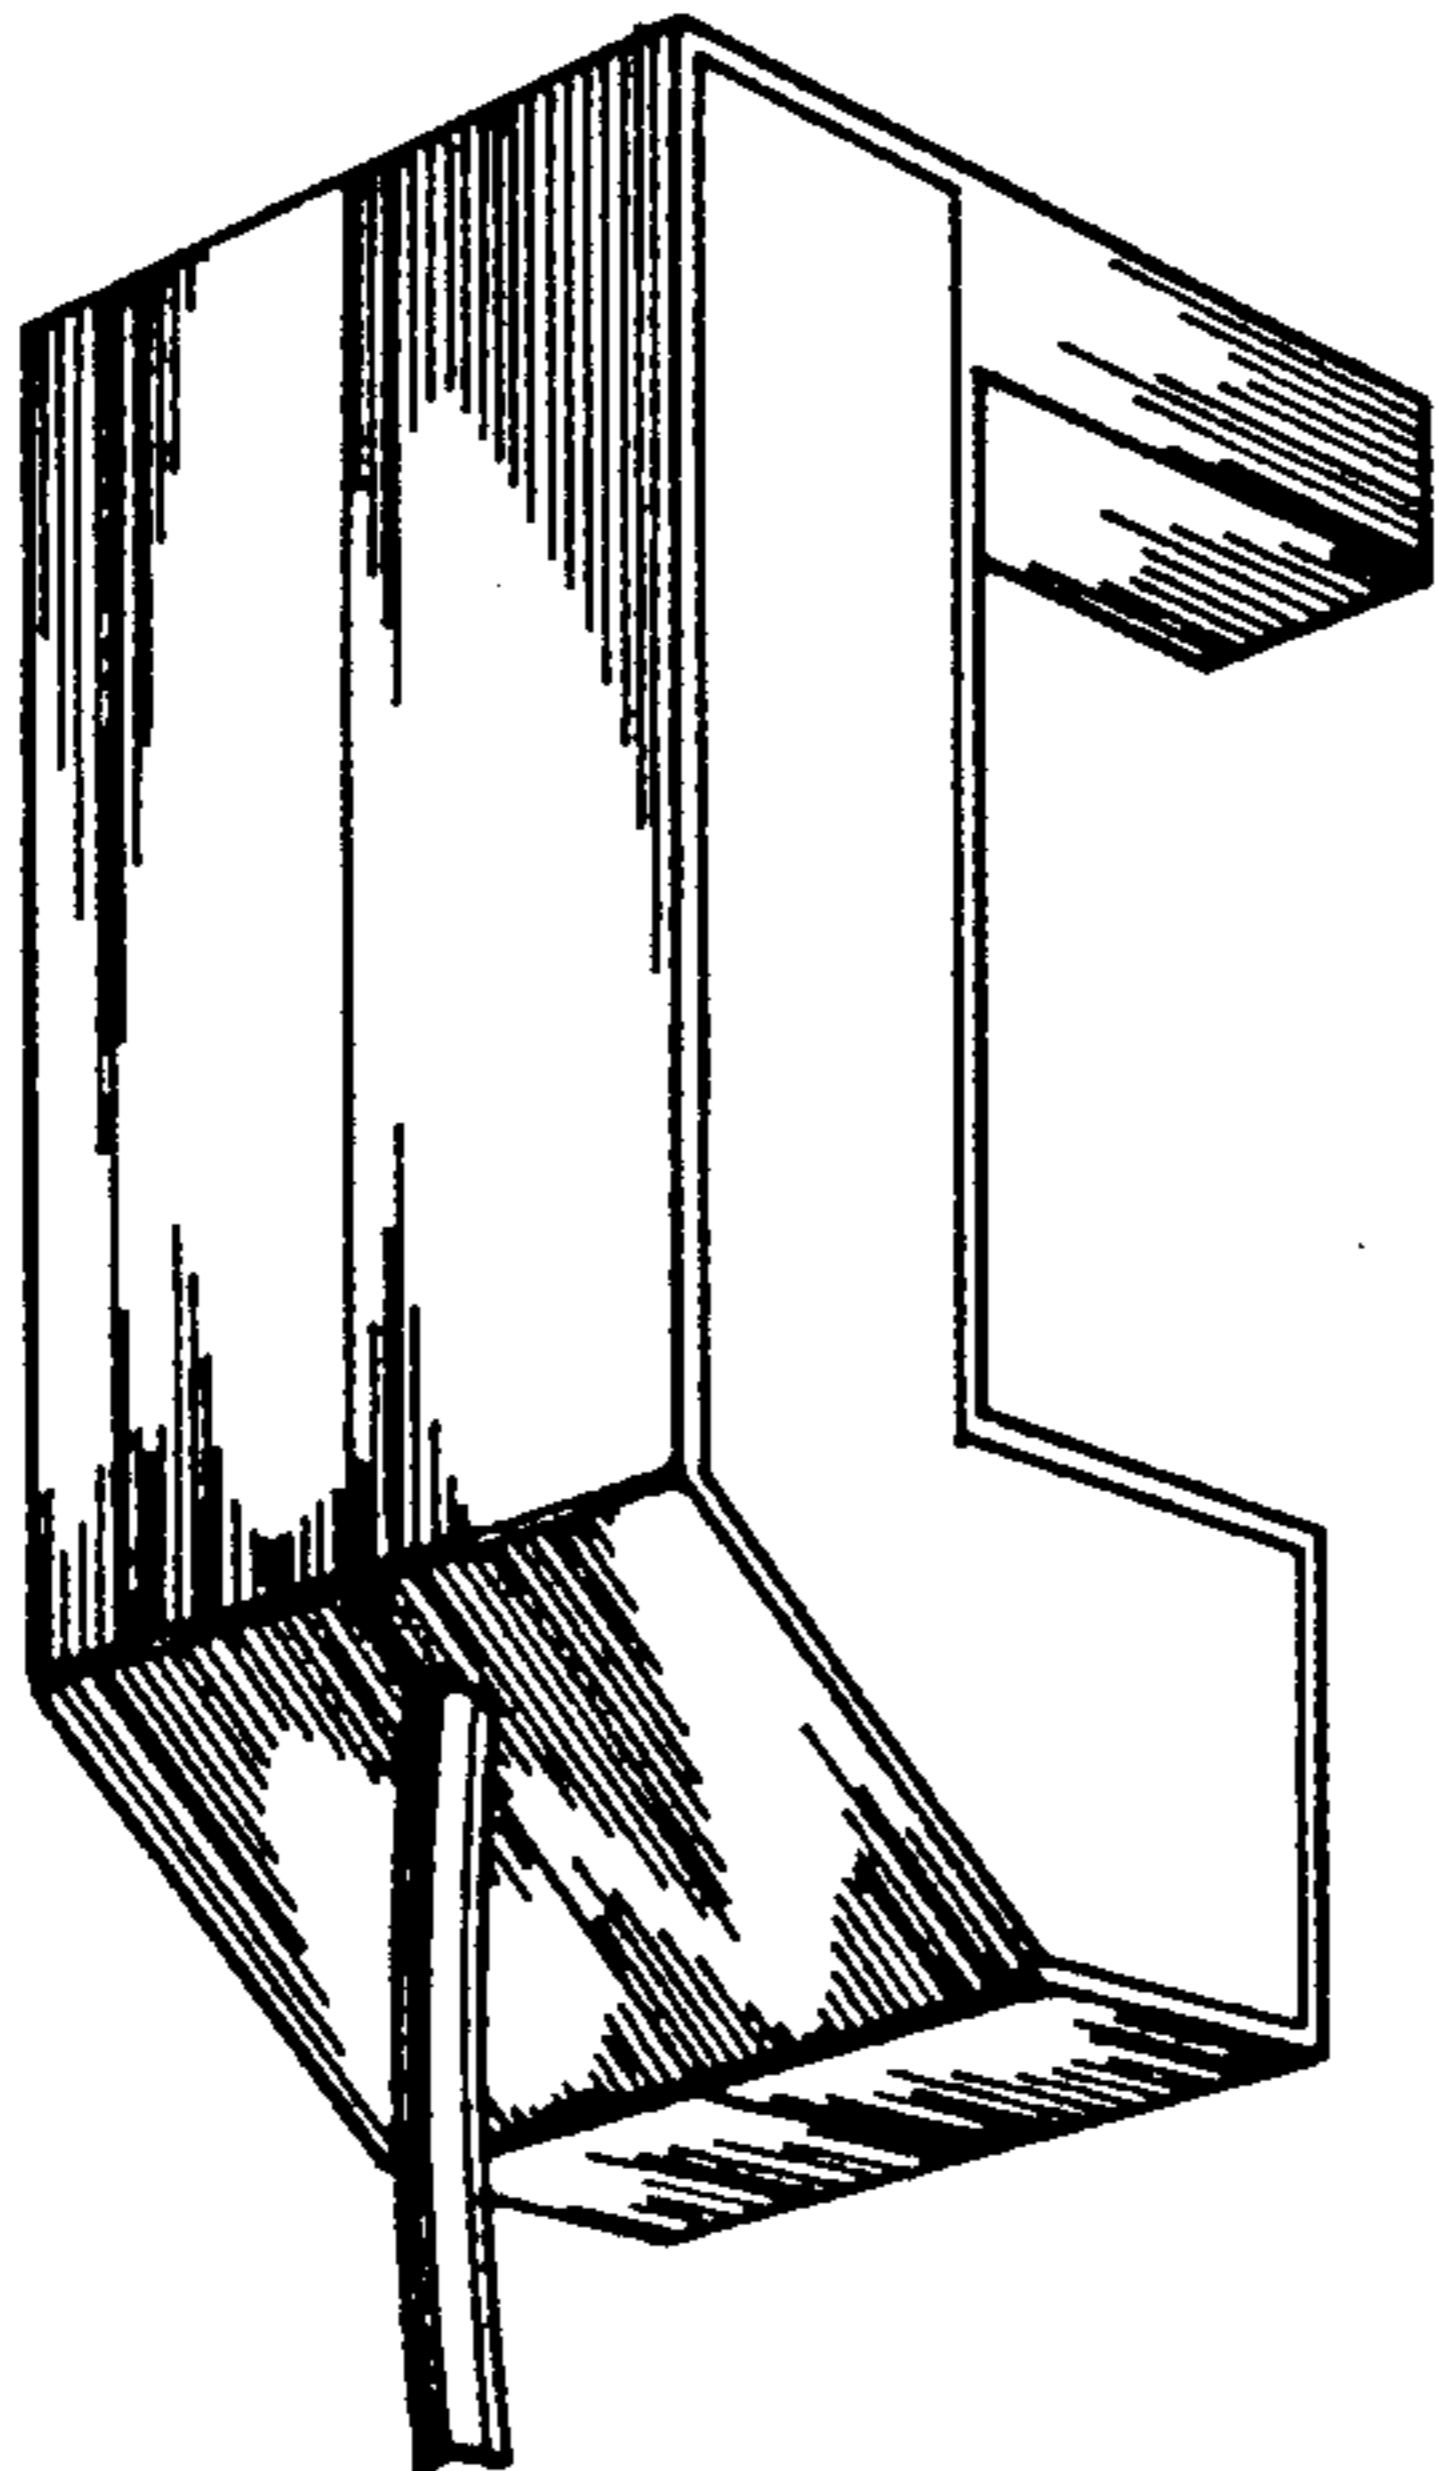


Fig. 7