

# United States Patent [19]

Spina

[11] Patent Number: **Des. 316,611**

[45] Date of Patent: **\*\* Apr. 30, 1991**

[54] HANDLE FOR SURGERY LAMP

[75] Inventor: **Charles Spina, Ross, Calif.**

[73] Assignee: **MDT Corporation, Torrance, Calif.**

[\*\*] Term: **14 Years**

[21] Appl. No.: **170,413**

[22] Filed: **Mar. 18, 1988**

[52] U.S. Cl. .... **D26/113**

[58] Field of Search ..... **D26/140, 138, 113, 60, D26/66; 362/804; 74/488, 489, 551.8, 551.9; 81/177.1, 177.6; 29/235**

[56] **References Cited**

**U.S. PATENT DOCUMENTS**

|            |         |                      |       |         |
|------------|---------|----------------------|-------|---------|
| D. 246,758 | 12/1977 | Ukai                 | ..... | D8/303  |
| D. 278,879 | 5/1985  | Hwung                | ..... | D8/303  |
| D. 289,206 | 4/1987  | Scoville, Jr. et al. | ..... | D26/113 |
| 3,896,680  | 7/1975  | Shoemaker            | ..... | 74/489  |

|           |         |                |       |            |
|-----------|---------|----------------|-------|------------|
| 4,149,432 | 4/1979  | Costahaude     | ..... | 74/489     |
| 4,559,671 | 12/1985 | Andrews et al. | ..... | 16/DIG. 24 |
| 4,605,124 | 8/1986  | Sandel et al.  | ..... | 16/DIG. 12 |
| 4,844,252 | 7/1989  | Barron et al.  | ..... | 362/804    |
| 4,895,044 | 1/1990  | Ekins          | ..... | D8/303     |


*Primary Examiner*—Wallace R. Burke  
*Assistant Examiner*—Marcus Jackson  
*Attorney, Agent, or Firm*—Trask, Britt & Rossa

[57] **CLAIM**

The ornamental design for a handle for surgery lamp, as shown and described.

**DESCRIPTION**

FIG. 1 is a top perspective view of a handle for surgery lamp showing my new design;  
FIG. 2 is a side elevational view thereof;  
FIG. 3 is an opposite side elevational view of FIG. 2 thereof;  
FIG. 4 is a top plan view thereof; and  
FIG. 5 is a bottom plan view thereof.

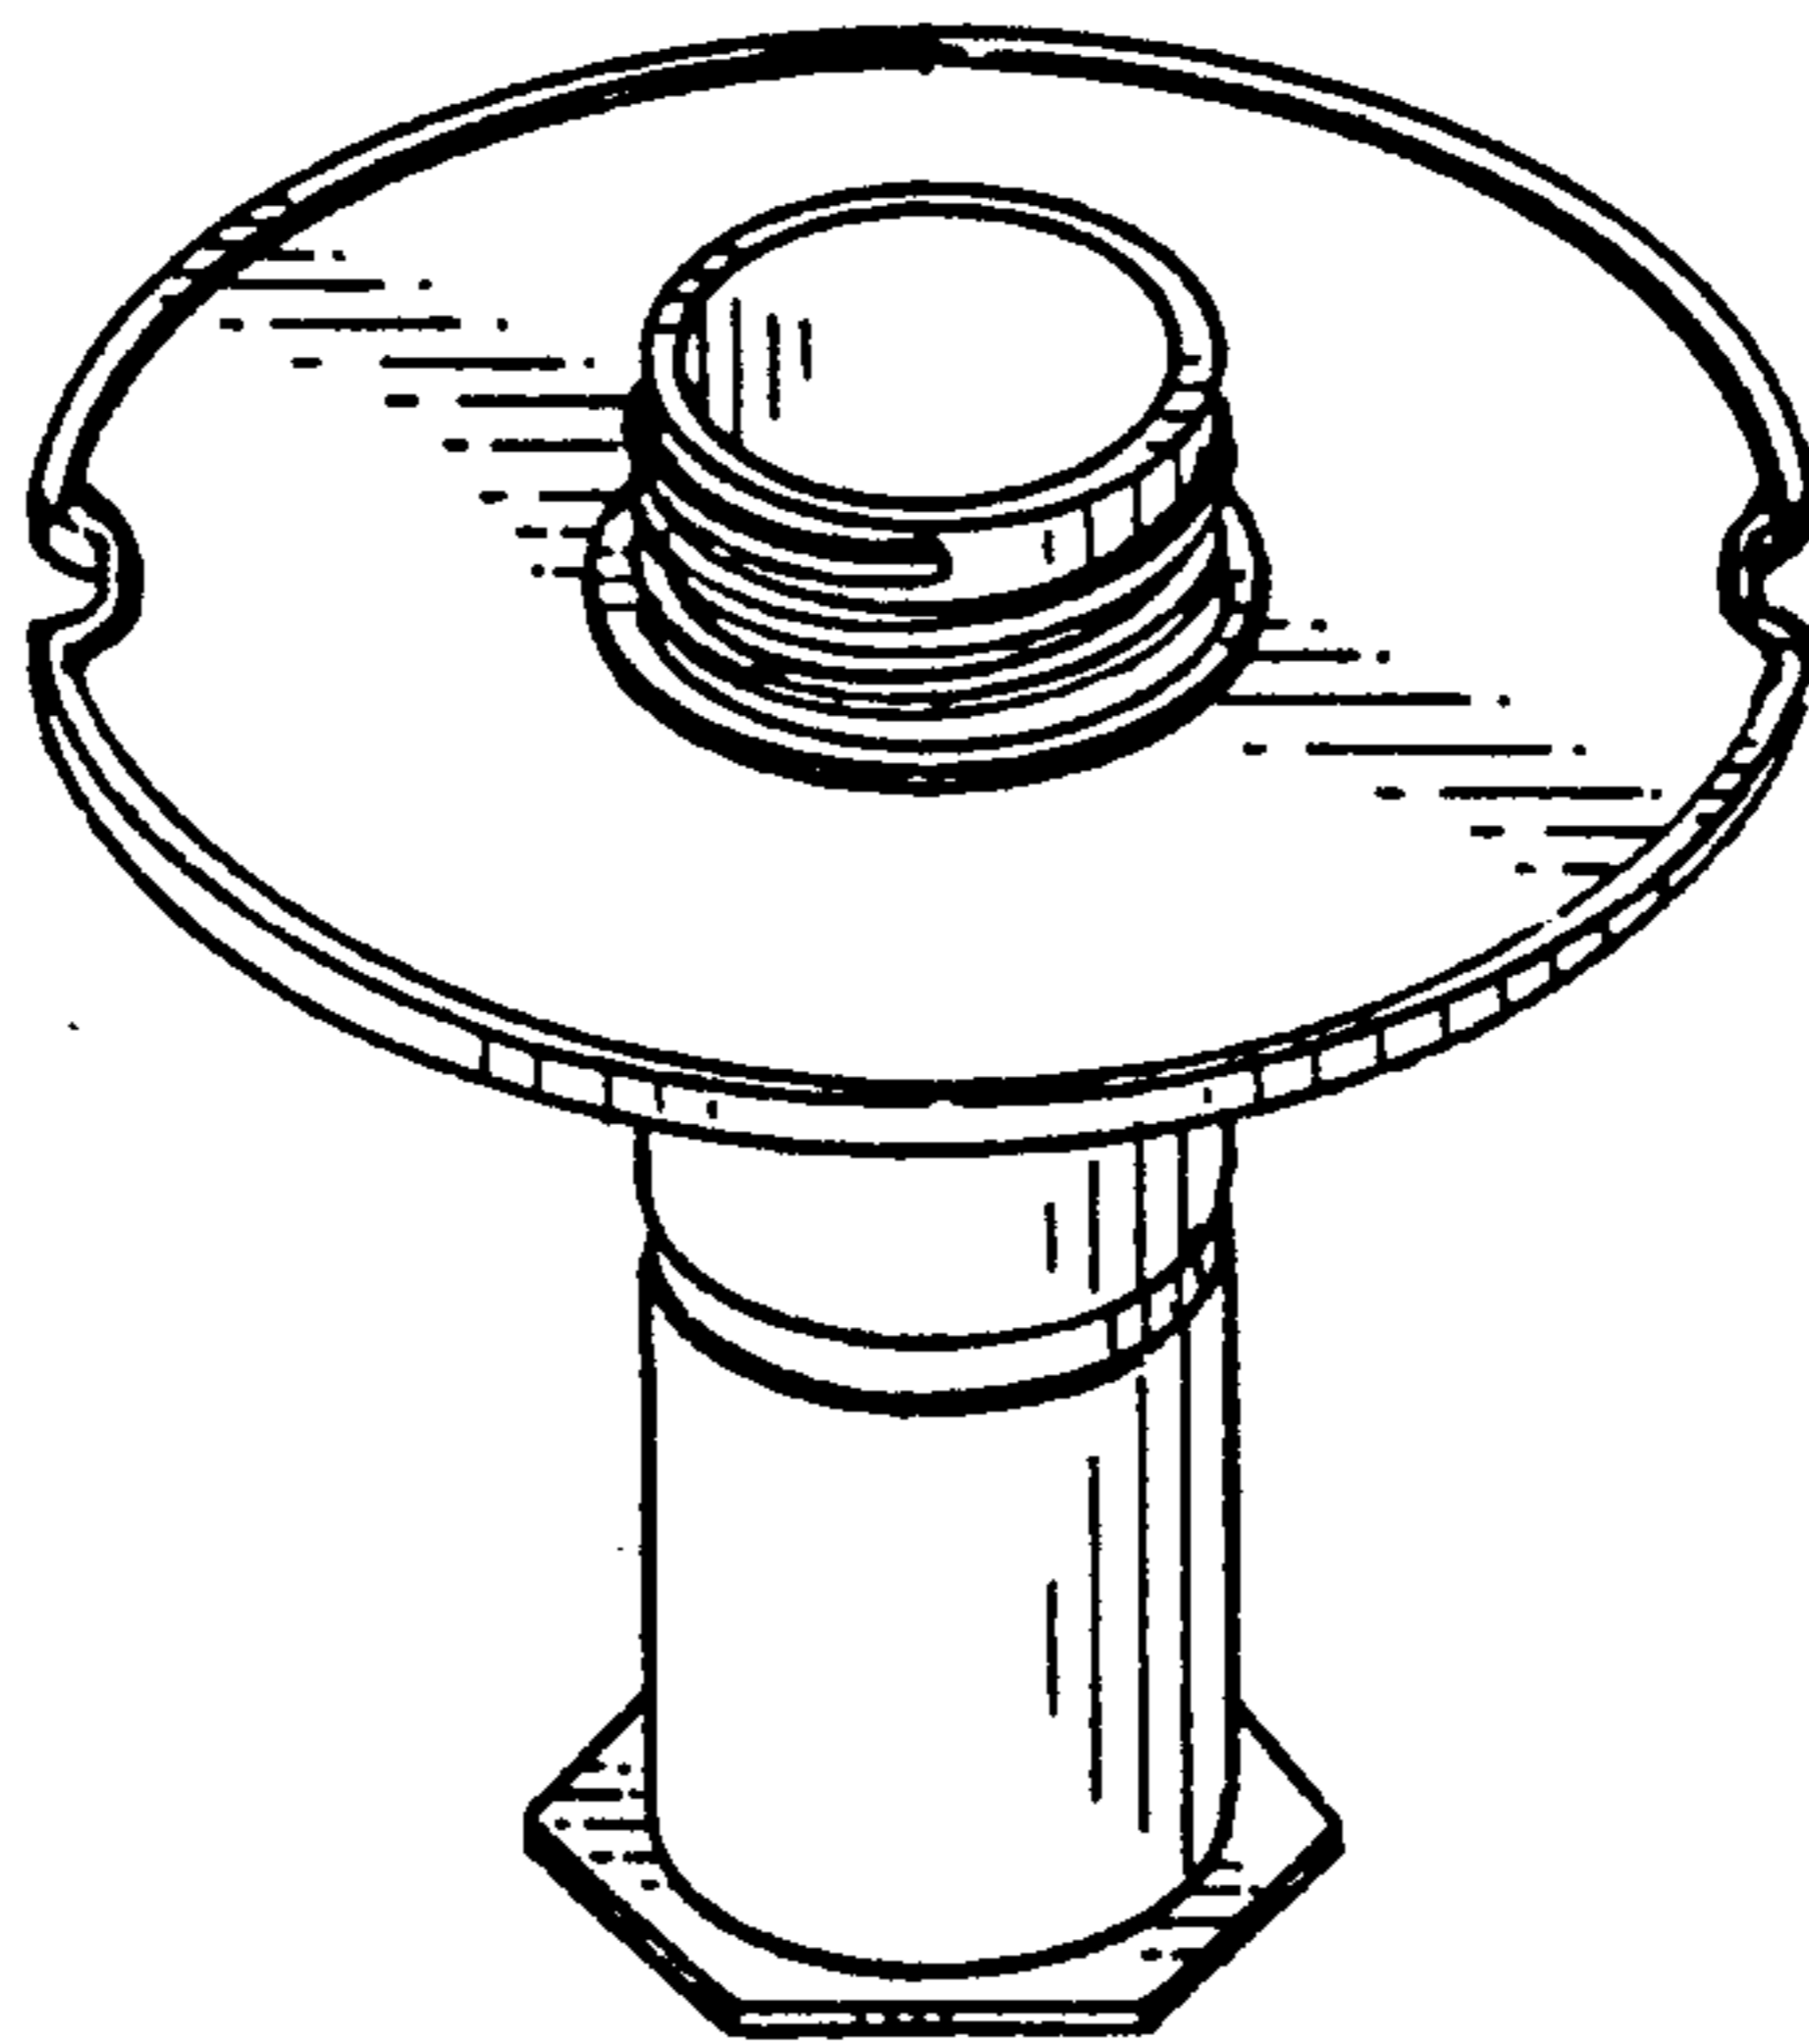

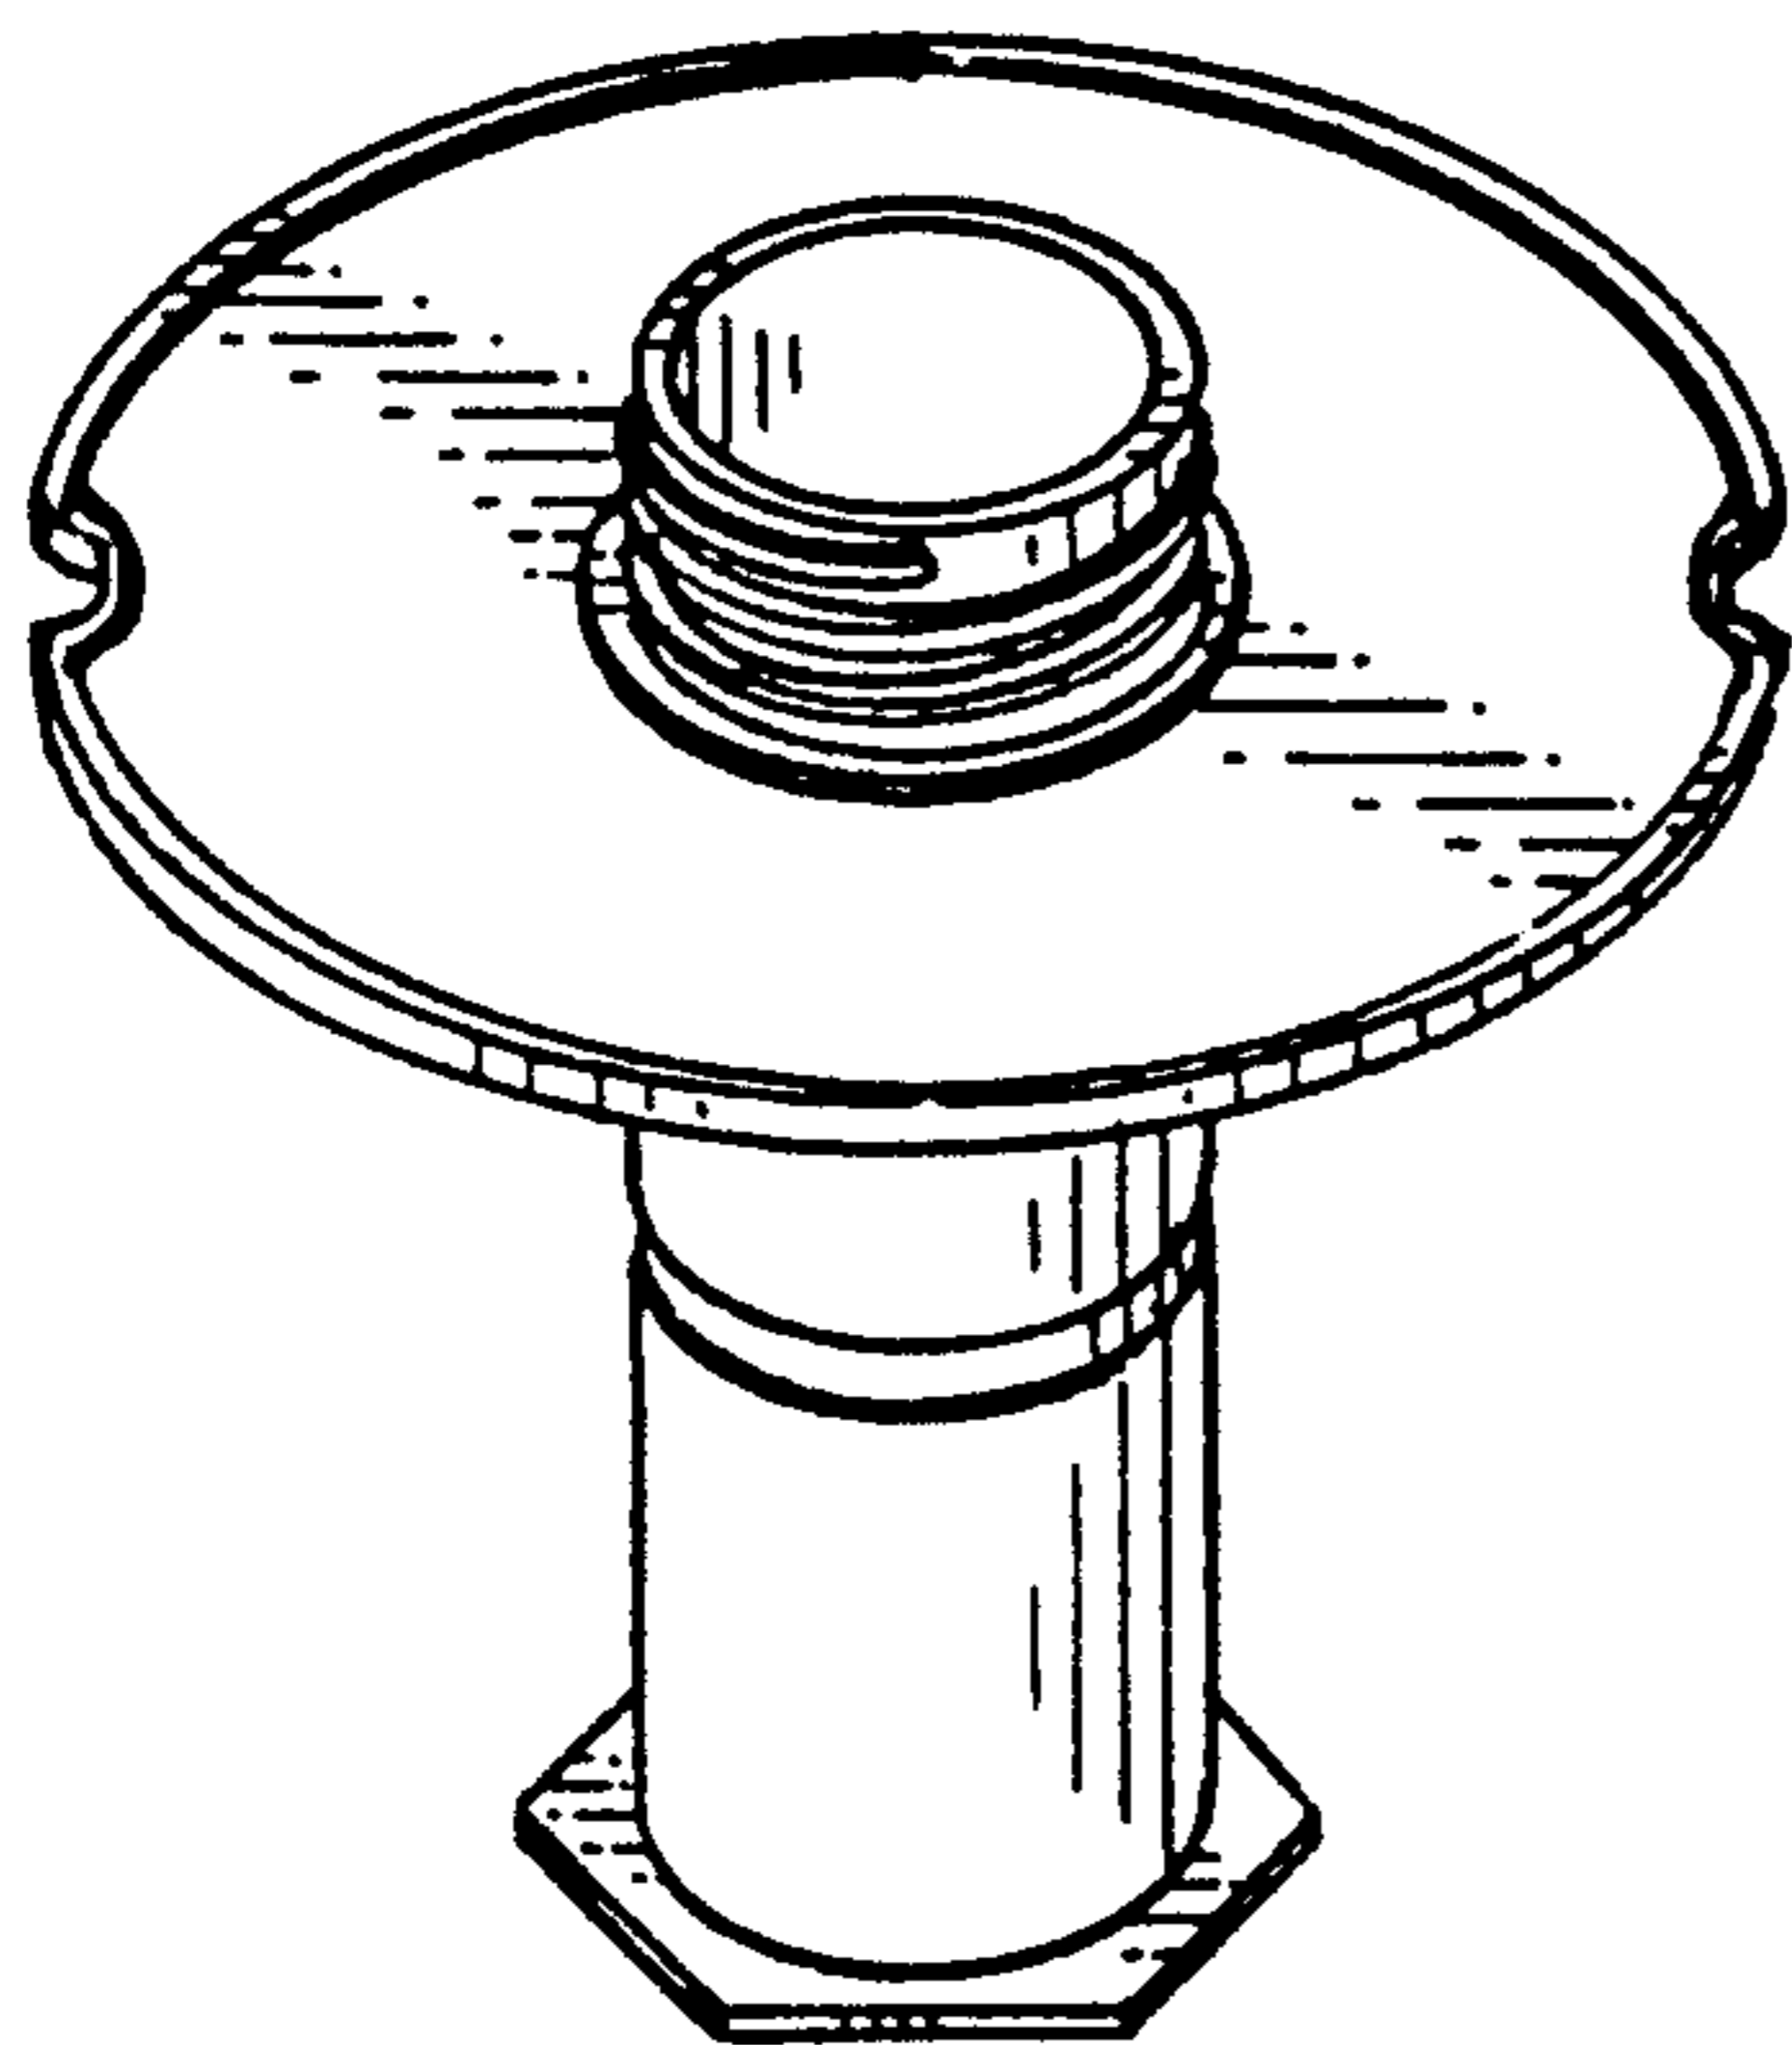


FIG. 1

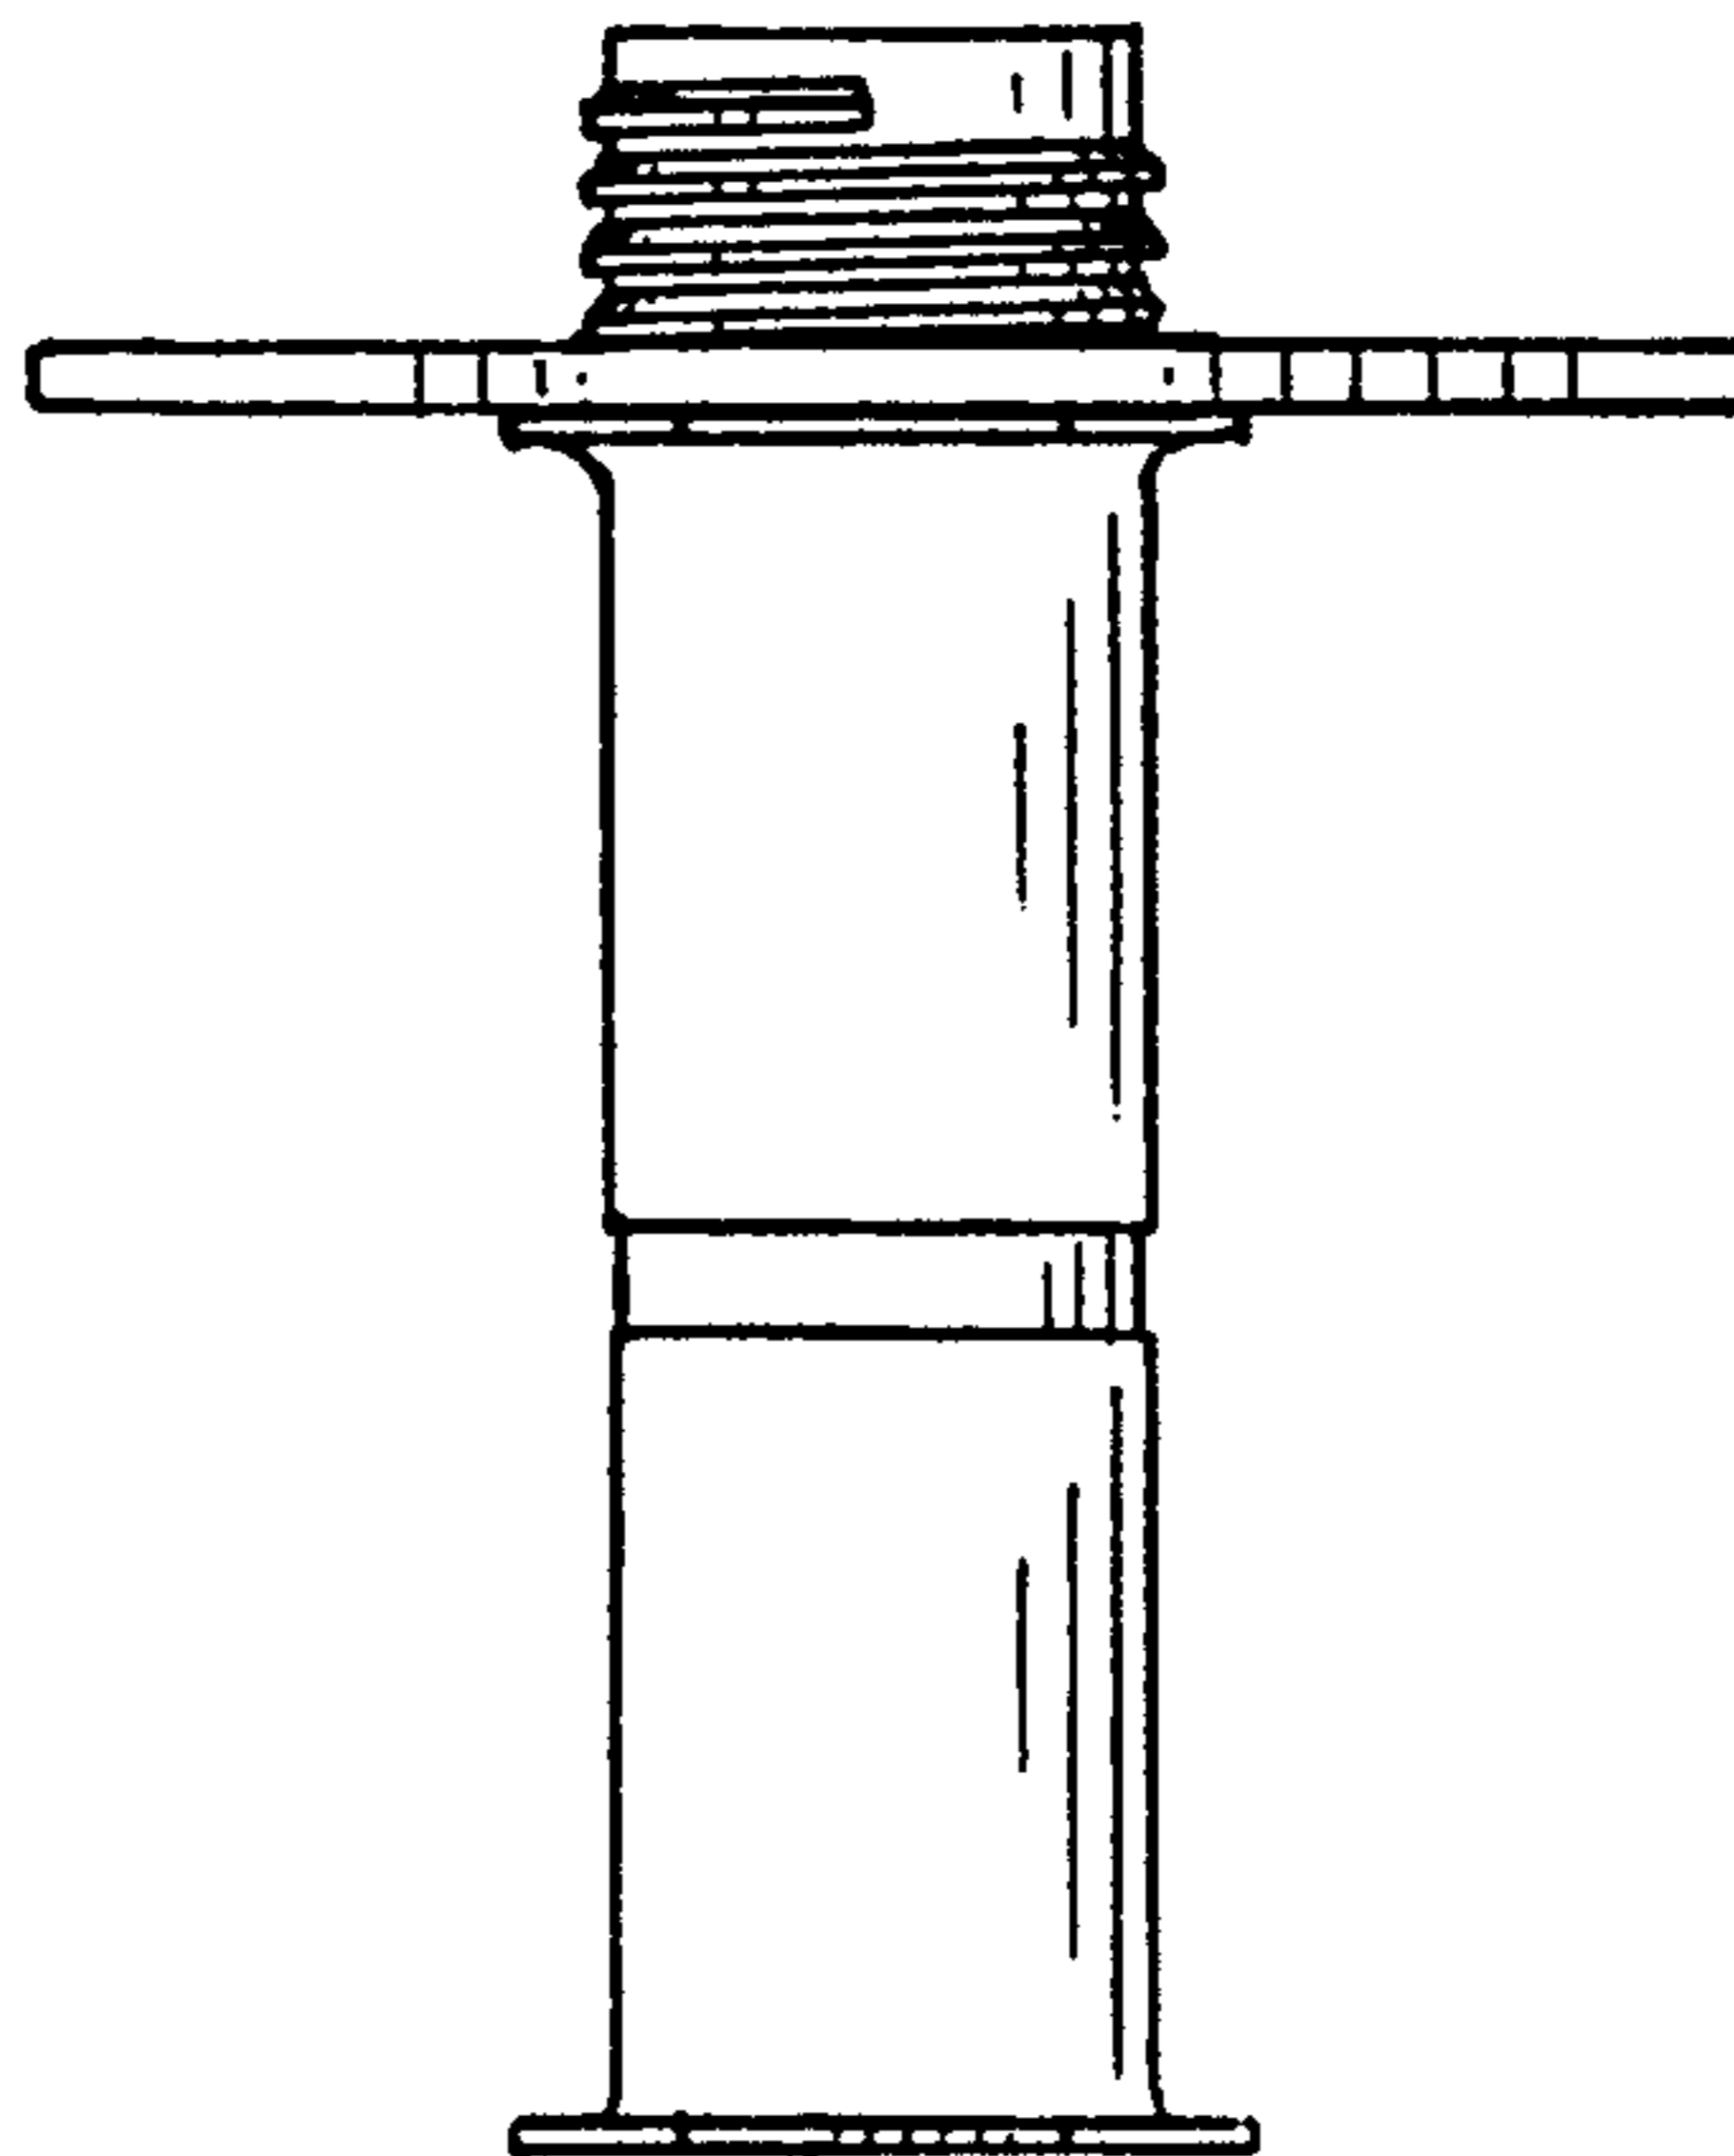


FIG. 2

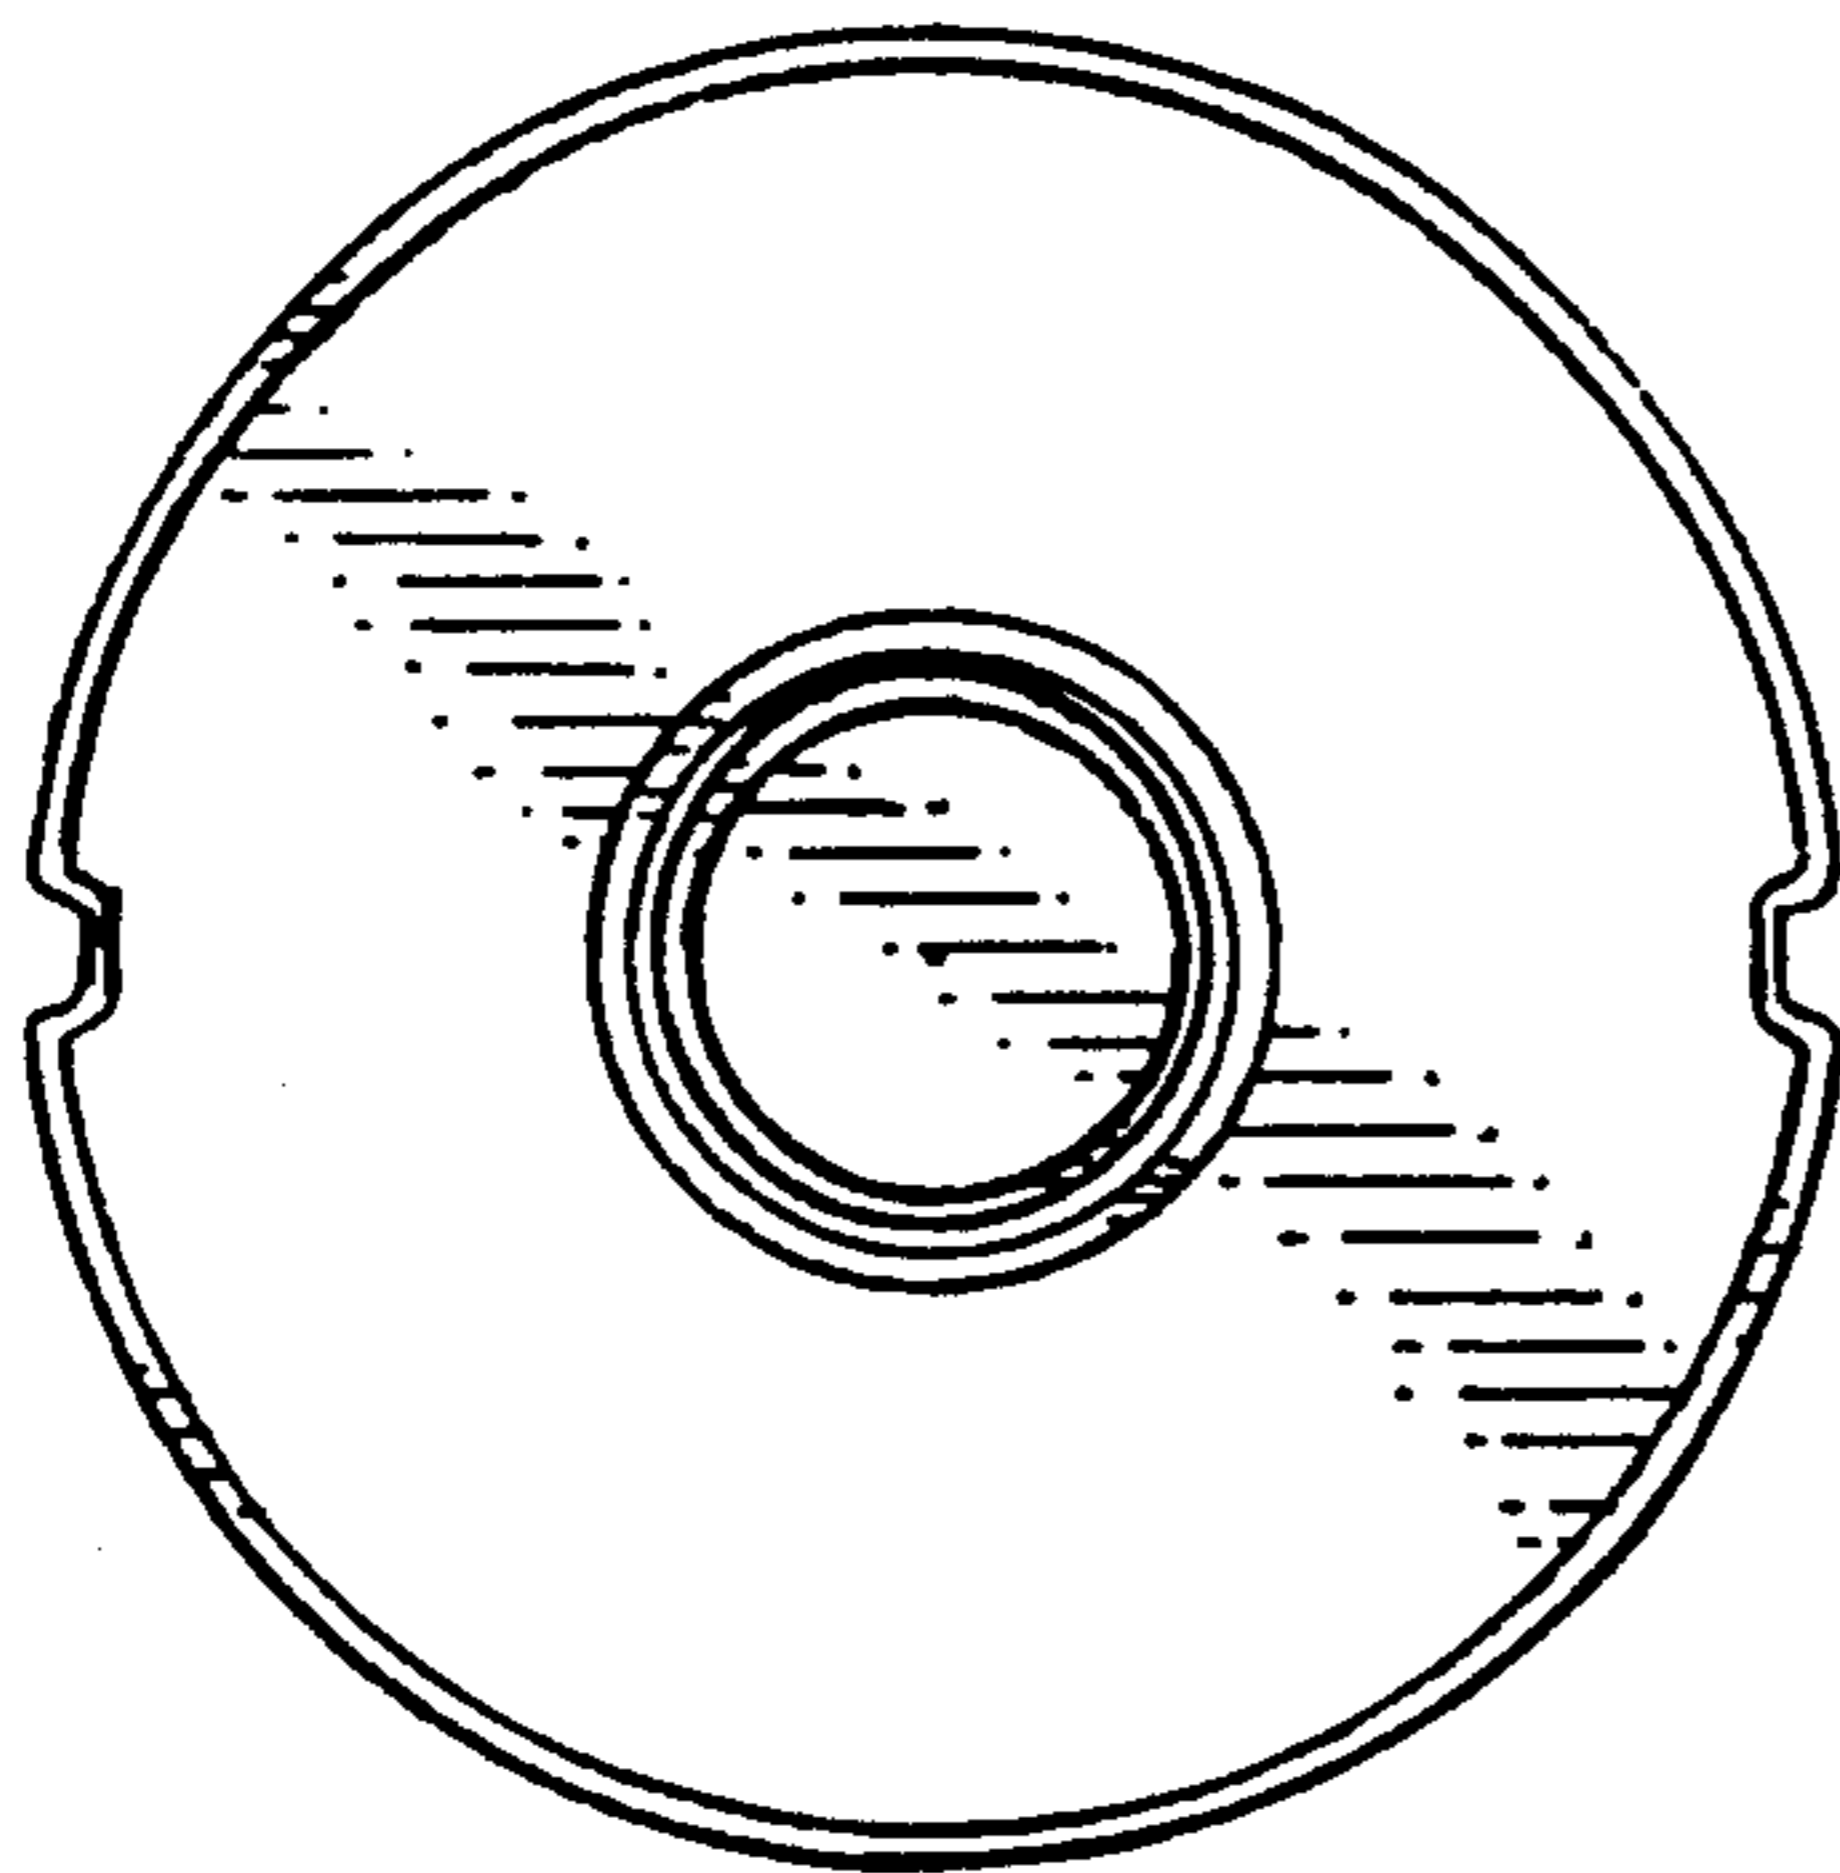


FIG. 4

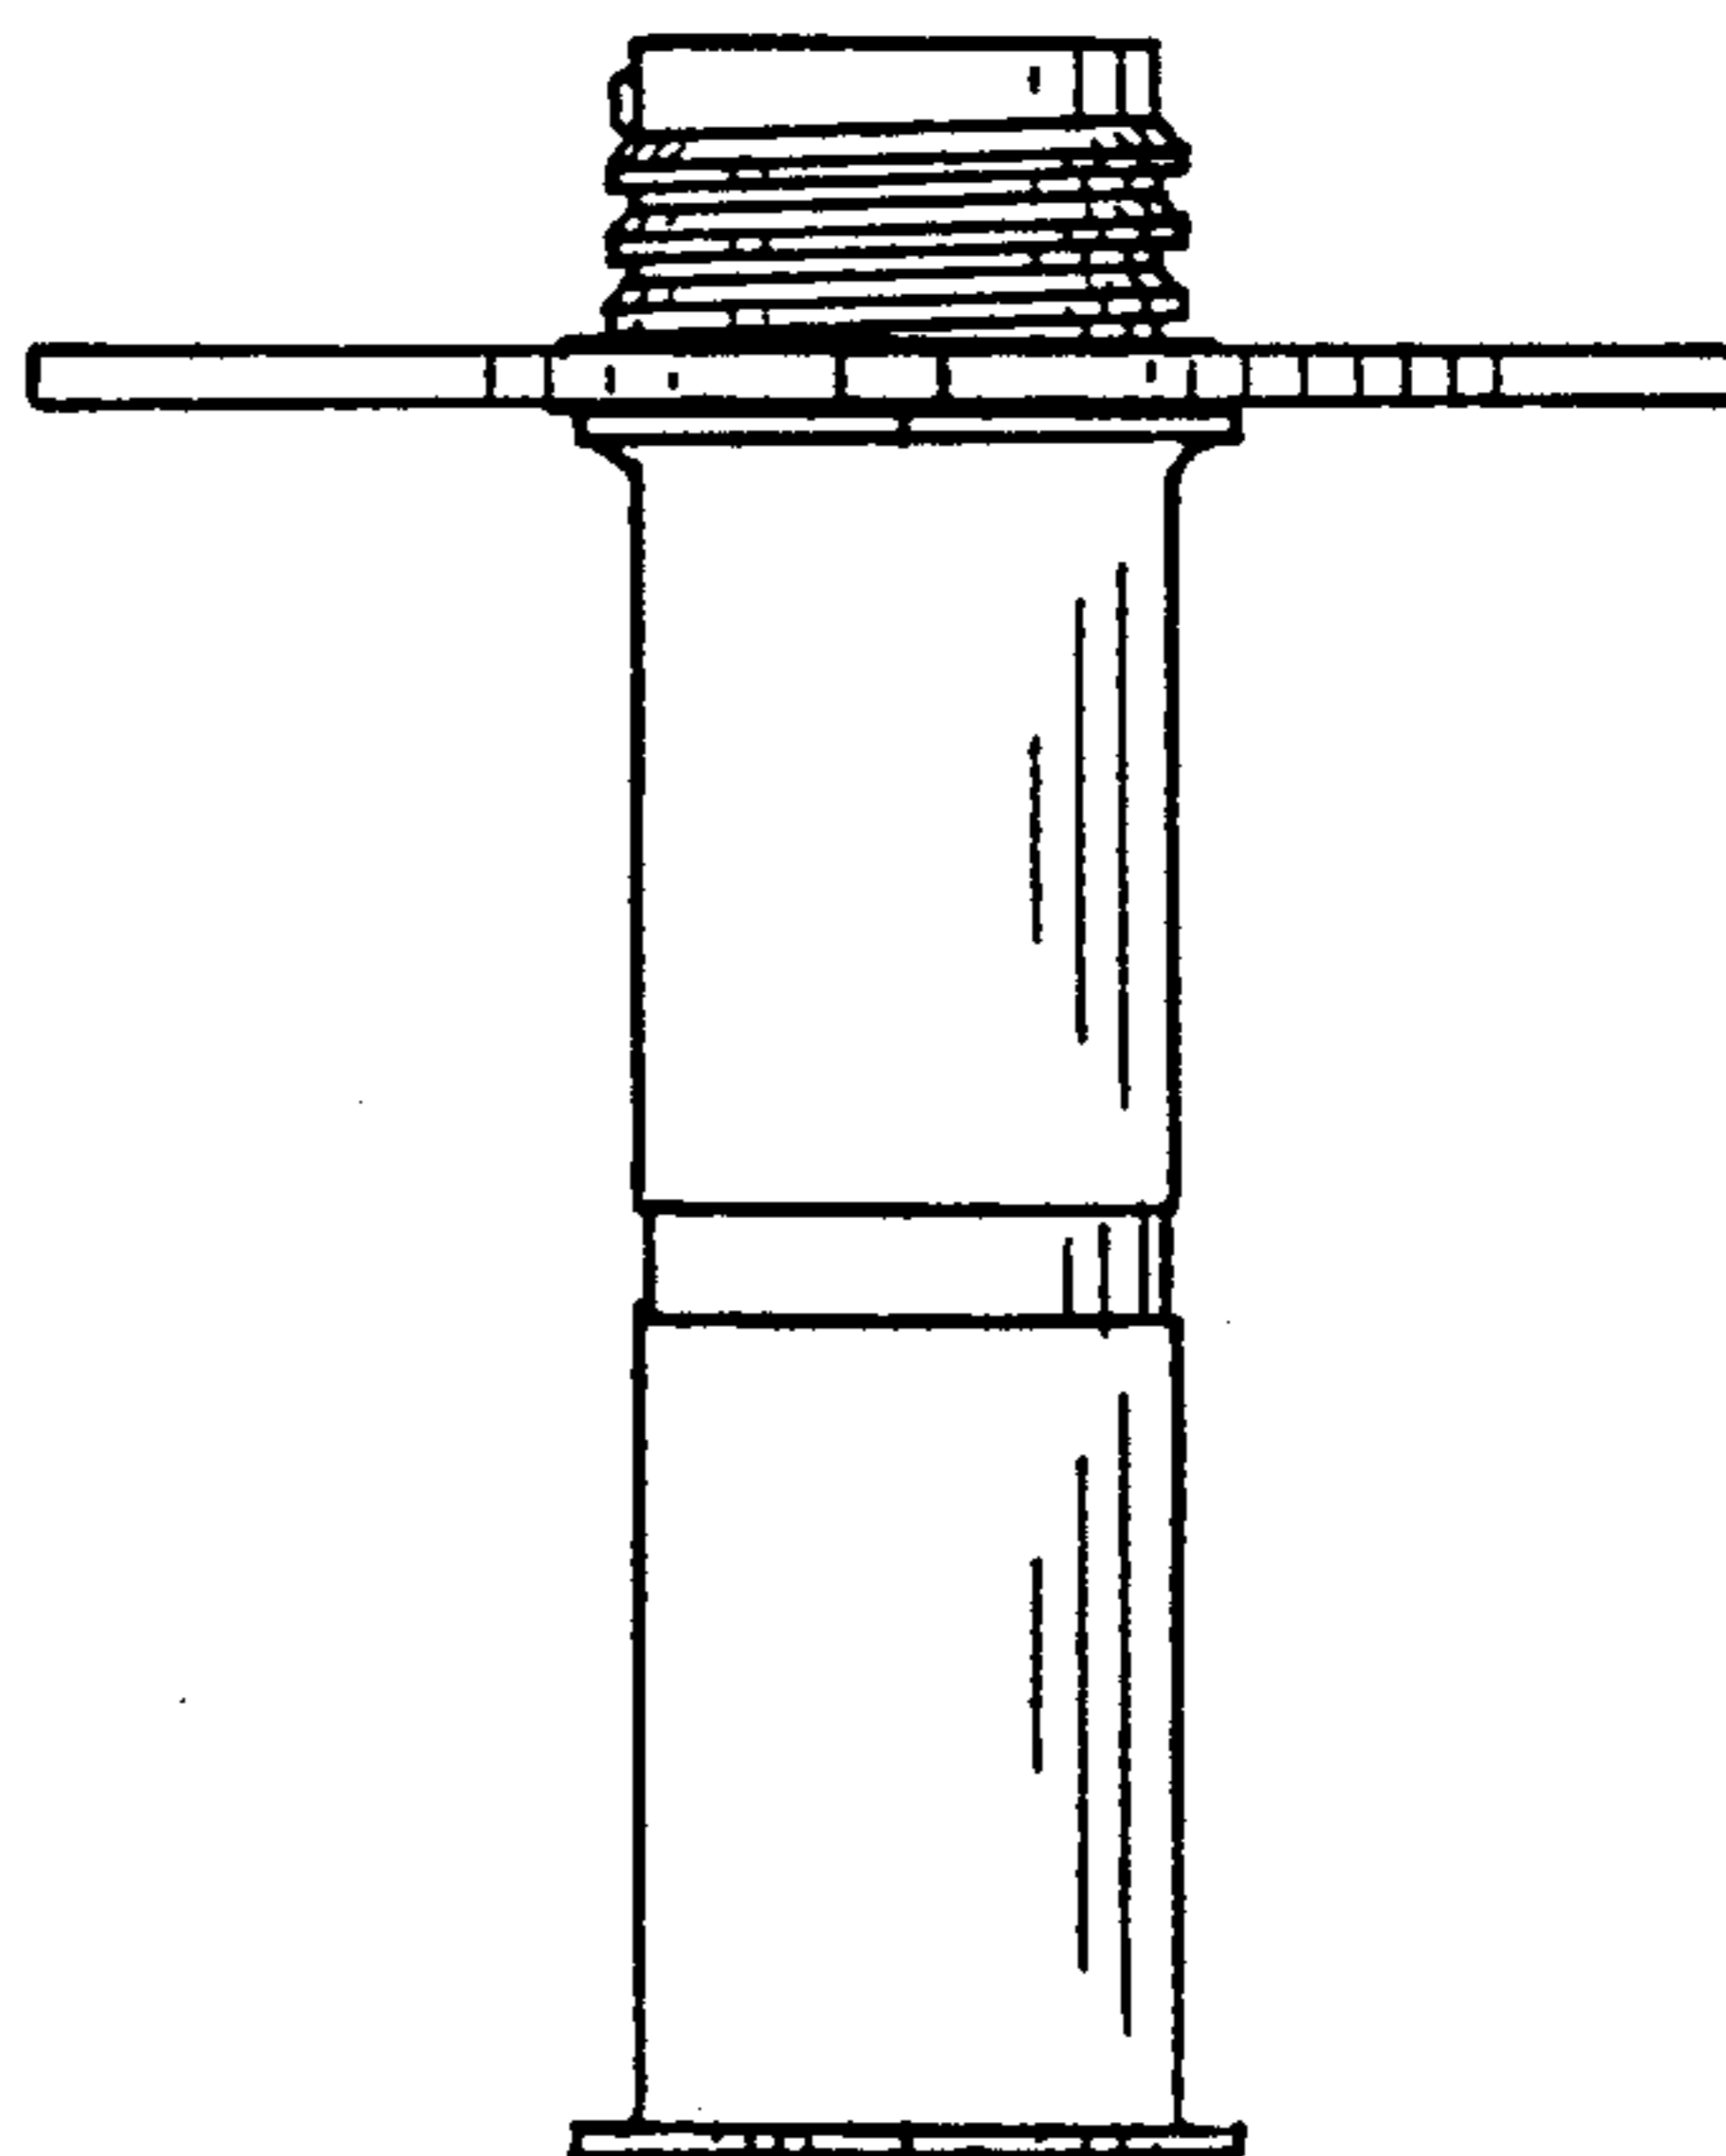


FIG. 3

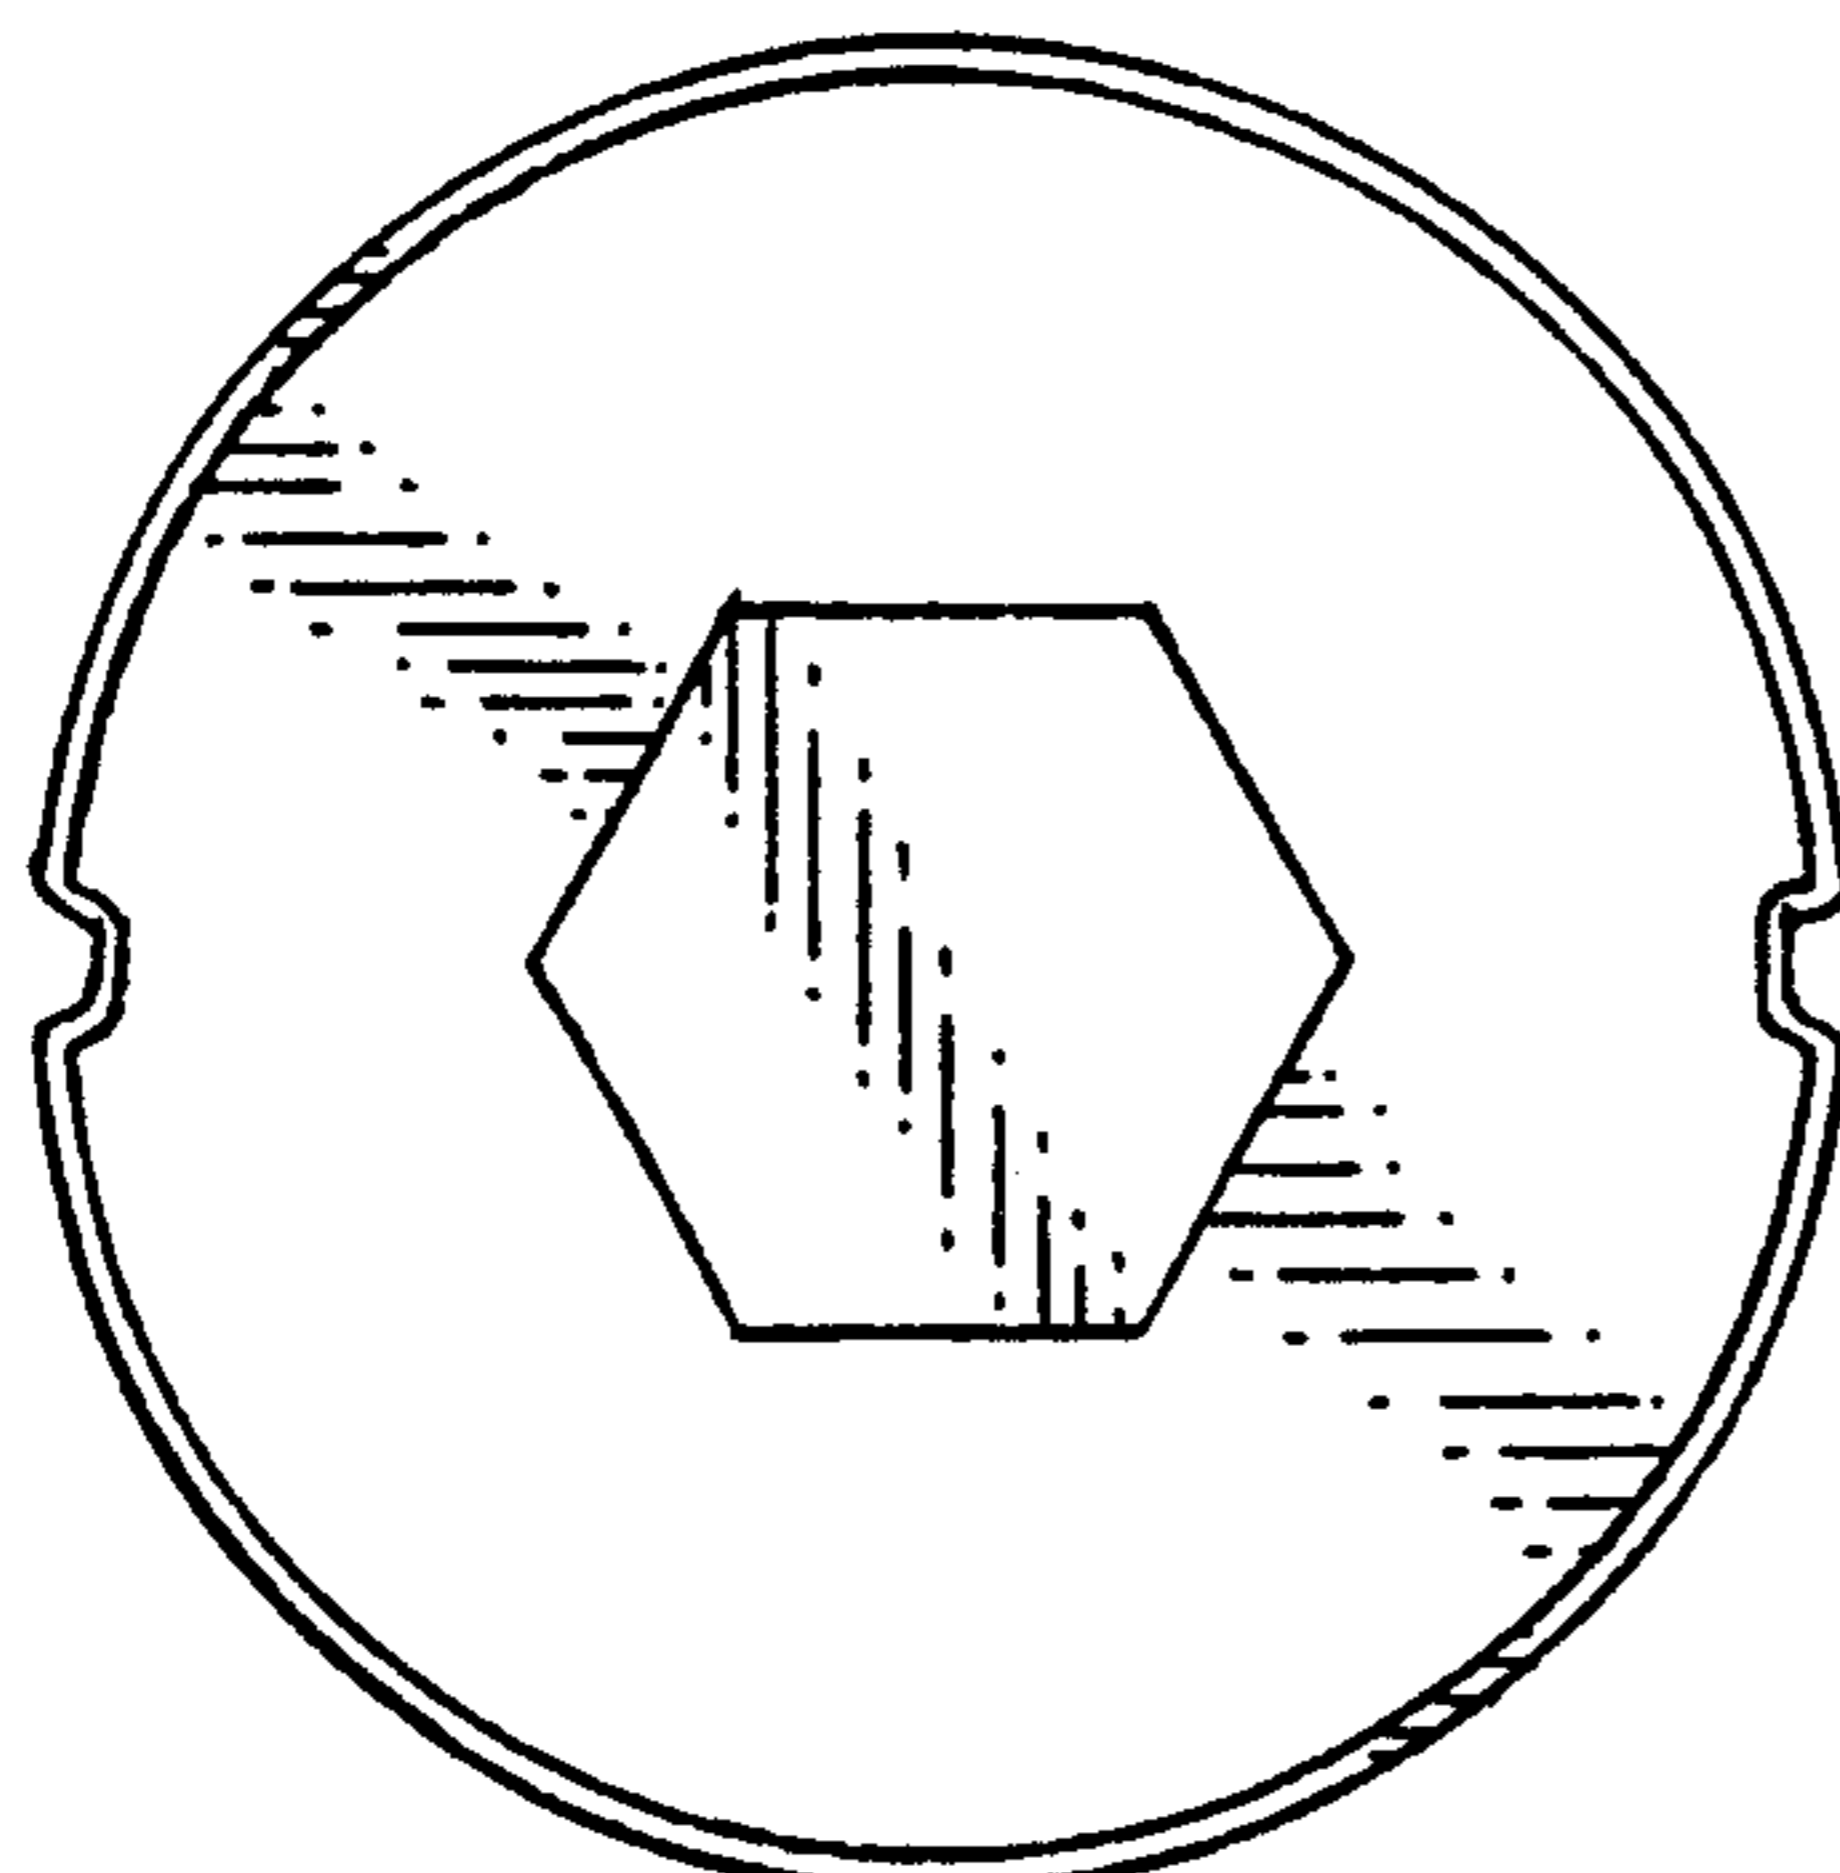


FIG. 5