

[54] EXPOSURE CONTROLLER FOR DENTAL X-RAY UNIT

[75] Inventor: Tetsuya Endo, Yokohama, Japan

[73] Assignee: Kabushiki Kaisha Tokyo Emix, Saitama, Japan

[**] Term: 14 Years

[21] Appl. No.: 269,548

[22] Filed: Nov. 10, 1988

[30] Foreign Application Priority Data

Aug. 1, 1988 [JP] Japan 63-30932

[52] U.S. Cl. D24/158; D14/100

[58] Field of Search D24/1.1, 2, 17; D14/100, 105, 106; 378/38

[56] References Cited

U.S. PATENT DOCUMENTS

D. 221,909 9/1971 De Lucia D24/2

D. 245,863 9/1977 Armbruster D24/1.1

D. 264,467 5/1982 Fischer D14/100 X

D. 291,195 8/1987 Shea D14/100

D. 294,371 2/1988 Phelps D24/2 X

D. 299,953 2/1989 King et al. D24/1.1

D. 302,809 8/1989 Boucher D14/100

D. 303,521 9/1989 Savio et al. D14/100

D. 308,420 6/1990 Frantz D24/17

Primary Examiner—Wallace R. Burke

Assistant Examiner—Freda S. Nunn

Attorney, Agent, or Firm—Fred Philpitt

[57] CLAIM

The ornamental design for an exposure controller for dental X-ray unit, as shown and described.

DESCRIPTION

FIG. 1 is a top, front perspective view of an exposure controller for dental X-ray unit showing my new design;

FIG. 2 is a front elevational view thereof;

FIG. 3 is a right side elevational view thereof;

FIG. 4 is a top plan view thereof;

FIG. 5 is a bottom plan view thereof;

FIG. 6 is a rear elevational view thereof;

FIG. 7 is a left side elevational view thereof.

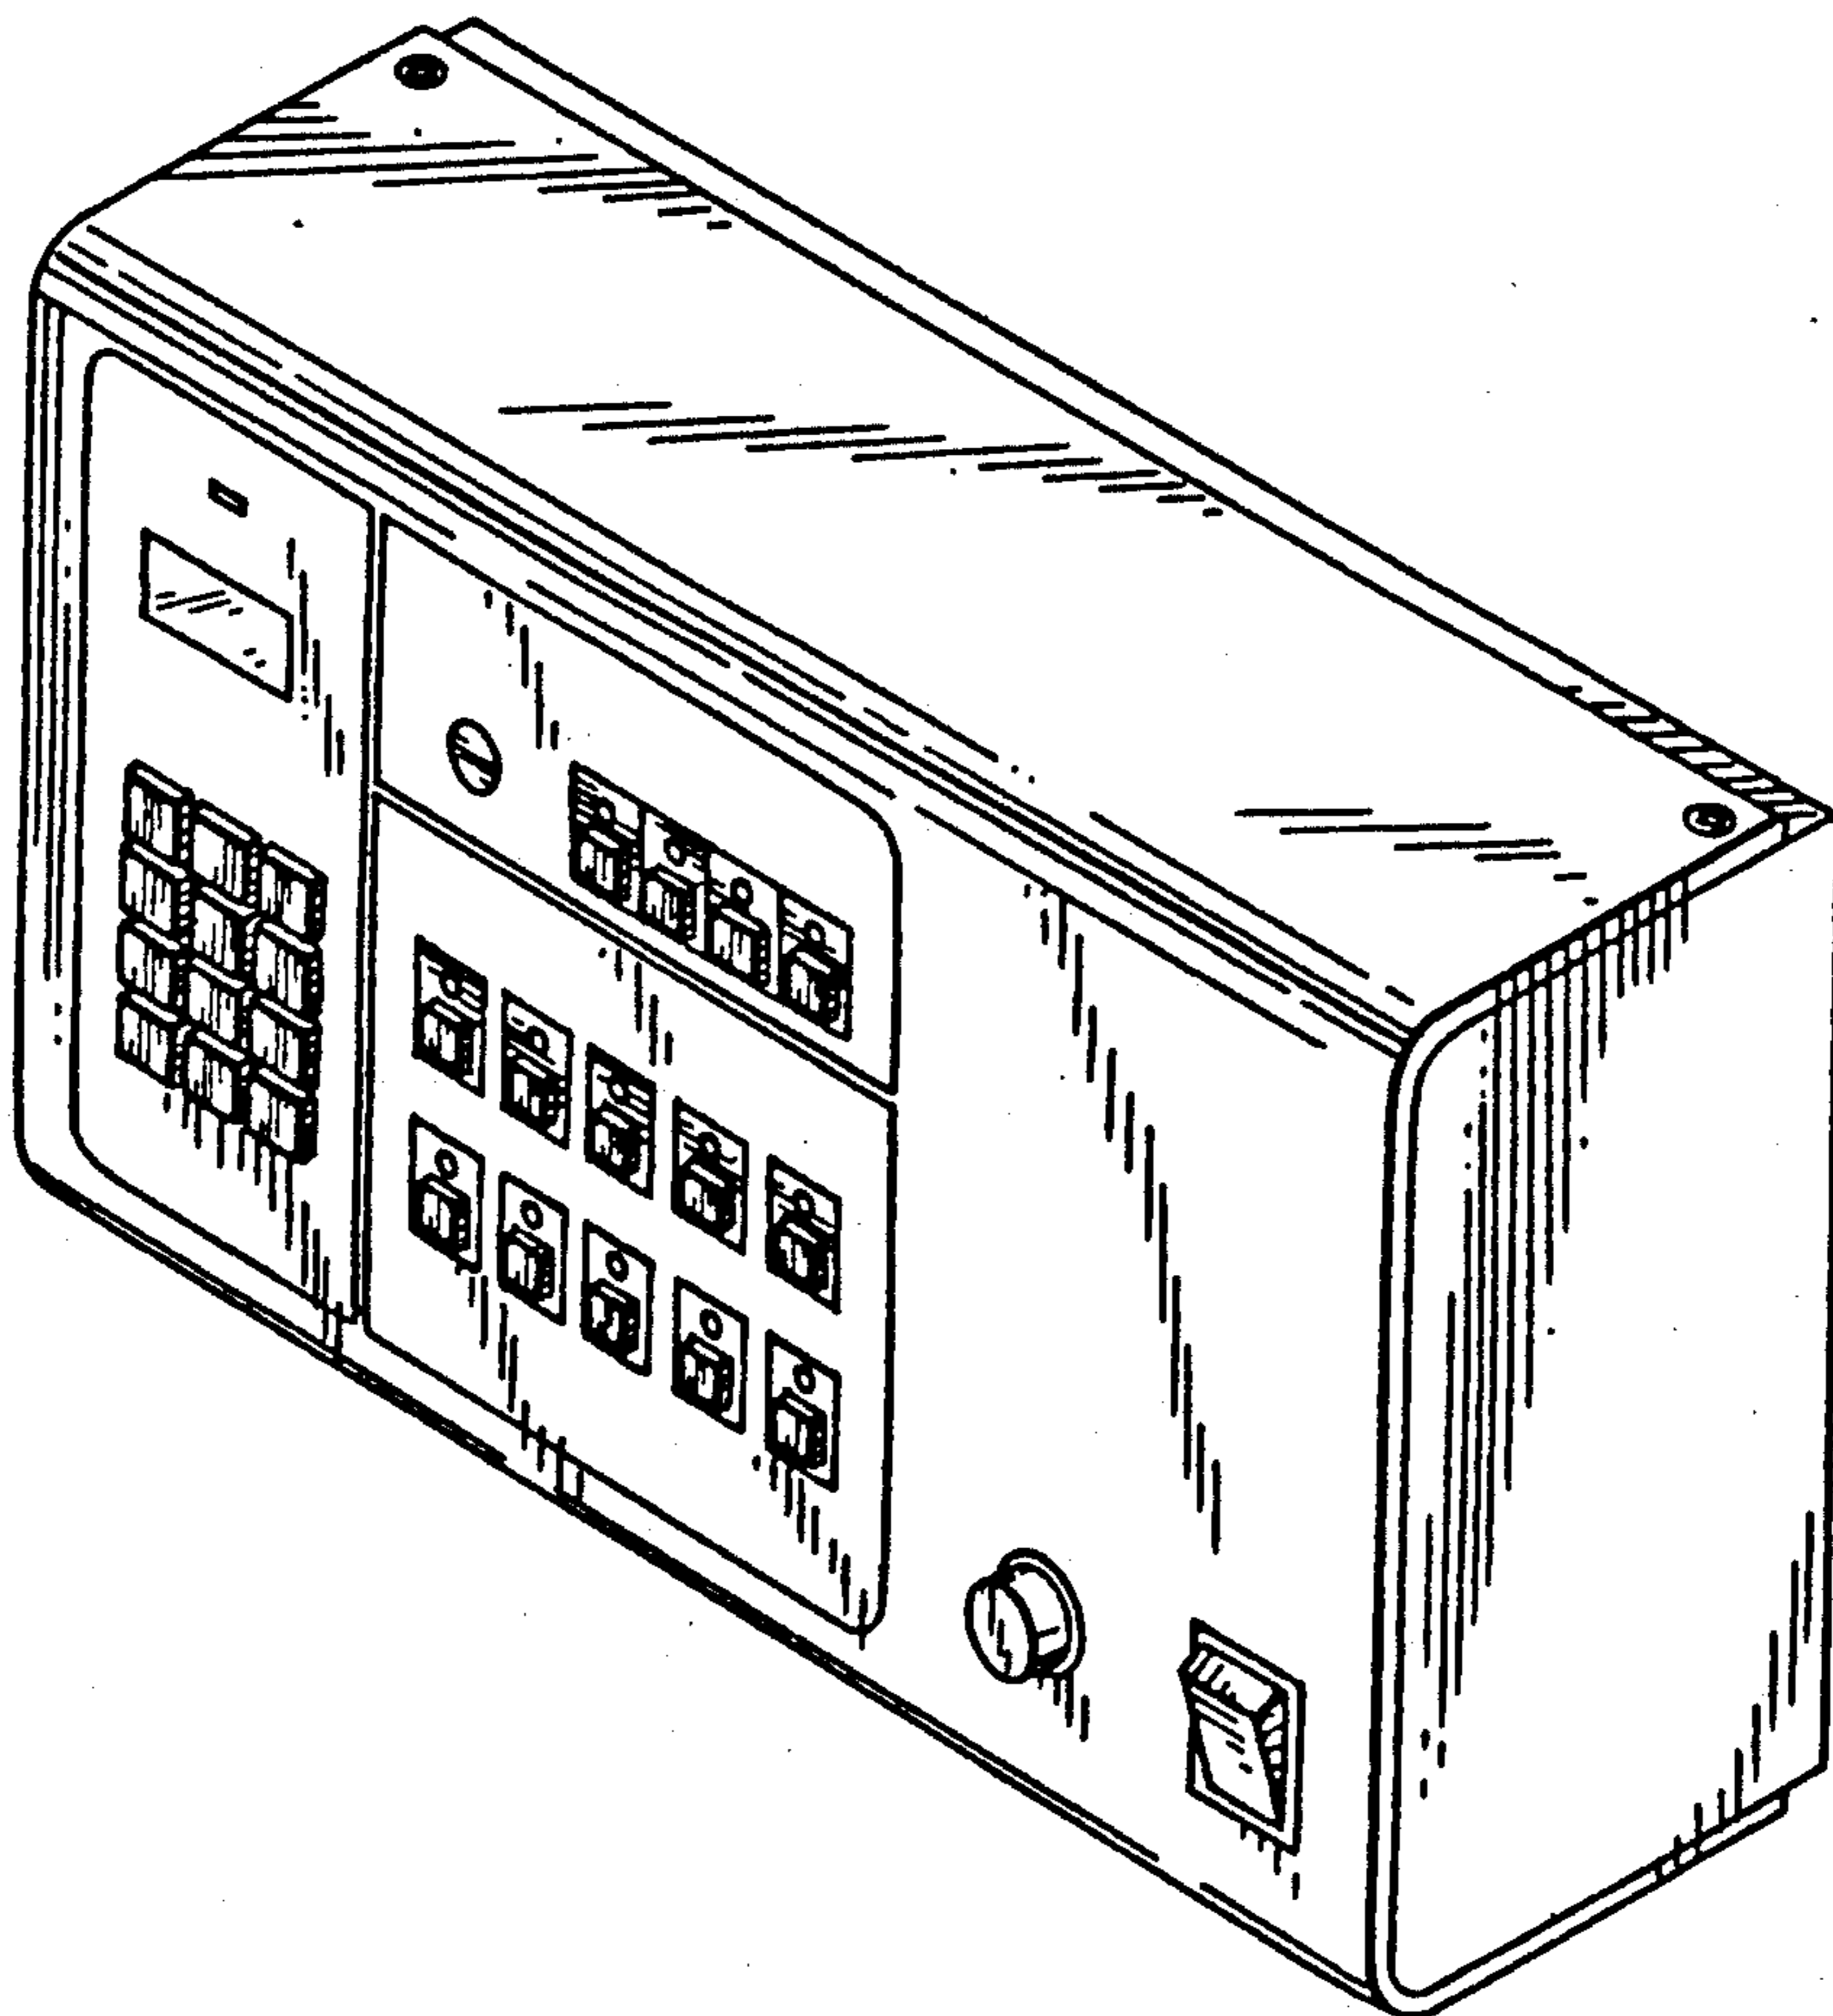


FIG. 1

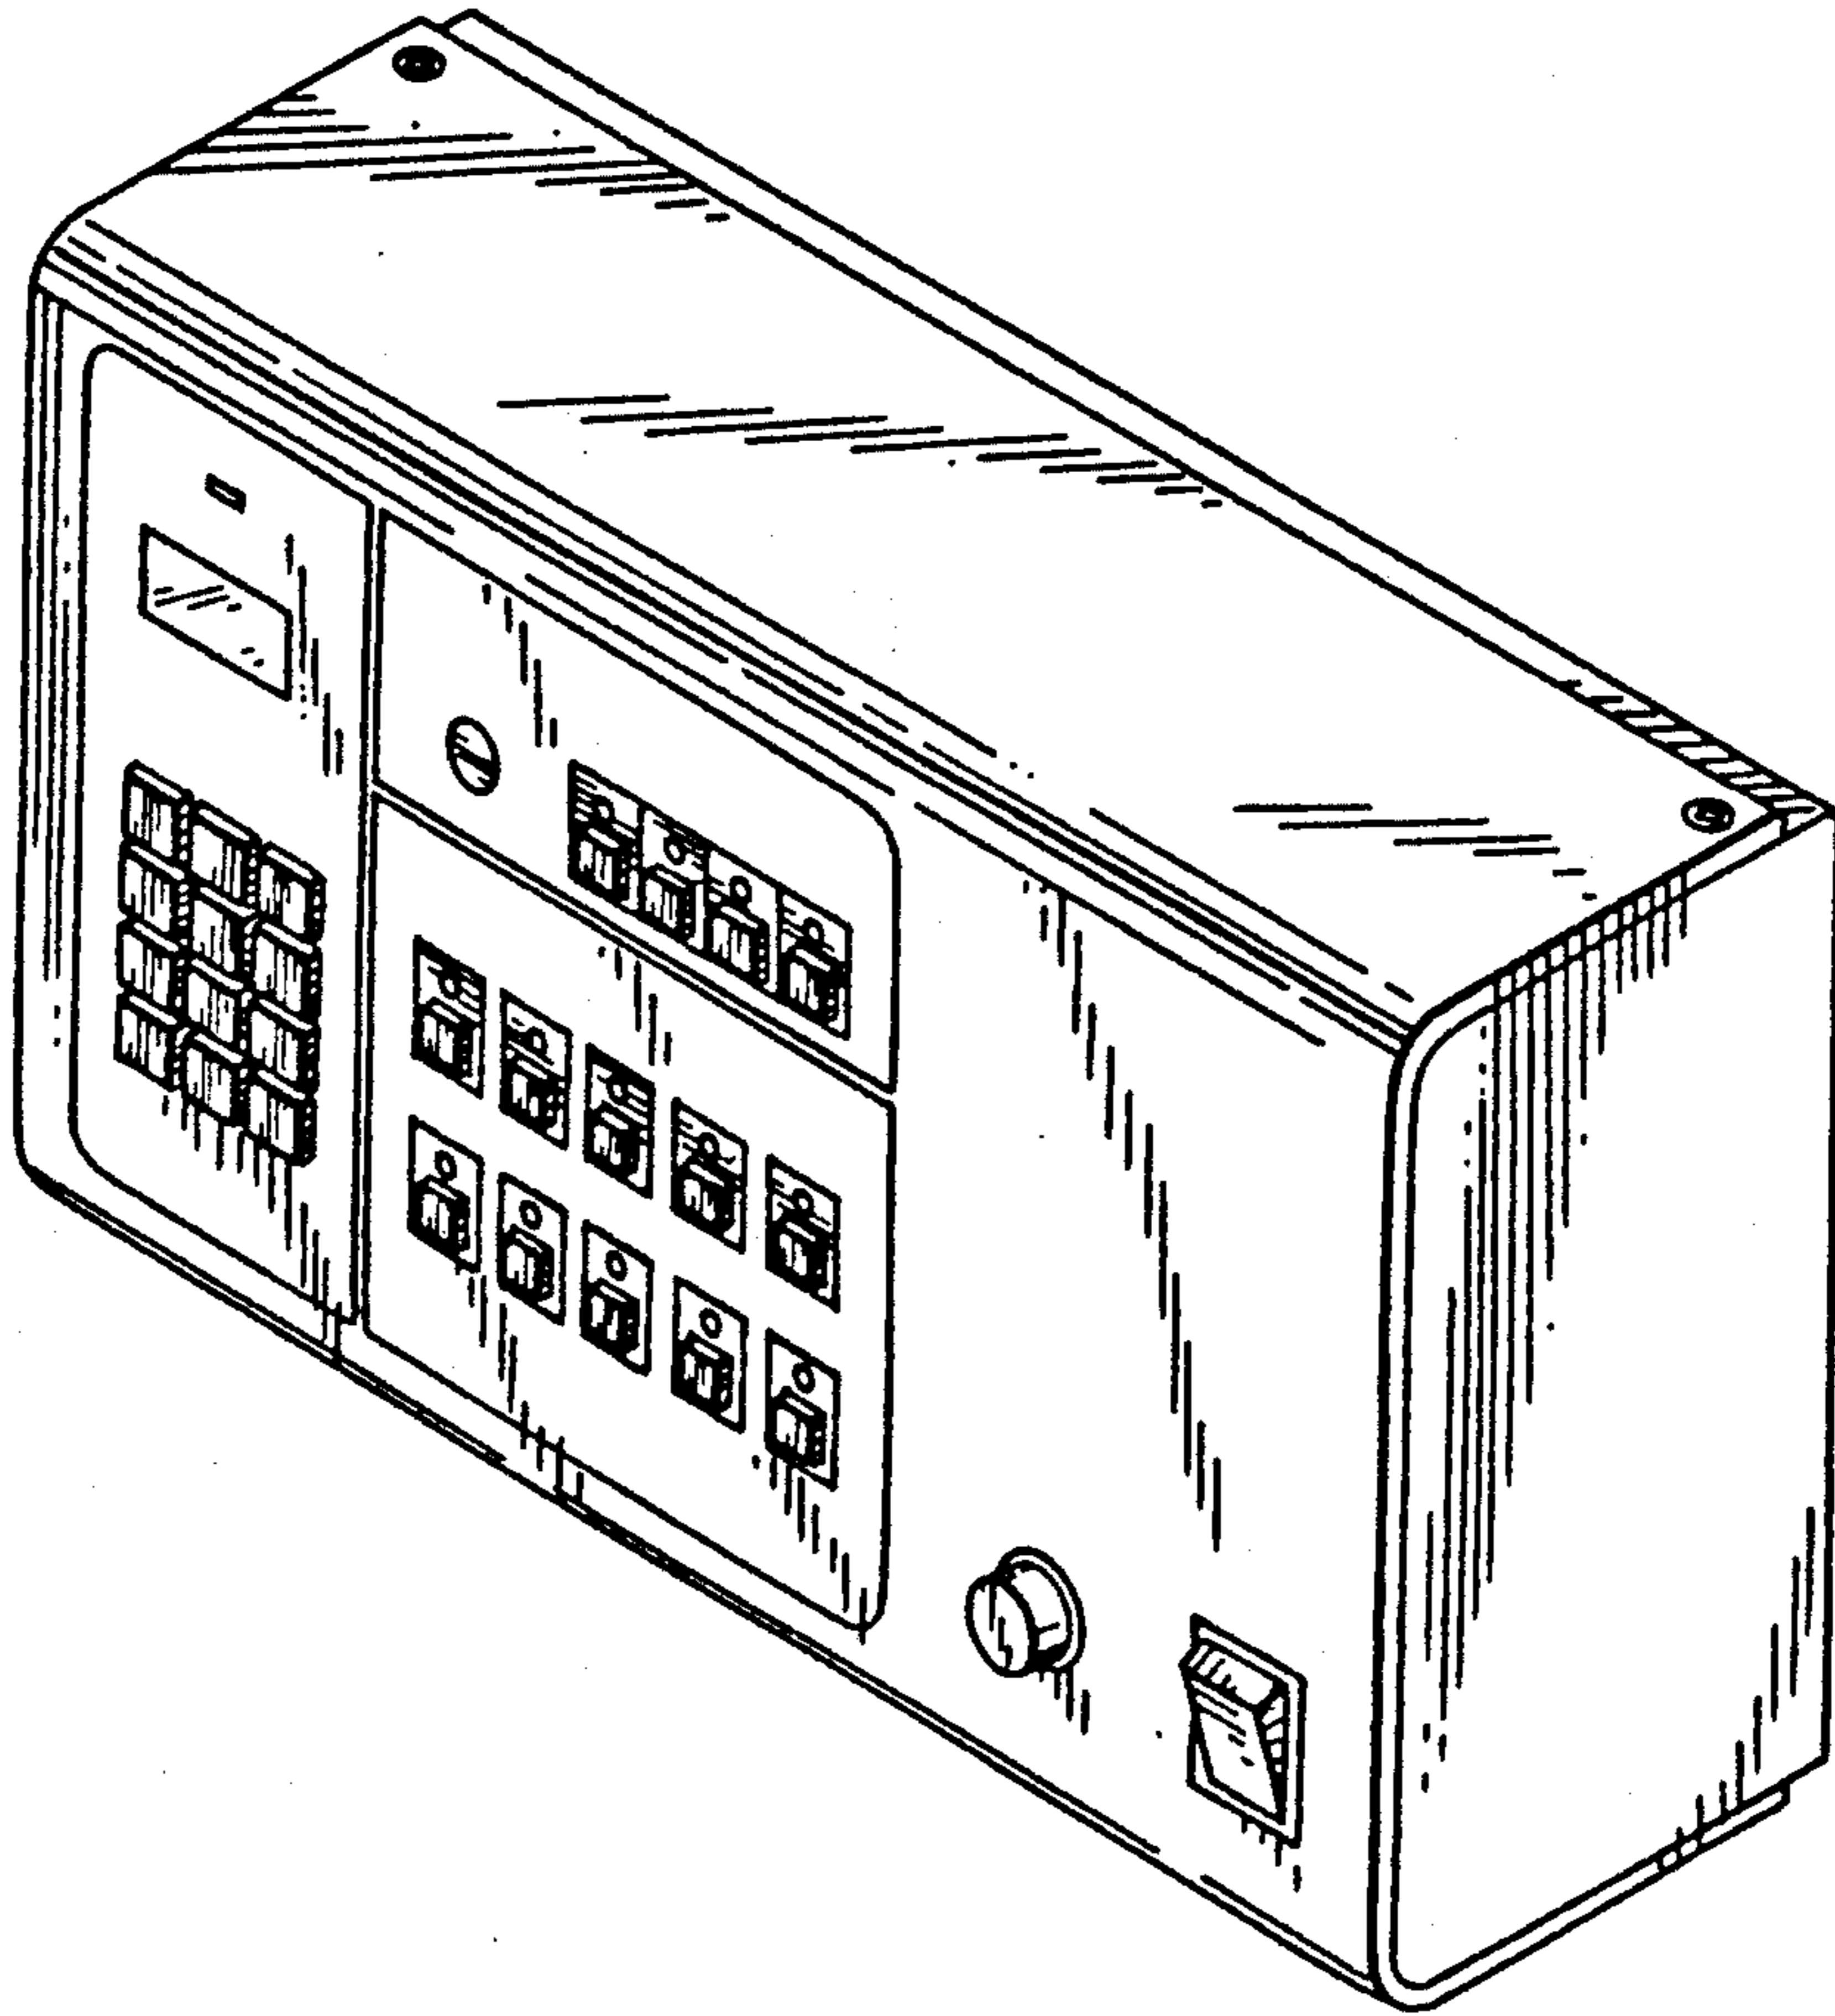


FIG. 2

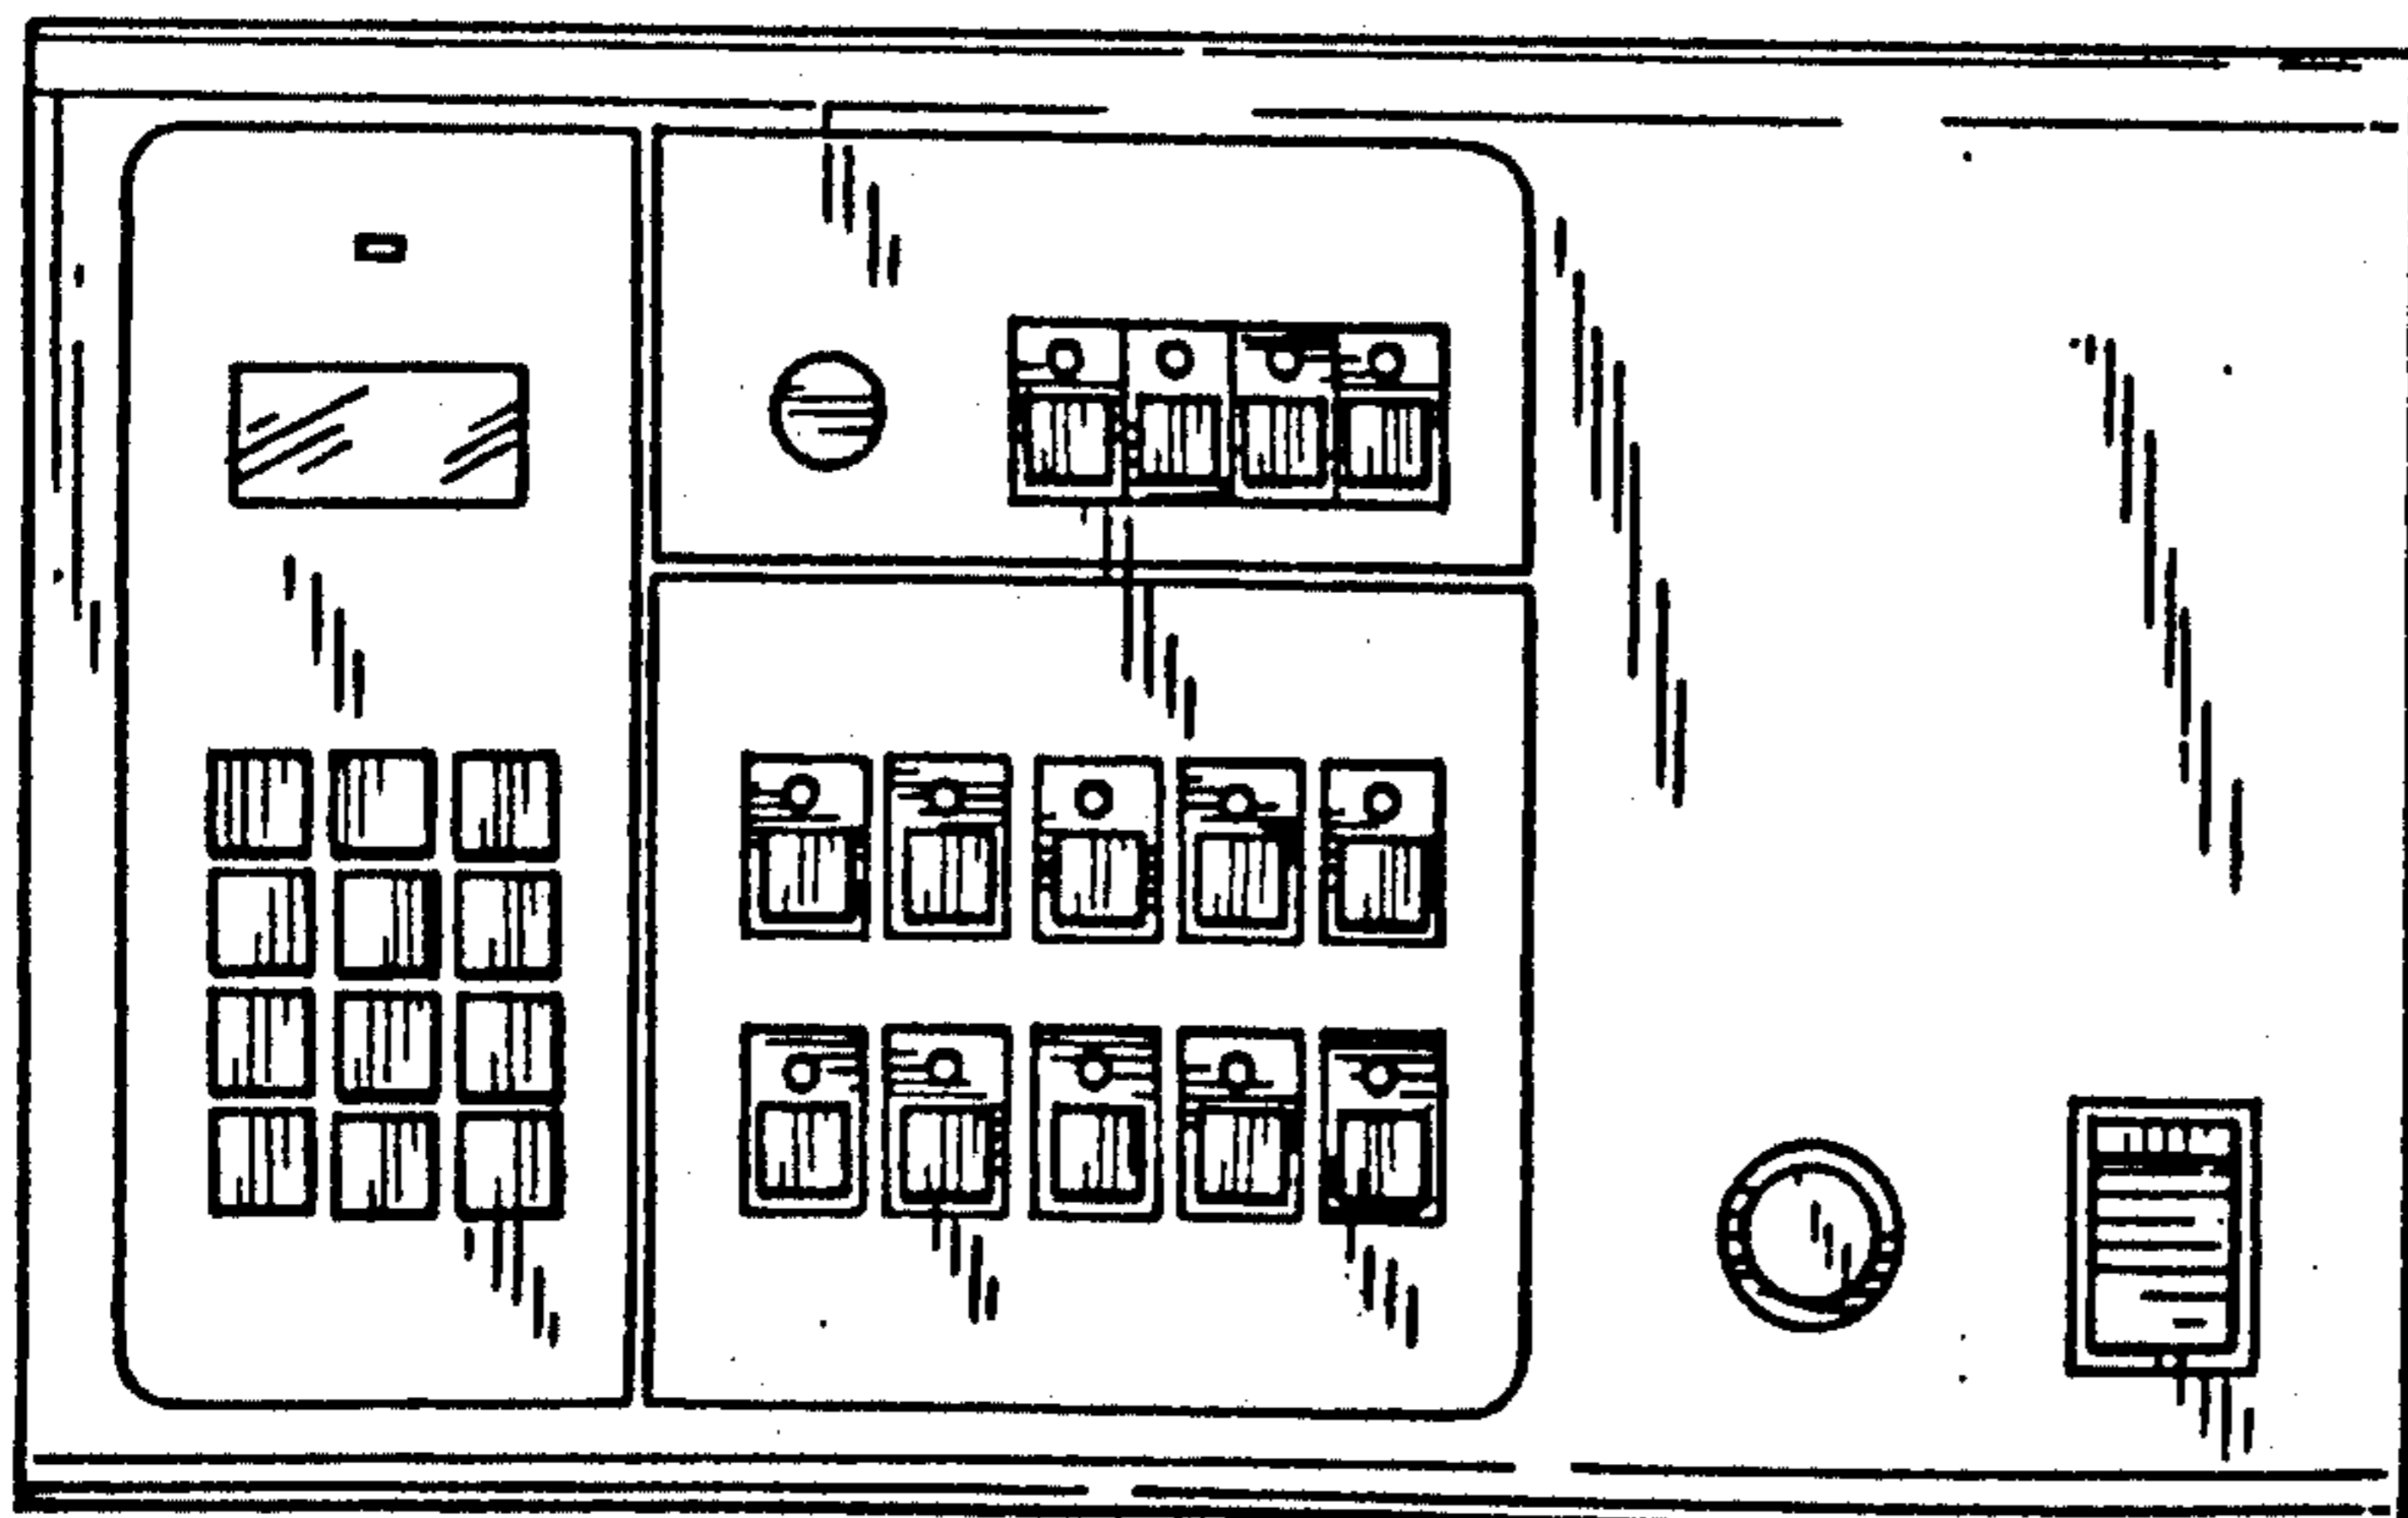


FIG. 3

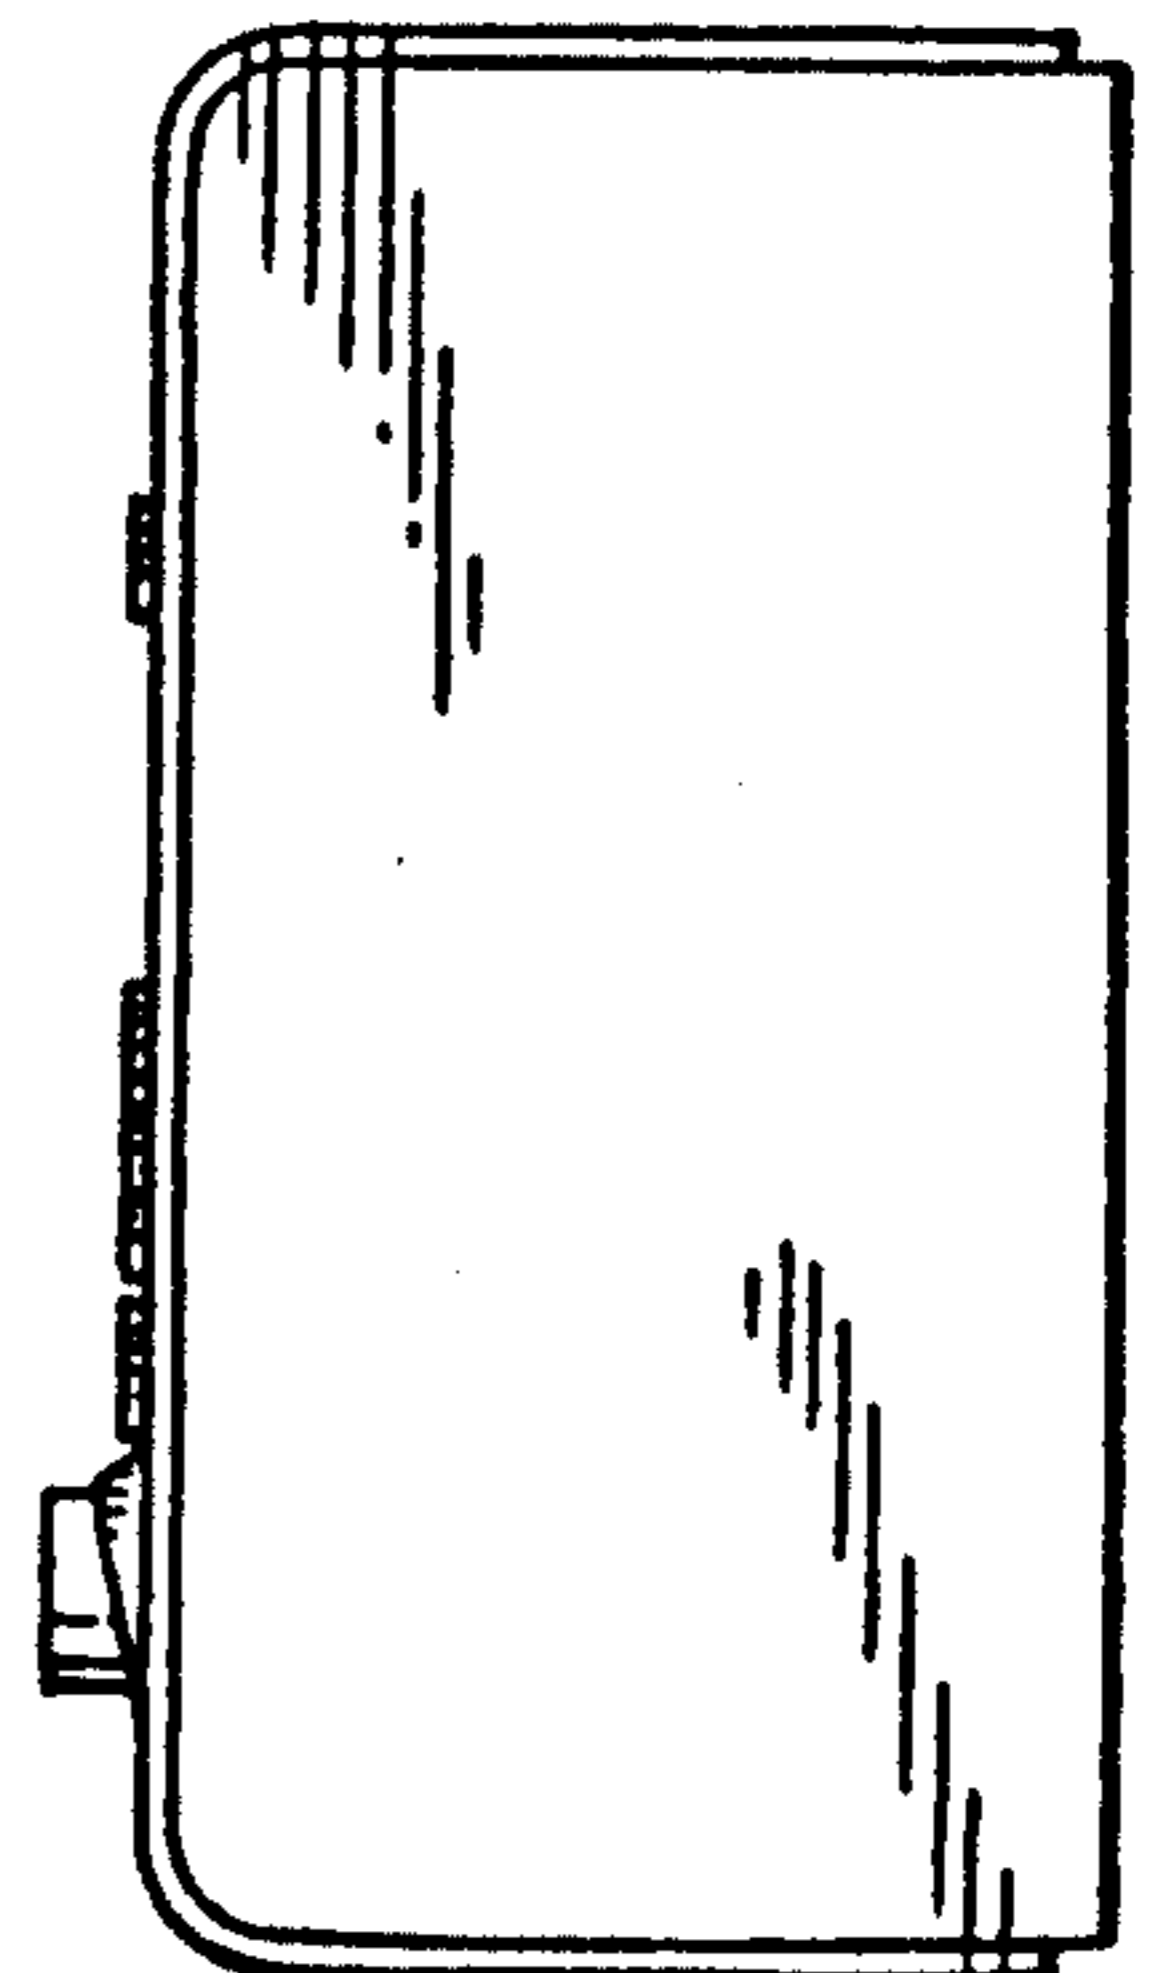


FIG. 4

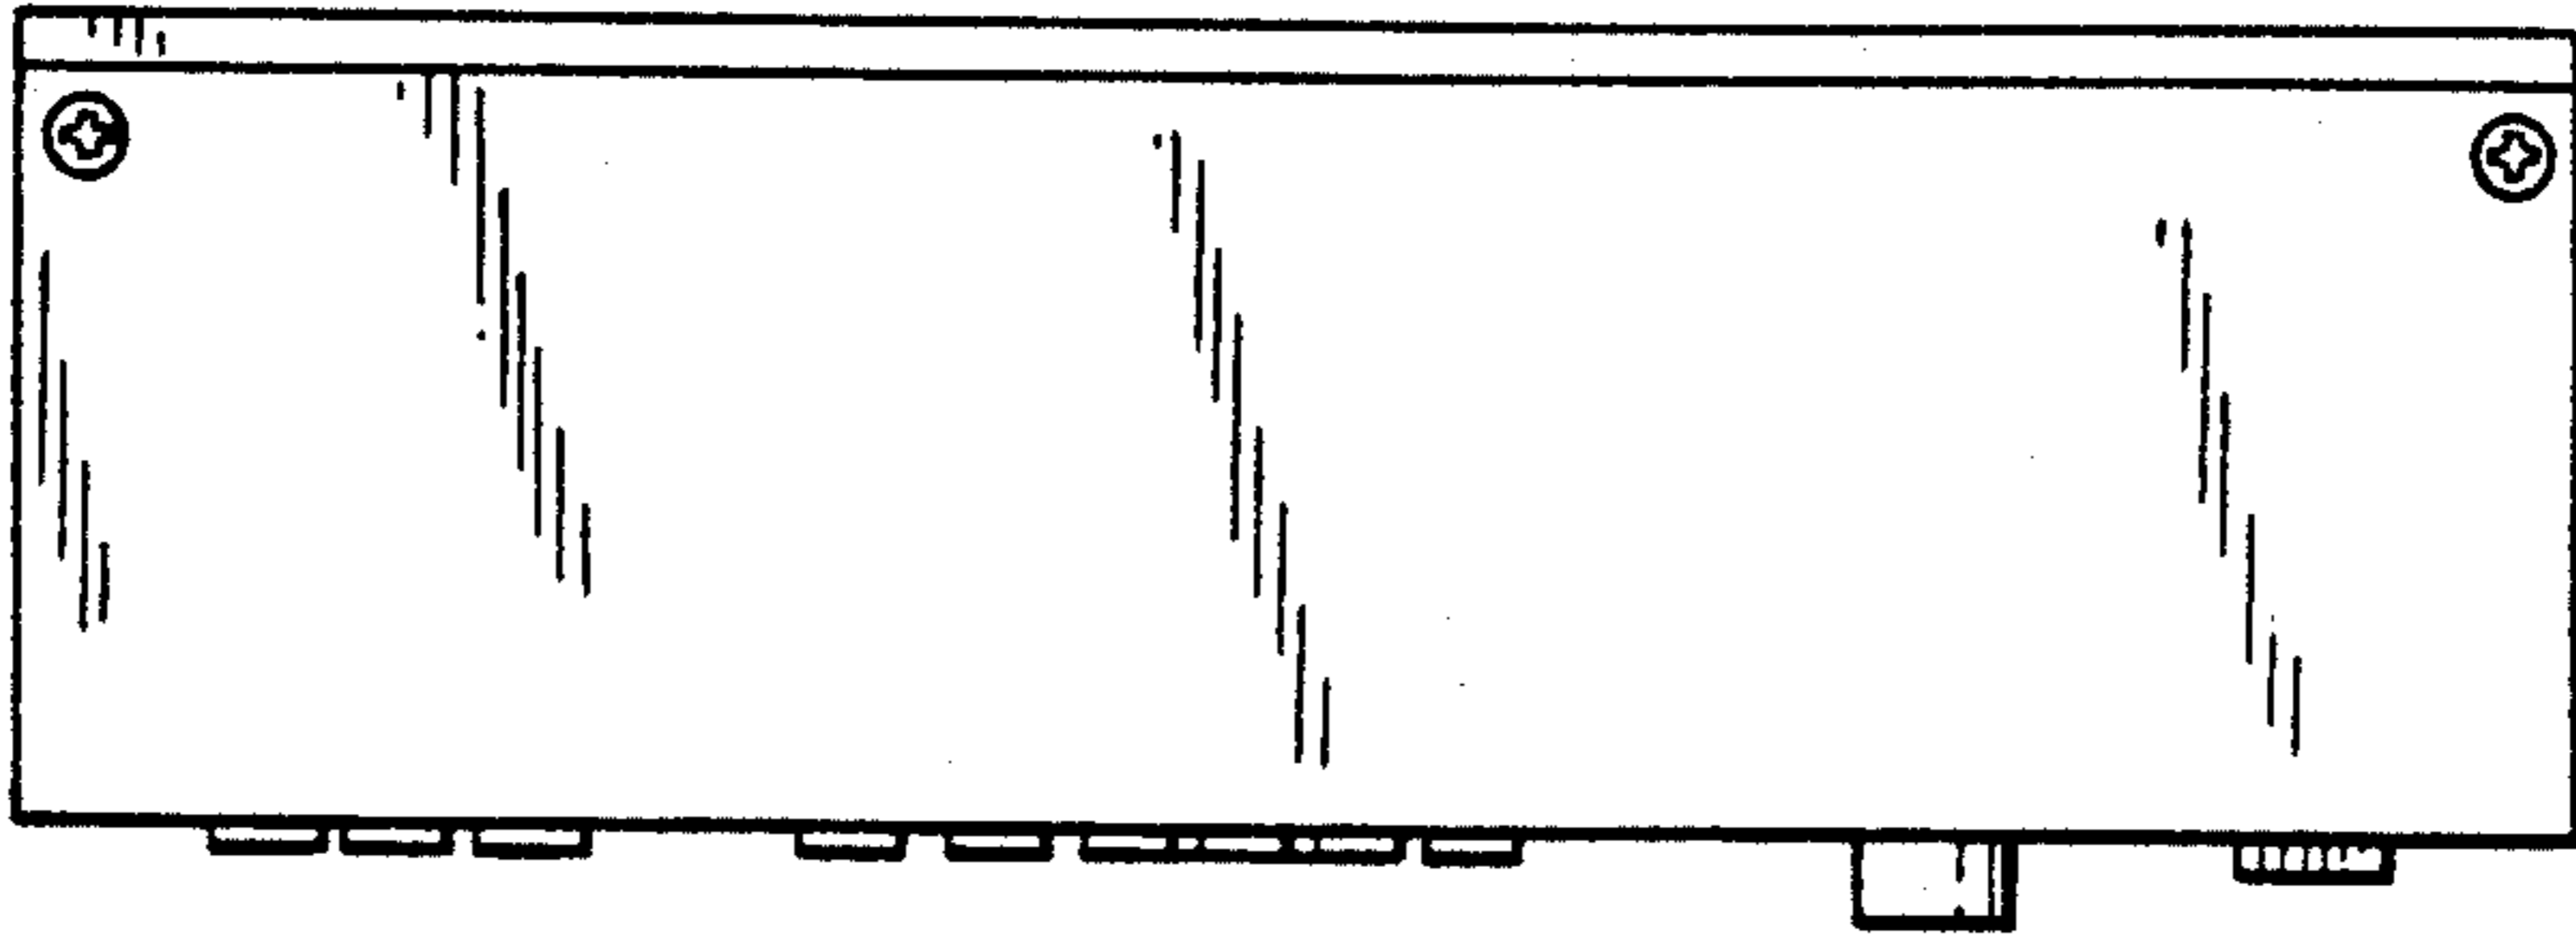


FIG. 5

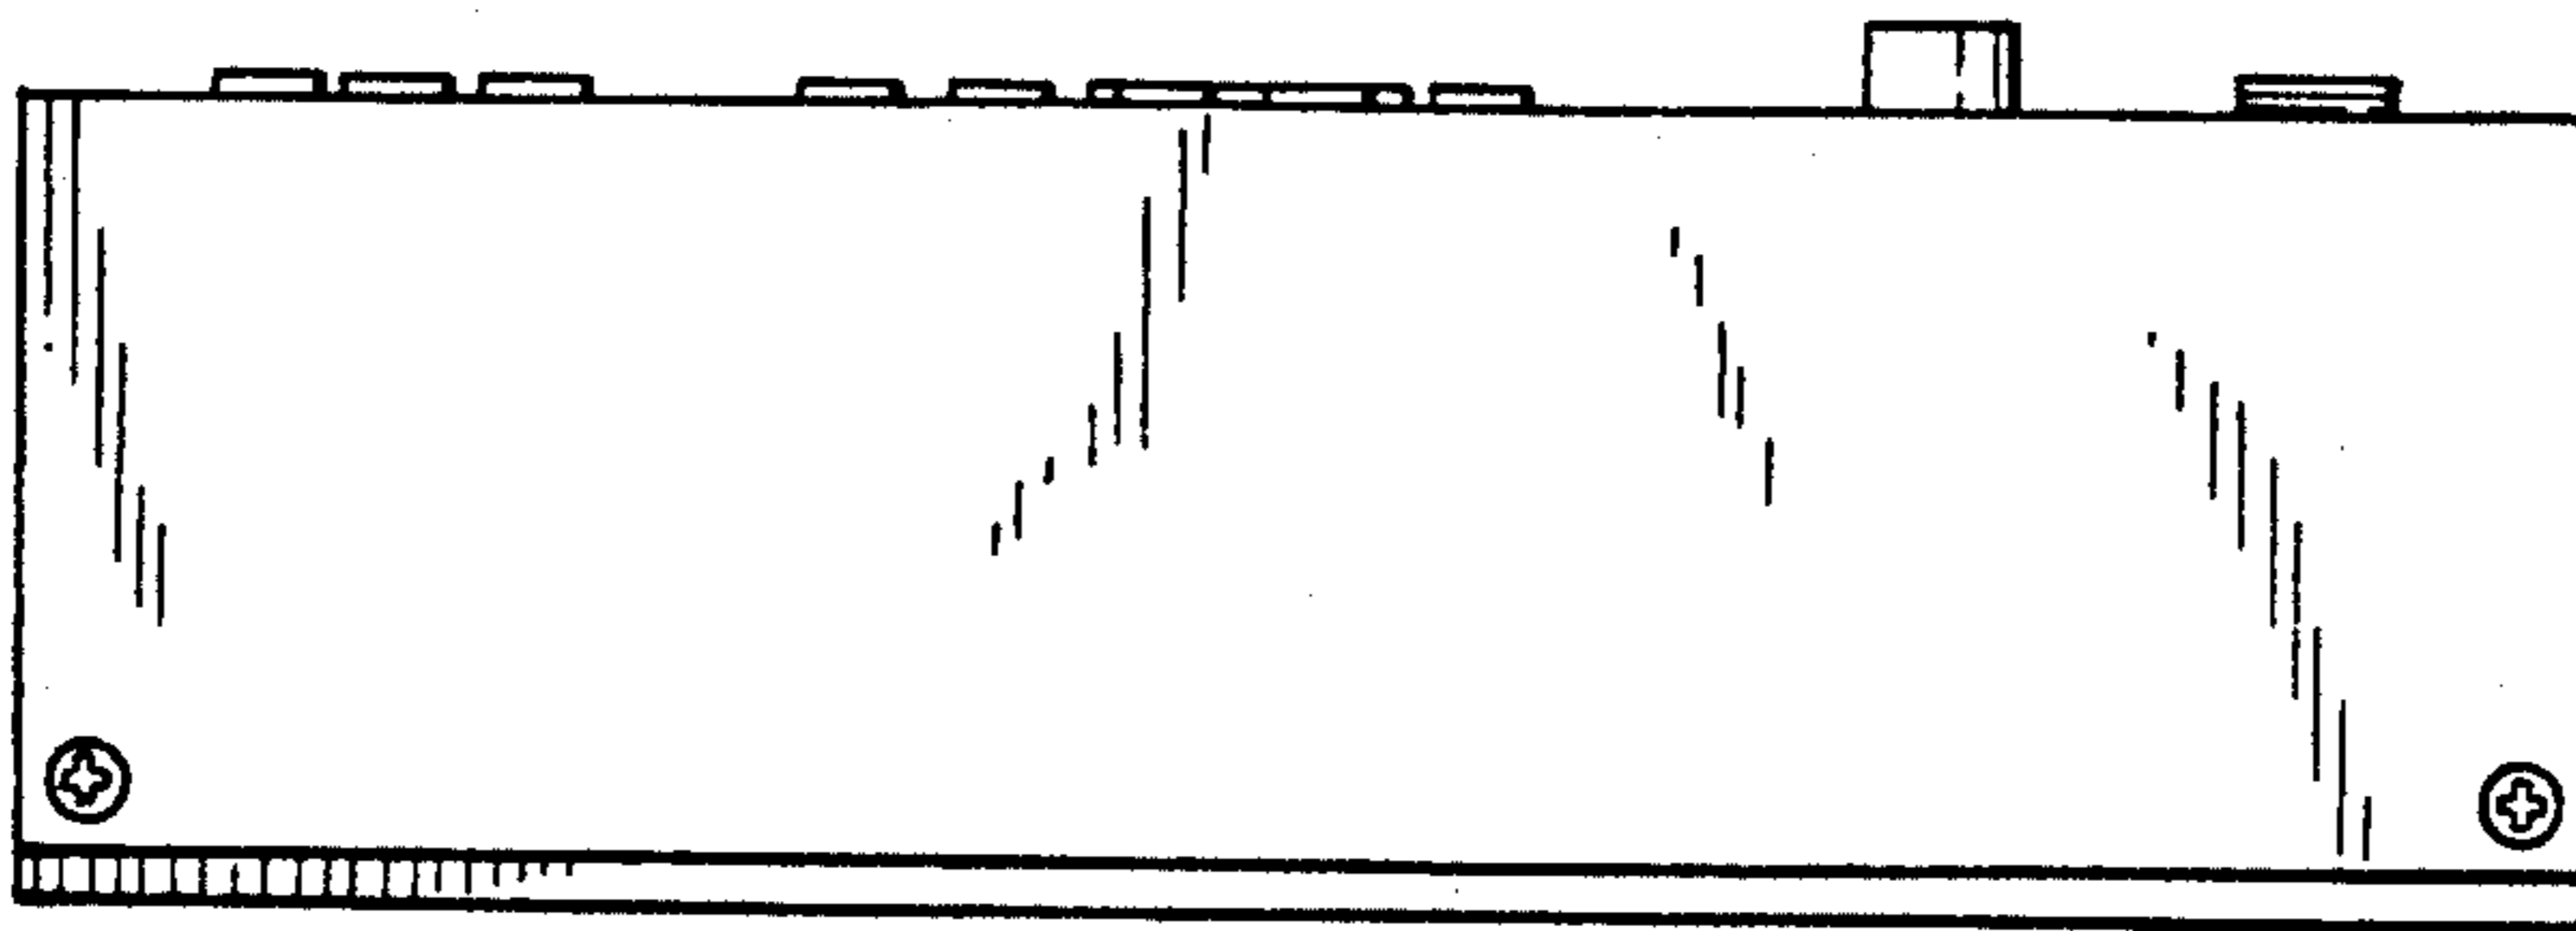


FIG. 6

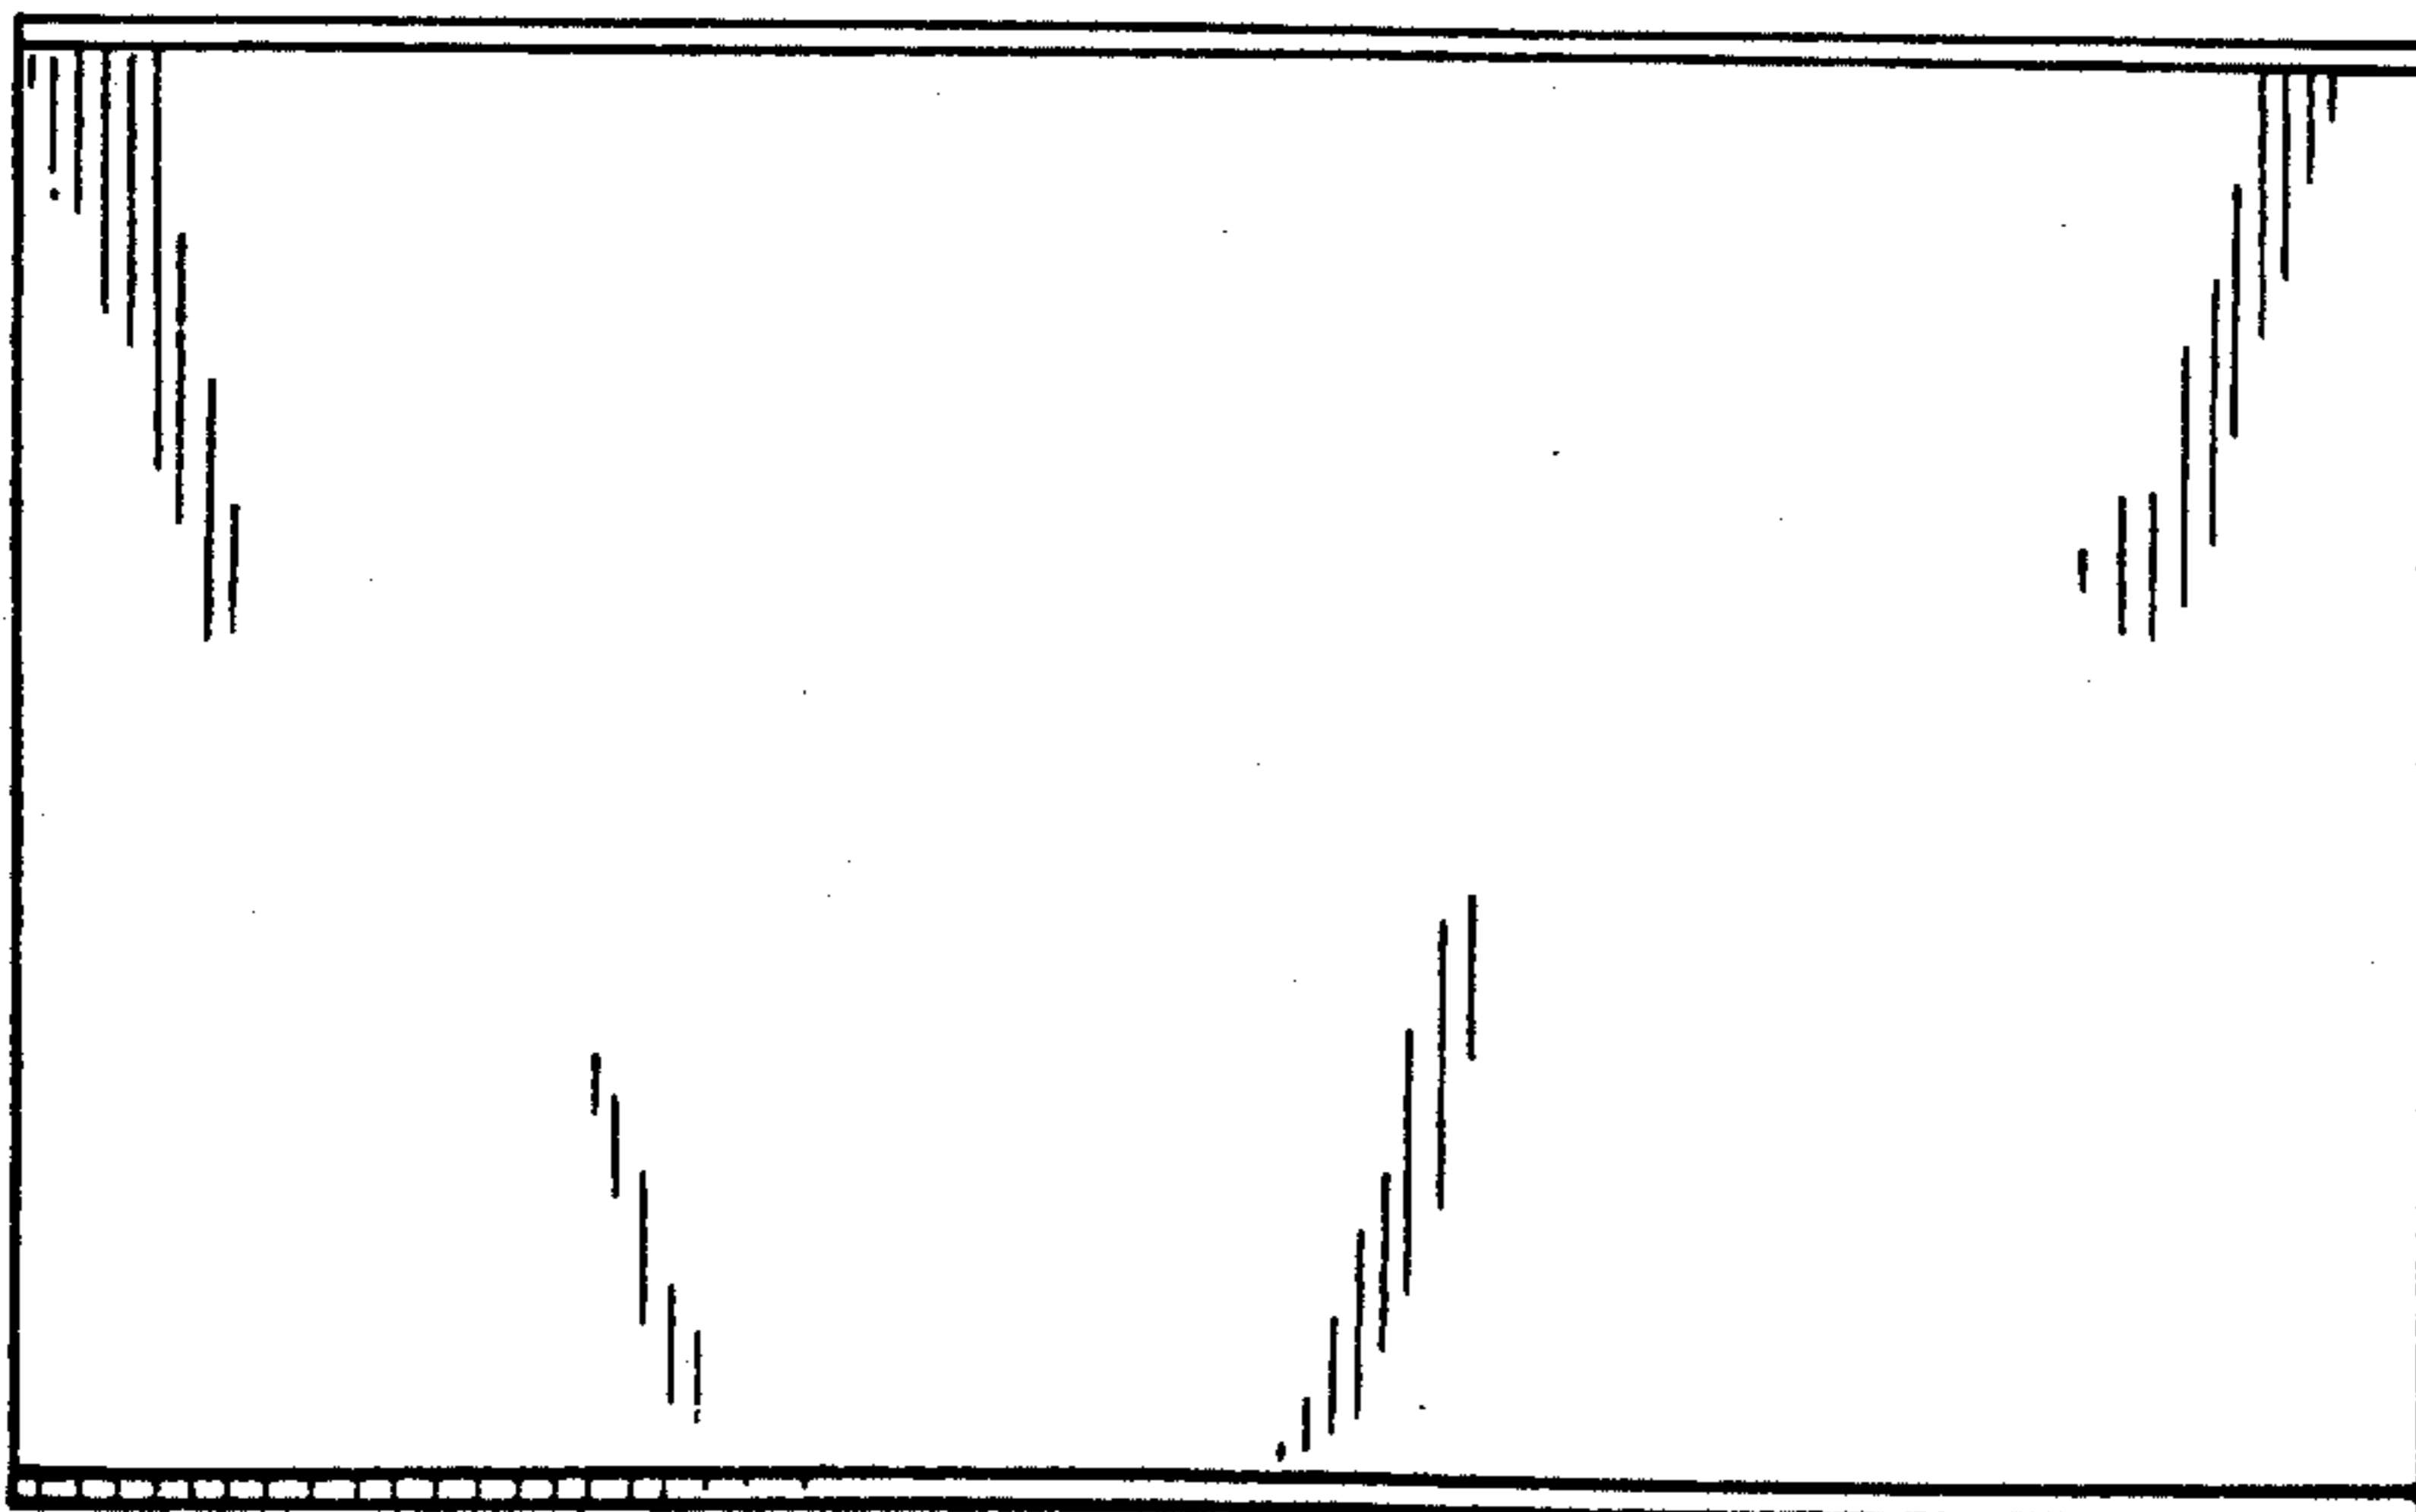


FIG. 7

