

United States Patent [19]

Yokoyama et al.

[11] Patent Number: **Des. 320,443**

[45] Date of Patent: **** Oct. 1, 1991**

[54] CLINICAL CHEMISTRY ANALYZER

[75] Inventors: **Masaru Yokoyama, Tama; Hiroyasu Uchida, Katsuta; Tetsuaki Abe, Katsuta; Takehide Sato, Katsuta, all of Japan**

[73] Assignee: **Hitachi, Ltd., Tokyo, Japan**

[**] Term: **14 Years**

[21] Appl. No.: **259,610**

[22] Filed: **Oct. 19, 1988**

[30] Foreign Application Priority Data

Jul. 22, 1988 [JP] Japan 63-29110

[52] U.S. Cl. **D24/231; D24/169**

[58] Field of Search D24/1.1, 8, 17;
422/63-68, 50; 436/43, 48; 356/39, 40, 41, 319;
D10/81, 46

[56] References Cited

U.S. PATENT DOCUMENTS

D. 298,854 12/1988 Kame et al. D24/1.1

D. 303,095 8/1989 Nagai et al. D24/1.1 X
D. 307,398 4/1990 Umemoto et al. D24/1.1 X
D. 314,049 1/1991 Katayama D24/1.1
4,078,895 3/1978 Moran D24/1.1 X
4,483,823 11/1984 Umetsu et al. D24/1.1 X

Primary Examiner—Stella Reid

Attorney, Agent, or Firm—Antonelli, Terry, Stout & Kraus

[57] CLAIM

The ornamental design for a clinical chemistry analyzer, as shown.

DESCRIPTION

FIG. 1 is a front, top and left side elevational perspective view of a clinical chemistry analyzer showing our new design;

FIG. 2 is front elevational view thereof;

FIG. 3 is a right side elevational view thereof;

FIG. 4 is a top plan view thereof;

FIG. 5 is a rear elevational view thereof;

FIG. 6 is a left side elevational view thereof and

FIG. 7 is a bottom plan view thereof.

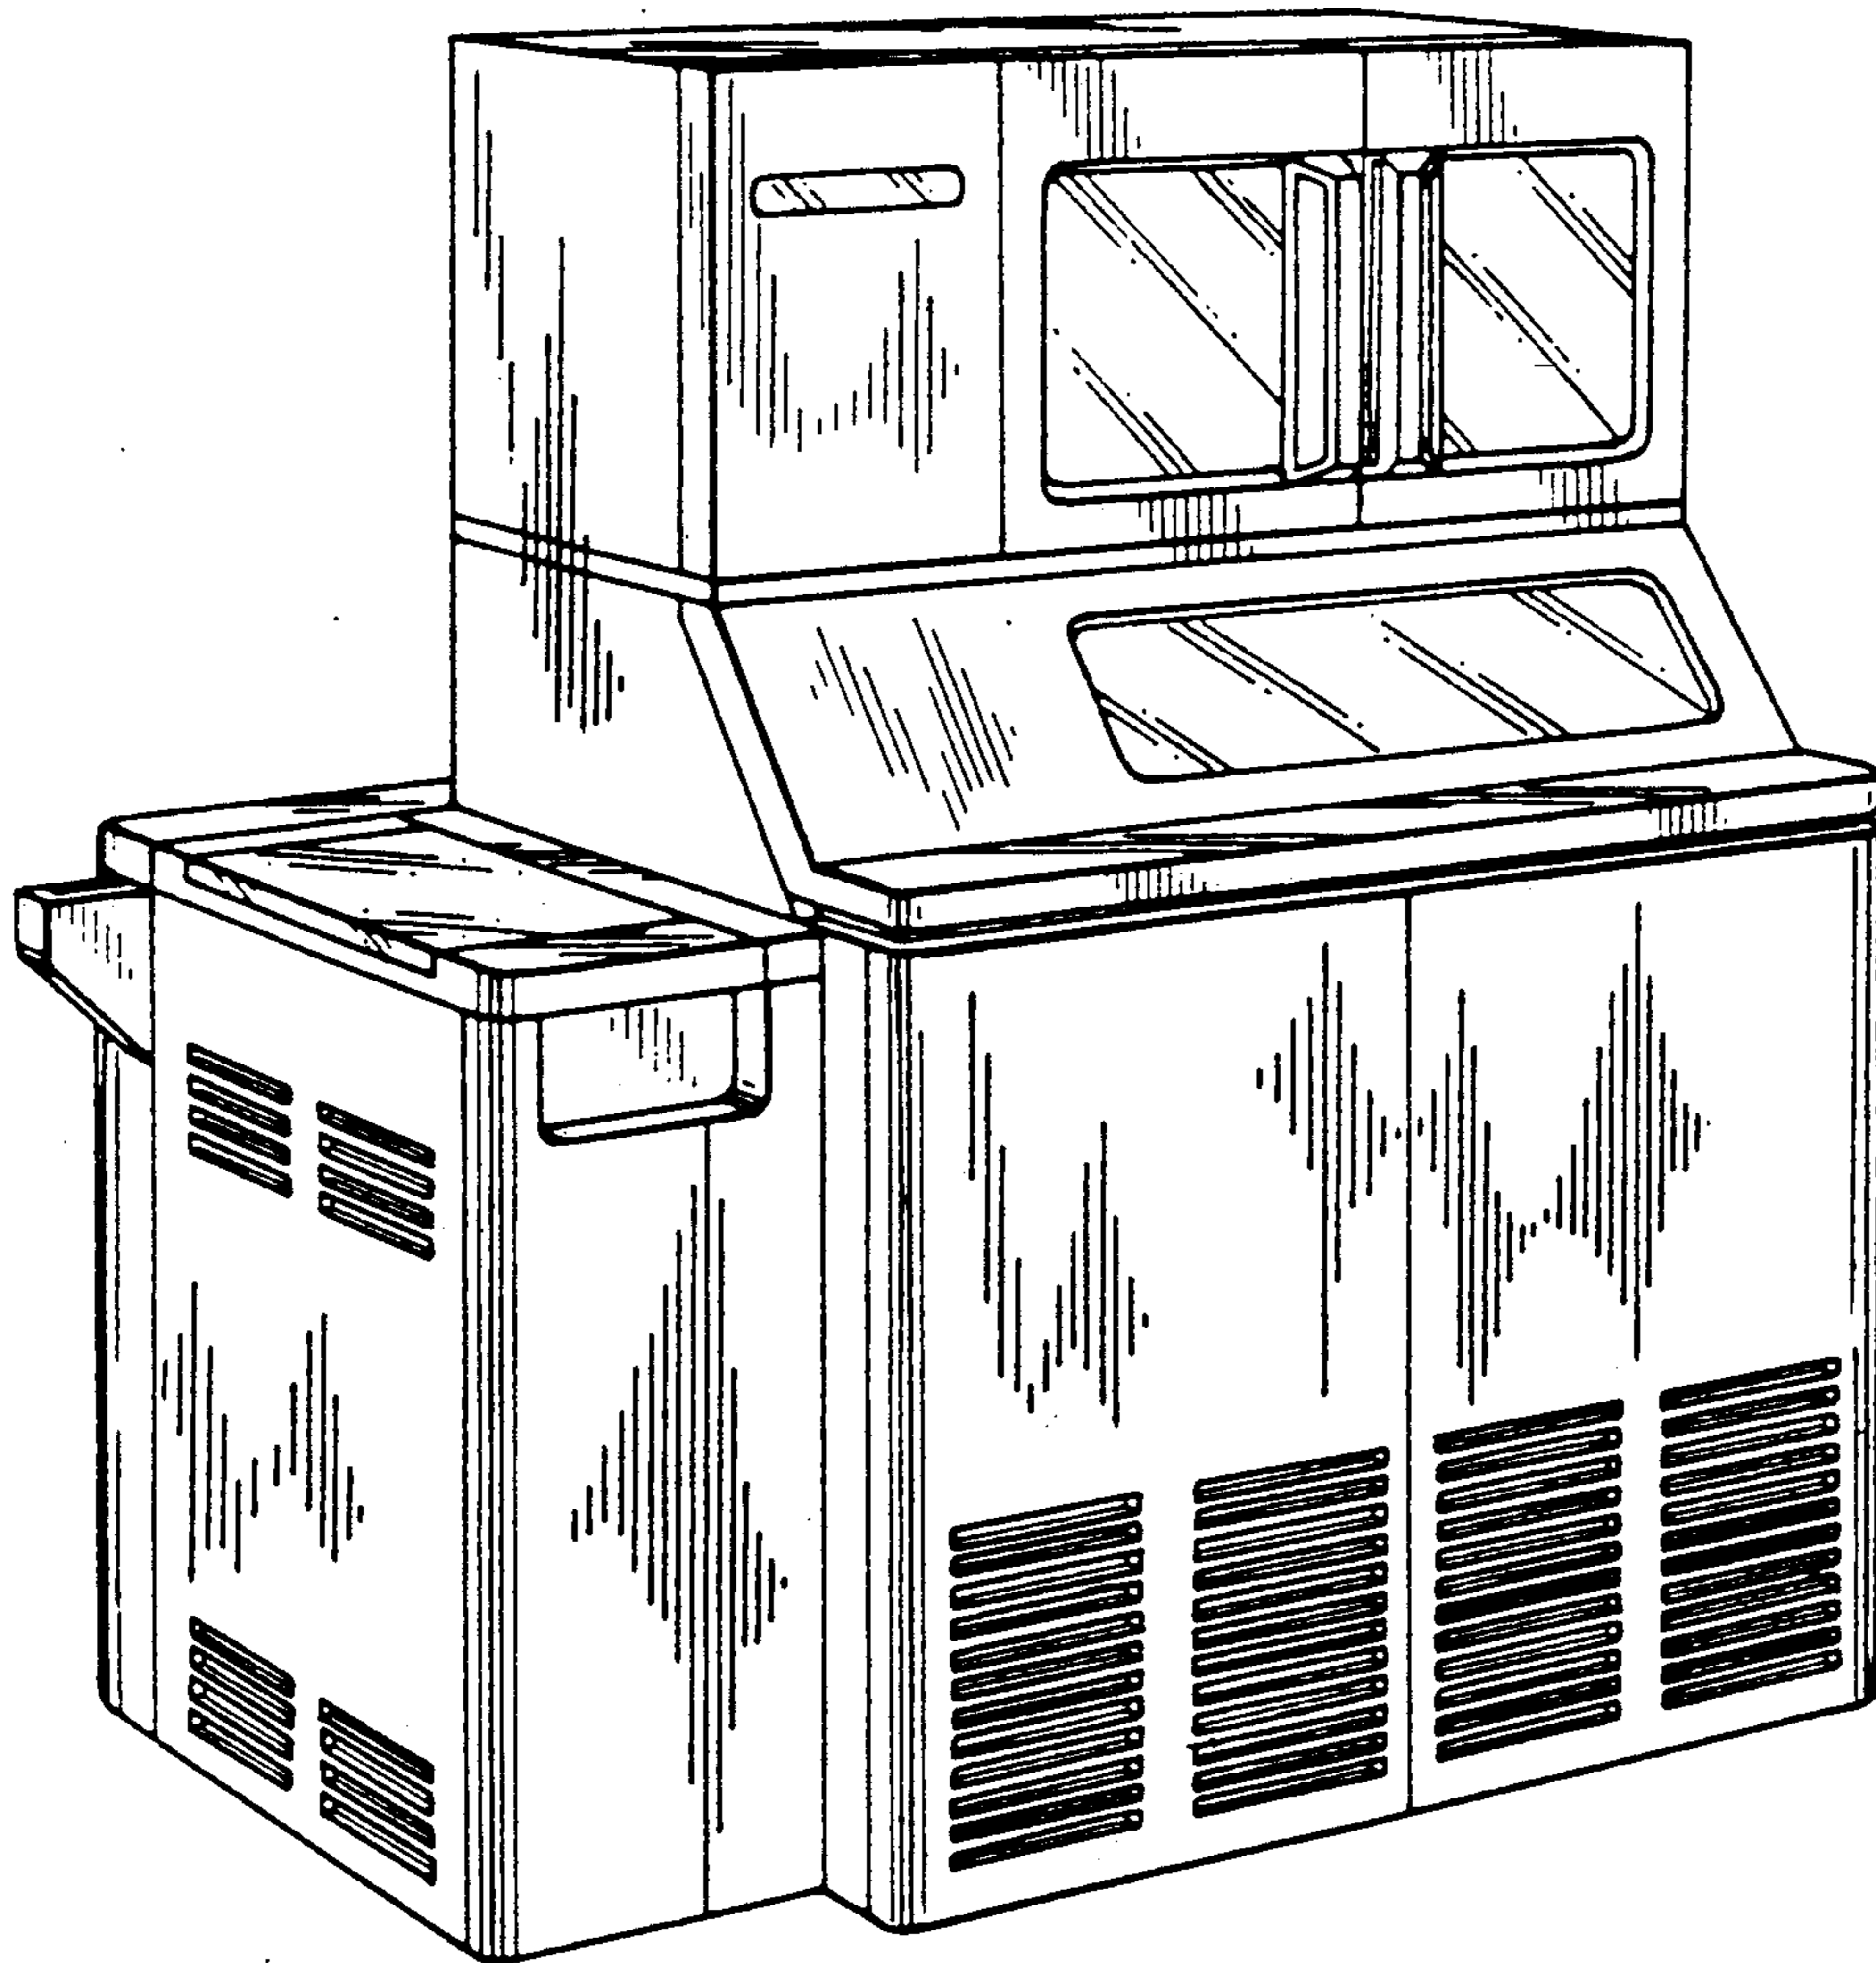


FIG. 1

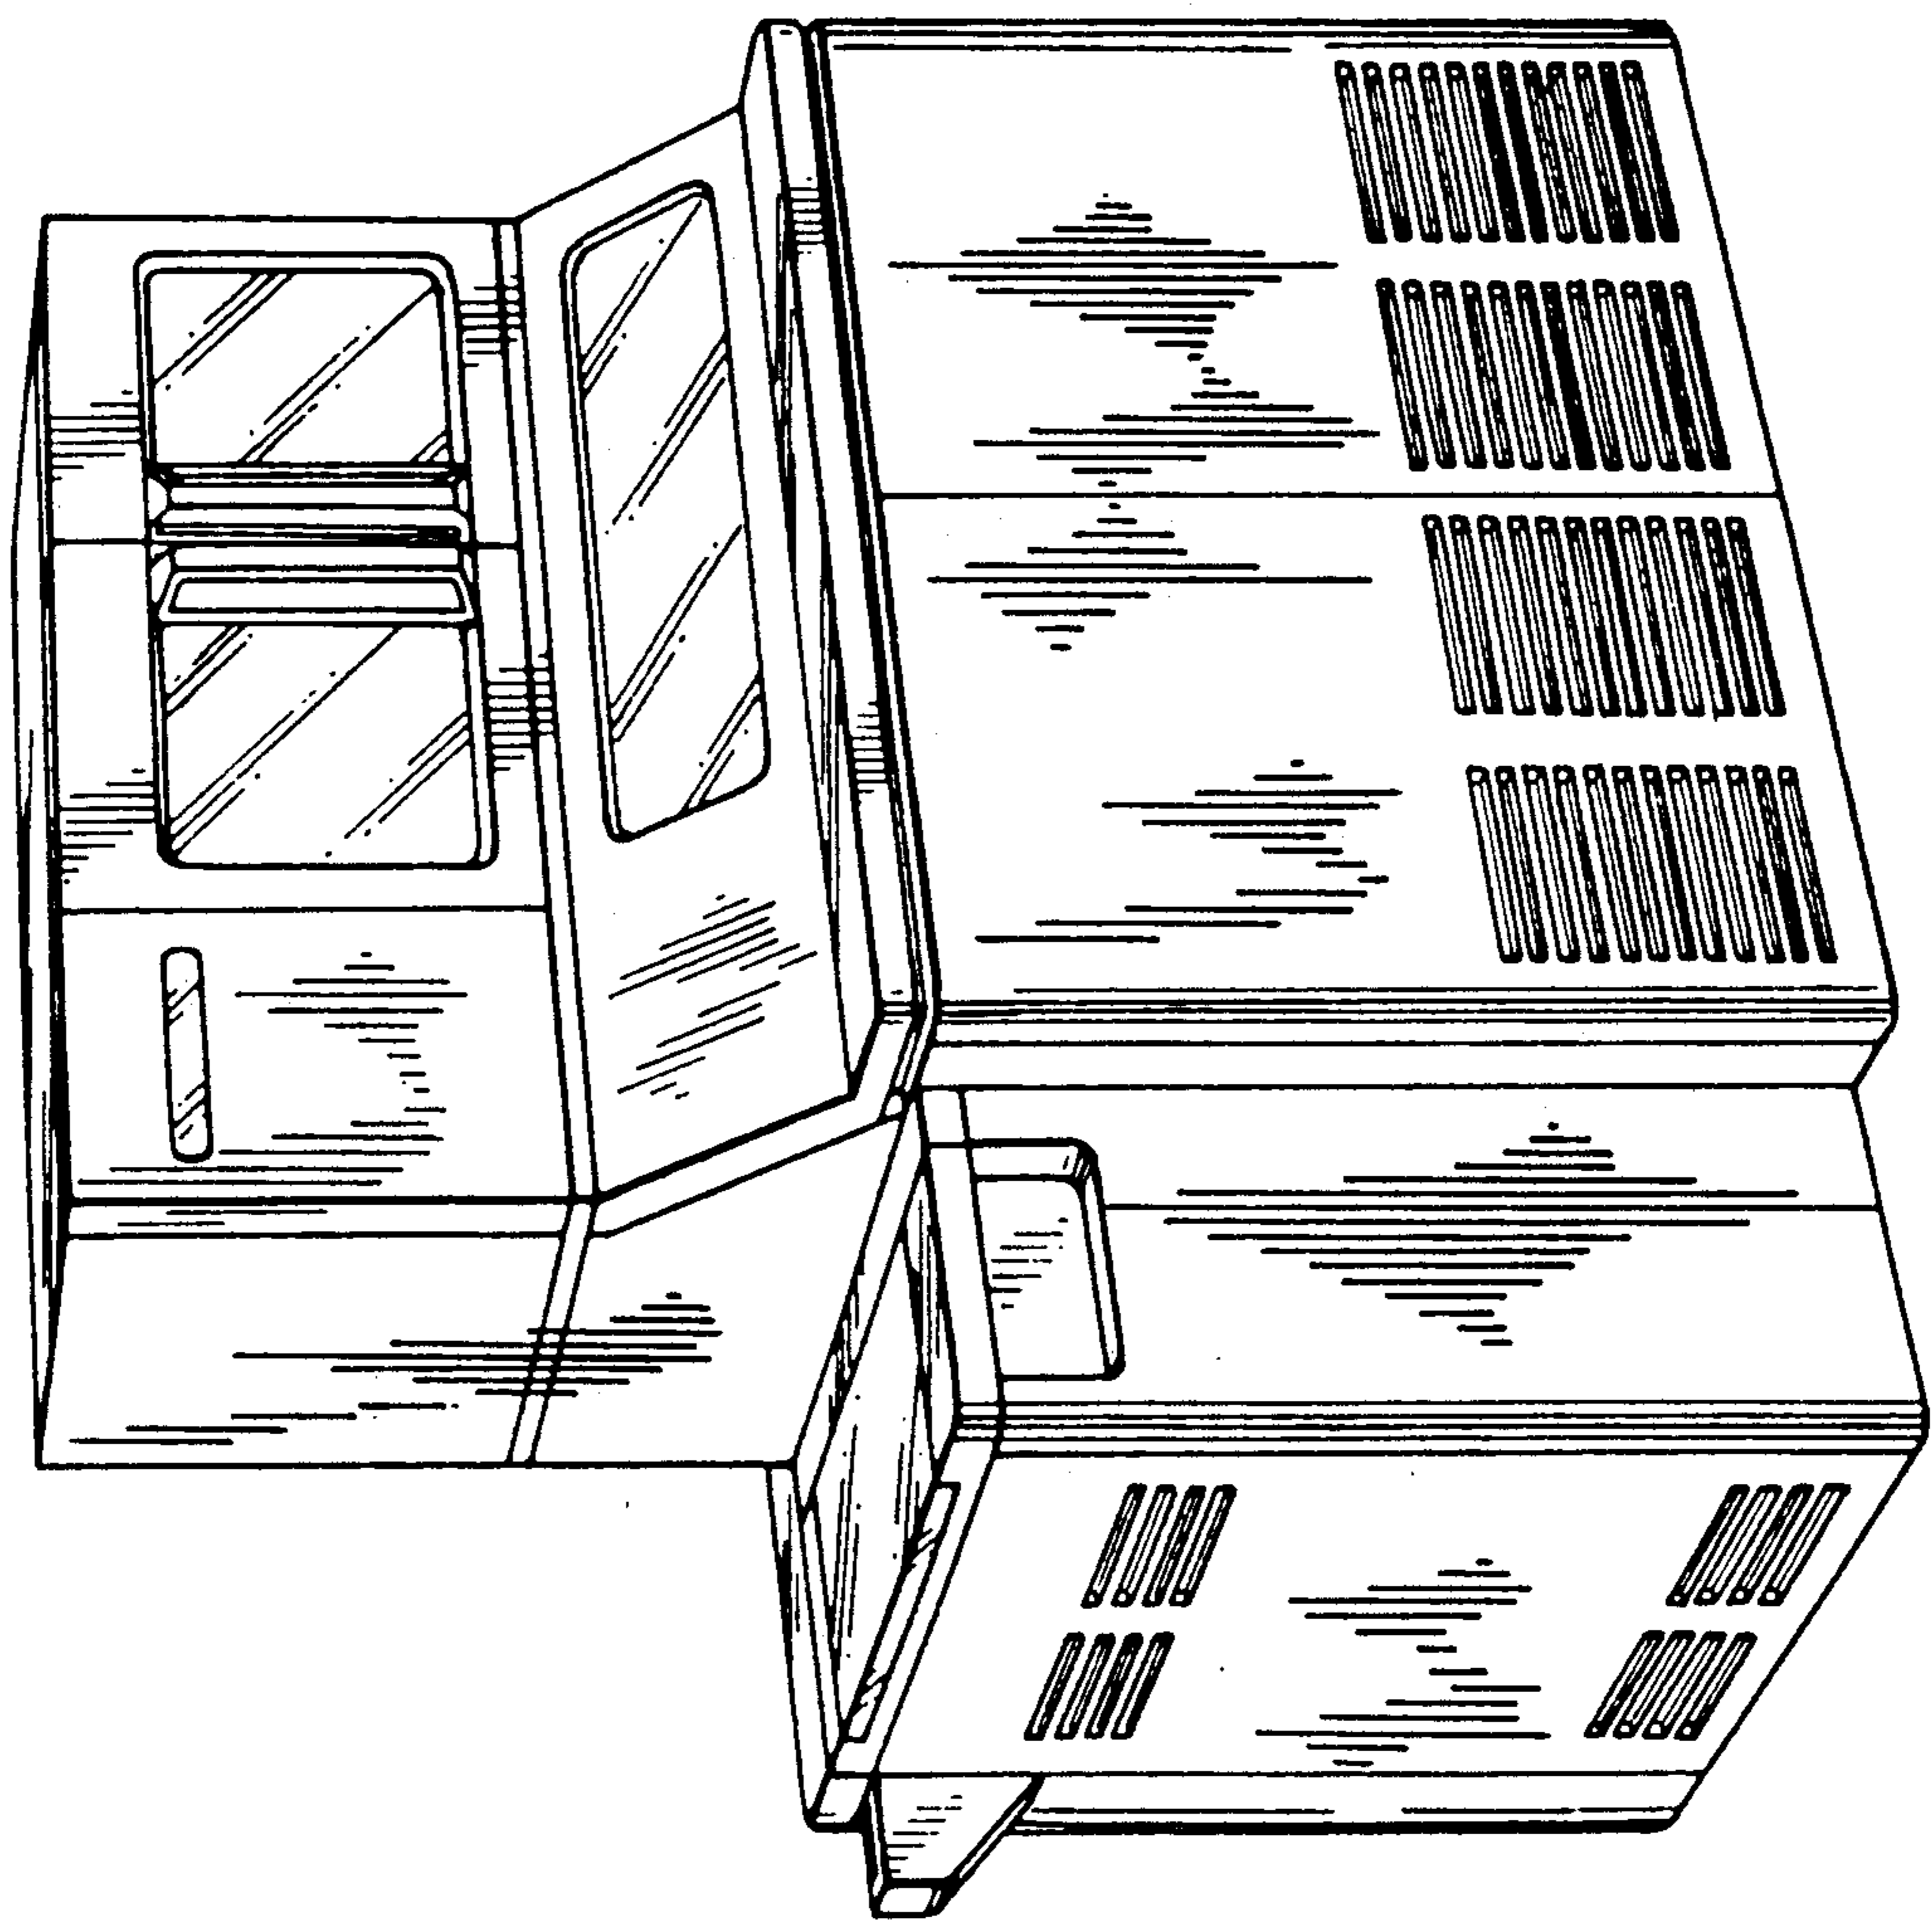


FIG. 3

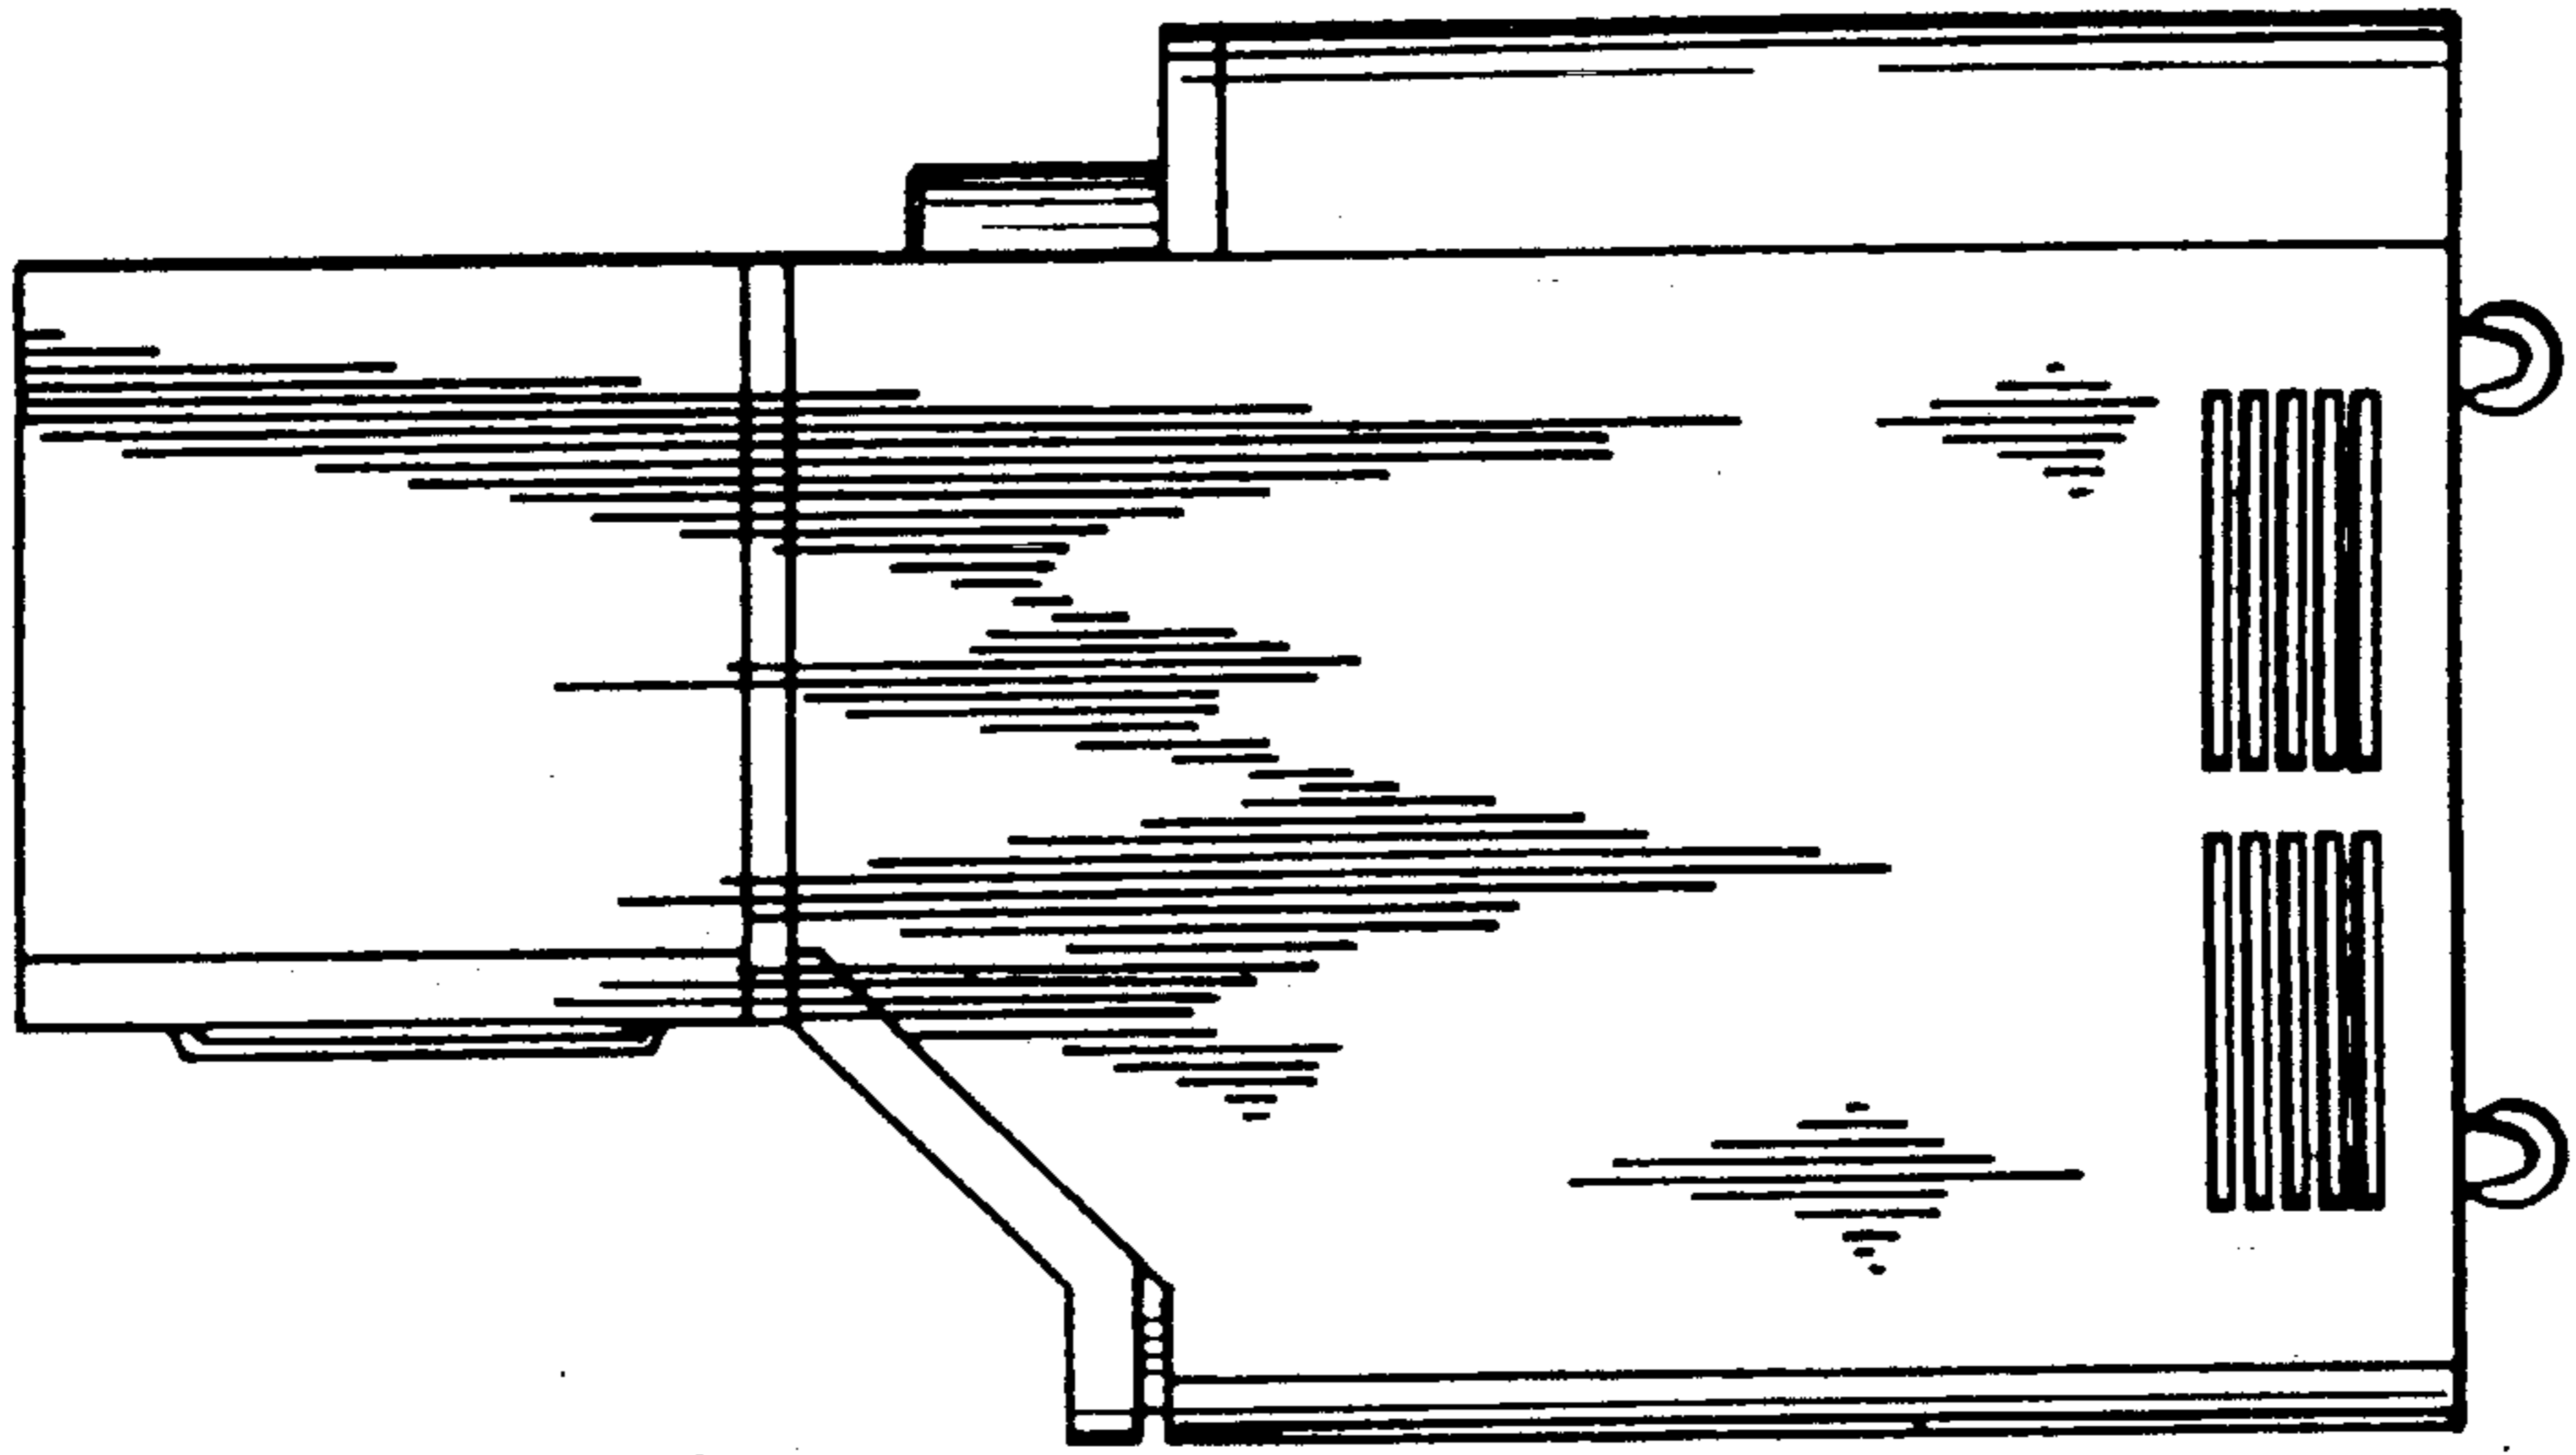


FIG. 2

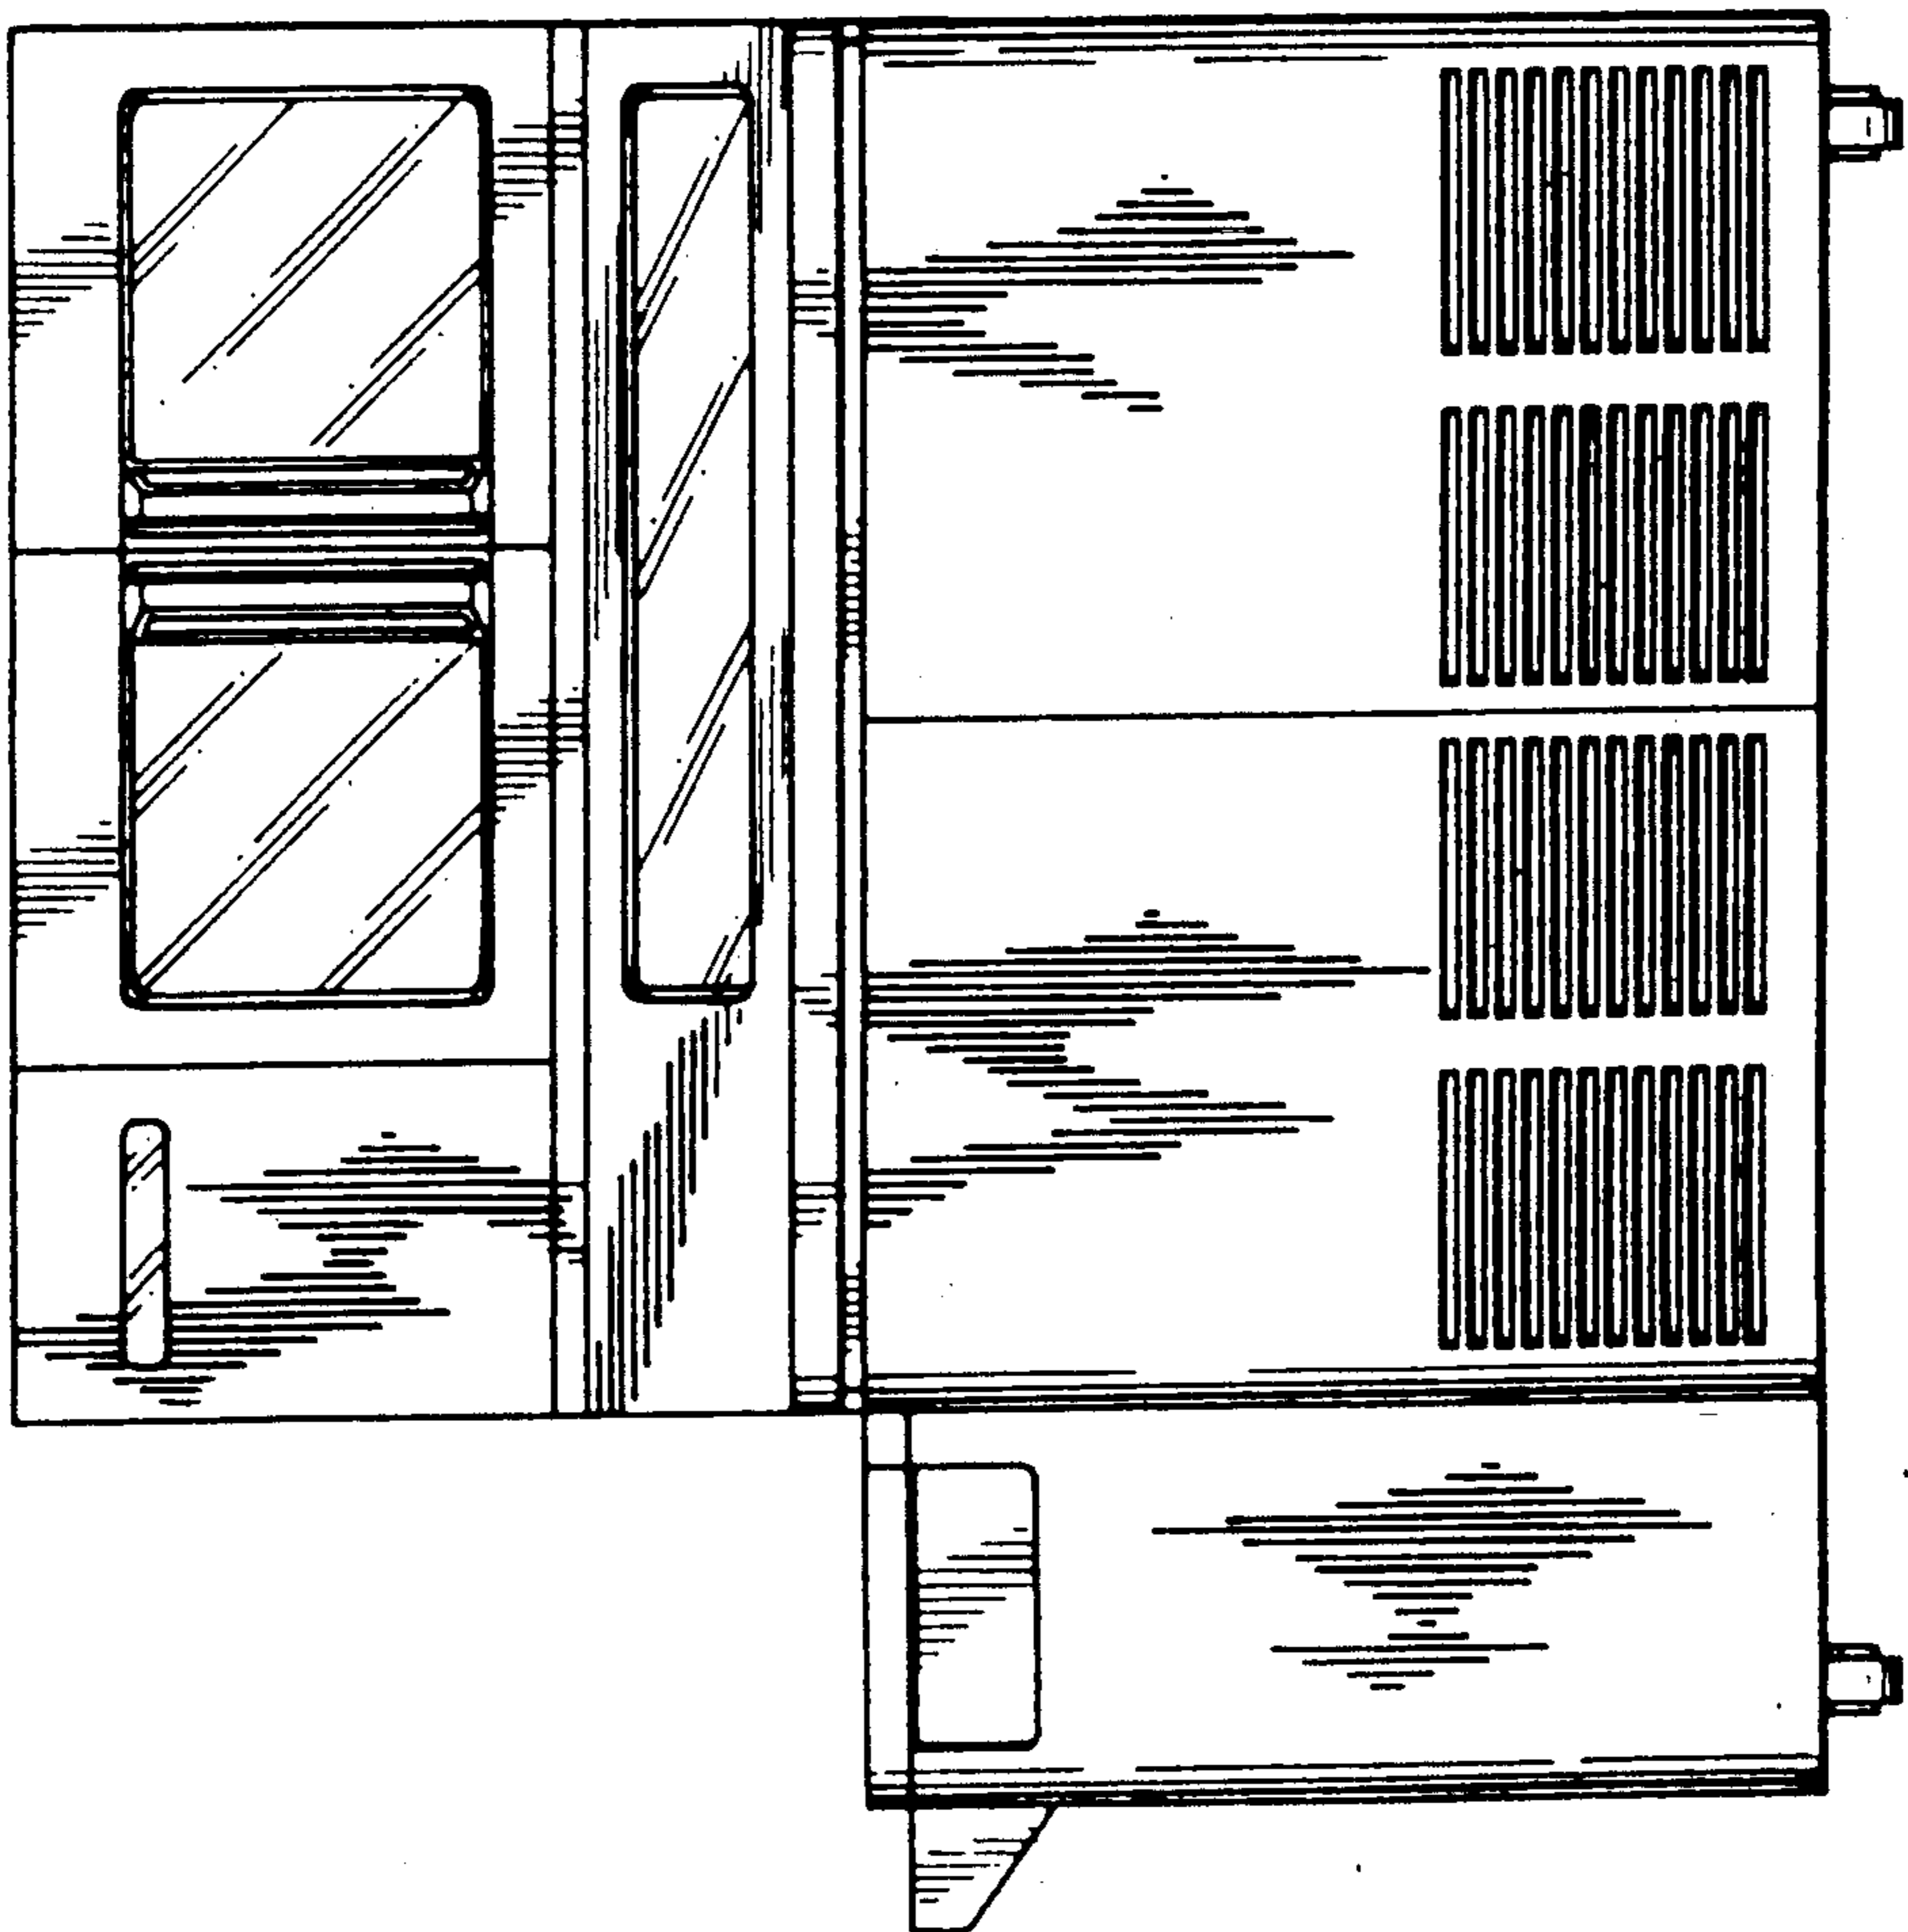


FIG. 4

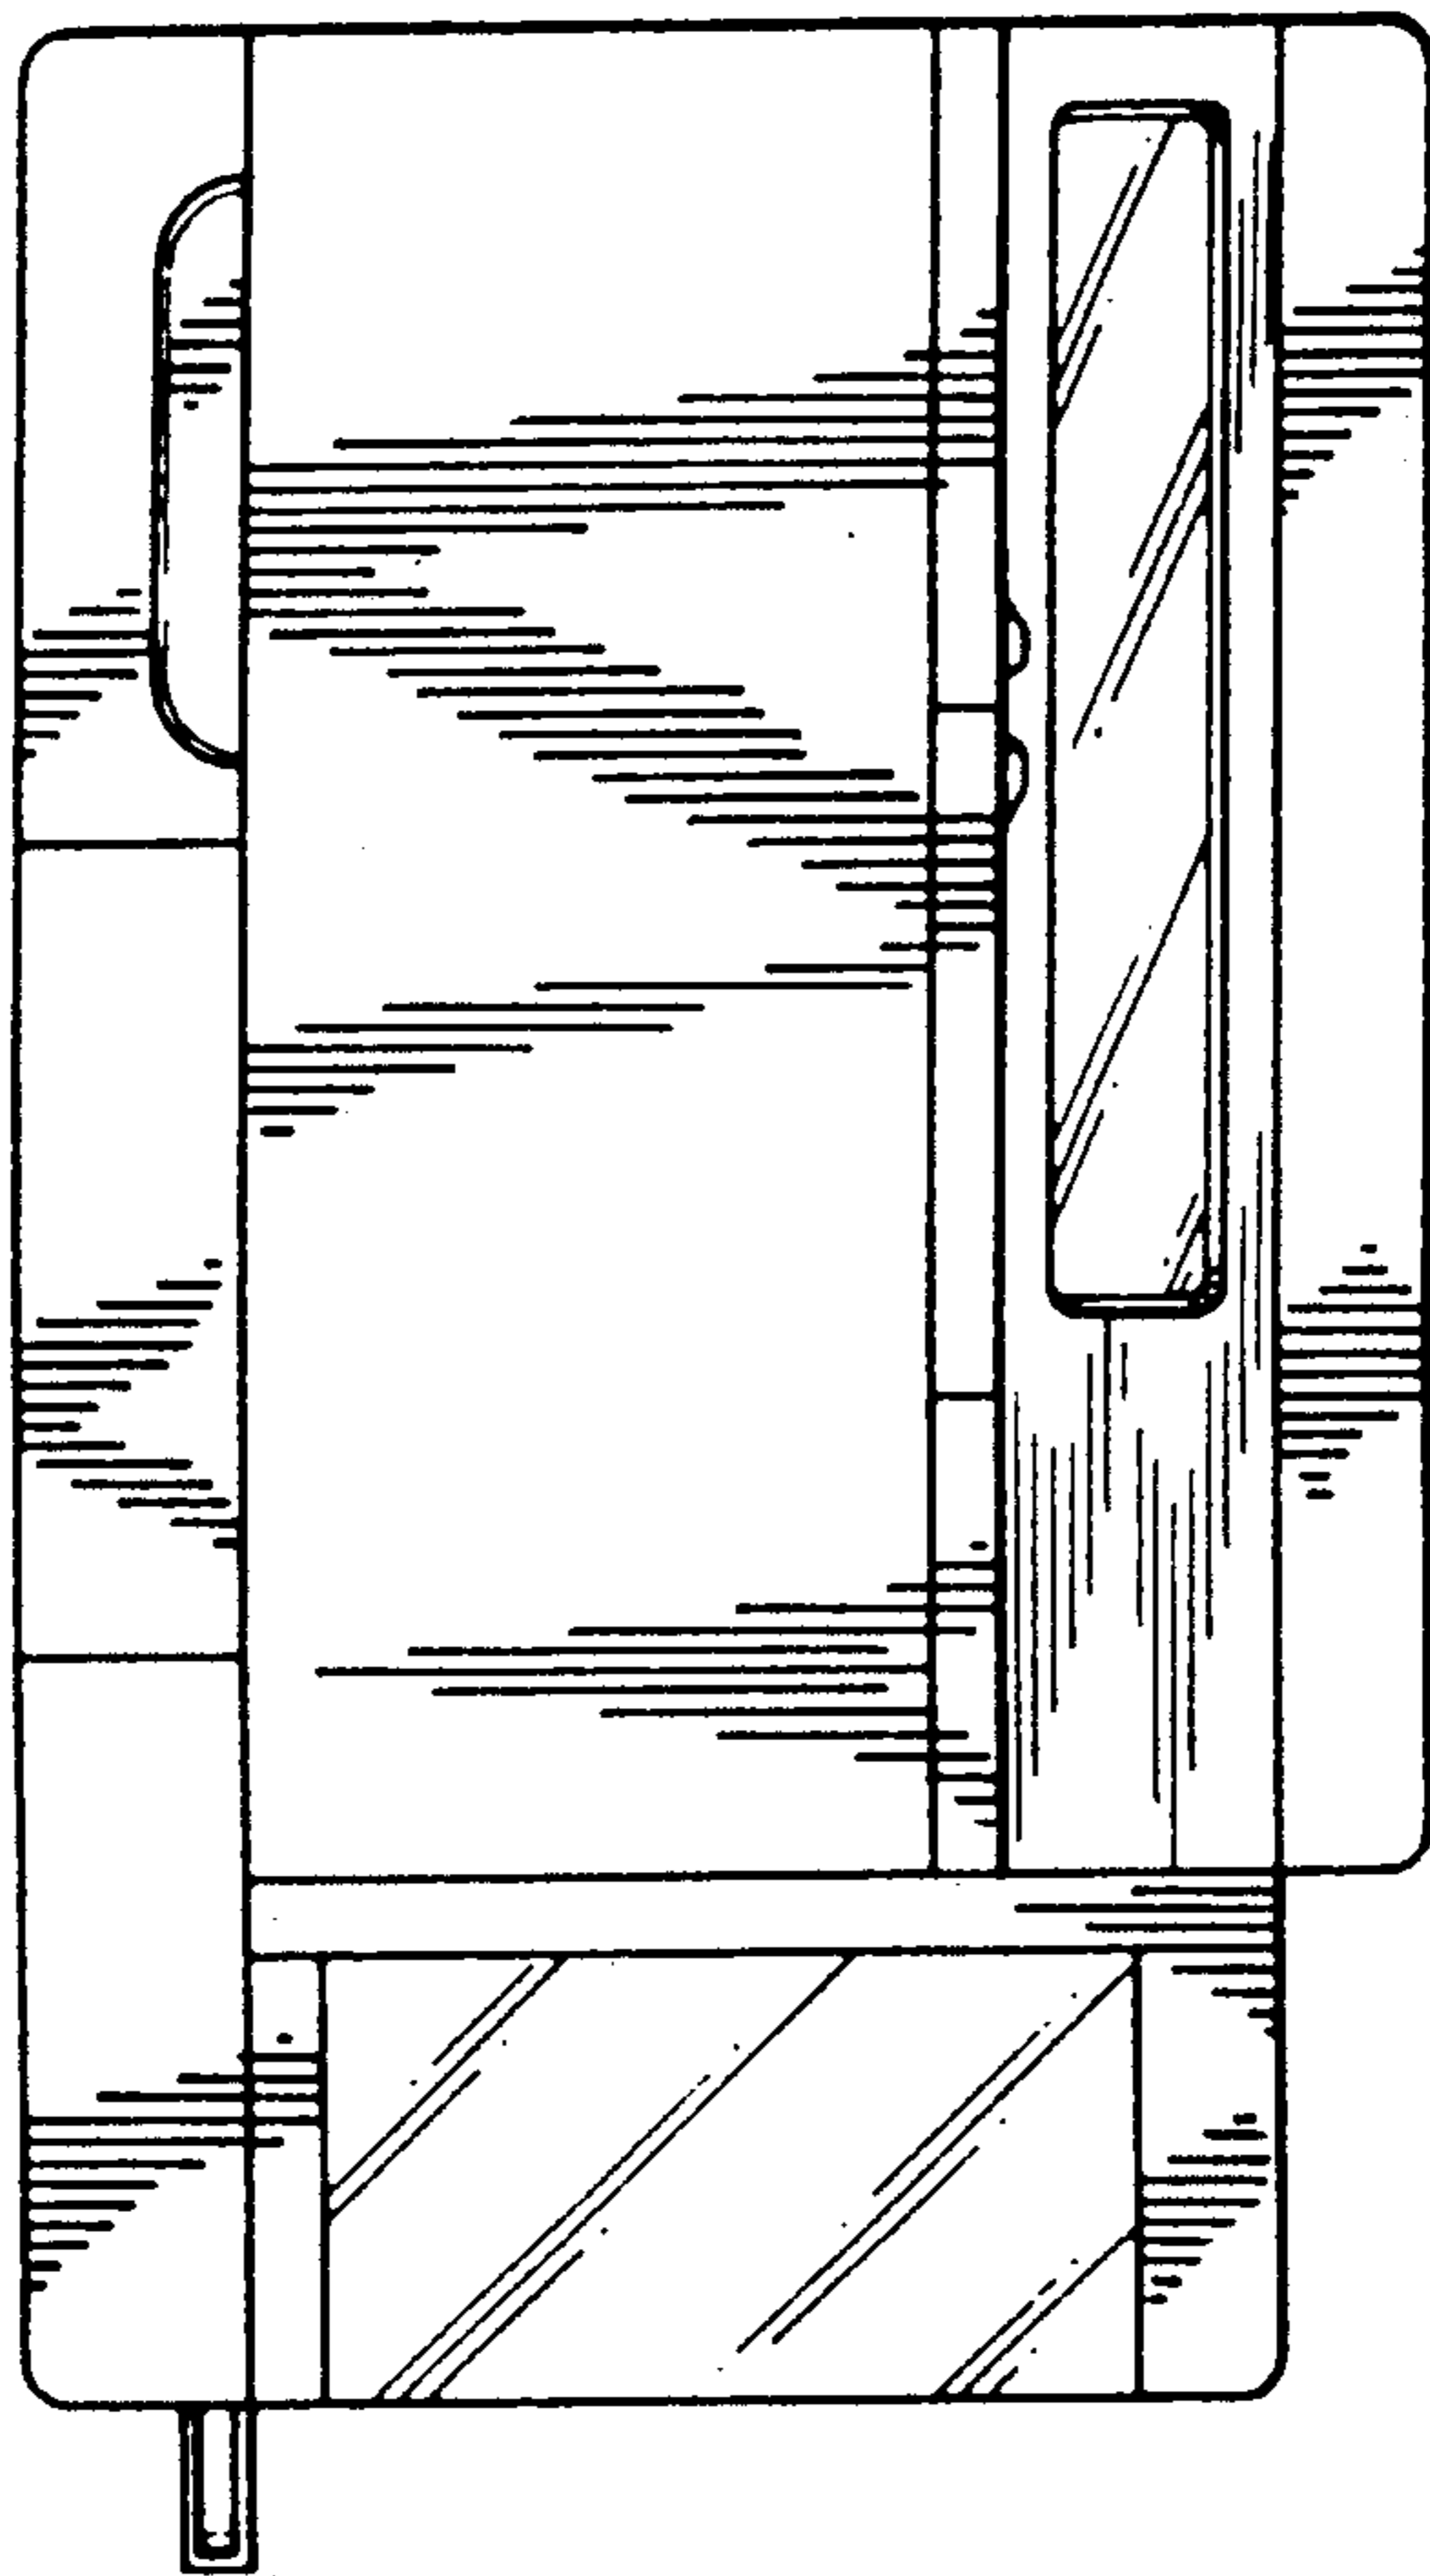


FIG. 6

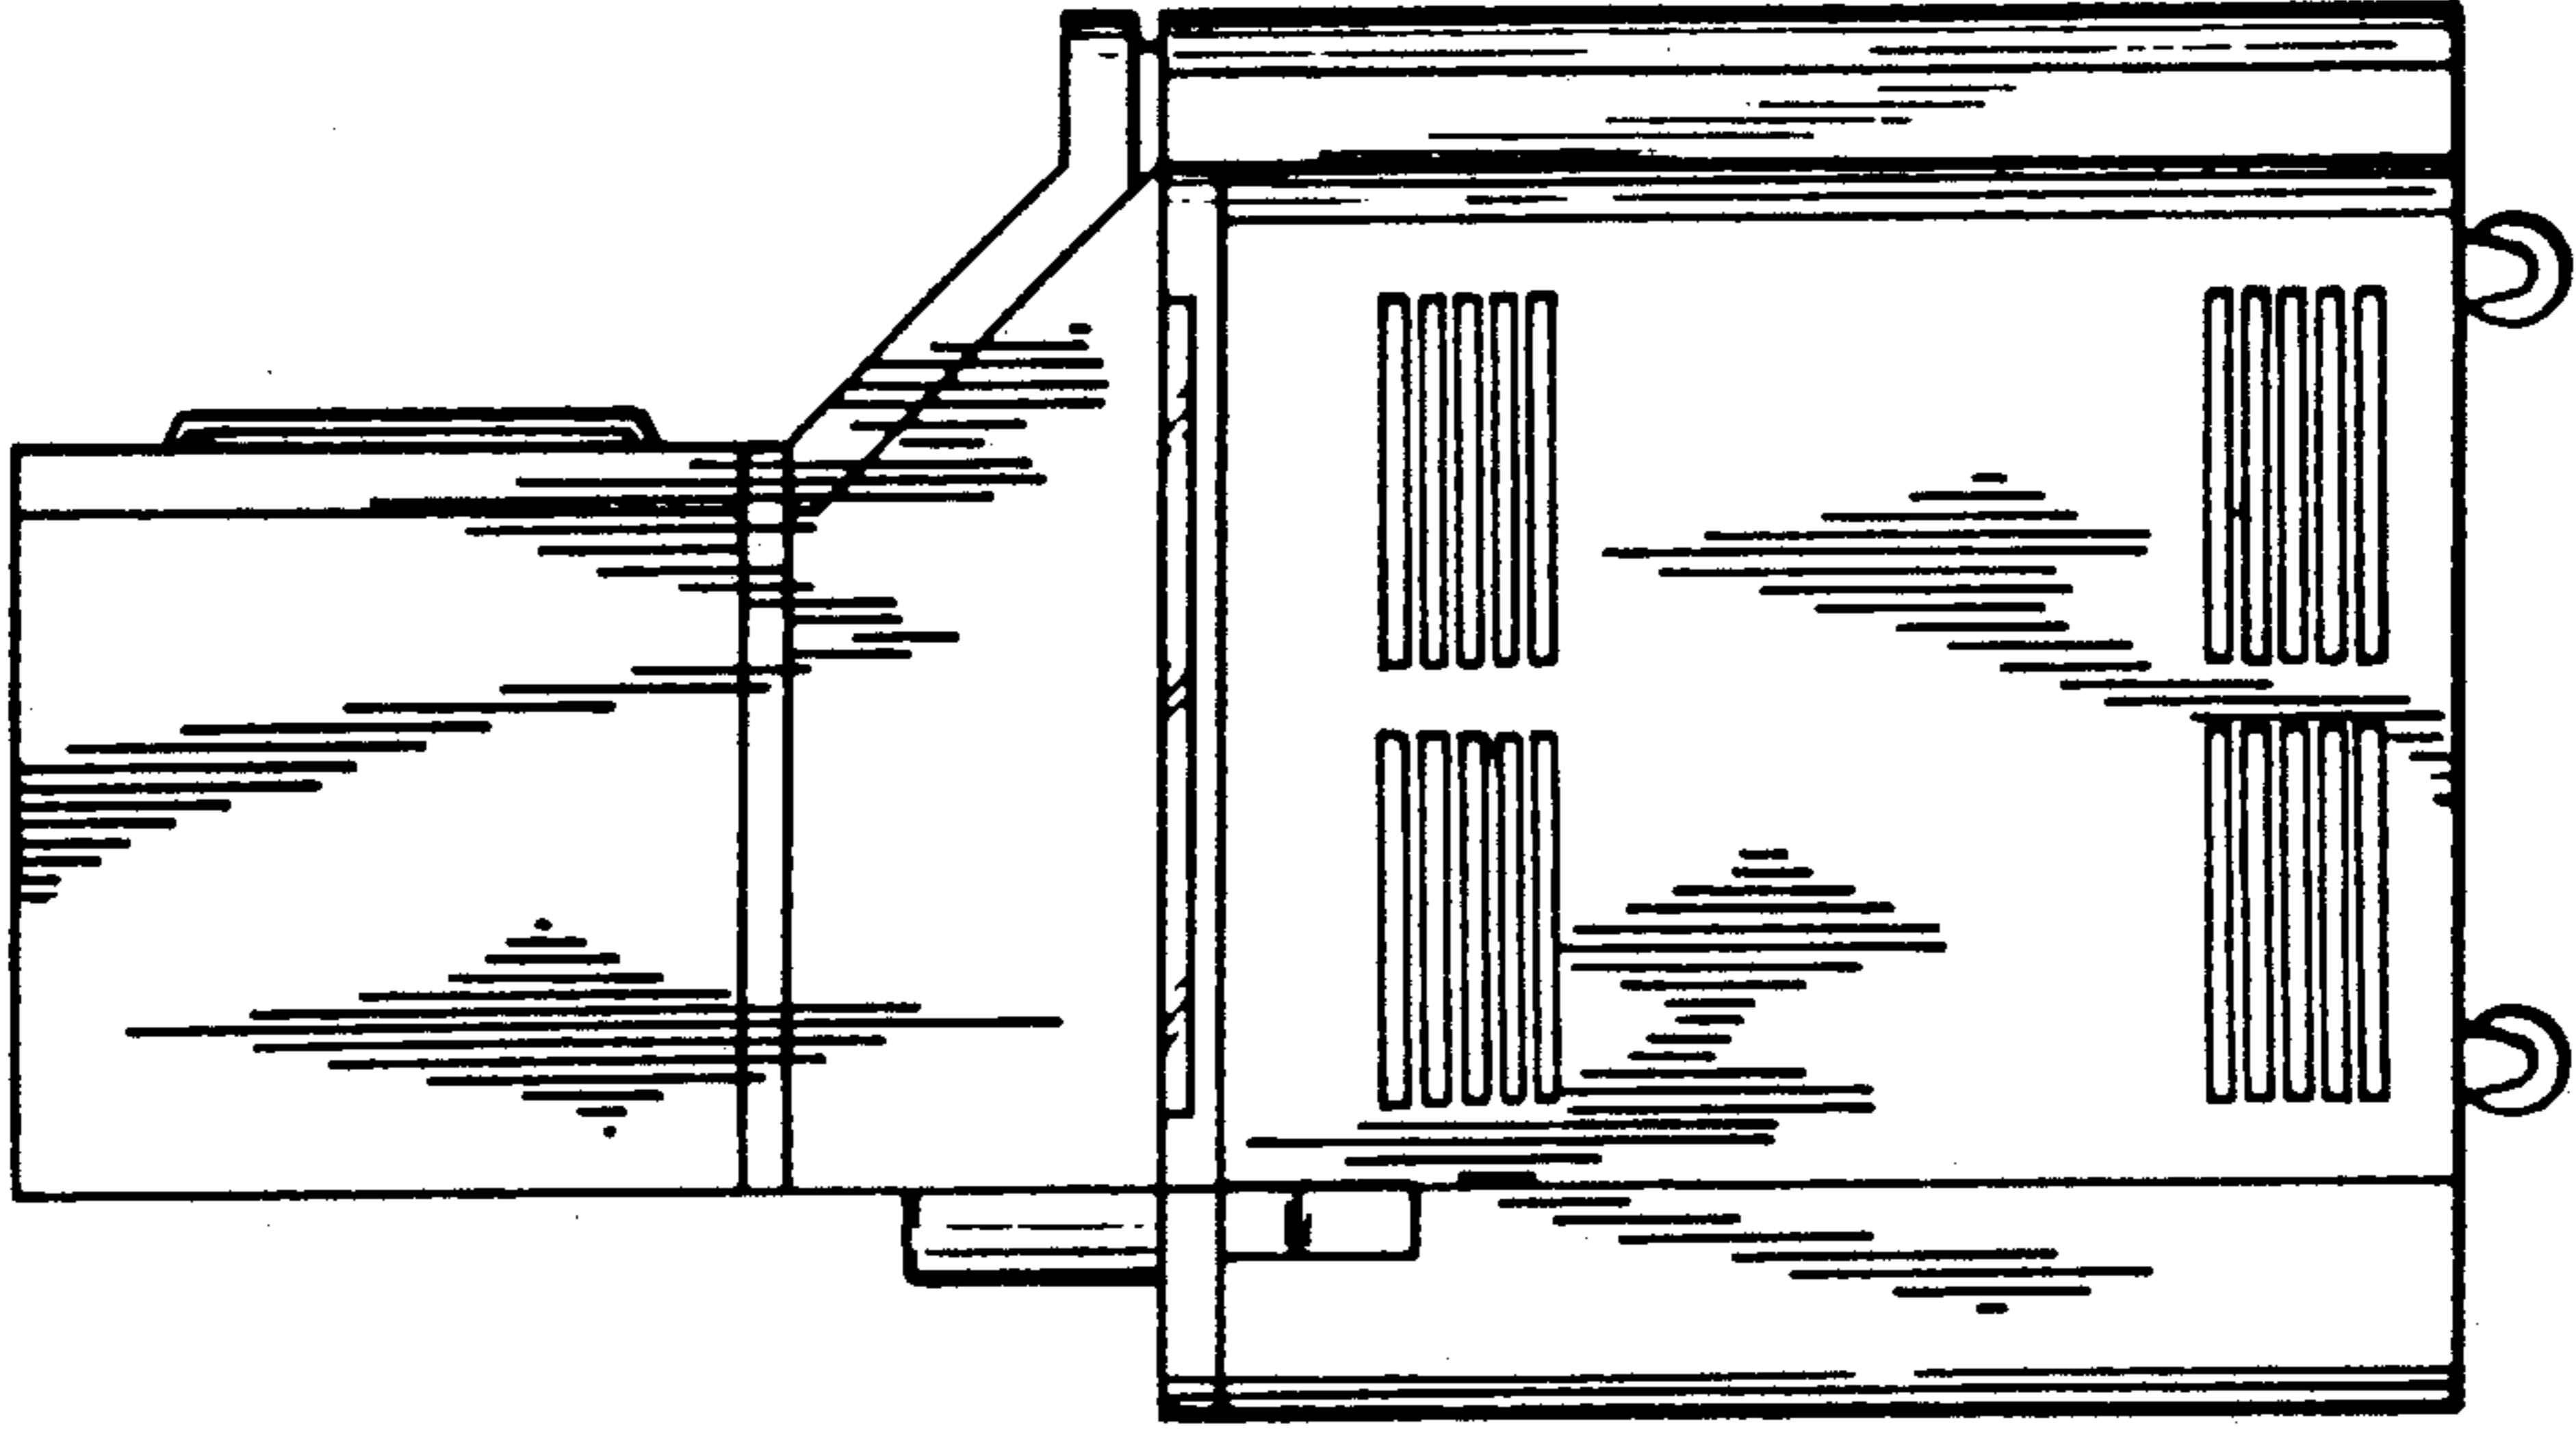


FIG. 5

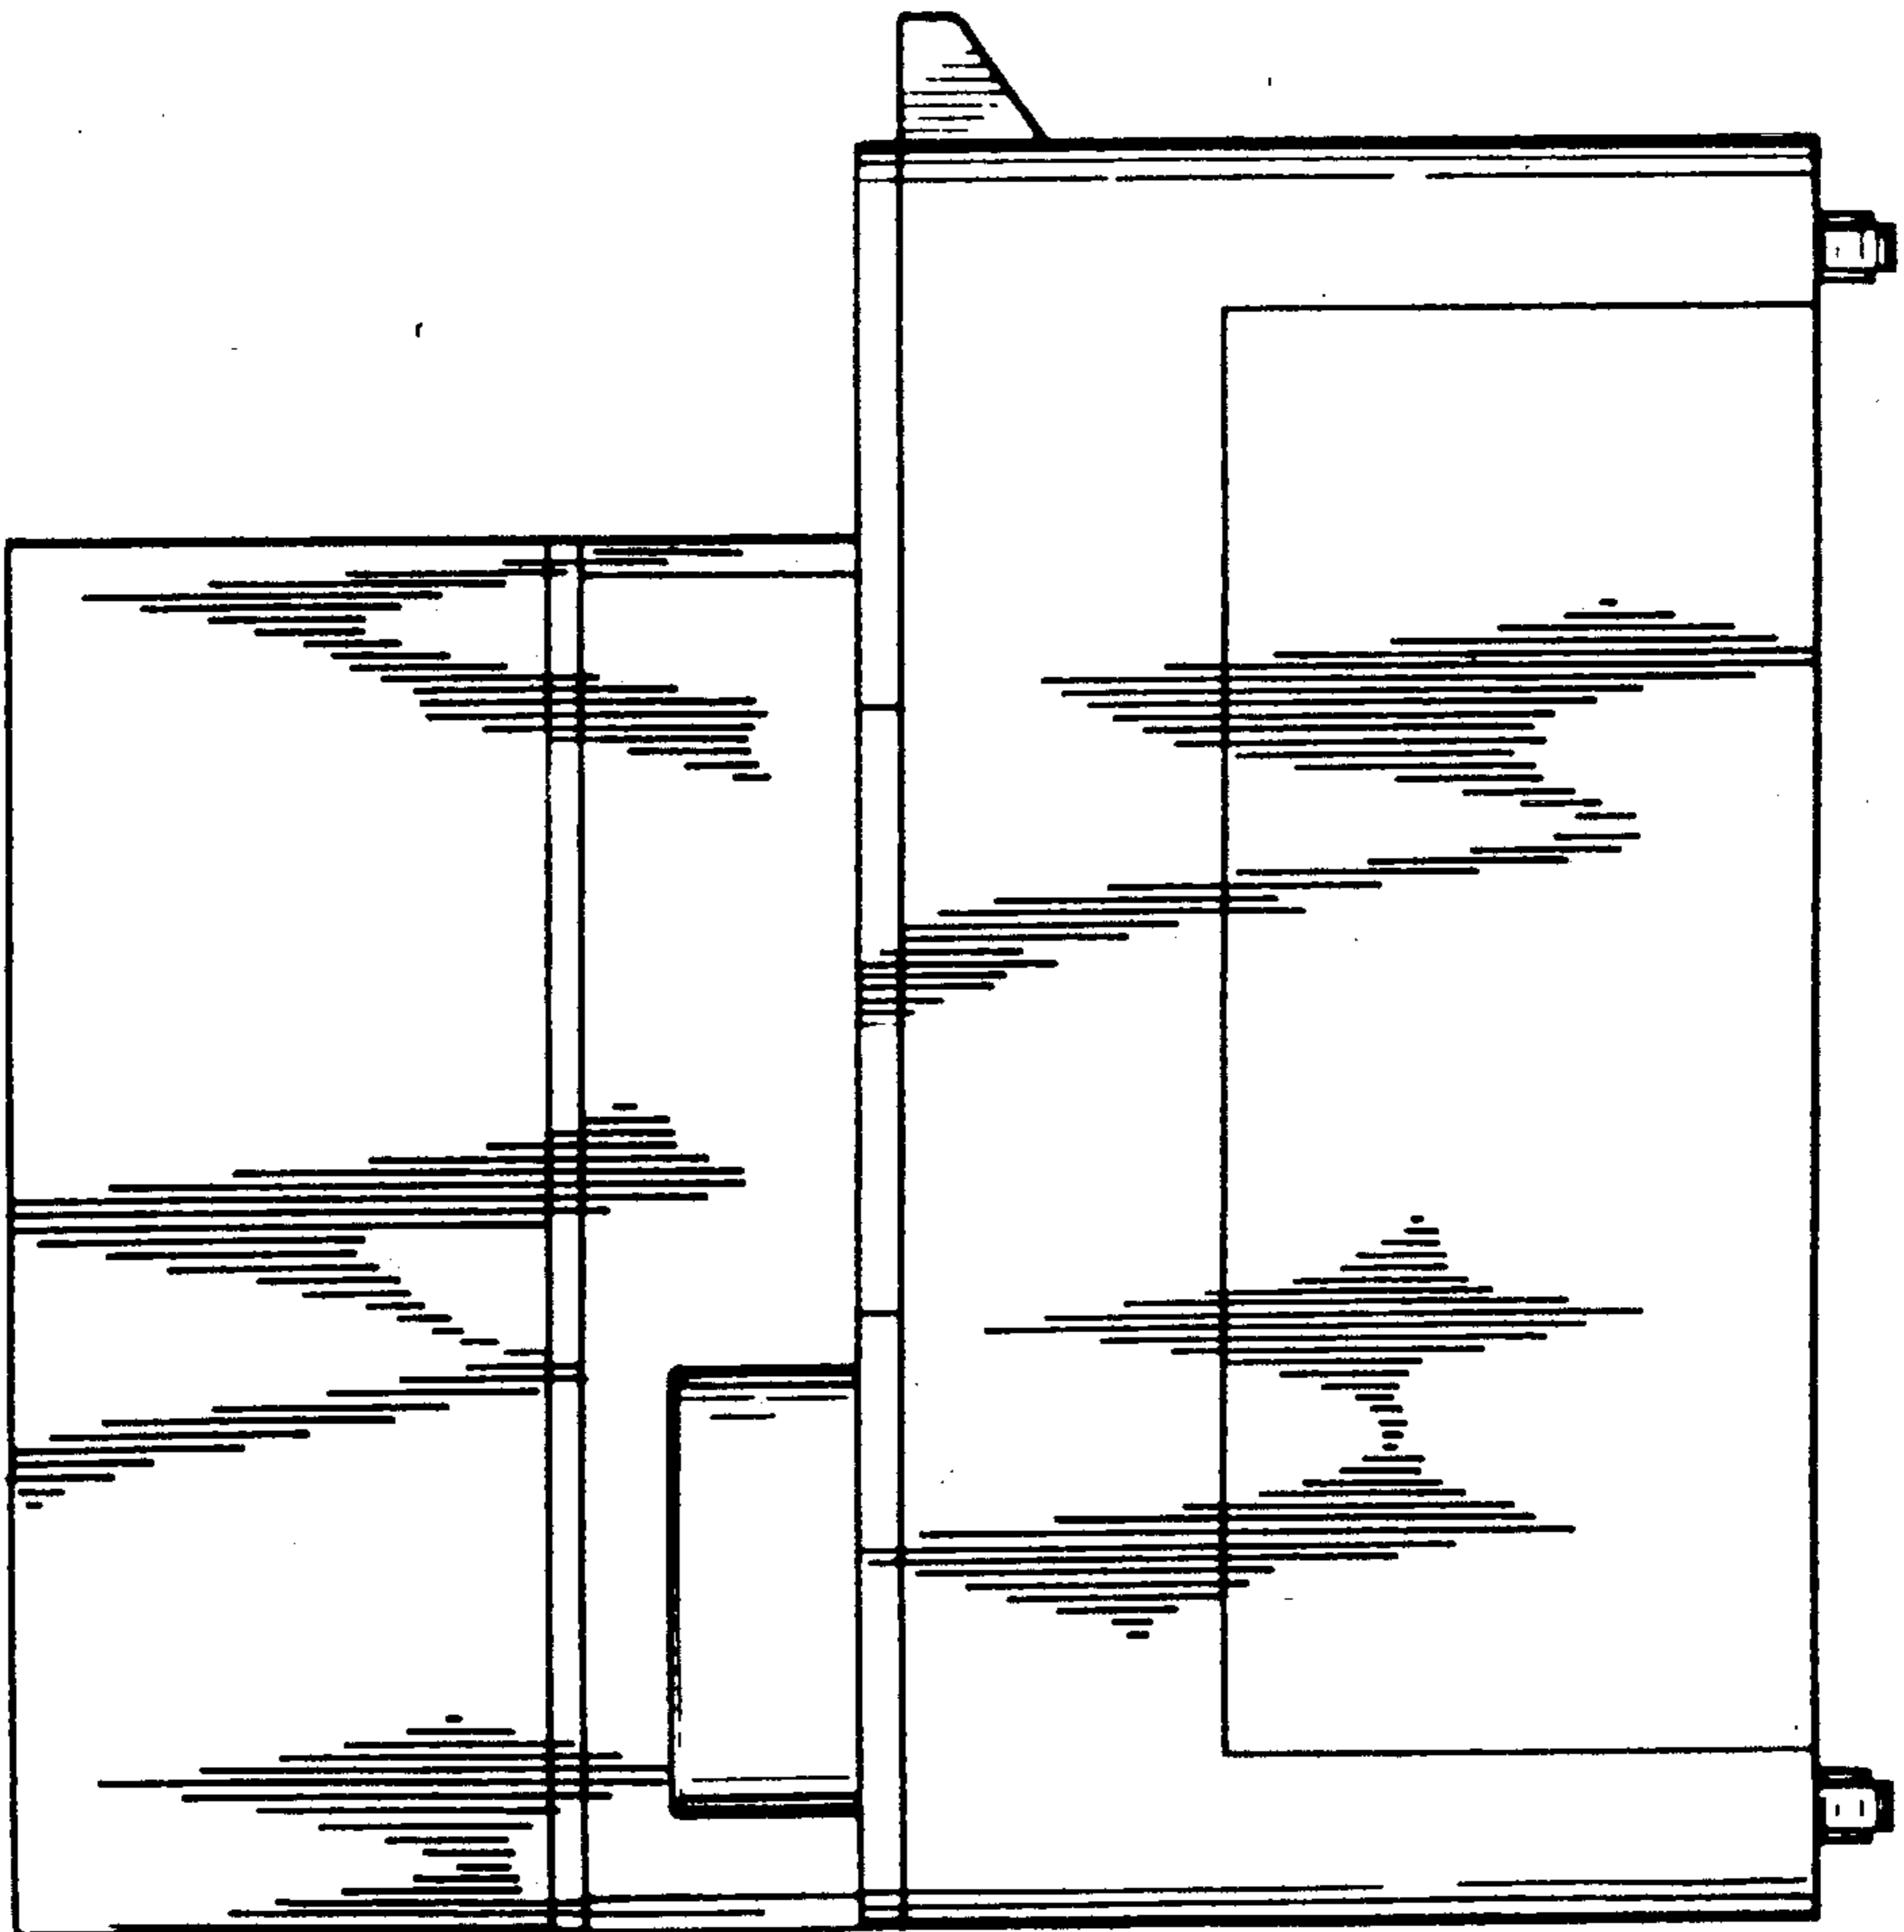


FIG. 7

