

[54] ALARM FOR PATIENTS IN HOSPITALS OR THE LIKE

[76] Inventors: Robert E. Gagnon, 31 Conlon Street, Winnipeg, Manitoba, Canada, R2C-4K6; Raymond Gagnon, 51 Sandrington Dr., Winnipeg, Manitoba, Canada, R2N-2J2

[\*\*] Term: 14 Years

[21] Appl. No.: 379,151

[22] Filed: Jul. 13, 1989

[52] U.S. Cl. .... D10/106

[58] Field of Search ..... D10/104, 106, 121, 75, D10/78, 57, 46; 340/565, 542, 566, 573, 571, 572, 542, 321, 328, 286.07, 286.06

[56] References Cited

U.S. PATENT DOCUMENTS

- D. 313,362 1/1991 Reich et al. .... D10/106
- D. 313,363 1/1991 Reich et al. .... D10/106
- 696,702 4/1902 Weitz ..... 340/687

- 2,592,989 3/1952 Wilson ..... 340/687
- 3,192,518 6/1965 Sliman ..... 340/687
- 3,595,228 7/1971 Simon ..... 340/687
- 3,651,512 3/1972 Summers ..... 340/286.07
- 4,228,426 10/1980 Roberts ..... 340/687
- 4,321,461 3/1982 Walter ..... 340/687
- 4,680,790 7/1987 Packard et al. .... 340/286.07
- 4,761,633 8/1988 Leff et al. .... 340/286.07


Primary Examiner—Wallace R. Burke  
Assistant Examiner—Marcus Jackson  
Attorney, Agent, or Firm—Terry M. Gernstein



[57] CLAIM

The ornamental design for an alarm for patients in hospitals or the like, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of an alarm for patients in hospitals or the like showing our new design, with the rod broken away to indicate indeterminate length; FIG. 2 is a left side elevational view thereof, with the cords broken away for ease of illustration; FIG. 3 is a top plan view thereof; FIG. 4 is a bottom plan view thereof.

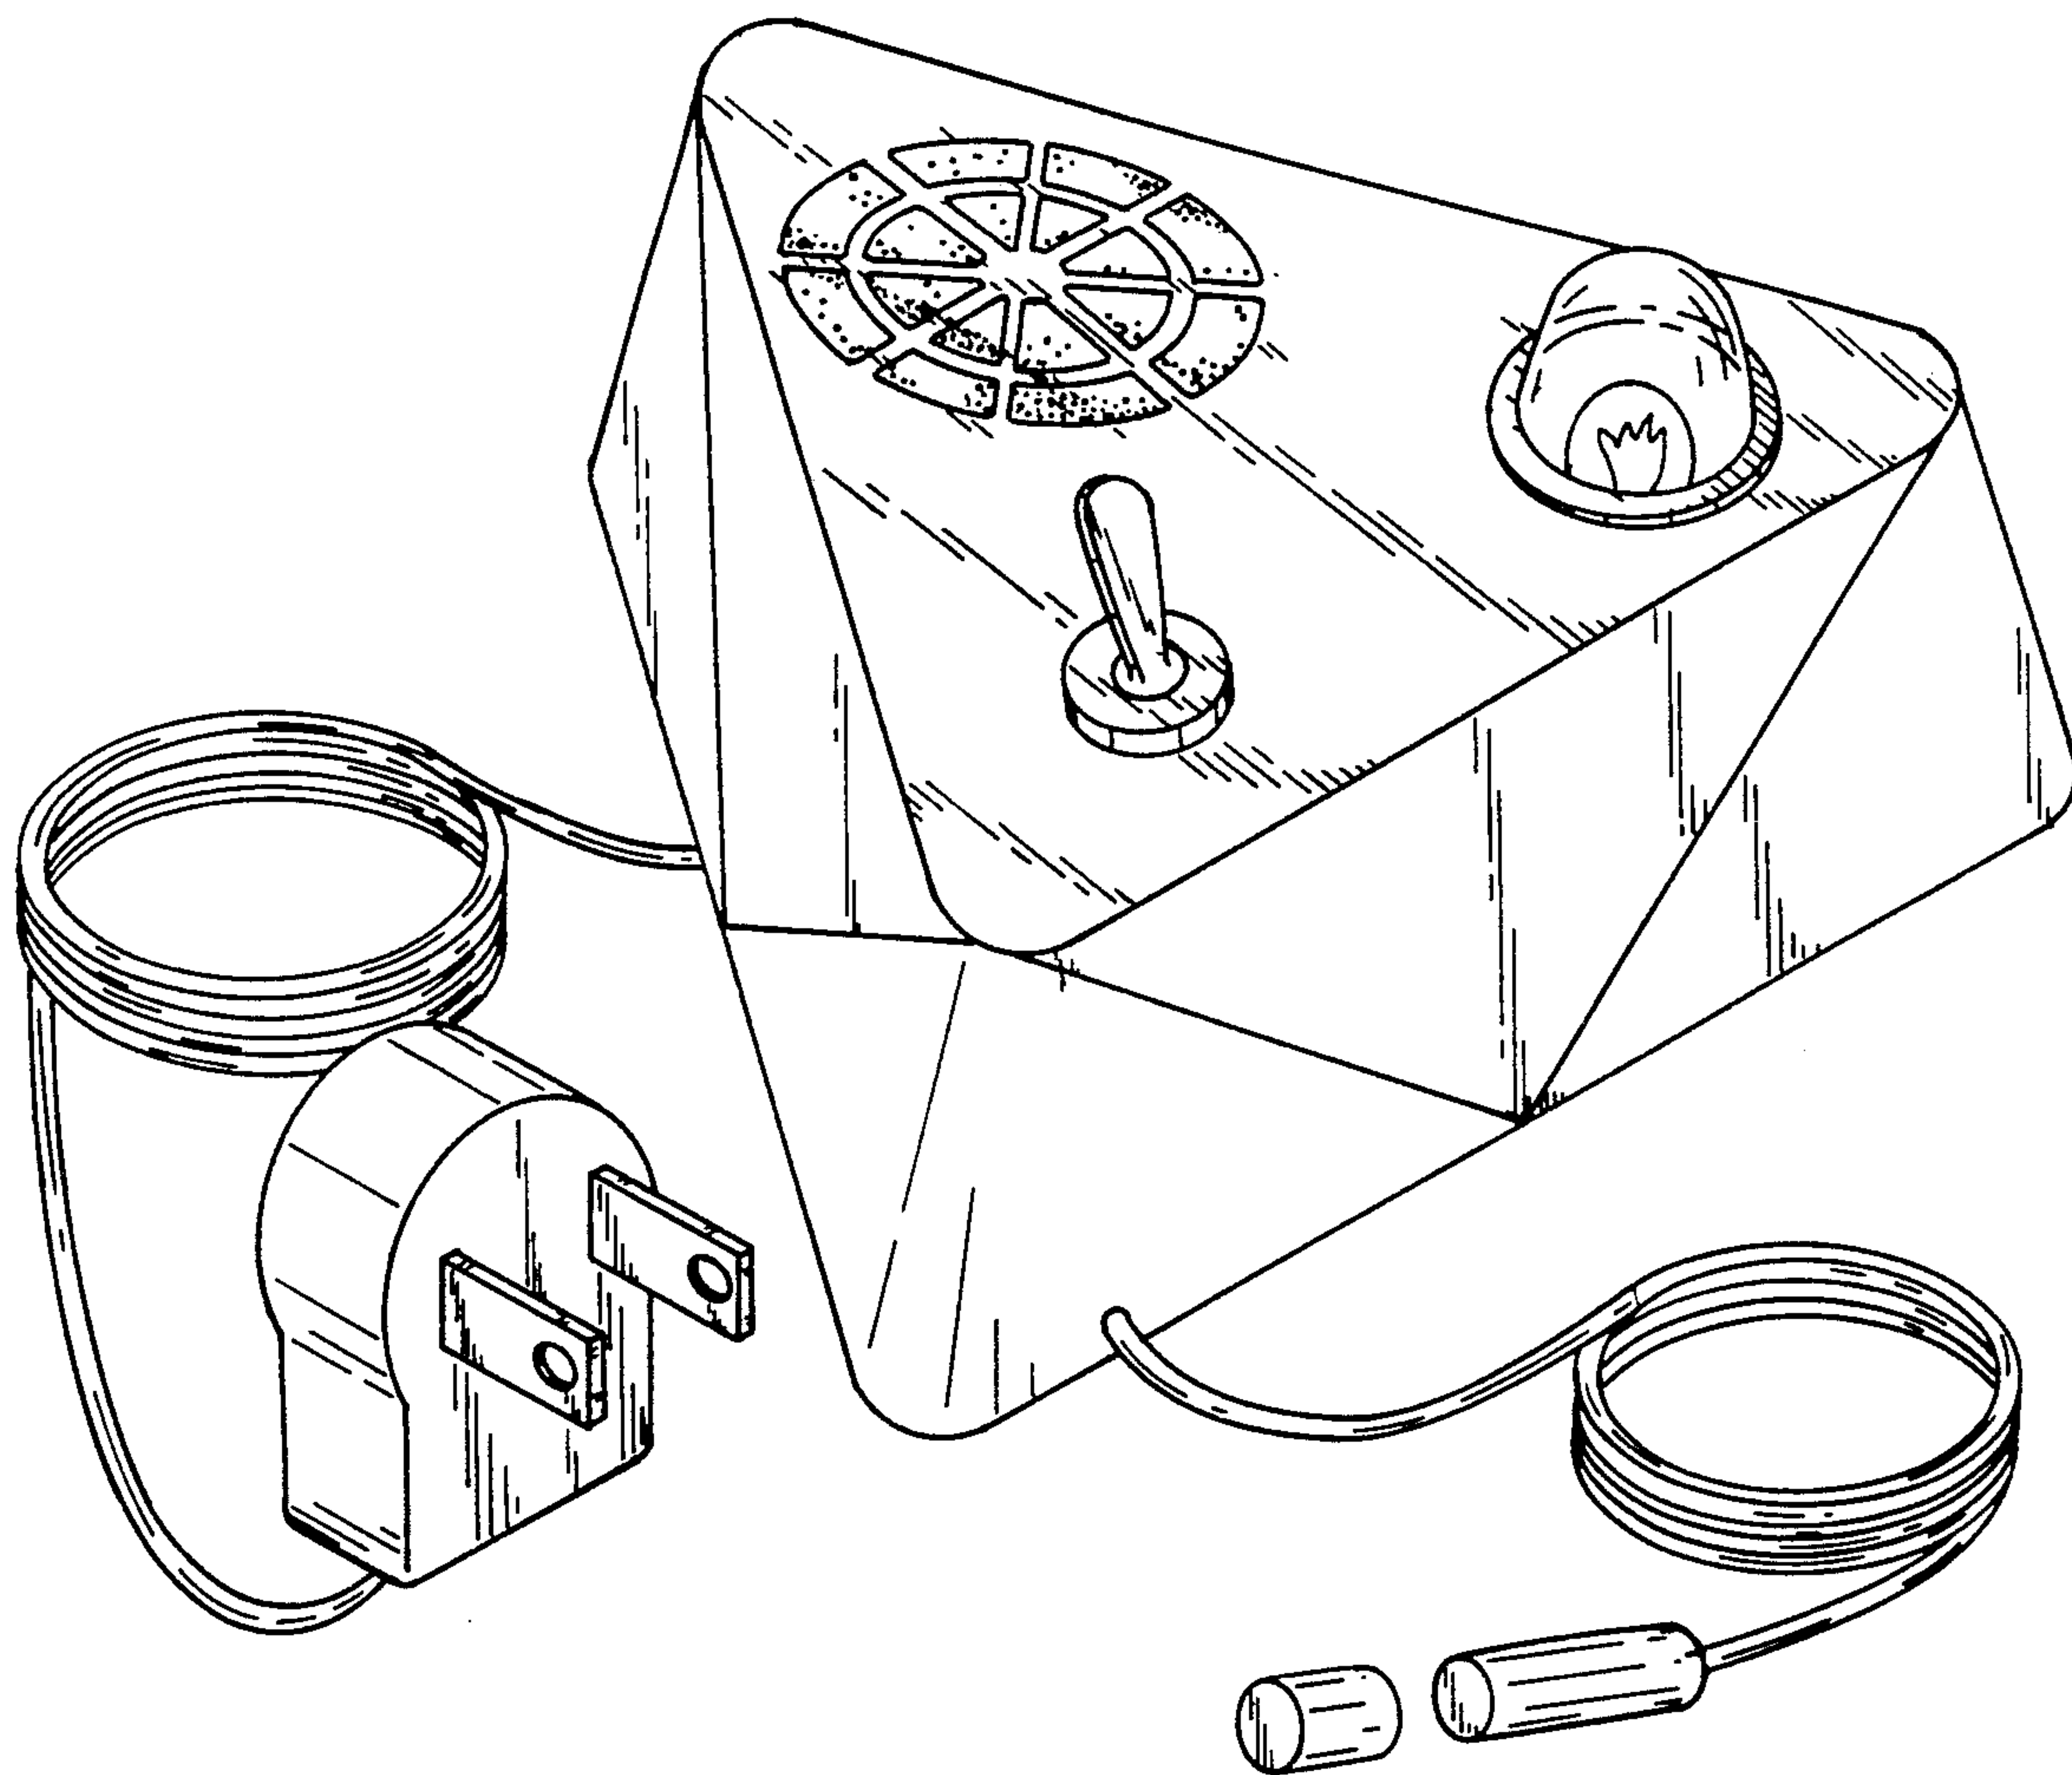

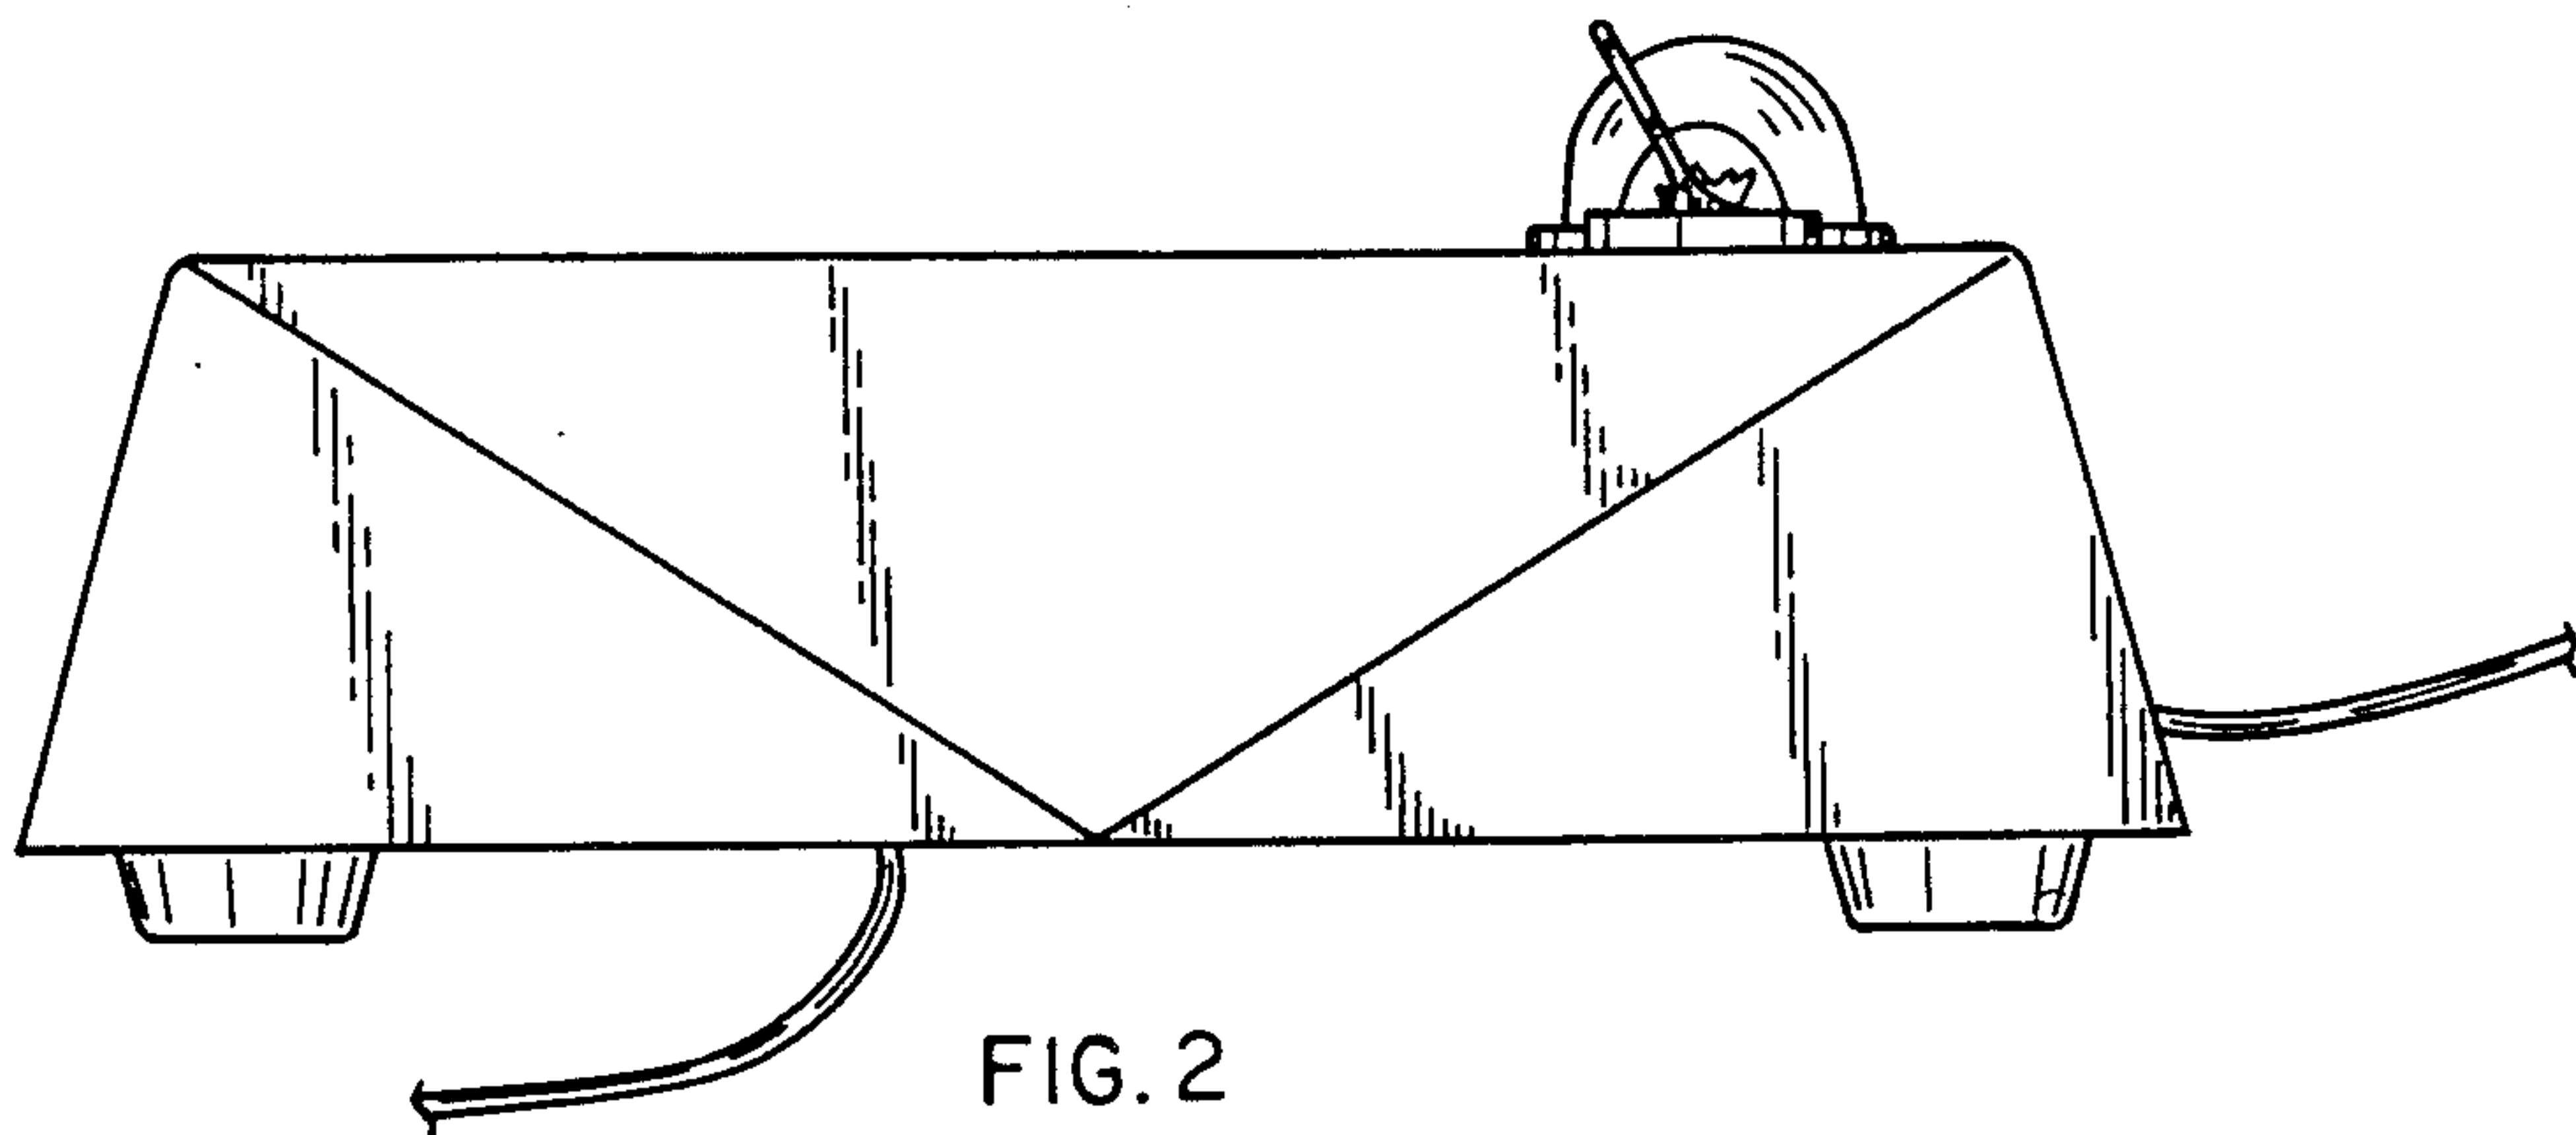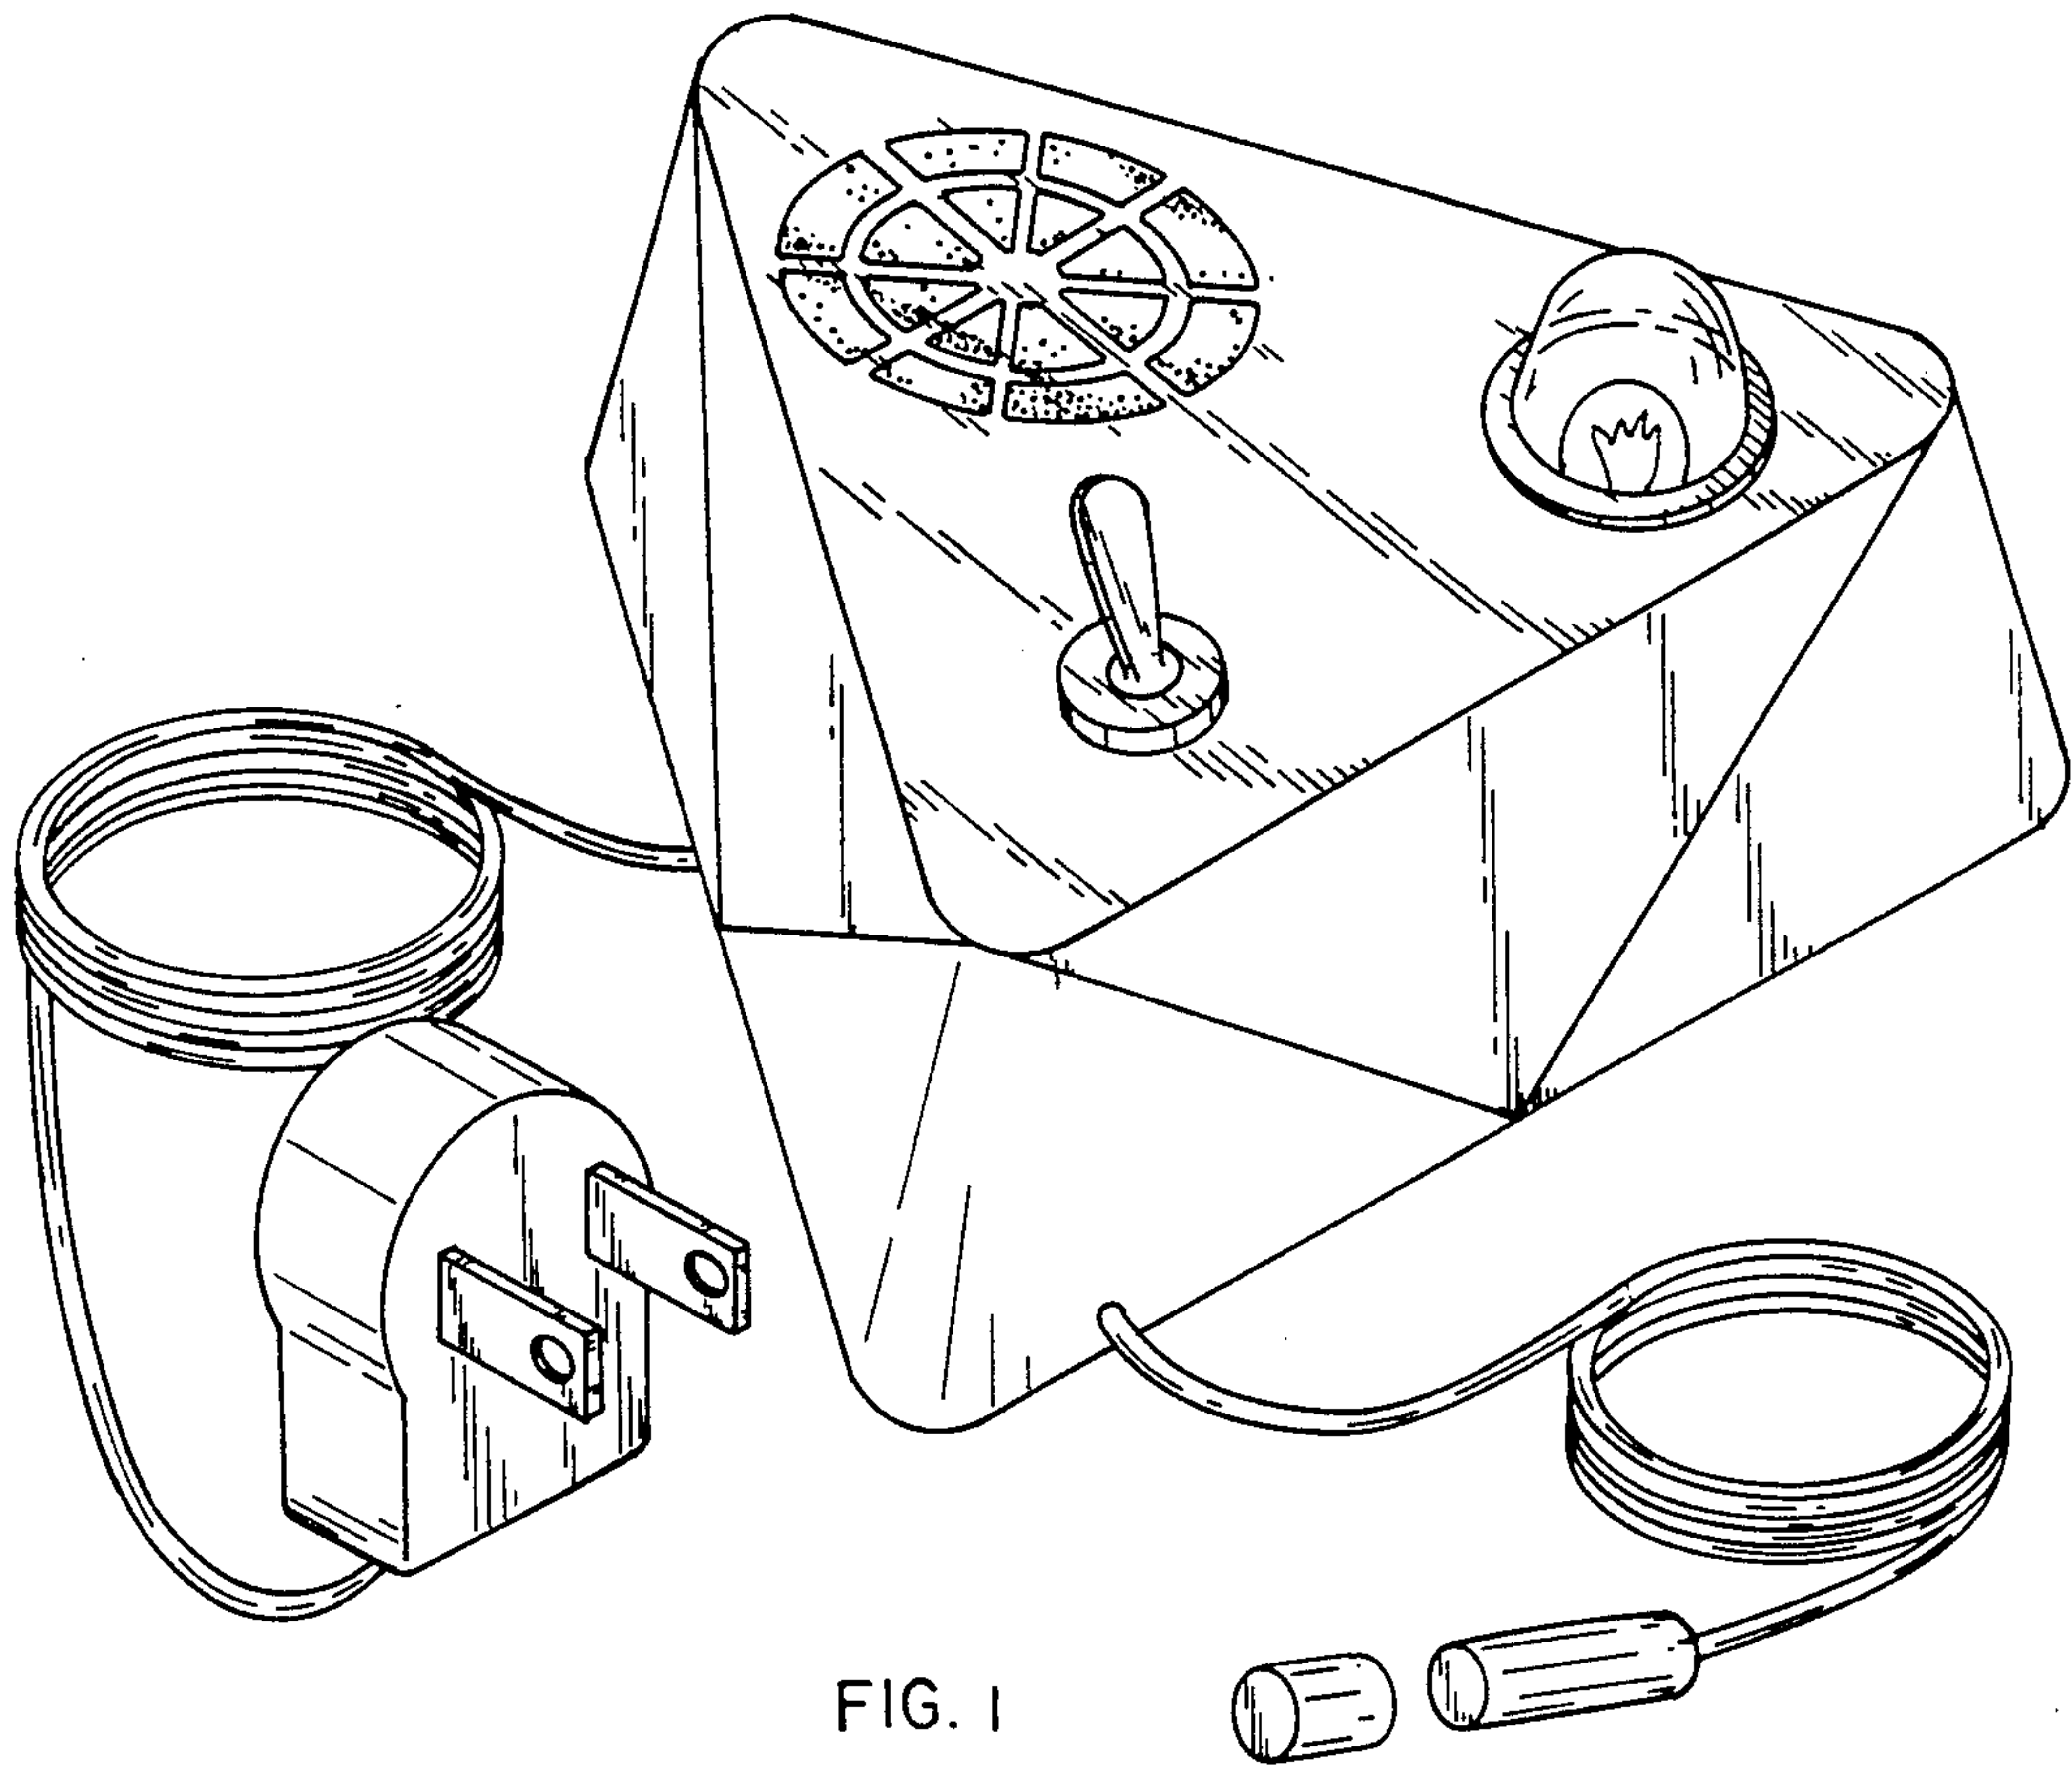

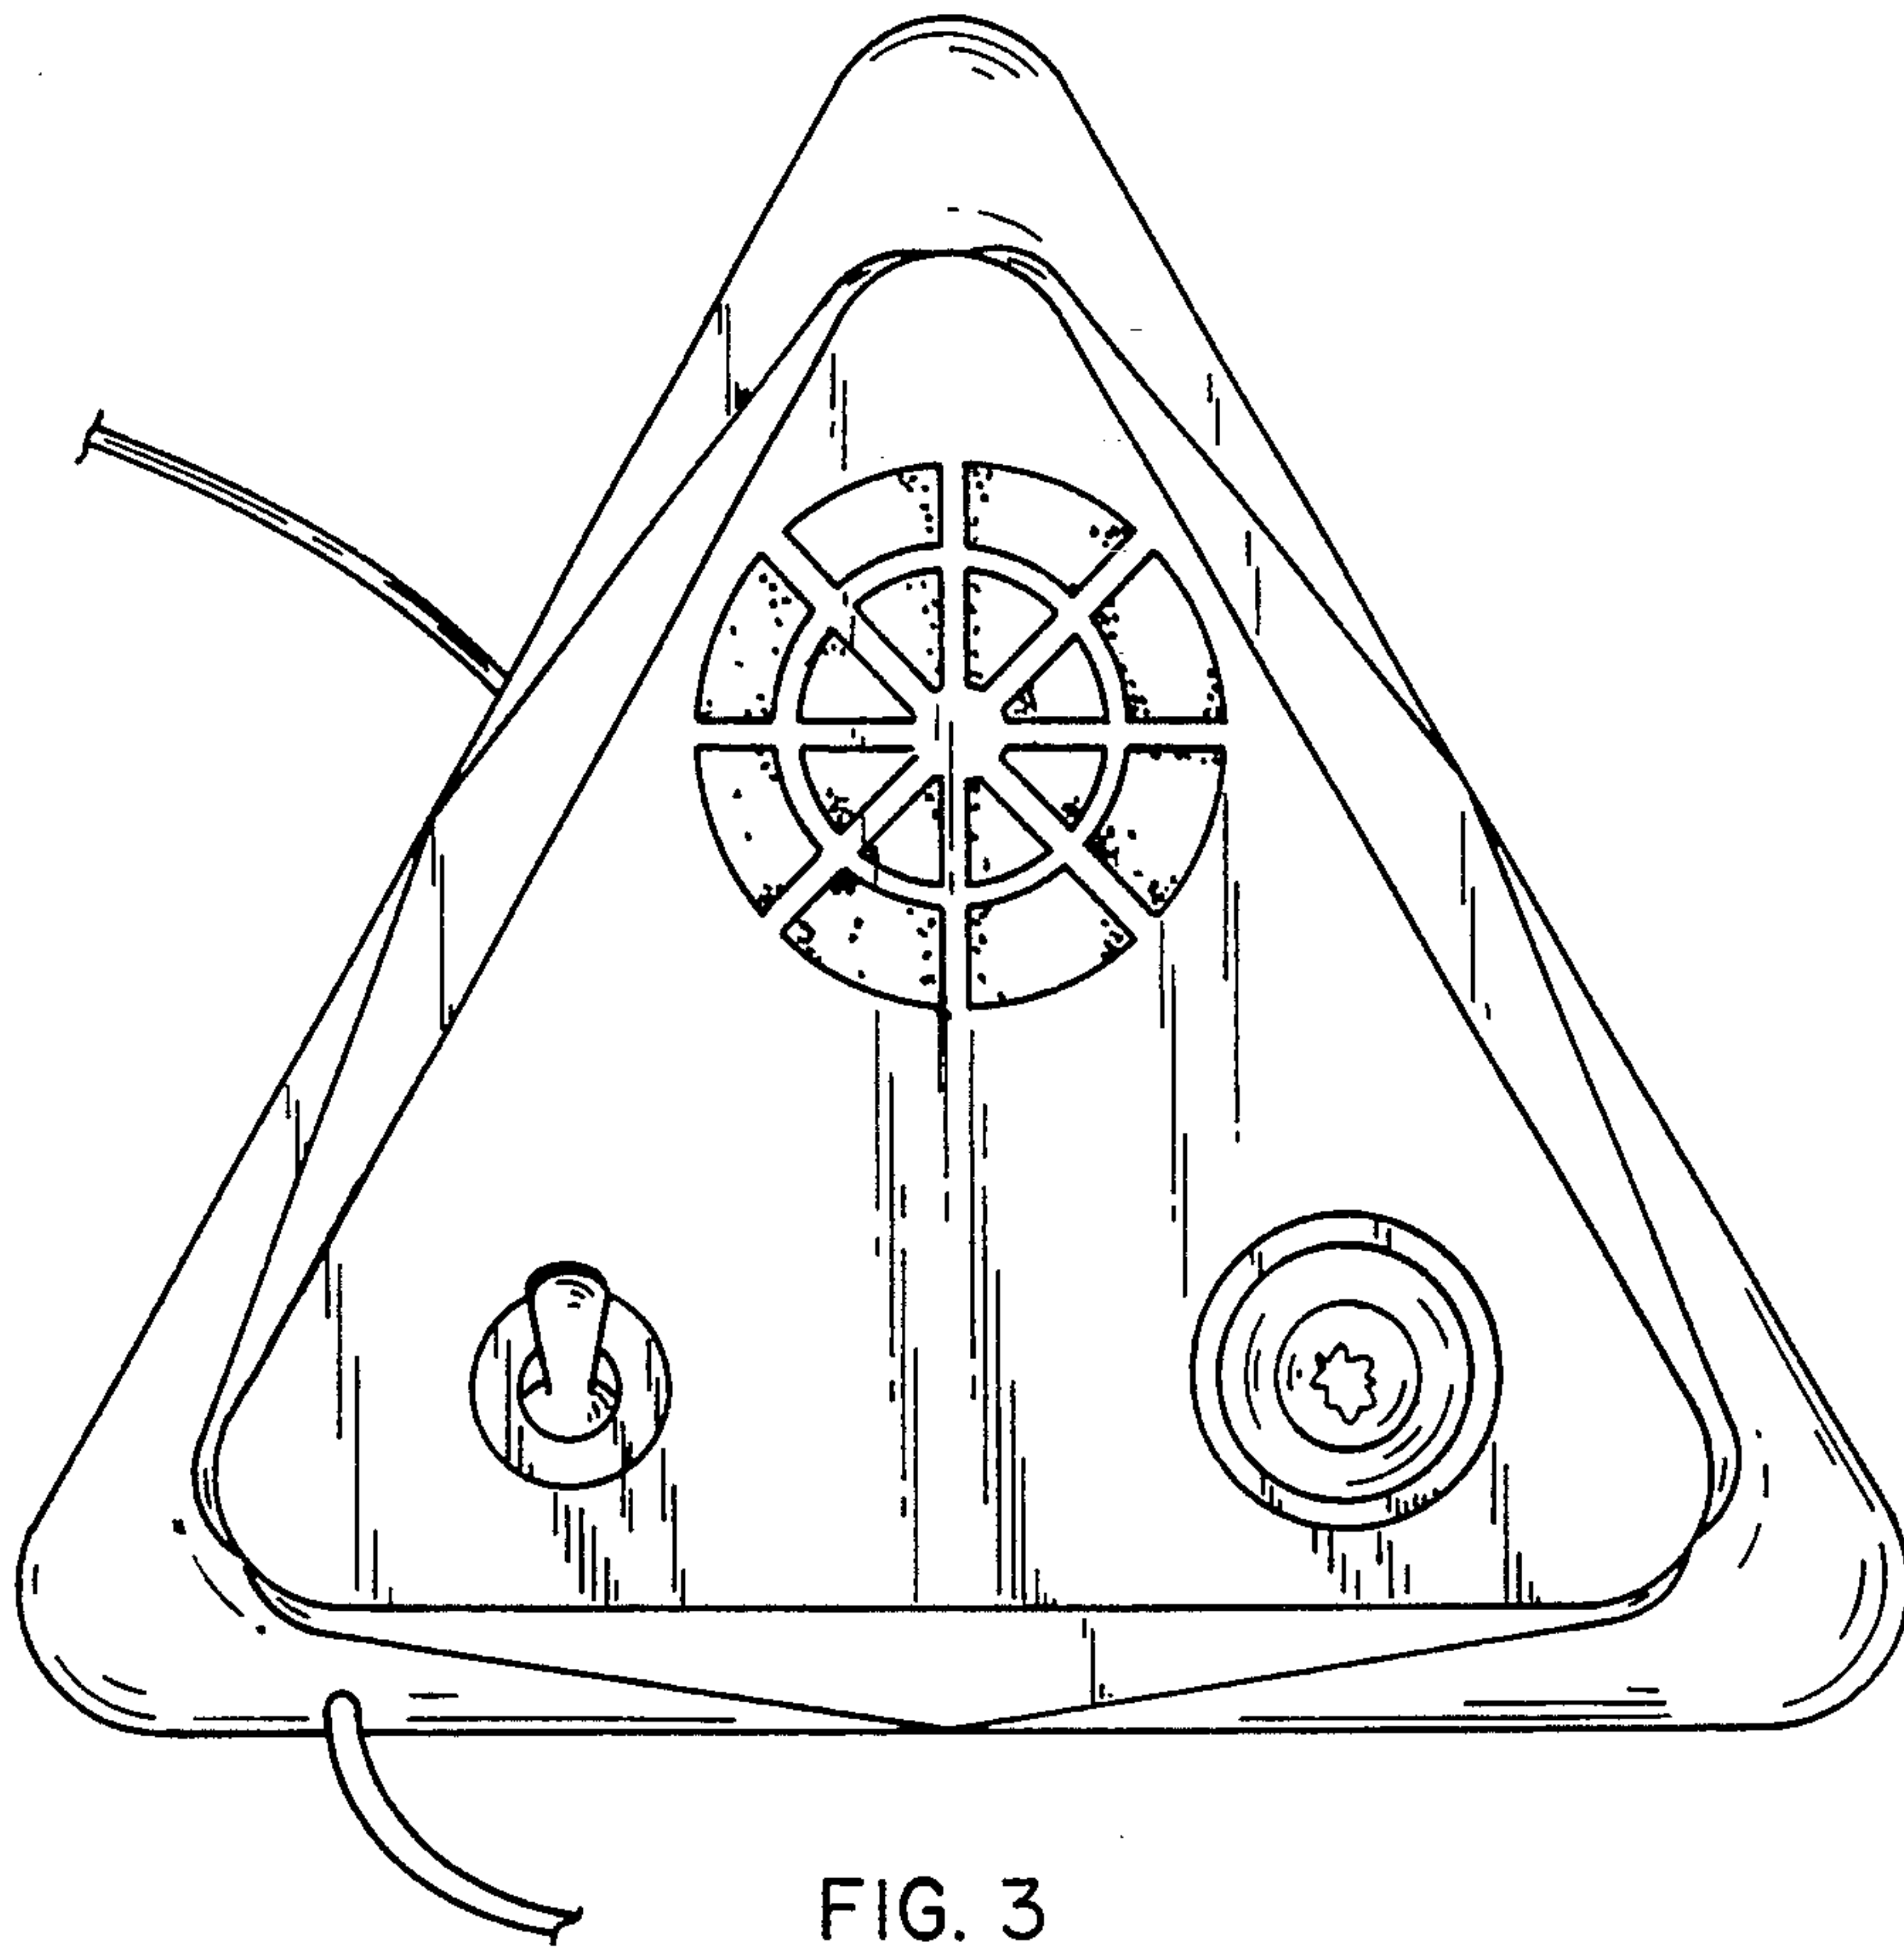


FIG. 3

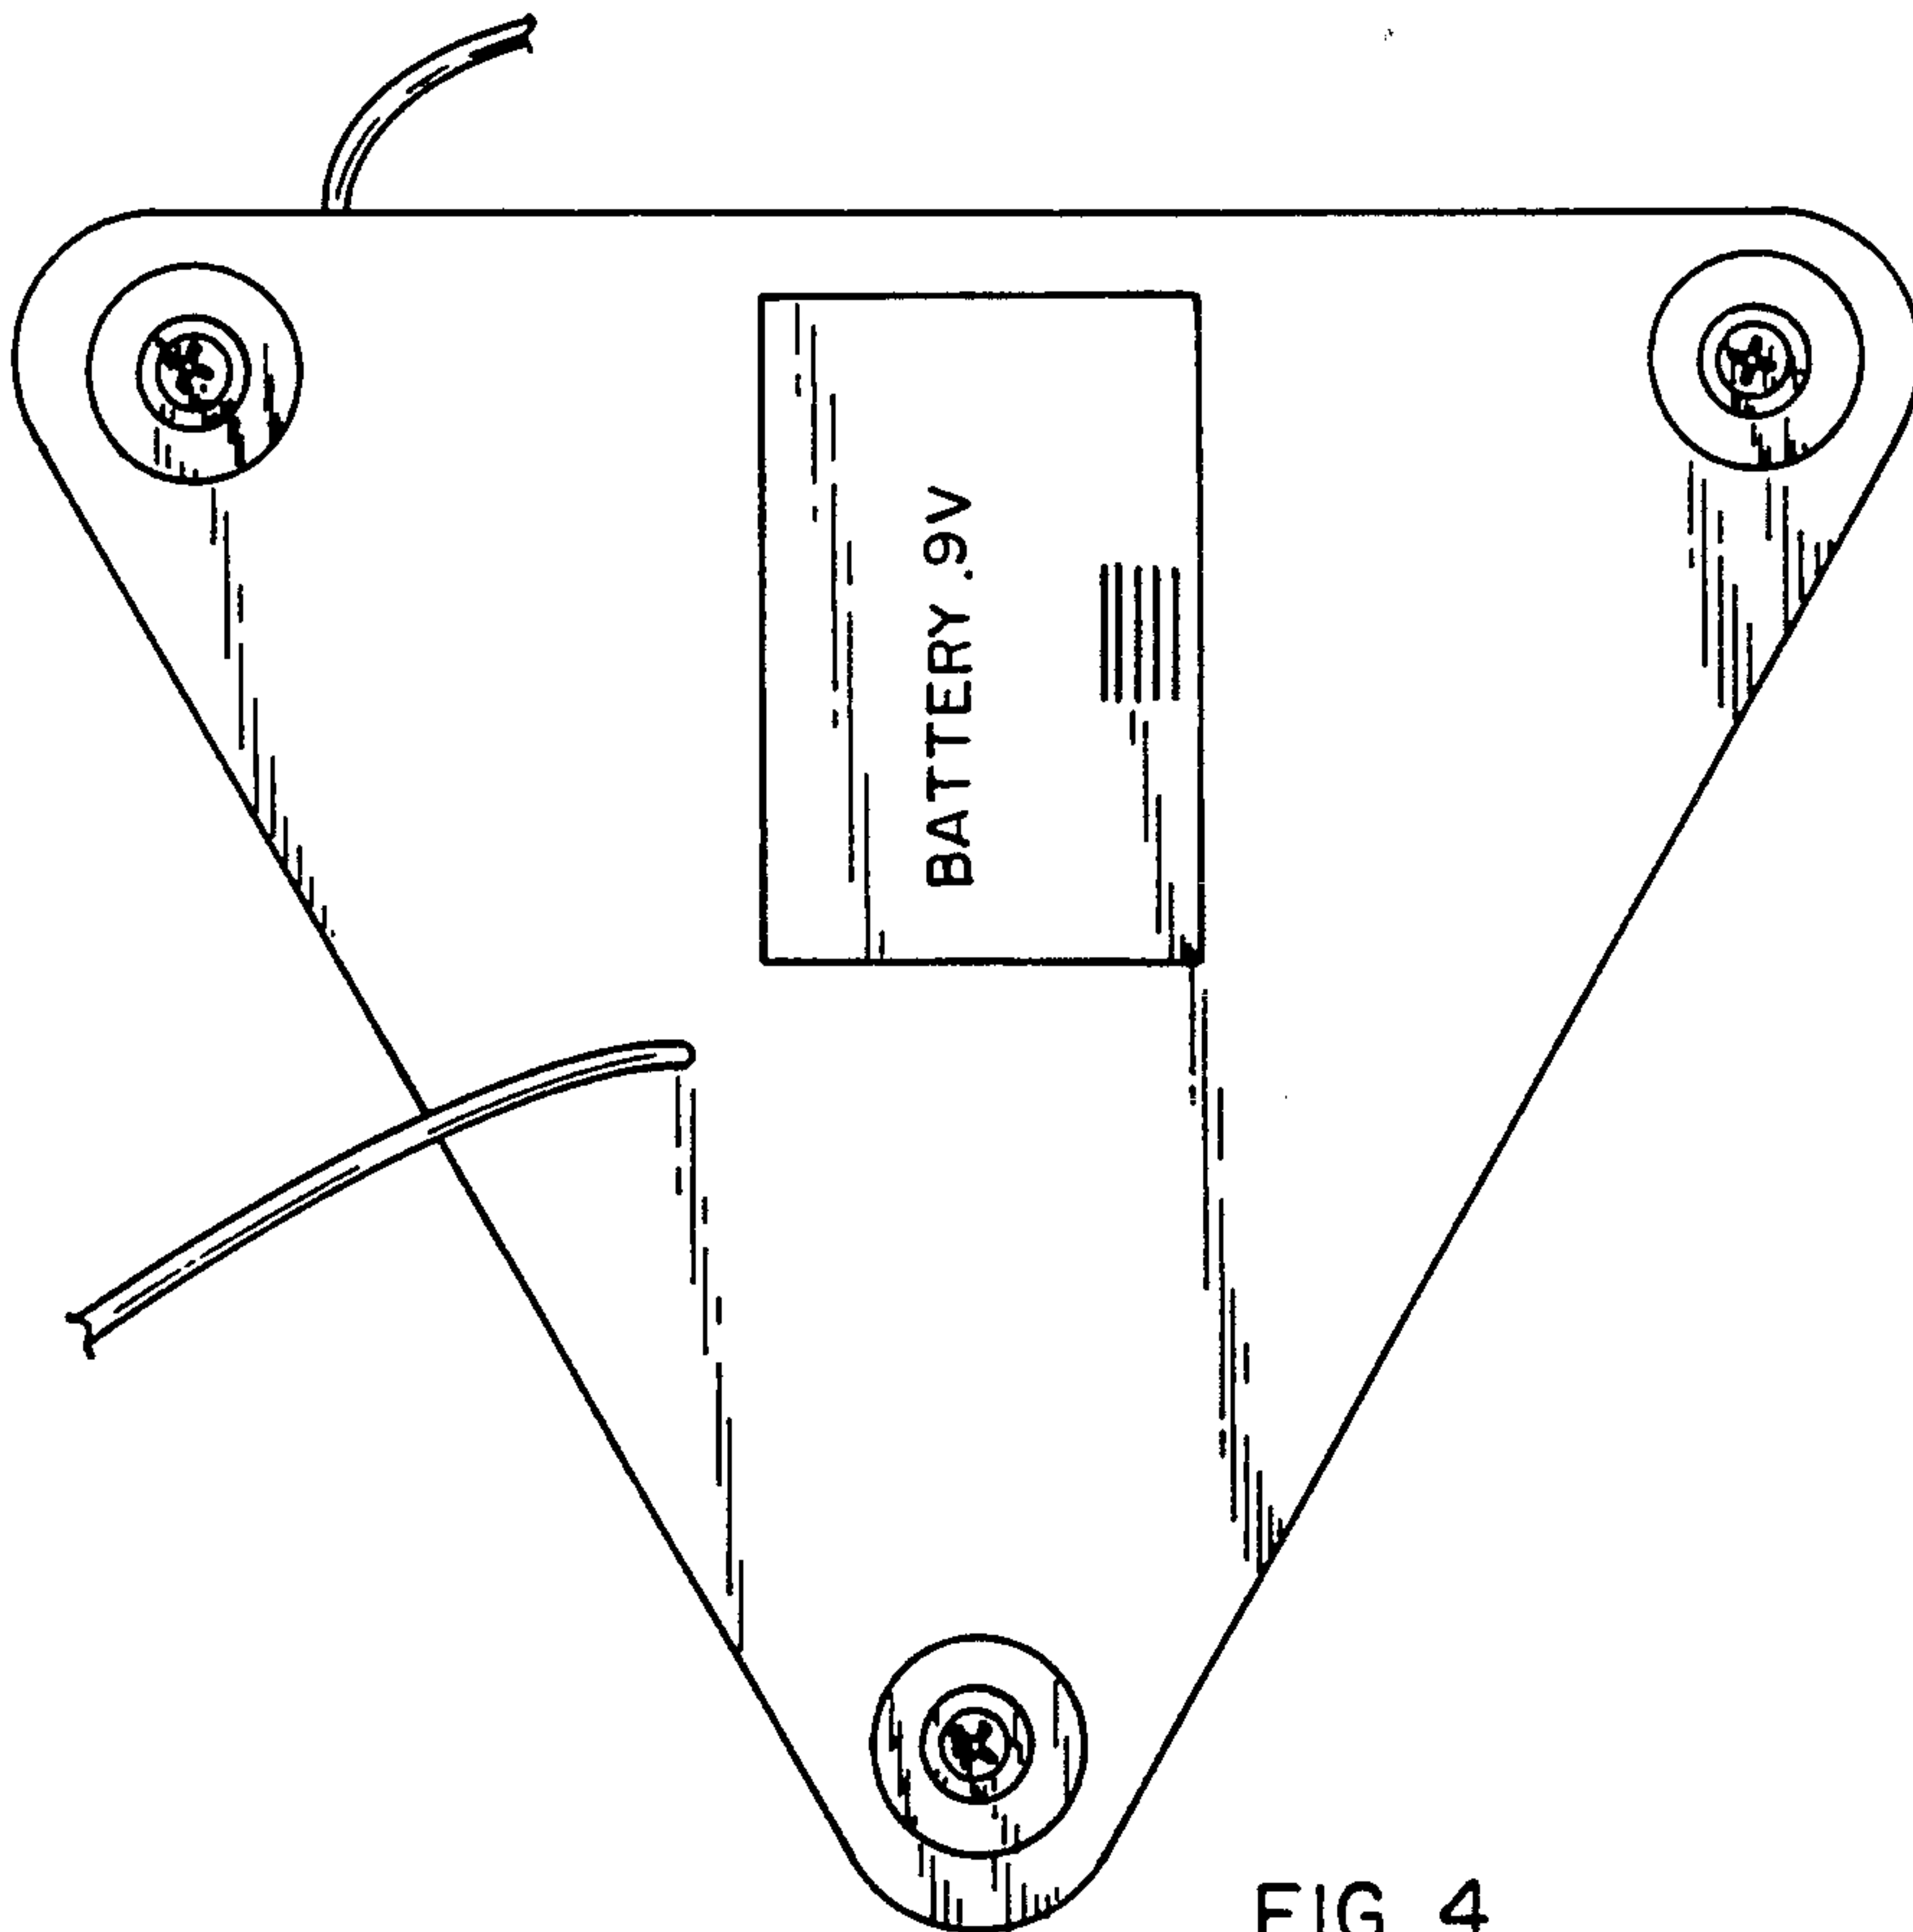


FIG. 4