

US00D325257S

United States Patent [19]

Andersen et al.

Des. 325,257 Patent Number:

Date of Patent: ** Apr. 7, 1992

CONTAINER FOR WASTE EXPELLED FROM A BLOOD GAS ANALYZER OR THE LIKE

Inventors: Joergen Andersen, Herlev; Ib O.

Sinnerup, Humlebaek; Kristian J. Hvidtfeldt, Virum, all of Denmark

Radiometer A/S, Denmark

Term: 14 Years

[21] Appl. No.: 454,120

[22] Filed: Dec. 21, 1989

[30] Foreign Application Priority Data

Jun. 23, 1989 [GB] United Kingdom 1060370

[58] 206/363, 366, 63.5; 422/81; 128/632, 635;

436/52, 68, 11; D9/370, 429

References Cited [56]

U.S. PATENT DOCUMENTS

3/1988 Burleigh et al. 128/635 X 5/1989 Pizziconi et al. 128/632

Primary Examiner—Stella Reid

Attorney, Agent, or Firm-Ostrolenk, Faber, Gerb & Soffen

[57]

CLAIM

The ornamental design for a container for waste expelled from a blood gas analyzer or the like, as shown.


DESCRIPTION


FIG. 1 is a perspective view of a container for waste expelled from a blood gas analyzer or the like, showing our new design;

FIG. 2 is a side elevational view thereof, the opposite side elevational view being identical;

FIG. 3 is a front elevational view thereof; and,

FIG. 4 is a bottom plan view thereof.

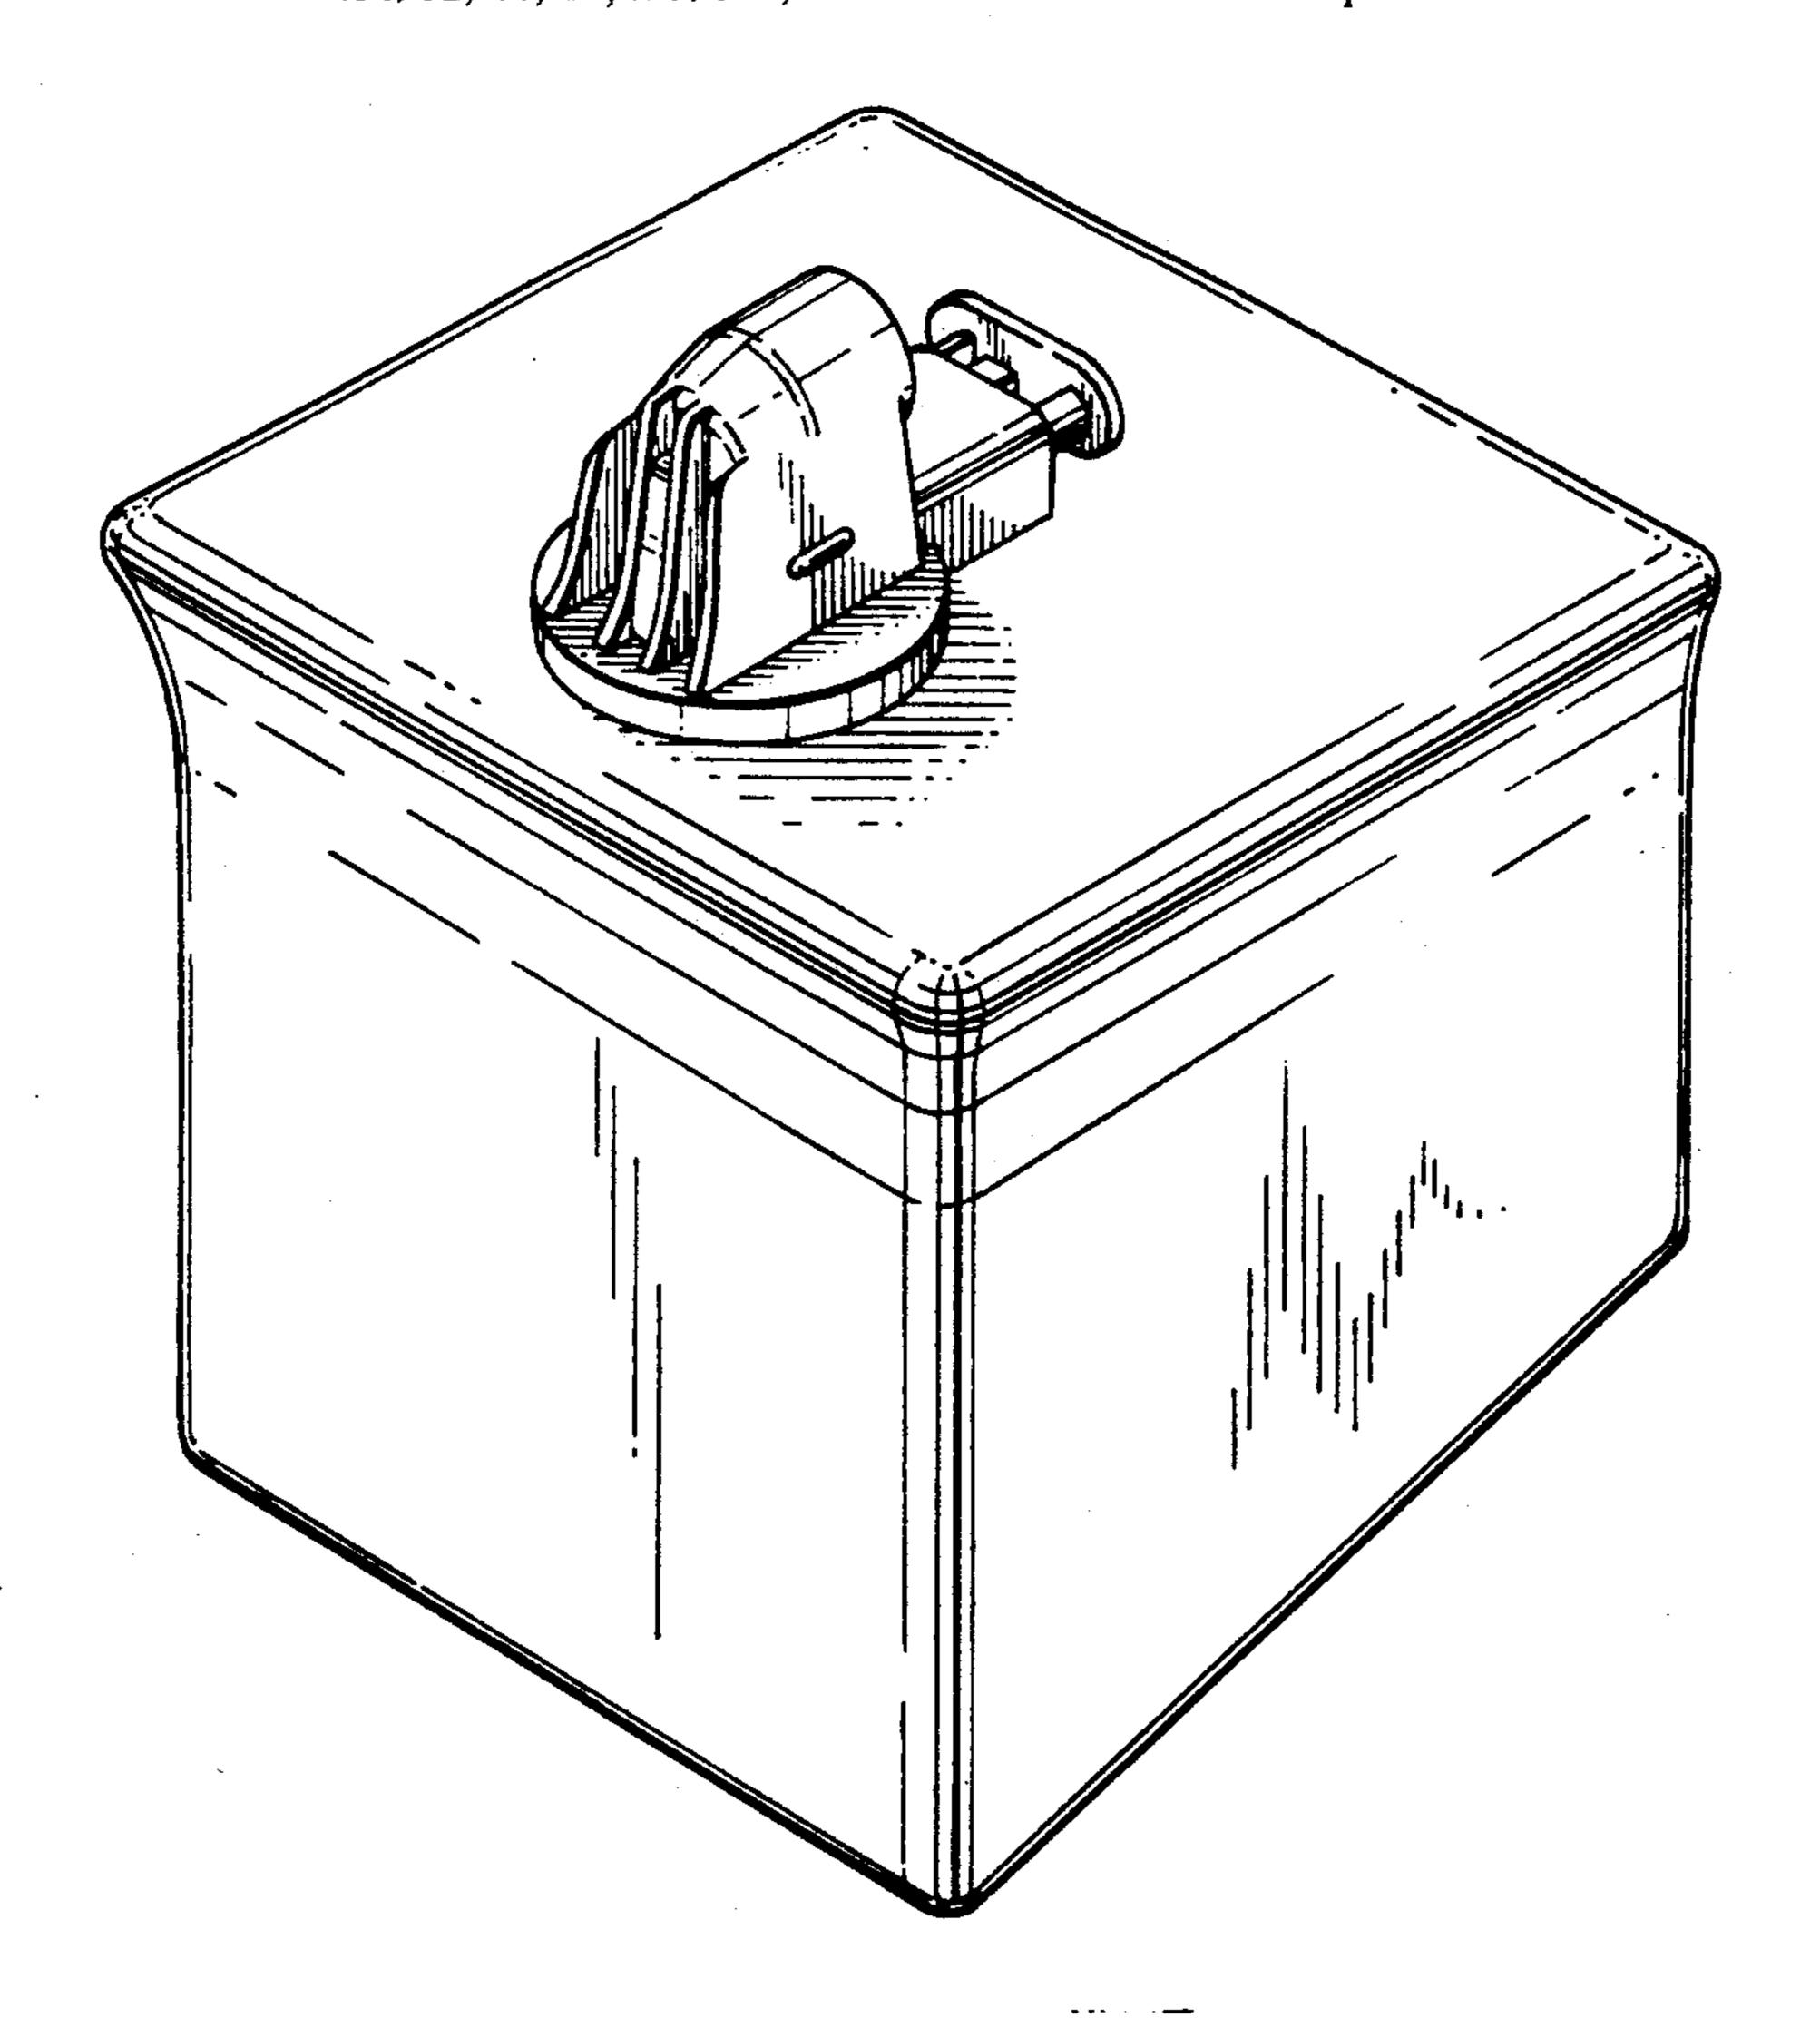

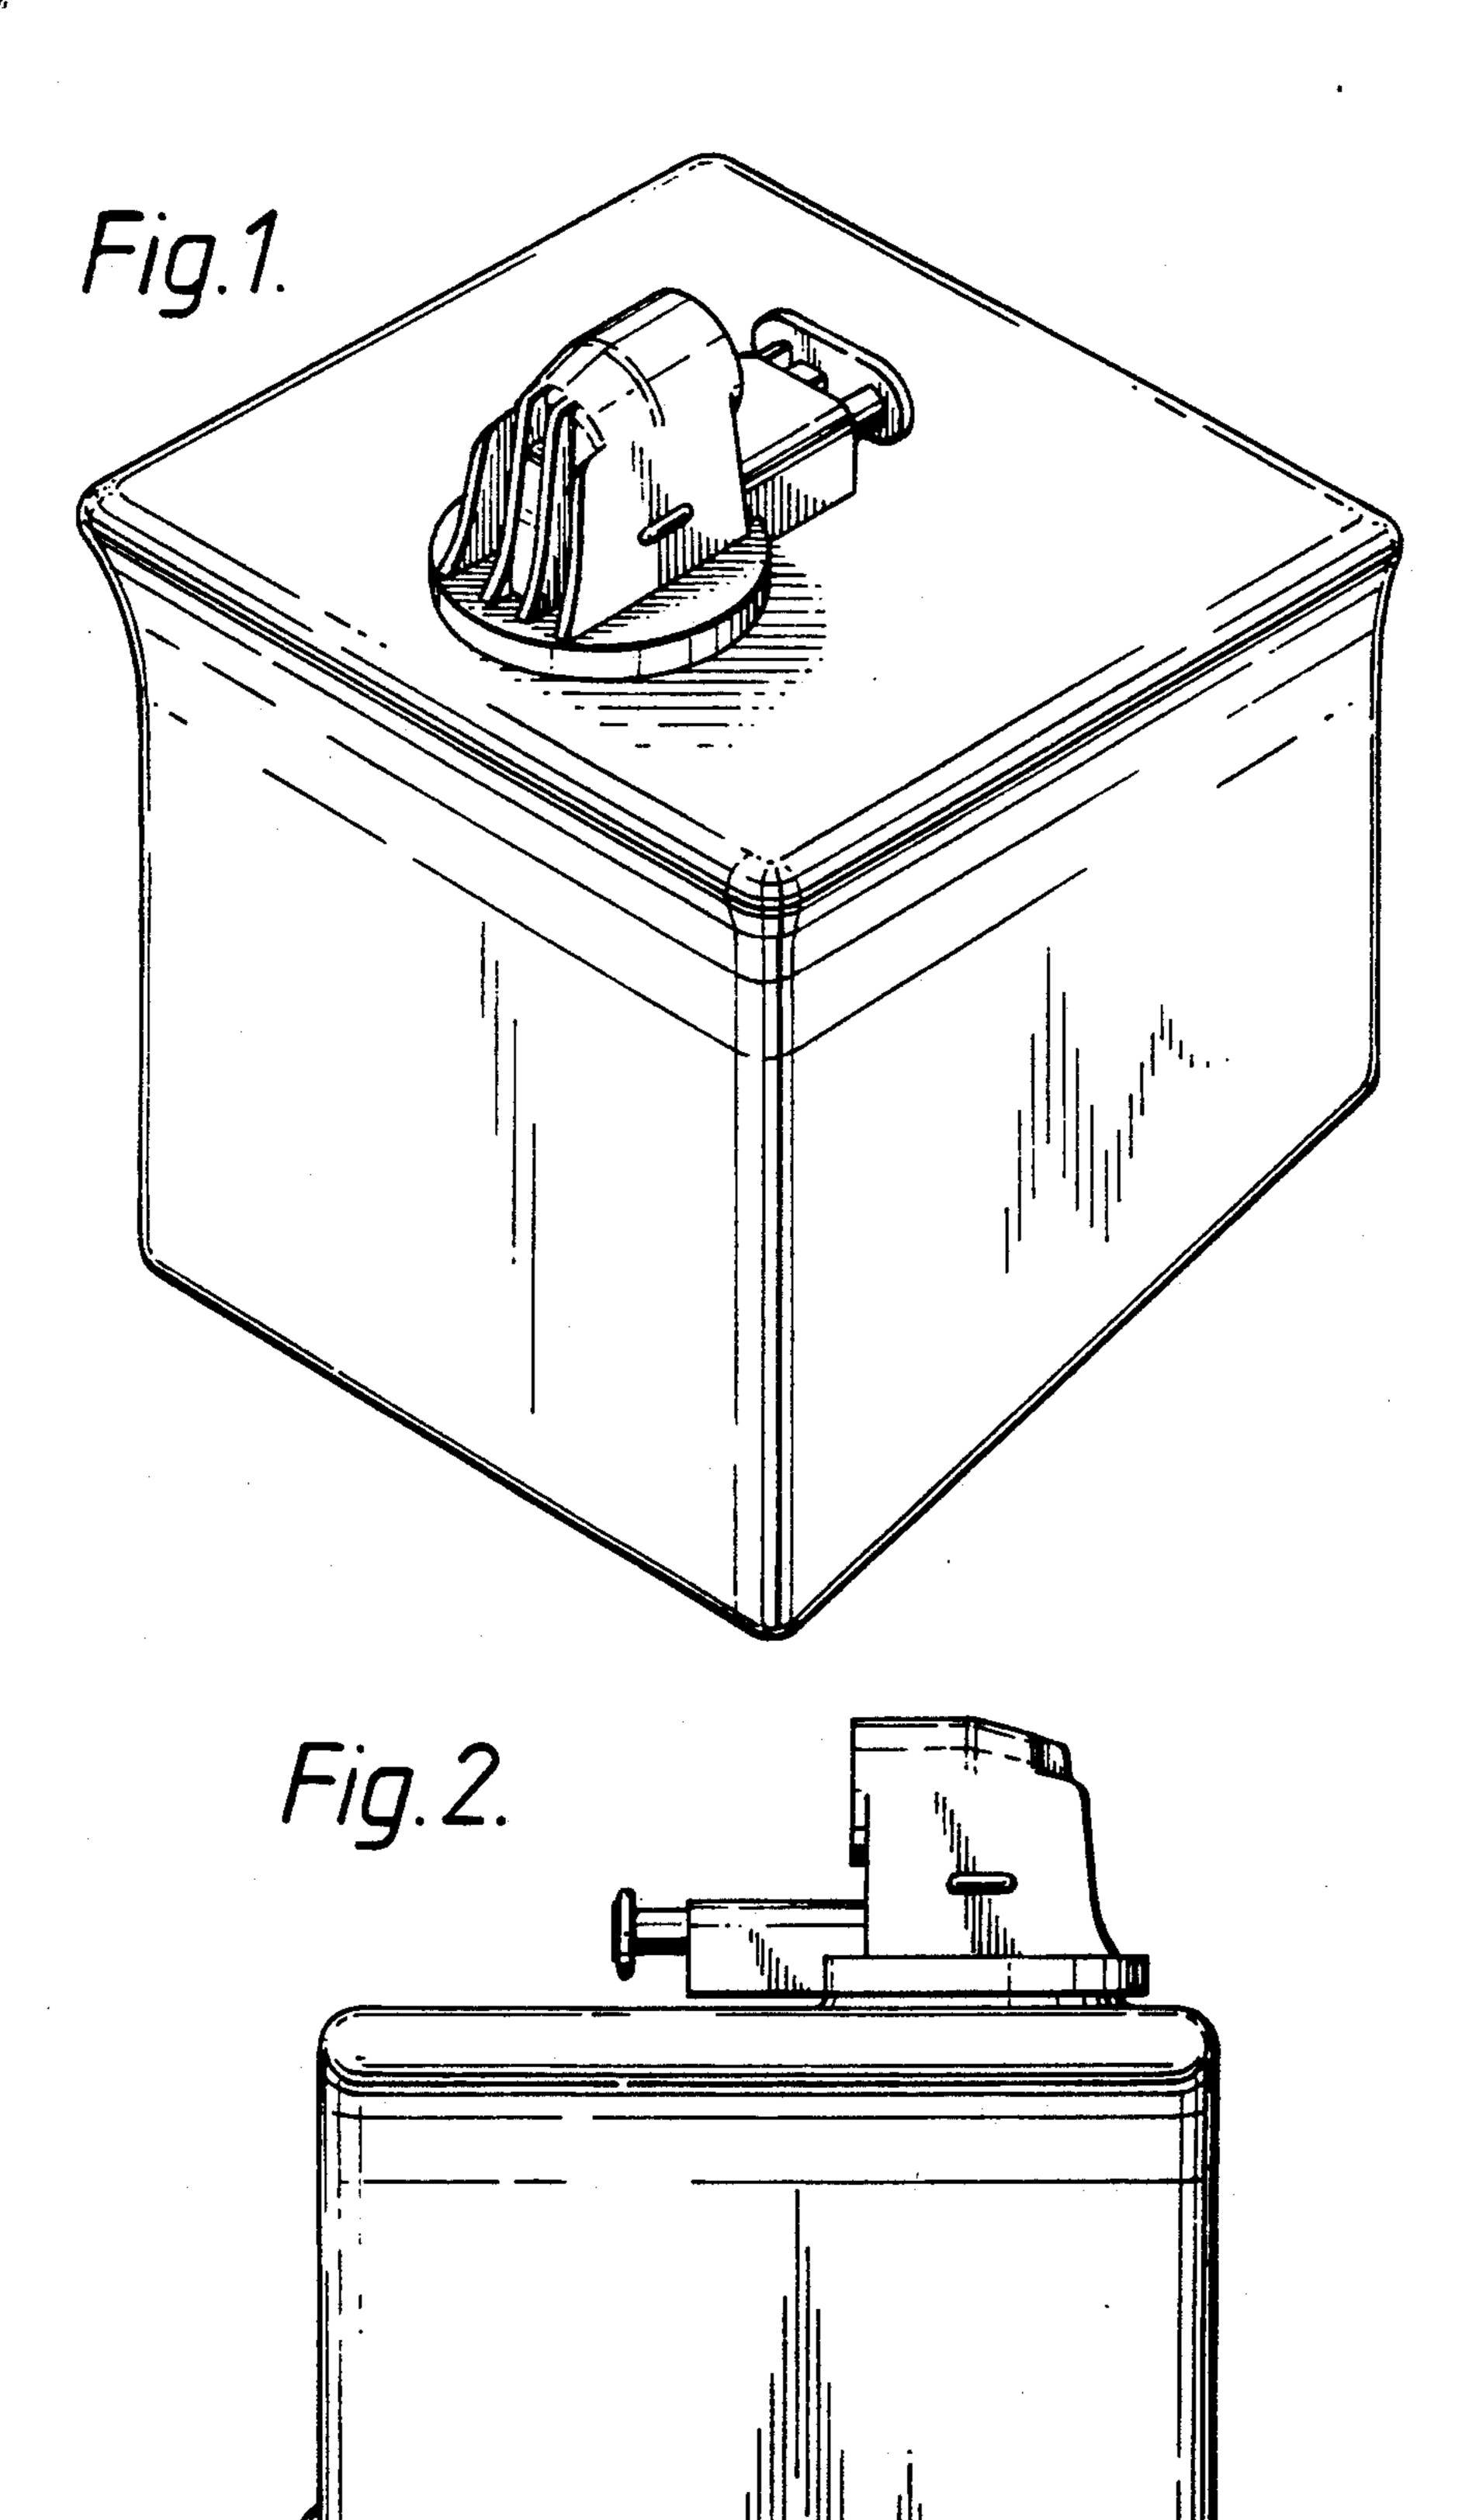


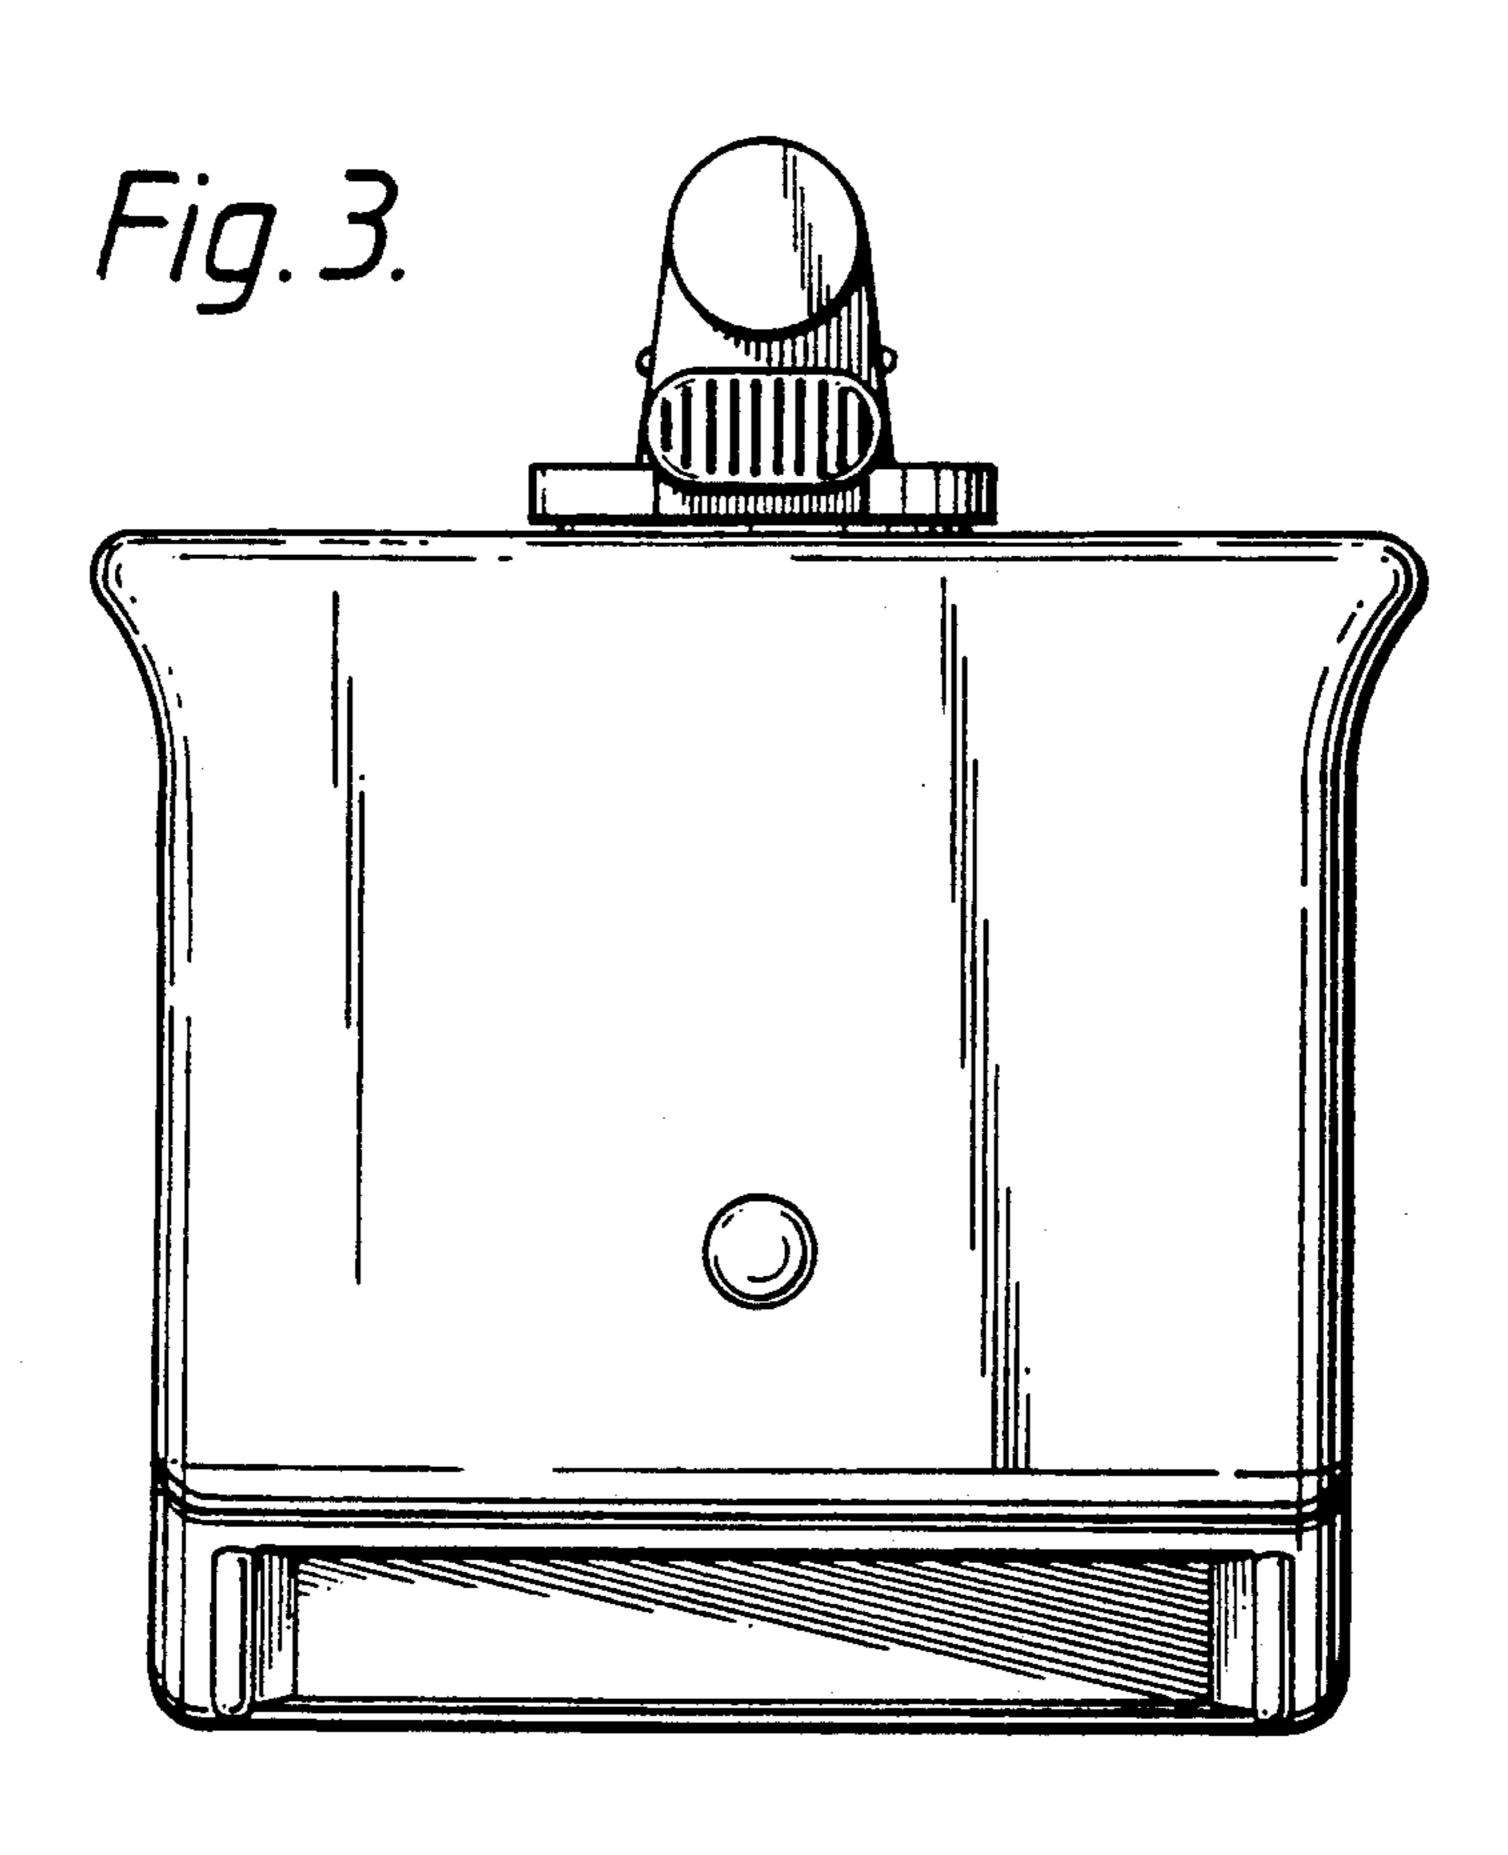


Fig.4.

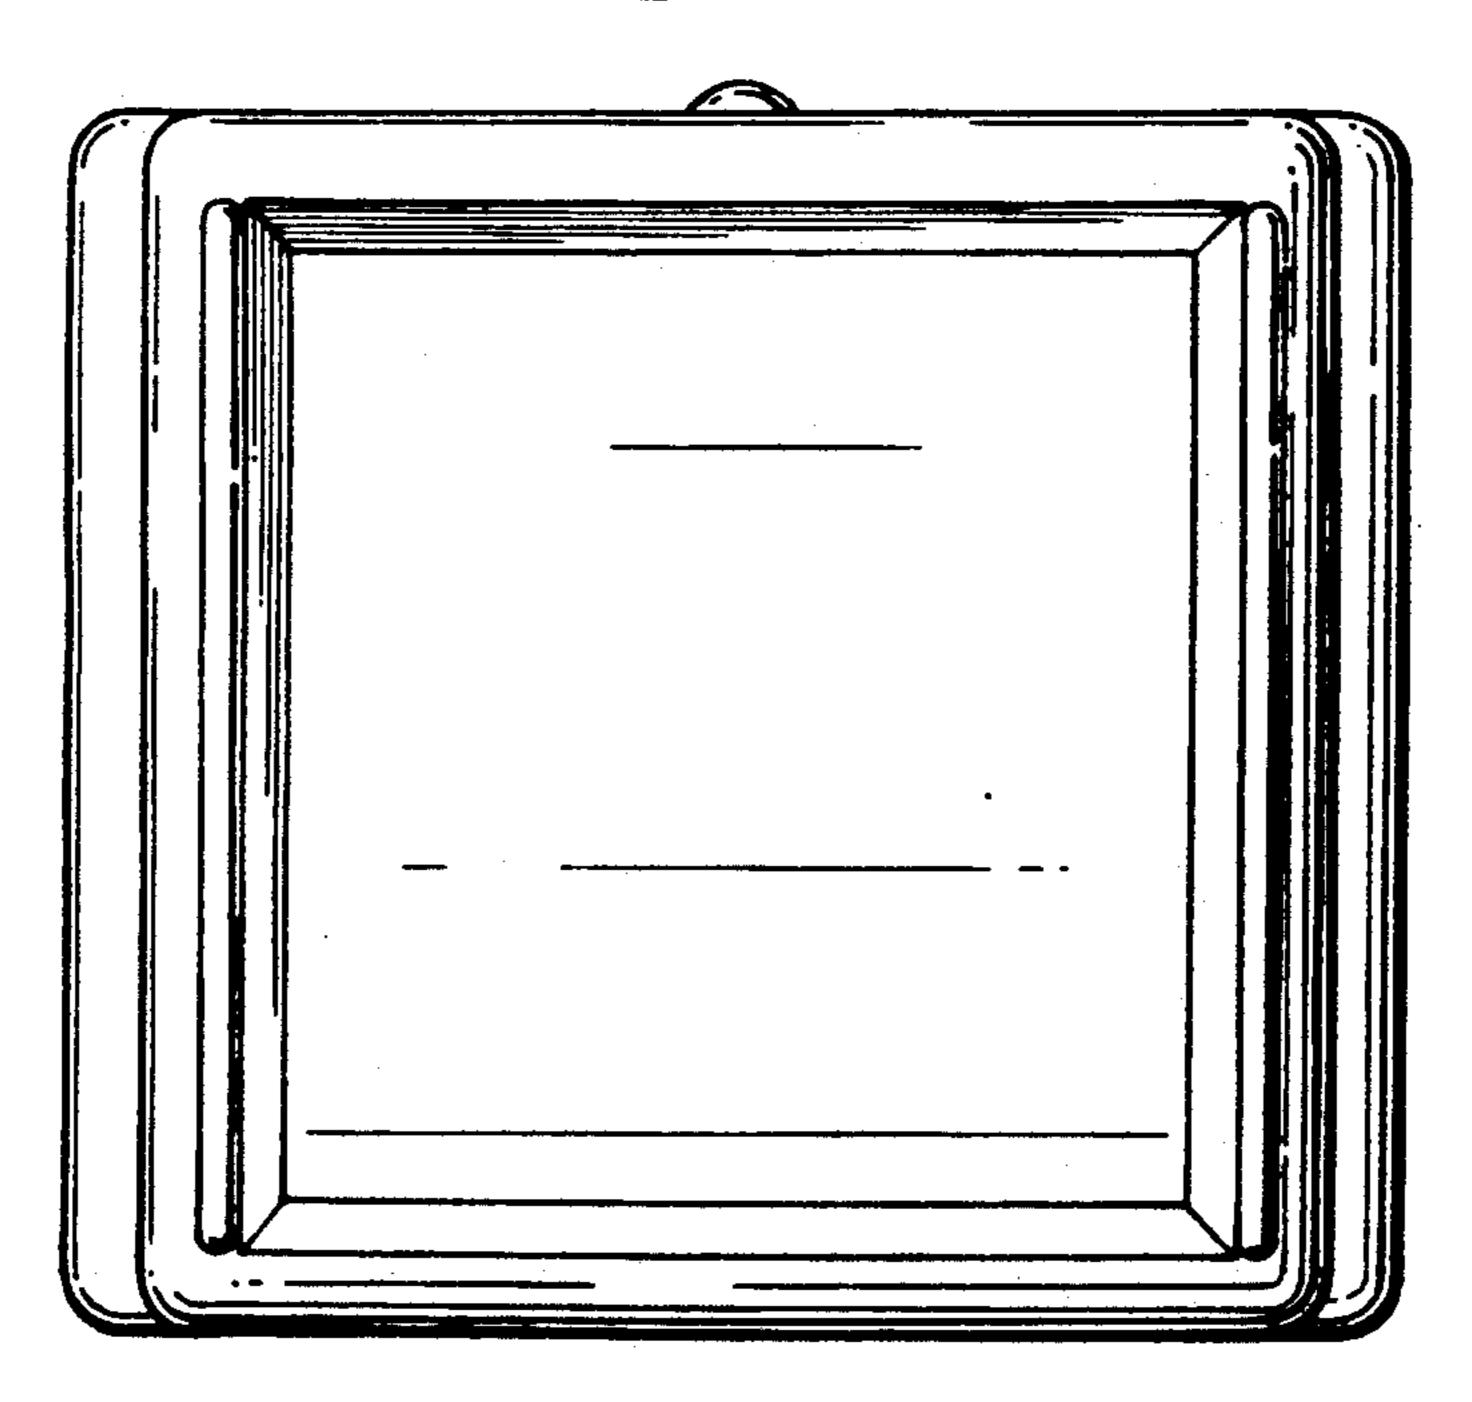

UNITED STATES PATENT AND TRADEMARK OFFICE CERTIFICATE OF CORRECTION

PATENT NO. : Des. 325,257

DATED : April 7, 1992

INVENTOR(S): J. Anderson, et al

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

On the title page:

In the claim: delete "a container for waste expelled from a blood gas analyzer or the like, " and read --container for liquid--.

Signed and Sealed this
Tenth Day of August, 1993

Attest:

Attesting Officer

MICHAEL K. KIRK

Acting Commissioner of Patents and Trademarks