

US00D325258S

United States Patent [19]

Andersen et al.

[11] Patent Number: Des. 325,258 [45] Date of Patent: ** Apr. 7, 1992

[54]	CONTAINER FOR WASTE EXPELLED
	FROM A BLOOD GAS ANALYZER OR THE
	LIKE

[75] Inventors: Joergen Andersen, Herlev; Ib O.

Sinnerup, Humlebaek; Kristian J. Hvidtfeldt, Virum, all of Denmark

[73] Assignee: Radiometer A/S, Denmark

[**] Term: 14 Years

[21] Appl. No.: 454,121

[22] Filed: Dec. 21, 1989

[30] Foreign Application Priority Data

[56] References Cited U.S. PATENT DOCUMENTS

D. 302,291	7/1989	Heubel et al D24/131
4,520,926	6/1985	Nelson D24/131 X
4,734,184	3/1988	Burleigh et al 128/635 X
4,832,034	5/1989	Pizziconi et al 128/632

Primary Examiner—Stella Reid Attorney, Agent, or Firm—Ostrolenk, Faber, Gerb & Soffen

[57] CLAIM

The ornamental design for a container for waste expelled from a blood gas analyzer or the like, as shown.


DESCRIPTION


FIG. 1 is a perspective view of a container for waste expelled from a blood gas analyzer or the like, showing our new design;

FIG. 2 is a side elevational view thereof, the opposite side elevational view being identical;


FIG. 3 is a front elevational view thereof; and,

FIG. 4 is a bottom plan view thereof.

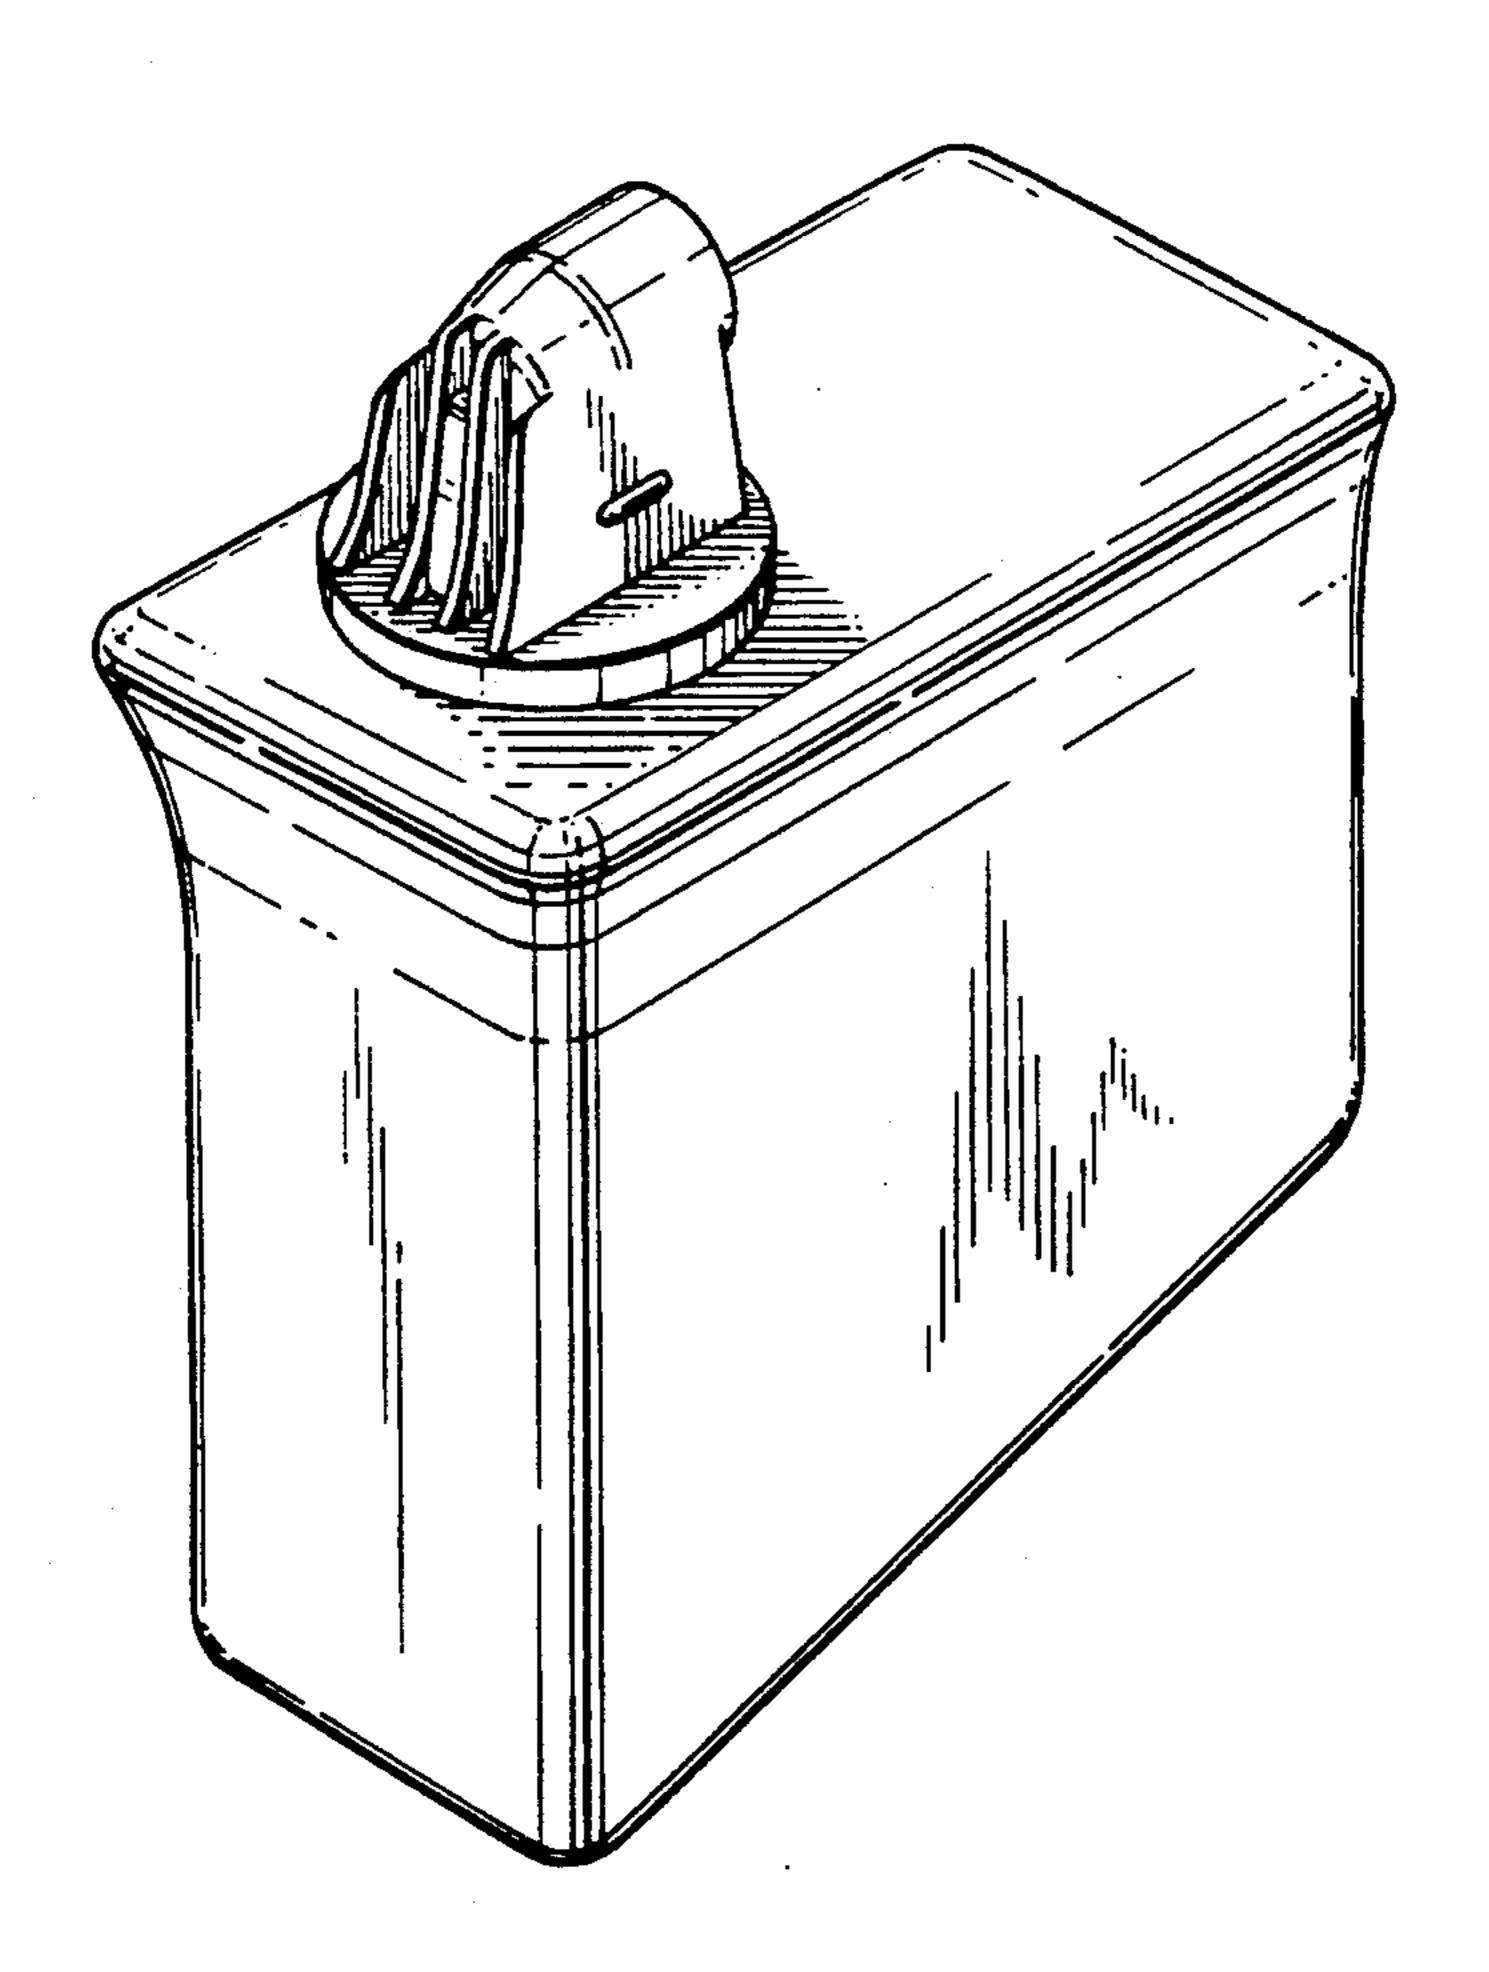

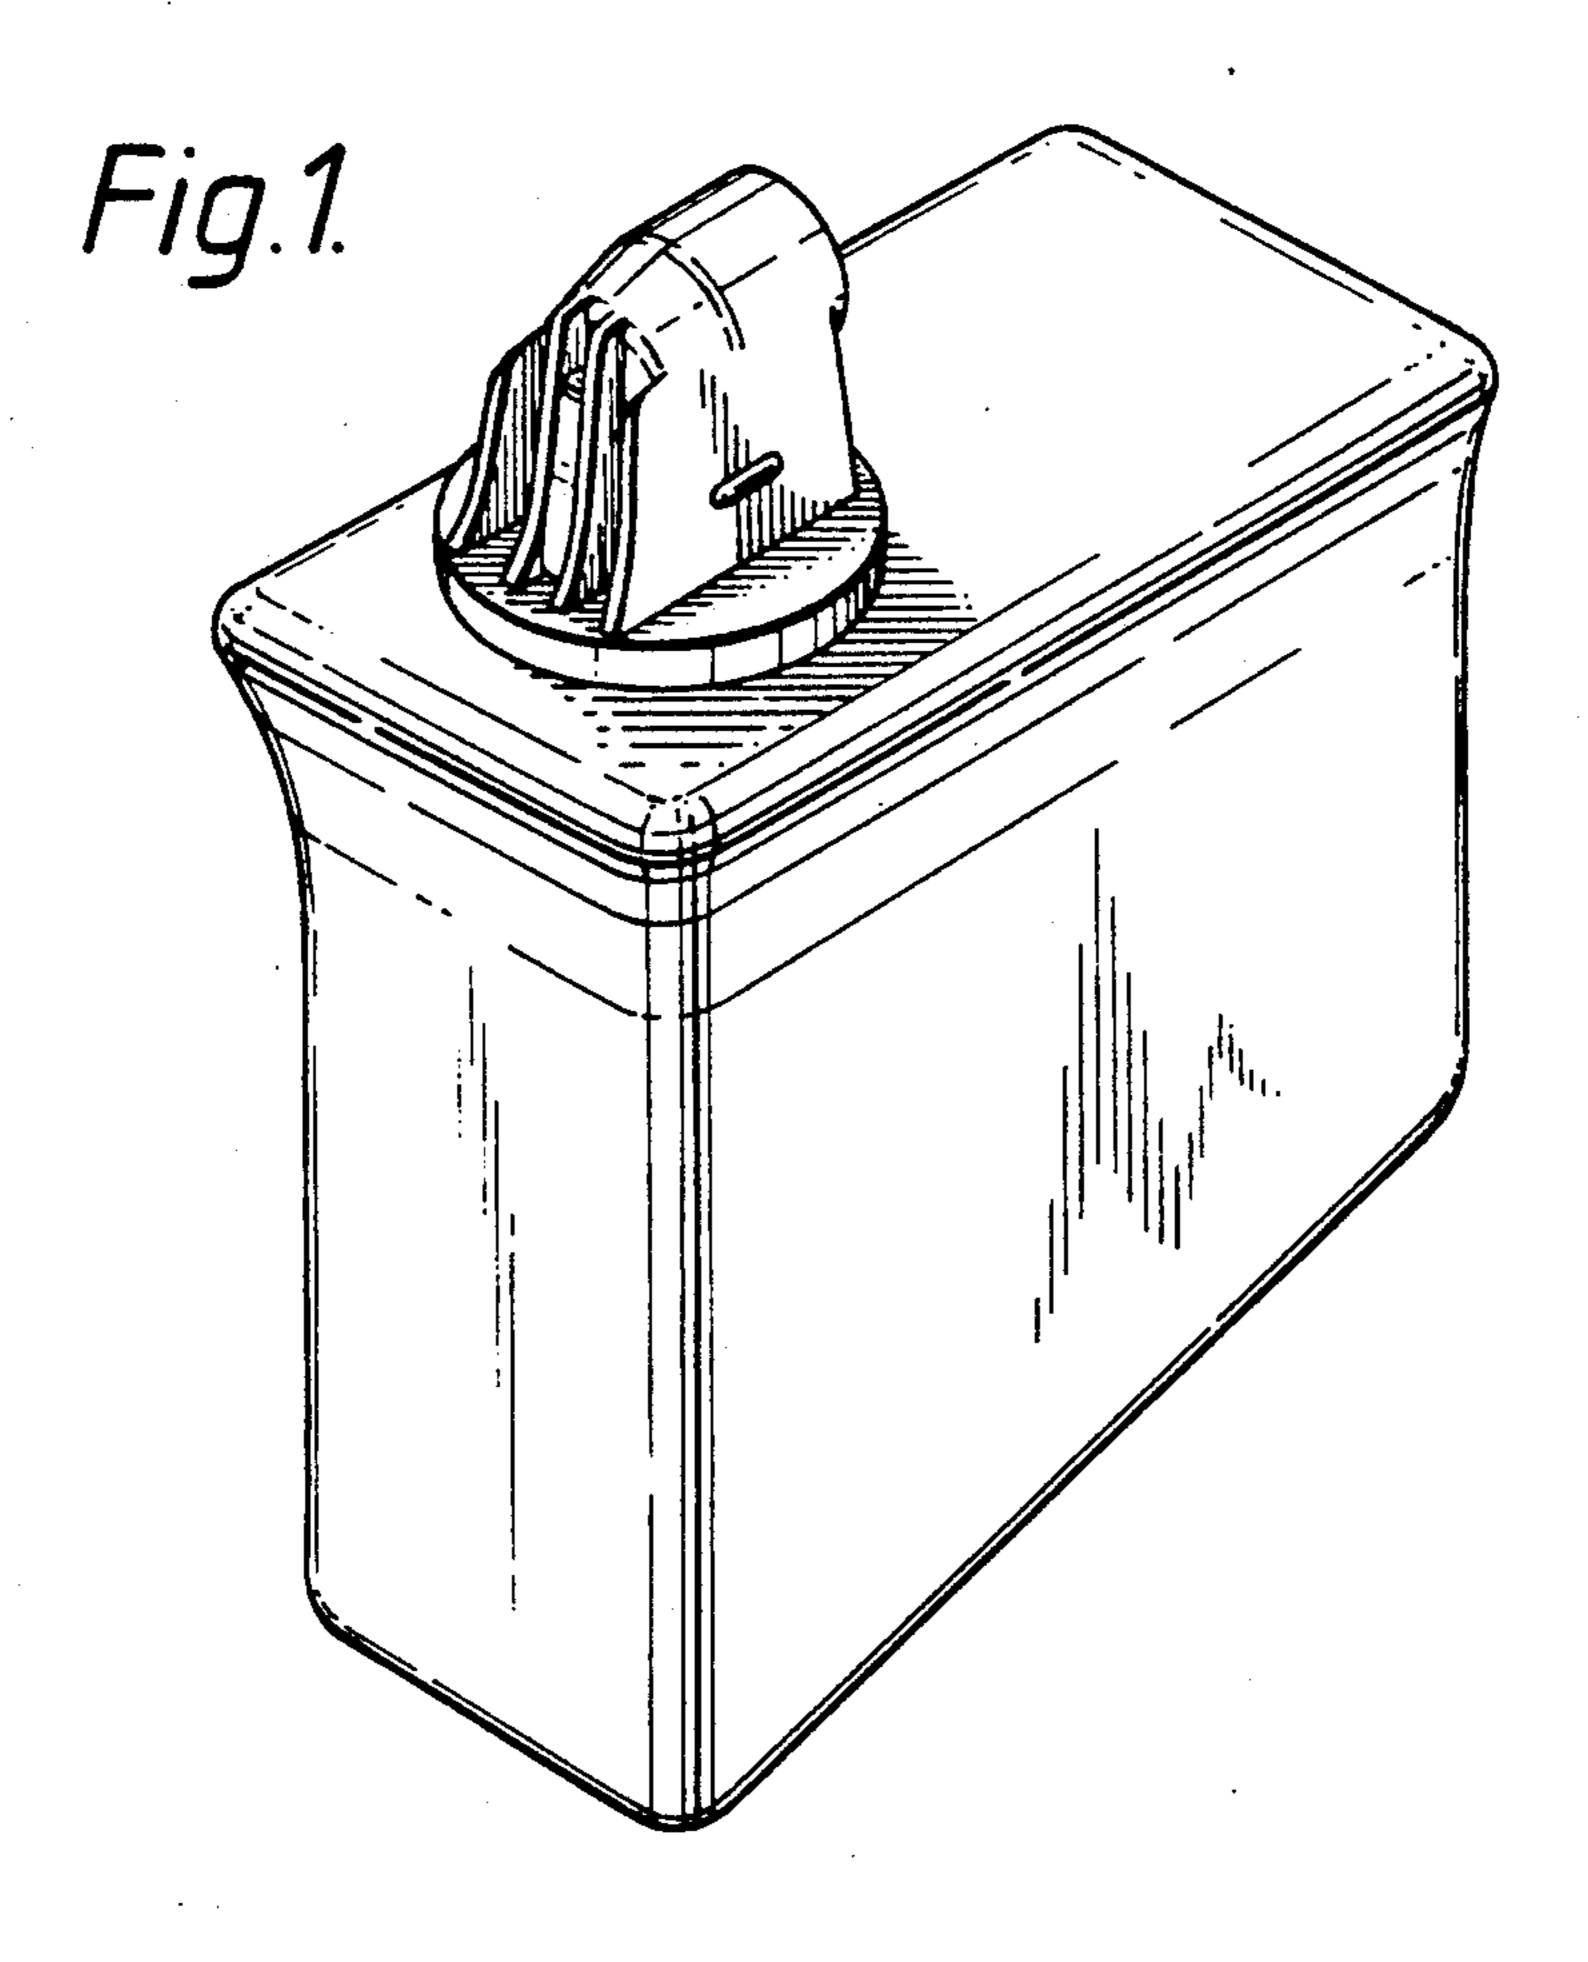

Apr. 7, 1992

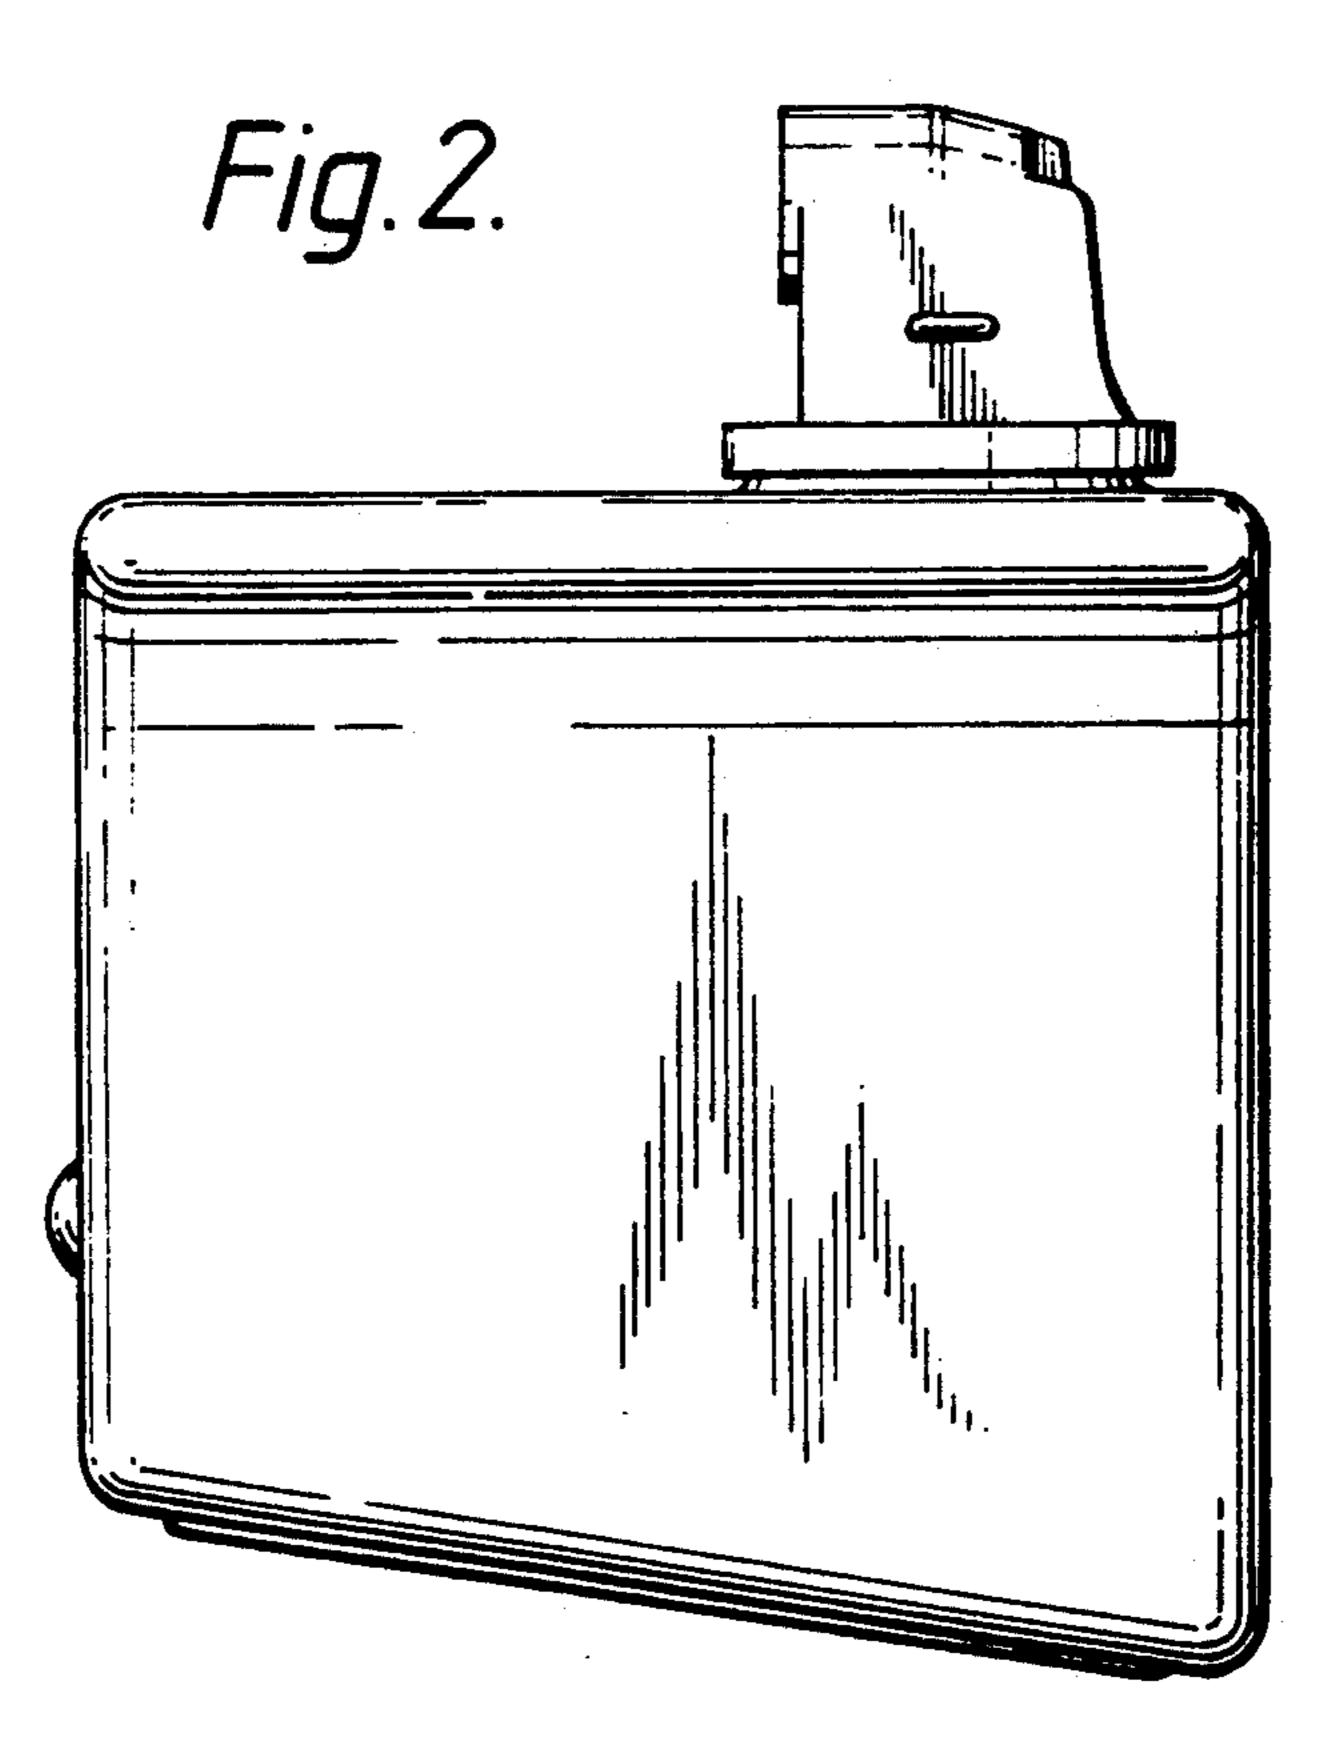


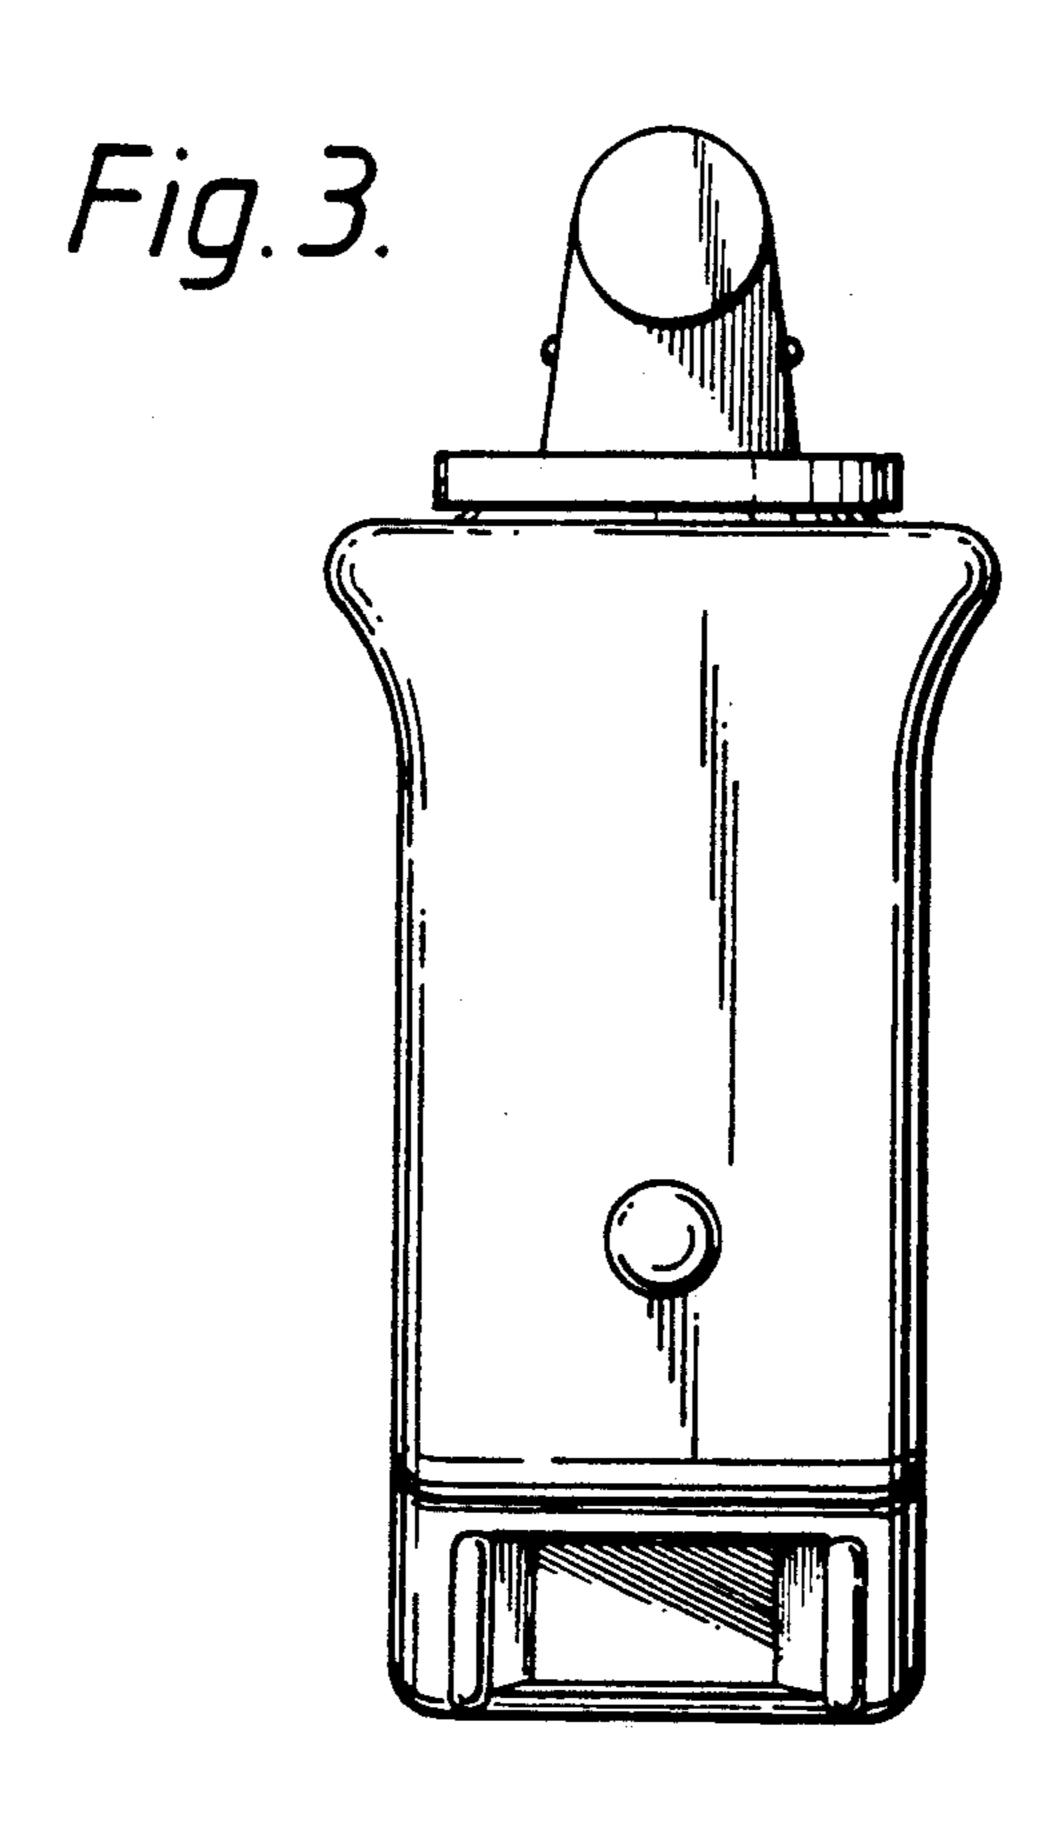


Fig. 4.

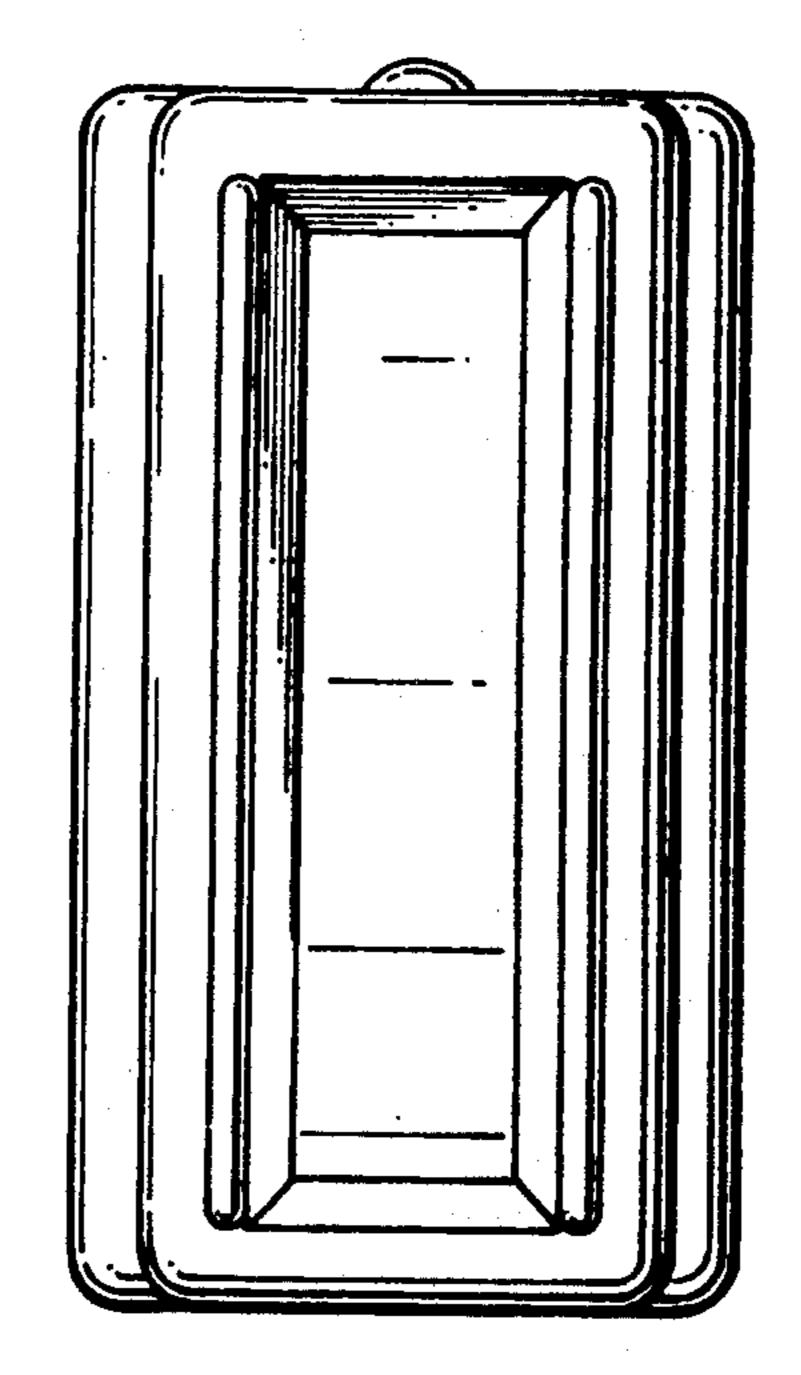

UNITED STATES PATENT AND TRADEMARK OFFICE CERTIFICATE OF CORRECTION

PATENT NO.: Des. 325,258

DATED : April 7, 1992

INVENTOR(S): J. Andersen et al.

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

On the title page: Item [57]:

In the Claim: delete "a container for waste expelled from a blood gas analyzer or the like," and read --container for liquid--.

Signed and Sealed this
Tenth Day of August, 1993

Attest:

MICHAEL K. KIRK

Attesting Officer

Acting Commissioner of Patents and Trademarks