



US00D332314S

United States Patent [19]

[11] Patent Number: **Des. 332,314**

Torai et al.

[45] Date of Patent: **** Jan. 5, 1993**

[54] **CLINICAL CHEMISTRY ANALYZER**

[75] Inventors: **Kazuki Torai, Kokubunji; Kazunori Hashimoto, Tachikawa; Isamu Takekoshi; Mitsuru Ohnuma, both of Tokyo; Hiroshi Satake, Katsuta, all of Japan**

[73] Assignee: **Hitachi, Ltd., Tokyo, Japan**

[**] Term: **14 Years**

[21] Appl. No.: **584,844**

[22] Filed: **Sep. 19, 1990**

[30] **Foreign Application Priority Data**

Jun. 27, 1990 [JP] Japan 2-21519

[52] U.S. Cl. **D24/231**

[58] Field of Search **D24/169, 232**

[56] **References Cited**

U.S. PATENT DOCUMENTS

- D. 281,310 11/1985 Hattori et al. D24/232 X
- D. 298,854 12/1988 Kame et al. D24/169 X
- D. 303,095 8/1989 Nagai et al. D24/232 X
- D. 307,398 4/1990 Umemoto et al. D24/232 X

- D. 319,307 8/1991 Sakagami et al. D24/232
- D. 320,073 9/1991 Sakagami et al. D24/232
- D. 320,443 10/1991 Yokoyama et al. D24/169 X
- 4,855,109 8/1989 Muraishi et al. 422/65 X
- 5,008,082 4/1991 Shaw 436/43

Primary Examiner—Stella Reid
Assistant Examiner—I. Simmons
Attorney, Agent, or Firm—Antonelli, Terry, Stout & Kraus

[57] **CLAIM**

The ornamental design for a clinical chemistry analyzer, as shown.

DESCRIPTION

FIG. 1 is a perspective view of a clinical chemistry analyzer showing our new design; FIG. 2 is a front elevational view thereof; FIG. 3 is a top plan view thereof; FIG. 4 is a right side elevational view thereof; FIG. 5 is a left side elevational view thereof; FIG. 6 is a rear elevational view thereof; FIG. 7 is a bottom plan view thereof; and, FIG. 8 is a perspective view thereof, with all covers in open condition.

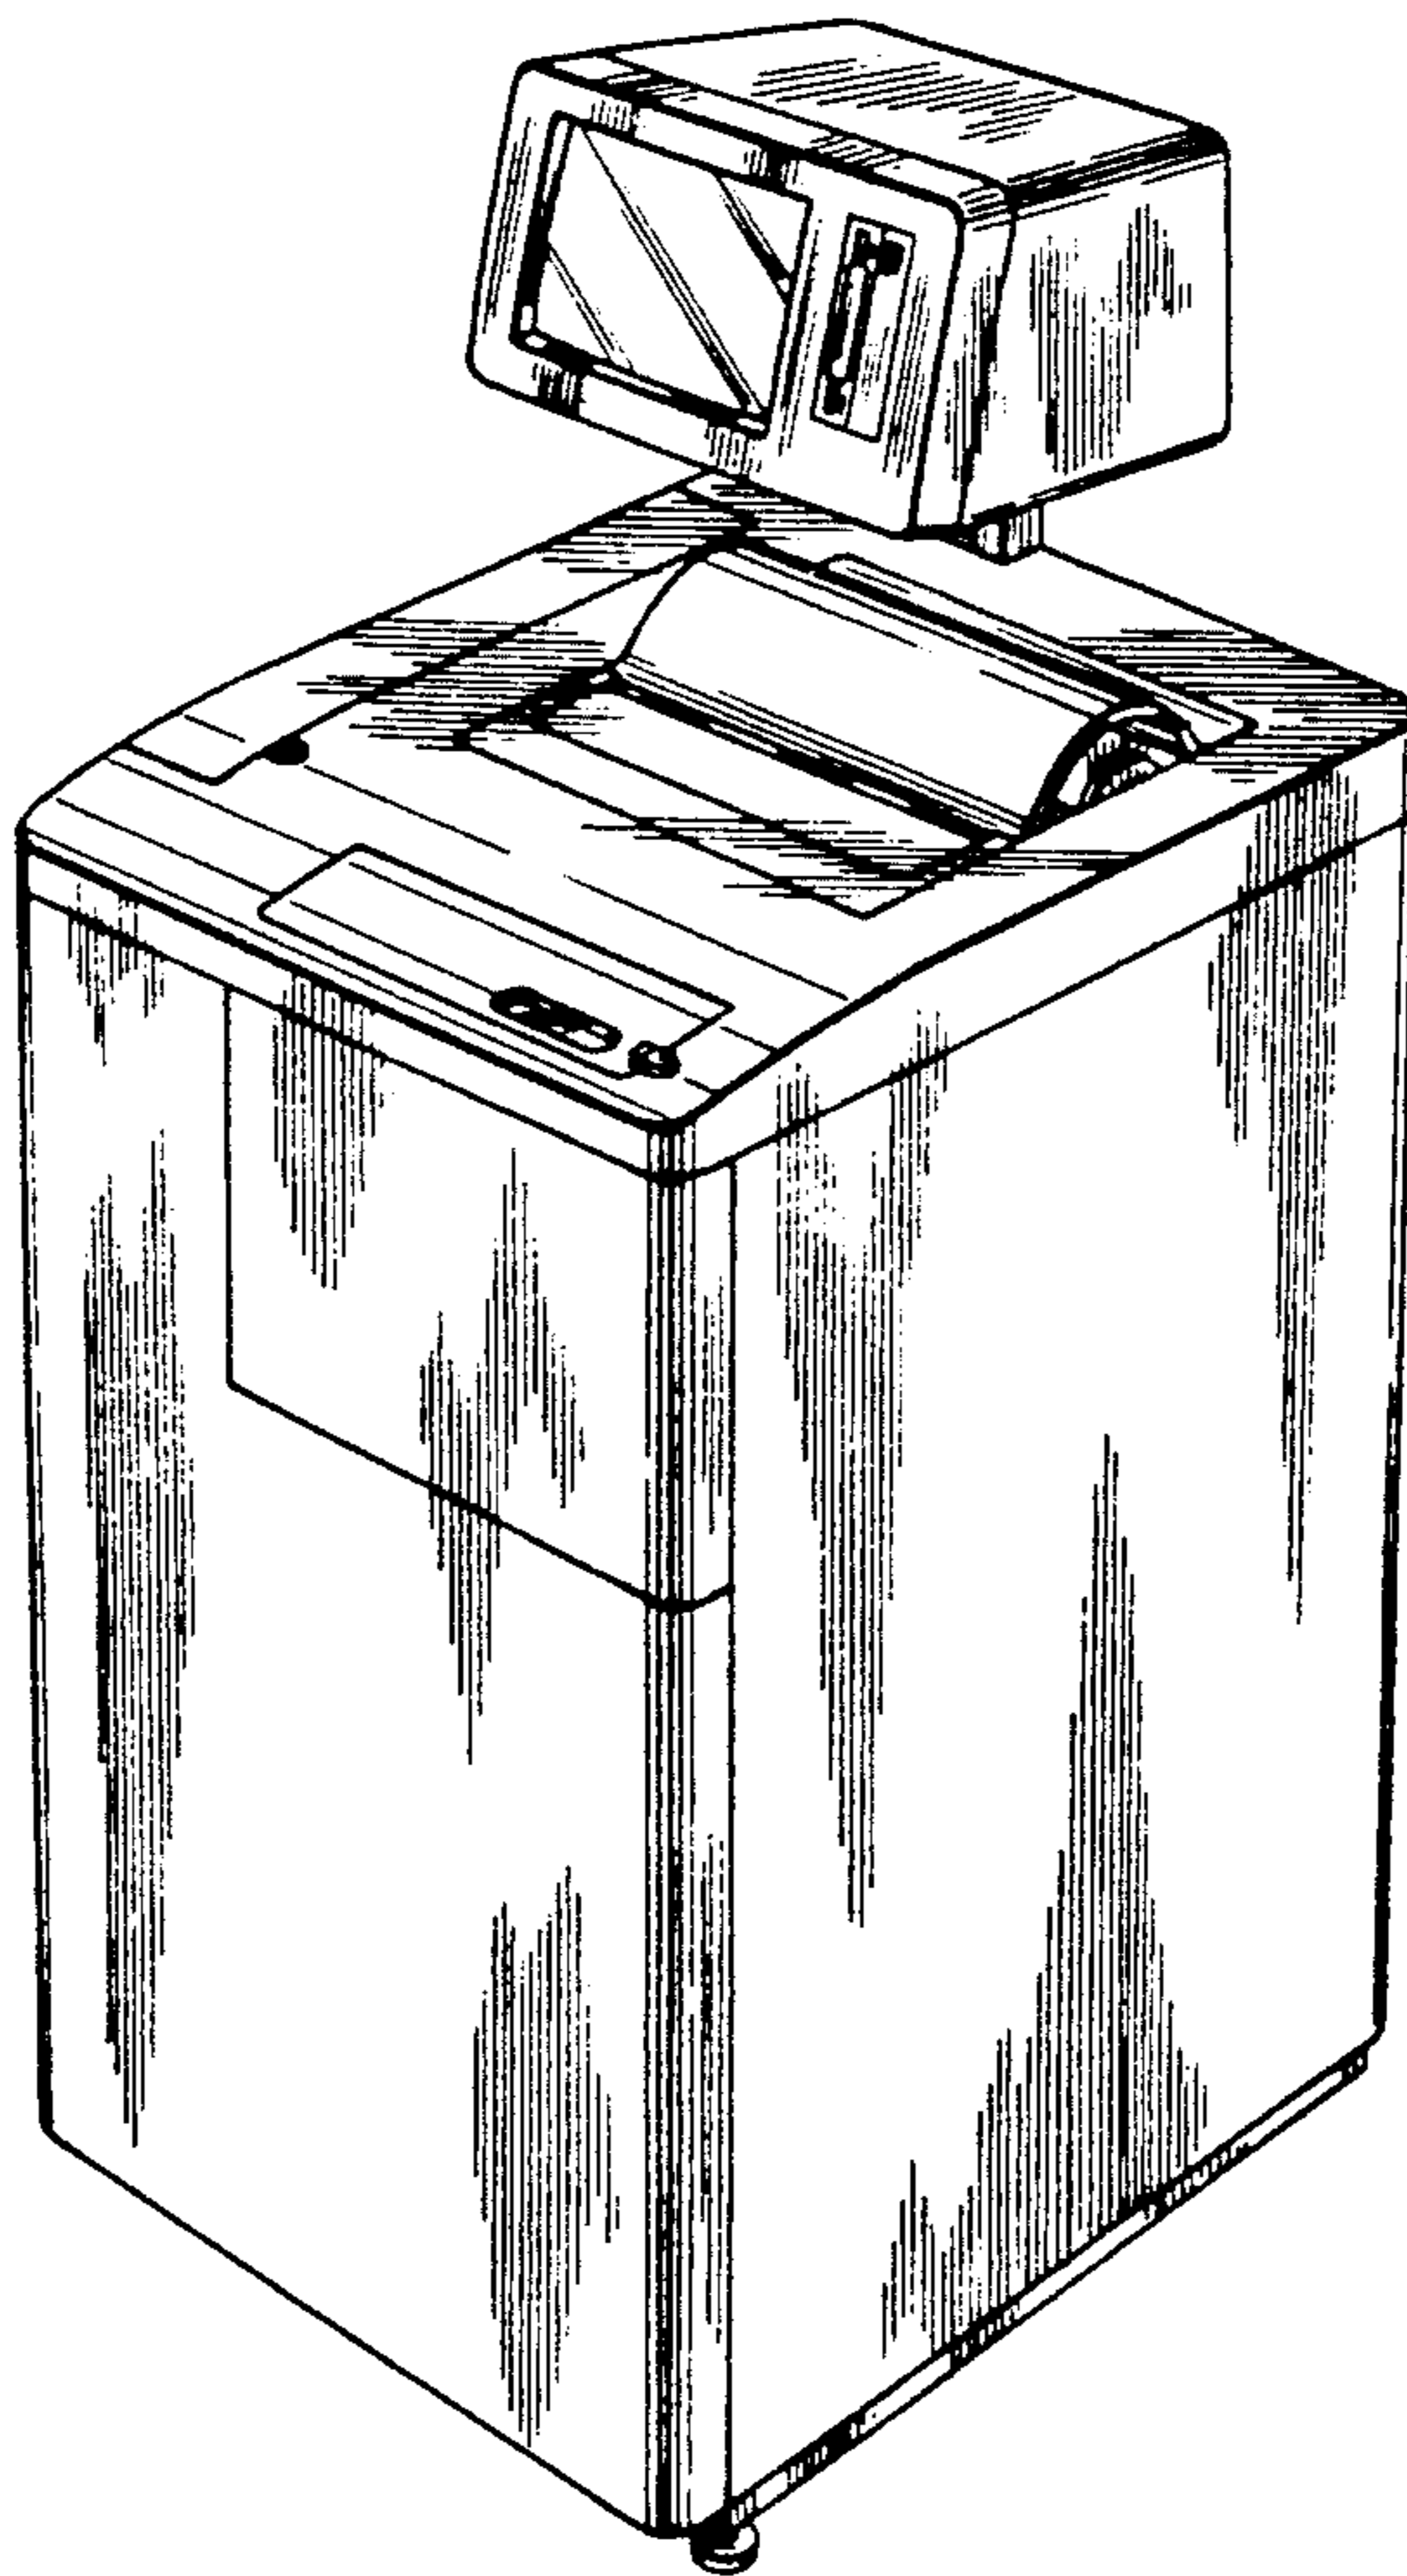


FIG. 1

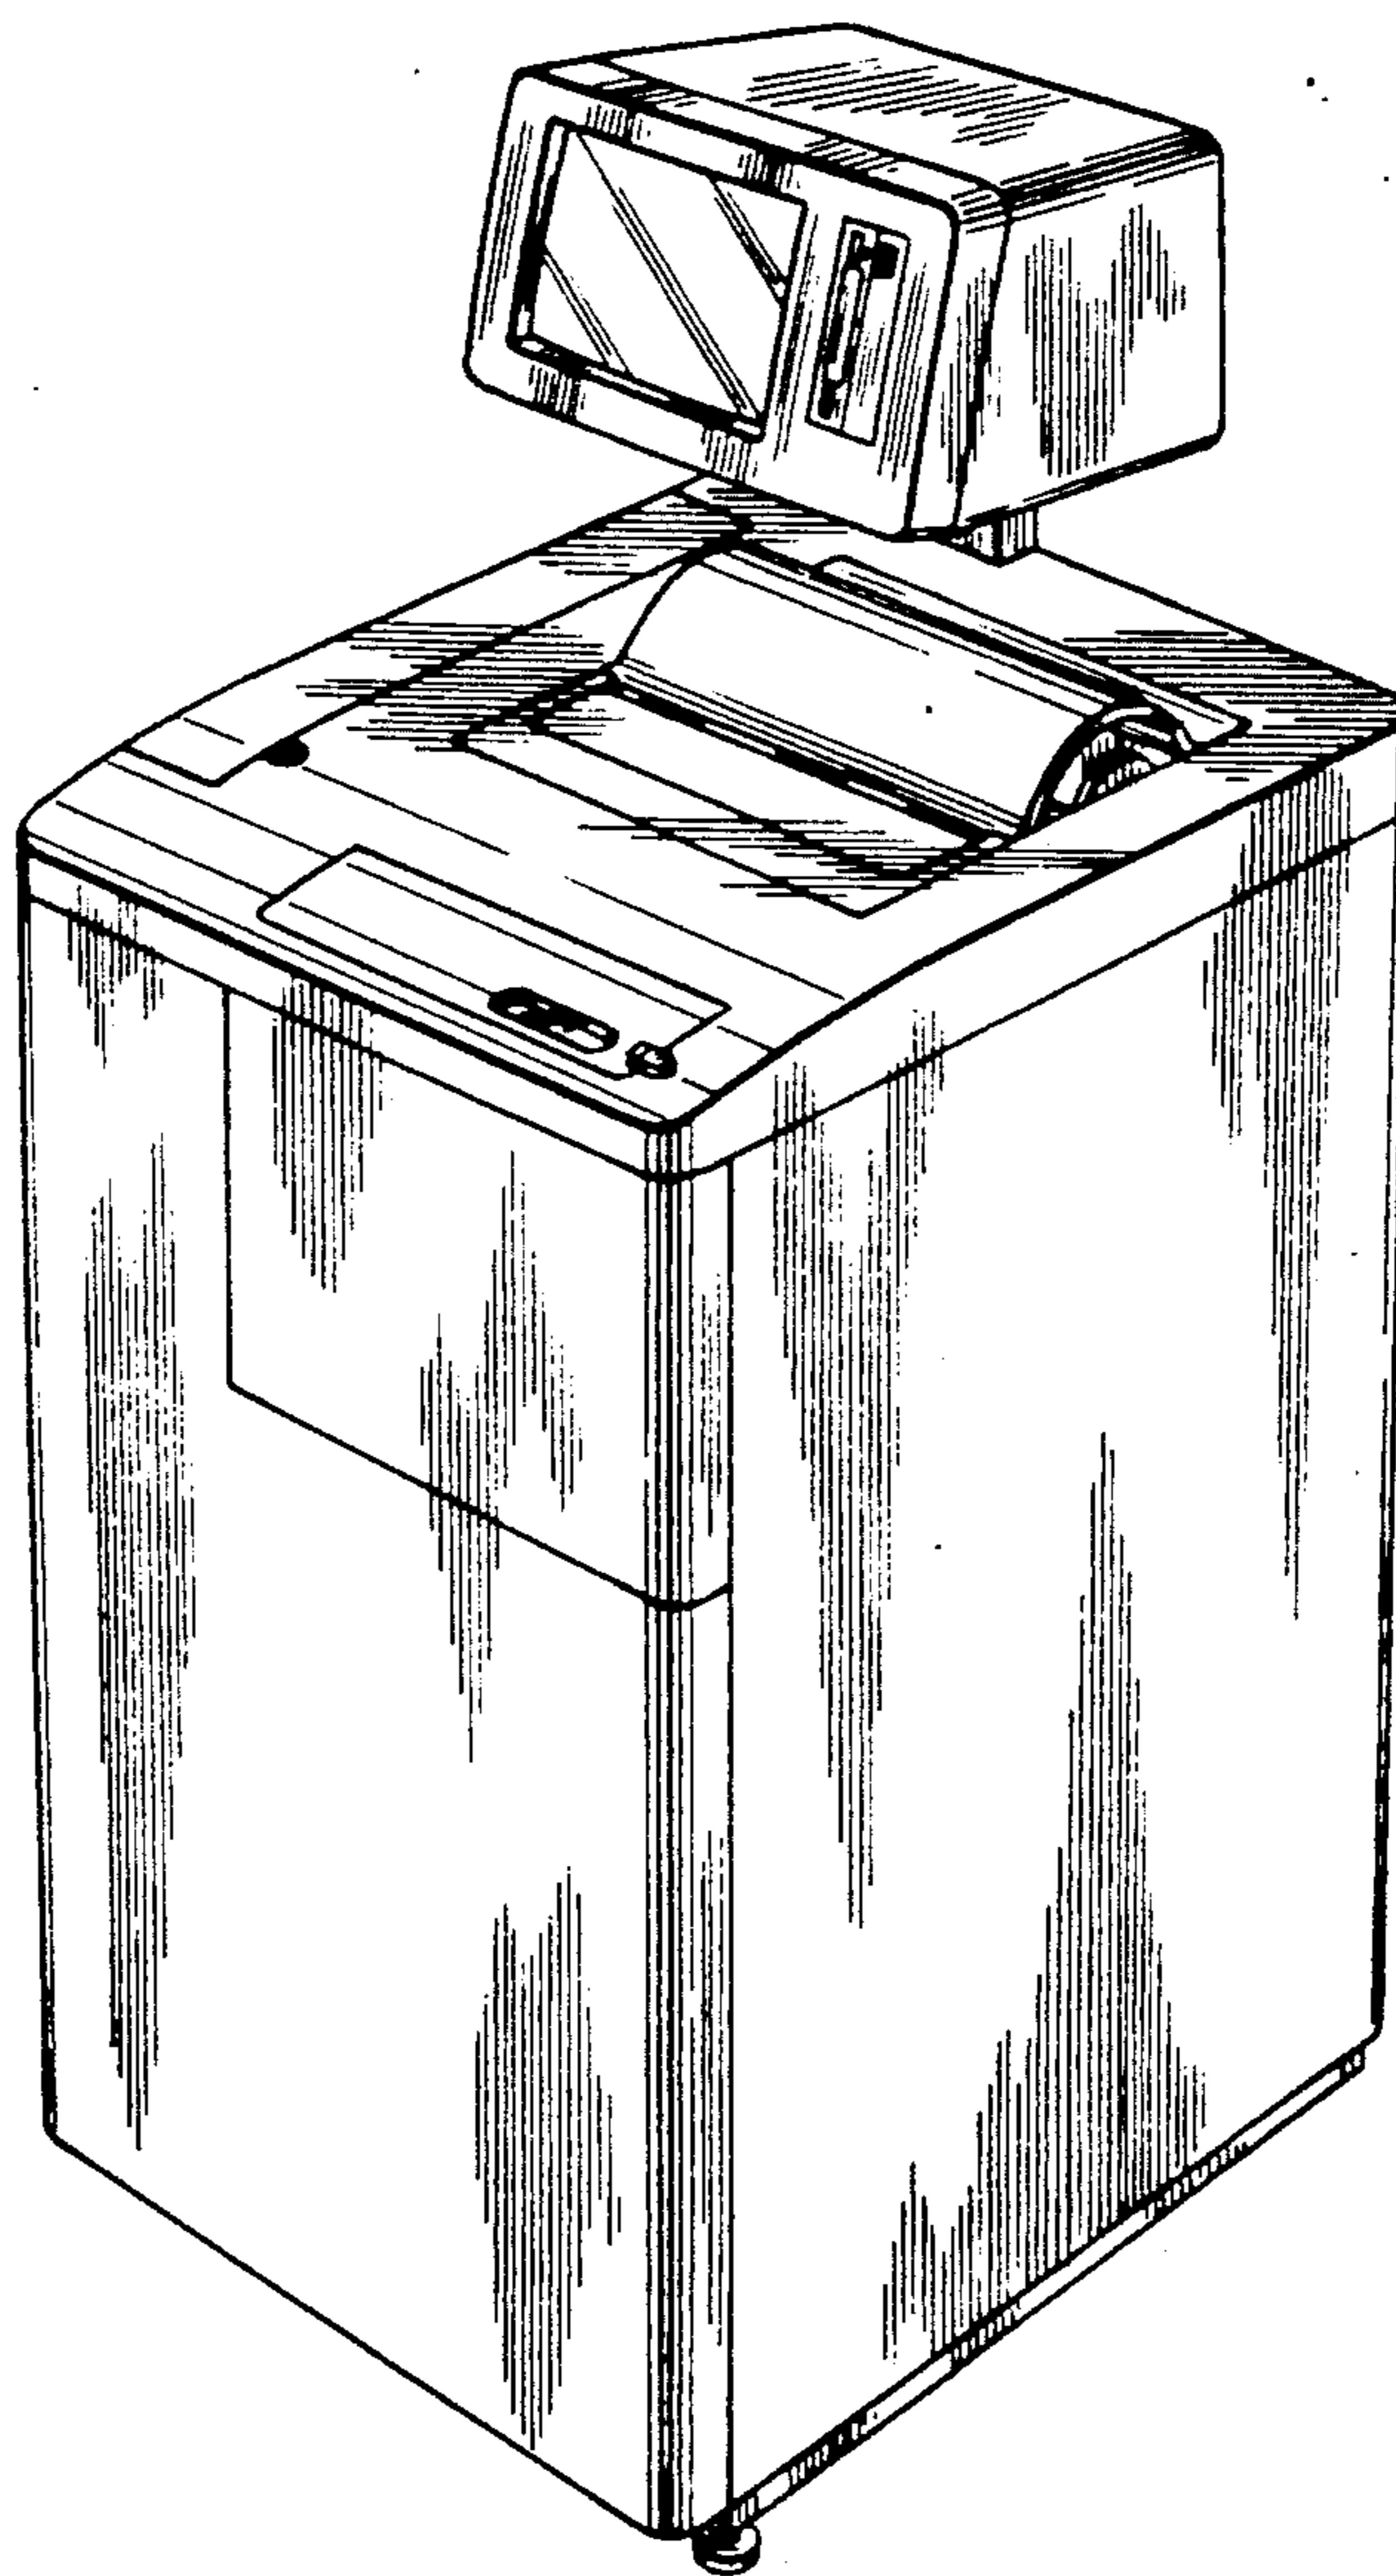


FIG. 2

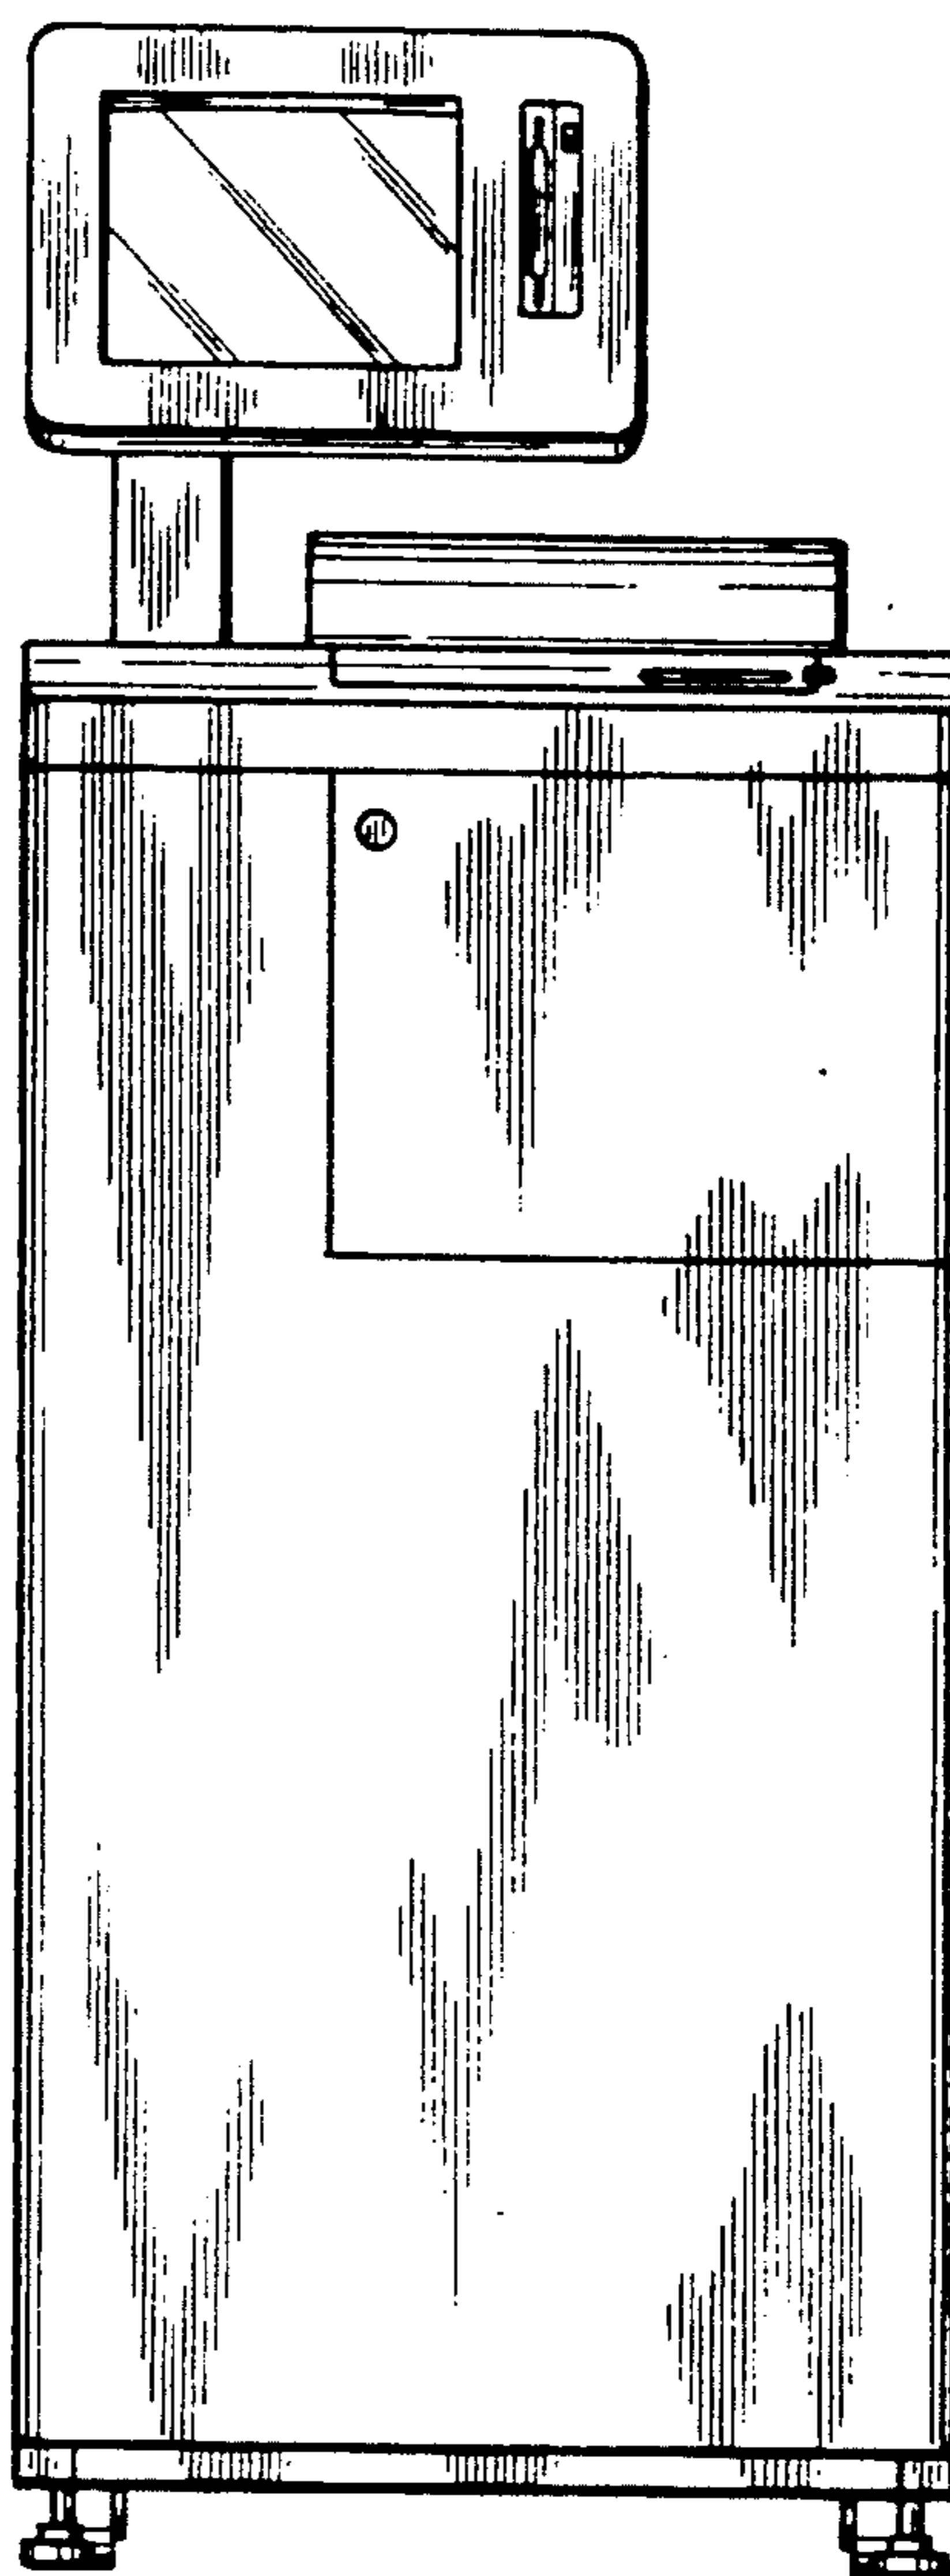


FIG. 3

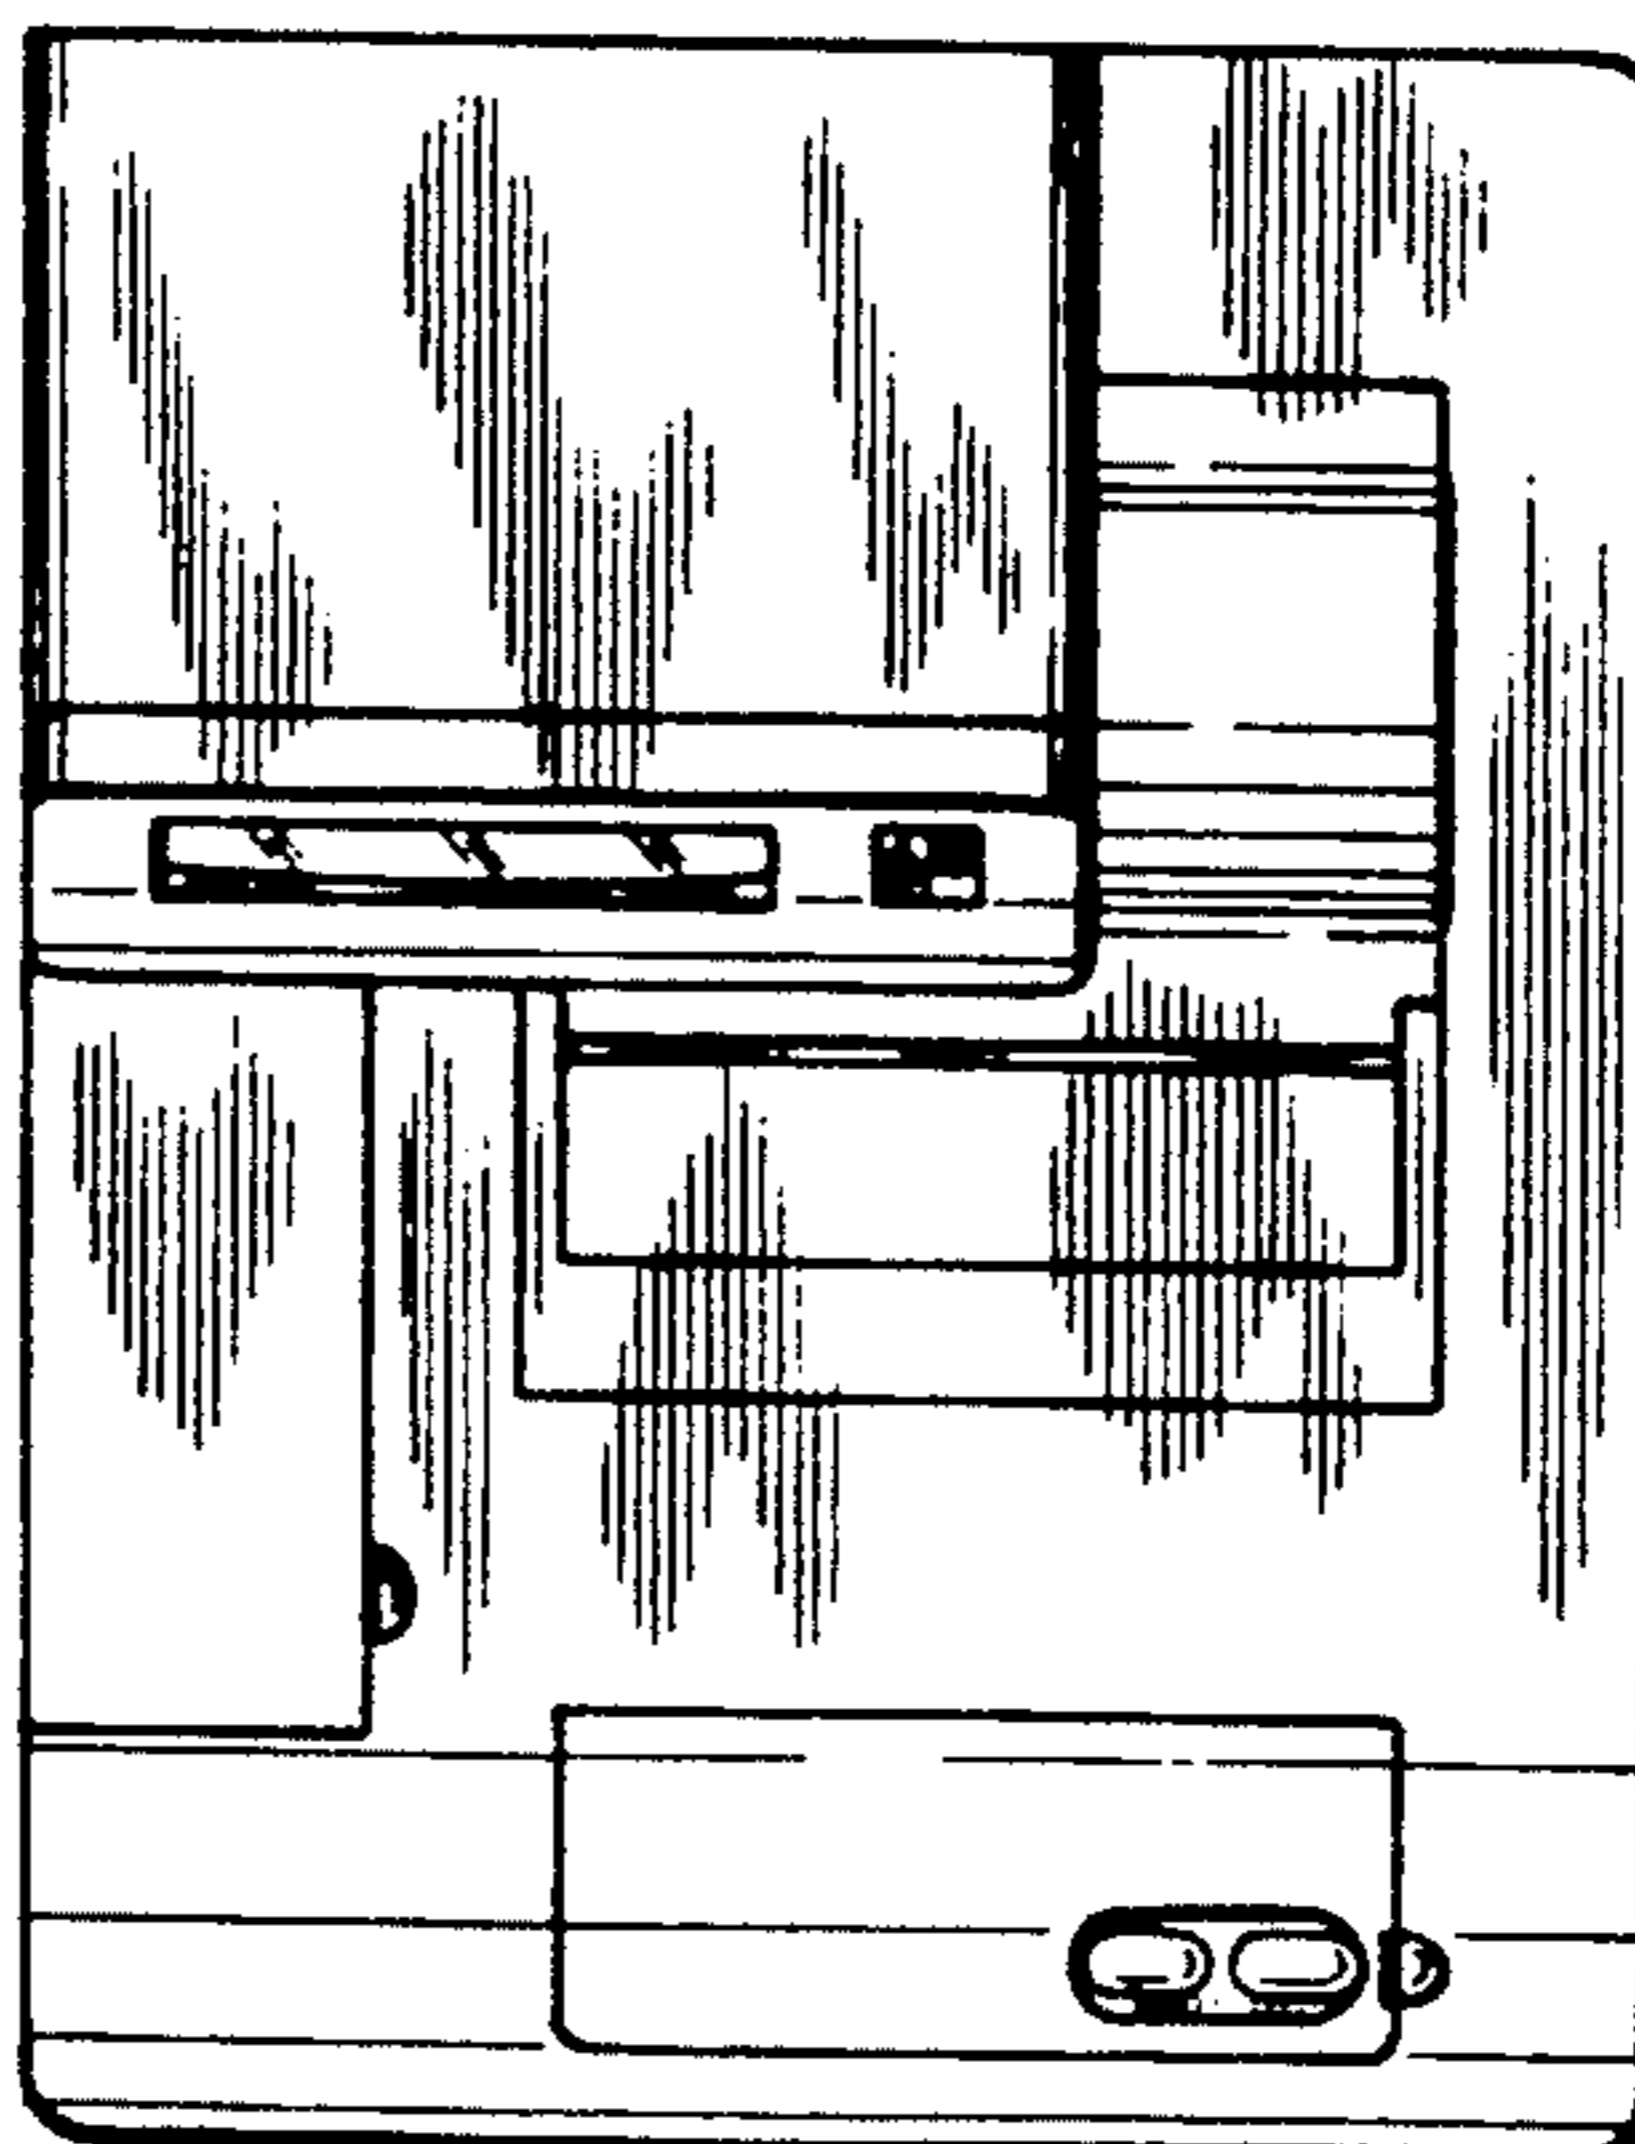


FIG. 4

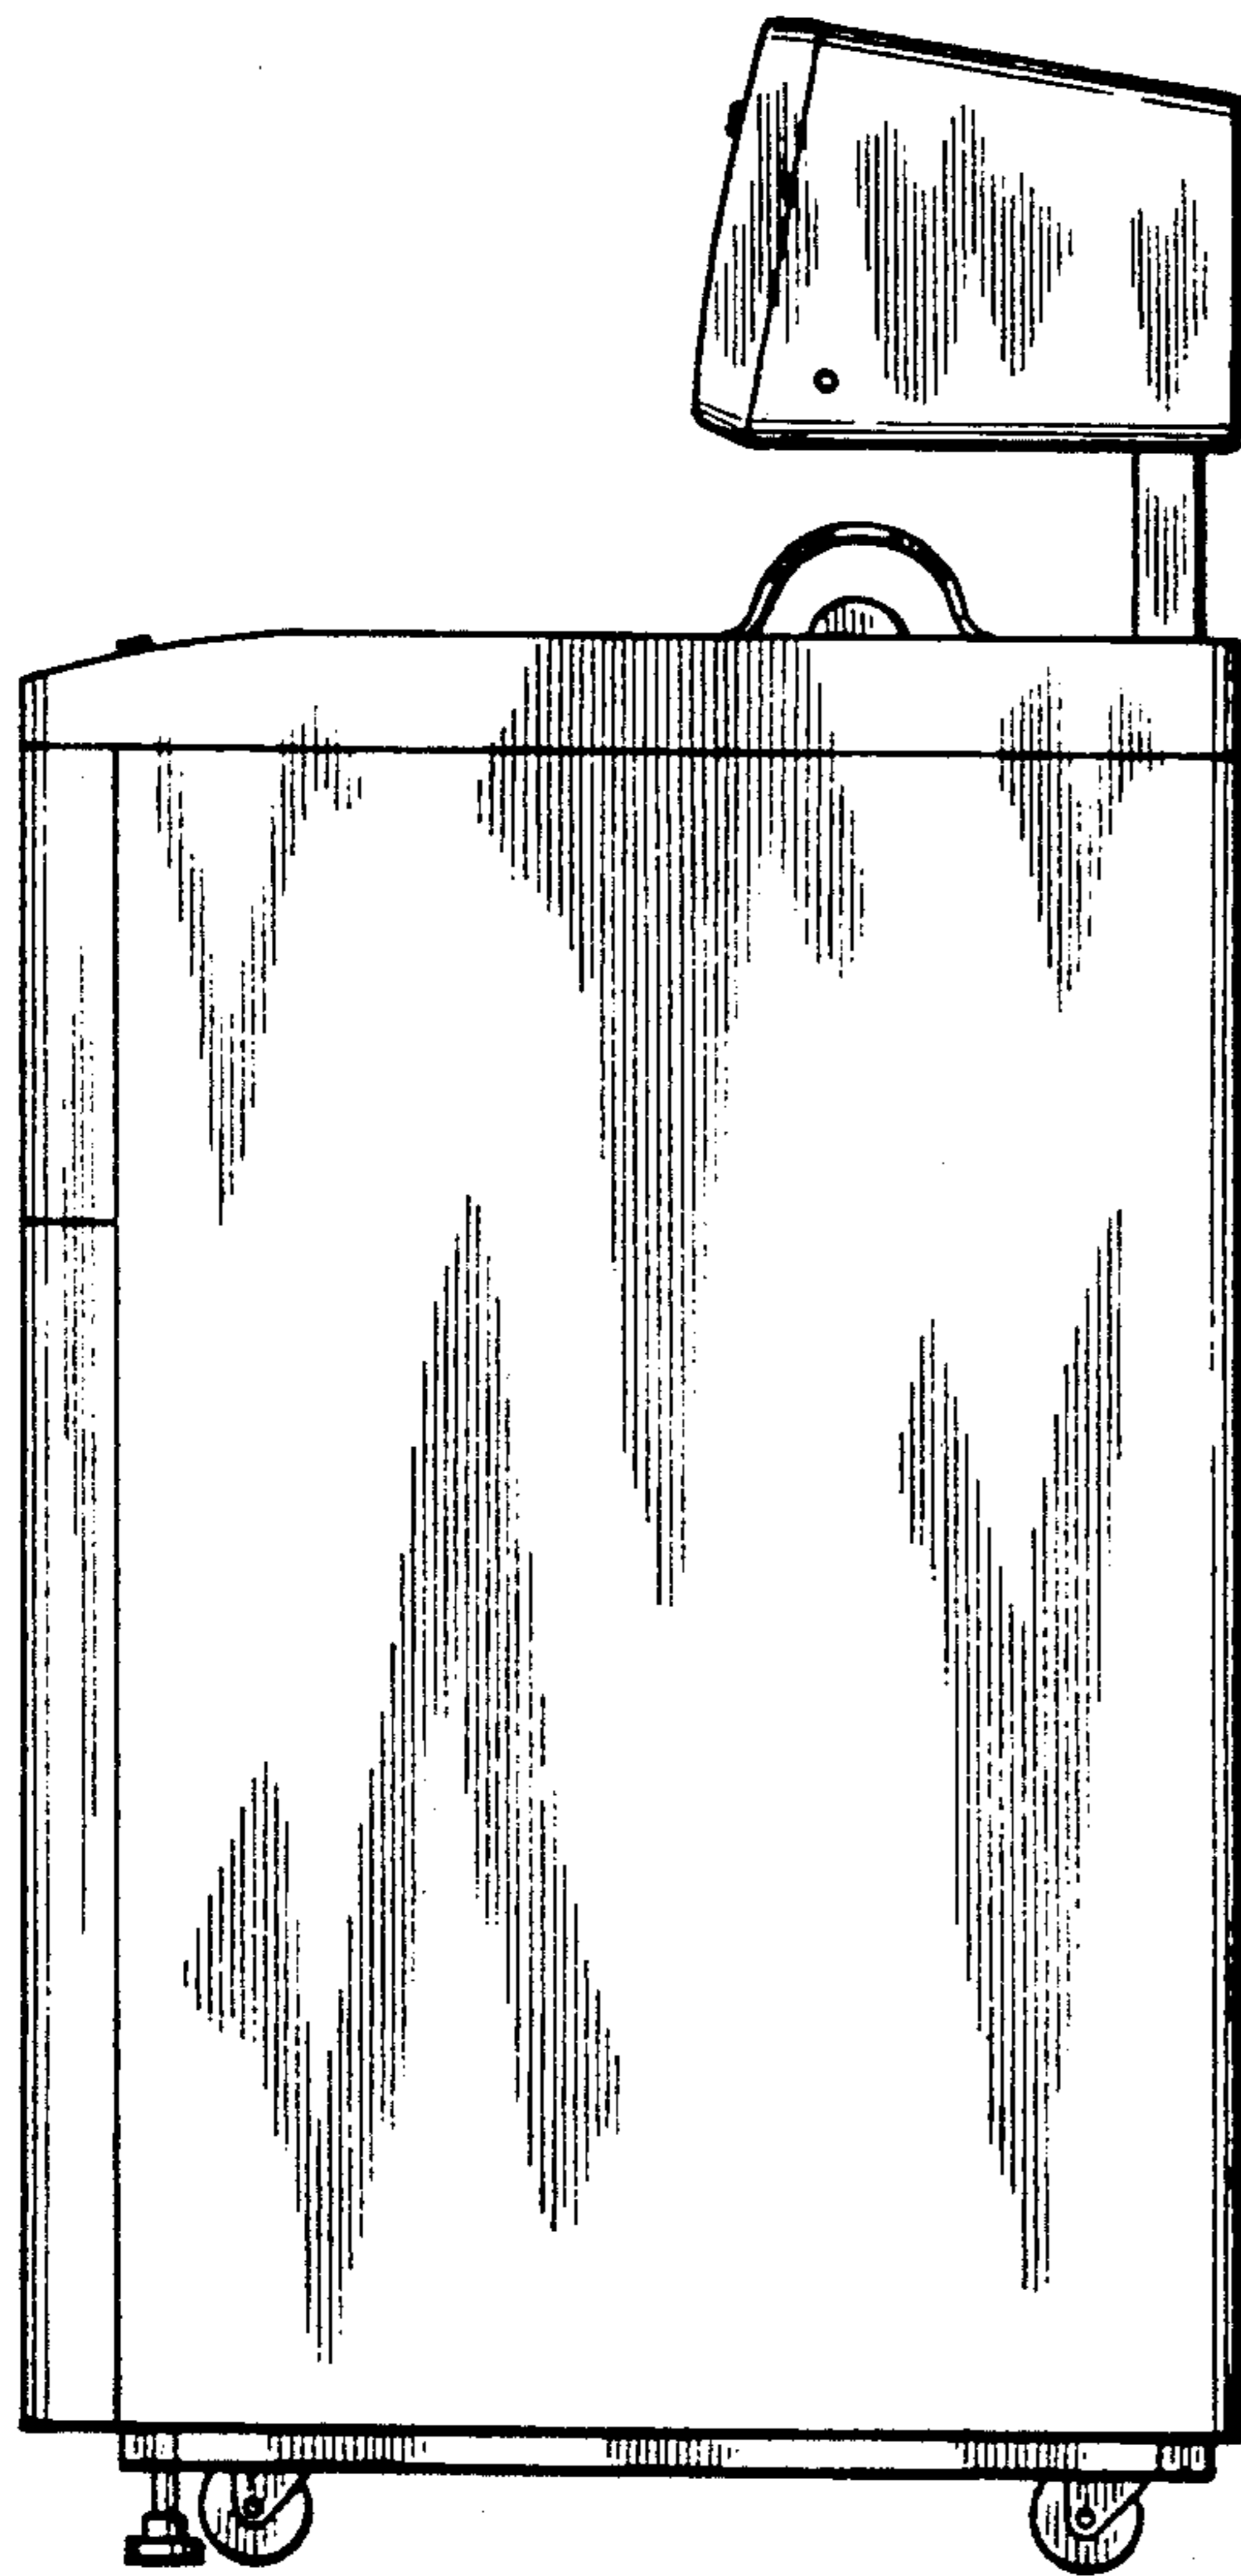


FIG. 5

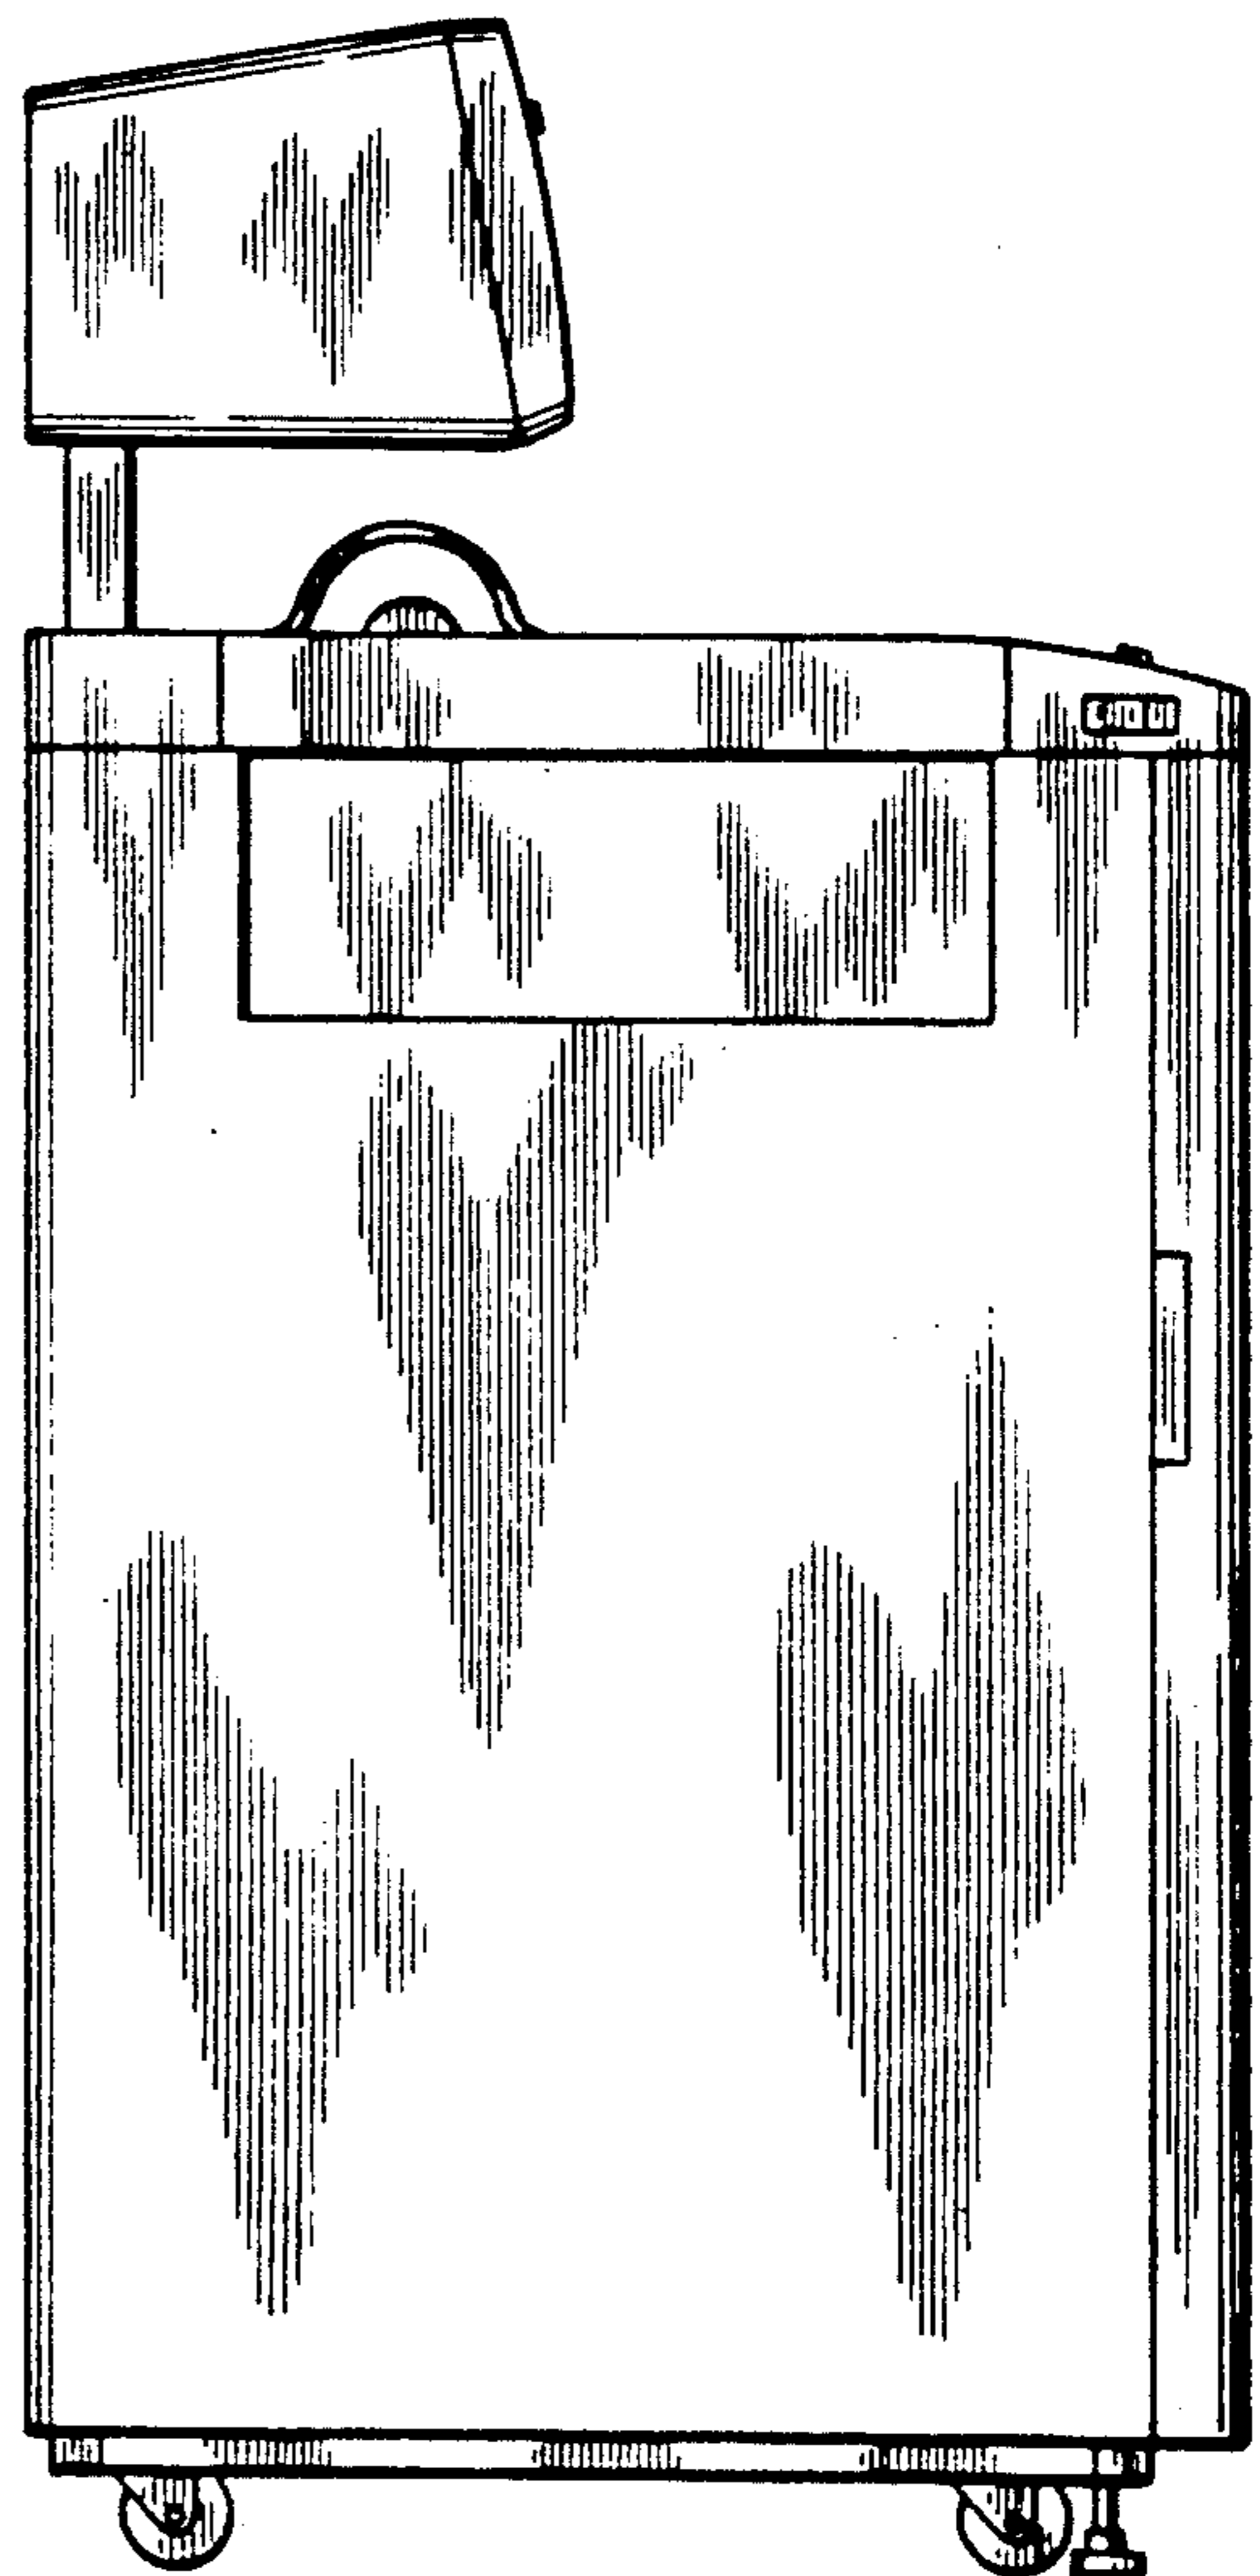


FIG. 6

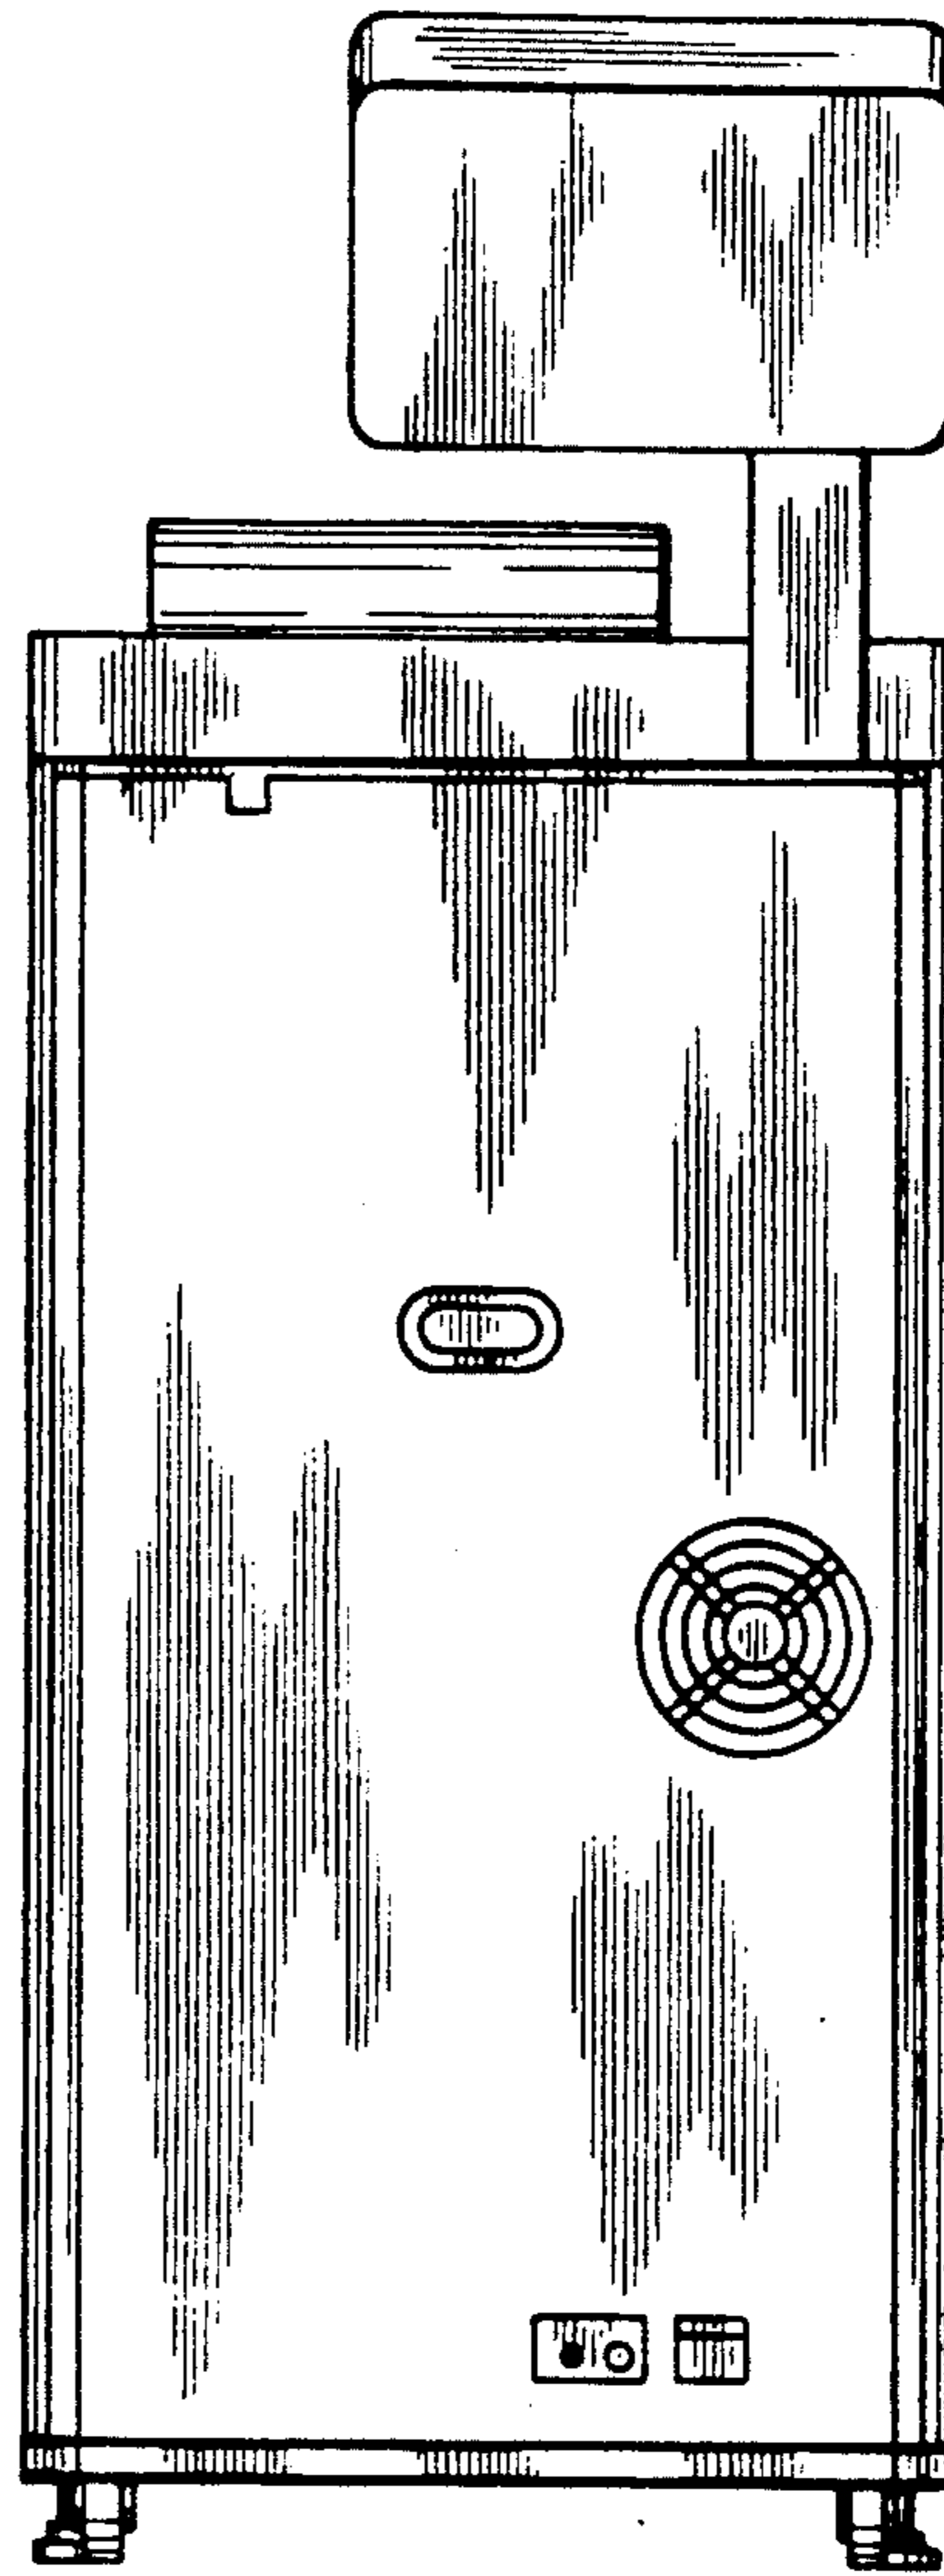


FIG. 7

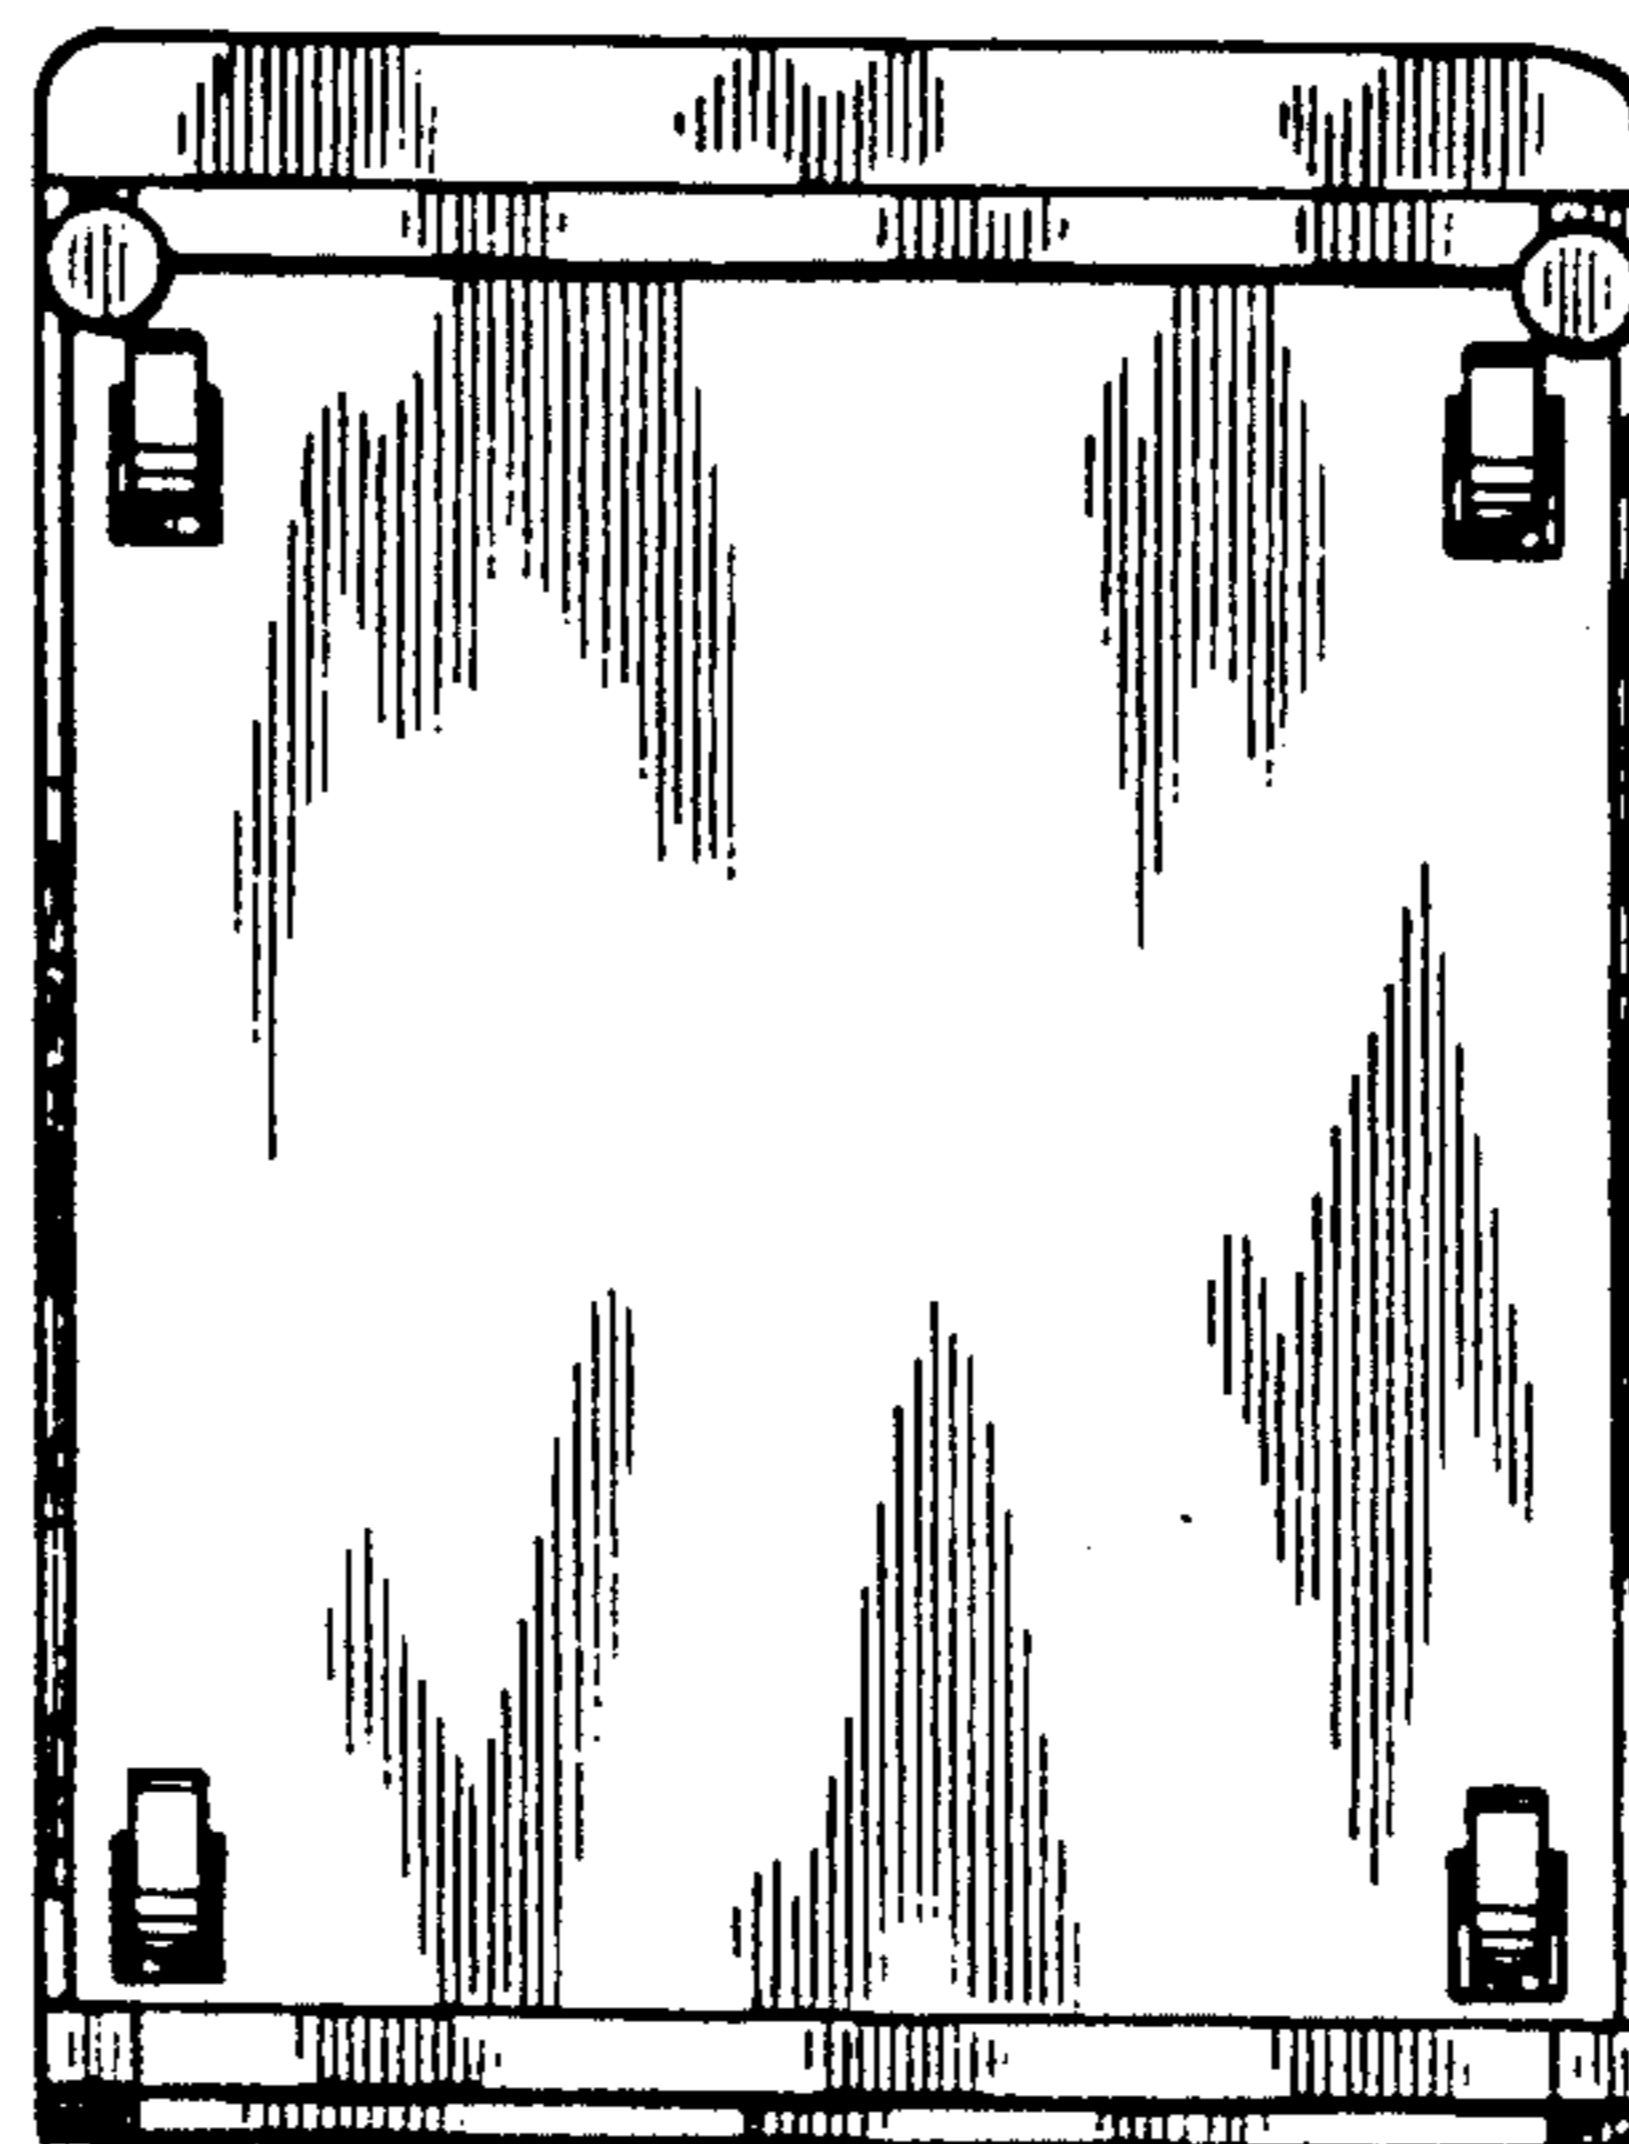


FIG. 8

