



US00D333004S

United States Patent [19]

McNamee et al.

[11] Patent Number: Des. 333,004

[45] Date of Patent: ** Feb. 2, 1993

[54] **VENTILATORY INSTRUMENT FOR MEASURING PEAK EXPIRATORY FLOW**

[75] Inventors: **George A. McNamee, Saffron Walden; James A. Stockwell; Ronald F. Checksfield, both of London, all of England**

[73] Assignee: **Ferraris Development and Engineering Company Limited, London, England**

[**] Term: **14 Years**

[21] Appl. No.: **589,891**

[22] Filed: **Sep. 28, 1990**

[30] **Foreign Application Priority Data**

Mar. 29, 1990 [GB] United Kingdom 2005774
[52] U.S. Cl. **D24/164**
[58] Field of Search **D24/164, 186; 73/239, 73/861.74, 861.77; 128/719, 721, 725, 727; 482/13**

[56] **References Cited**

U.S. PATENT DOCUMENTS

D. 325,634 4/1992 Sweeney, Jr. D24/164
2,892,348 6/1959 Ekstrom, Jr. 73/228
3,367,324 2/1968 De Bono D24/164 X
3,857,277 12/1974 Moore 73/28

3,946,726 3/1976 Pikul 128/725
3,955,415 5/1976 Sharon 73/228
4,041,935 8/1977 Garbe 128/2.08
4,638,812 1/1987 Häkkinen 128/726
4,787,627 11/1988 Daubenspeck 482/13
5,137,026 8/1992 Waterson et al. 128/725

FOREIGN PATENT DOCUMENTS

8906275 8/1977 Fed. Rep. of Germany .
WO84/02642 8/1984 PCT Int'l Appl. .
WO89/02065 8/1989 PCT Int'l Appl. .


Primary Examiner—Alan P. Douglas
Assistant Examiner—Antoine D. Davis
Attorney, Agent, or Firm—Nixon & Vanderhye

[57] **CLAIM**

The ornamental design for a ventilatory instrument for measuring peak expiratory flow, as shown and described.

DESCRIPTION

FIG. 1 is a front elevational view of a ventilatory instrument for measuring peak expiratory flow showing our new design;
FIG. 2 is a rear elevational view thereof;
FIG. 3 is a right side elevational view thereof, the left side elevational view being a mirror image;
FIG. 4 is a top plan view thereof; and,
FIG. 5 is a bottom plan view thereof.

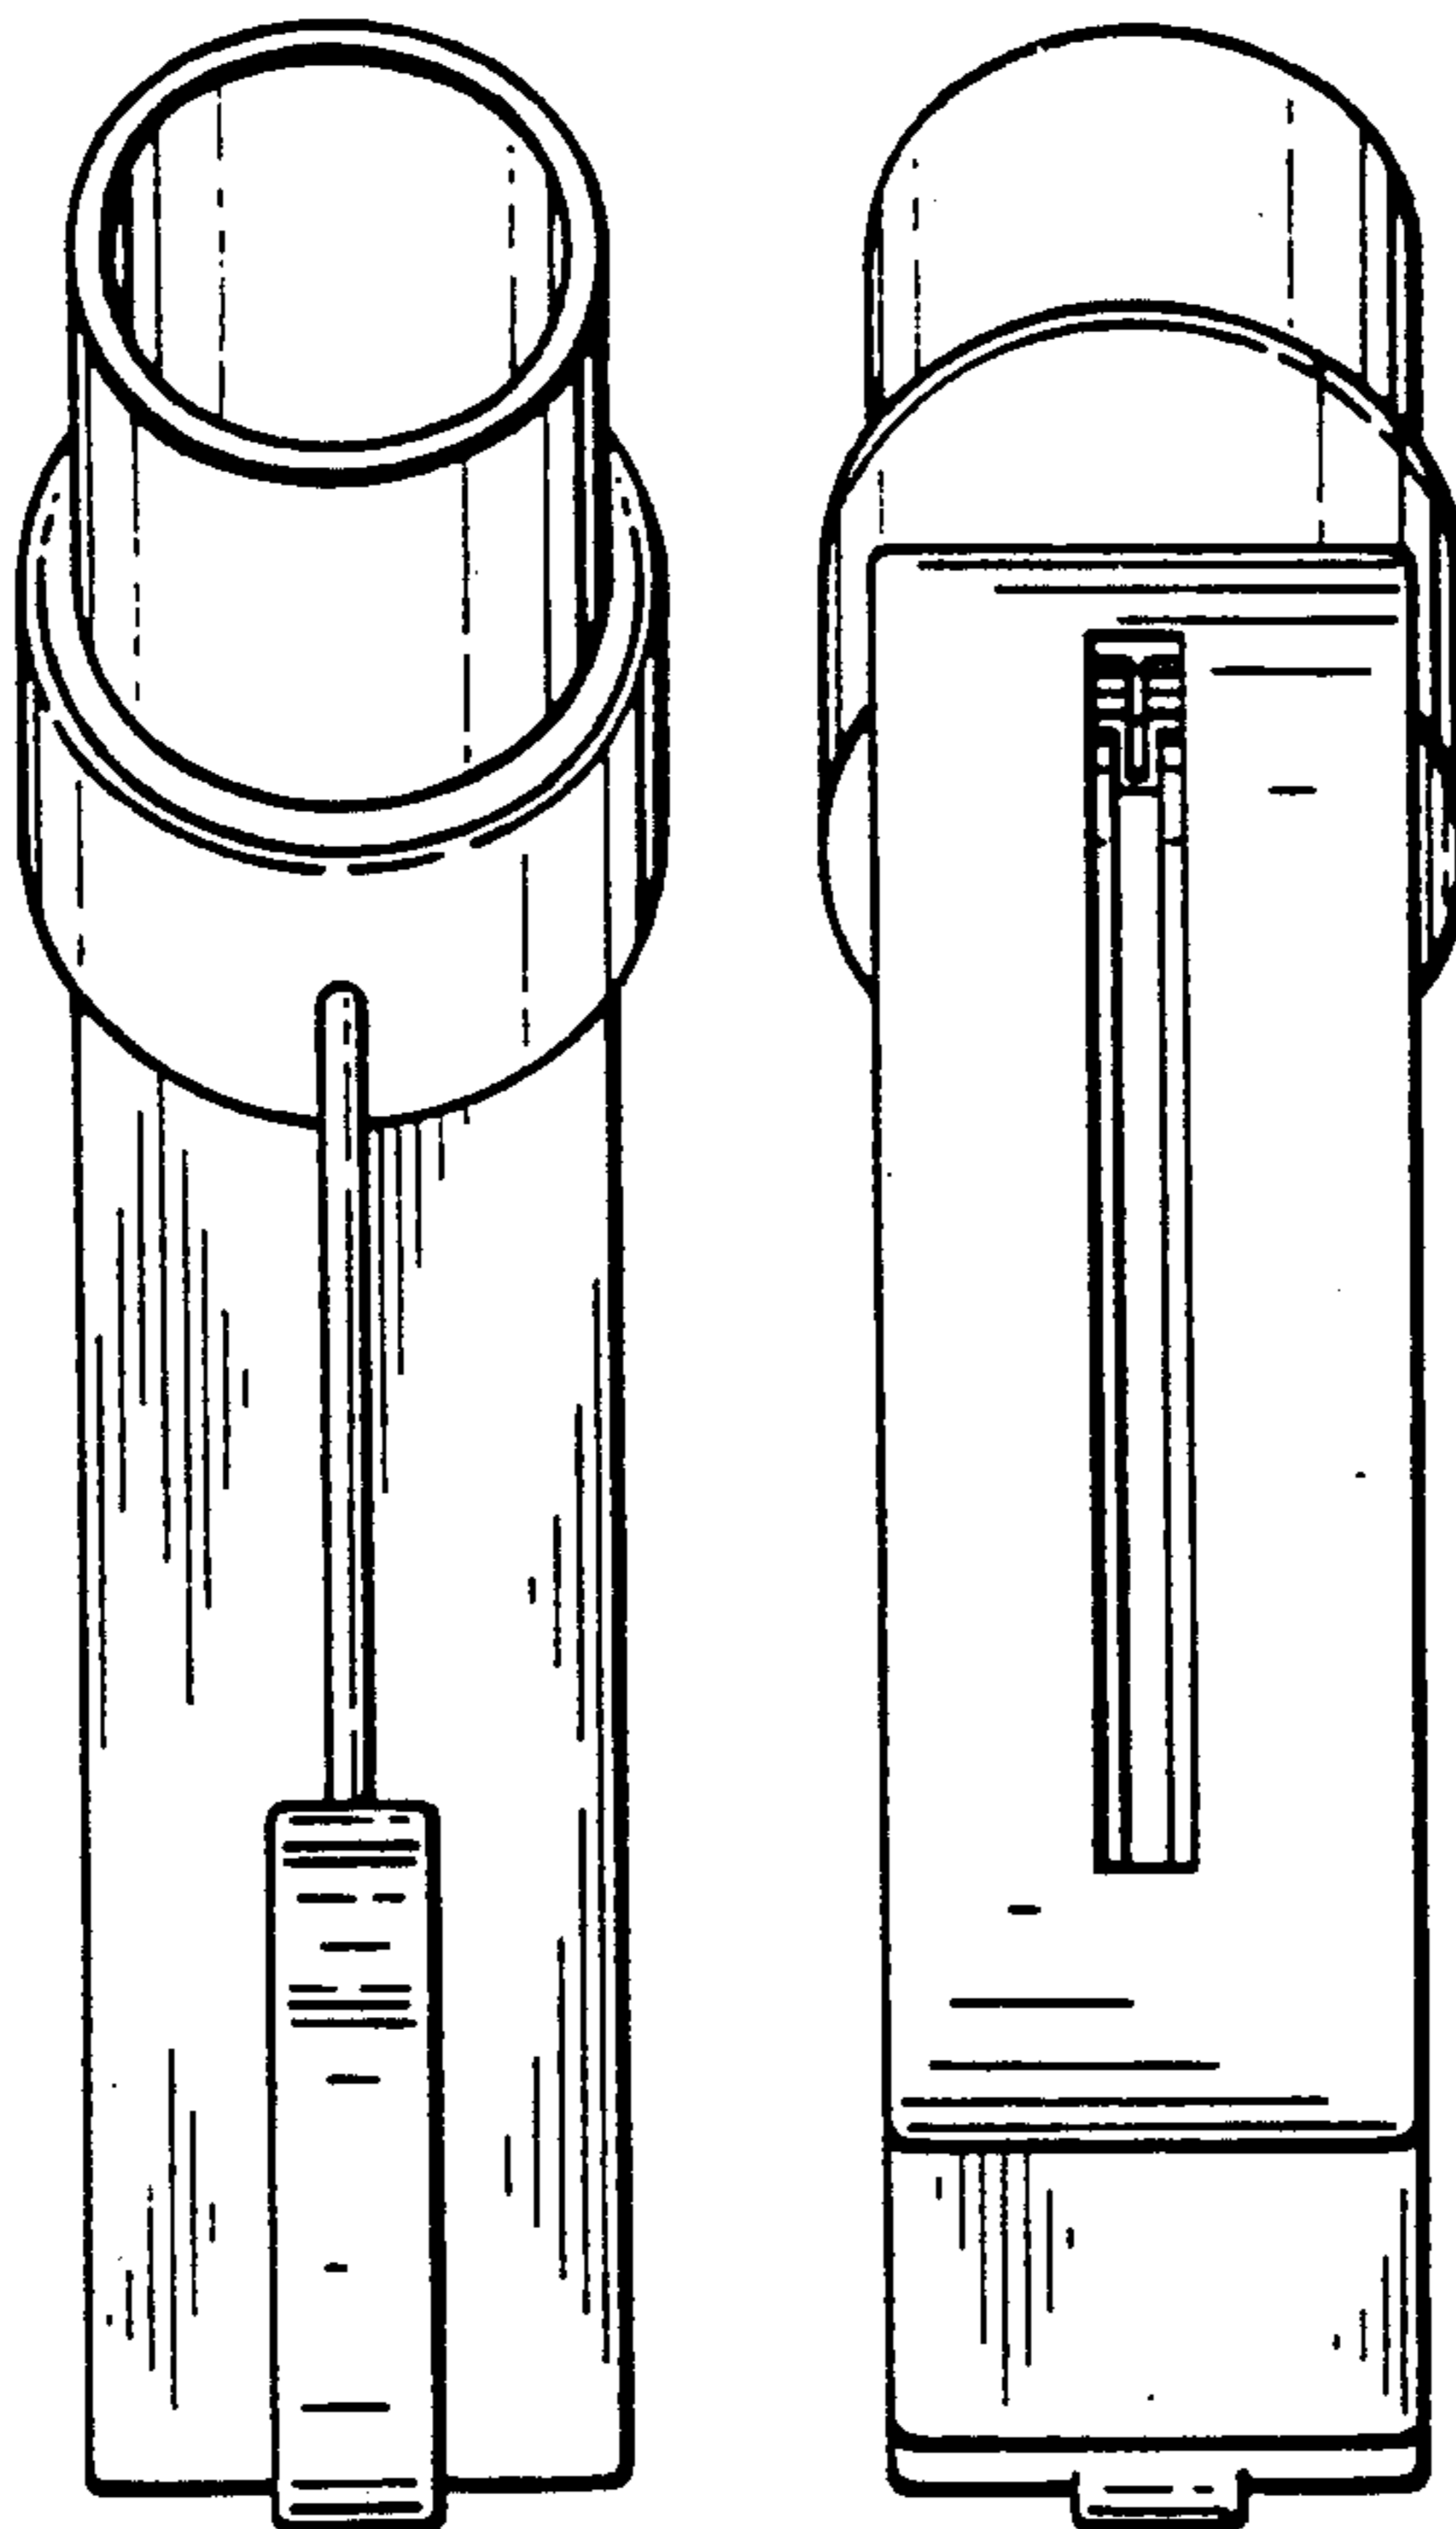

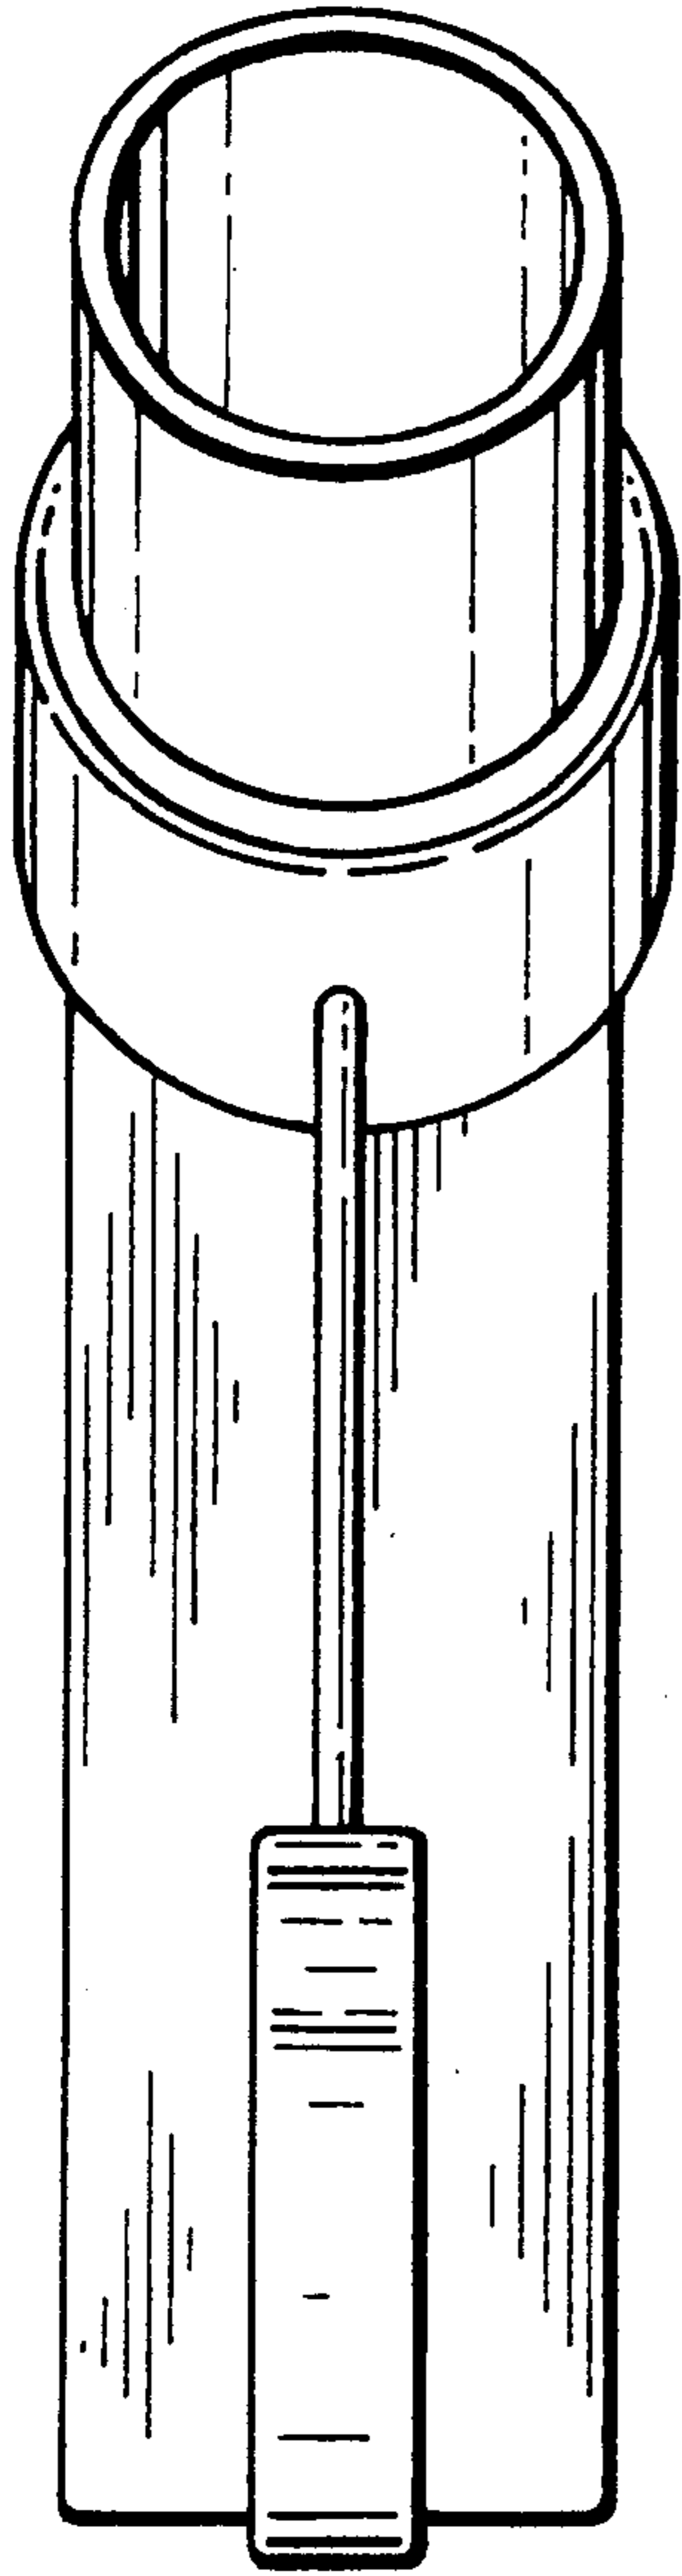


FIG. 1

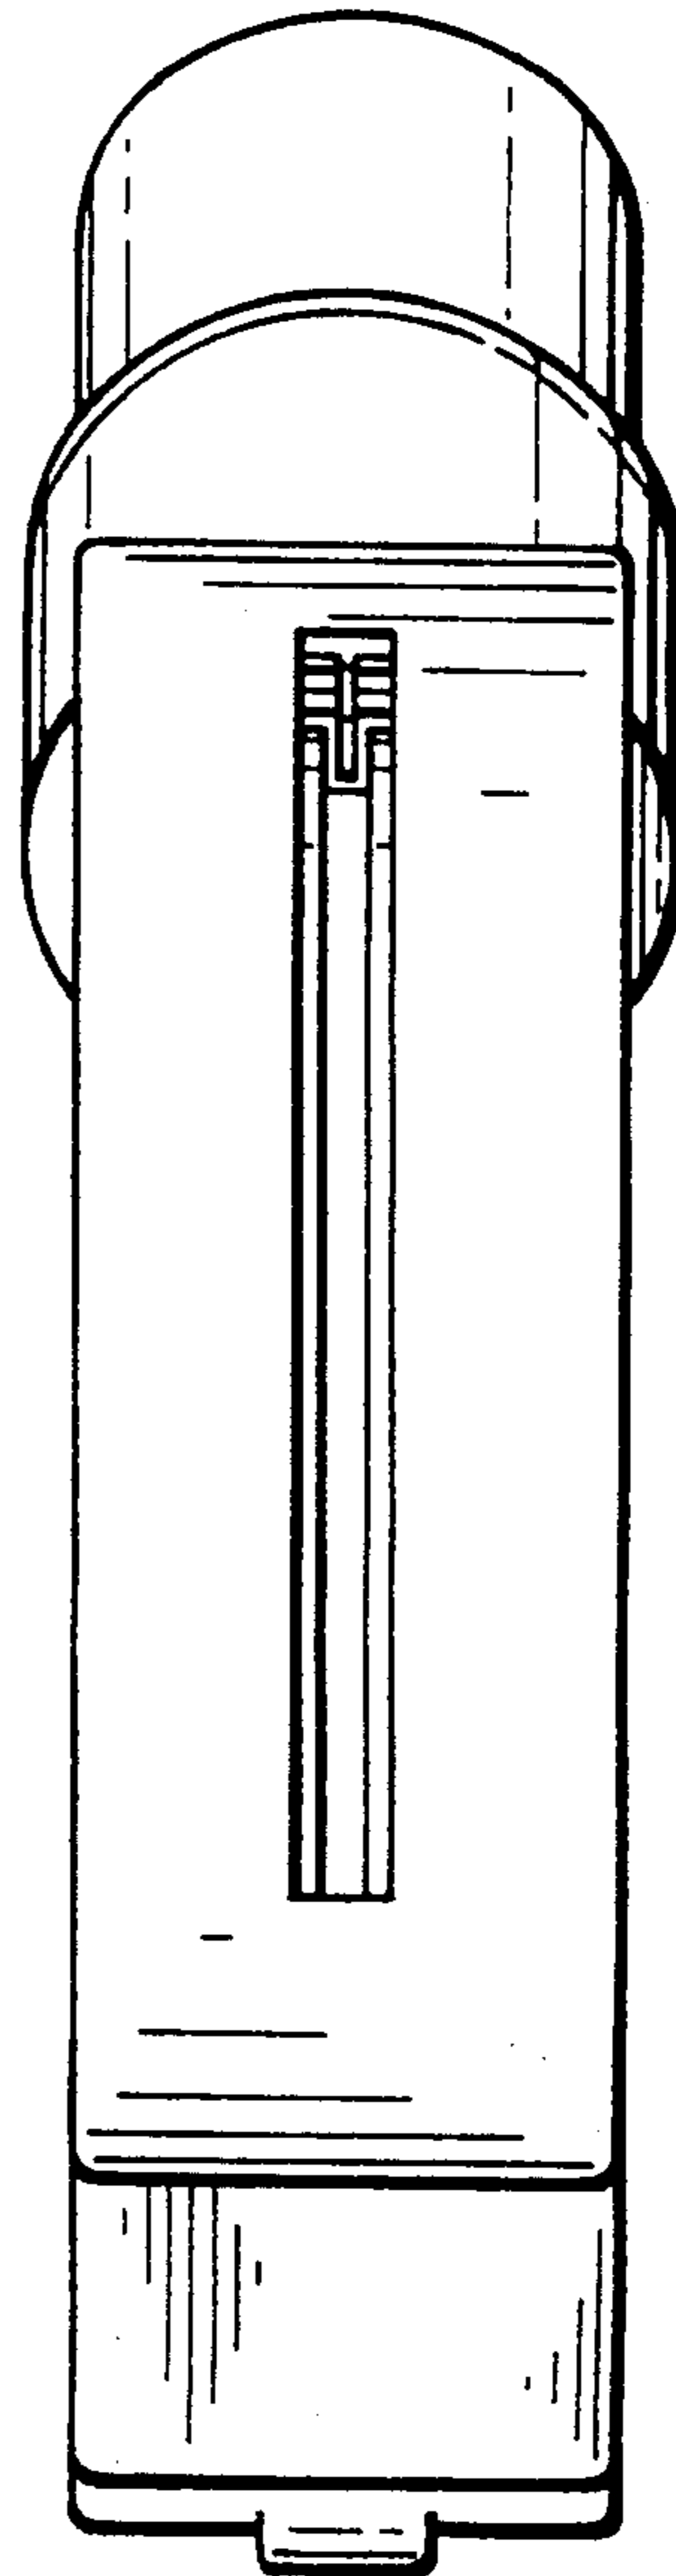


FIG. 2

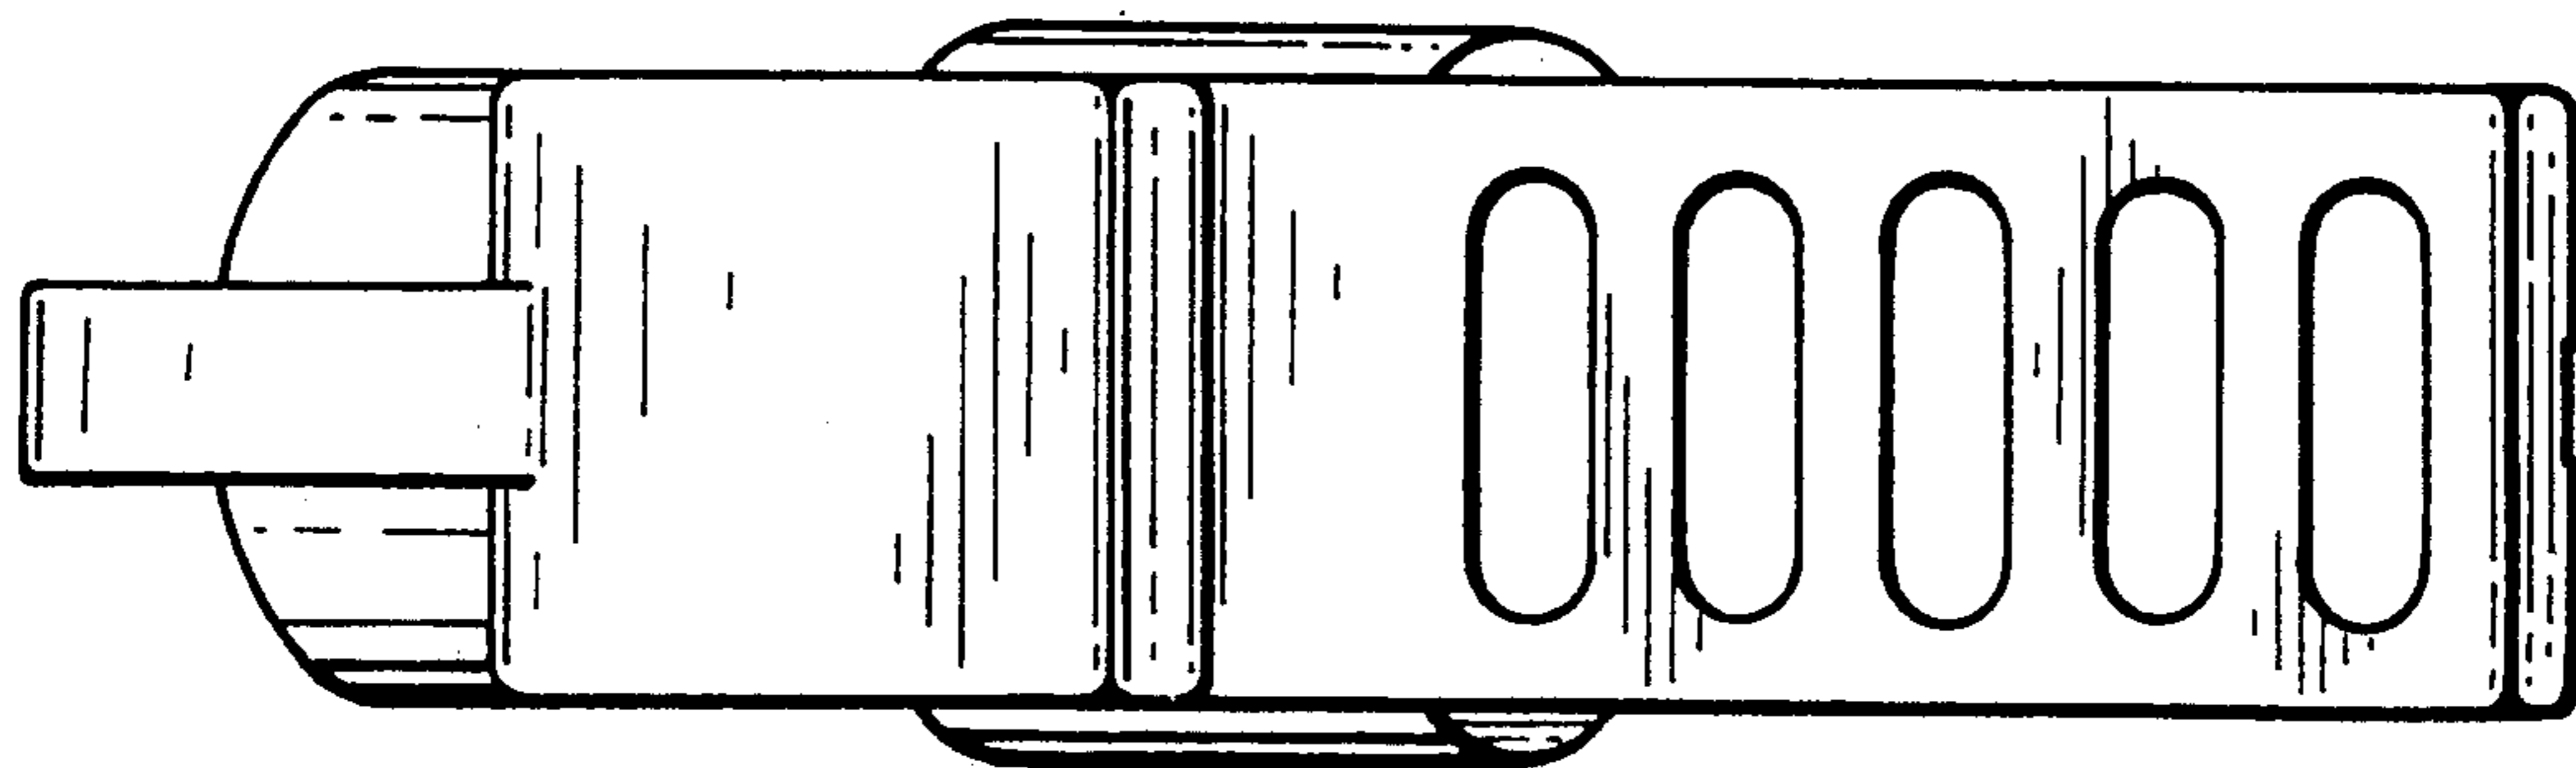


FIG. 5

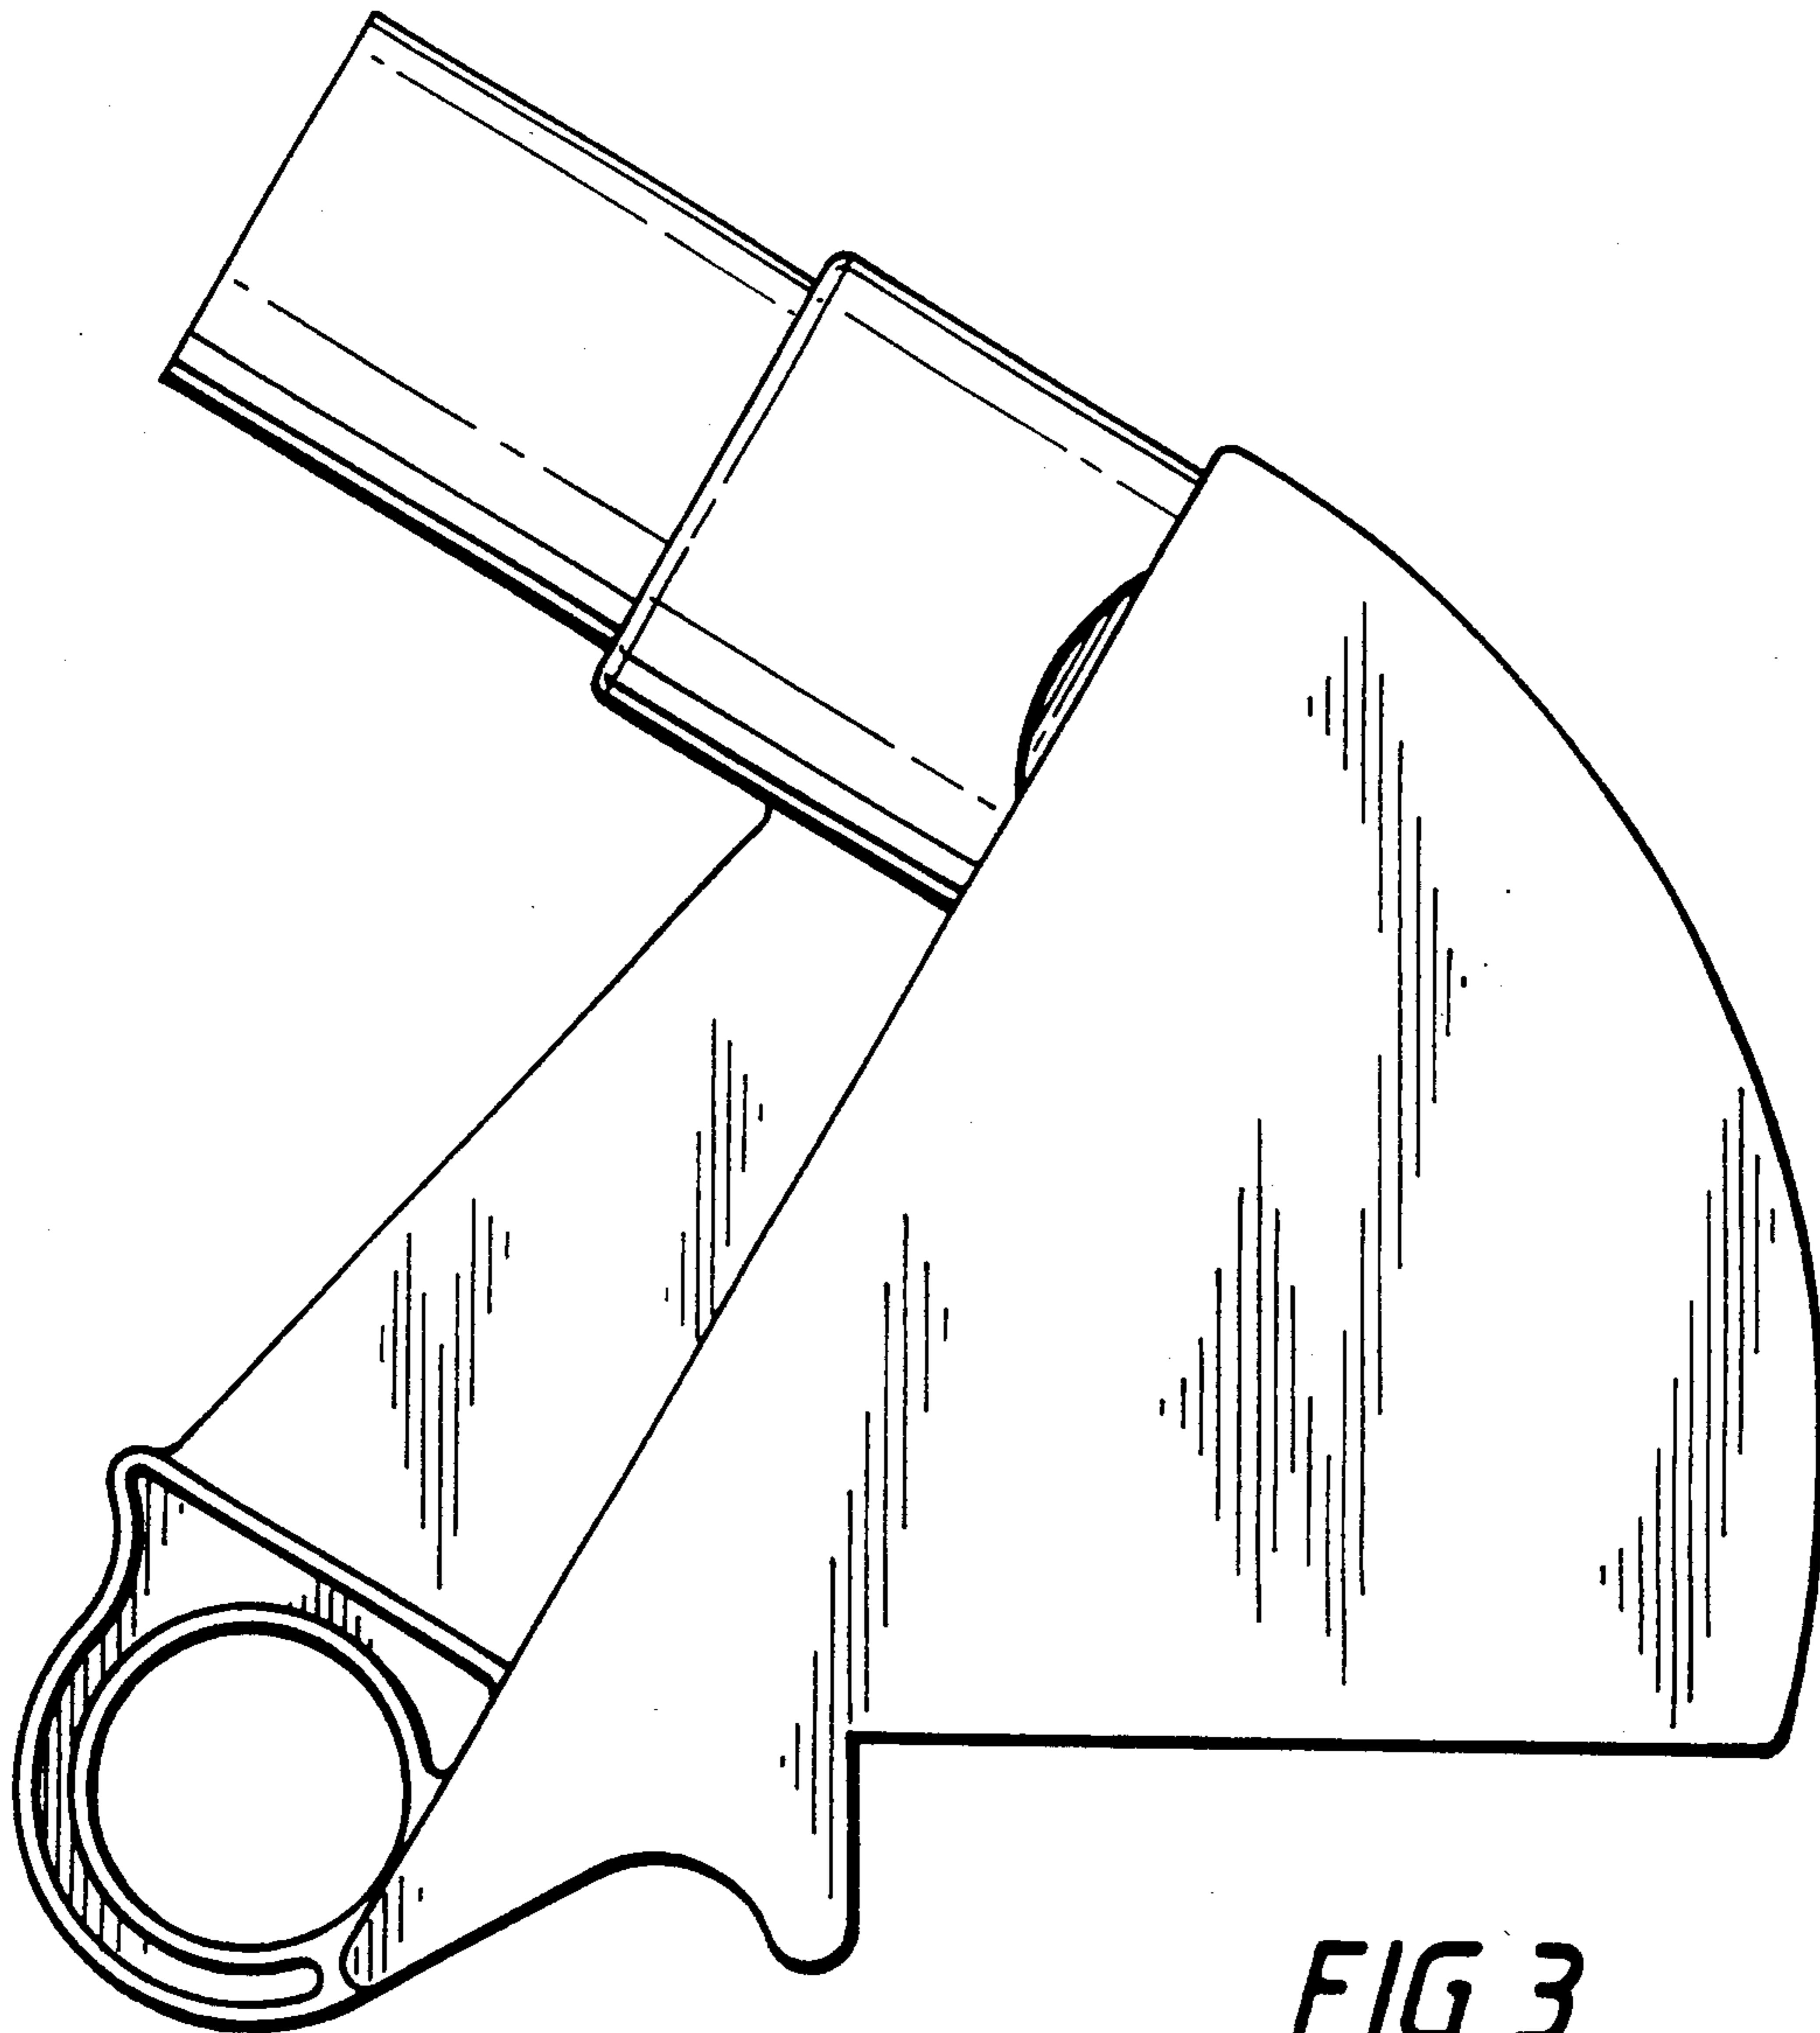


FIG. 3

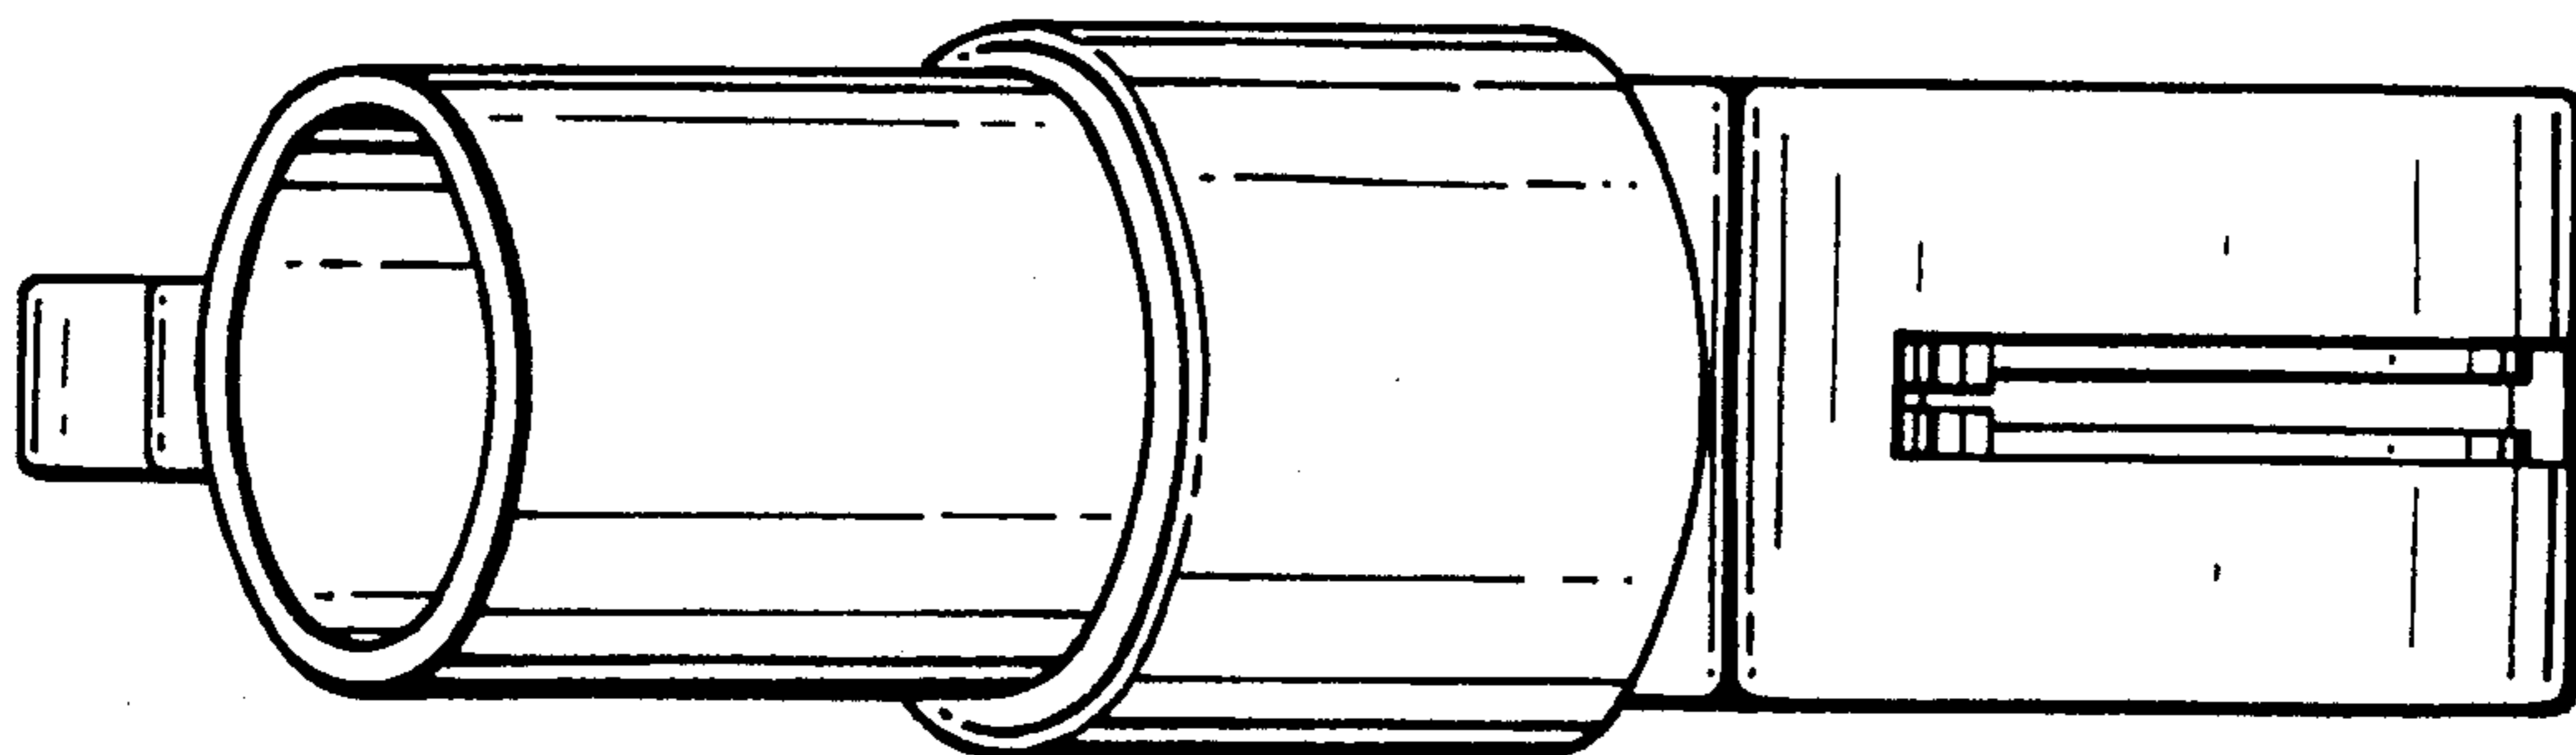


FIG. 4