



US00D338163S

# United States Patent [19]

[11] Patent Number: **Des. 338,163**

Atsumi et al.

[45] Date of Patent: **\*\* Aug. 10, 1993**

[54] **RADIATION CLINICAL THERMOMETER**

[75] Inventors: **Kaname Atsumi, Tokyo; Kazuo Nagata, Yokohama, both of Japan**

[73] Assignee: **Citizen Watch Co., Ltd., Tokyo, Japan**

[\*\*] Term: **14 Years**

[21] Appl. No.: **757,507**

[22] Filed: **Sep. 11, 1991**

[30] **Foreign Application Priority Data**

Mar. 12, 1991 [JP] Japan ..... 3-6427

[52] U.S. Cl. .... **D10/57**

[58] Field of Search ..... **D10/57; 128/664, 736; 374/126, 130, 128, 129, 133, 170, 208, 209**

[56] **References Cited**

**U.S. PATENT DOCUMENTS**

D. 254,189 2/1980 Prosky ..... D10/57

D. 287,473 12/1986 Ueno ..... D10/57

D. 330,681 11/1992 Yamada et al. .... D10/57  
4,602,642 7/1986 O'Hara et al. .  
4,784,149 11/1988 Berman et al. .  
4,932,789 6/1990 Egawa et al. .  
5,056,048 10/1991 Seperant ..... 374/170 X

*Primary Examiner*—Alan P. Douglas  
*Assistant Examiner*—A. D. Davis  
*Attorney, Agent, or Firm*—Cushman, Darby & Cushman

[57] **CLAIM**

The ornamental design for a radiation clinical thermometer, as shown and described.

**DESCRIPTION**

FIG. 1 is a front and left side perspective view of a radiation clinical thermometer showing our new design; FIG. 2 is a front elevational view thereof; FIG. 3 is a rear elevational view thereof; FIG. 4 is a top plan view thereof, the bottom plan view being a mirror image; FIG. 5 is a left side elevational view thereof; and, FIG. 6 is a right side elevational view thereof.

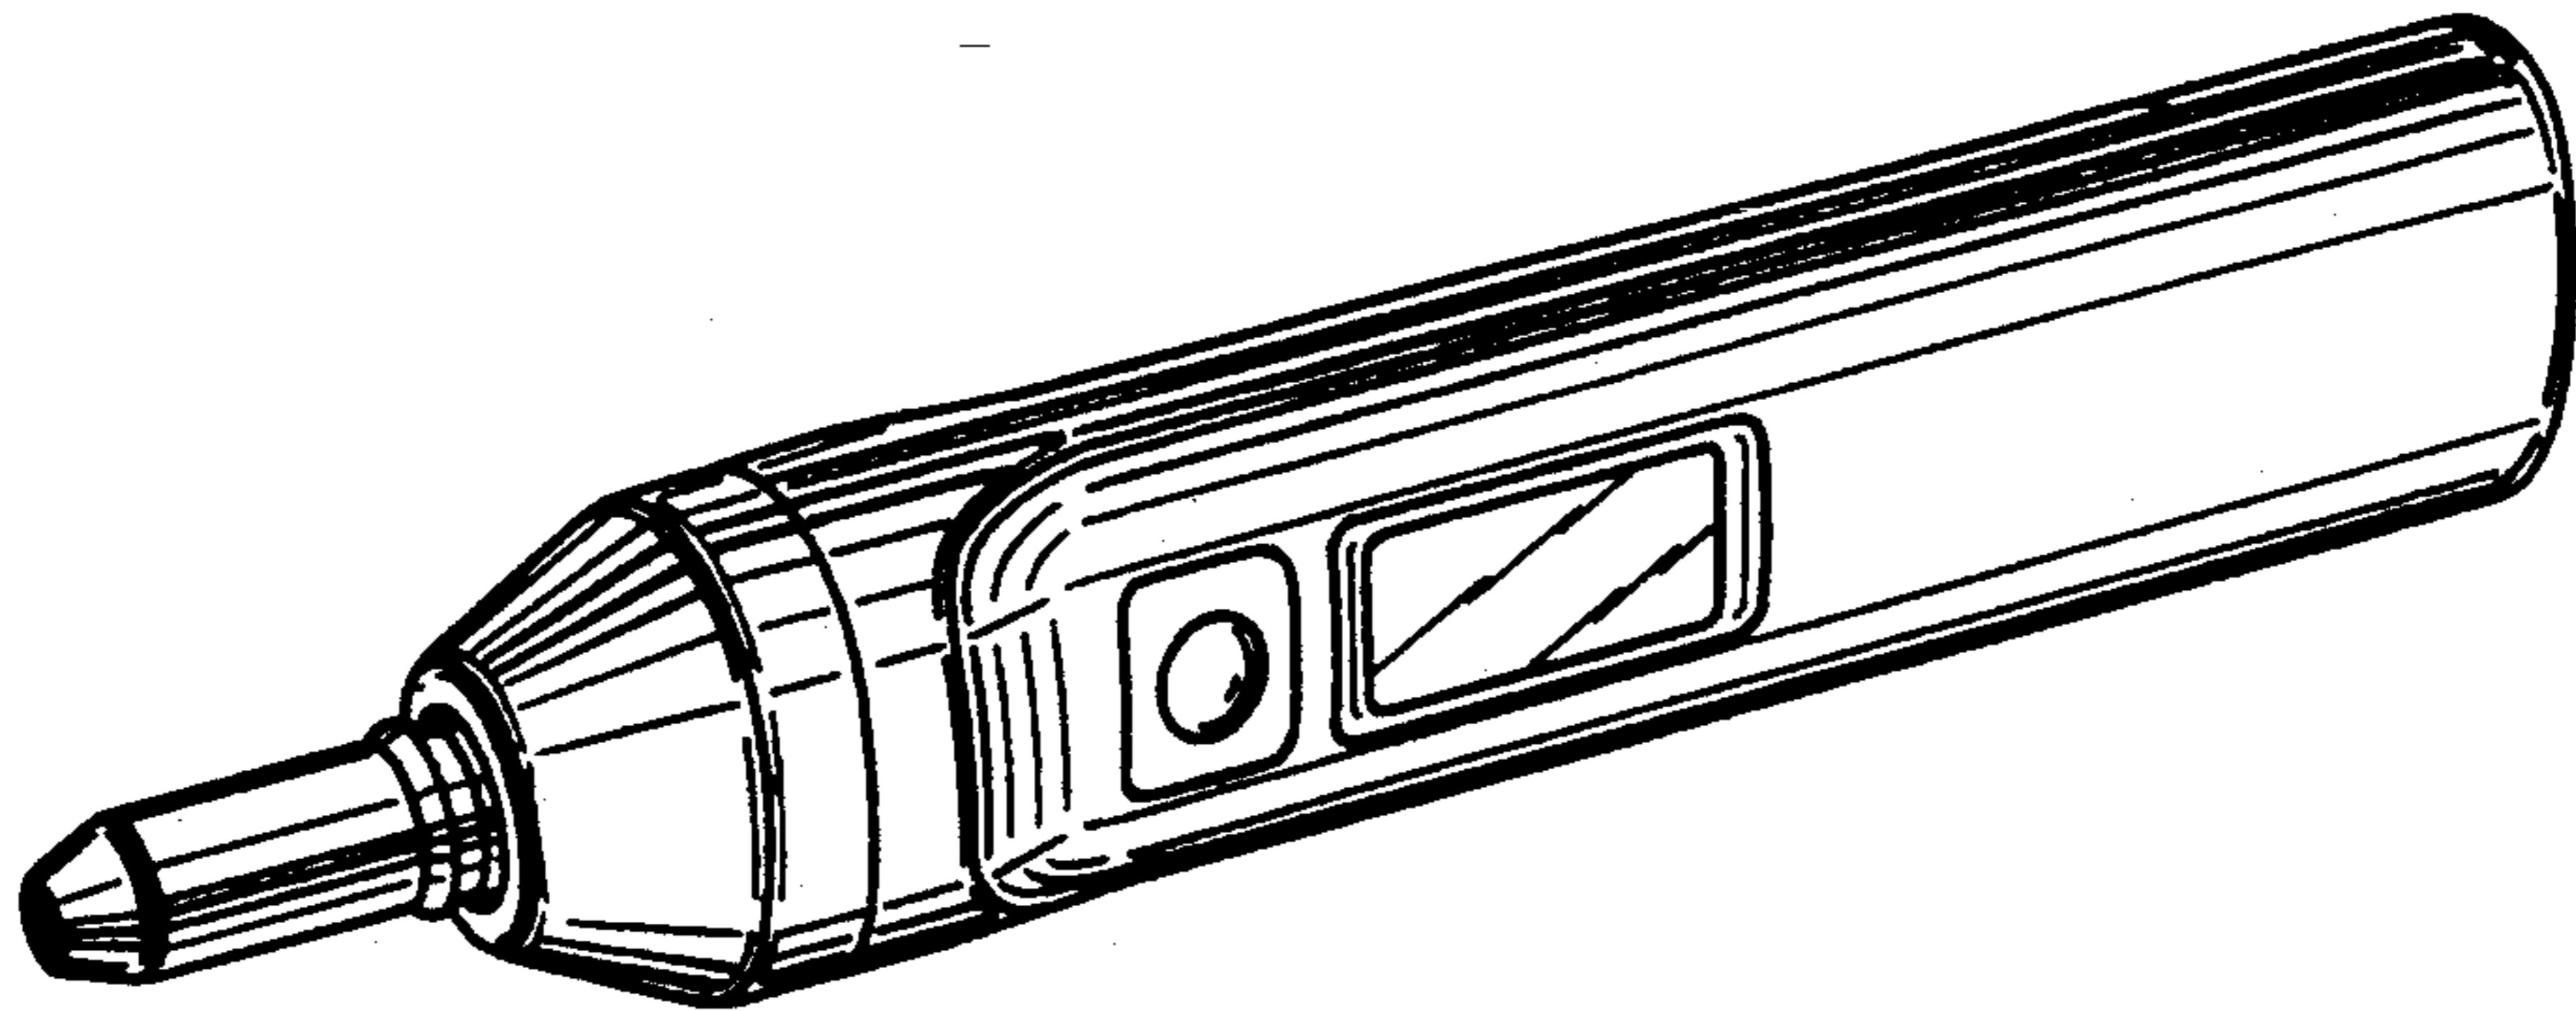


FIG. 1

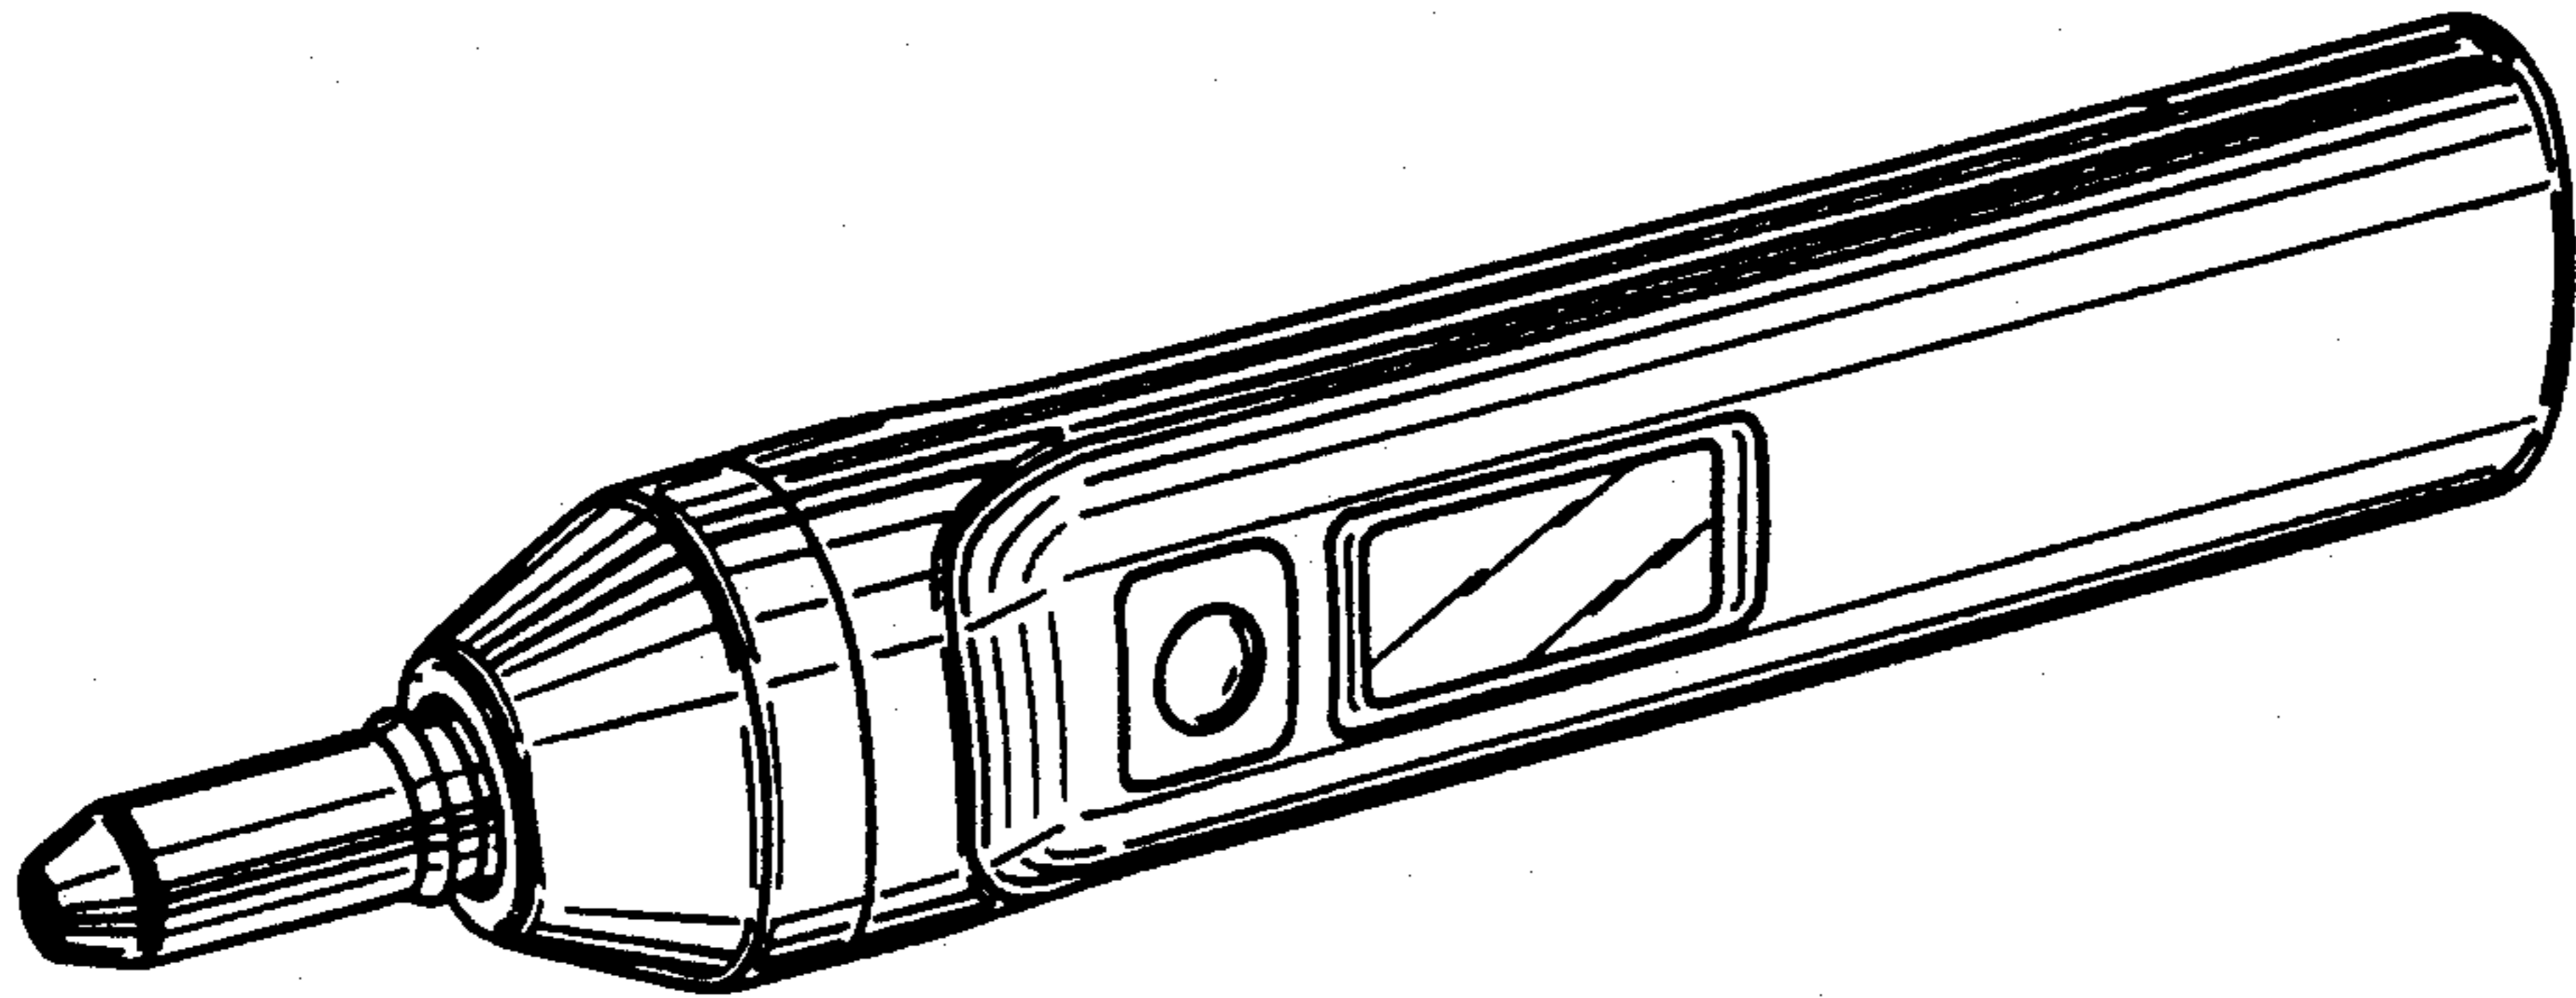


FIG. 2

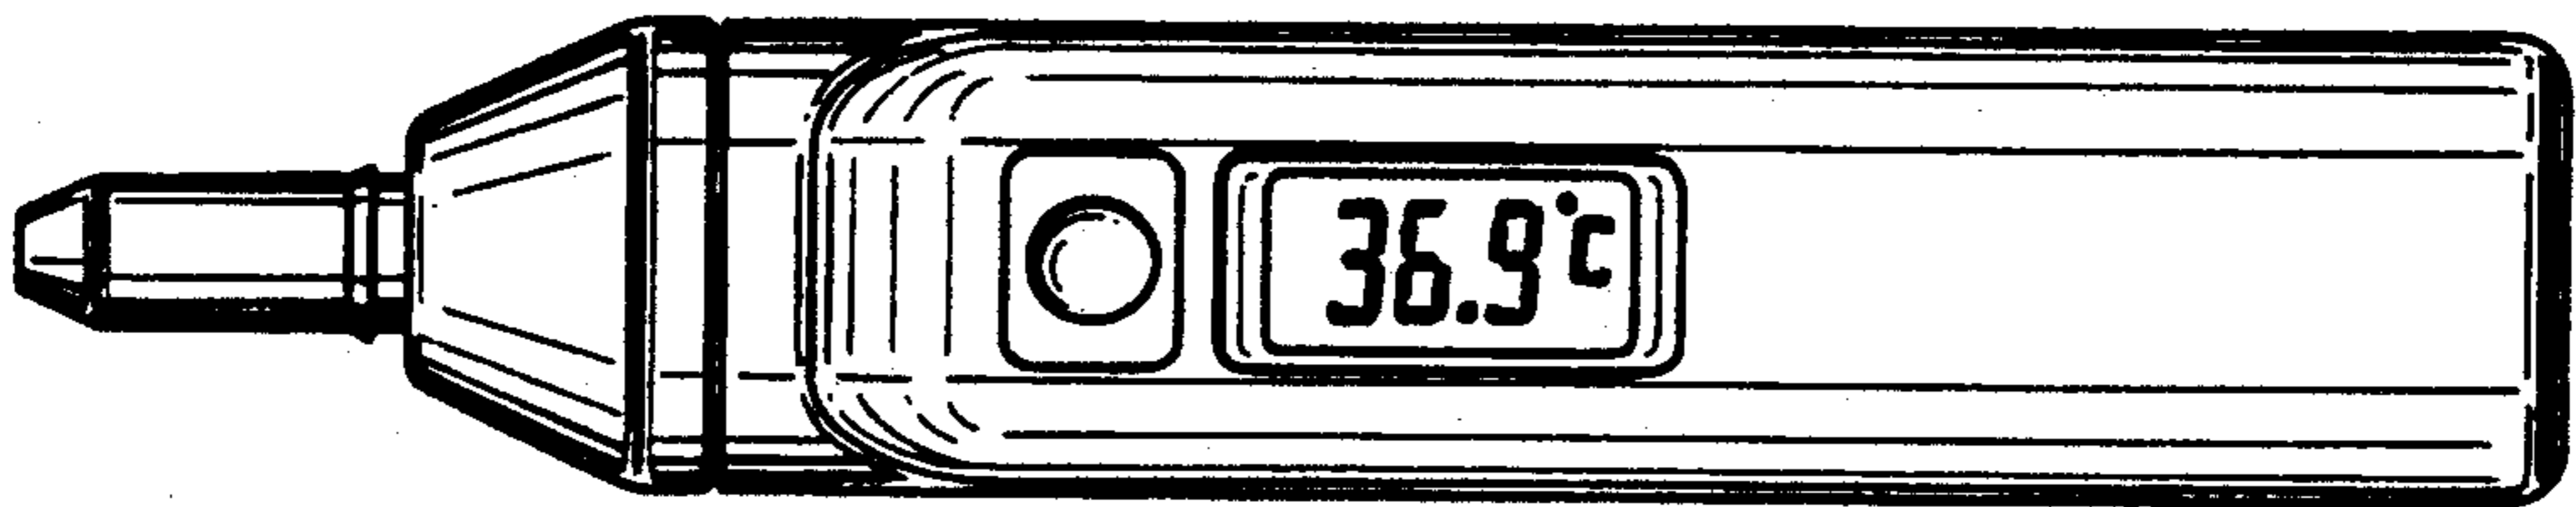


FIG. 3

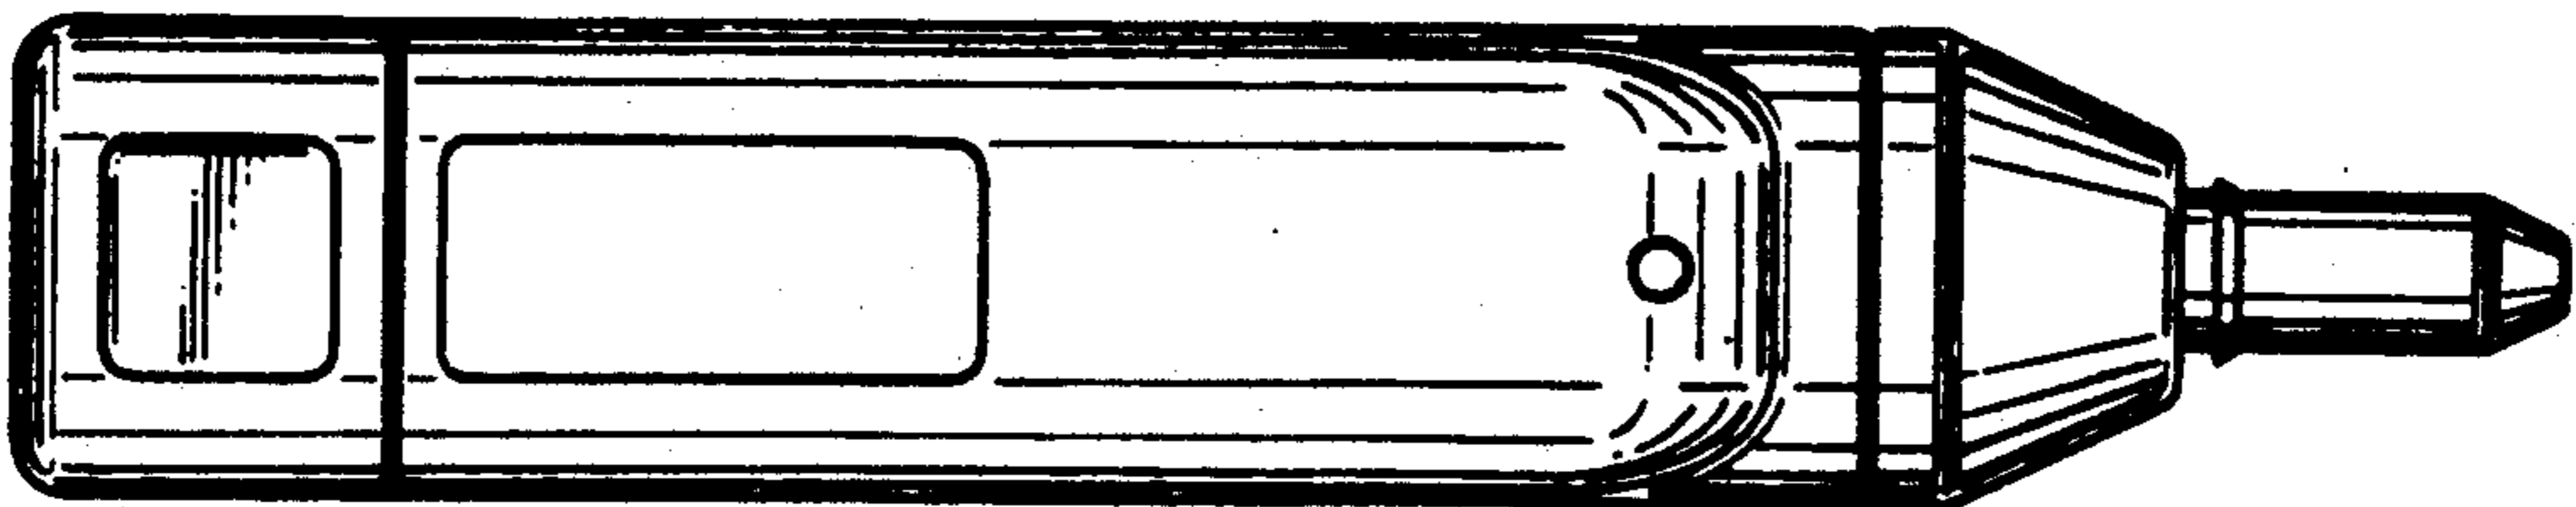


FIG.4

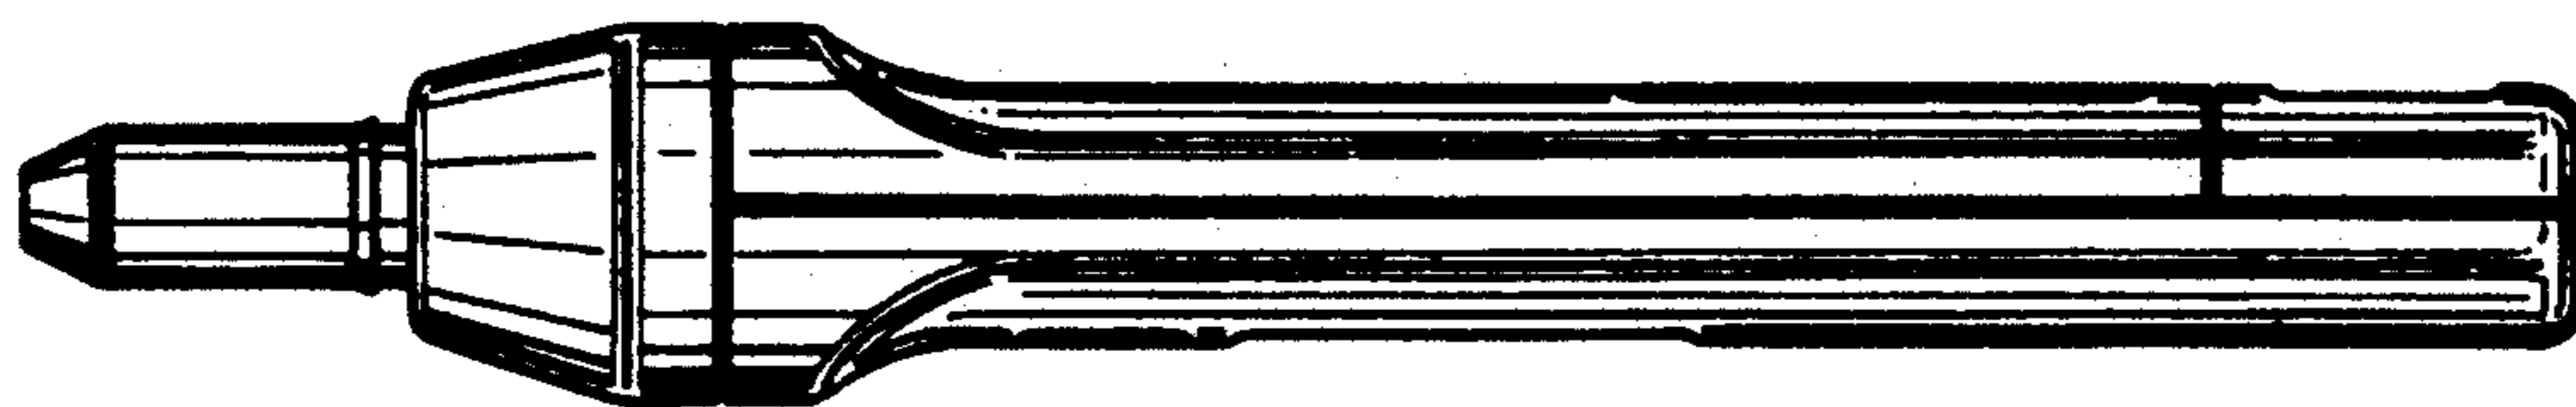


FIG.5

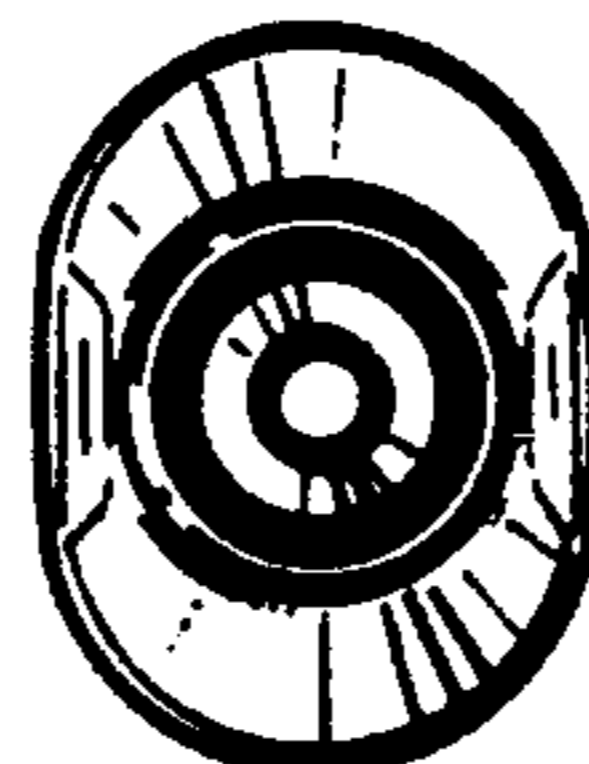


FIG.6

