



US00D338275S

United States Patent [19]

Fischer et al.

[11] Patent Number: Des. 338,275

[45] Date of Patent: ** Aug. 10, 1993

[54] **COMBINED CLINICAL-CHEMICAL ANALYZER EVALUATION UNIT AND WORK STATION**

[75] Inventors: **Arthur Fischer, Munich; Heinz-Dieter Engert, Seefeld, both of Fed. Rep. of Germany**

[73] Assignee: **Bayer Diagnostics, GmbH, Munich, Fed. Rep. of Germany**

[**] Term: **14 Years**

[21] Appl. No.: **431,520**

[22] Filed: **Nov. 3, 1989**

[30] **Foreign Application Priority Data**

May 3, 1989 [DE] Fed. Rep. of Germany 8903318
[52] U.S. Cl. **D24/232; D24/216; D24/223**

[58] Field of Search **D24/234, 223, 216, 231, D24/232; 422/65, 67, 63, 64, 100, 102; 436/47, 48; 356/446, 416, 246**

[56] **References Cited**

U.S. PATENT DOCUMENTS

4,429,373 1/1984 Fletcher et al. 422/65 X
4,459,265 7/1984 Berglund 422/65 X
4,791,461 12/1988 Kishimoto et al. 356/446

5,104,621 4/1992 Pfost et al. 422/65 X


Primary Examiner—Stella Reid

[57] **CLAIM**

The ornamental design for a combined clinical-chemical analyzer evaluation unit and work station, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a clinical-chemical analyzer evaluation unit, showing my new design, with cover removed;
FIG. 2 is a side perspective view thereof, with cover attached;
FIG. 3 is a front elevational view thereof;
FIG. 4 is a side perspective view thereof, opposite that shown in FIG. 2;
FIG. 5 is a rear elevational view thereof;
FIG. 6 is a bottom plan view thereof;
FIG. 7 is a perspective view of a work station;
FIG. 8 is a side perspective view thereof;
FIG. 9 is a side perspective view thereof, opposite that shown in FIG. 8;
FIG. 10 is a rear elevational view thereof;
FIG. 11 is a top plan view thereof;
FIG. 12 is a bottom plan view thereof; and,
FIG. 13 is a perspective view of the combined clinical-chemical analyzer evaluation unit and work station with the cover removed on the analyzer.

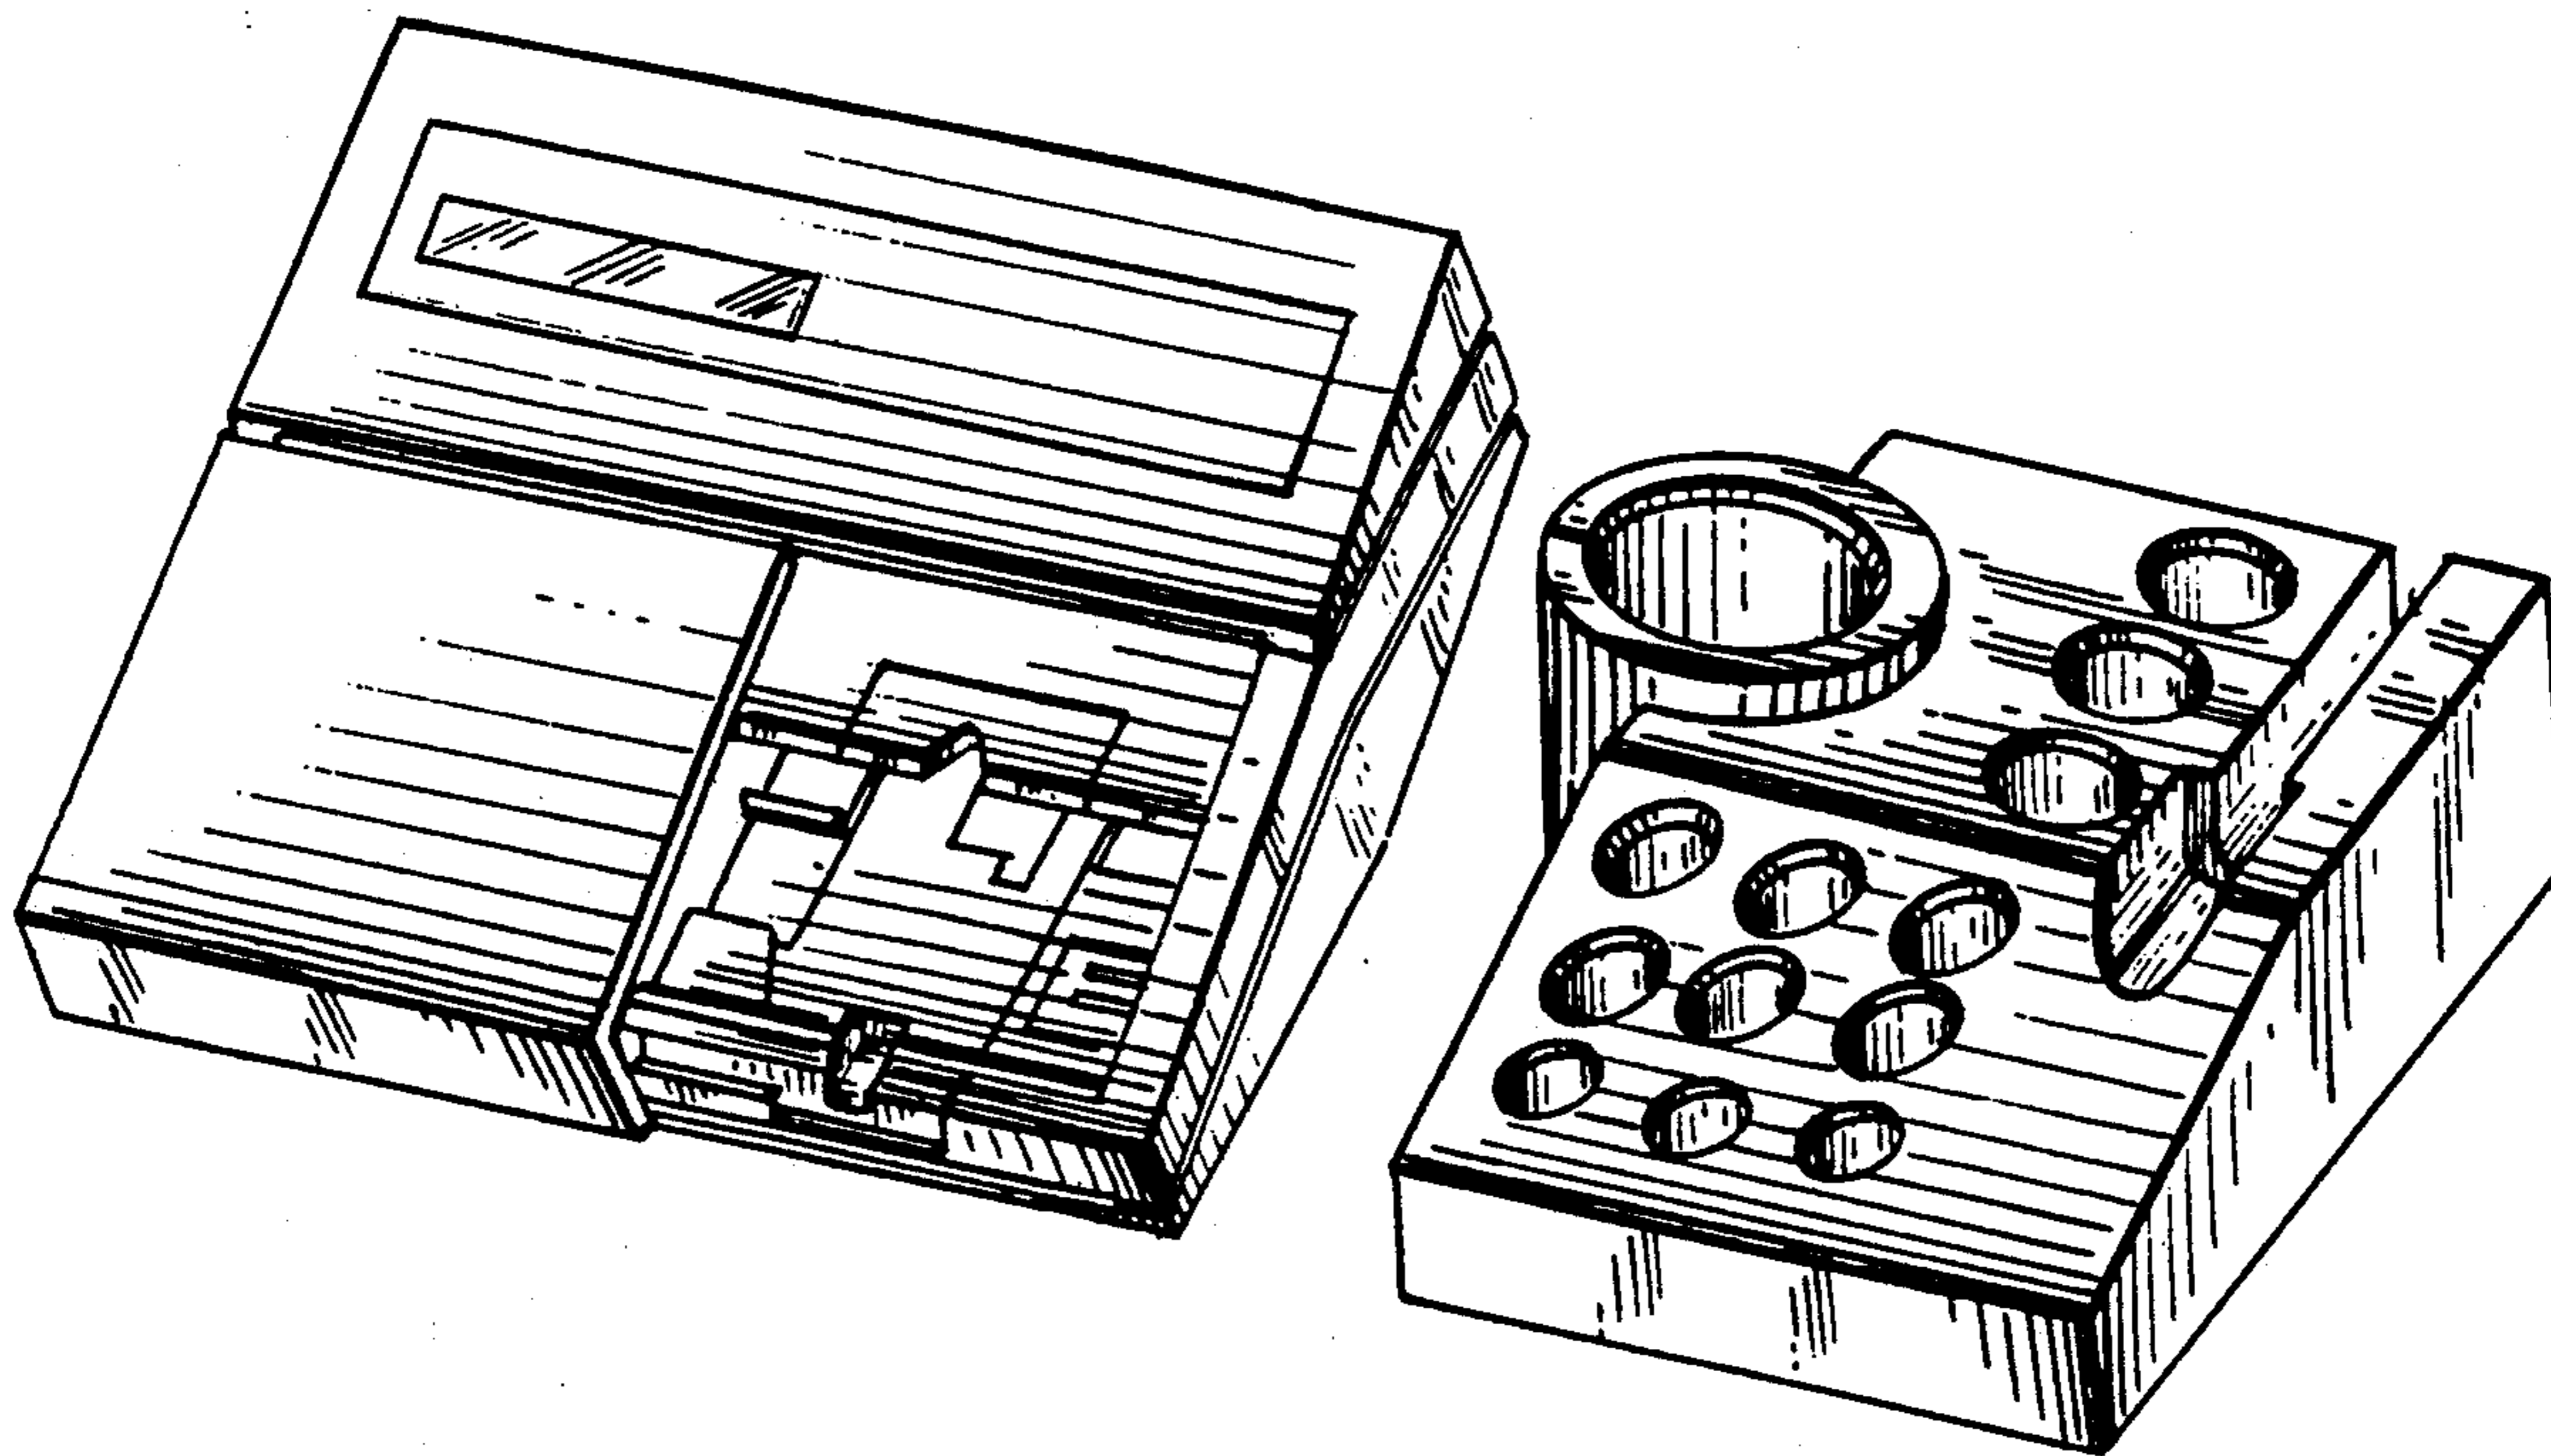

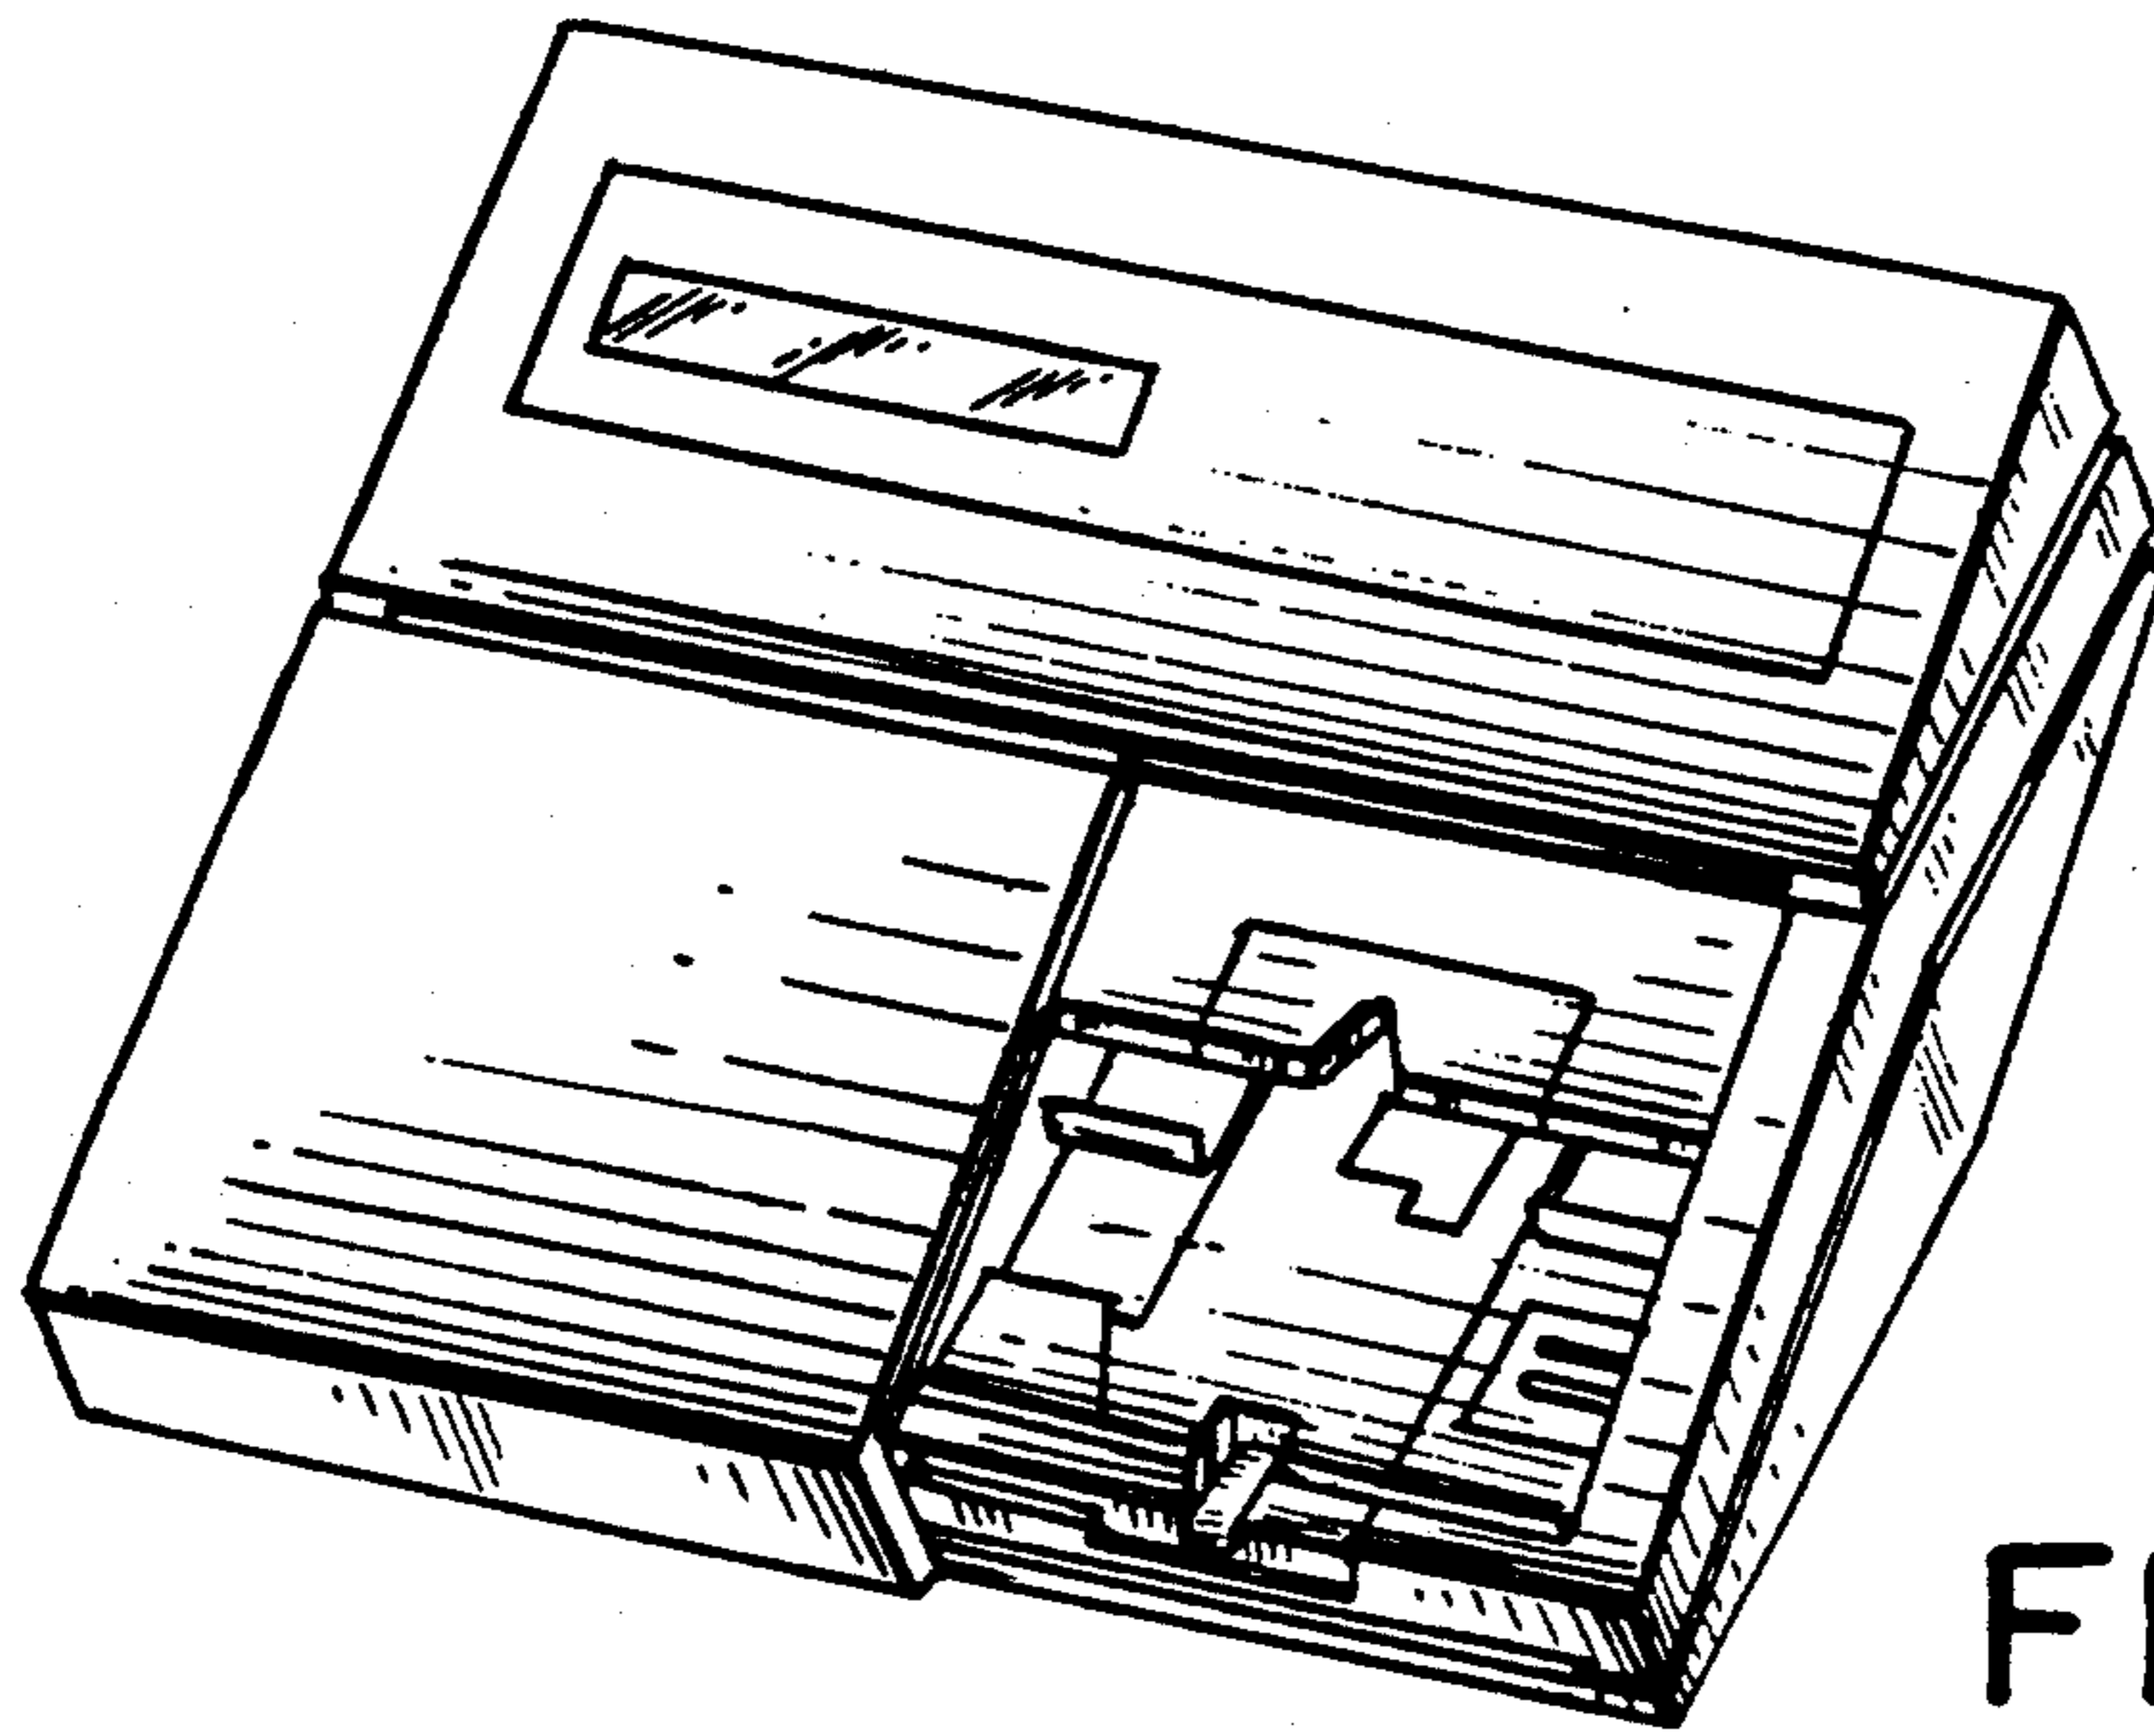


FIG. 1

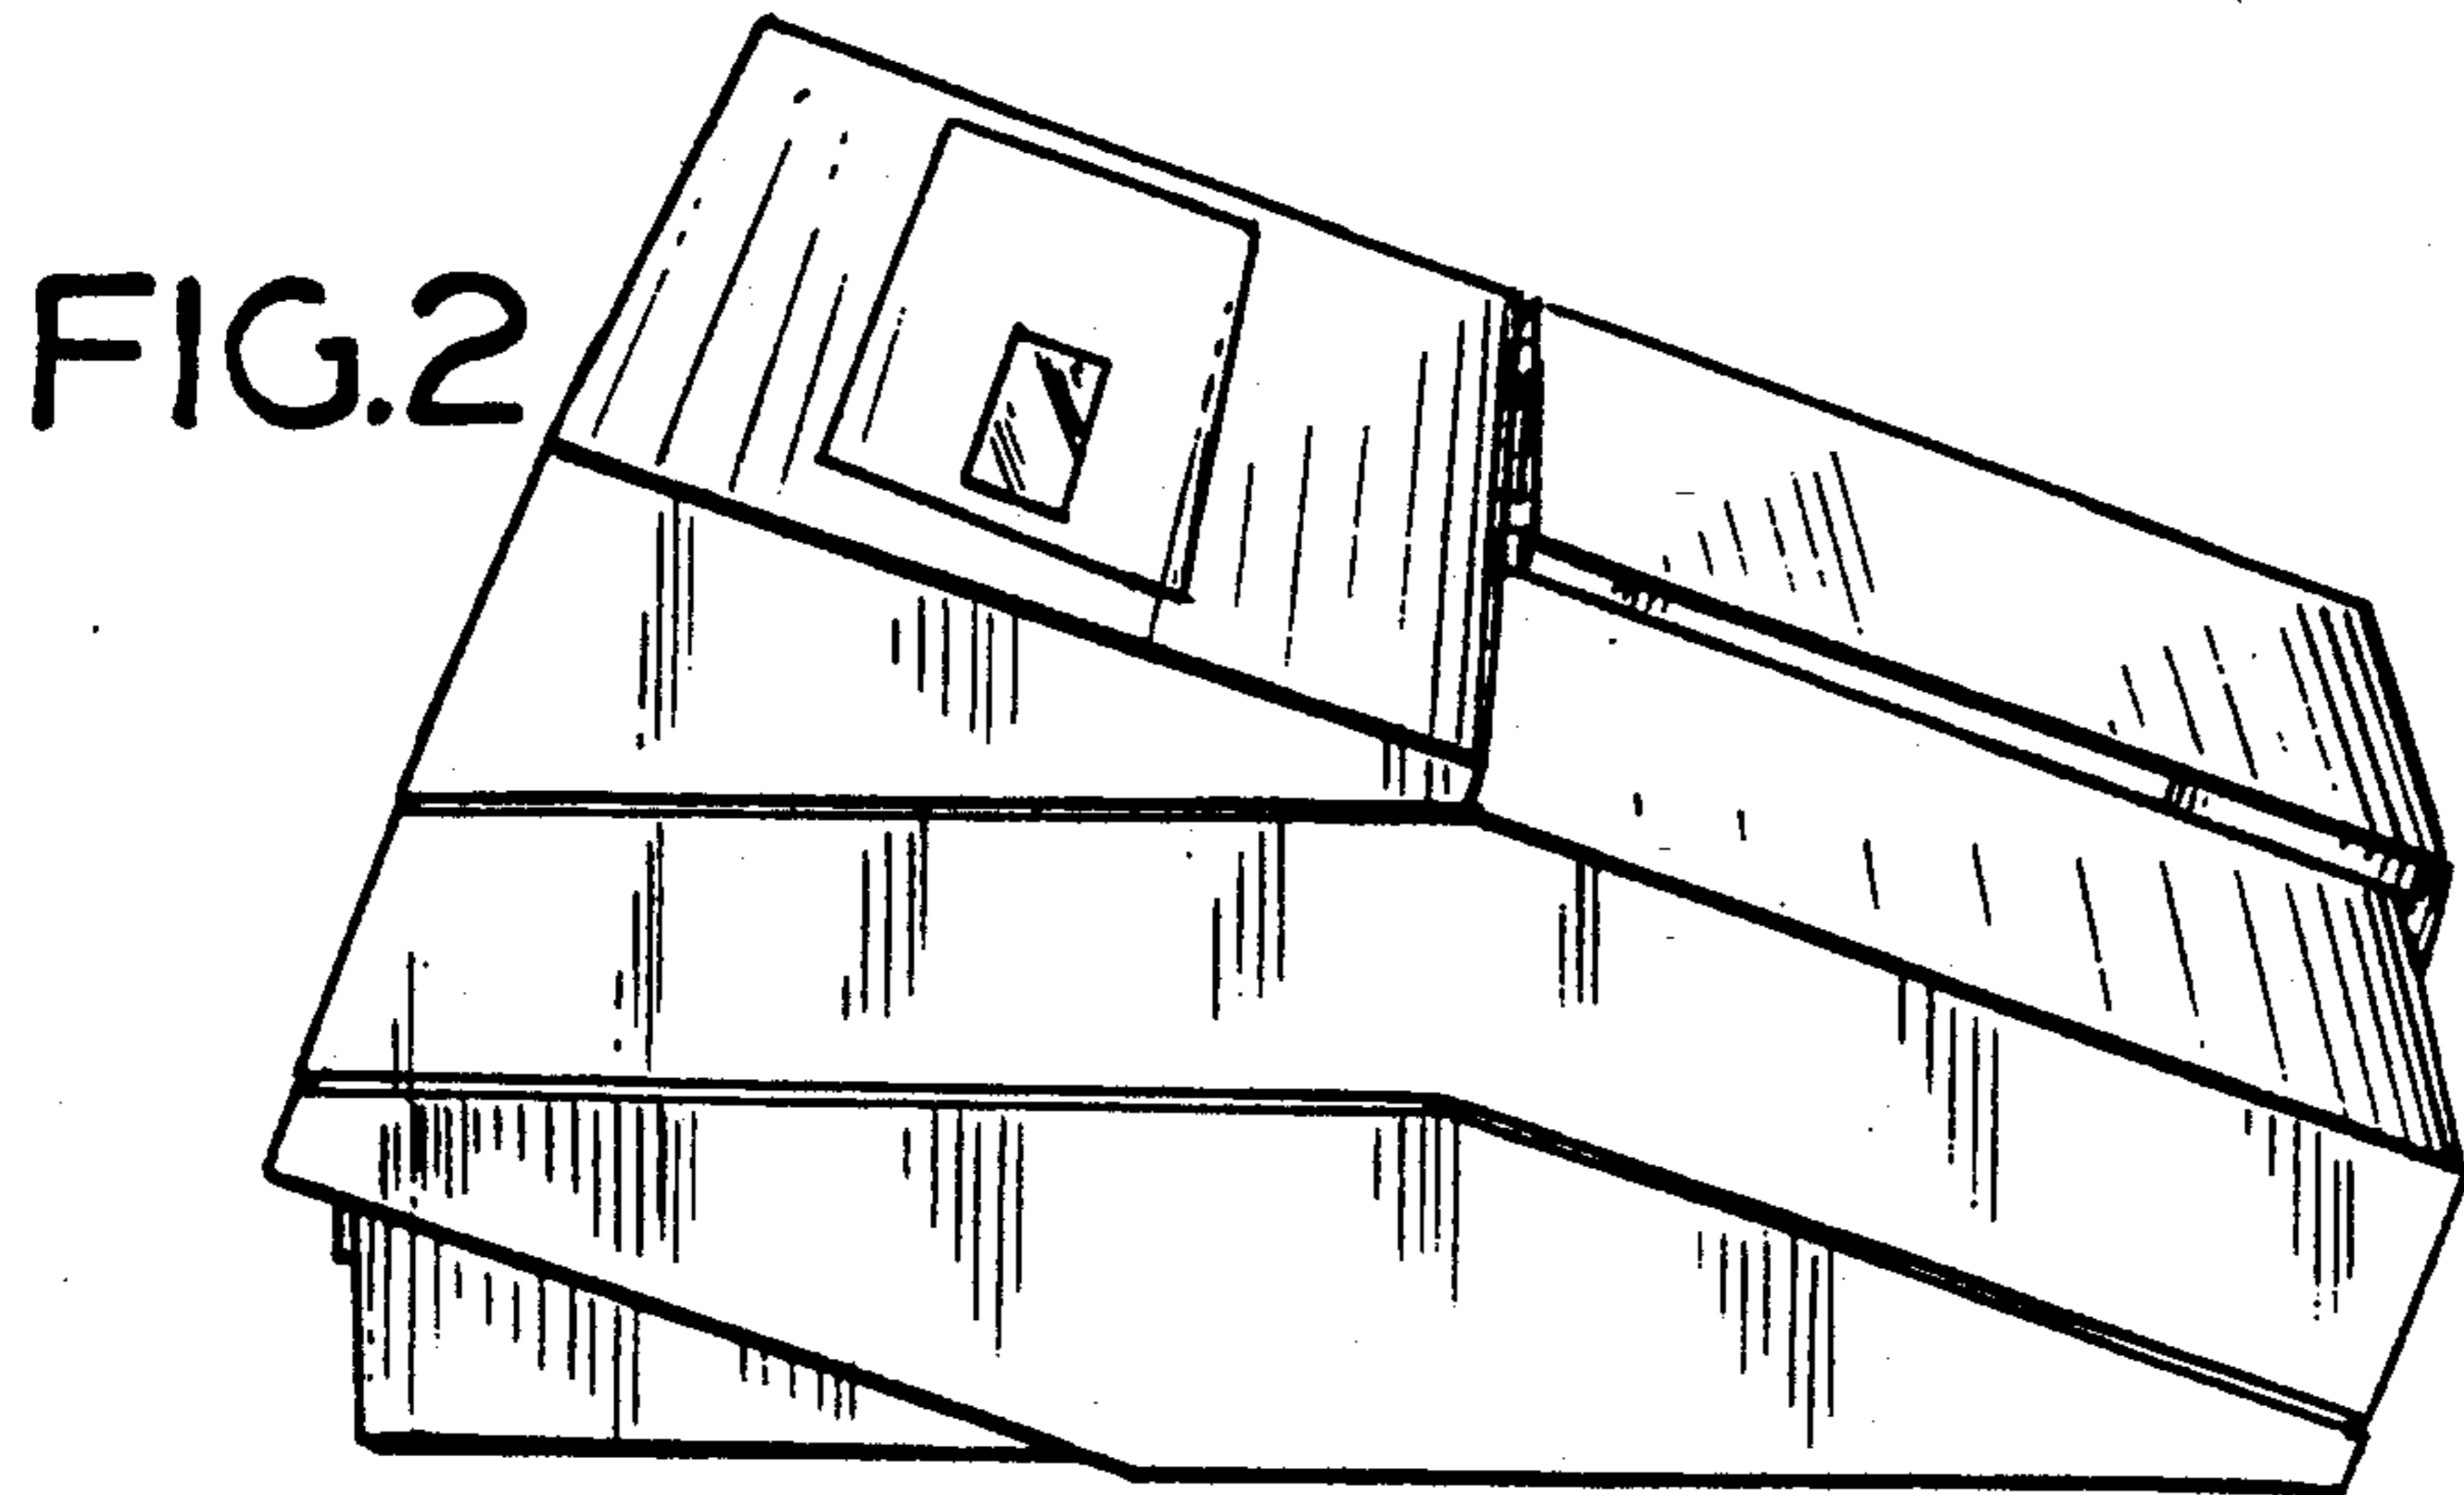


FIG. 2

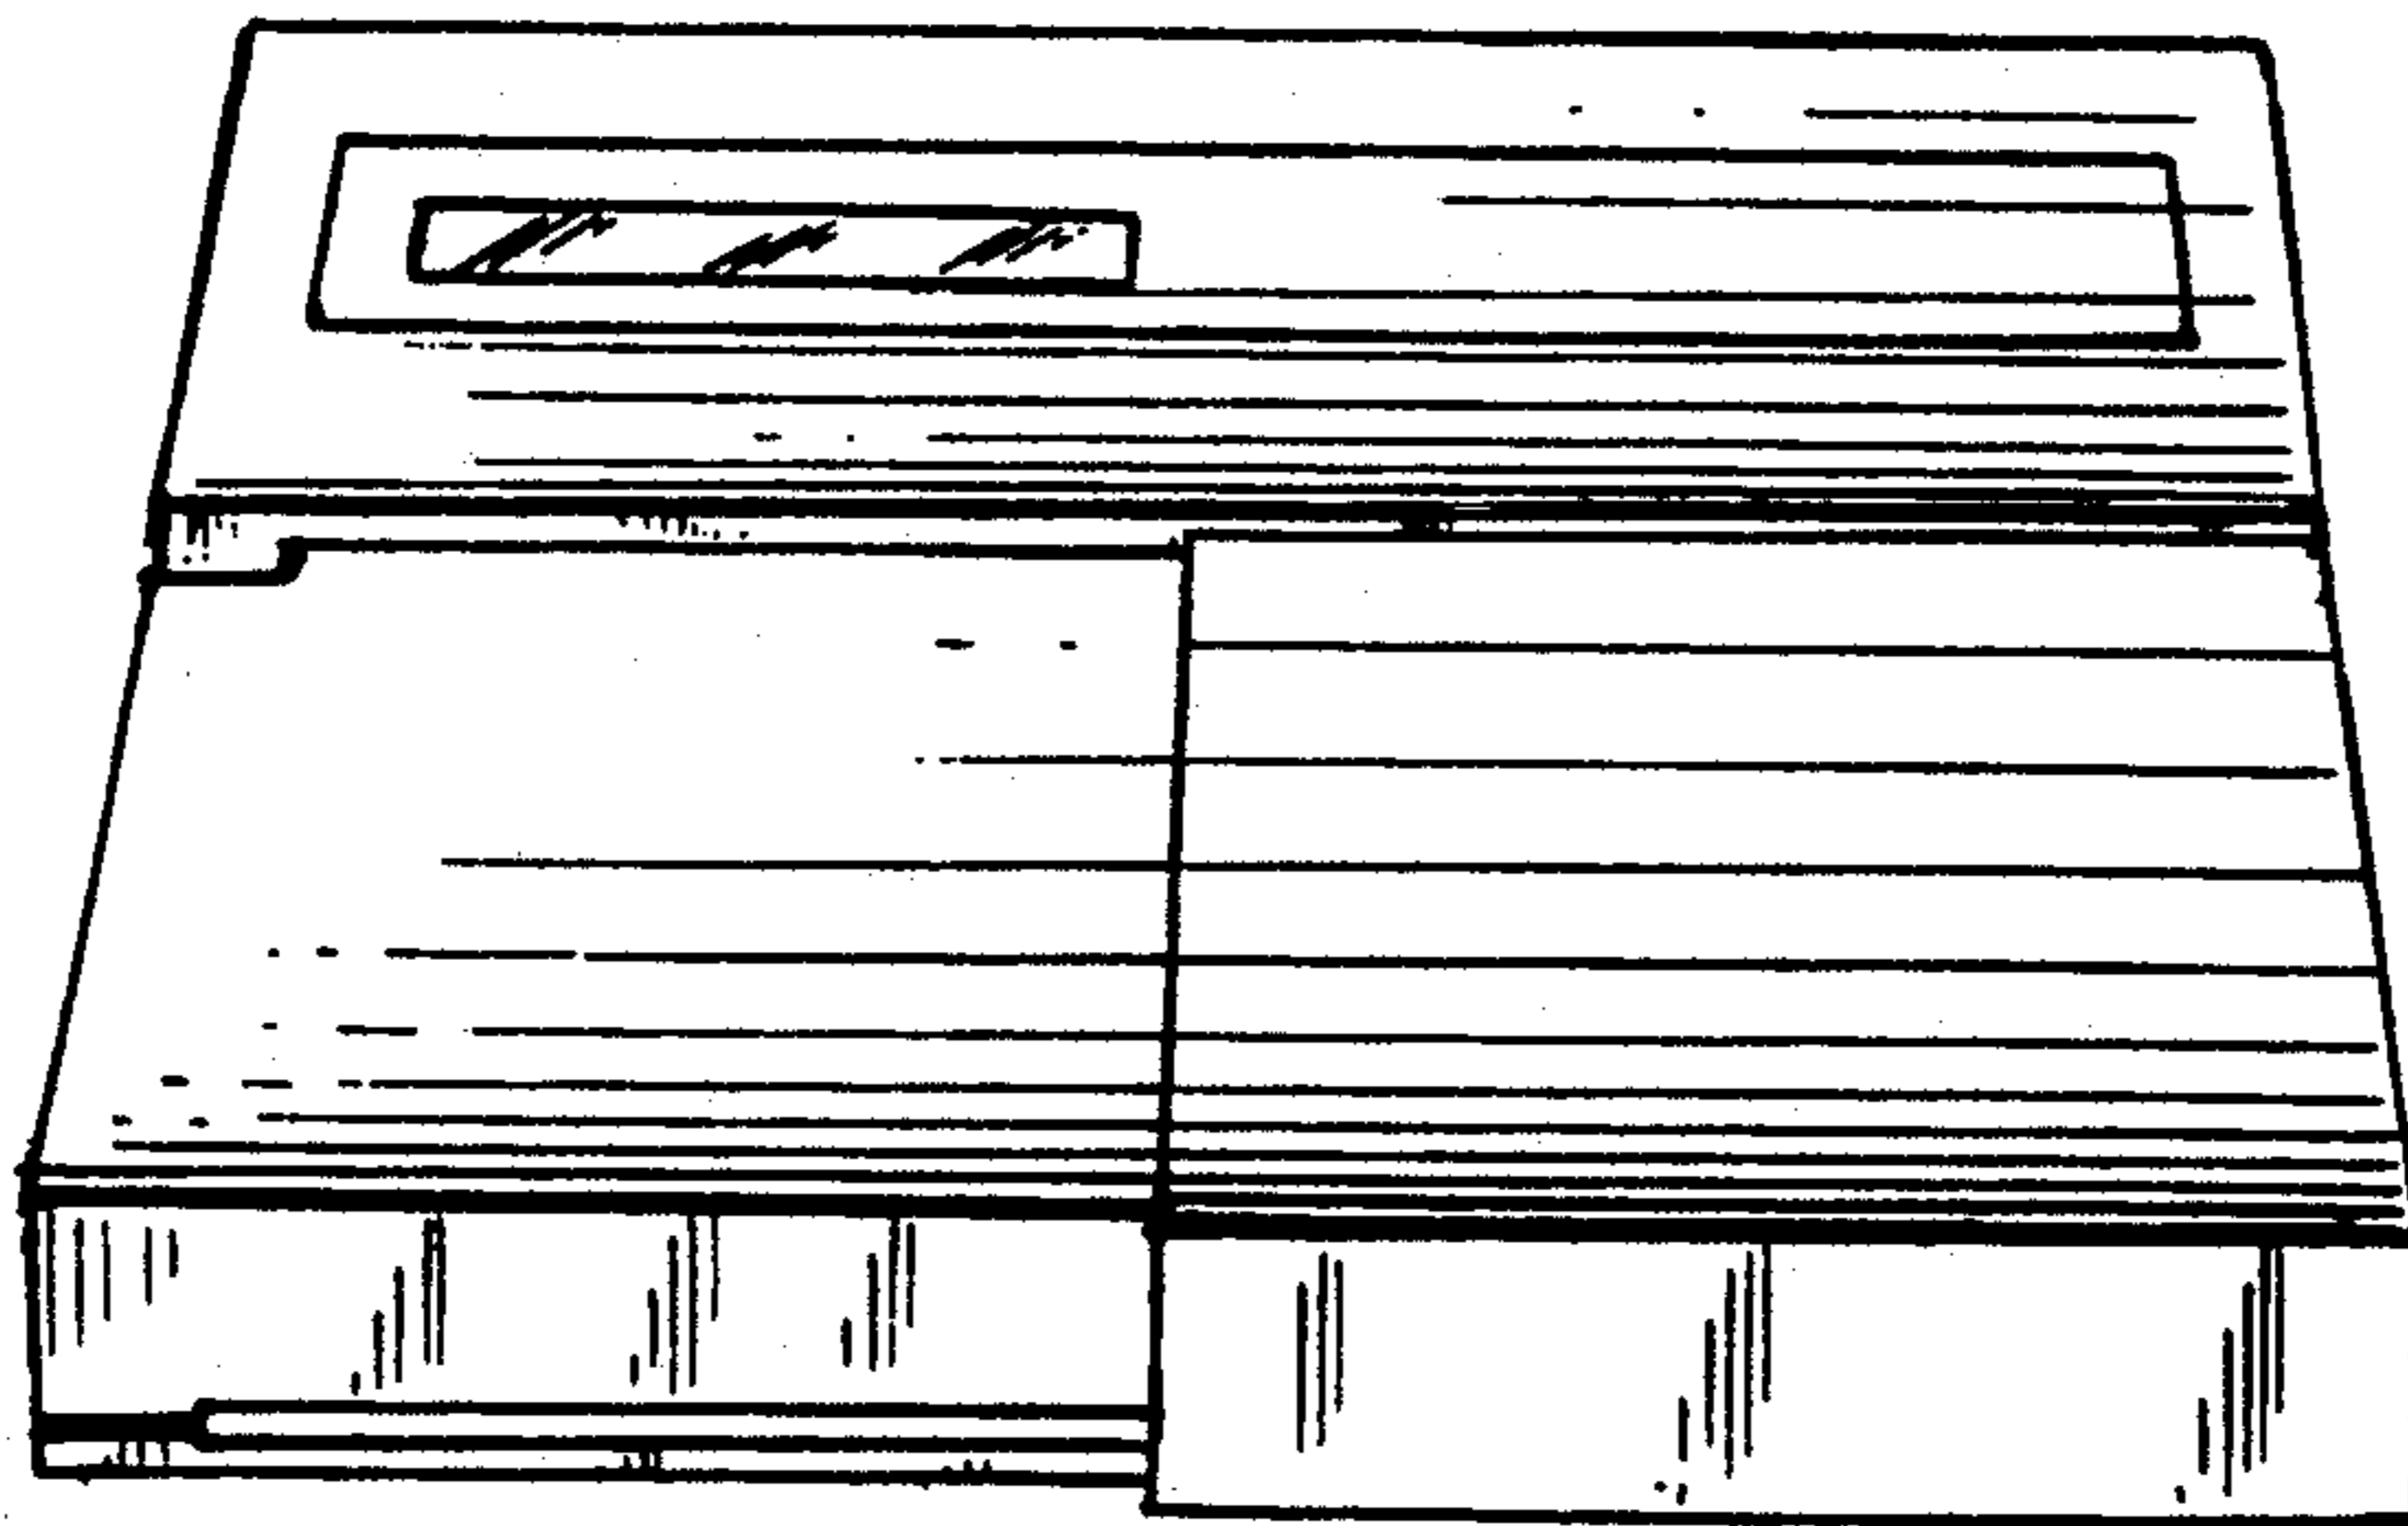


FIG. 3

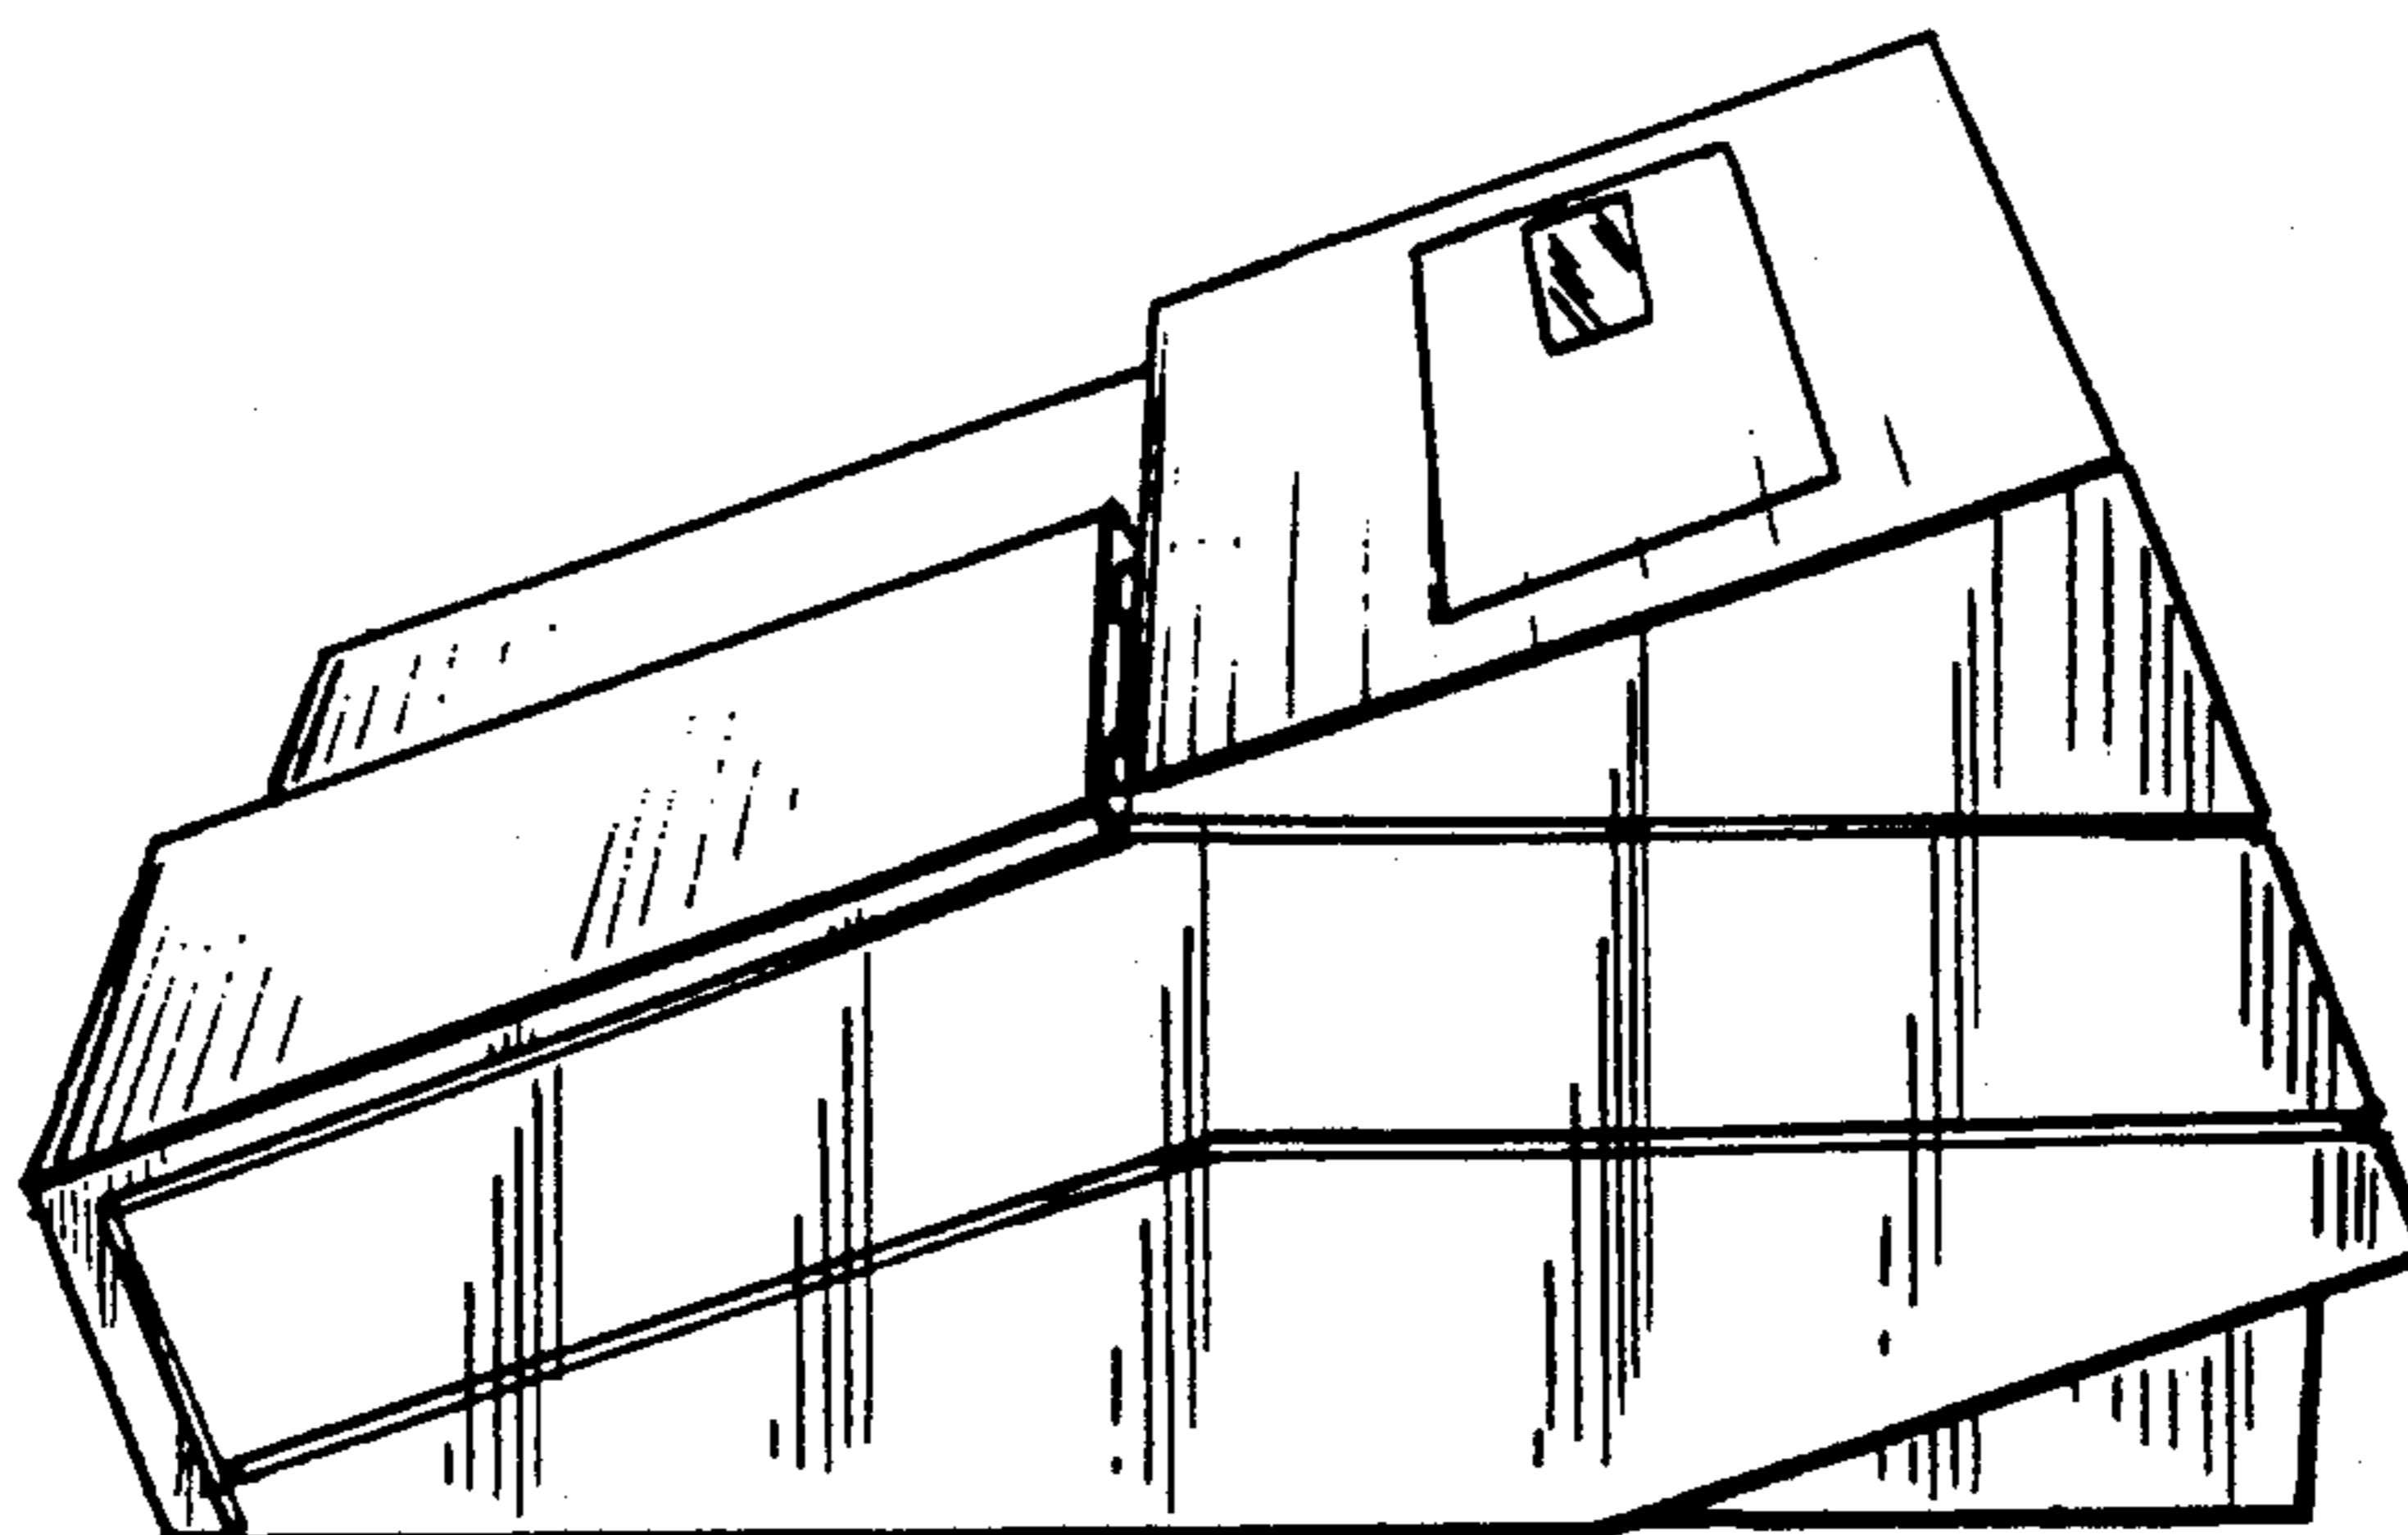


FIG. 4

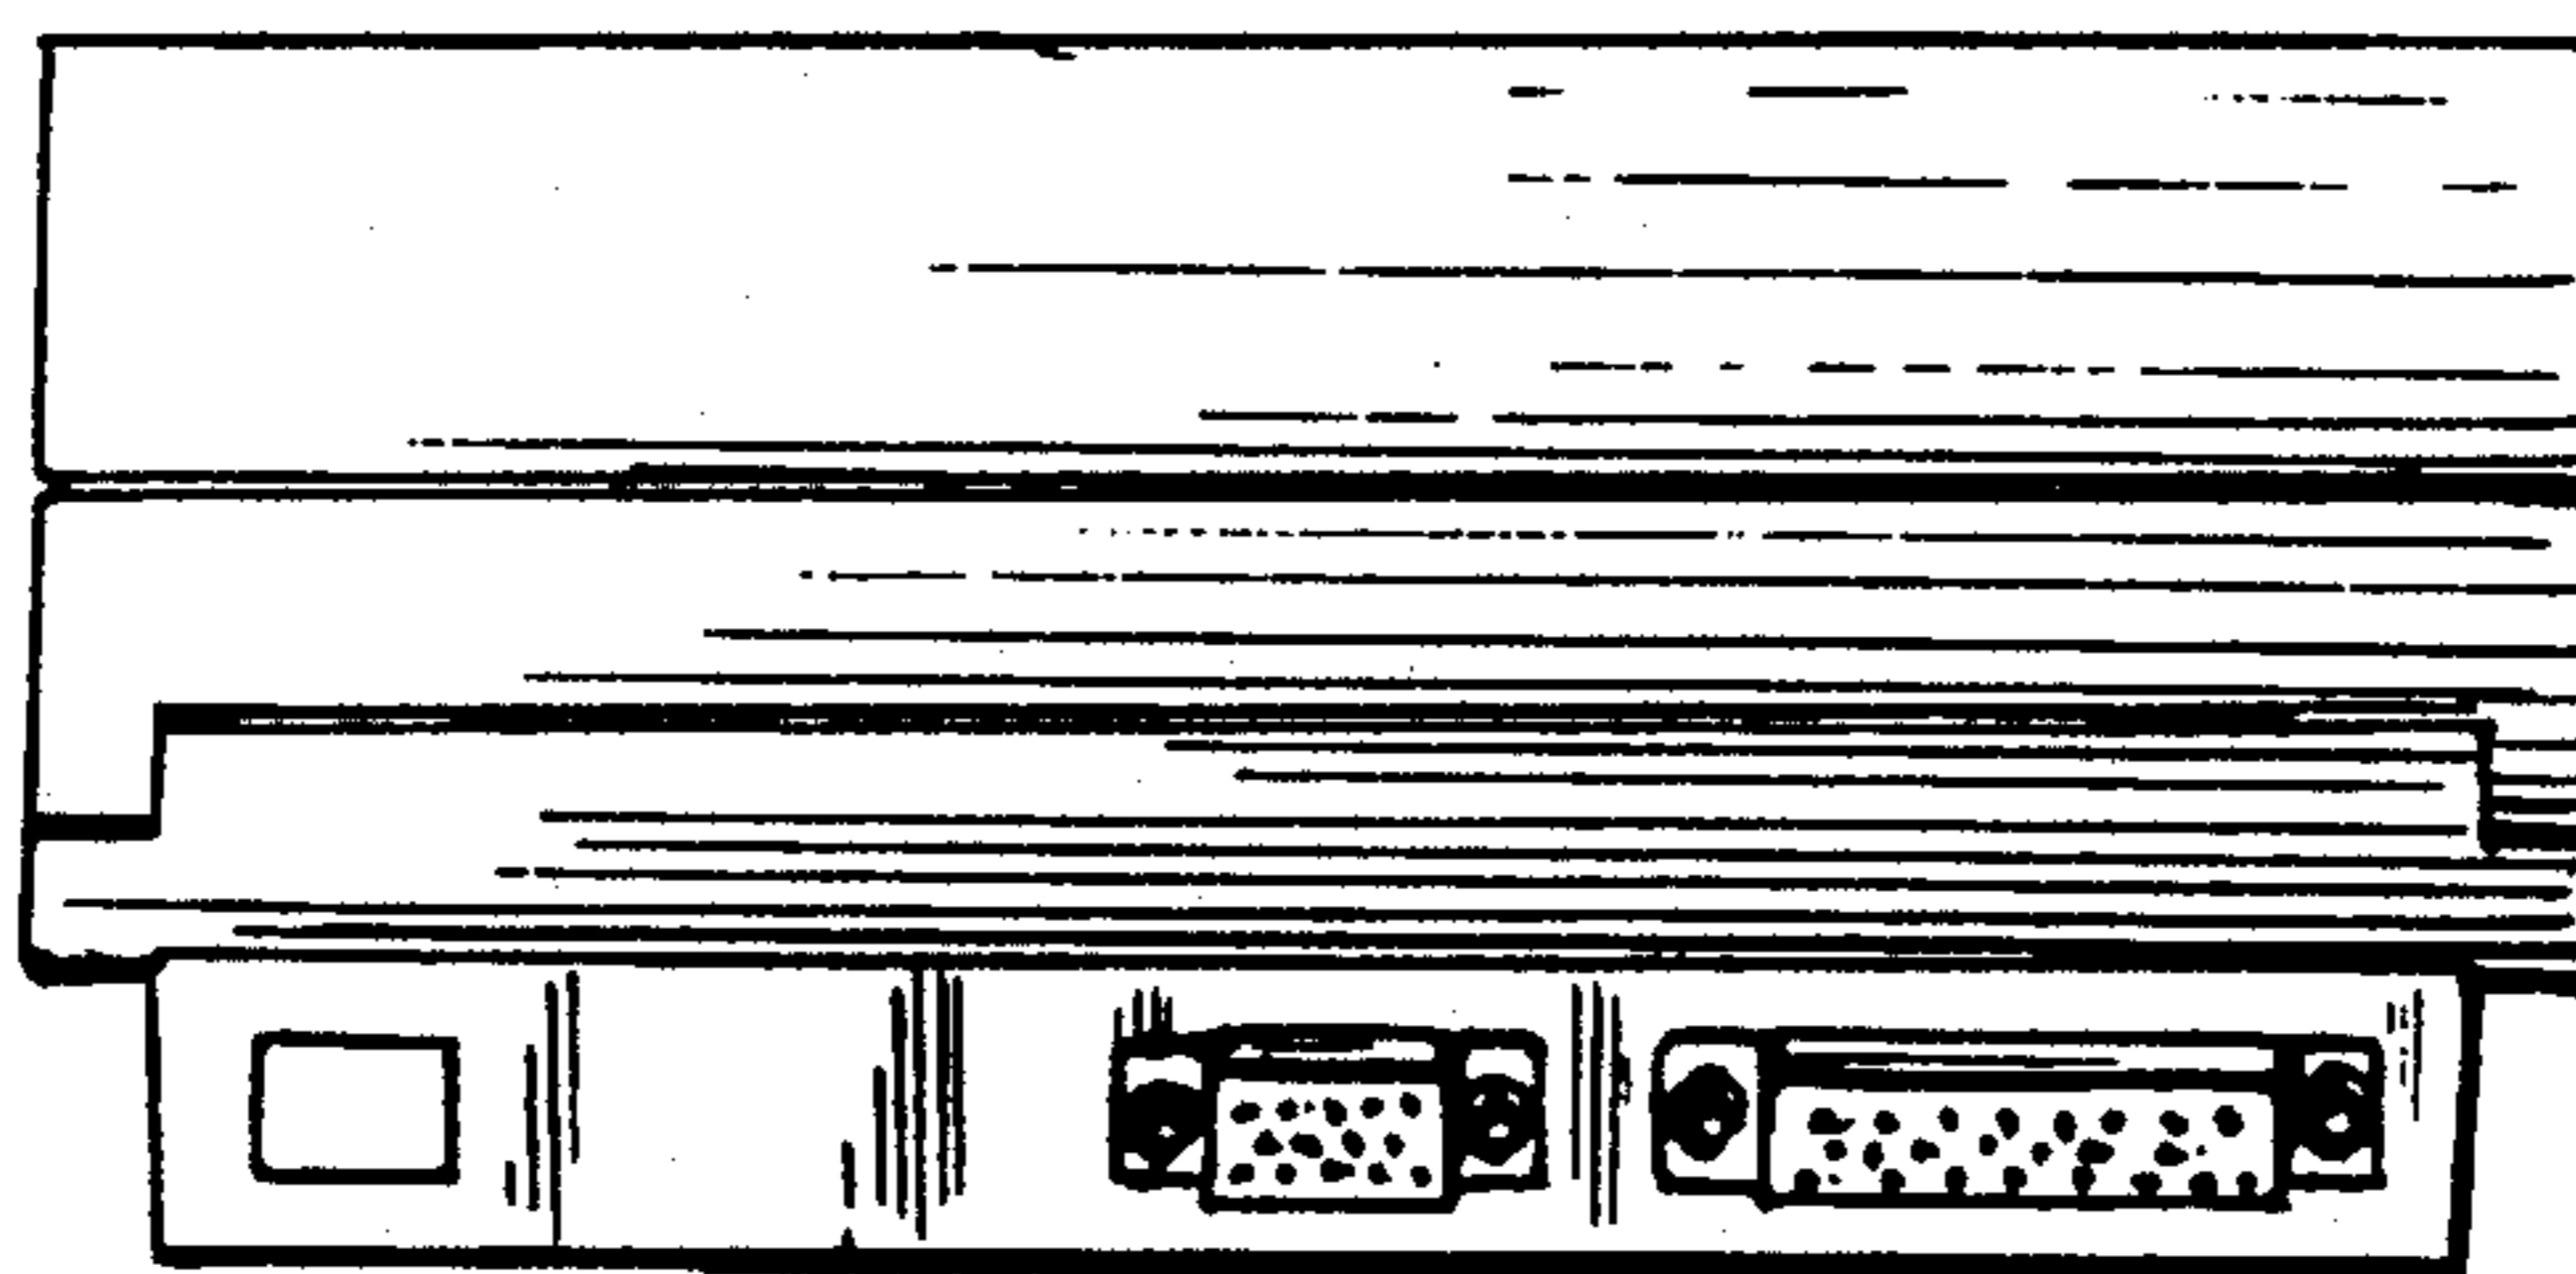


FIG. 5

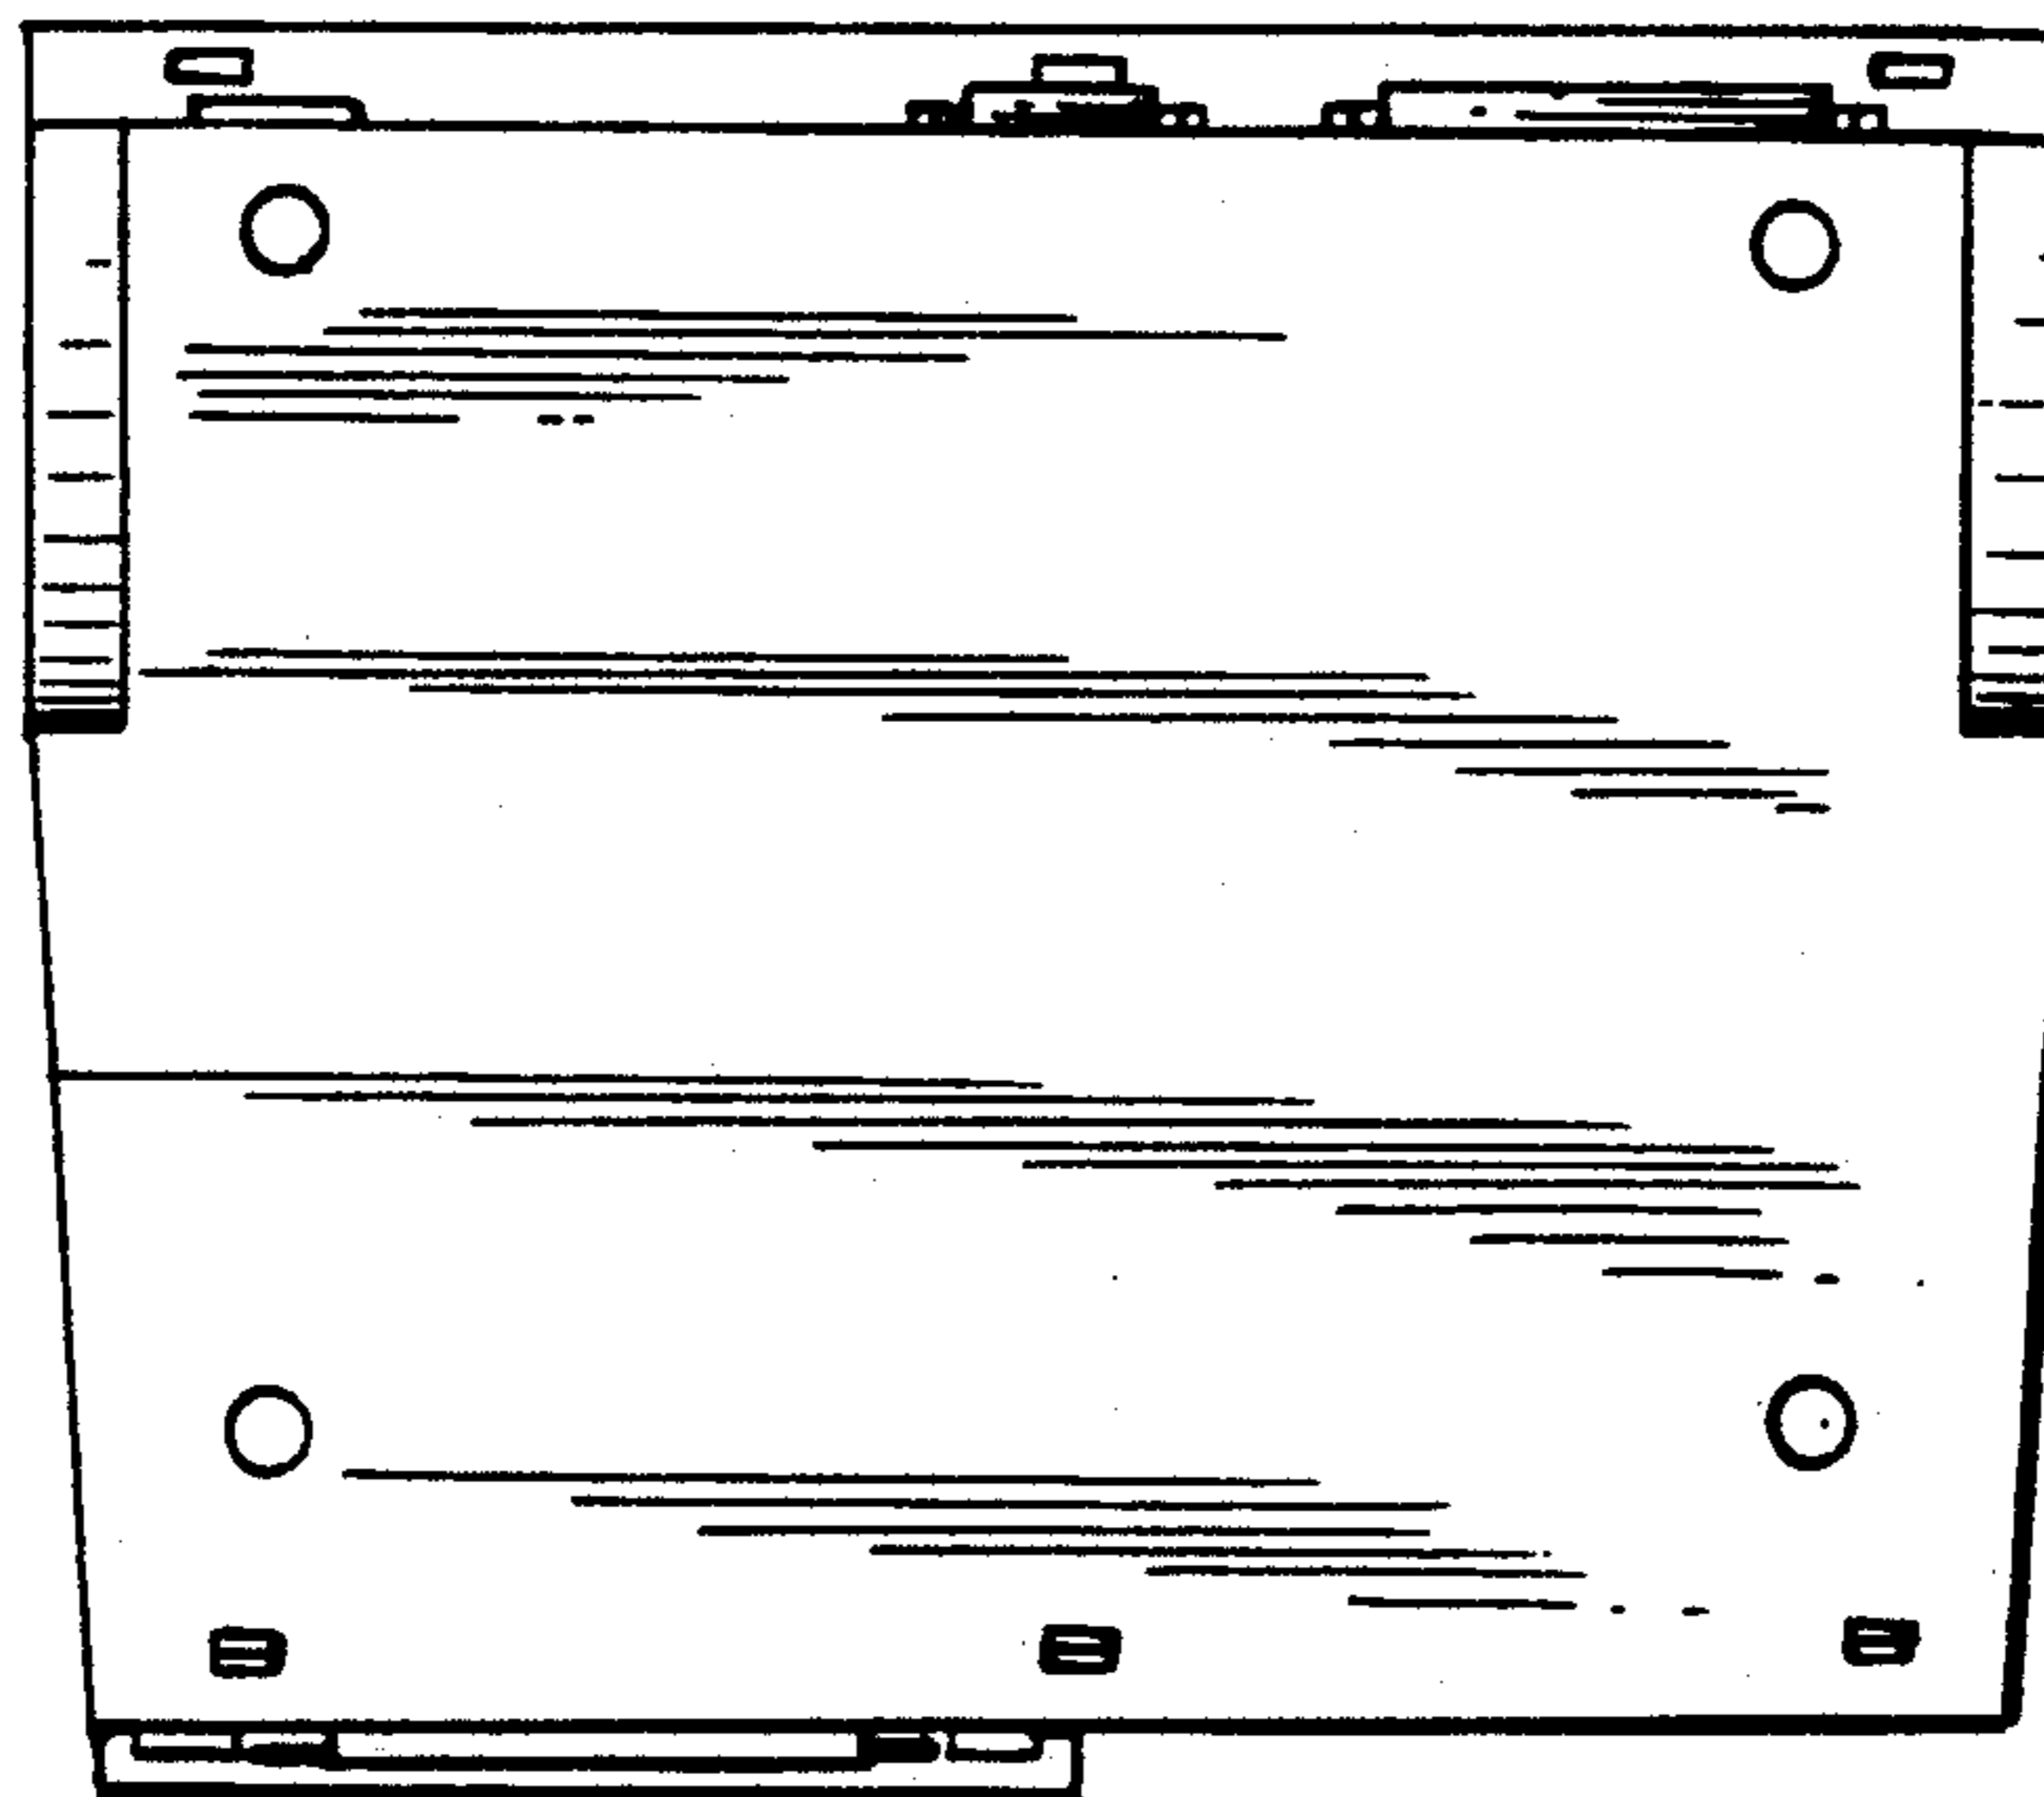


FIG. 6

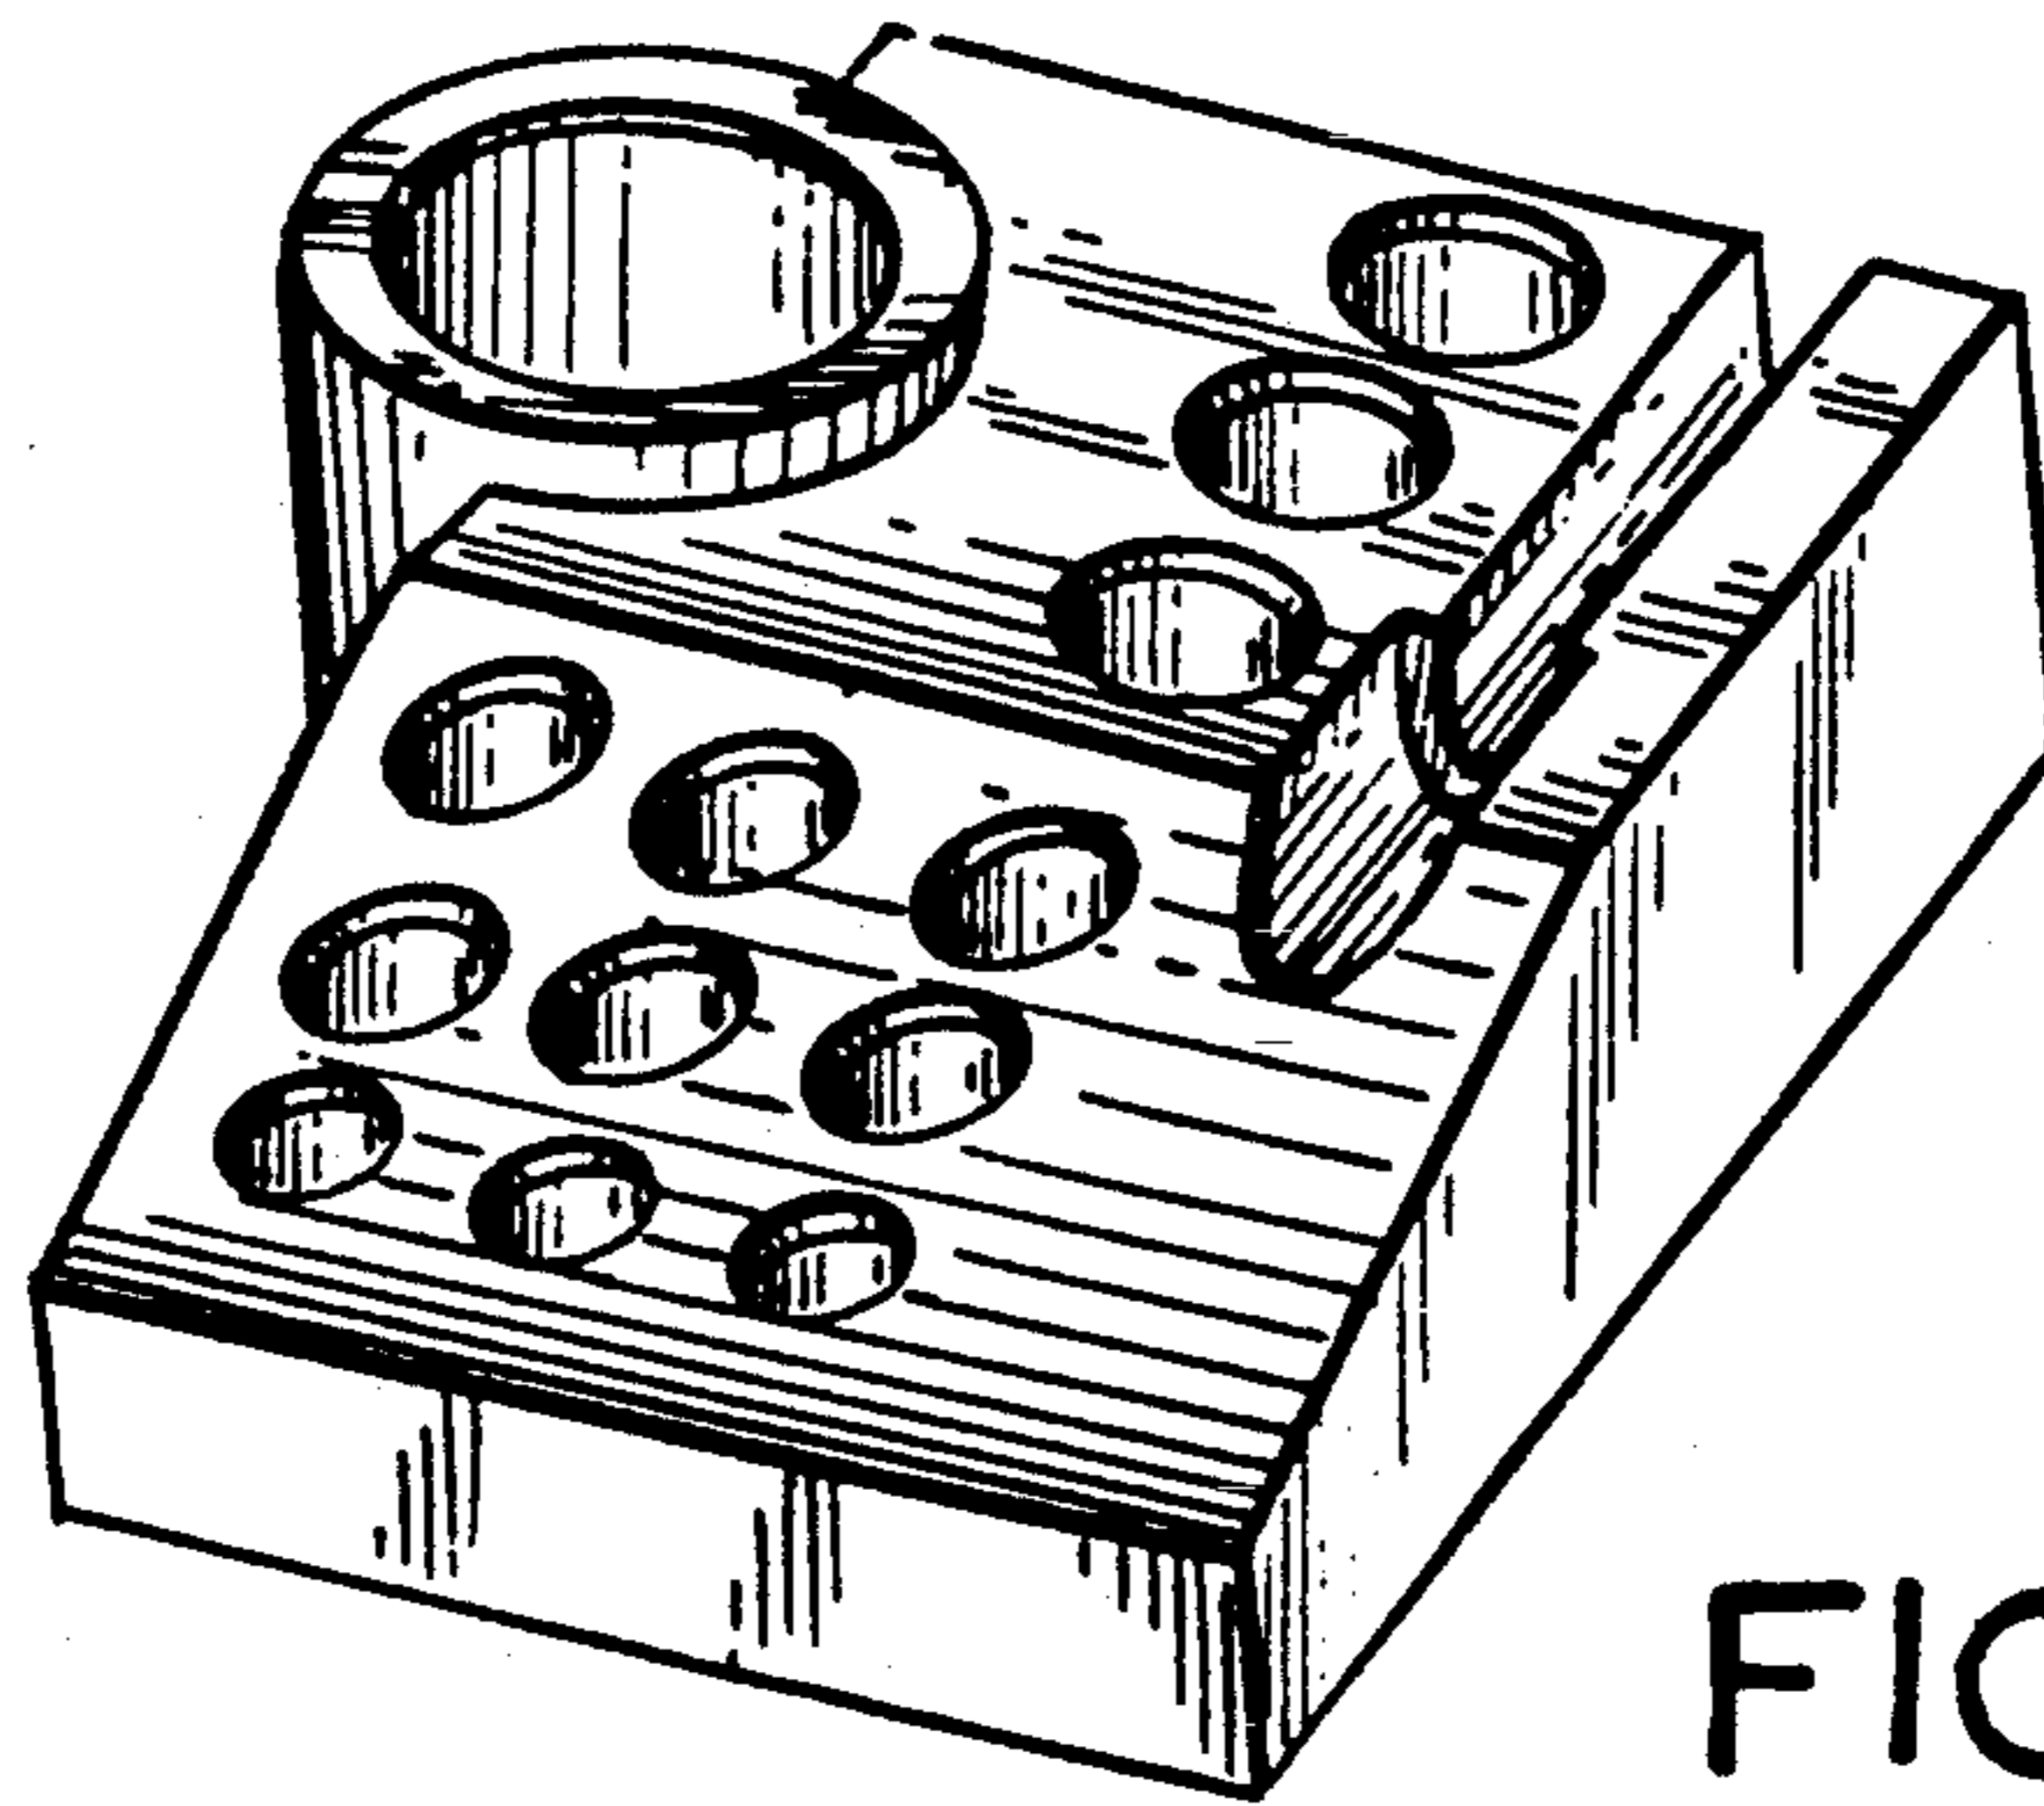


FIG. 7

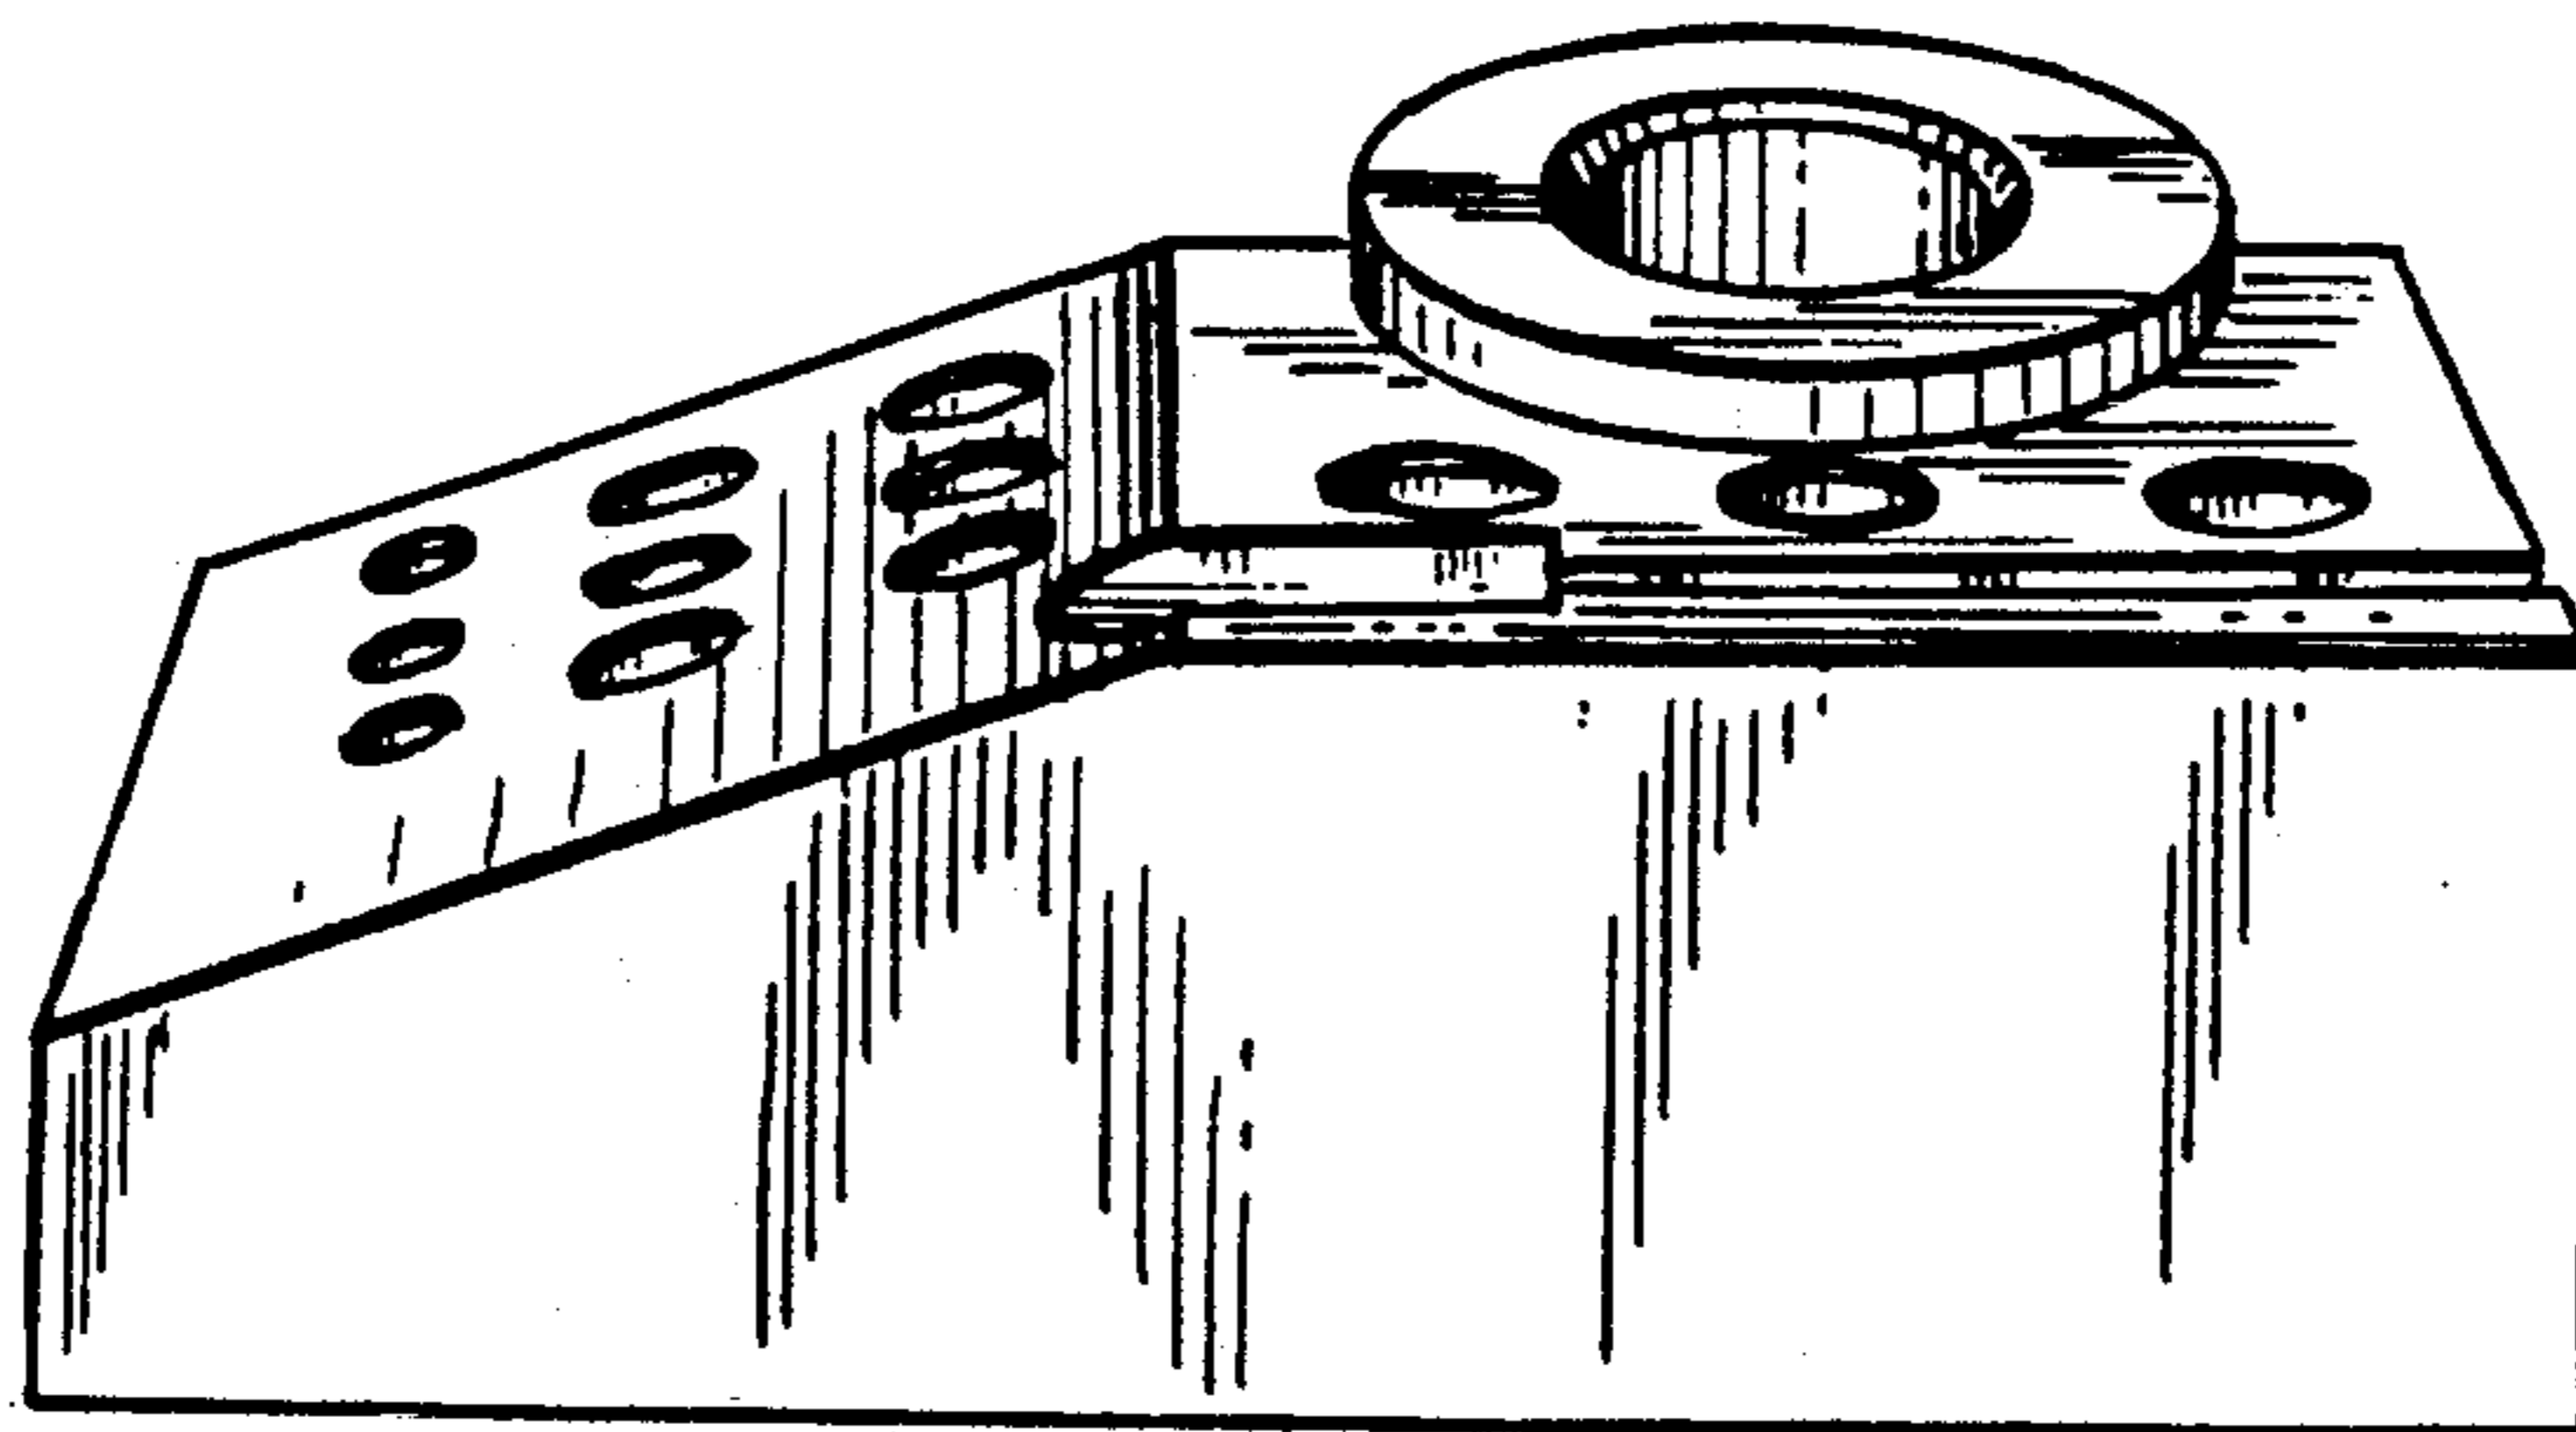


FIG. 8

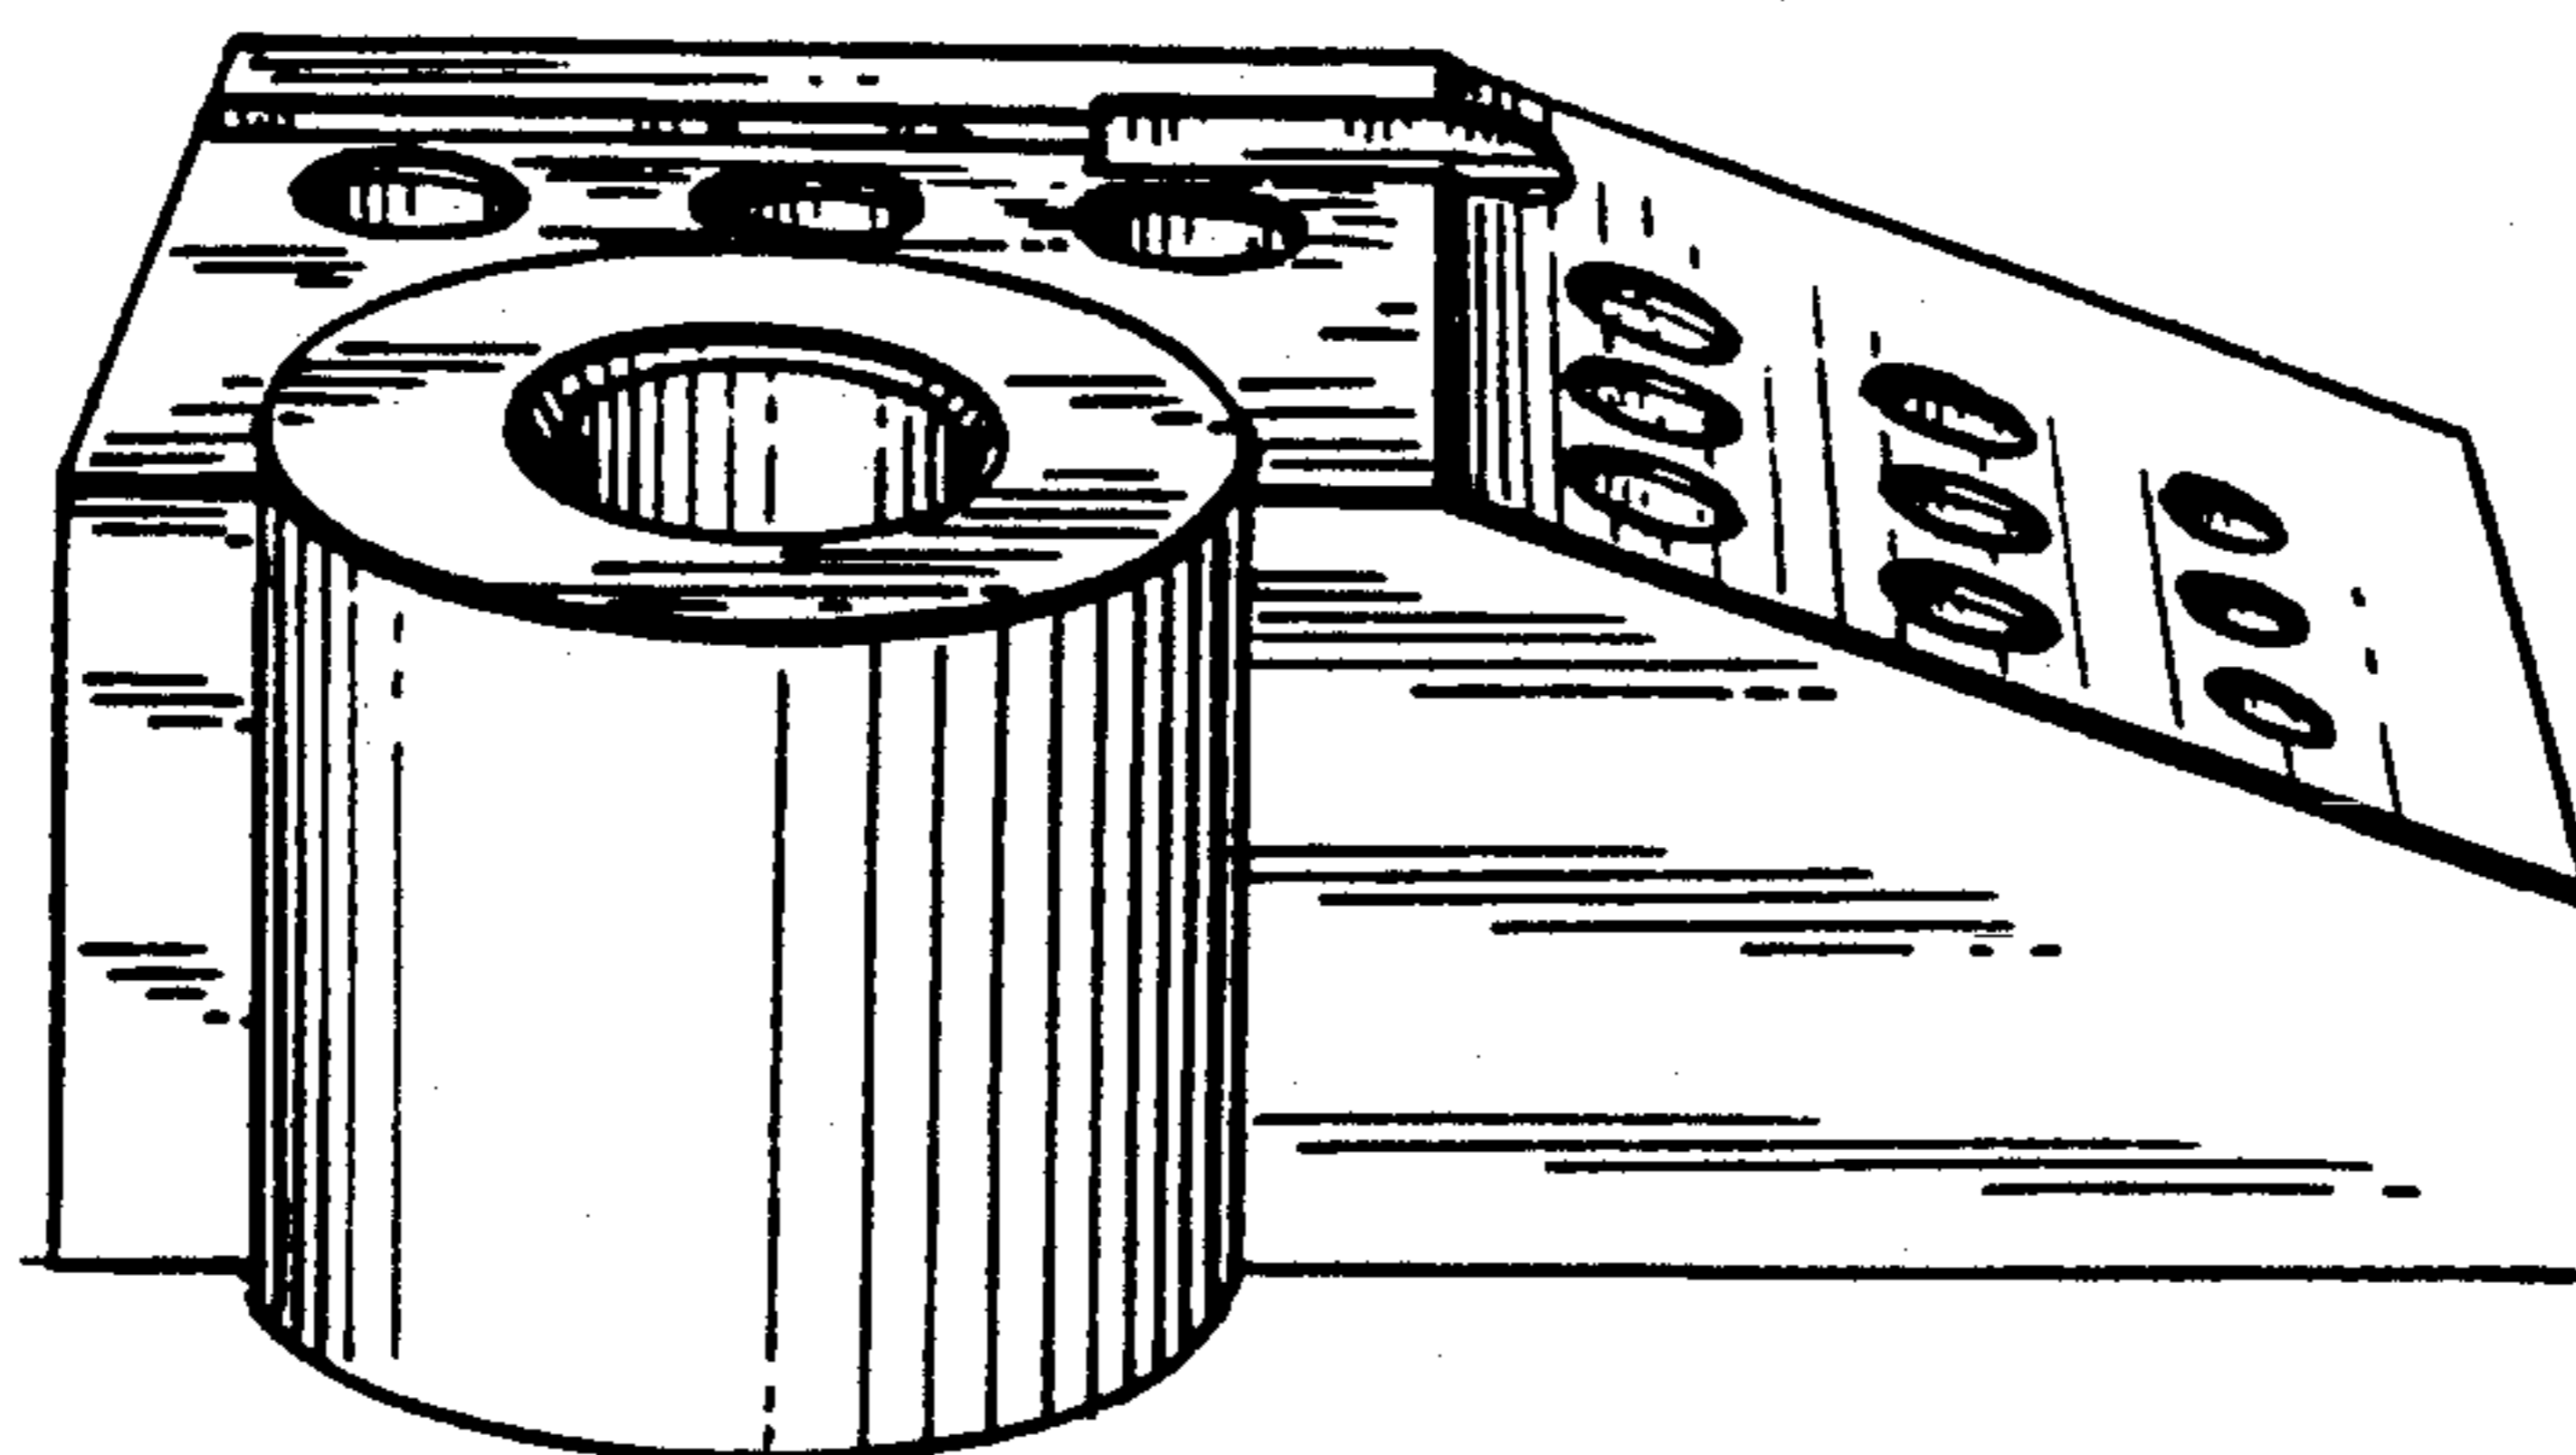


FIG. 9

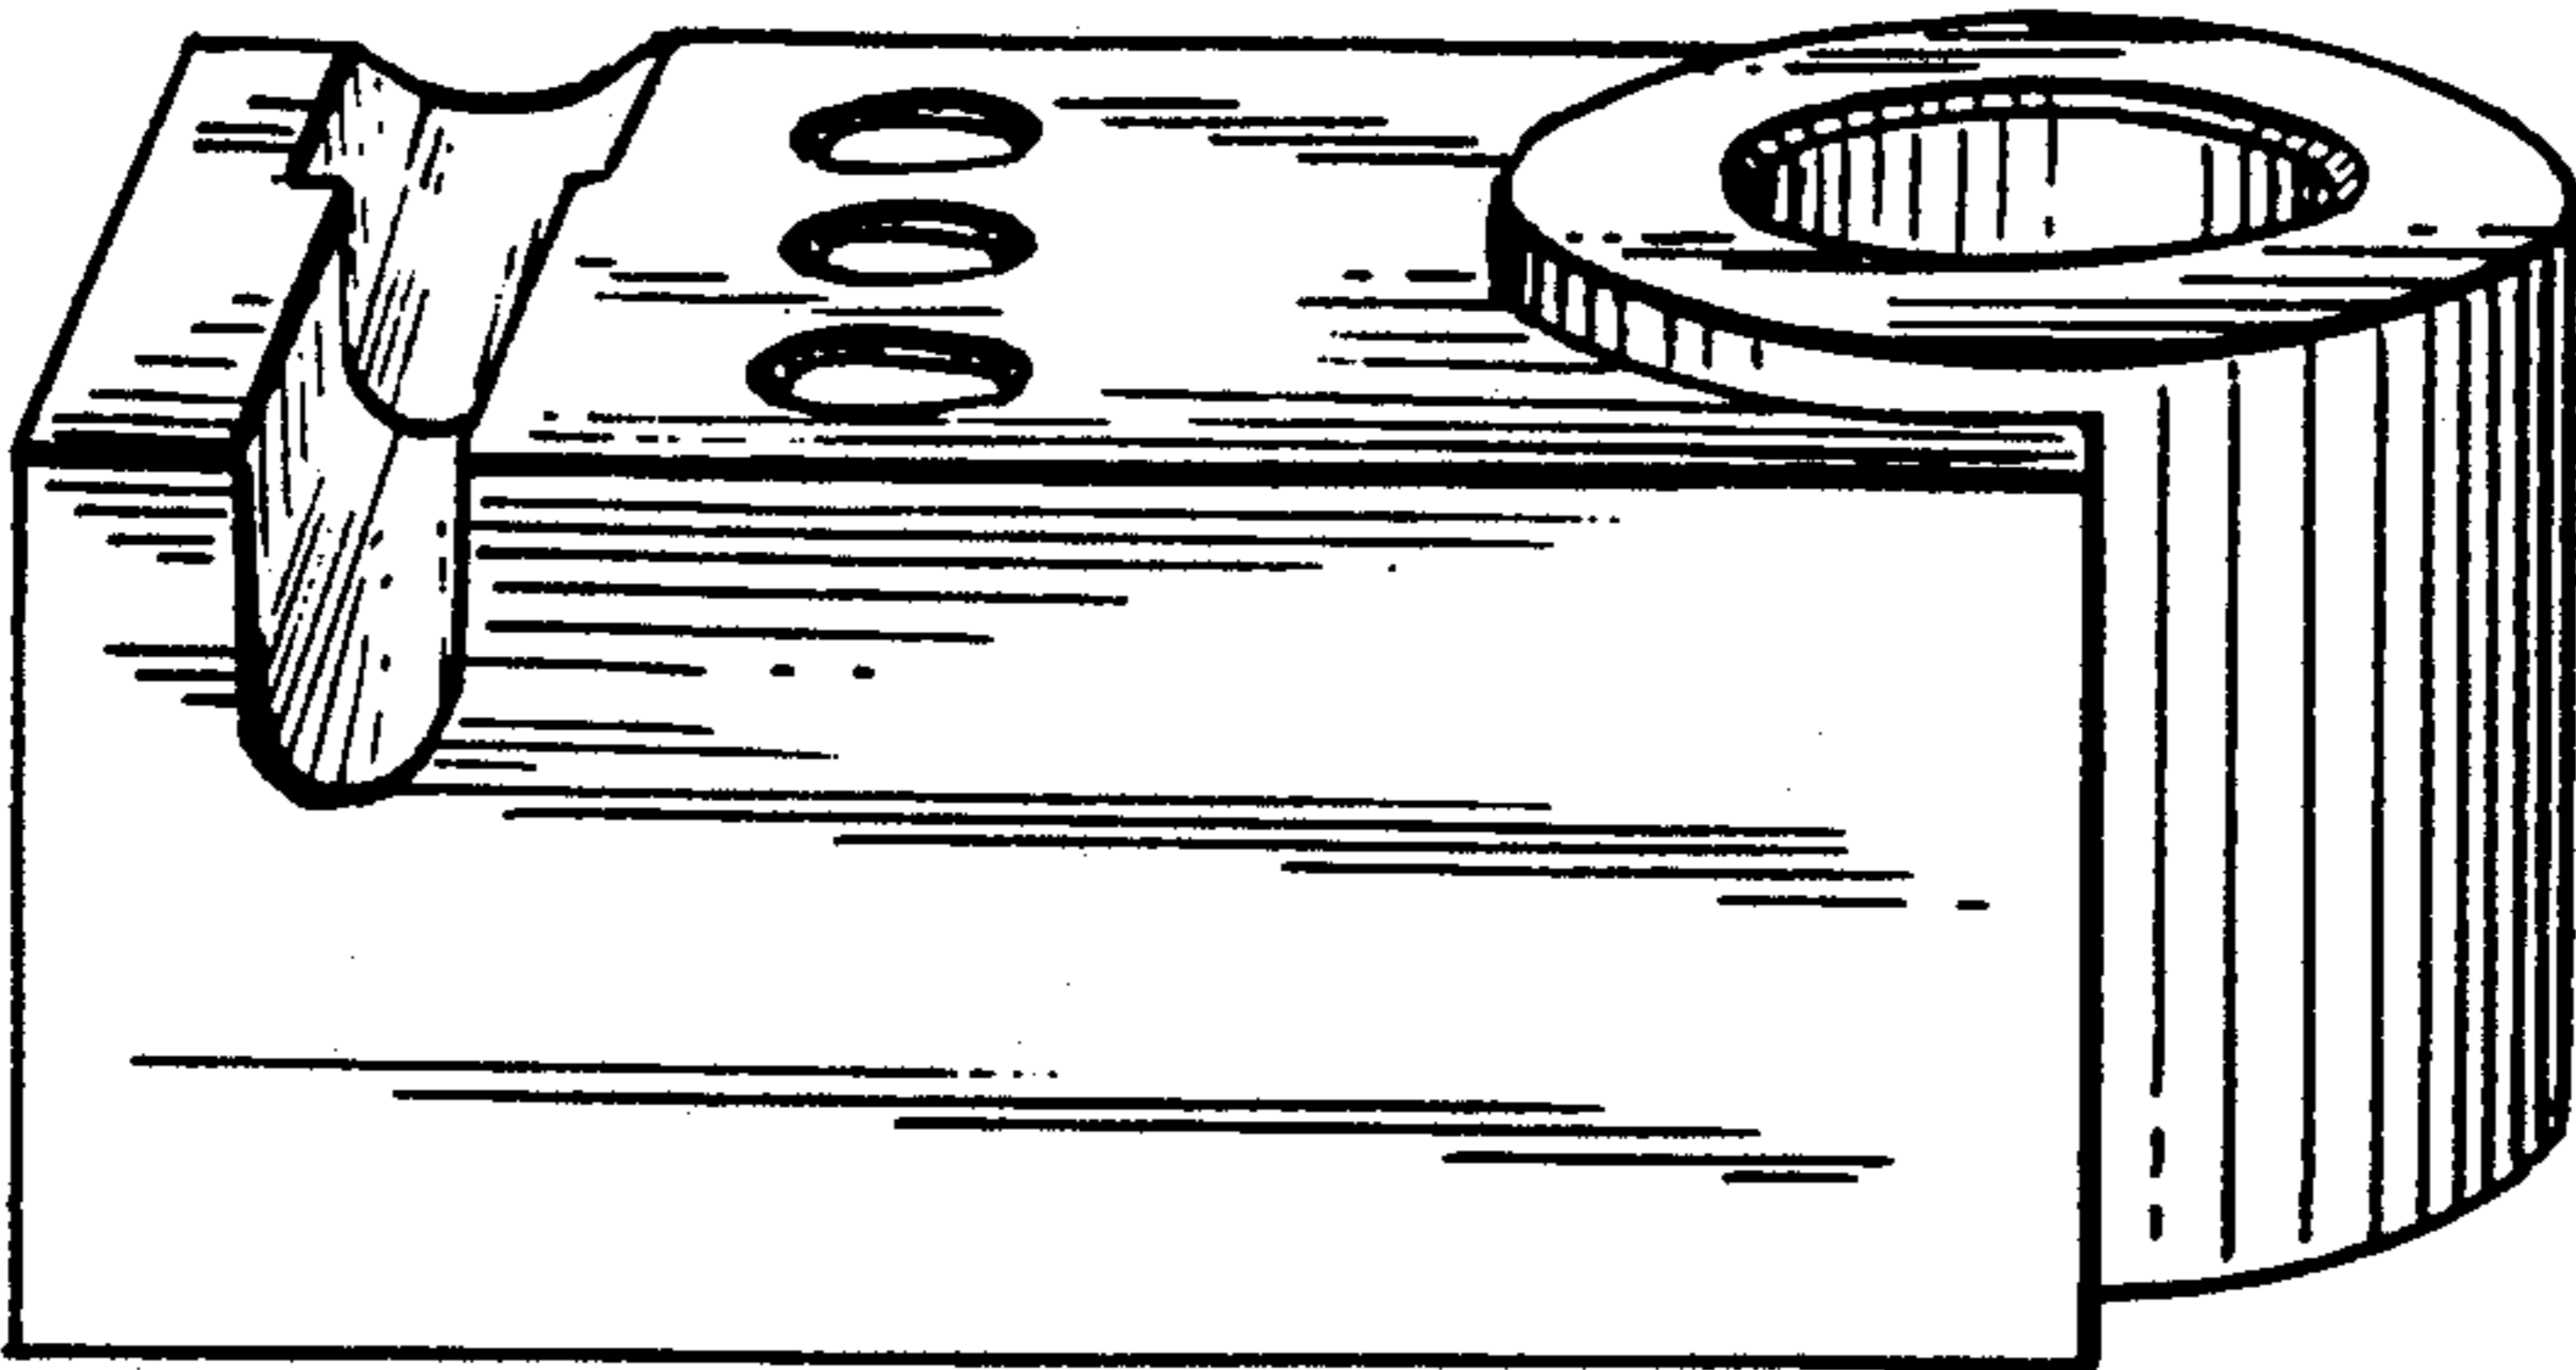


FIG. 10

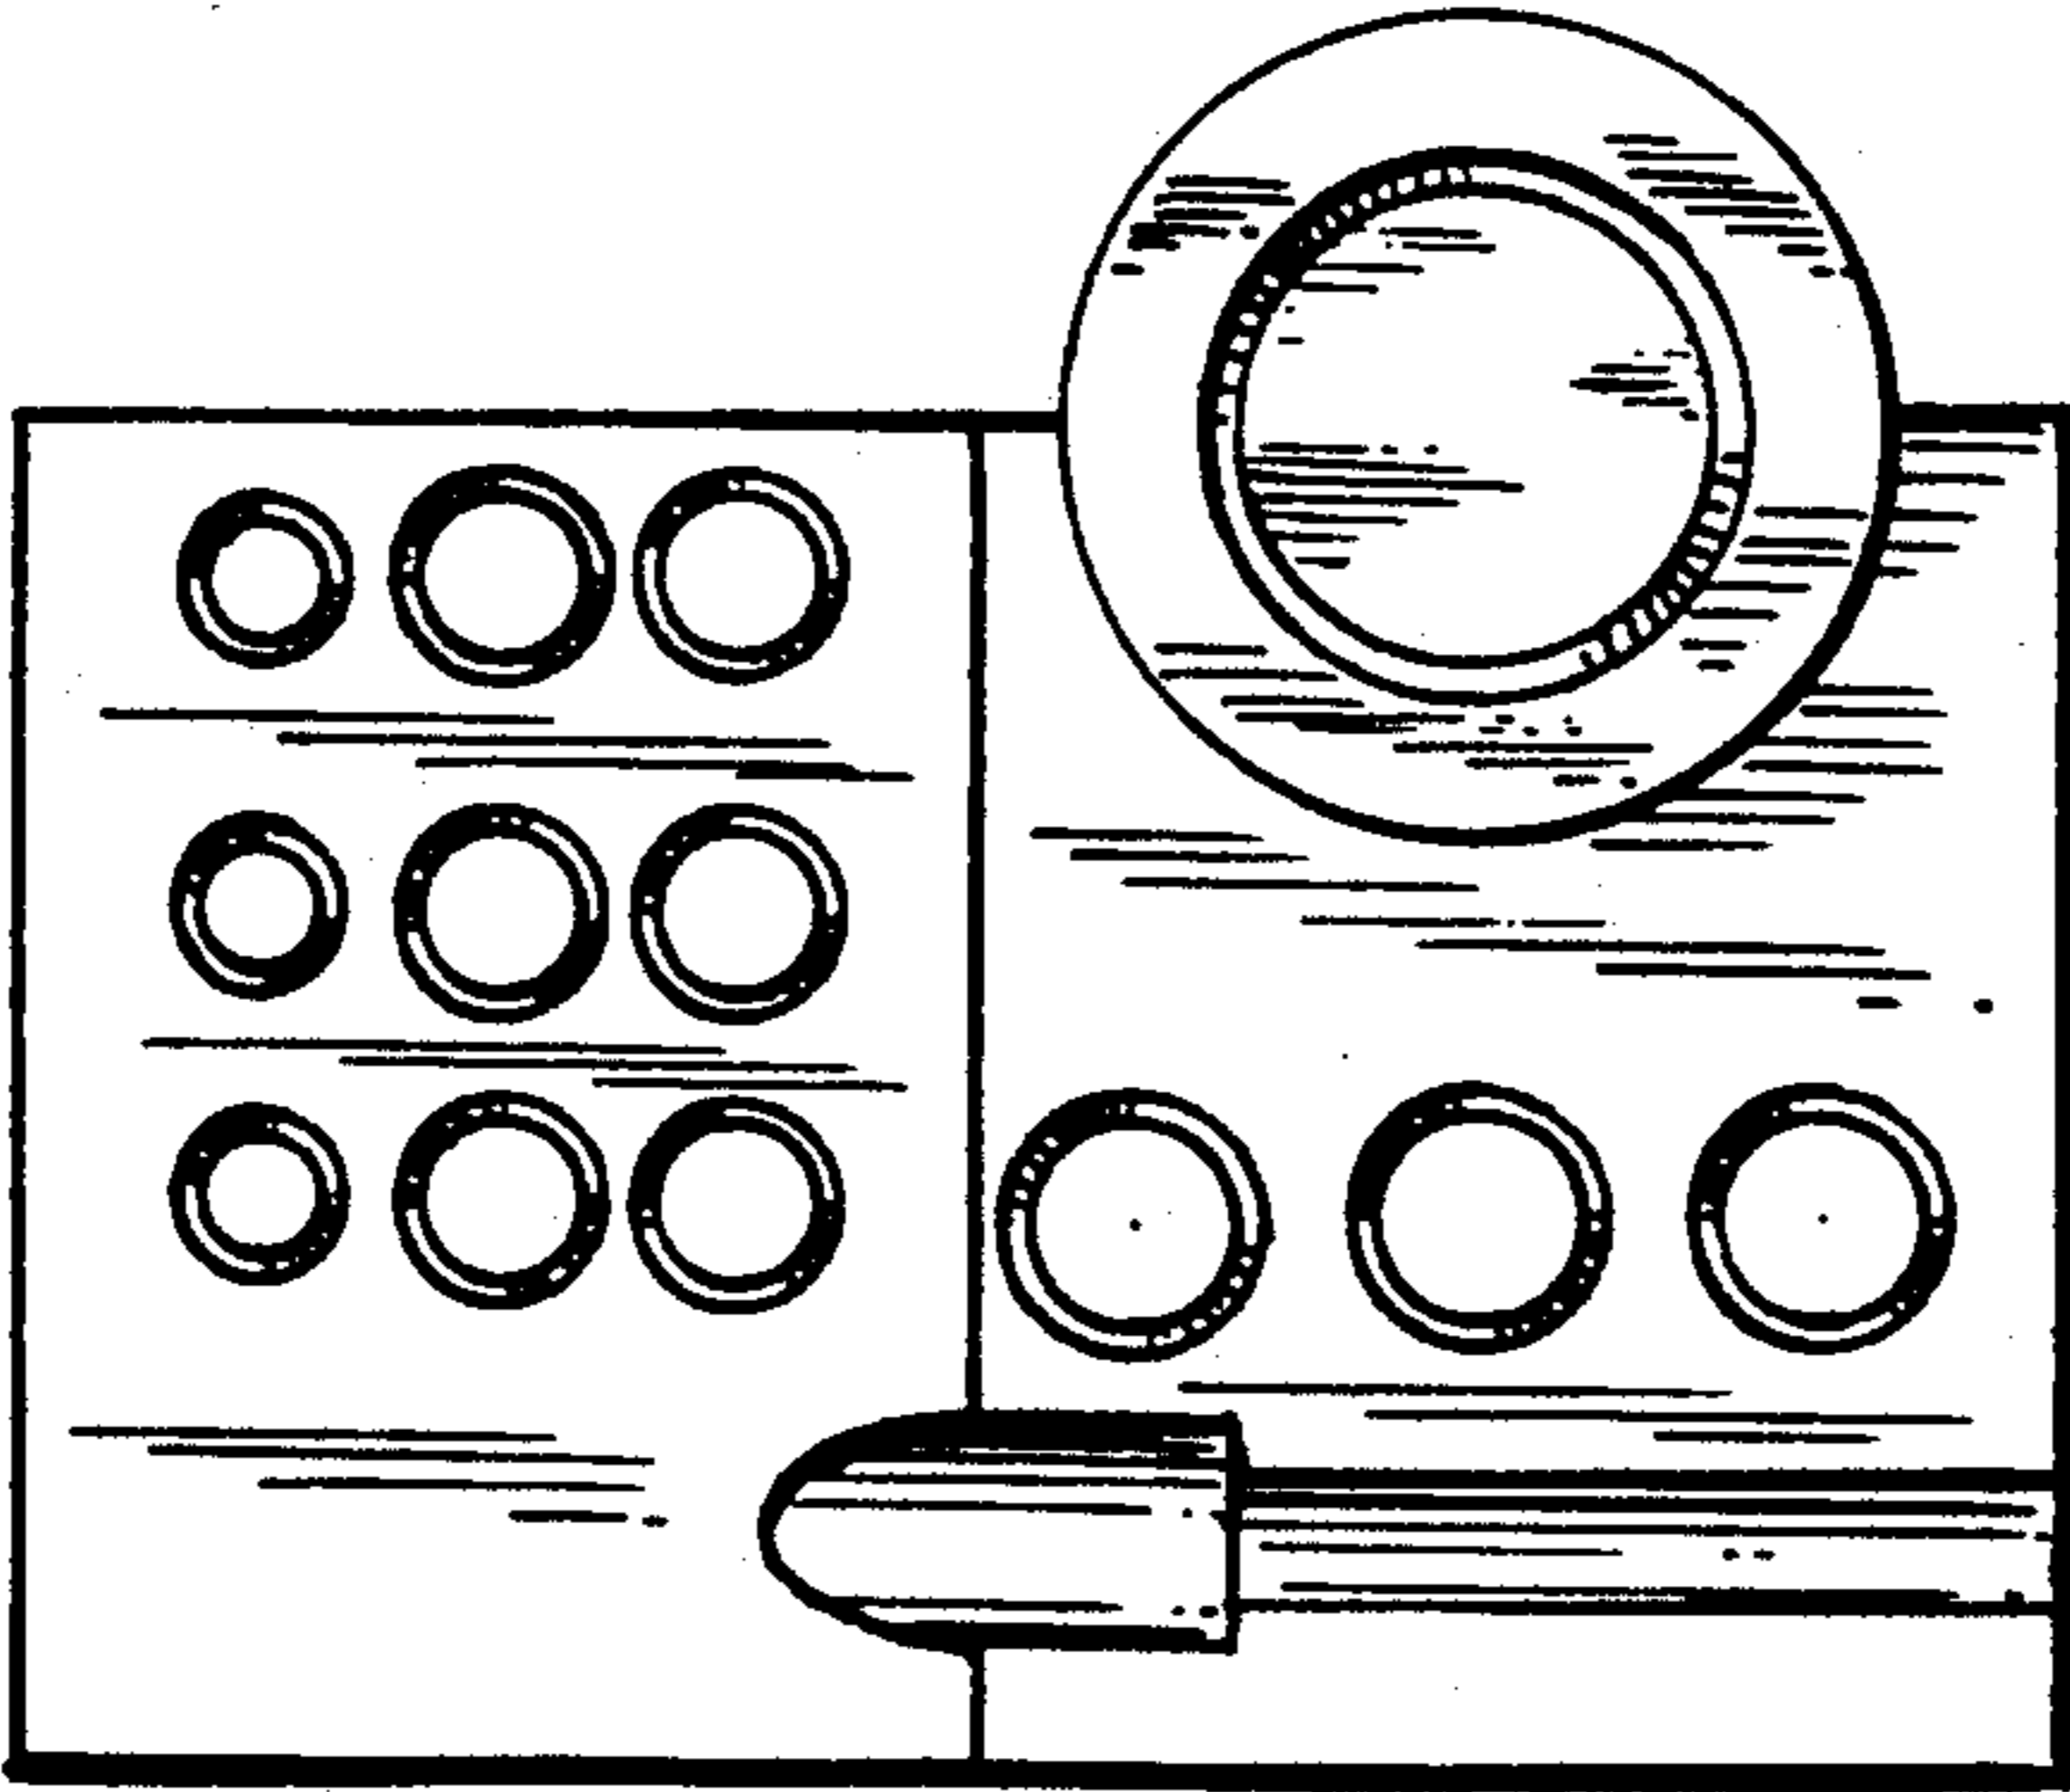


FIG. 11

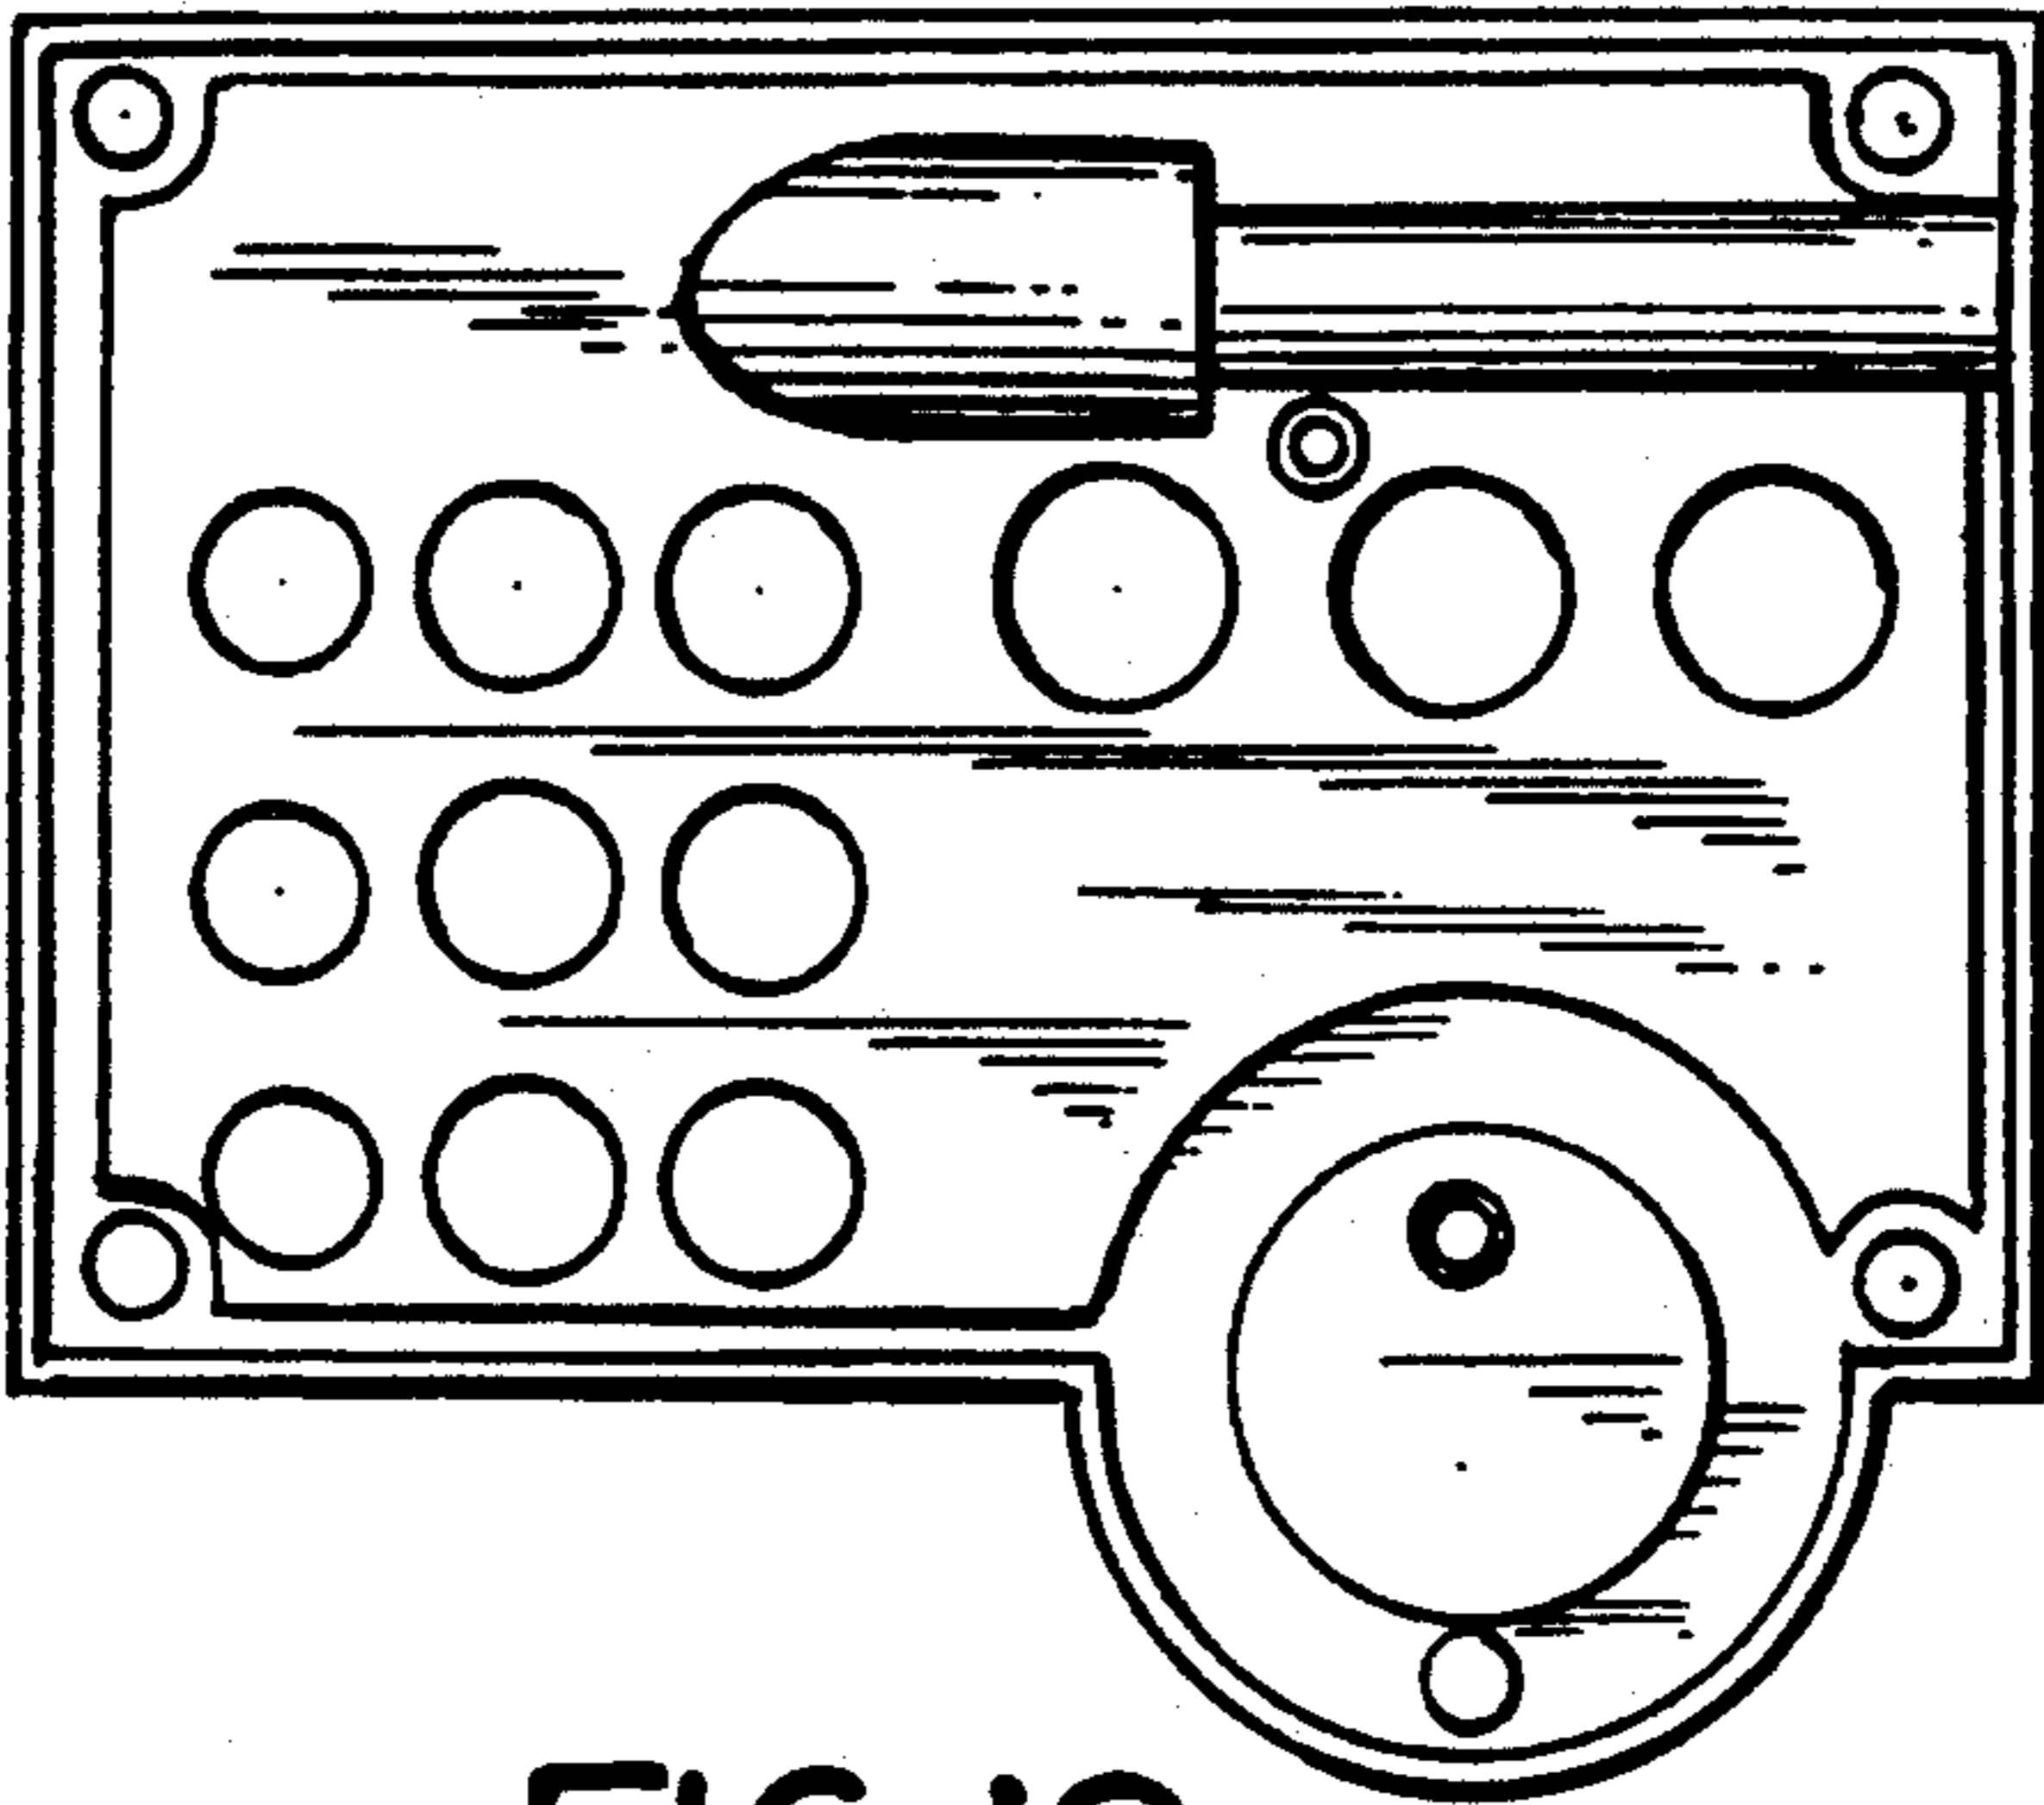


FIG. 12

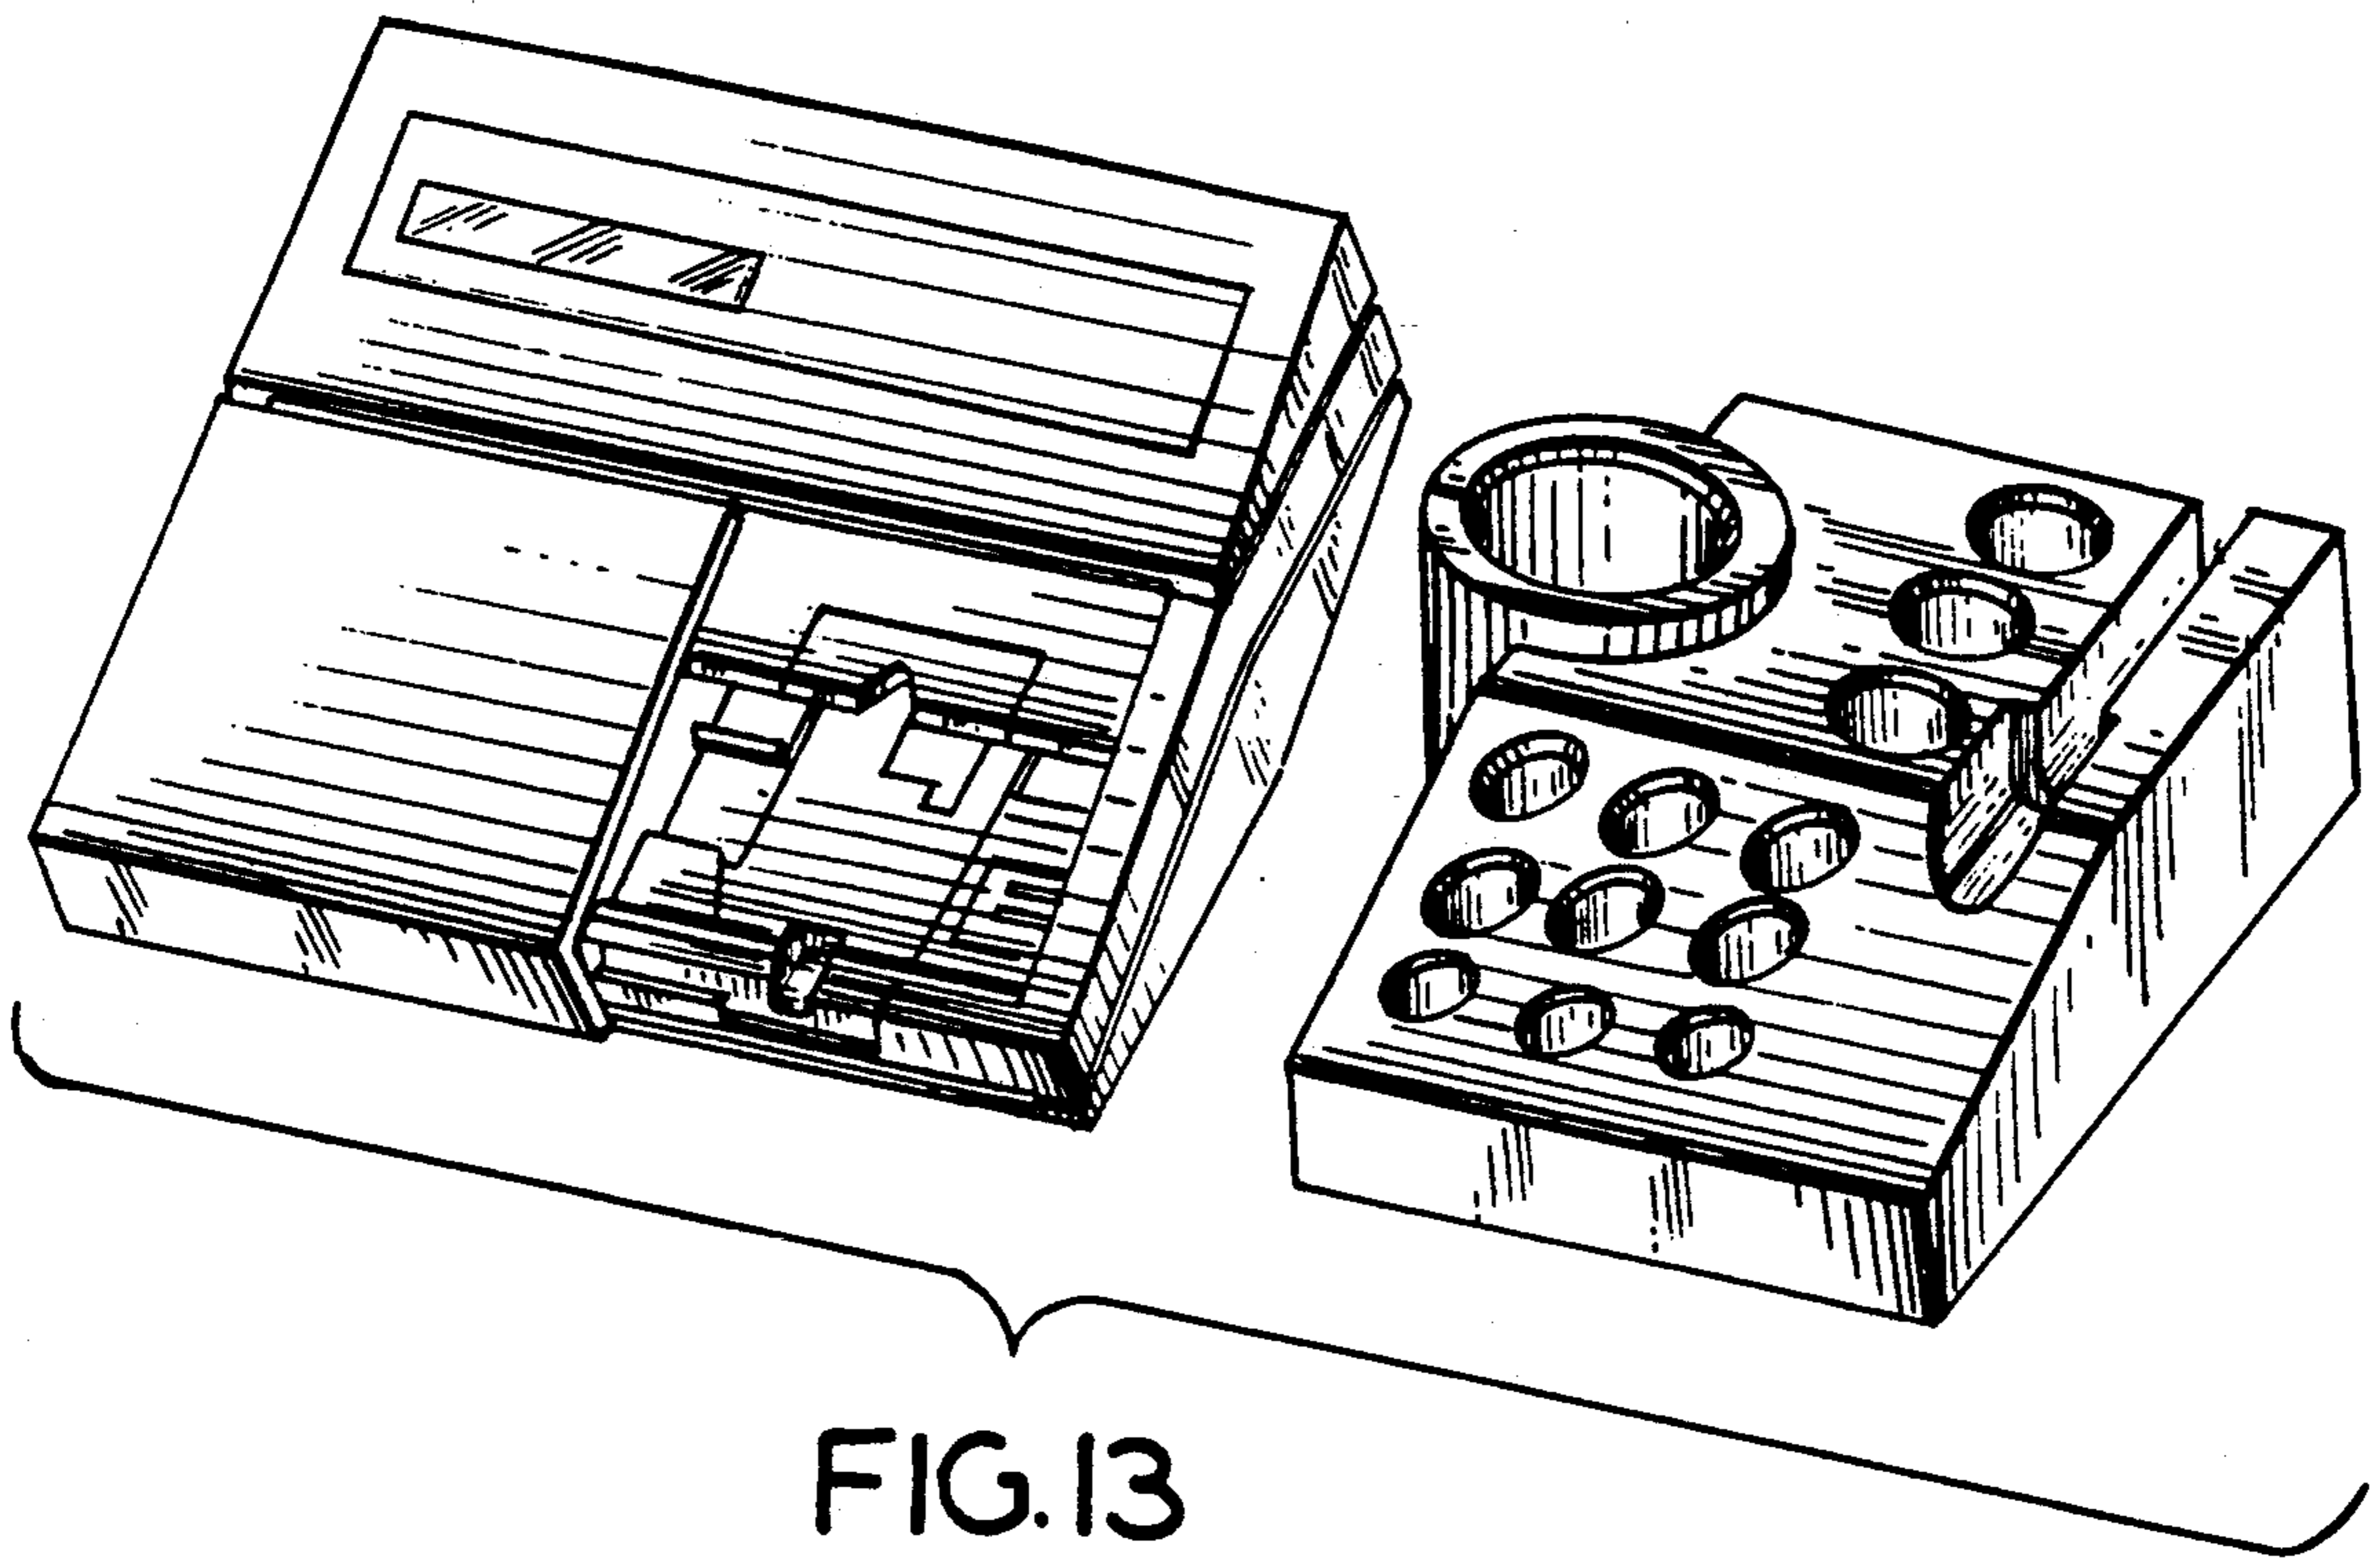


FIG. 13