



US00D339639S

United States Patent [19]

[11] Patent Number: **Des. 339,639**

Ohnuma et al.

[45] Date of Patent: **** Sep. 21, 1993**

[54] **BIOCHEMICAL ANALYZER**

[56] **References Cited**

[75] Inventors: **Mitsuru Ohnuma, Tokyo; Kazunori Hashimoto, Tachikawa; Hiroshi Mitsumaki, Mito; Katsuaki Takahashi, Katsuta, all of Japan**

U.S. PATENT DOCUMENTS

D. 264,873	6/1982	Olson et al.	D24/232 X
D. 314,049	1/1991	Katayama	D24/232 X
D. 319,100	8/1991	Umemoto et al.	D24/232 X
4,781,891	11/1988	Galle et al.	422/65 X
5,130,095	7/1992	Ricchio et al.	422/63

[73] Assignee: **Hitachi, Ltd., Tokyo, Japan**

Primary Examiner—A. Hugo Word
Assistant Examiner—Ian Simmons
Attorney, Agent, or Firm—Antonelli, Terry, Stout & Kraus

[**] Term: **14 Years**

[57] CLAIM

[21] Appl. No.: **659,152**

The ornamental design for a biochemical analyzer, as shown.

[22] Filed: **Feb. 22, 1991**

DESCRIPTION

[30] Foreign Application Priority Data

Jan. 25, 1991 [JP] Japan 3-300598

[52] U.S. Cl. **D24/232; D24/186; D24/231**

[58] Field of Search **D24/186, 216, 231, 160, D24/232, 185; D10/81; 422/63, 64, 66, 67, 68.1, 99, 105, 65; 436/43**

FIG. 1 is a front top right side perspective view of a biochemical analyzer showing our new design; FIG. 2 is a front elevational view thereof; FIG. 3 is a top plan elevational view thereof; FIG. 4 is a right side elevational view thereof; FIG. 5 is a rear elevational view thereof; FIG. 6 is a bottom plan view thereof; and, FIG. 7 is a perspective view thereof, with the cover in open condition.

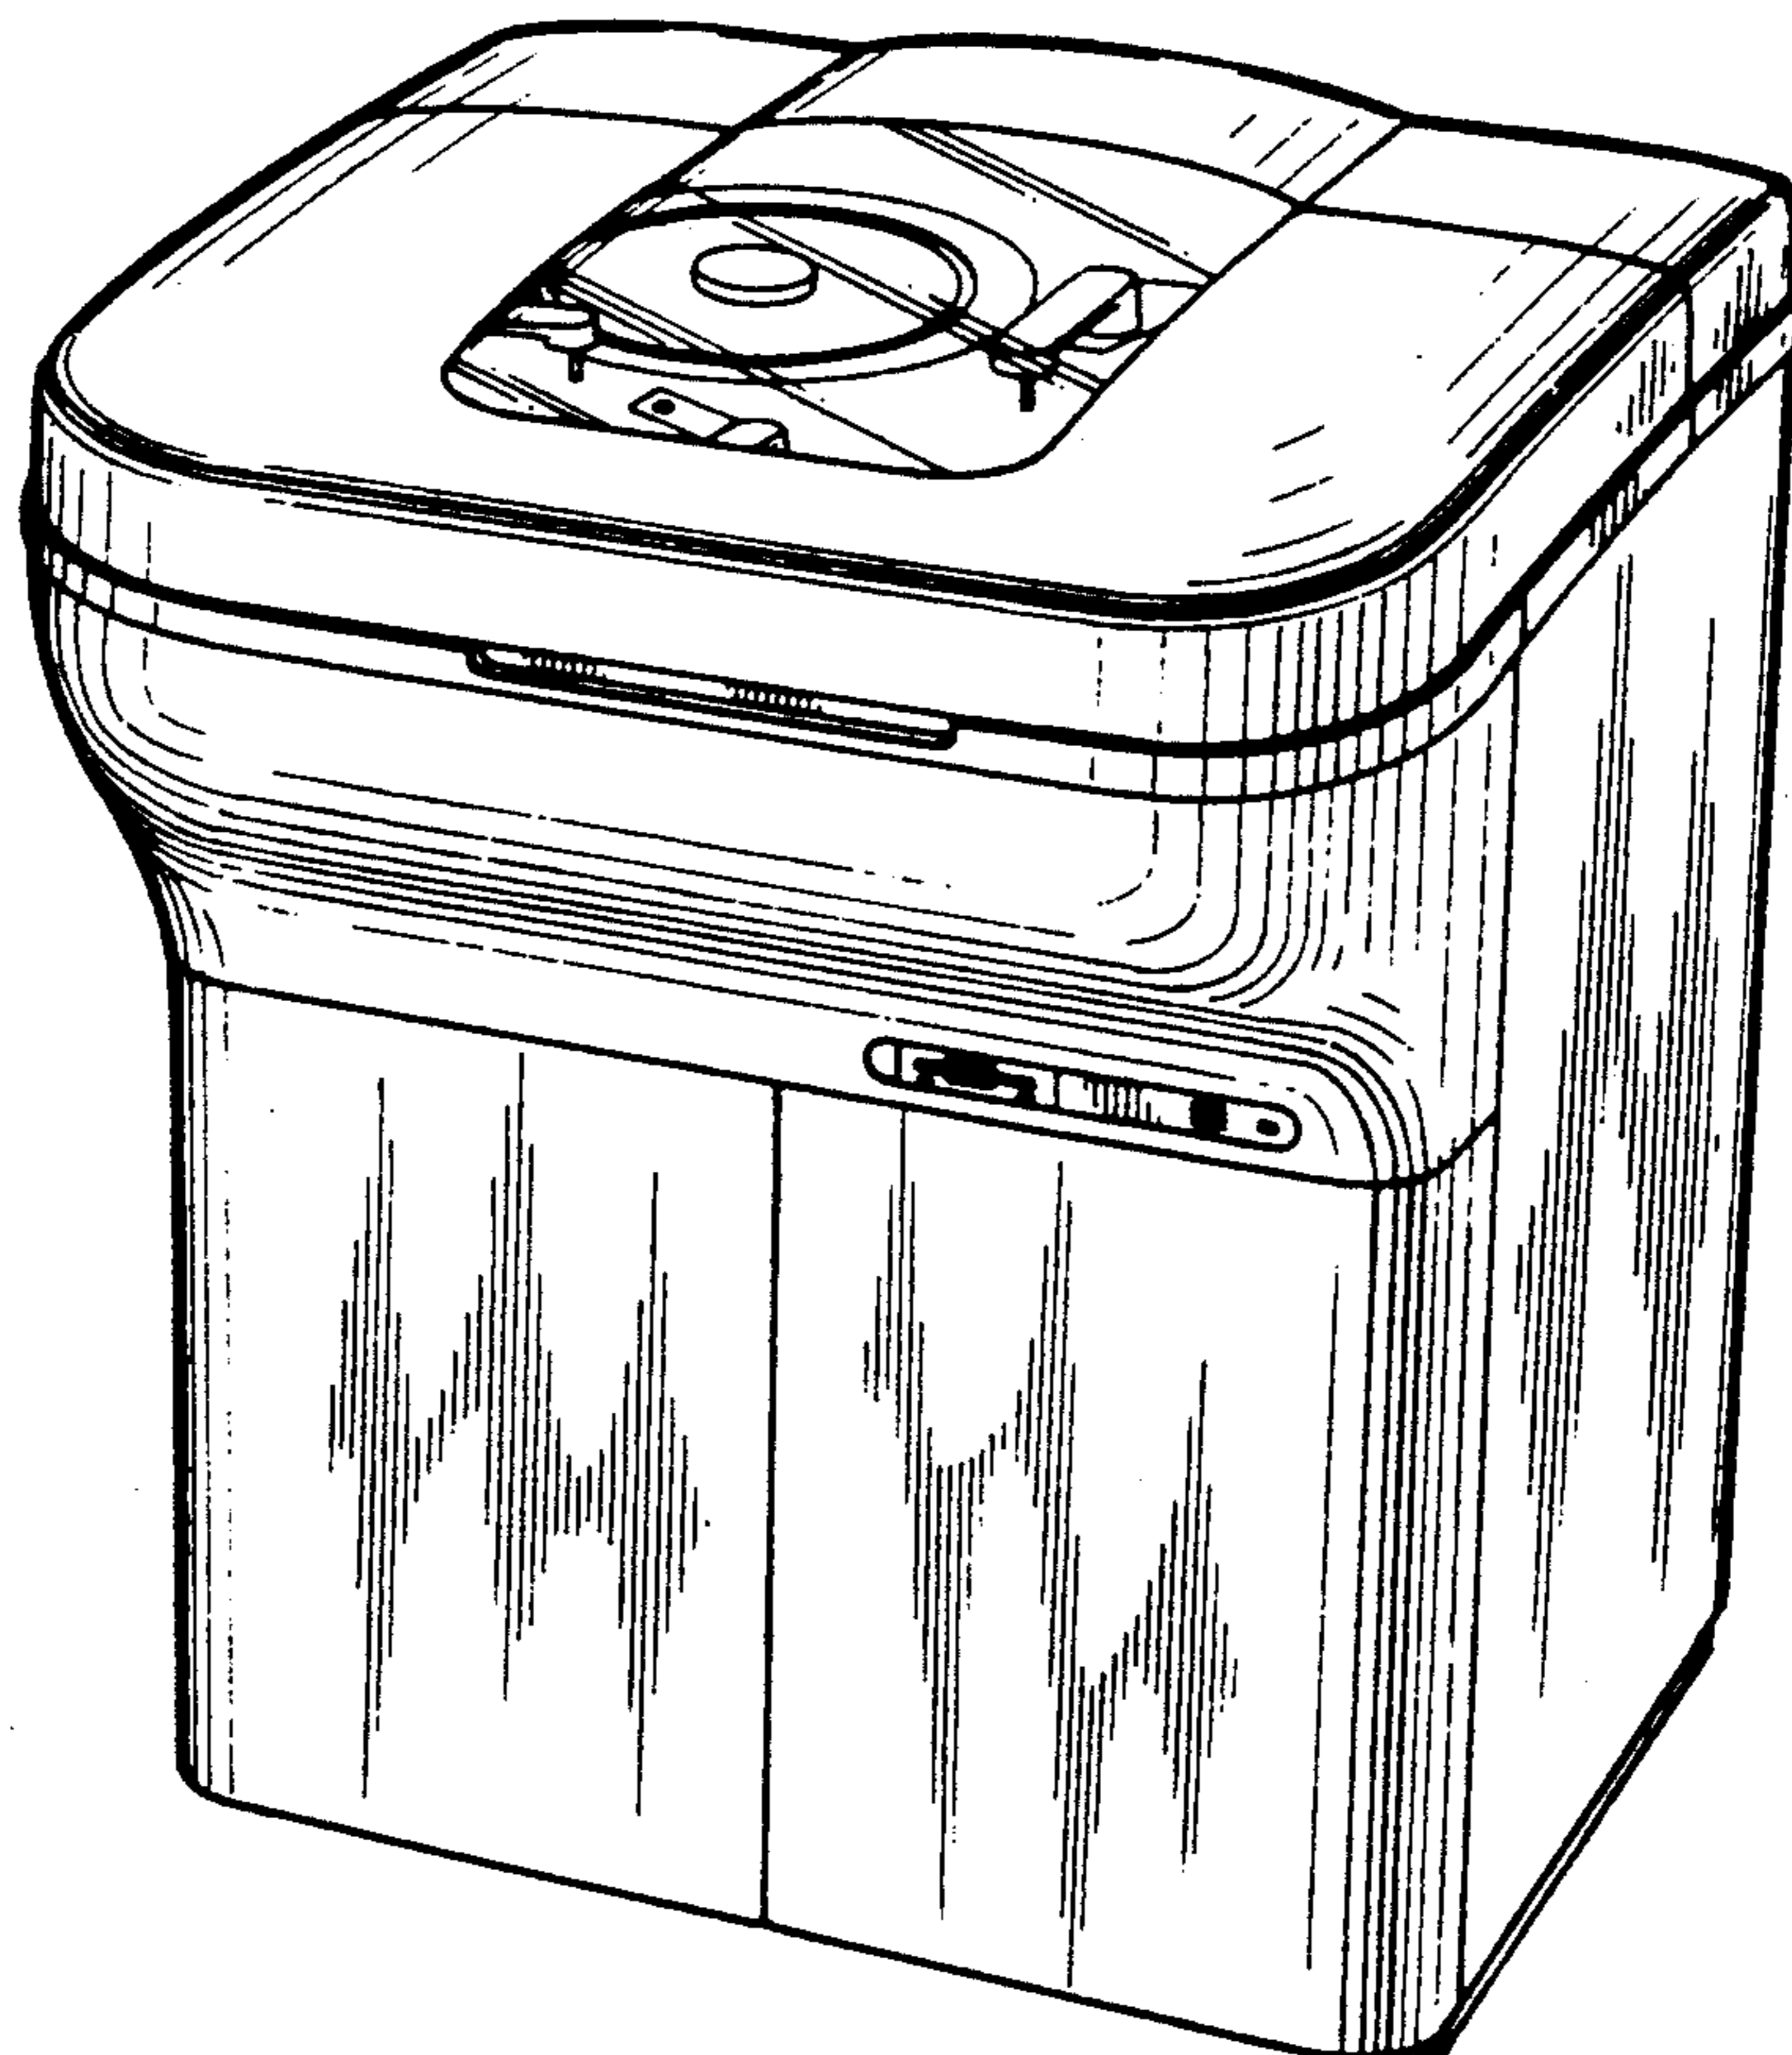


FIG. 1

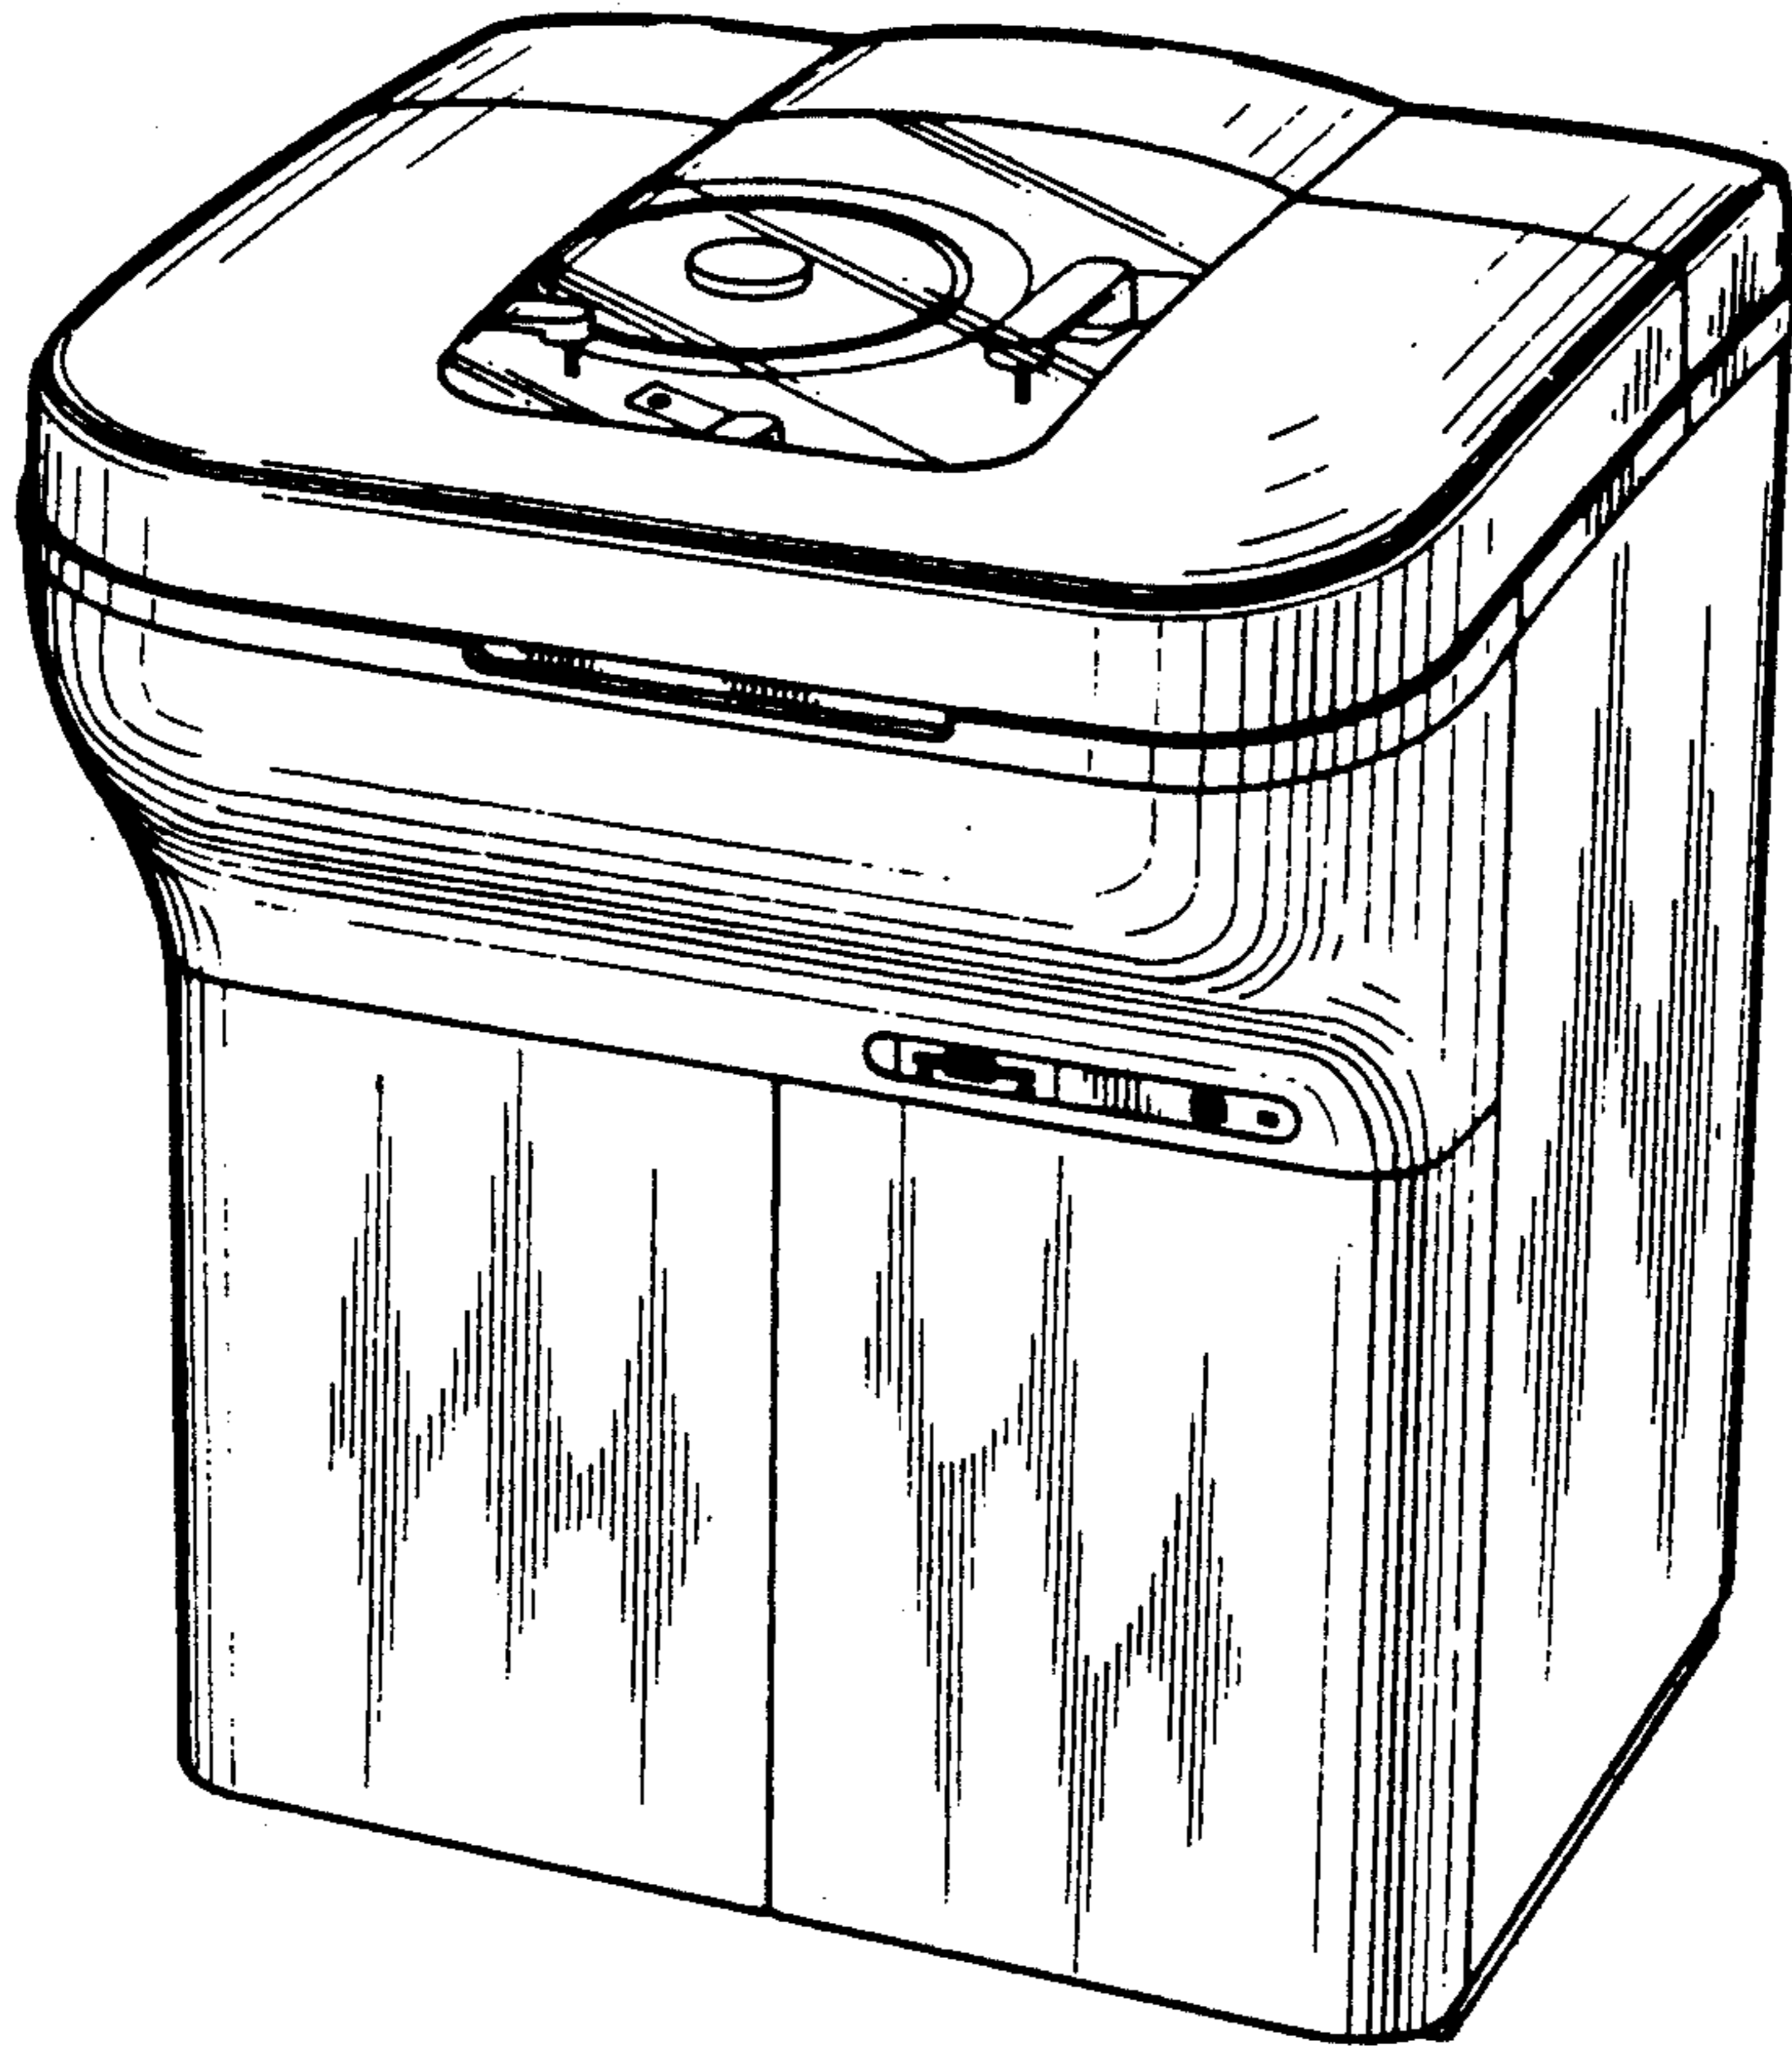


FIG. 2

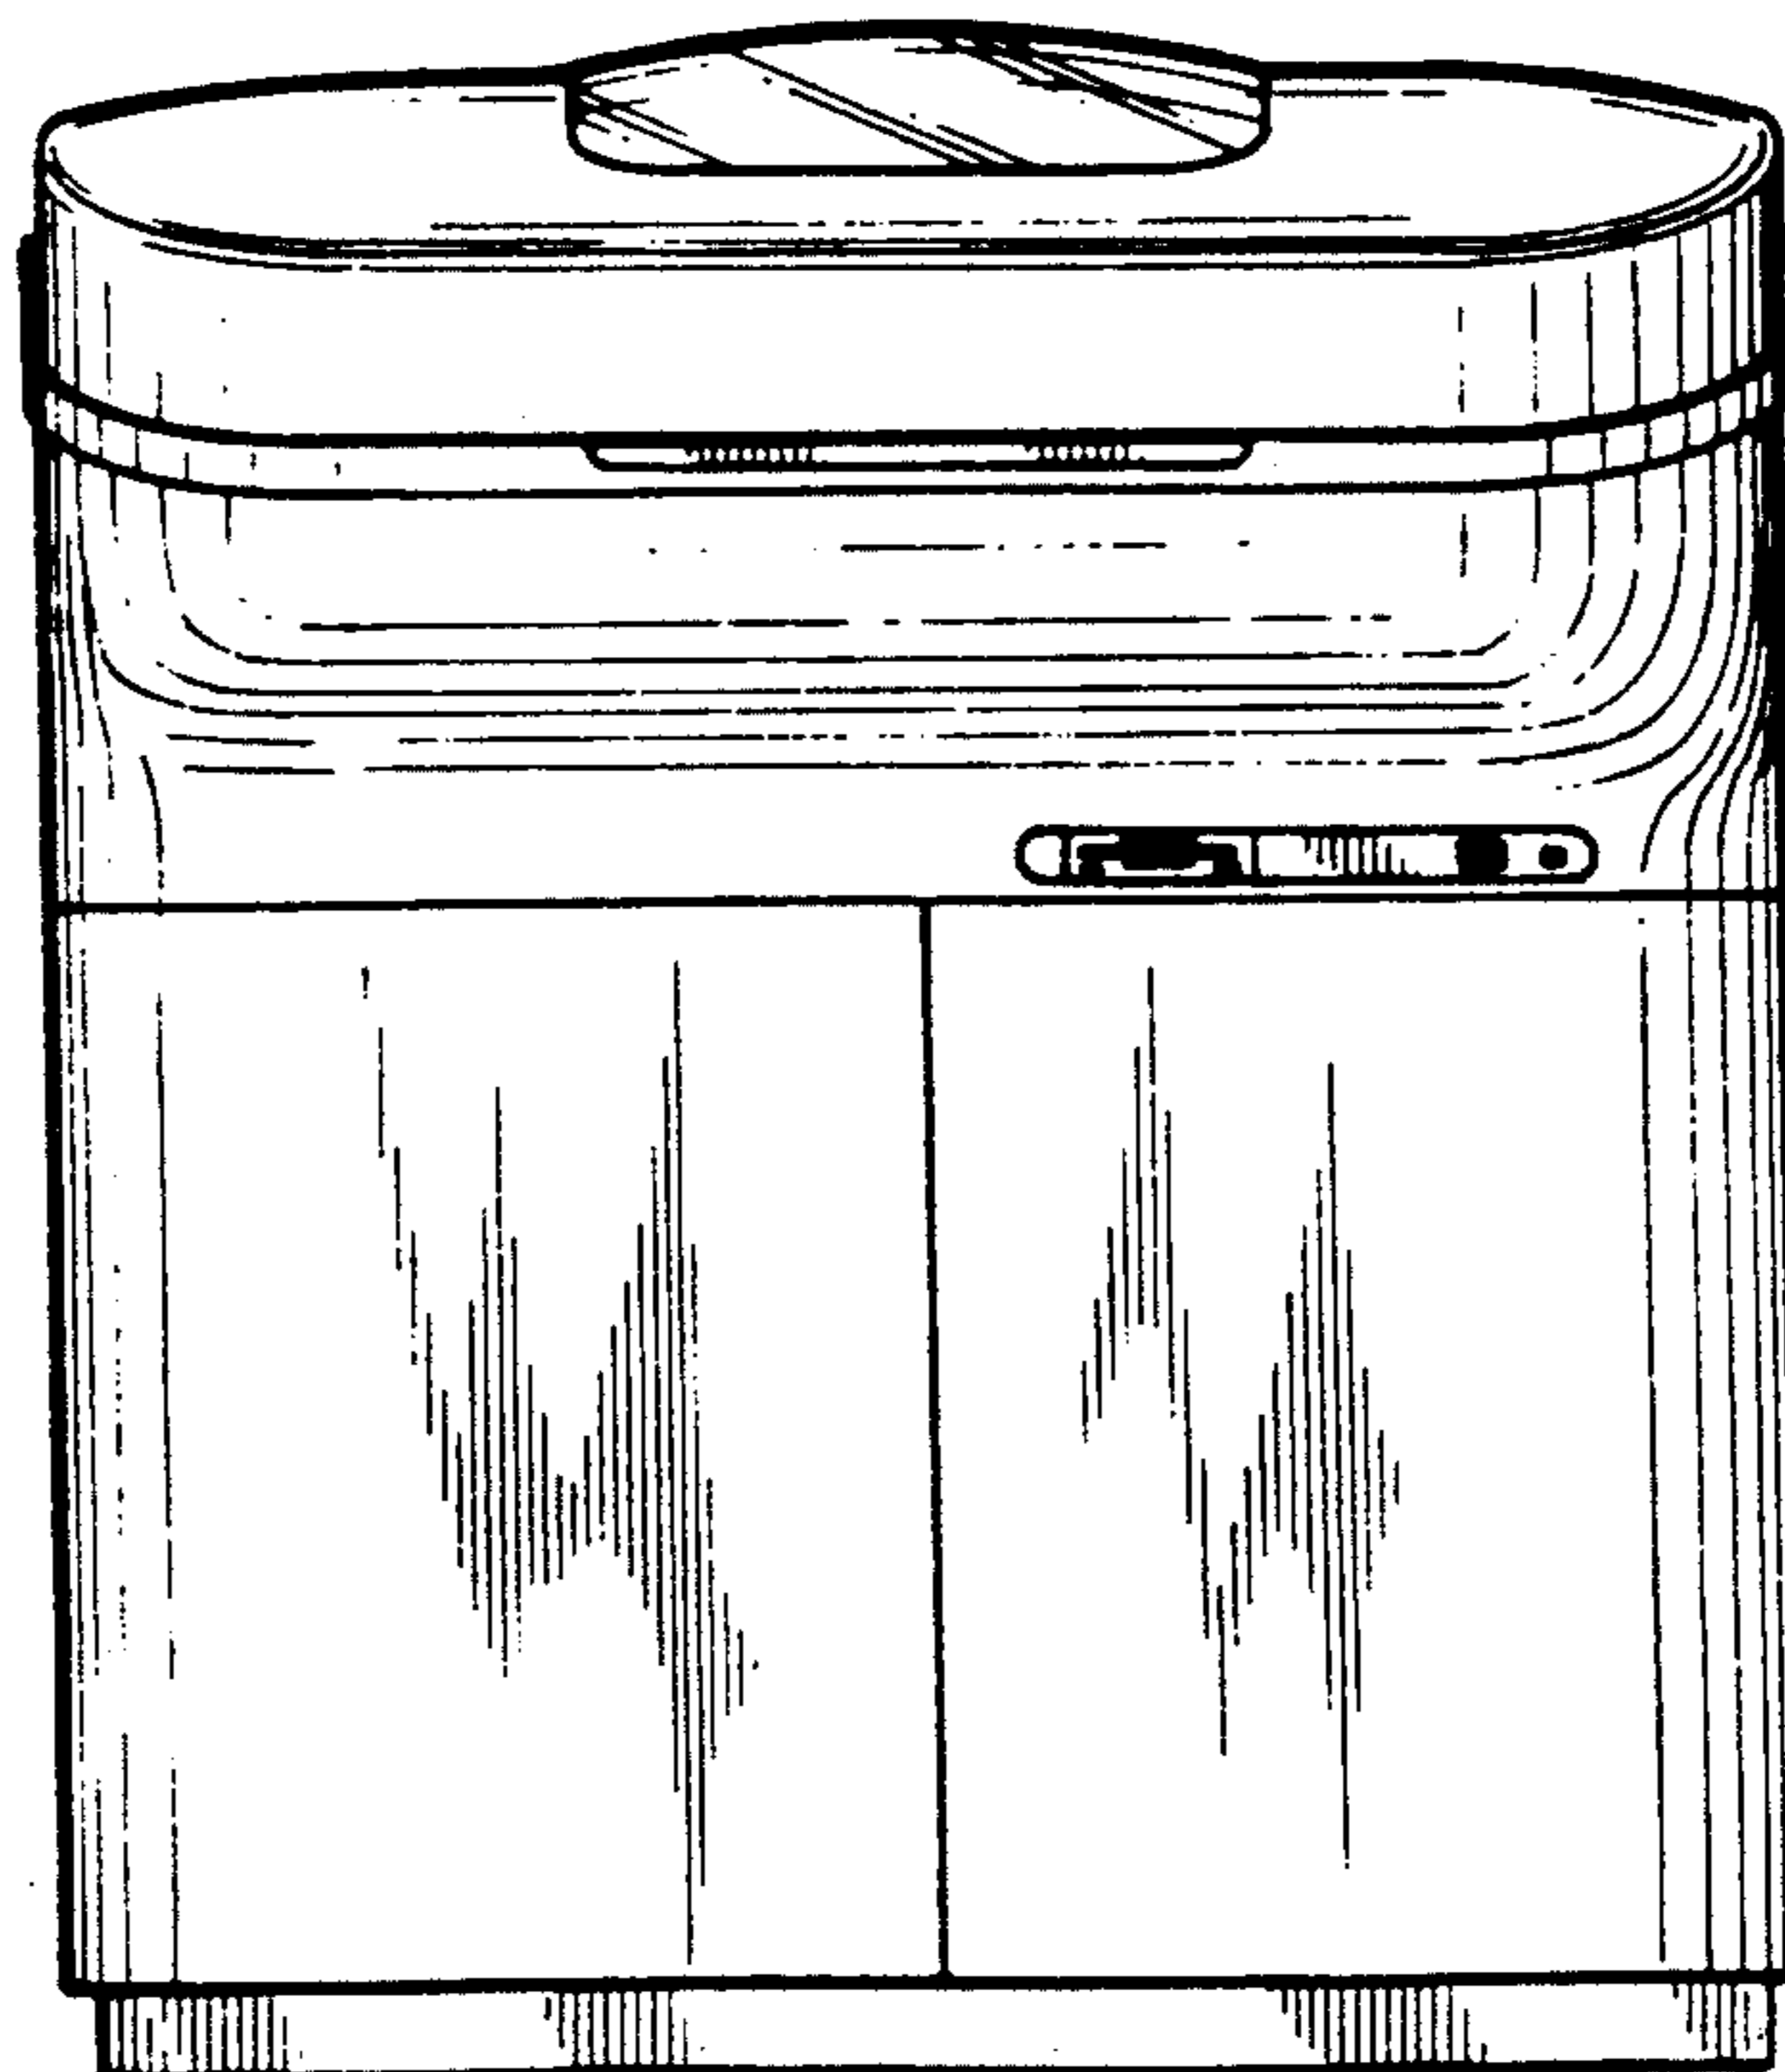


FIG. 3

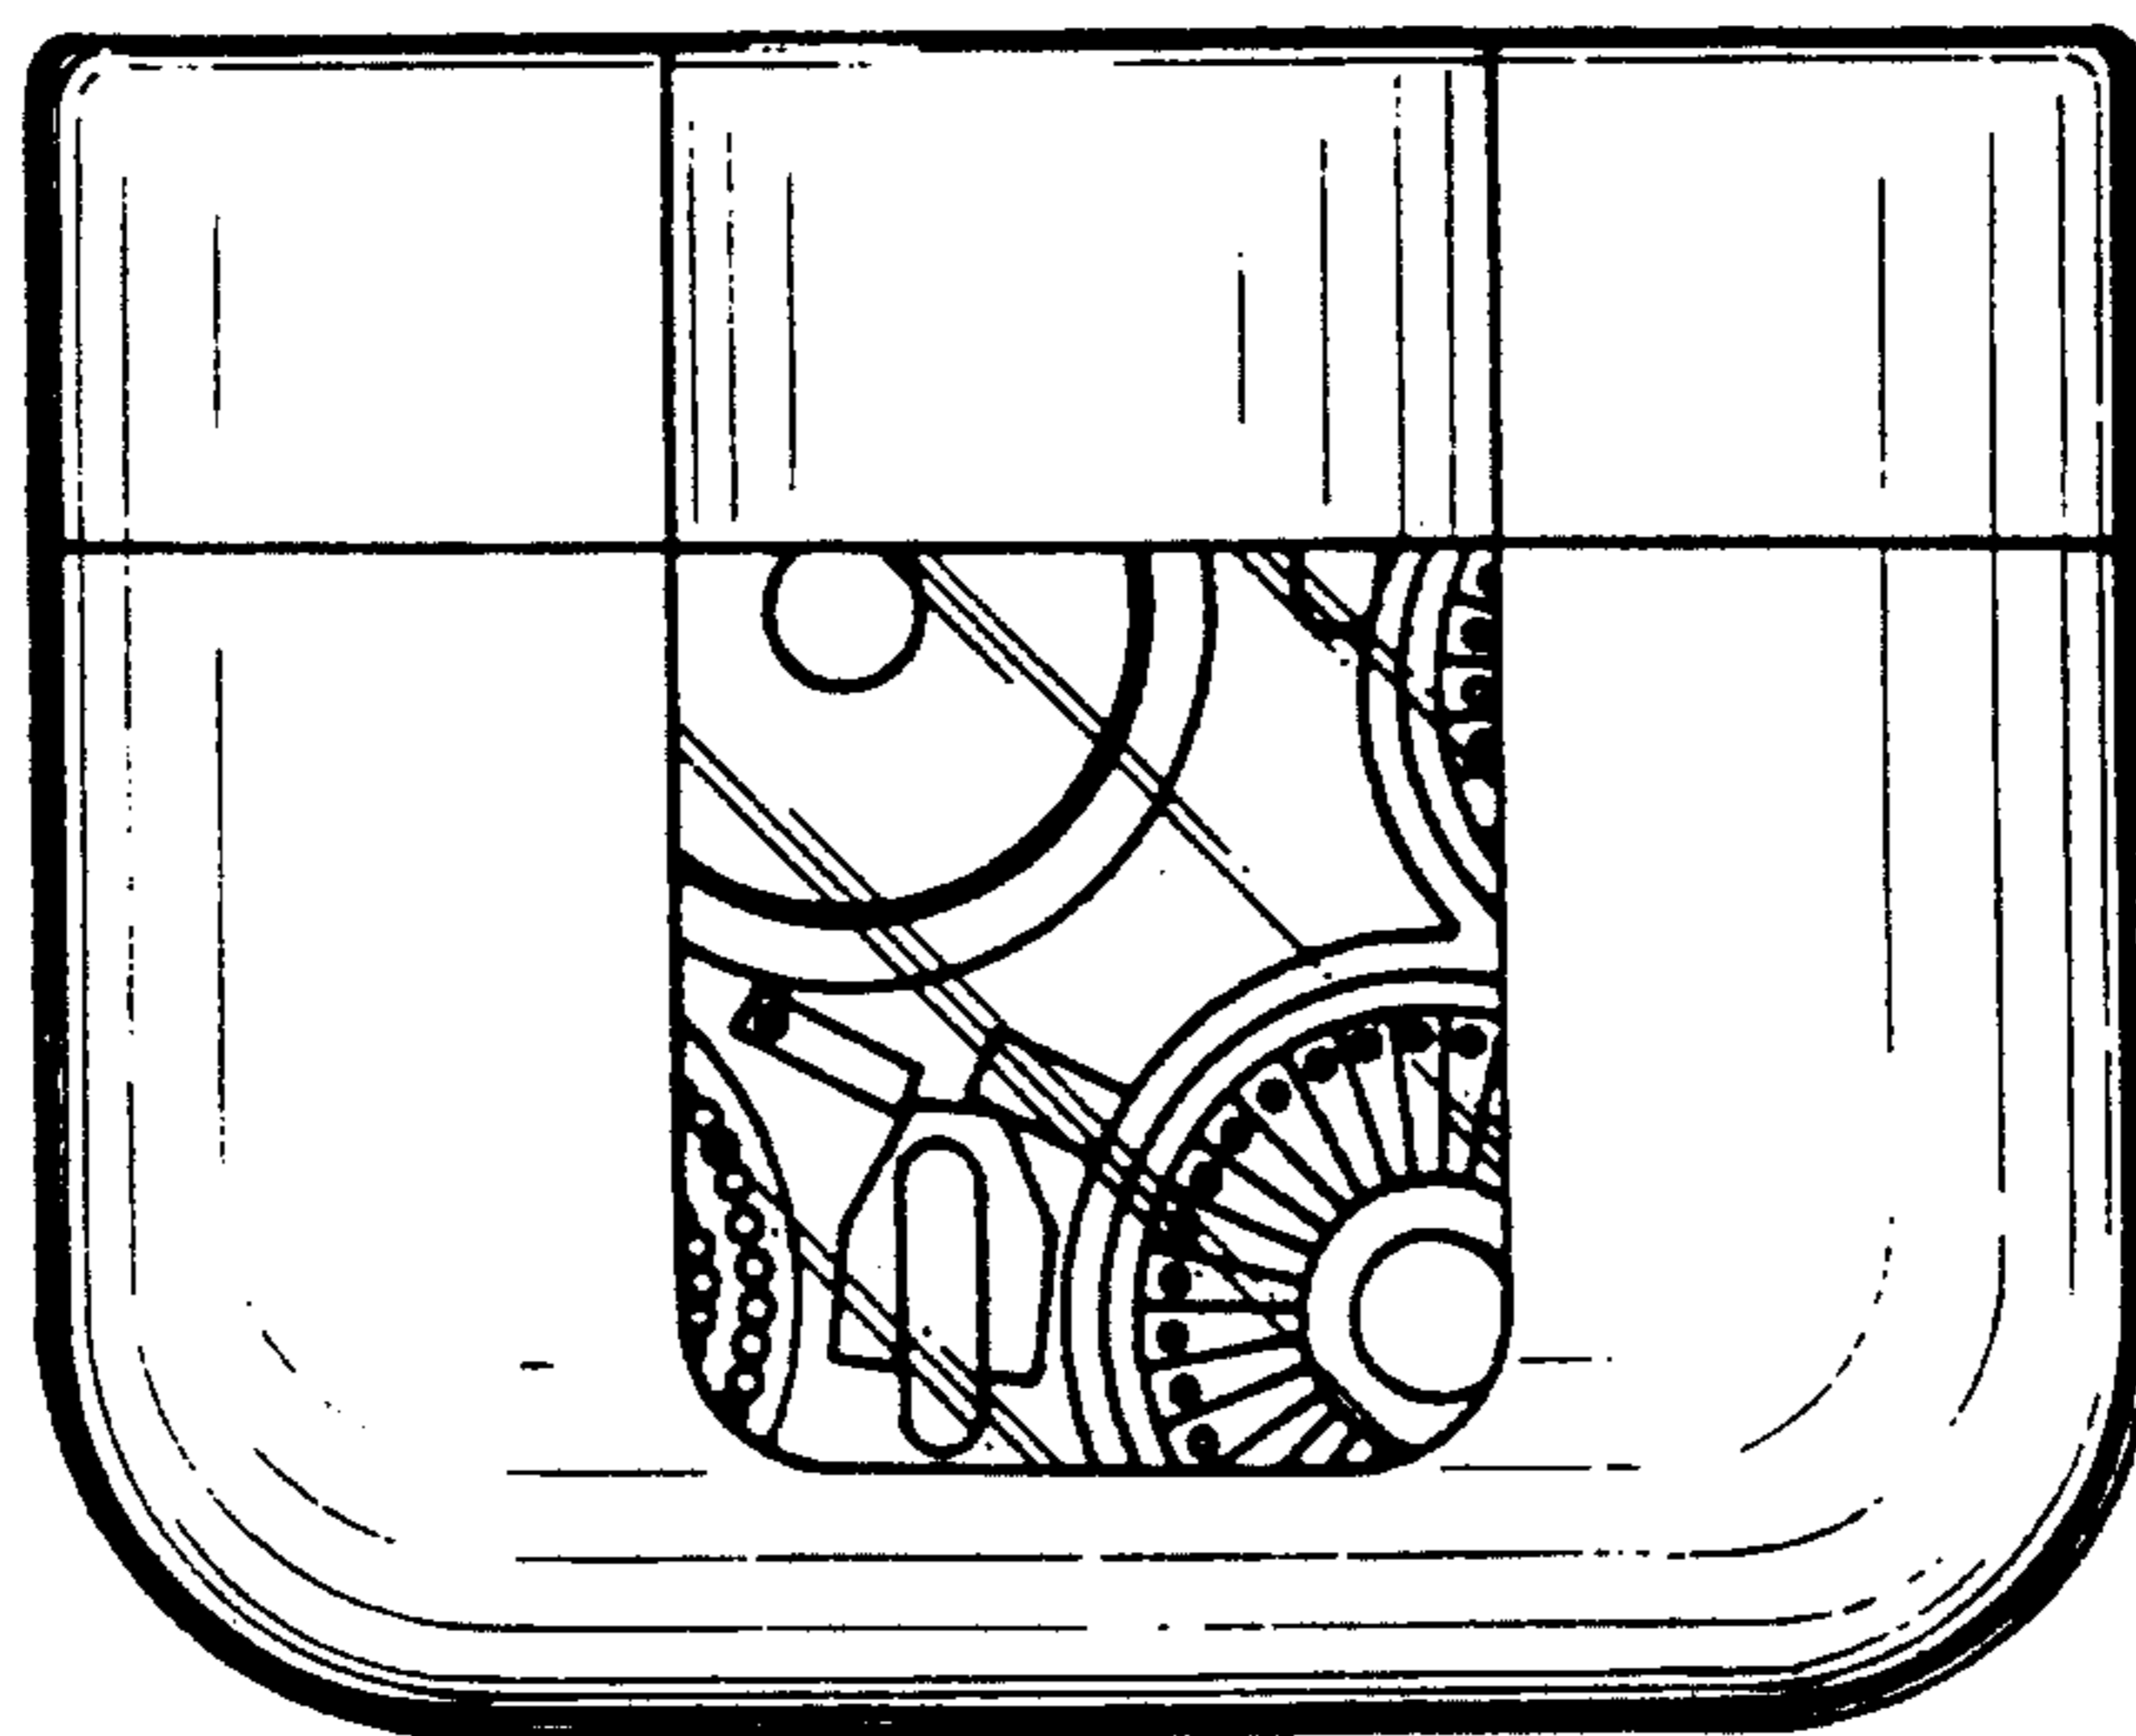


FIG. 4

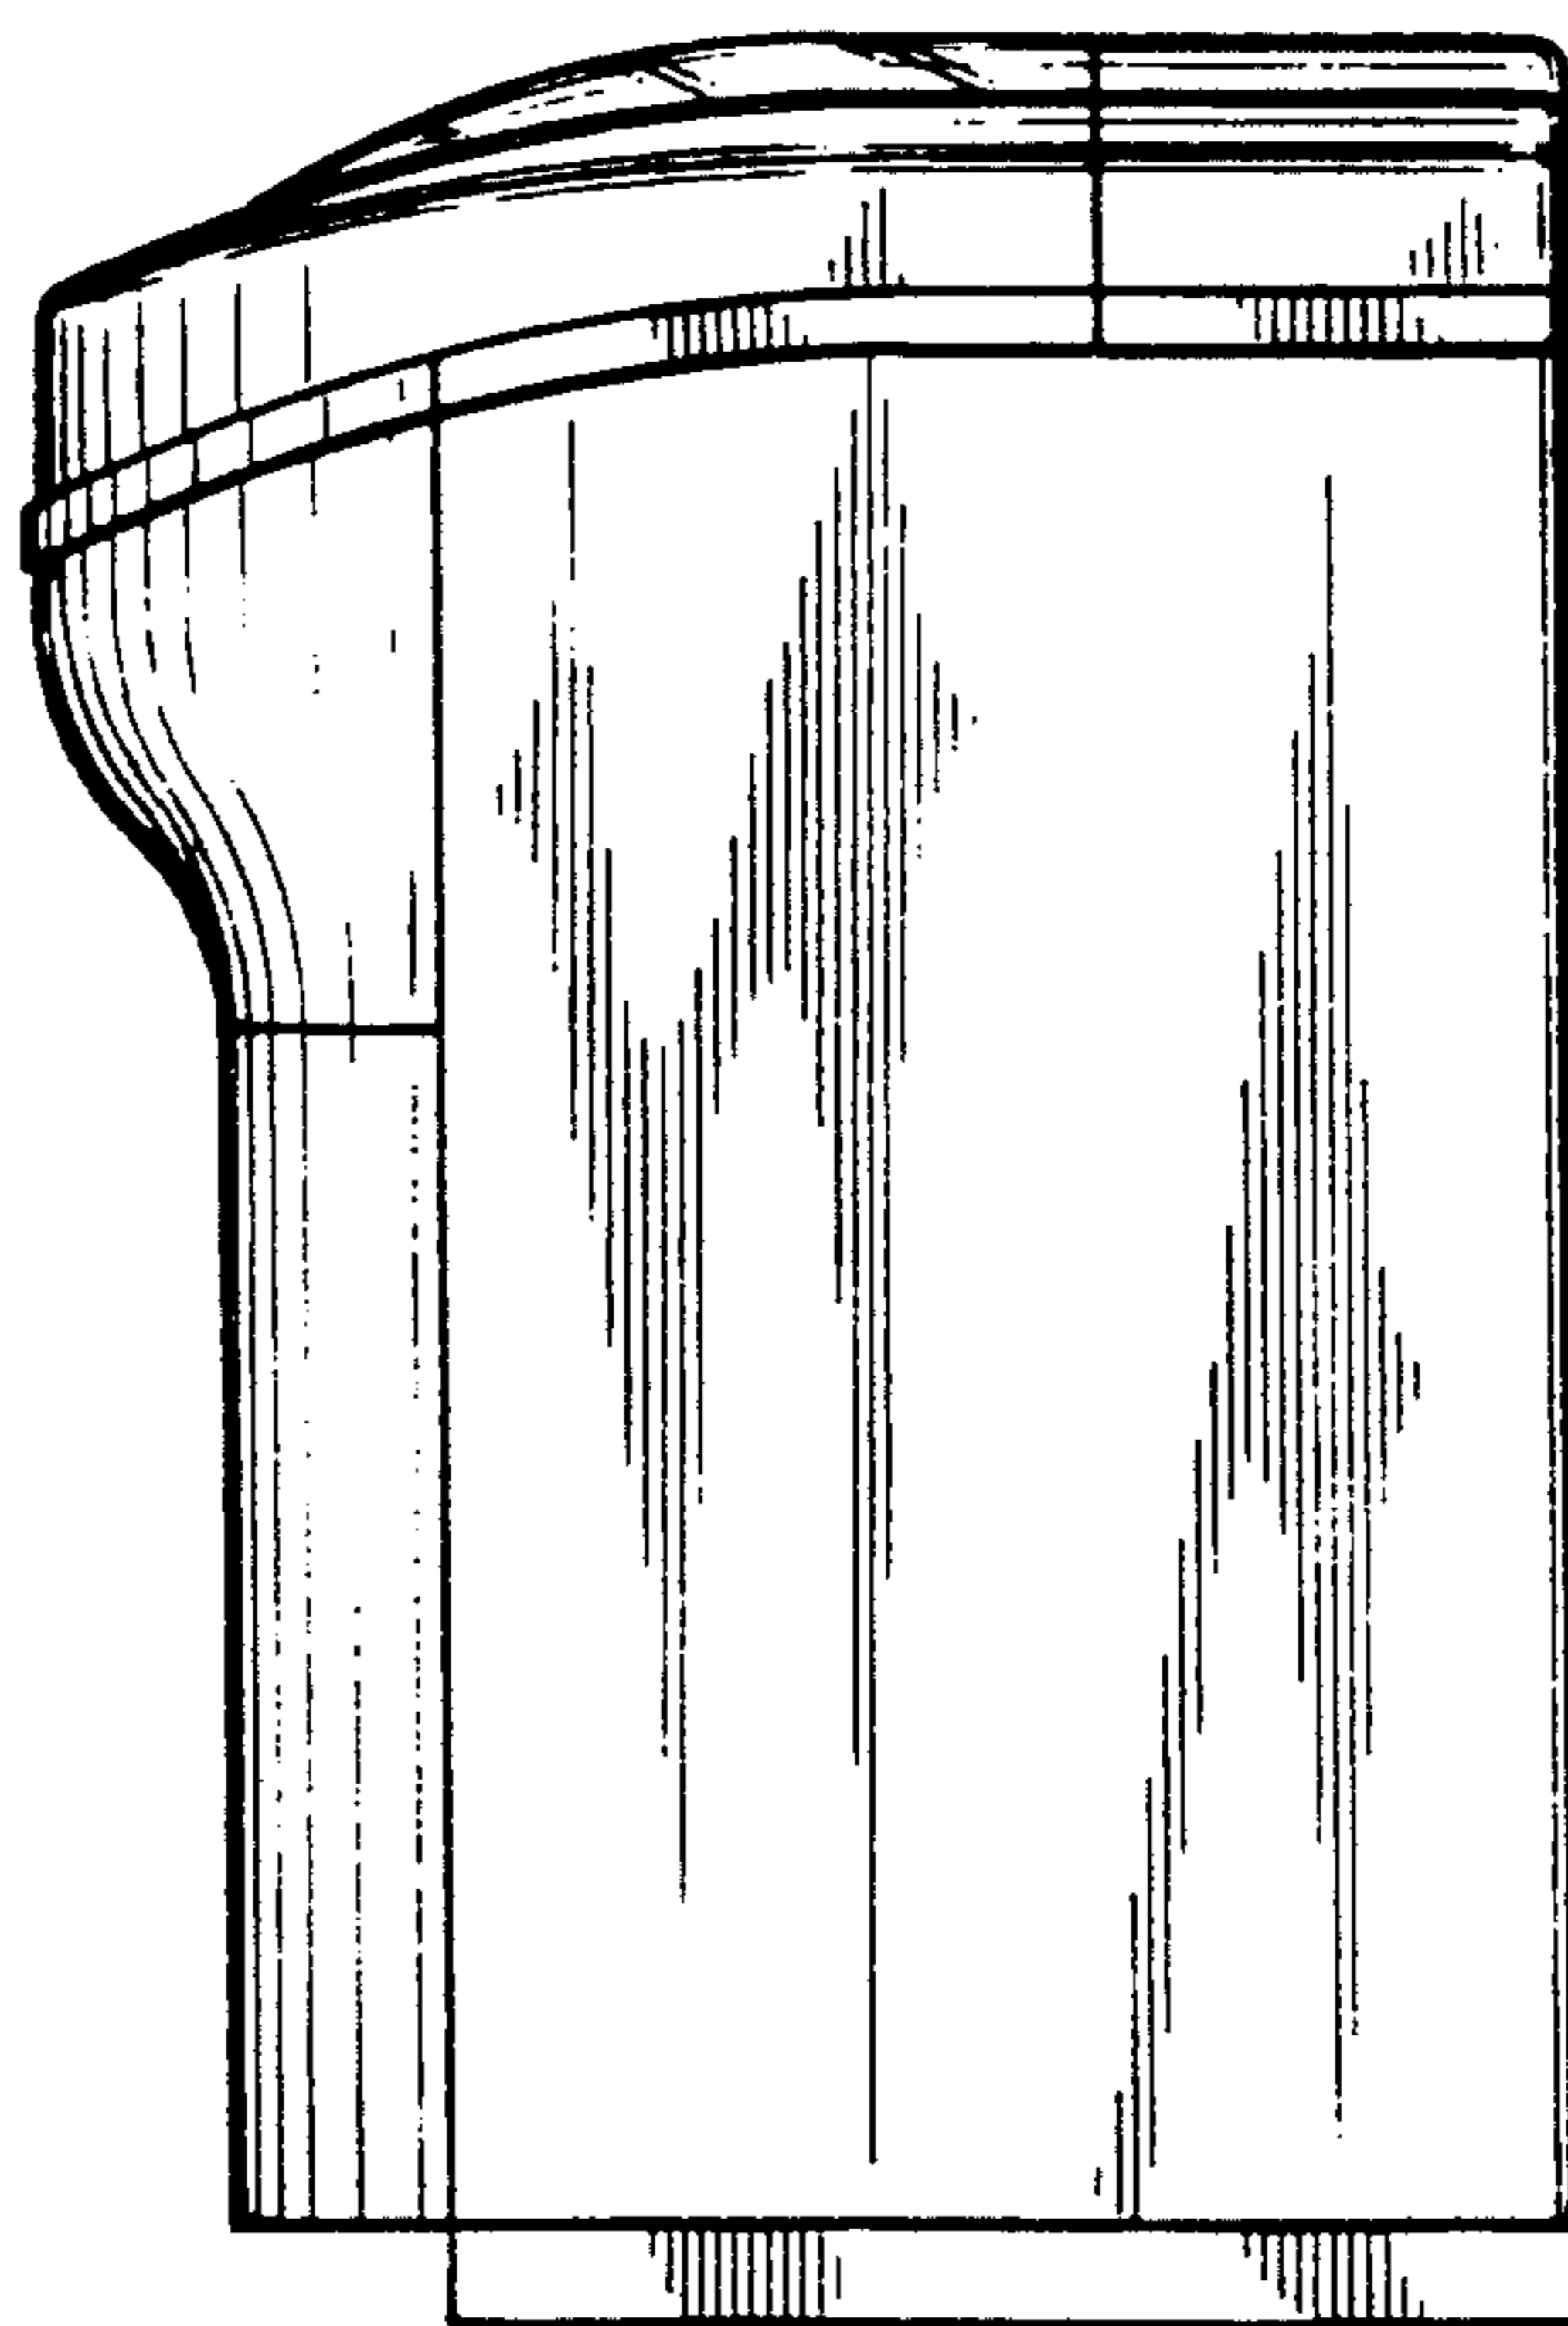


FIG. 5

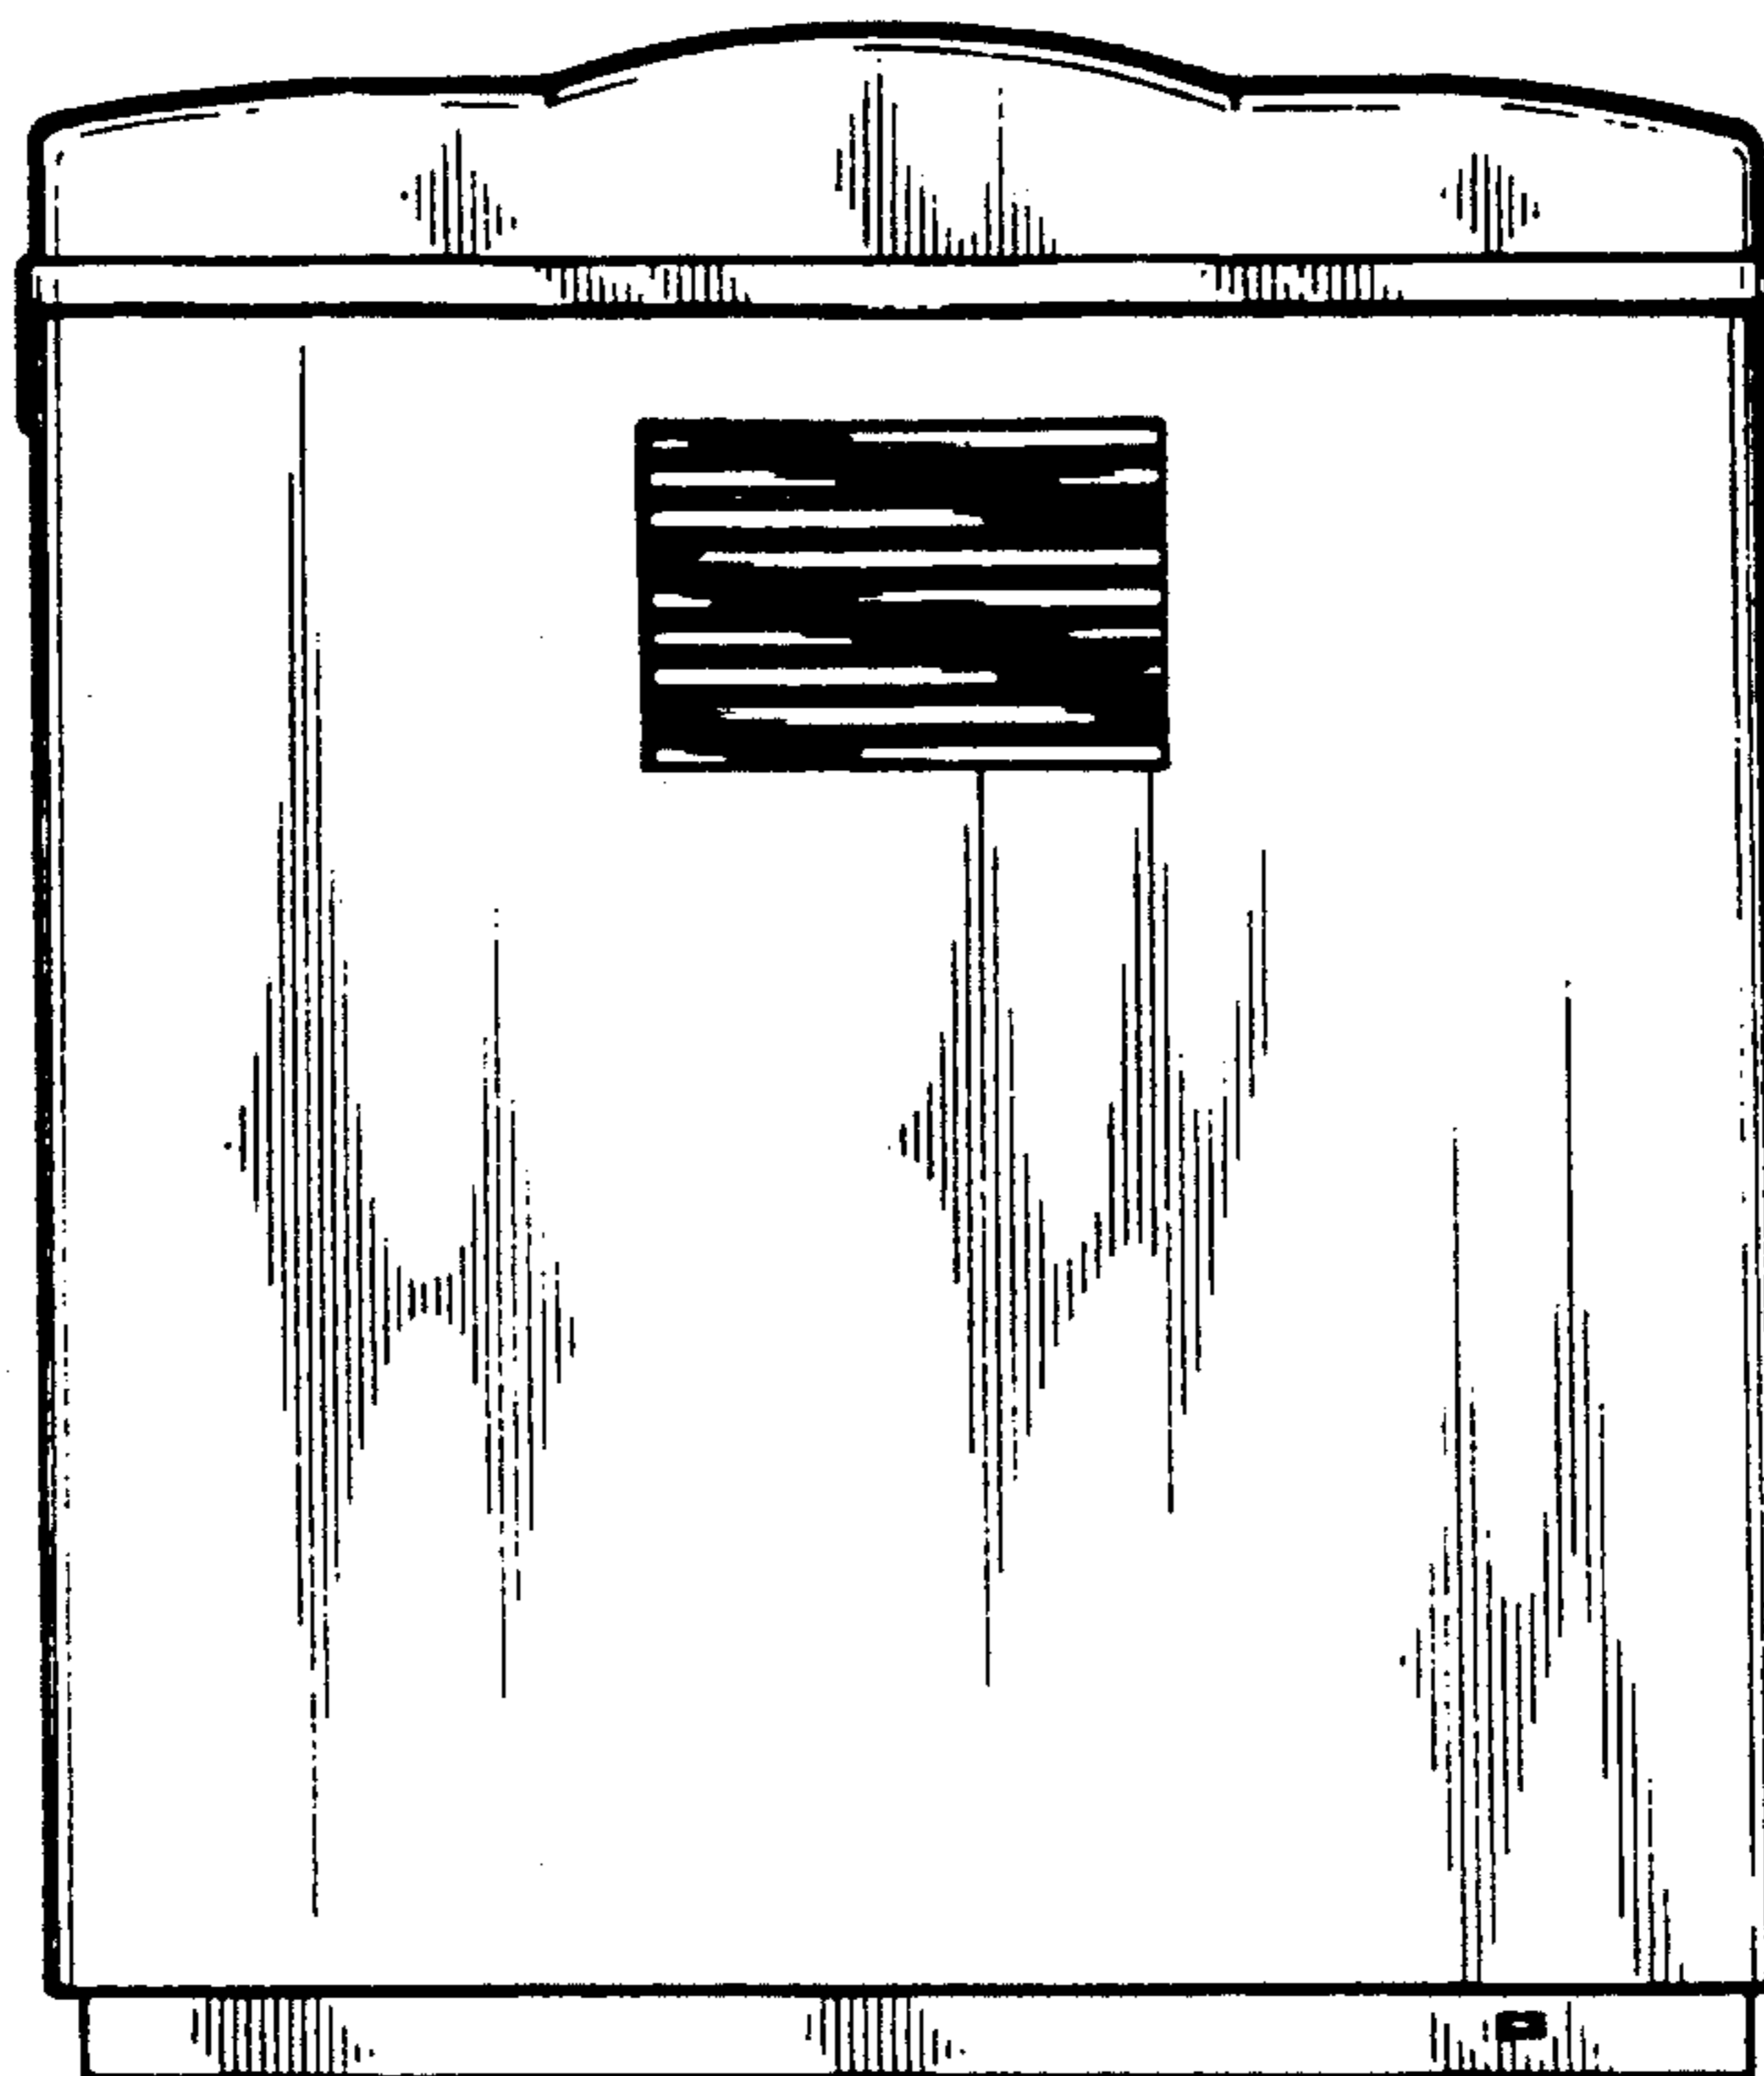


FIG. 6

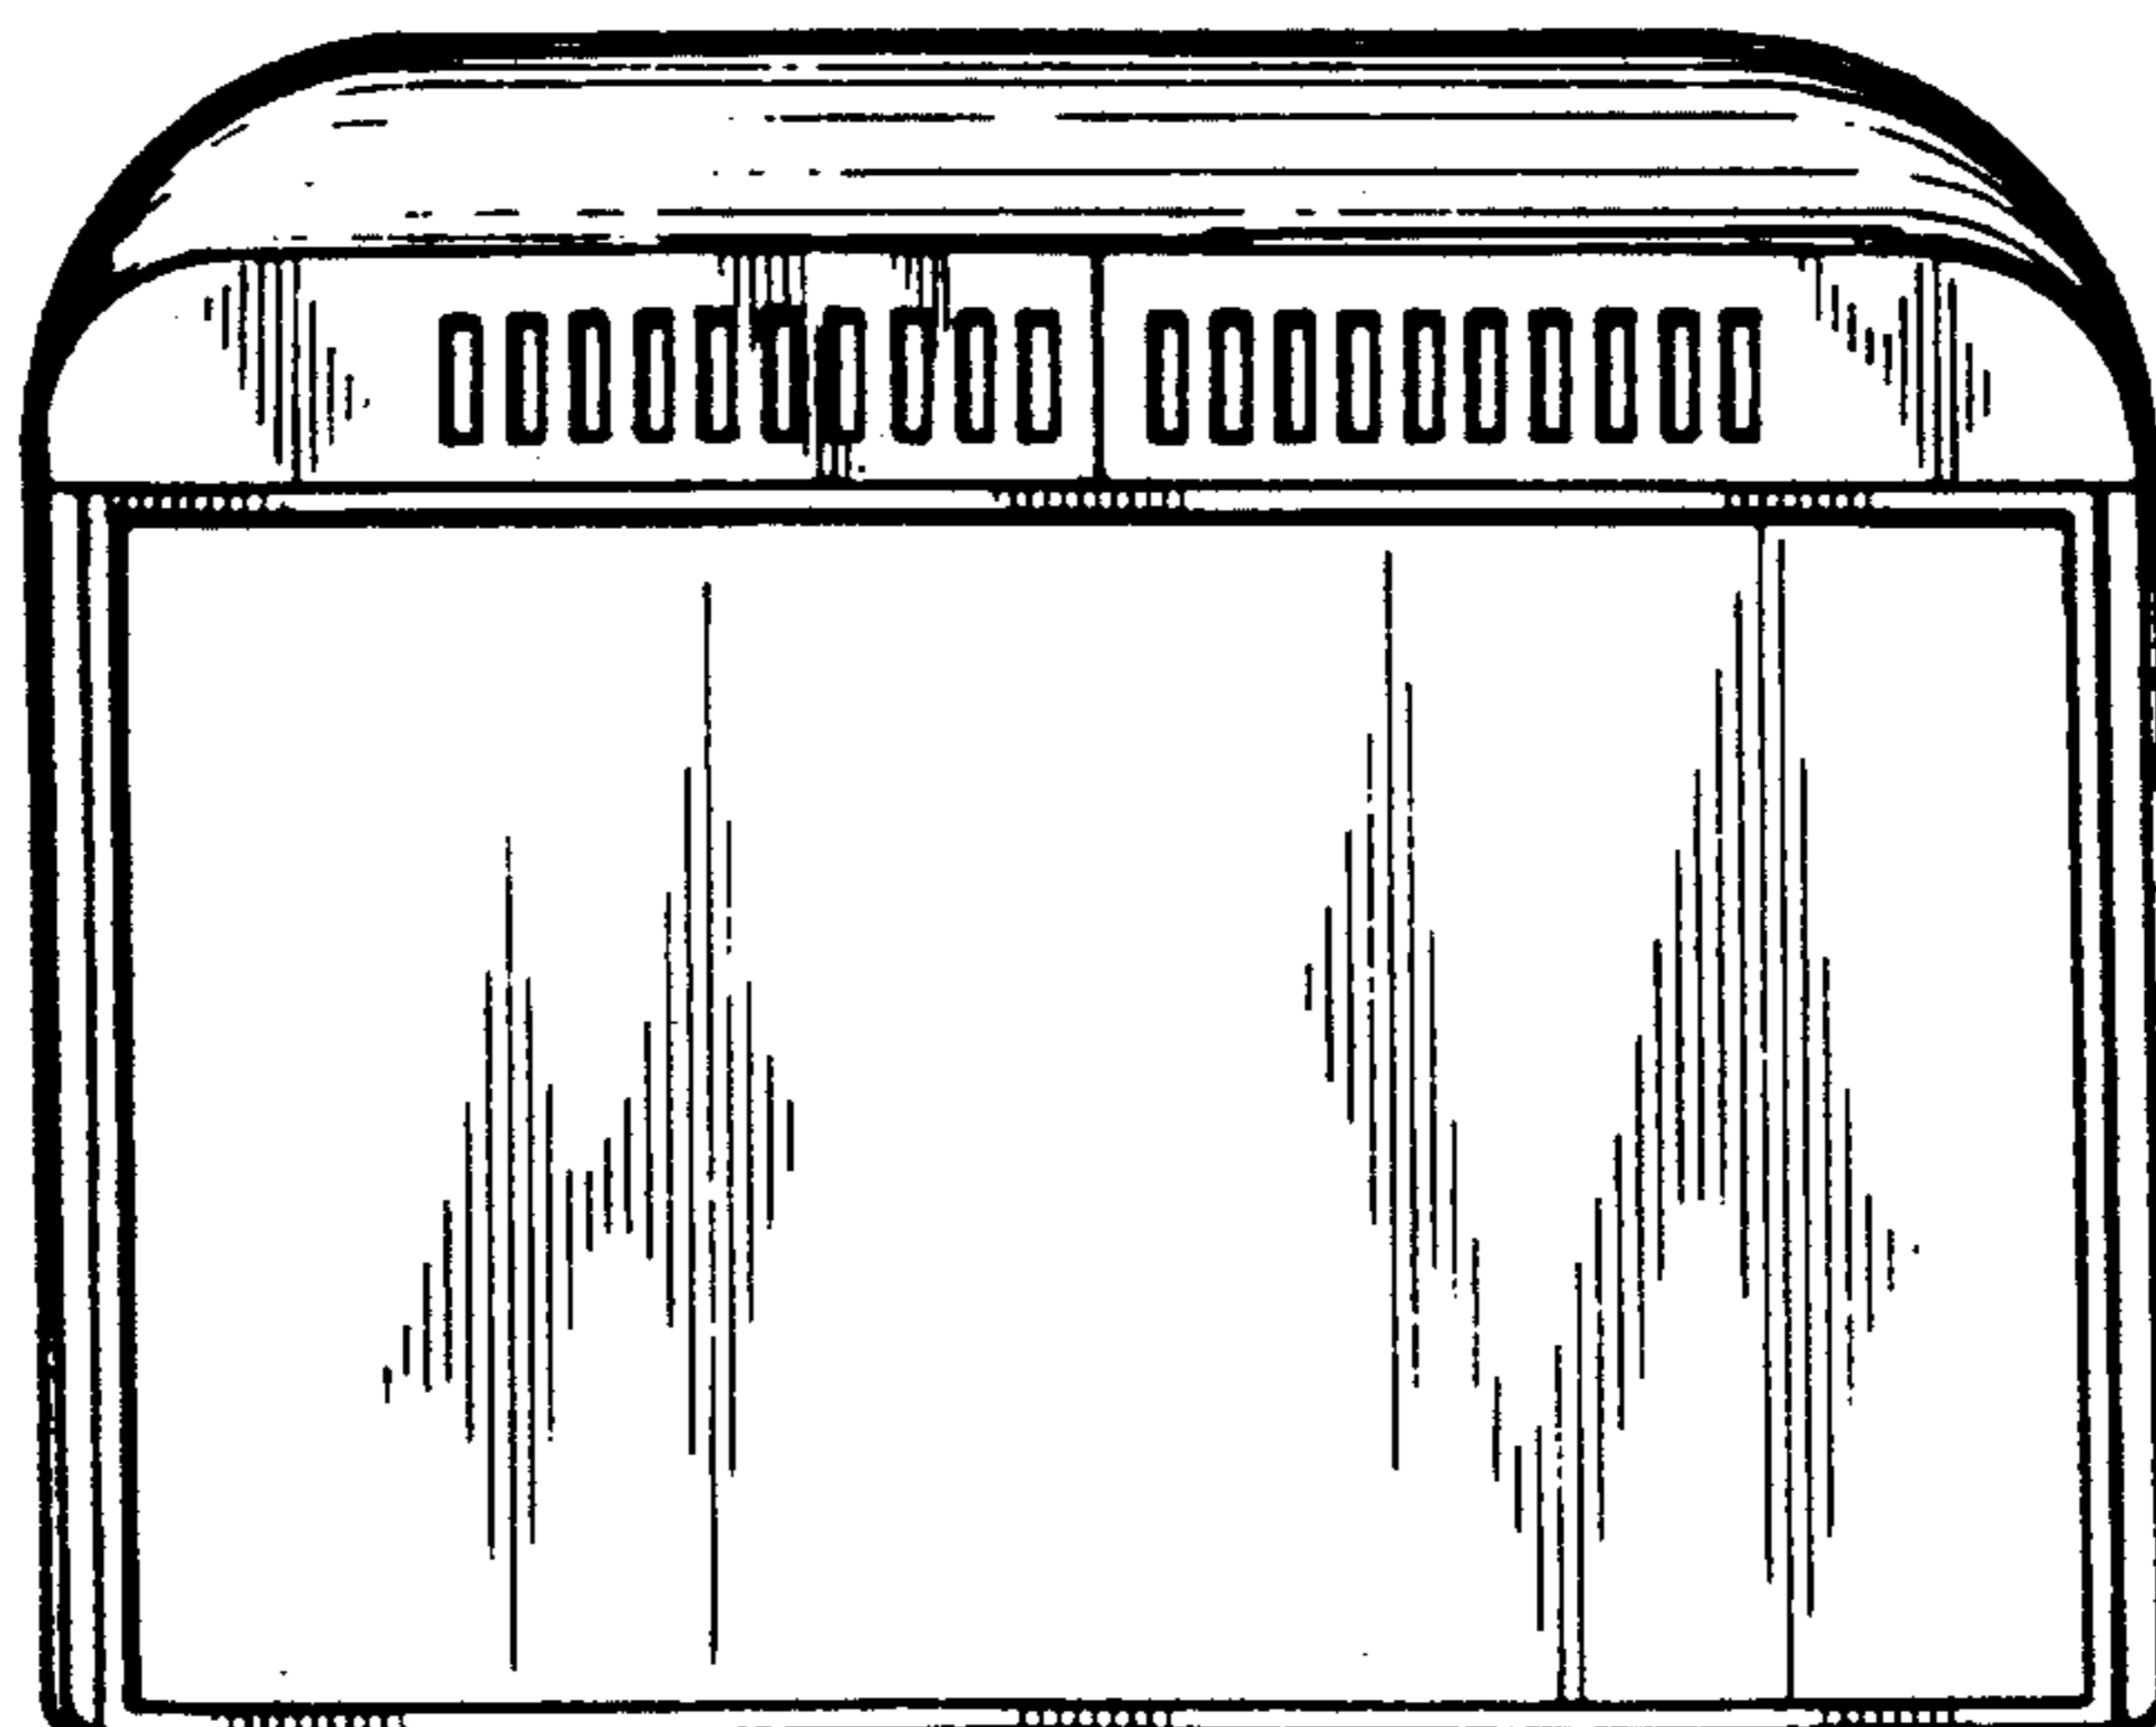


FIG. 7

