



US00D340289S

# United States Patent [19]

[11] Patent Number: **Des. 340,289**

Gerber

[45] Date of Patent: **\*\* Oct. 12, 1993**

[54] **DIAGNOSTIC TESTING MATERIAL**

[76] Inventor: **Jan Gerber, 23, Bartokhof, NL-2402 GC, Alphen ad/Rijn, Netherlands**

[\*\*] Term: **14 Years**

[21] Appl. No.: **909,992**

[22] Filed: **Jul. 7, 1992**

[30] **Foreign Application Priority Data**

Jan. 30, 1992 [WO] World Int. Prop. O. .... DM/021839

[52] U.S. Cl. .... **D24/223; D24/225**

[58] Field of Search ..... **D24/223, 224, 225, 226, D24/227; 206/557, 558, 564, 569; 422/102, 104**

[56] **References Cited**

**U.S. PATENT DOCUMENTS**

- D. 239,548 4/1976 Schiff et al. .... D24/225
- D. 274,261 6/1984 Valencia ..... D24/225
- D. 277,699 2/1985 Valencia ..... D24/225

- D. 283,159 3/1986 Godsey ..... D24/223
- 3,469,686 9/1969 Gutsche et al. .... 206/558 X
- 5,141,718 8/1992 Clark ..... 422/102 X


*Primary Examiner*—Nelson C. Holtje  
*Assistant Examiner*—Antoine D. Davis  
*Attorney, Agent, or Firm*—Watson, Cole, Grindle & Watson

[57] **CLAIM**

An ornamental design for a diagnostic testing material, as shown and described.

**DESCRIPTION**

FIG. 1 is an exploded perspective view of a diagnostic testing material, showing my new design; FIG. 2 is a top plan view thereof, the bottom being flat and unadorned; FIG. 3 is a side elevational view thereof, the opposite side view being a mirror image; and, FIG. 4 is an end view thereof, the opposite end view being a mirror image.

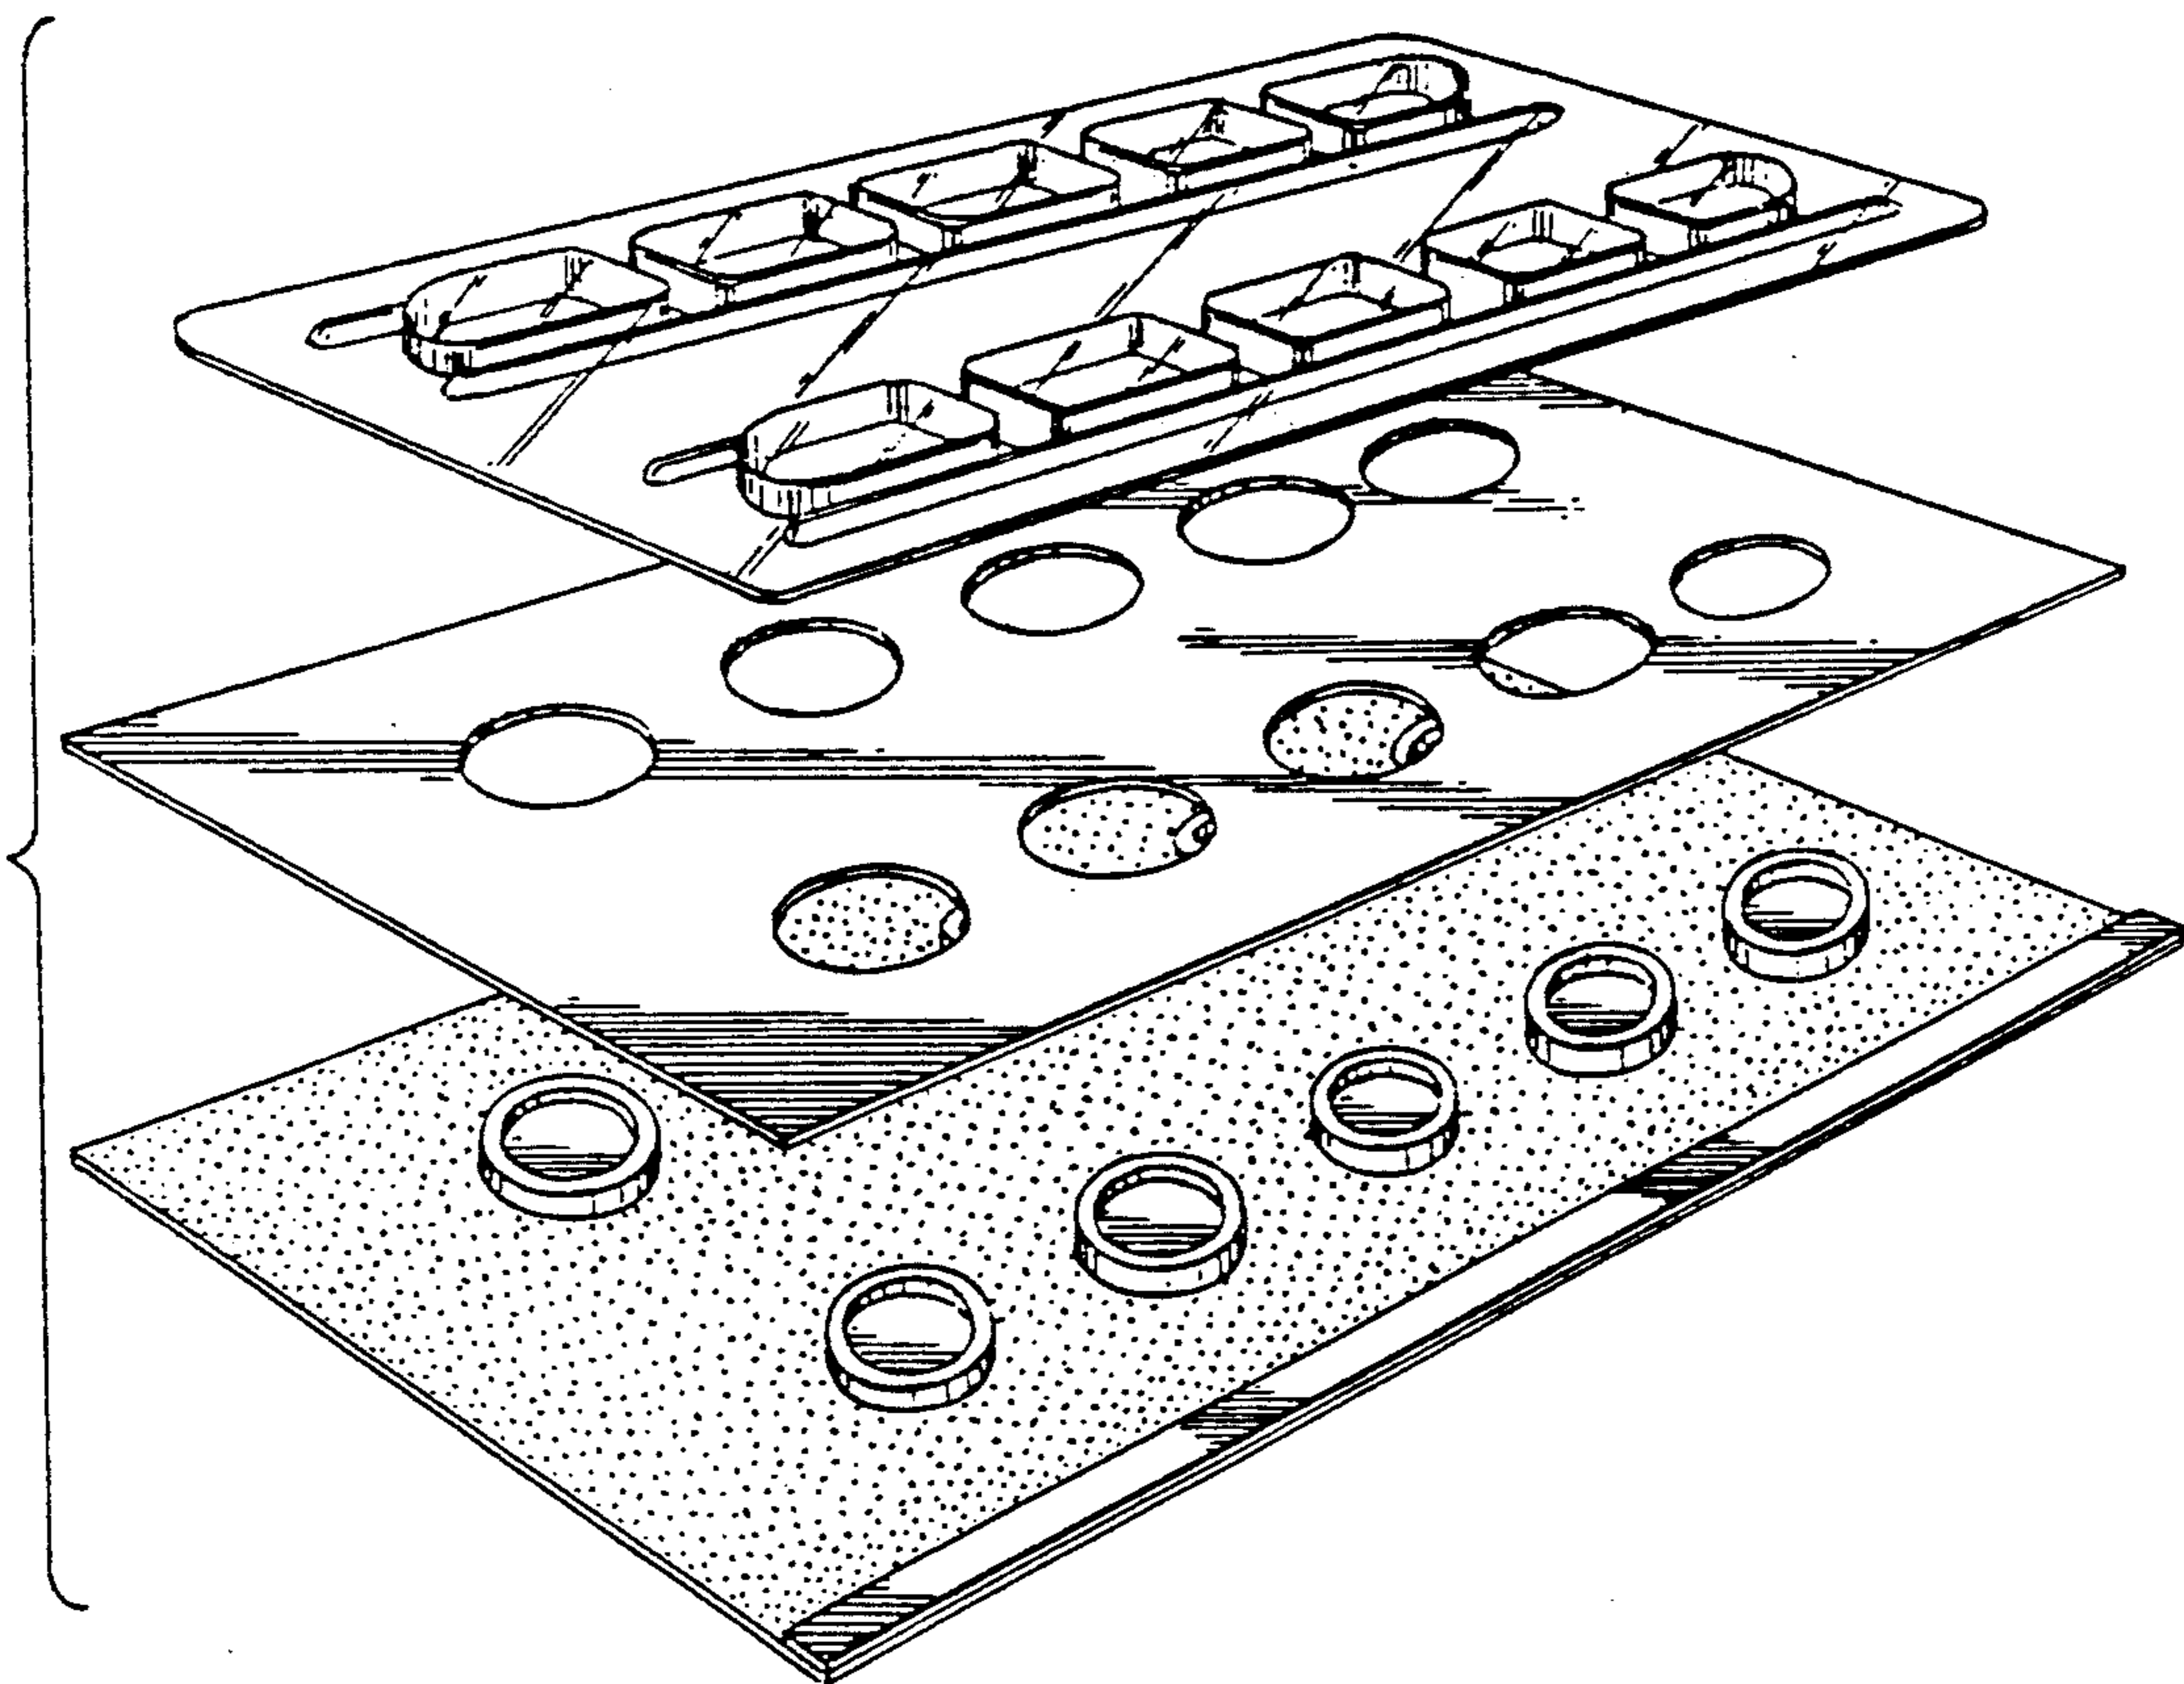

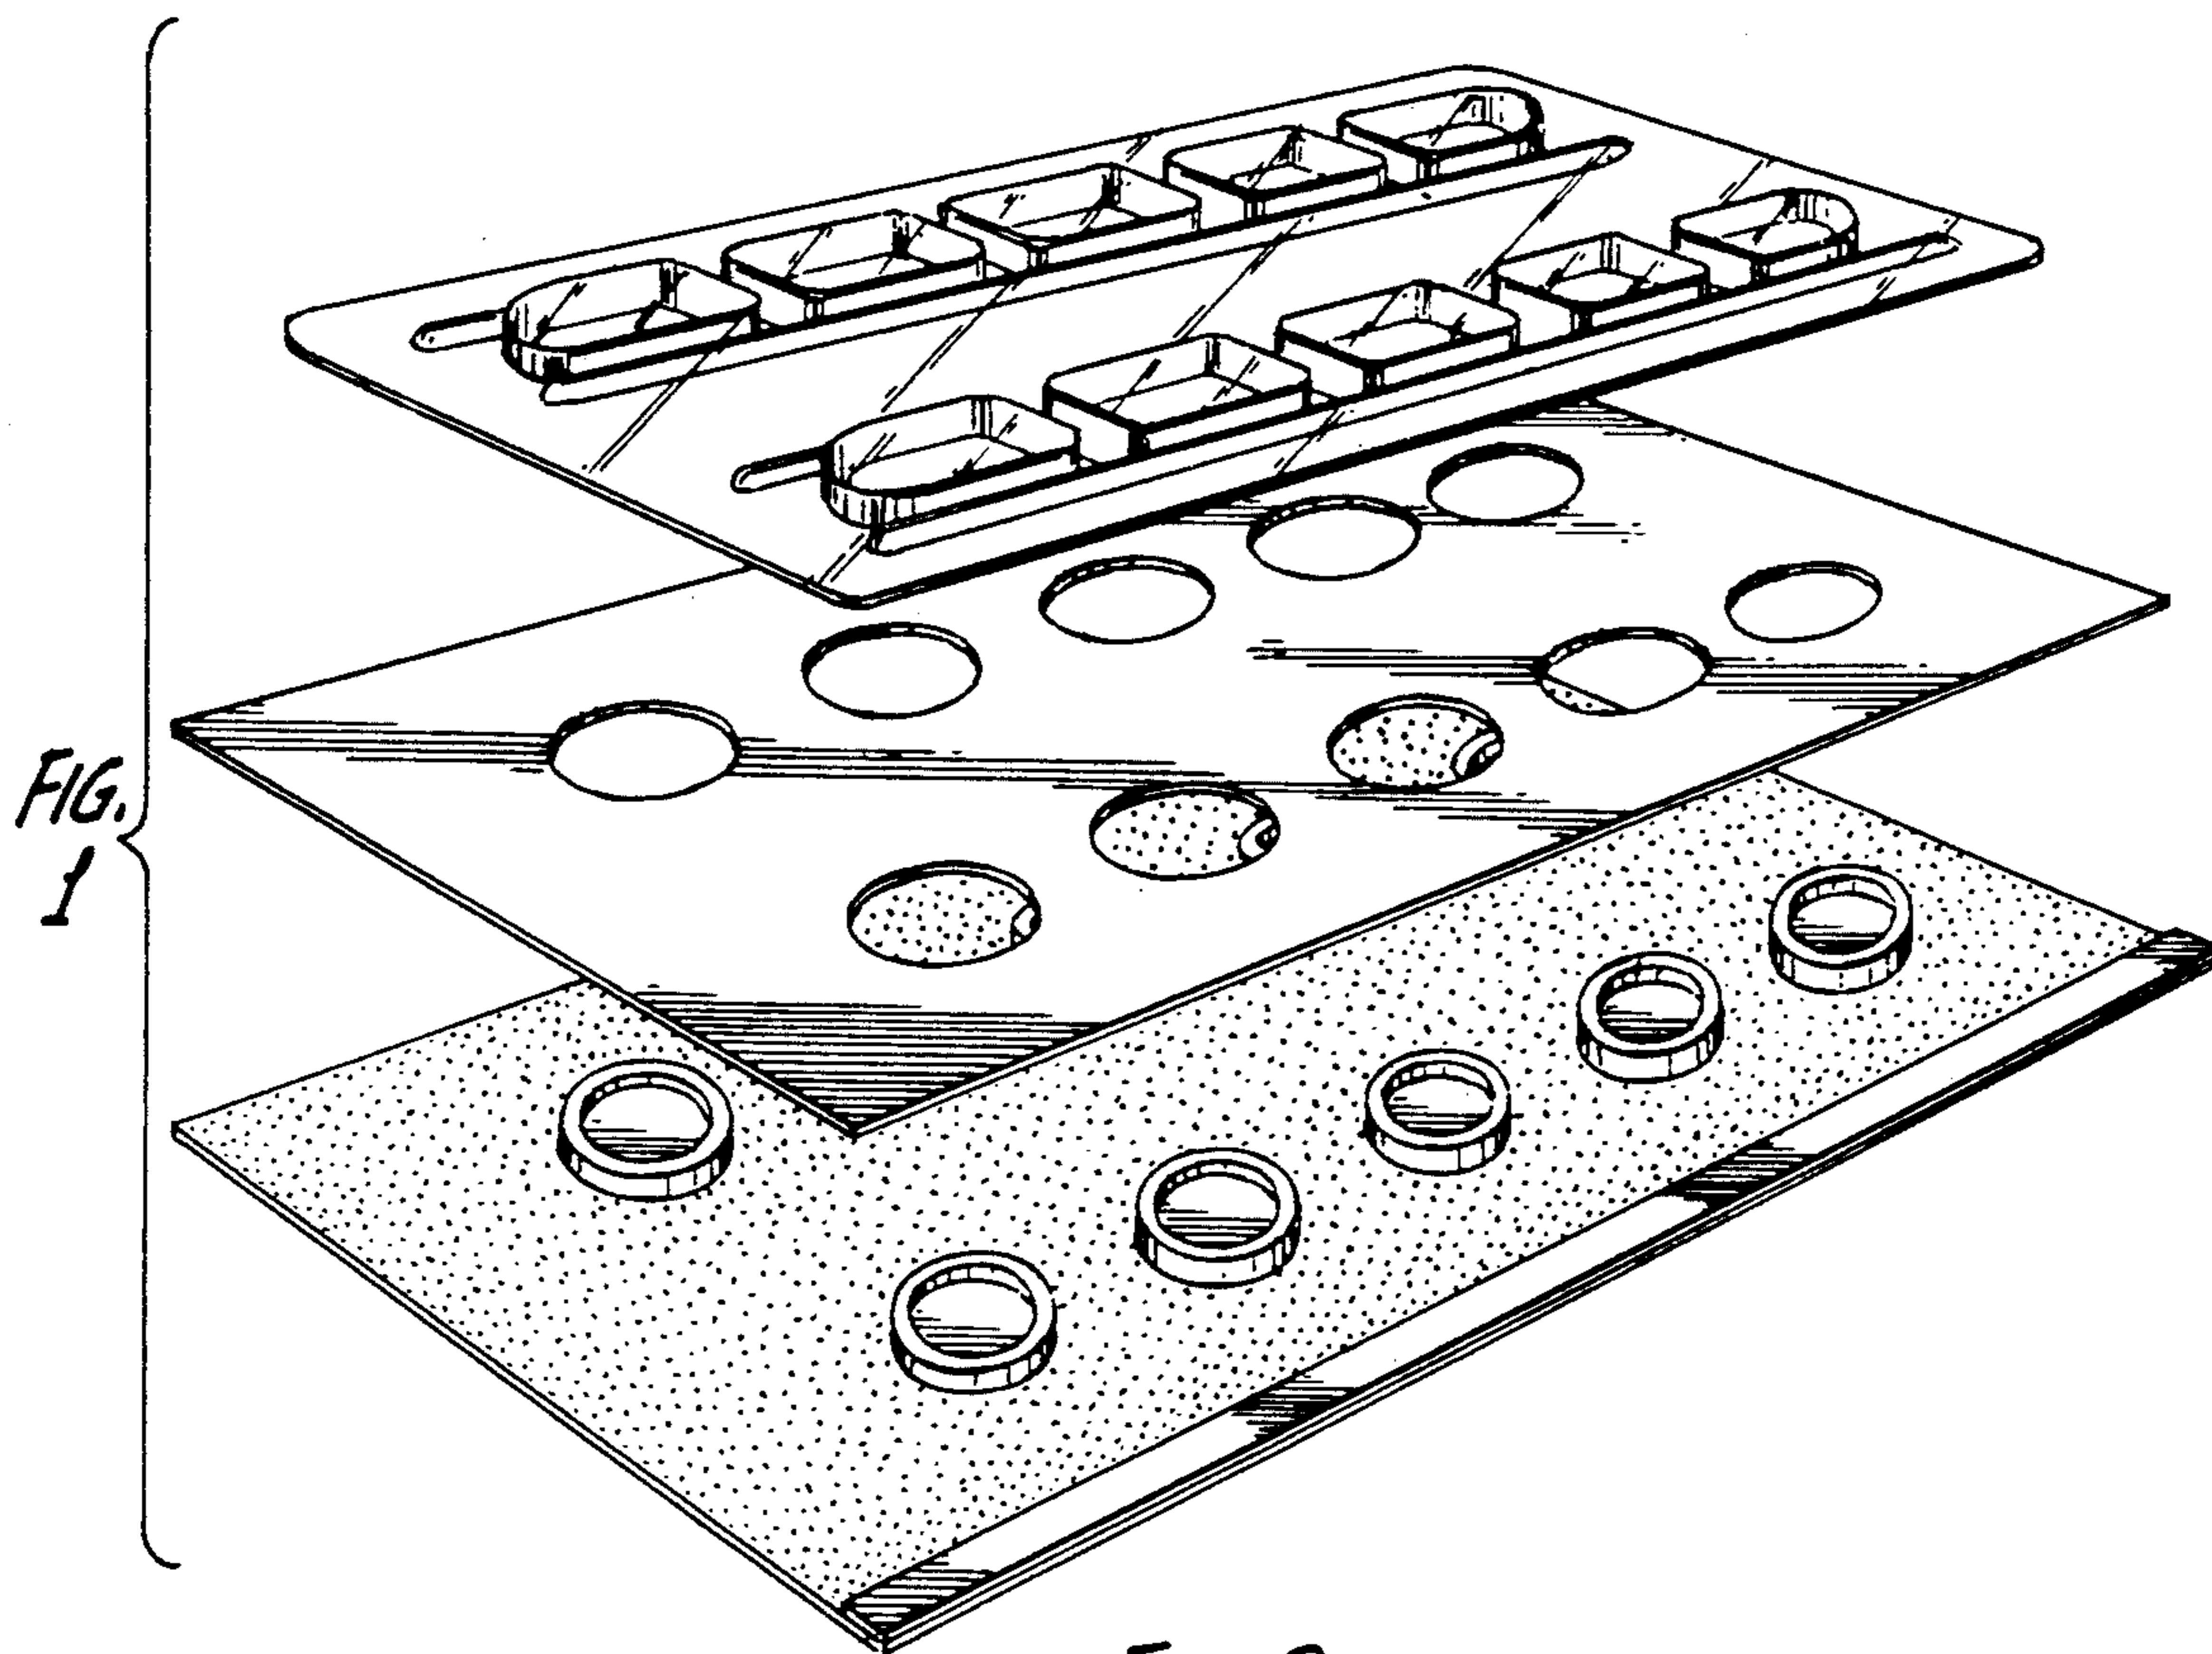


FIG. 2

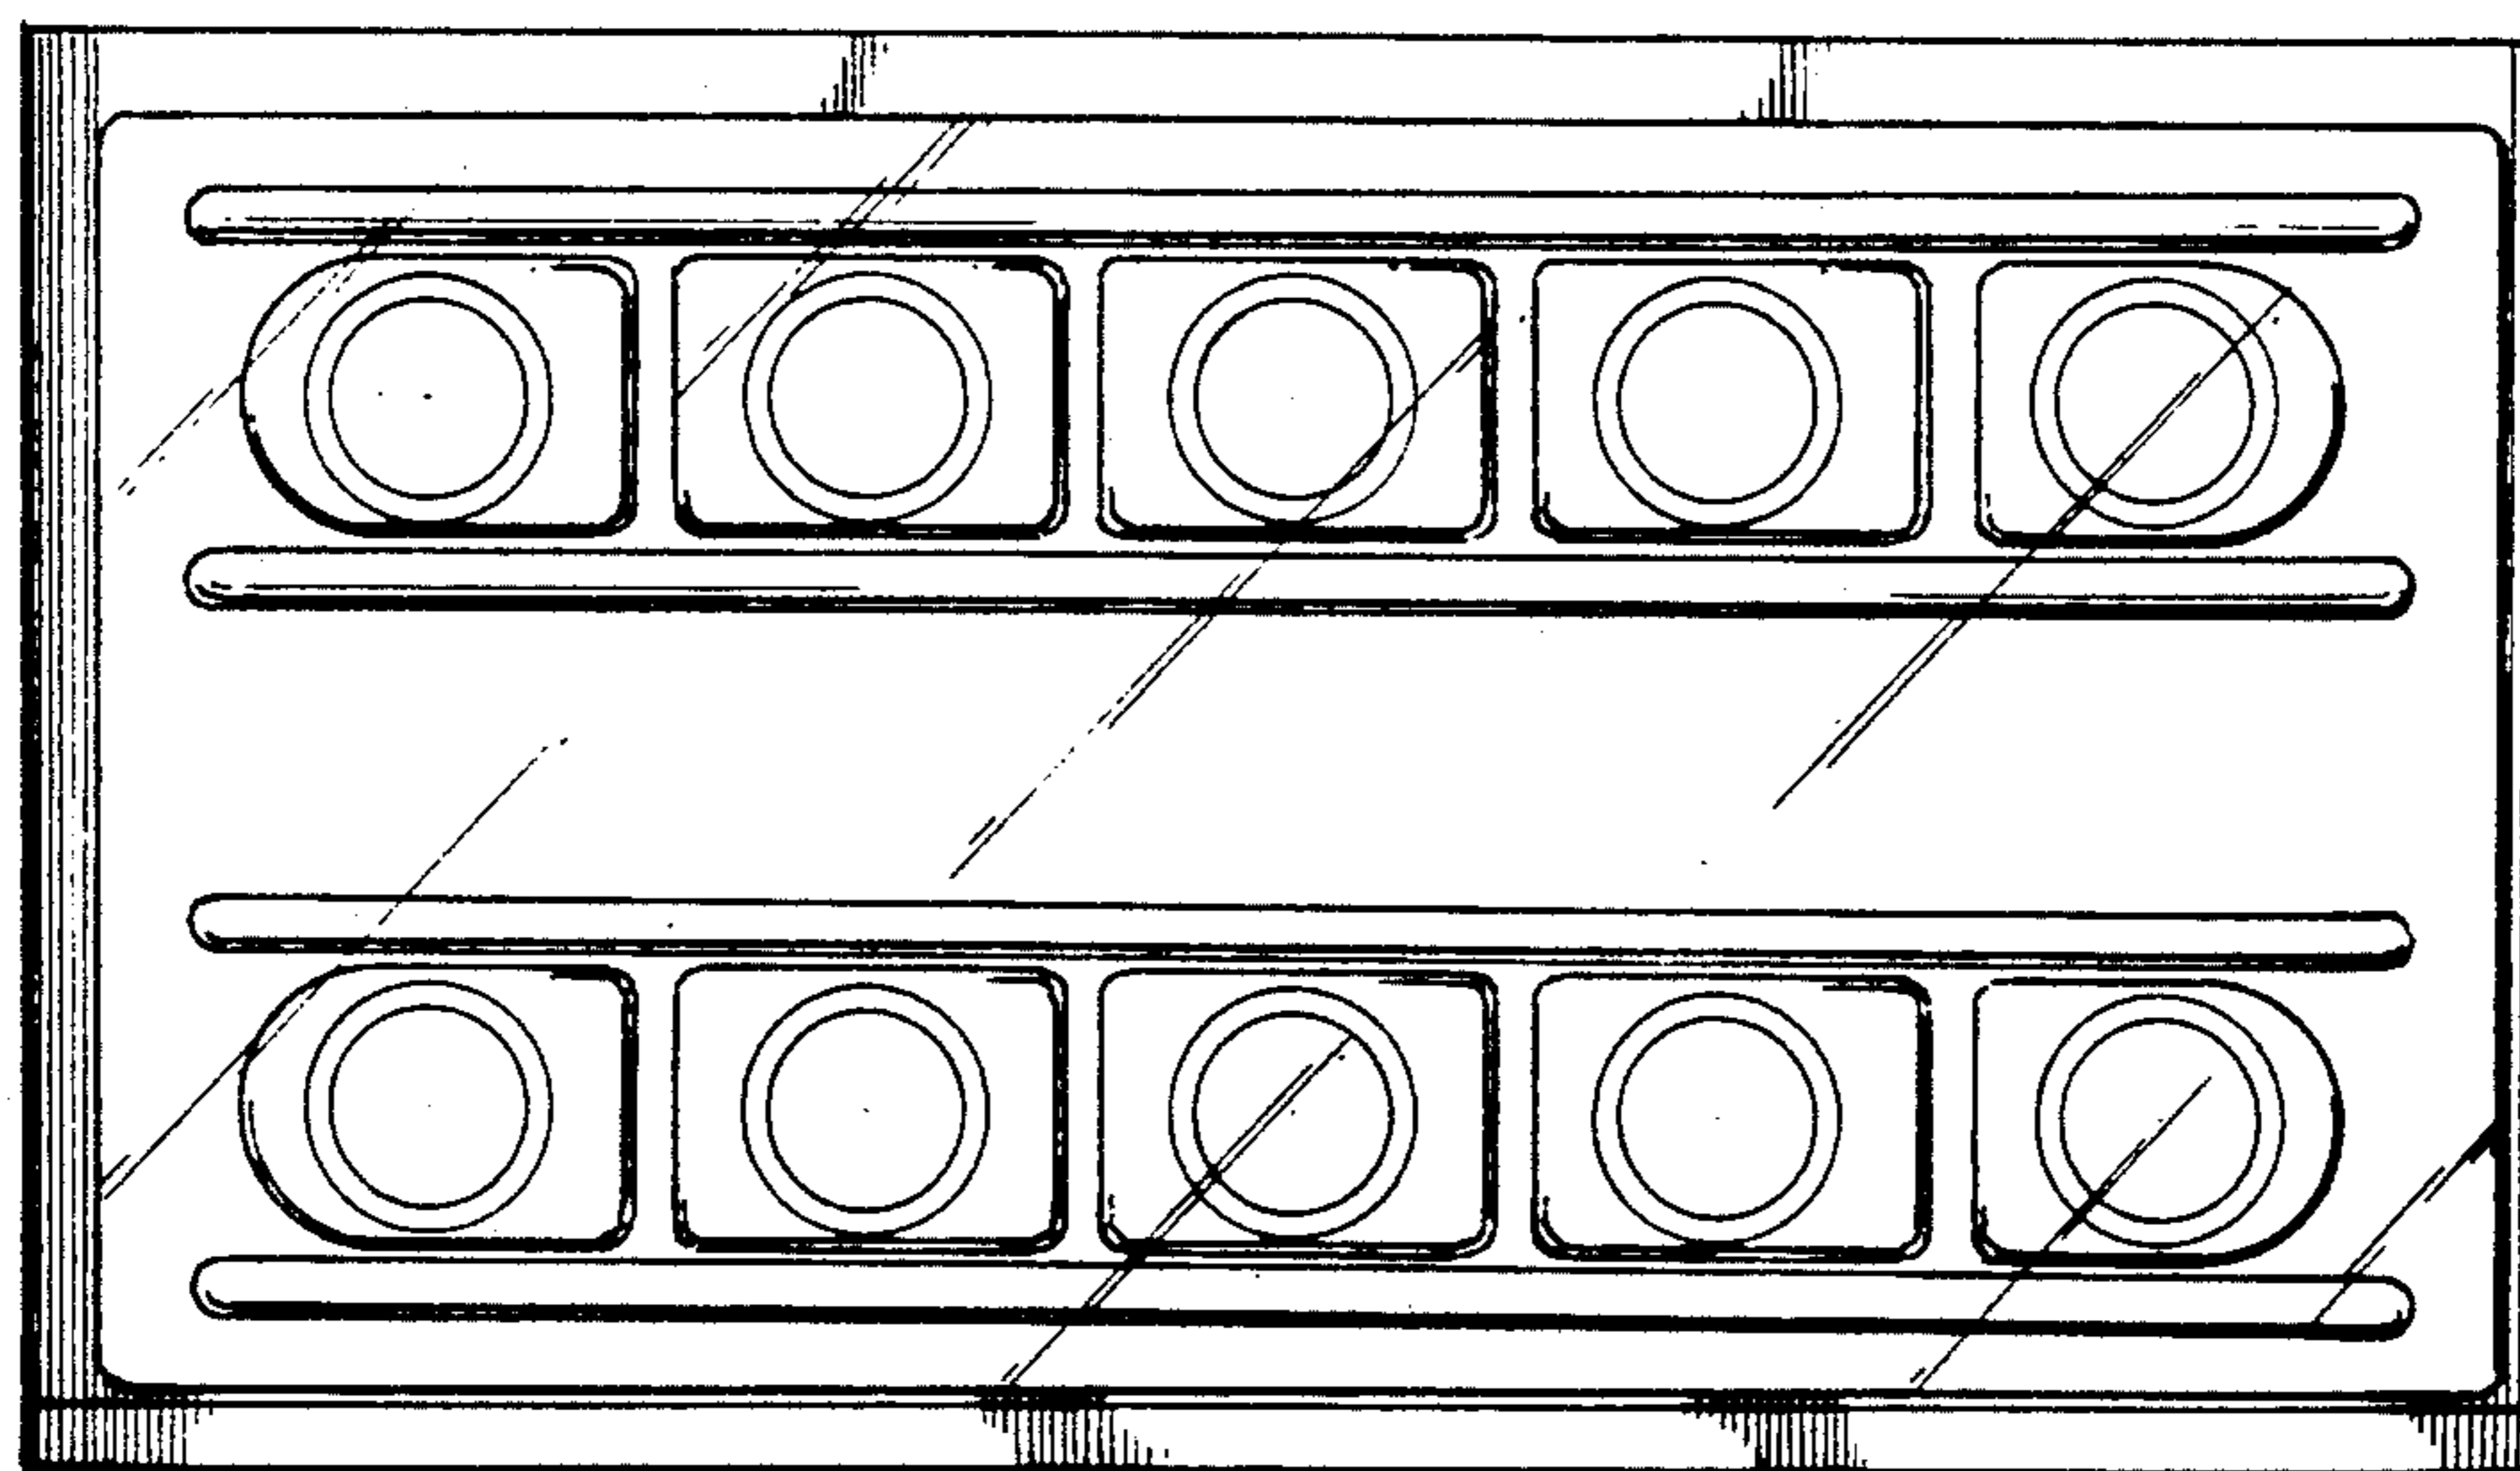


FIG. 3



FIG. 4

