



US00D342313S

United States Patent [19]

[11] Patent Number: Des. 342,313

Hood et al.

[45] Date of Patent: ** Dec. 14, 1993

[54] **ULTRASONIC CUTTING OSTEOTOME**

[75] Inventors: **Larry L. Hood, Laguna Hills; Gregg Hughes, El Toro, both of Calif.**

[73] Assignee: **Advanced Osseous Technologies, Inc., Aliso Viejo, Calif.**

[**] Term: **14 Years**

[21] Appl. No.: **714,097**

[22] Filed: **Jun. 11, 1991**

[52] U.S. Cl. **D24/146; D24/133**

[58] Field of Search **D24/146, 147, 170, 231, D24/232; D8/47, 101, 98; D19/35; 606/79, 83, 169; 604/22; 128/24 AA, 24 A; 30/167, 168, 169**

[56] **References Cited**

U.S. PATENT DOCUMENTS

| | | | |
|------------|---------|----------------------|-----------|
| D. 289,084 | 3/1987 | Freitag | D24/144 |
| 1,092,447 | 4/1914 | Leland | 30/167 |
| 2,714,890 | 8/1955 | Vang . | |
| 3,086,288 | 4/1963 | Balamuth et al. . | |
| 3,526,219 | 9/1970 | Balamuth . | |
| 3,589,363 | 6/1971 | Banko et al. . | |
| 3,693,613 | 9/1972 | Kelman . | |
| 3,809,977 | 5/1974 | Balamuth et al. . | |
| 3,823,717 | 7/1974 | Pohlman et al. . | |
| 3,862,630 | 1/1975 | Balamuth . | |
| 3,990,452 | 11/1976 | Murry et al. . | |
| 4,041,947 | 8/1977 | Weiss et al. . | |
| 4,063,557 | 12/1977 | Wuchinich et al. . | |
| 4,184,510 | 1/1980 | Murry et al. . | |
| 4,188,952 | 2/1980 | Loschilov et al. . | |
| 4,248,232 | 2/1981 | Engelbrecht et al. . | |
| 4,298,074 | 11/1981 | Matthen . | |
| 4,425,115 | 1/1984 | Wuchinich . | |
| 4,660,557 | 4/1987 | Collis, Jr. | D24/147 X |
| 4,705,038 | 11/1987 | Sjostrom et al. . | |
| 4,705,500 | 11/1987 | Reimels et al. . | |
| 4,750,488 | 6/1988 | Wuchinich et al. . | |
| 4,832,683 | 5/1989 | Idemoto et al. . | |
| 4,834,081 | 5/1989 | Van Zile . | |
| 4,846,161 | 7/1989 | Roger . | |
| 5,019,083 | 5/1991 | Klapper et al. . | |

OTHER PUBLICATIONS

Orthopedic Catalog "Richards Manufacturing Co" pp. 10, 14, 20.

Codman Catalog For Surgical Products. 1984 p. 82 Elevators, Periosteal item A (65-1030) ©1984.

"Complete Replacement Arthroplasty of the Hip by the Ring Prosthesis", The Journal of Bone and Joint Surgery, P. A. Ring, pp. 720-731 (British) vol. 50B, No. 4, Nov. 1968.

"A New Technique for Removal of Broken Femoral Stems in Total Hip Replacement" by William H. Harris, et al., The Journal of Bone and Joint Surgery, vol. 63-A, No. 5, Jun. 1981.

Biological Fixation of the Porocoat AML® Hip—Manual for Pre-Operative Planning and Recommended Surgical Technique (1984) by Charles A. Engh, M.D. and J. Dennis Bobyn, Ph.D.

"Proximal Femoral Osteotomy in Difficult Revision Hip Surgery: How to Revise the Unrevisable" by Hugh H. Cameron, Ph.D., Contemporary Orthopaedics, May 1989, vol. 18, No. 5.

Photographs 1-3 illustrating an ultrasonic aspiration surgical tool used in neural surgery, designed by Dr. David Wuchinich and disclosed in 1967.

Photographs 4-15 illustrating three ultrasonic surgical tools manufactured by Quinton and distributed by Howmedica, Inc. in 1985.

Primary Examiner—A. Hugo Word

Assistant Examiner—I. Simmons

Attorney, Agent, or Firm—Knobbe, Martens, Olson & Bear

[57] **CLAIM**

The ornamental design for an ultrasonic cutting osteotome, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of the ultrasonic cutting osteotome showing our new design;


FIG. 2 is a top plan view thereof, the view opposite that disclosed in FIG. 2 is identical to that shown in FIG. 2;

FIG. 3 is a side elevational view thereof, the view opposite to that disclosed in FIG. 3 is identical to that shown in FIG. 3;

FIG. 4 is an end elevational view thereof; and,

FIG. 5 is an end elevational view opposite that shown in FIG. 4;

The broken line showing of the connector in FIGS. 1-3 is for illustrative purposes only and forms no part of the claimed design.

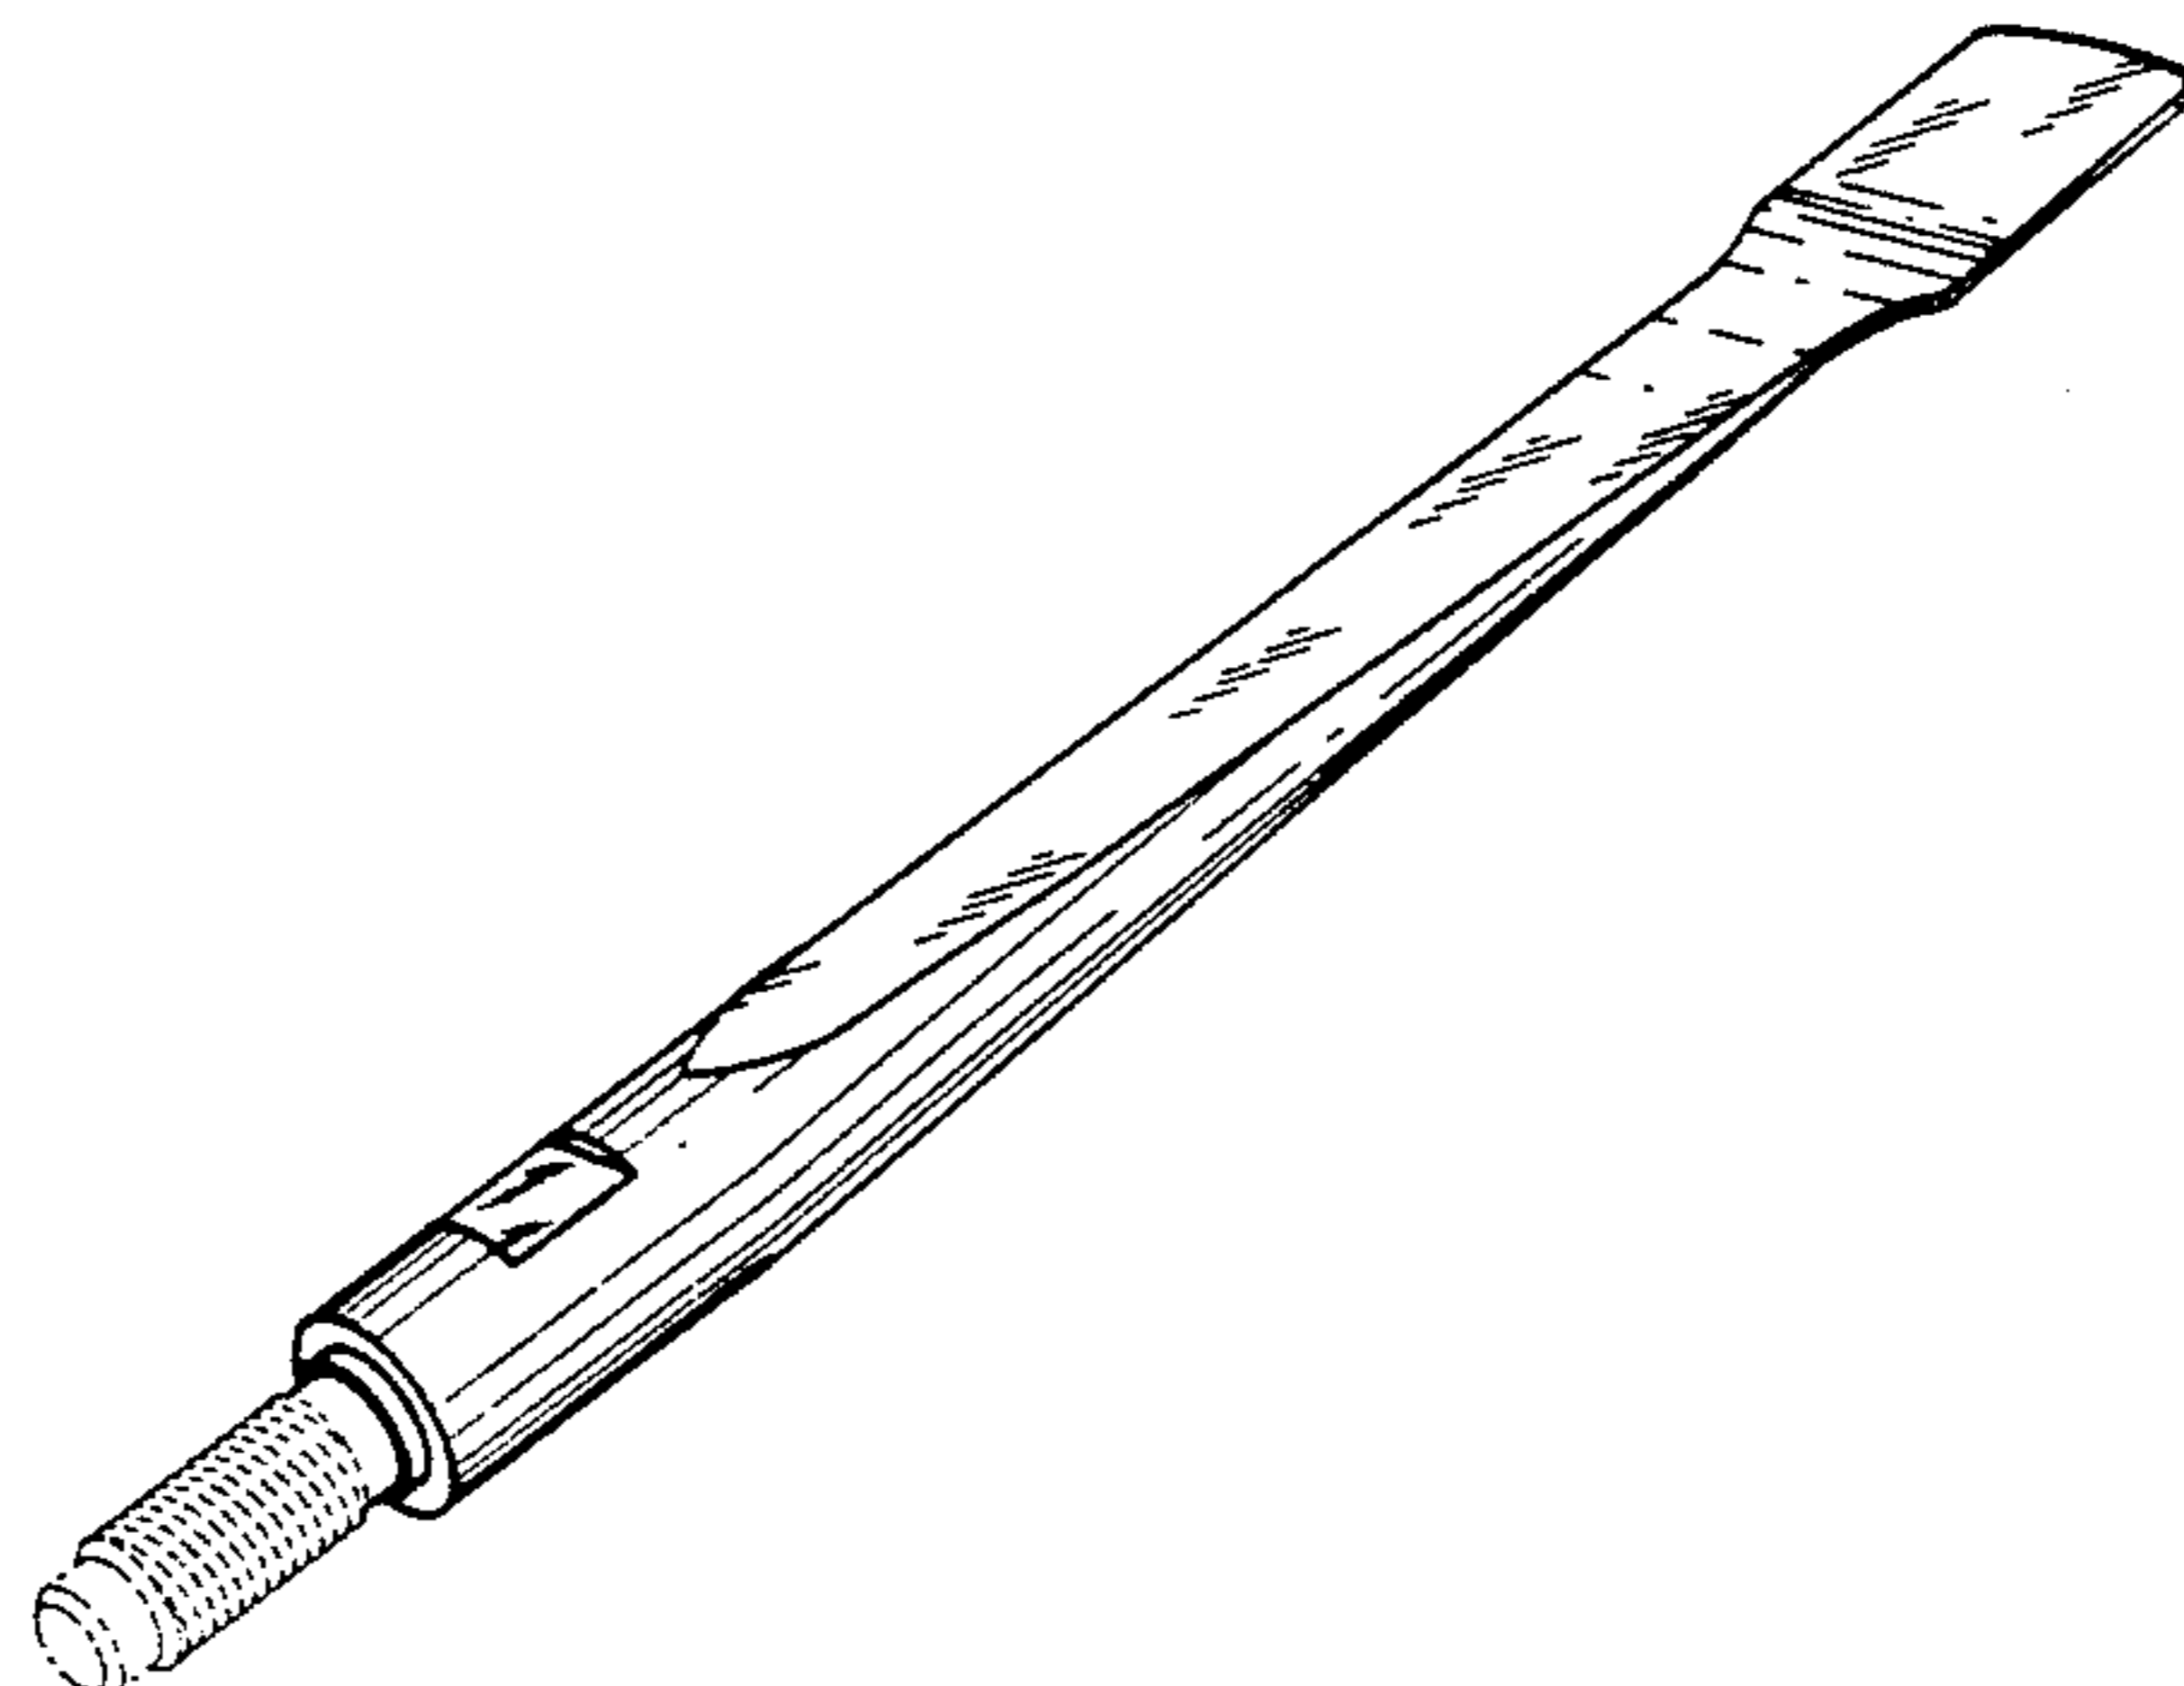

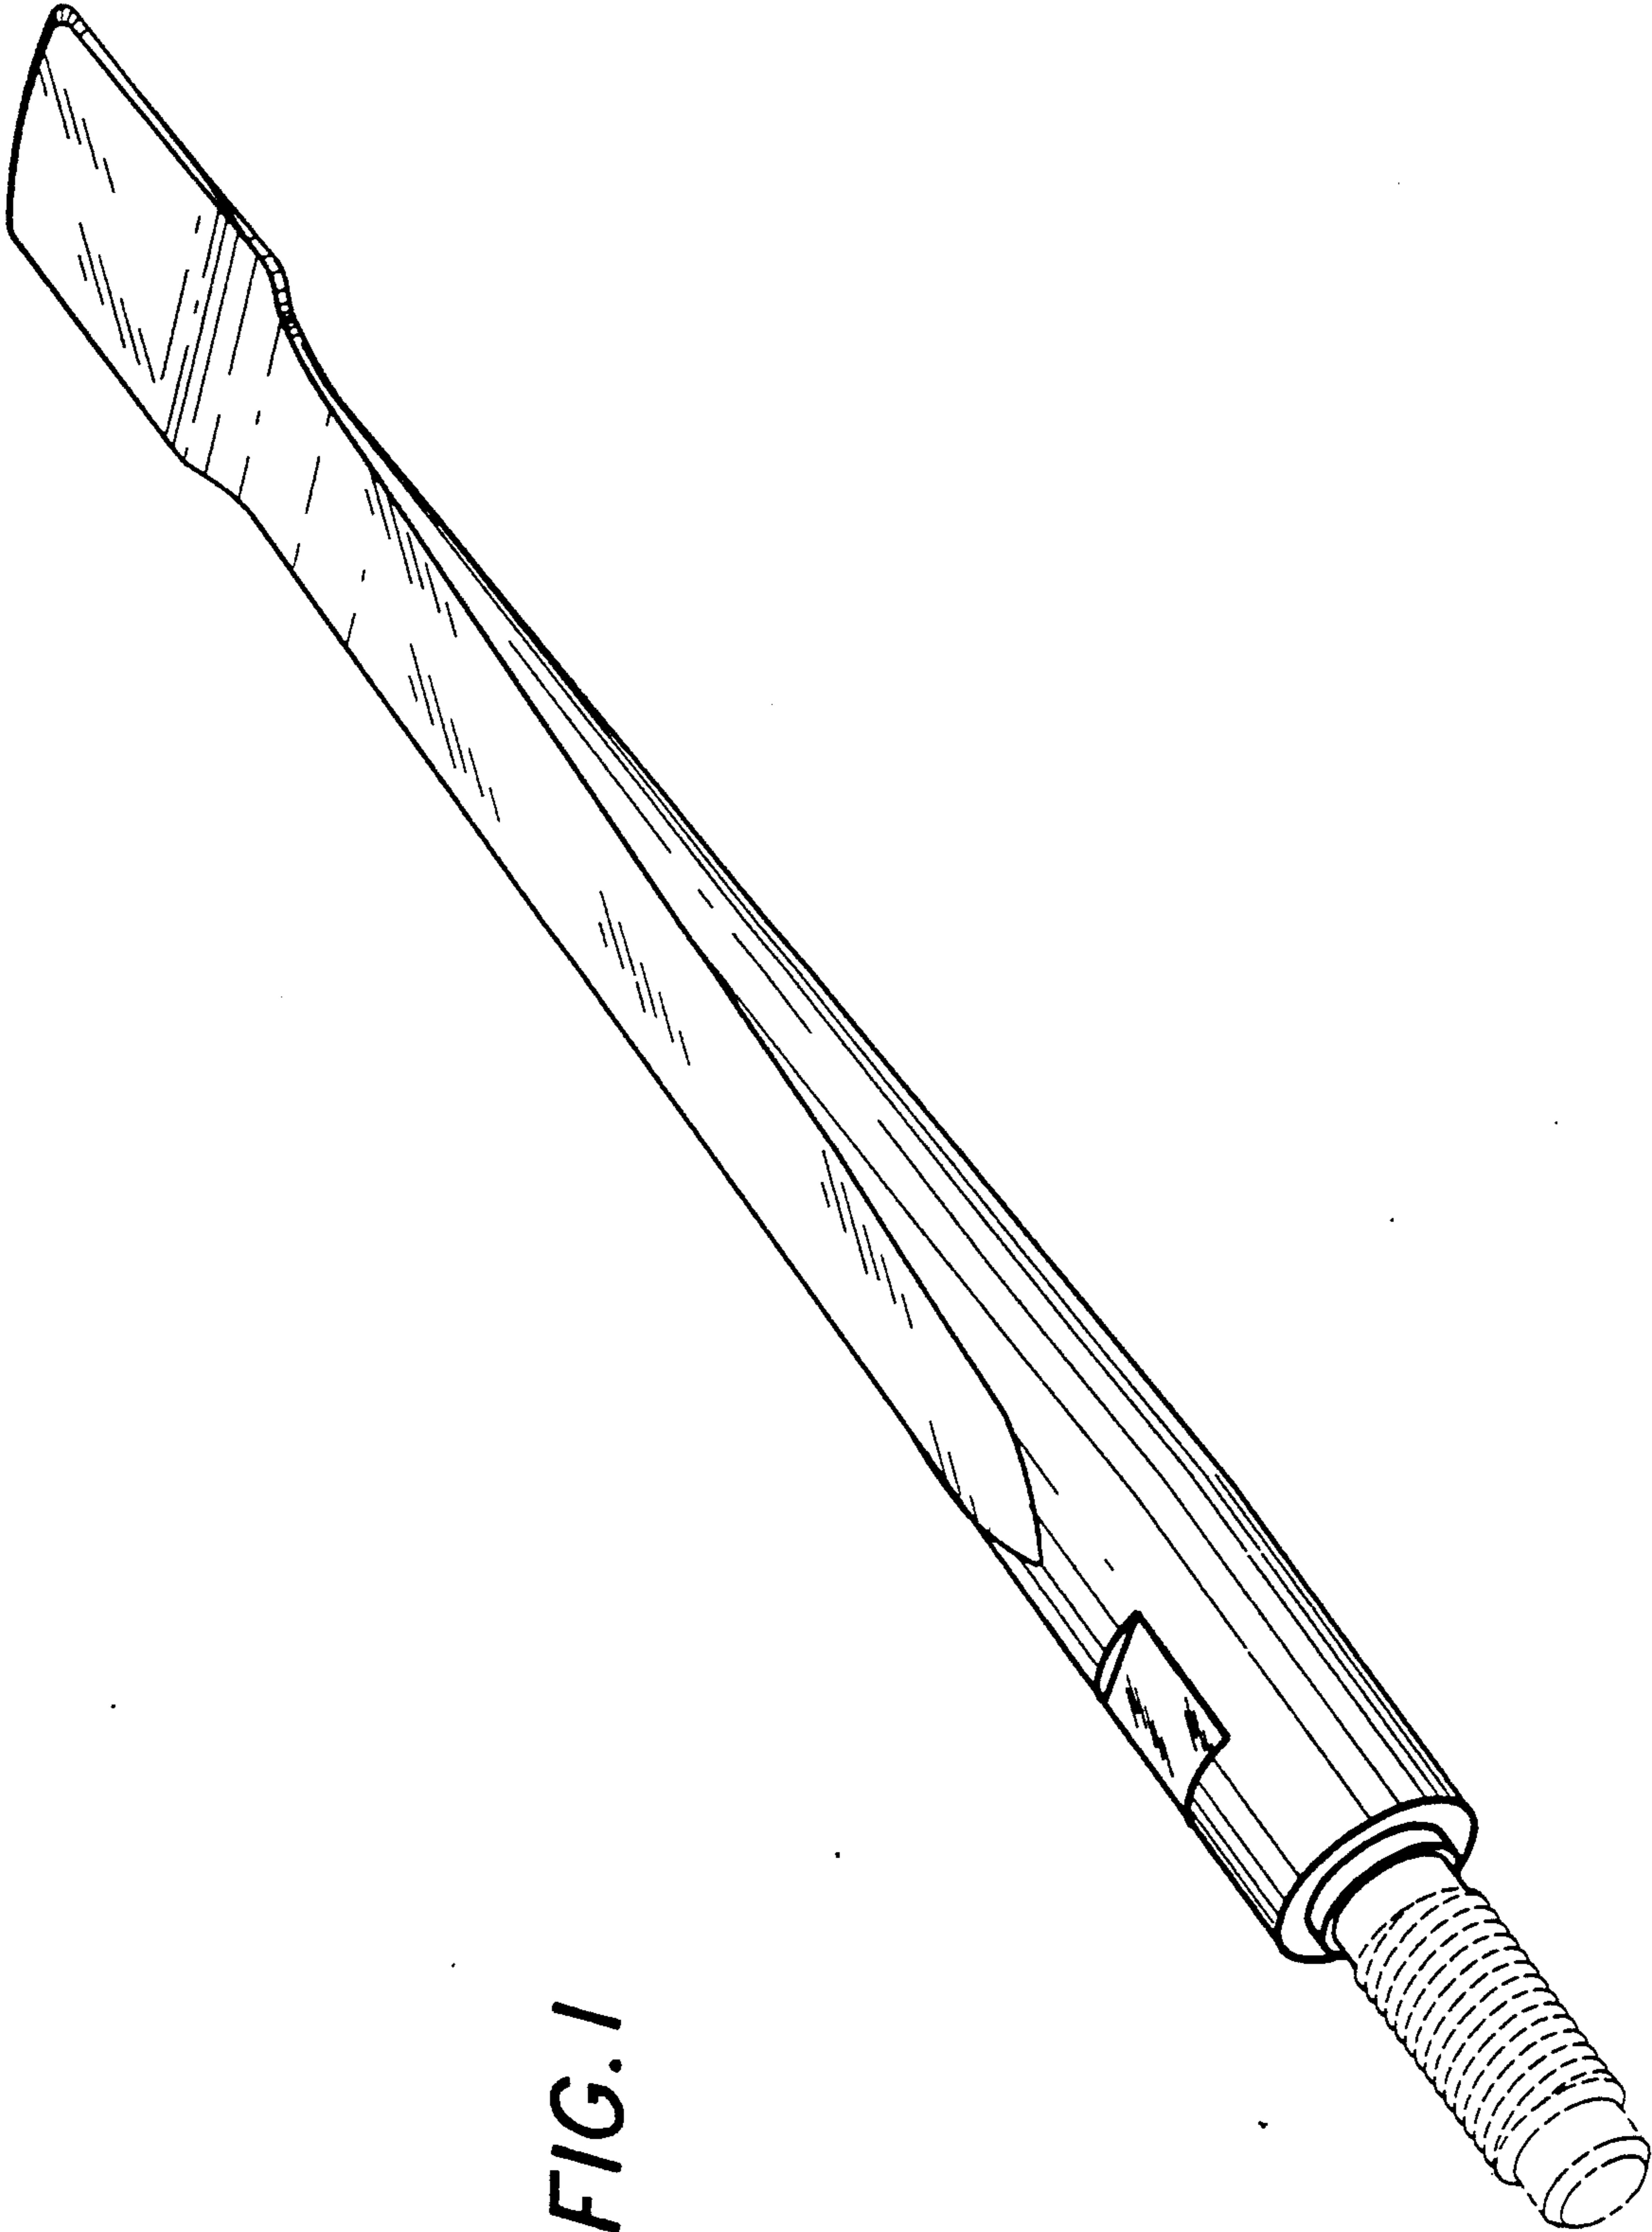


FIG. 1

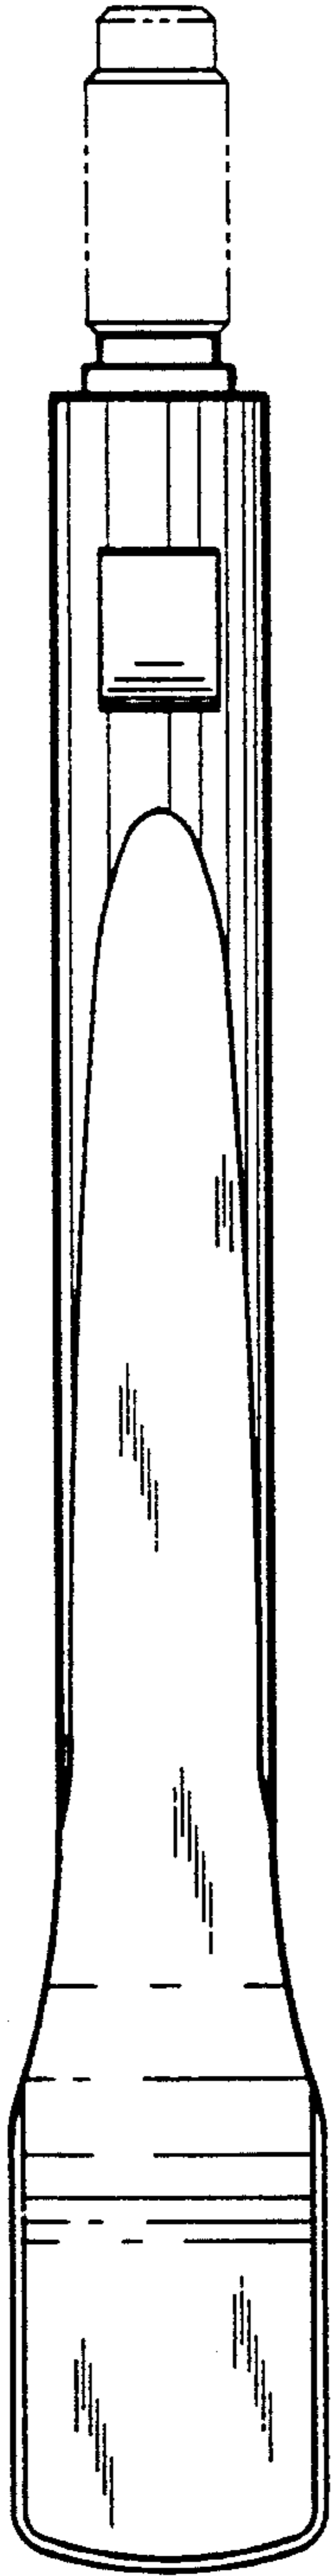


FIG. 2

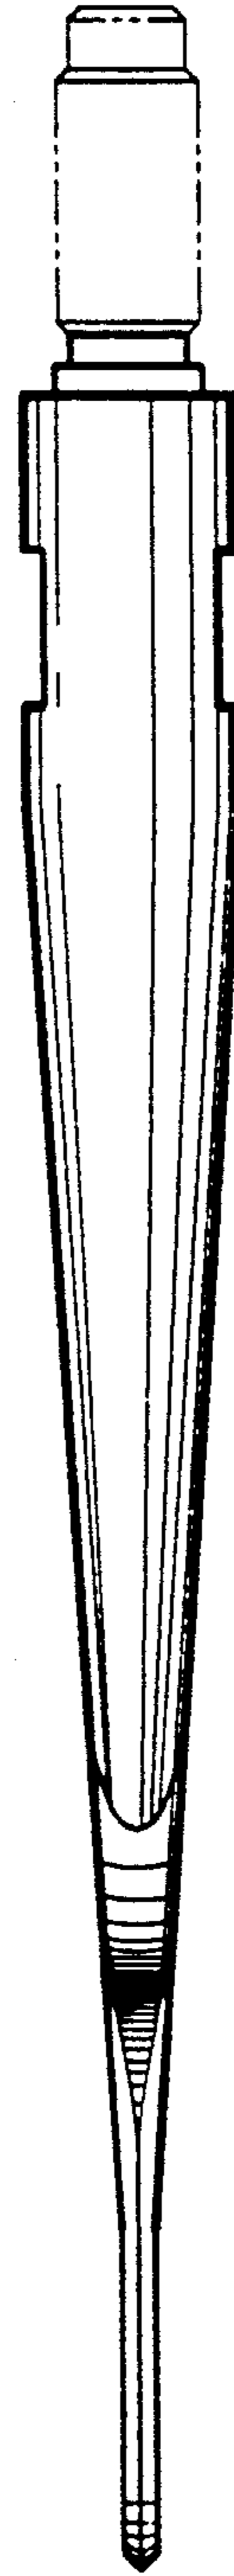


FIG. 3

FIG. 4

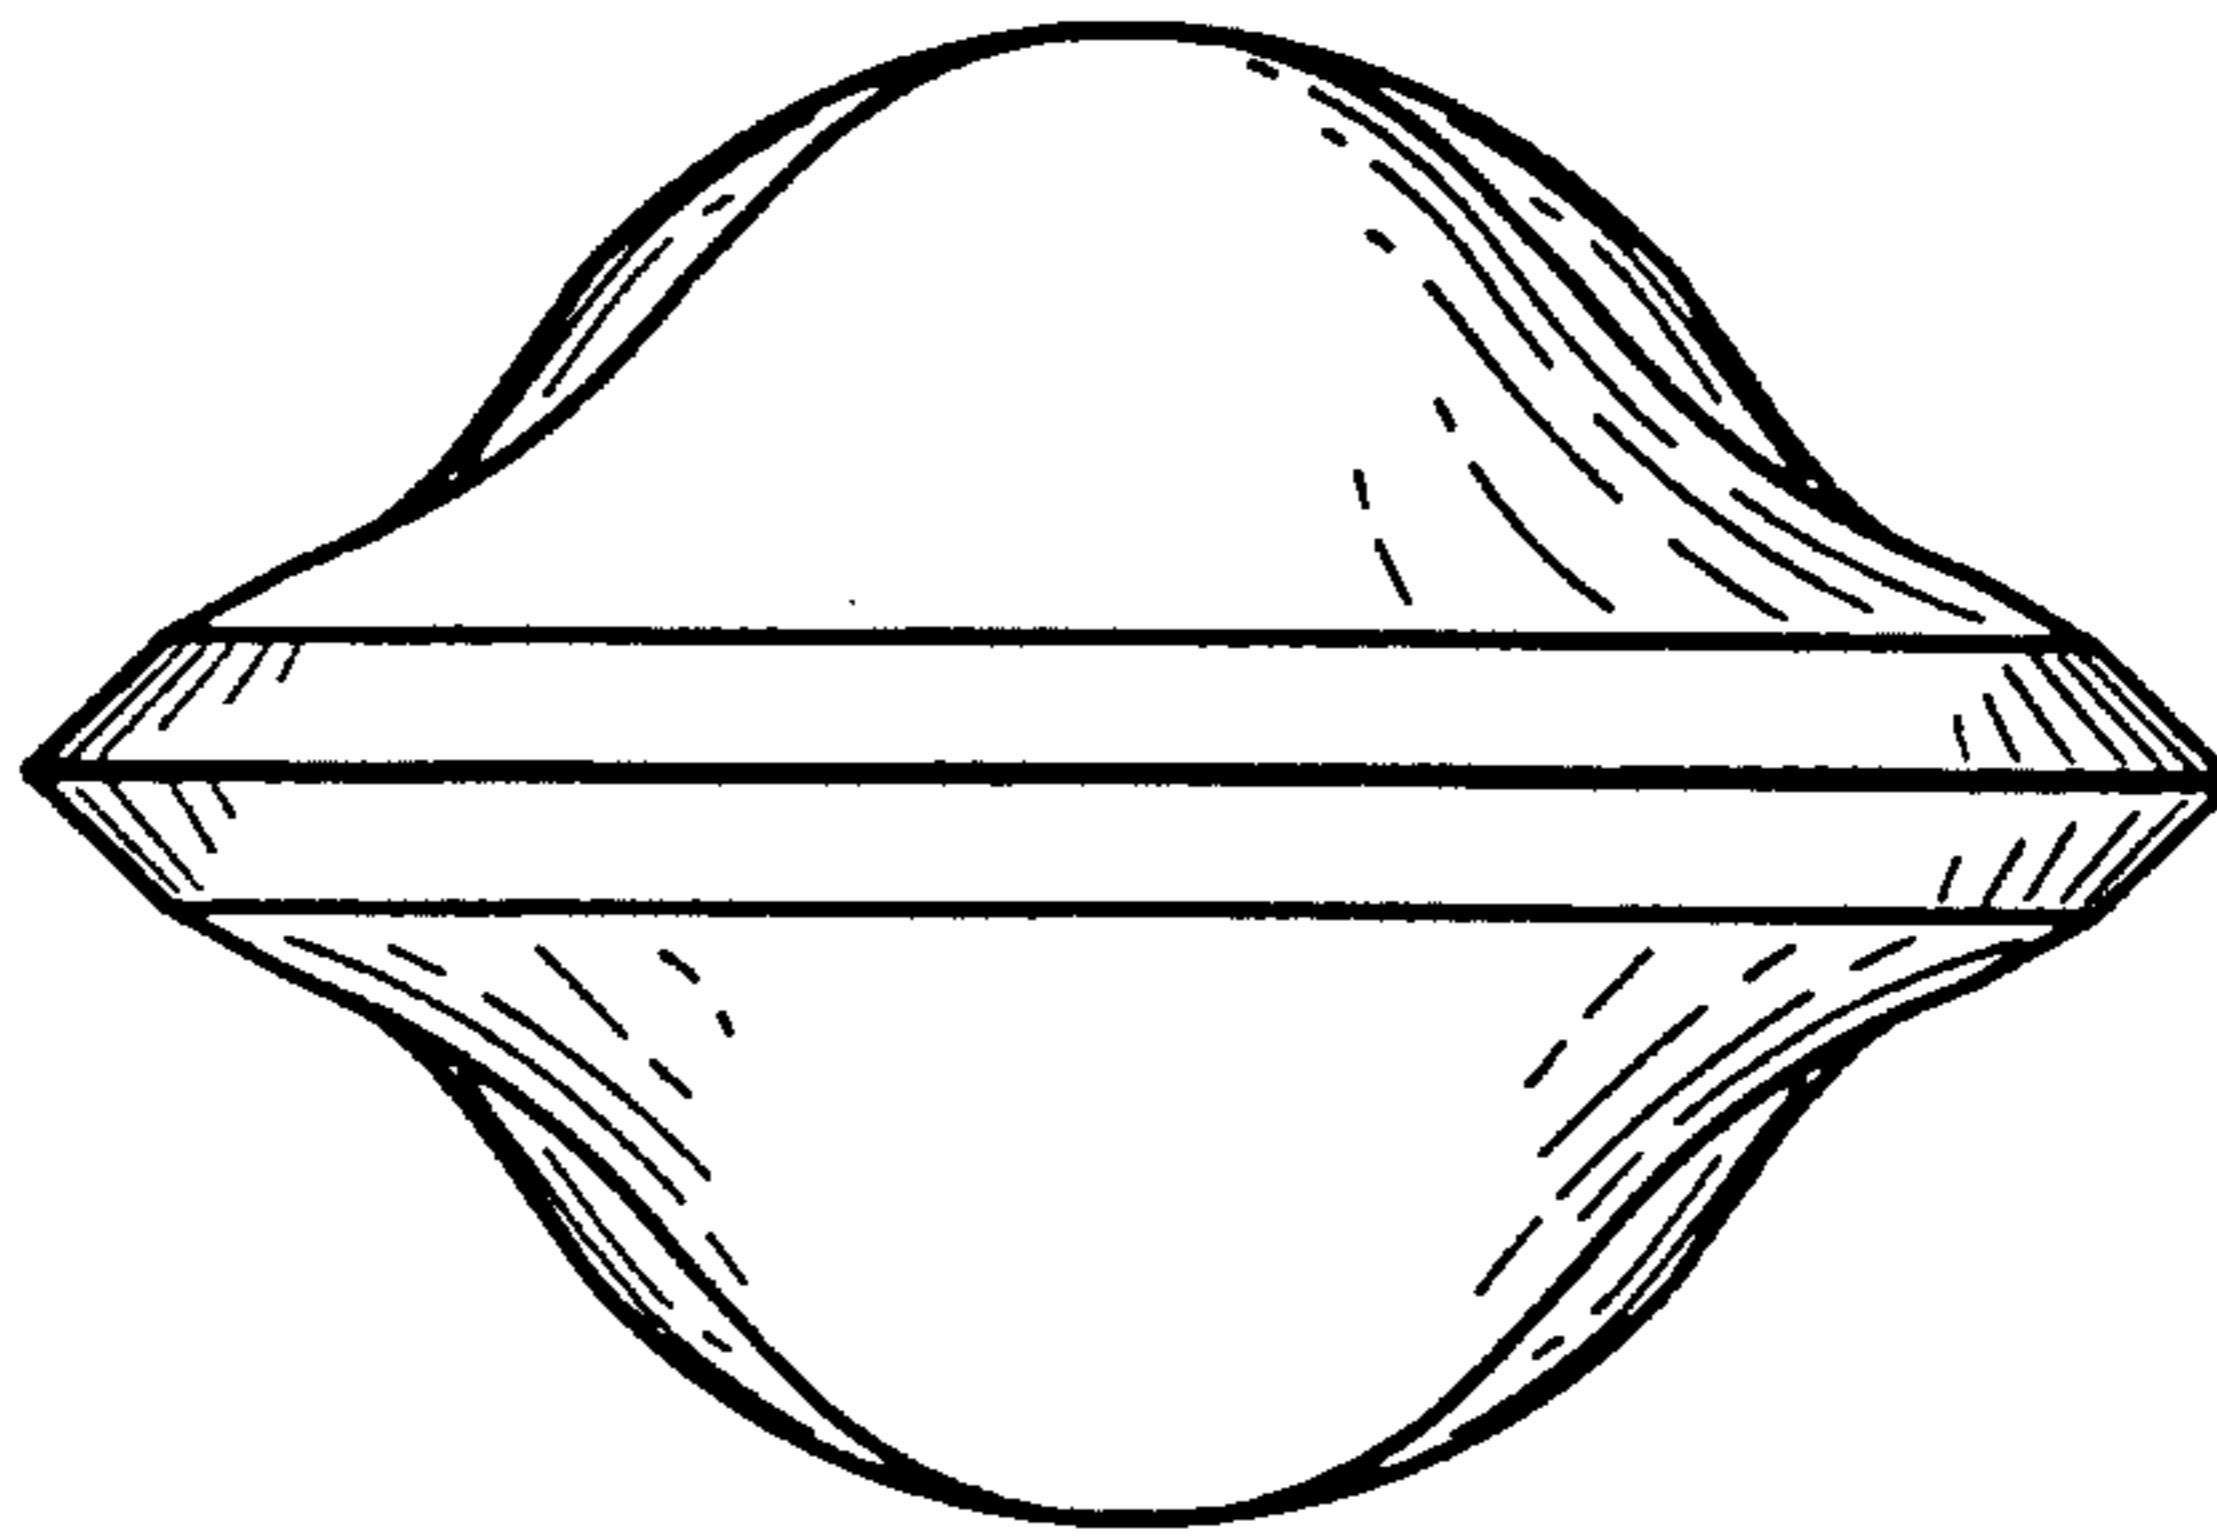


FIG. 5

