



US00D344902S

# United States Patent [19]

North et al.

[11] Patent Number: **Des. 344,902**

[45] Date of Patent: **\*\* Mar. 8, 1994**

## [54] DIAGNOSTIC ELECTRODE

[75] Inventors: **John R. North**, Durrington, United Kingdom; **Robert L. Kay**, Thousand Oaks; **Jonathan Ivy**, Ventura, both of Calif.

[73] Assignee: **Porton Diagnostics, Inc.**, Westlake Village, Calif.

[\*\*] Term: **14 Years**

[21] Appl. No.: **917,601**

[22] Filed: **Jul. 21, 1992**

[52] U.S. Cl. .... **D10/78**

[58] Field of Search ..... **607/4, 27, 29; 128/798, 128/802, 803, 741, 420.5, 639; 204/400, 416-420; D10/80; D24/150**

## [56] References Cited

### U.S. PATENT DOCUMENTS

4,655,899 4/1987 Saito et al. .... 204/416 X  
4,664,772 5/1987 Zaccari et al. .... 204/416 X


*Primary Examiner*—Alan P. Douglas  
*Assistant Examiner*—Antoine D. Davis  
*Attorney, Agent, or Firm*—Kenyon & Kenyon


## [57] CLAIM

The ornamental design for a diagnostic electrode, as shown and described.

## DESCRIPTION


FIG. 1 is a top right side perspective view of a diagnostic electrode showing our new design; FIG. 2 is a top plan view thereof; FIG. 3 is a bottom plan view thereof; FIG. 4 is a rear elevational view thereof; FIG. 5 is a front elevational view thereof; and, FIG. 6 is a right side view thereof.

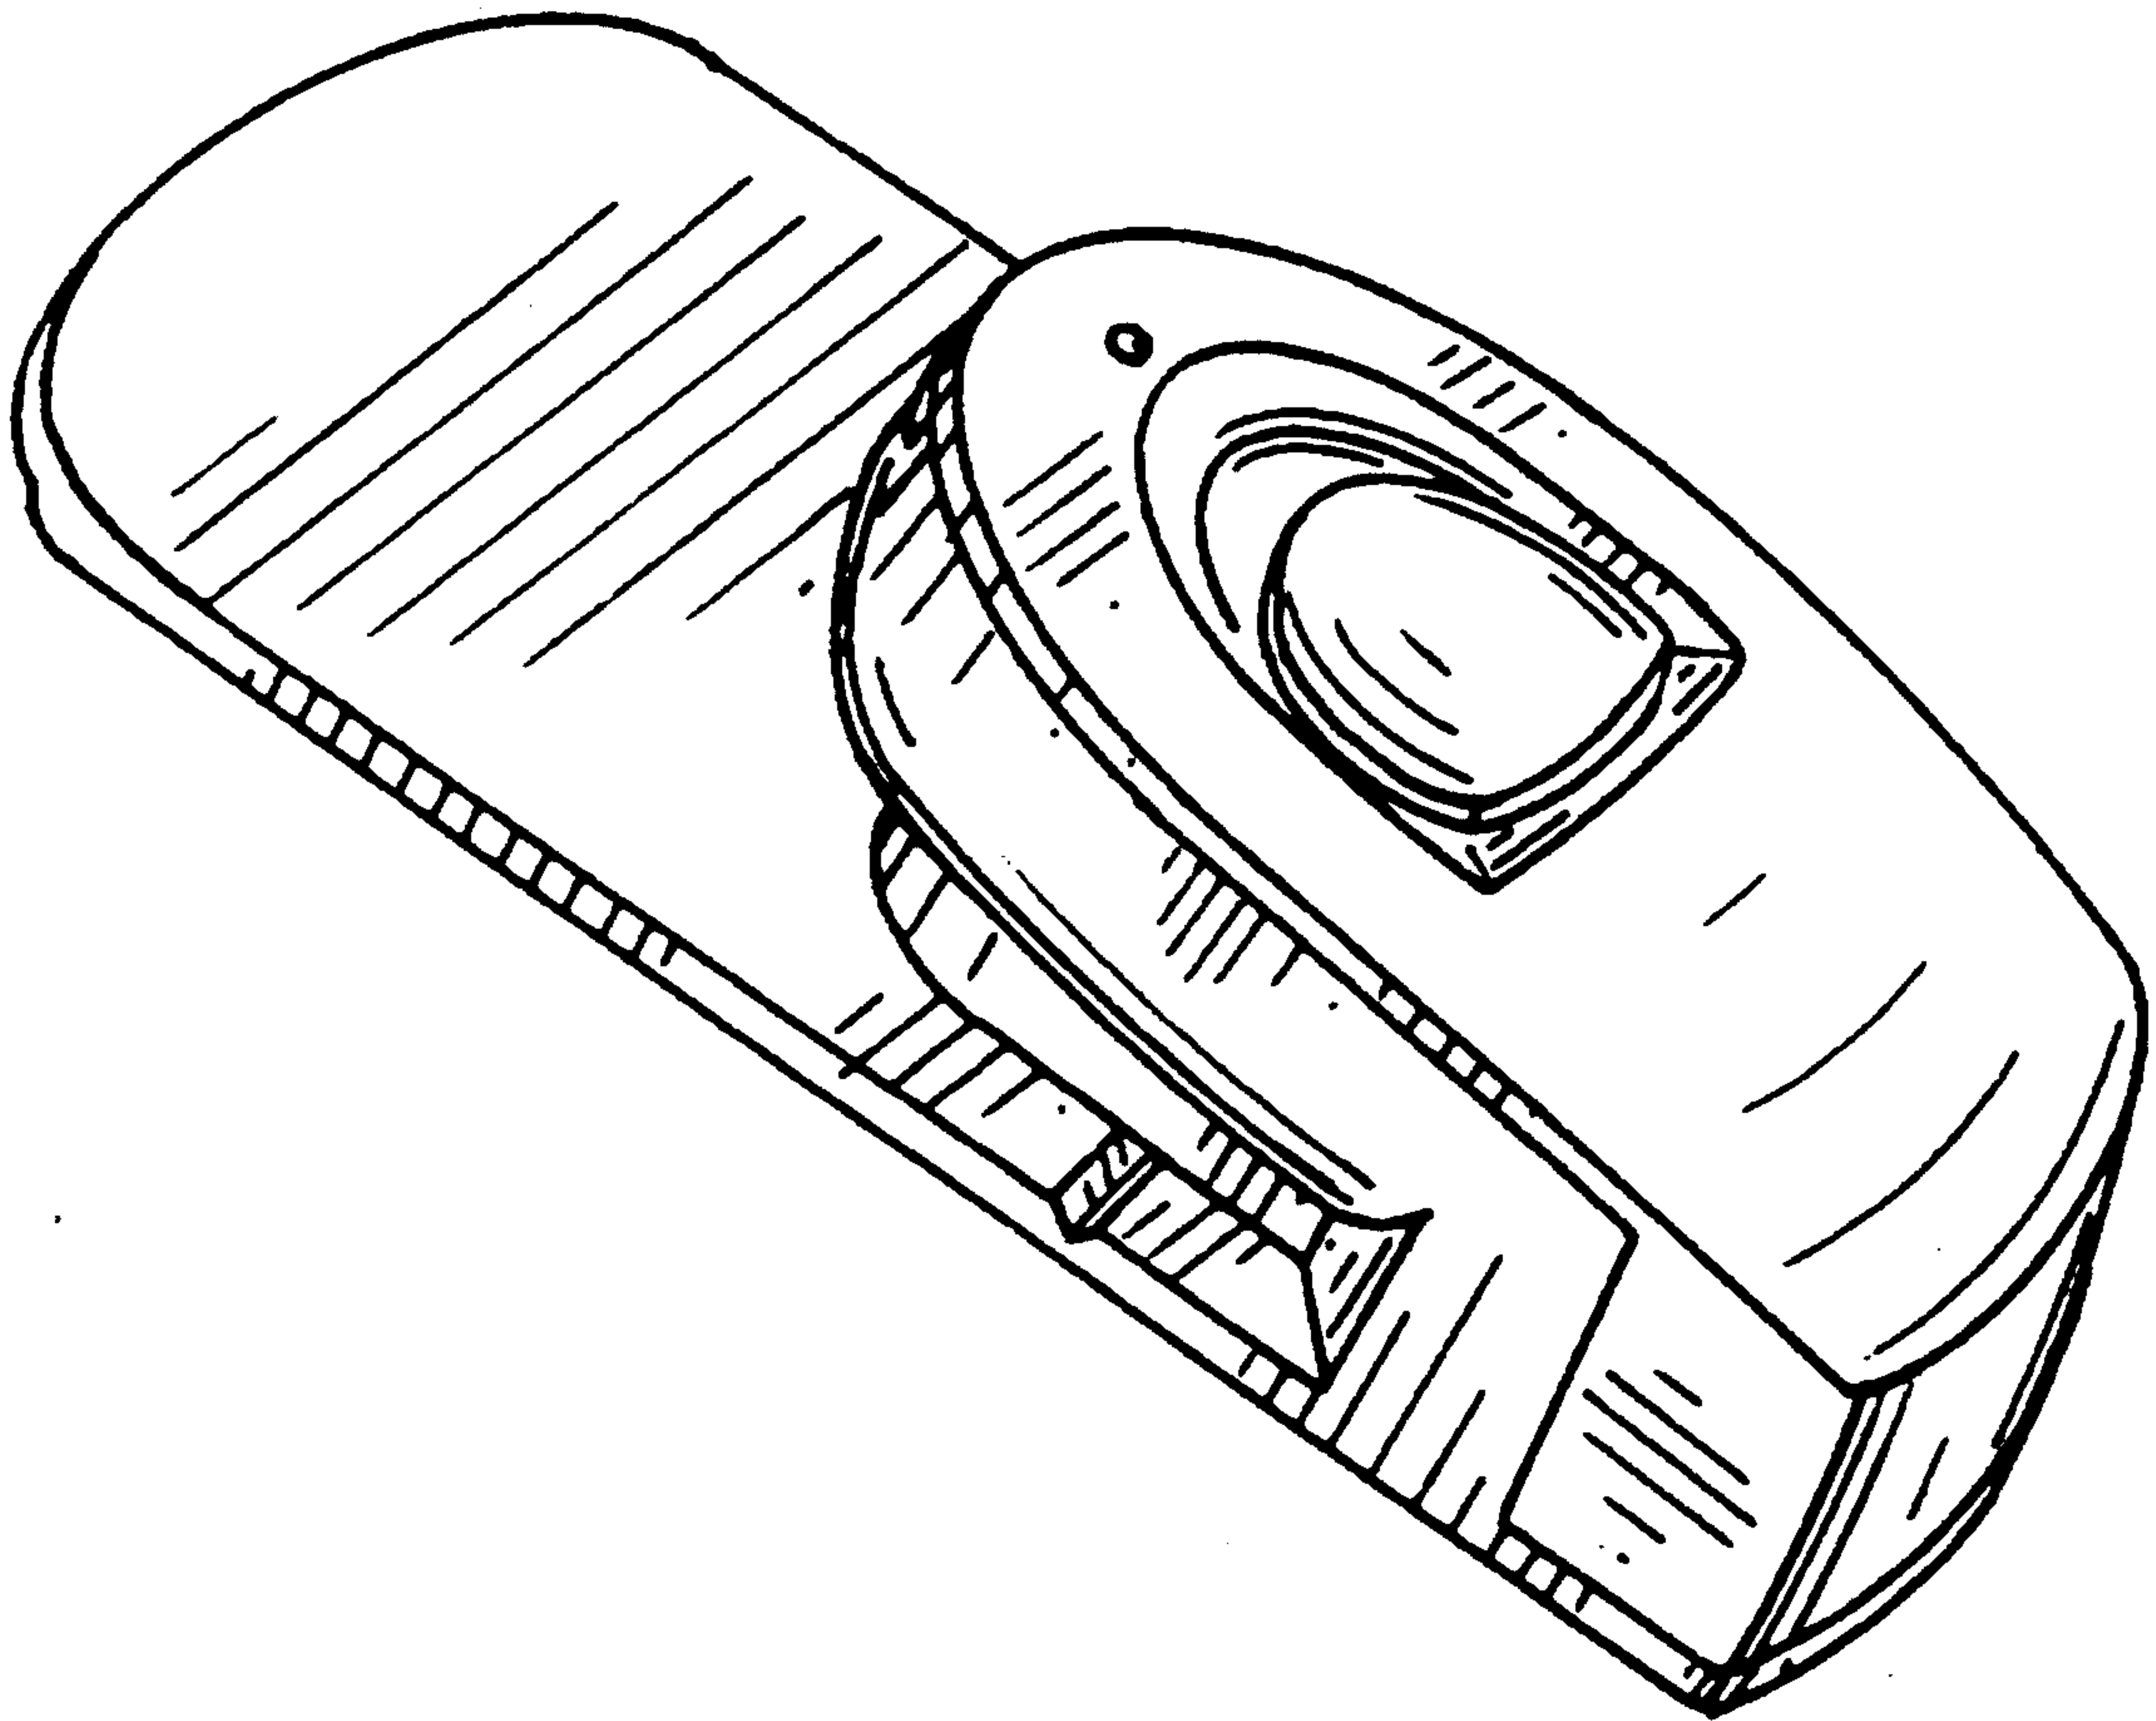



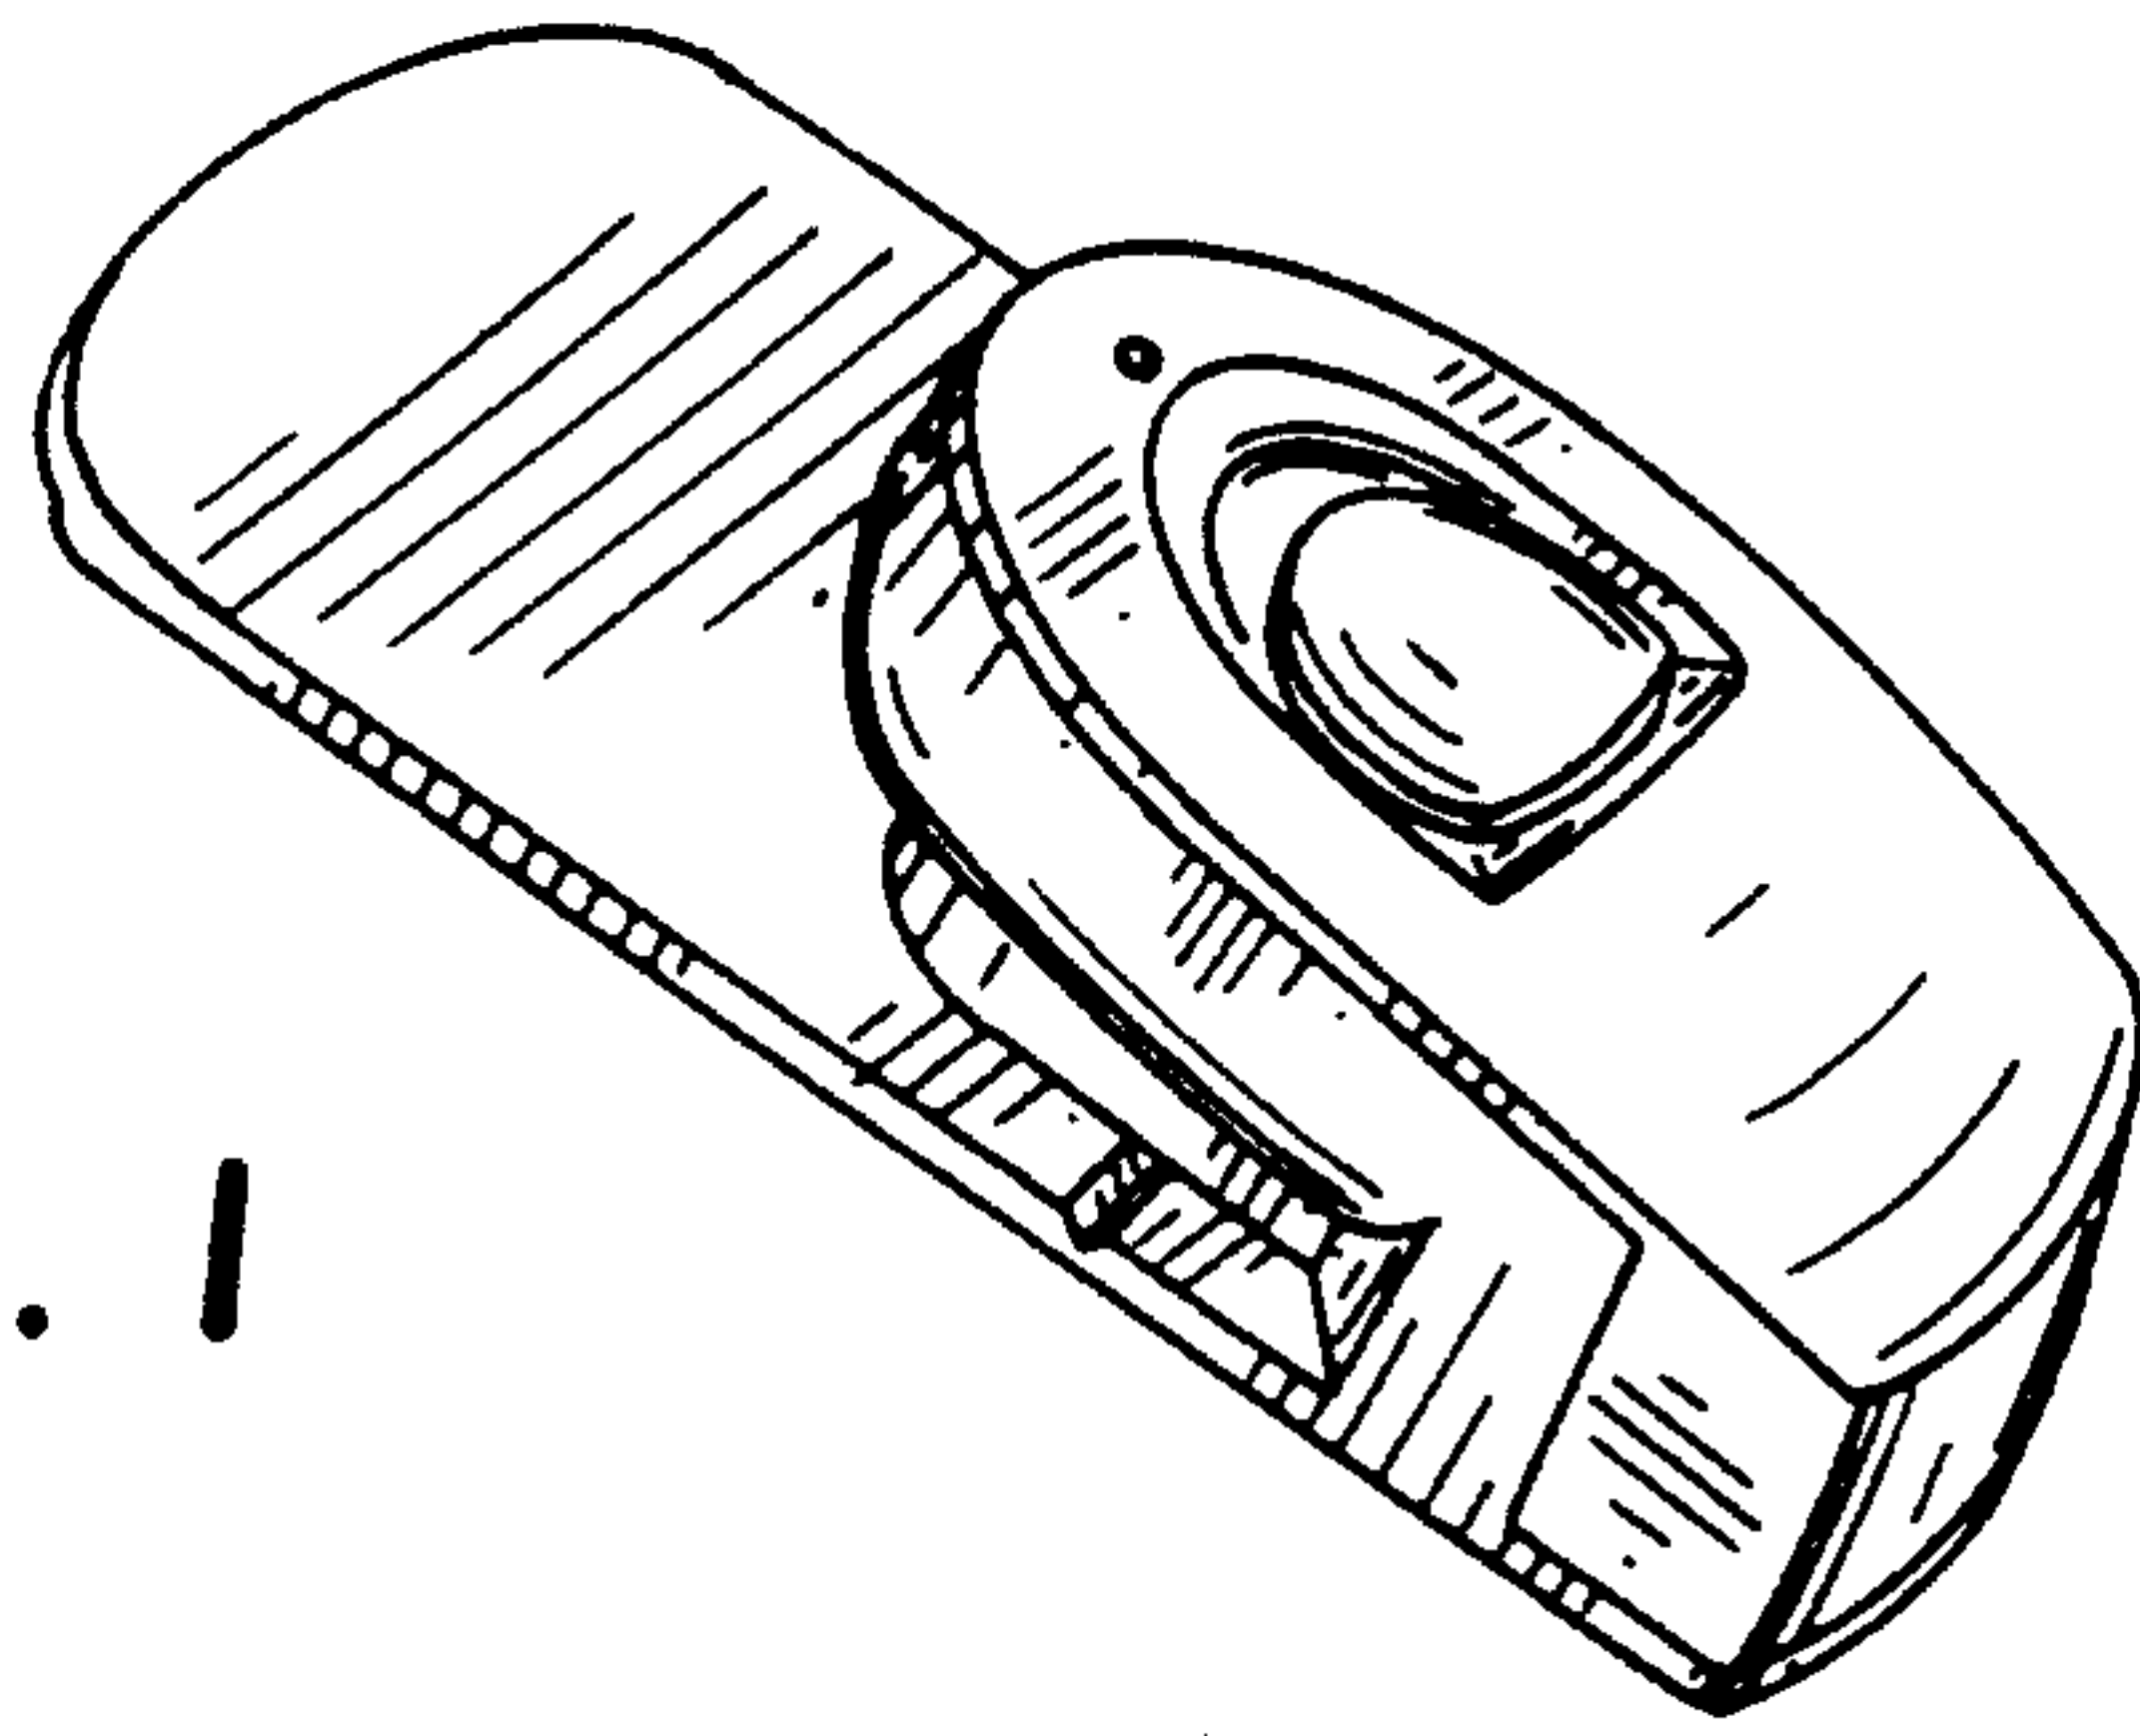


**FIG. 1**

**FIG. 2**

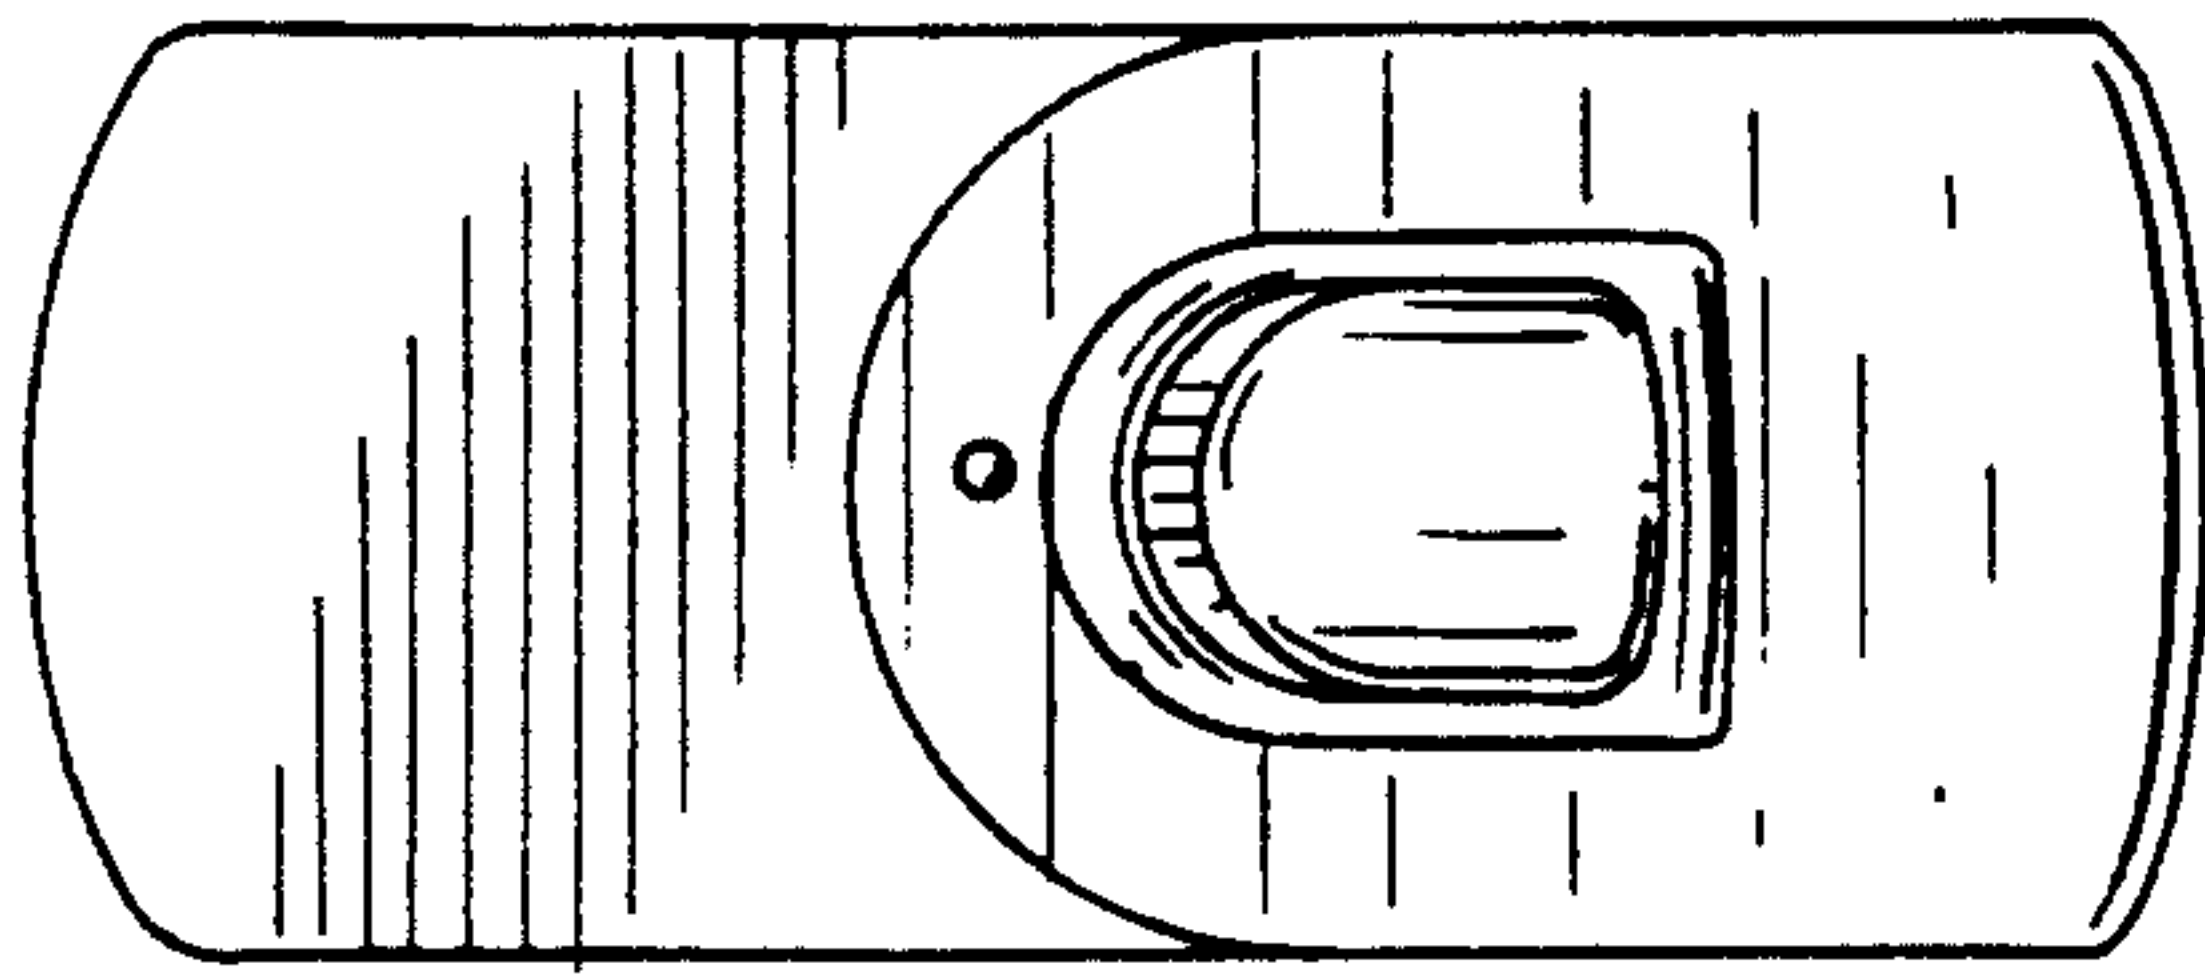


**FIG. 4**

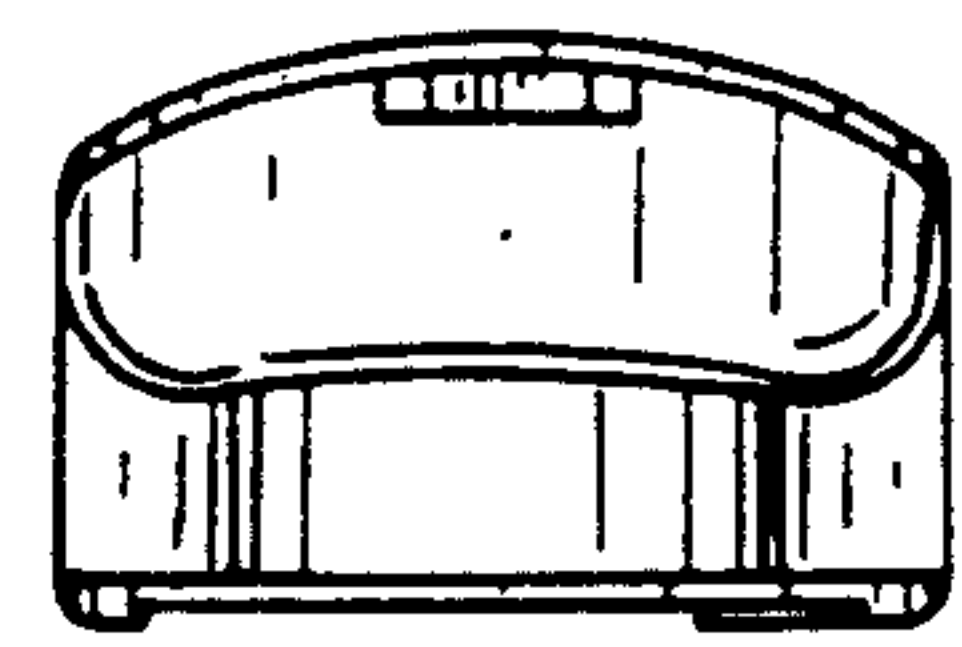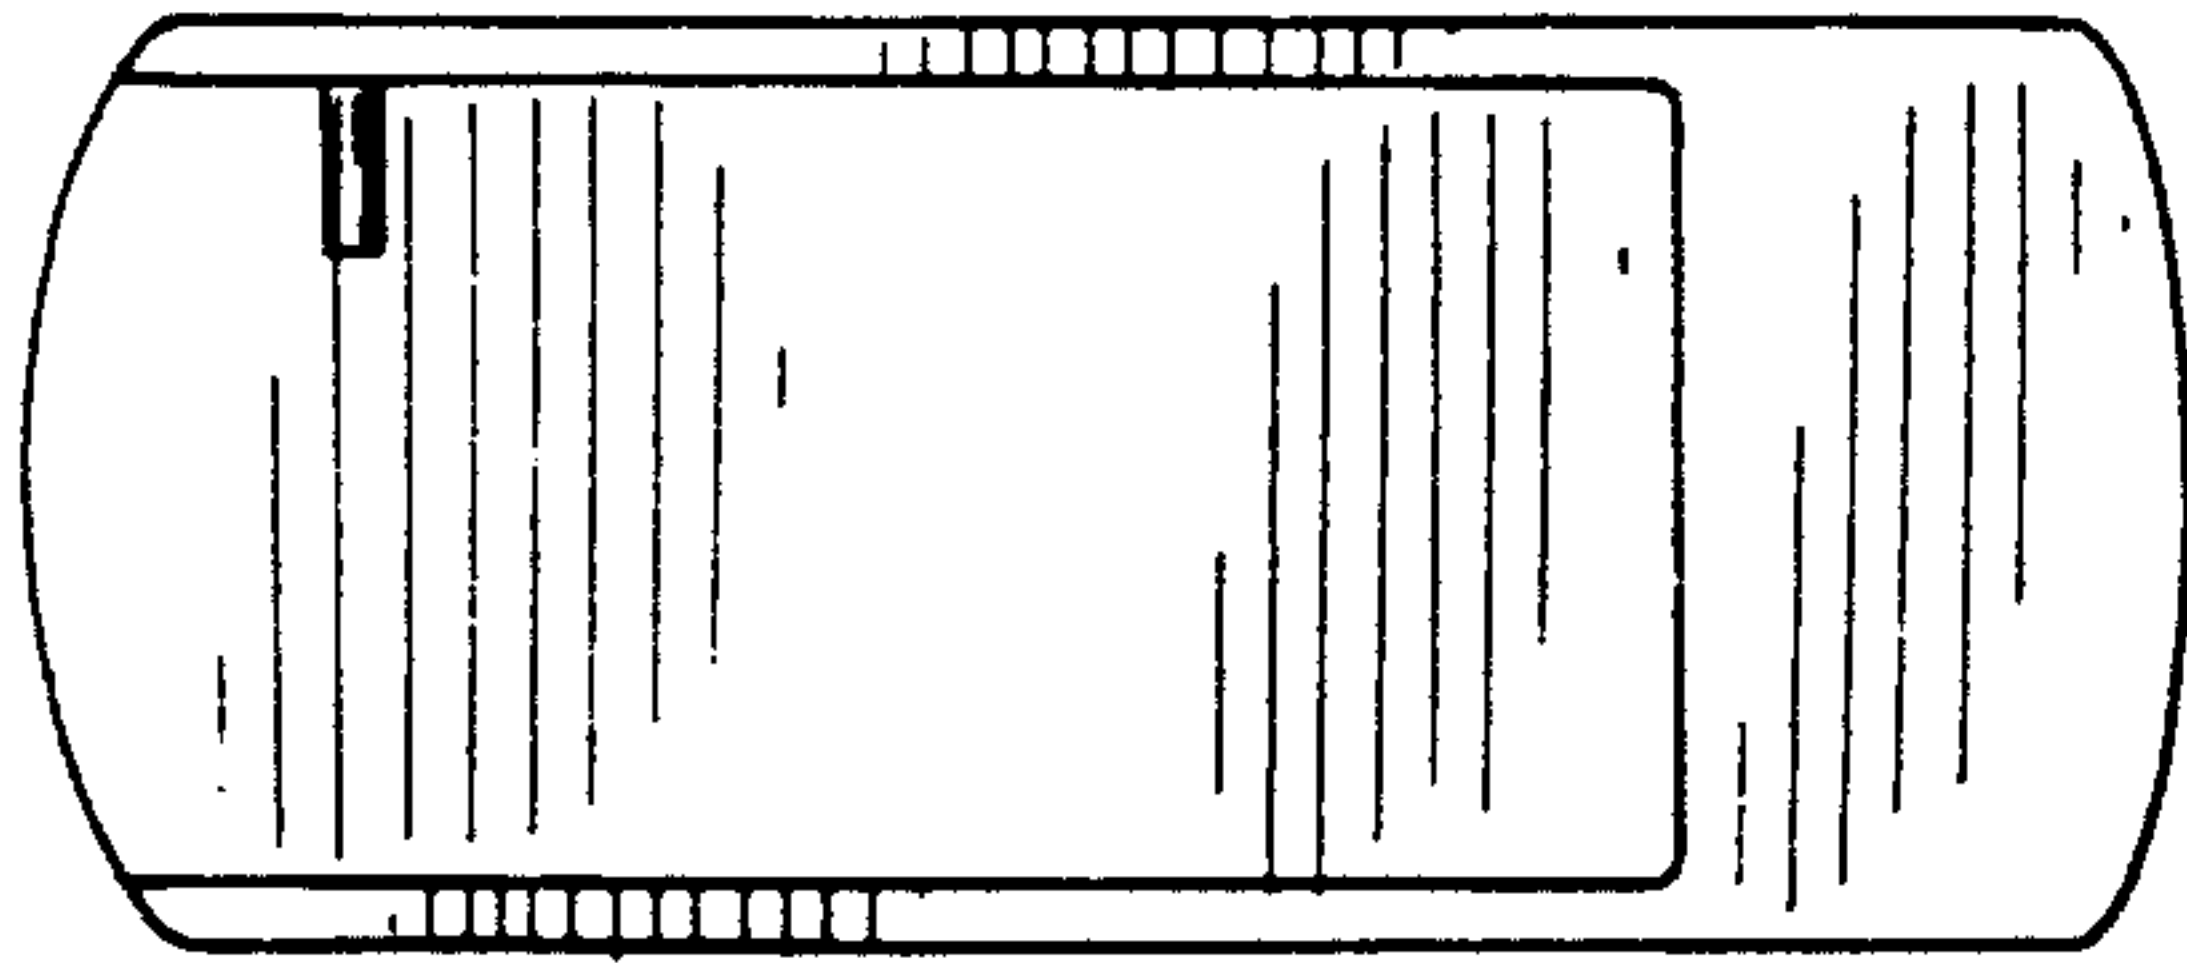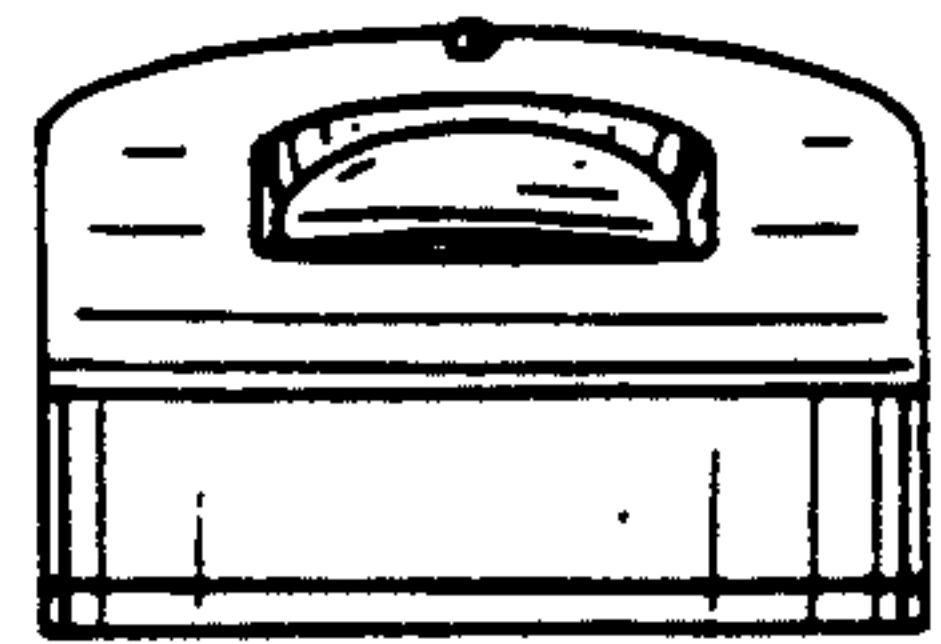

**FIG. 3**

**FIG. 5**

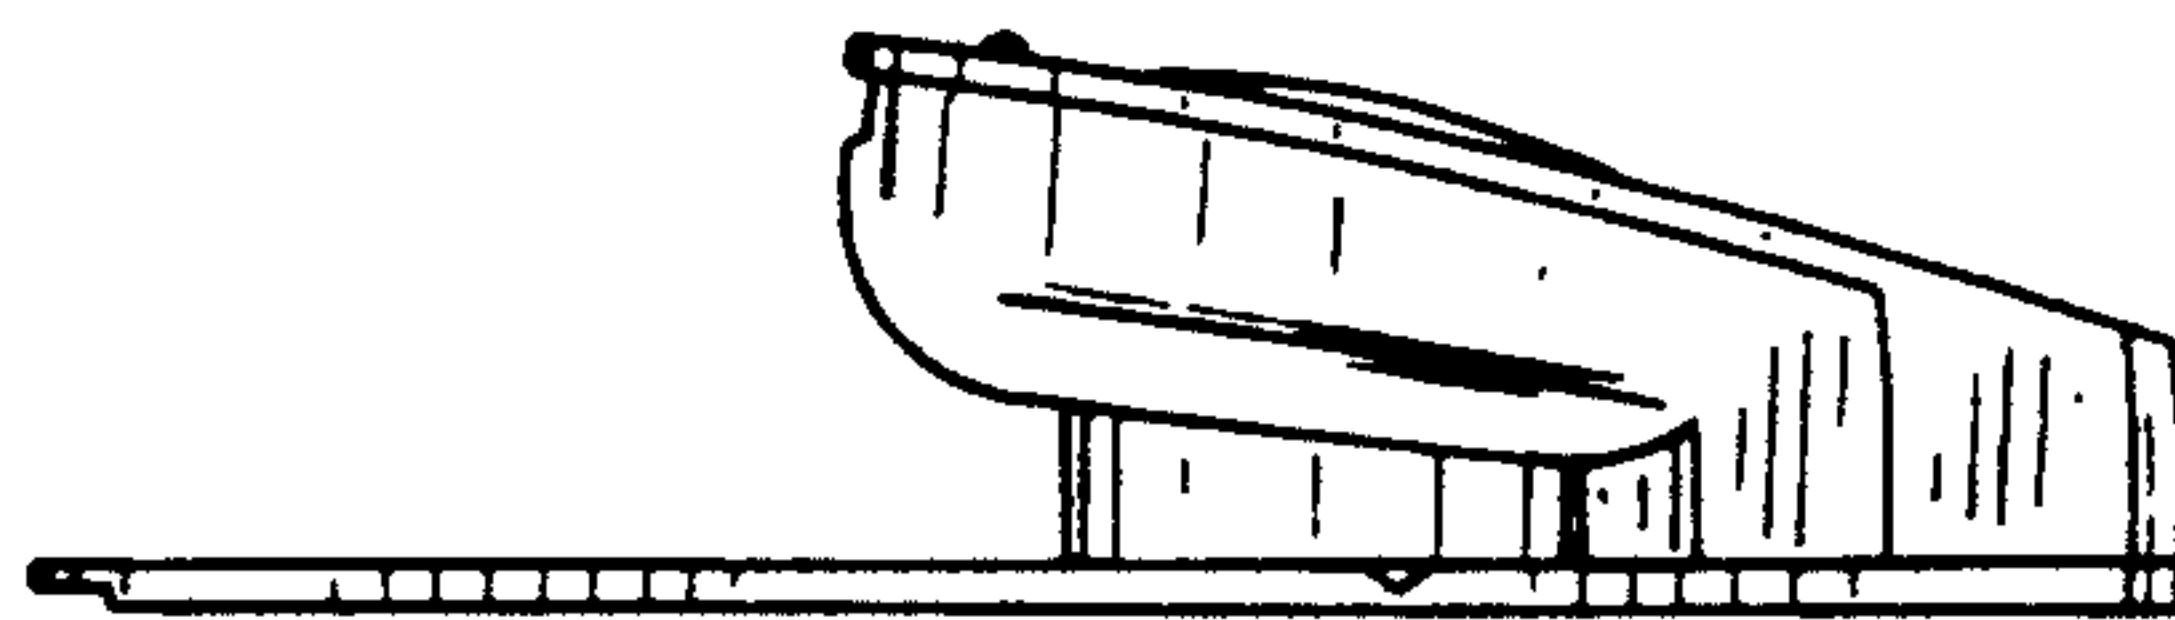

**FIG. 6**