



US00D346124S

# United States Patent [19]

Kovacevic

[11] Patent Number: **Des. 346,124**

[45] Date of Patent: **\*\* Apr. 19, 1994**

[54] **BREAST COMPLIANCE MEASURING DEVICE**

[75] Inventor: **Nebojsa Kovacevic**, Plymouth, Minn.

[73] Assignee: **N.K. Biotechnical Engineering Company**, Minneapolis, Minn.

[\*\*] Term: **14 Years**

[21] Appl. No.: **1,640**

[22] Filed: **Nov. 18, 1992**

[52] U.S. Cl. .... **D10/84; D10/65**

[58] Field of Search ..... **33/511, 512; 128/774, 128/736, 915; D10/65, 46, 83, 84, 85; D24/158, 186**

[56] **References Cited**

**U.S. PATENT DOCUMENTS**

D. 330,865	11/1992	Peletis et al. ....	D10/84
4,132,224	1/1979	Randolph .....	128/2
5,009,233	4/1991	Petrohilos .....	128/774 X
5,027,828	7/1991	Kovacevic et al. ....	128/774

**OTHER PUBLICATIONS**

Article entitled "Standard Test Method for Rubber Property-Durometer Hardness" from *Annual Book of ASTM Standards*, vol. 09.02.

Article entitled "Instrumentation System for Breast Engorgement Evaluation" by C. D. Ferris.

*Primary Examiner*—Alan P. Douglas

*Assistant Examiner*—Antoine D. Davis

*Attorney, Agent, or Firm*—Westman, Champlin & Kelly

[57] **CLAIM**

The ornamental design for a breast compliance measuring device, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of a breast compliance measuring device showing my new design;


FIG. 2 is a side view thereof;


FIG. 3 is a top plan view thereof;

FIG. 4 is a front plan view thereof;


FIG. 5 is a rear plan view thereof; and,

FIG. 6 is a bottom plan view thereof.

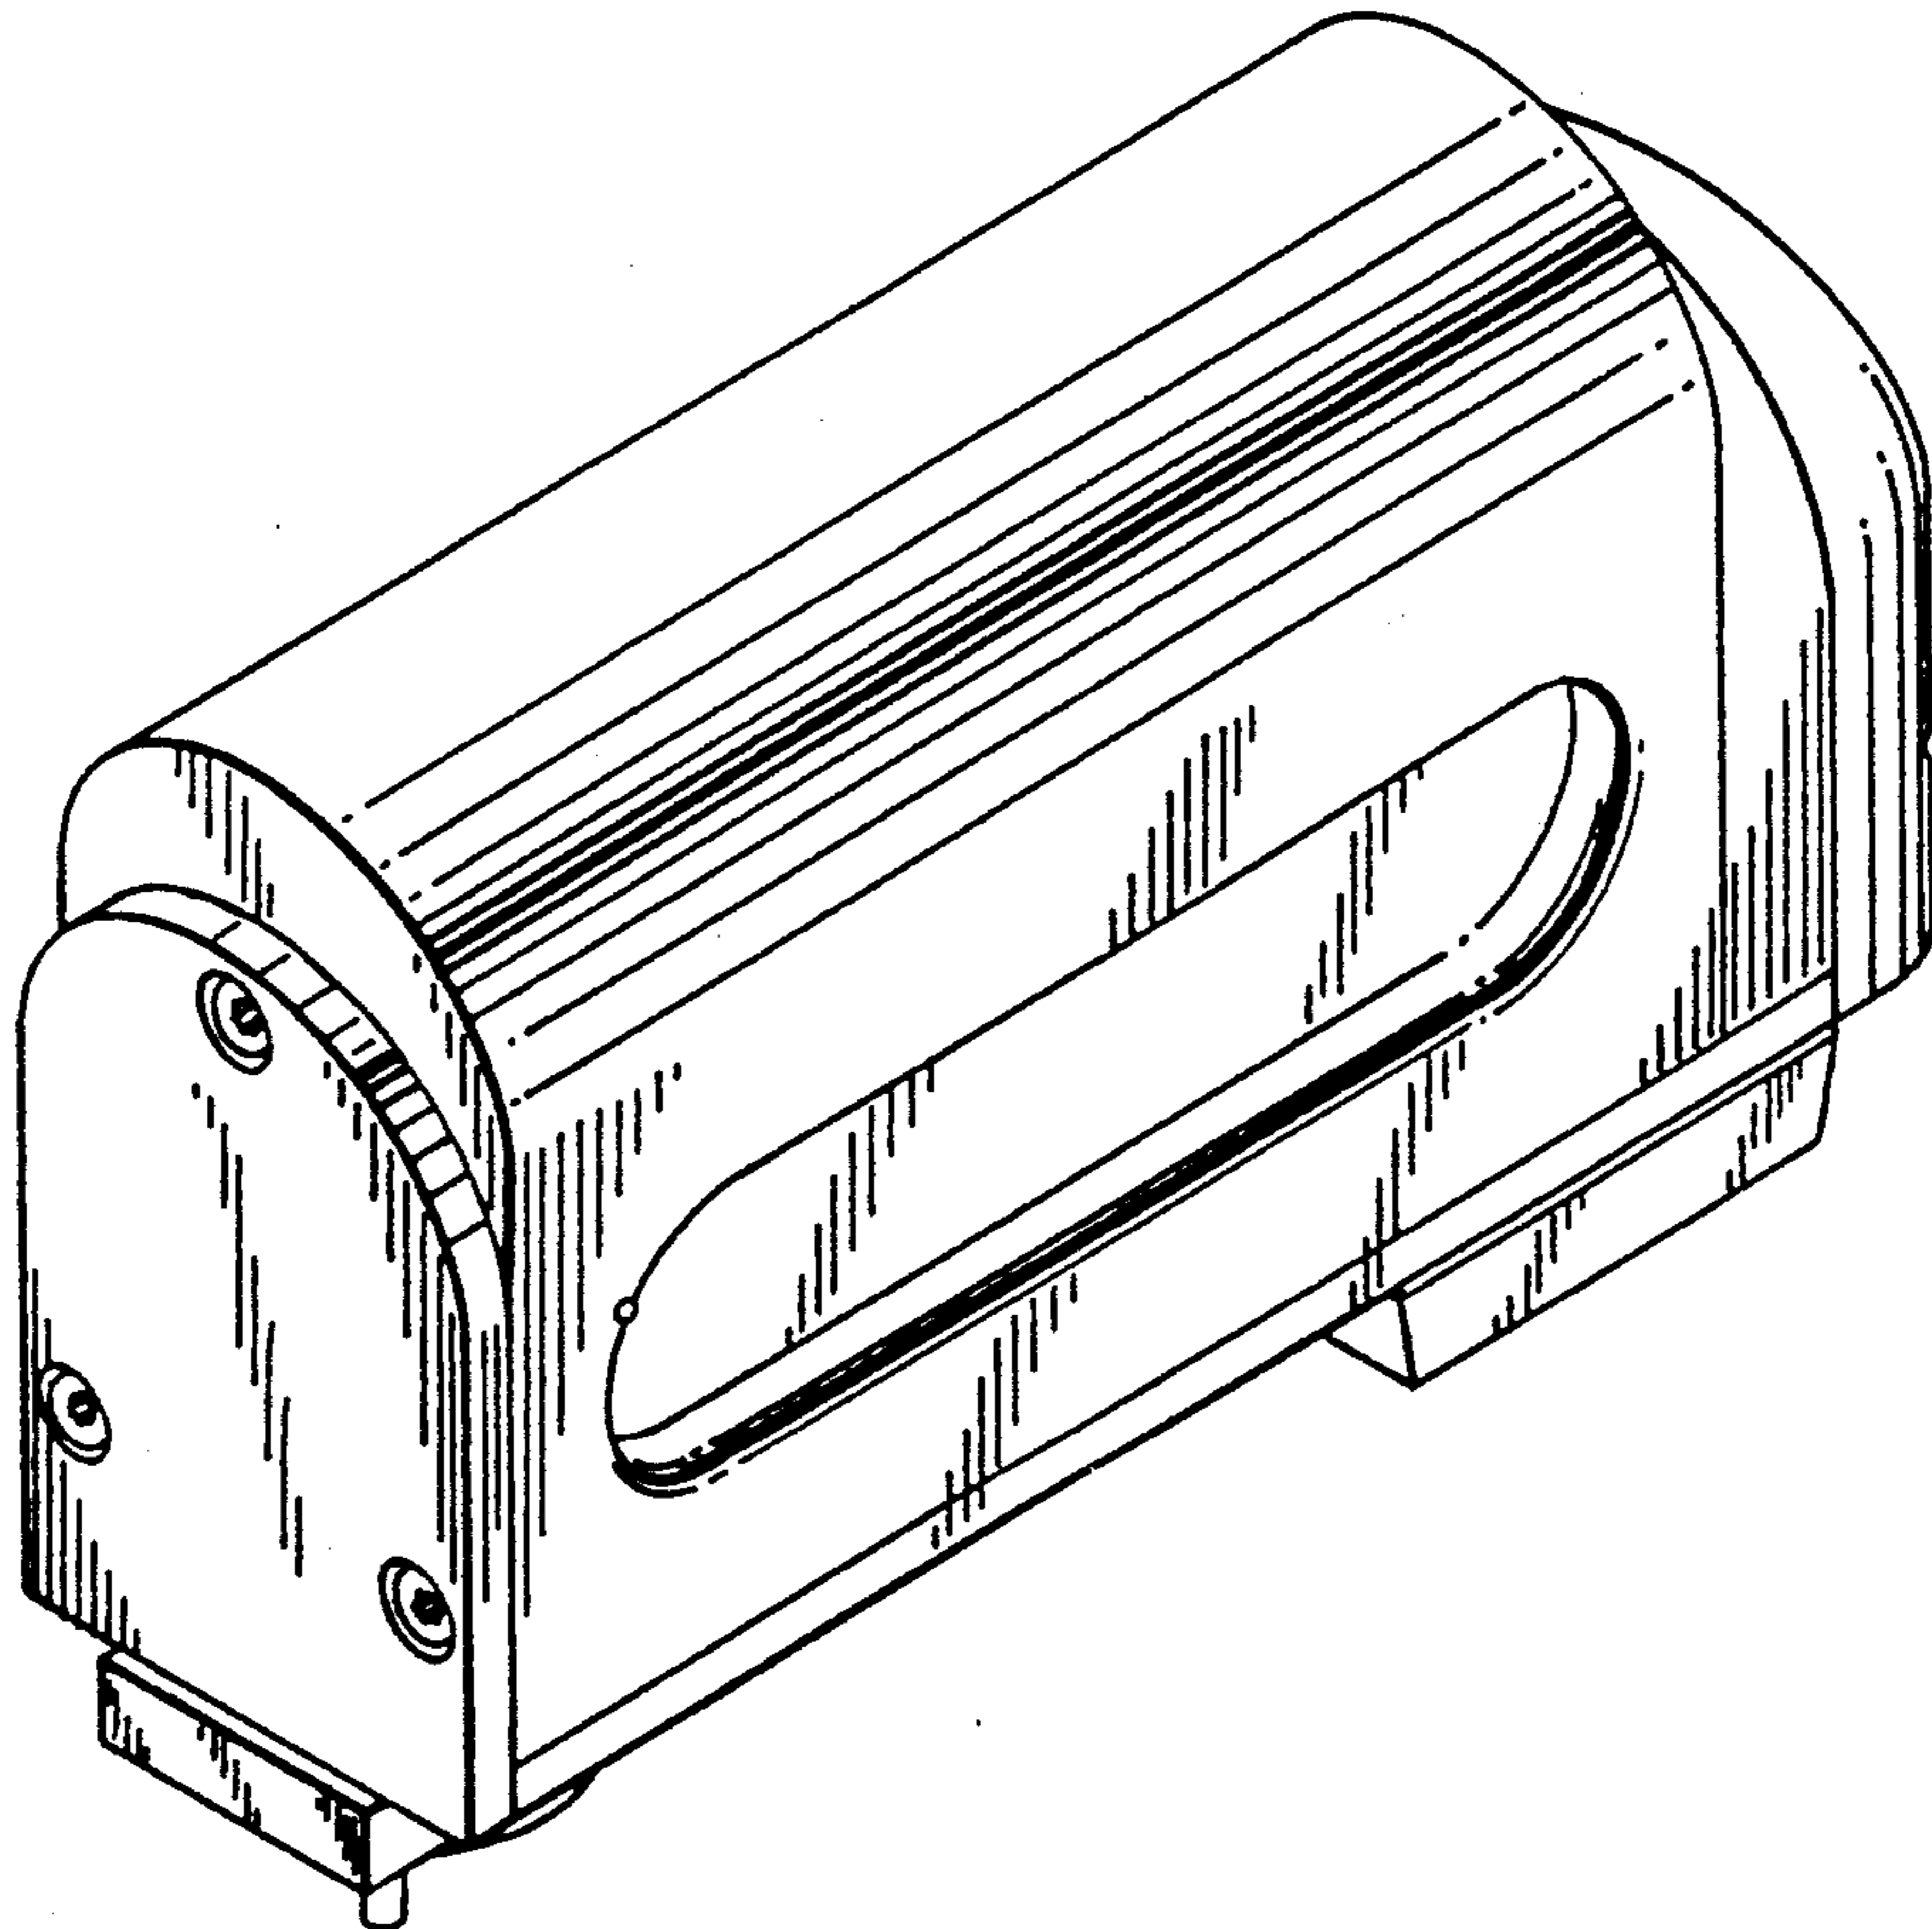


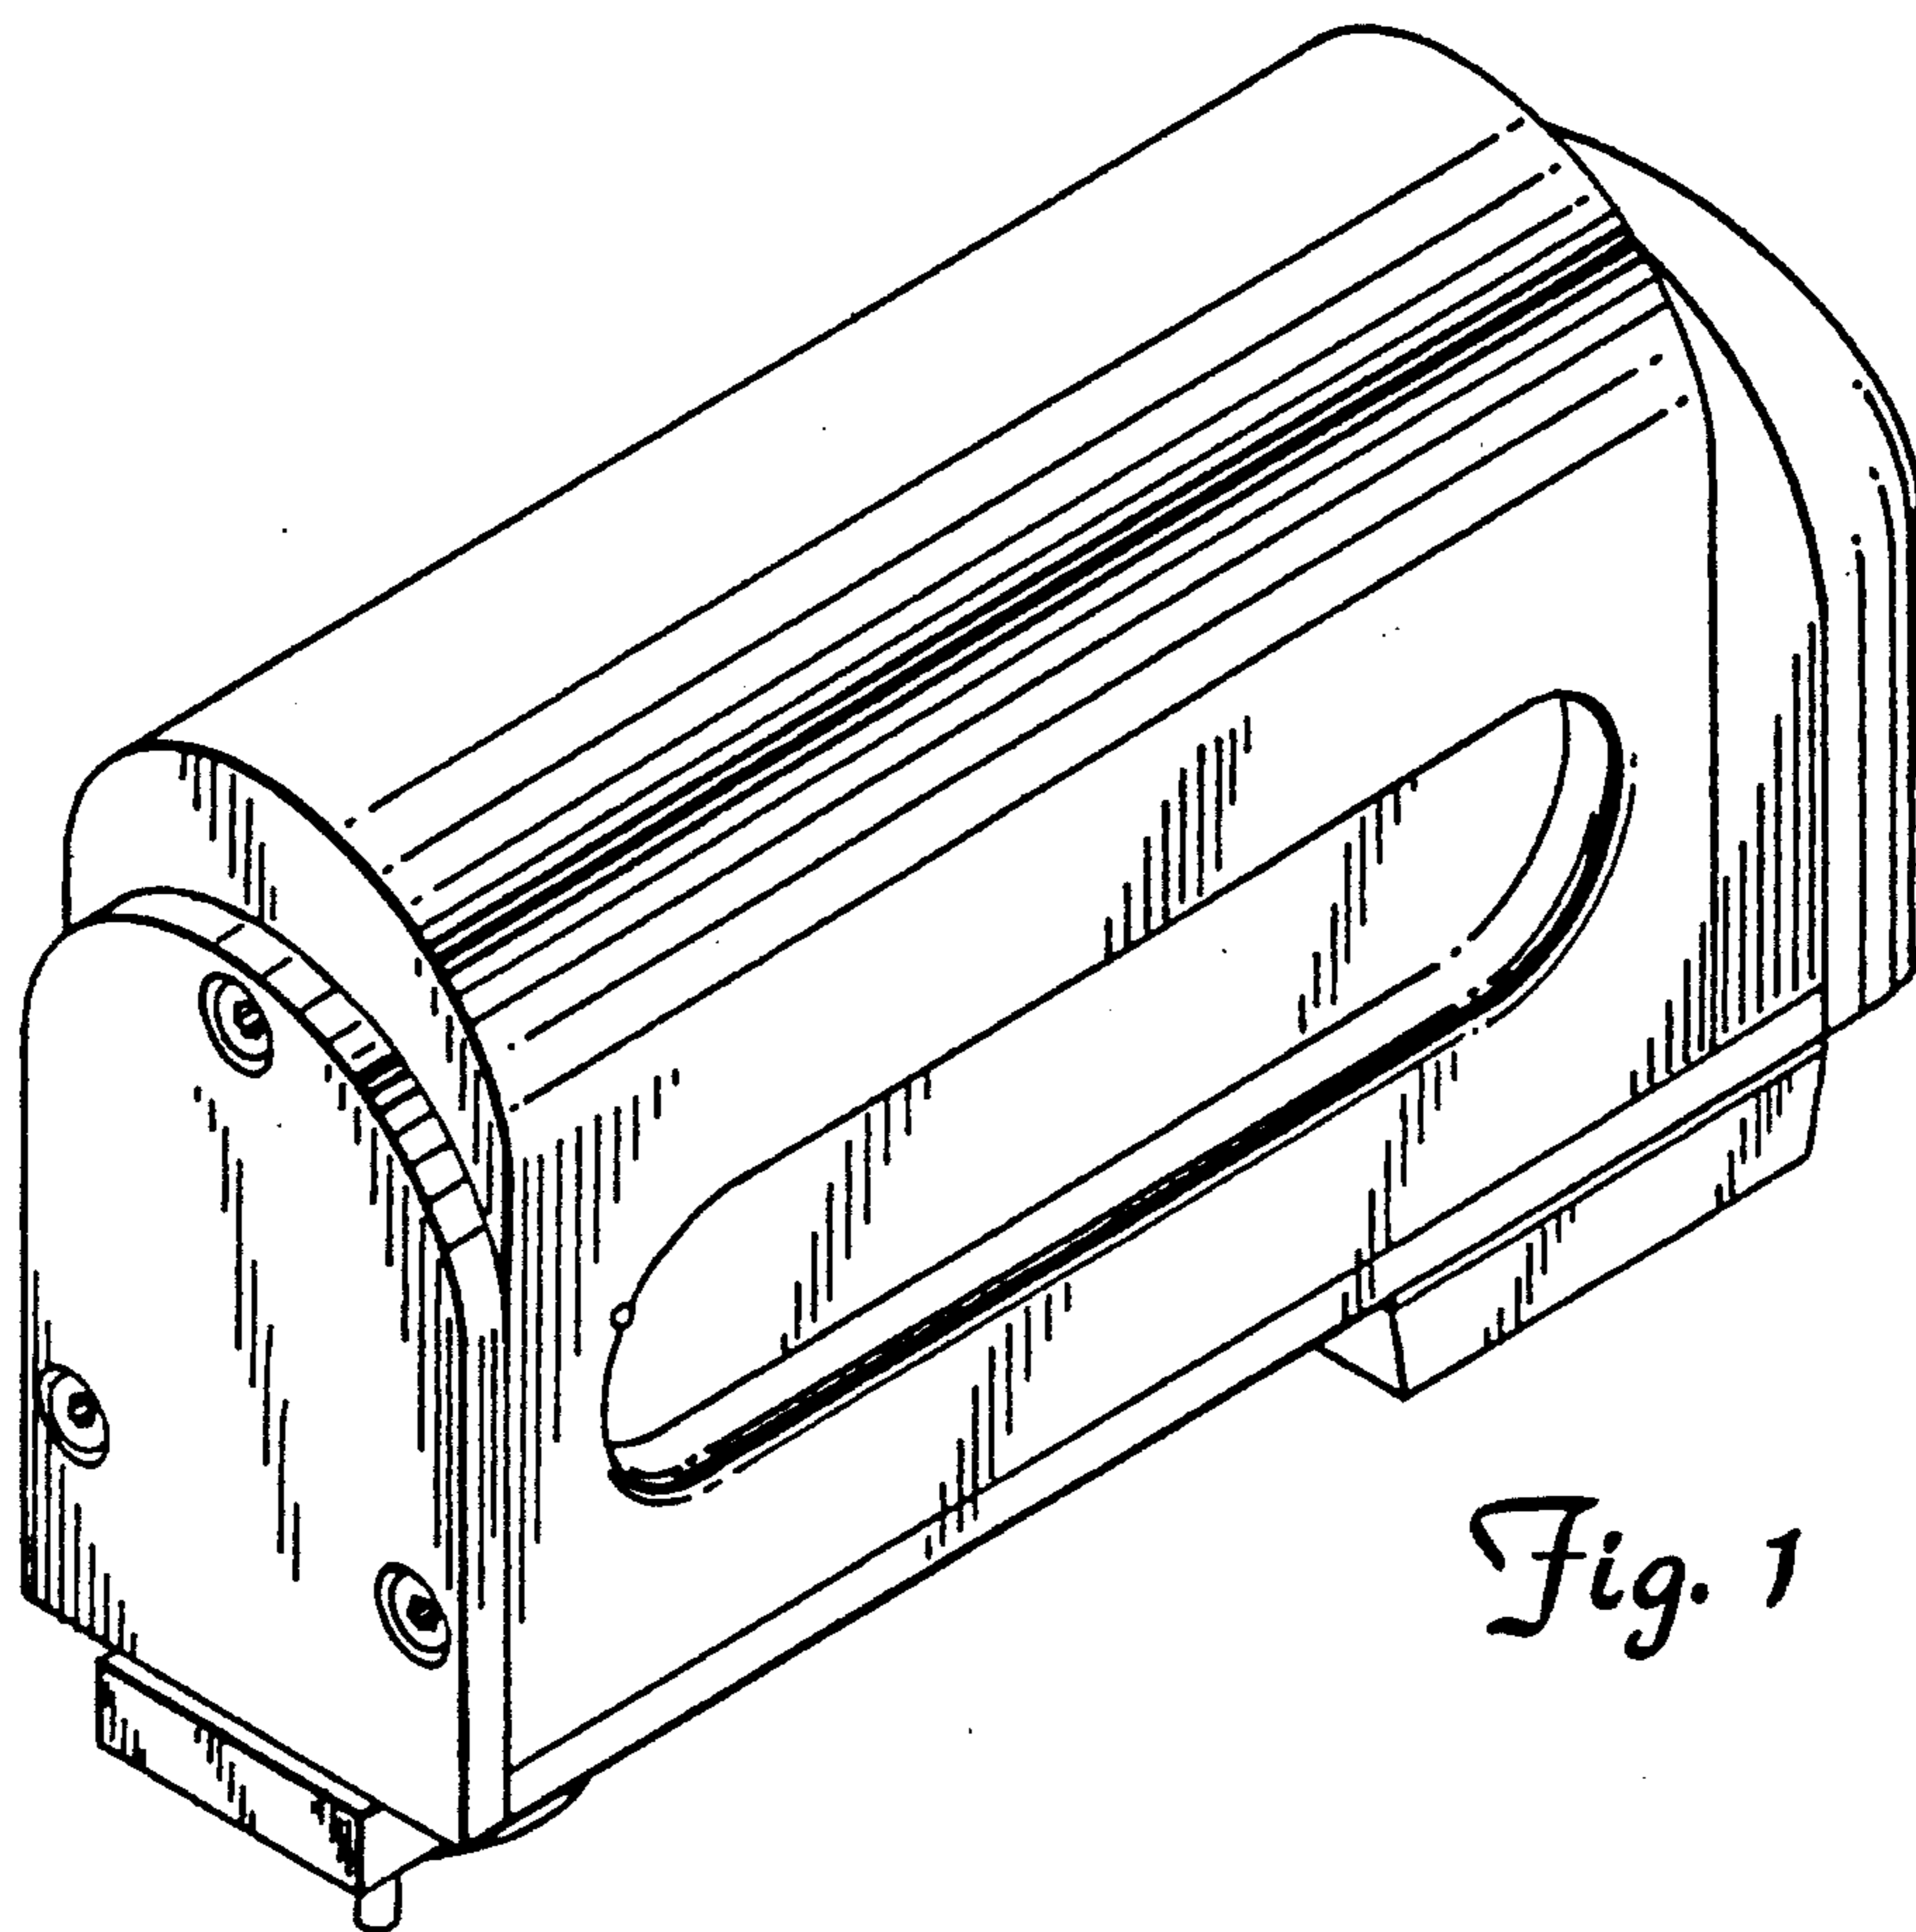


*Fig. 1*

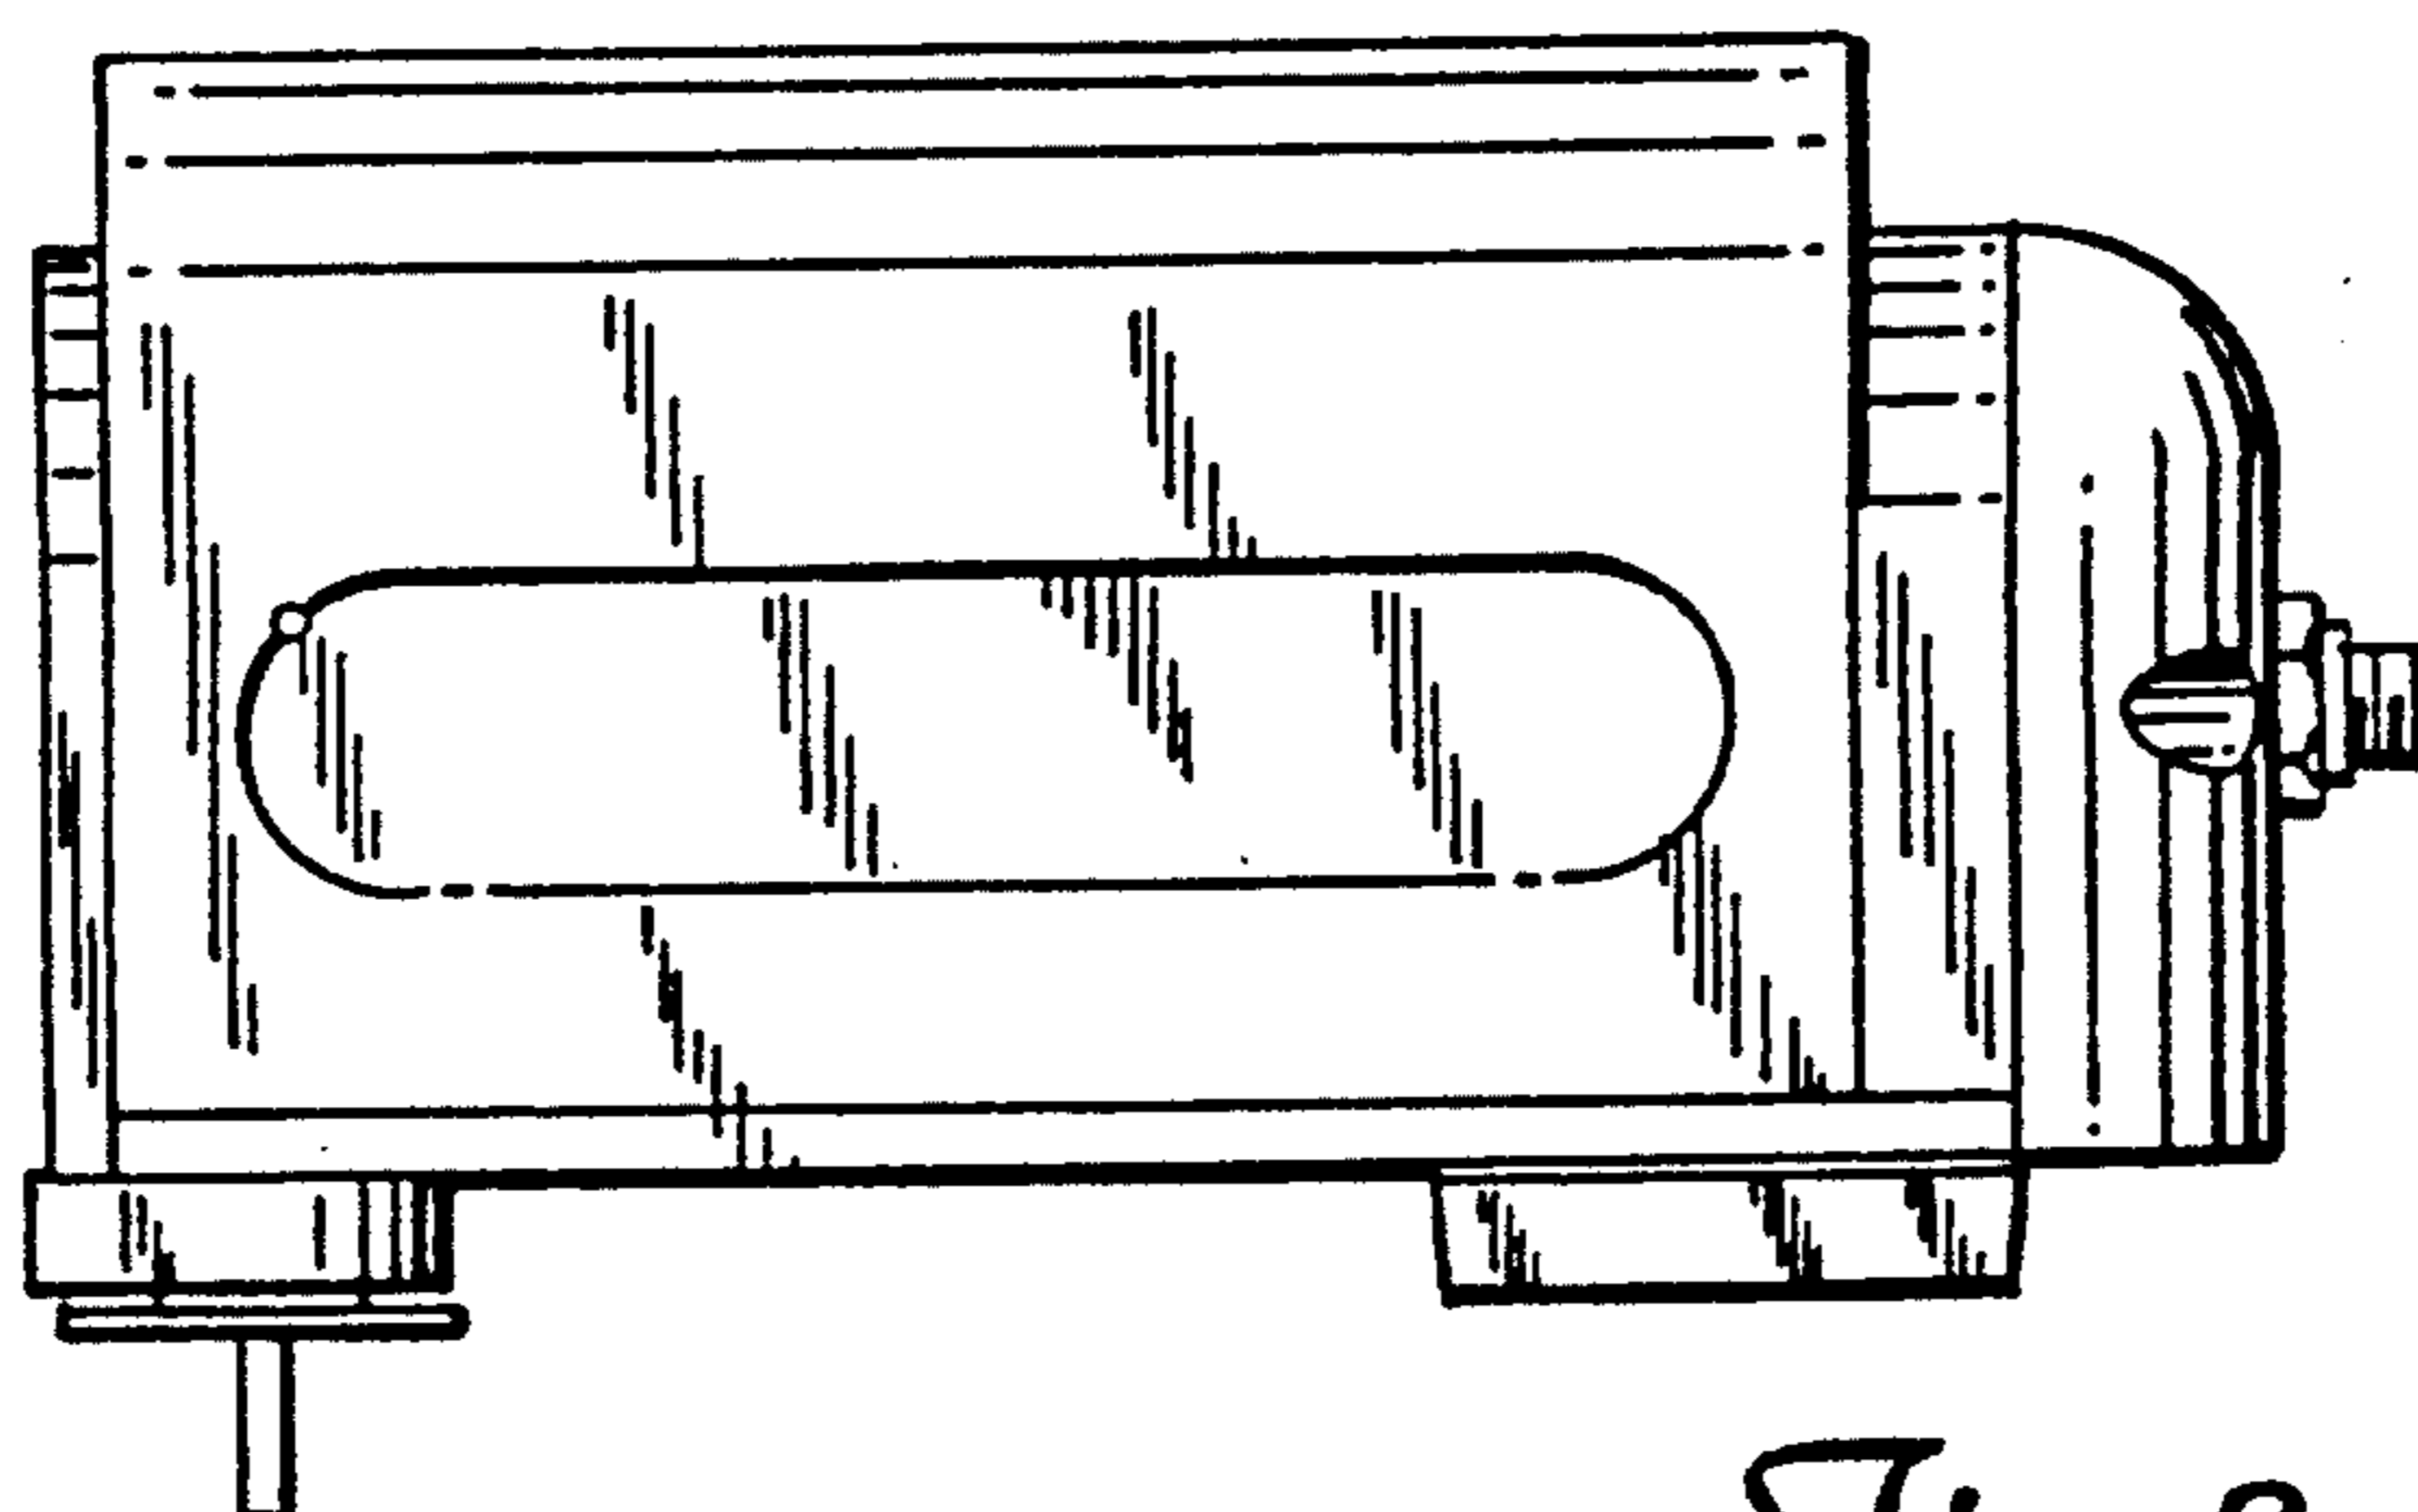


*Fig. 2*

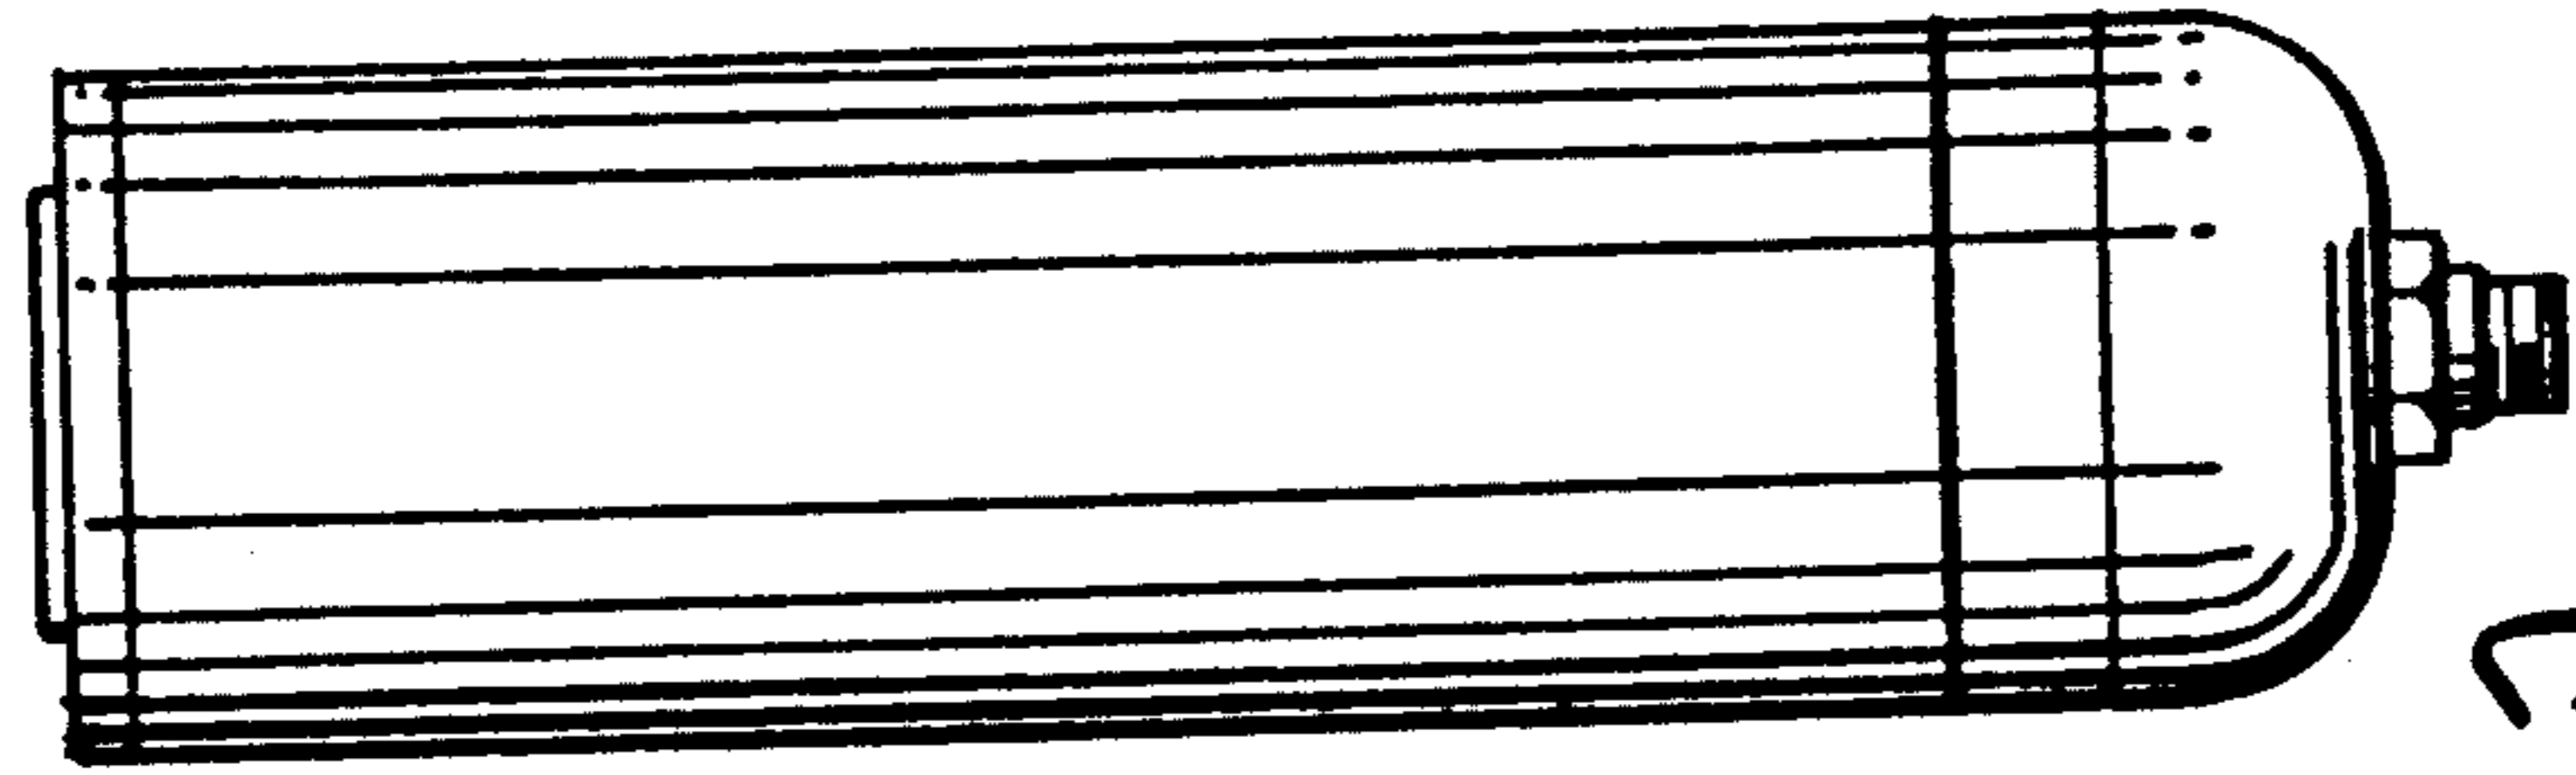


*Fig. 3*

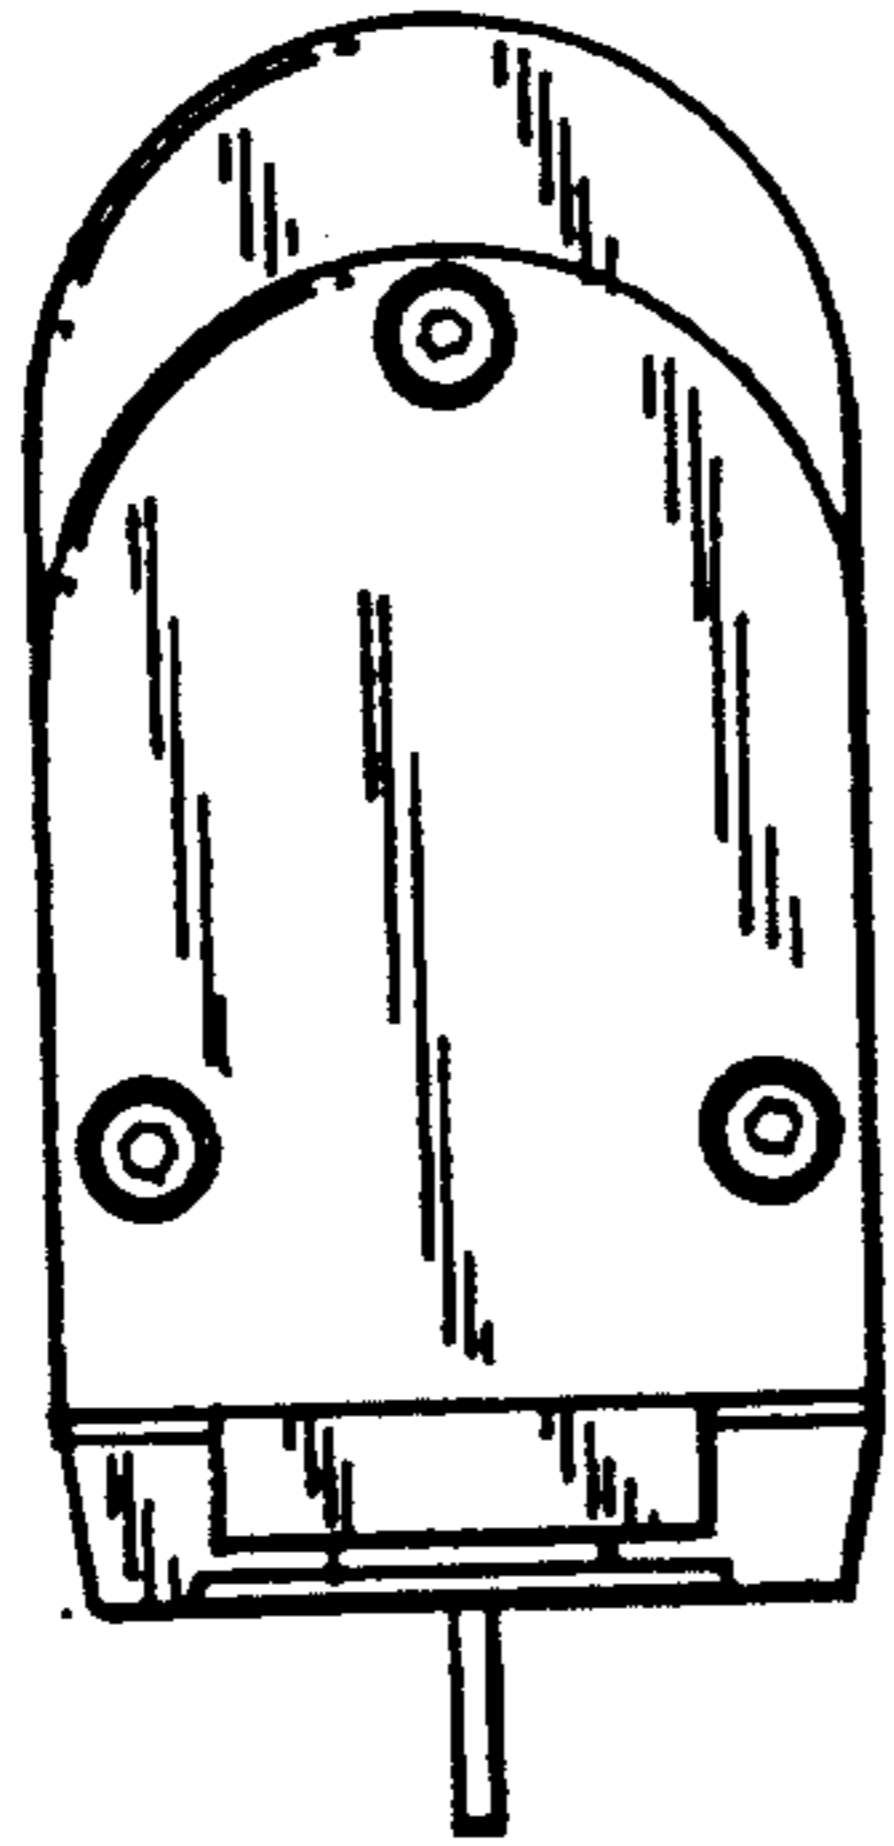

*Fig. 4*

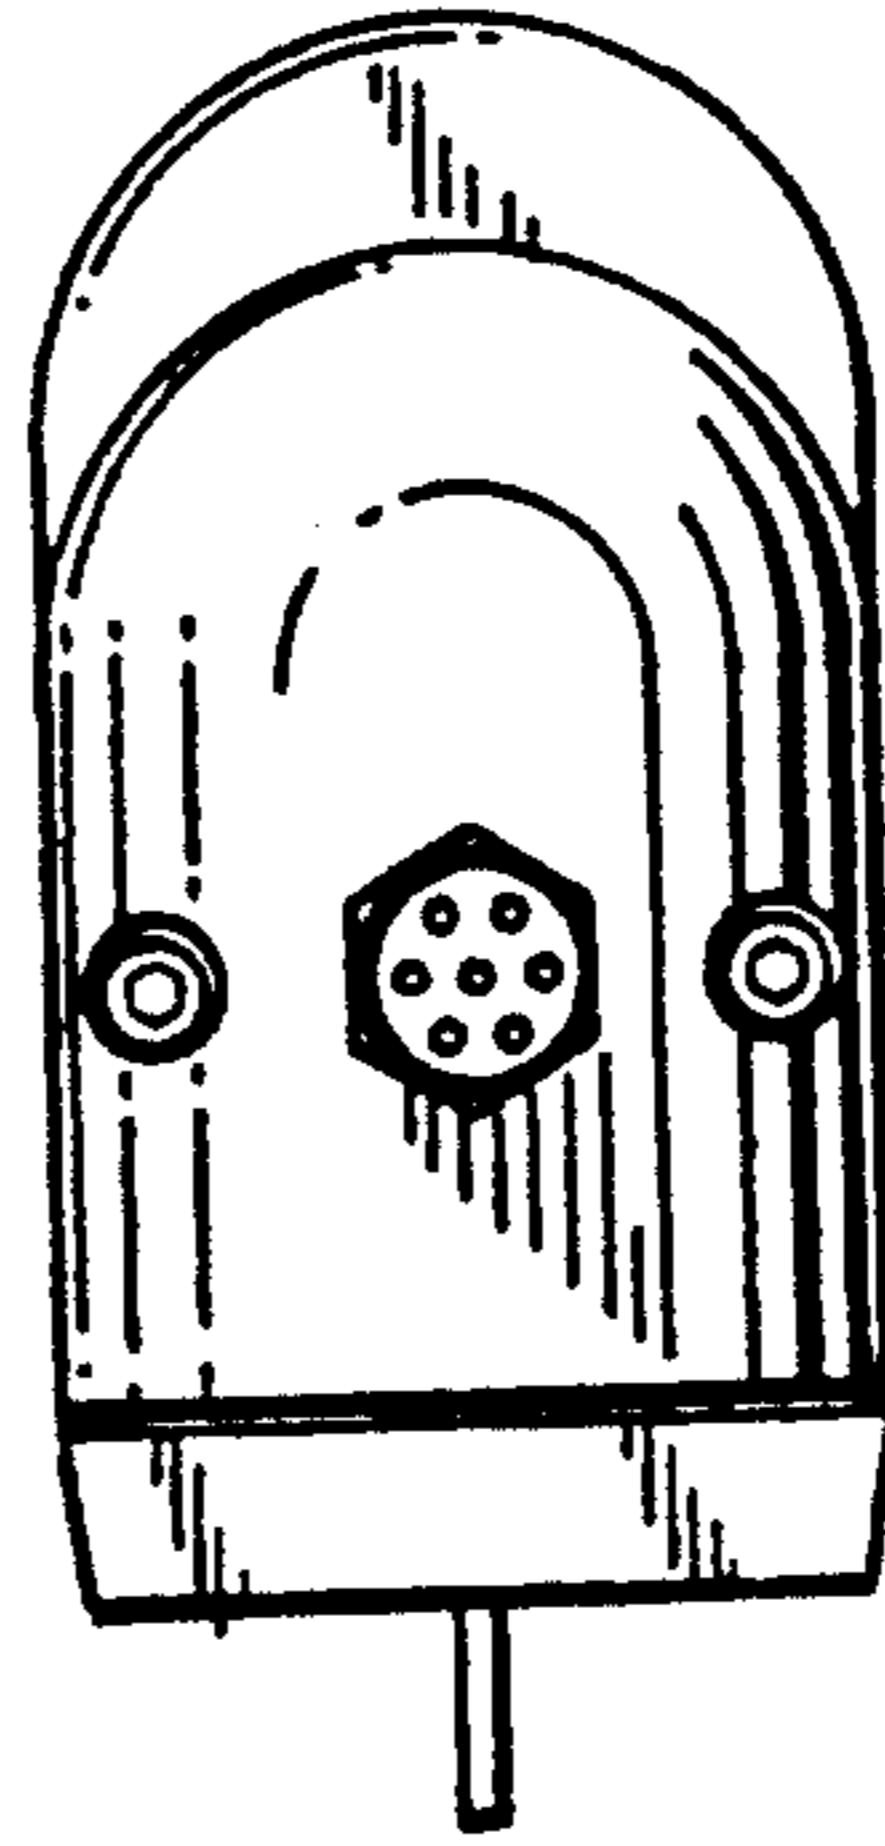

*Fig. 5*

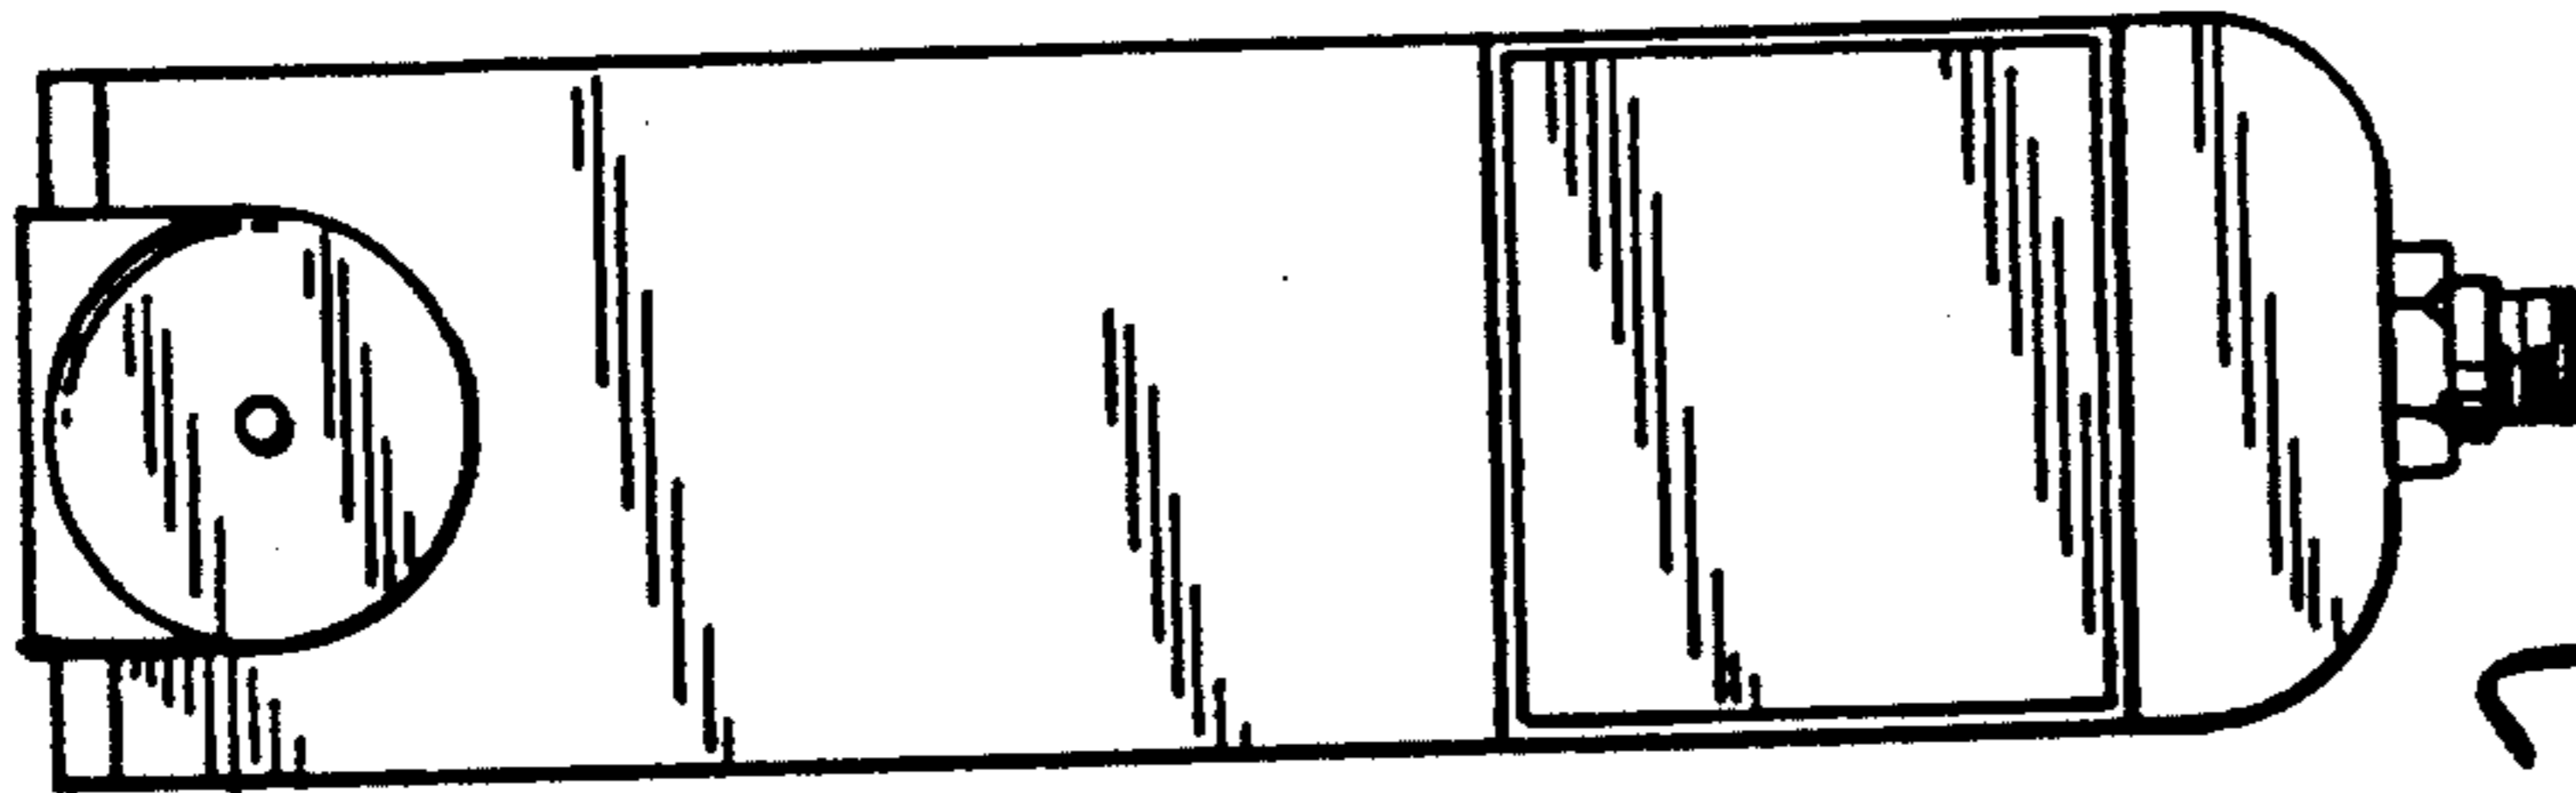

*Fig. 6*