



US00D346124S

United States Patent [19]

[11] Patent Number: **Des. 346,124**

Kovacevic

[45] Date of Patent: **** Apr. 19, 1994**

[54] BREAST COMPLIANCE MEASURING DEVICE

[75] Inventor: **Nebojsa Kovacevic**, Plymouth, Minn.

[73] Assignee: **N.K. Biotechnical Engineering Company**, Minneapolis, Minn.

[**] Term: **14 Years**

[21] Appl. No.: **1,640**

[22] Filed: **Nov. 18, 1992**

[52] U.S. Cl. **D10/84; D10/65**

[58] Field of Search **33/511, 512; 128/774, 128/736, 915; D10/65, 46, 83, 84, 85; D24/158, 186**

[56] References Cited

U.S. PATENT DOCUMENTS

D. 330,865	11/1992	Peletis et al.	D10/84
4,132,224	1/1979	Randolph	128/2
5,009,233	4/1991	Petrohilos	128/774 X
5,027,828	7/1991	Kovacevic et al.	128/774

OTHER PUBLICATIONS

Article entitled "Standard Test Method for Rubber Property-Durometer Hardness" from *Annual Book of ASTM Standards*, vol. 09.02.

Article entitled "Instrumentation System for Breast Engorgement Evaluation" by C. D. Ferris.

Primary Examiner—Alan P. Douglas

Assistant Examiner—Antoine D. Davis

Attorney, Agent, or Firm—Westman, Champlin & Kelly

[57] CLAIM

The ornamental design for a breast compliance measuring device, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of a breast compliance measuring device showing my new design;


FIG. 2 is a side view thereof;

FIG. 3 is a top plan view thereof;

FIG. 4 is a front plan view thereof;

FIG. 5 is a rear plan view thereof; and,

FIG. 6 is a bottom plan view thereof.

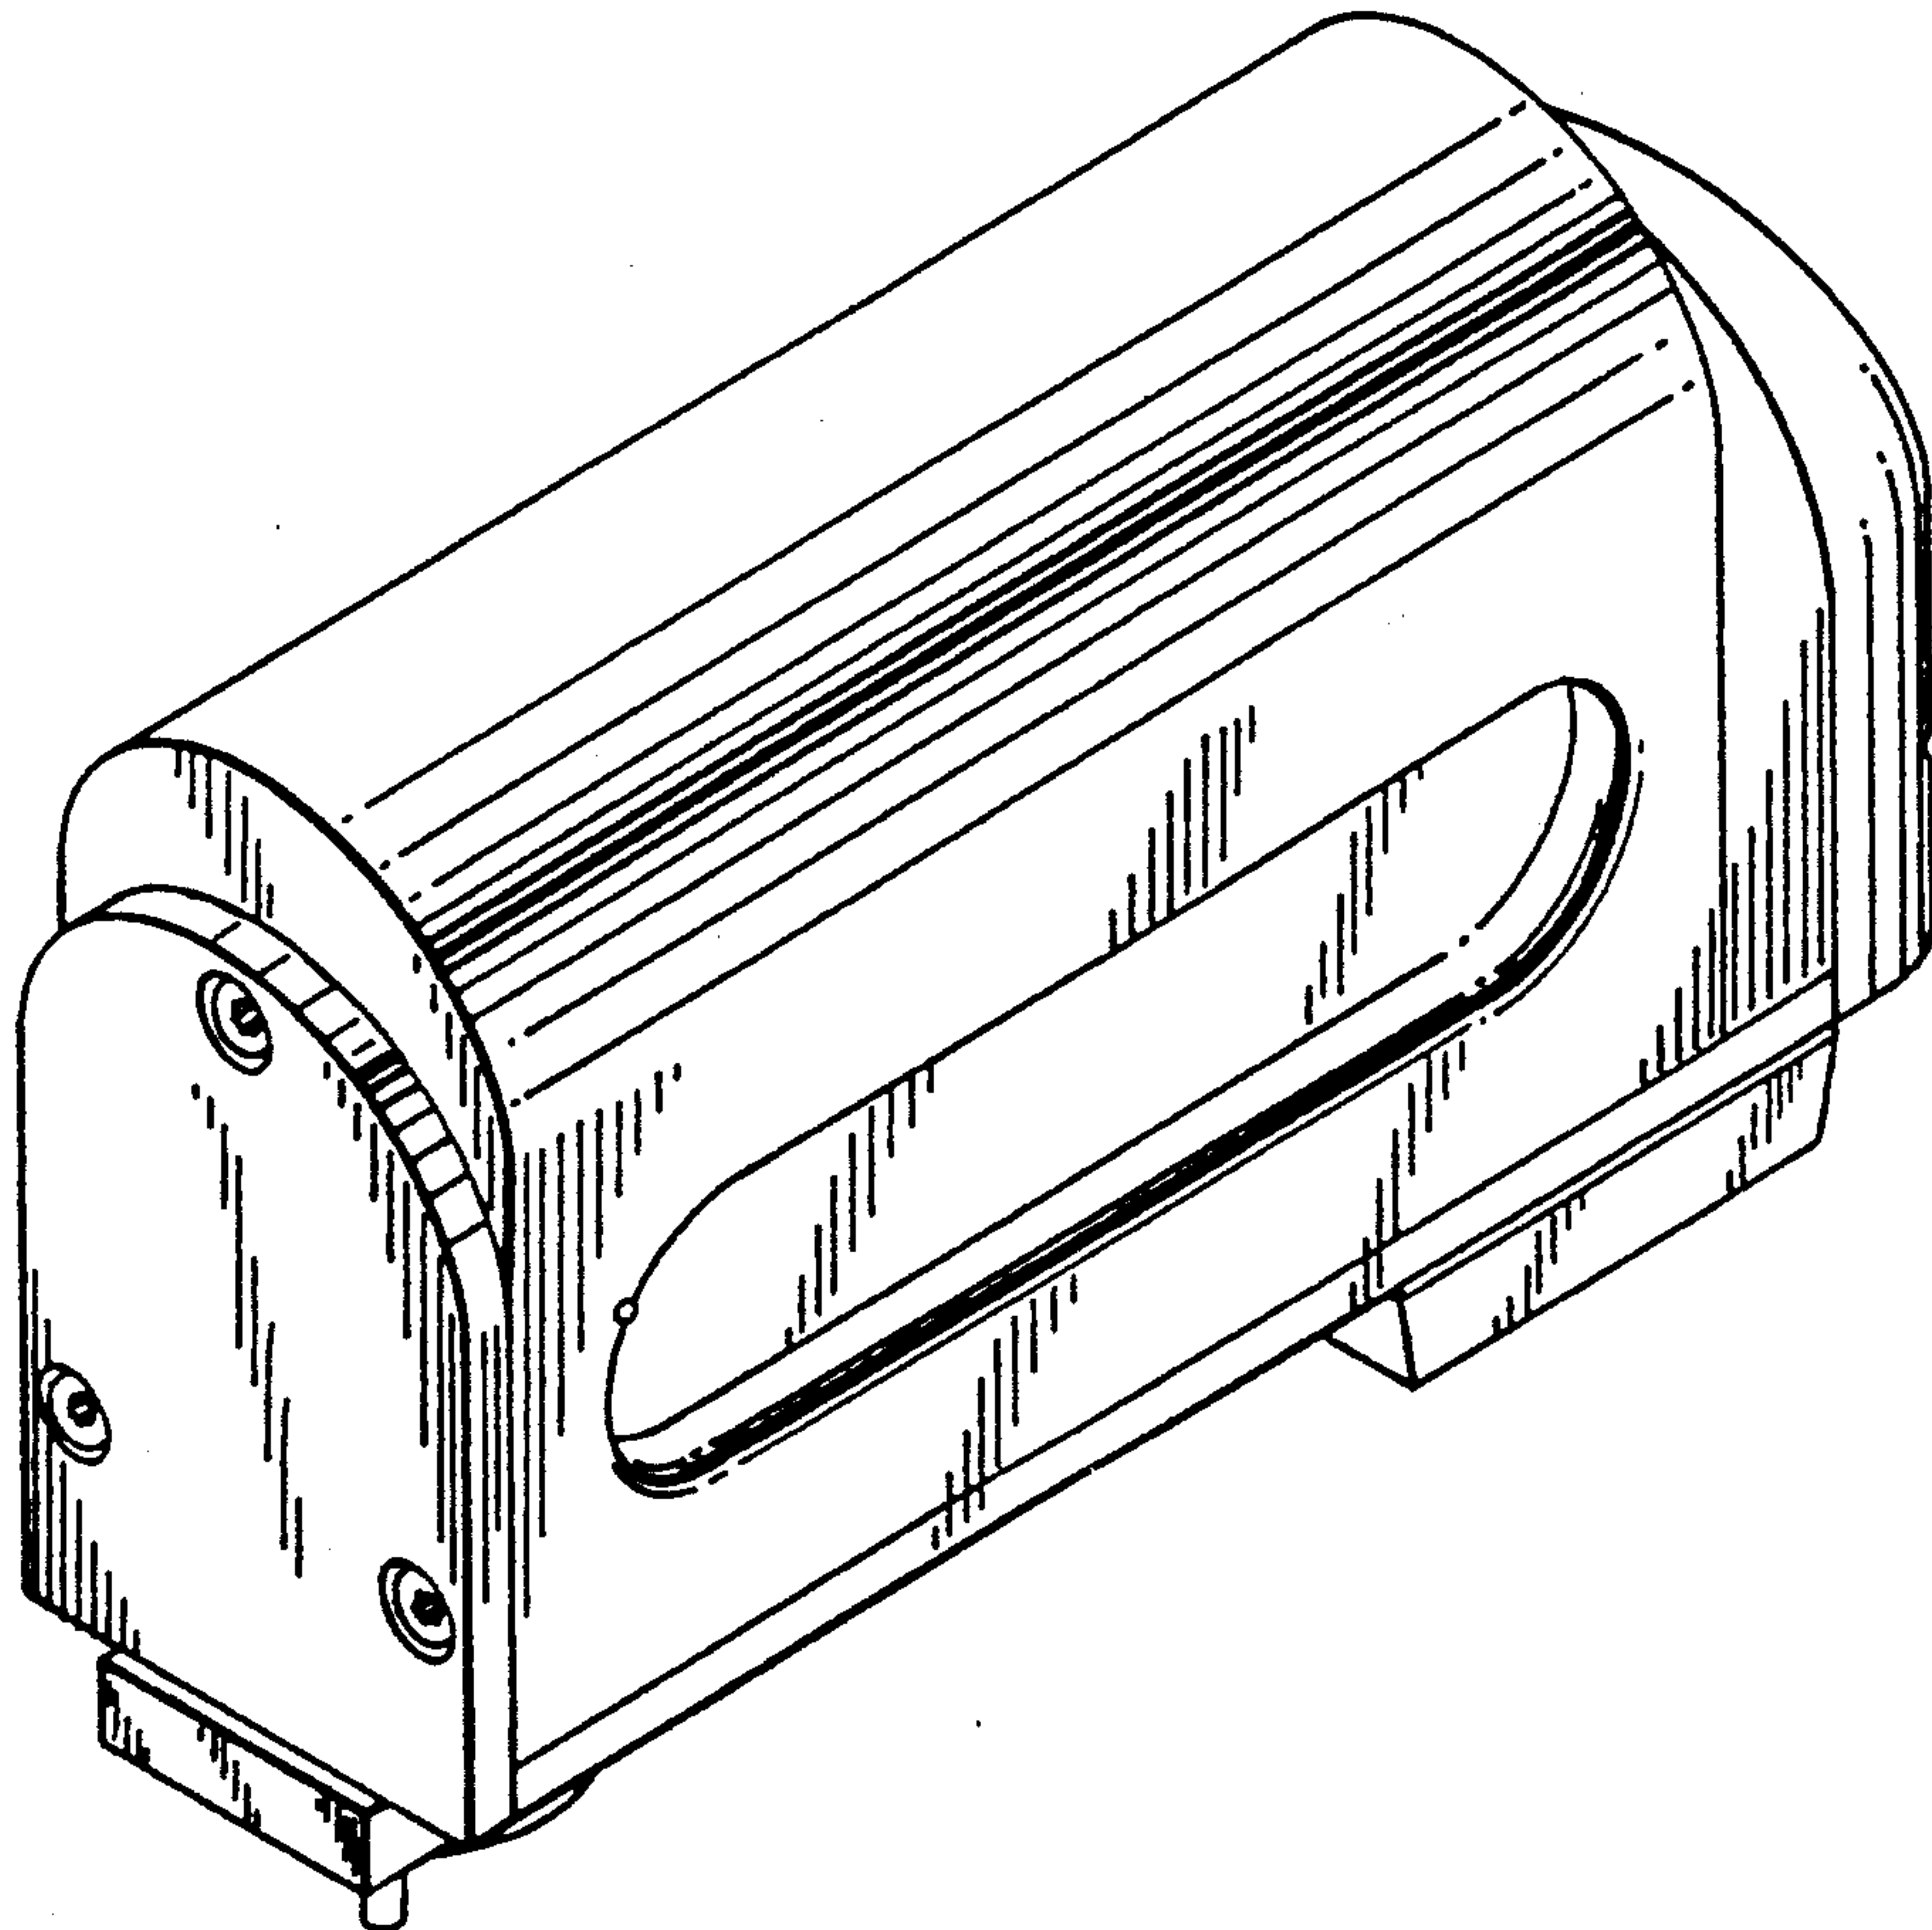

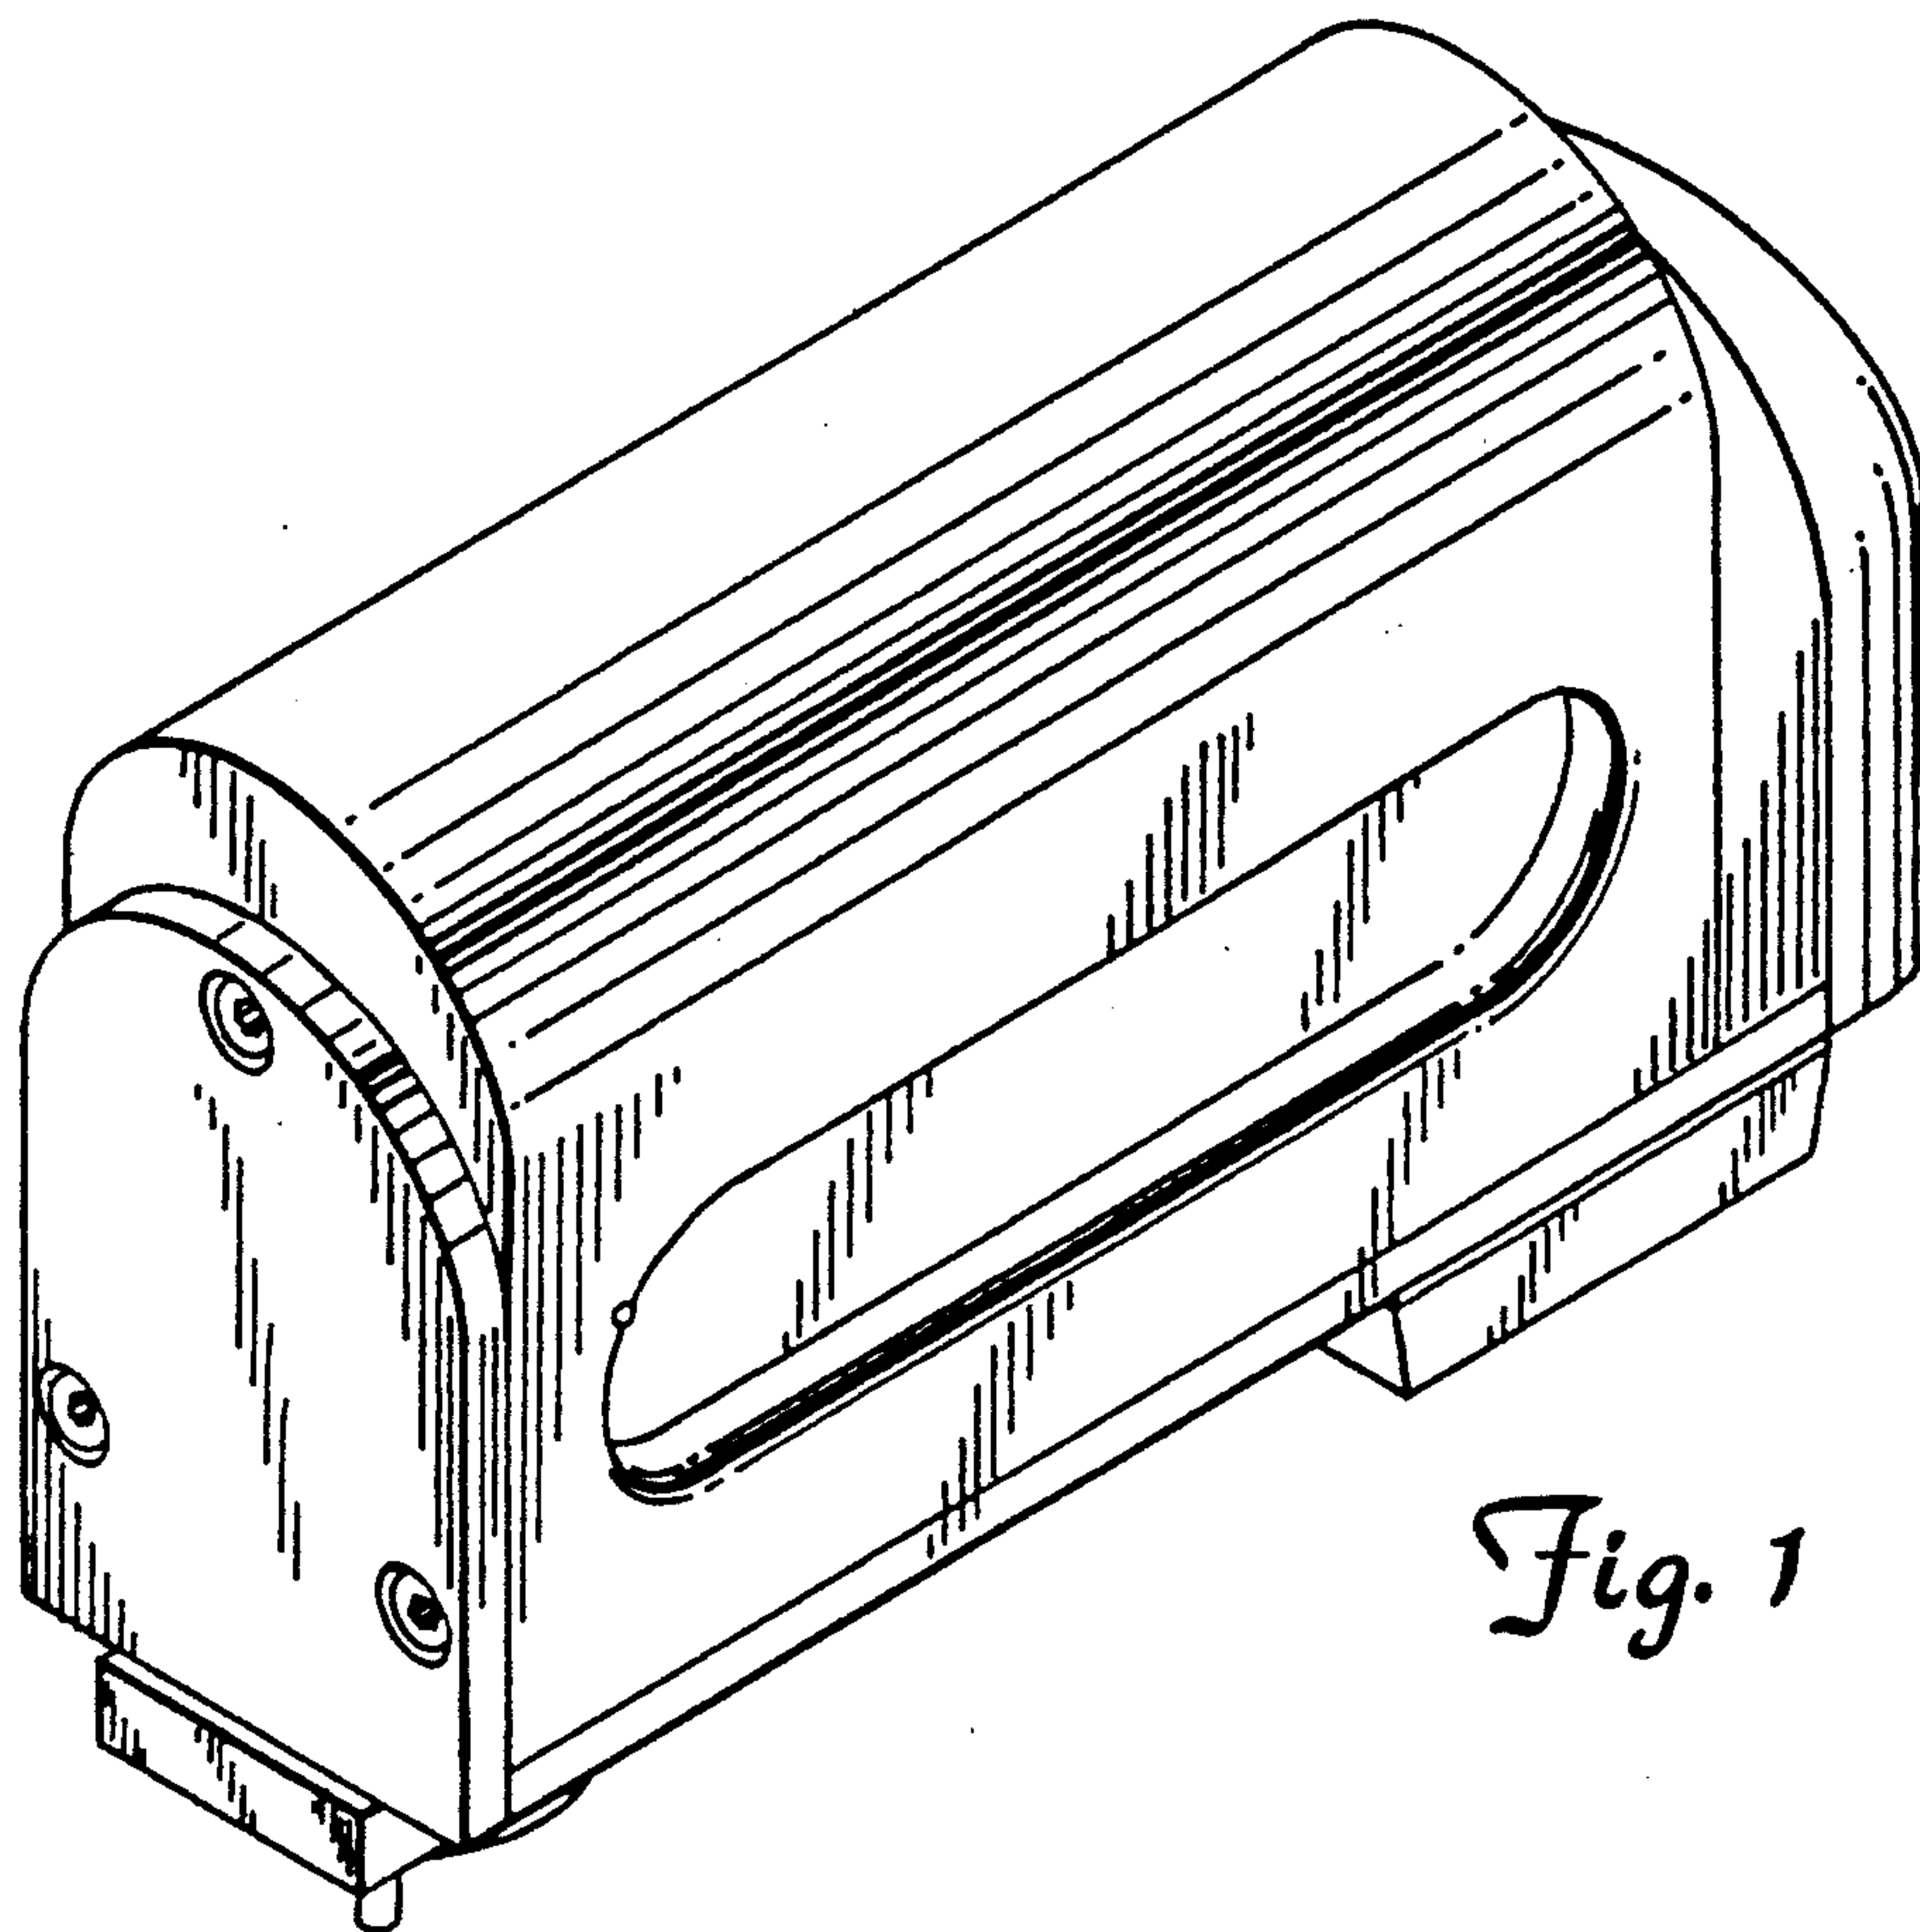


Fig. 1

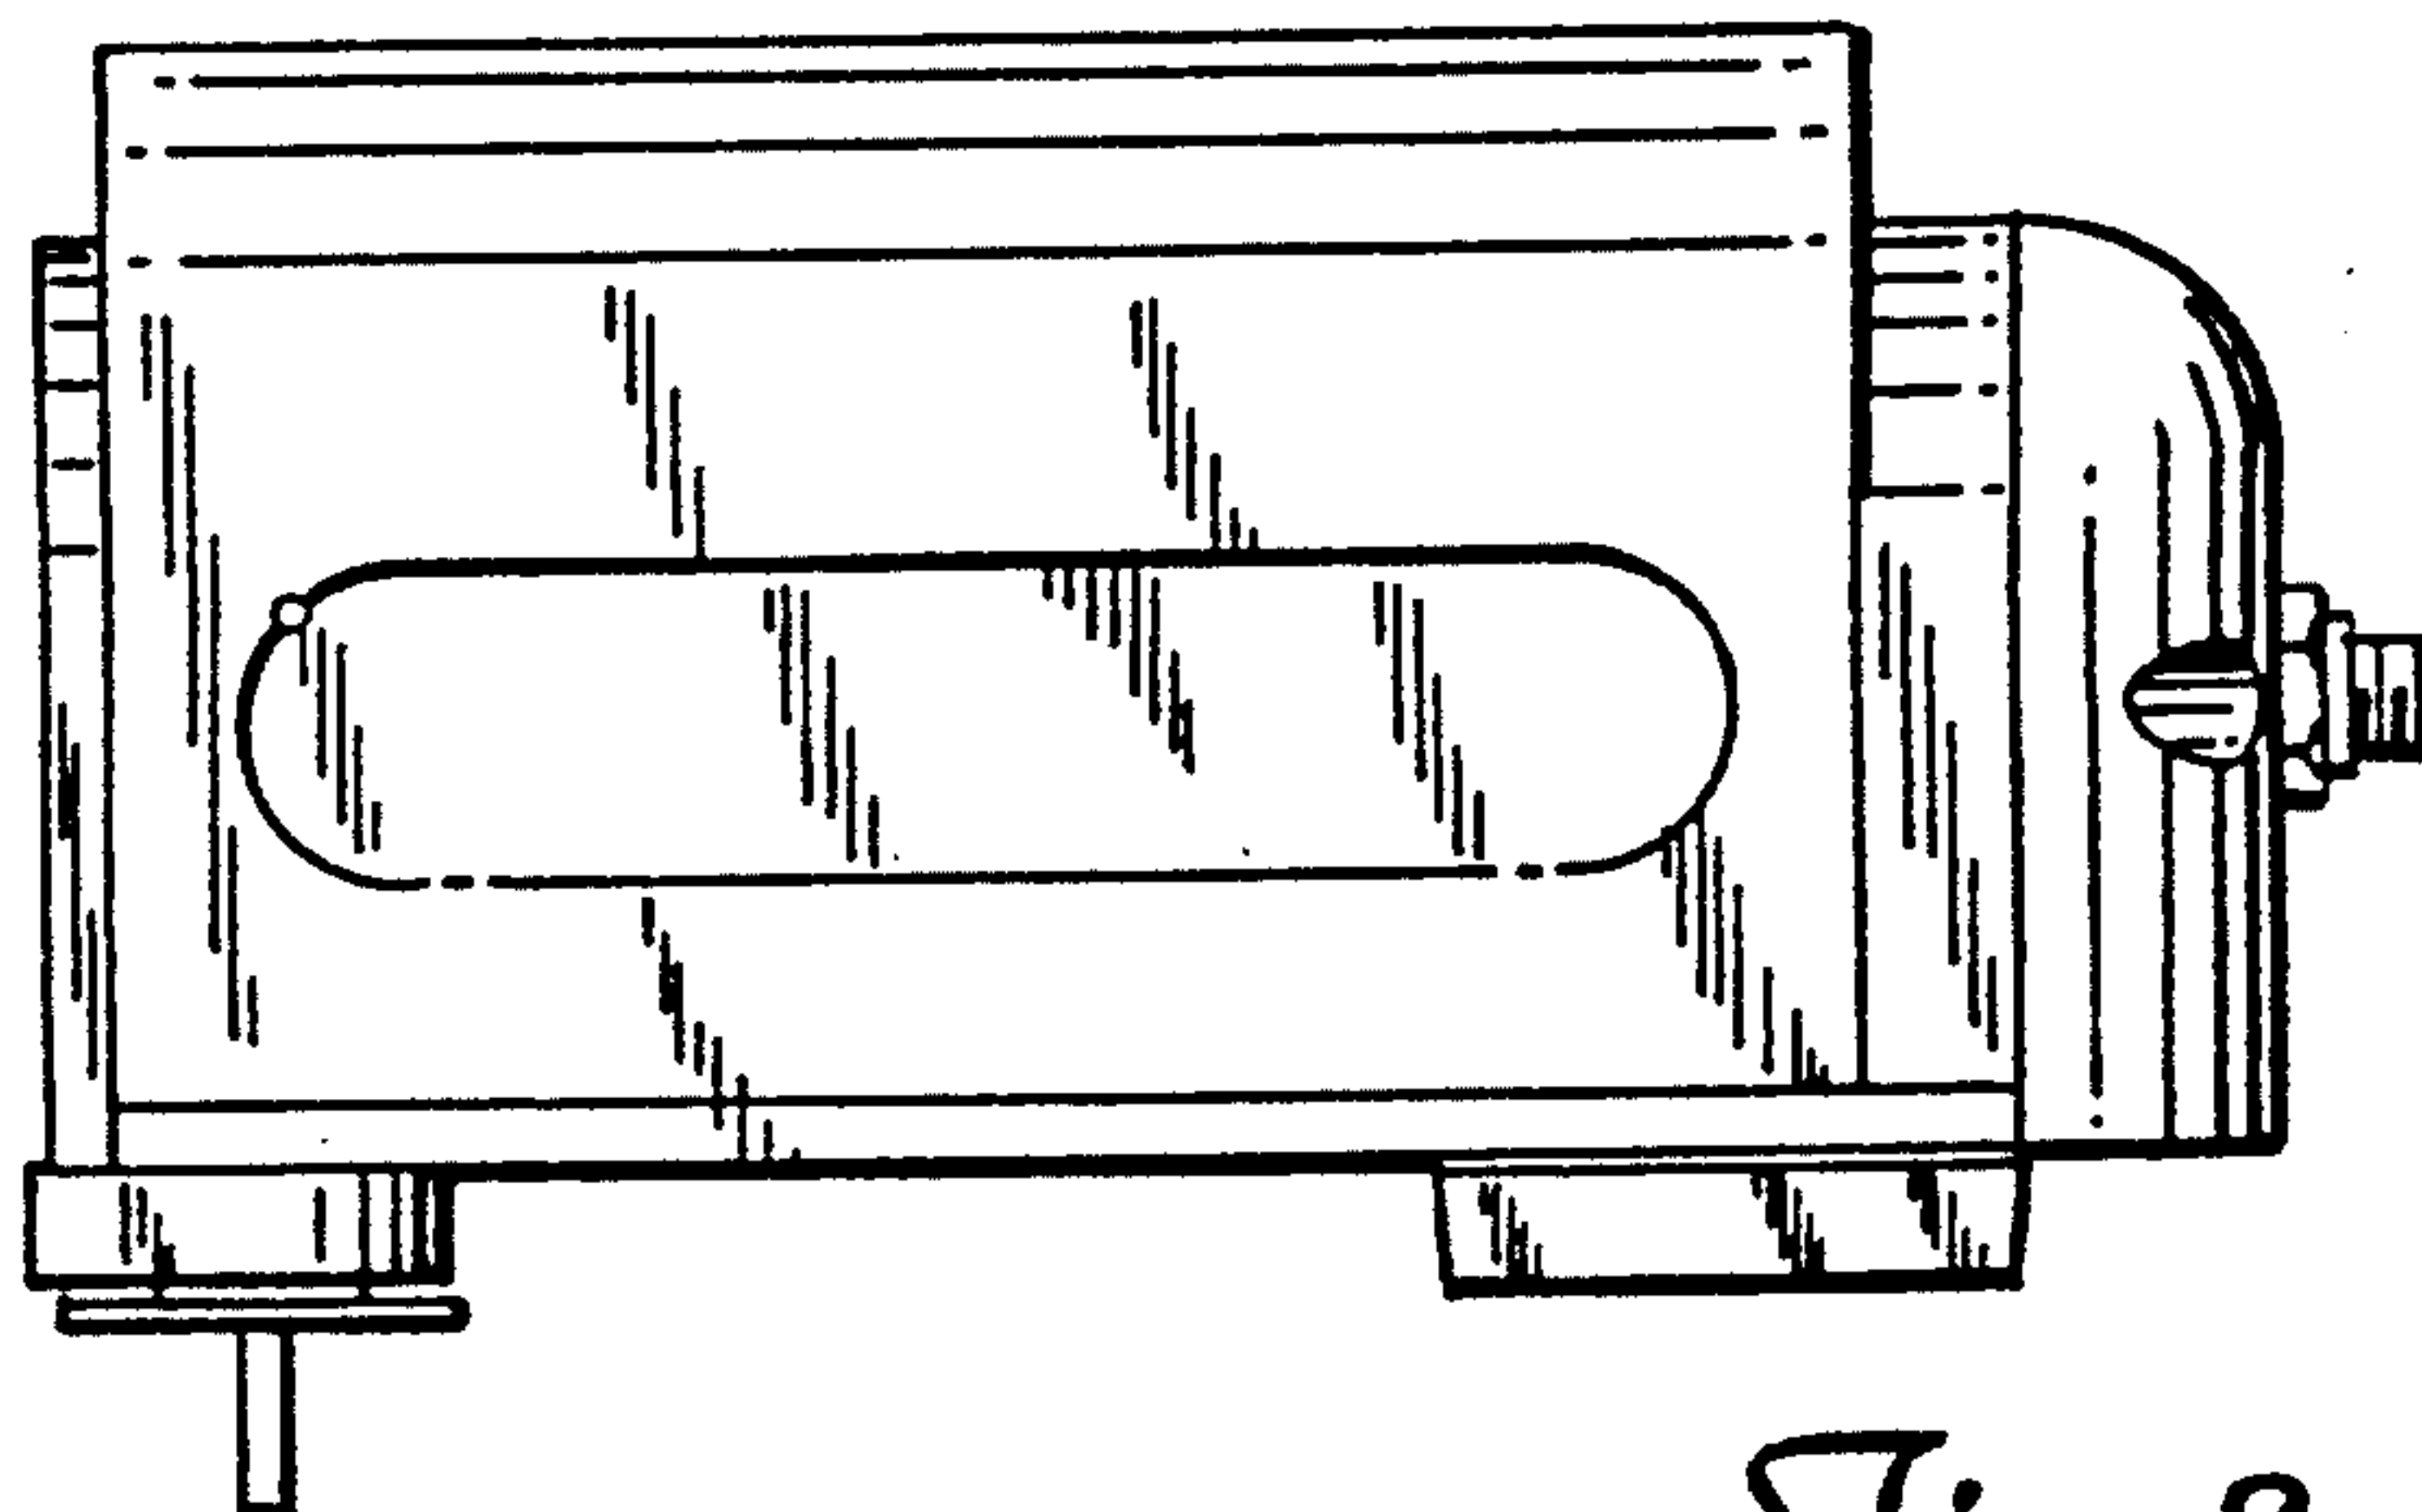


Fig. 2



Fig. 3

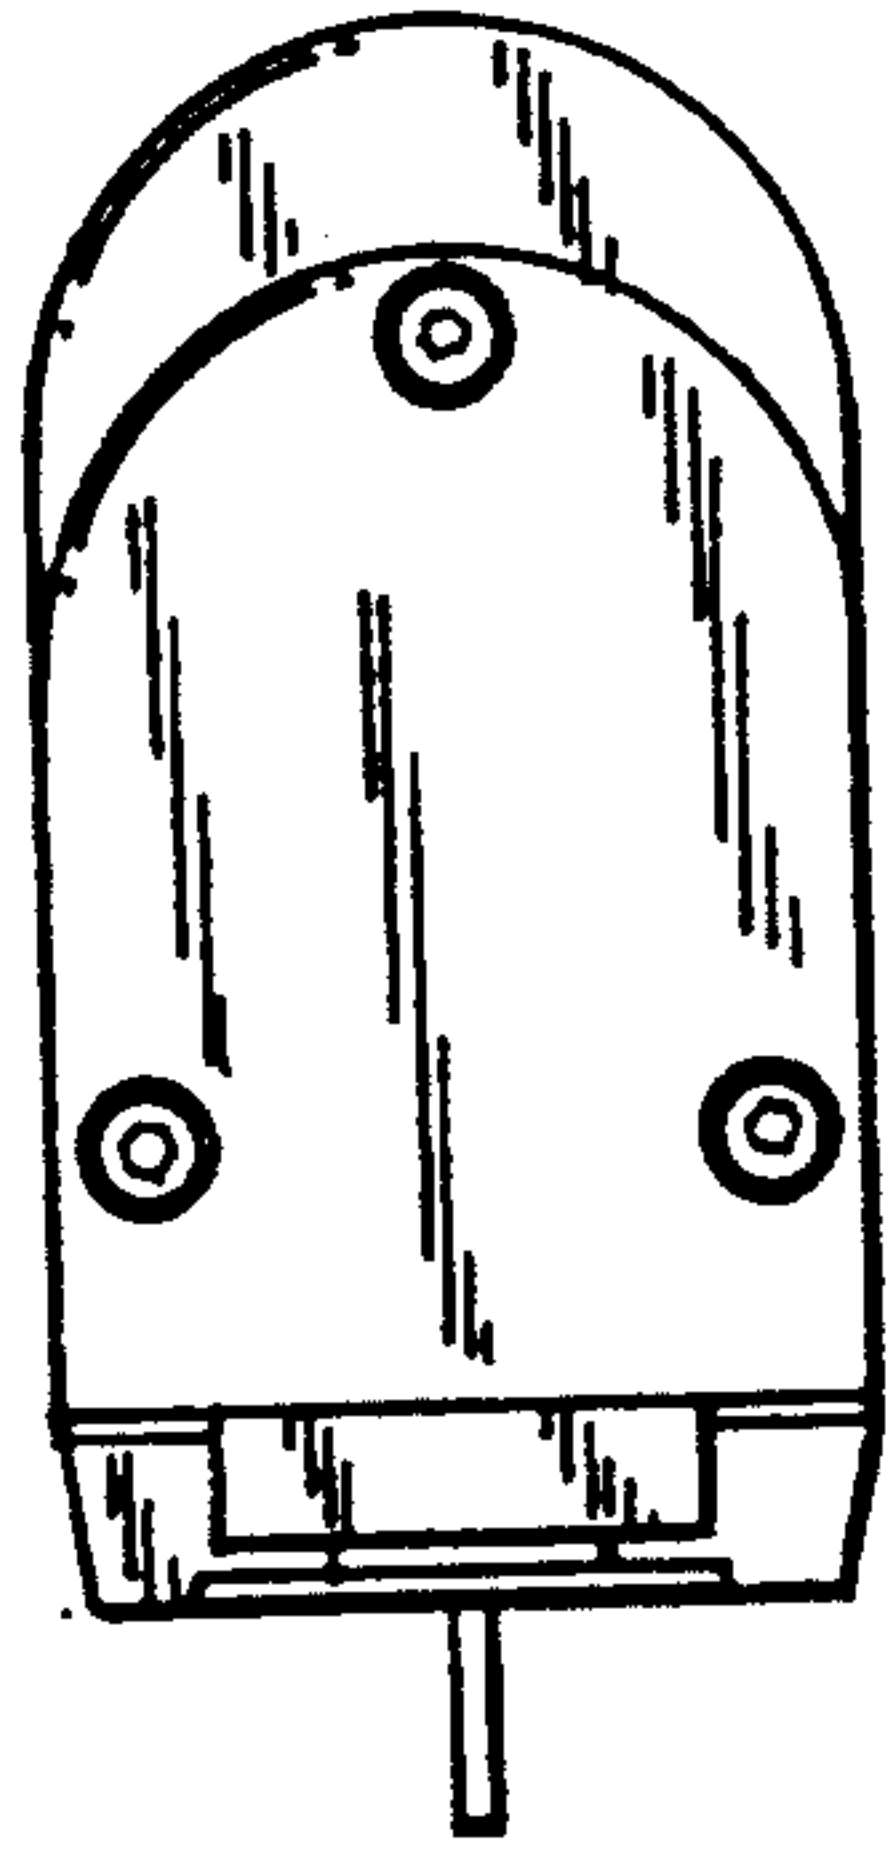


Fig. 4

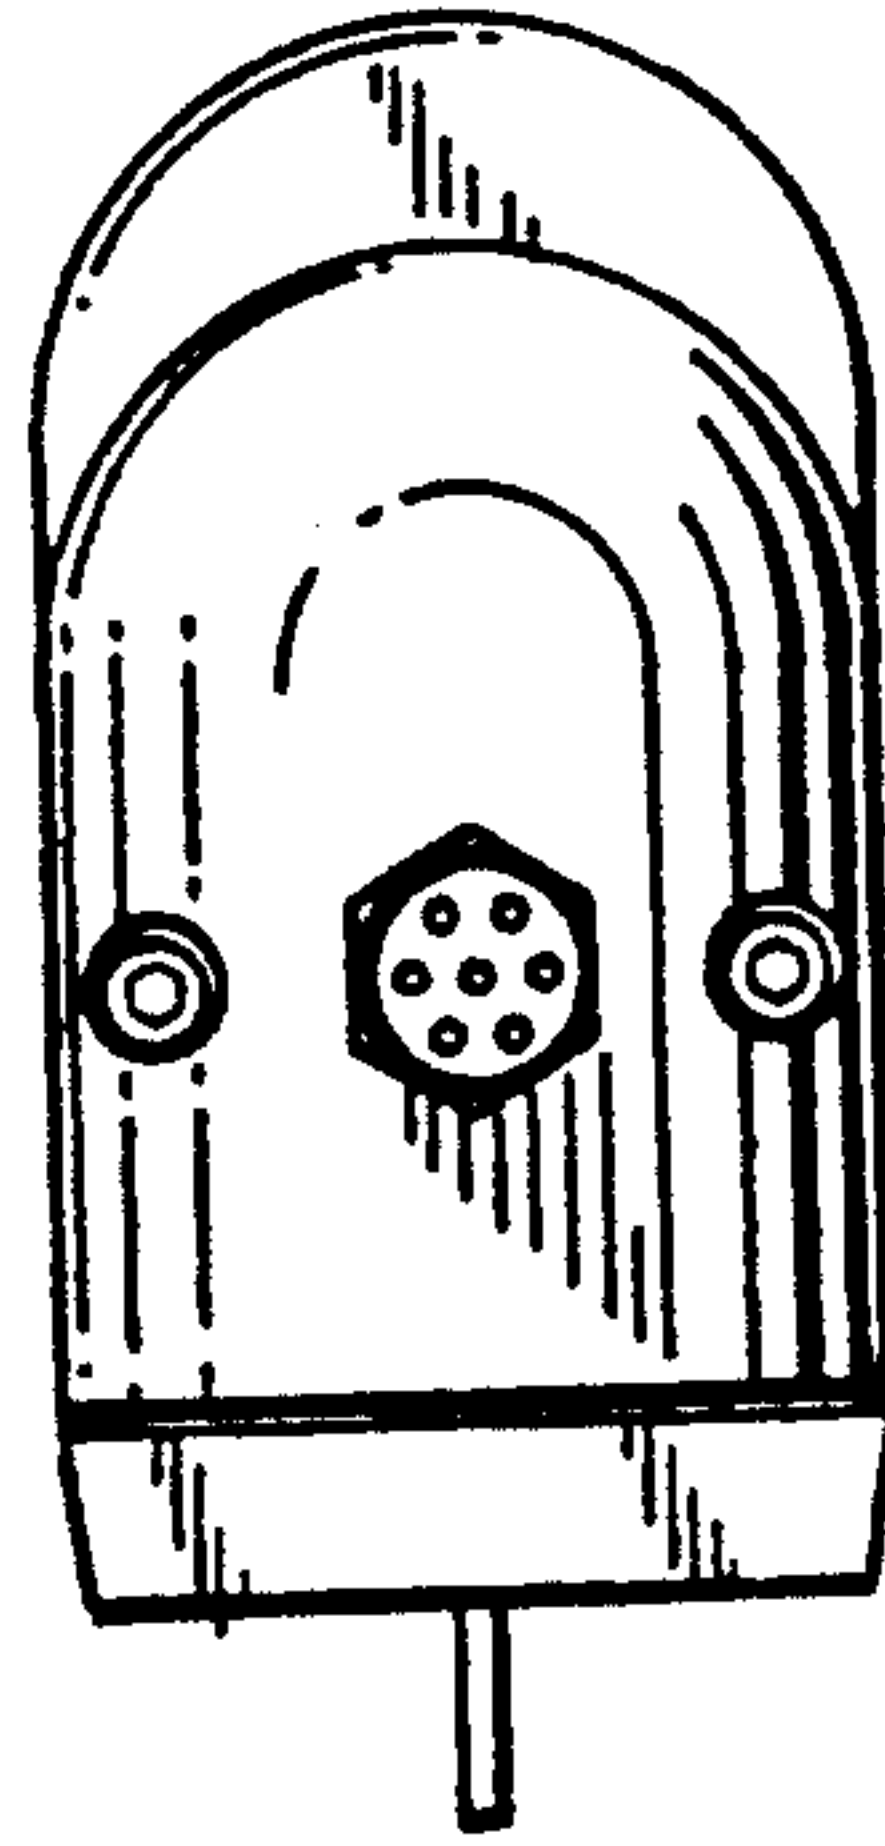


Fig. 5

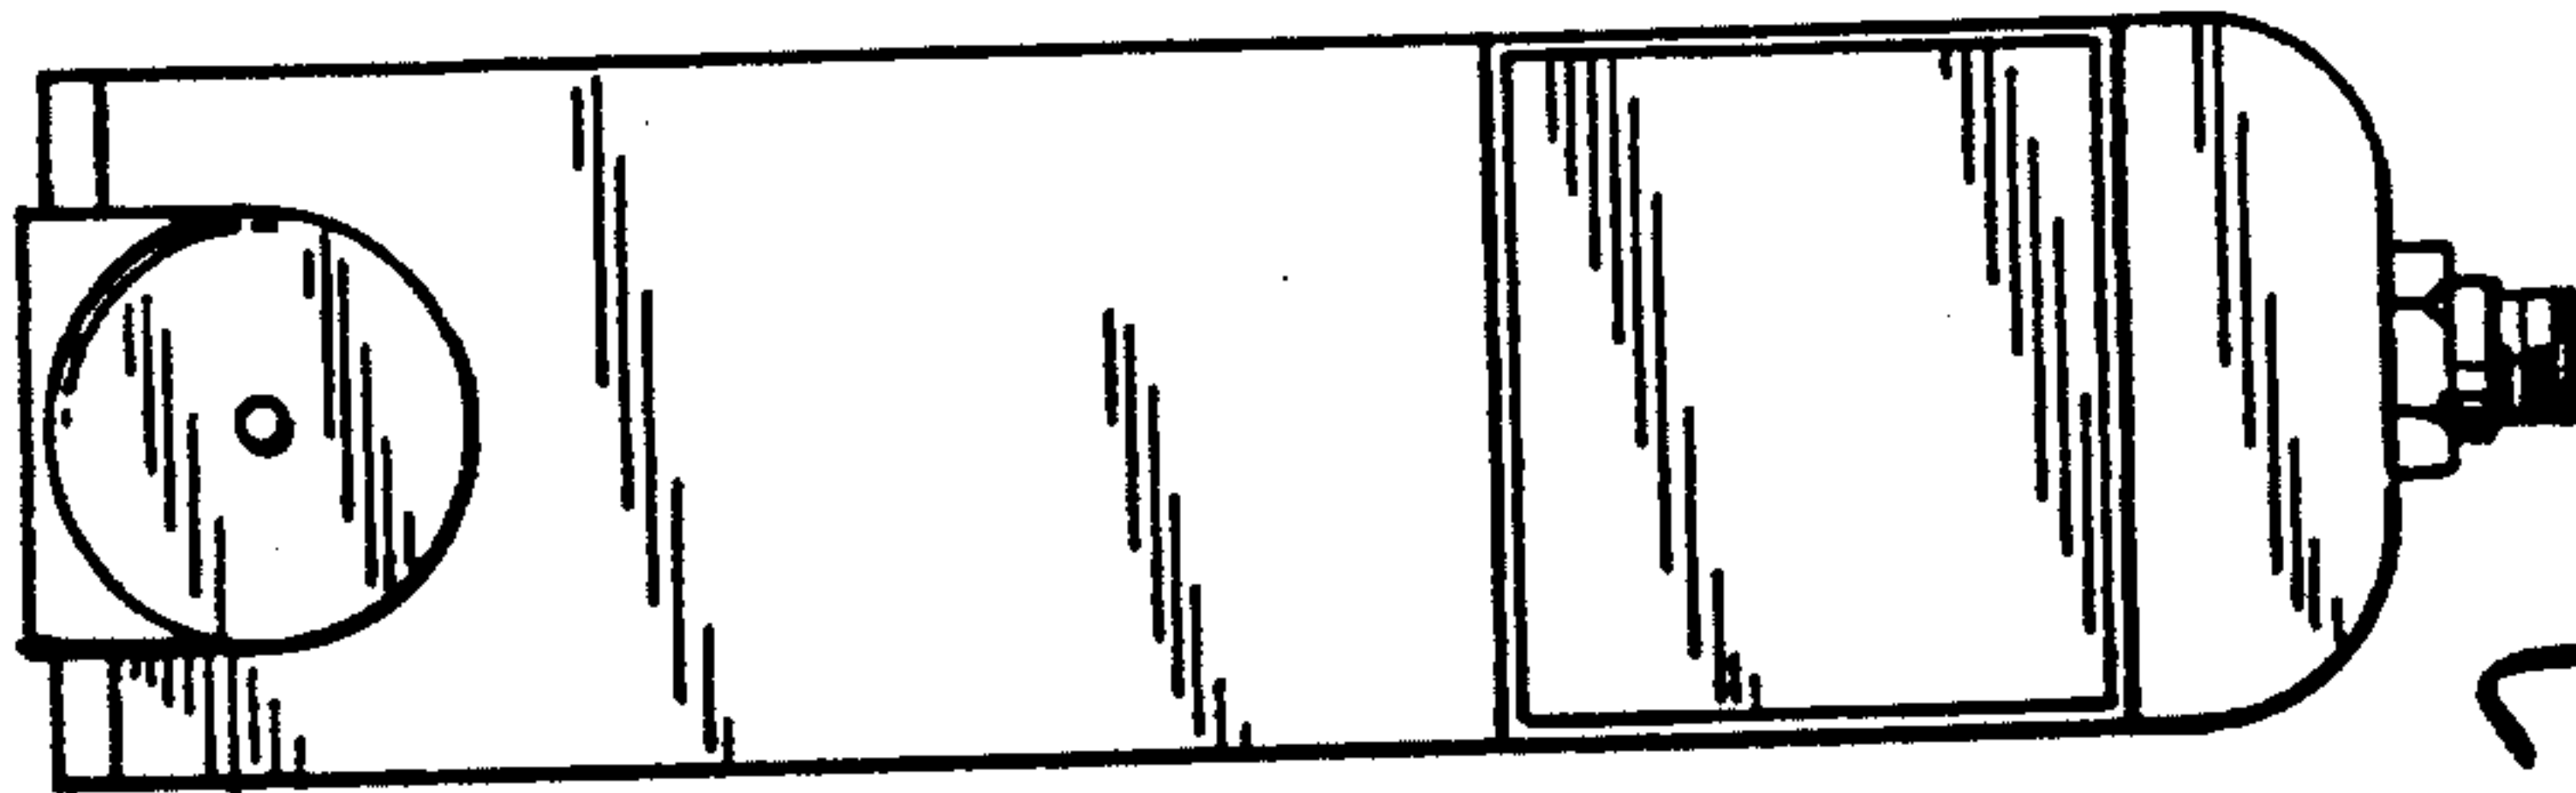


Fig. 6