



US00D347479S

**United States Patent** [19]  
**Hansen et al.**

[11] **Patent Number: Des. 347,479**  
[45] **Date of Patent: \*\* May 31, 1994**

[54] **BOTTLE FOR A LABORATORY ANALYZER** [56]

**References Cited**

**U.S. PATENT DOCUMENTS**

[75] **Inventors: Christian M. Hansen; Robert C. Butcher, Jr., both of Medway; Kevin D. Lear, Franklin, all of Mass.**

D. 250,573 12/1978 Evangelista et al. .... D9/526  
D. 264,127 4/1982 Peterson ..... D24/224  
D. 285,725 9/1986 Franchere ..... D9/526 X  
D. 287,638 1/1987 Moore et al. .... D24/224  
D. 291,730 9/1987 Kelln et al. .... D24/224  
D. 328,431 8/1992 Skidmore et al. .... D9/523  
5,152,965 10/1992 Fish et al. .... D24/224 X

[73] **Assignee: Ciba Corning Diagnostics Corp., Medfield, Mass.**

[\*] **Notice: The portion of the term of this patent subsequent to Nov. 9, 2007 has been disclaimed.**

*Primary Examiner*—A. Hugo Word  
*Assistant Examiner*—I. Simmons  
*Attorney, Agent, or Firm*—Nicholas I. Slepchuk, Jr.; Arthur S. Morgenstern; Judith A. Roesler

[\*\*] **Term: 14 Years**

[57] **CLAIM**

The ornamental design for a bottle for a laboratory analyzer, as shown and described.

[21] **Appl. No.: 869,344**


**DESCRIPTION**


[22] **Filed: Apr. 15, 1992**

[52] **U.S. Cl. .... D24/224; D9/526; D24/121**


[58] **Field of Search .... D9/520, 523, 526, 572, D9/347, 341; 215/1 C; 220/23.4, 476, 480, 481; 356/246, 244; 422/72, 102, 103, 104; 436/165, 166, 145; D24/224, 121**

FIG. 1 is a side elevational view of a bottle for a laboratory analyzer showing our new design, the opposite side elevational view being a mirror image thereto; FIG. 2 is a bottom plan view; FIG. 3 is a top plan view; FIG. 4 is a front elevational view; FIG. 5 is a rear elevational view; and, FIG. 6 is a perspective view.

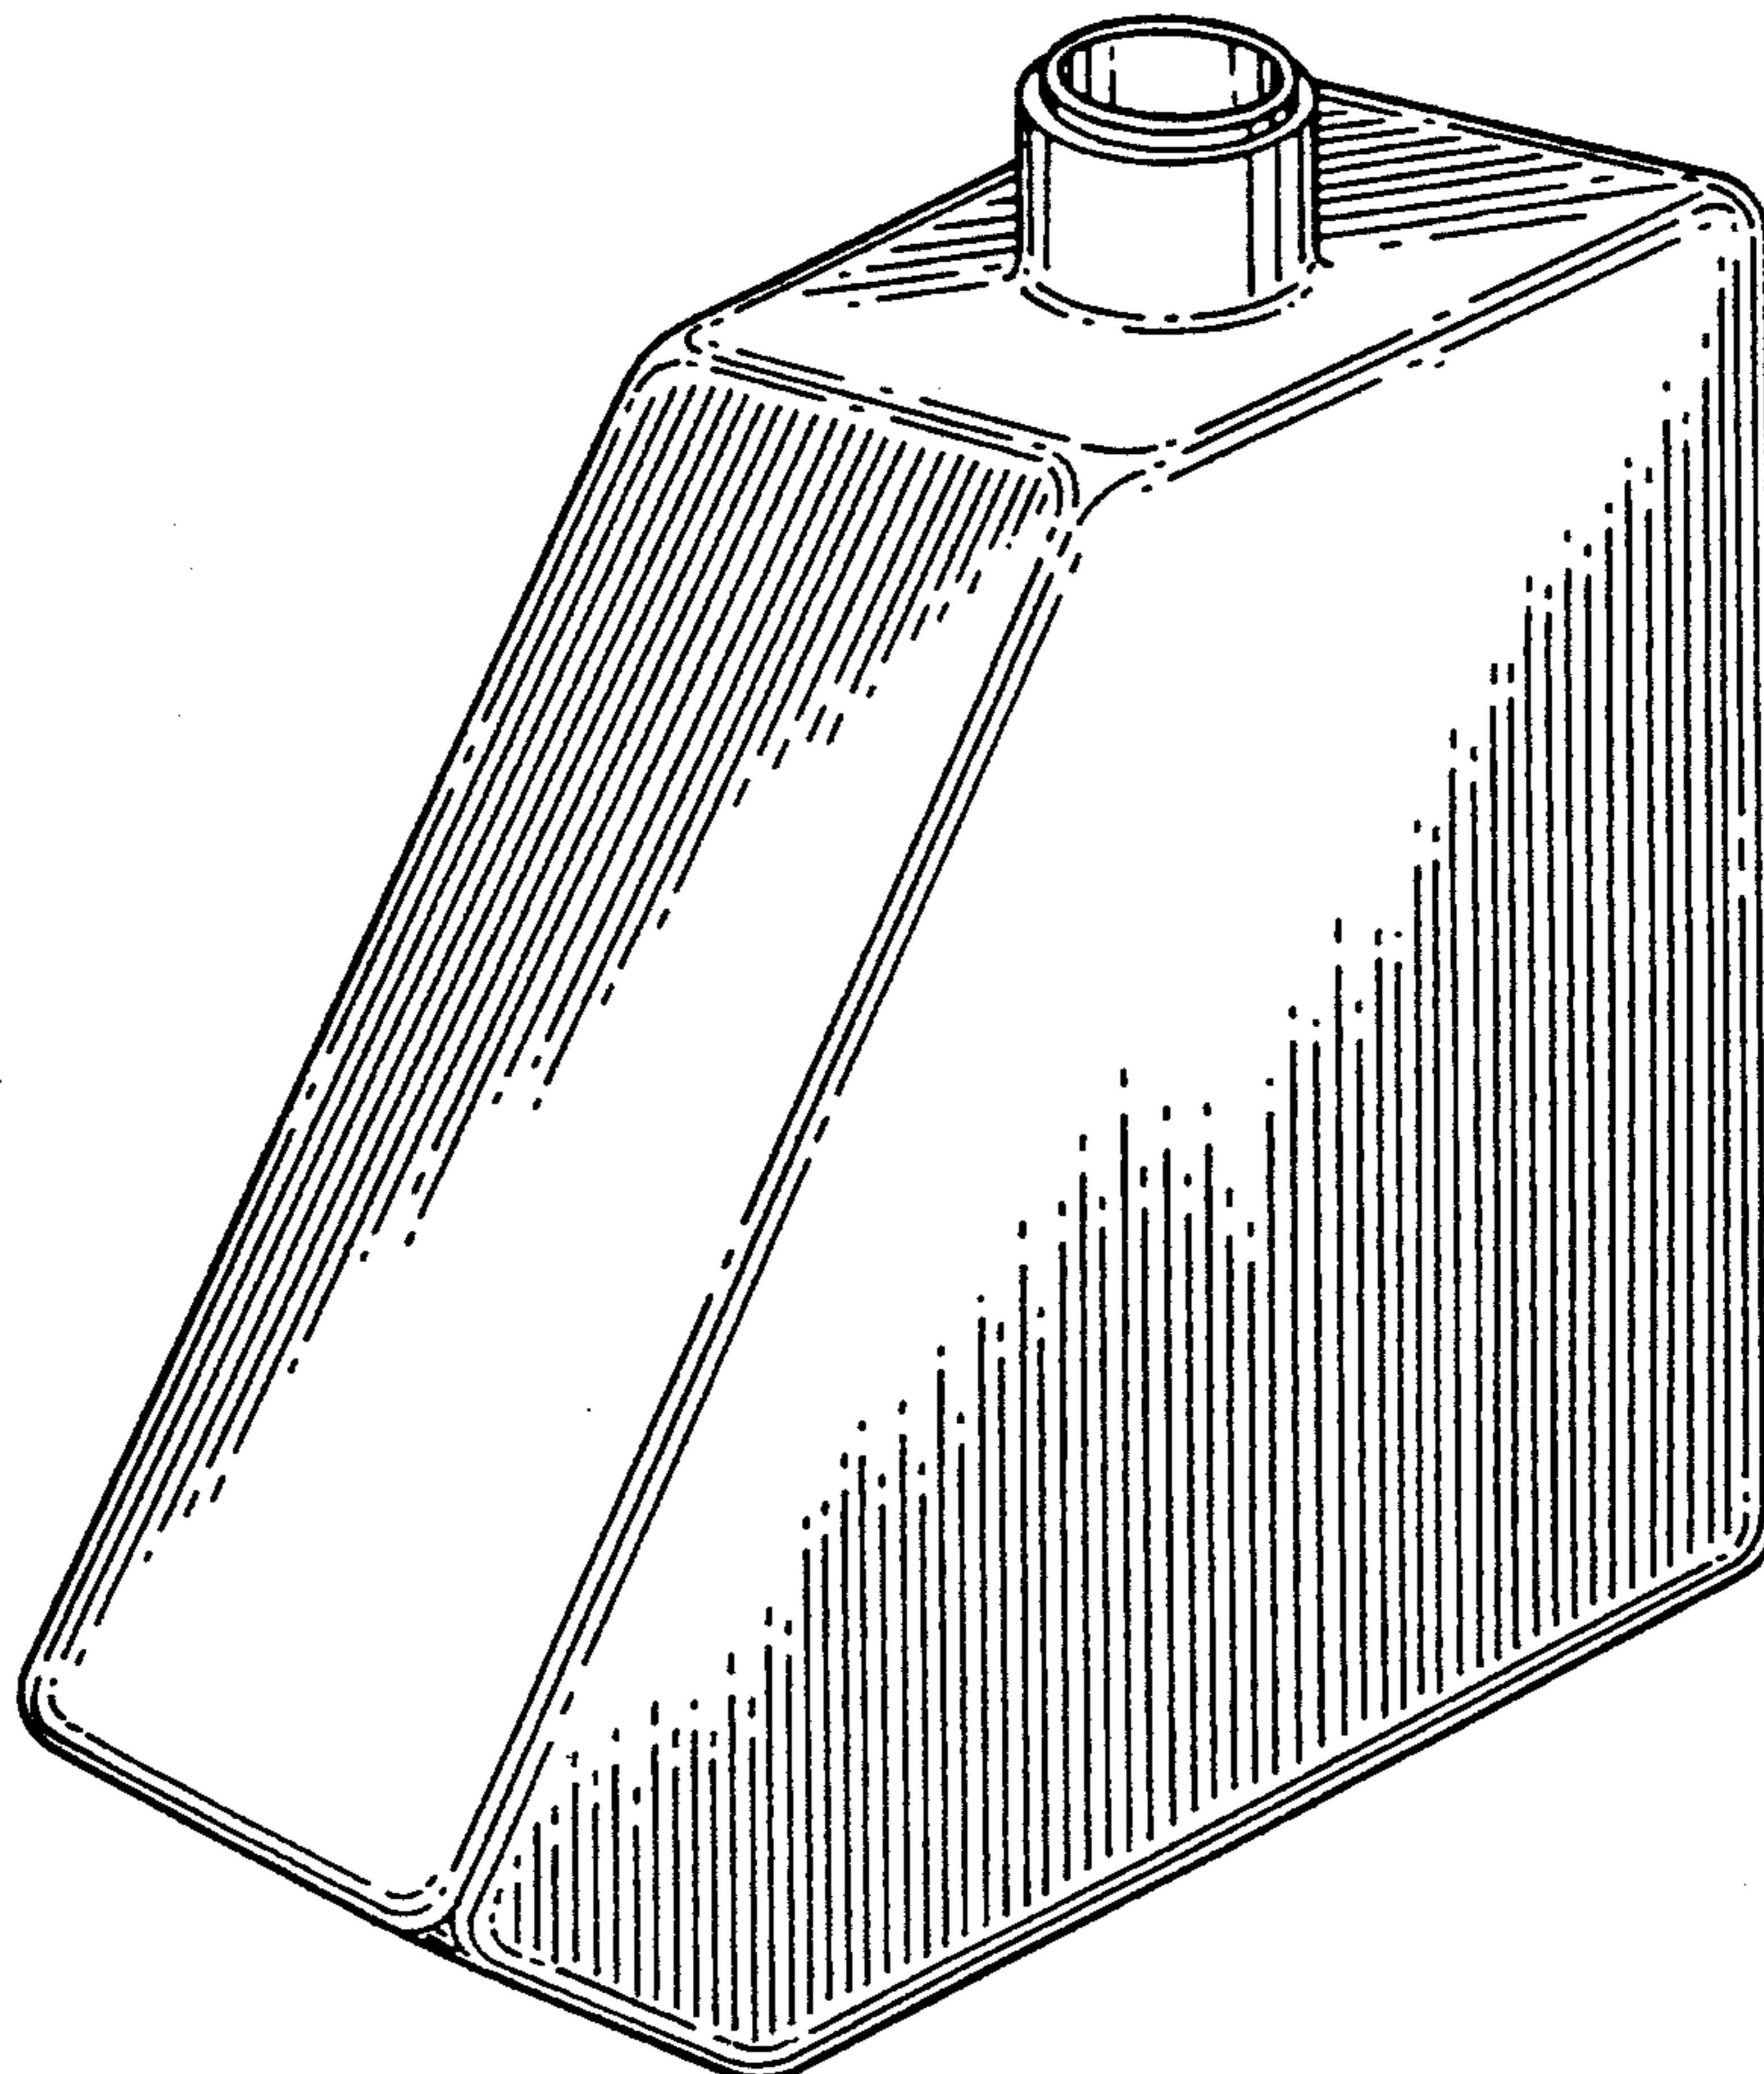


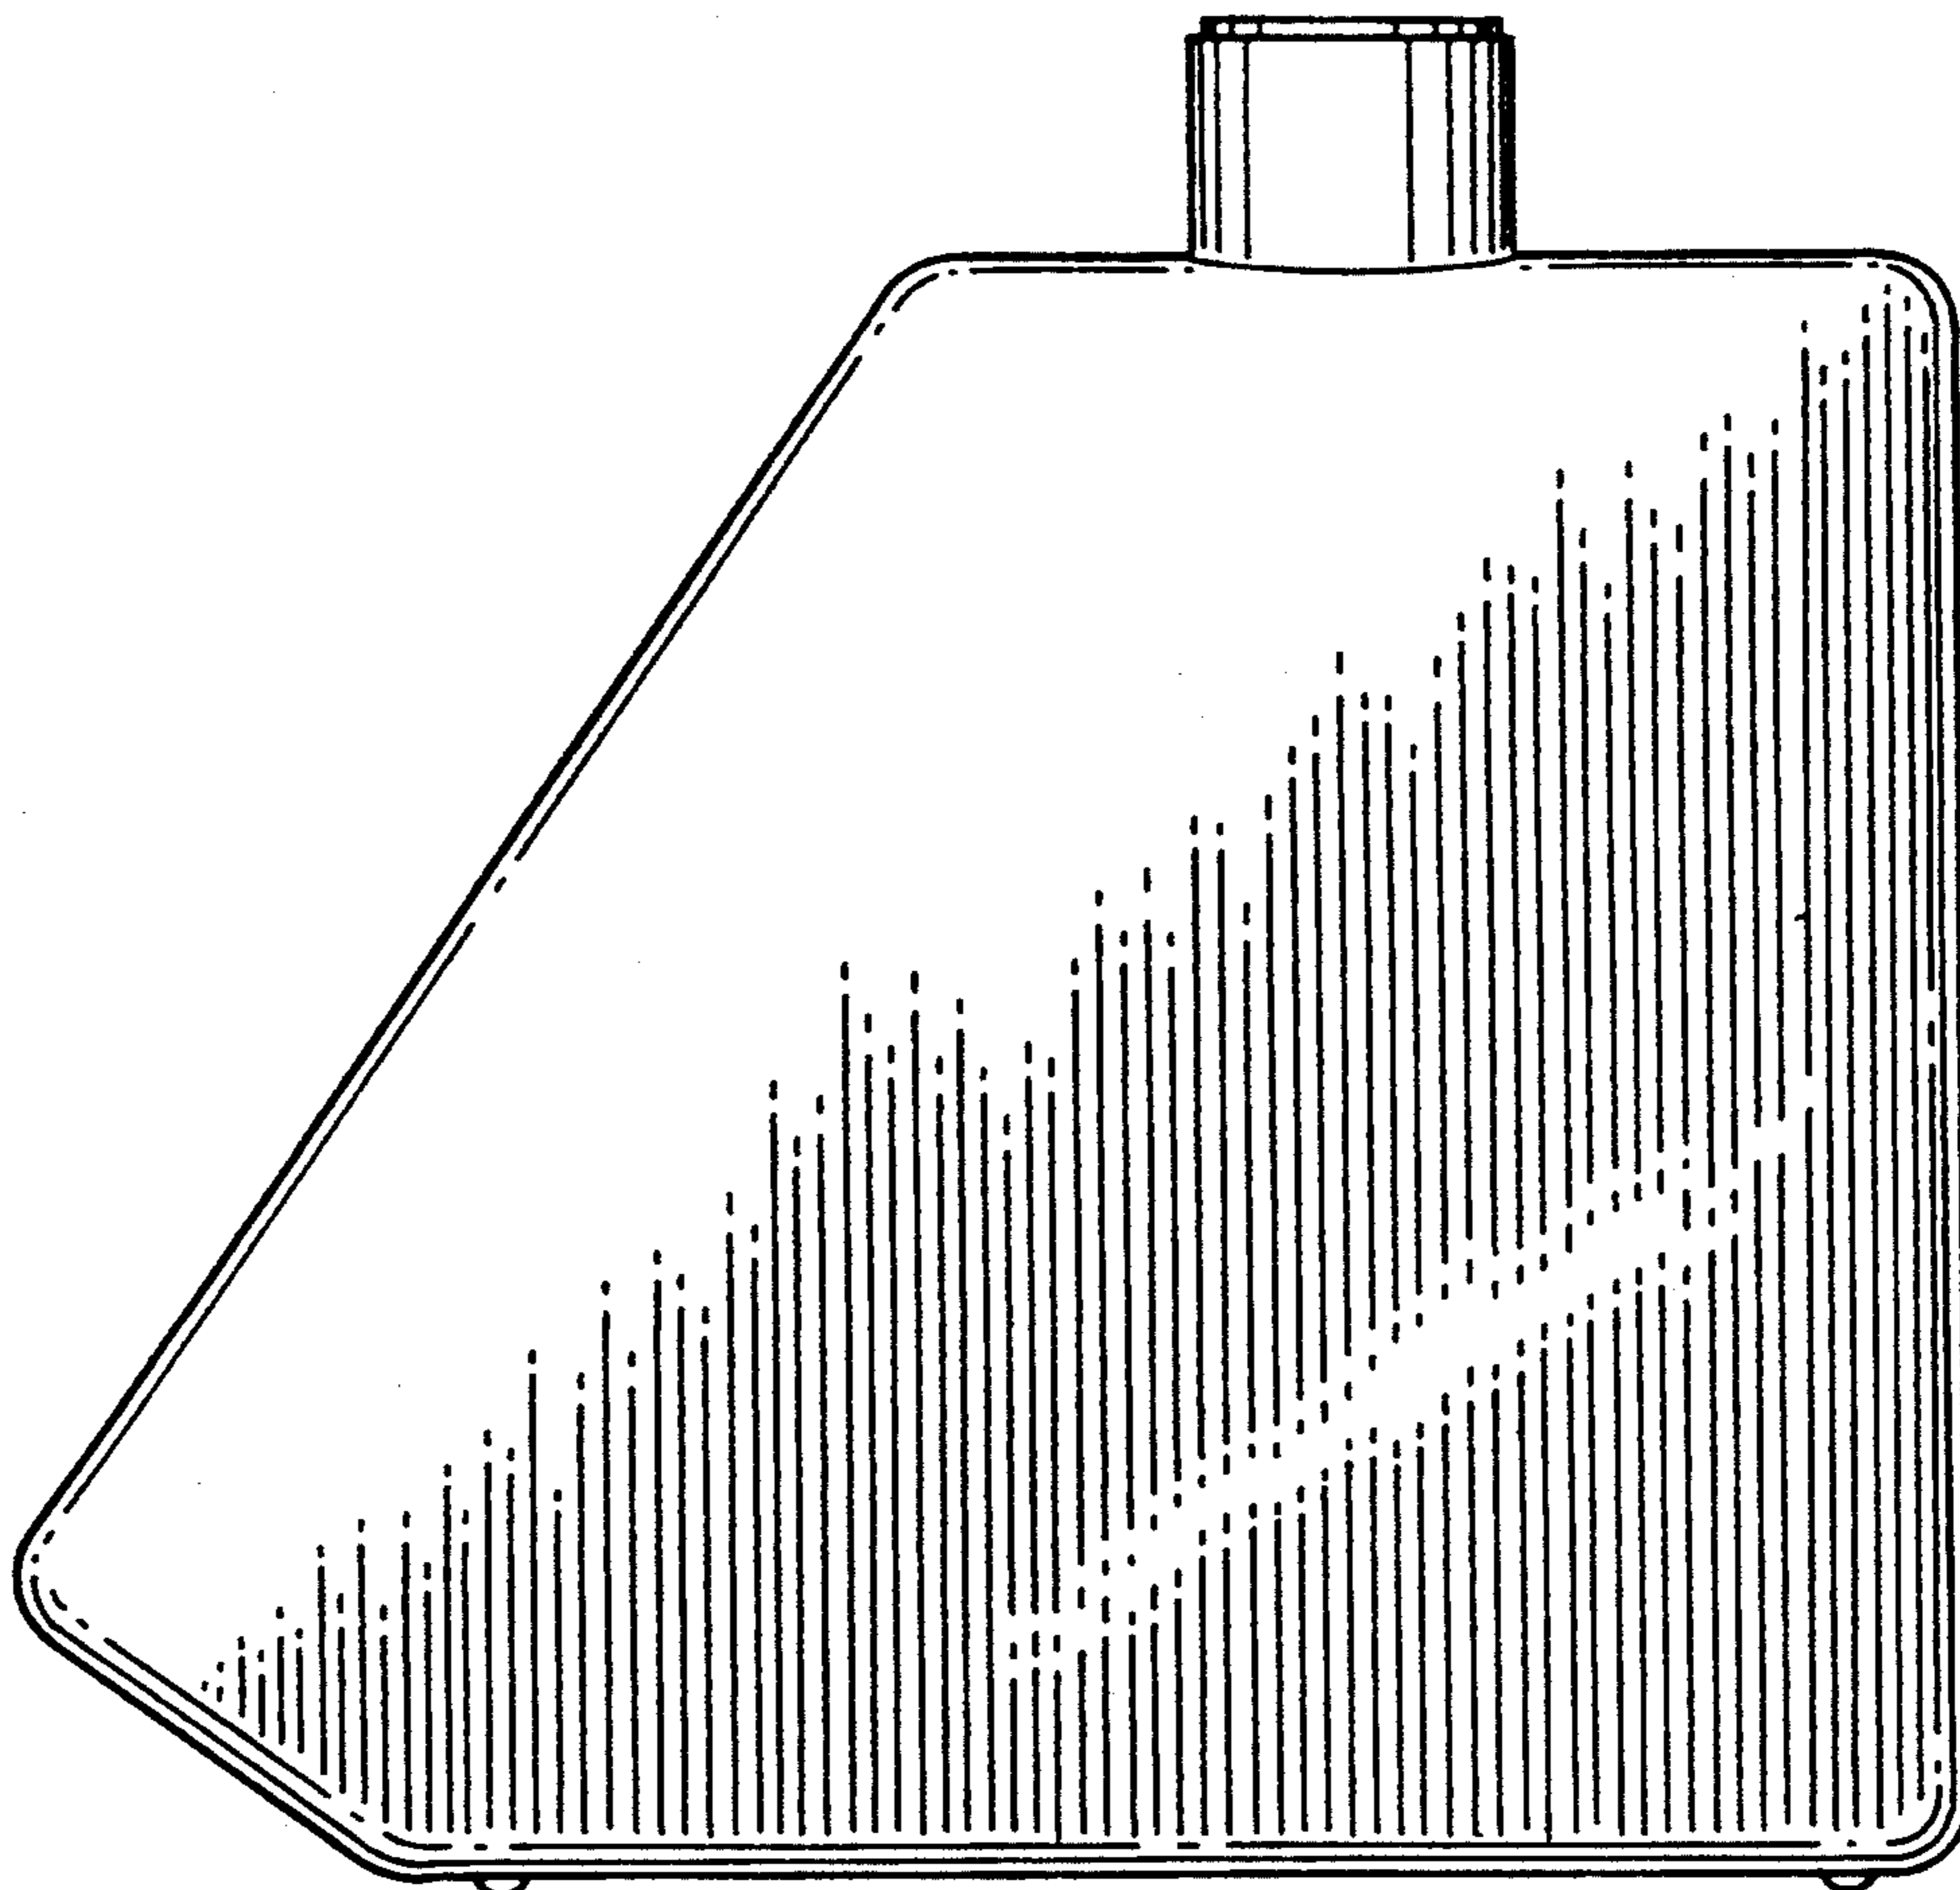


*Fig. 1*

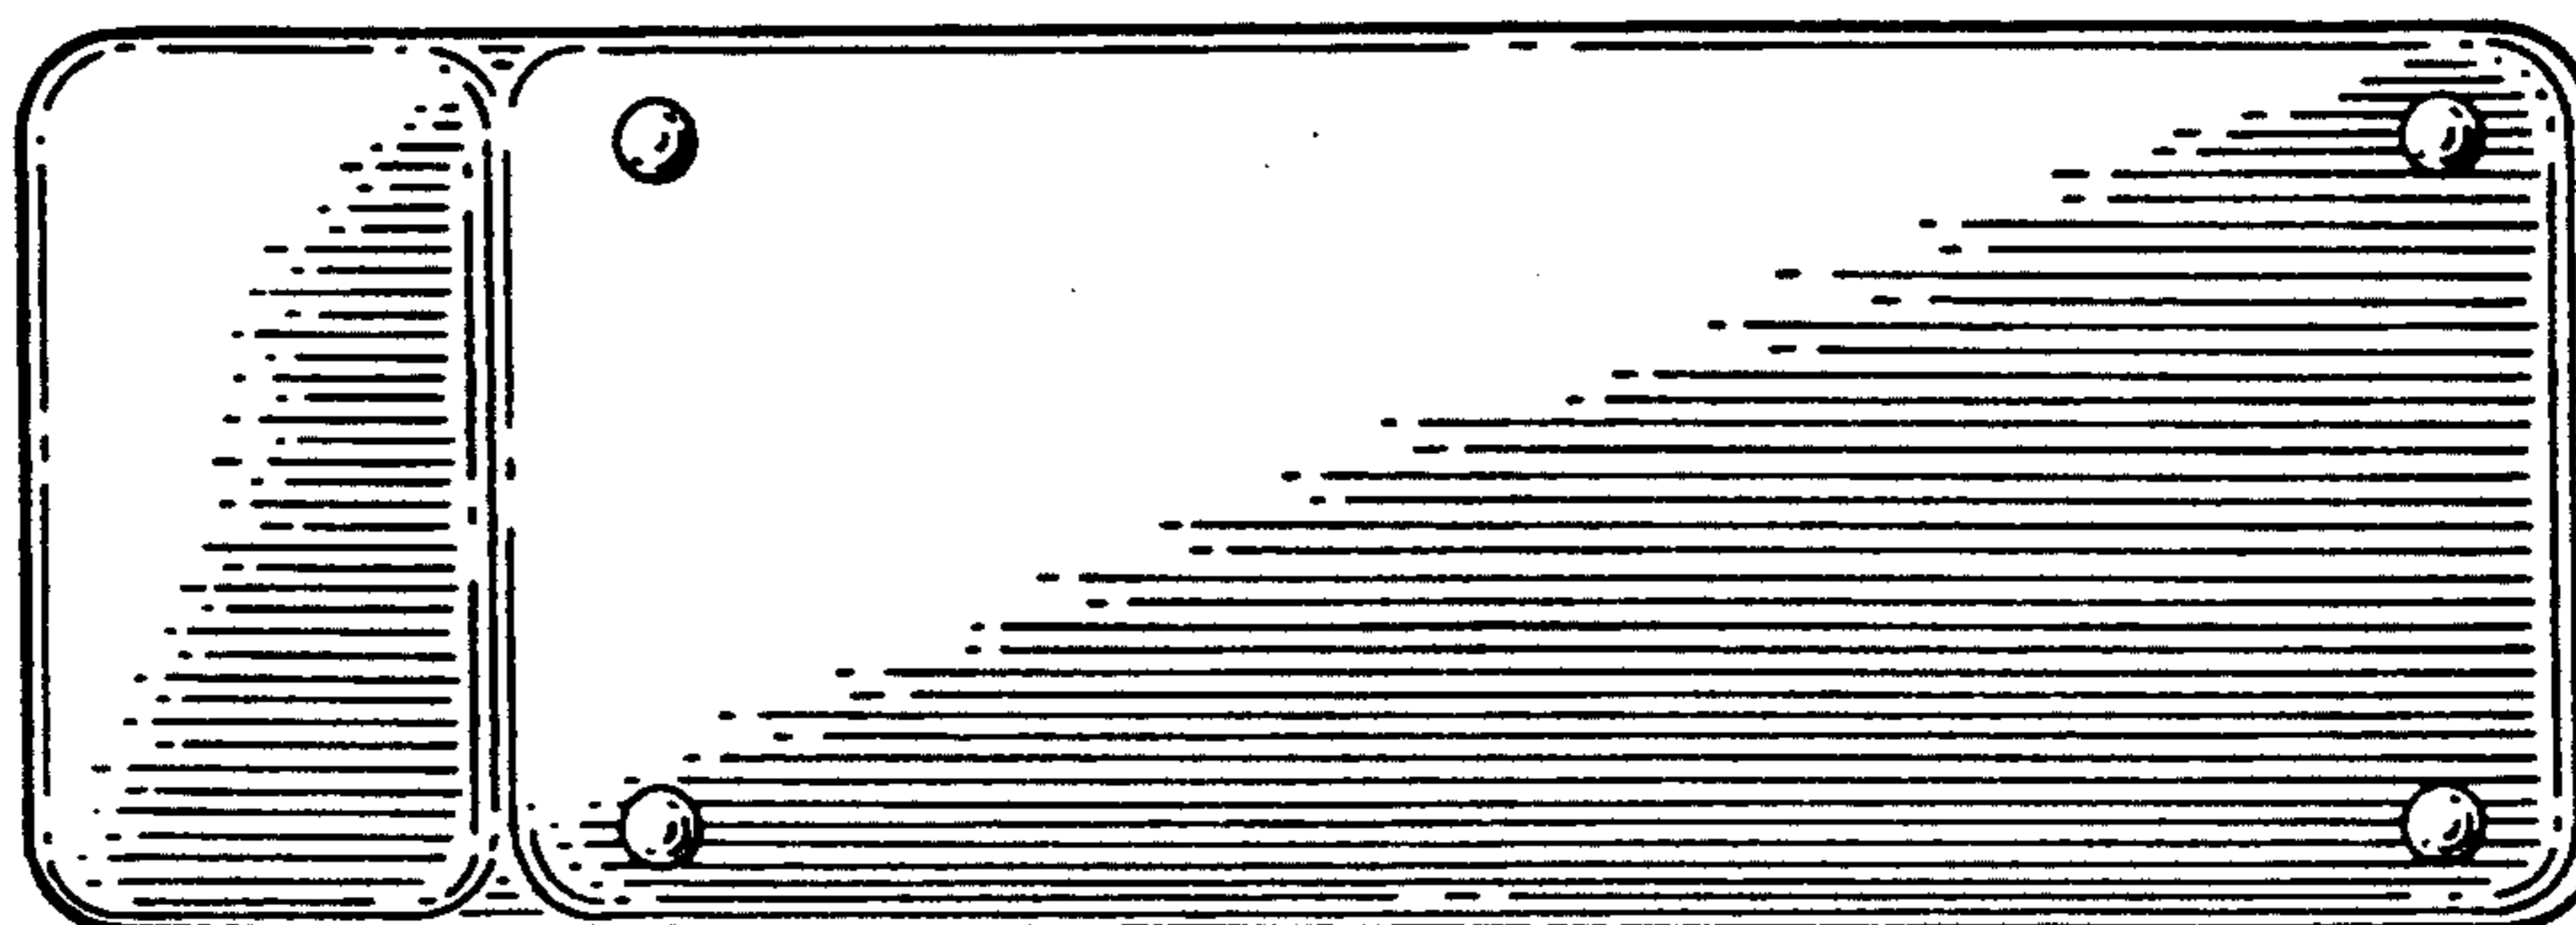


*Fig. 2*

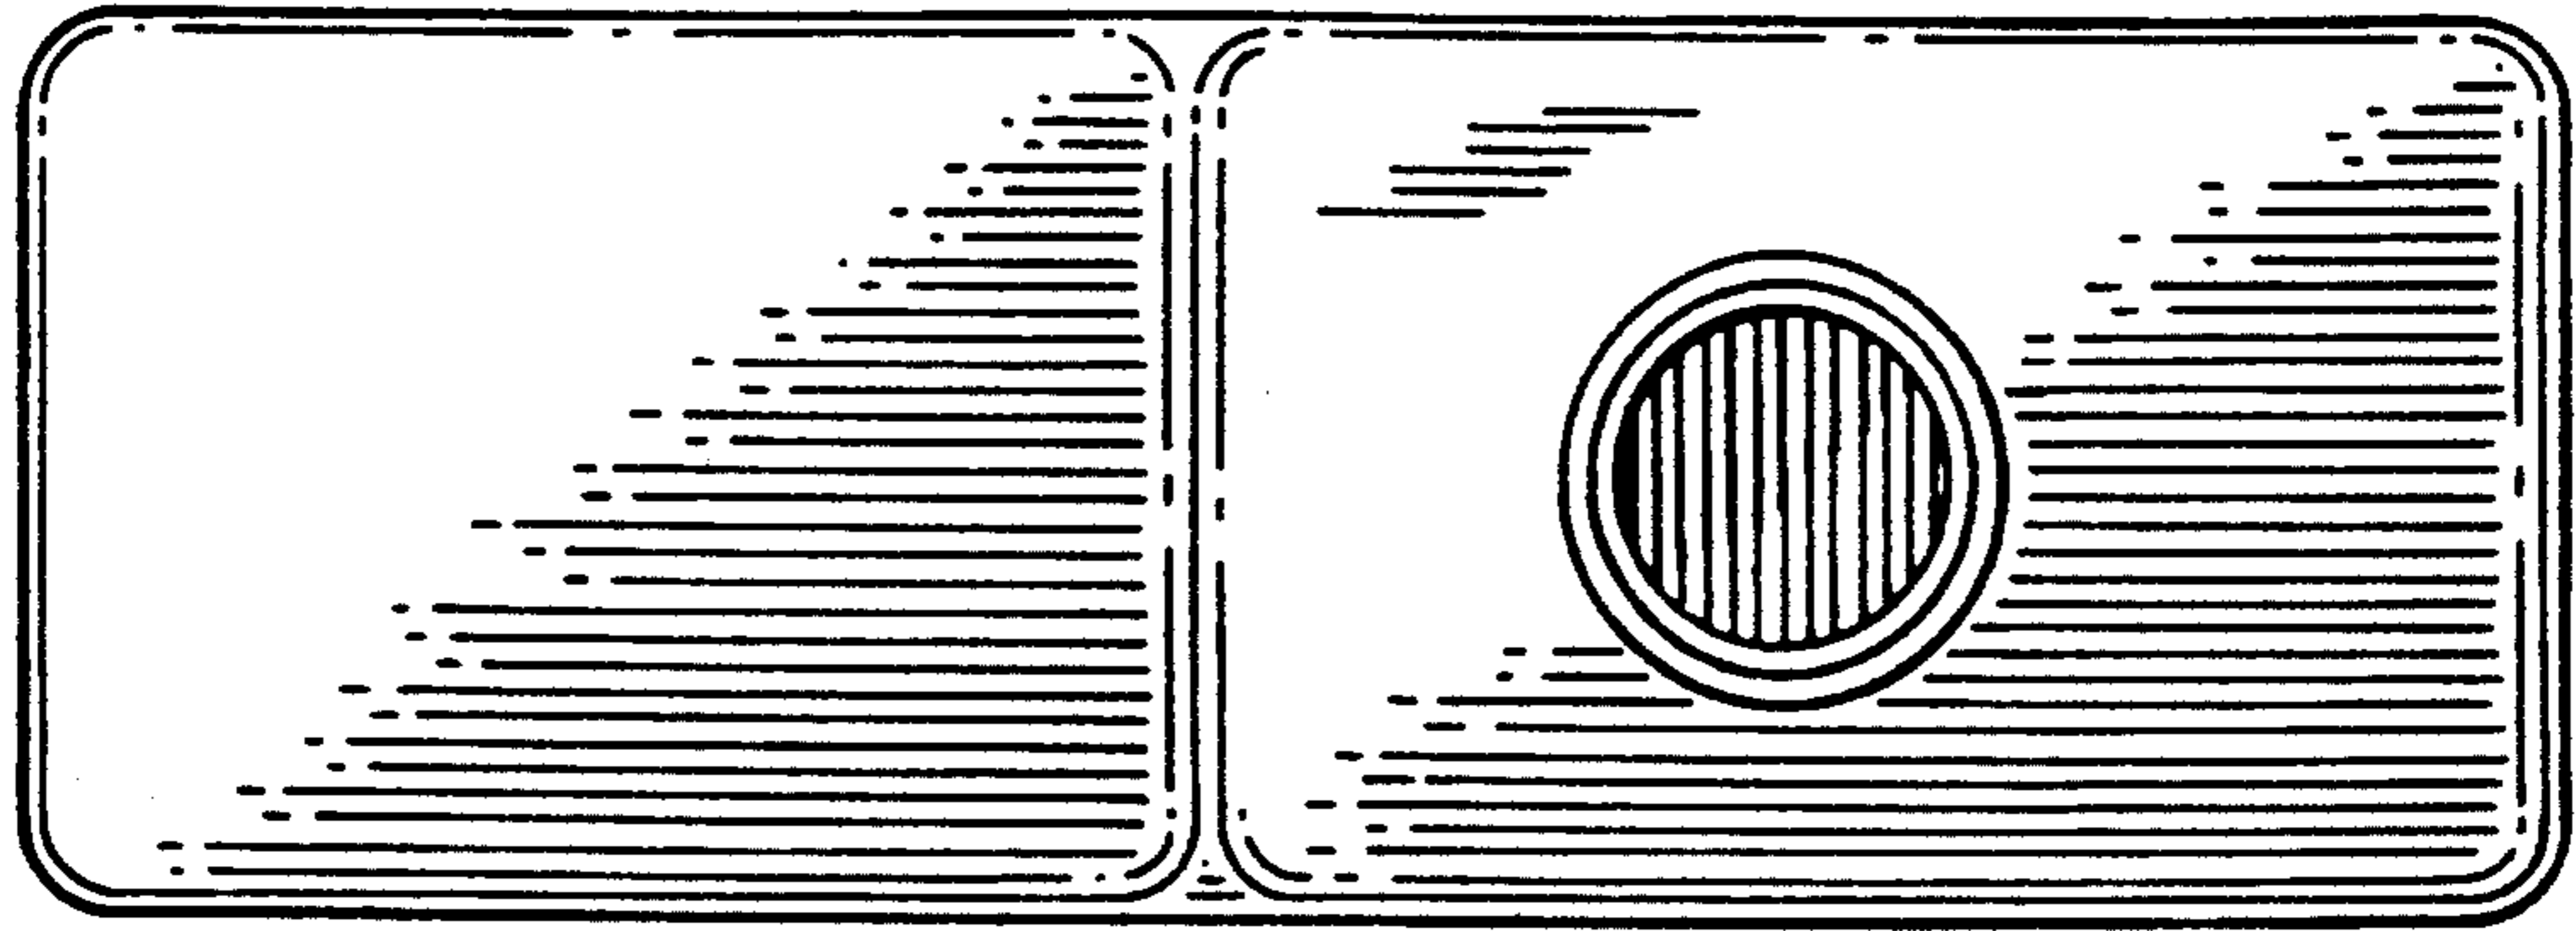


*Fig. 3*

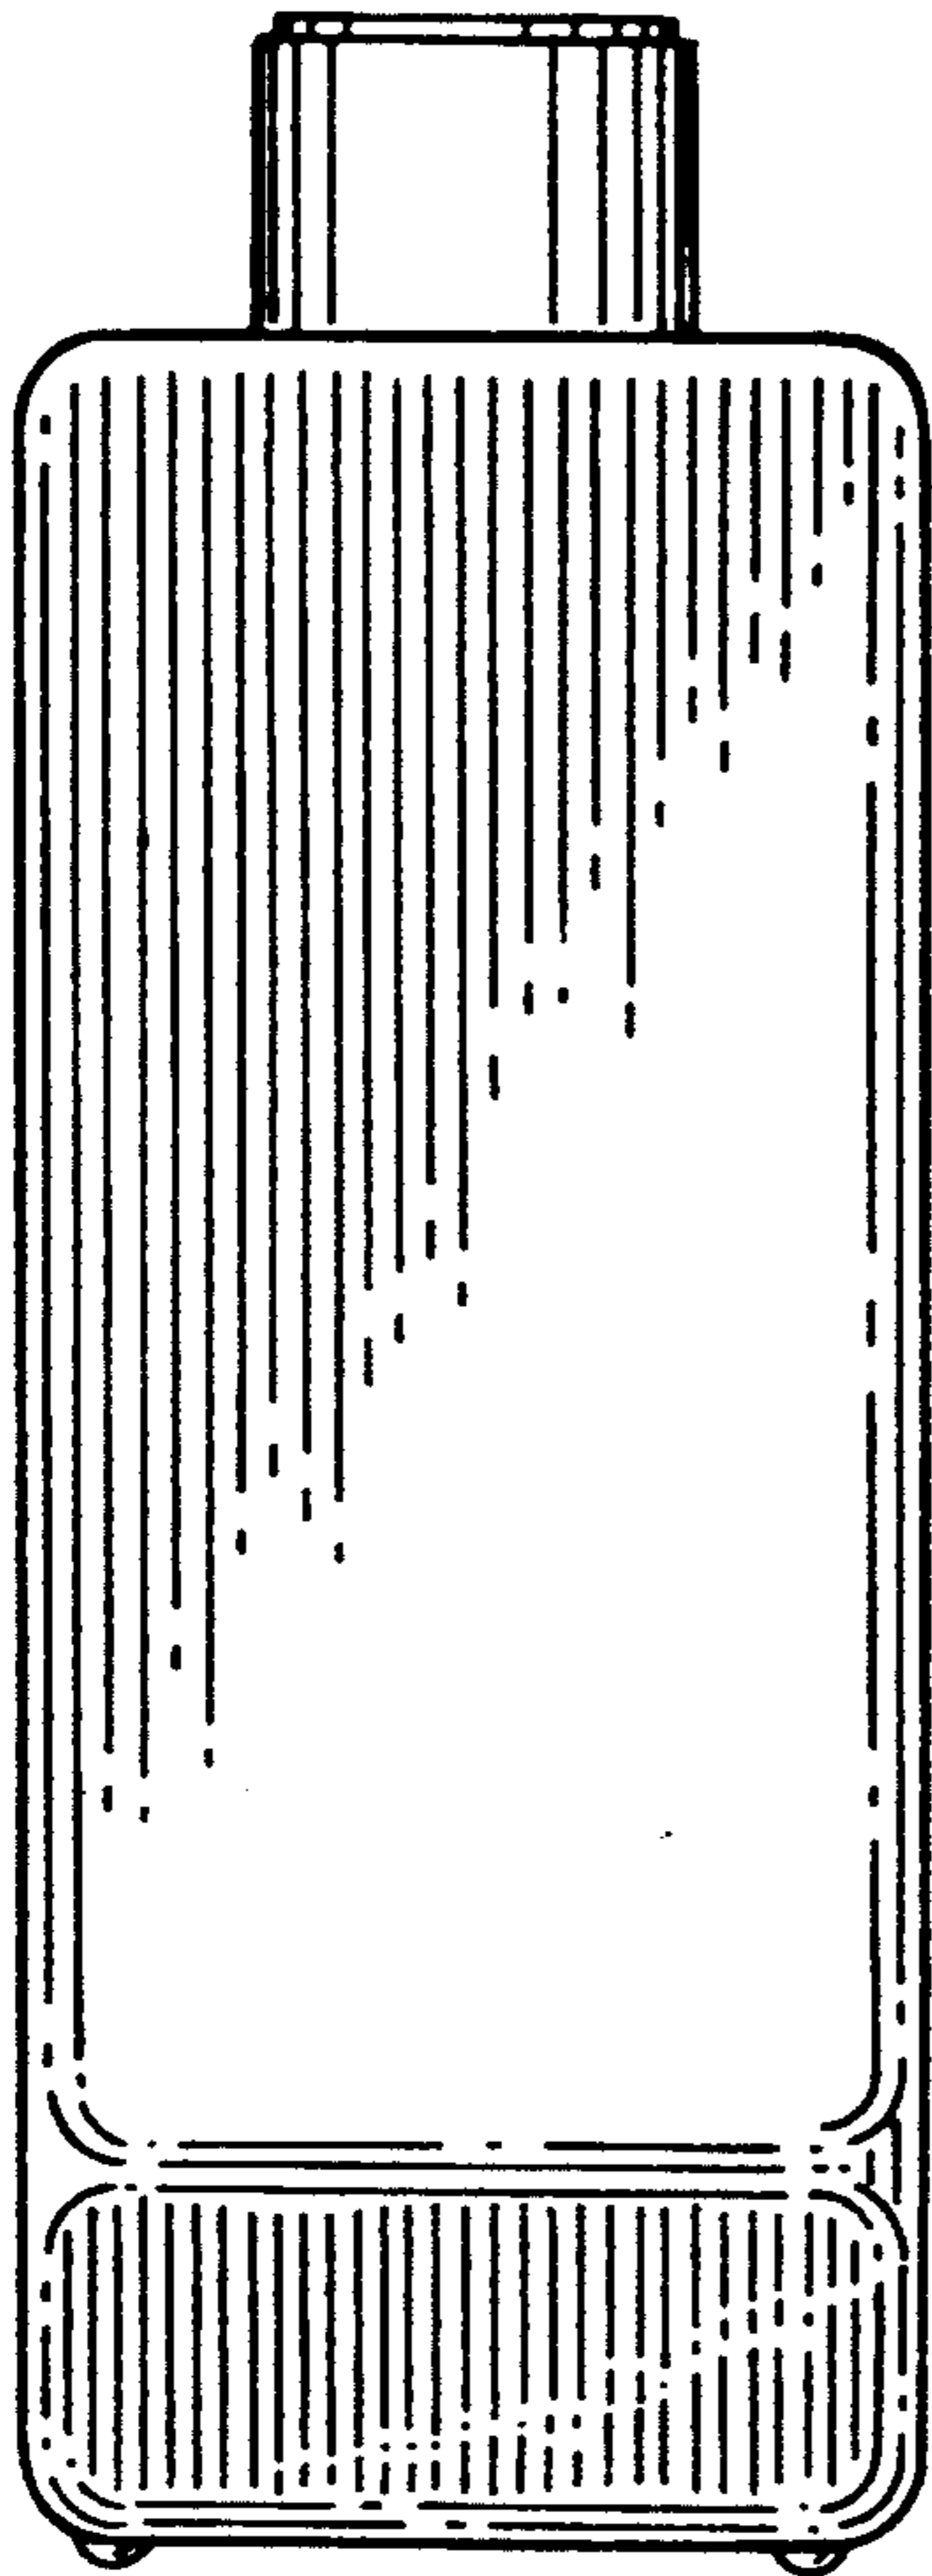

*Fig. 4*

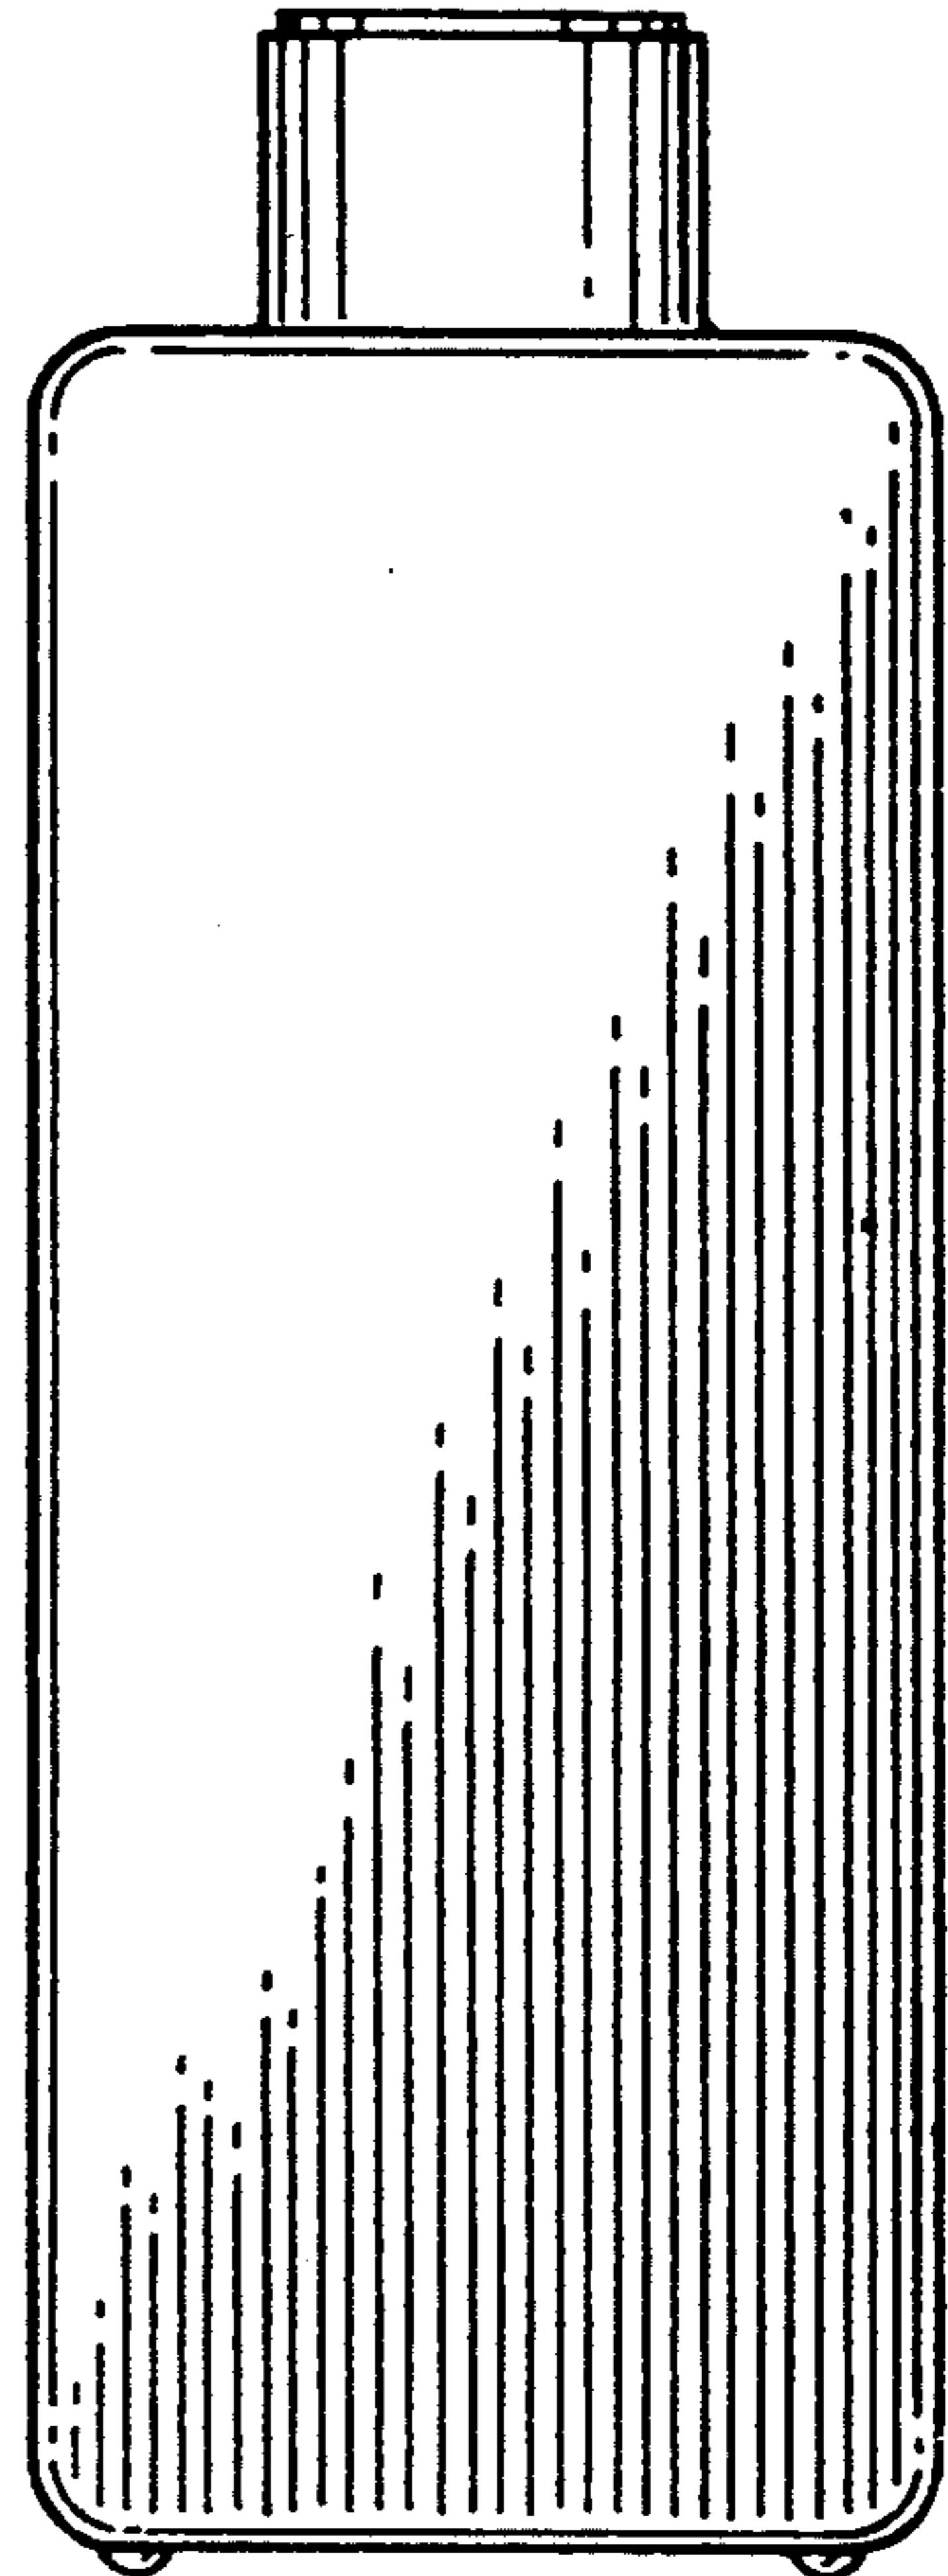

*Fig. 5*

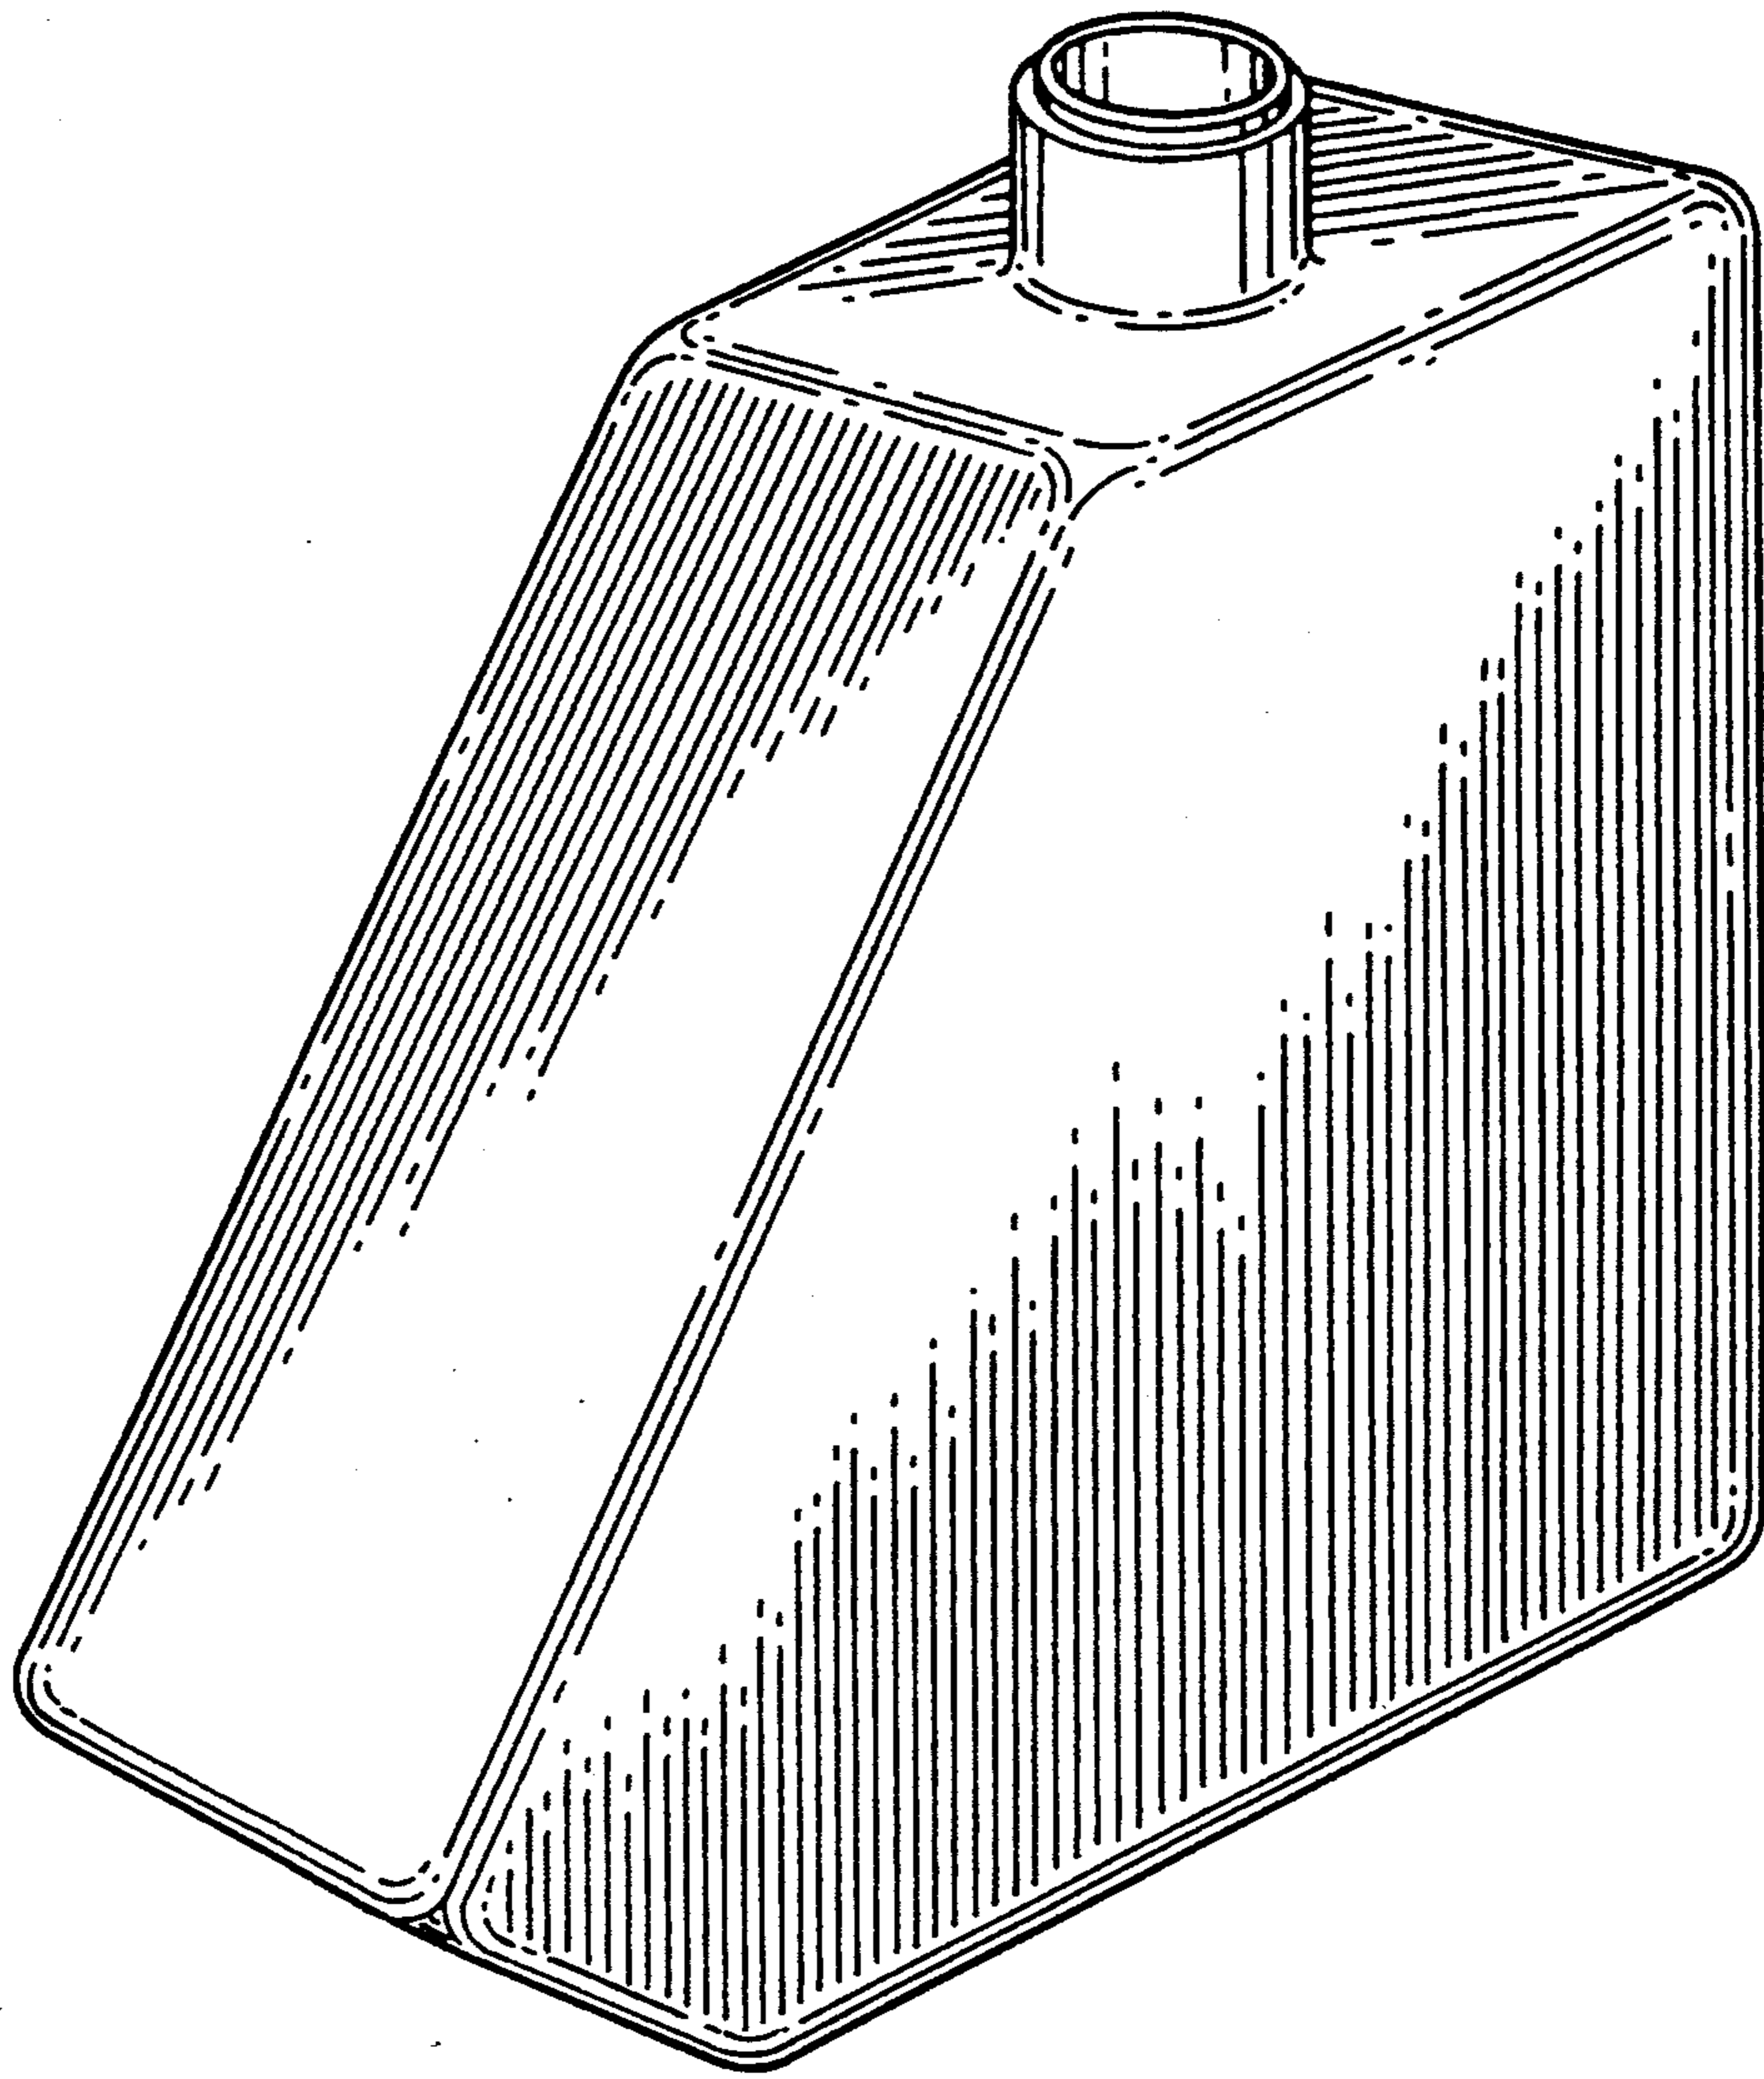

*Fig. 6*