



US00D352350S

United States Patent [19]

[11] Patent Number: **Des. 352,350**

Rambo et al.

[45] Date of Patent: **** Nov. 8, 1994**

[54] **APPARATUS FOR REMOVING SMOKE AND LIQUID FROM A SURGICAL SITE IN A HOSPITAL OPERATING ROOM**

[75] Inventors: **Robert D. Rambo**, Sellersville, Pa.;
John Yorke, Canastota, N.Y.

[73] Assignee: **Medical Development Systems, Inc.**,
Colmar, Pa.

[**] Term: **14 Years**

[21] Appl. No.: **8,460**

[22] Filed: **May 19, 1993**

[52] U.S. Cl. **D23/364; D34/25**

[58] Field of Search 422/120, 124; 55/356,
55/279, 472, 471; D23/364, 365, 366, 355;
D34/17, 19, 24, 25

[56] **References Cited**

U.S. PATENT DOCUMENTS

D. 143,088	12/1945	Maultsby, Jr.	D34/25
D. 325,252	4/1992	Morris et al.	D23/364
4,737,173	4/1988	Kudirka et al.	55/471
5,230,723	7/1993	Travis et al.	55/472
5,240,478	8/1993	Messina	55/279

OTHER PUBLICATIONS

AirSafe Smoke Filtration System ES-2000, copyright 1992, Stackhouse Incorporated, pertinent pages: cover page and p. 16.

Primary Examiner—Lisa P. Lichtenstein
Attorney, Agent, or Firm—Charles S. McGuire

[57] **CLAIM**

The ornamental design for an apparatus for removing smoke and liquid from a surgical site in a hospital operating room, as shown and described.

DESCRIPTION

FIG. 1 is a perspective view of an apparatus for removing smoke and liquid from a surgical site, showing our new design;

FIG. 2 is a front elevational view thereof;


FIG. 3 is a side elevational view thereof, the opposite side being a mirror image of that shown;

FIG. 4 is a rear elevational view thereof;

FIG. 5 is a top plan view thereof; and,

FIG. 6 is a bottom plan view thereof.

The cross-hatching in FIGS. 1, 4, 5 and 6 represents screening and is understood to extend through out the areas represented.

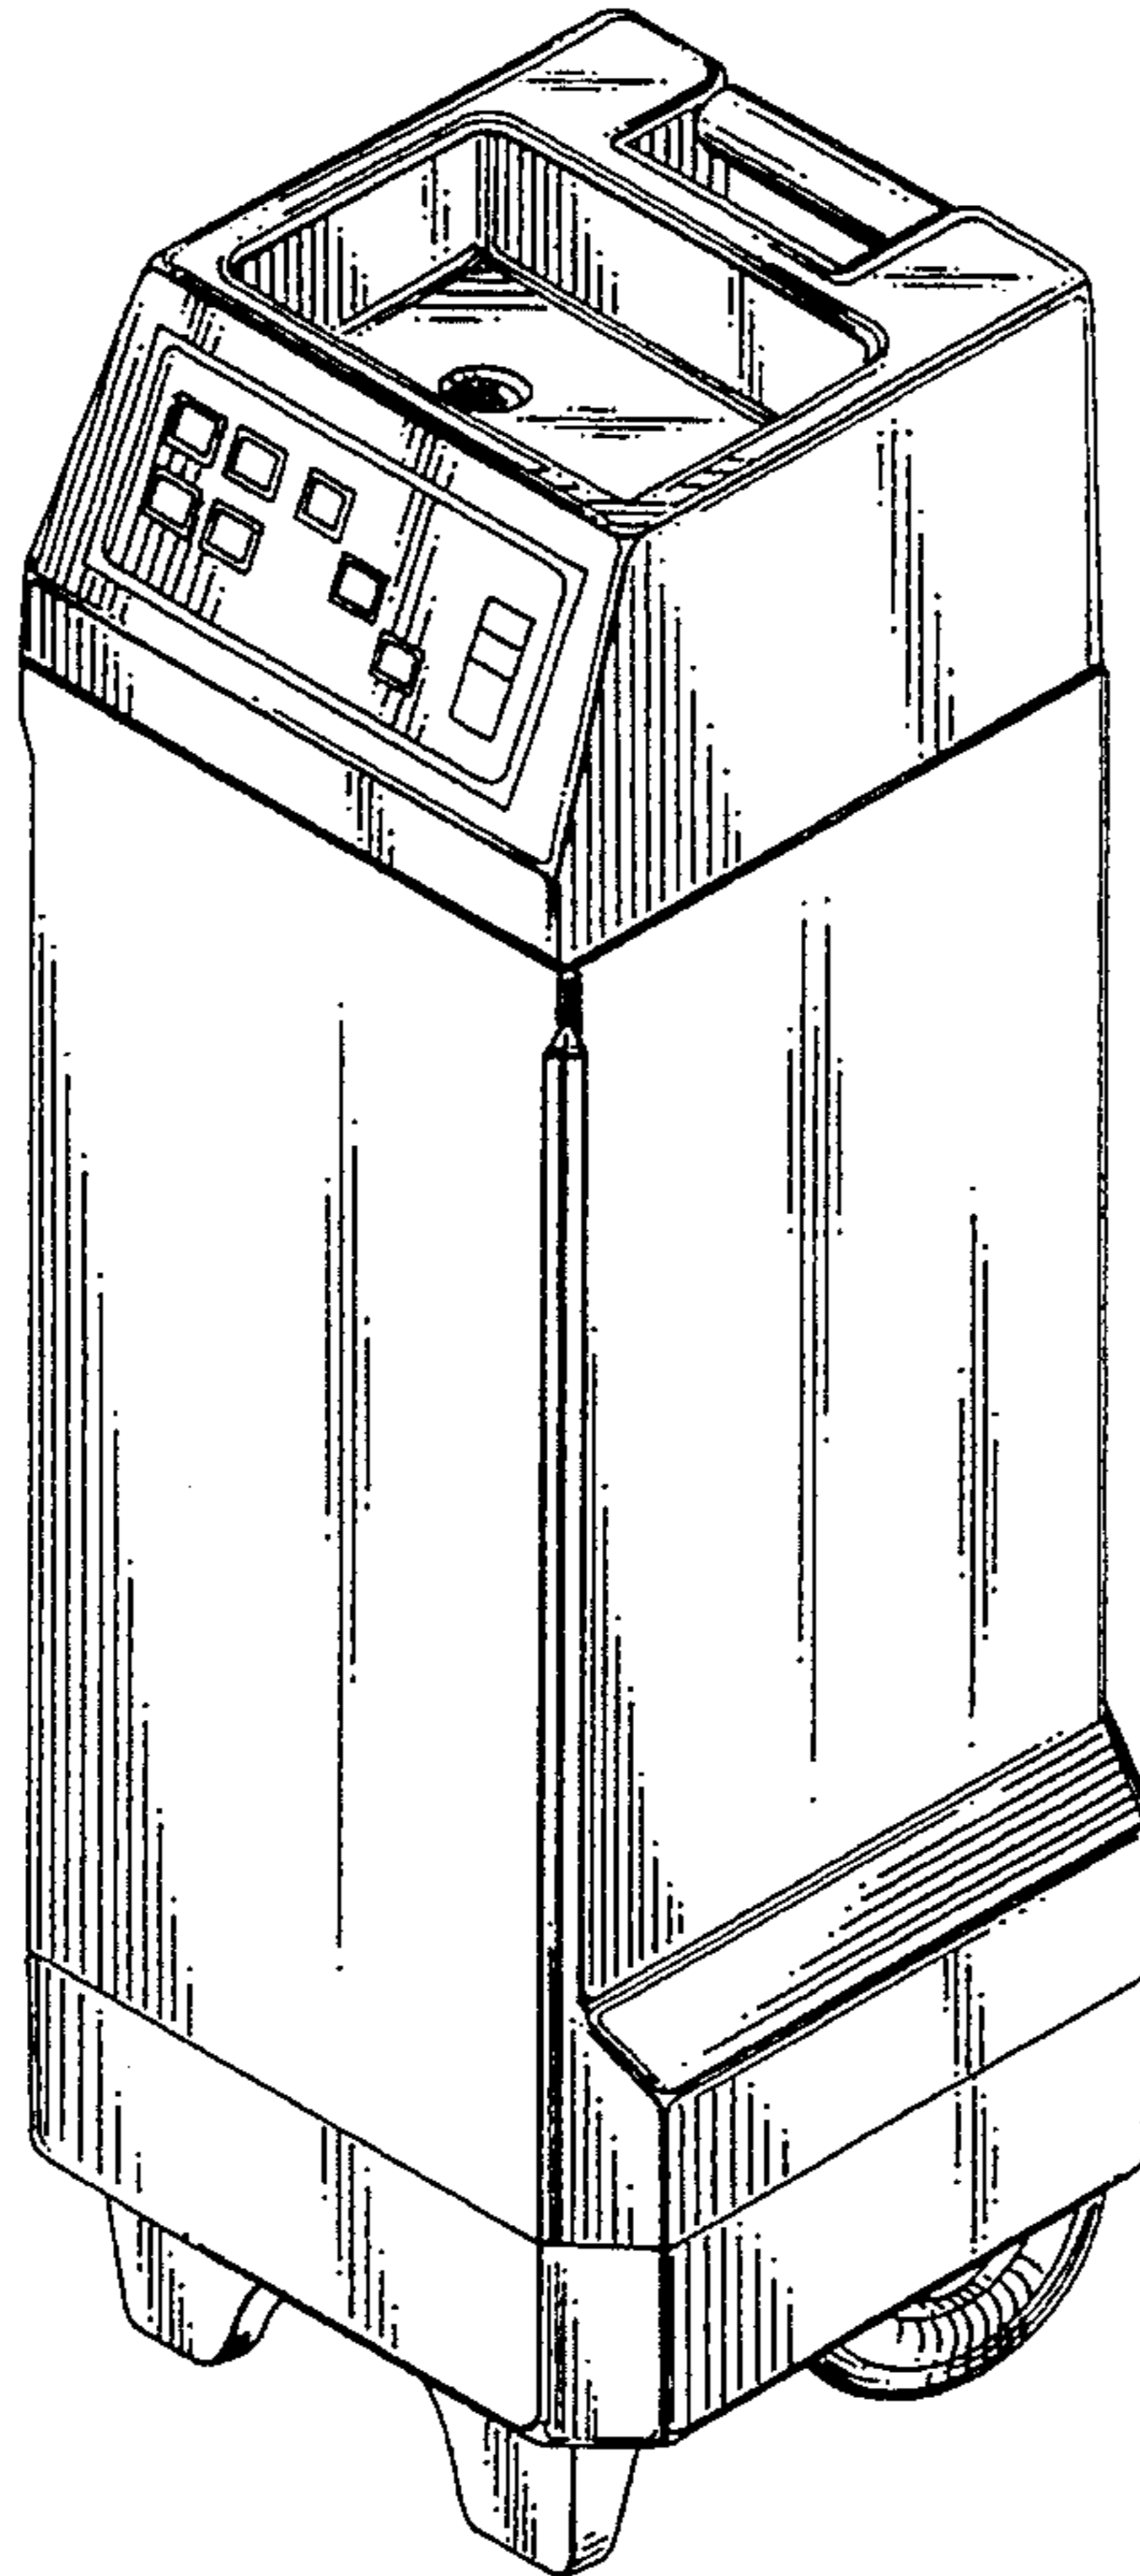

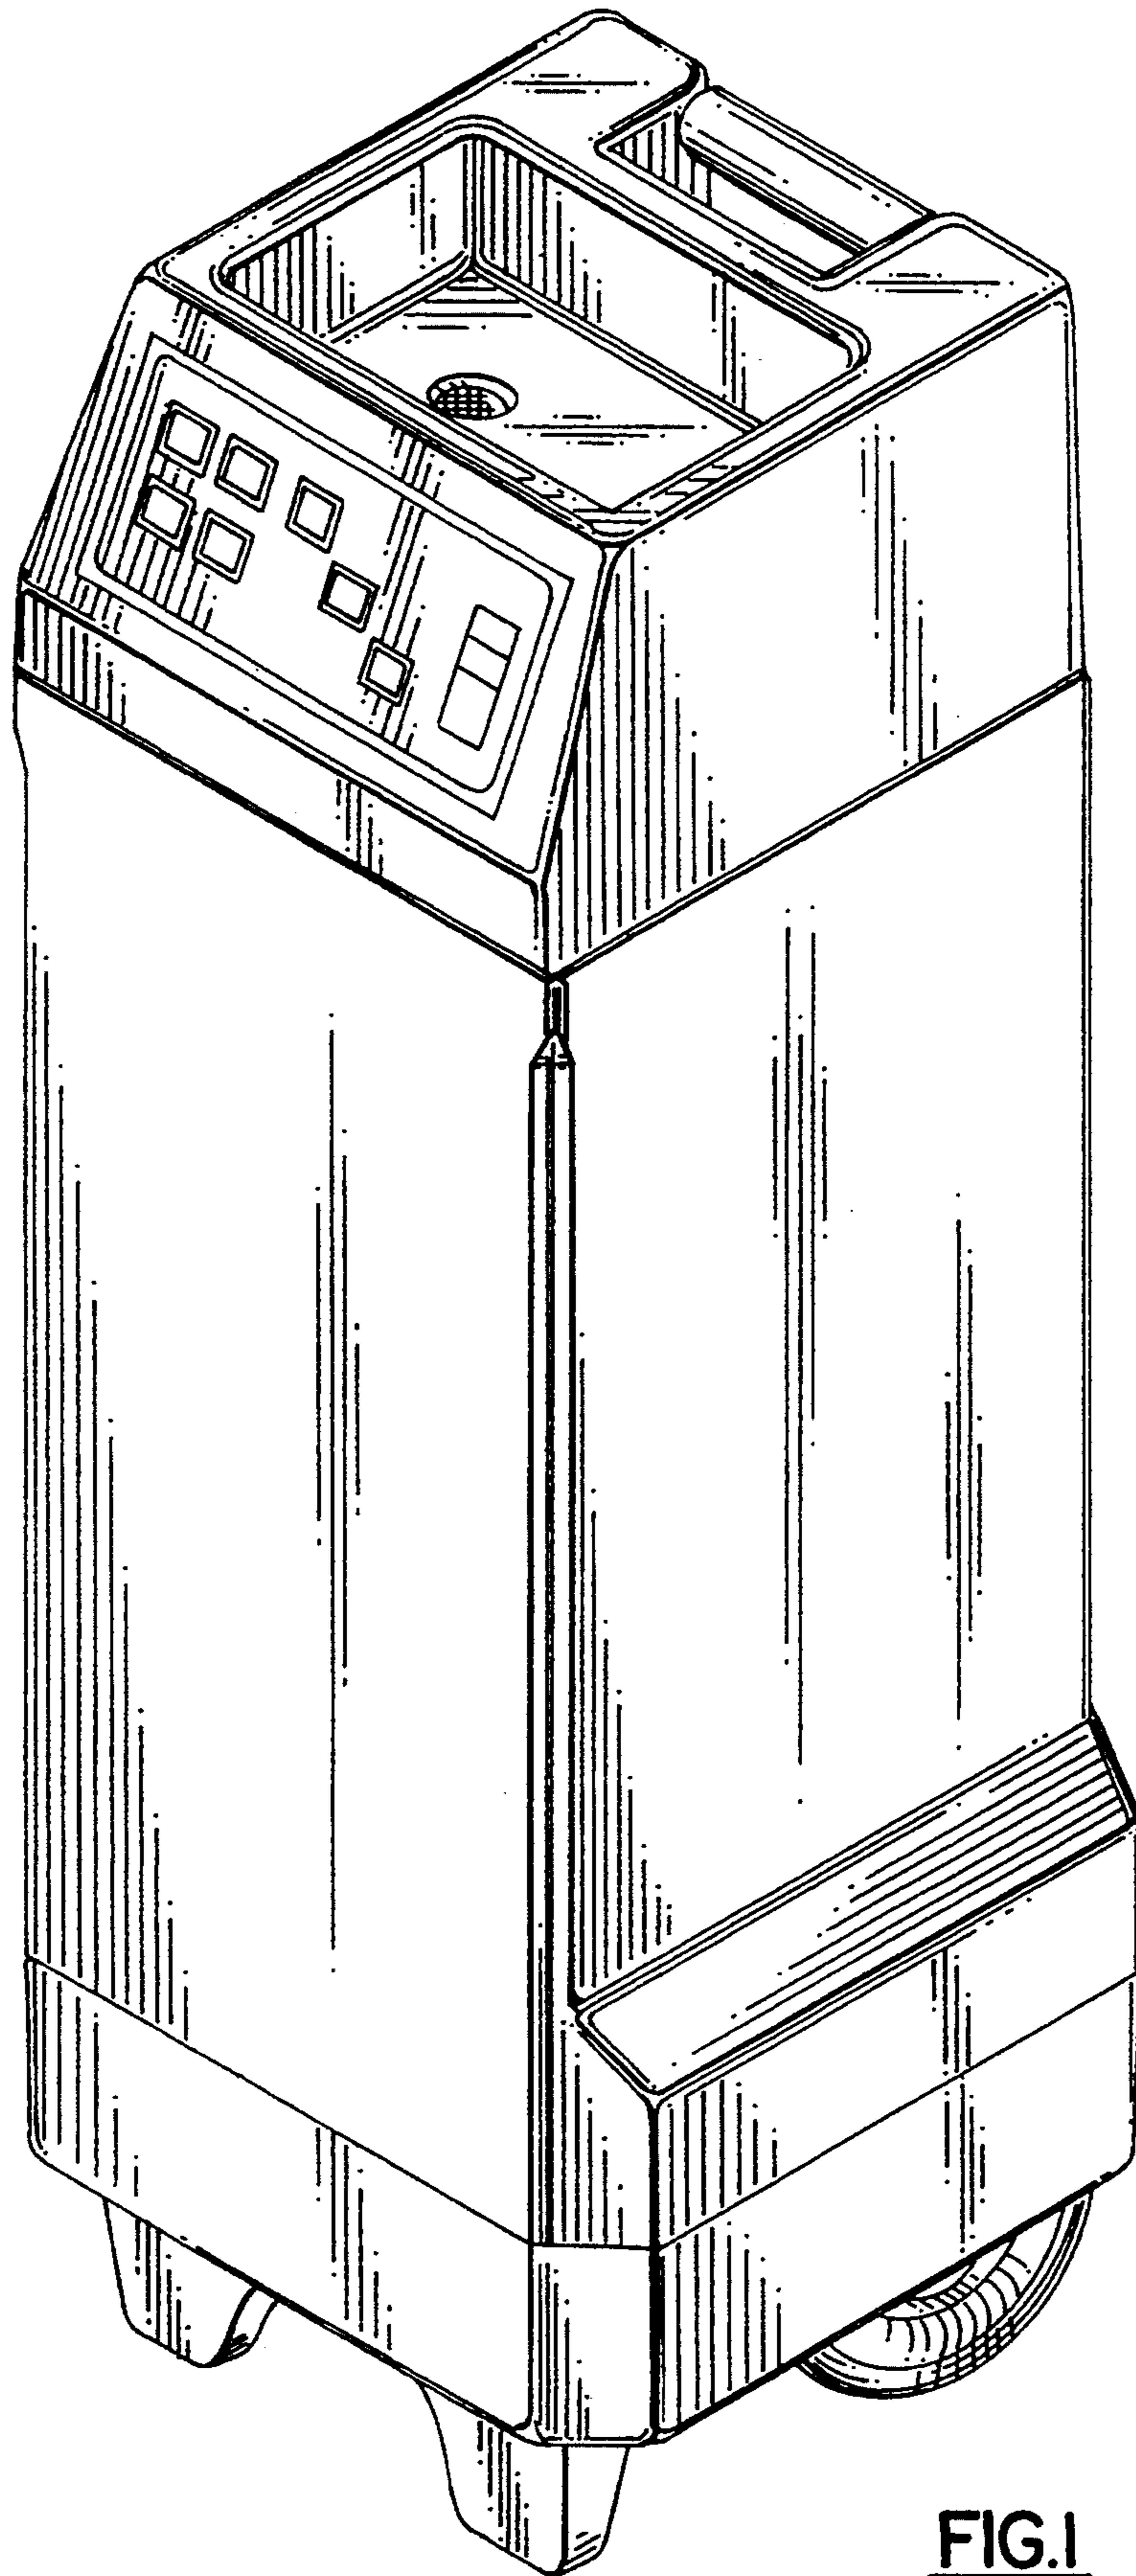


FIG.1

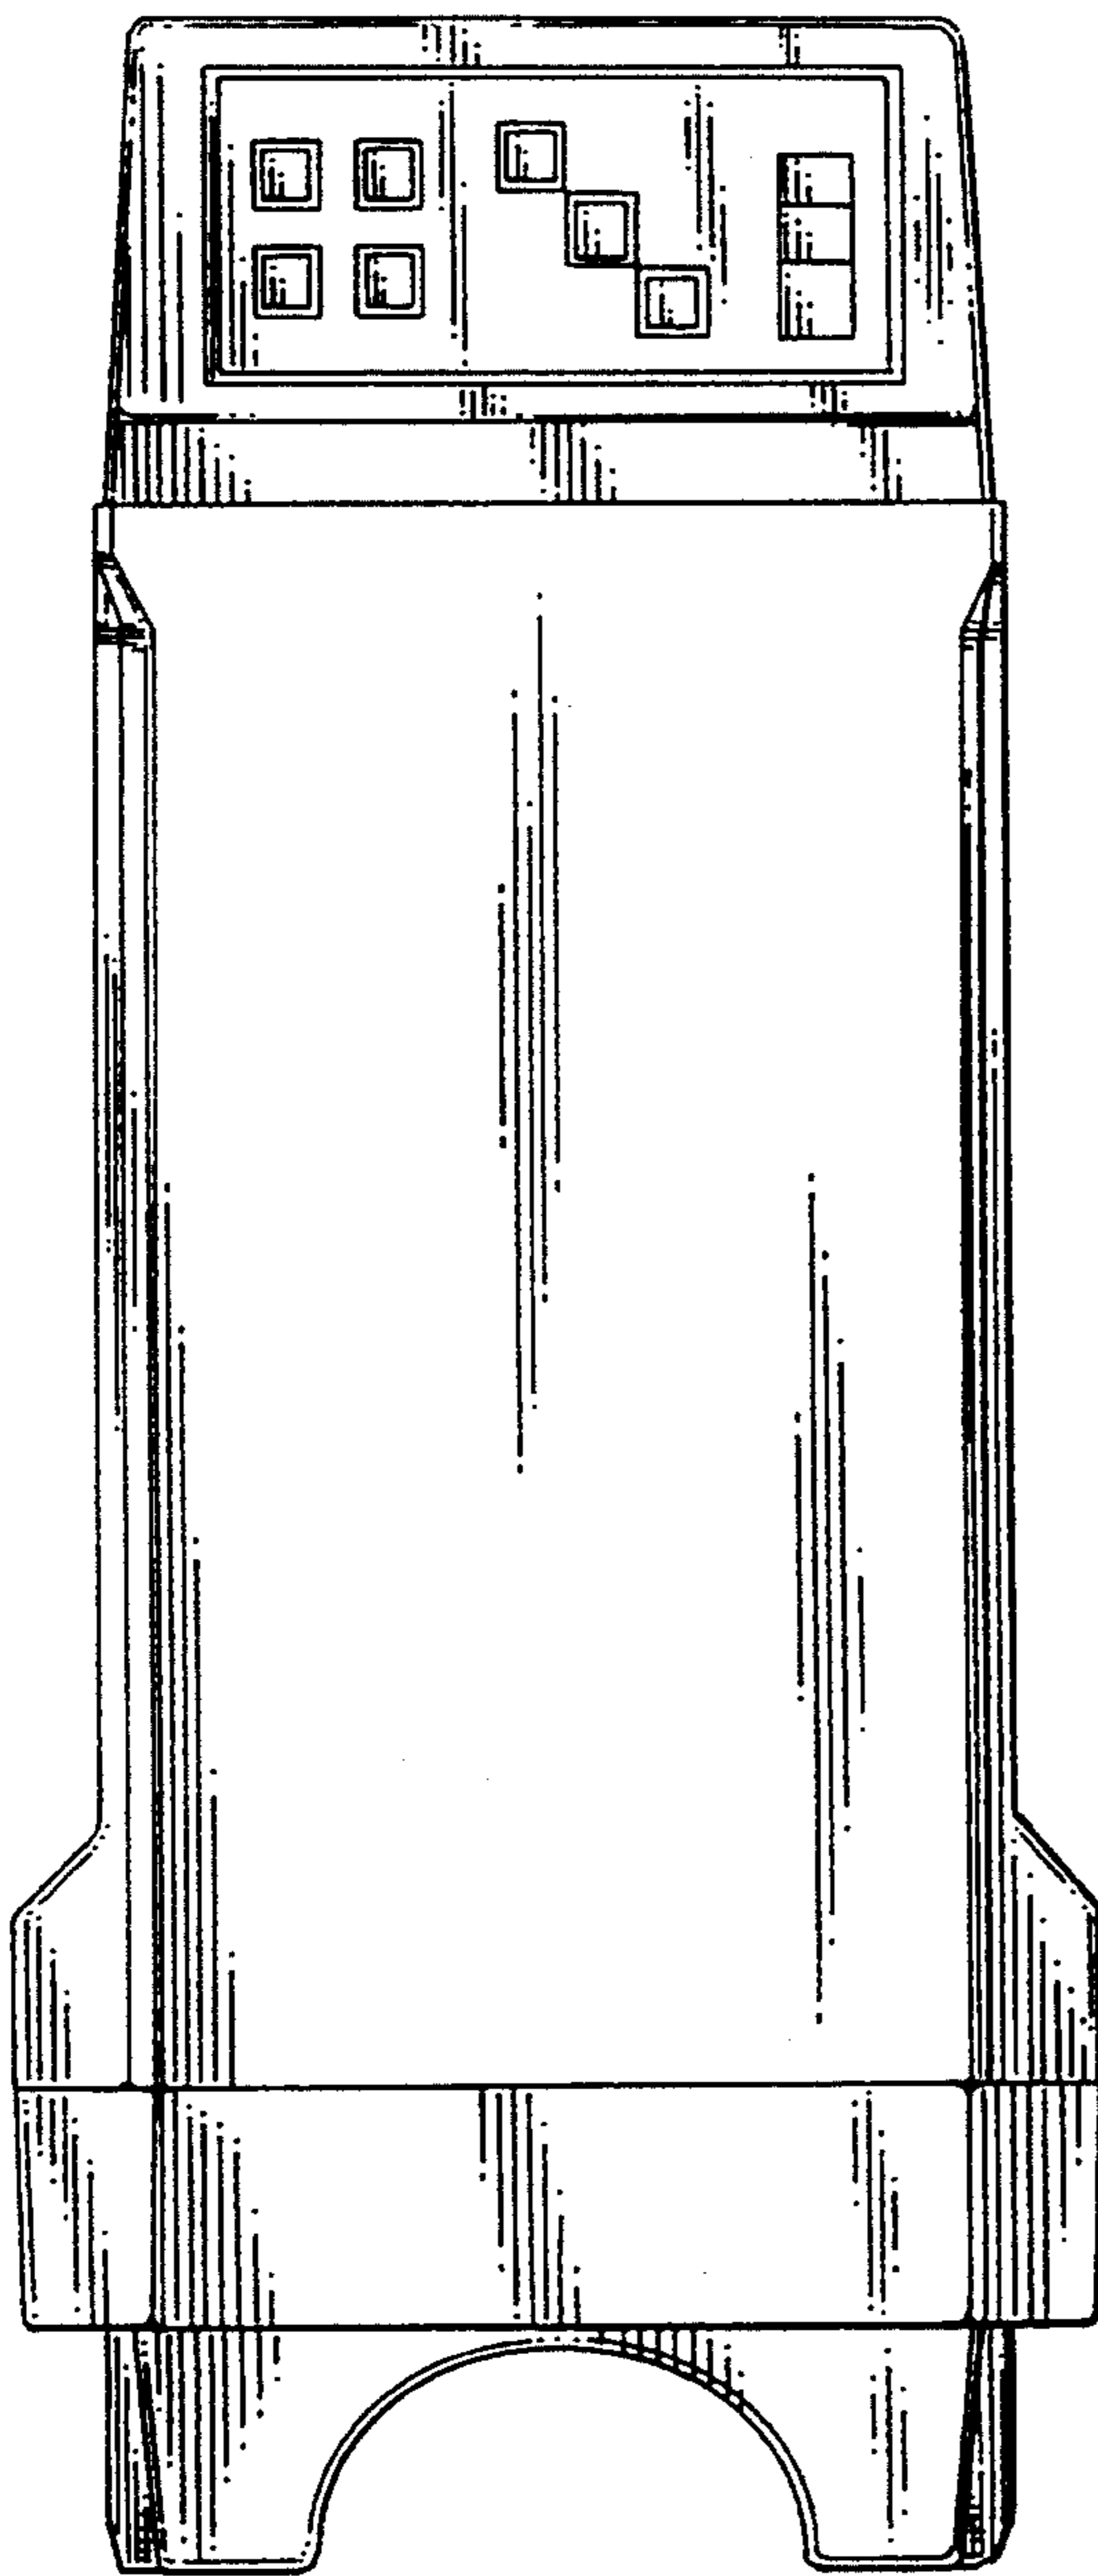


FIG. 2

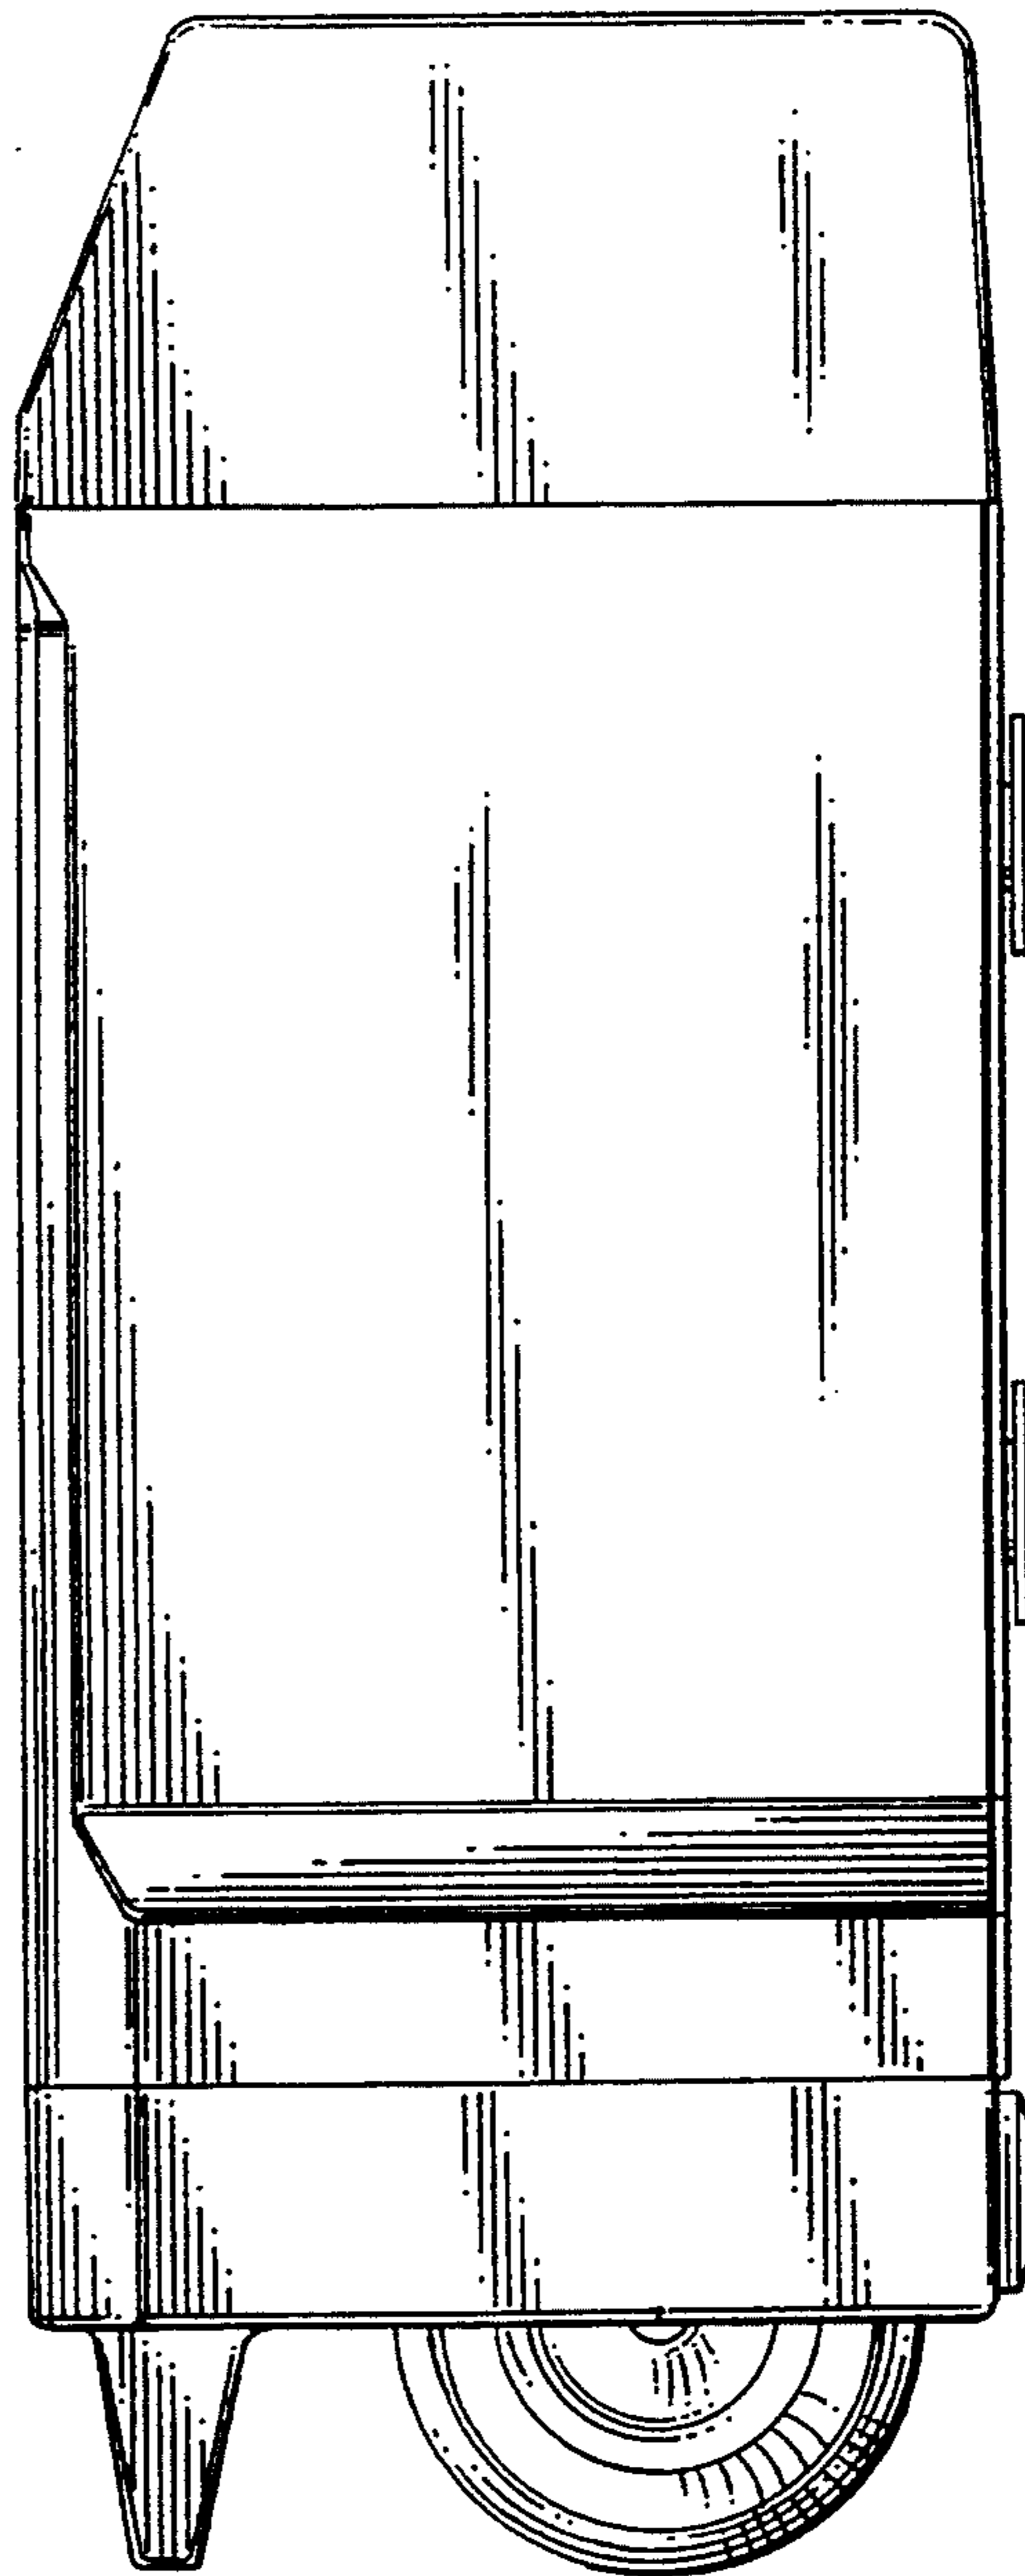


FIG. 3

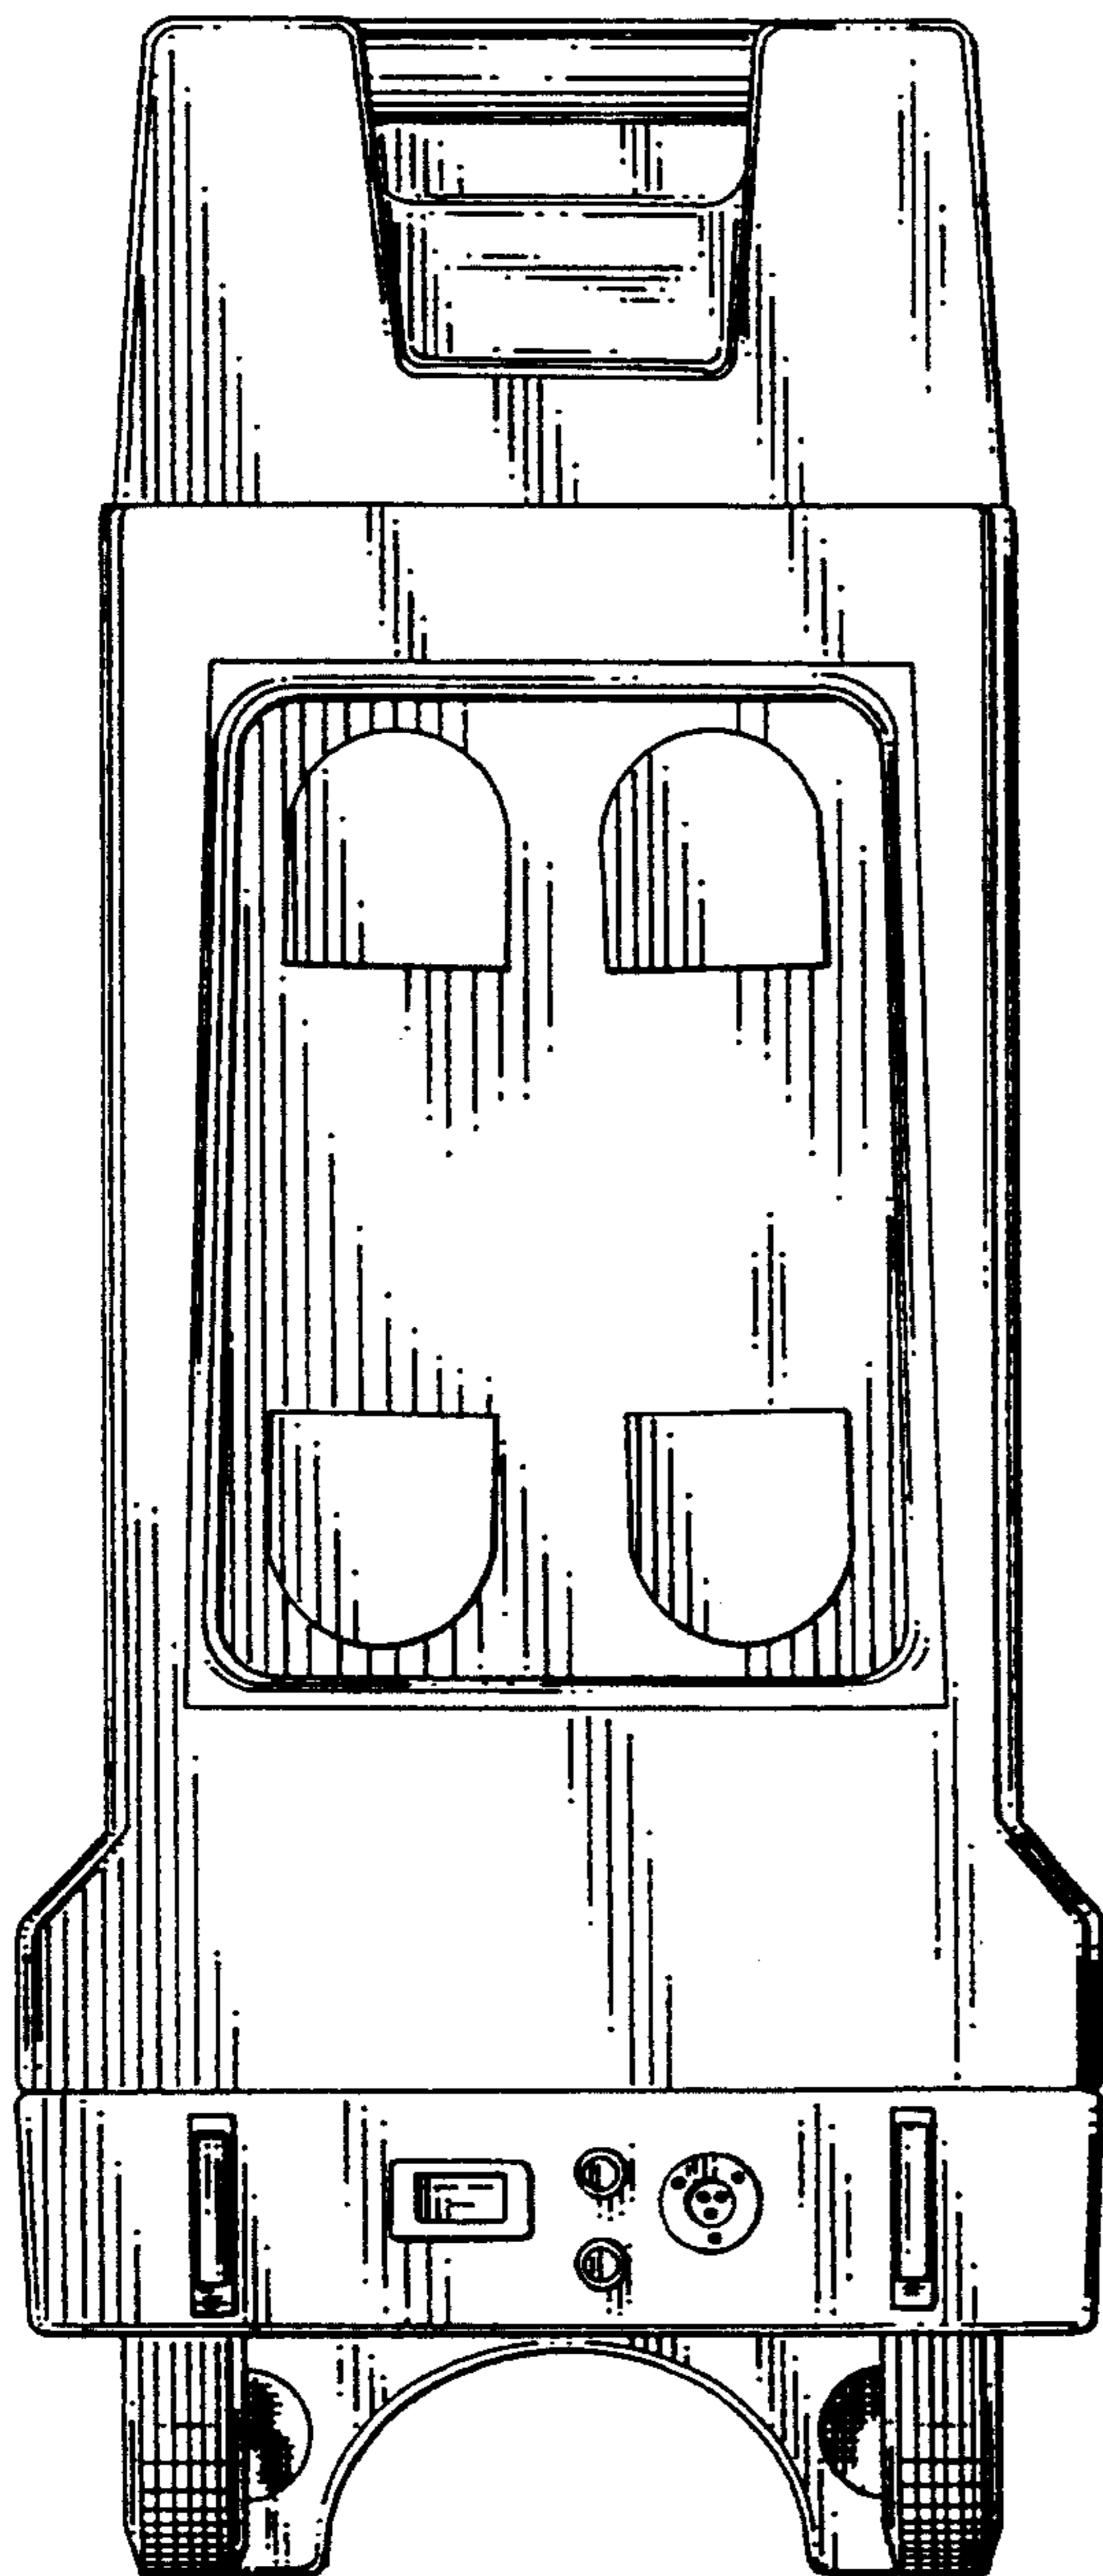


FIG.4

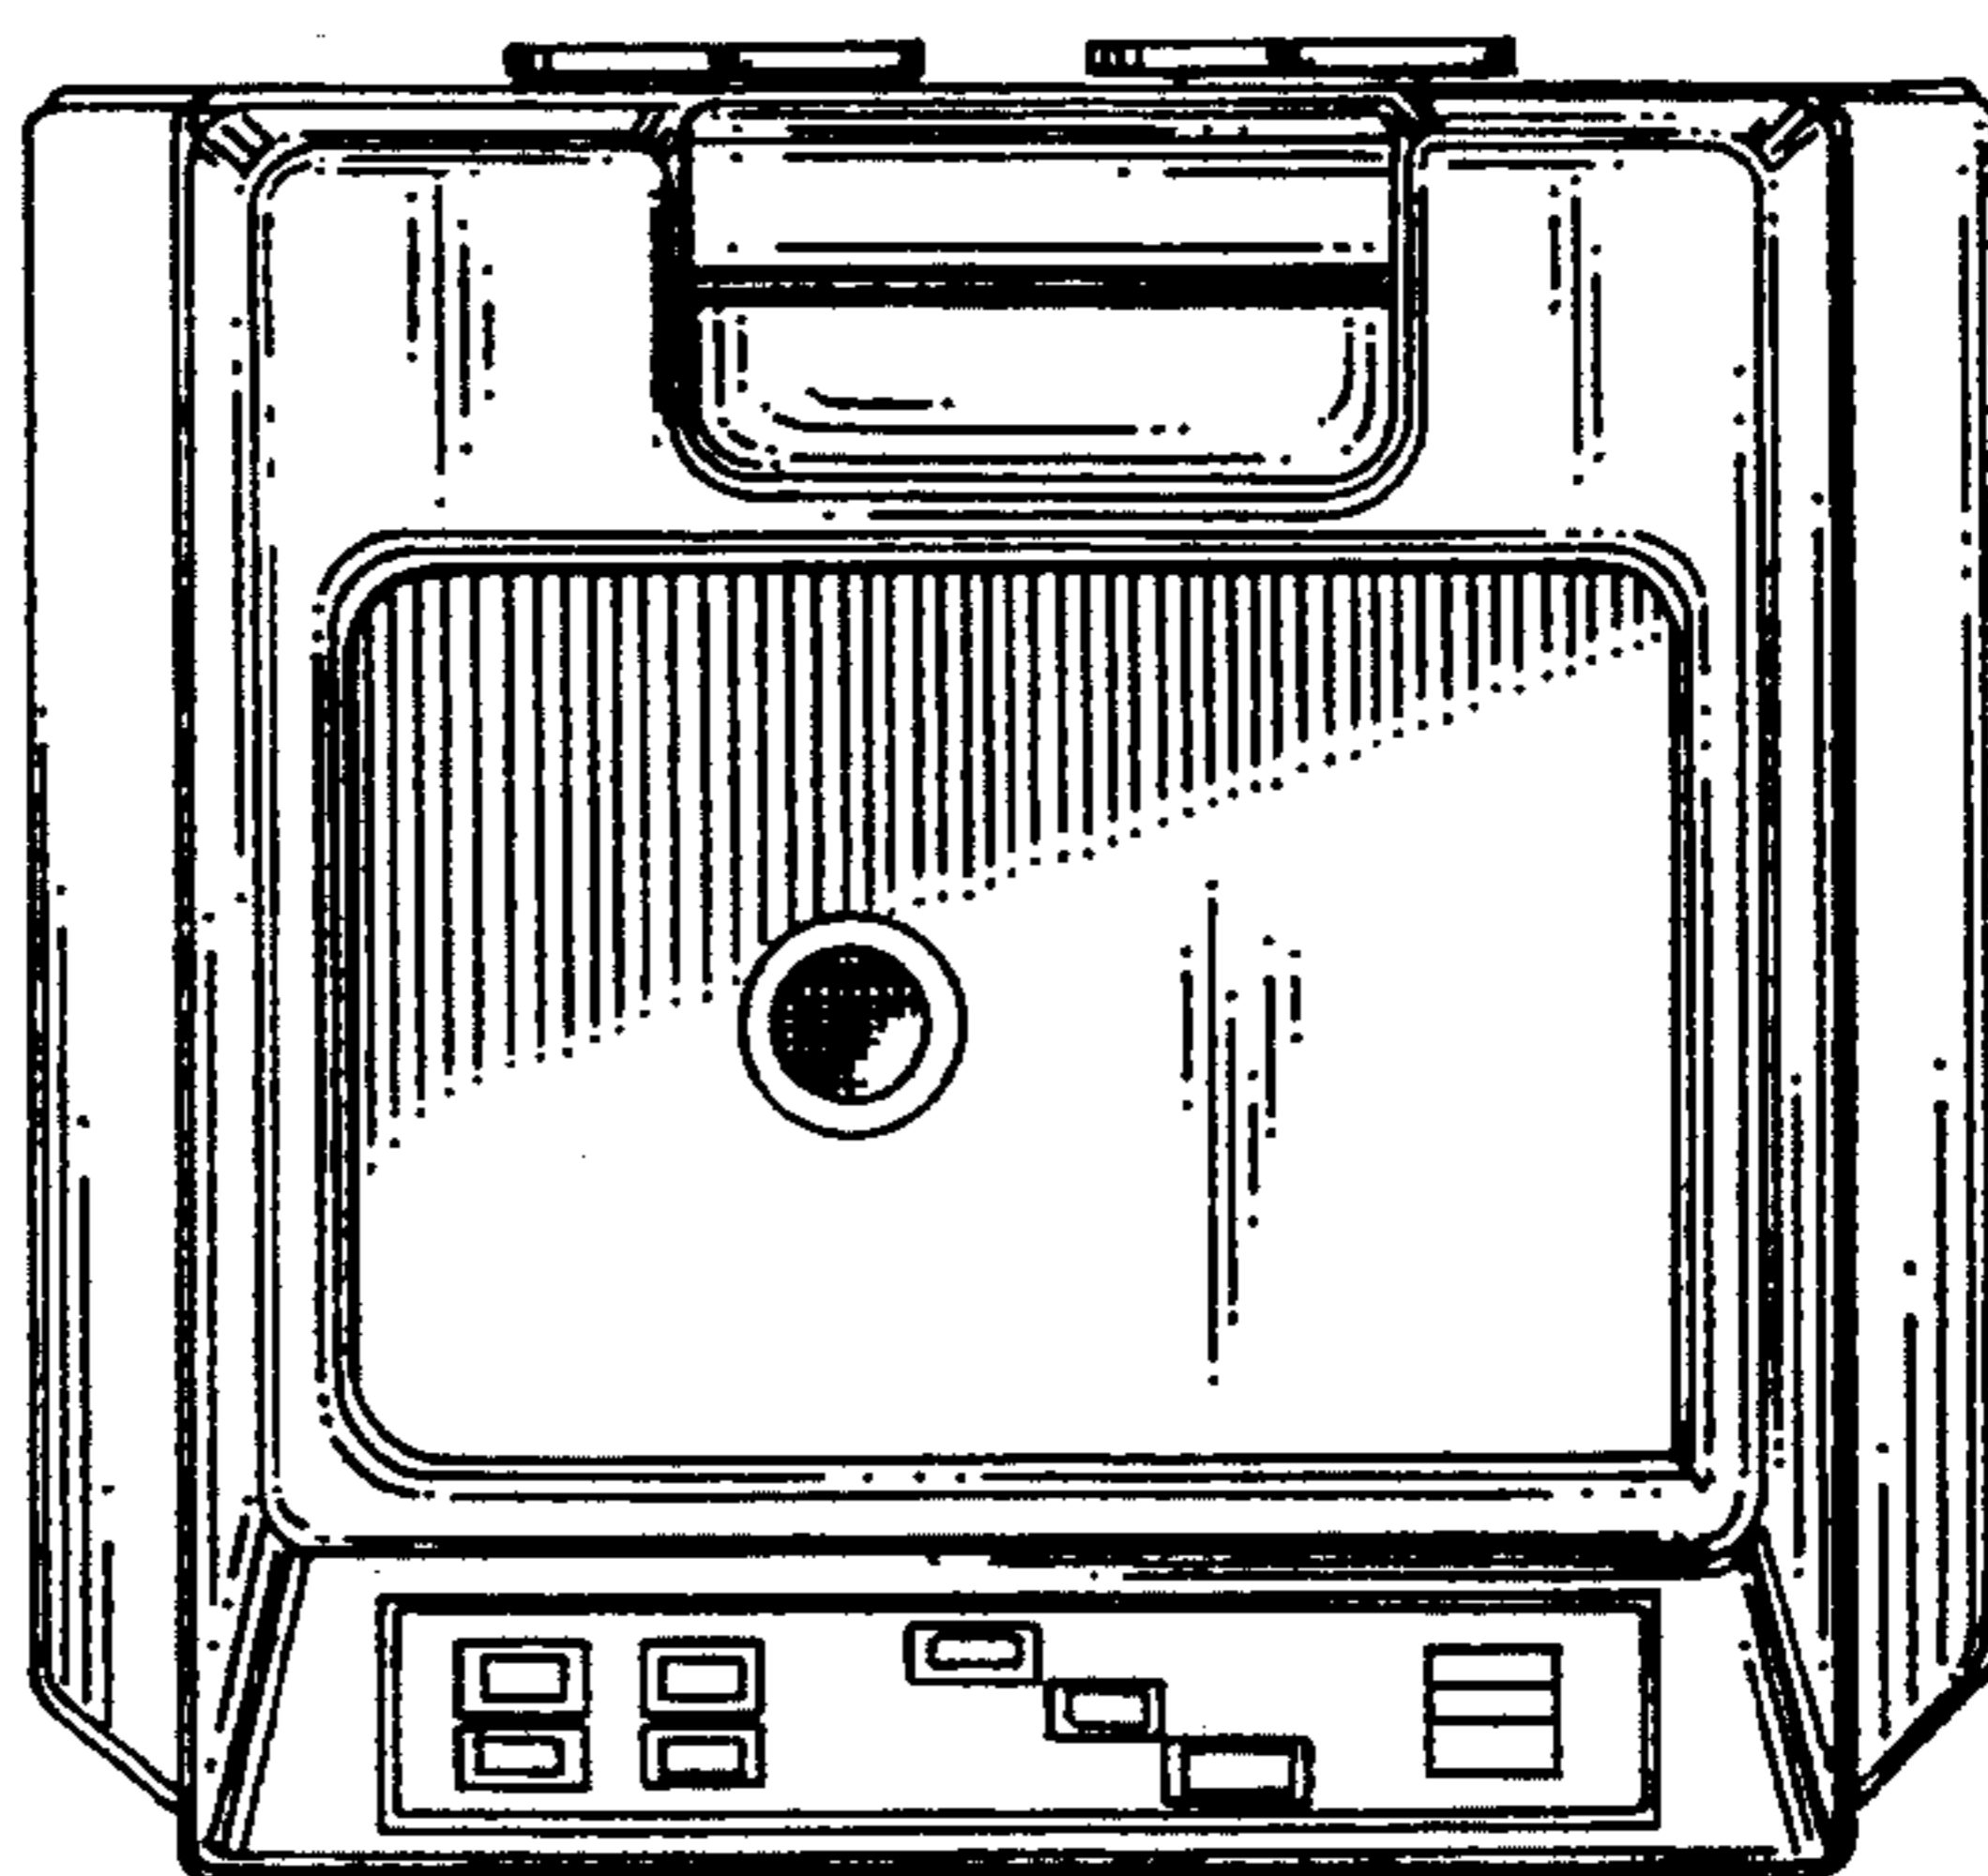


FIG.5

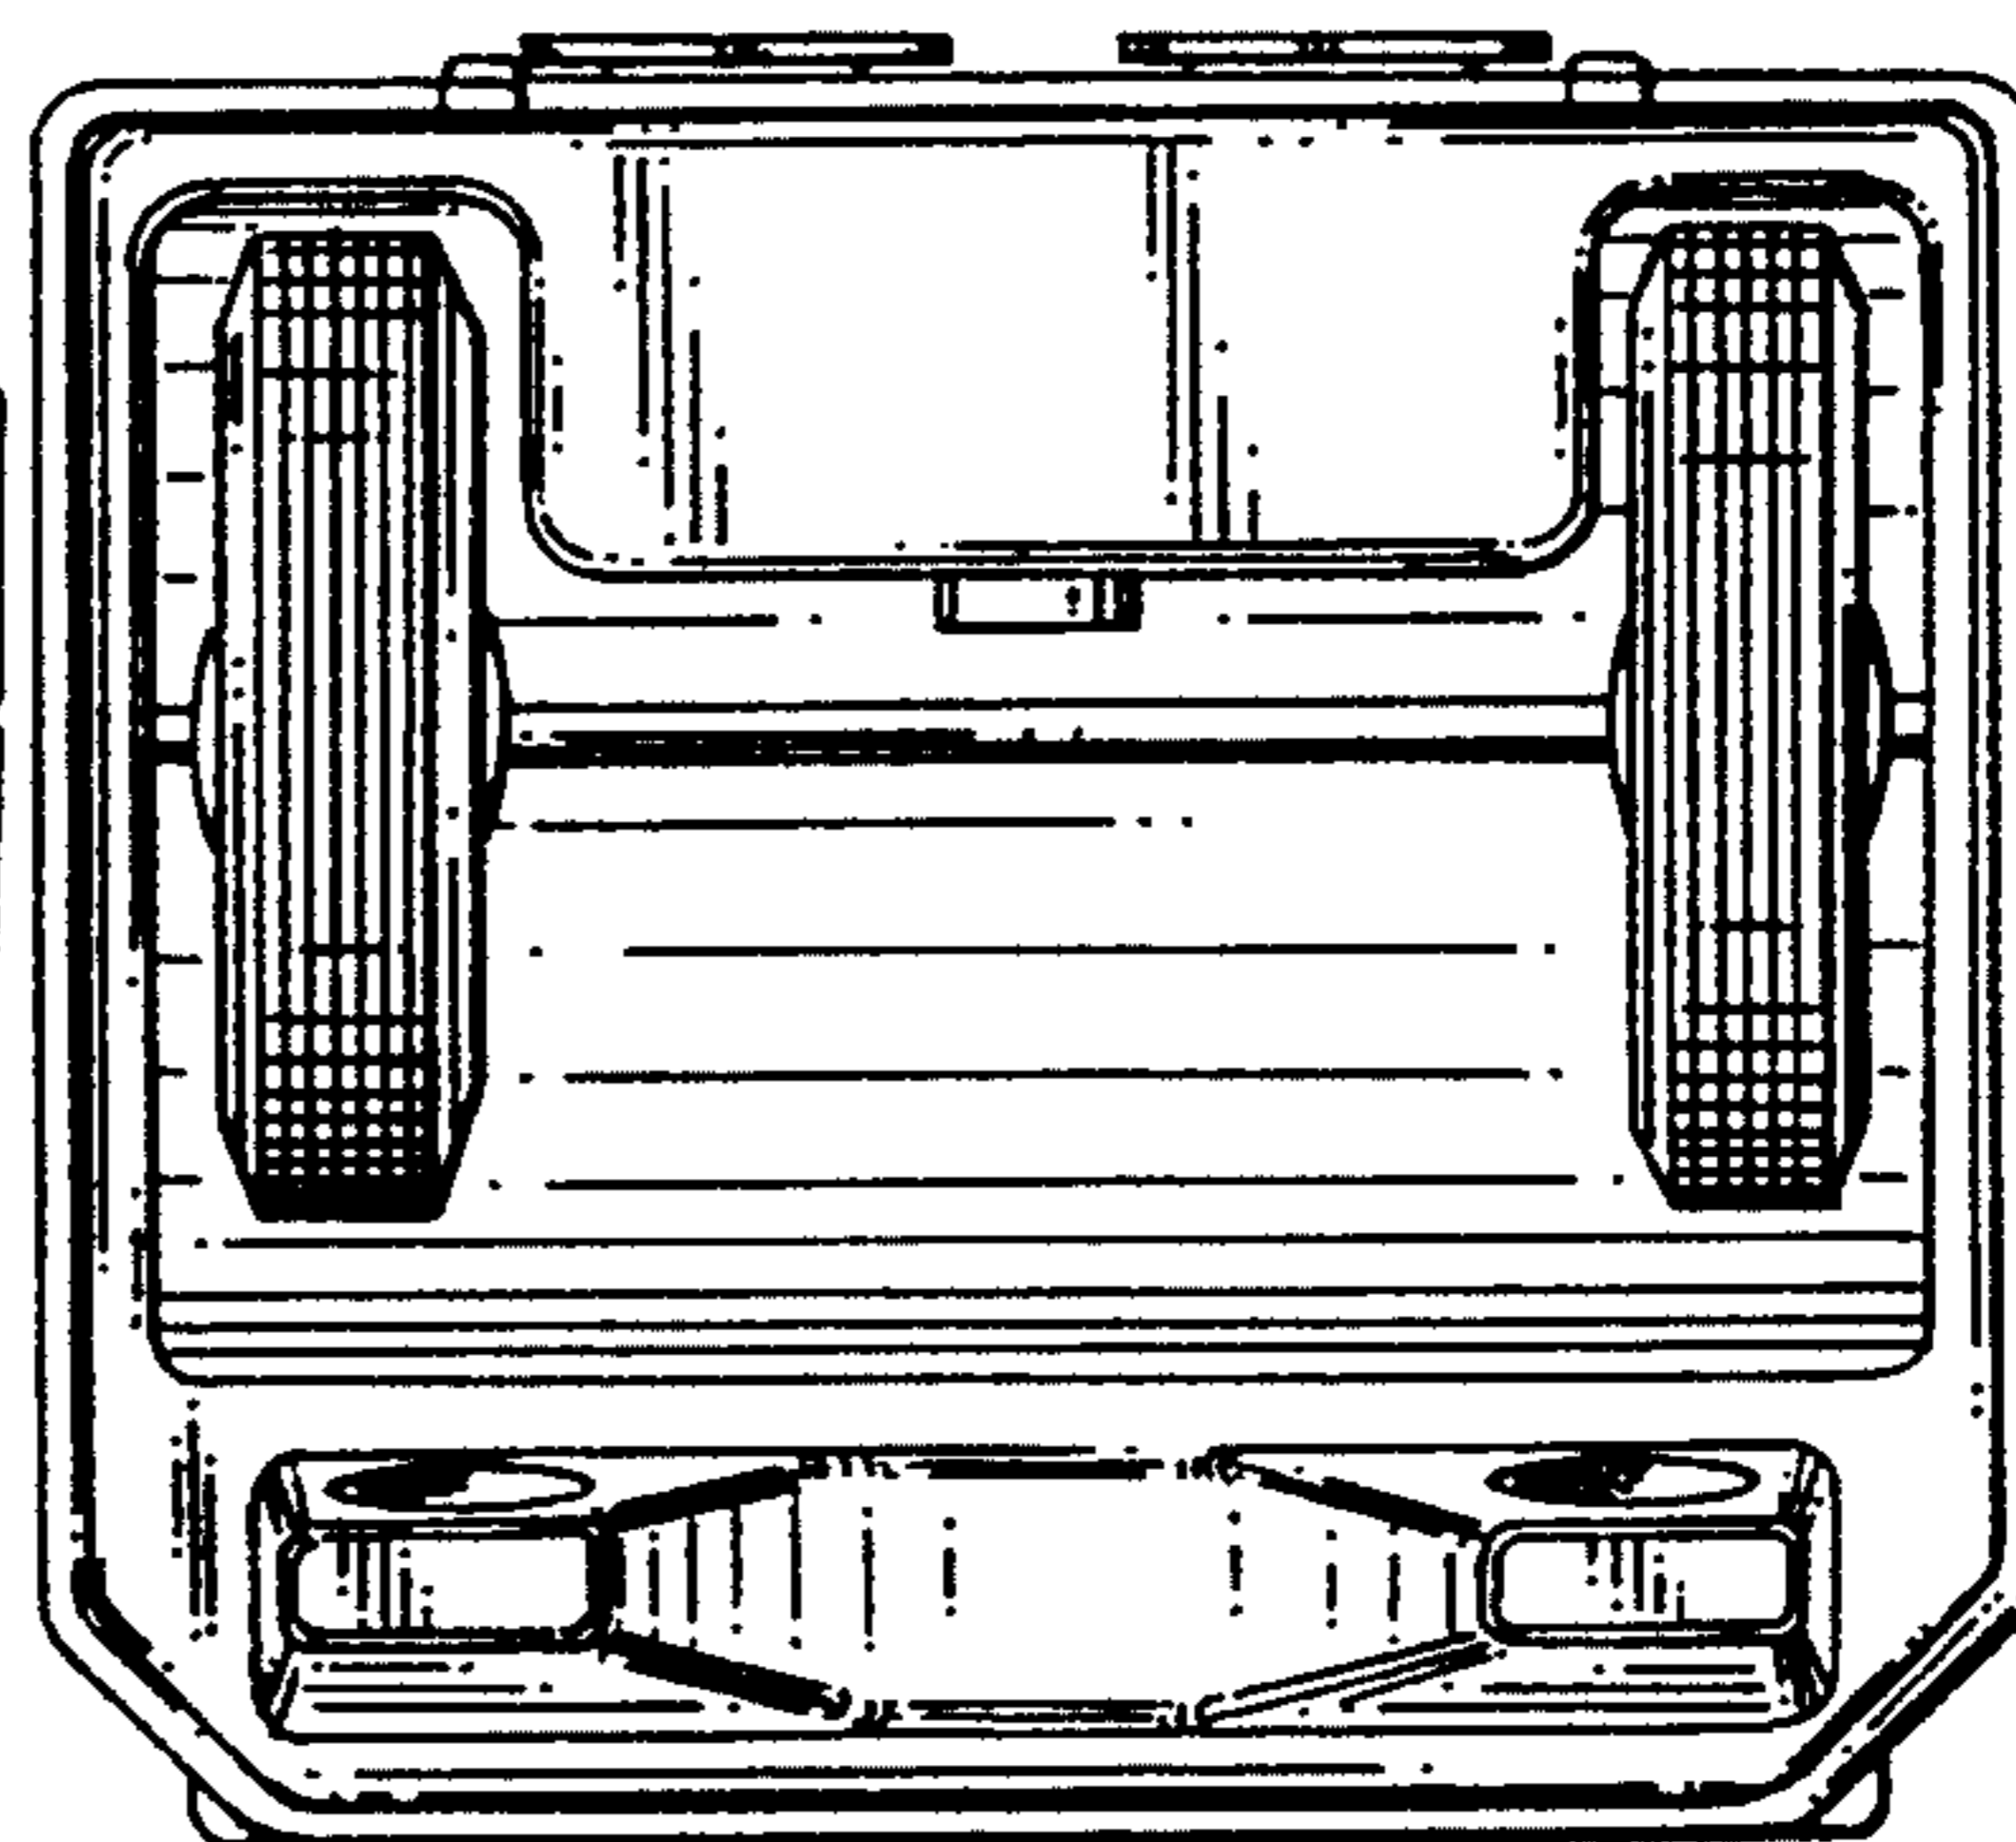


FIG.6