



US00D355717S

# United States Patent [19]

Murakami et al.

[11] Patent Number: Des. 355,717

[45] Date of Patent: \*\* Feb. 21, 1995

[54] **COMBINED X-RAY CONTROL BOARD AND SUPPORT STRUCTURE FOR MEDICAL TREATMENT**

[75] Inventors: **Makoto Murakami; Takahisa Yoneyama**, both of Yokohama, Japan

[73] Assignee: **Kabushiki Kaisha Toshiba**, Kawasaki, Japan

[\*\*] Term: **14 Years**

[21] Appl. No.: **11,237**

[22] Filed: **Jul. 30, 1993**

[30] **Foreign Application Priority Data**

Apr. 1, 1993 [JP] Japan ..... 5-9361

[52] U.S. Cl. .... **D24/158; D14/103; D14/104**

[58] **Field of Search** ..... **D24/158; 378/208, 204, 378/193, 195, 162, 117, 116, 115, 114, 19; 128/653.2; 382/6.4, 54, 51, 48; 250/322; D14/103, 104**

[56] **References Cited**

**U.S. PATENT DOCUMENTS**

- 4,160,906 7/1979 Daniels et al. .... 250/322.1
- 4,773,086 9/1988 Fujita et al. .... 378/4
- 4,969,167 11/1990 Zupancic et al. .... 378/19

- 4,991,193 2/1991 Cecil et al. .... 378/117
- 5,272,760 12/1993 Echerer et al. .... 382/6

**FOREIGN PATENT DOCUMENTS**

120451 11/1991 Rep. of Korea .

**OTHER PUBLICATIONS**

Siemens Catalog of Angiotron, "Control Desk".  
Siemens Catalog of Cut Film Changer.  
Siemens Catalog, published Apr. 1991.

*Primary Examiner*—Stella Reid  
*Attorney, Agent, or Firm*—Oblon, Spivak, McClelland, Maier, & Neustadt

[57] **CLAIM**

The ornamental design for a combined x-ray control board and support structure for medical treatment, as shown.

**DESCRIPTION**

FIG. 1 is a front, top and right side perspective view of a combined x-ray control board and support structure for medical treatment, showing our new design; FIG. 2 is a reduced front elevational view thereof; FIG. 3 is a right side elevational view thereof; FIG. 4 is a top plan view thereof; FIG. 5 is a rear elevational view thereof; FIG. 6 is a left side elevational view thereof; and, FIG. 7 is a bottom plan view thereof.

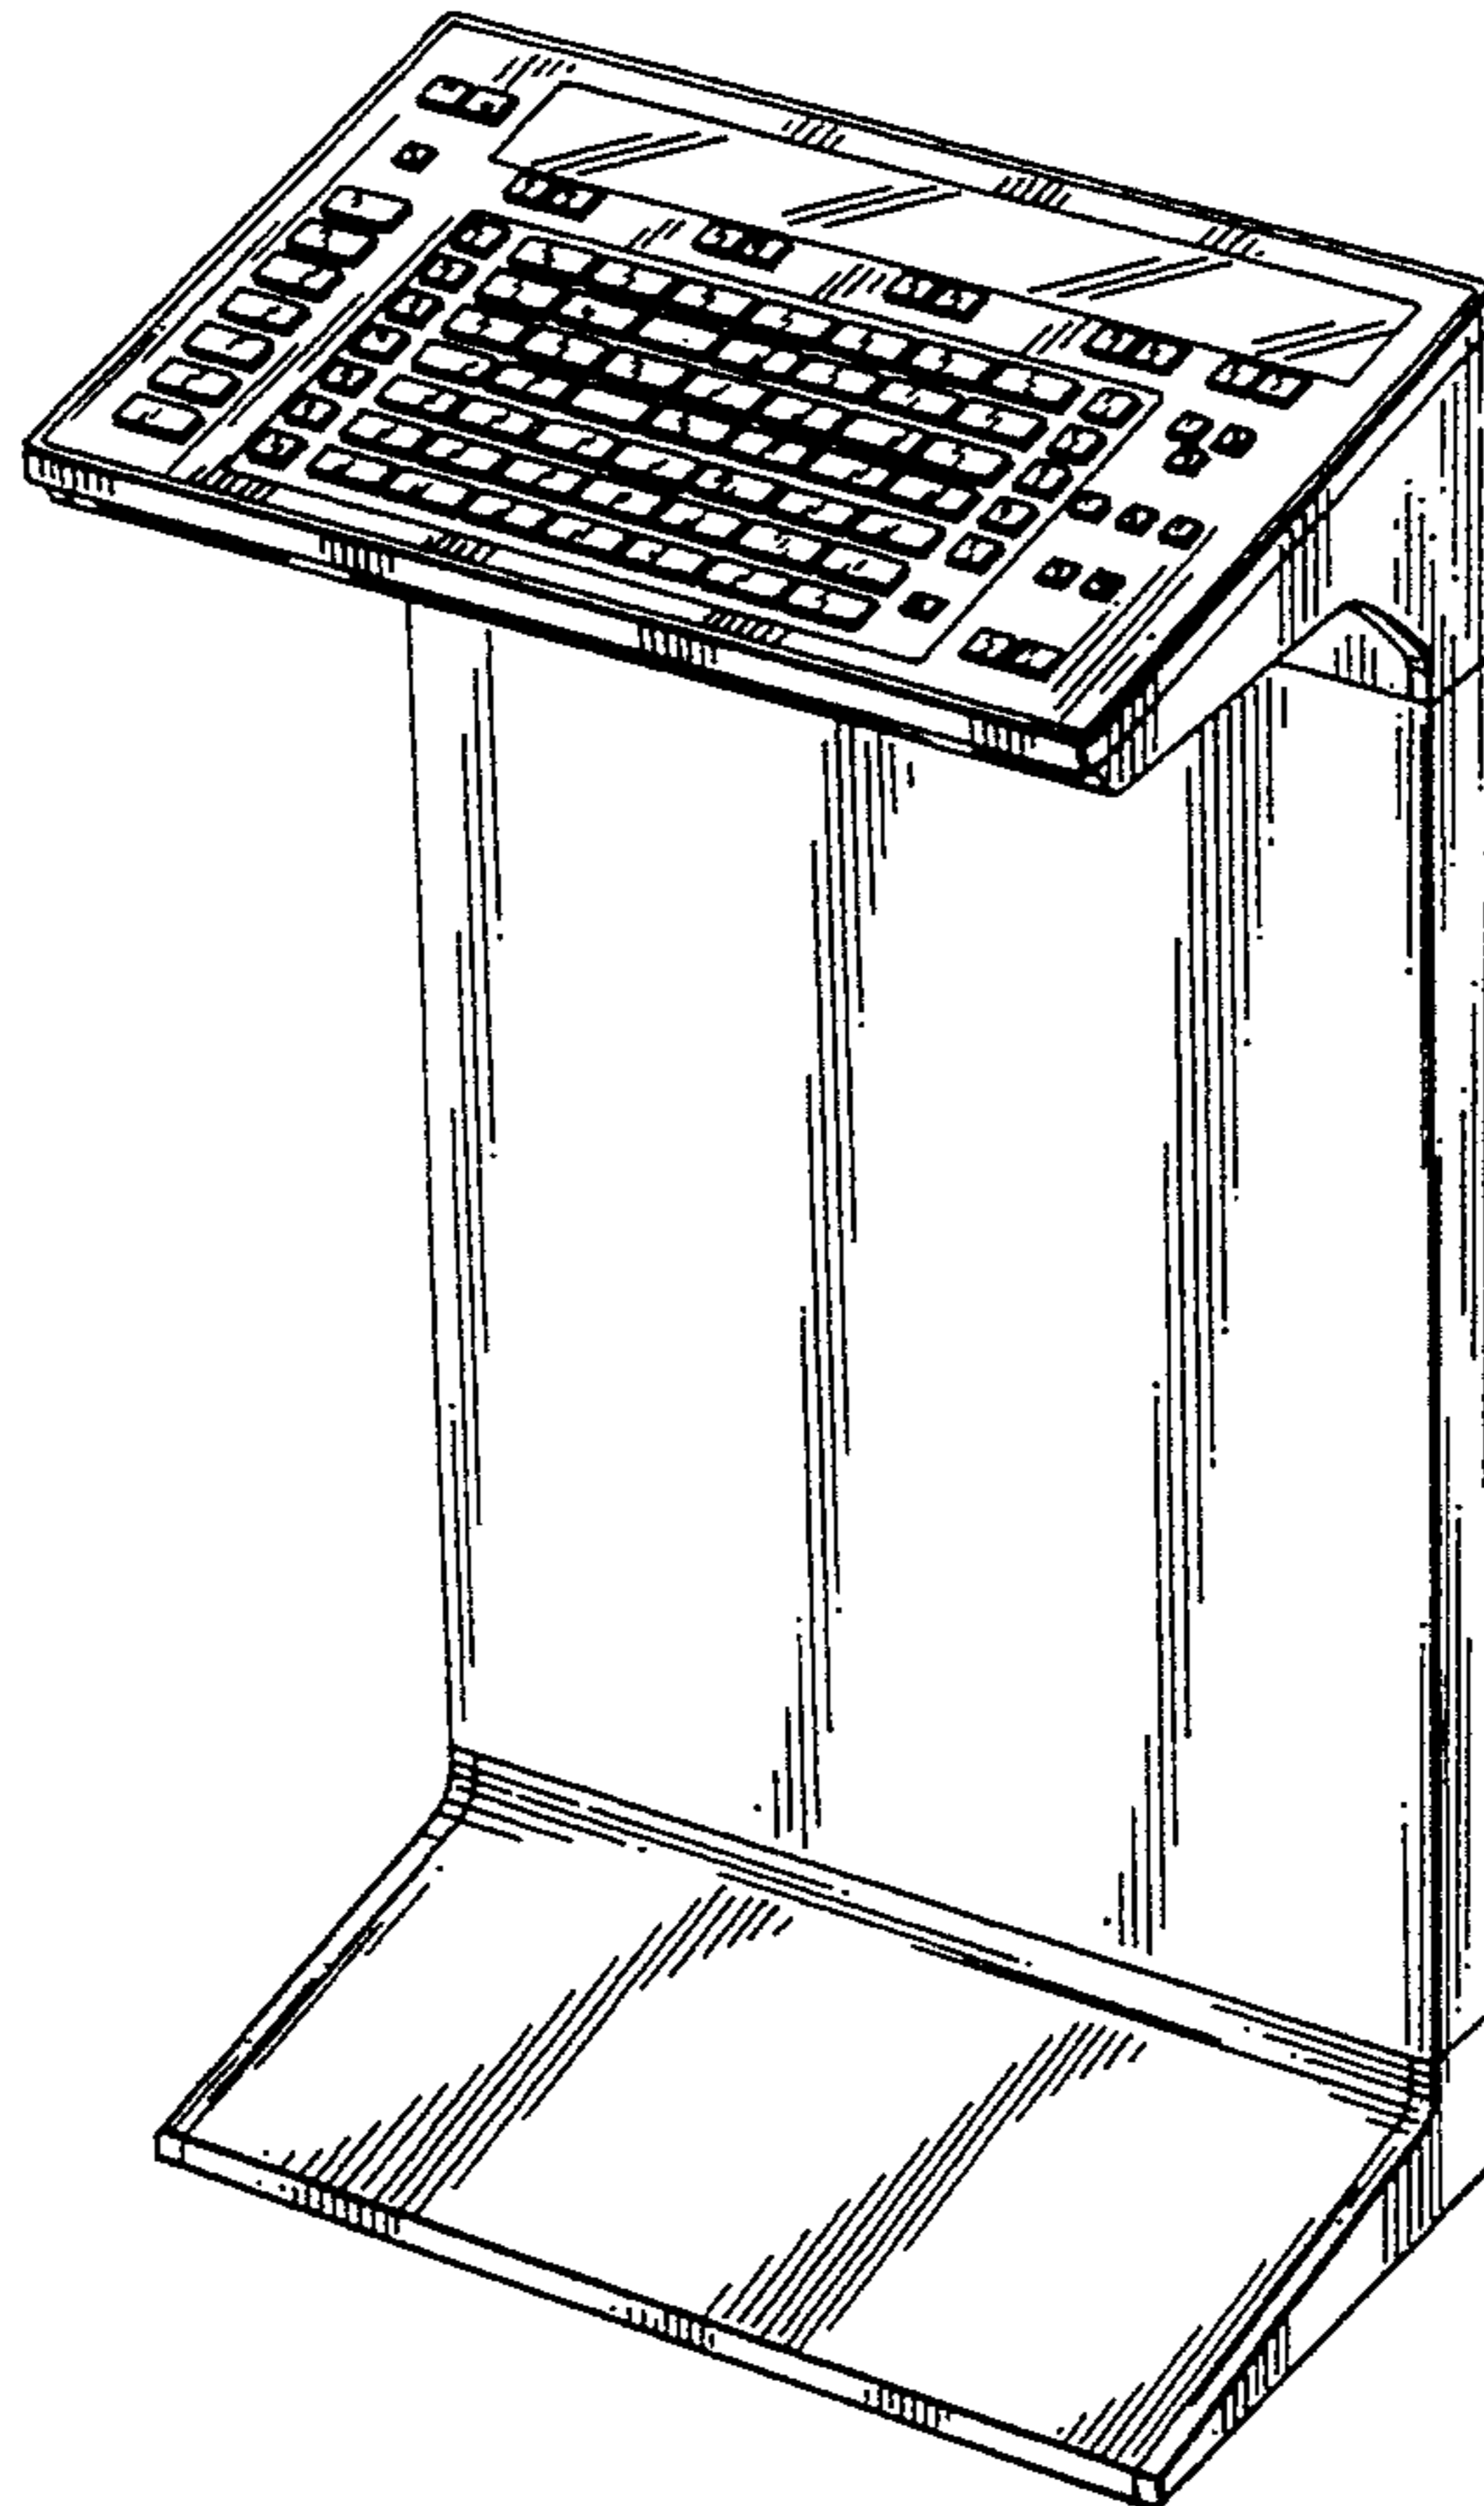


FIG. 1

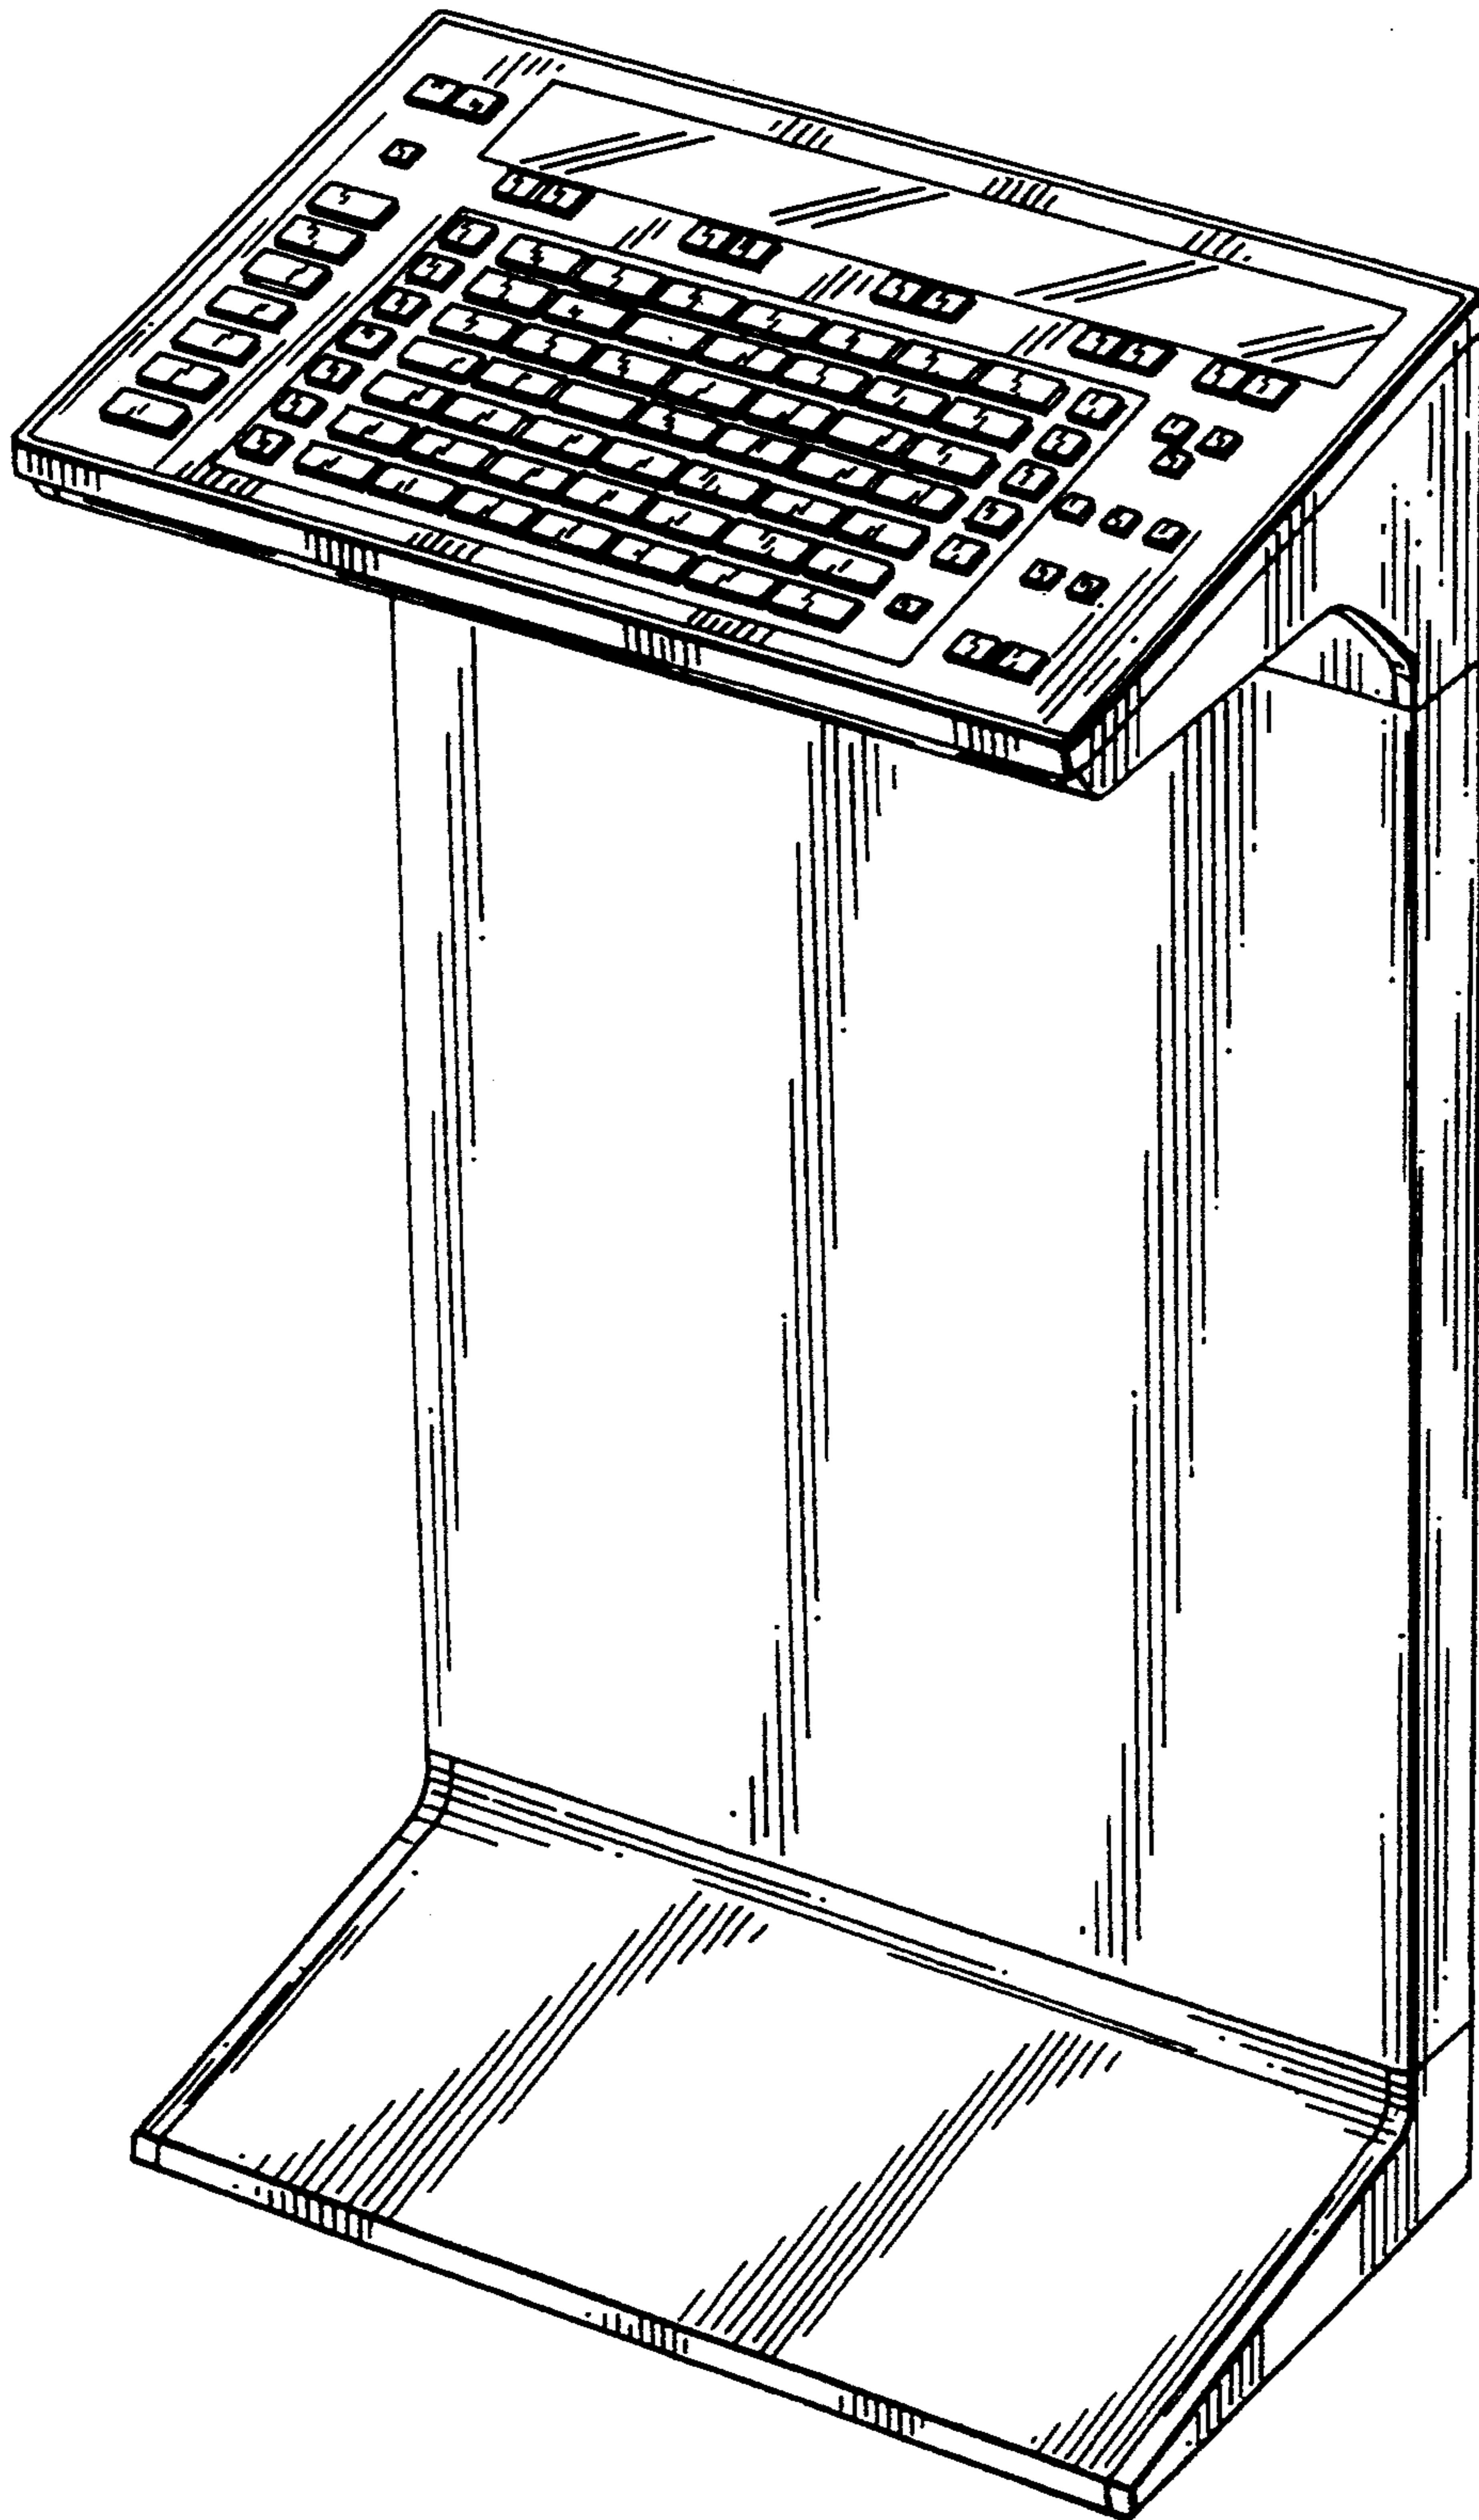


FIG. 2

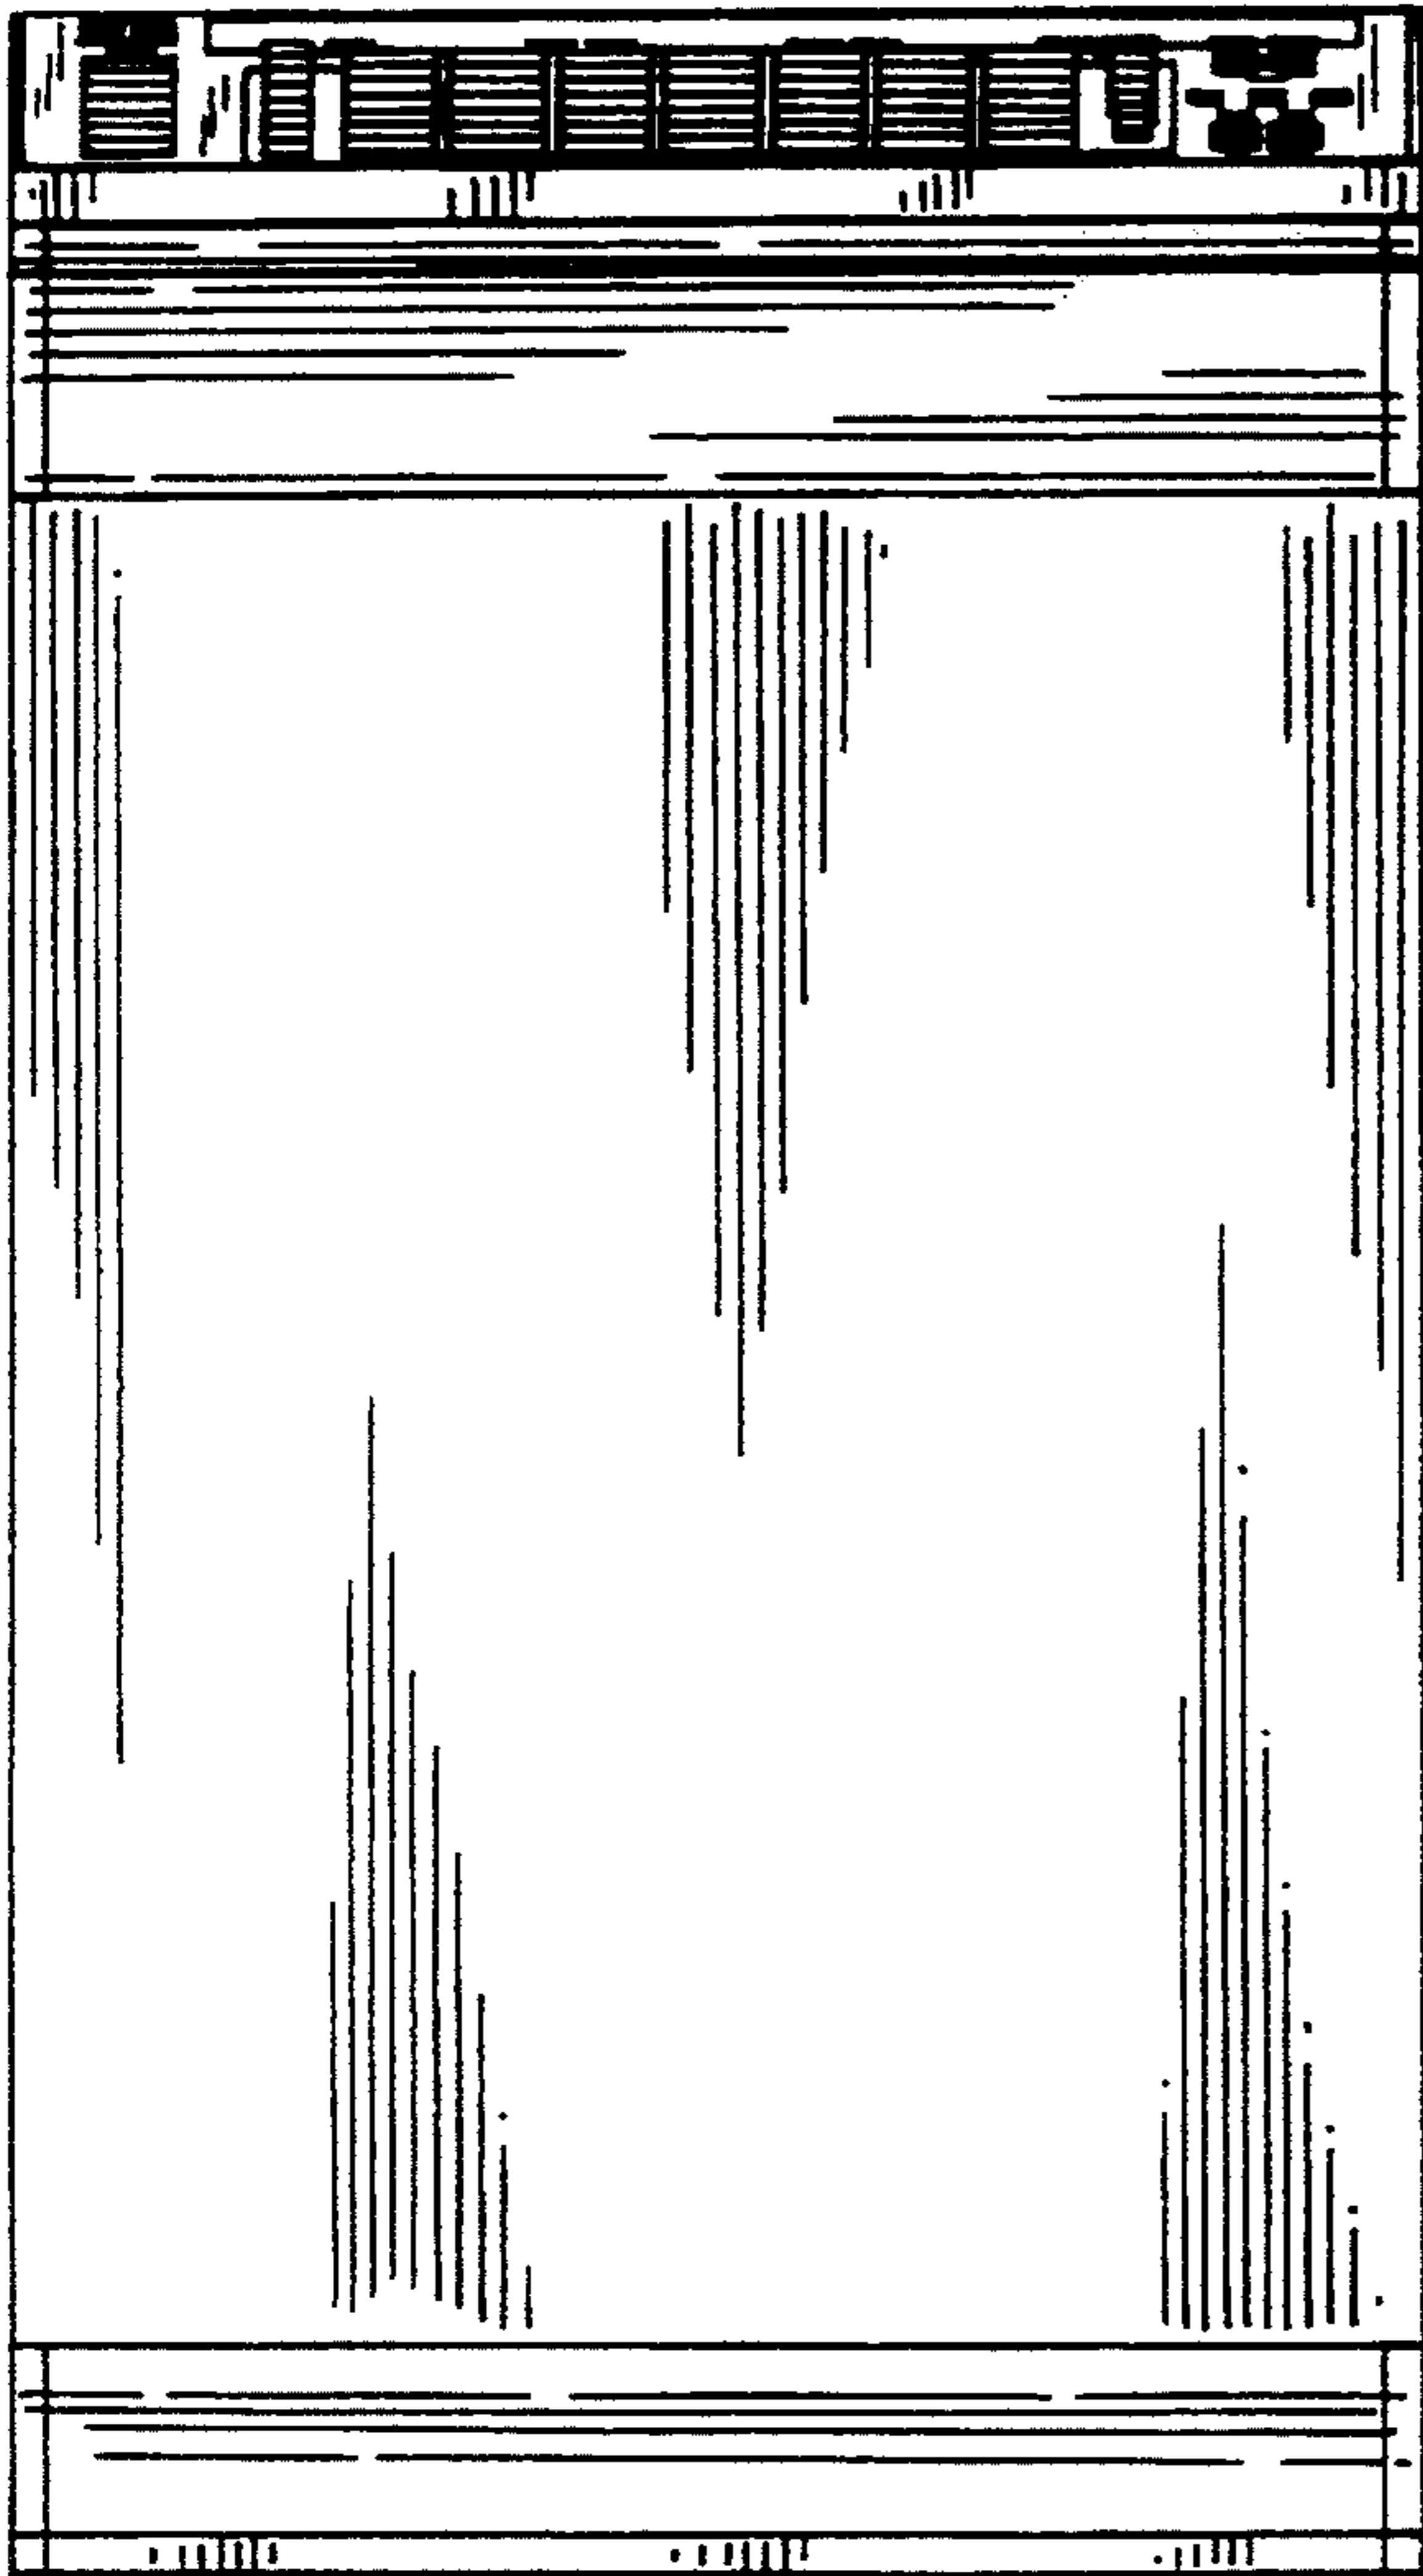


FIG. 3

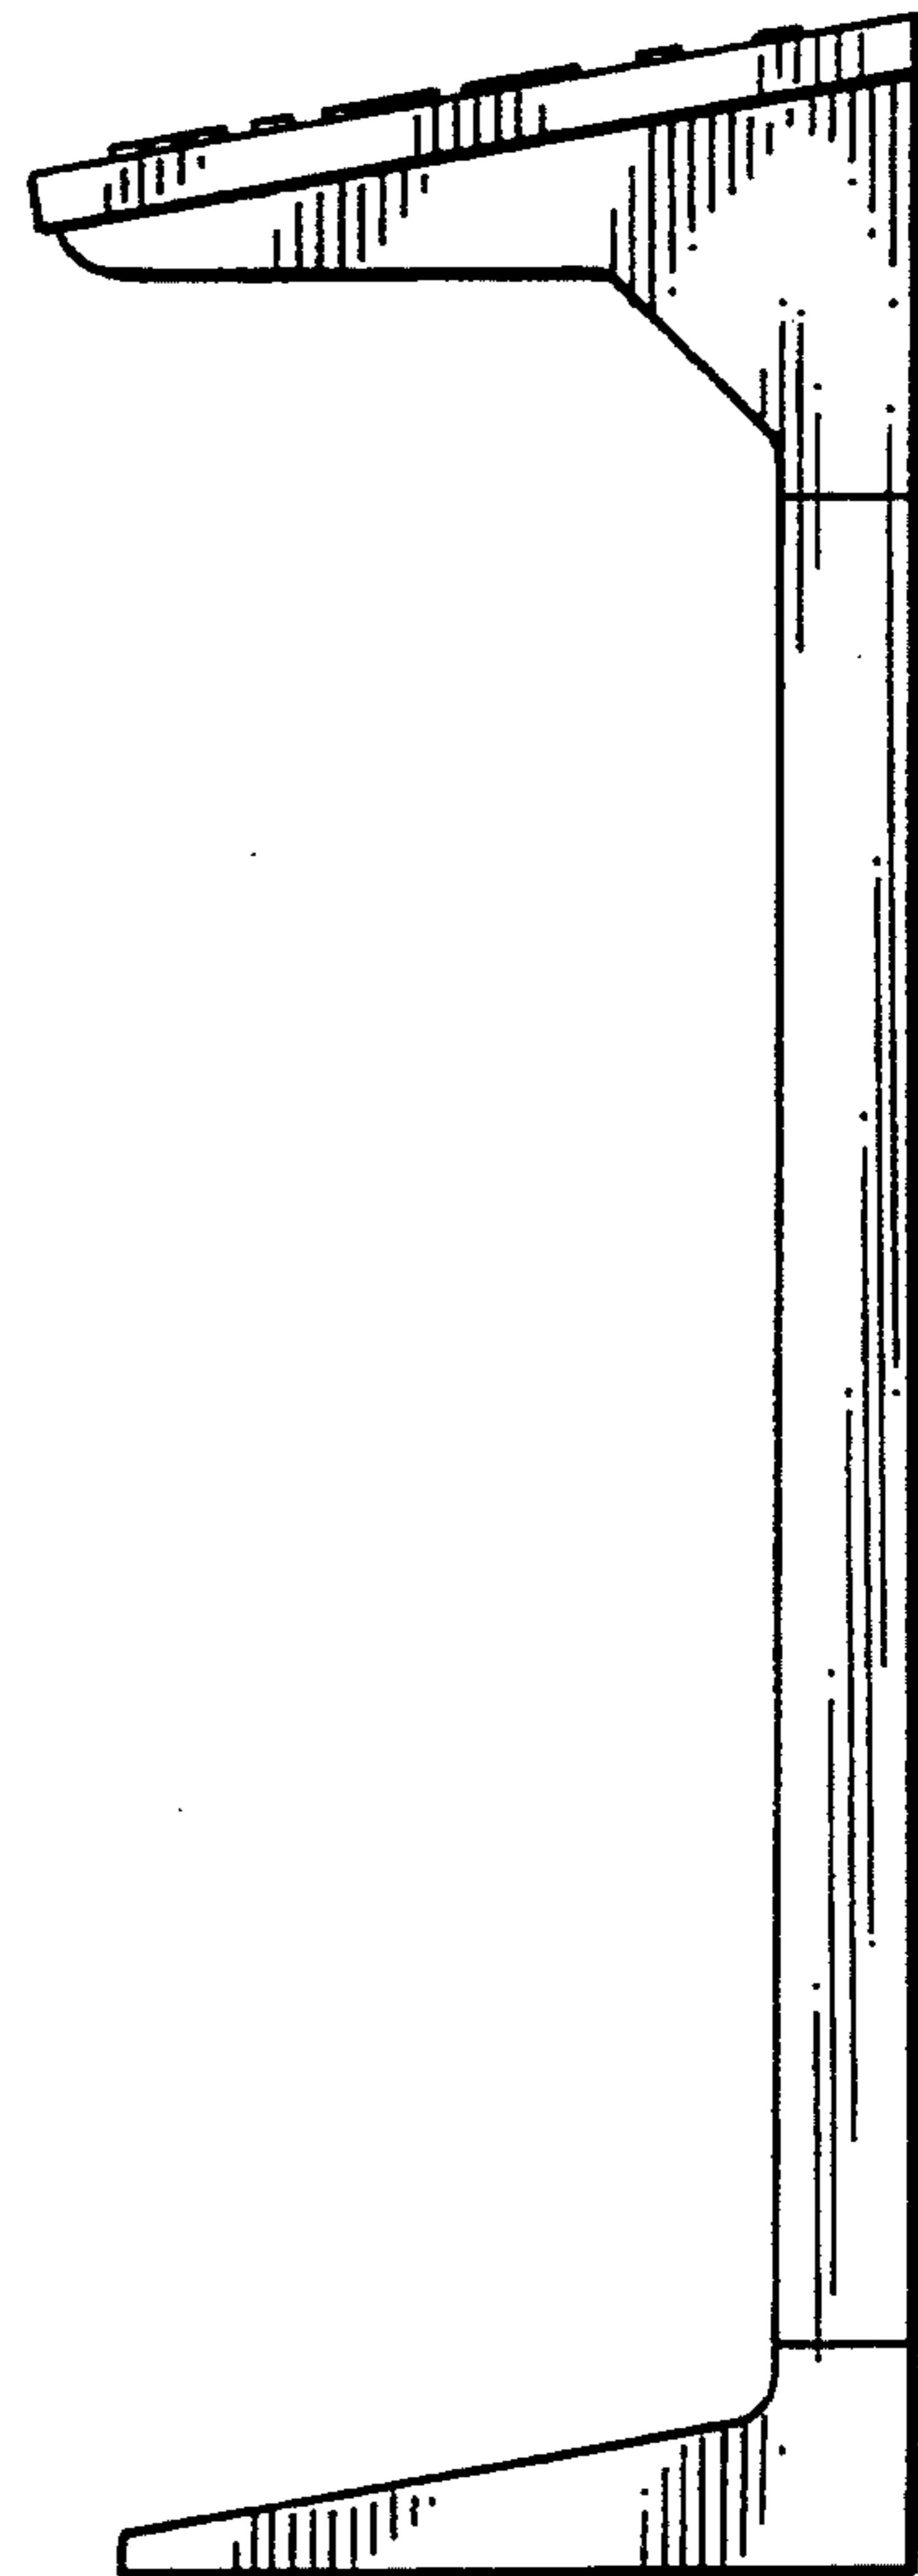


FIG. 4

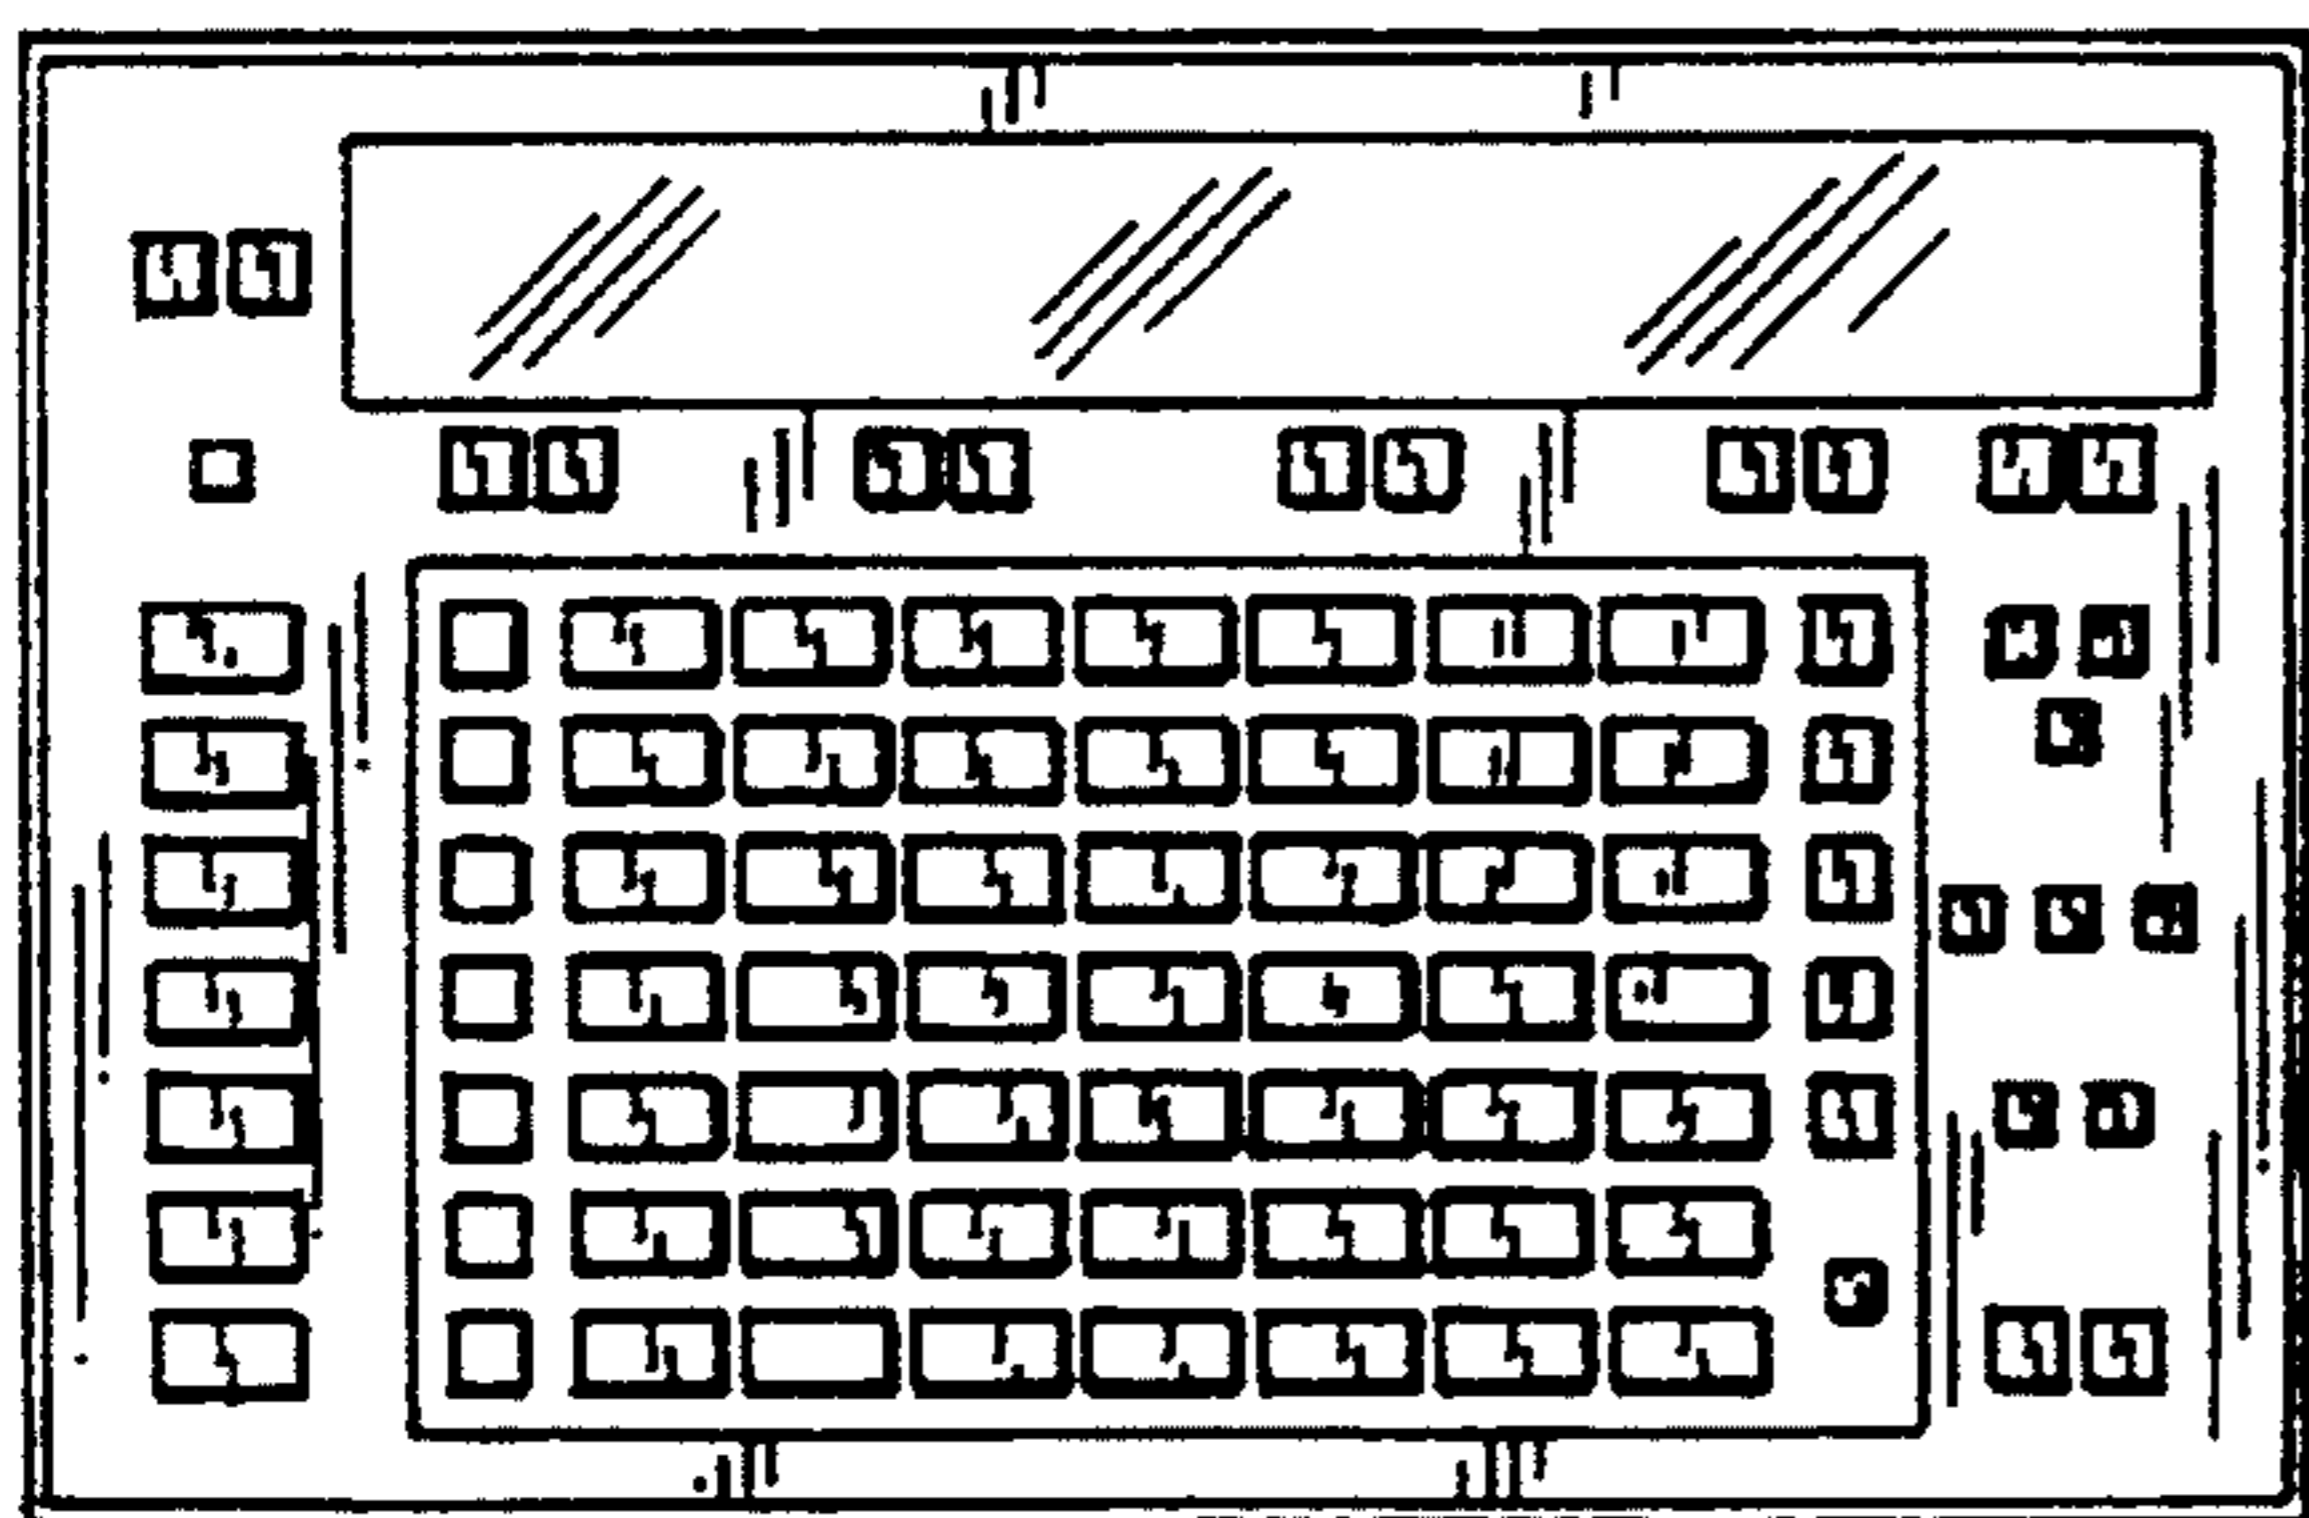


FIG. 5

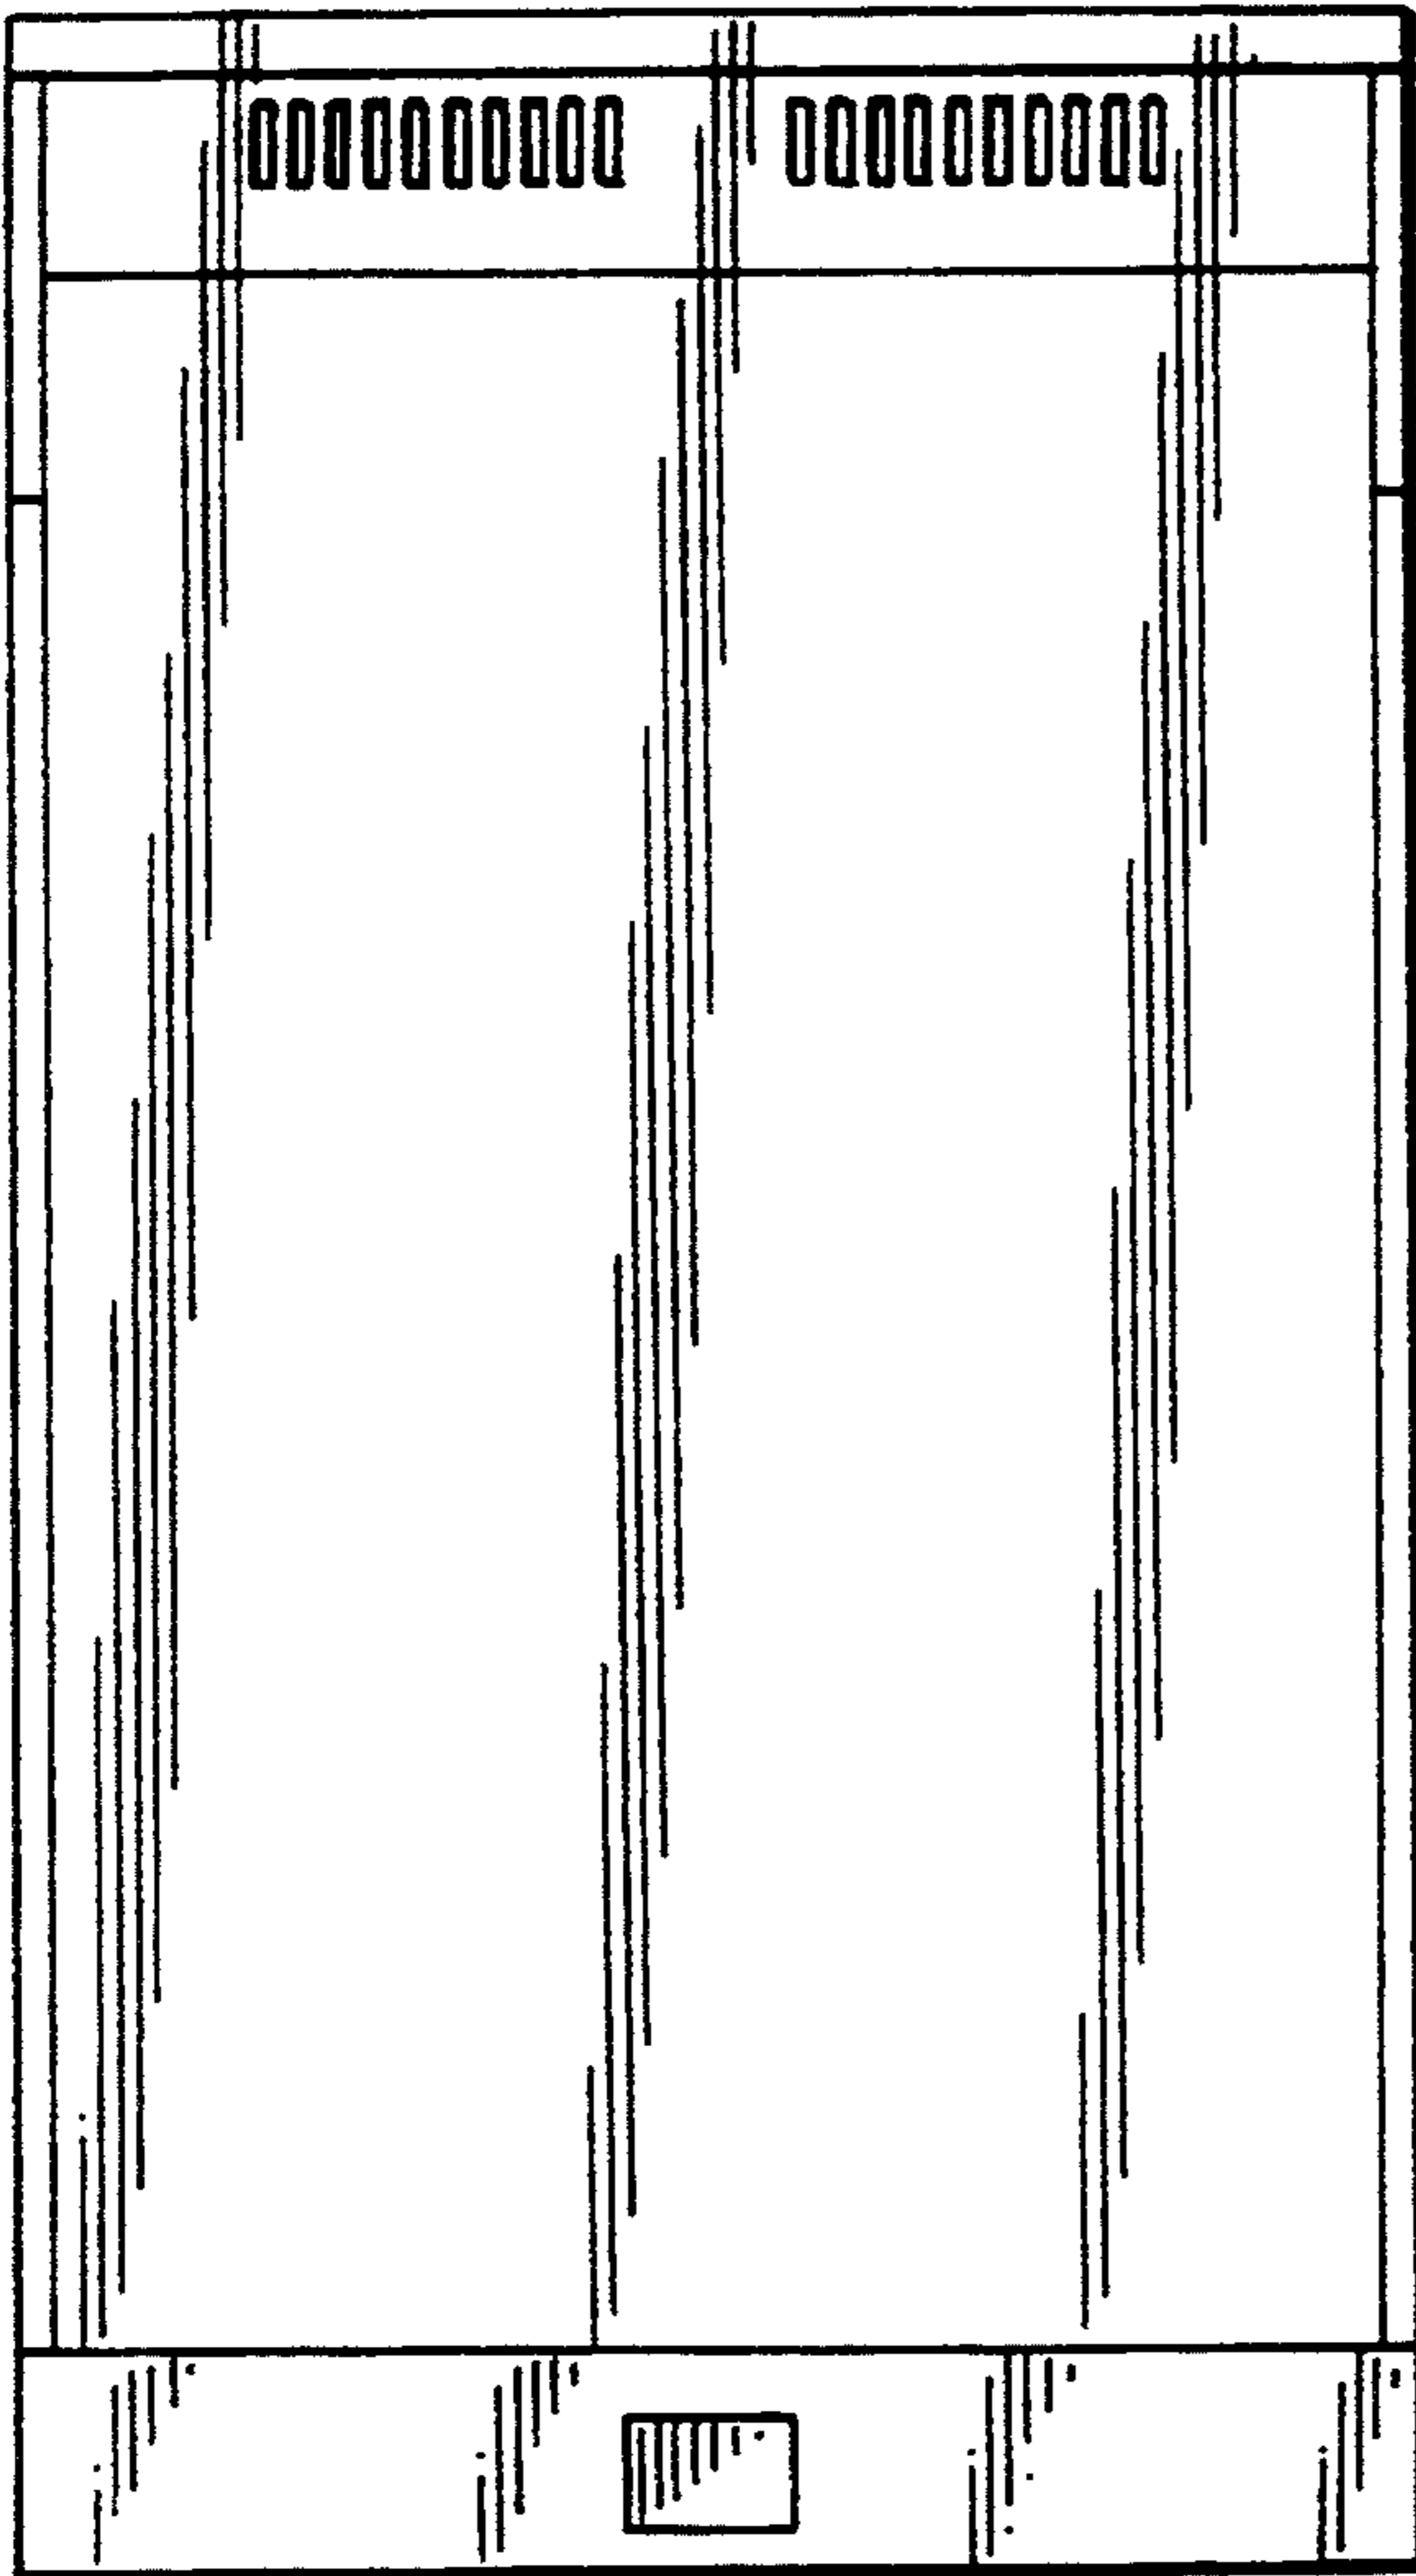


FIG. 6

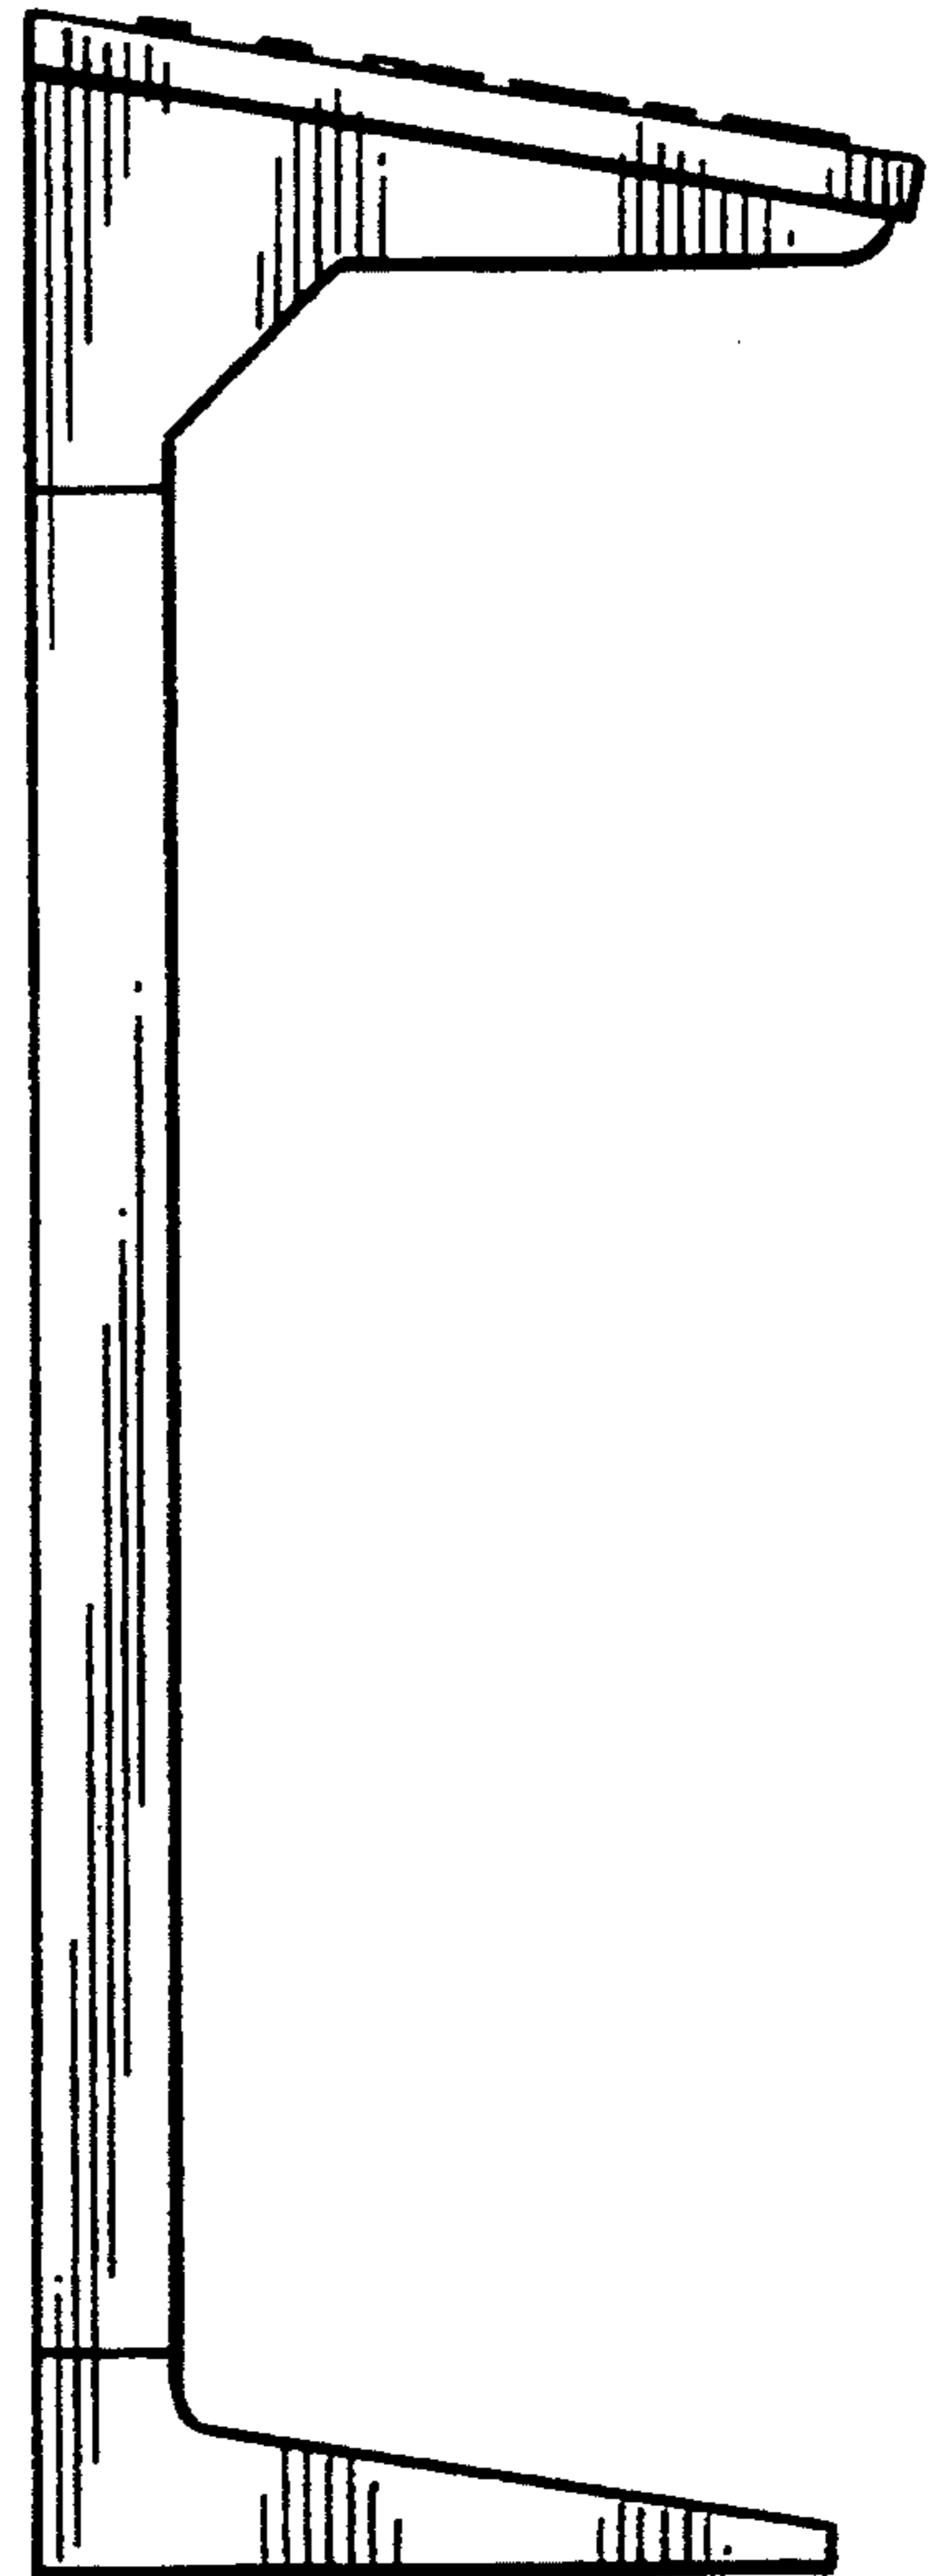


FIG. 7

