



US00D355718S

United States Patent [19]
McMullen

[11] **Patent Number: Des. 355,718**
[45] **Date of Patent: ** Feb. 21, 1995**

[54] **VIDEO FLUORO IMAGING CHAIR FOR
DYSPHAGIA STUDIES**

5,249,838 10/1993 Kulpa et al. 297/328

[75] **Inventor: Craig T. McMullen, Colorado
Springs, Colo.**

Primary Examiner—Stella Reid
Attorney, Agent, or Firm—Dorr, Carson, Sloan &
Peterson

[73] **Assignee: Robert E. Giustra, Monument, Colo.**

[57] **CLAIM**

[**] **Term: 14 Years**

The ornamental design for a video fluoro imaging chair
for dysphagia studies, as shown and described.

[21] **Appl. No.: 14,611**

DESCRIPTION

[22] **Filed: Oct. 25, 1993**

[52] **U.S. Cl. D24/158**

[58] **Field of Search D24/158; 378/180, 179,
378/178, 156, 208; 297/328, 302**

FIG. 1 is a perspective view of a video fluoro imaging
chair for dysphagia studies, showing my new design,
the broken line showing is for illustrative purposes only
and forms no part of the claimed design;

FIG. 2 is a front elevational view thereof;

FIG. 3 is a right side elevational view thereof, the left
side elevational view being a mirror image thereto;

FIG. 4 is a rear elevational view thereof;

FIG. 5 is a top plan view thereof; and,

FIG. 6 is a bottom plan view thereof.

[56] **References Cited**

U.S. PATENT DOCUMENTS

3,655,968 4/1972 Moore et al. 378/178
4,464,780 8/1984 Ruiz 378/178



Fig. 1

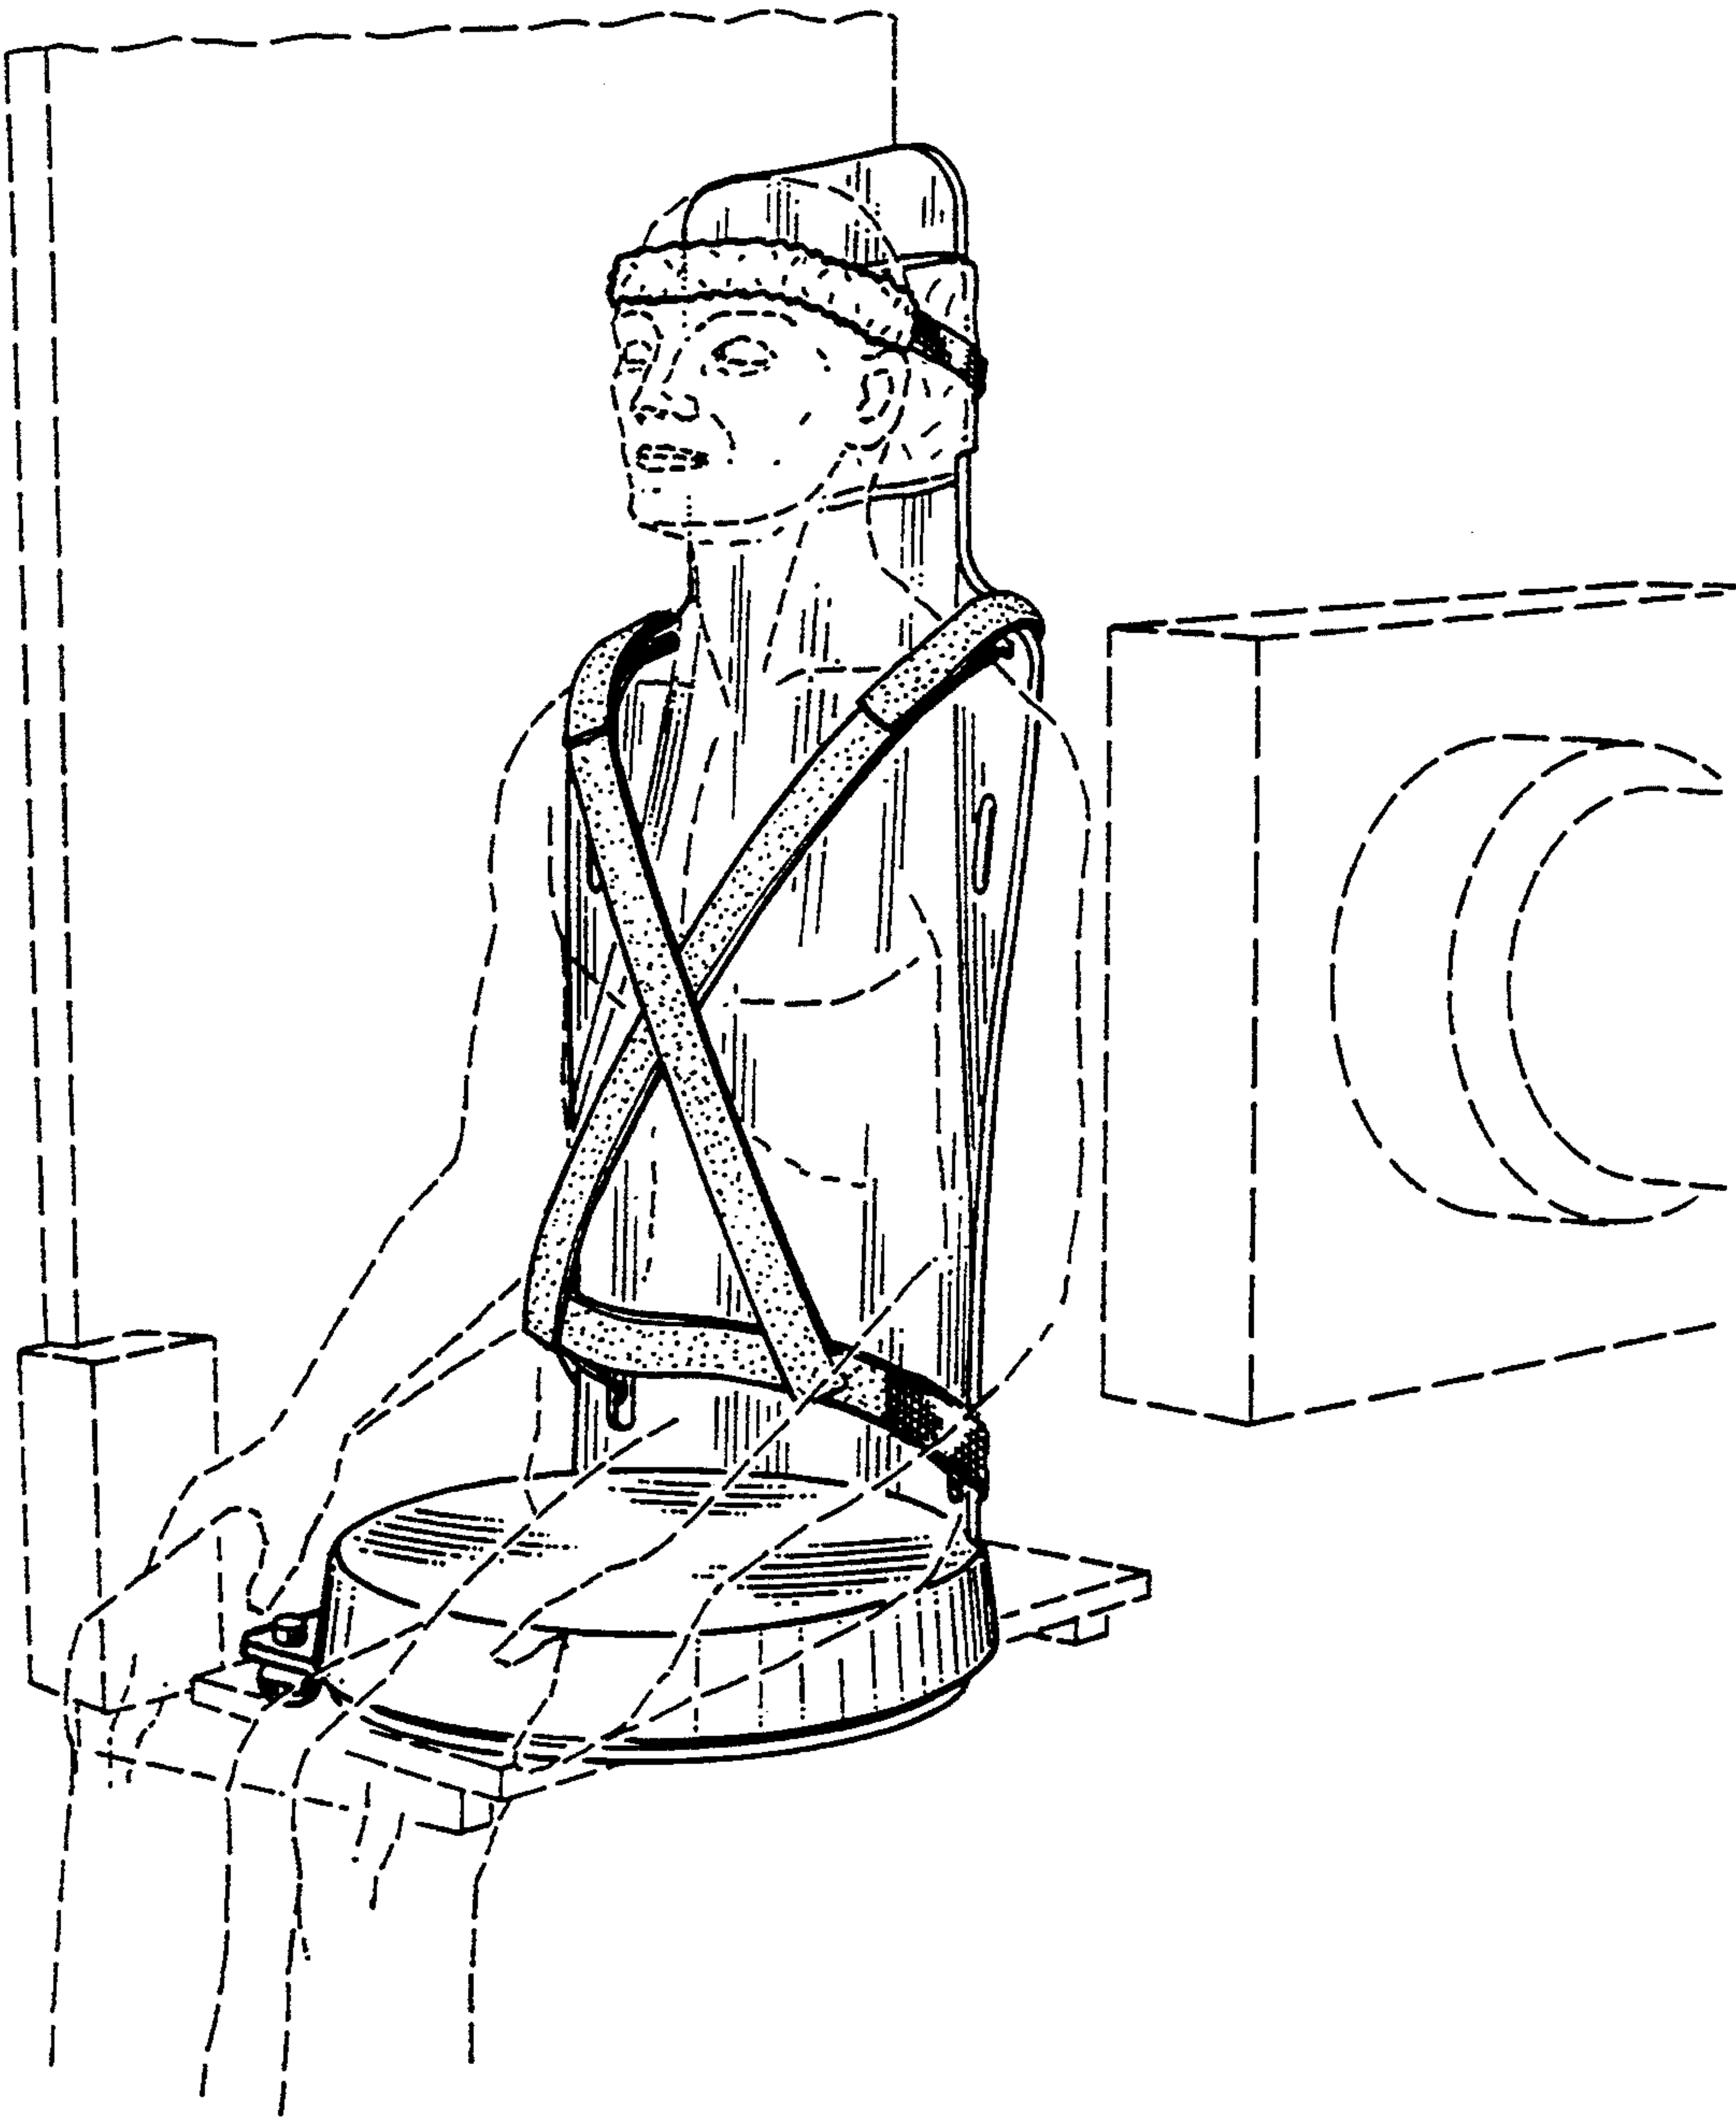


Fig. 3

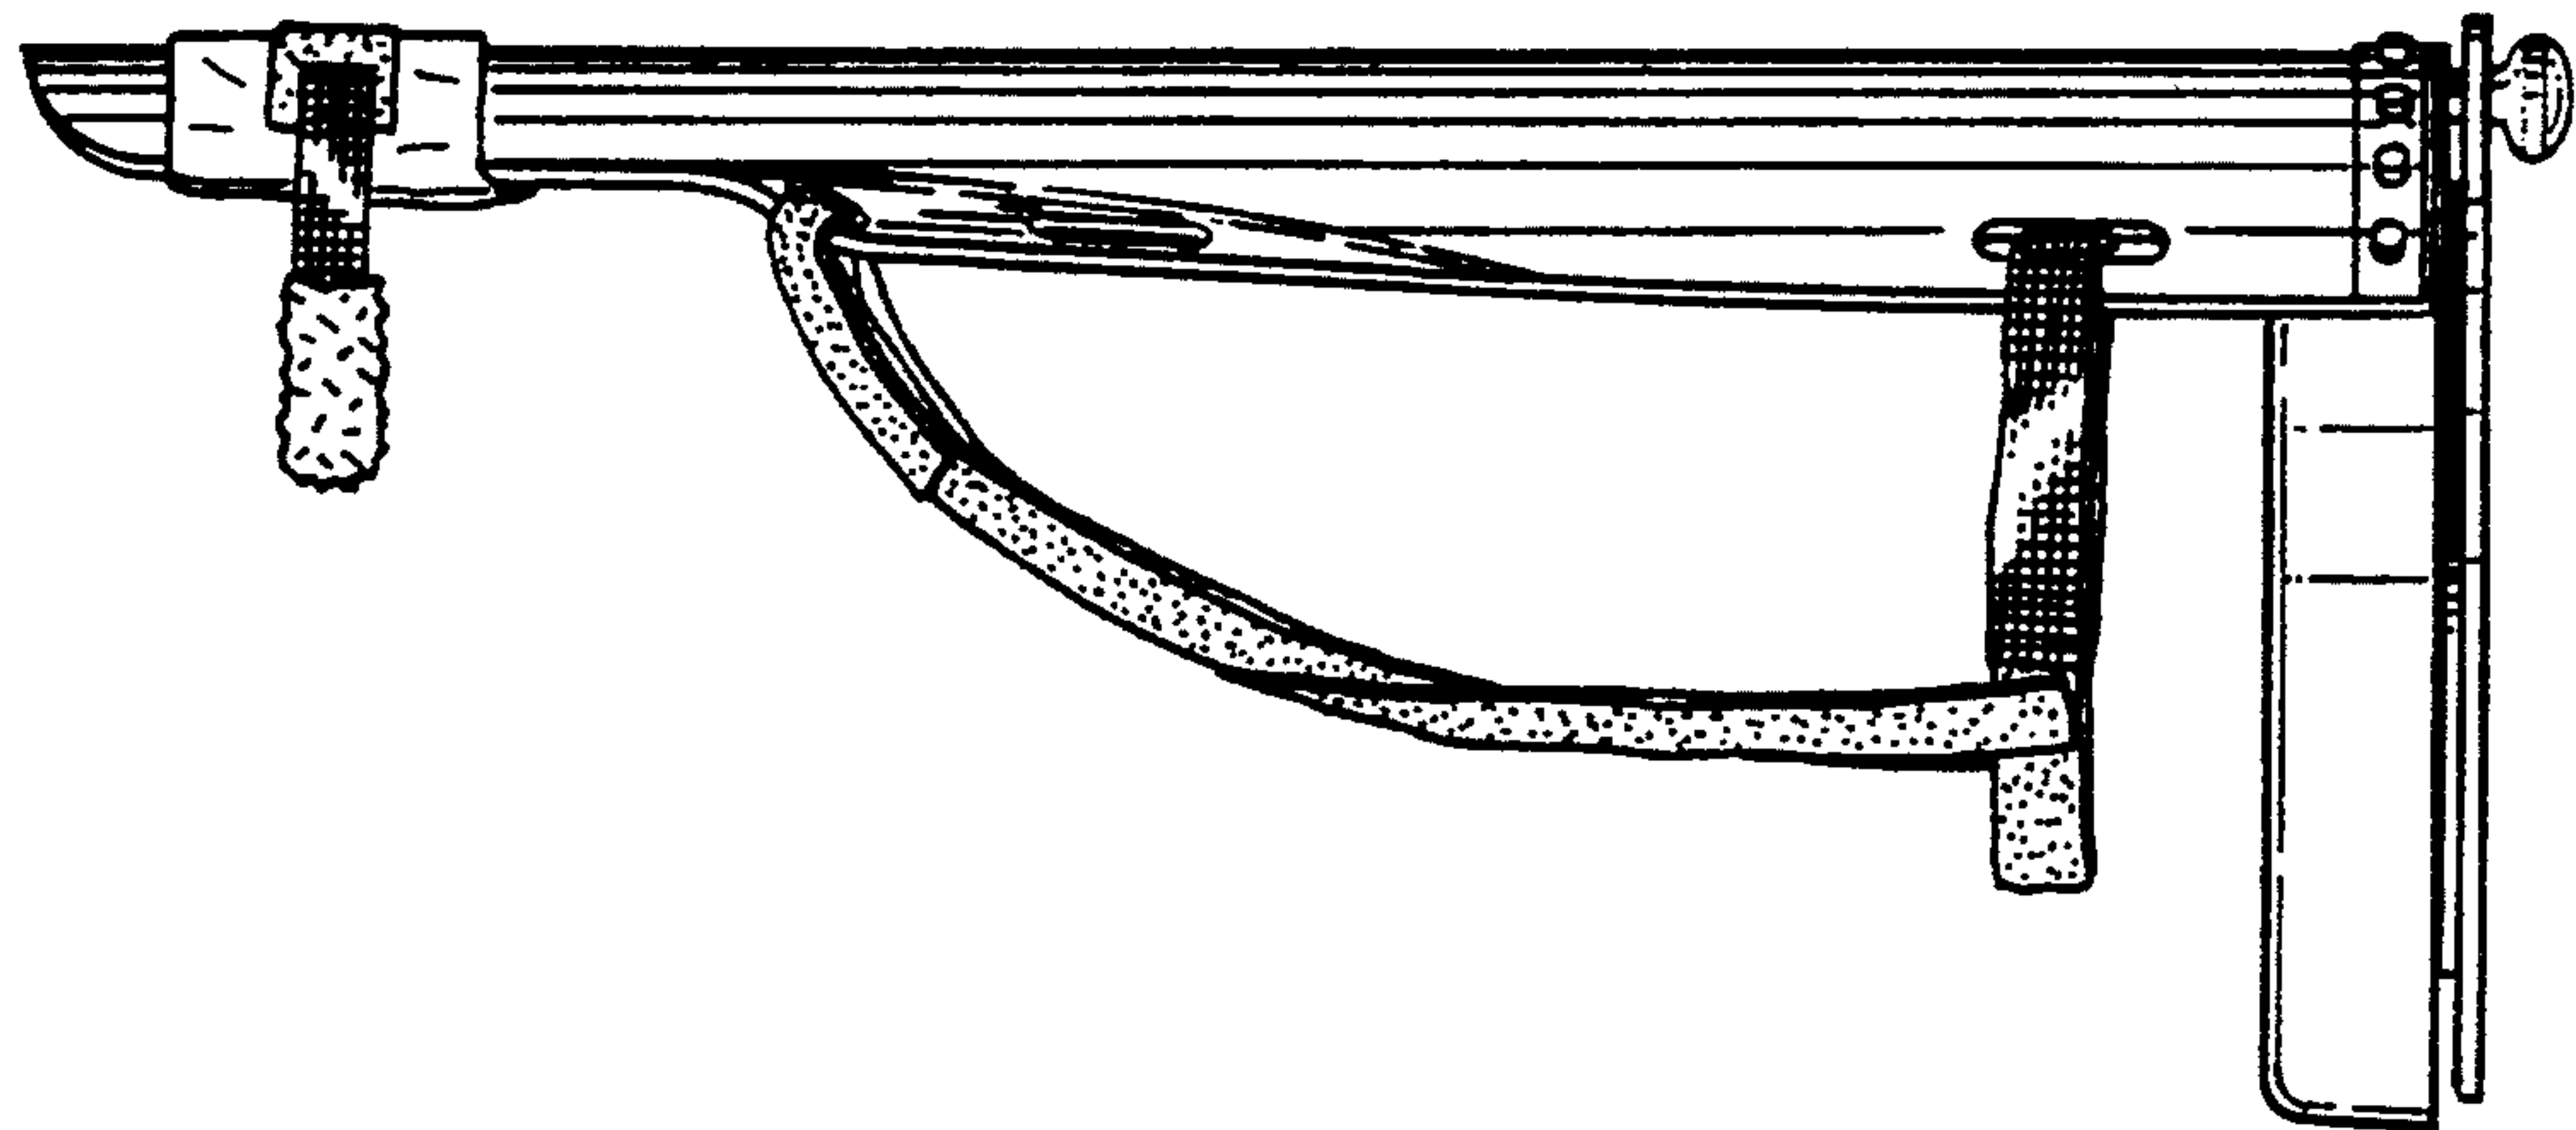


Fig. 2

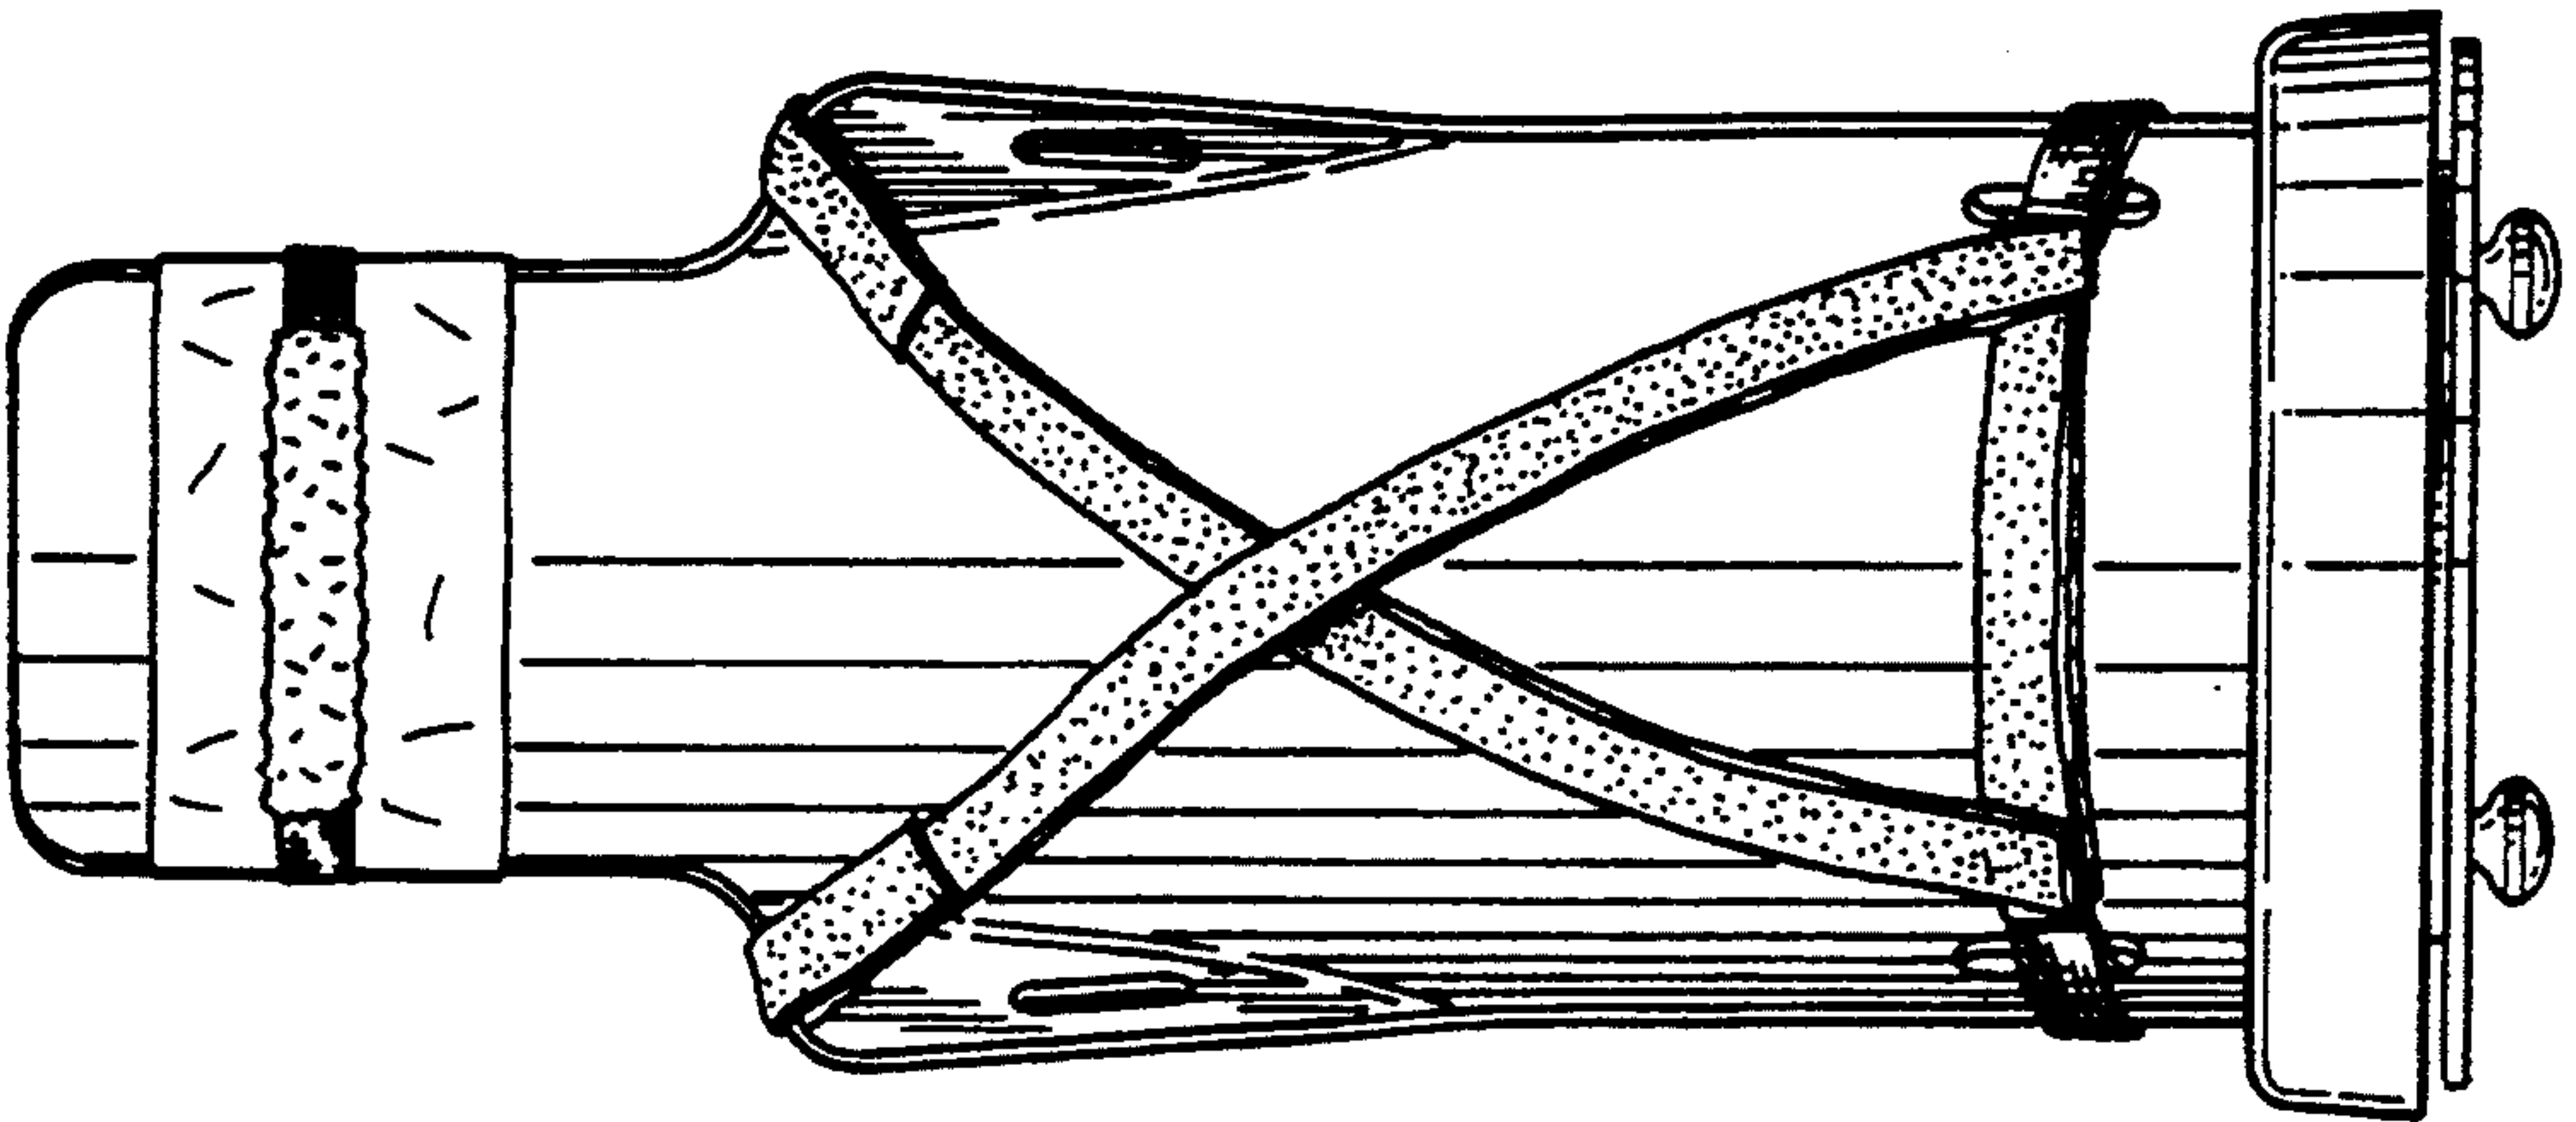


Fig. 4

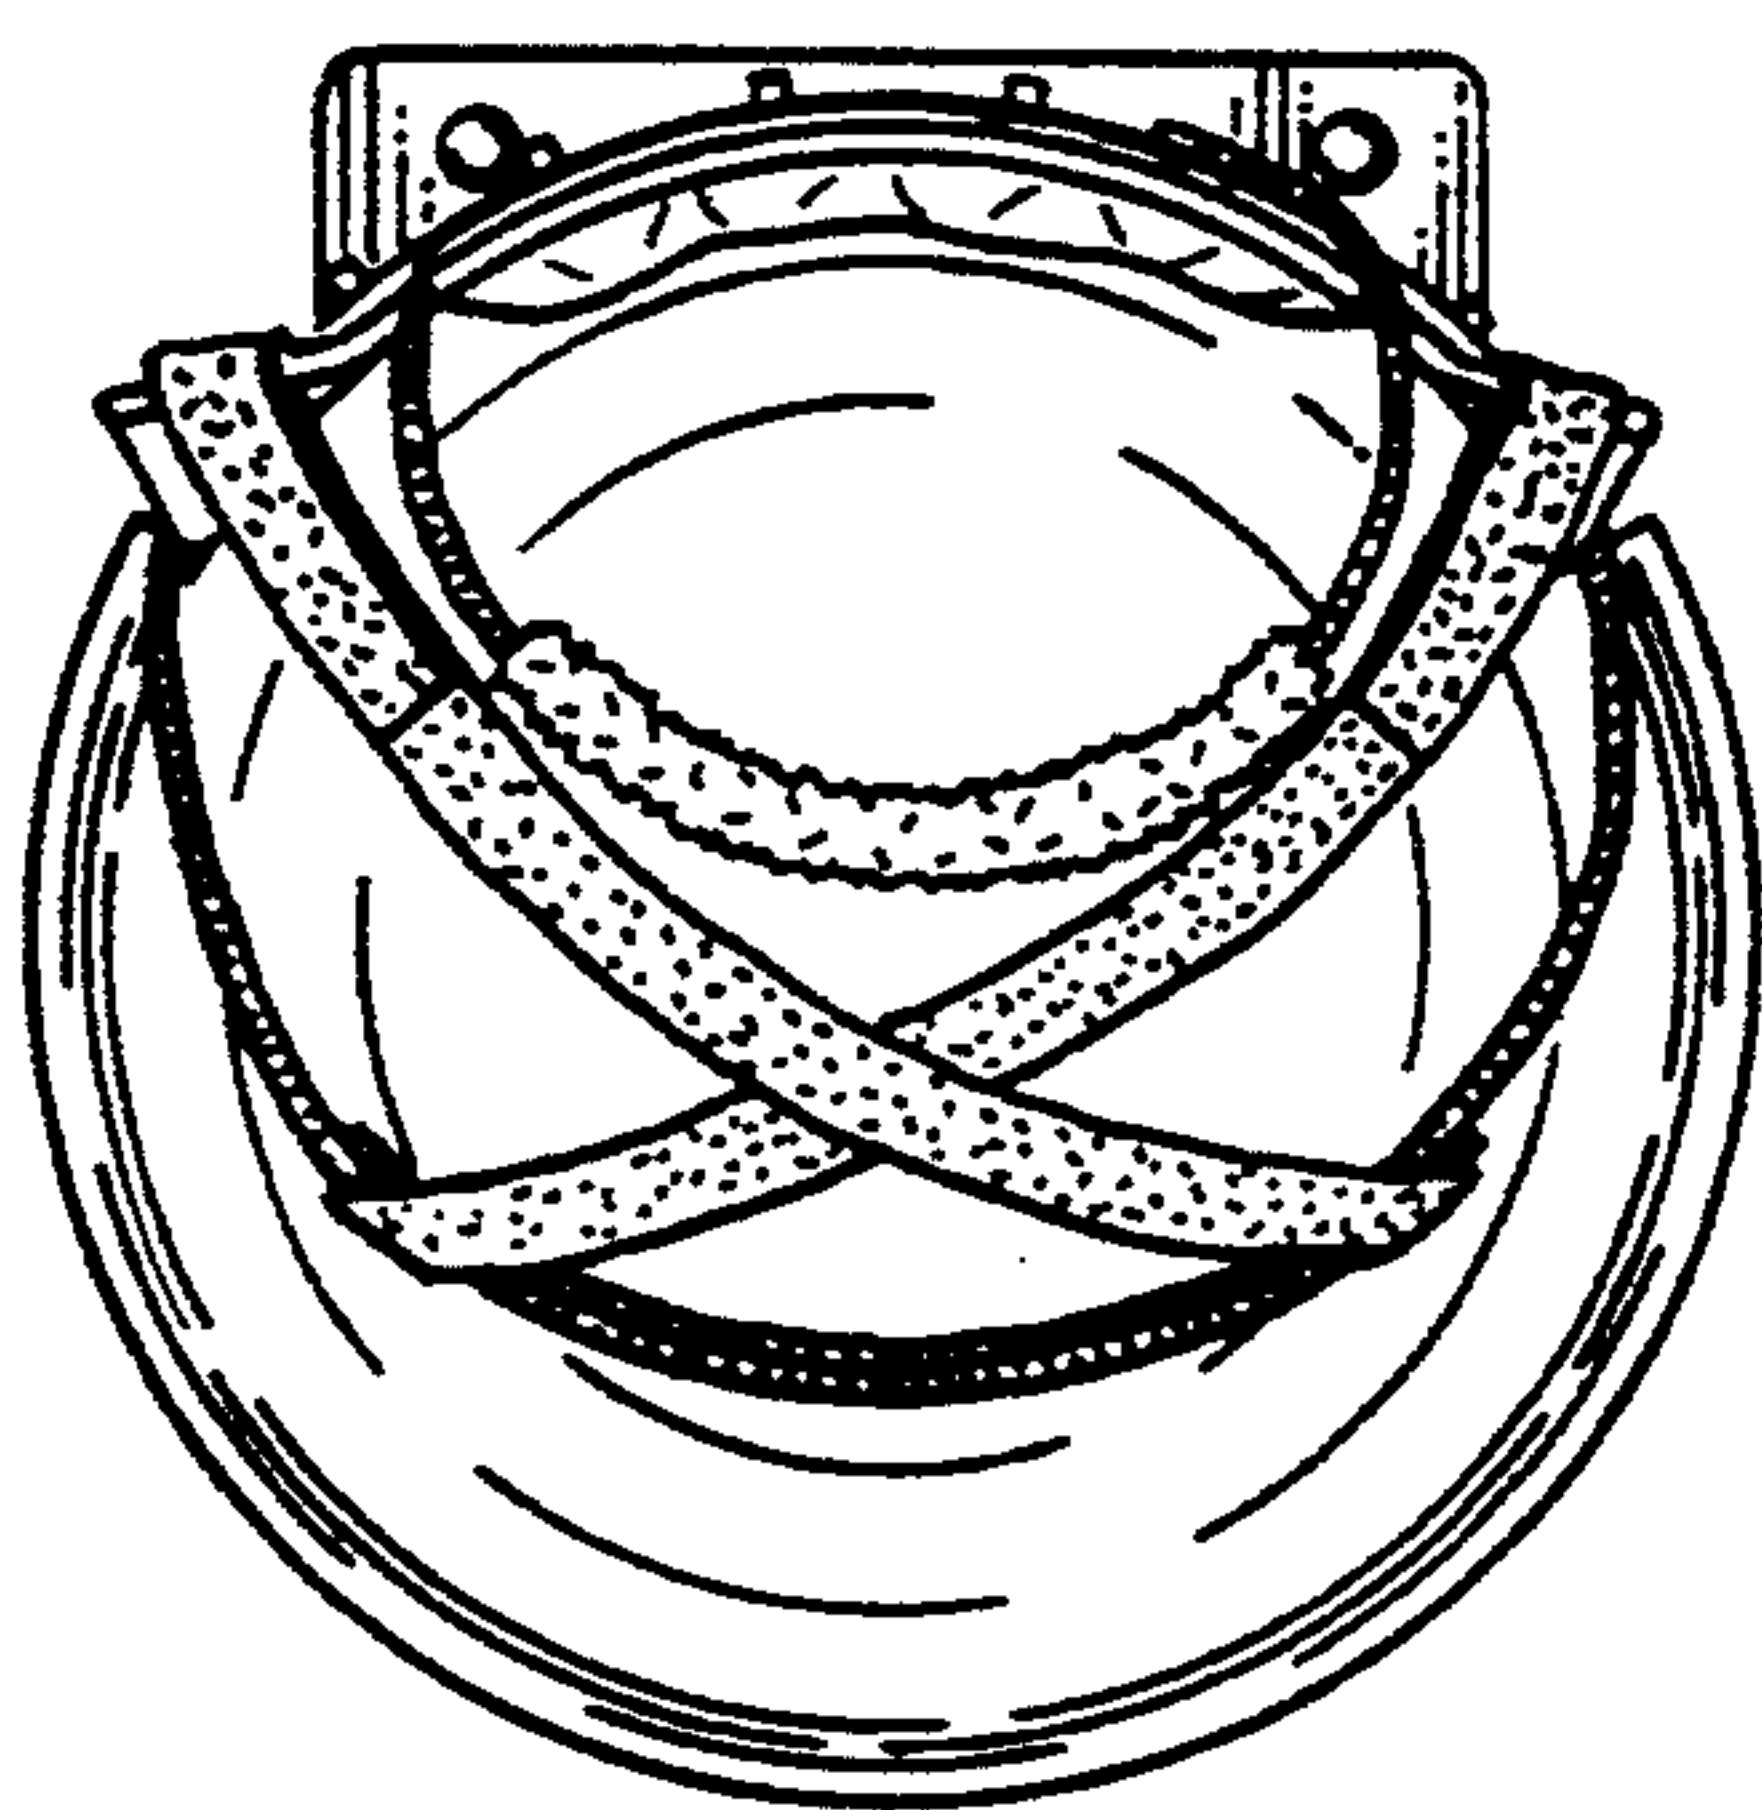
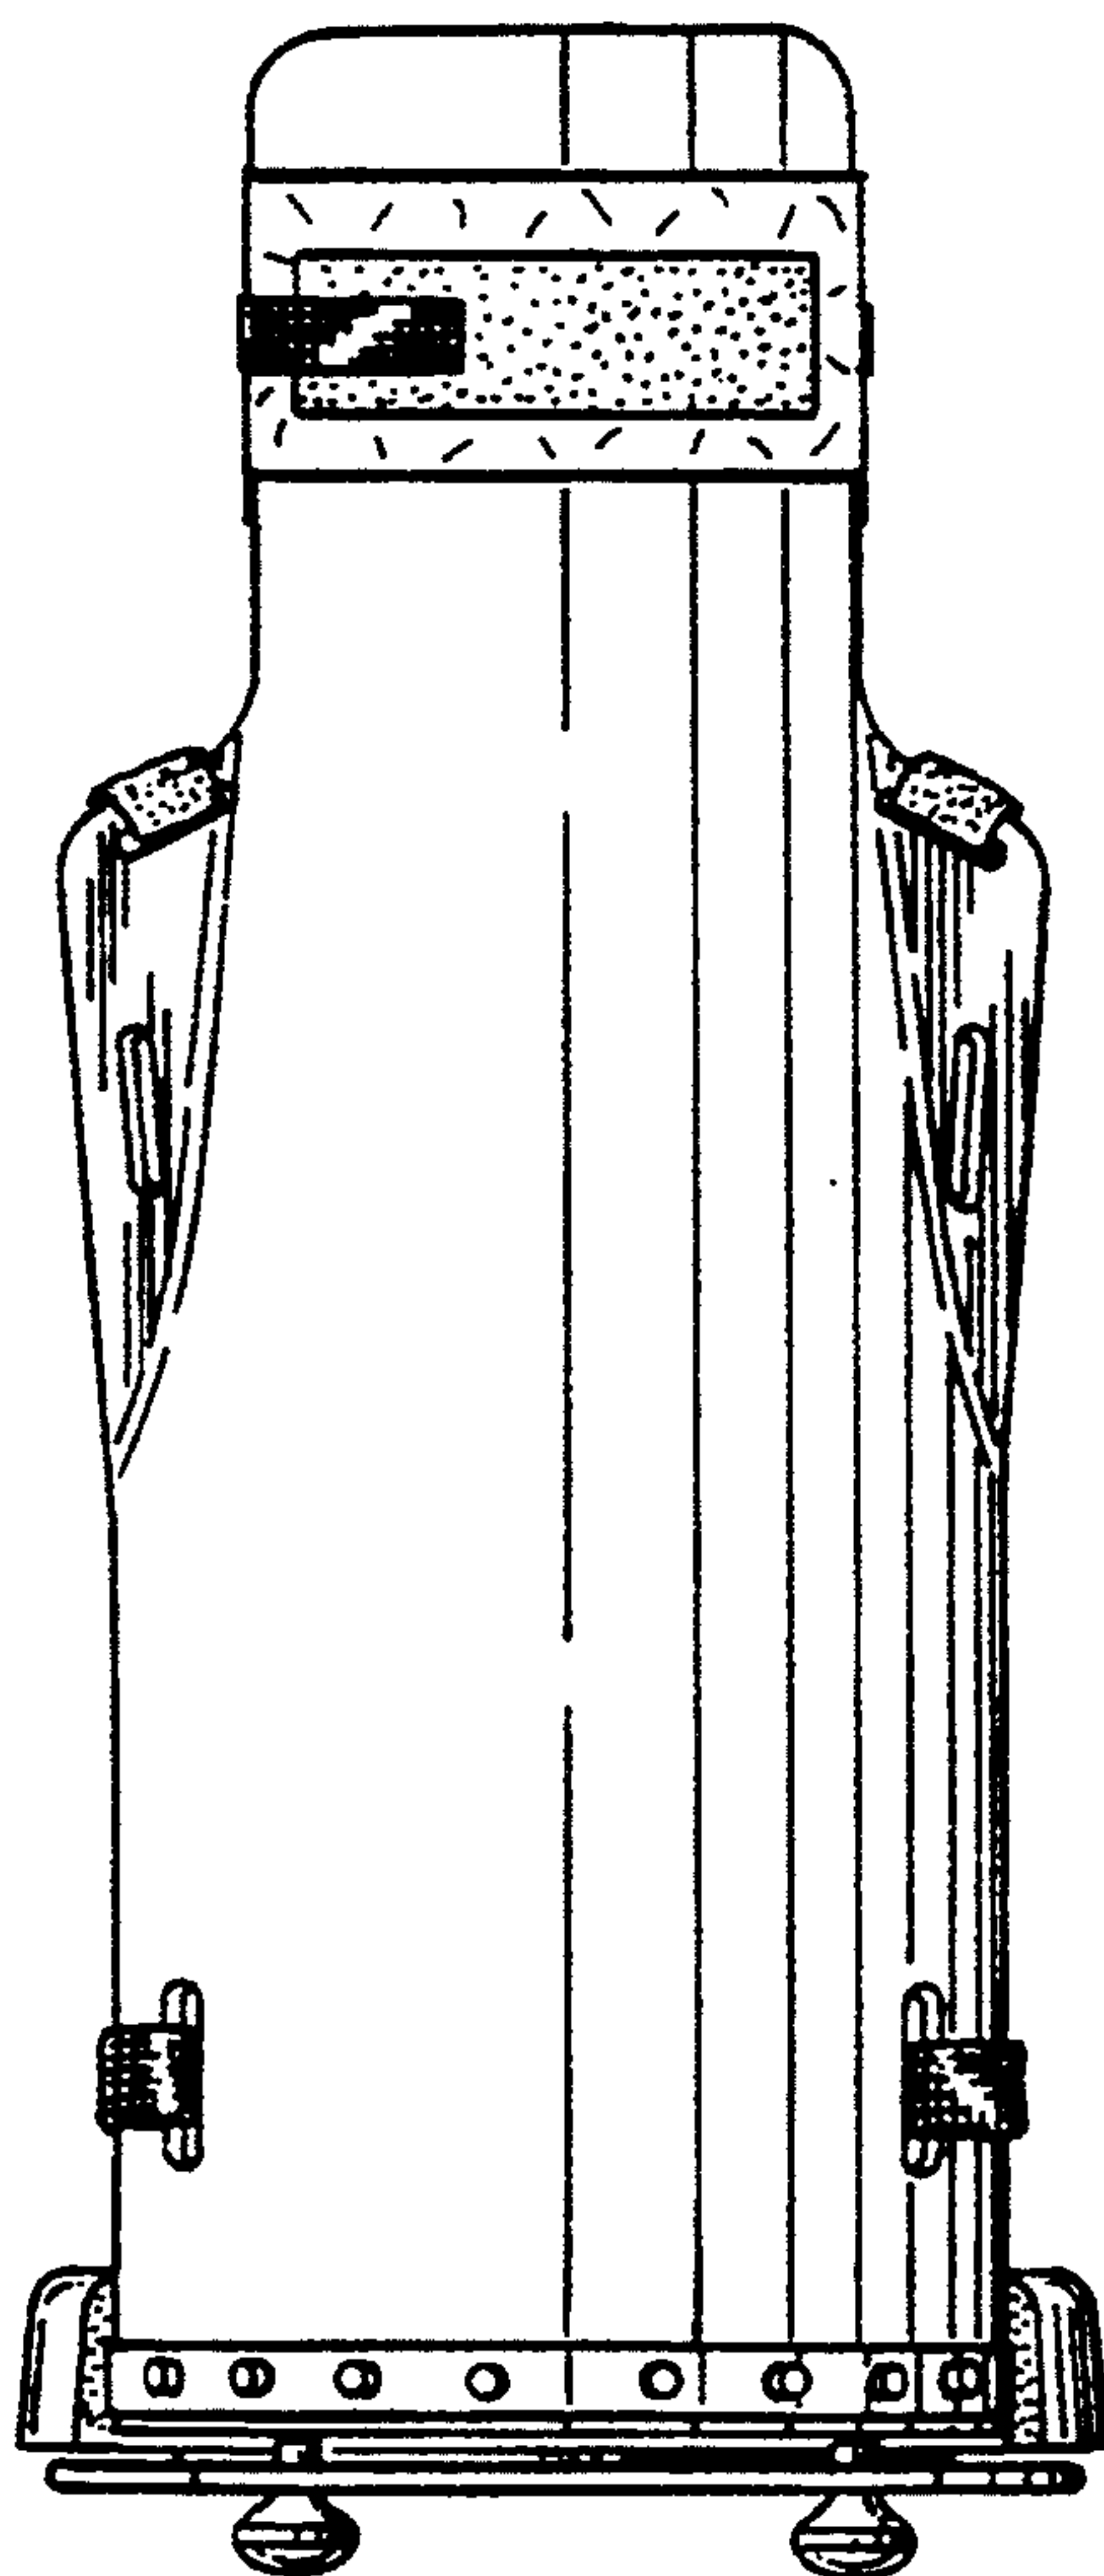


Fig. 5

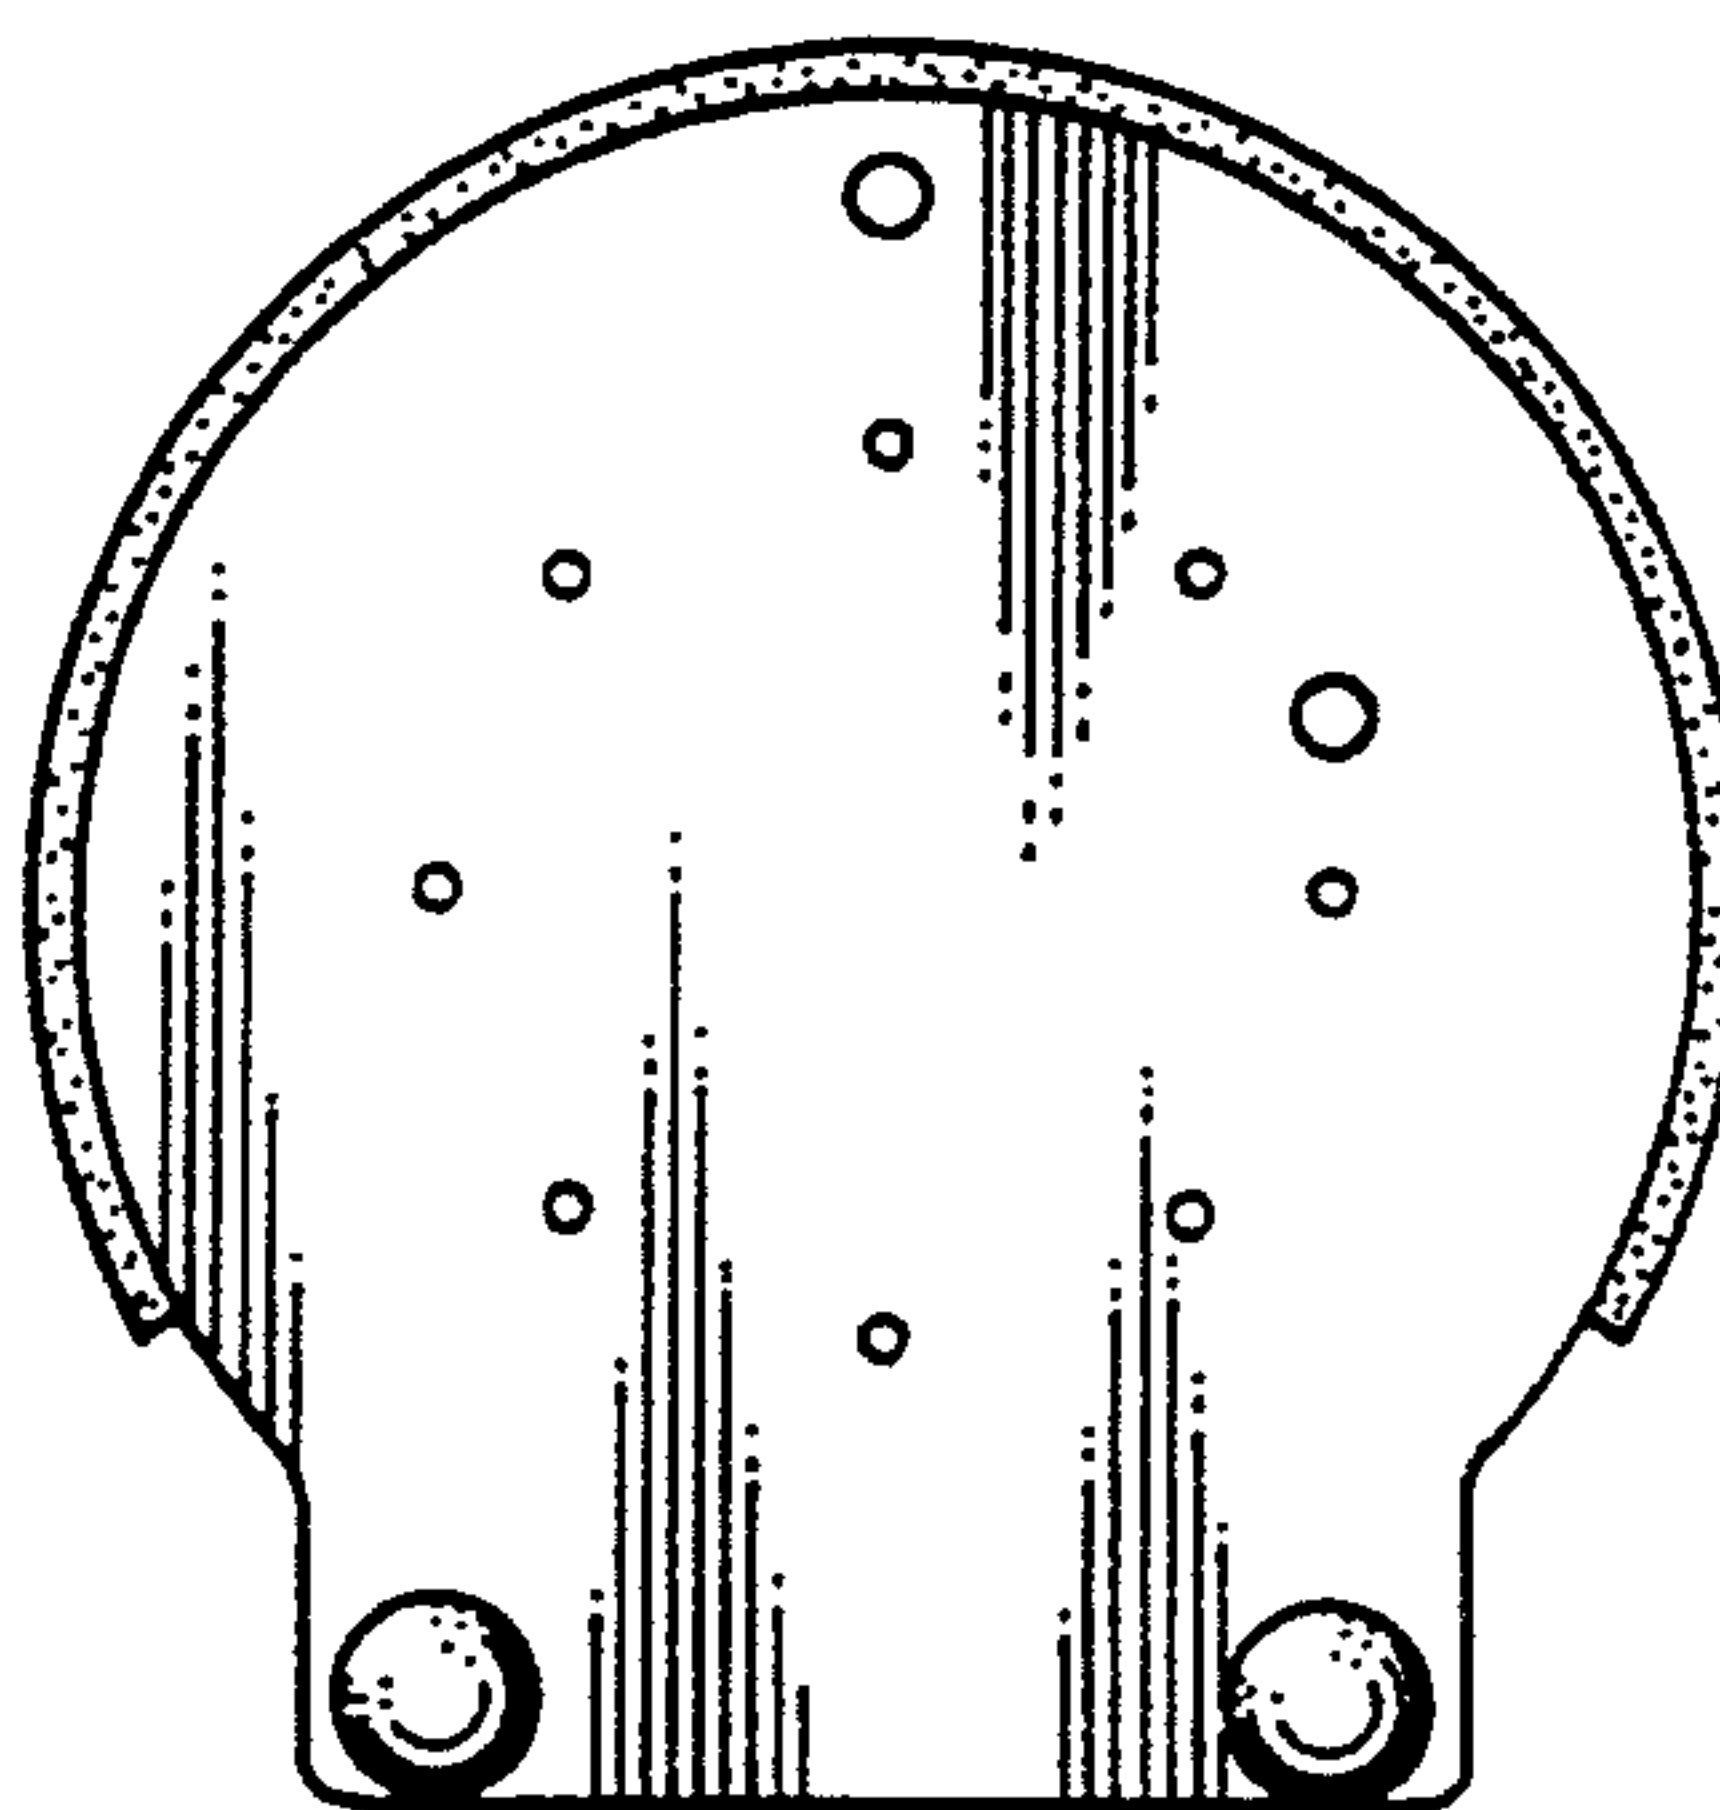


Fig. 6