



US00D355718S

**United States Patent** [19]  
**McMullen**

[11] **Patent Number: Des. 355,718**  
[45] **Date of Patent: \*\* Feb. 21, 1995**

[54] **VIDEO FLUORO IMAGING CHAIR FOR DYSPHAGIA STUDIES**

5,249,838 10/1993 Kulpa et al. .... 297/328

[75] **Inventor: Craig T. McMullen, Colorado Springs, Colo.**

*Primary Examiner—Stella Reid*  
*Attorney, Agent, or Firm—Dorr, Carson, Sloan & Peterson*

[73] **Assignee: Robert E. Giustra, Monument, Colo.**

[57] **CLAIM**

[\*\*] **Term: 14 Years**

The ornamental design for a video fluoro imaging chair for dysphagia studies, as shown and described.

[21] **Appl. No.: 14,611**

**DESCRIPTION**

[22] **Filed: Oct. 25, 1993**

[52] **U.S. Cl. .... D24/158**

[58] **Field of Search .... D24/158; 378/180, 179, 378/178, 156, 208; 297/328, 302**

FIG. 1 is a perspective view of a video fluoro imaging chair for dysphagia studies, showing my new design, the broken line showing is for illustrative purposes only and forms no part of the claimed design; FIG. 2 is a front elevational view thereof; FIG. 3 is a right side elevational view thereof, the left side elevational view being a mirror image thereto; FIG. 4 is a rear elevational view thereof; FIG. 5 is a top plan view thereof; and, FIG. 6 is a bottom plan view thereof.

[56] **References Cited**

**U.S. PATENT DOCUMENTS**

3,655,968 4/1972 Moore et al. .... 378/178  
4,464,780 8/1984 Ruiz ..... 378/178



Fig. 1



Fig. 3

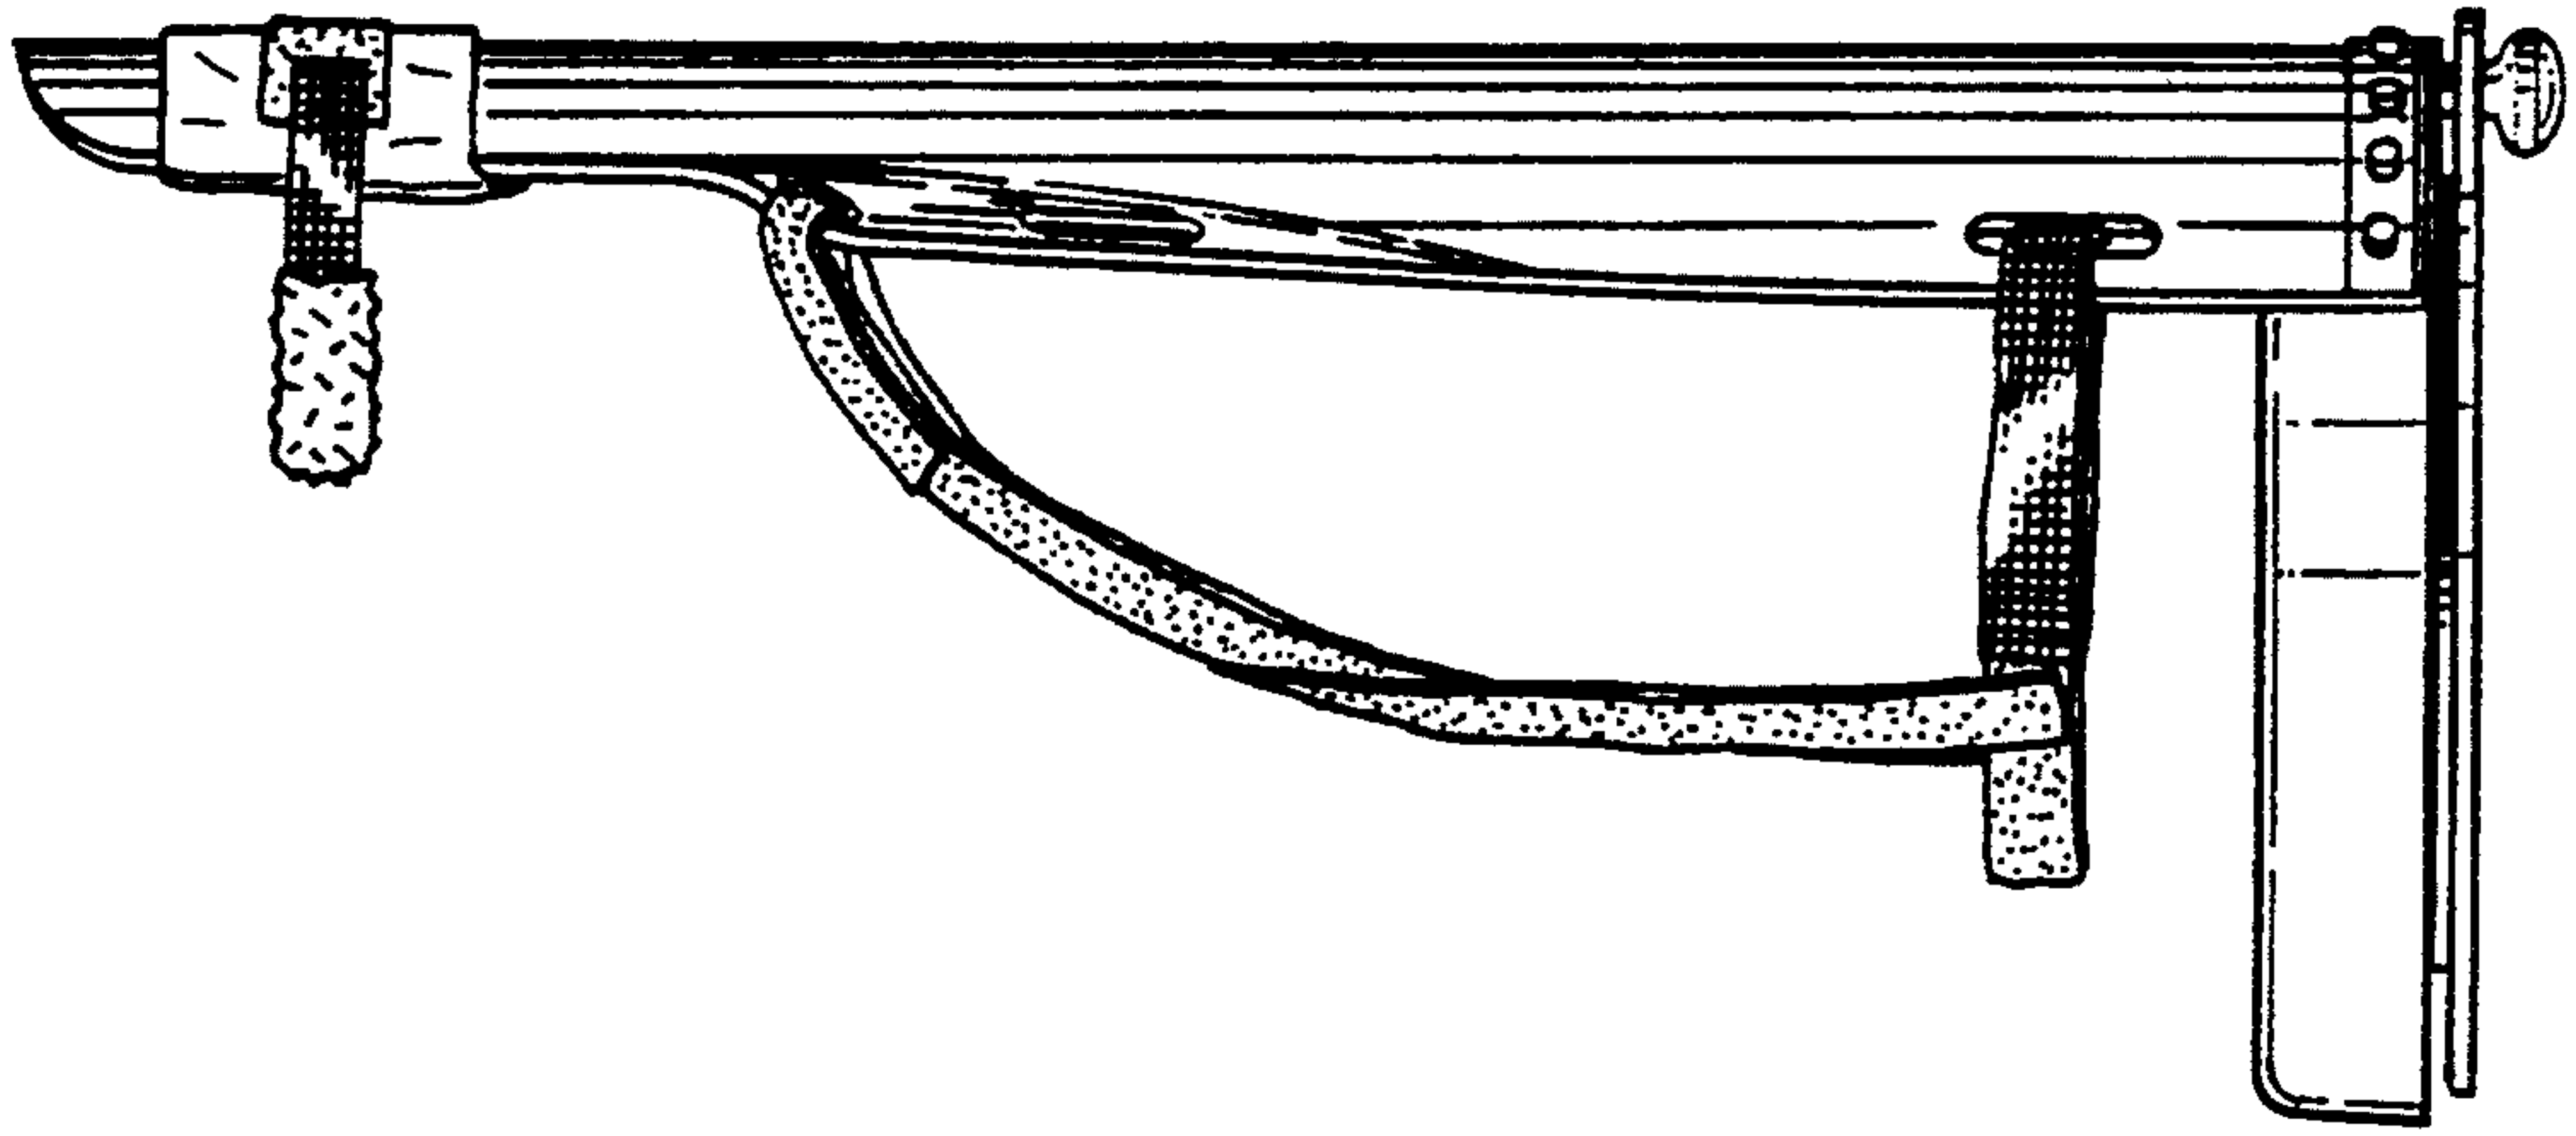


Fig. 2

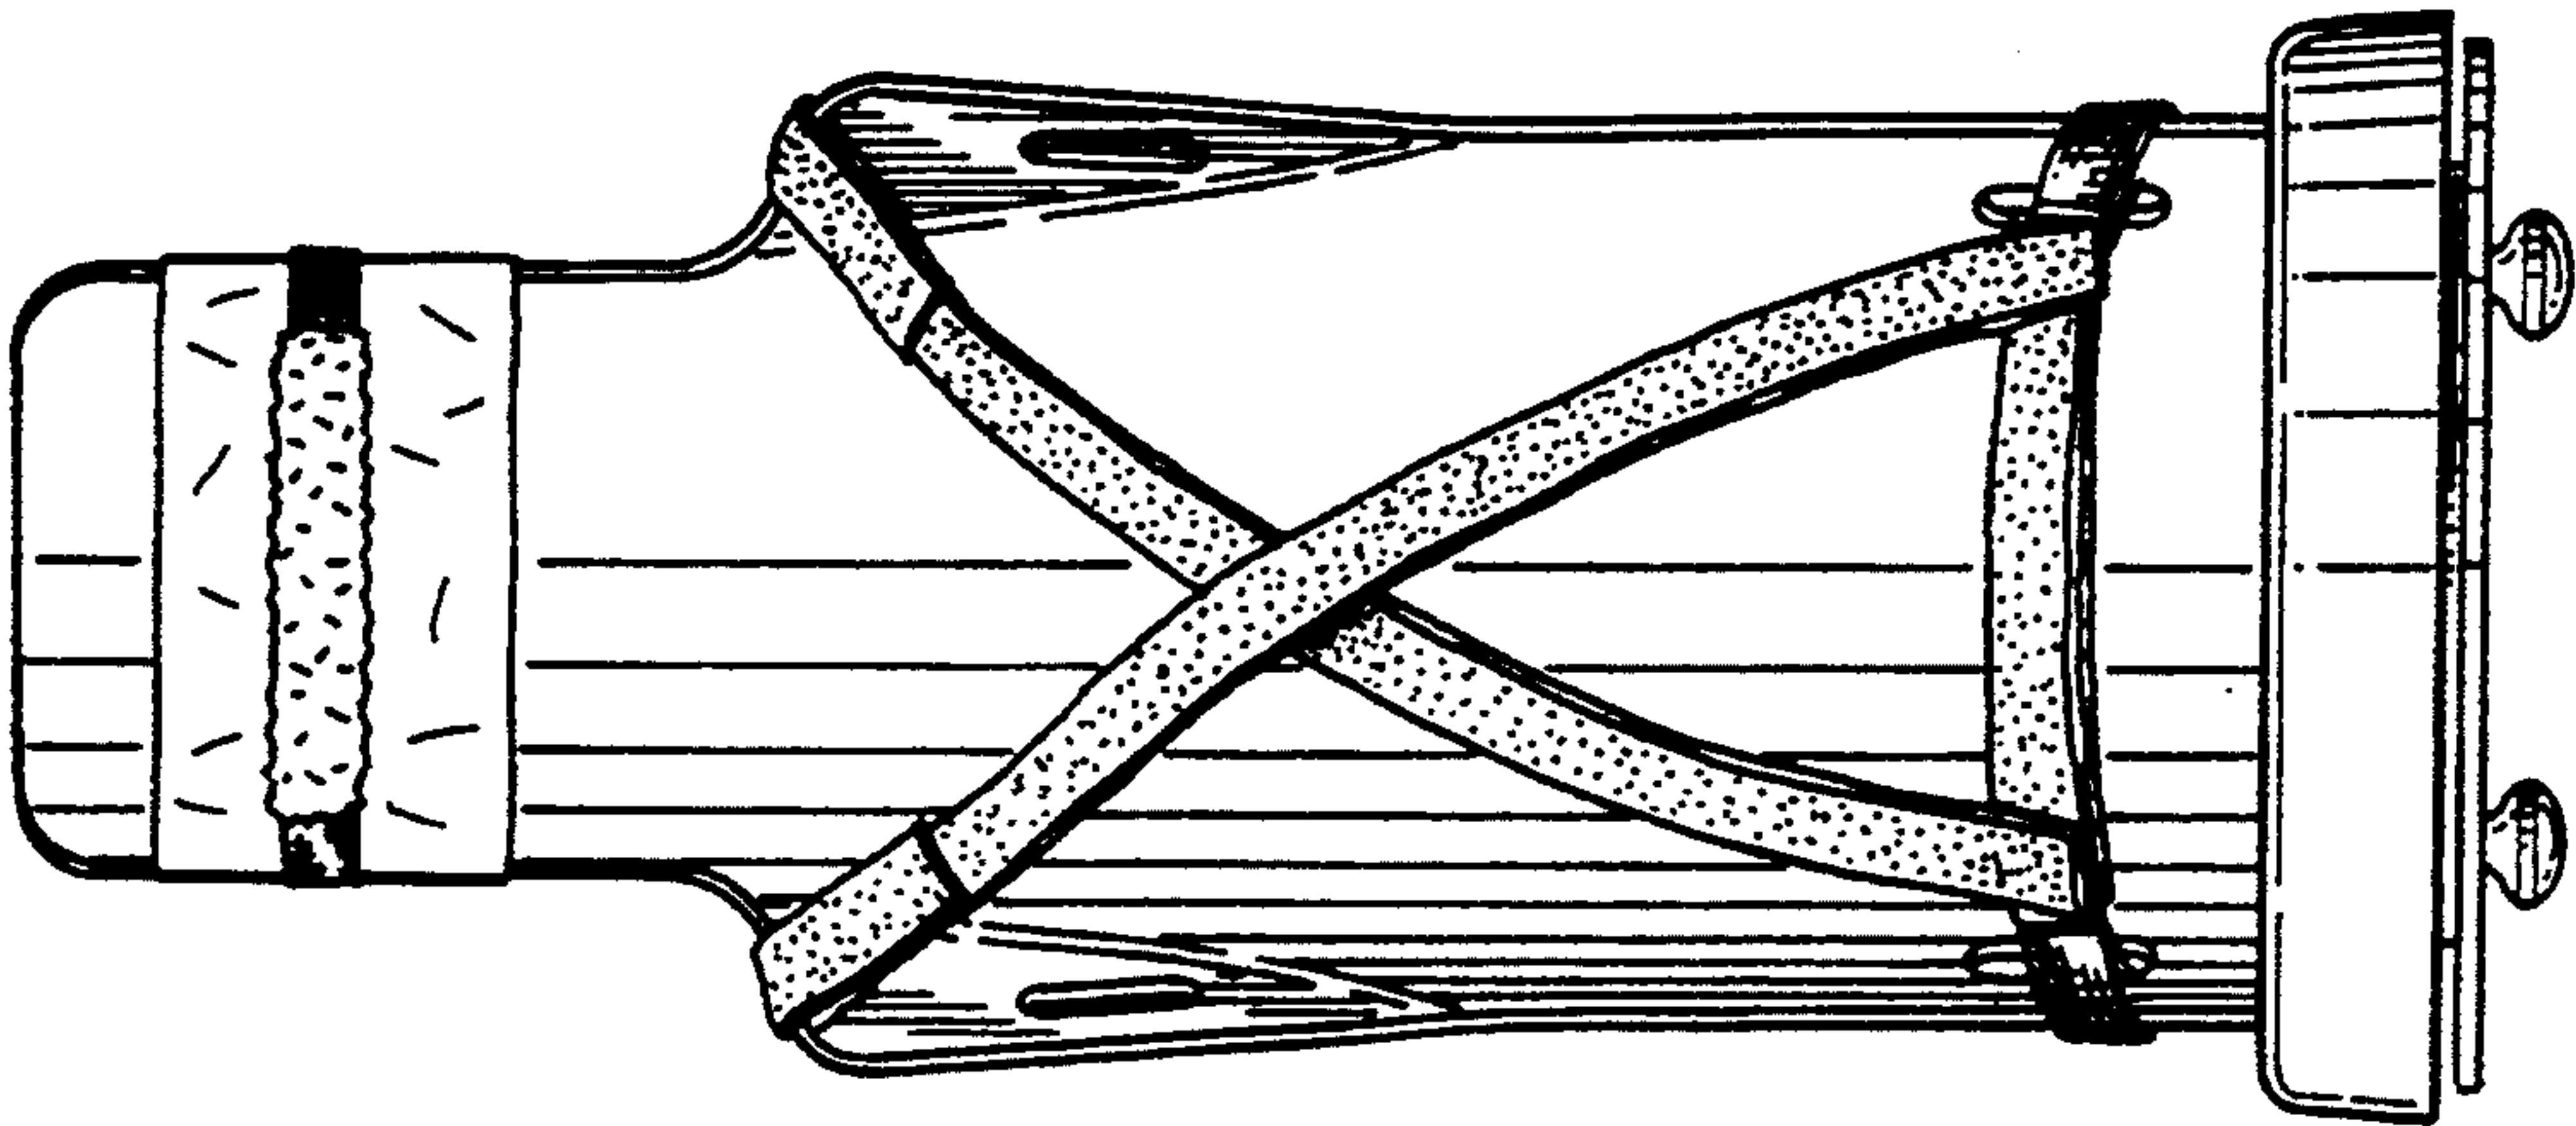


Fig. 4

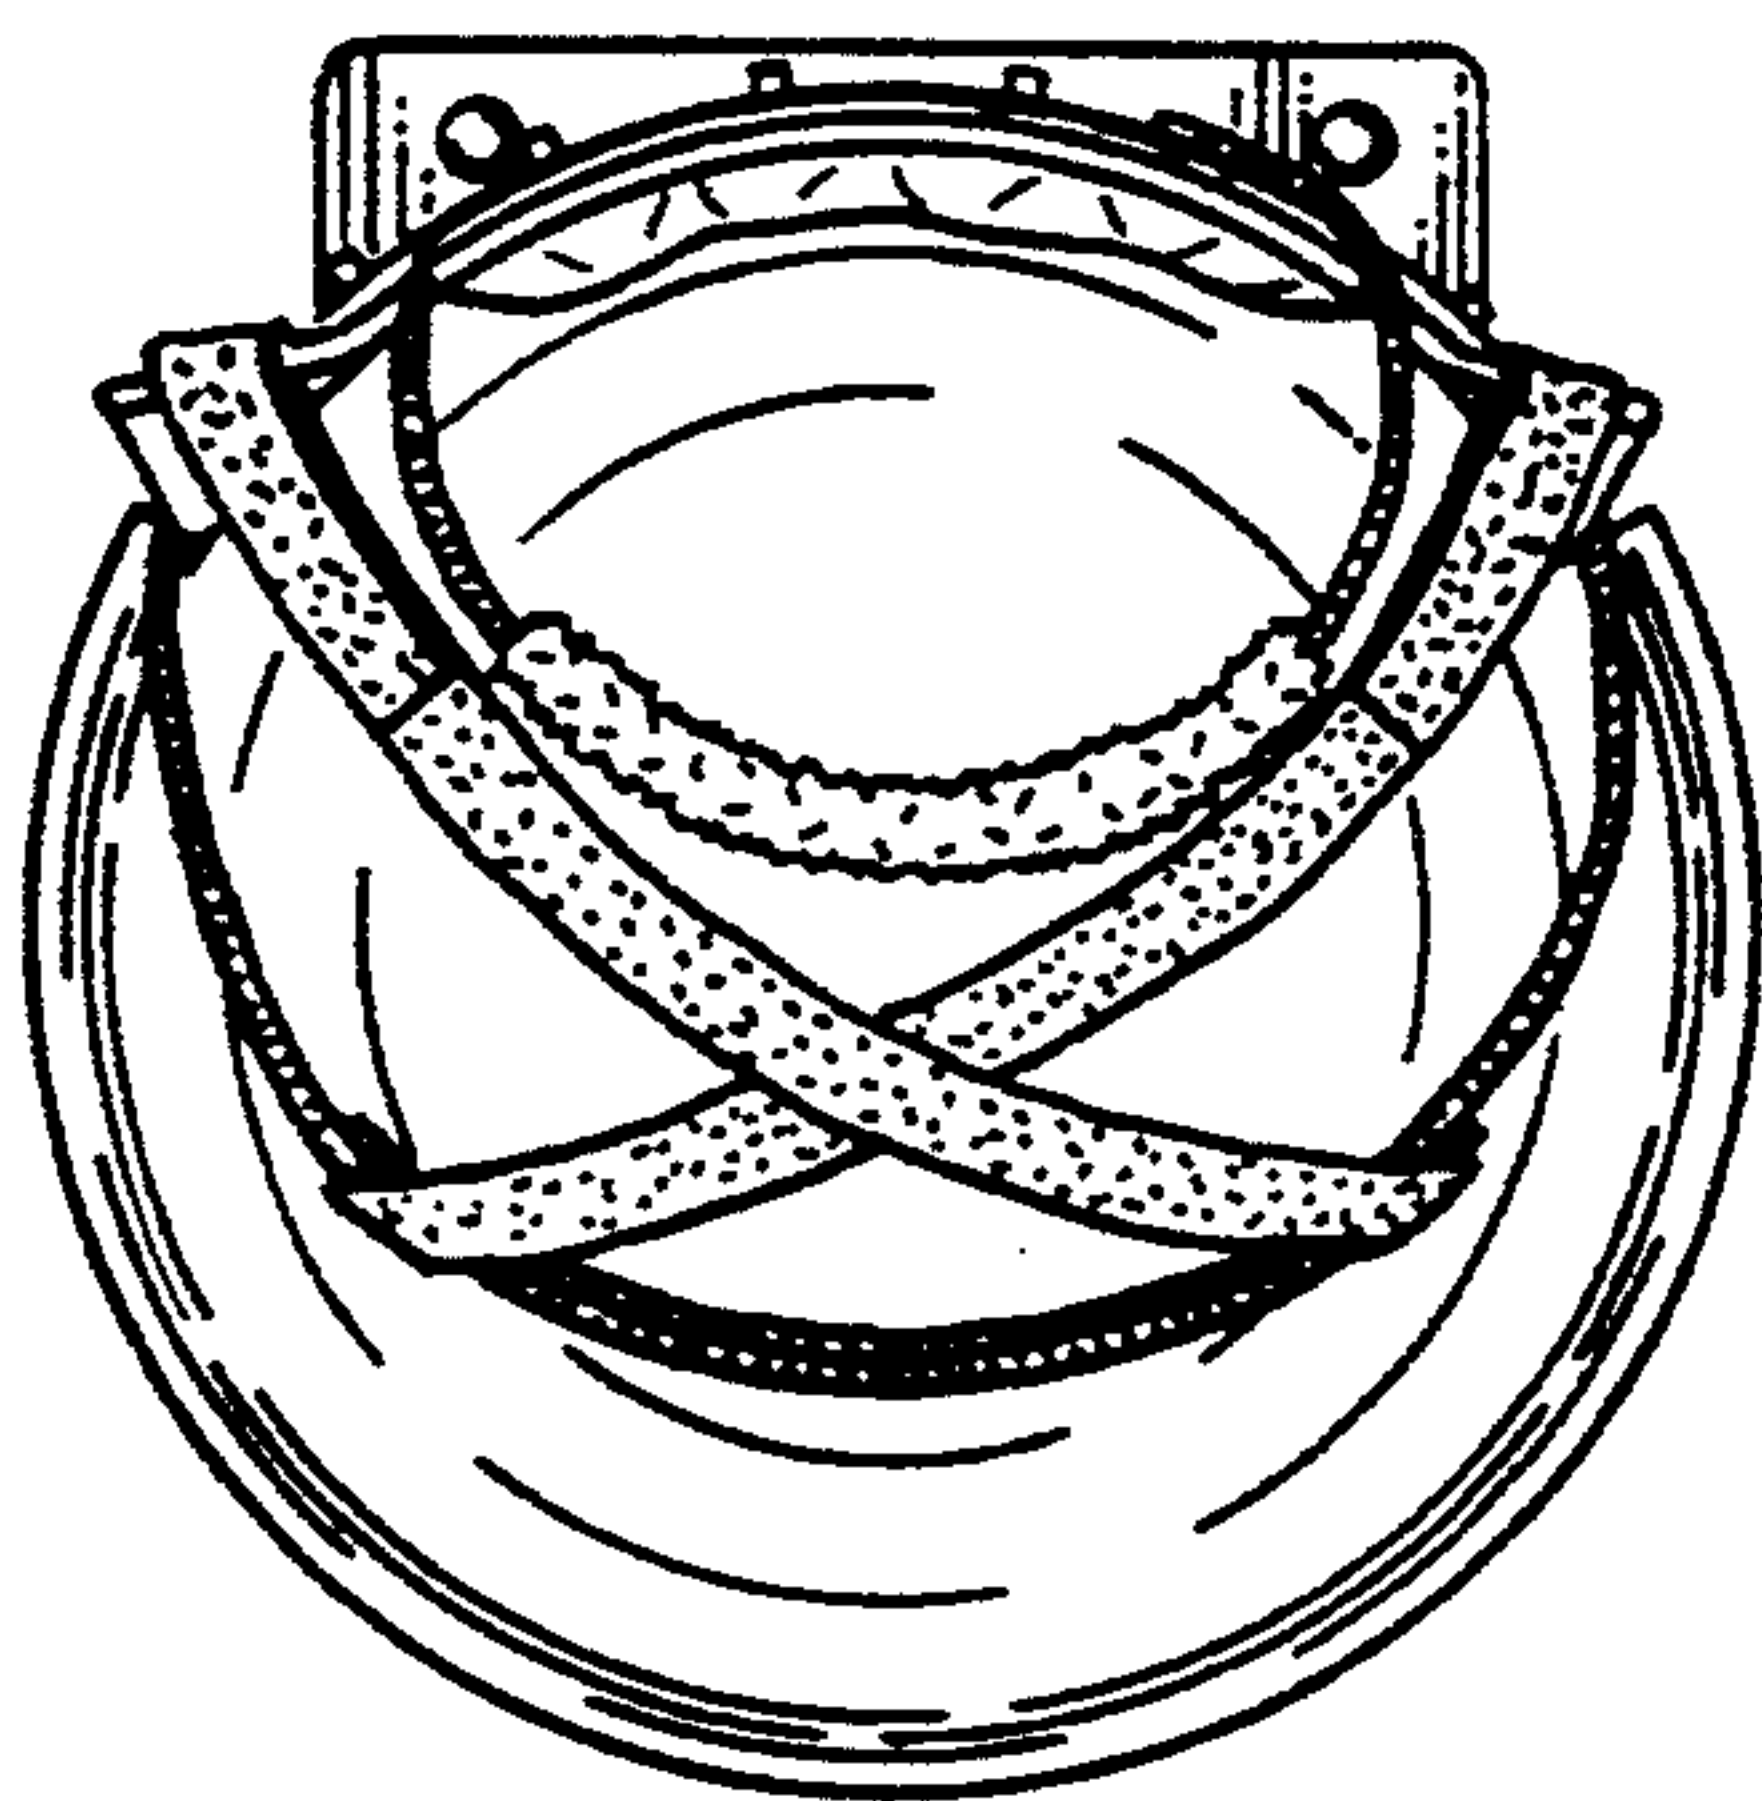
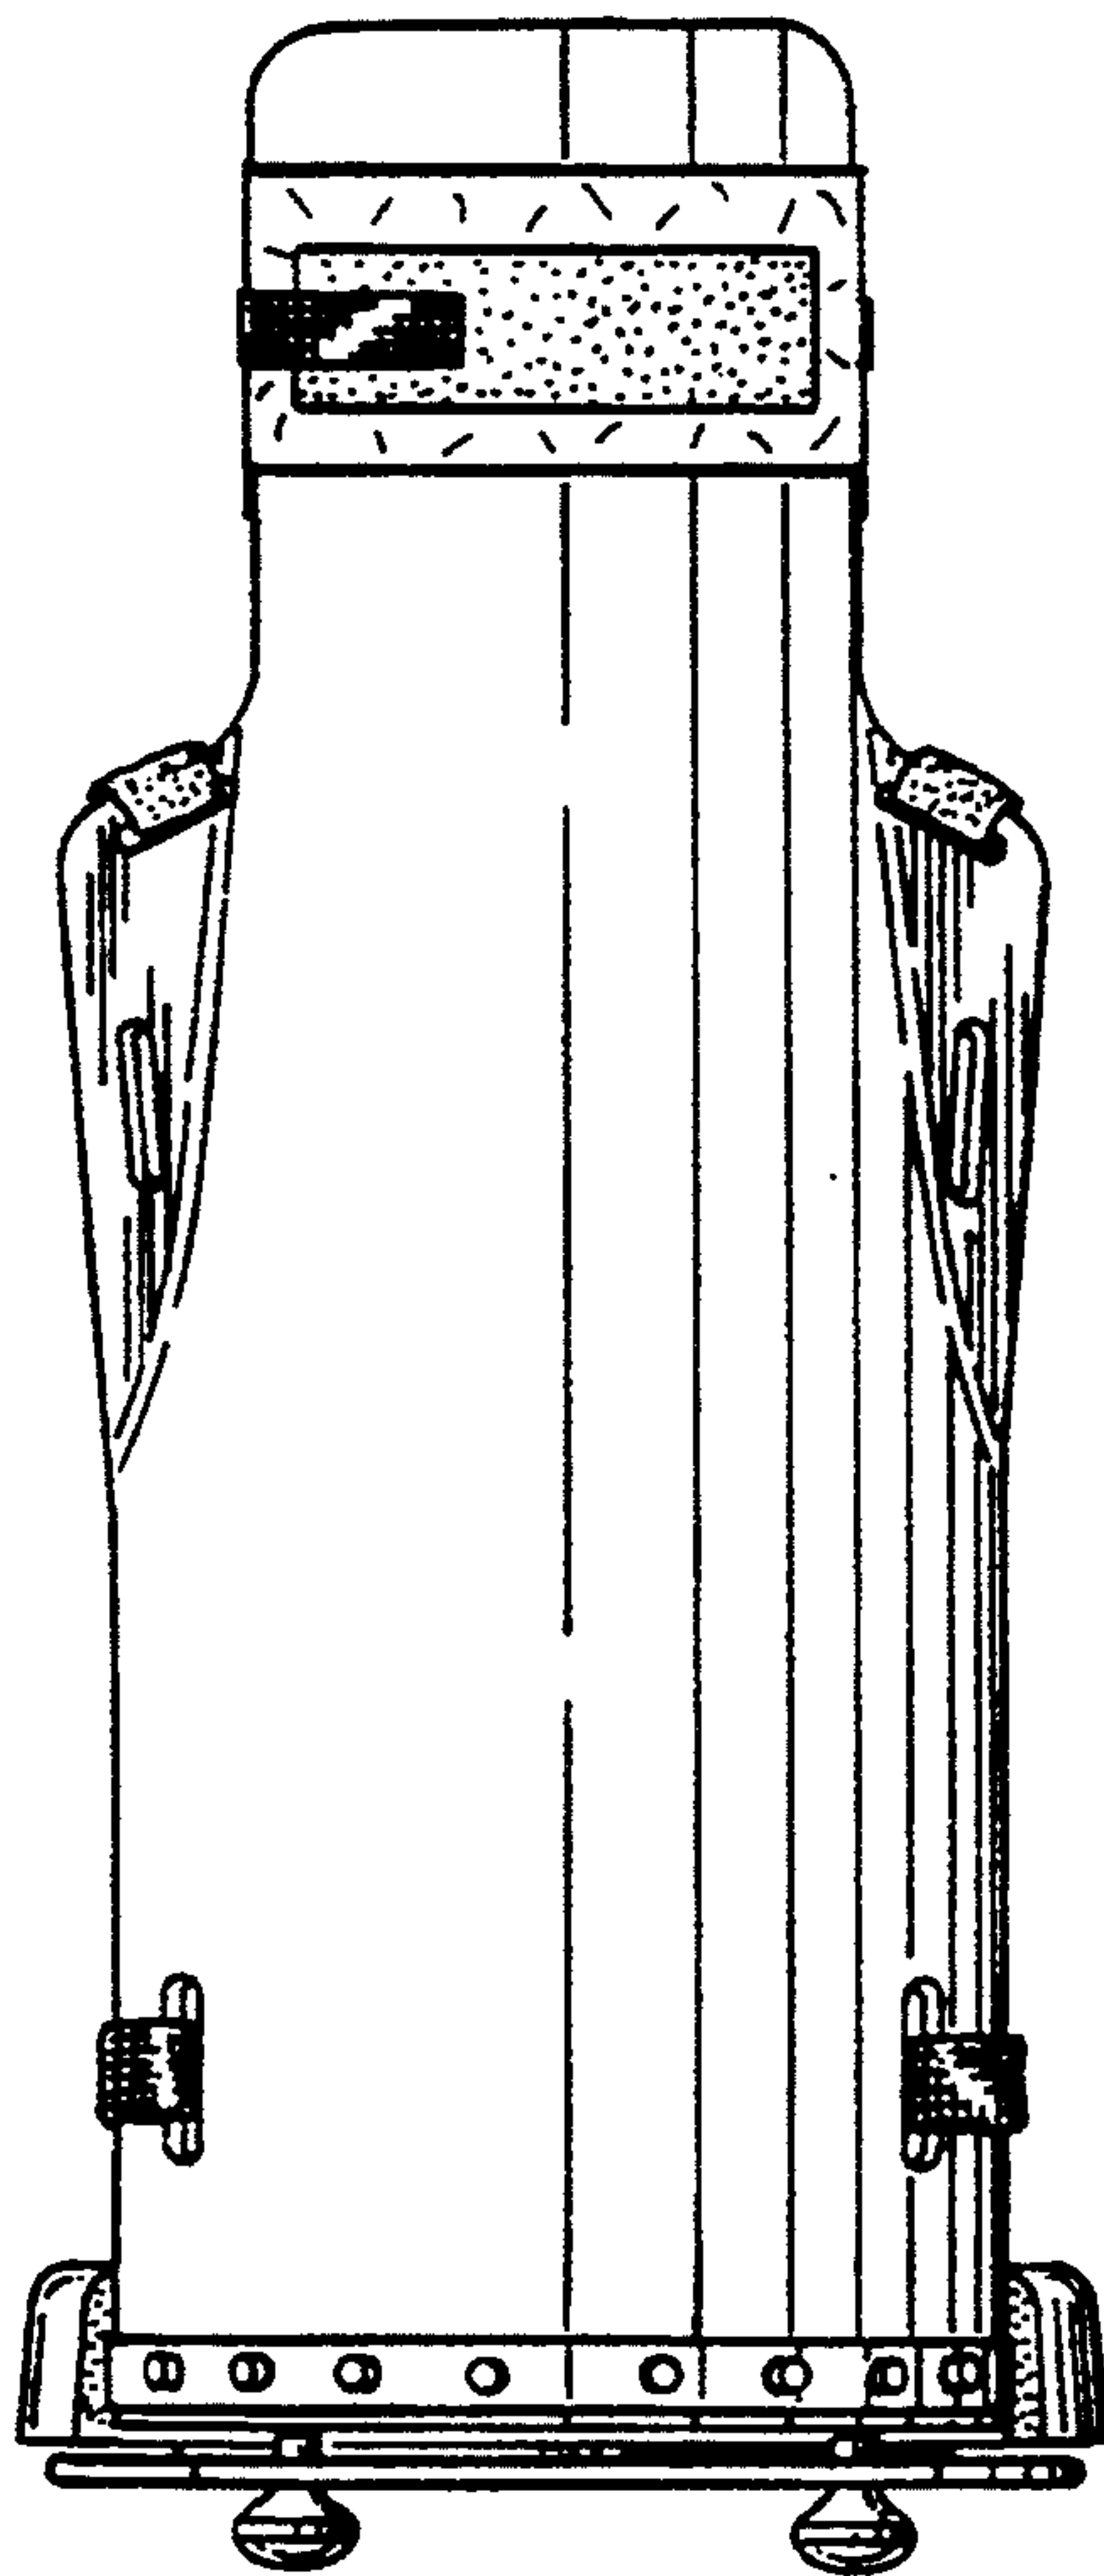


Fig. 5

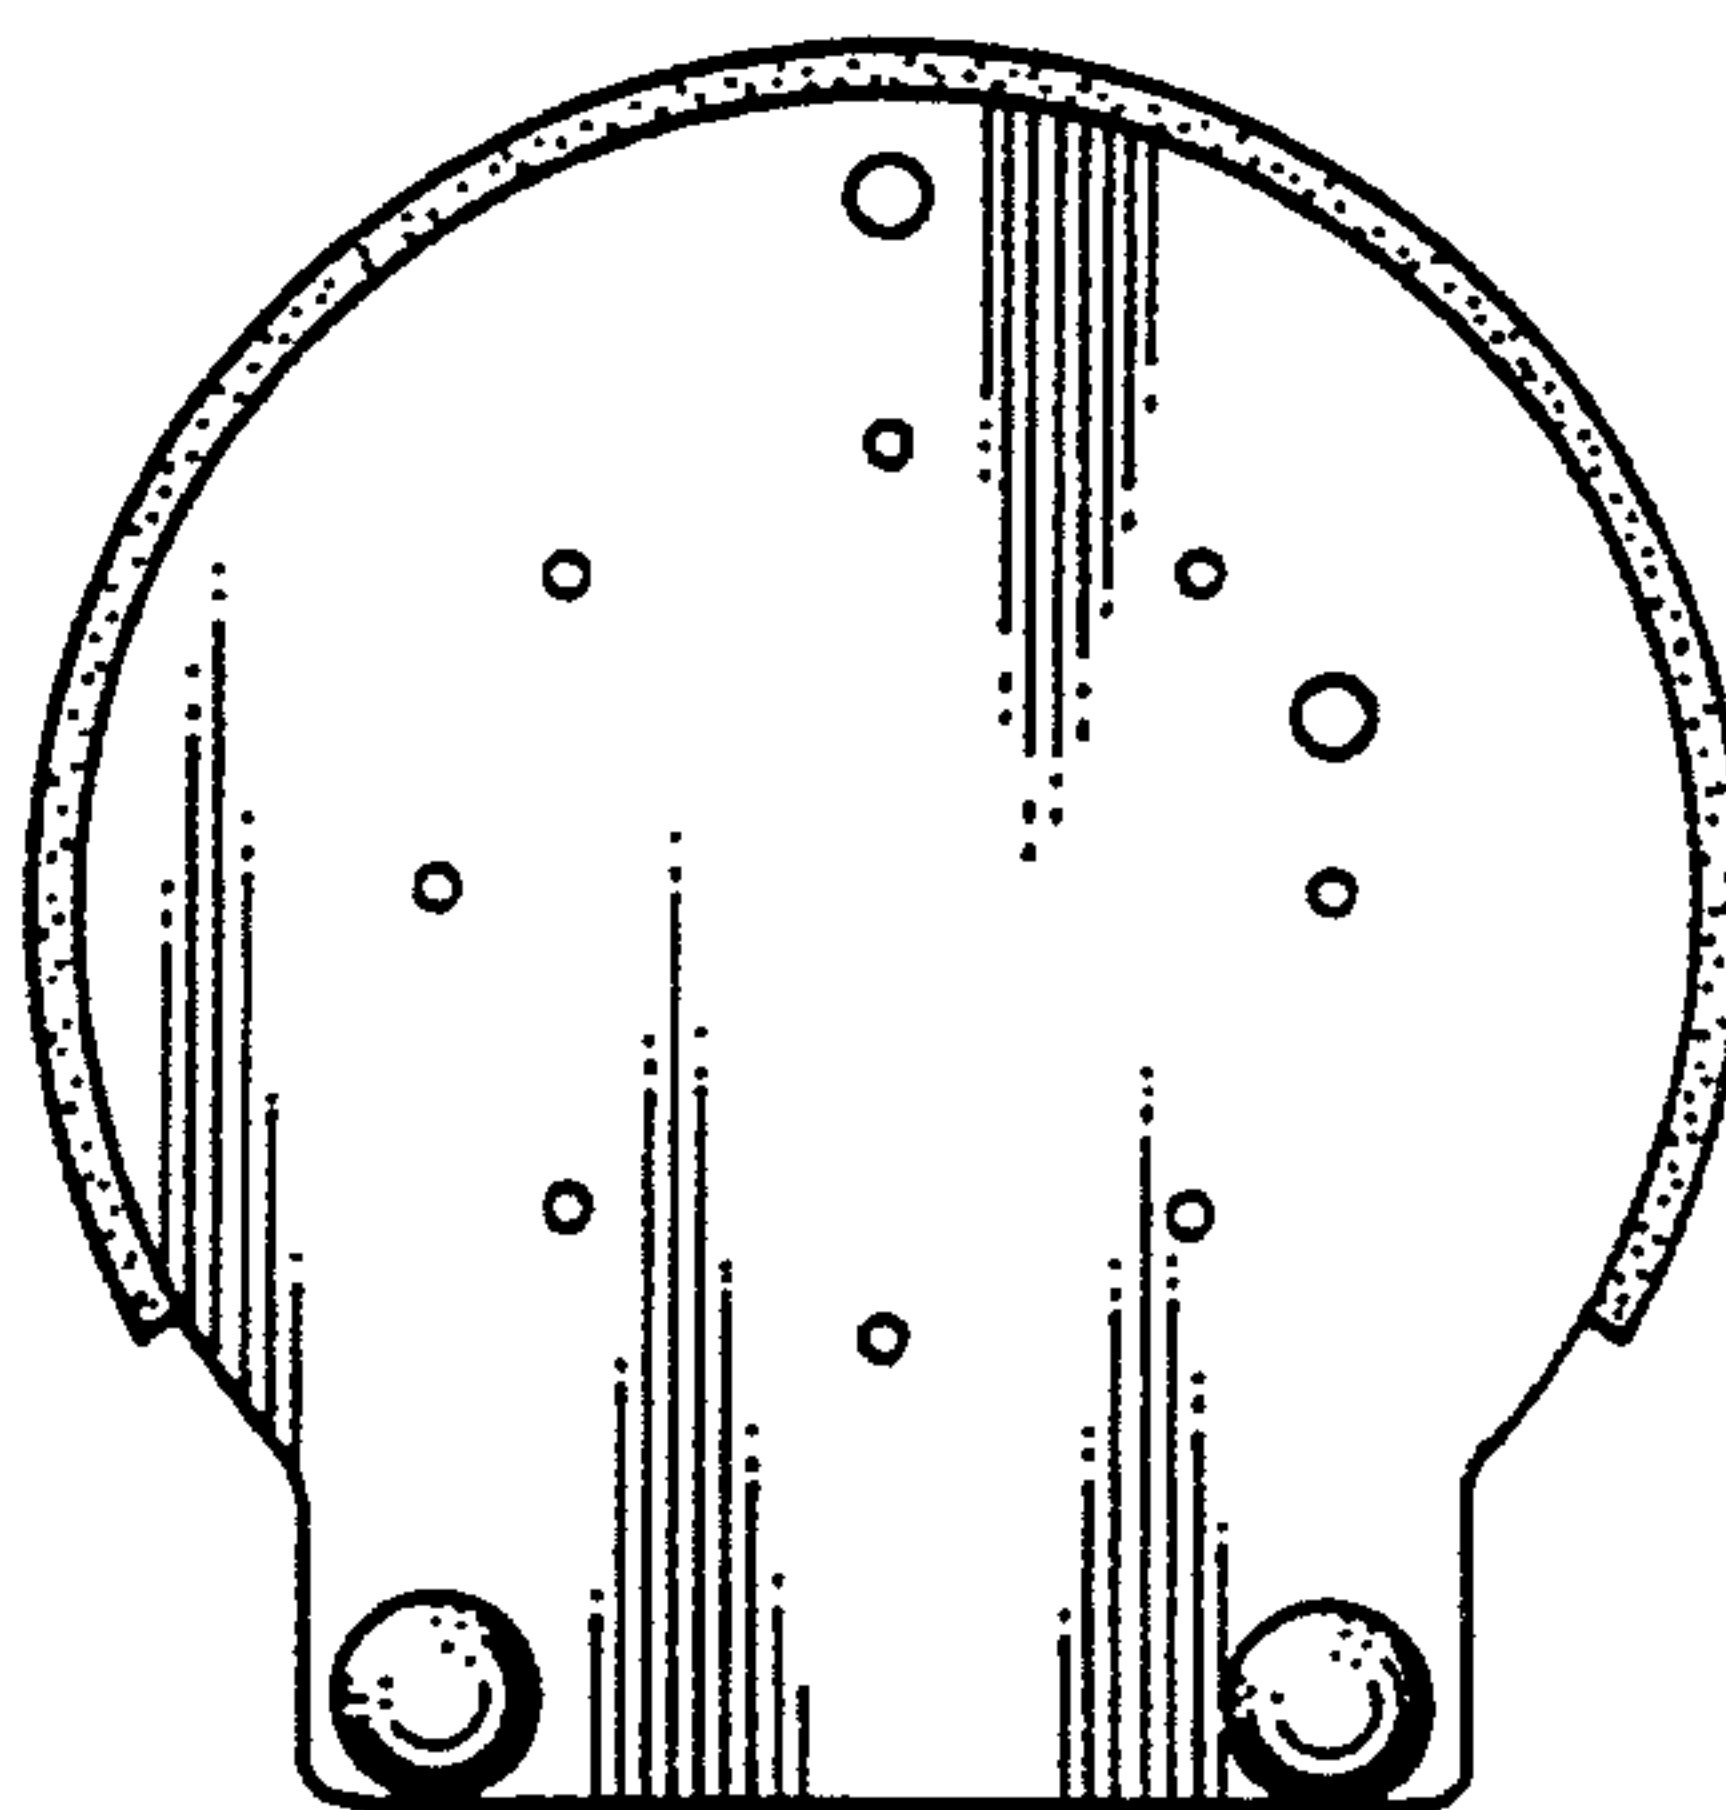


Fig. 6