



US00D356870S

# United States Patent [19]

[11] Patent Number: **Des. 356,870**

Ivers et al.

[45] Date of Patent: **\*\* Mar. 28, 1995**

[54] **PULSE OXIMETRY SENSOR**

[75] Inventors: **David L. Ivers, Jupiter; Stanley R. Mach, Palm Beach Gardens, both of Fla.**

[73] Assignee: **Marquette Electronics, Inc., Milwaukee, Wis.**

[\*\*] Term: **14 Years**

[21] Appl. No.: **8,884**

[22] Filed: **May 26, 1993**

[52] U.S. Cl. .... **D24/164**

[58] Field of Search ..... **D24/165, 167, 169; 128/633, 632**

4,964,408 10/1990 Hink et al. .... 128/633  
 5,035,243 7/1991 Muz ..... 128/633  
 5,080,098 1/1992 Willett et al. .... 128/633  
 5,249,576 10/1993 Goldberger et al. .... 128/632

*Primary Examiner*—Stella Reid  
*Attorney, Agent, or Firm*—Michael, Best & Friedrich

### [57] CLAIM

The ornamental design for a pulse oximetry sensor, as shown and described.


### DESCRIPTION

FIG. 1 is a perspective view of a pulse oximetry sensor illustrating our invention;  
 FIG. 2 is a right side view thereof, the left side being a mirror image of the right side;  
 FIG. 3 is a front view thereof;  
 FIG. 4 is a rear view thereof;  
 FIG. 5 is a top view thereof;  
 FIG. 6 is a bottom view thereof;  
 FIG. 7 is a perspective view of an alternate embodiment of the invention which is identical in all respects to the embodiment of FIGS. 1-6 except for the front end; and,  
 FIG. 8 is a bottom view of the embodiment of FIG. 7.

### [56] References Cited

#### U.S. PATENT DOCUMENTS

D. 326,715	6/1992	Schmidt .....	D24/164
4,685,464	8/1987	Goldberger et al. ....	128/633
4,825,879	5/1989	Tan et al. ....	128/633
4,867,165	9/1989	Noller et al. ....	128/633
4,883,055	11/1989	Merrick .....	128/633
4,913,150	4/1990	Cheung et al. ....	128/633

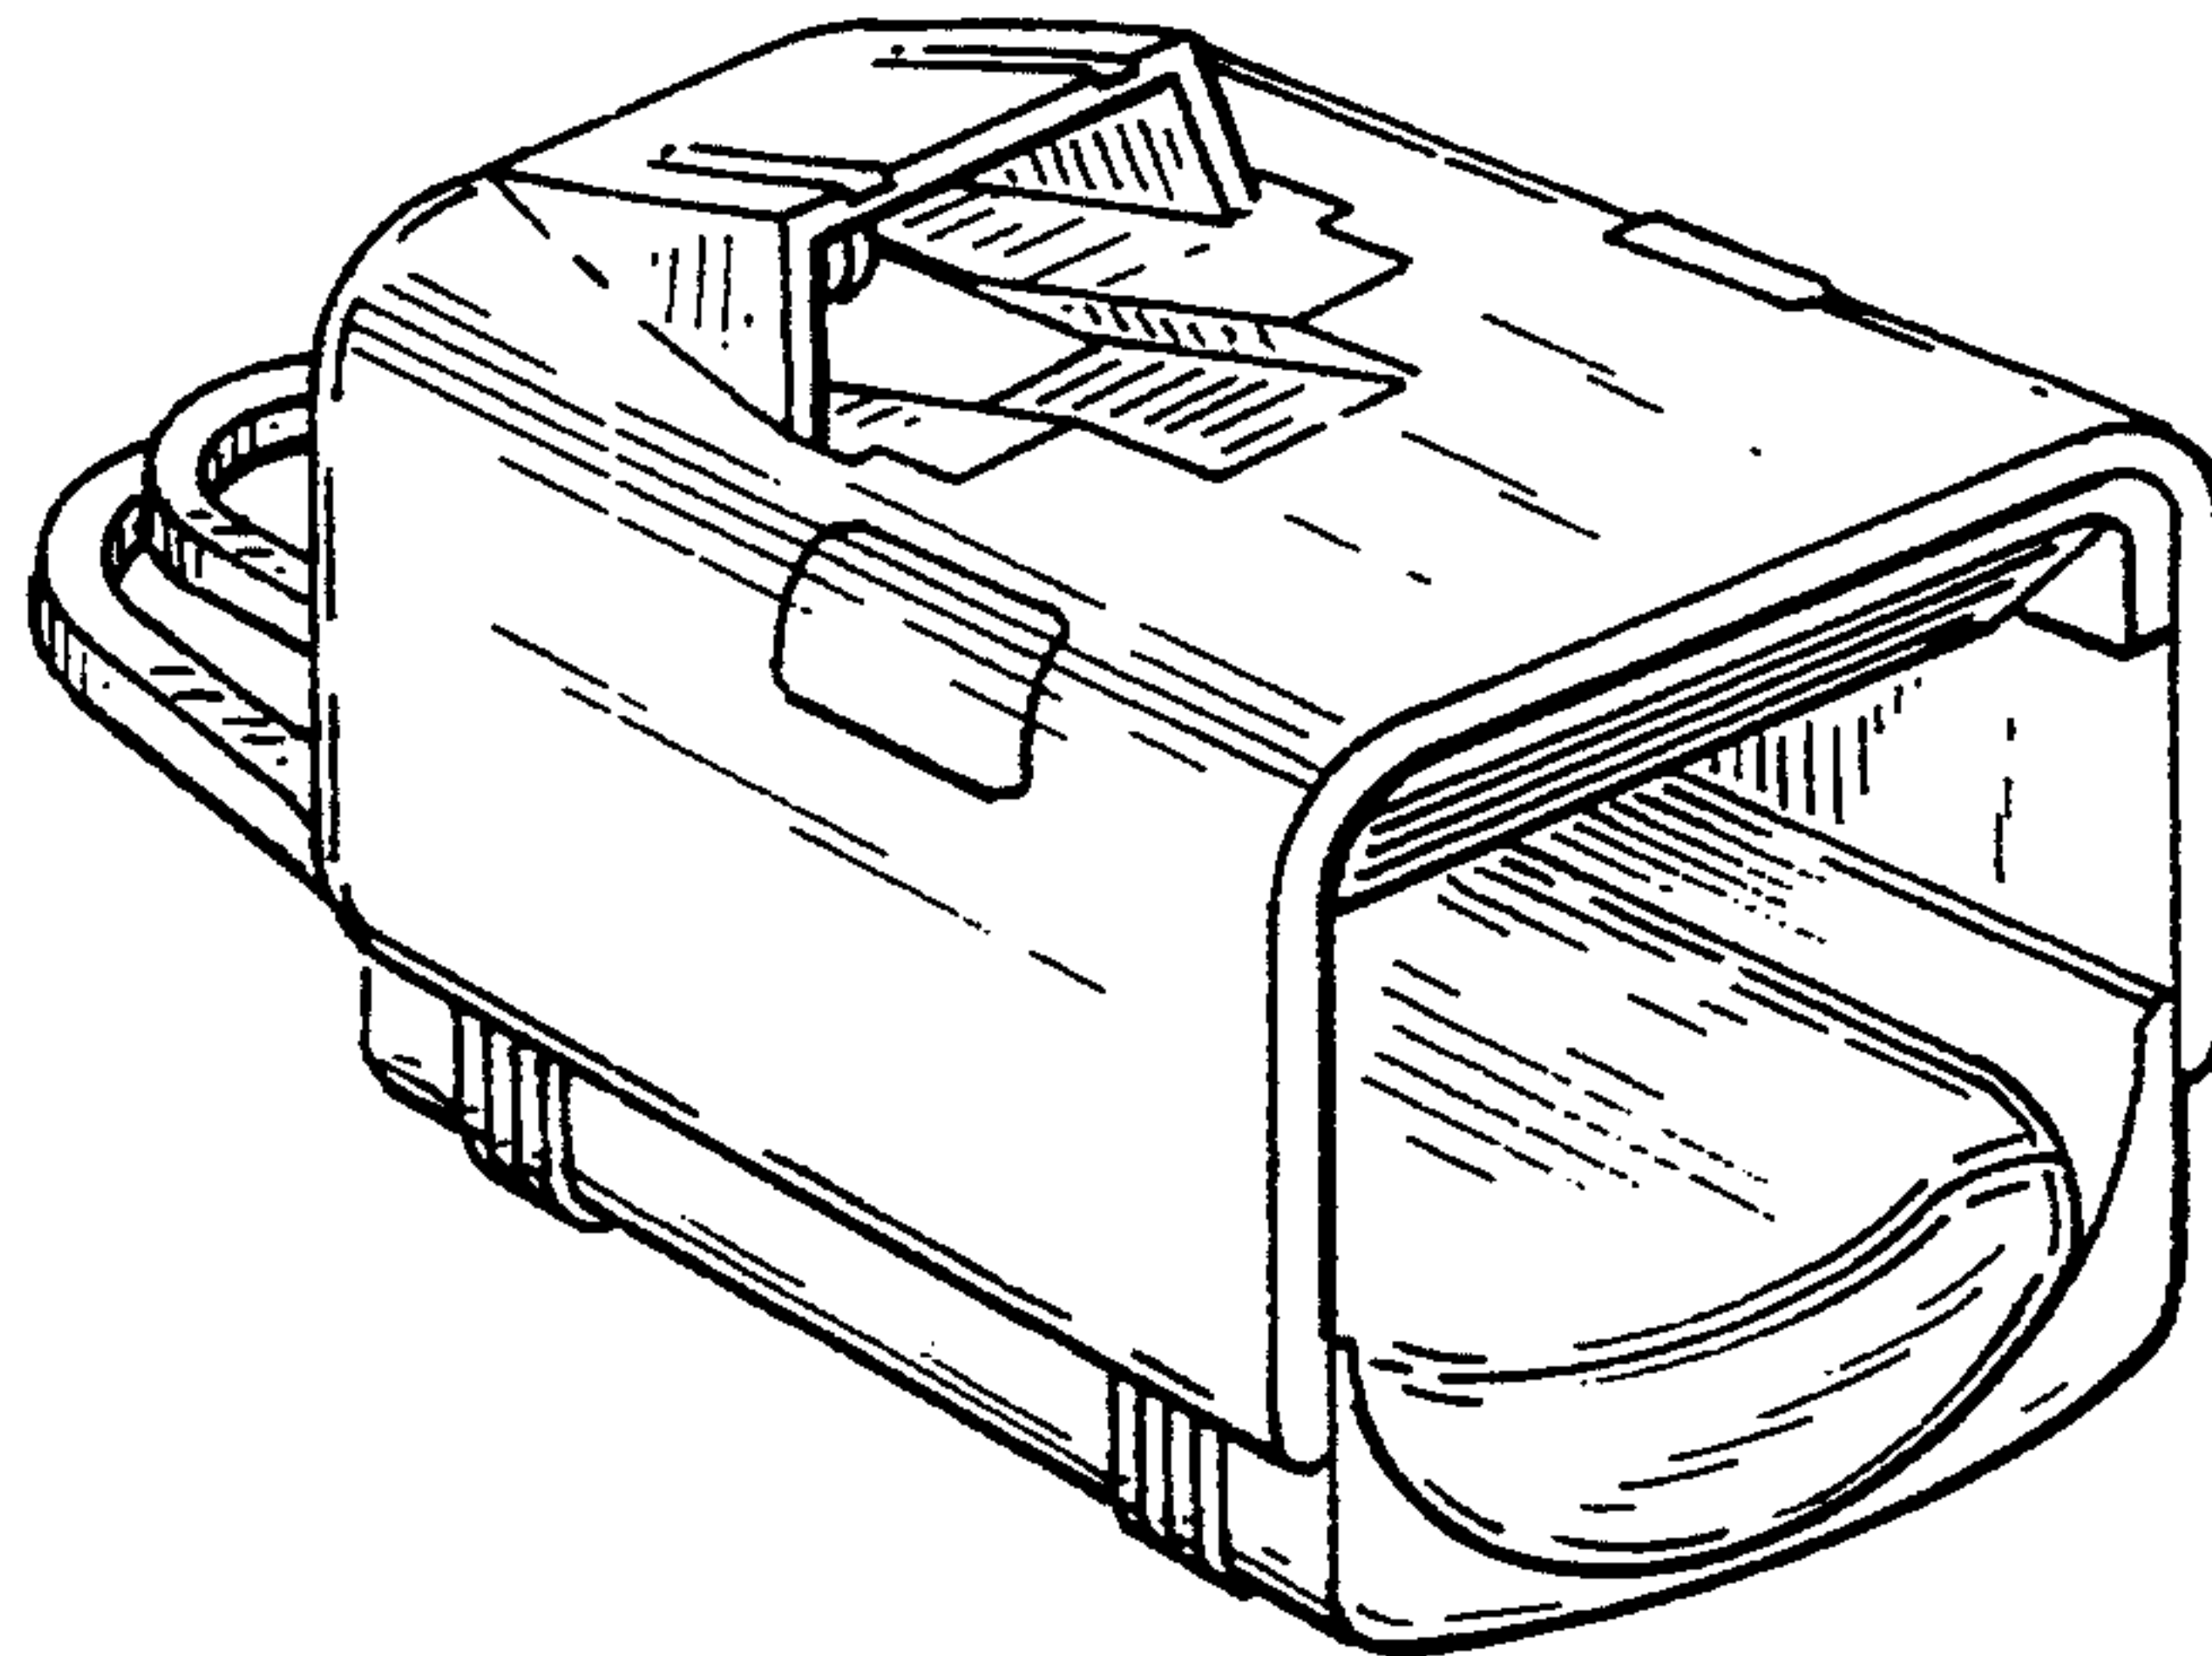

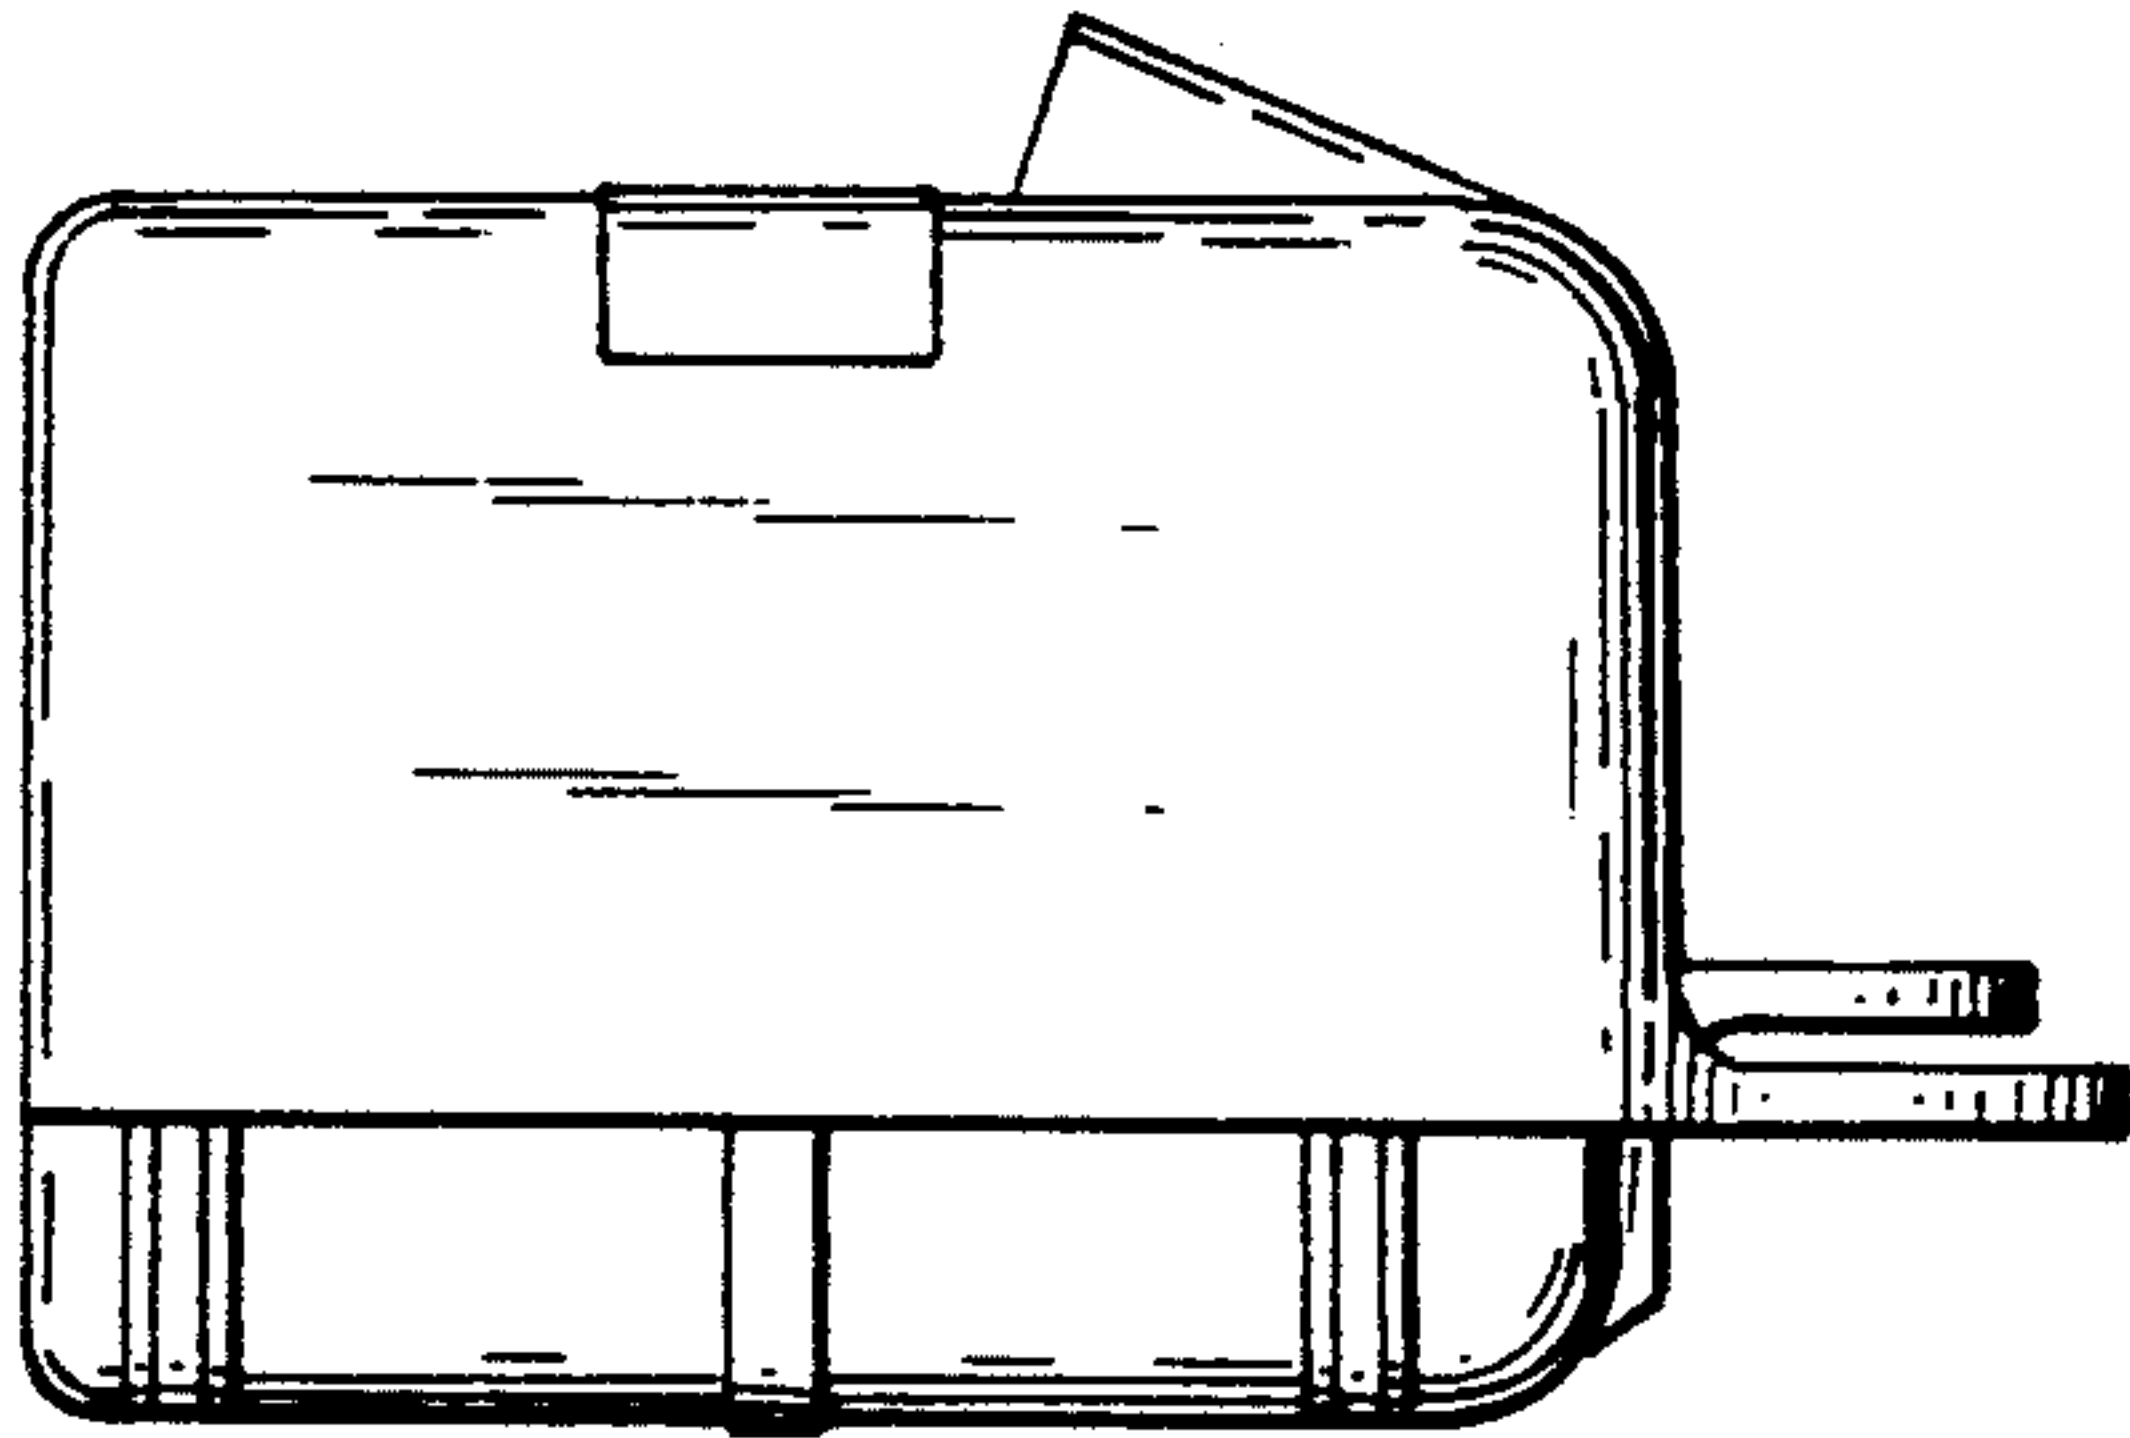
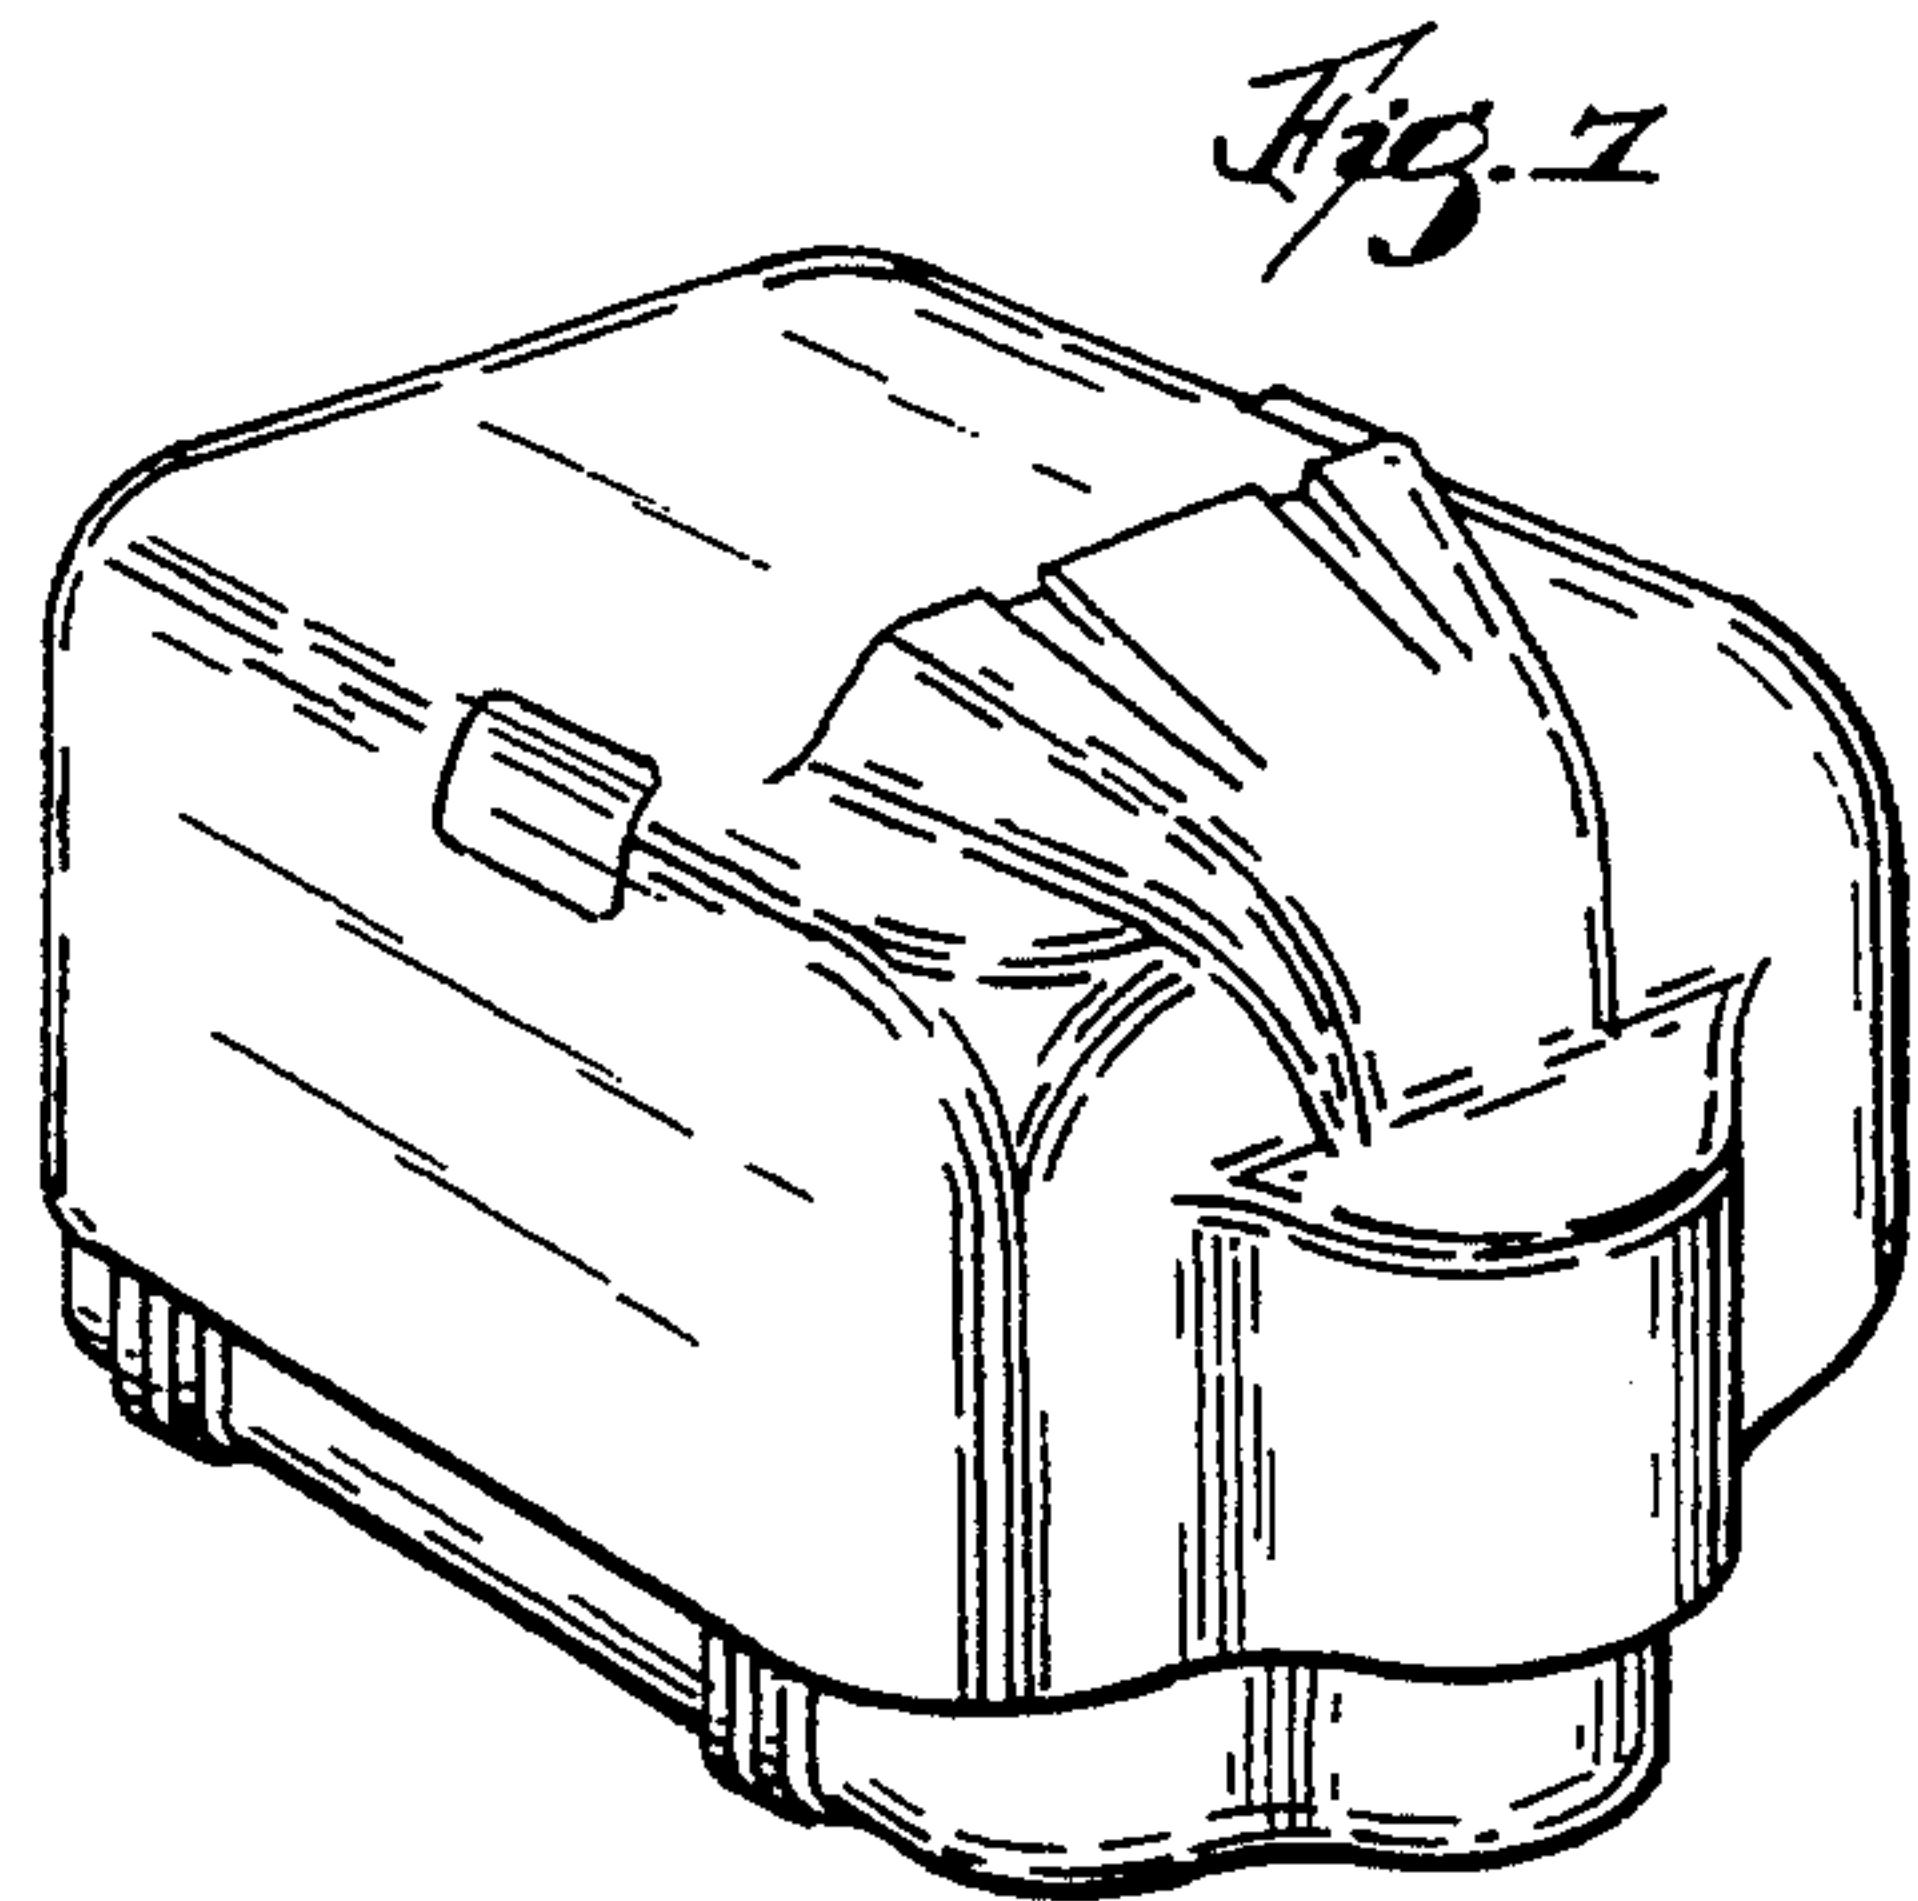
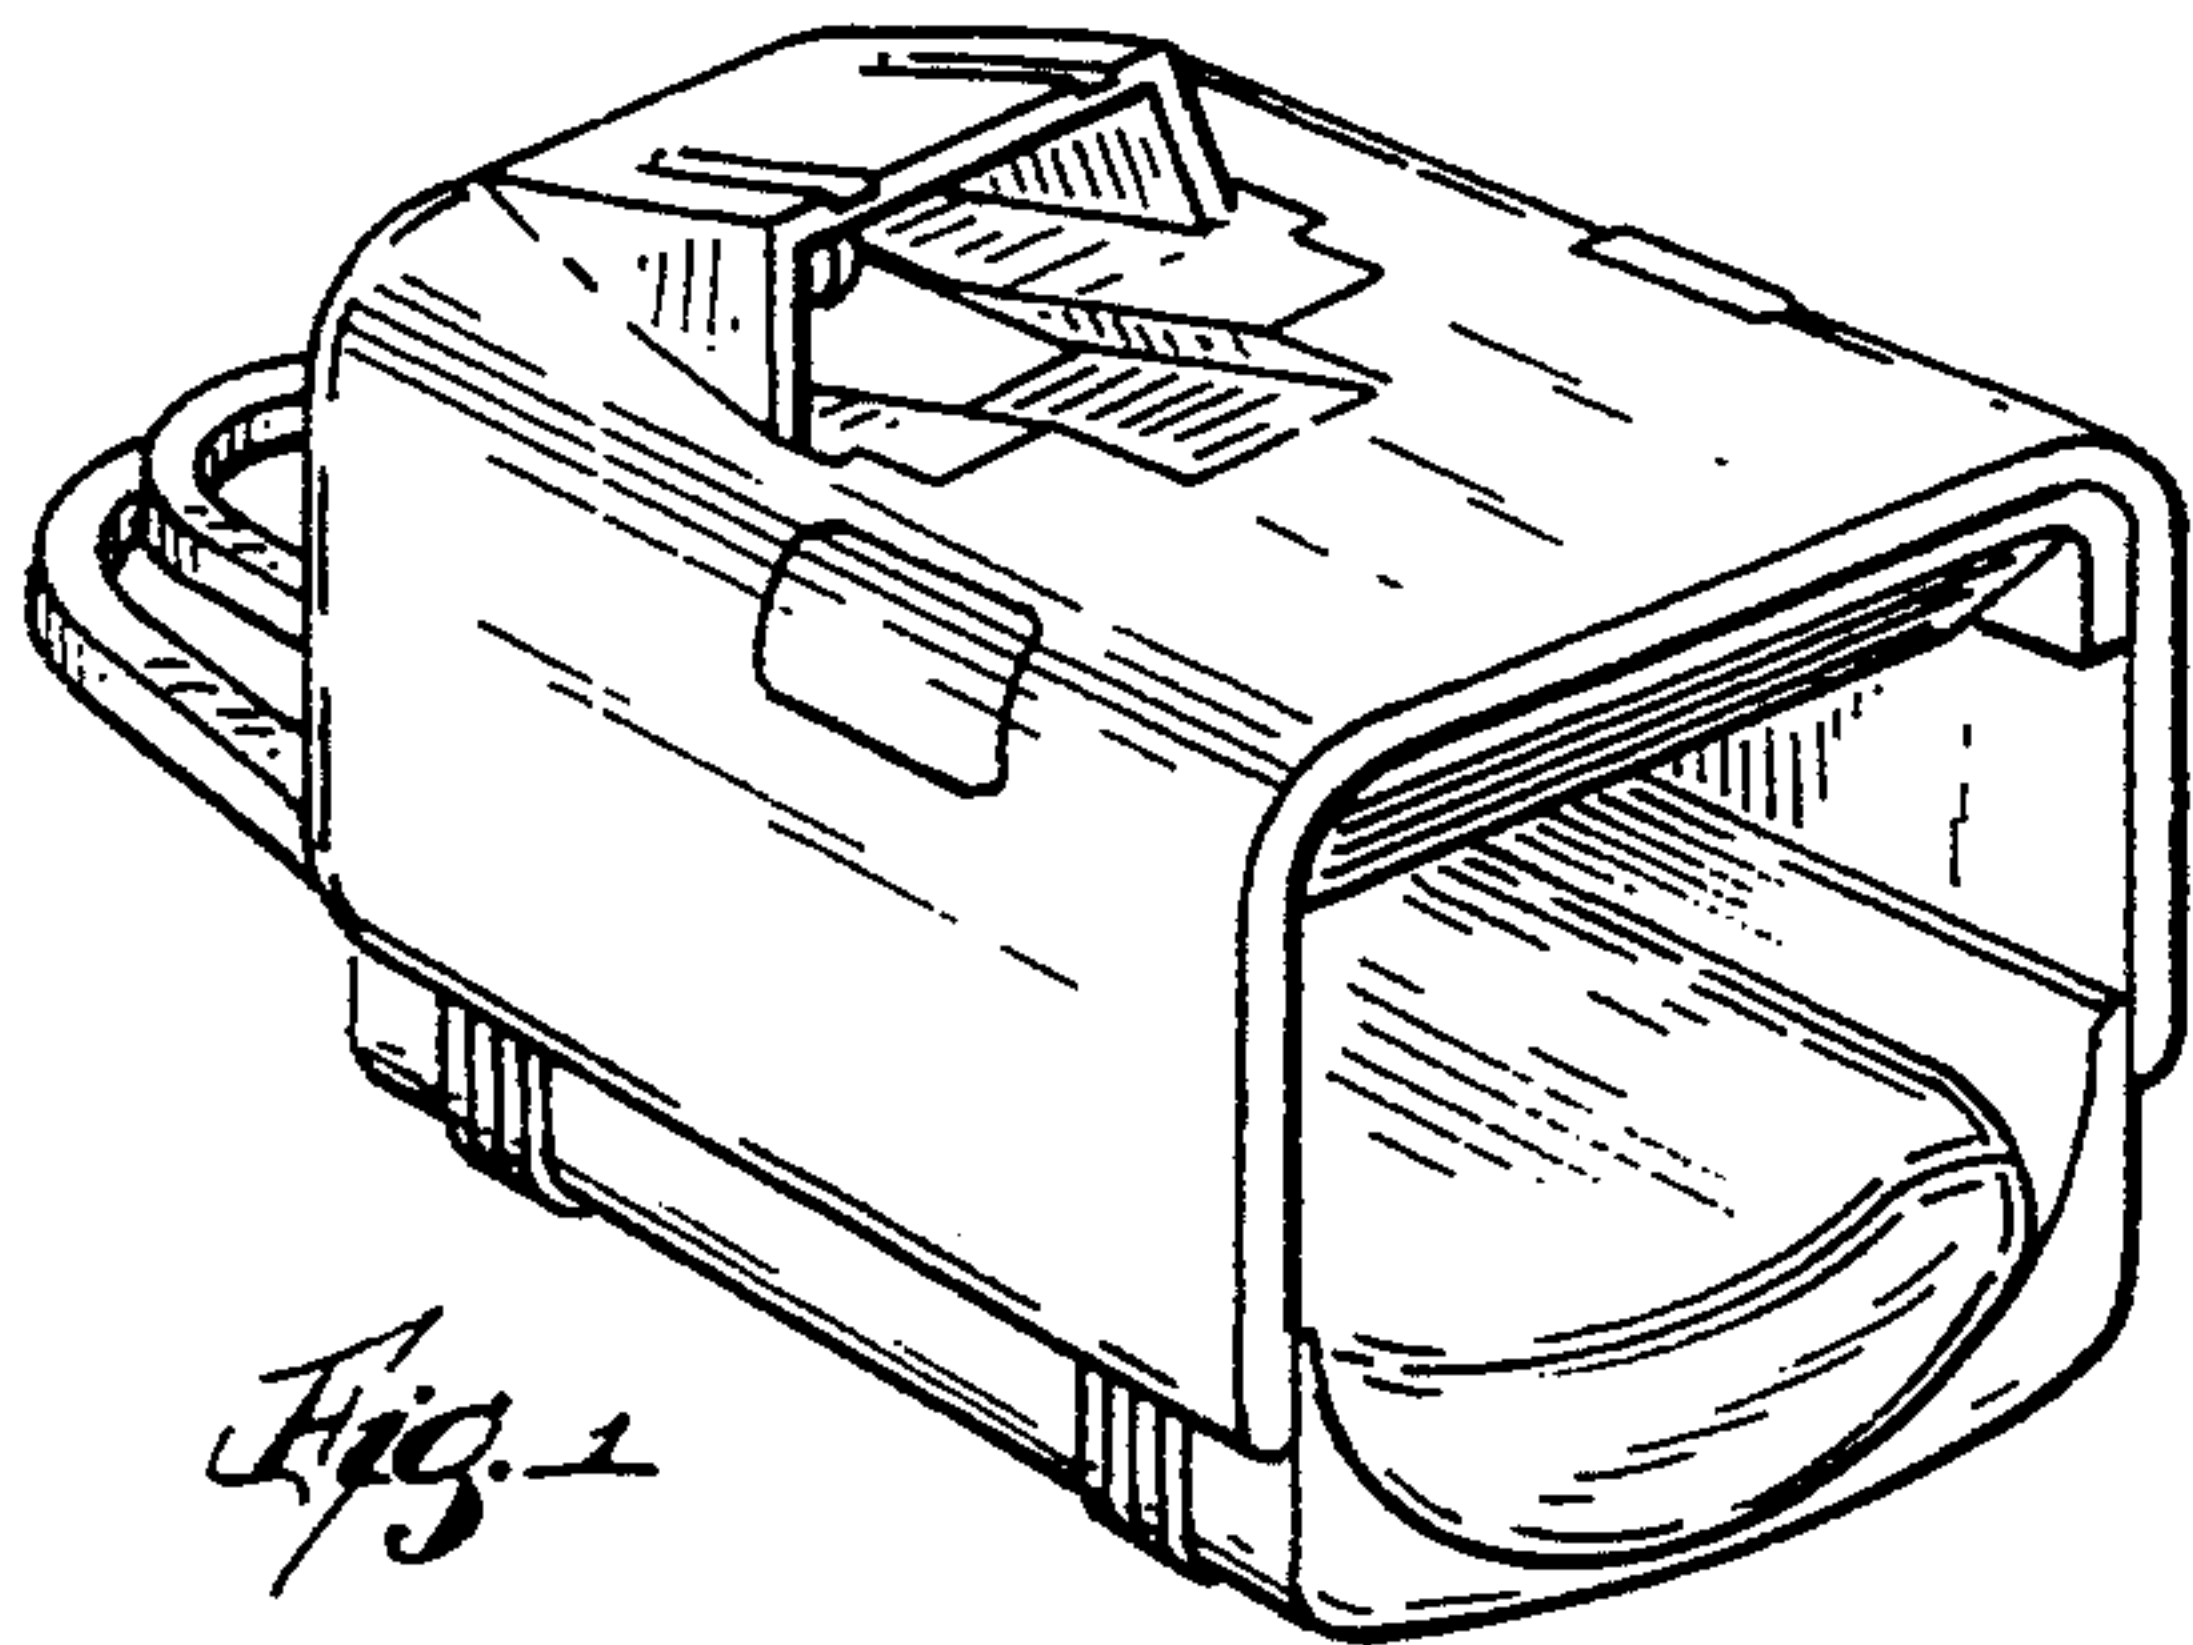


Fig. 3

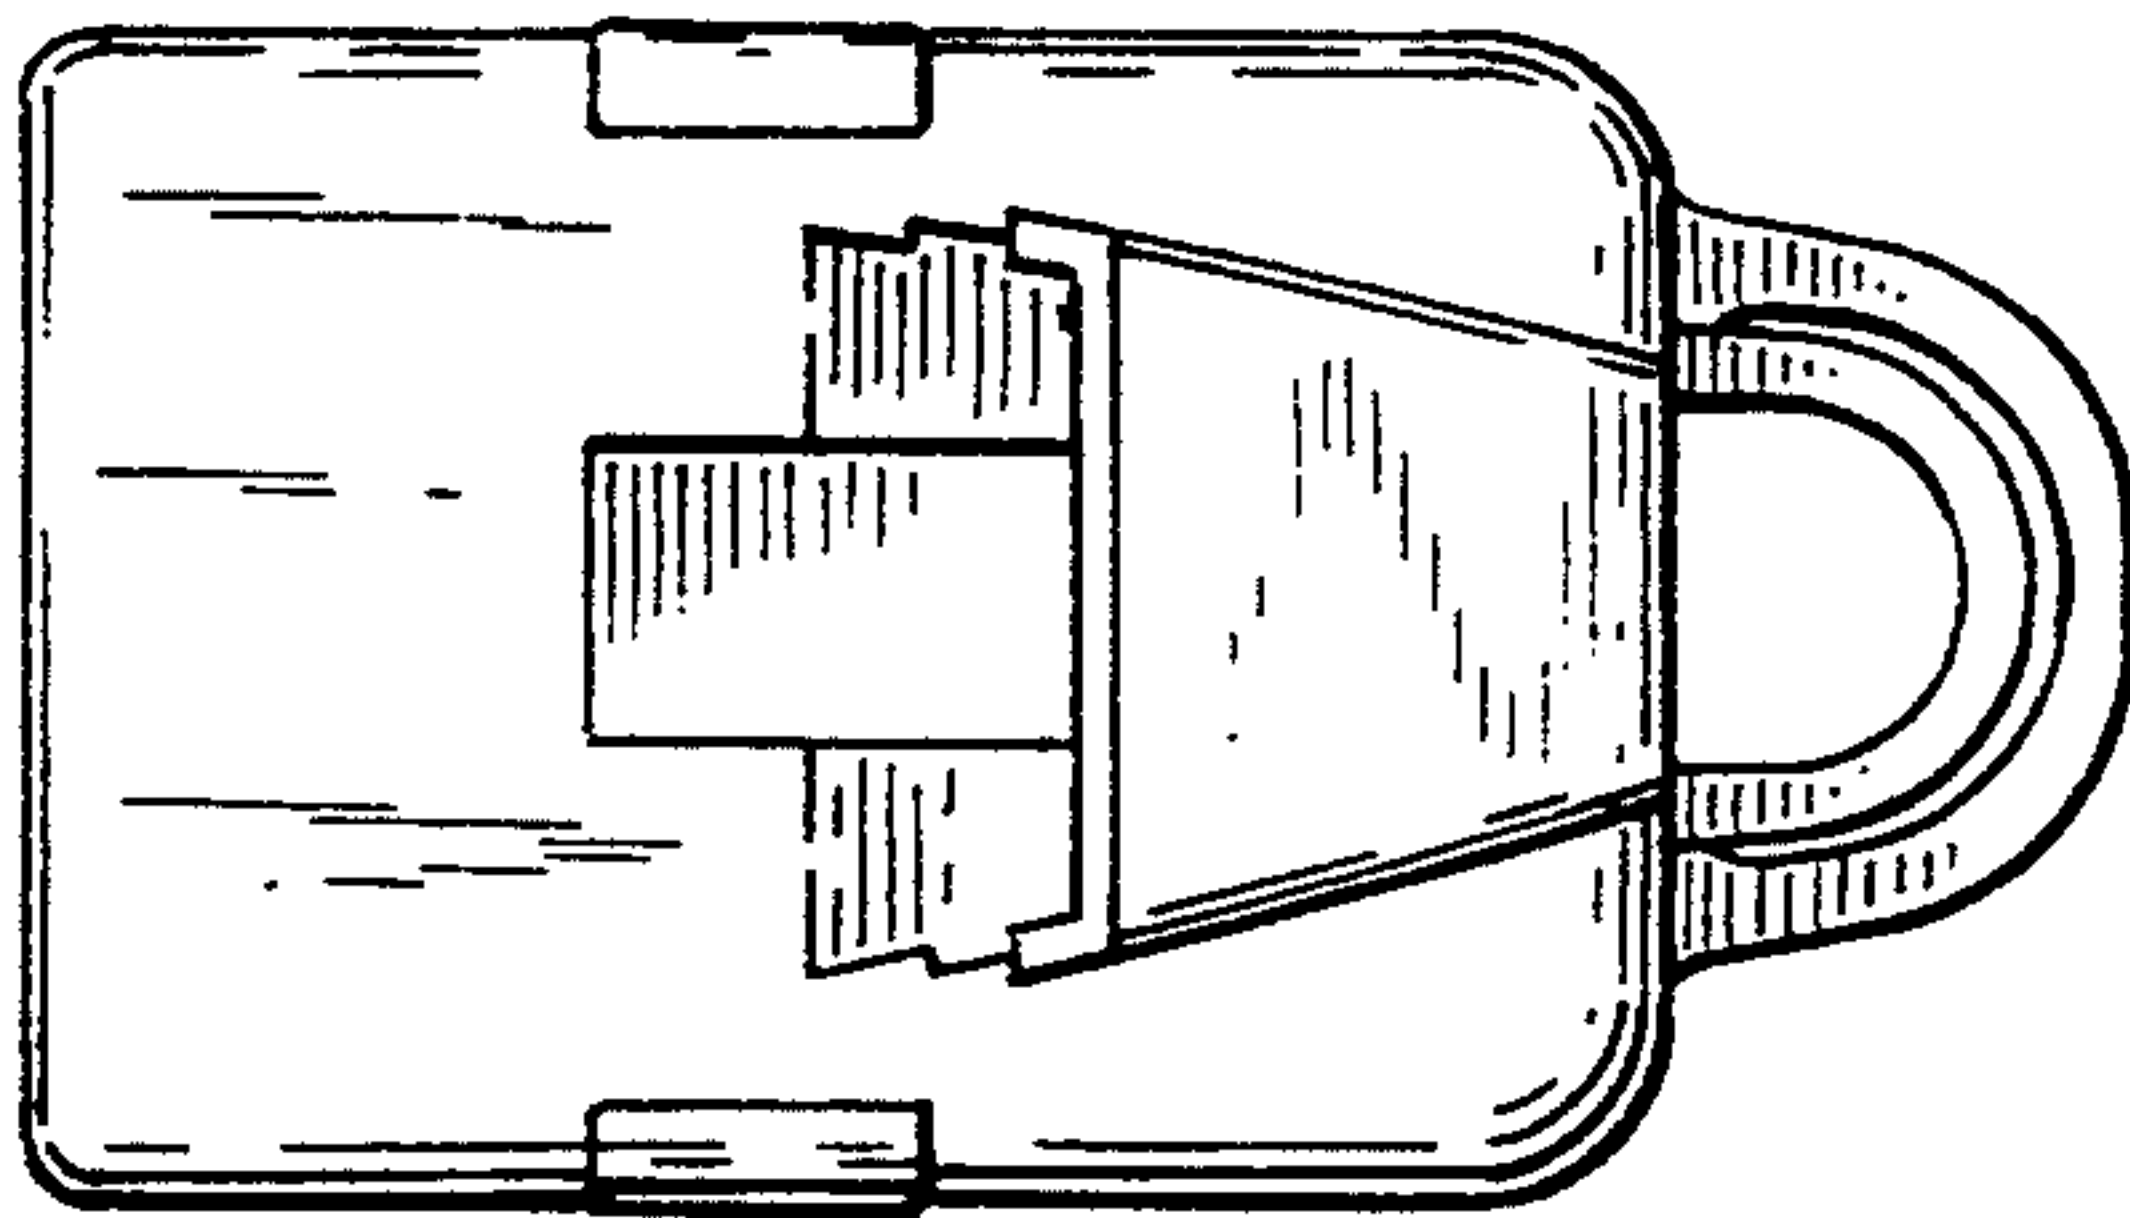
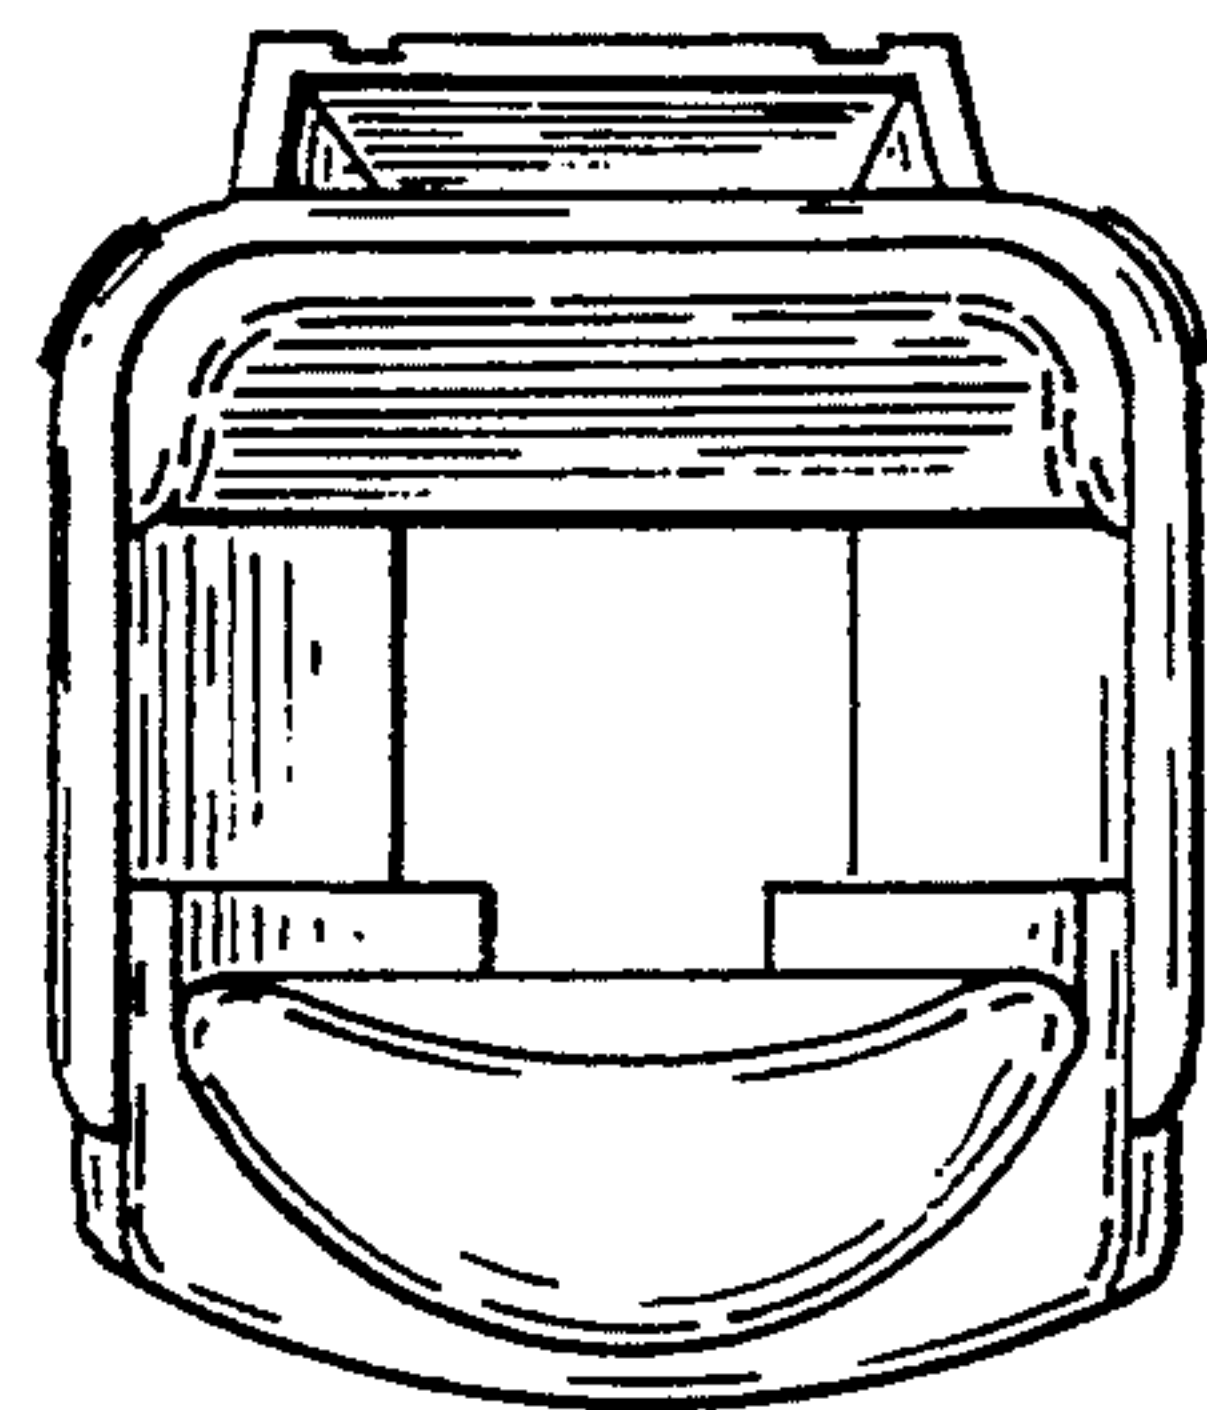


Fig. 5

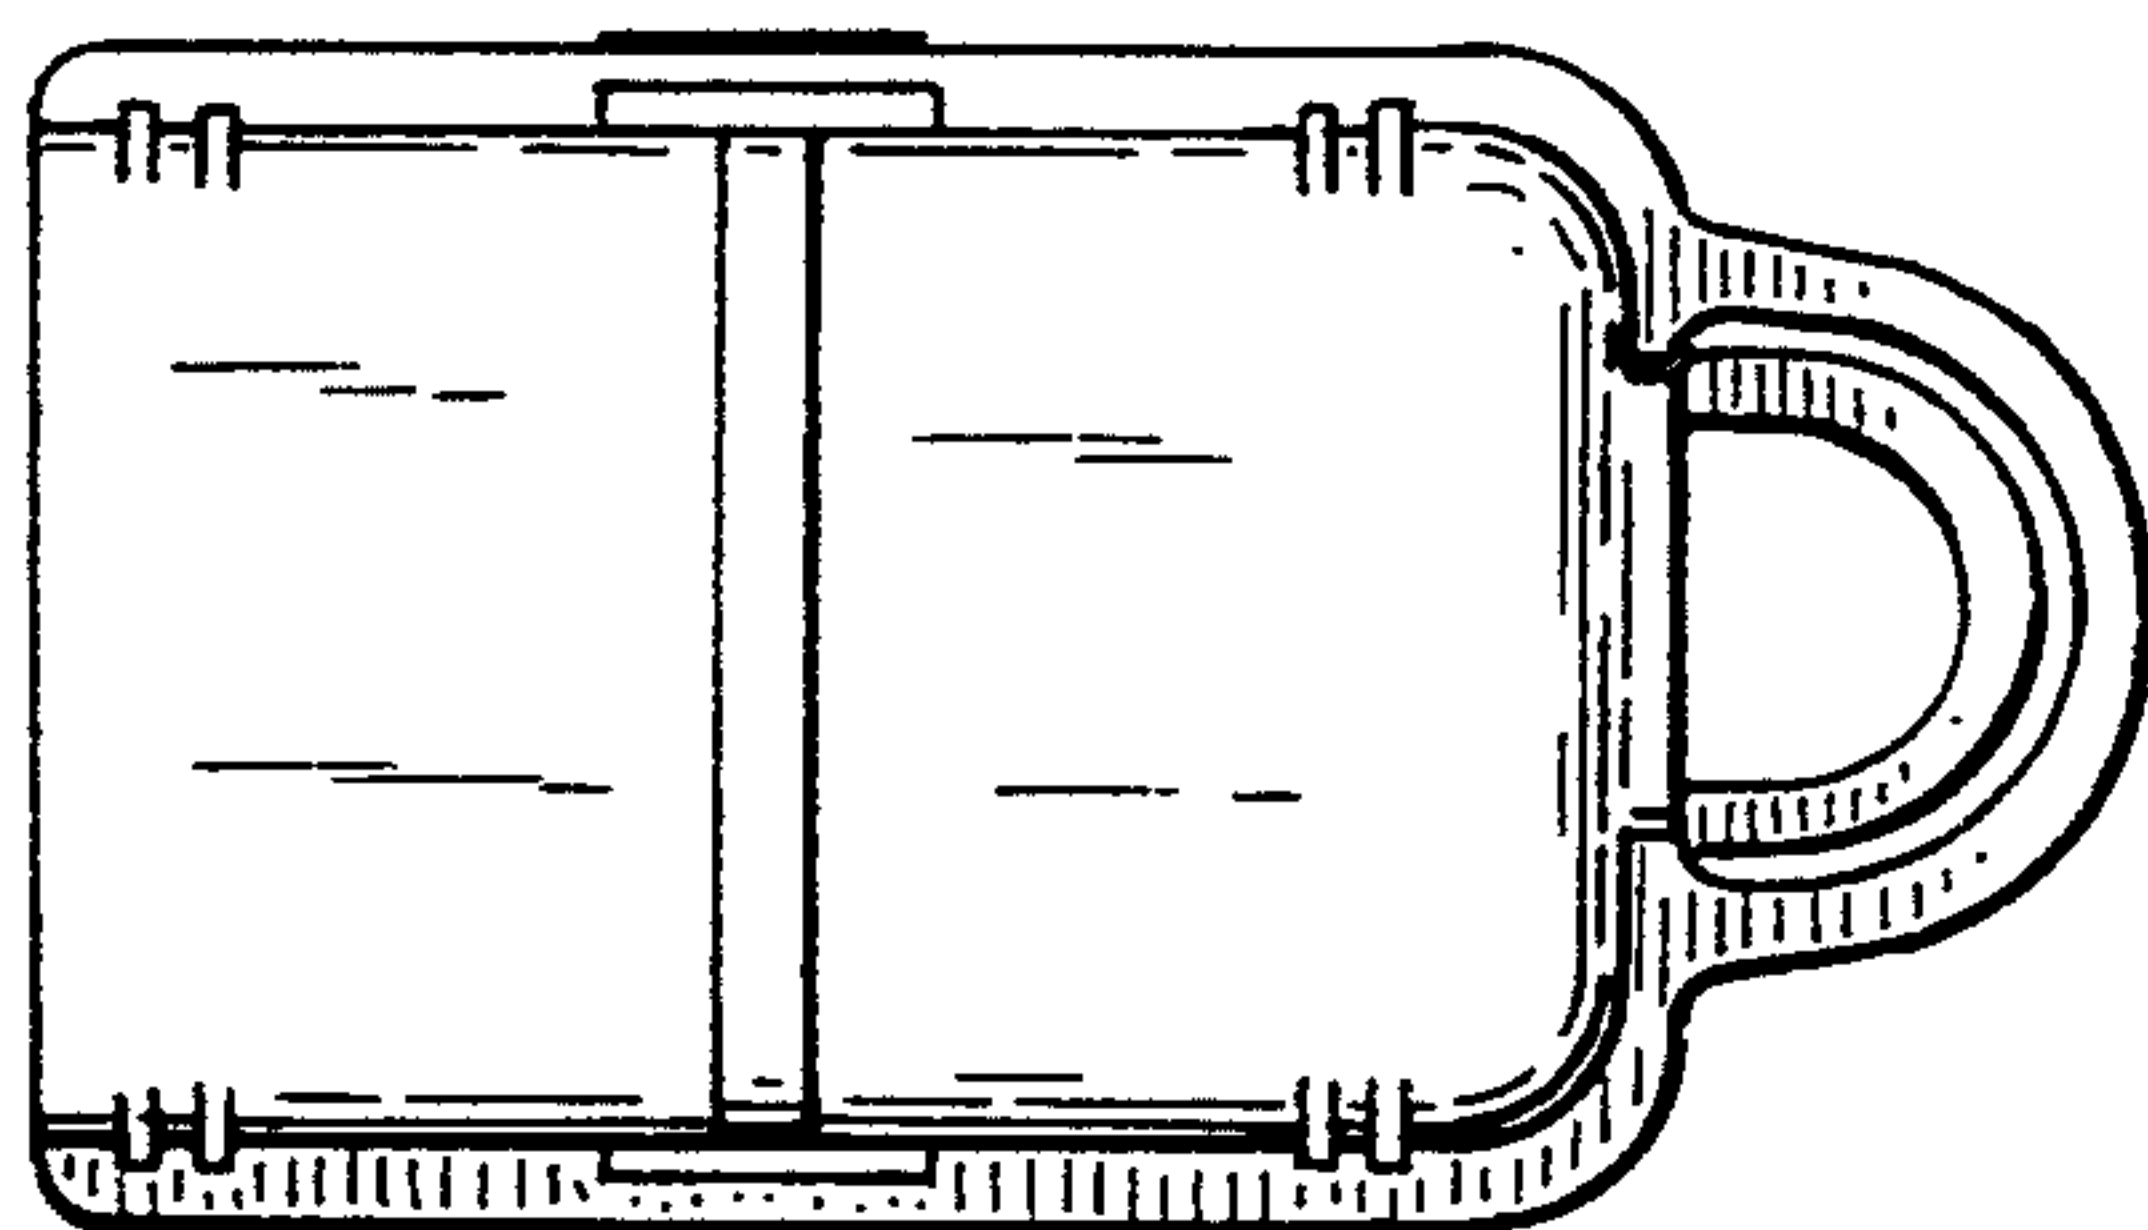


Fig. 6

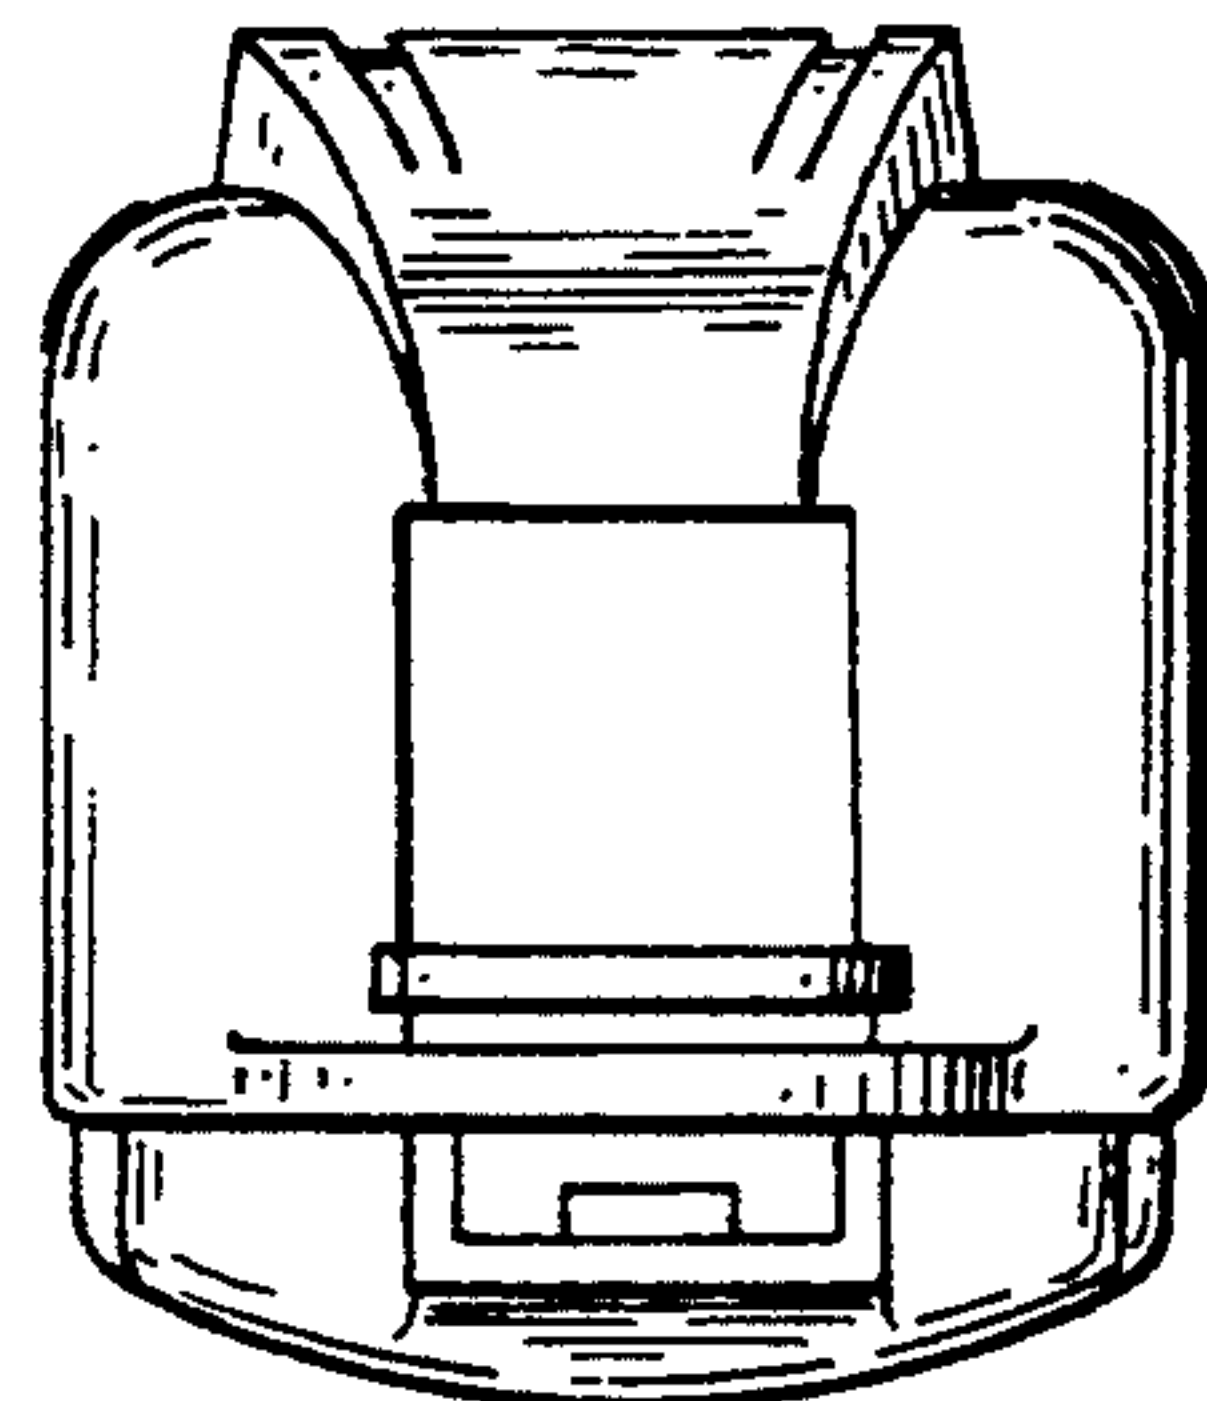
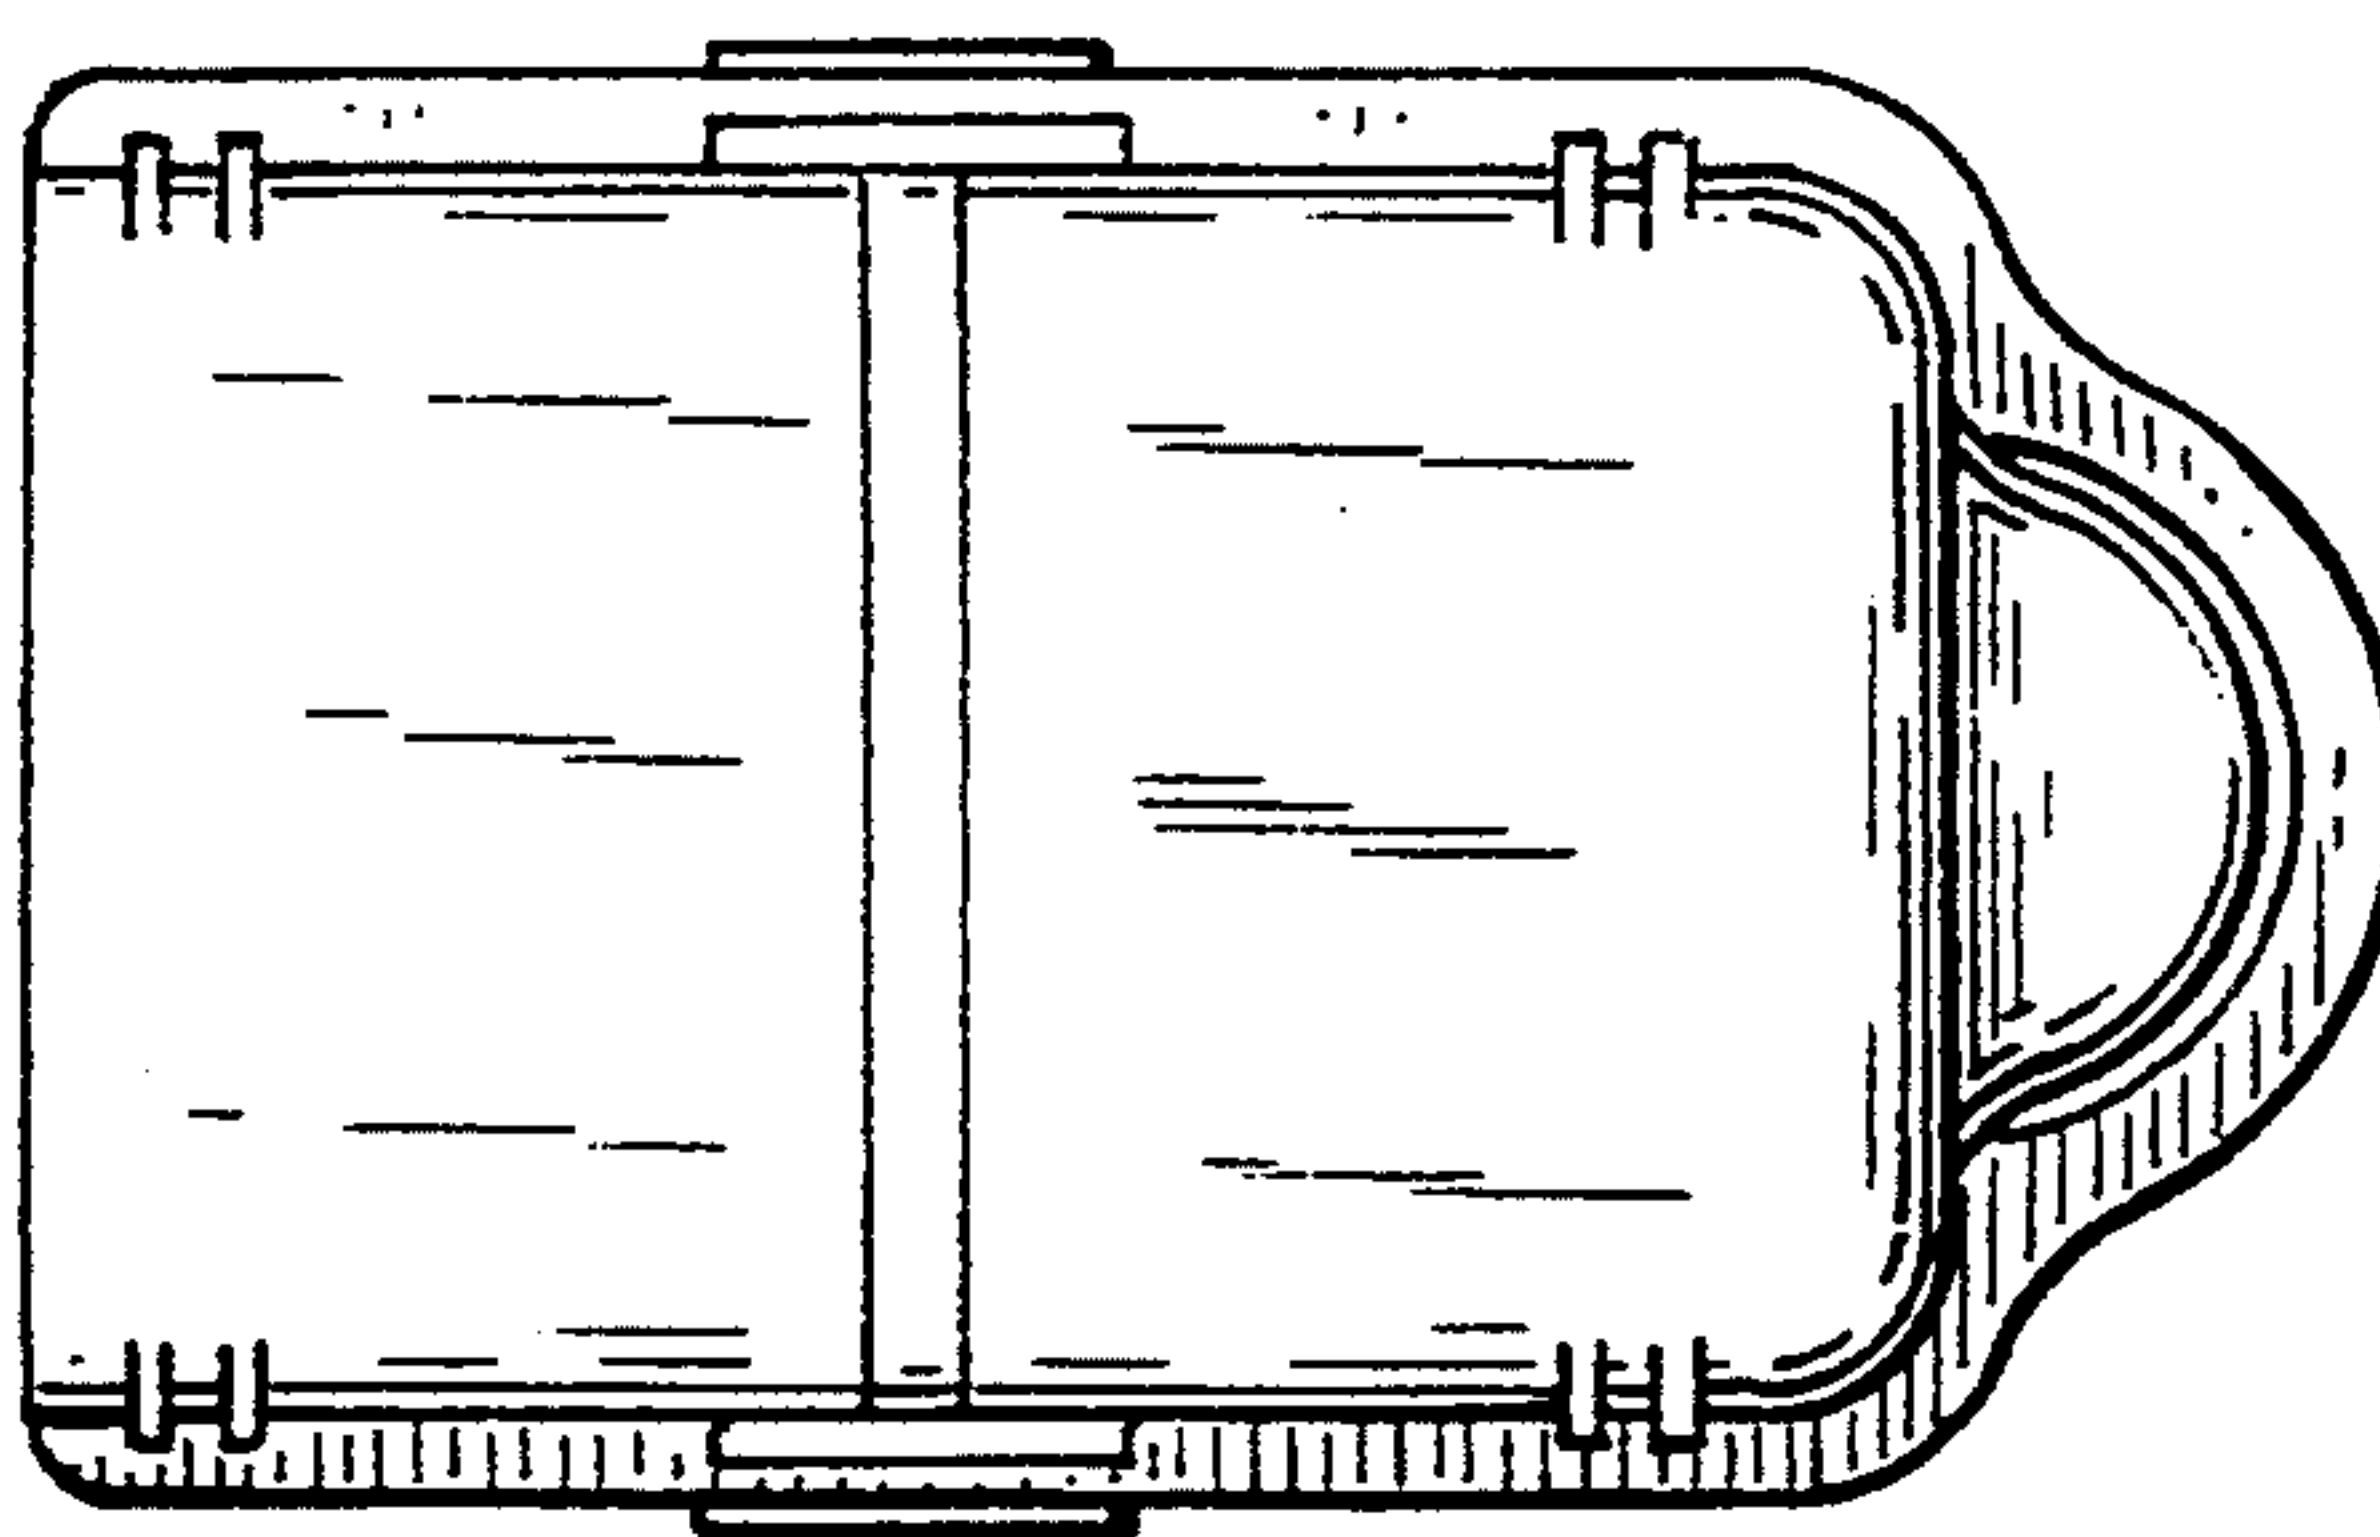


Fig. 4



*Fig. 8*