



US00D357069S

United States Patent [19]

[11] Patent Number: **Des. 357,069**

Plahn et al.

[45] Date of Patent: **** Apr. 4, 1995**

[54] **MEDICAL ELECTRODE**

[75] Inventors: **Susan K. Plahn, Seattle; Brian K. Neil, Issaquah, both of Wash.**

[73] Assignee: **Quinton Instrument Company, Bothell, Wash.**

[**] Term: **14 Years**

[21] Appl. No.: **12,173**

[22] Filed: **Aug. 25, 1993**

4,700,710 10/1987 Hoffman .
 4,706,680 11/1987 Keusch et al. .
 4,738,263 4/1988 Seebach et al. .
 4,757,817 7/1988 Healy .
 4,768,514 9/1988 De Marzo .
 4,777,954 10/1988 Keusch et al. .
 4,798,208 1/1989 Faasse, Jr. .
 4,838,273 6/1989 Cartmell .
 4,934,383 6/1990 Glumac .
 5,114,424 5/1992 Hagen et al. .

FOREIGN PATENT DOCUMENTS

2240928 8/1991 United Kingdom .

Related U.S. Application Data

[63] Continuation-in-part of Ser. No. 101,869, Aug. 4, 1993.

[52] U.S. Cl. **D24/187**

[58] Field of Search **D24/187; 128/641, 640, 128/639**

OTHER PUBLICATIONS

3M Co., "3M Announces the New High Performance Red Dot® Monitoring Electrode" brochure, date unknown.

Ver-Med, "Ver-Med Breathable Electrode" brochure, date unknown.

Ferris Mfg., Co., "Ferris Trace-Itt Pregelled Disposable Pads for the EKG Lab" literature, date unknown.

Medtronic Andover Medical, "ClearTrace™ Monitoring Electrode with Adhesive Gel" literature, date unknown.

Primary Examiner—Stella Reid

Attorney, Agent, or Firm—Andrew J. Beck; Montgomery W. Smith; Richard D. Allison

[56] References Cited

U.S. PATENT DOCUMENTS

Re. 32,724 8/1988 Cartmell .
 D. 240,166 6/1976 Cartmell et al. **D24/187**
 3,487,827 1/1970 Edmark 128/641
 4,027,664 6/1977 Heavner, Jr. et al. 128/641
 4,029,086 6/1977 Corasanti .
 4,155,354 5/1979 Rasmussen .
 4,166,453 9/1979 McClelland 128/639
 4,257,424 3/1981 Cartmell .
 4,265,253 5/1981 Abraham .
 4,270,544 6/1981 Gilden et al. .
 4,274,419 6/1981 Tam et al. .
 4,300,575 11/1981 Wilson .
 4,311,152 1/1982 Modes et al. .
 4,319,579 3/1982 Cartmell .
 4,331,153 5/1982 Healy .
 4,488,557 12/1984 Engel .
 4,524,087 6/1985 Engel .
 4,539,996 9/1985 Engel .
 4,559,950 12/1985 Vaughan et al. .
 4,595,013 6/1986 Jones et al. .
 4,674,511 6/1987 Cartmell .
 4,679,564 7/1987 Sessions .

[57] CLAIM

The ornamental design for a medical electrode, as shown.

DESCRIPTION

FIG. 1 is a front elevational view of a medical electrode, showing our new design;
 FIG. 2 is a rear elevational view thereof;
 FIG. 3 is a top plan view thereof;
 FIG. 4 is a bottom plan view thereof;
 FIG. 5 is a left side elevational view thereof; and,
 FIG. 6 is a right side elevational view thereof.

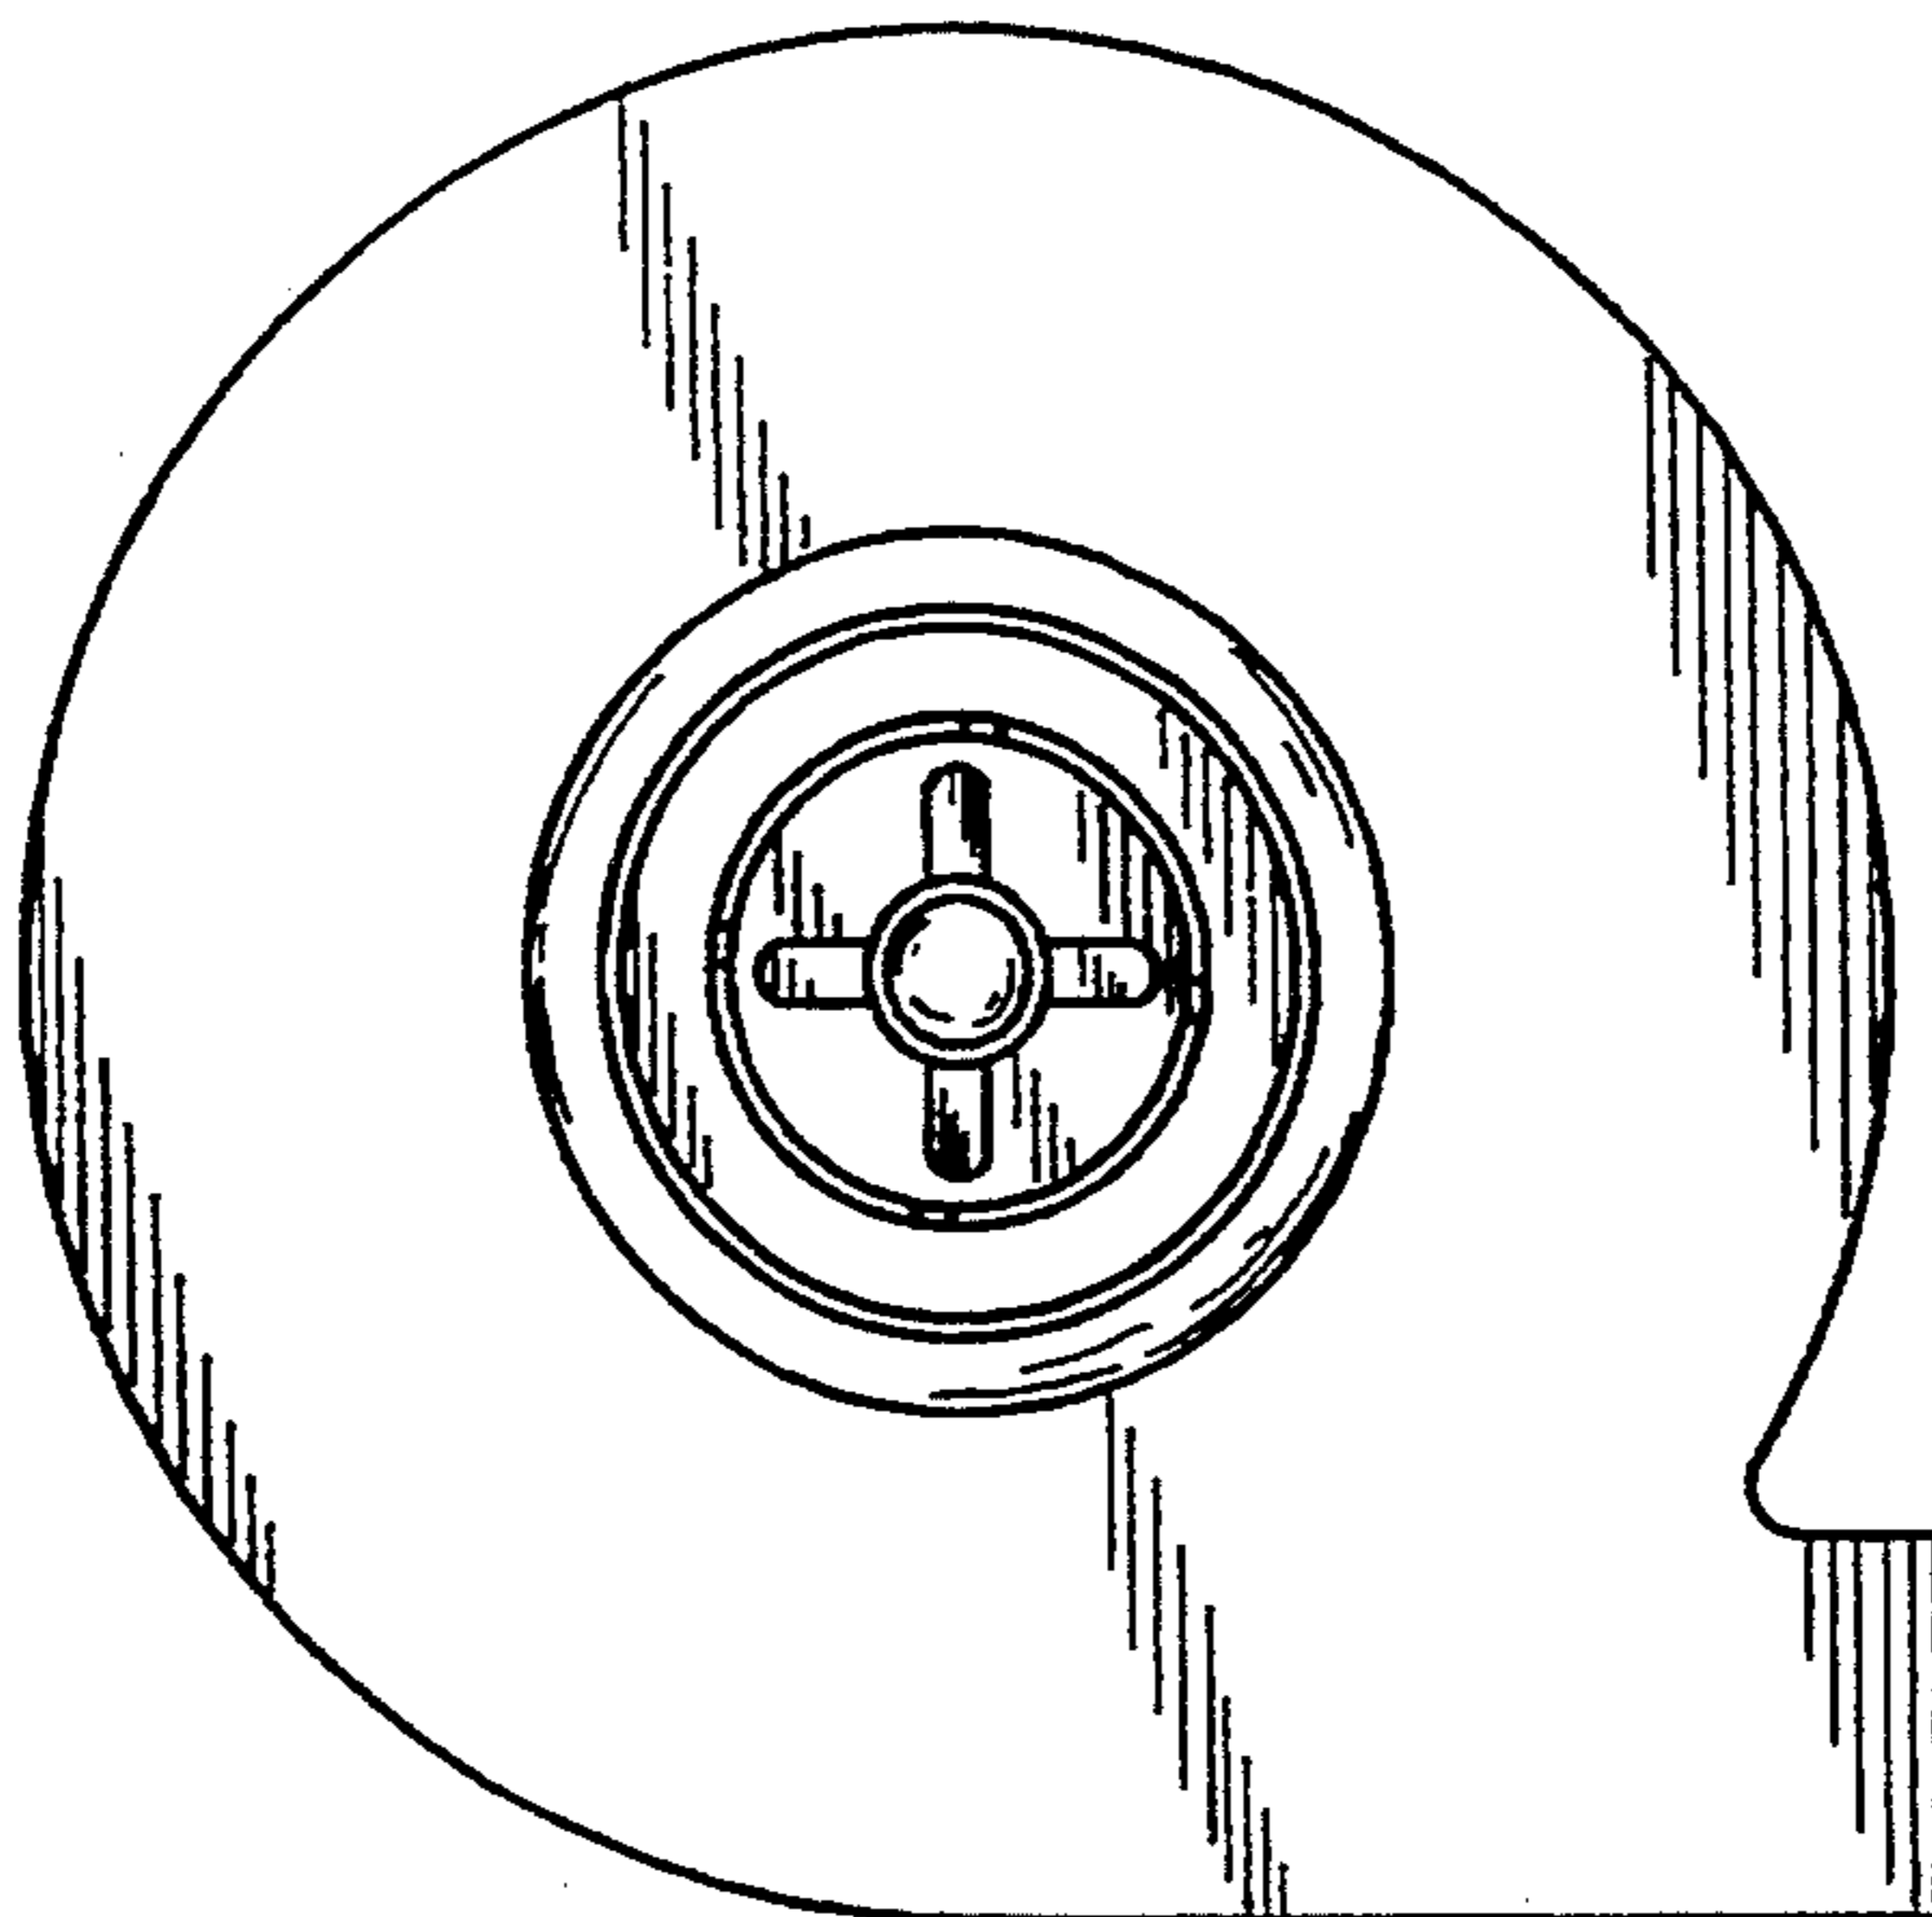


FIG. 1

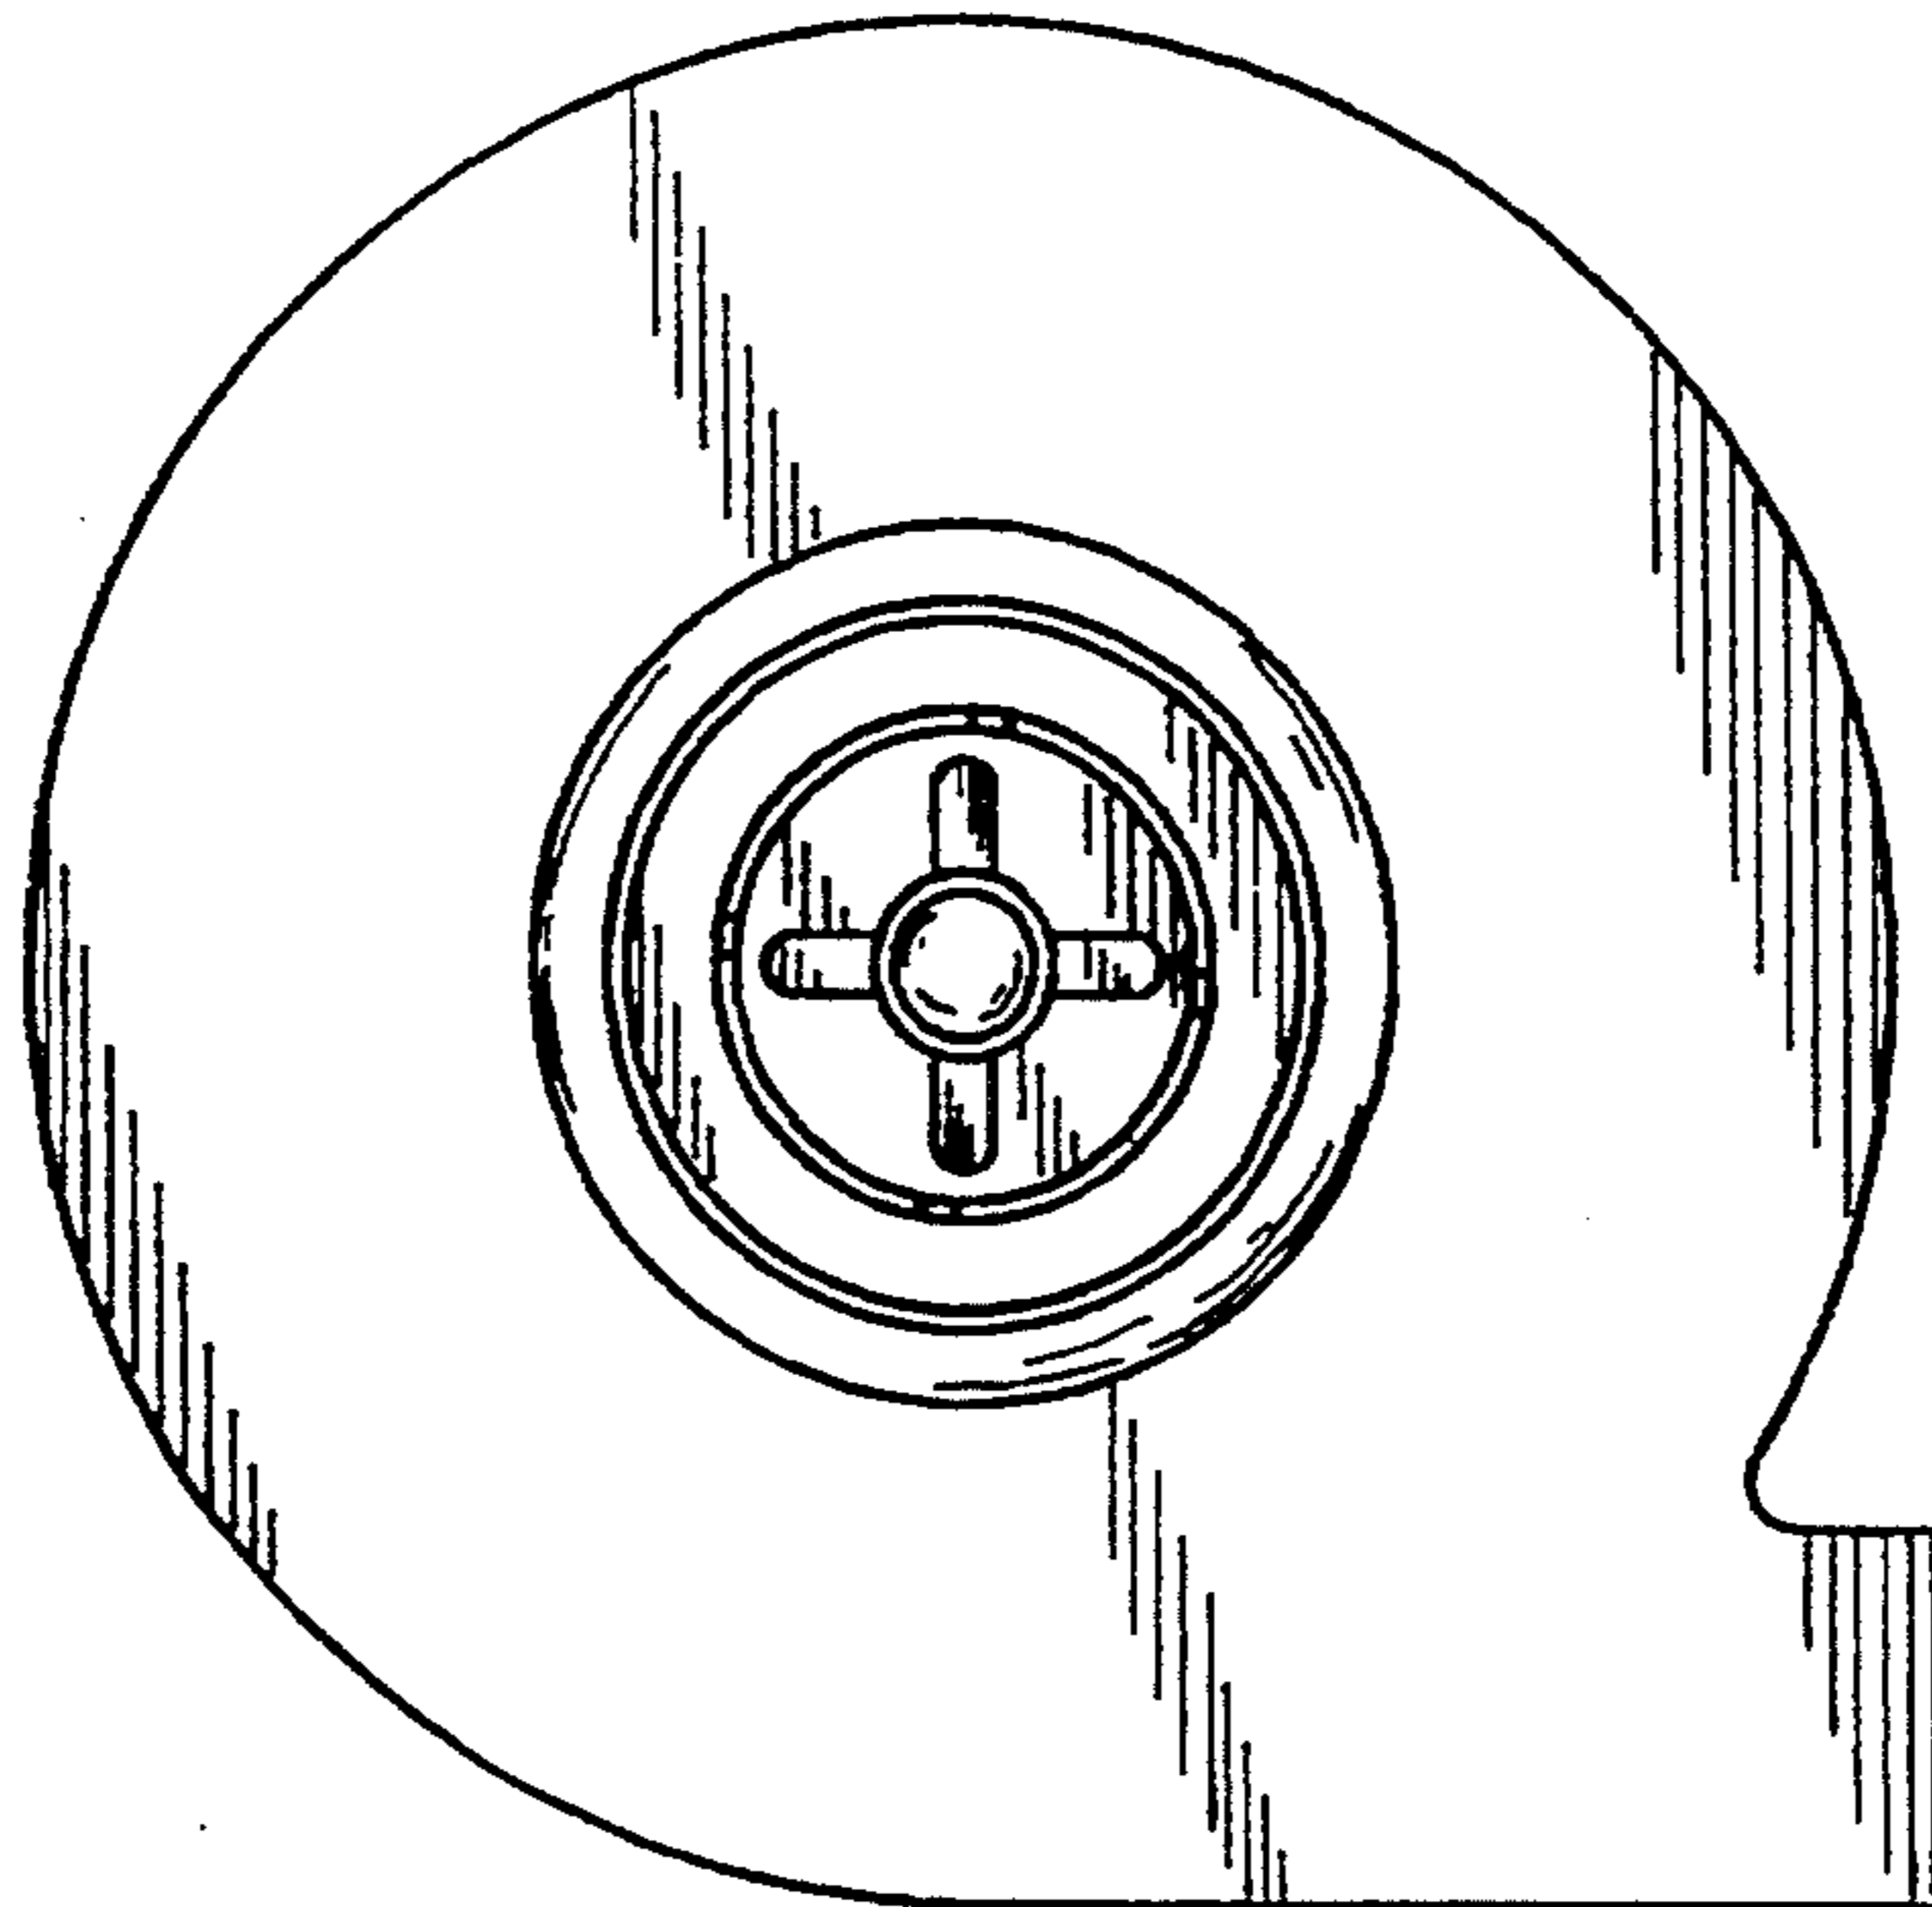


FIG. 2

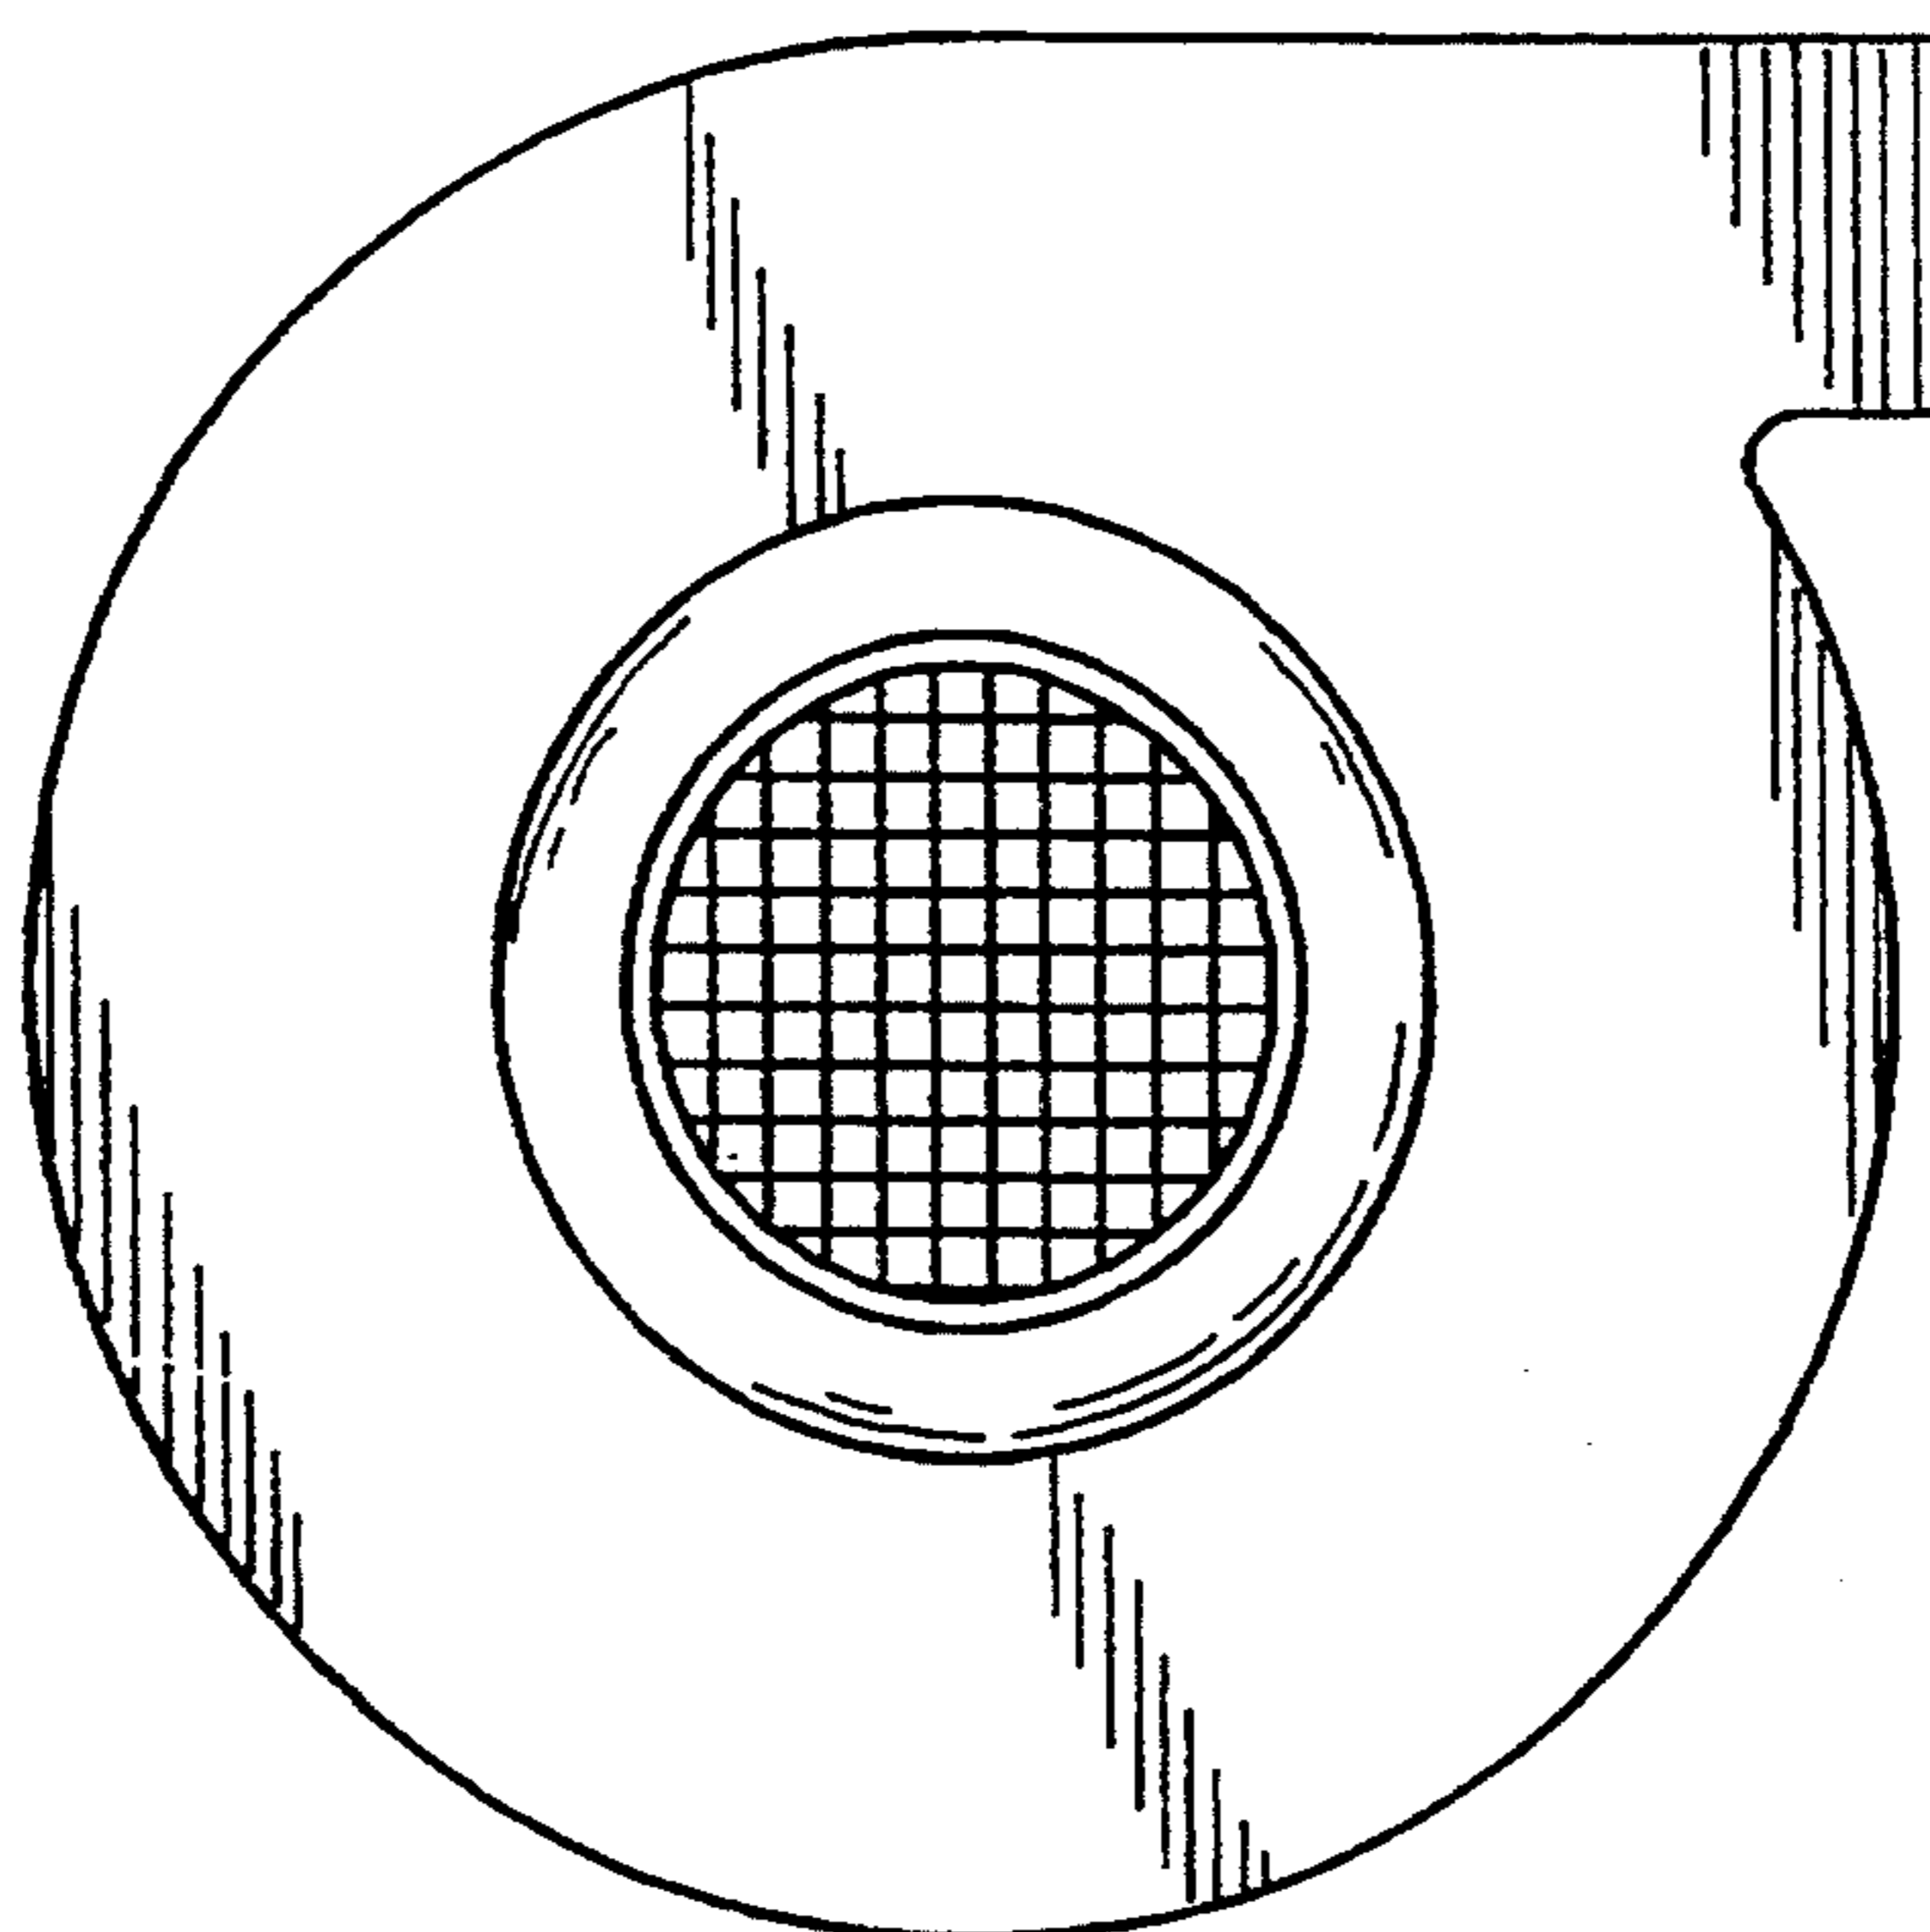


FIG. 3

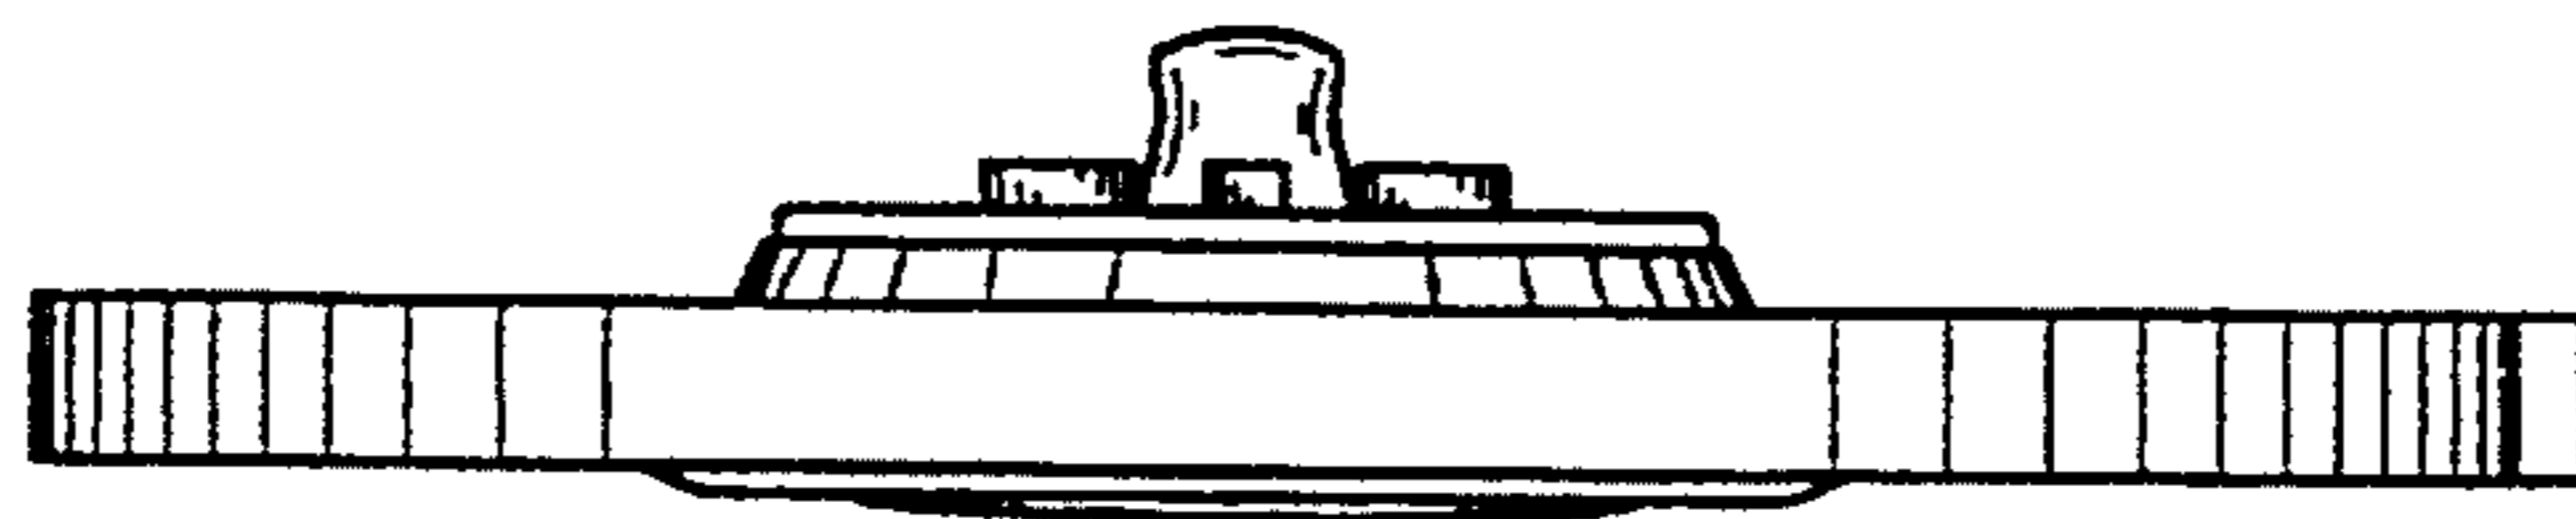


FIG. 4

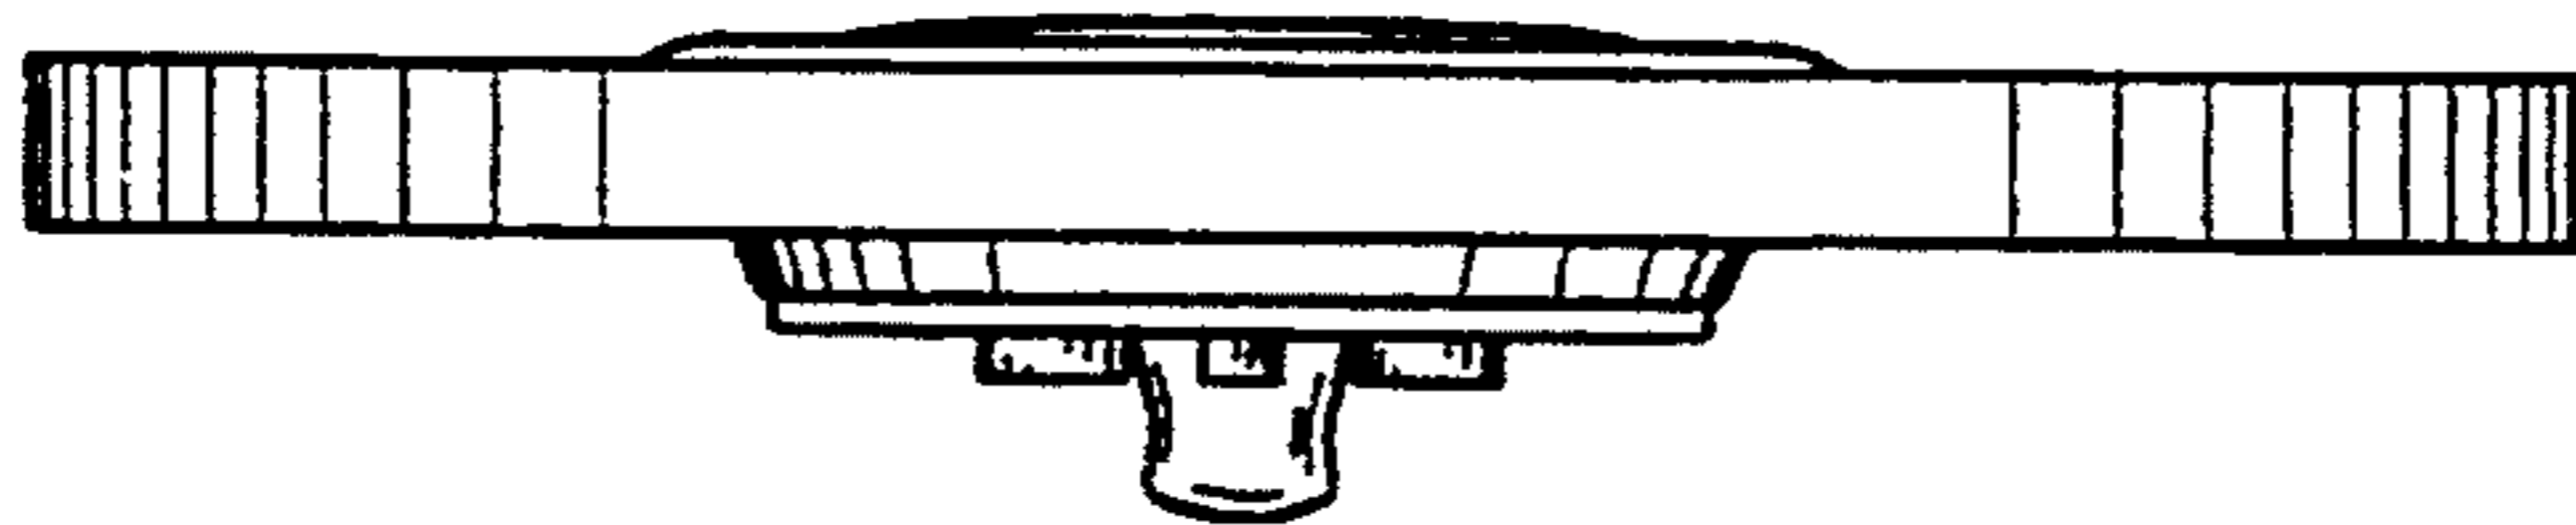


FIG. 5

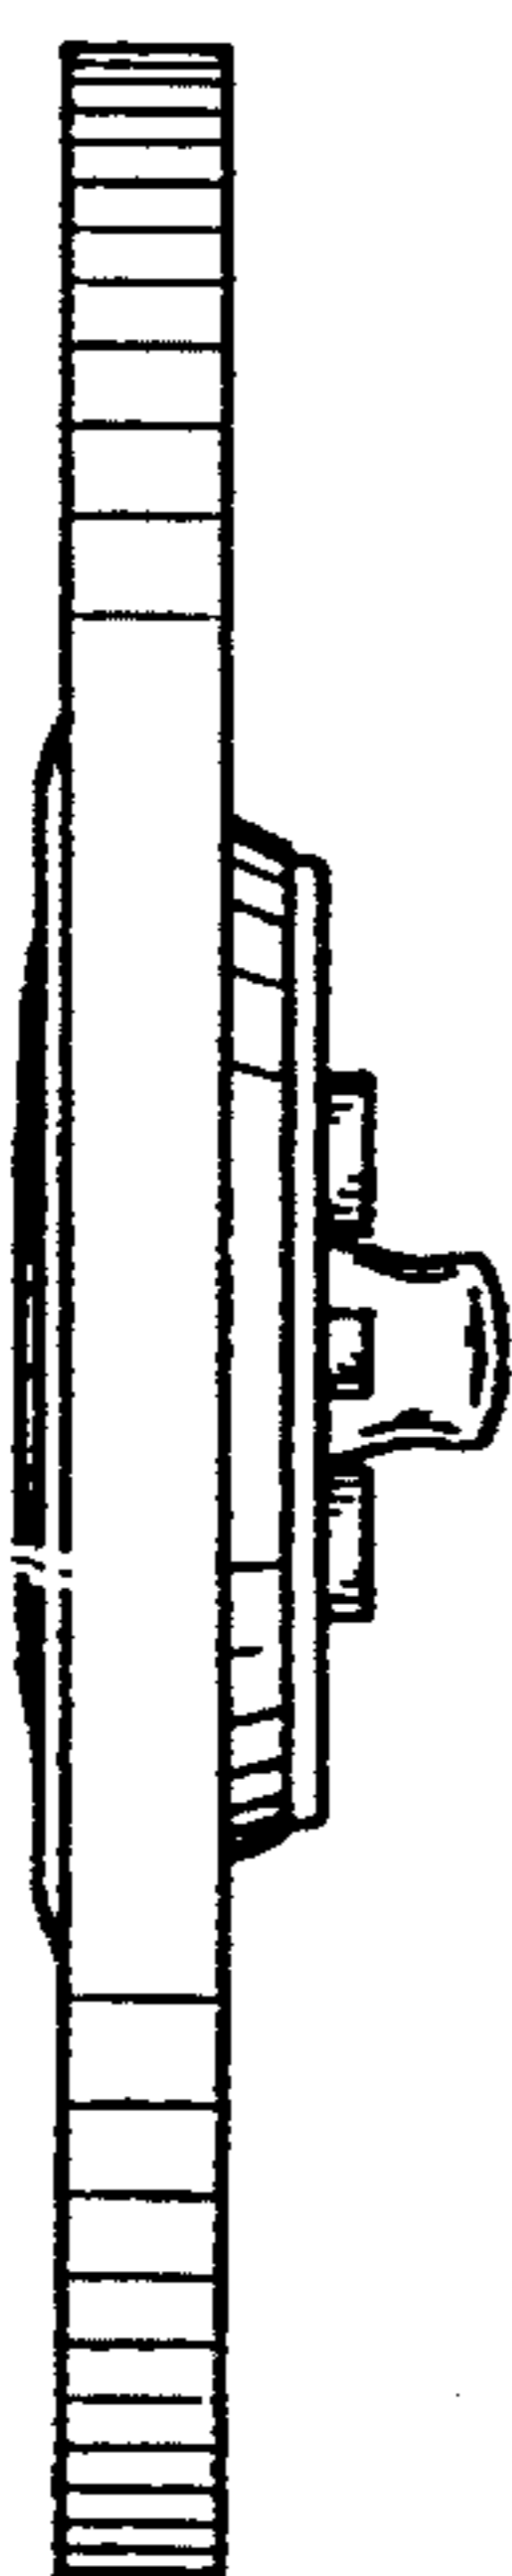


FIG. 6

