



US00D357876S

United States Patent [19]

McConnell

[11] Patent Number: Des. 357,876
[45] Date of Patent: ** May 2, 1995

[54] DIAGNOSTIC TESTER

[75] Inventor: Patrick N. McConnell, Goshen, Ind.

[73] Assignee: The Dometic Corporation, Lagrange, Ind.

[**] Term: 14 Years

[21] Appl. No.: 9,364

[22] Filed: Jun. 10, 1993

[52] U.S. Cl. D10/78

[58] Field of Search D10/46, 78; D14/115;
62/125, 127, 236, 237; 340/516, 586, 679, 693;
360/77.1, 133; 371/15.1-29.5

[56] References Cited

U.S. PATENT DOCUMENTS

| | | | | |
|------------|---------|--------------------|-------|---------|
| D. 267,950 | 2/1983 | Autt | | D14/115 |
| D. 268,030 | 2/1983 | Autt | | D14/115 |
| D. 313,563 | 1/1991 | Mieczkowski et al. | | D10/78 |
| D. 315,691 | 3/1991 | Morgan | | D10/78 |
| D. 339,994 | 10/1993 | Rohmann | | D10/78 |


Primary Examiner—Alan P. Douglas
Assistant Examiner—Antoine D. Davis
Attorney, Agent, or Firm—Pearne, Gordon, McCoy & Granger

[57] CLAIM

The ornamental design for a diagnostic tester, as shown and described.

DESCRIPTION

FIG. 1 shows a perspective view of the diagnostic tester with its applications module removed;
FIG. 2 shows the diagnostic tester with its applications module installed;
FIG. 3 shows a top view of the diagnostic tester;
FIG. 4 shows a bottom view of the diagnostic tester;
FIG. 5 shows a front end view of the diagnostic tester;
FIG. 6 shows a rear end view of the diagnostic tester;
FIG. 7 shows a right side view of the diagnostic tester;
FIG. 8 shows a left side view of the diagnostic tester;
FIG. 9 shows a perspective view of the applications module;
FIG. 10 shows a rear end view of the applications module;
FIG. 11 shows a top view of the applications module, with the bottom view being identical;
FIG. 12 shows a right side elevational view of the applications module, with the left side elevational view being identical; and,
FIG. 13 shows a front end view of the applications module.
The applications module has been removed for ease of illustration in FIGS. 3, 4, 5, 7 and 8. The diagnostic tester has been removed for ease of illustration in FIGS. 9-13.

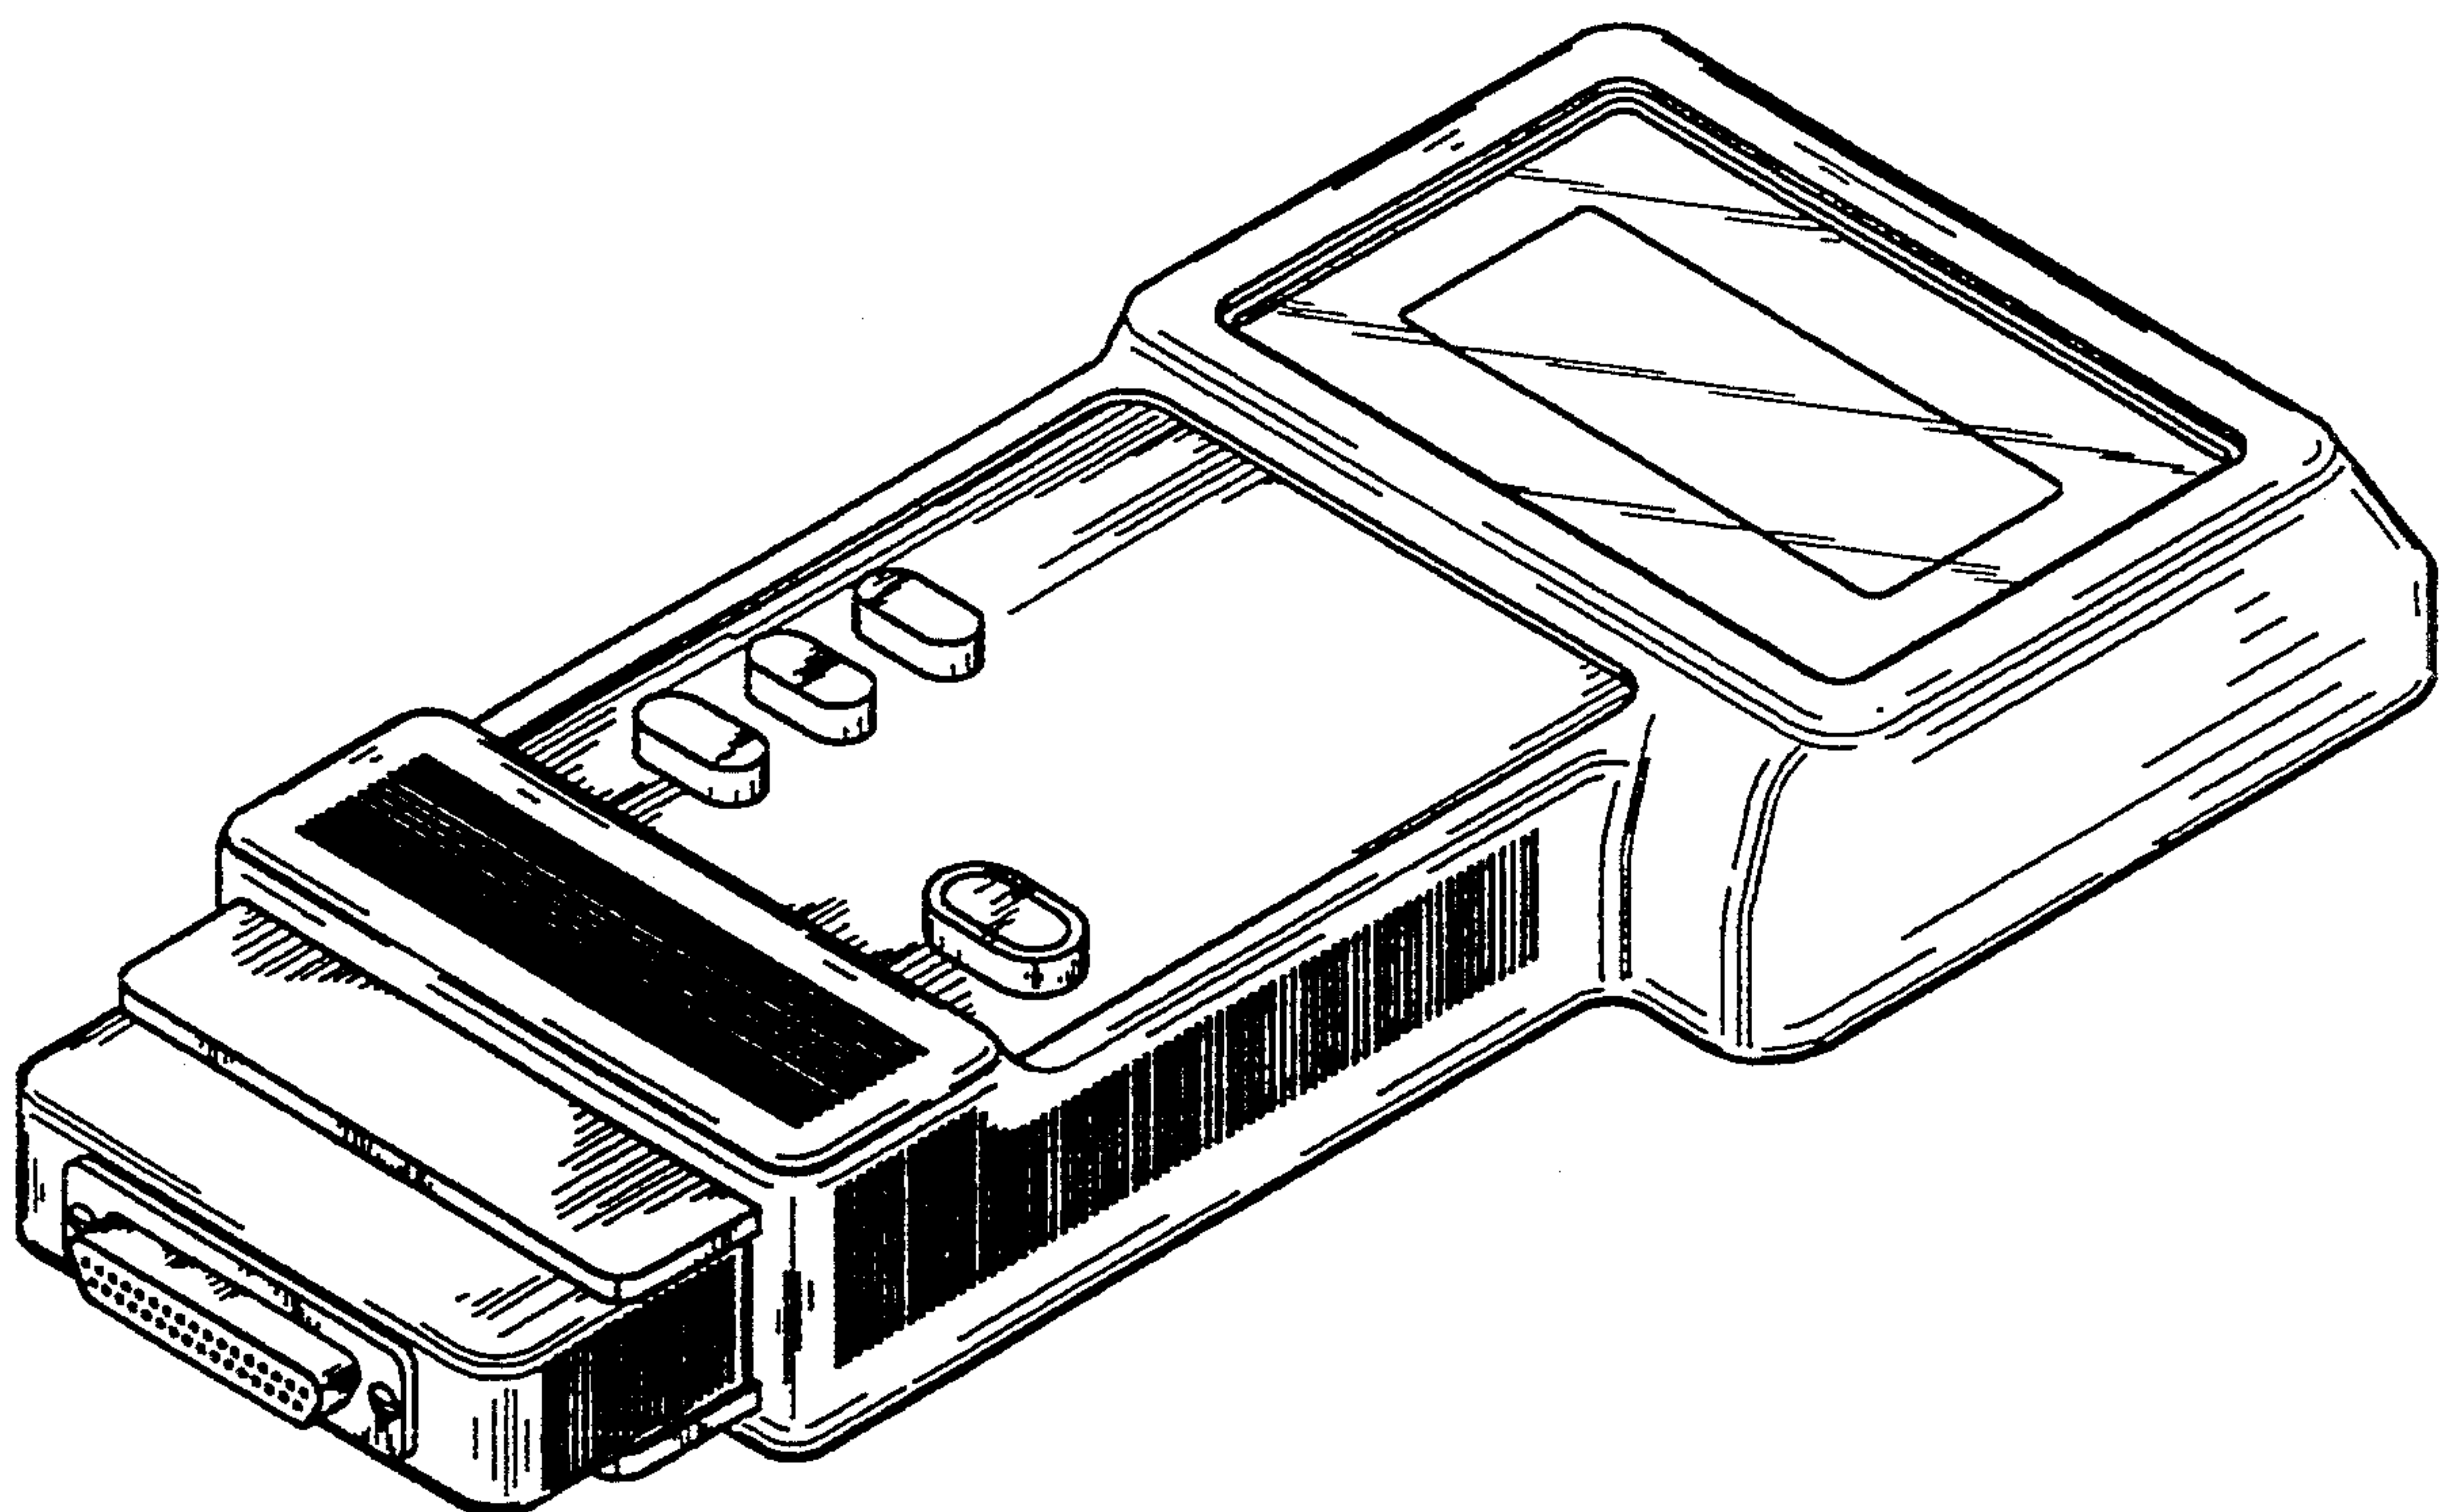

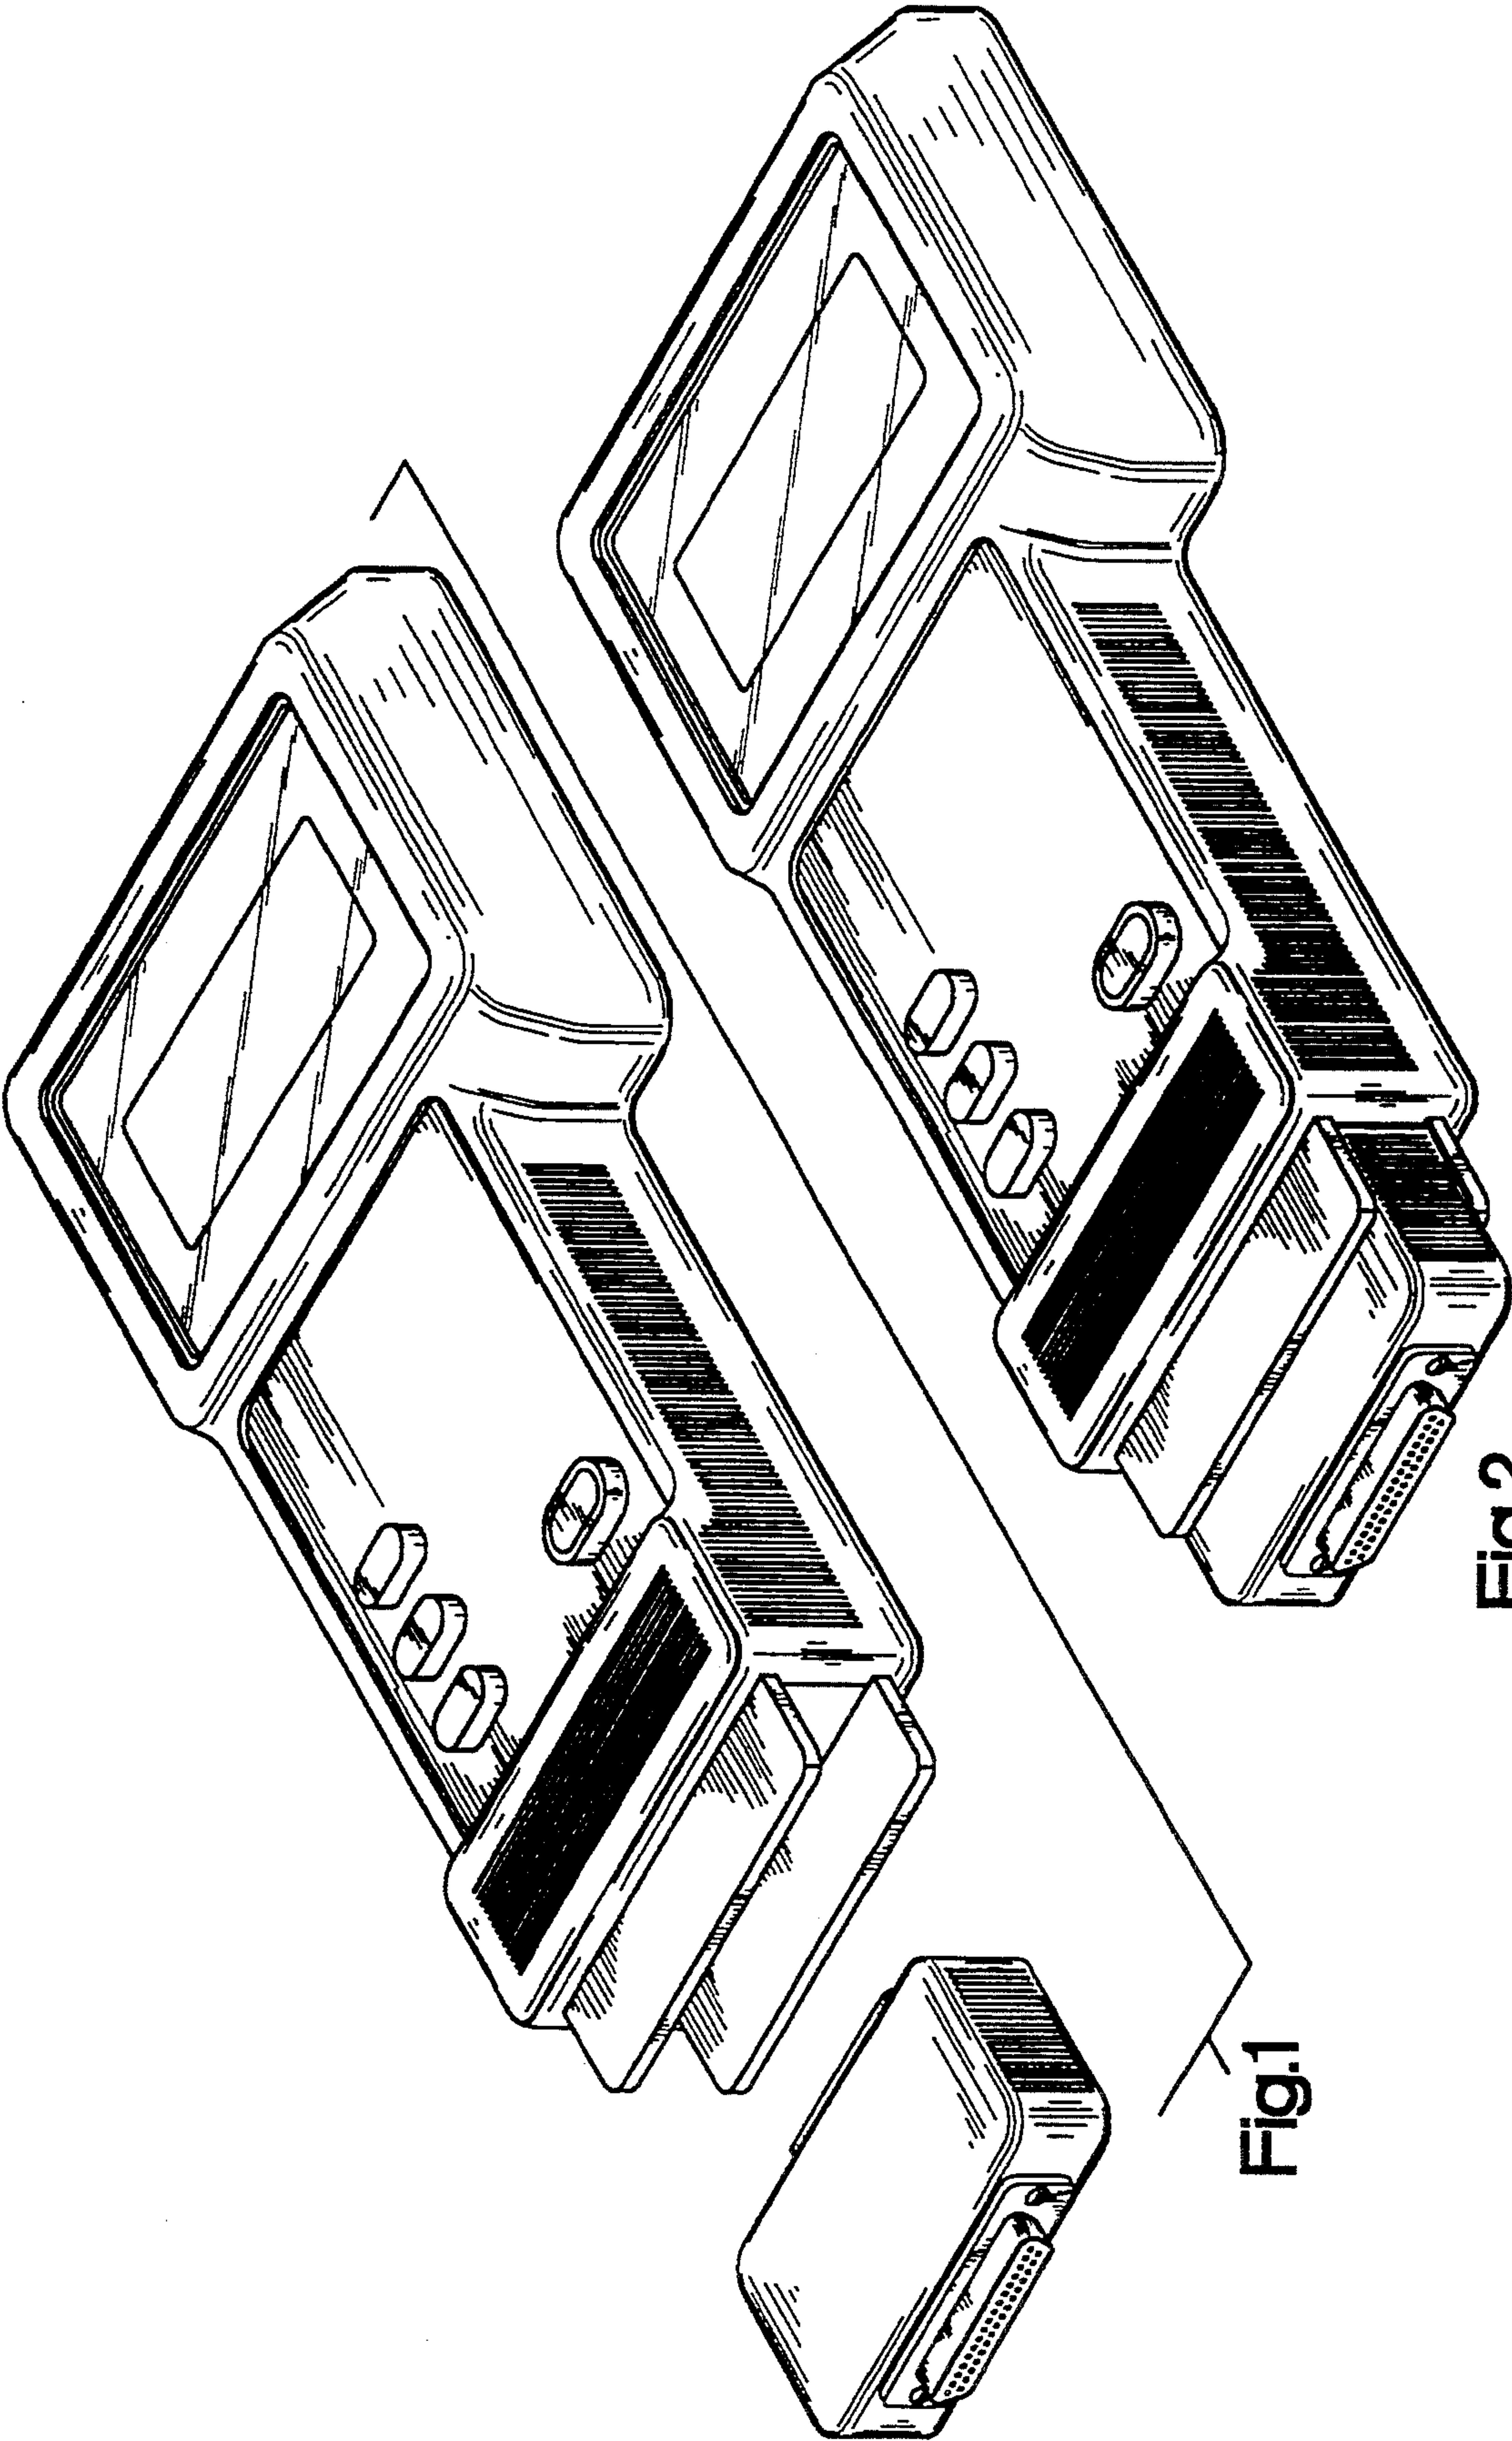


Fig.2

Fig.1

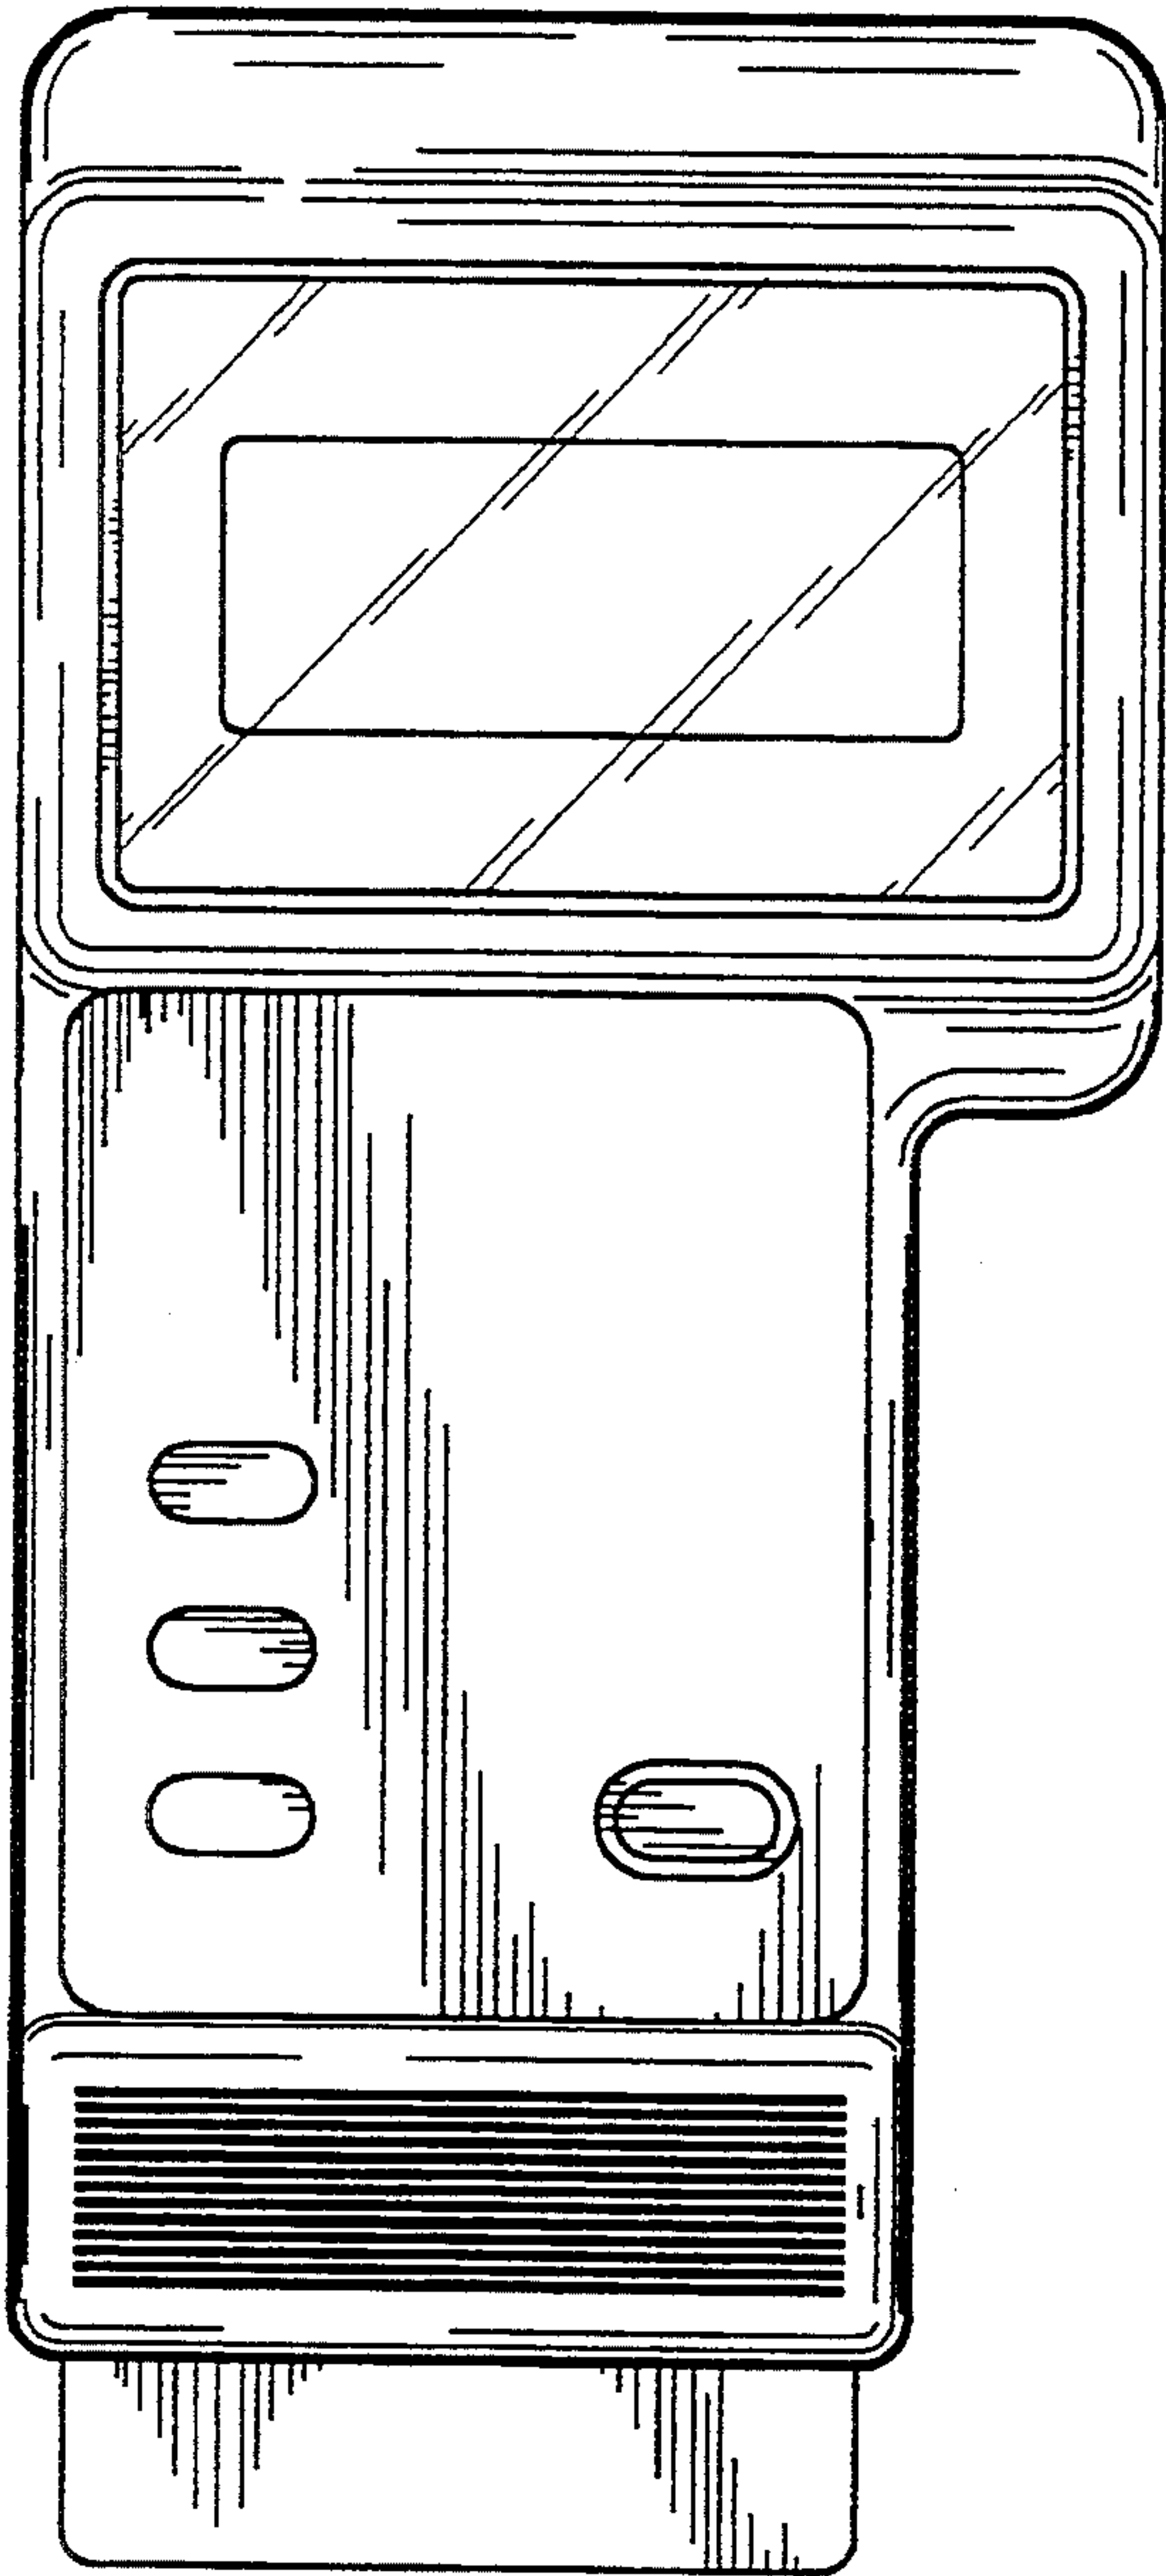


Fig.3

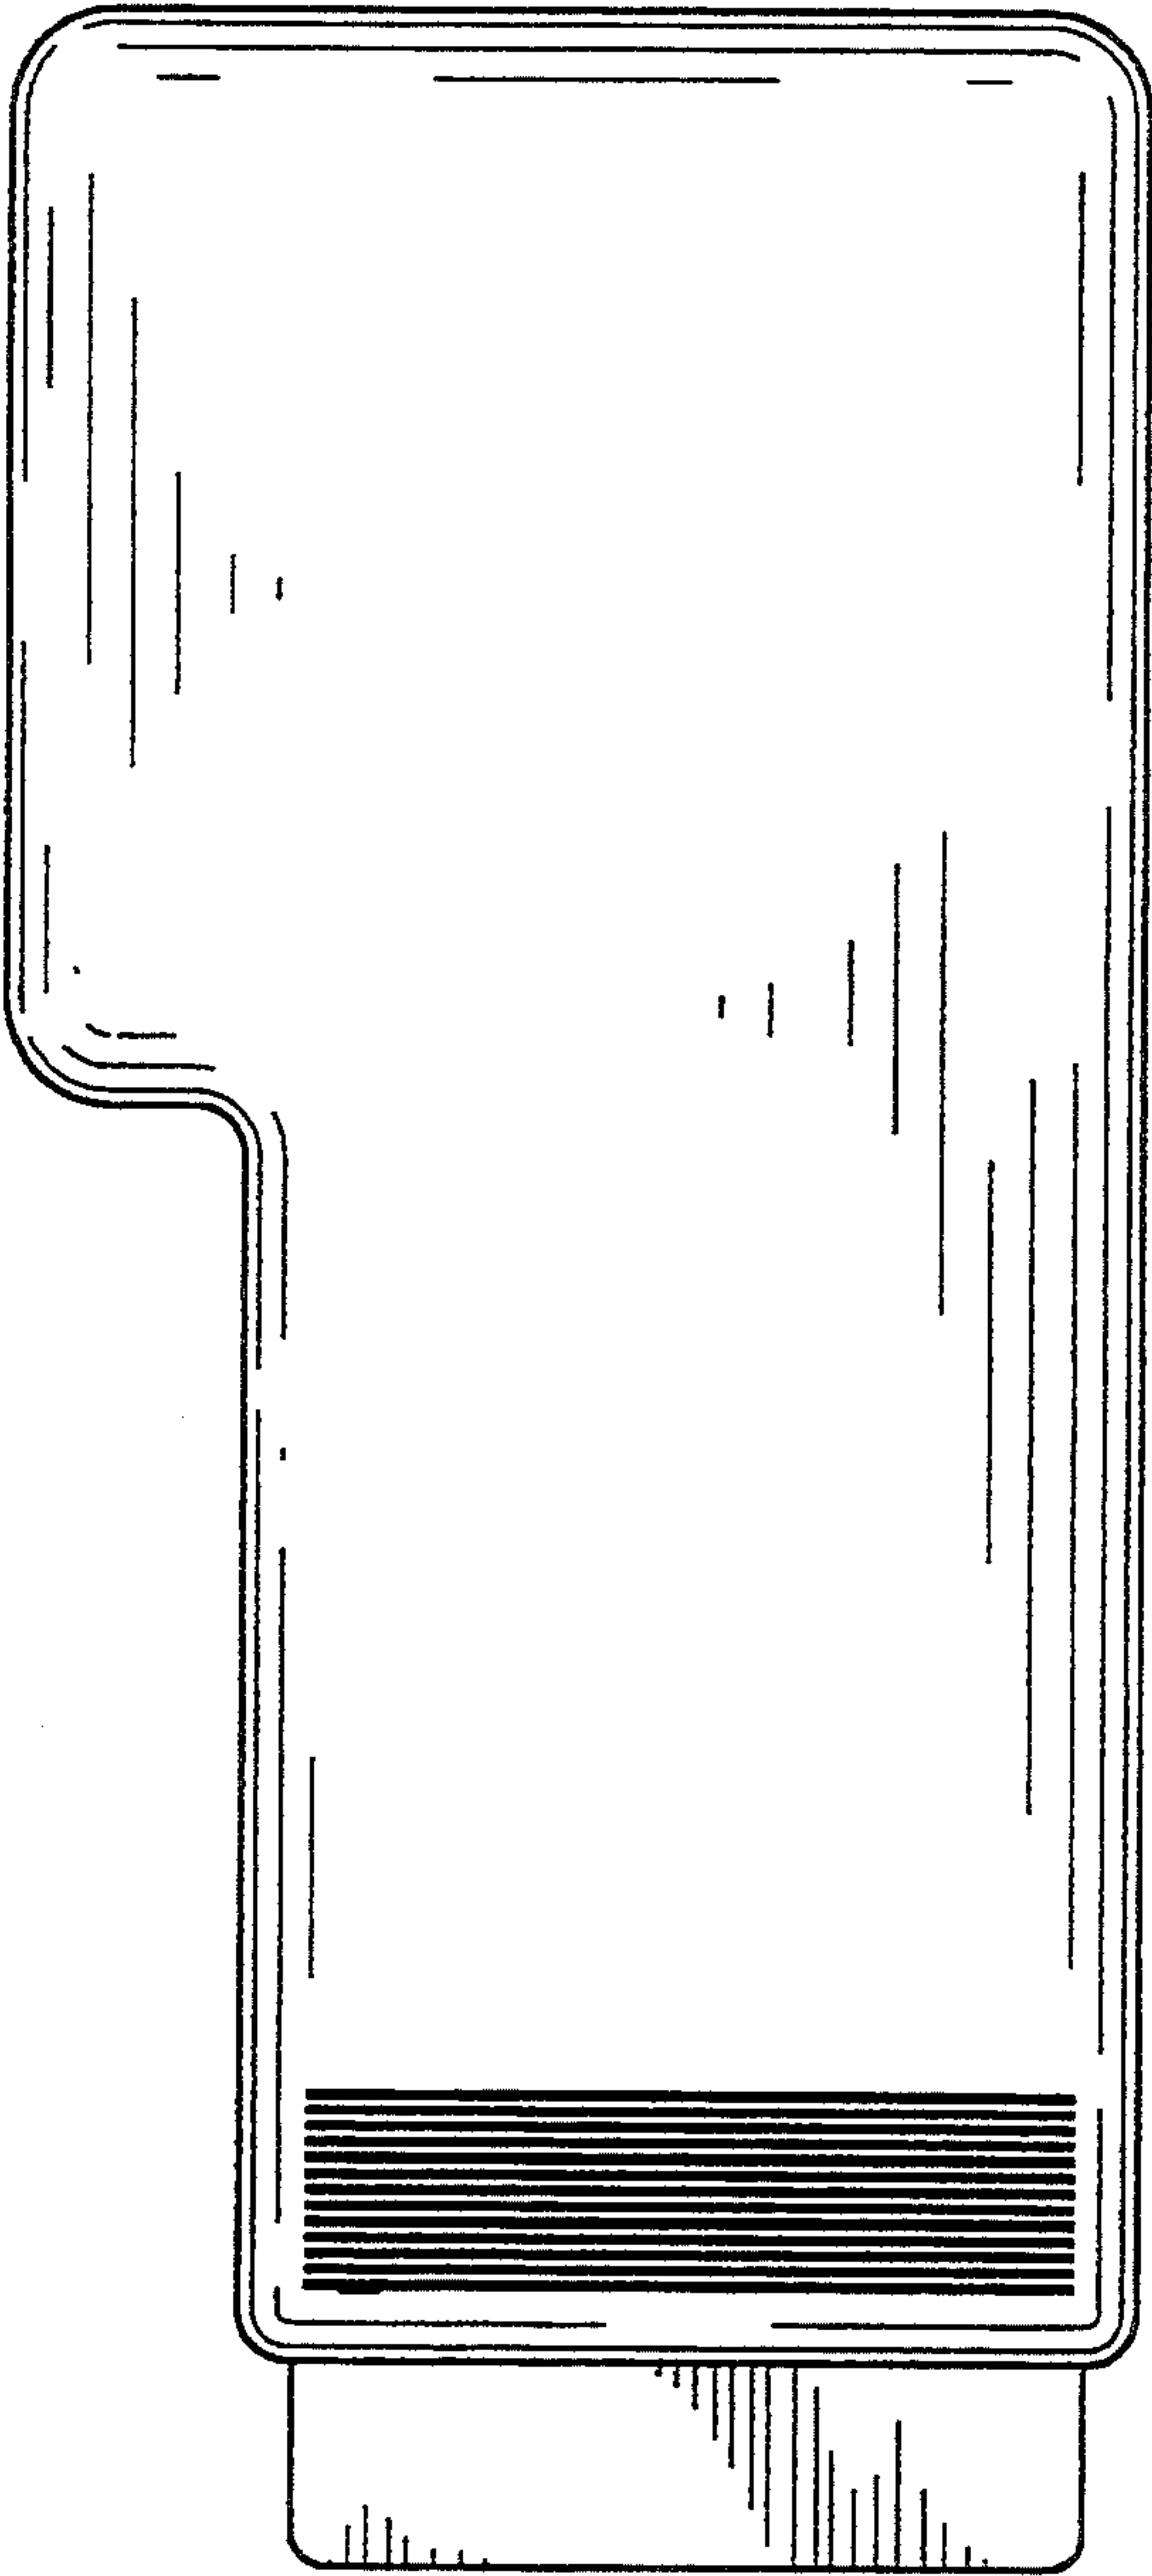


Fig.4

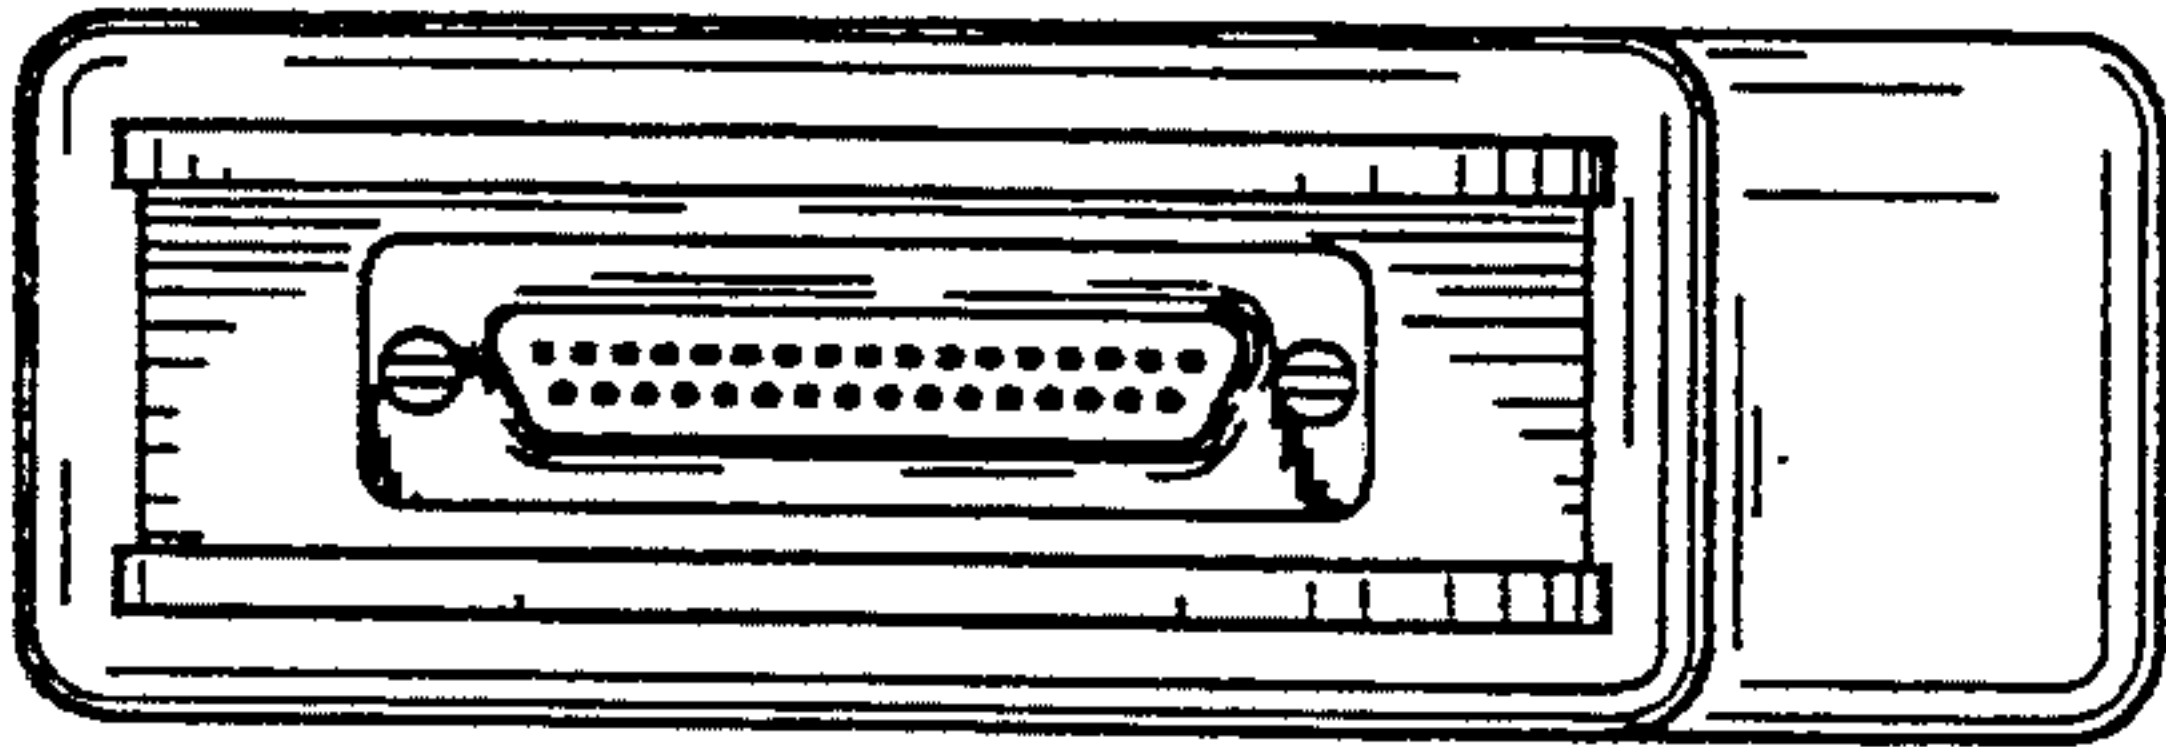


Fig.5

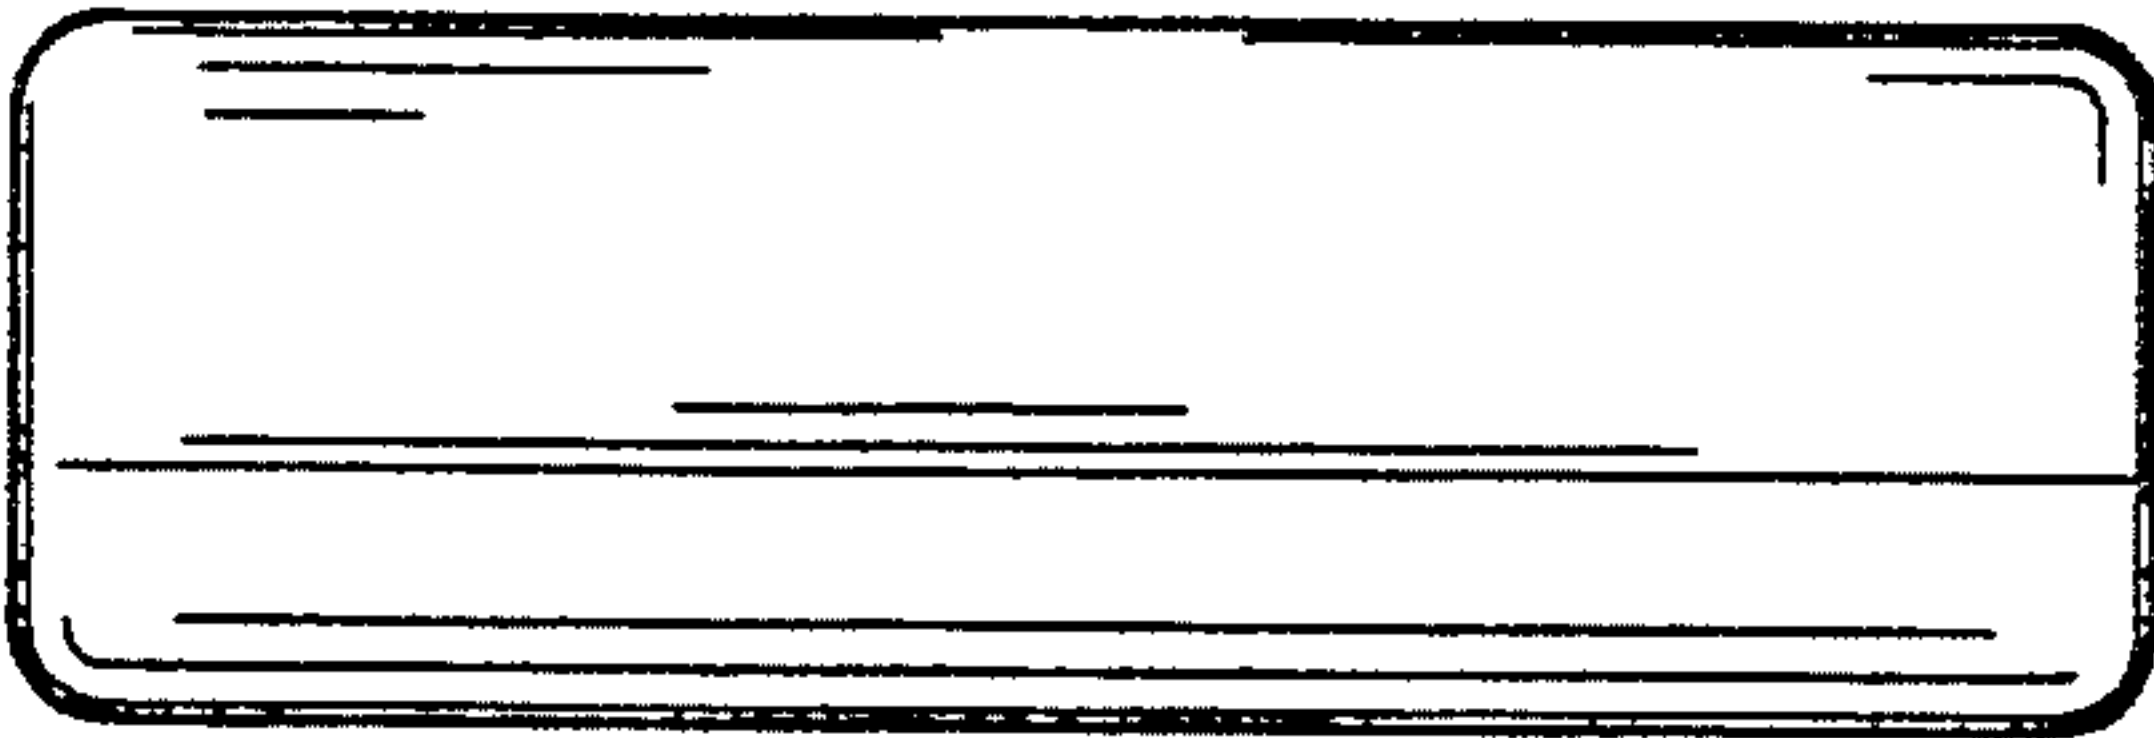


Fig.6

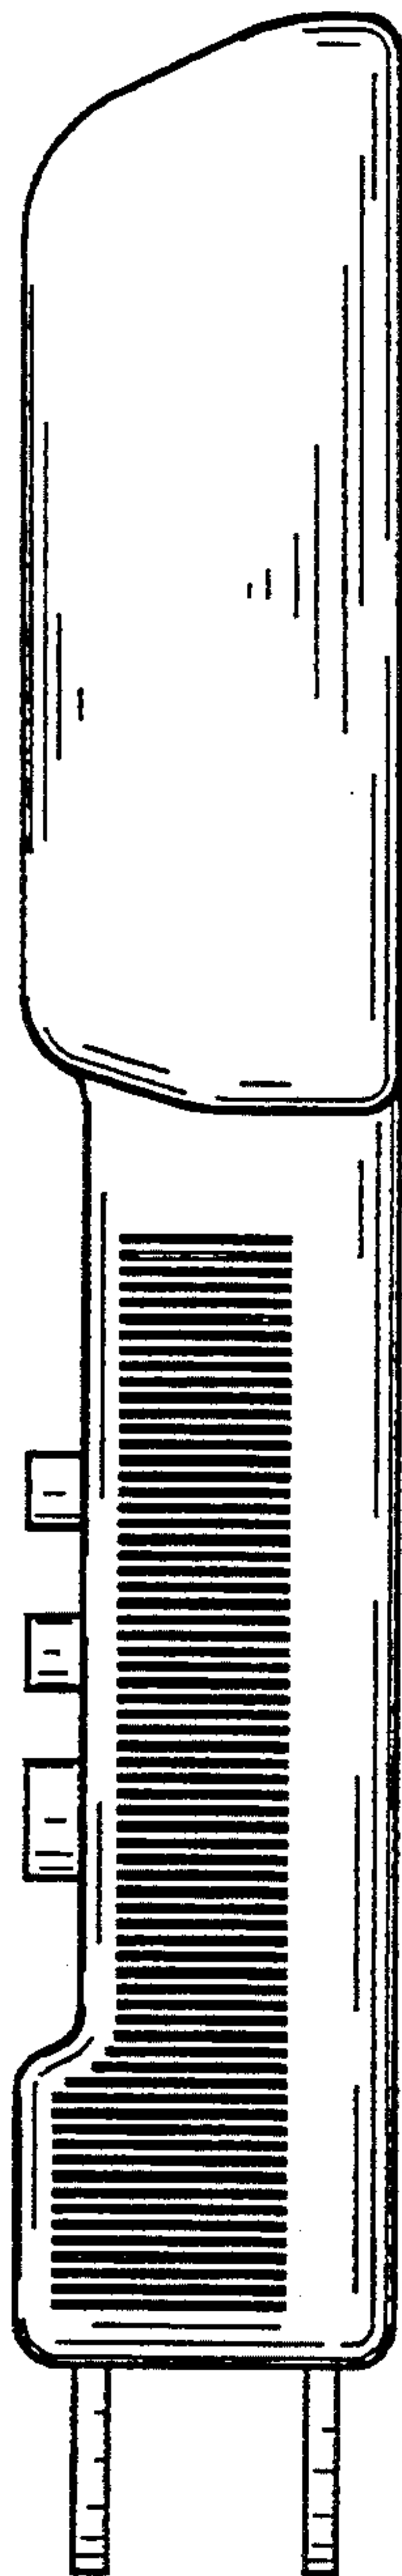


Fig.7

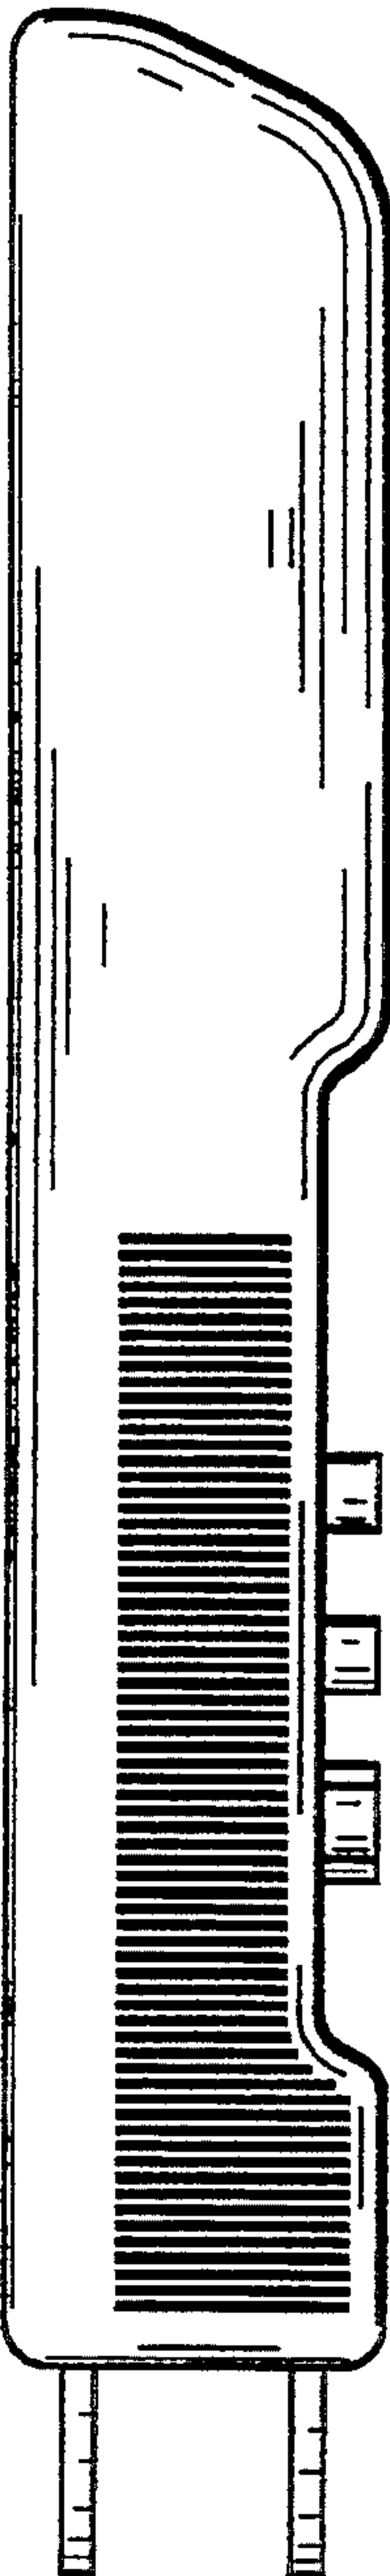


Fig.8

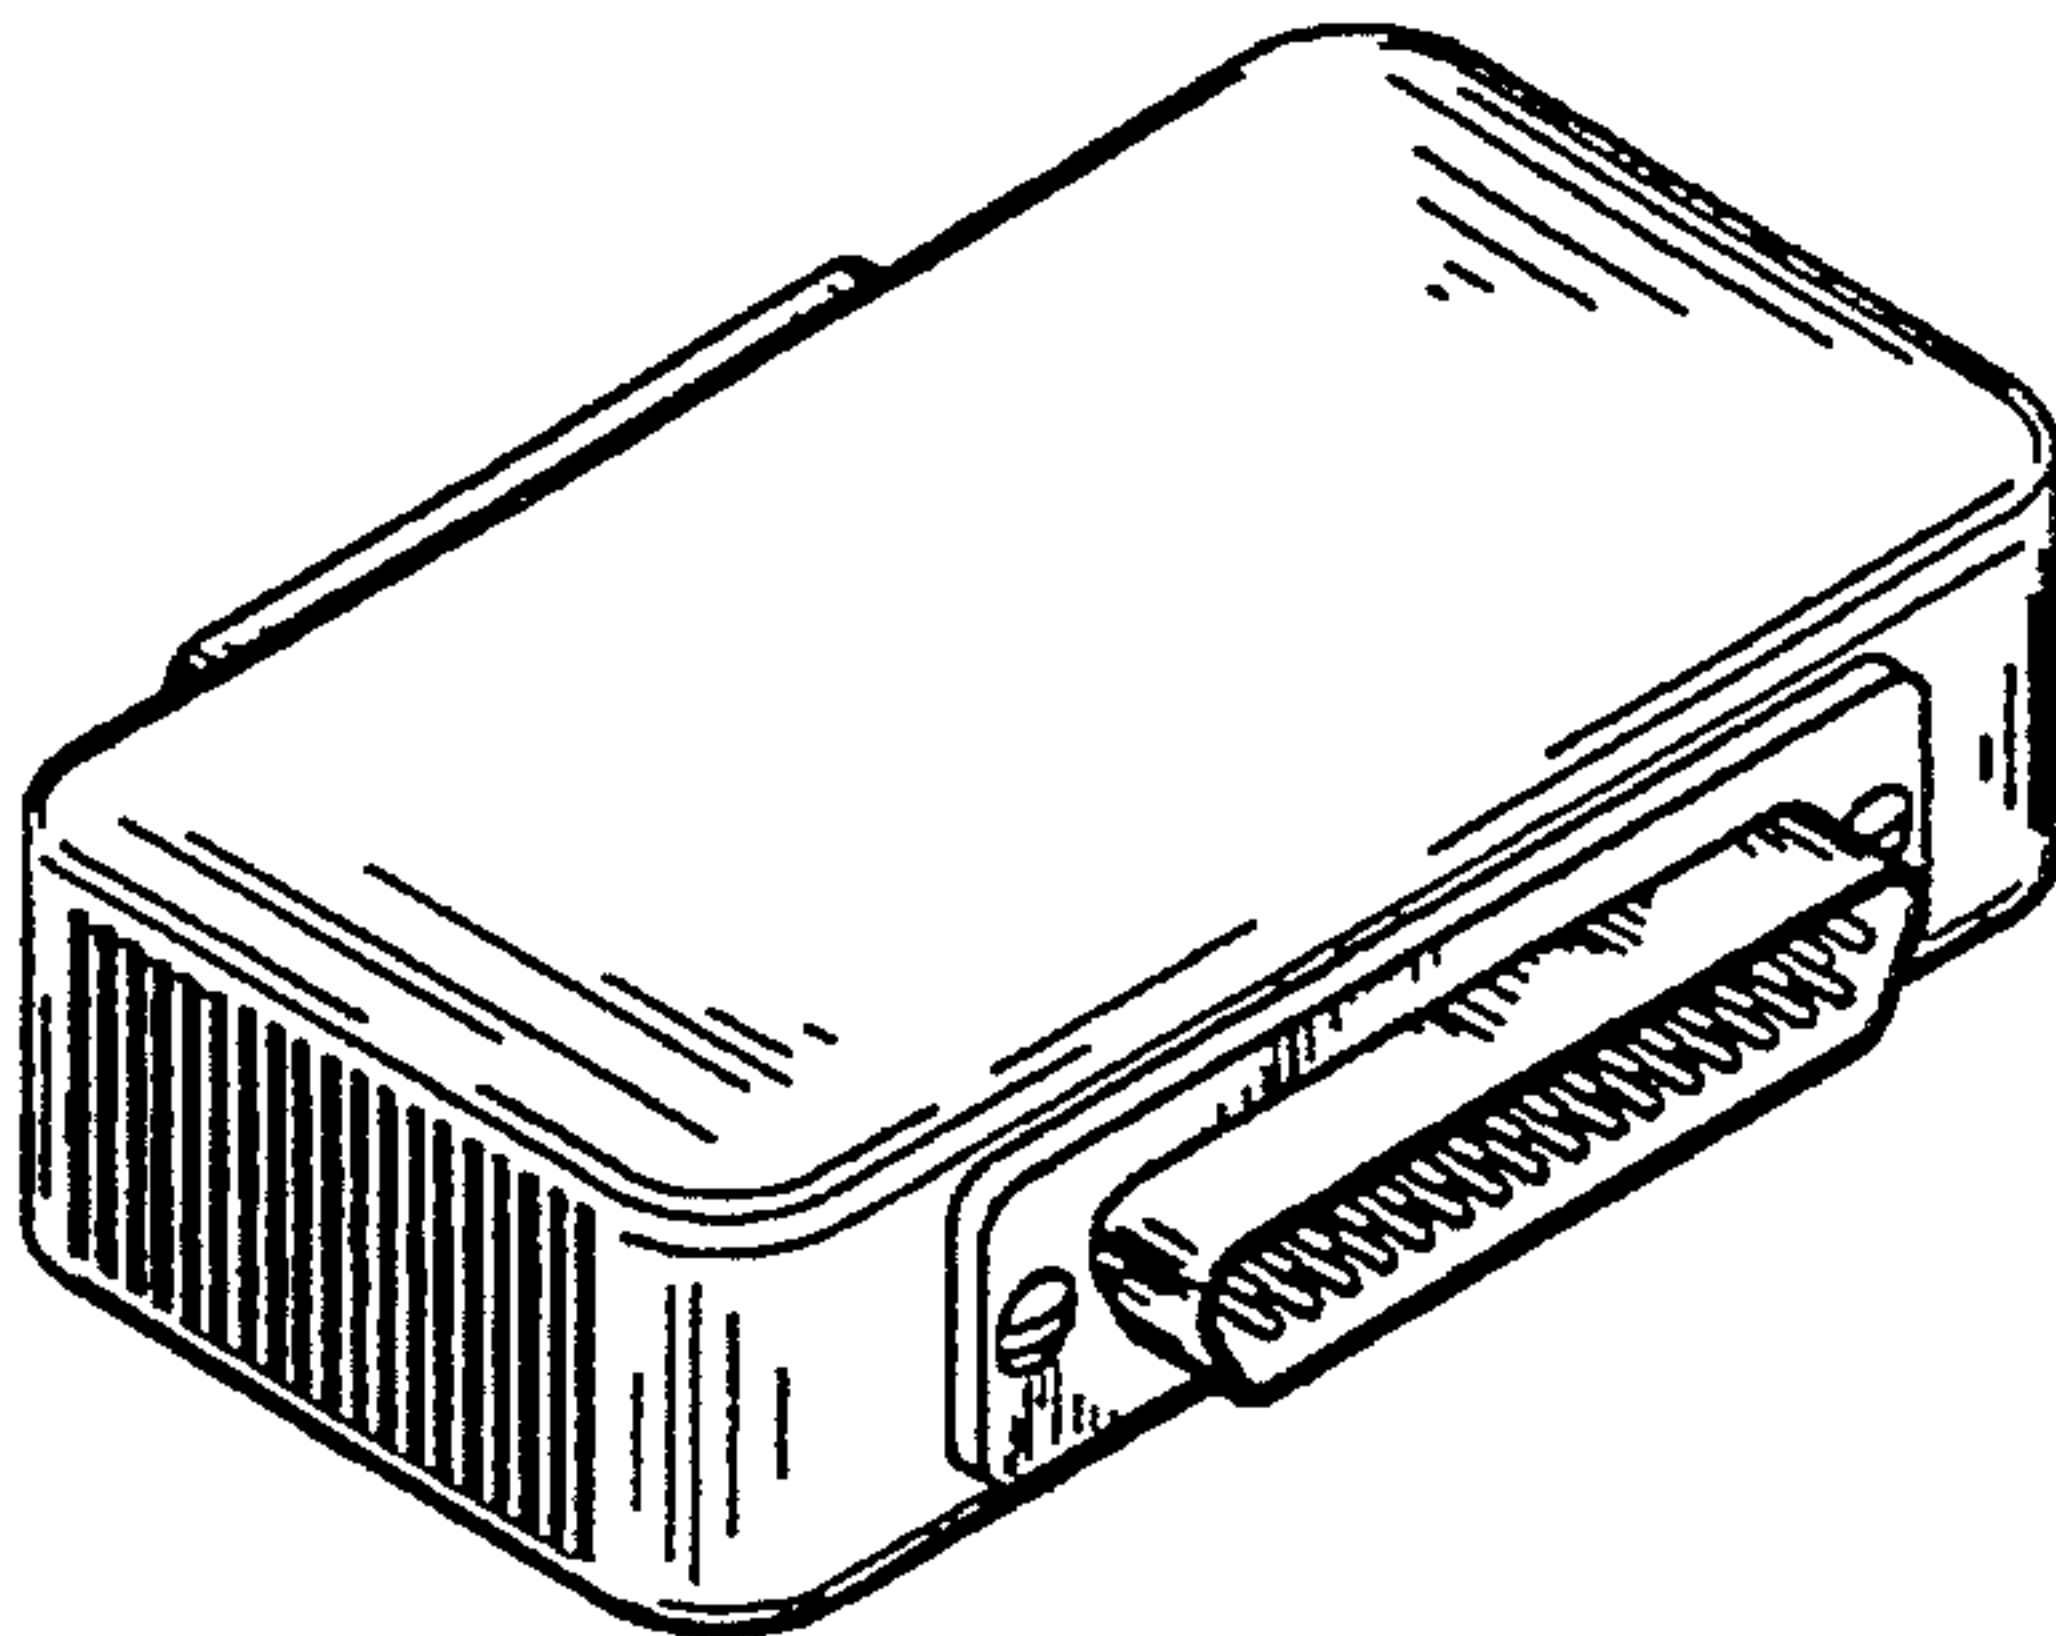


Fig.9

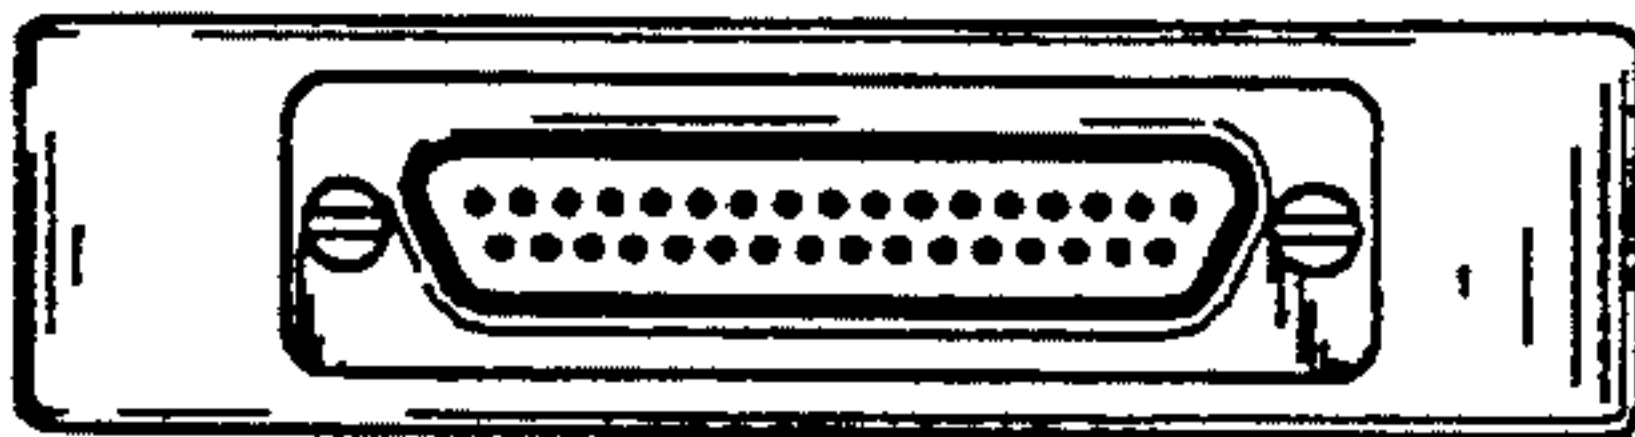


Fig.10

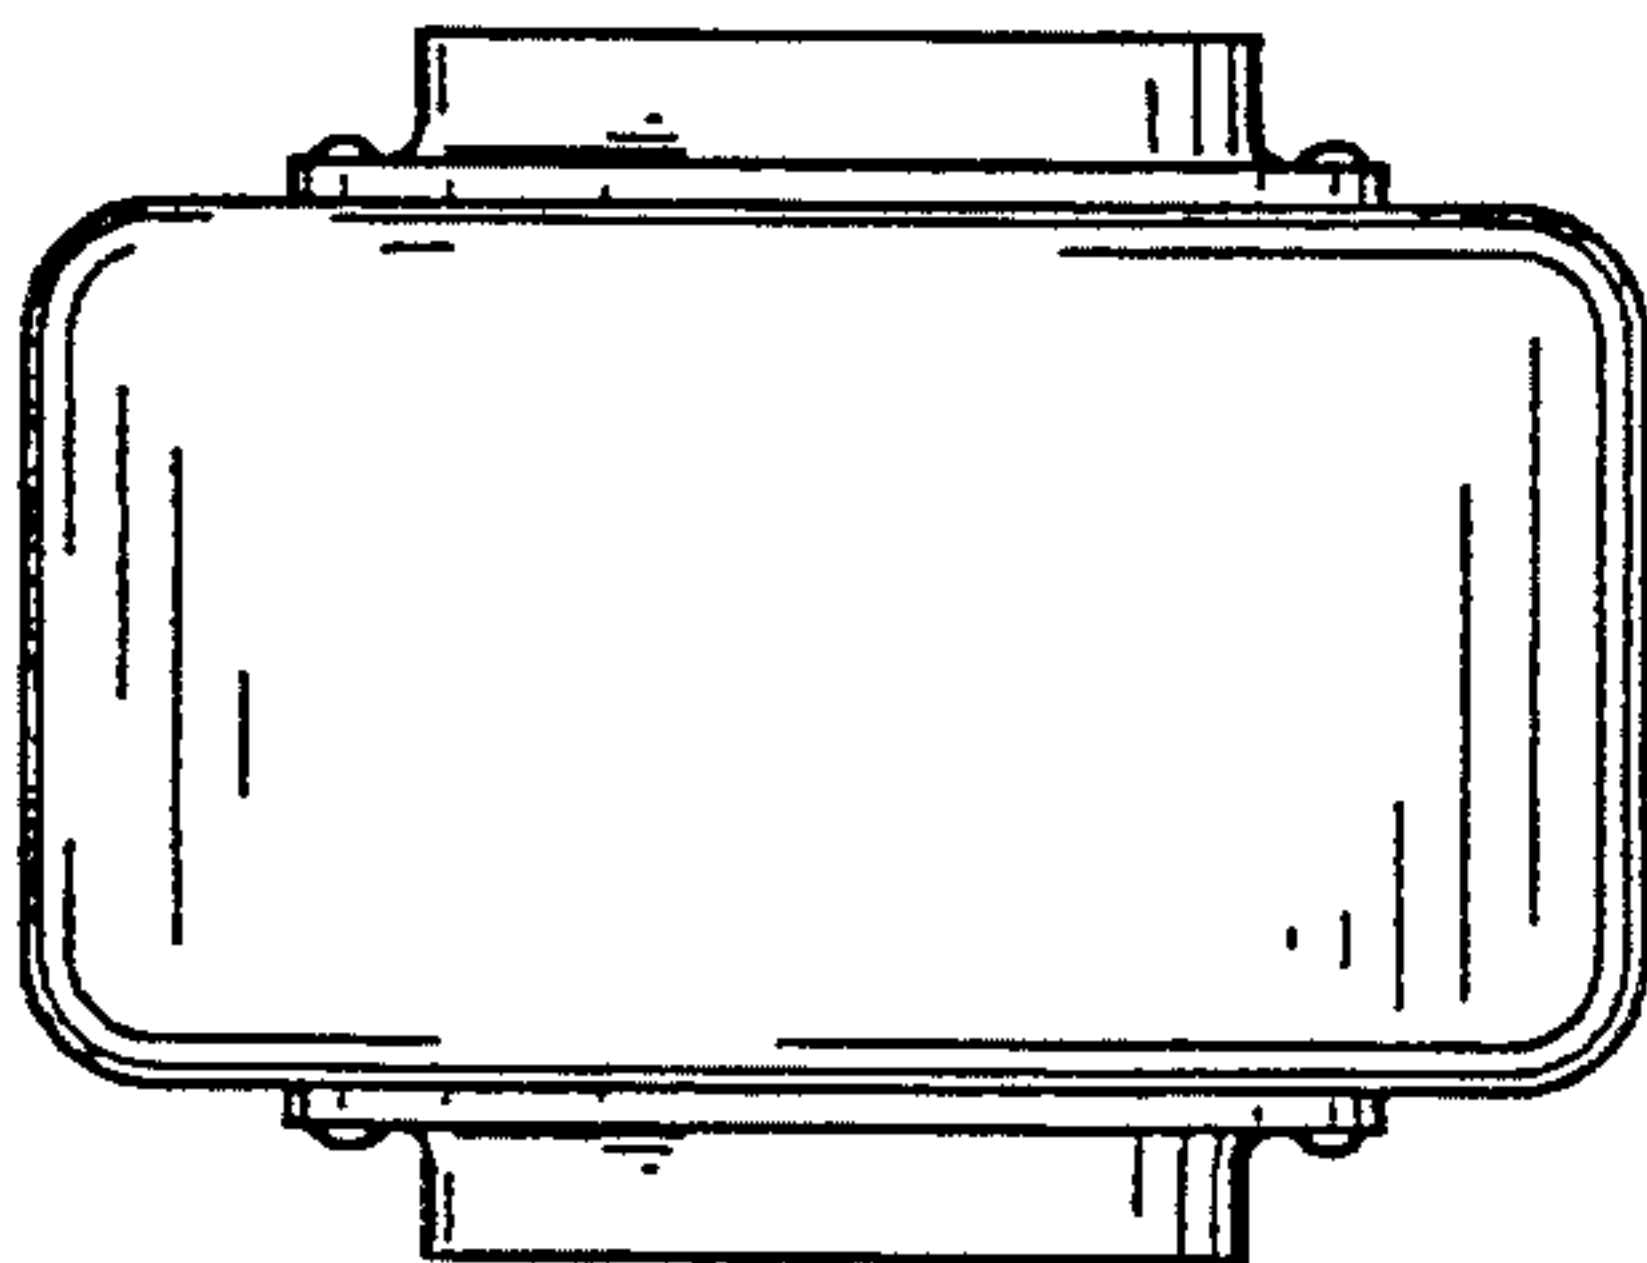


Fig.11



Fig.12

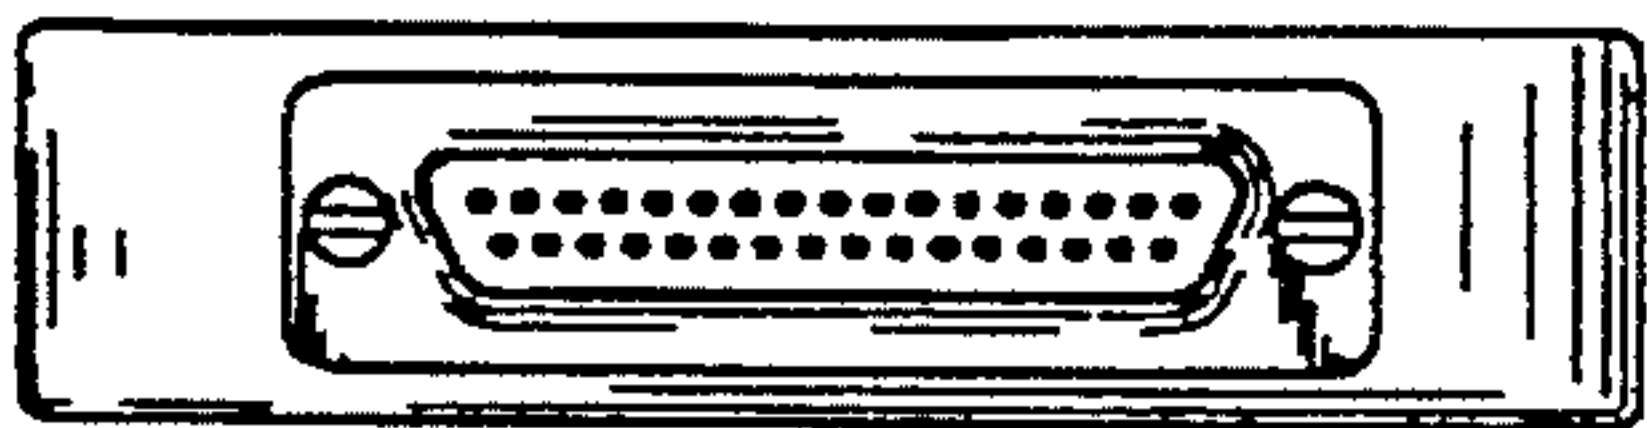


Fig.13