



US00D361129S

United States Patent [19]

Collins et al.

[11] Patent Number: Des. 361,129

[45] Date of Patent: ** Aug. 8, 1995

[54] COMBINED BLOOD COAGULATION MEASURING INSTRUMENT AND TEST STRIP

[75] Inventors: Rick L. Collins, Cicero; Martin T. Gerber, Carmel; Daniel L. Kennedy; Brett S. Lewis, both of Indianapolis, all of Ind.; James D. Morrow, Oakpark, Ill.; Peter L. Sebastian, Worms, Germany; David E. Storvick, Indianapolis; Charles L. Thomeczek, Jr., Fishers, both of Ind.

[73] Assignee: Boehringer Mannheim Corporation, Indianapolis, Ind.

[**] Term: 14 Years

[21] Appl. No.: 14,881

[22] Filed: Nov. 2, 1993

[52] U.S. Cl. D24/169; D24/186

[58] Field of Search D24/216, 169, 186, 232, D24/231, 169, 225; 430/66; 422/73, 63, 99, 102; 128/635, 770, 771, 763, 764, 765; 73/864.91, 864.87, 864.81

[56] References Cited

U.S. PATENT DOCUMENTS

D. 318,331	7/1991	Phillips et al.	D24/186 X
D. 325,781	4/1992	Moller-Jensen	D24/169
4,599,219	7/1986	Cooper et al.	422/61
5,110,727	5/1992	Oberhardt	422/58 X
5,231,576	7/1993	Suzuki et al.	128/677 X
5,281,395	1/1994	Markart et al.	D24/232 X
5,302,348	4/1994	Cusack et al.	422/102 X

Primary Examiner—A. Hugo Word

Assistant Examiner—I. Simmons

Attorney, Agent, or Firm—Barnes & Thornburg

[57] CLAIM

The ornamental design for a combined blood coagulation measuring instrument and test strip, as shown and described.

DESCRIPTION

FIG. 1 is a front elevational view of the blood coagulation measuring instrument as seen in FIG. 6, with the test strip removed;

FIG. 2 is a top plan view;

FIG. 3 is a right side elevational view, with the left side elevational view being a mirror image thereof;

FIG. 4 is a rear elevational view;

FIG. 5 is a bottom plan view thereof;


FIG. 6 is a front elevational view of a combined blood coagulation measuring instrument and test strip showing our new design with the test strip inserted therein, the rear elevational view being a mirror image of FIG. 4;

FIG. 7 is a top plan view of the design illustrated in FIG. 6;

FIG. 8 is a right side elevational view of the design illustrated in FIGS. 6–7, with the left side elevational view of the design of FIGS. 6–7 being a mirror image of FIG. 8;

FIG. 9 is a bottom plan view of the design of FIGS. 6–8; and

FIG. 10 is a perspective view thereof, with the test strip shown in separated condition.

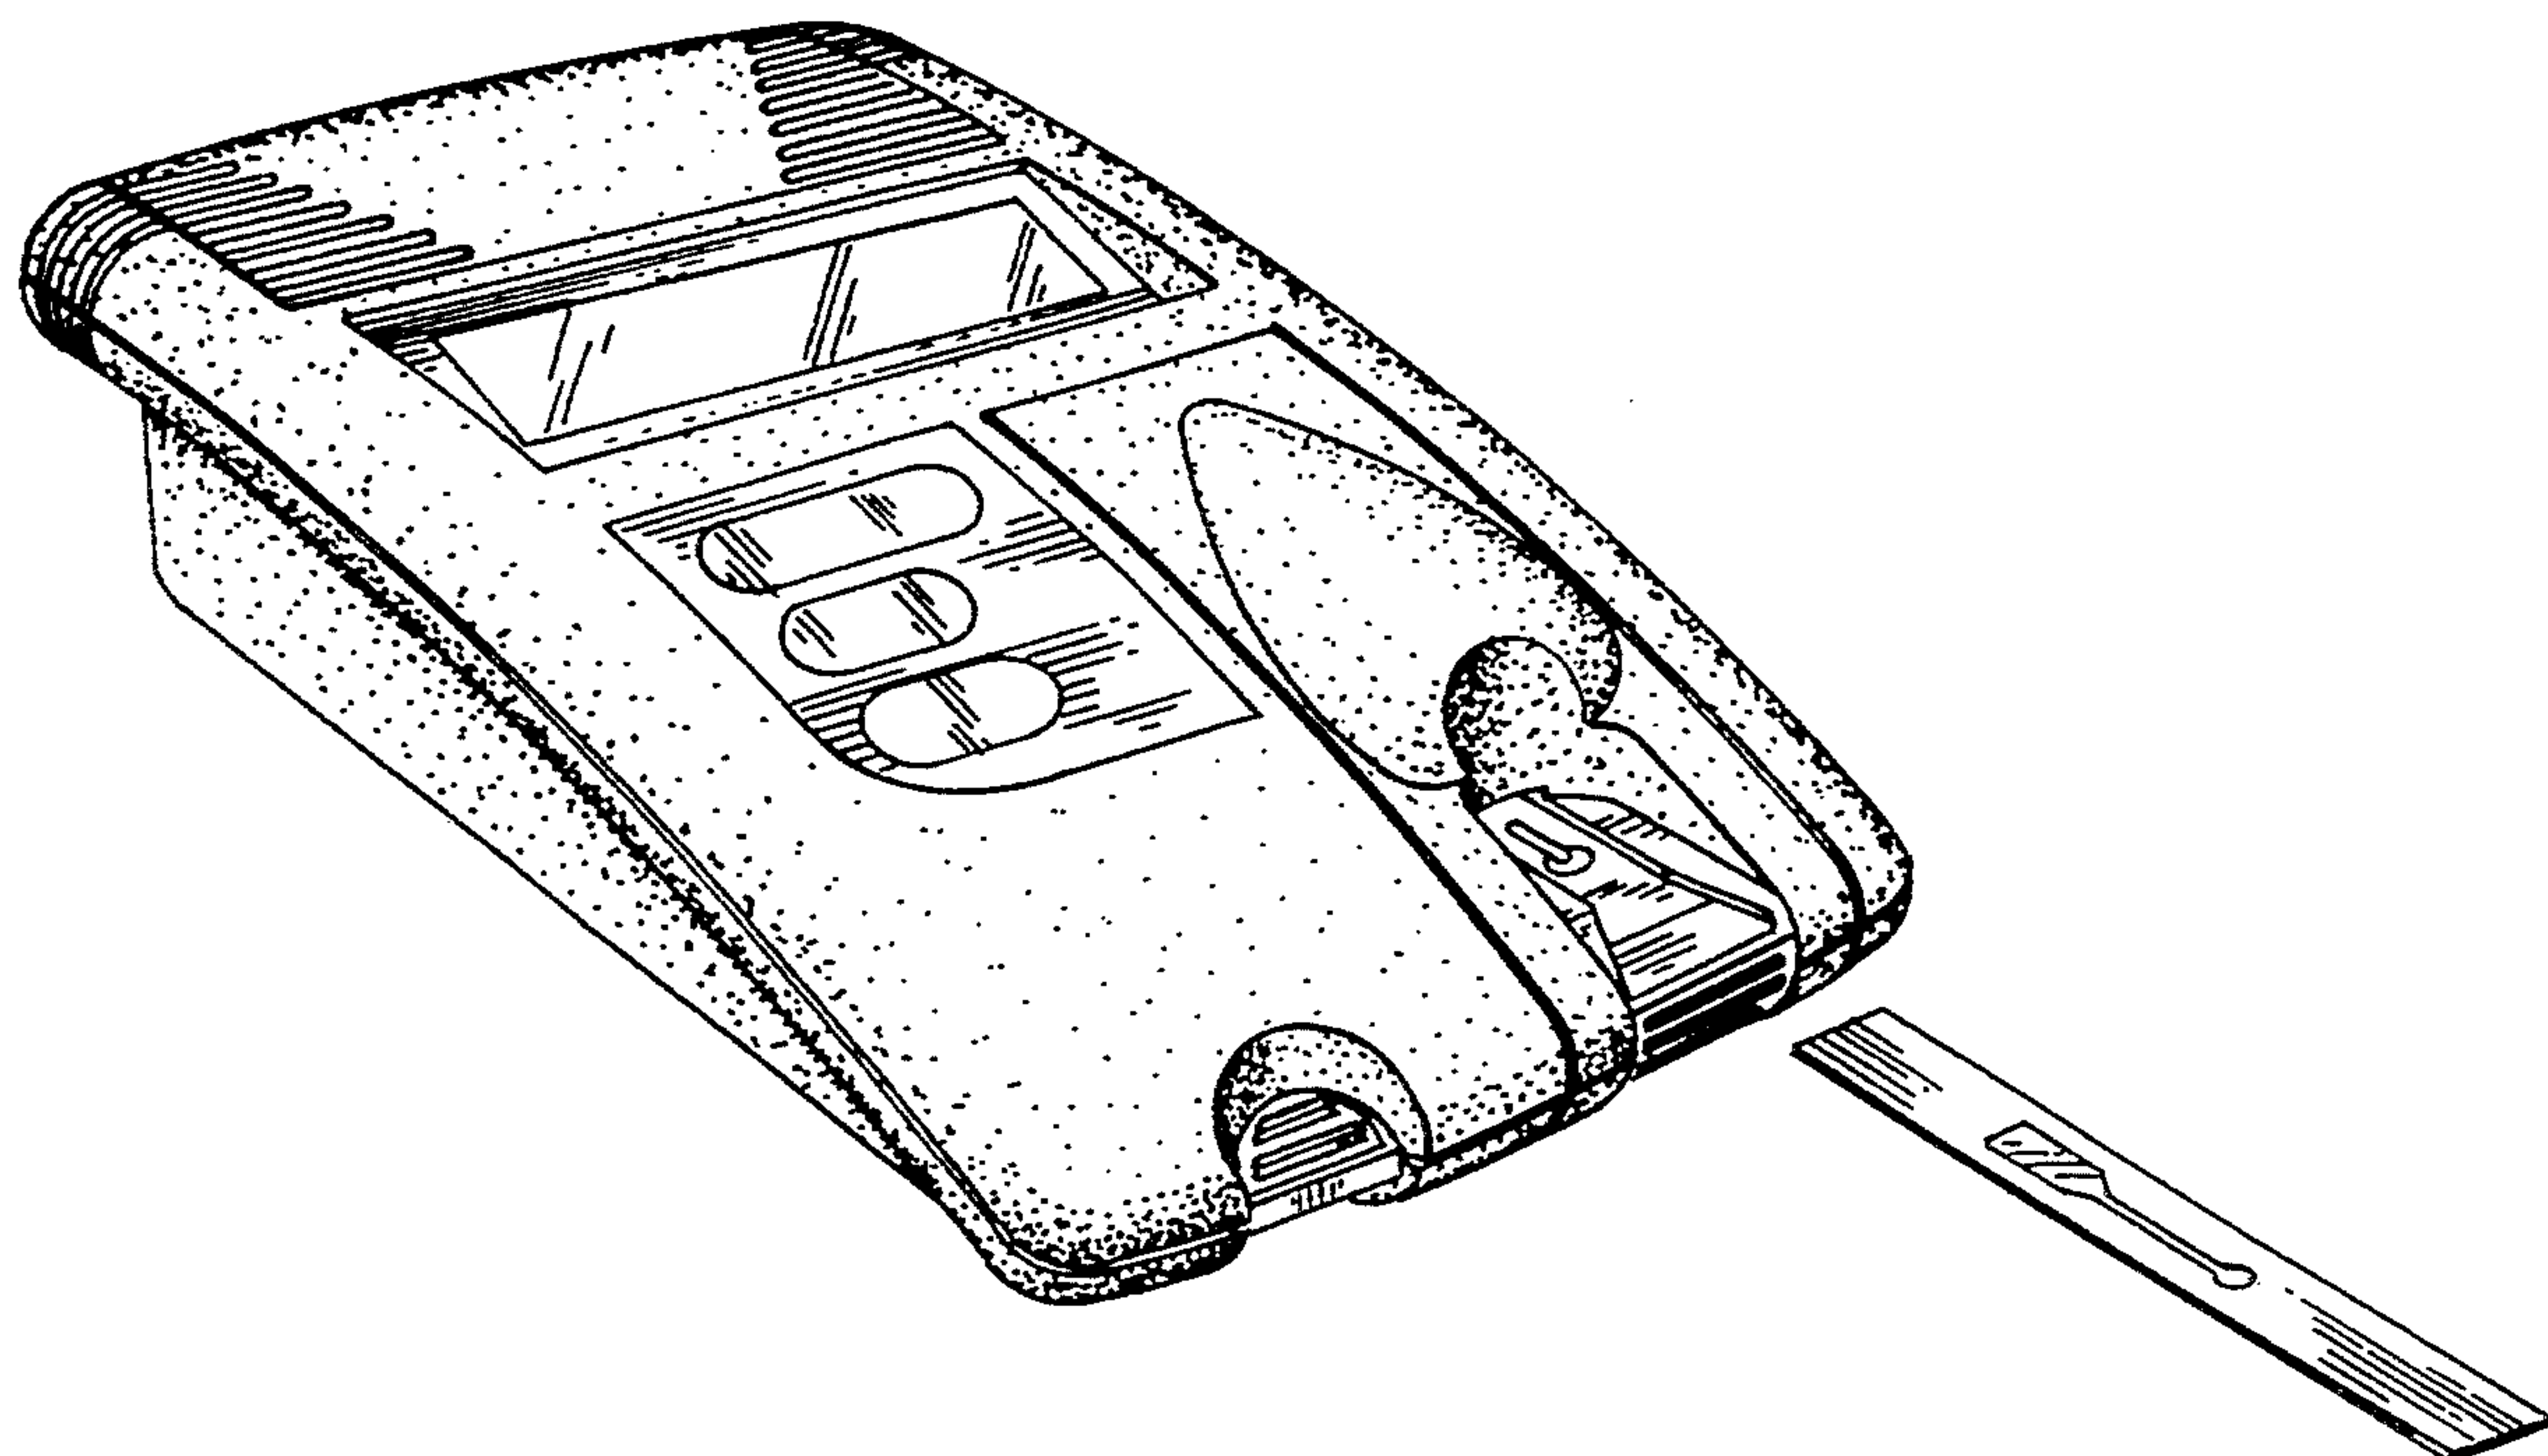

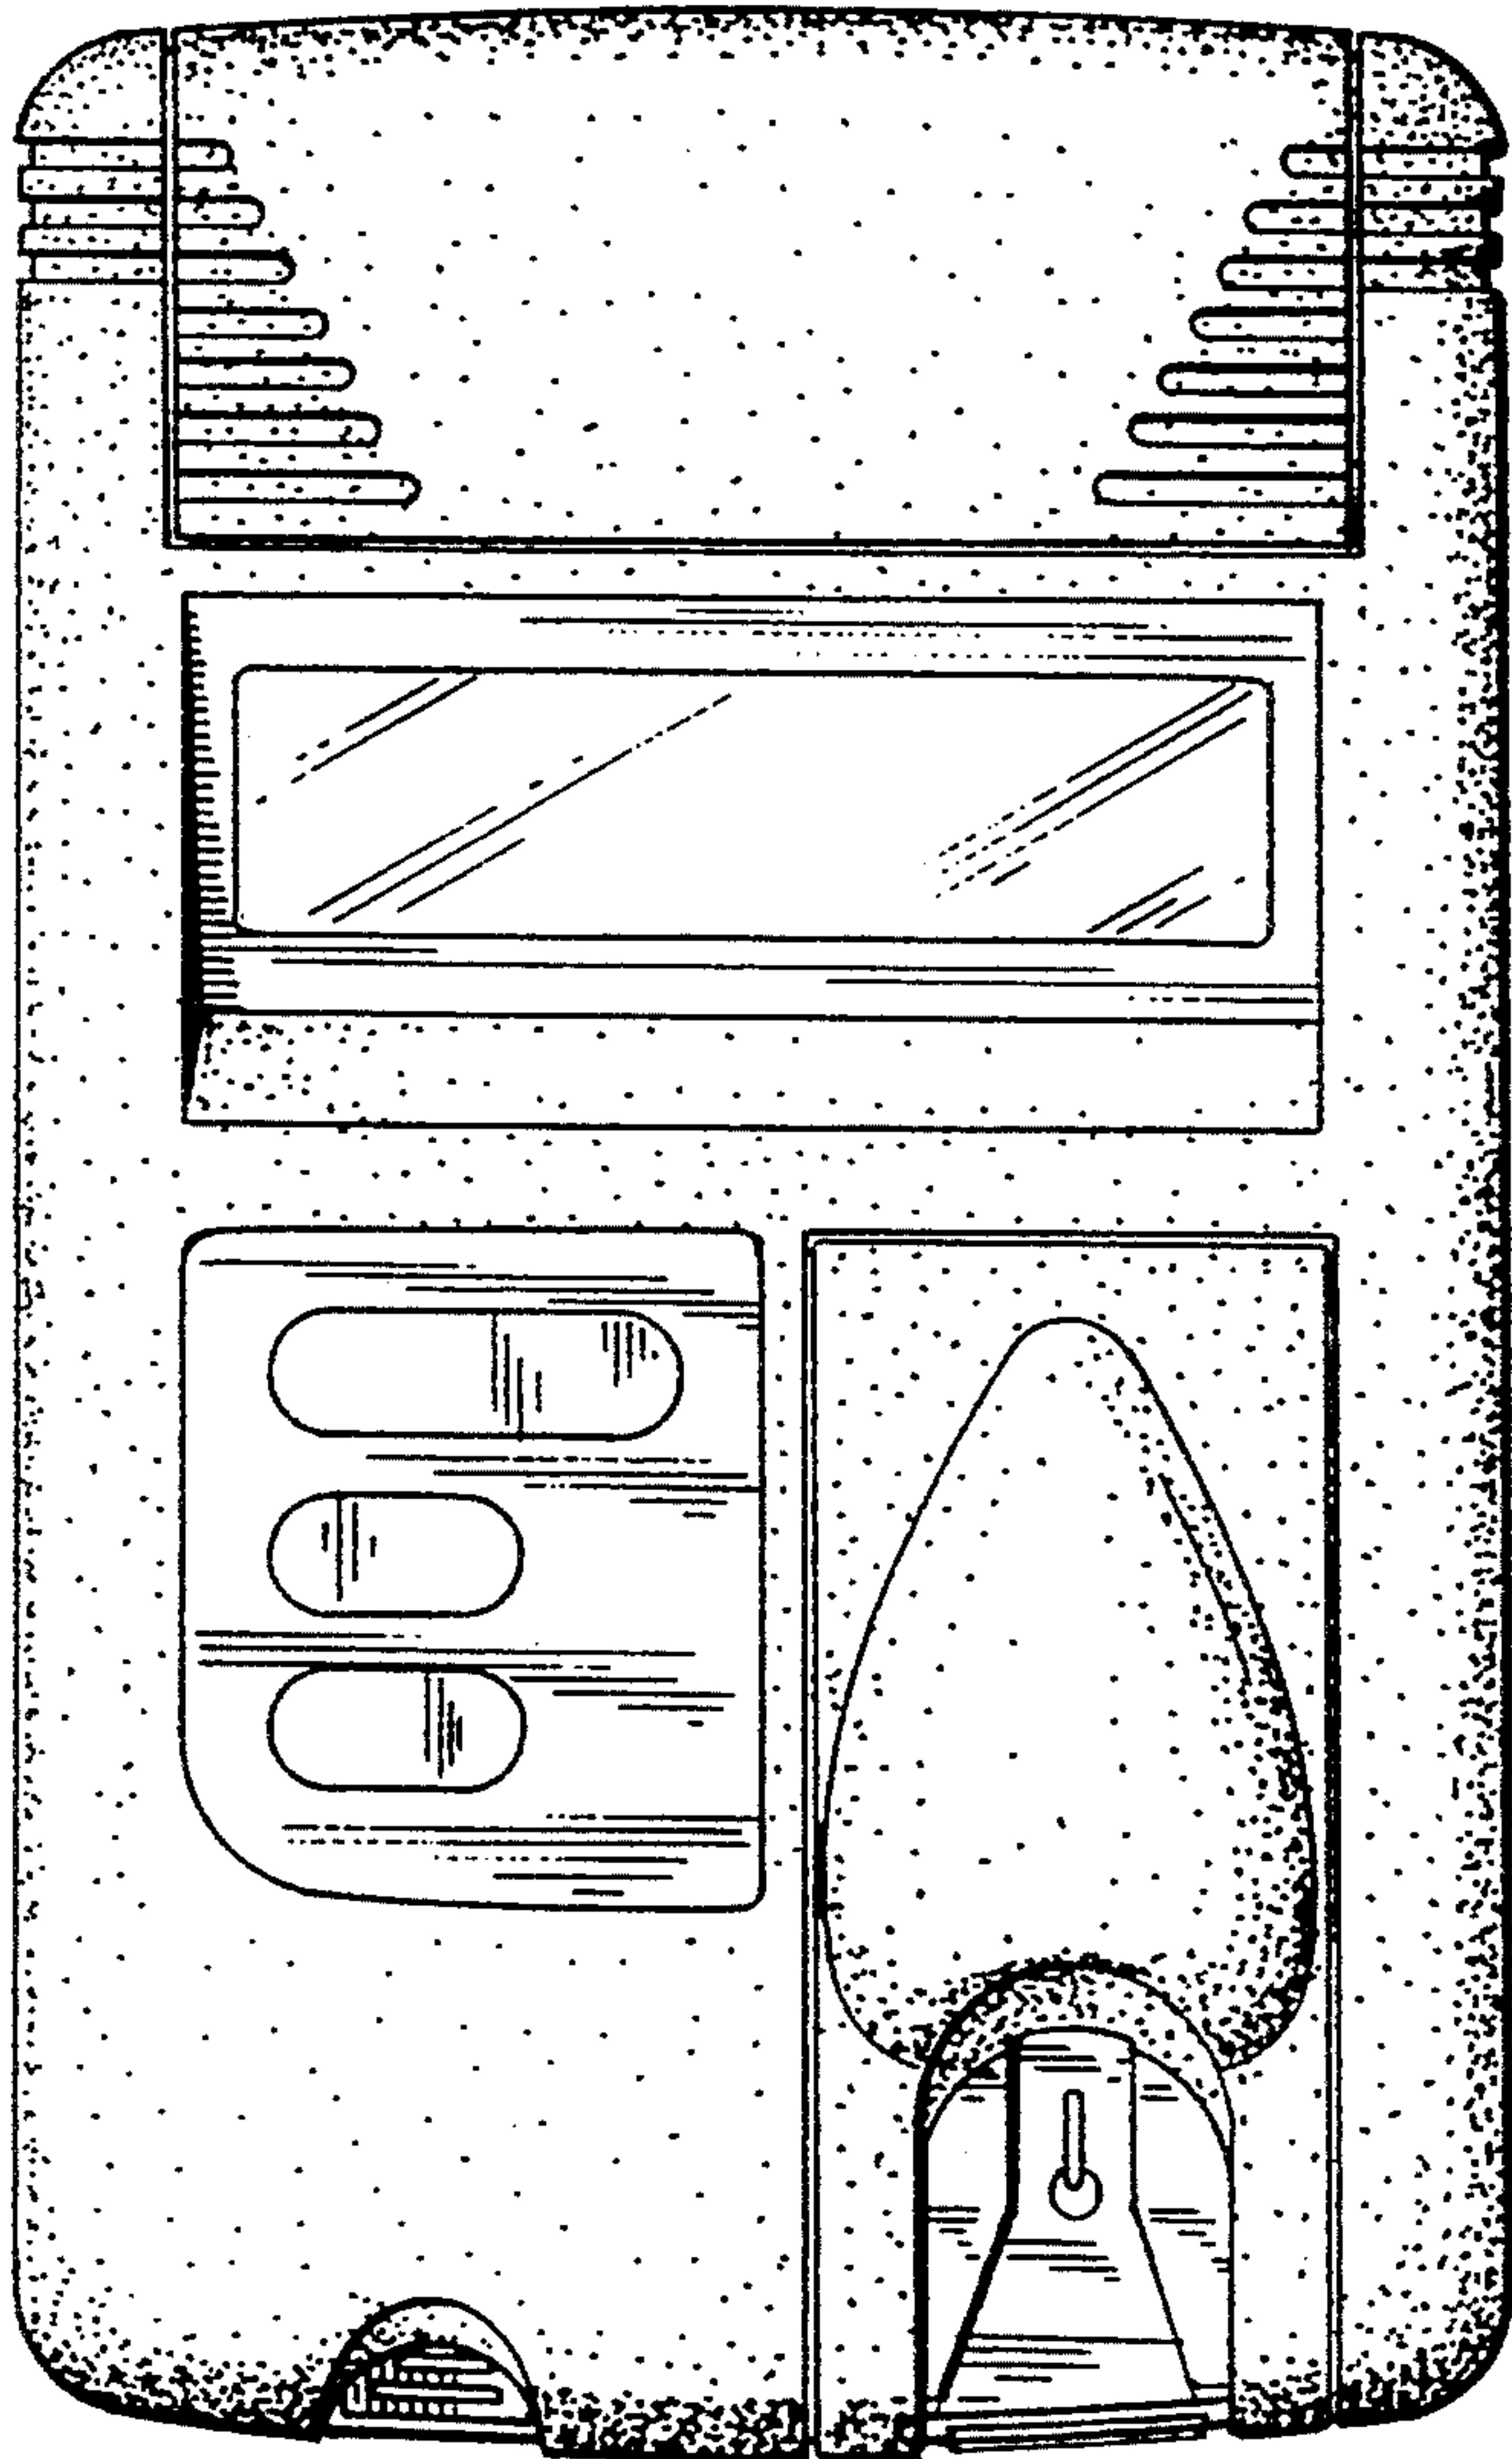


FIG. 2

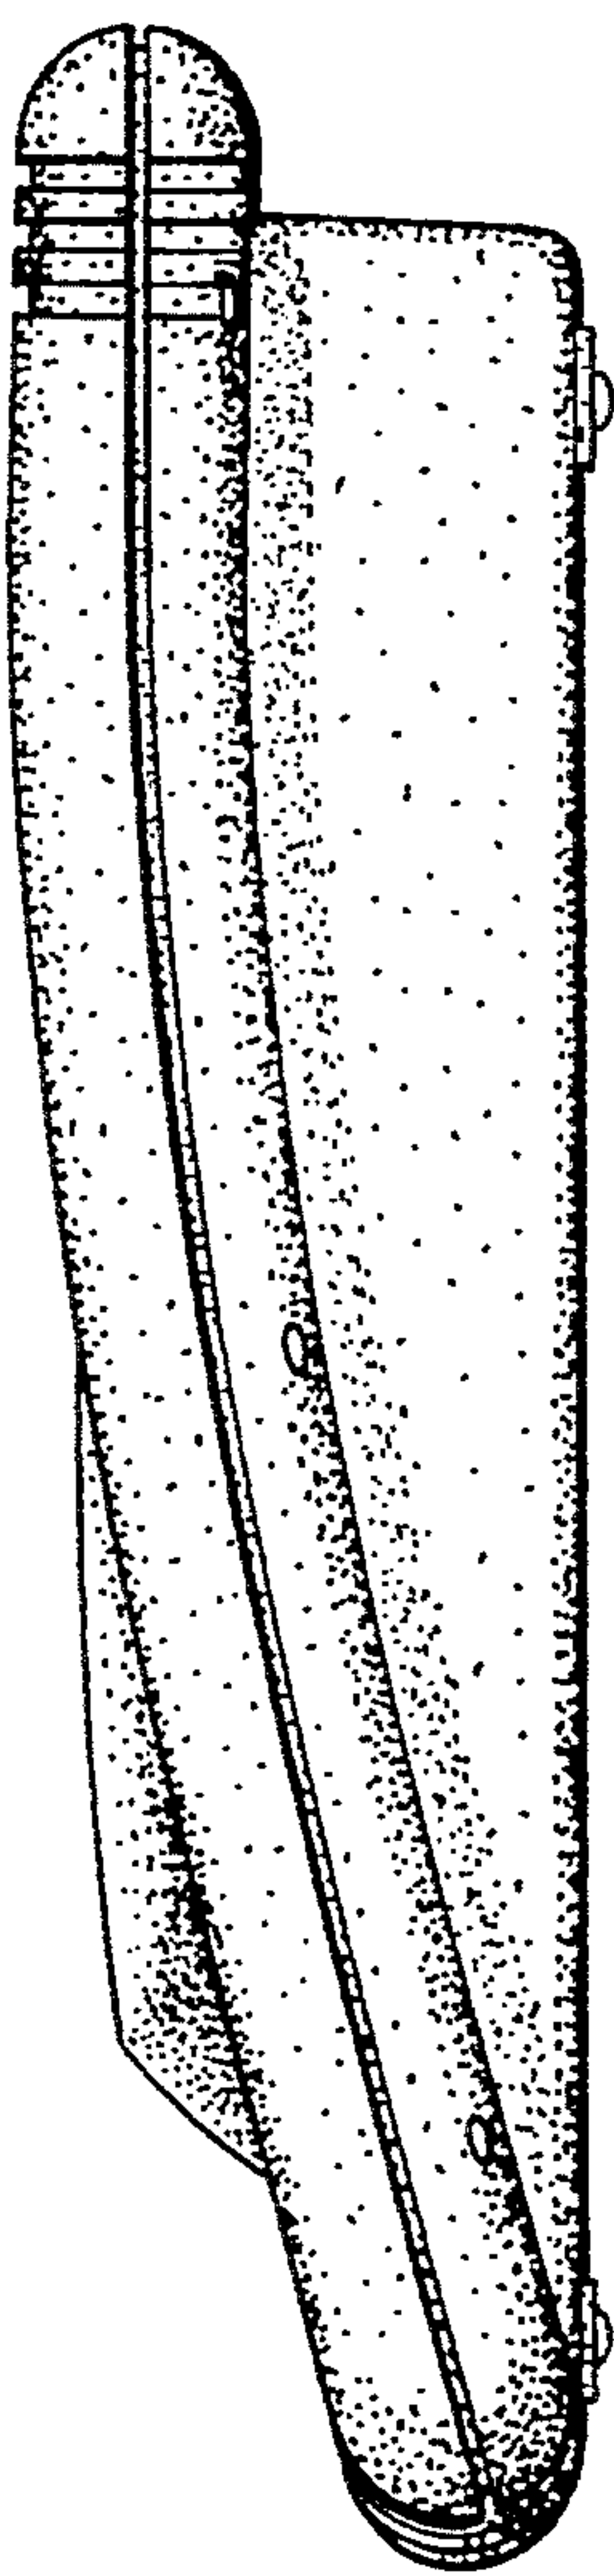


FIG. 3

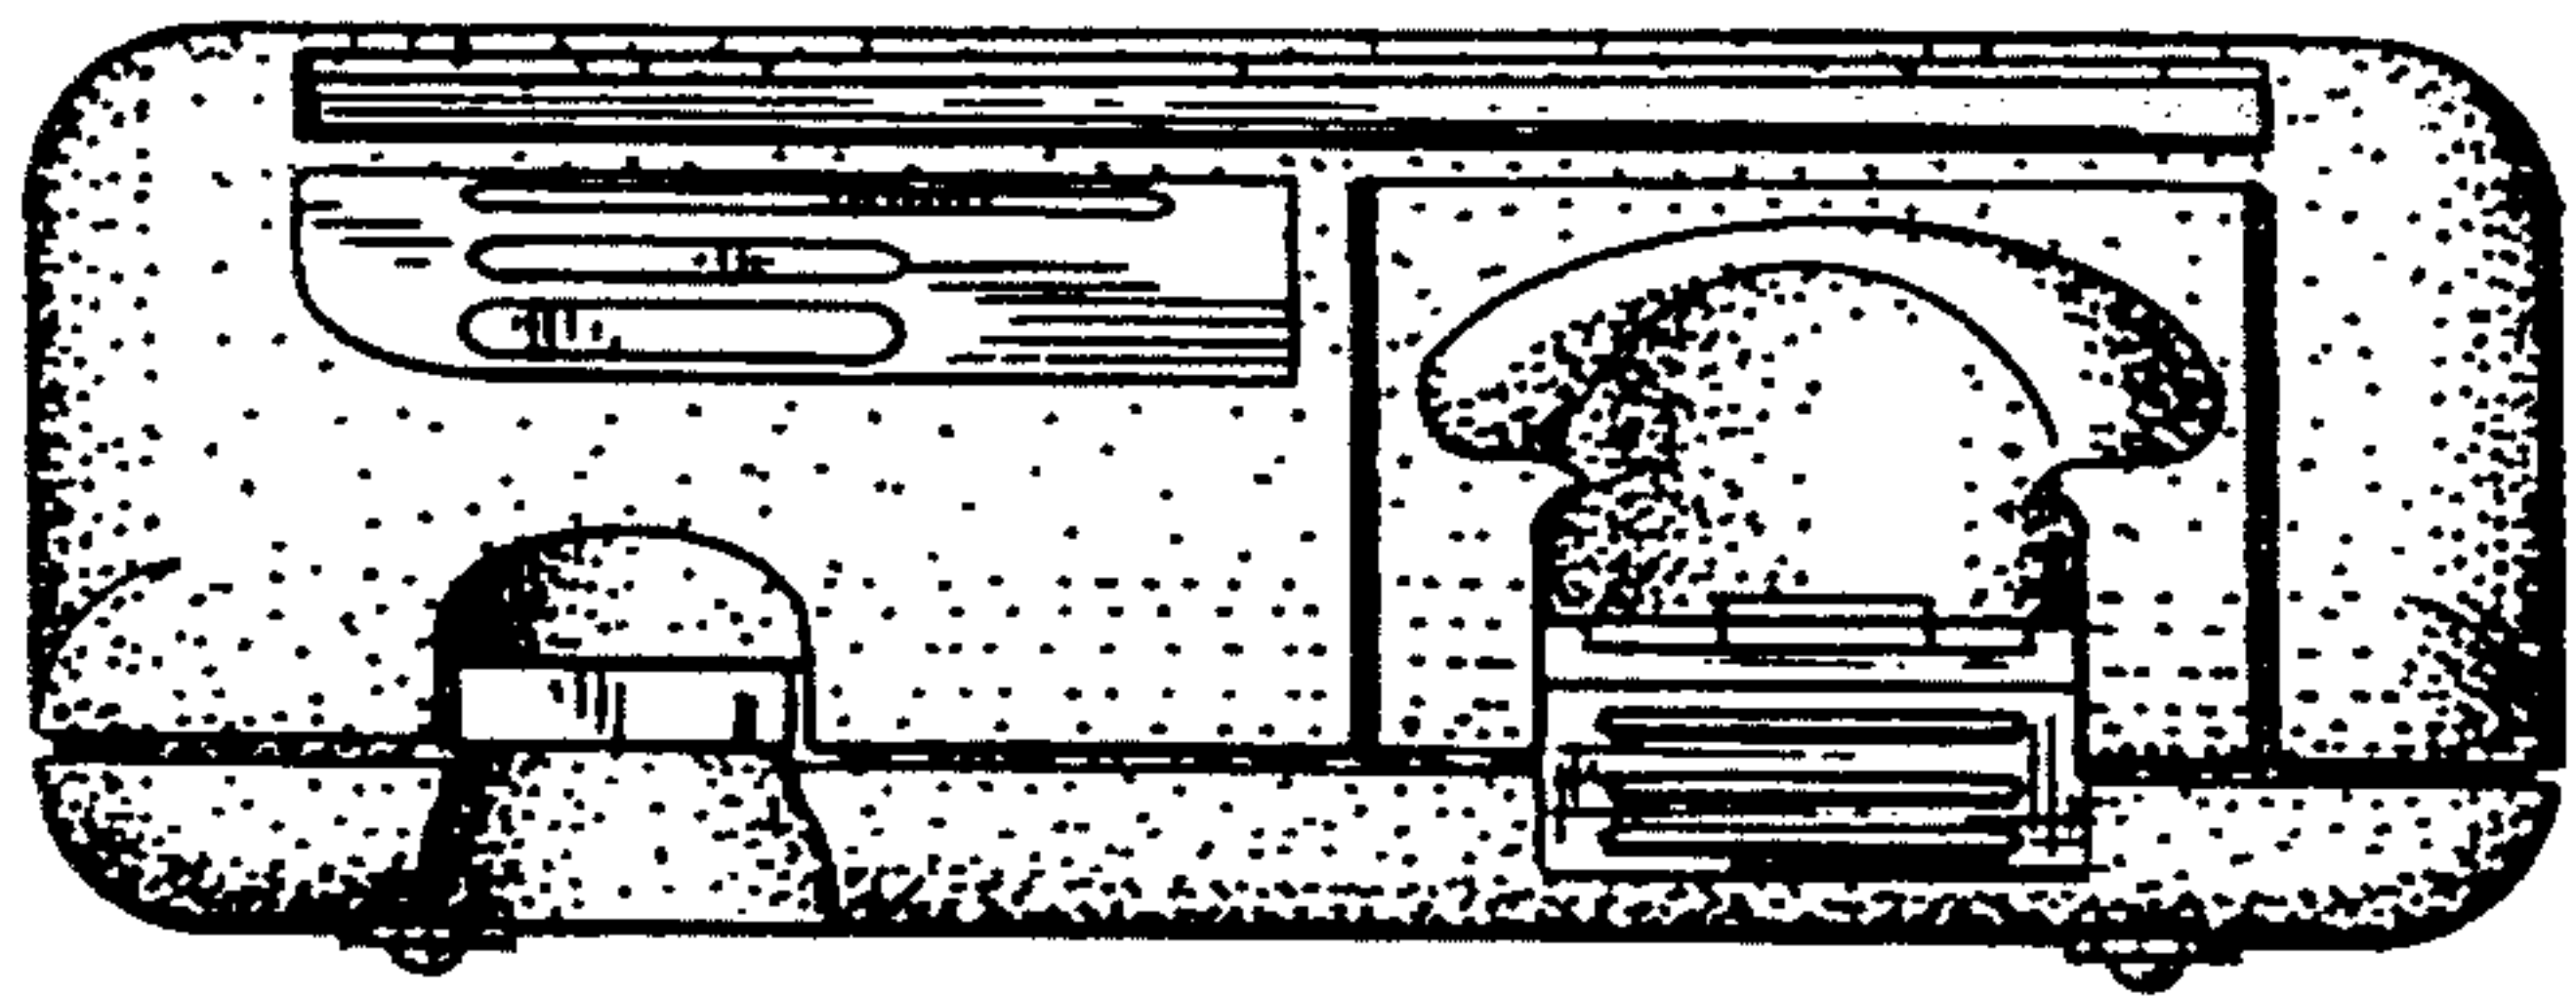


FIG. 1

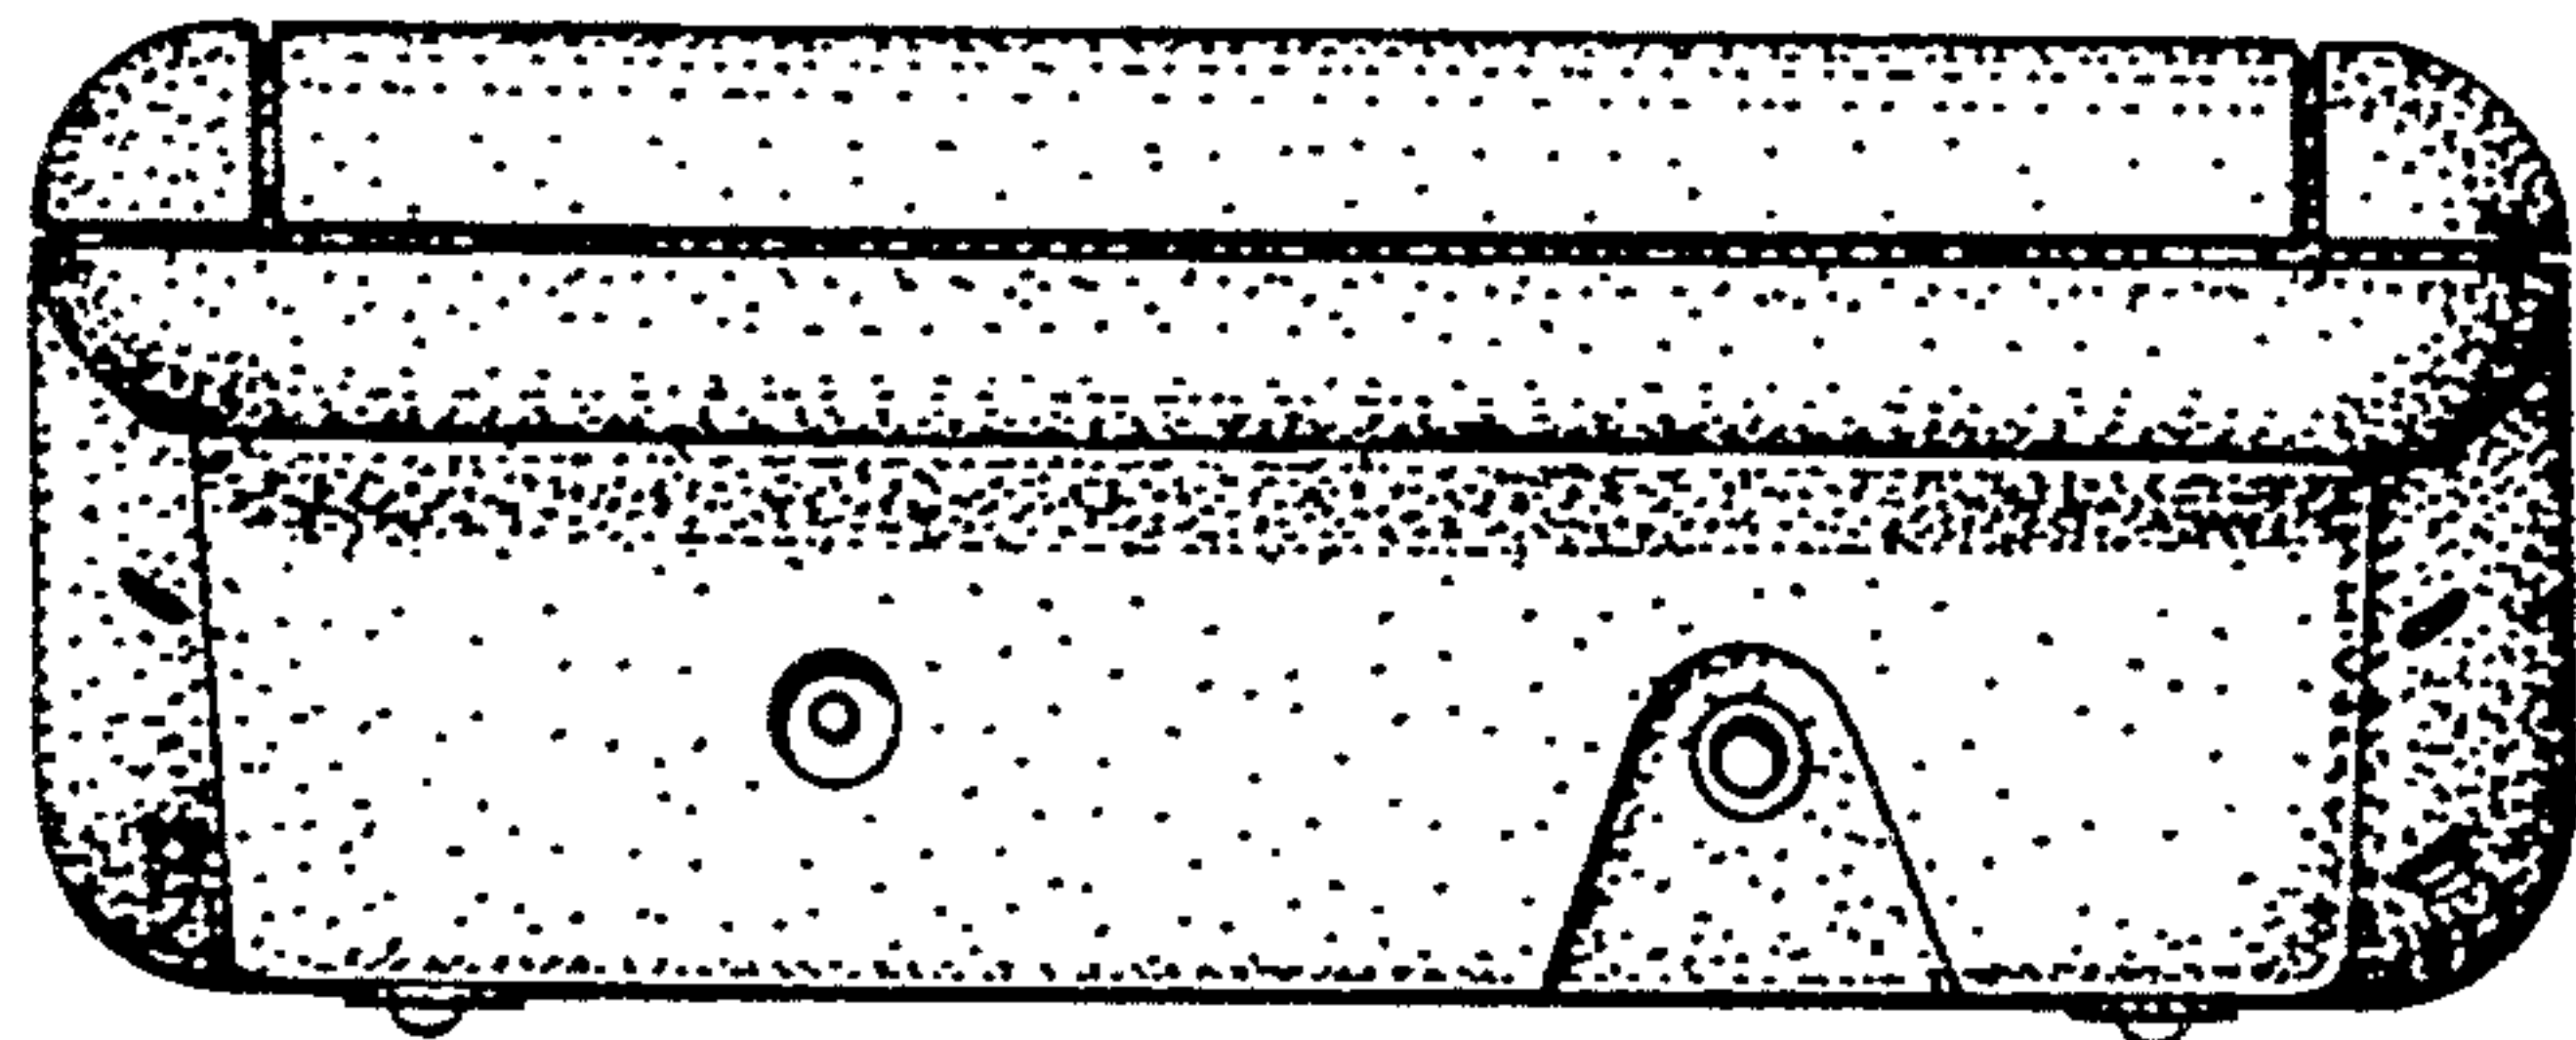


FIG. 4

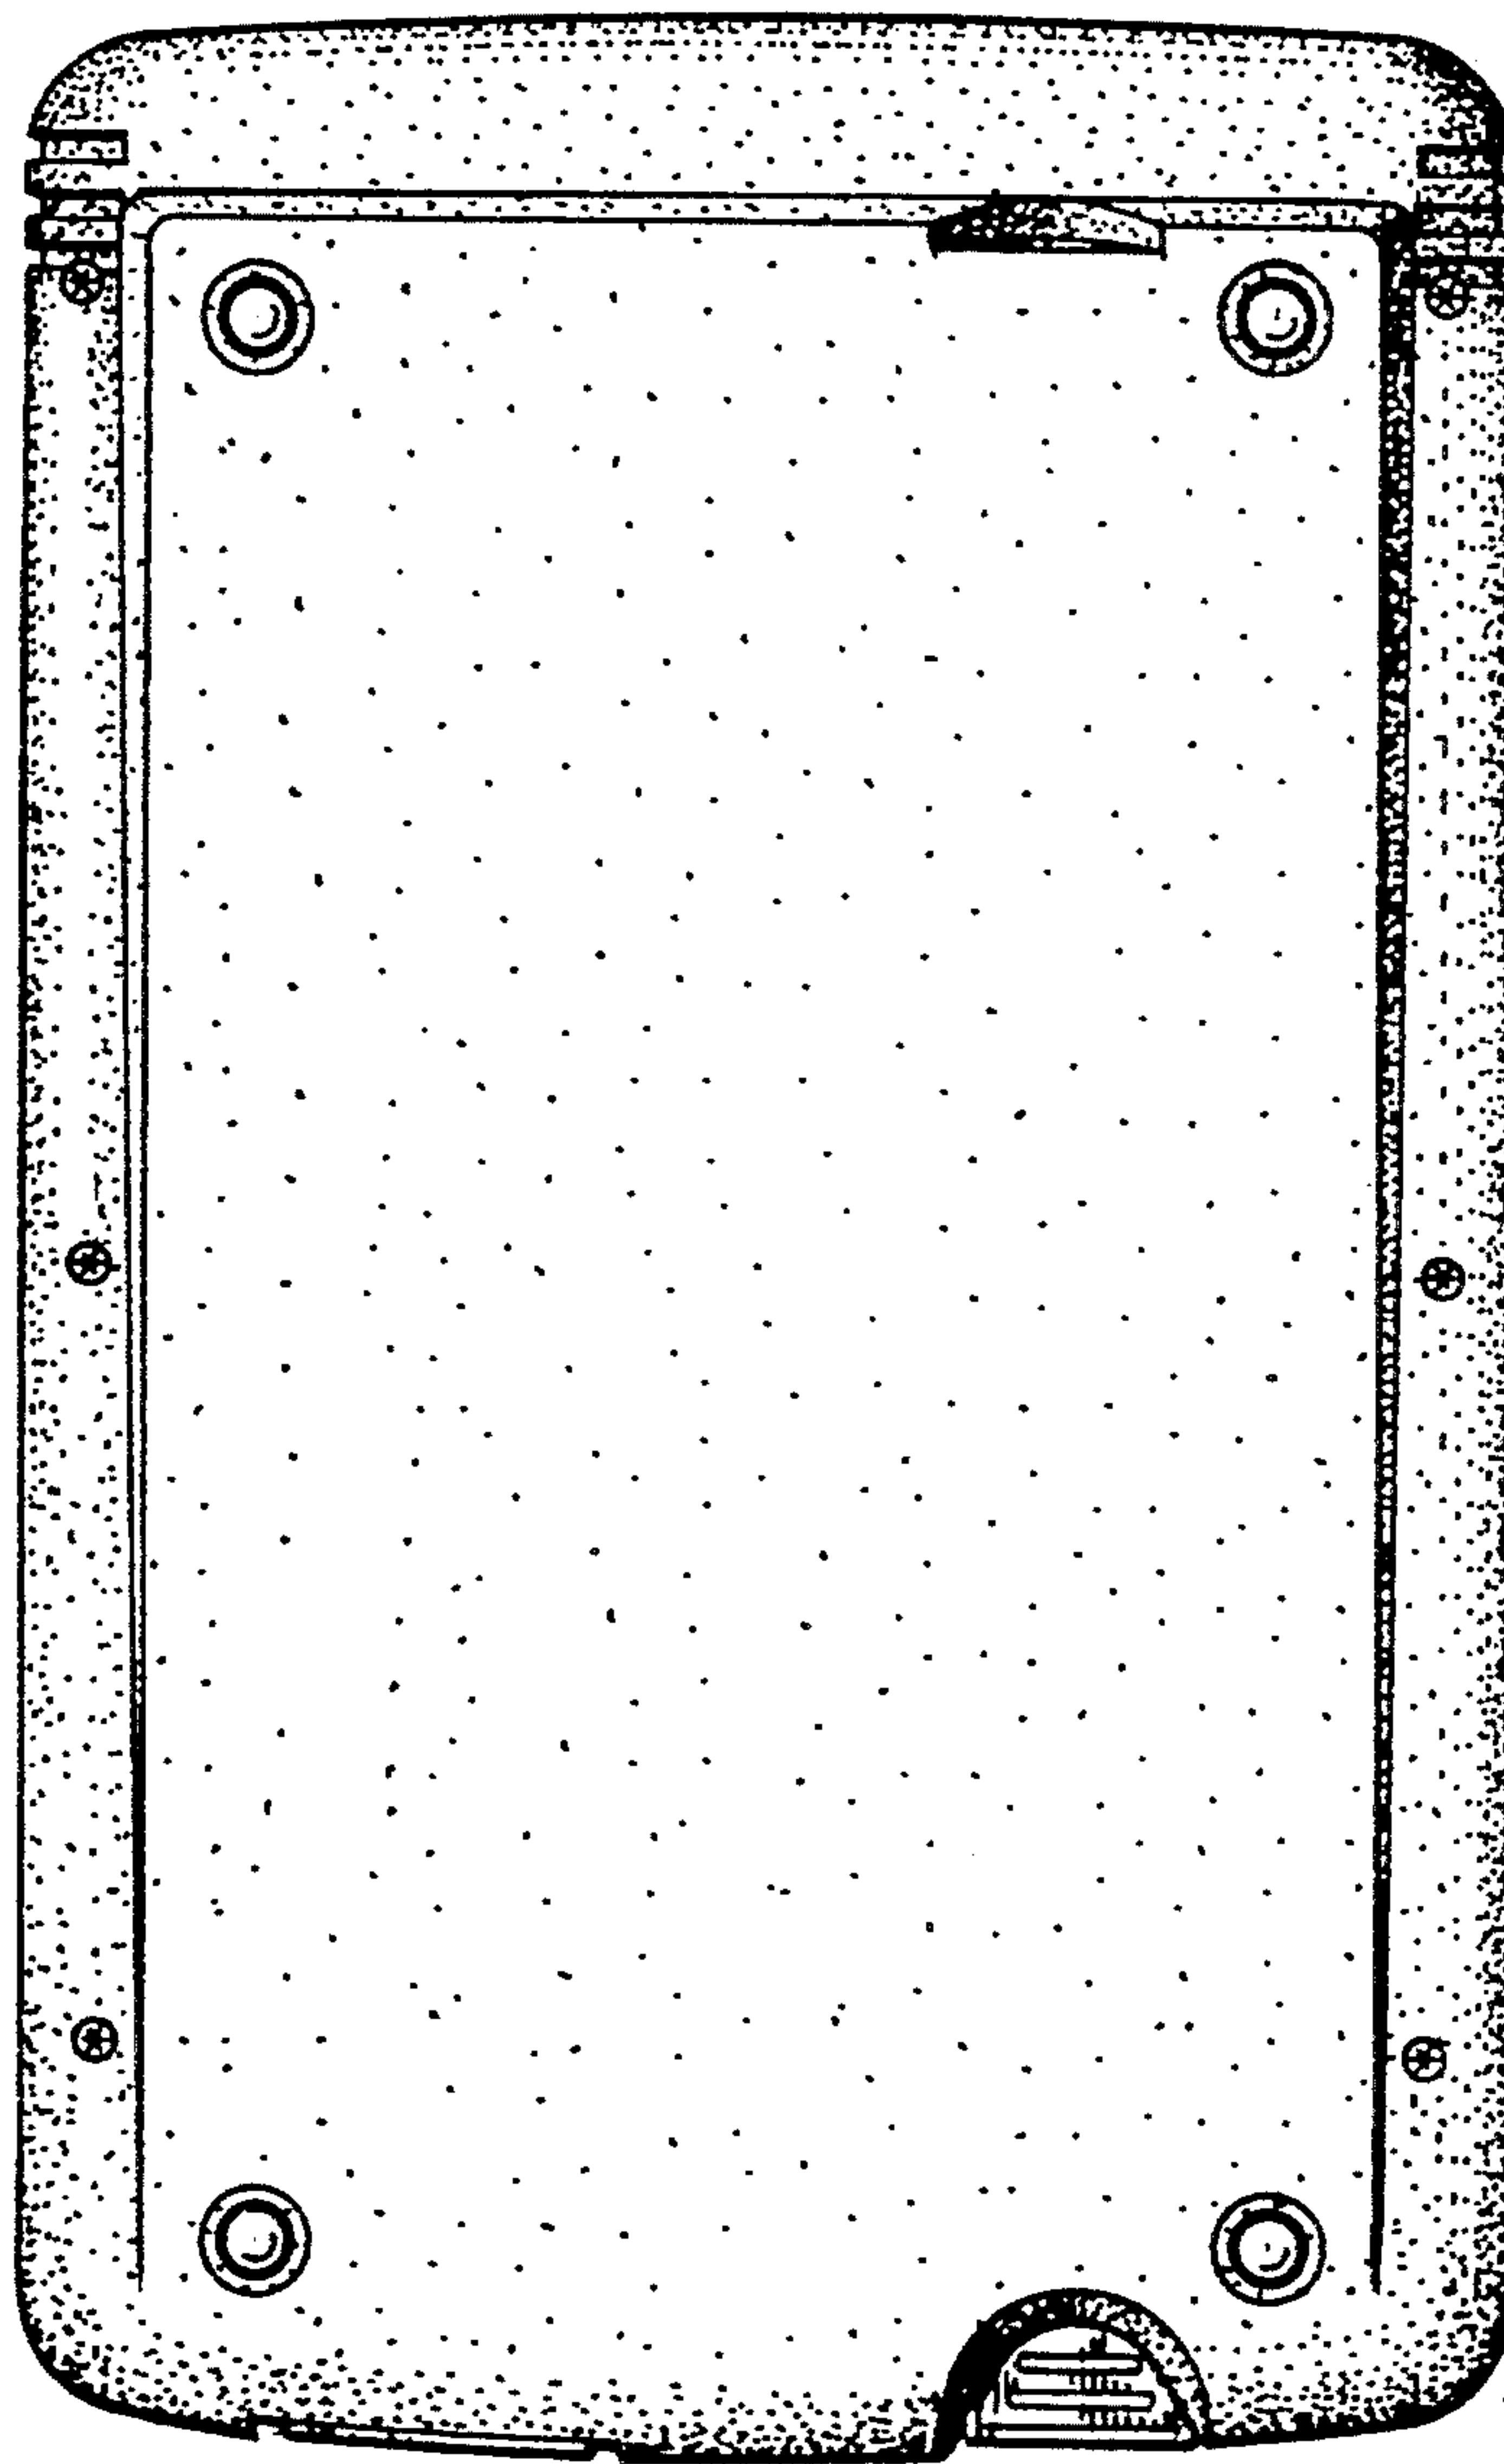


FIG 5

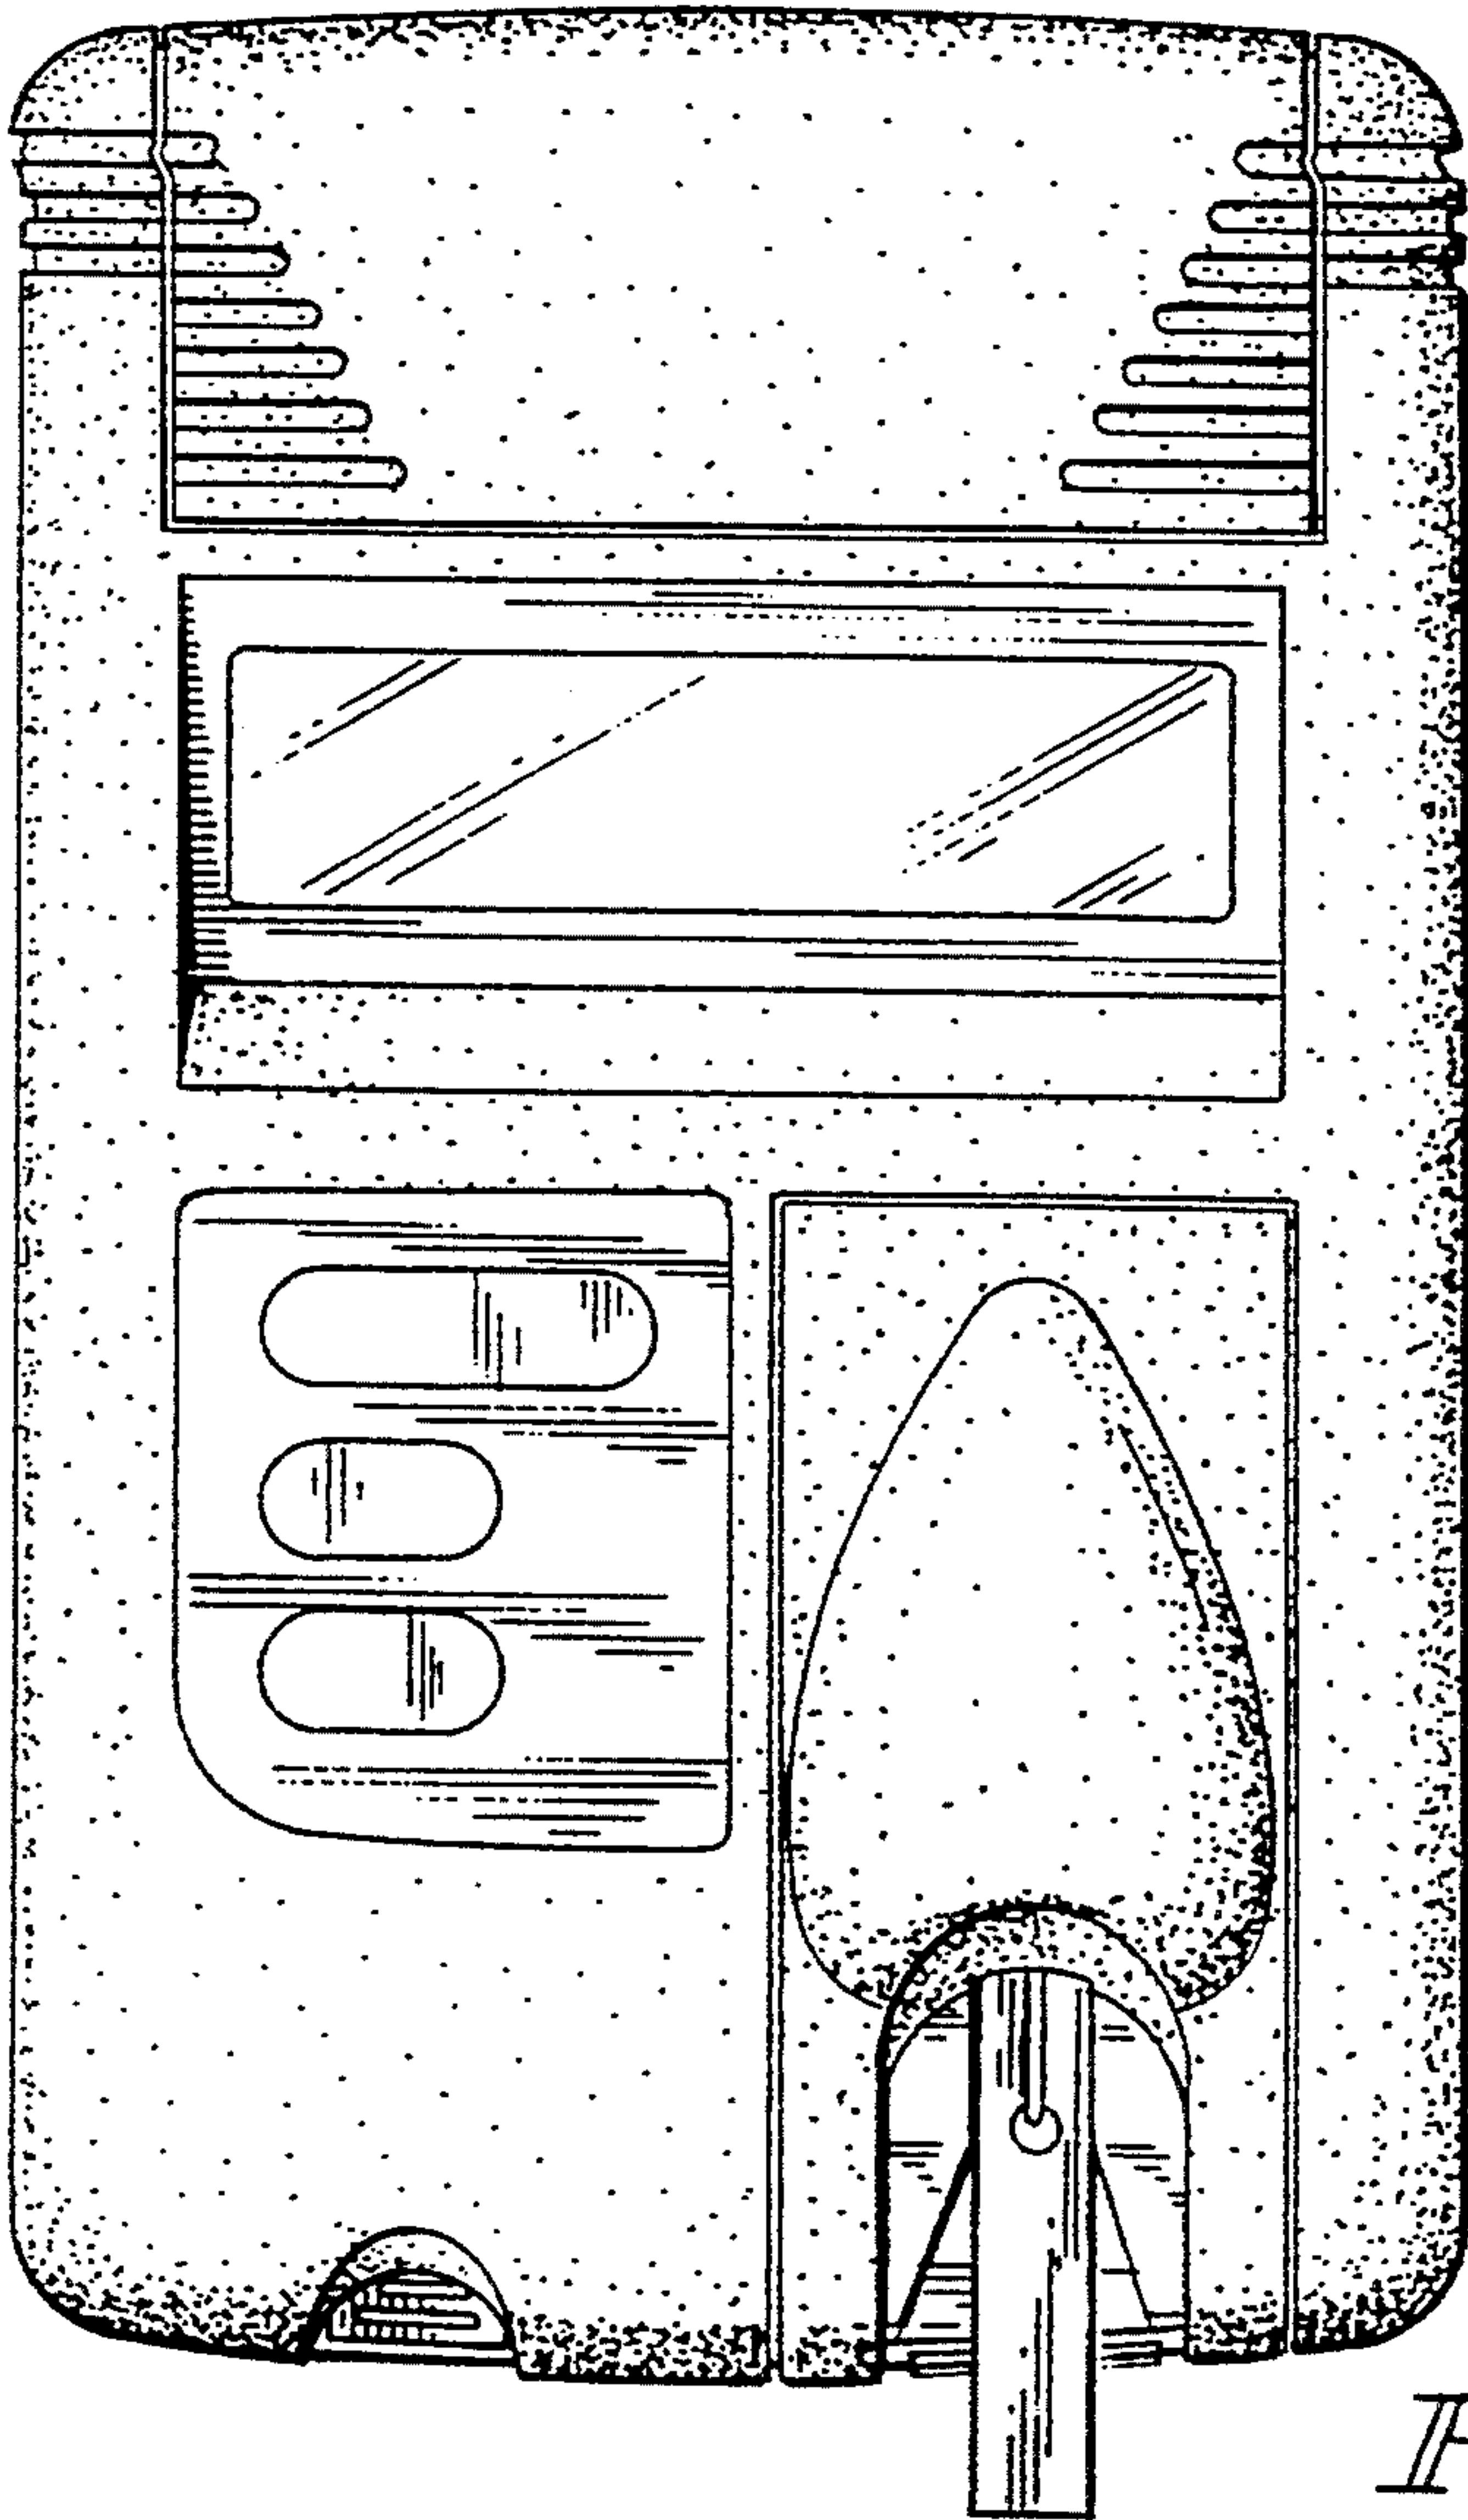


FIG. 7

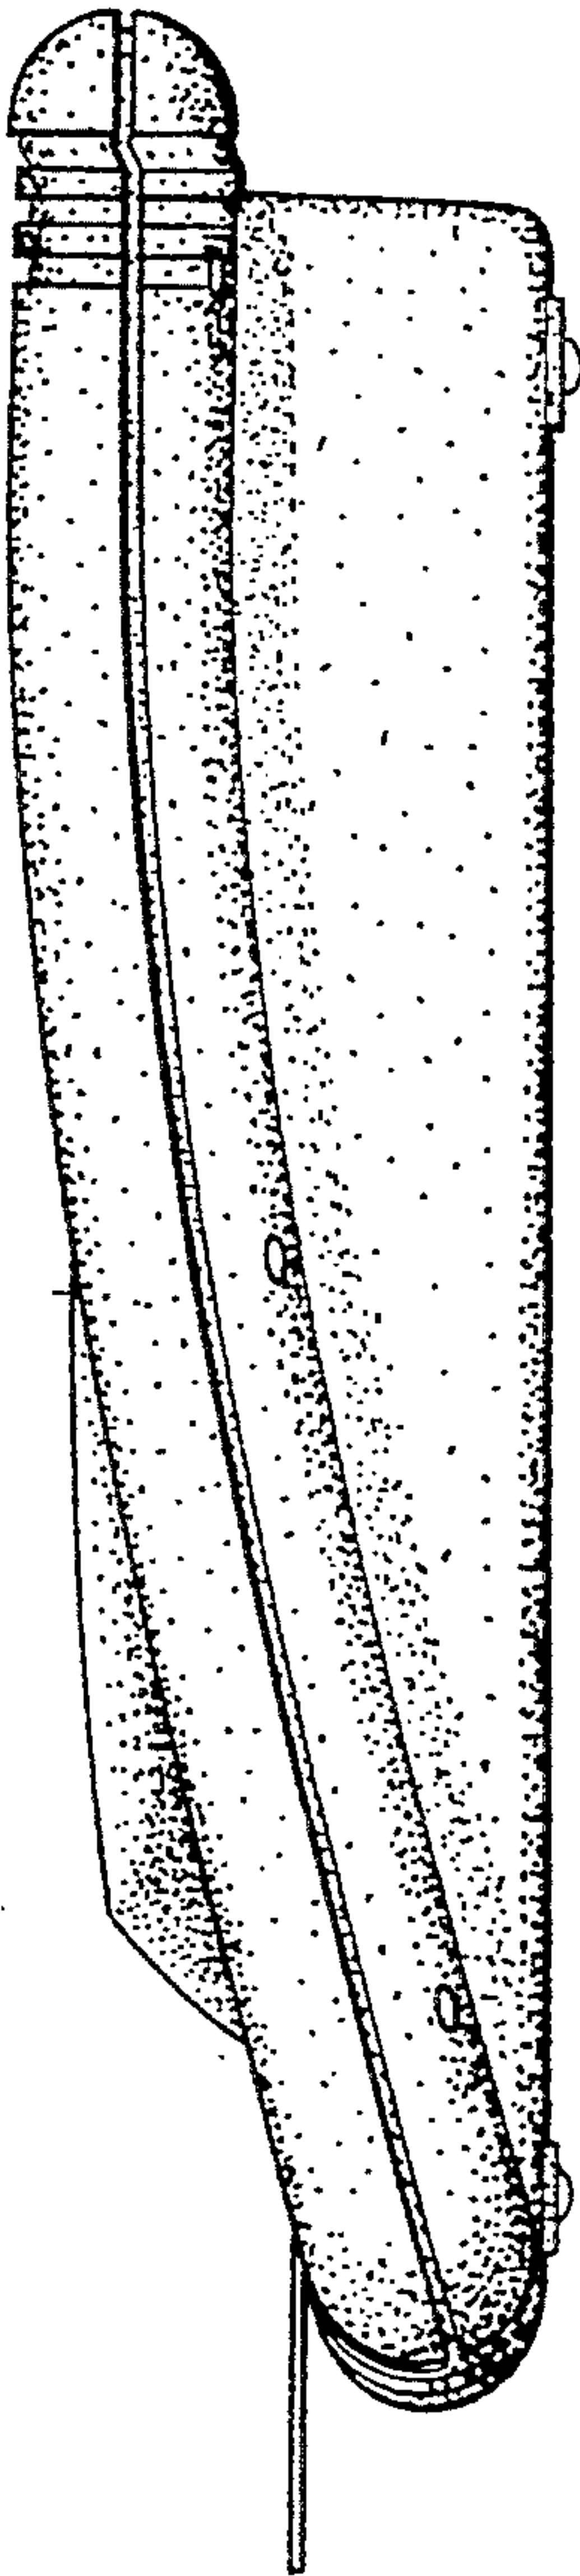


FIG. 8

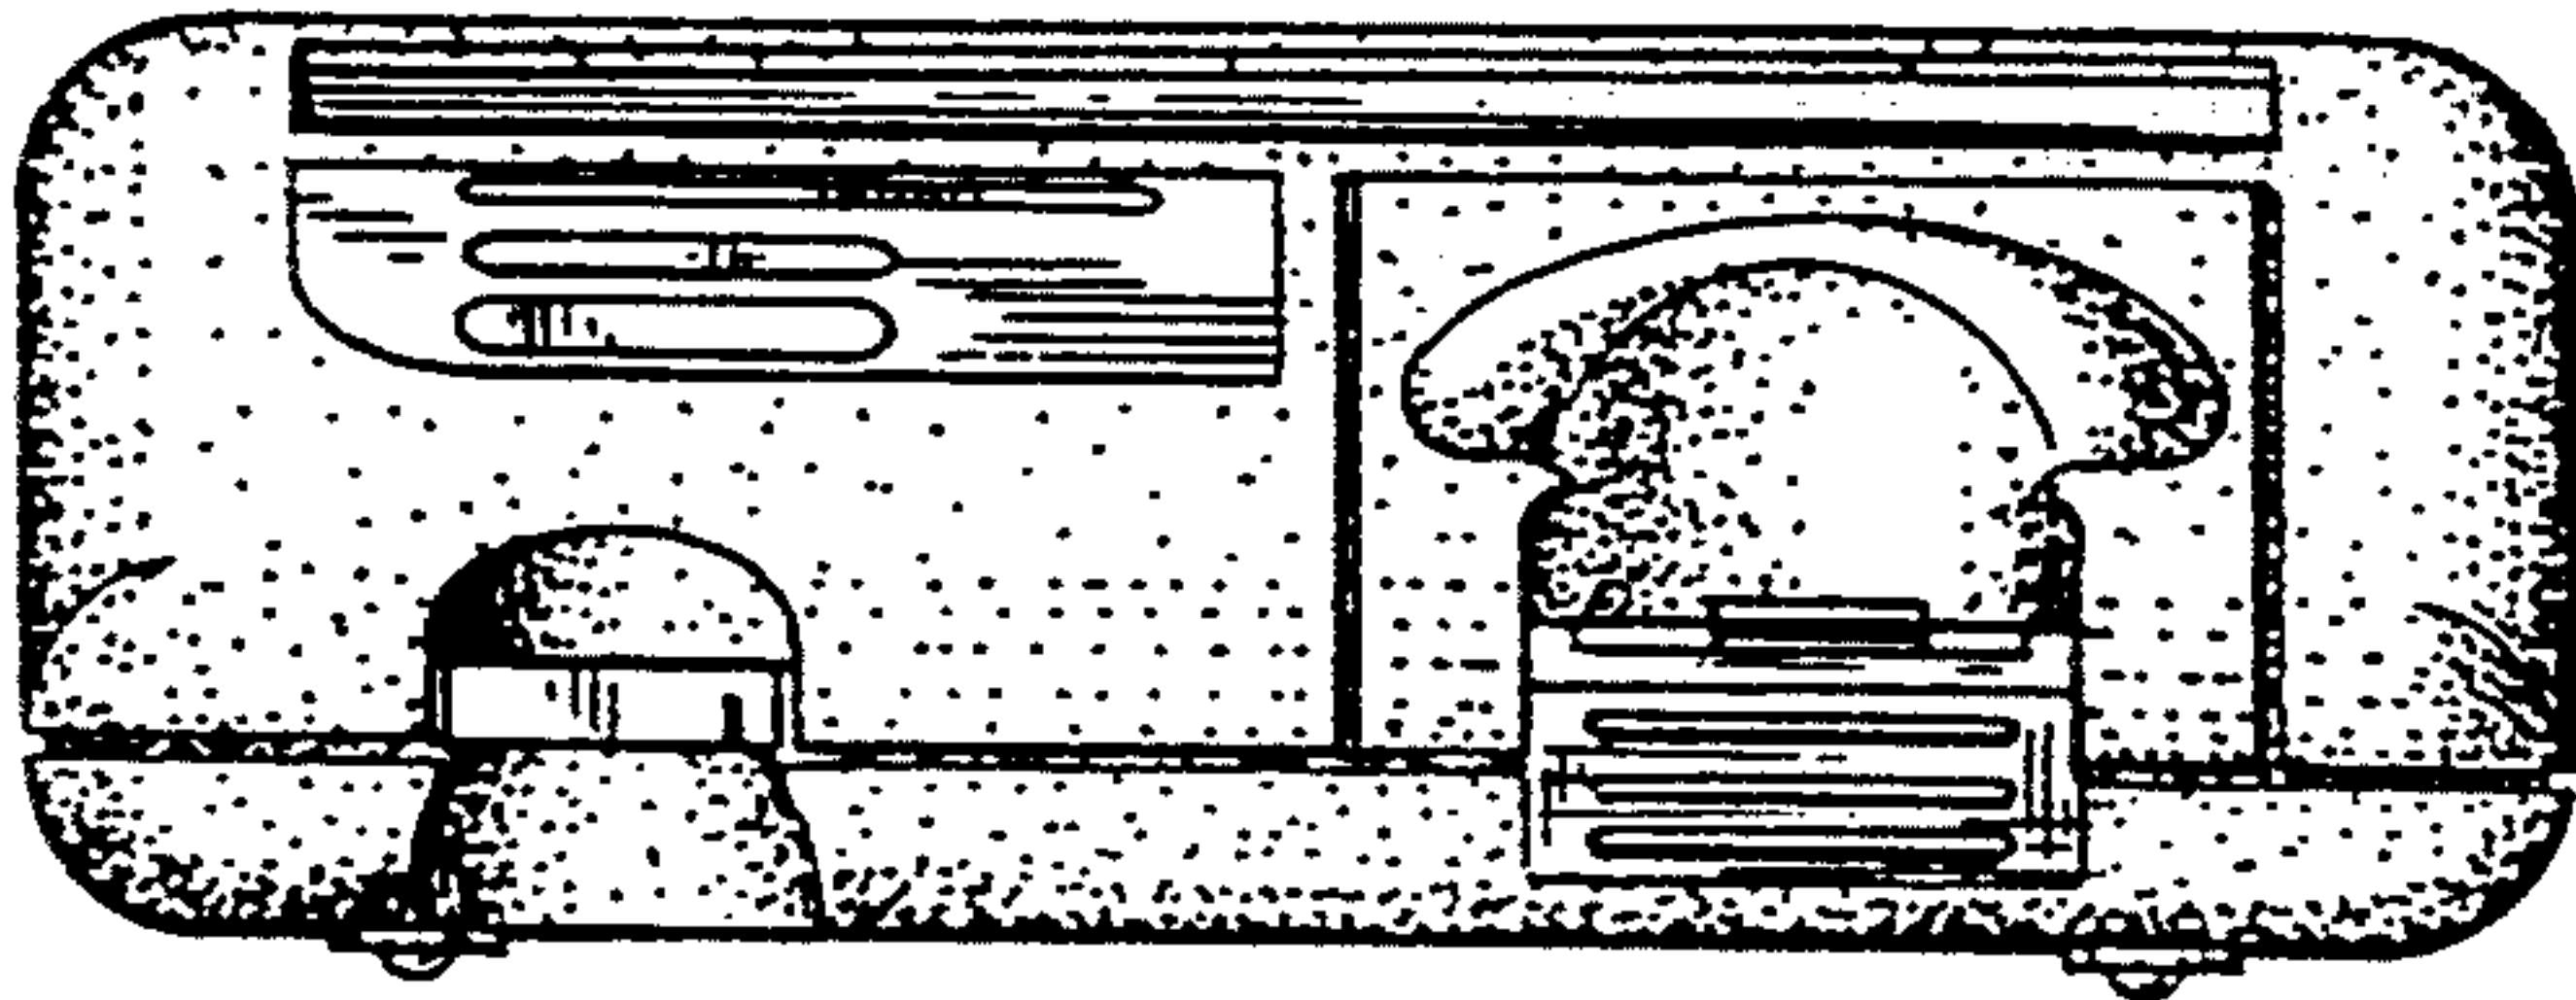


FIG. 6

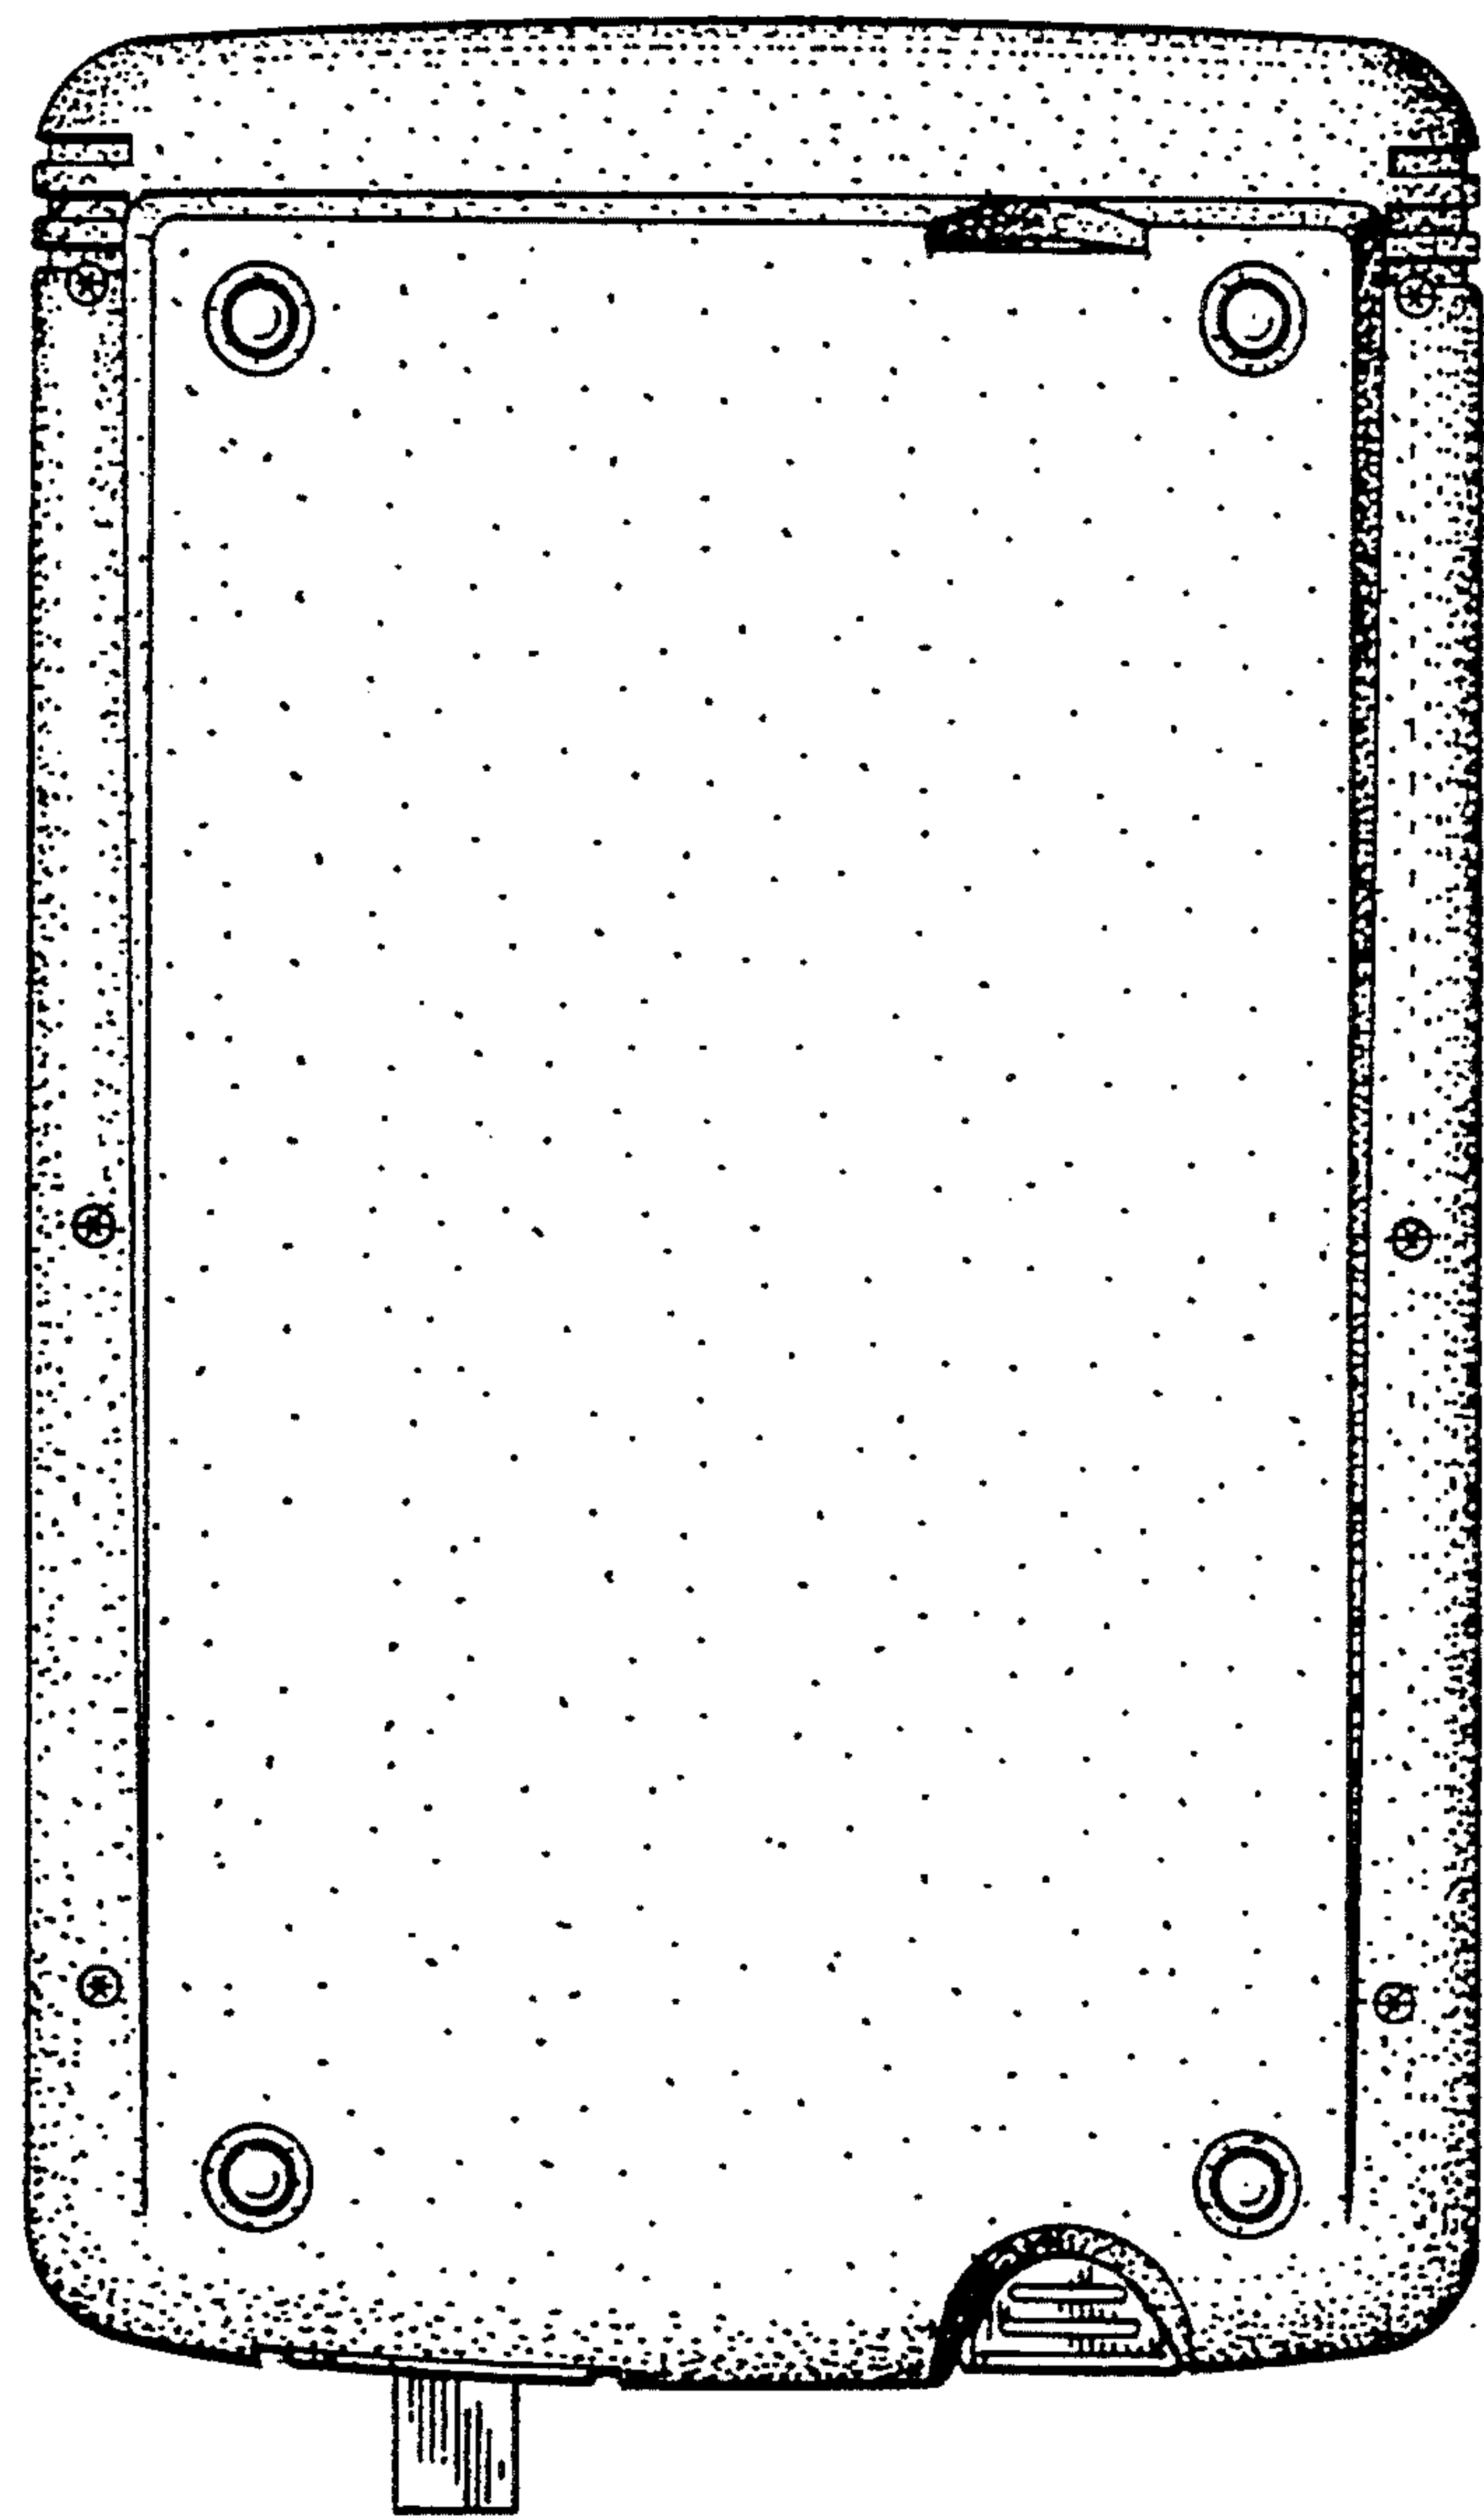


FIG. 9

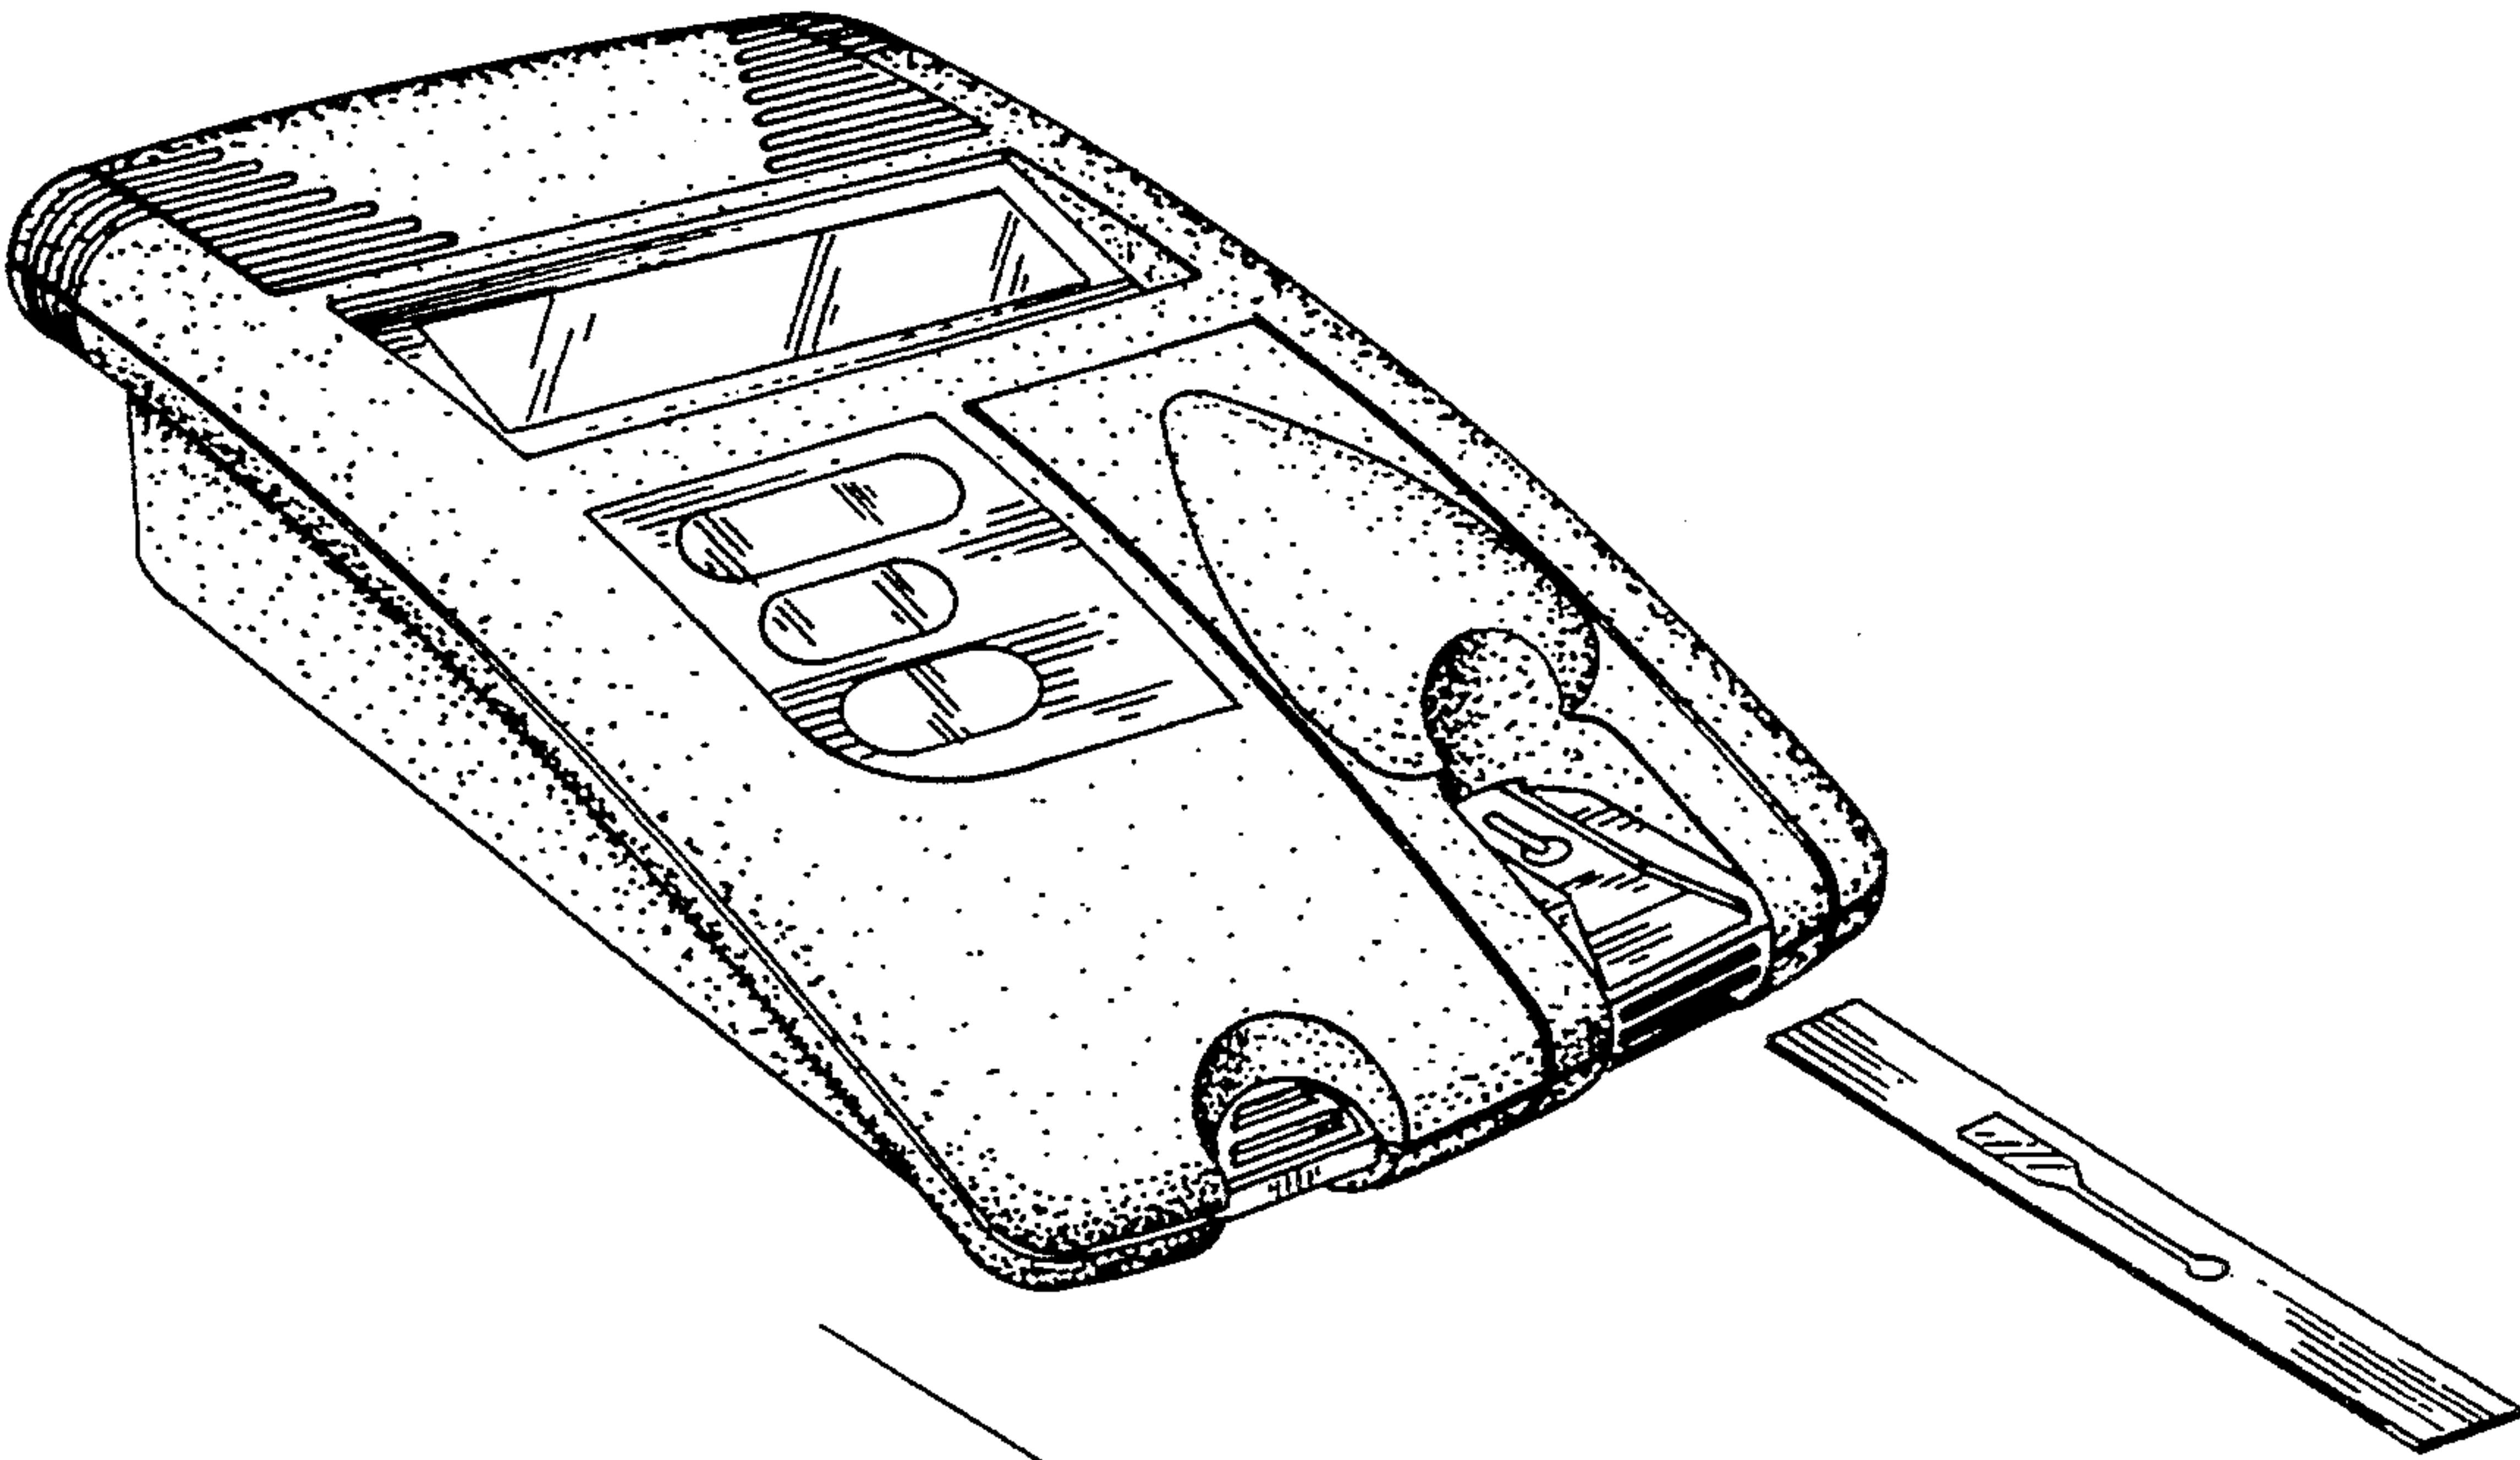


FIG. 10