



US00D361619S

# United States Patent [19]

[11] Patent Number: **Des. 361,619**

Phleps et al.

[45] Date of Patent: **\*\* Aug. 22, 1995**

[54] **INTRAORAL SENSOR FOR A DENTAL X-RAY APPARATUS**

4,150,296 4/1979 Edeland et al. .... 378/170

[75] Inventors: **Tilman Phleps; Michael Doebert,**  
both of Lorsch, Germany

[73] Assignee: **Siemens Aktiengesellschaft, Munich,**  
Germany

[\*\*] Term: **14 Years**

[21] Appl. No.: **19,969**

[22] Filed: **Mar. 15, 1994**

[30] **Foreign Application Priority Data**

Nov. 17, 1993 [WO] WIPO ..... DM/002358

[52] U.S. Cl. .... **D24/158**

[58] Field of Search ..... D24/158, 176, 186;  
433/29, 229; 378/170, 168, 184

[56] **References Cited**

**U.S. PATENT DOCUMENTS**

D. 355,964 2/1995 Nelvig ..... D24/158  
1,657,230 1/1928 Simonton ..... 378/170  
1,667,442 4/1928 Sikes ..... 378/170

**OTHER PUBLICATIONS**

Sales Brochure "VISUALIX", Philips Medical Systems, date unknown.

Sales Brochure "SENS-A-RAY"™, Regam Medical Systems AB, Sundsvoll, Sweden, date unknown.

Sales Brochure "RVG-S", Trophy GmbH, Keh-l-am-Rhein, Germany, date unknown.

*Primary Examiner*—Stella Reid


*Attorney, Agent, or Firm*—Hill, Steadman & Simpson

[57] **CLAIM**

The ornamental design for an intraoral sensor for a dental x-ray apparatus, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of an intraoral sensor for a dental x-ray apparatus, showing our new design; FIG. 2 is a front elevational view thereof; FIG. 3 is a top plan view thereof; FIG. 4 is a side elevational view of FIG. 2, the left side elevational view being a mirror image; FIG. 5 is a back elevational view thereof; and, FIG. 6 is a bottom plan view thereof.

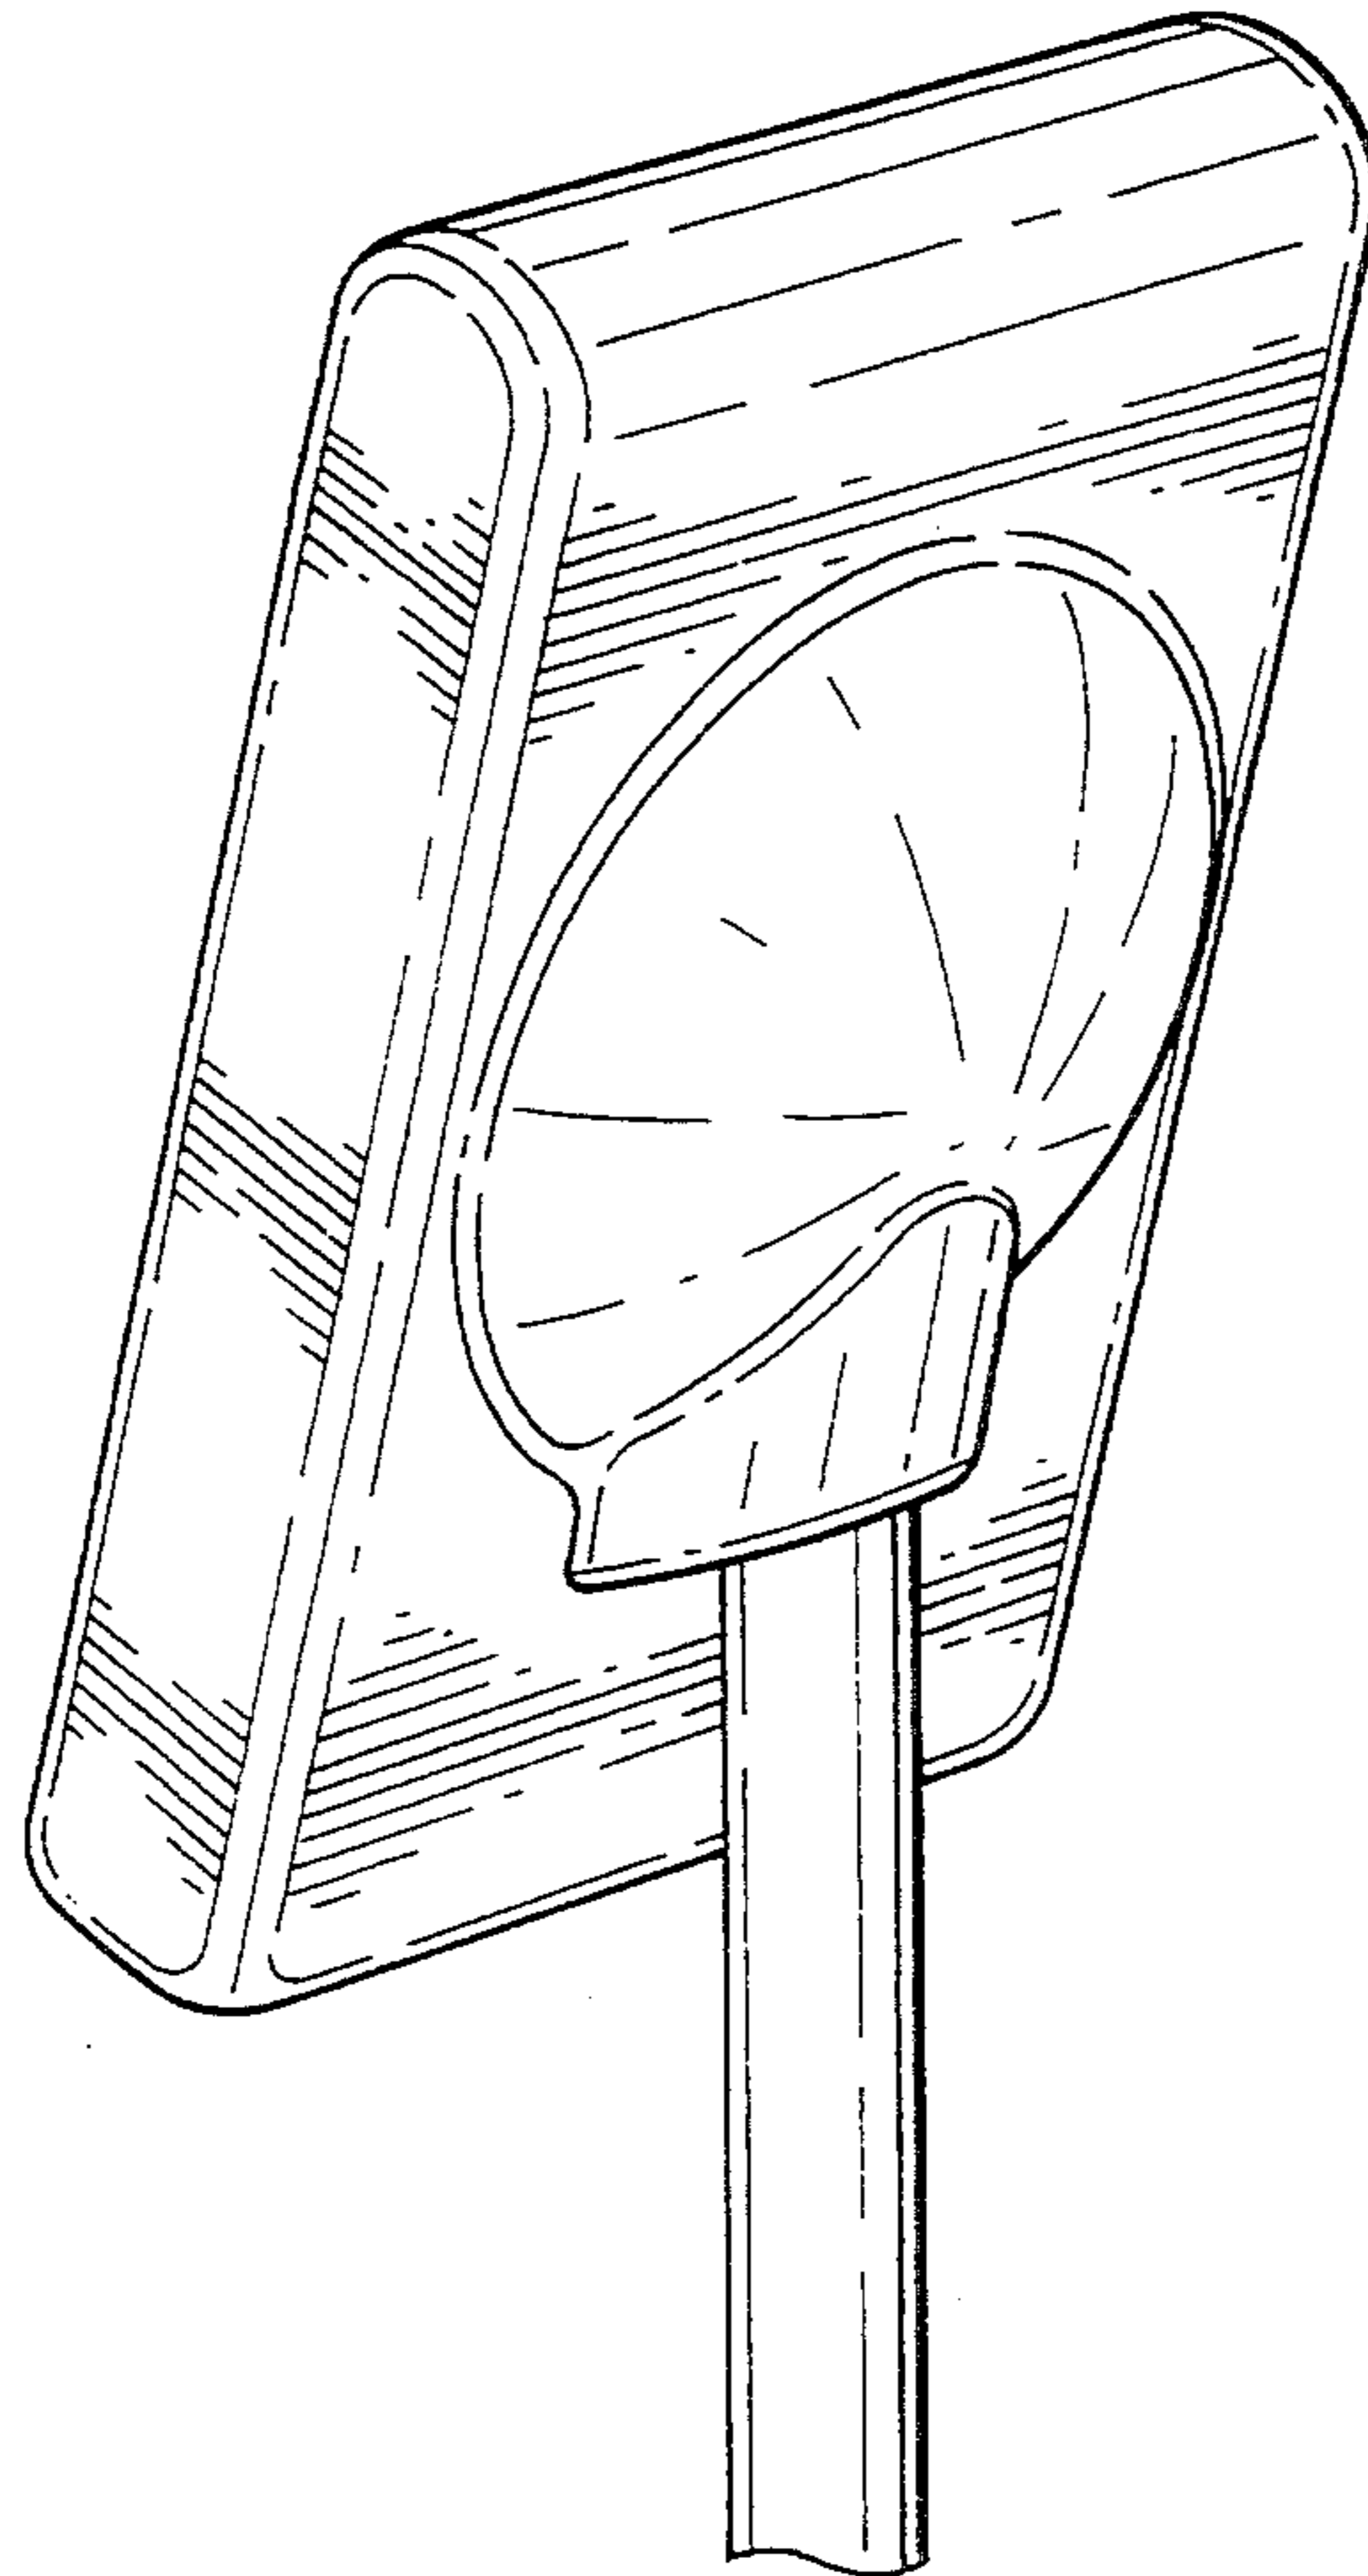

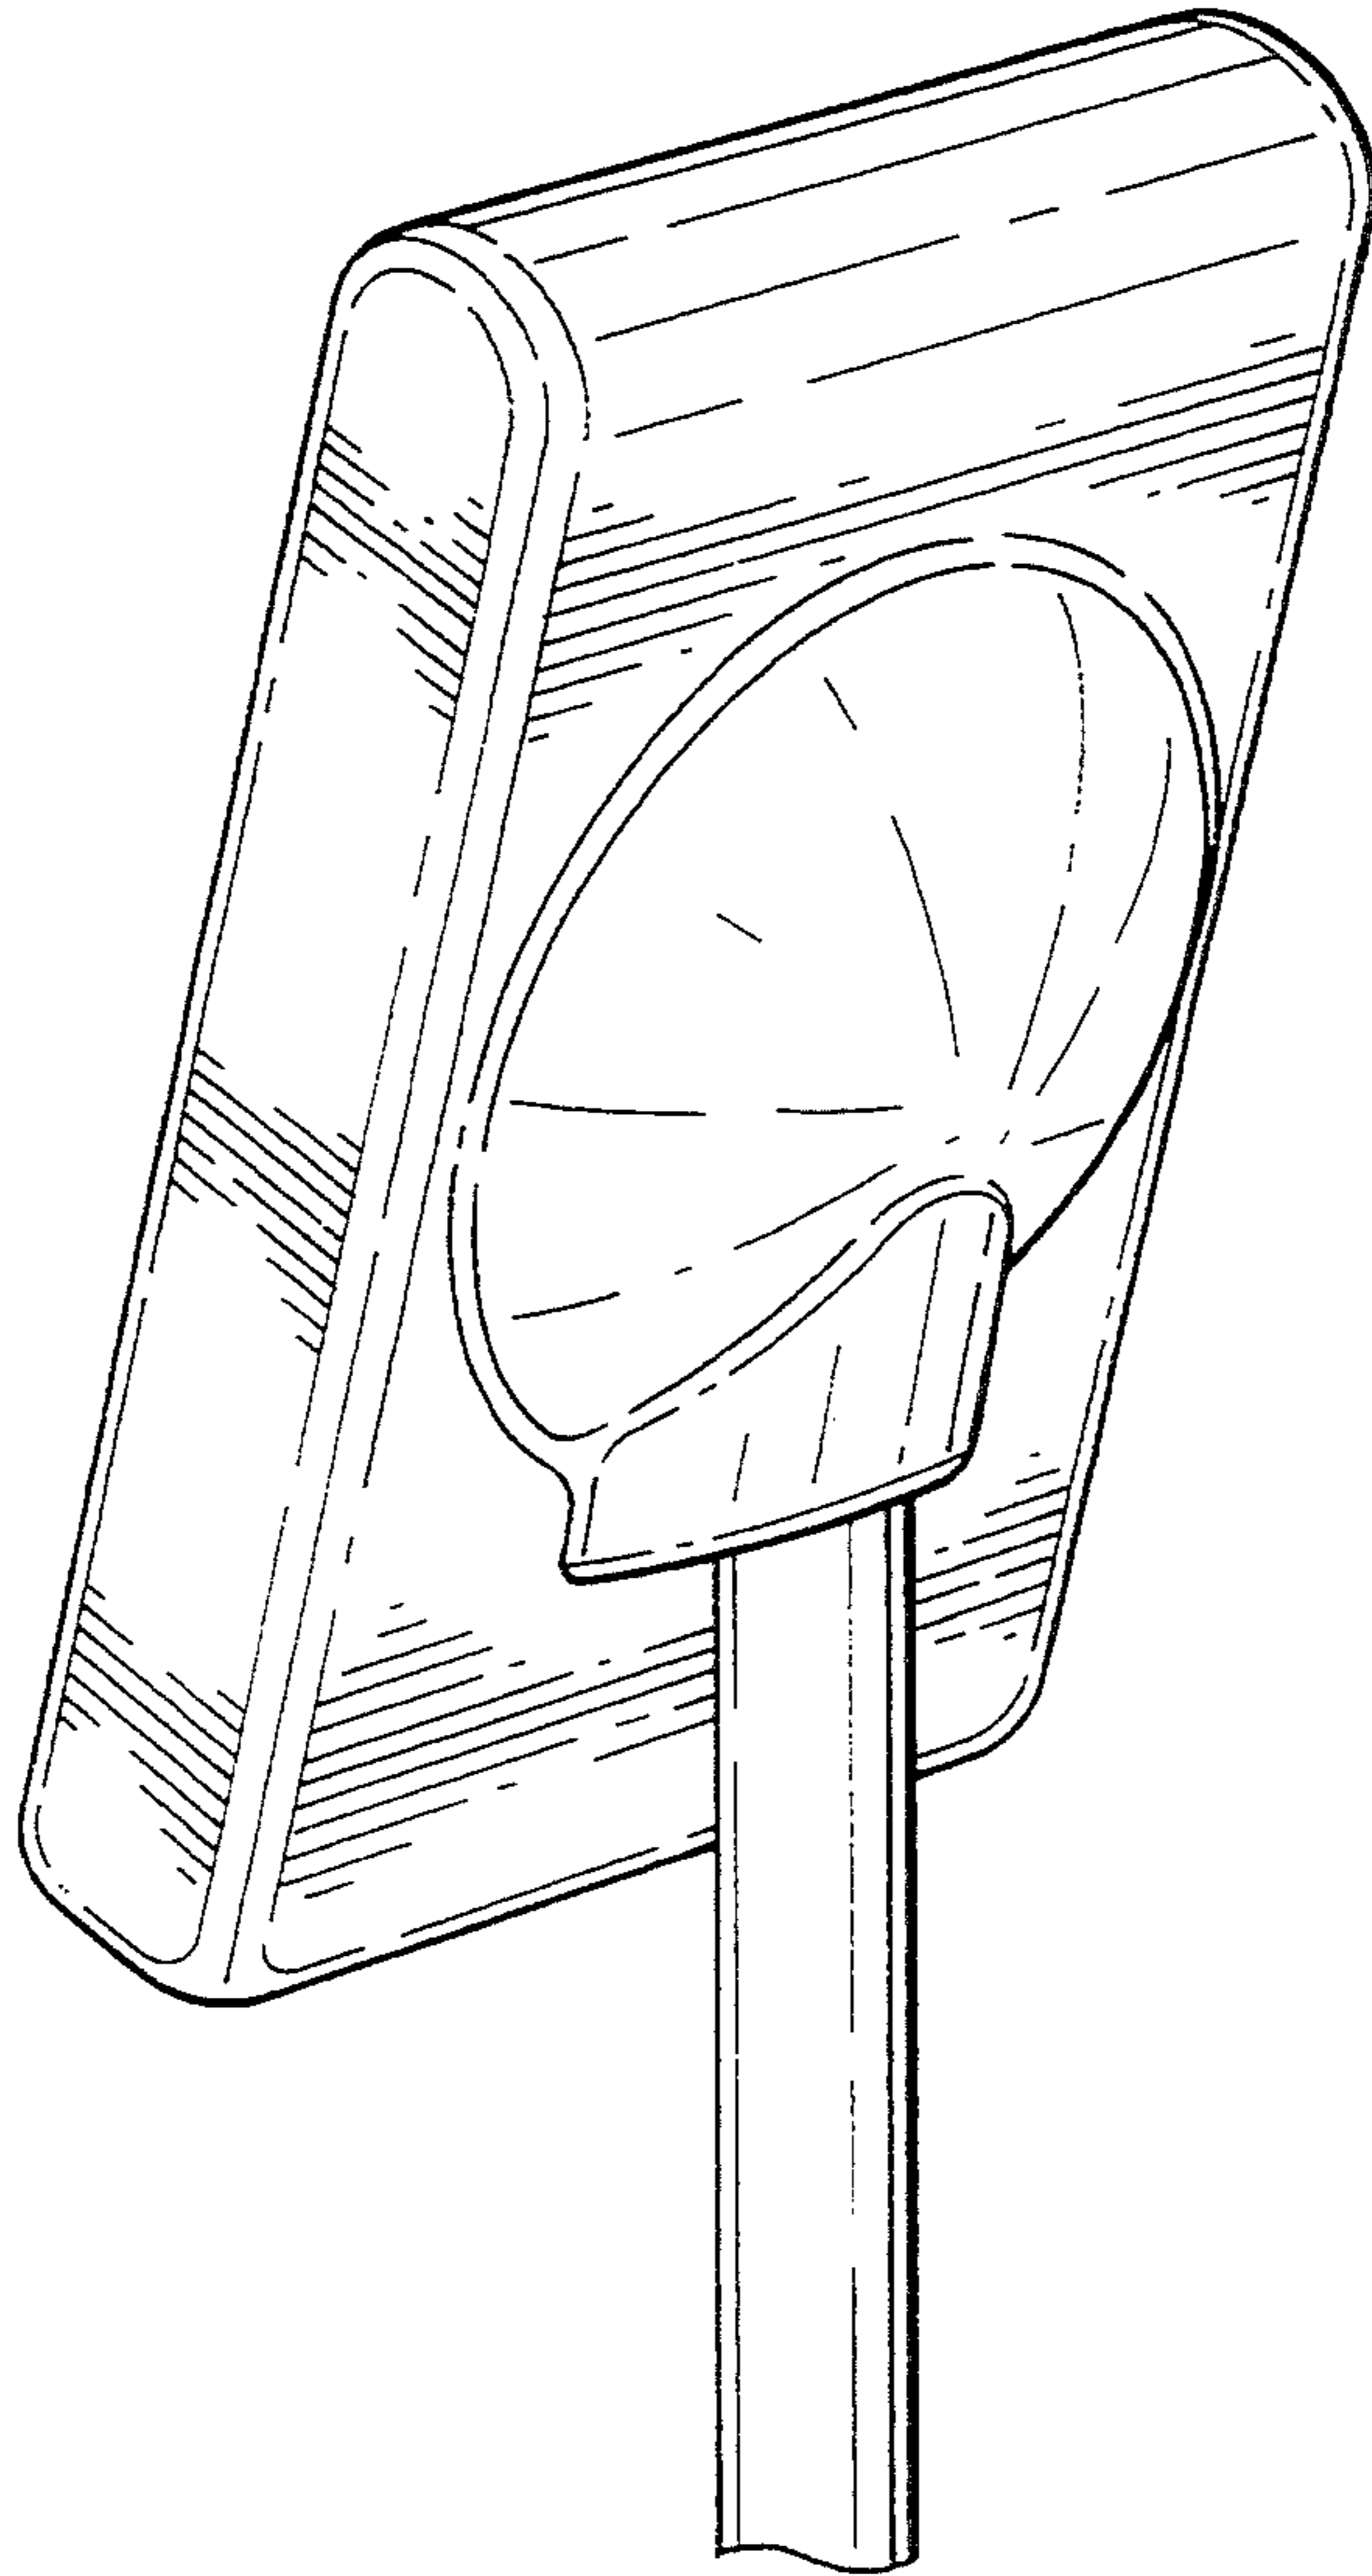


FIG 1

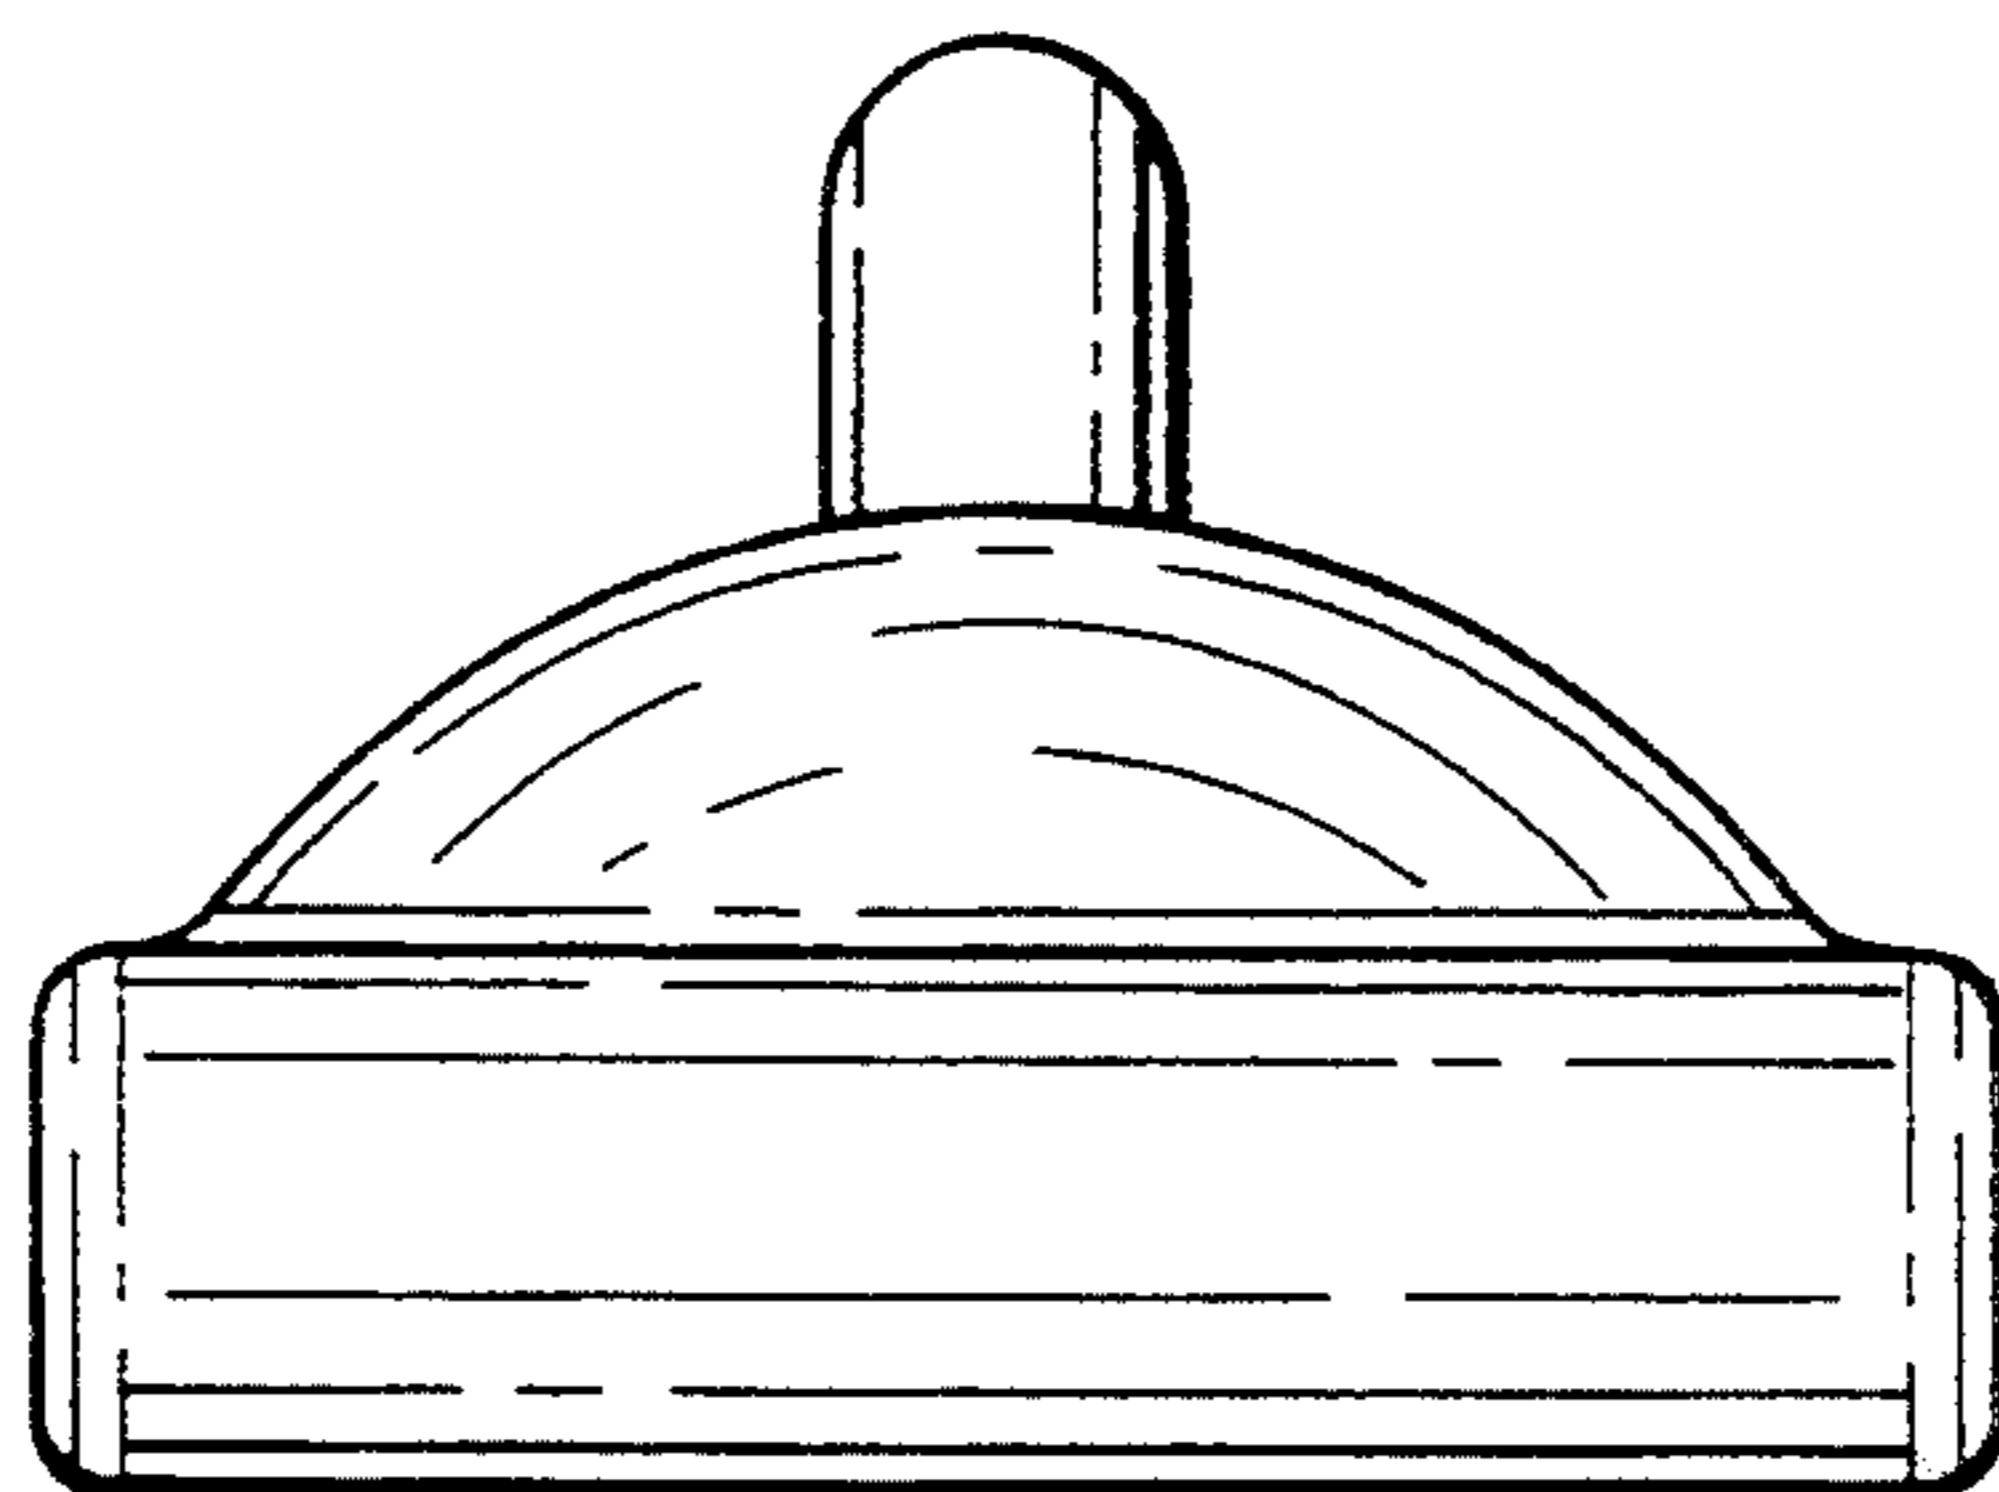


FIG 3

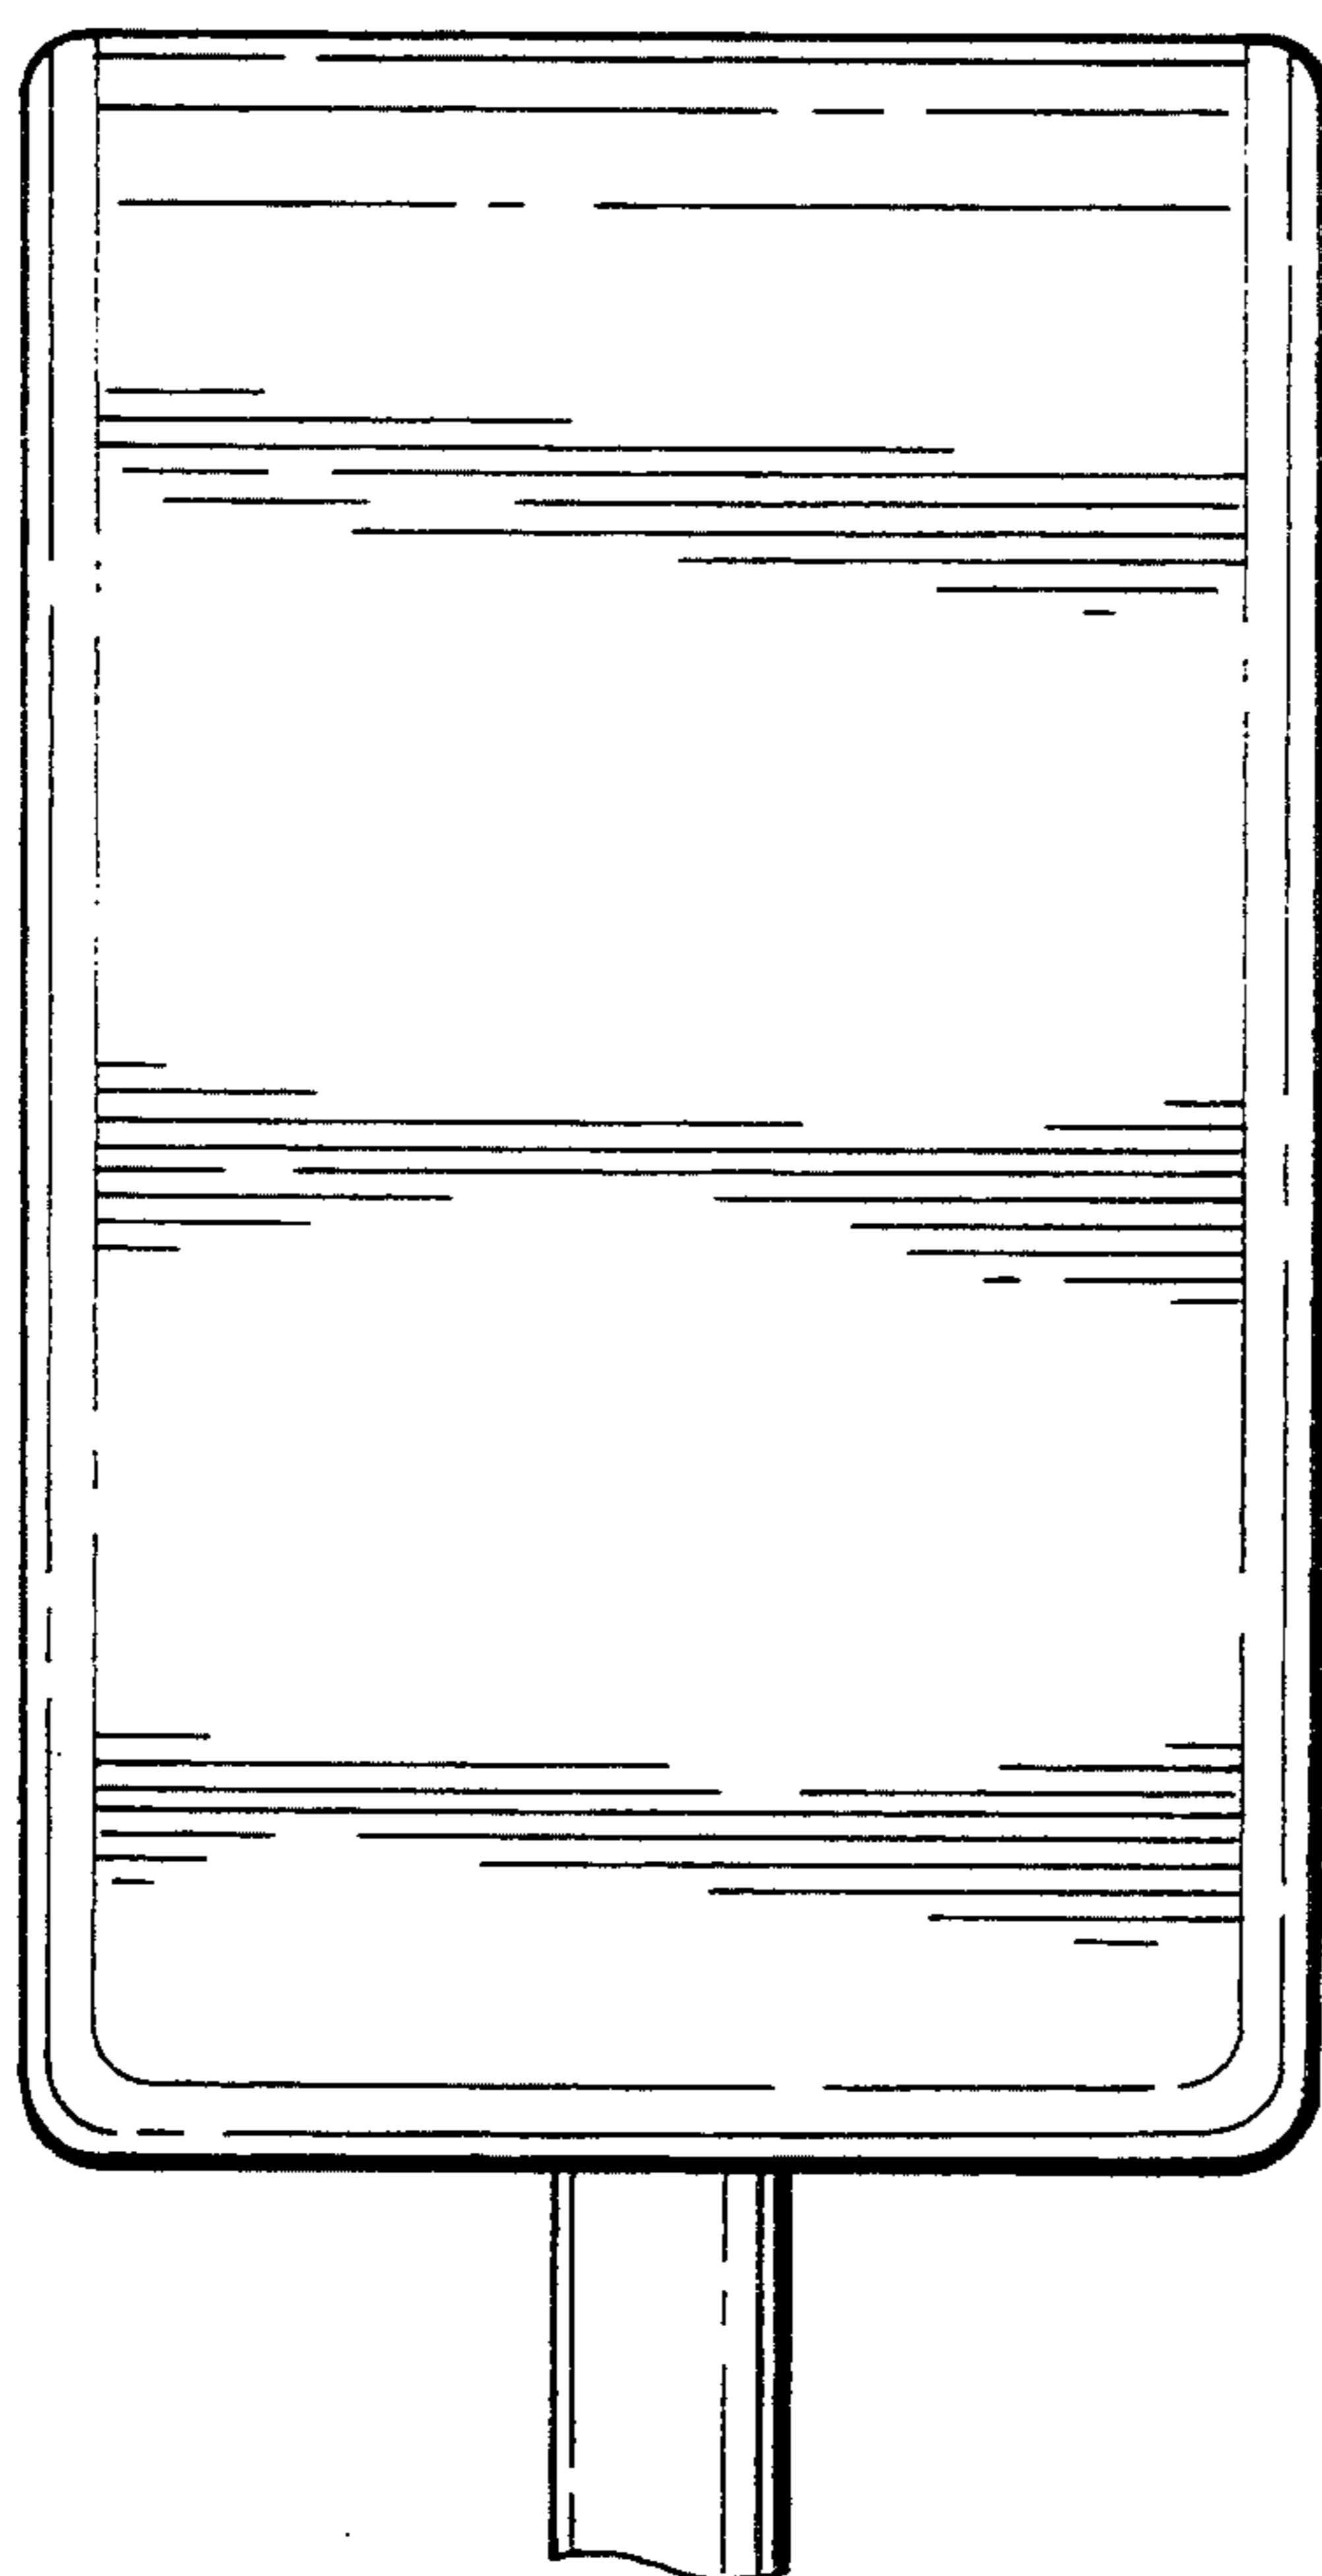


FIG 2

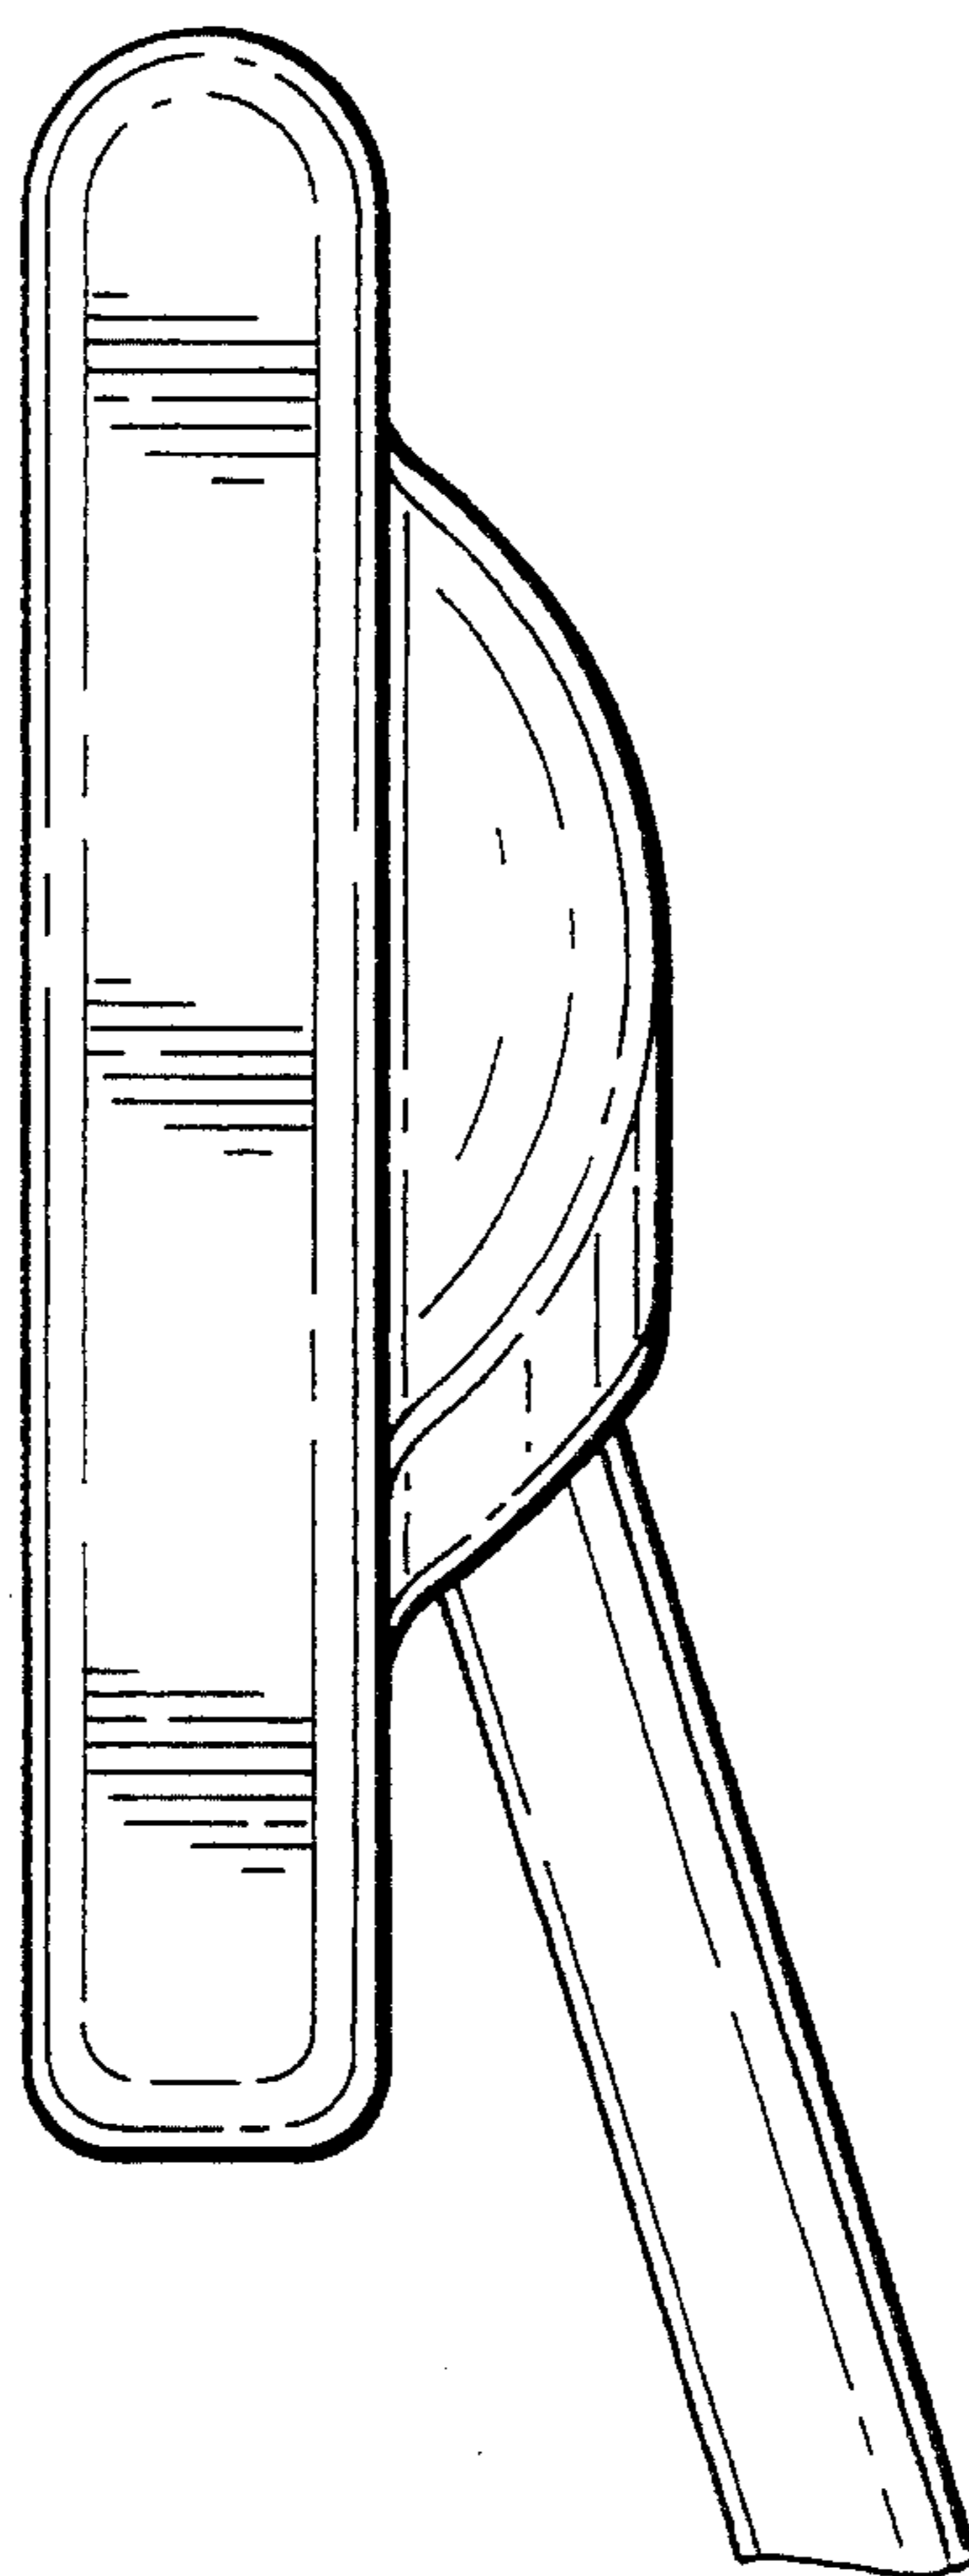


FIG 4

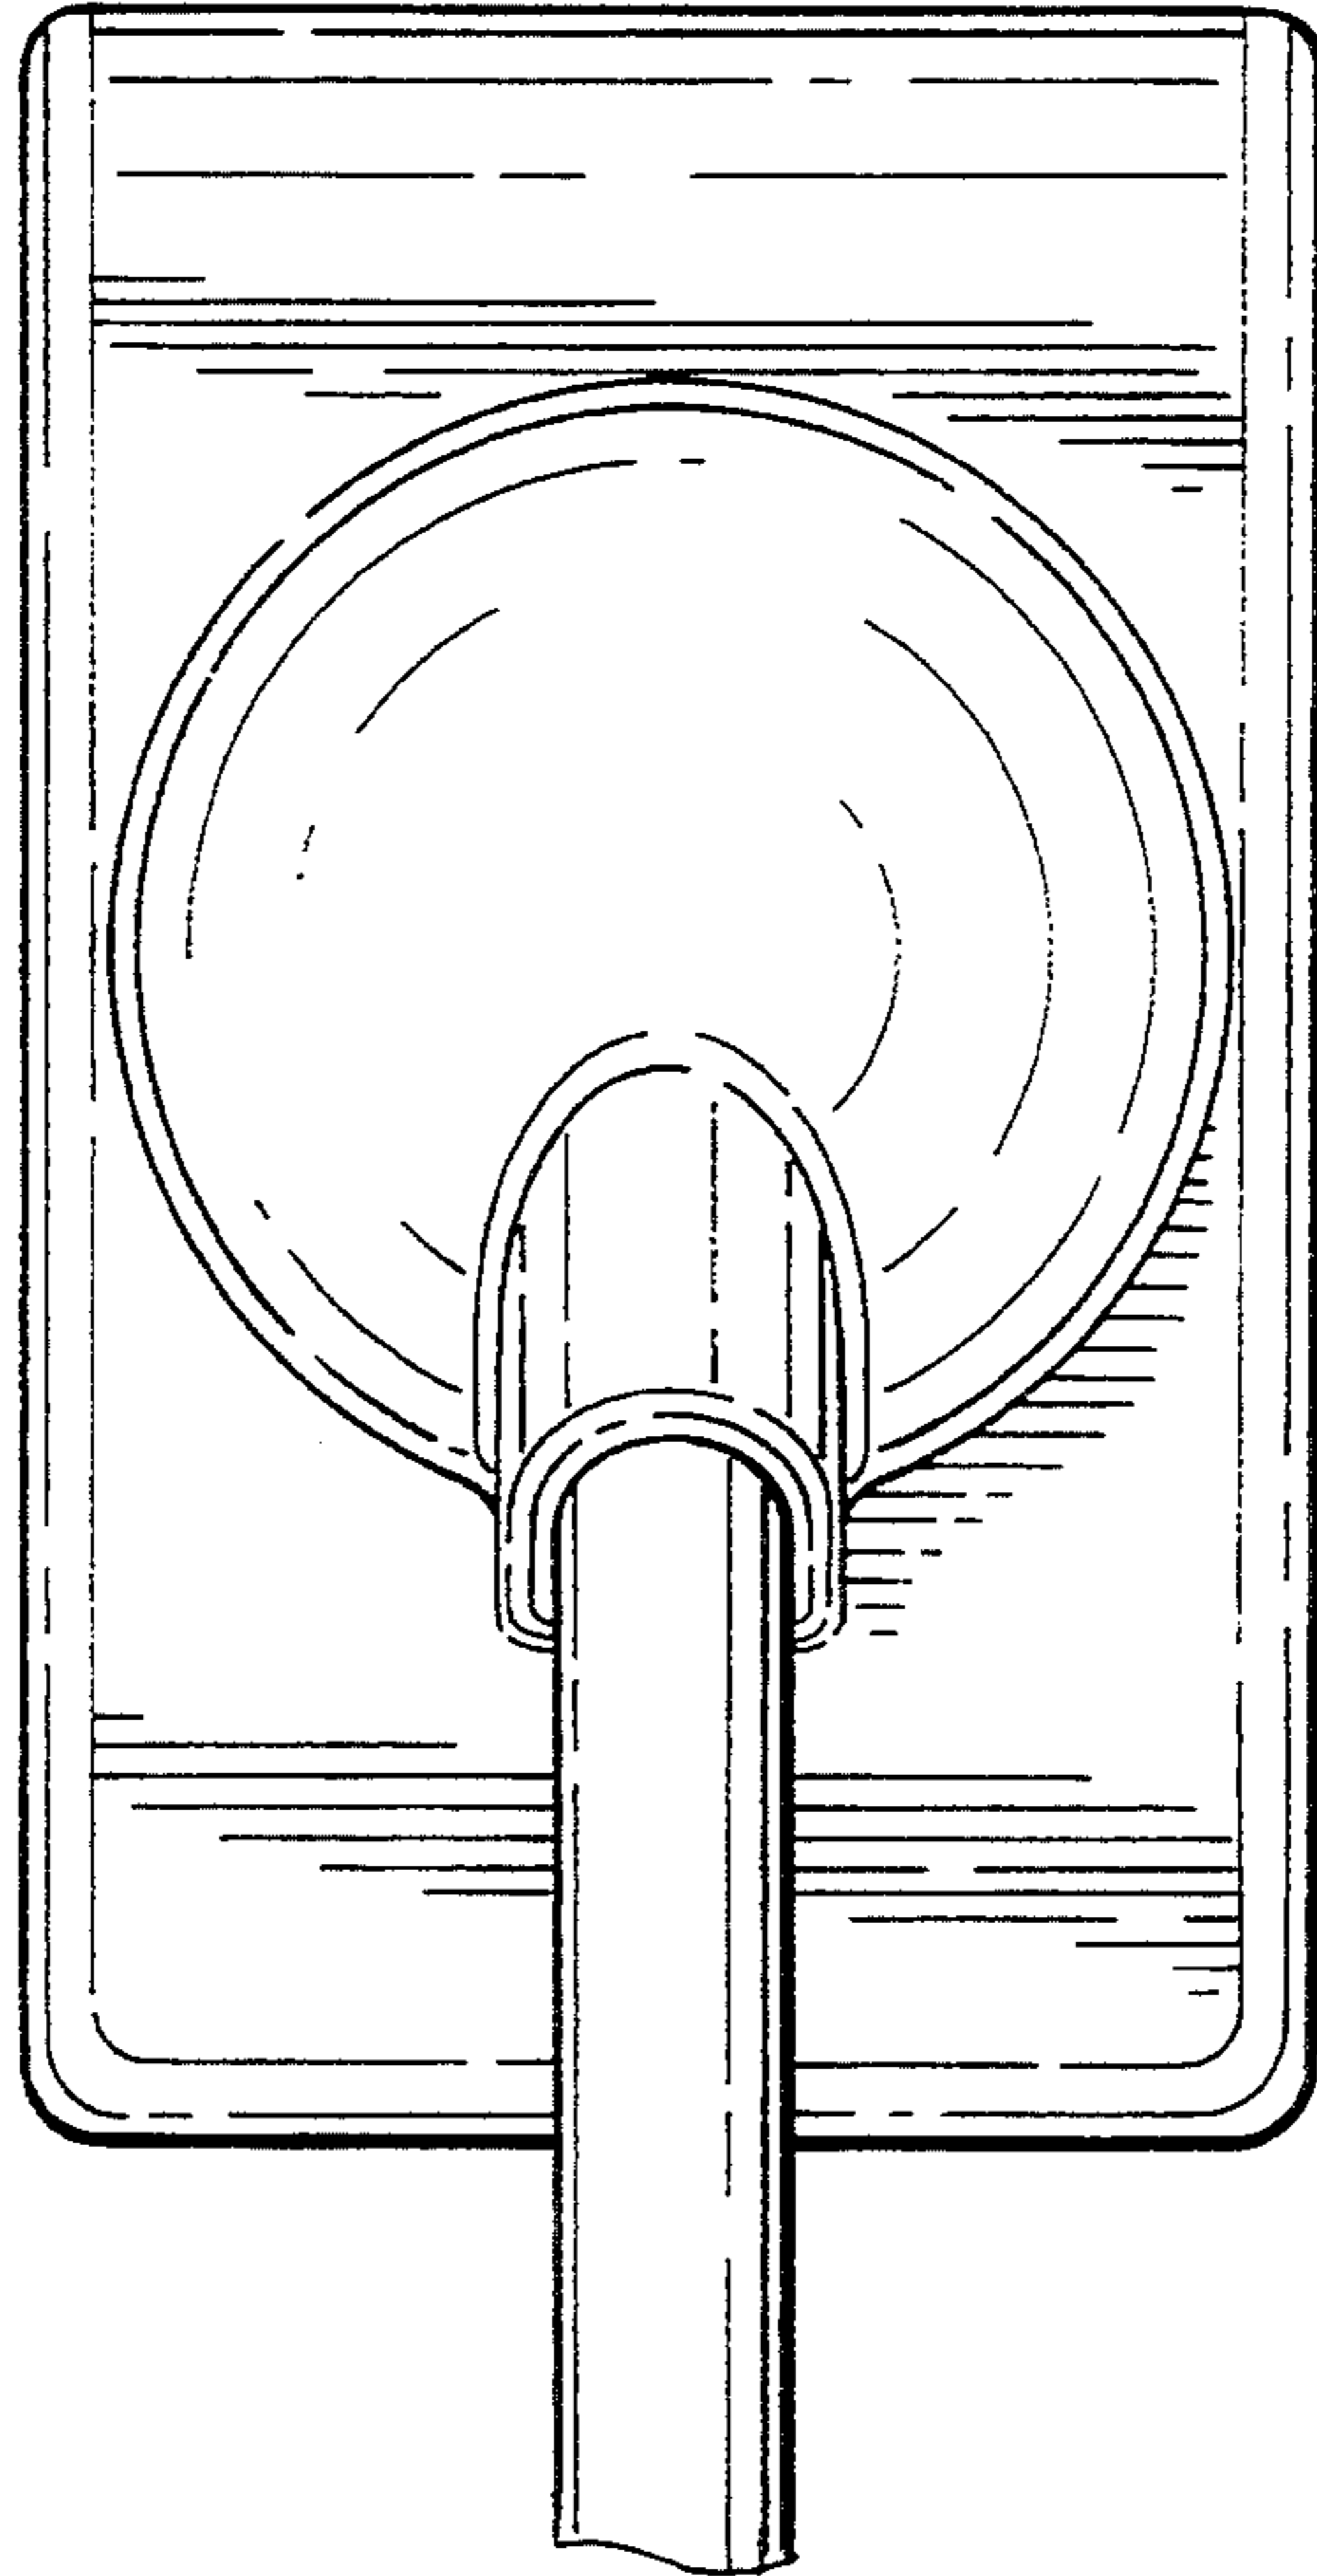


FIG 5

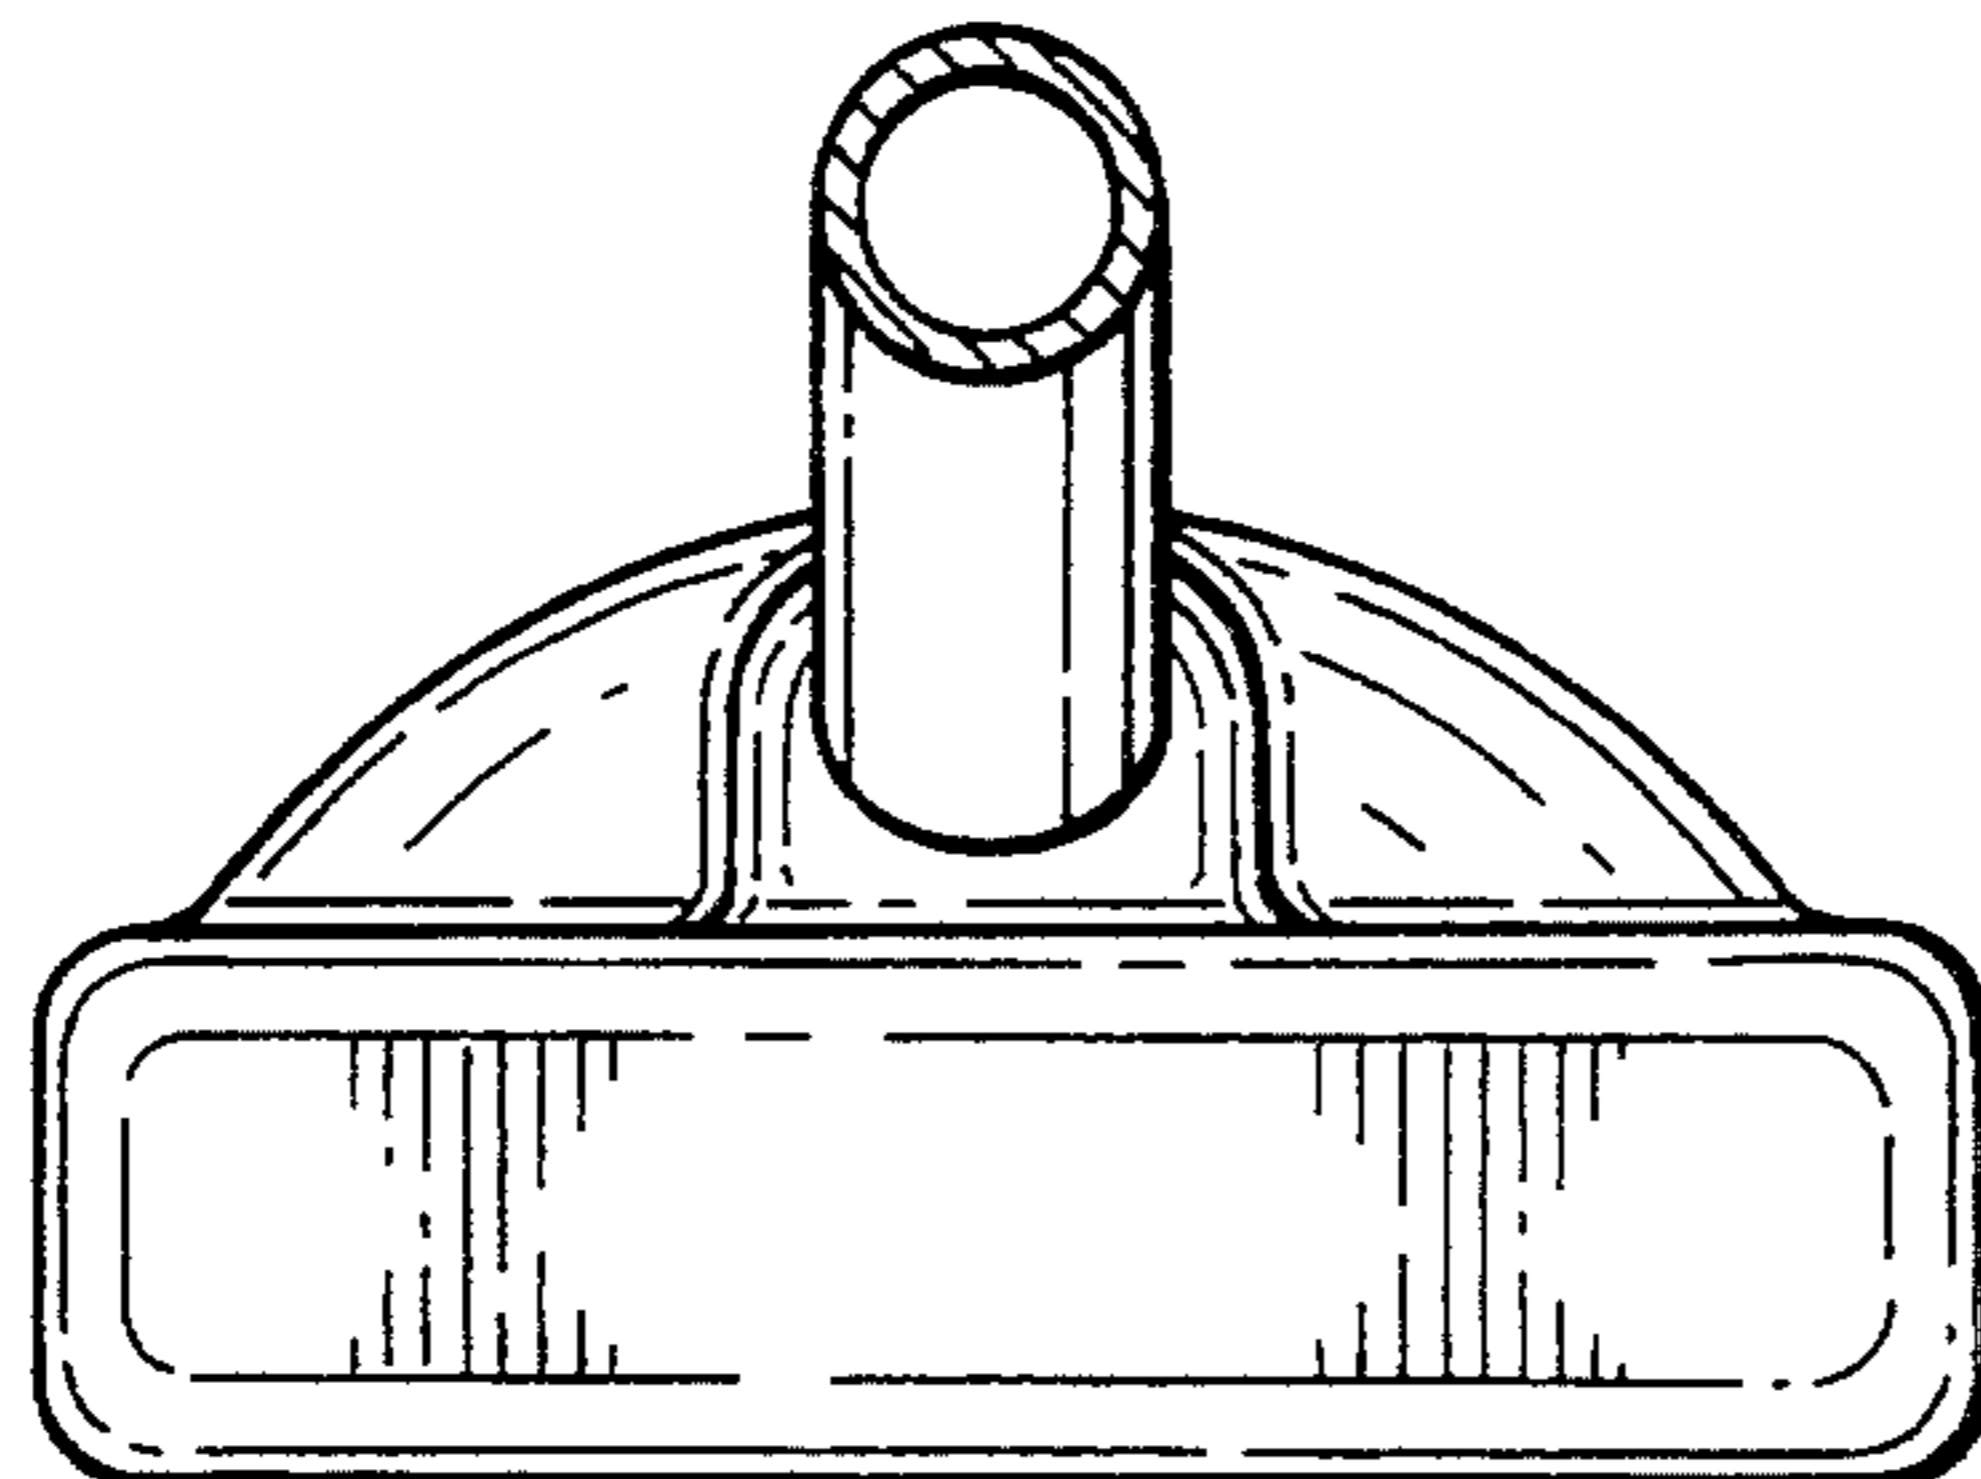


FIG 6