



US00D363124S

United States Patent [19]
Savage et al.

[11] **Patent Number:** **Des. 363,124**
[45] **Date of Patent:** ****Oct. 10, 1995**

[54] **SENSOR CARTRIDGE FOR A FLUID
ANALYTE ANALYZER**

[75] Inventors: **Douglas R. Savage**, Del Mar; **Richard
J. Koerner**, San Diego; **Allan L.
Cameron**, Santa Monica, all of Calif.

[73] Assignee: **PPG Industries, Inc.**, Pittsburgh, Pa.

[**] Term: **14 Years**

[21] Appl. No.: **8,496**

[22] Filed: **May 18, 1993**

Related U.S. Application Data

[63] Continuation-in-part of Ser. No. 885,203, May 18, 1992,
abandoned.

[52] U.S. Cl. **D24/169**

[58] Field of Search D24/169, 165,
D24/186; 128/634, 635, 665, 667, 673,
689, DIG. 13; D10/81

[56] **References Cited**

U.S. PATENT DOCUMENTS

5,046,496 1/1991 Betts et al. 128/635

Primary Examiner—Stella Reid

Attorney, Agent, or Firm—Kenneth J. Stachel

[57] **CLAIM**

The ornamental design for a sensor cartridge for a fluid
analyte analyzer, as shown and described.

DESCRIPTION

FIG. 1 is a top and right side perspective view of a sensor
cartridge for a fluid analyte analyzer;

FIG. 2 is a left side elevational view thereof;

FIG. 3 is a right side elevational view thereof;


FIG. 4 is a front elevational view thereof;

FIG. 5 is a back elevational view thereof;

FIG. 6 is a bottom elevational view thereof; and,

FIG. 7 is a top plan view thereof.

1 Claim, 1 Drawing Sheet

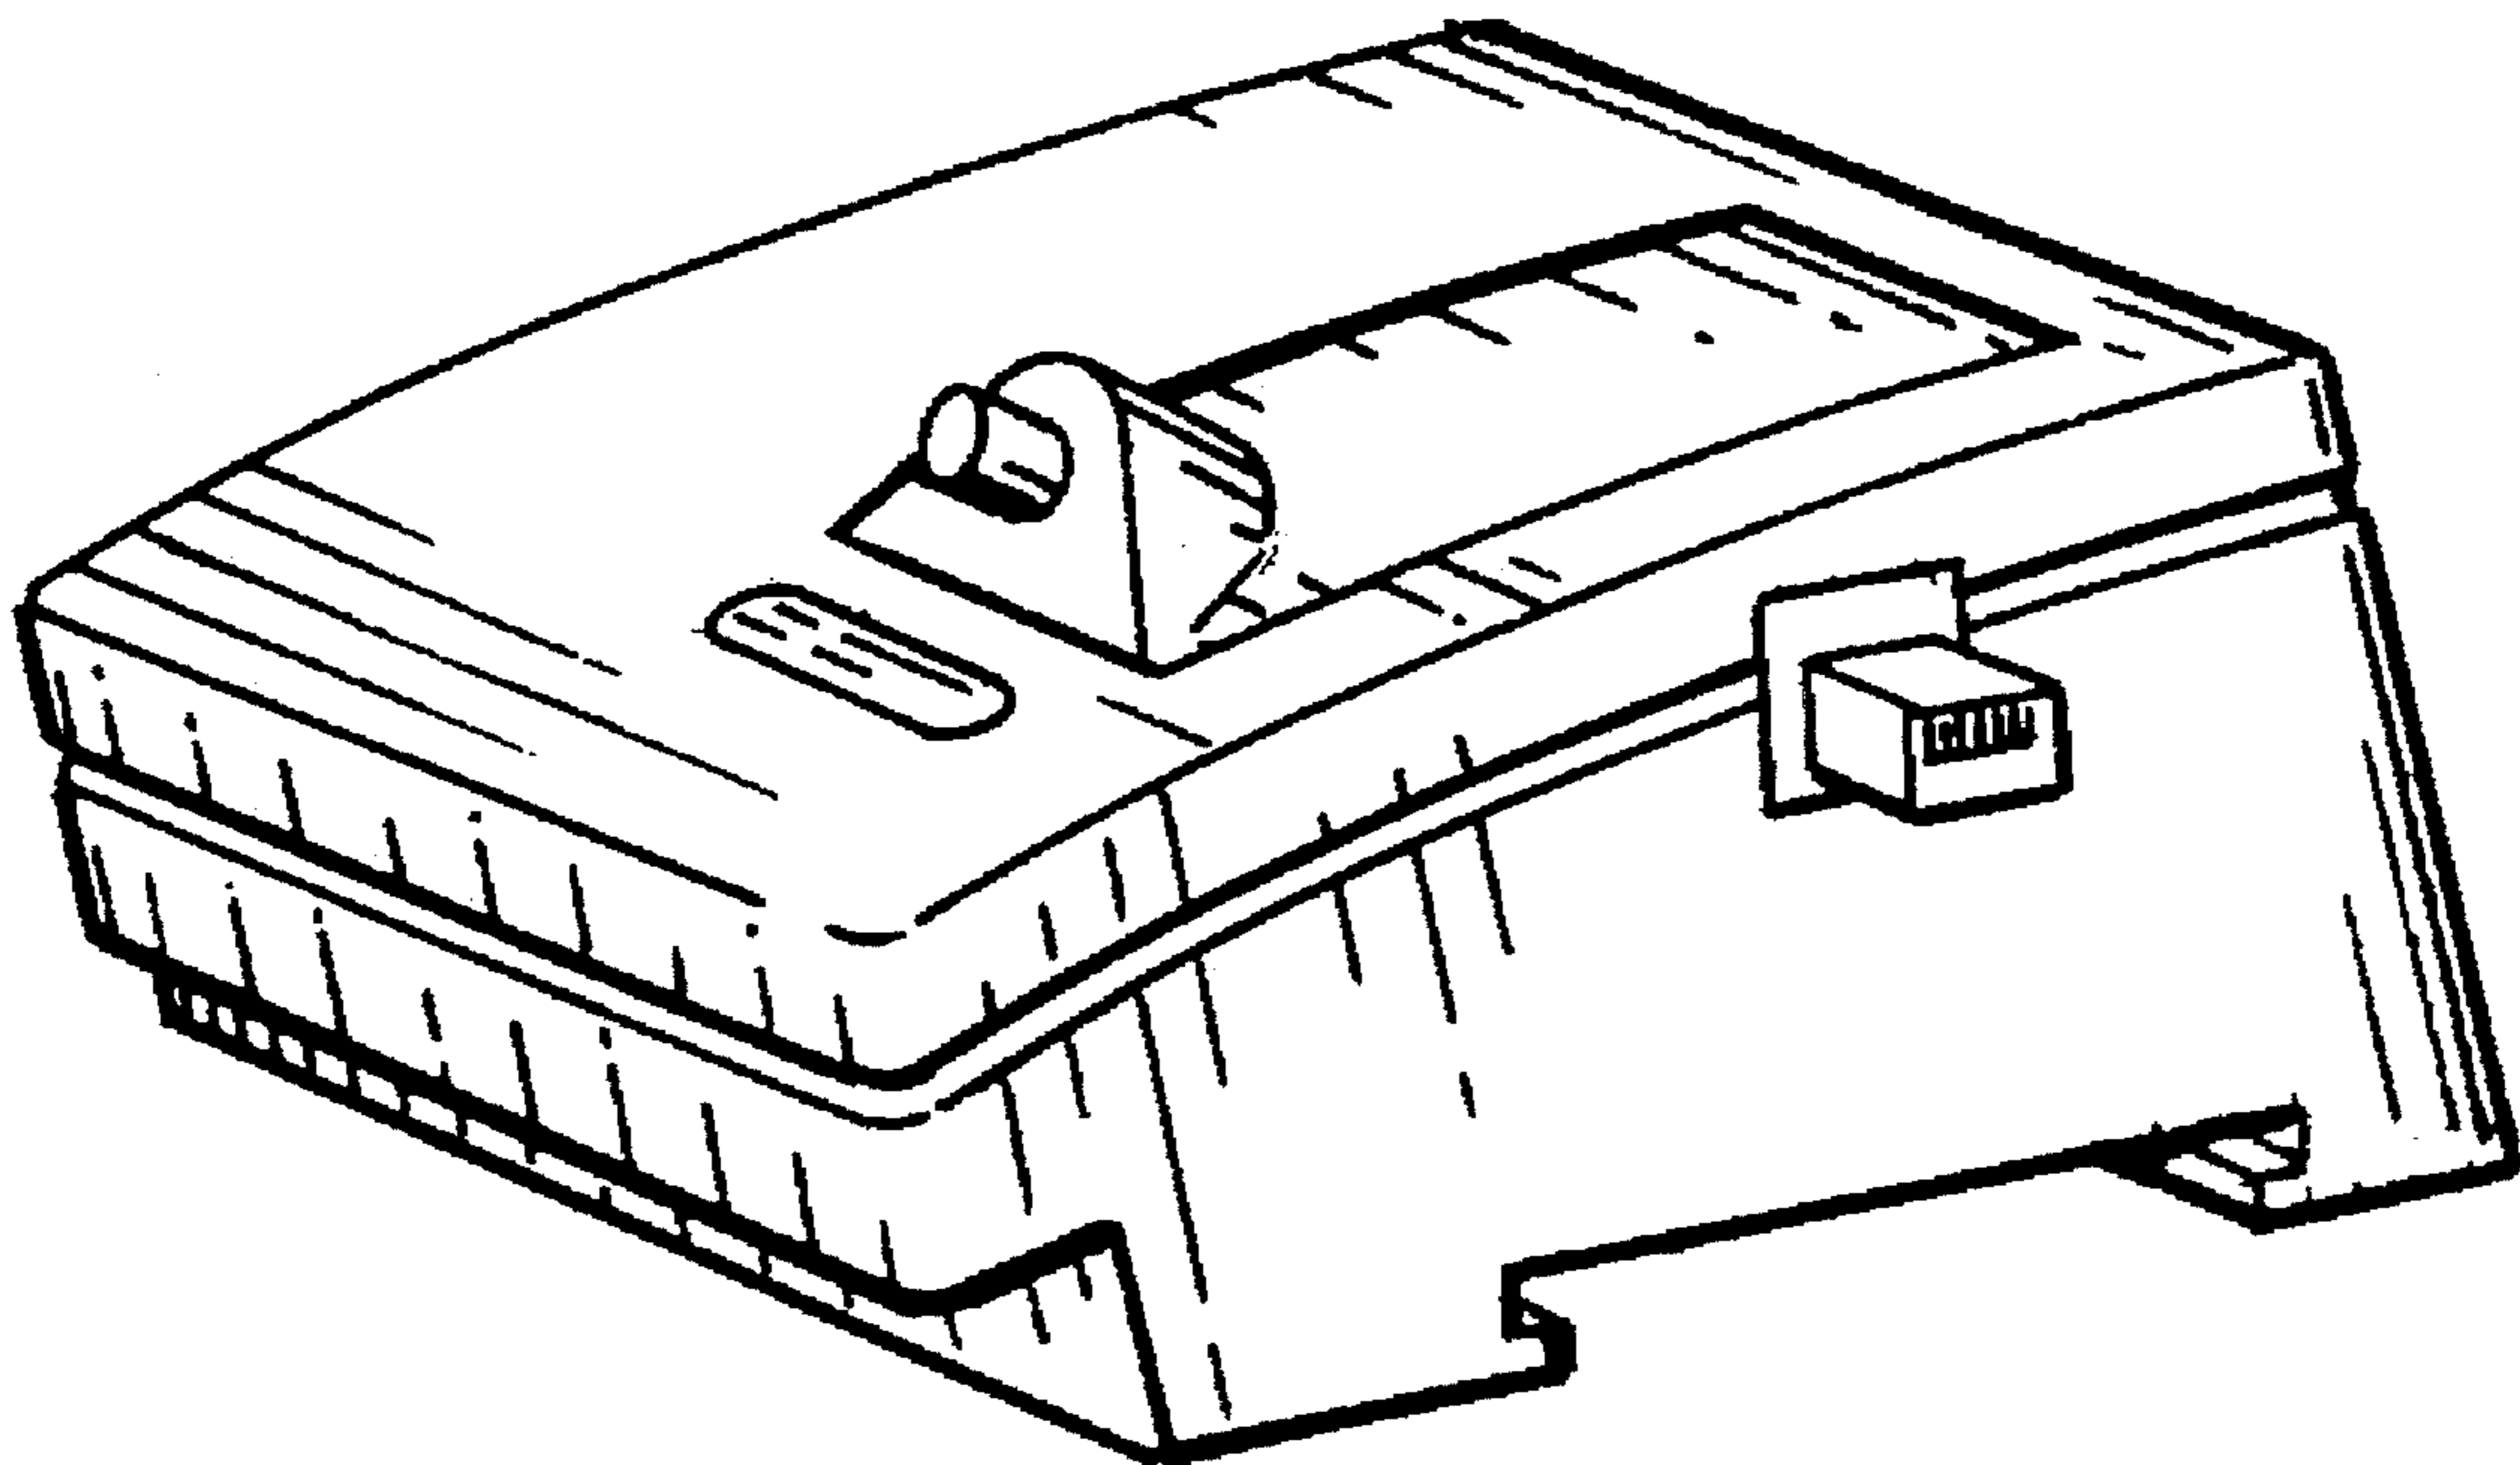

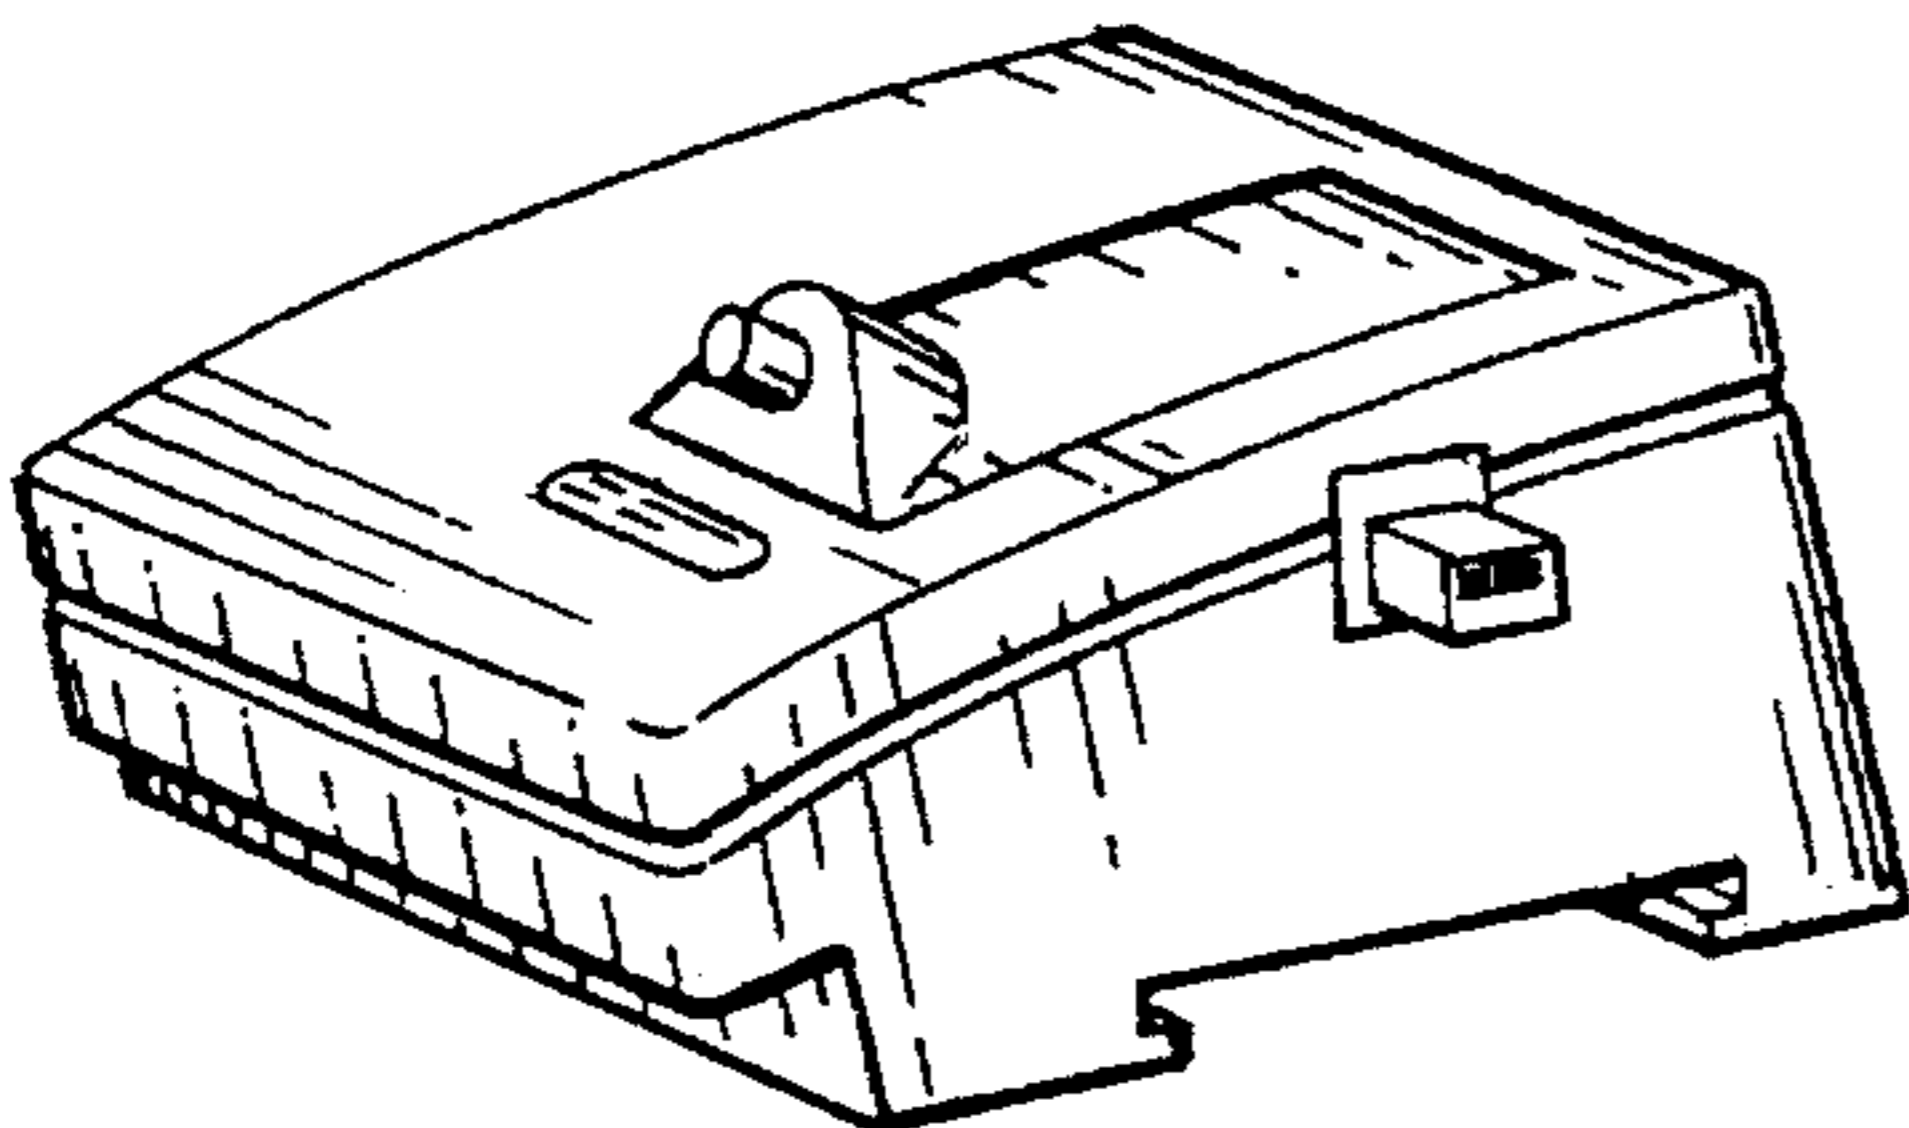


FIG. 1

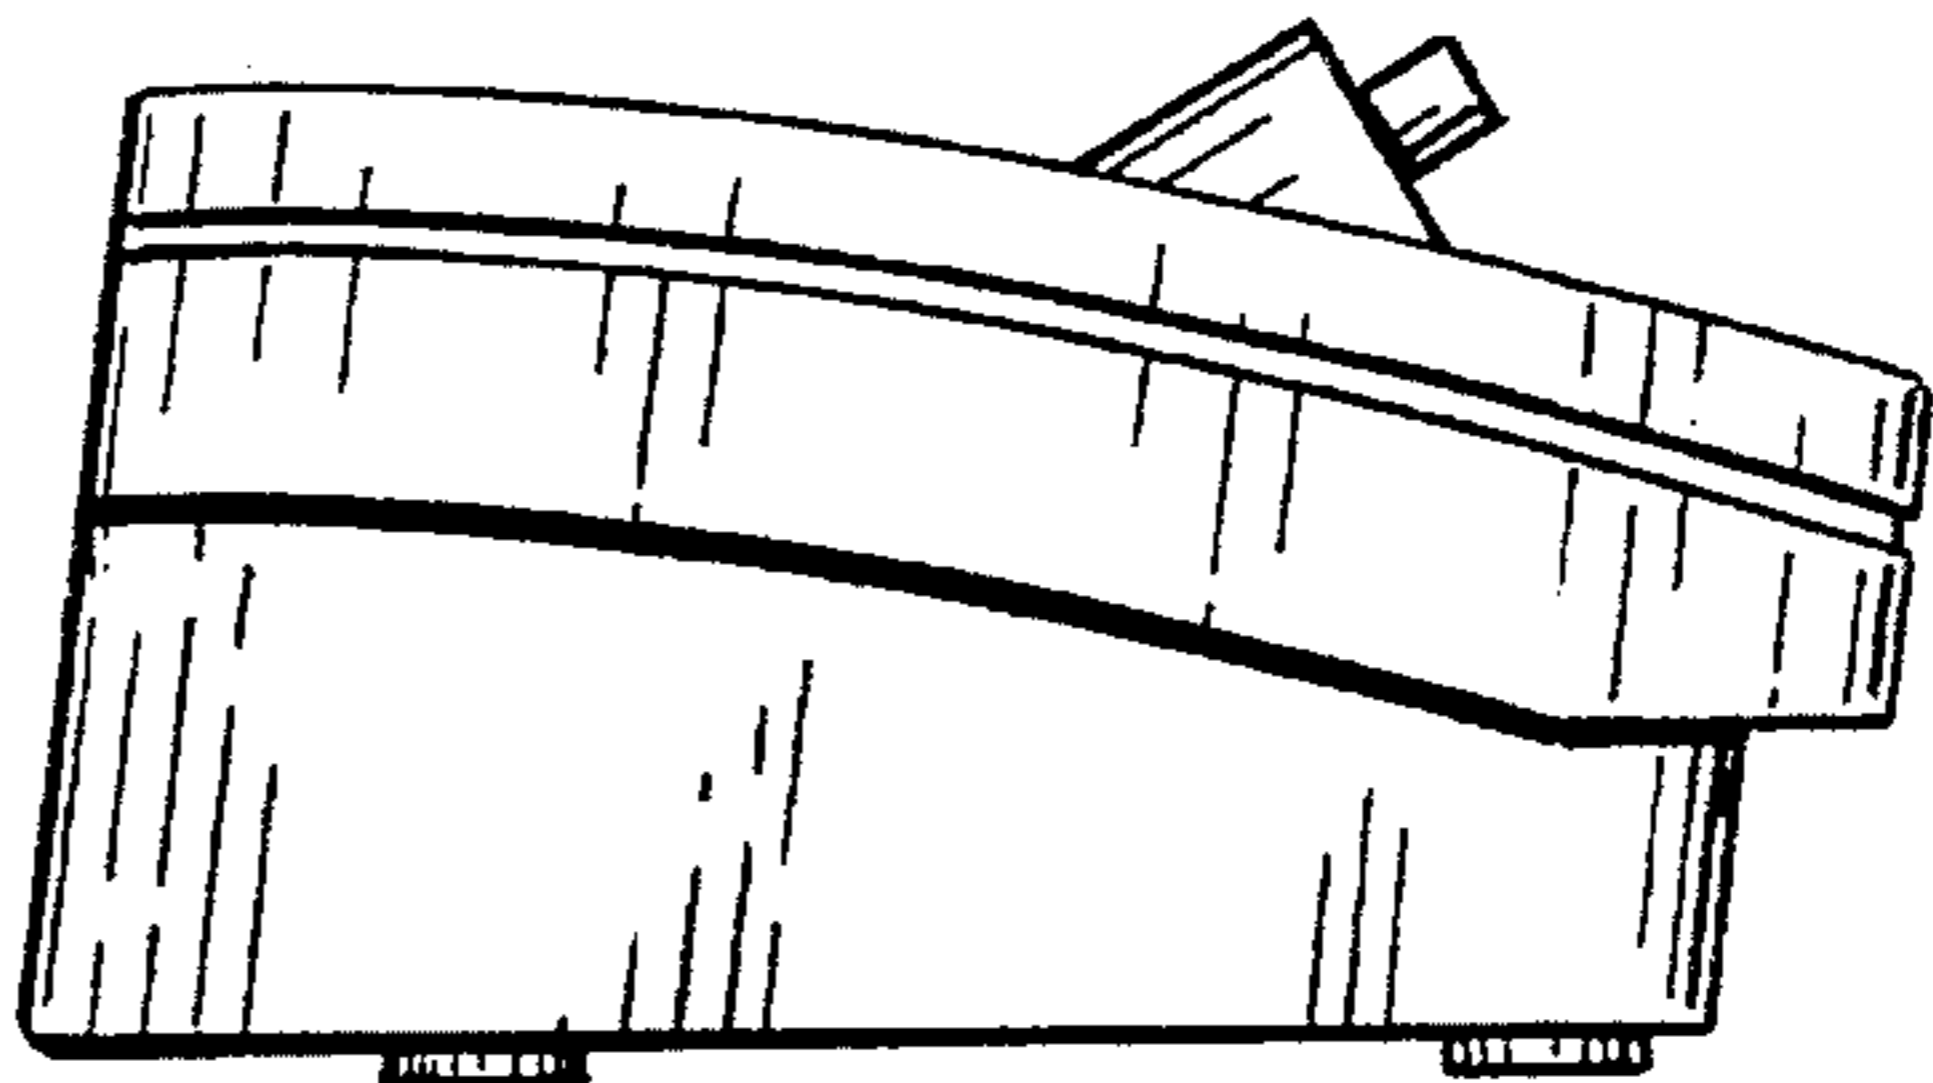


FIG. 2

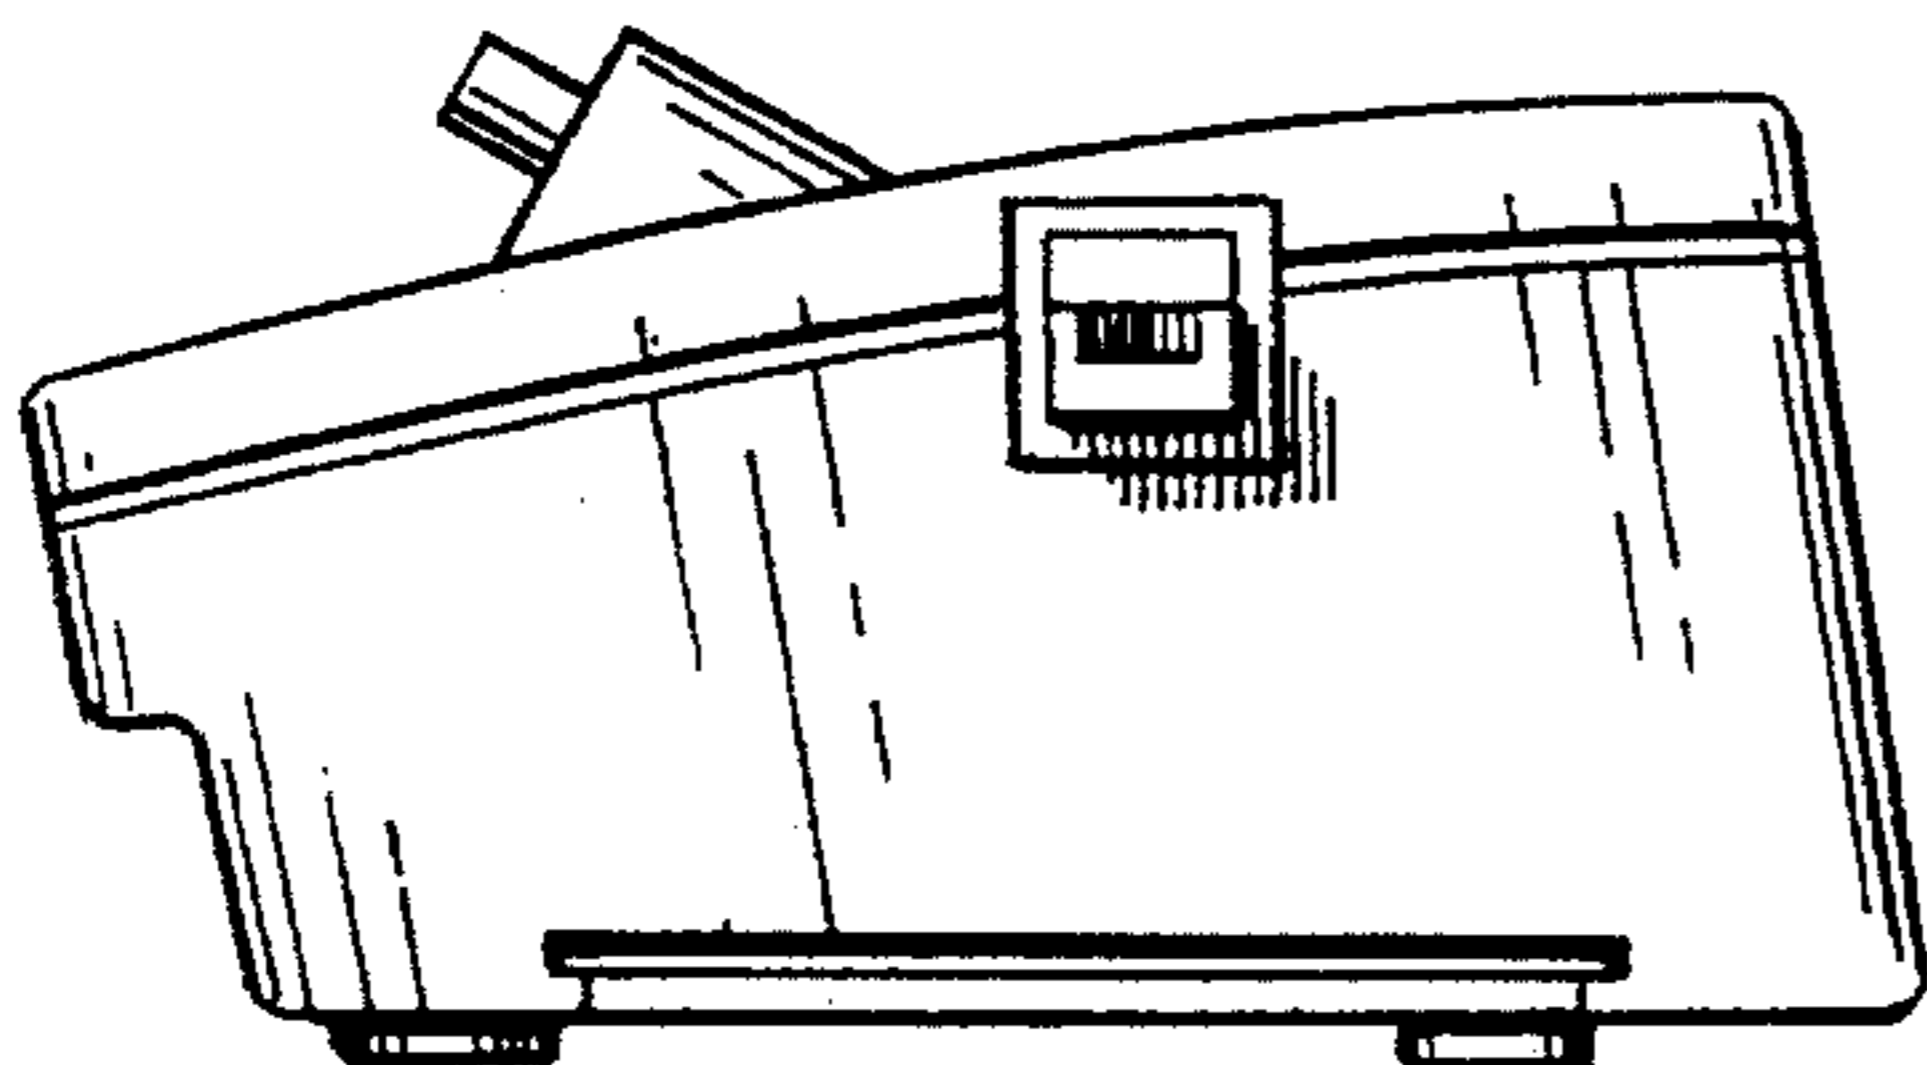


FIG. 3

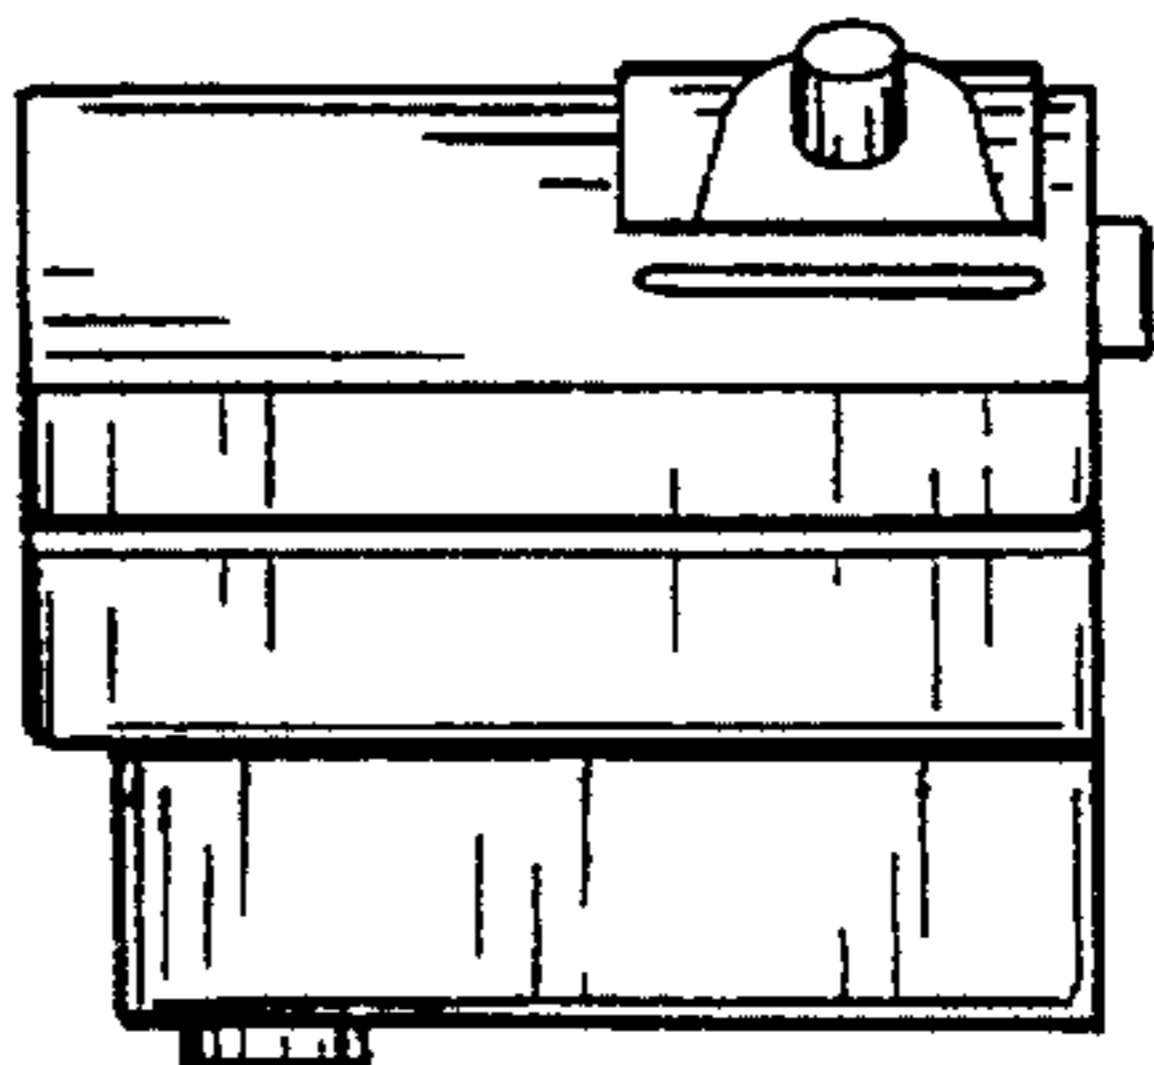


FIG. 4

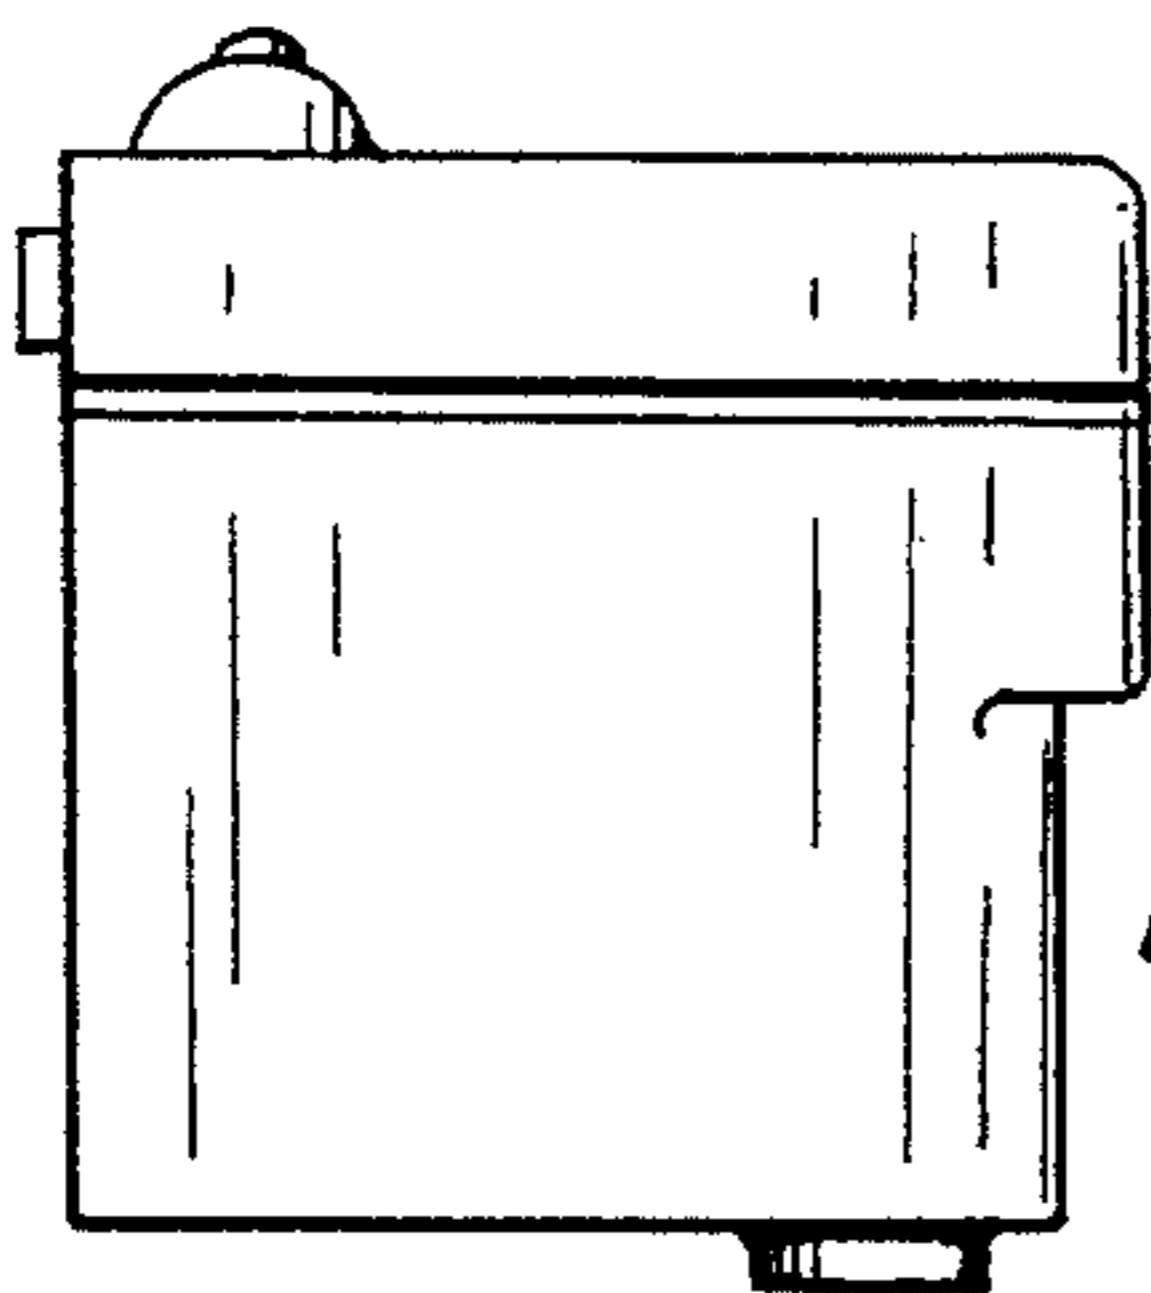


FIG. 5

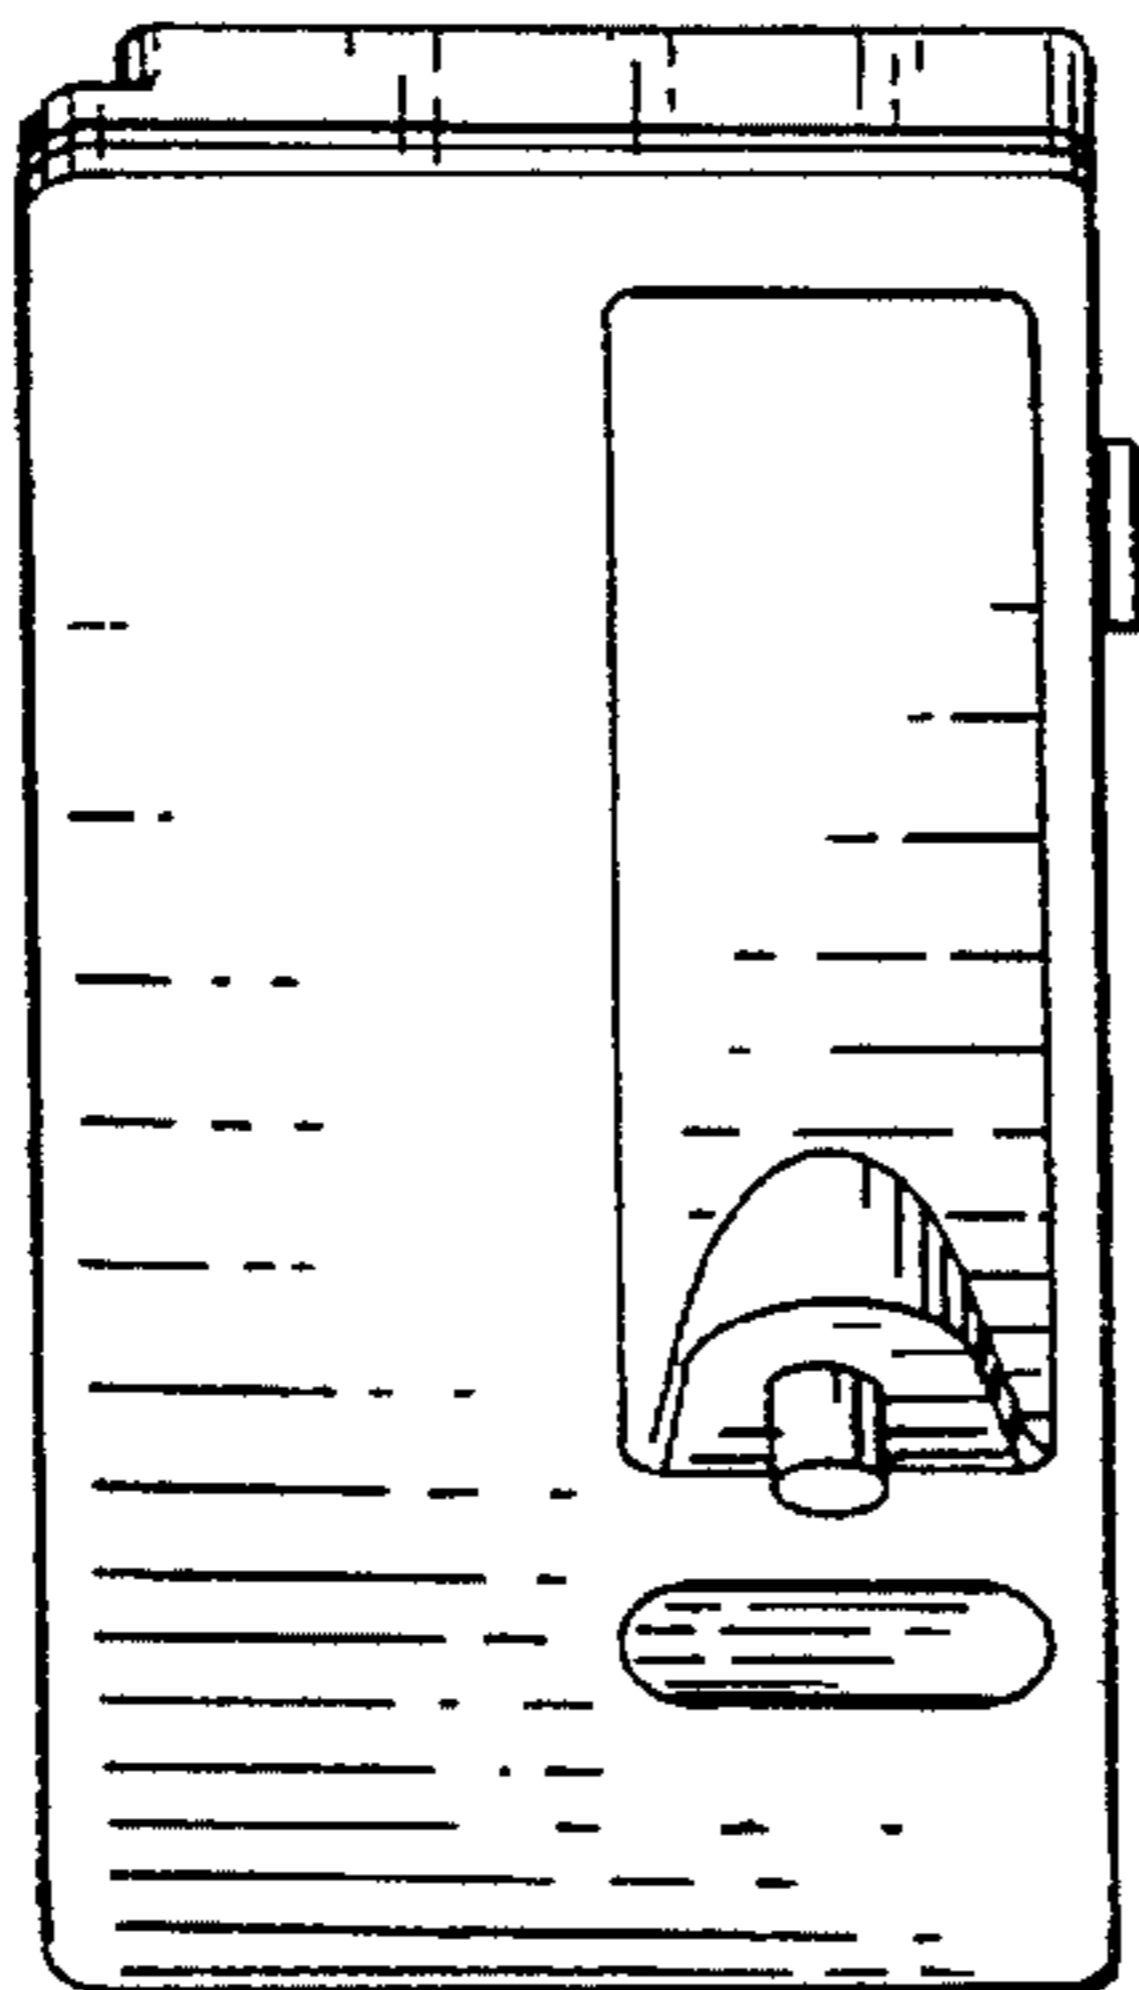


FIG. 7

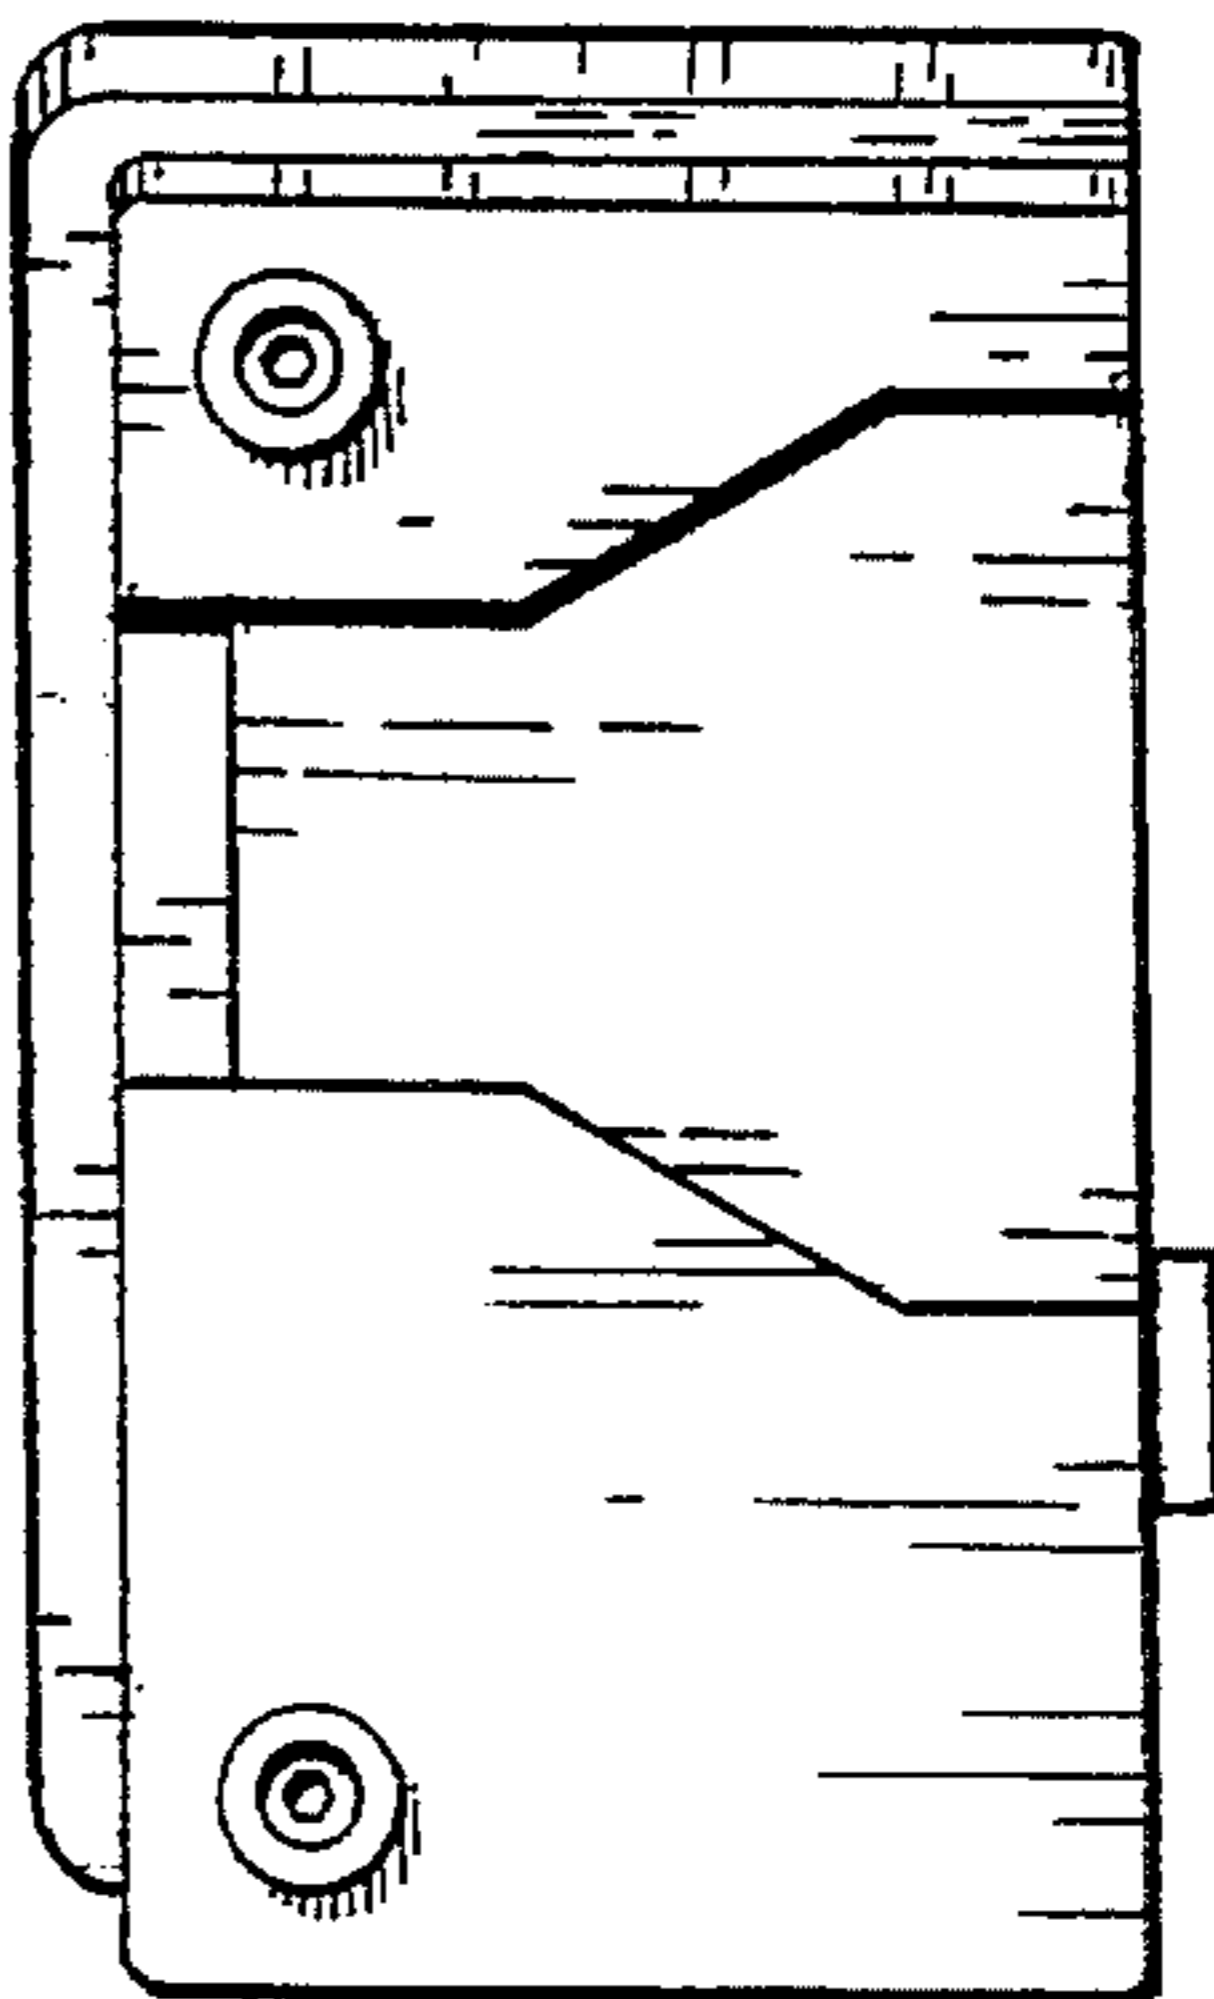


FIG. 6

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : Des. 363,124

Page 1 of 2

DATED : October 10, 1995

INVENTOR(S) : Savage et al

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

On the title page: Item [56]

Under "References Cited" on the face page of the patent, the cited foreign references and other publications were not listed:

US 3,710,778	1/73	Cornelius
US 4,201,222	5/80	Haase
US 4,549,951	10/85	Knudson et al.
US 4,615,340	10/86	Cronenberg et al.
US 4,654,127	3/87	Baker et al.
US 4,913,703	4/90	Pasqualucci et al.
US 4,929,426	5/90	Bodai et al.
D 331,286	11/92	Cameron et al.
D 333,992	3/93	Anderson
WO 85/02257	5/85	PCT
WO 92/08130	5/92	PCT

Information Brochure entitled "Pick A Card" by Johnson & Johnson Professional Diagnostics Inc.

Arden Medical Systems, Inc. Prospectus, published by Engler-Budd & Co. Inc., 1986

UNITED STATES PATENT AND TRADEMARK OFFICE
CERTIFICATE OF CORRECTION

PATENT NO. : Des. 363,124
DATED : October 10, 1995
INVENTOR(S) : Savage et al

Page 2 of 2

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

Information Brochure entitled "World Wide" by Johnson & Johnson
Professional Diagnostics Inc., December 1987

Information Brochure re Diametrics Medical Inc. entitled "Private
Placement Memorandum" by Vector Securities International, Sept. 1992

Prospectus Re: Diametrics Medical Inc., June 1993

Information Brochure re IRMATM Blood Analysis System, Diametrics
Medical Inc., May 1993

Design Application, USSN 29/008,497, filed May 1993

Signed and Sealed this
Twenty-seventh Day of August, 1996

Attest:



BRUCE LEHMAN

Attesting Officer

Commissioner of Patents and Trademarks