



US00D363541S

# United States Patent [19]

Cottone, Sr. et al.

[11] Patent Number: **Des. 363,541**

[45] Date of Patent: **\*\*Oct. 24, 1995**

[54] **ROTATING ADAPTER FOR A CATHETER**

5,222,773 6/1993 Boehme ..... 285/93 X

5,281,206 1/1994 Lopez ..... 604/905 X

5,286,067 2/1994 Choksi ..... 285/93 X

[75] Inventors: **Joseph R. Cottone, Sr.**, Marietta;  
**Anthony J. Cottone**, Ball Ground, both  
of Ga.

*Primary Examiner*—Louis S. Zarfes  
*Assistant Examiner*—I. Simmons  
*Attorney, Agent, or Firm*—Veal & Marsh

[73] Assignee: **Maxxim Medical, Inc.**, Sugar Land,  
Tex.

[57] **CLAIM**

[\*\*] Term: **14 Years**

The ornamental design for a rotating adapter for a catheter,  
as shown and described.

[21] Appl. No.: **953,588**

**DESCRIPTION**

[22] Filed: **Sep. 29, 1992**

[52] U.S. Cl. .... **D24/129**

[58] Field of Search ..... D24/129, 108;  
604/29, 283, 905, 256; 285/93, 305, 313,  
315, 322


FIG. 1 is a front perspective view of our design;  
FIG. 2 is a rear perspective view of our design;  
FIG. 3 is a top plan view thereof, with the bottom plan view  
being the mirror image thereof;  
FIG. 4 is a right side view thereof, with the left side view  
being the mirror image thereof;  
FIG. 5 is an exploded view thereof, the broken line showing  
of the rubber gasket is for illustrative purposes only and  
forms no part of the claimed design;  
FIG. 6 is a front end view thereof;  
FIG. 7 is a rear end view thereof.

[56] **References Cited**


**U.S. PATENT DOCUMENTS**

- 4,254,773 3/1981 Waldbillig .
- 4,296,949 10/1981 Muetterties et al. .... 285/93 X
- 4,932,114 6/1990 Morse et al. .
- 4,994,048 2/1991 Metzger ..... 604/905 X
- 5,181,508 1/1993 Poole, Jr. .... D24/129 X


**1 Claim, 4 Drawing Sheets**

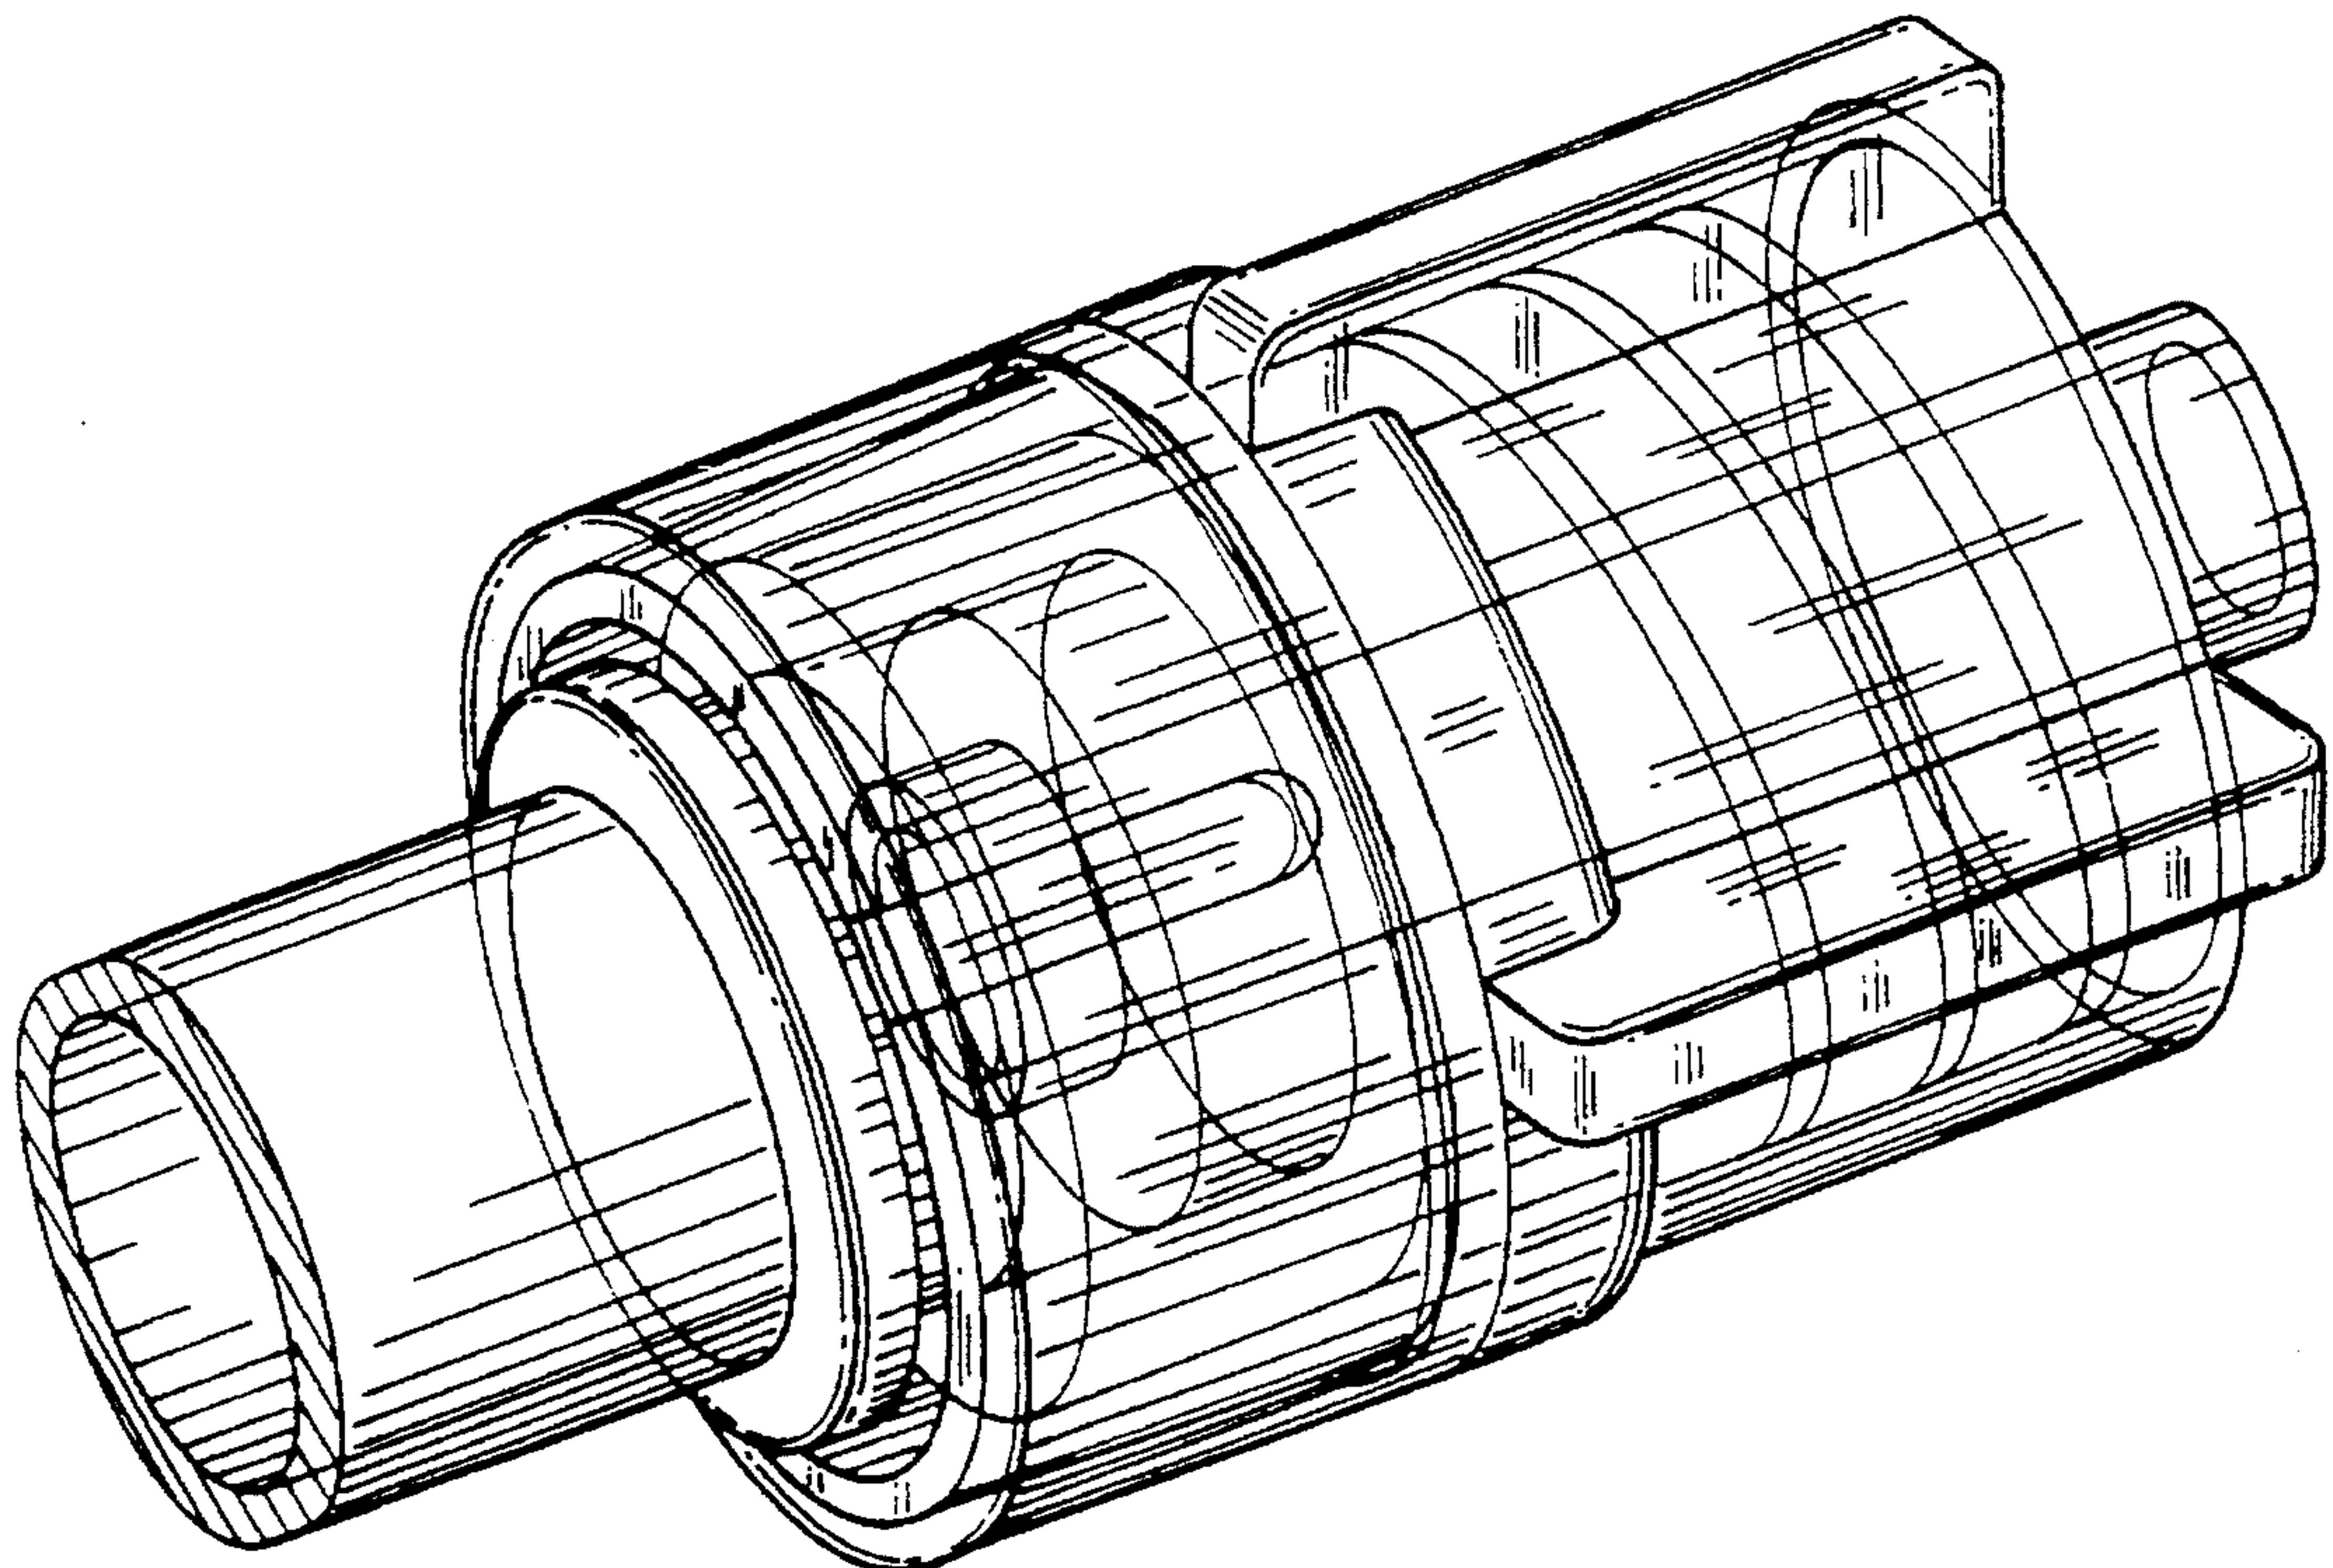




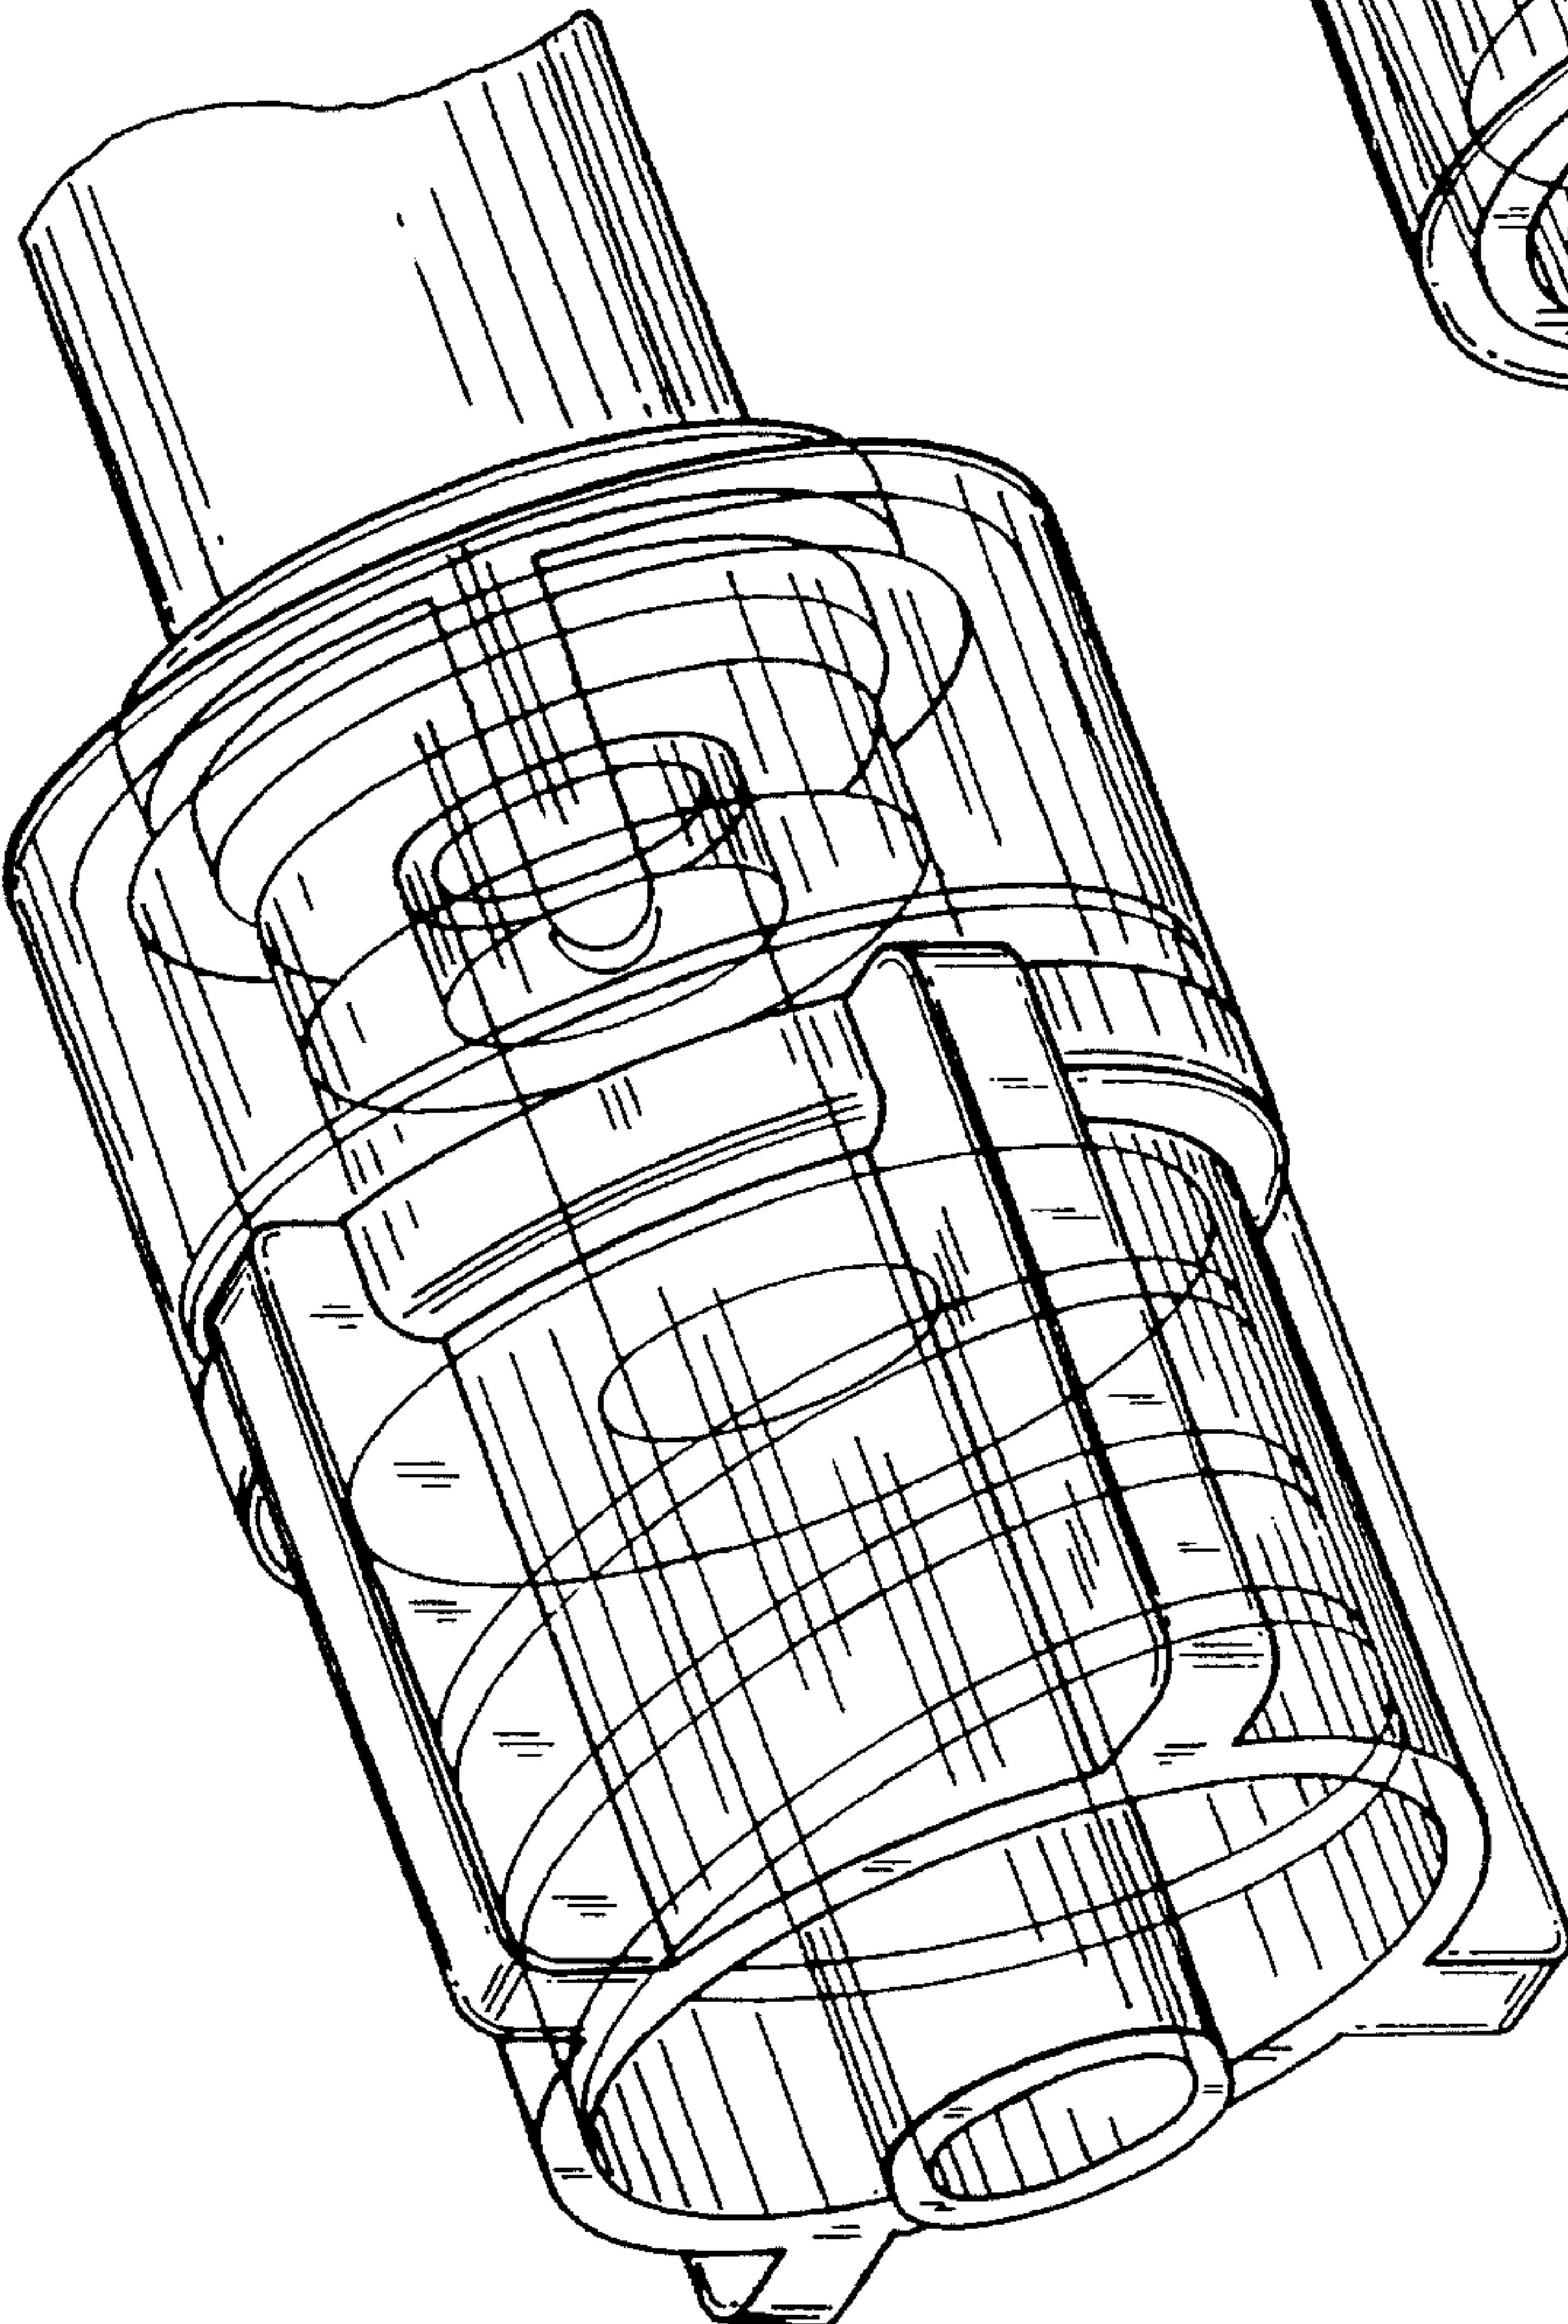

**FIG. 1**

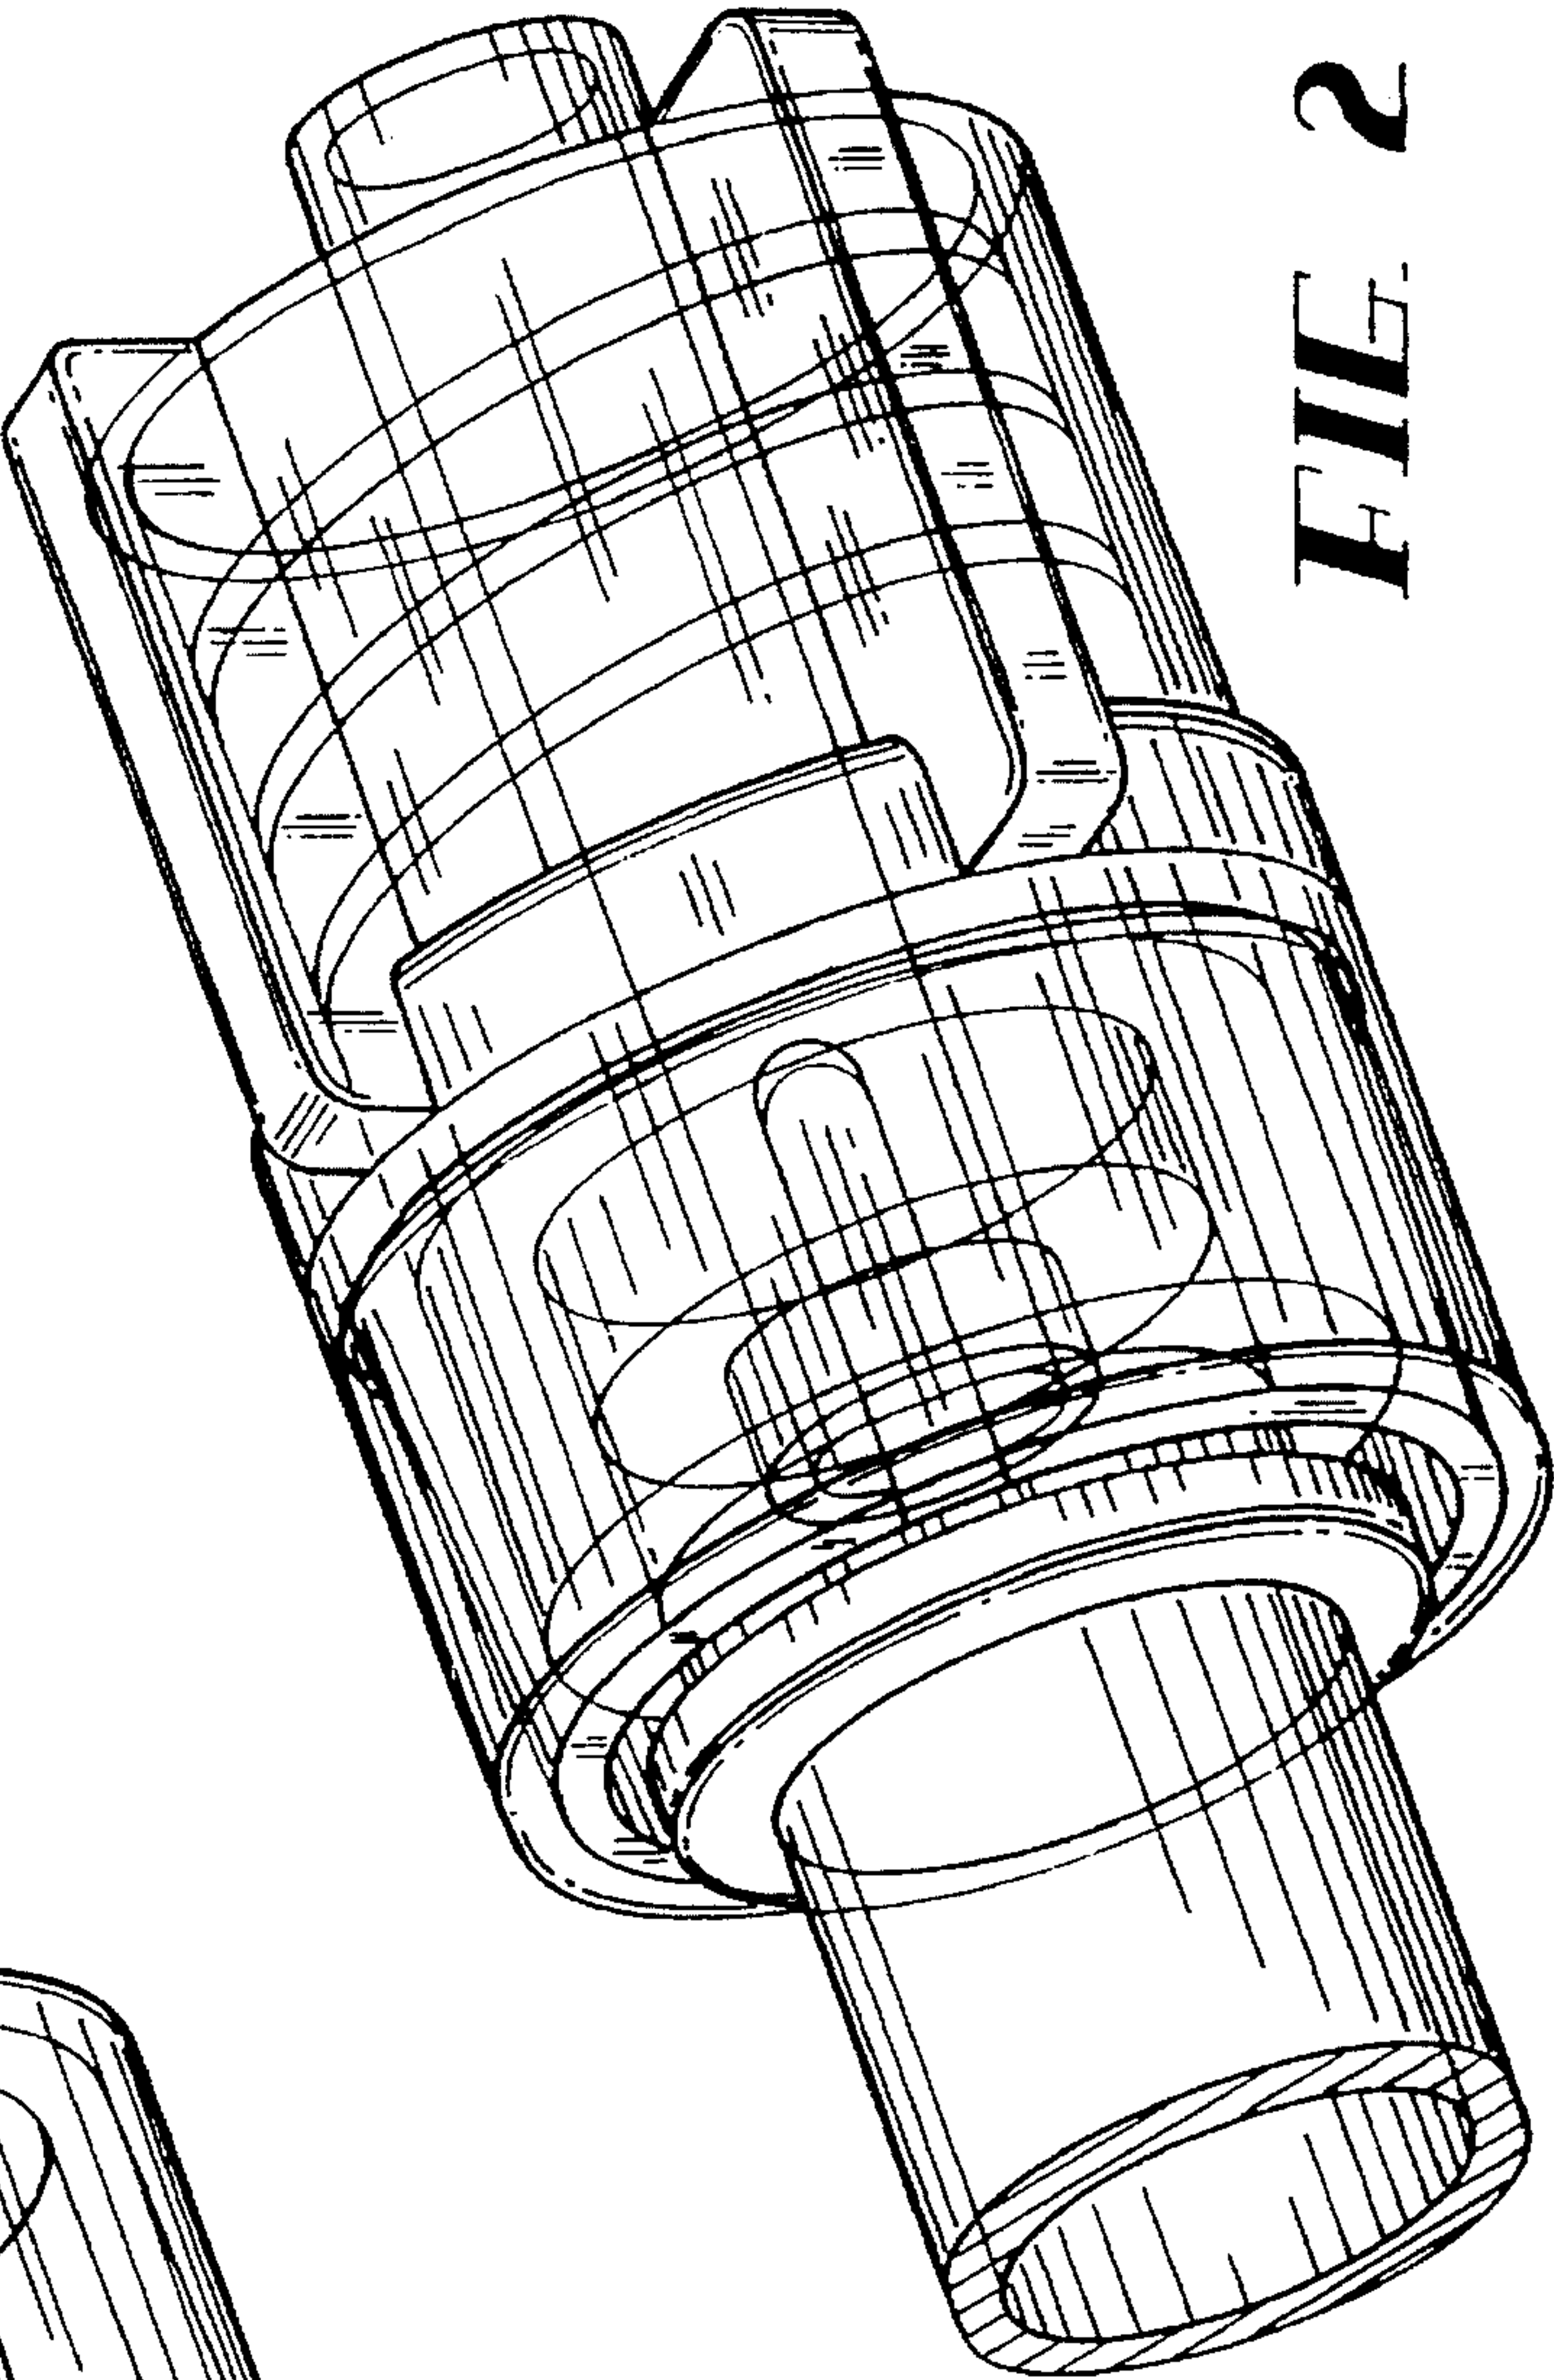


**FIG. 2**

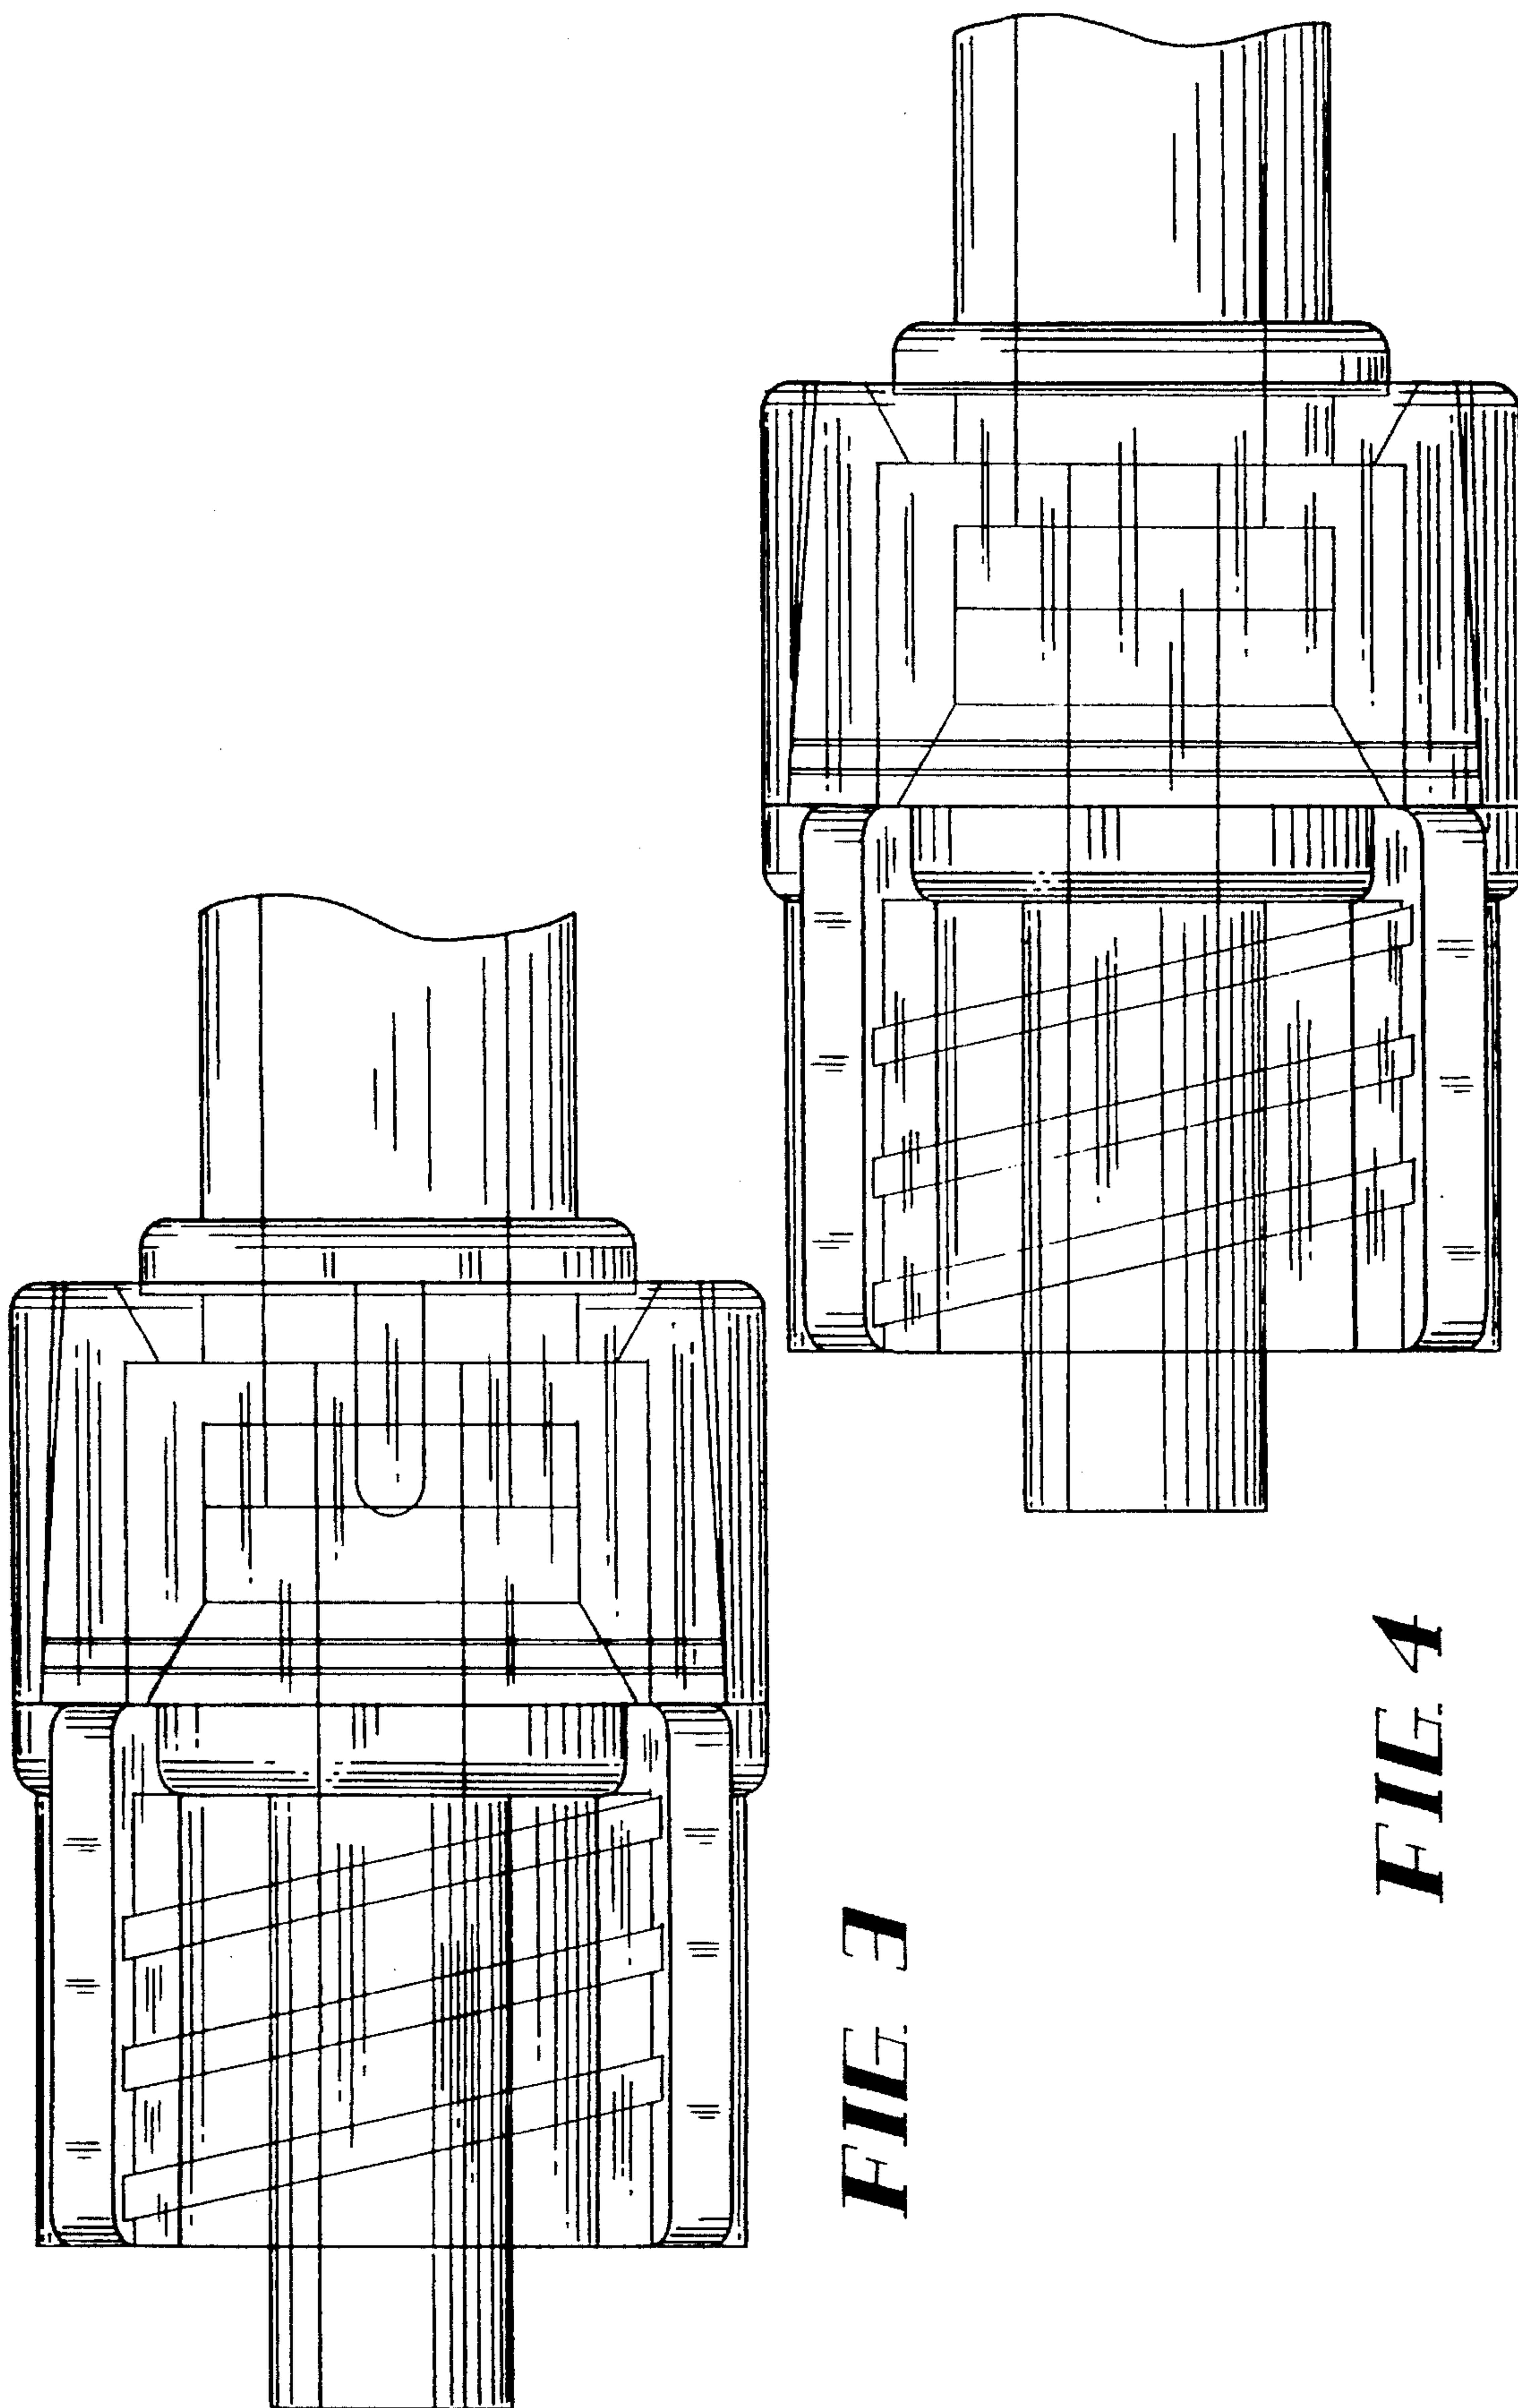


**FIG. 3**

**FIG. 4**

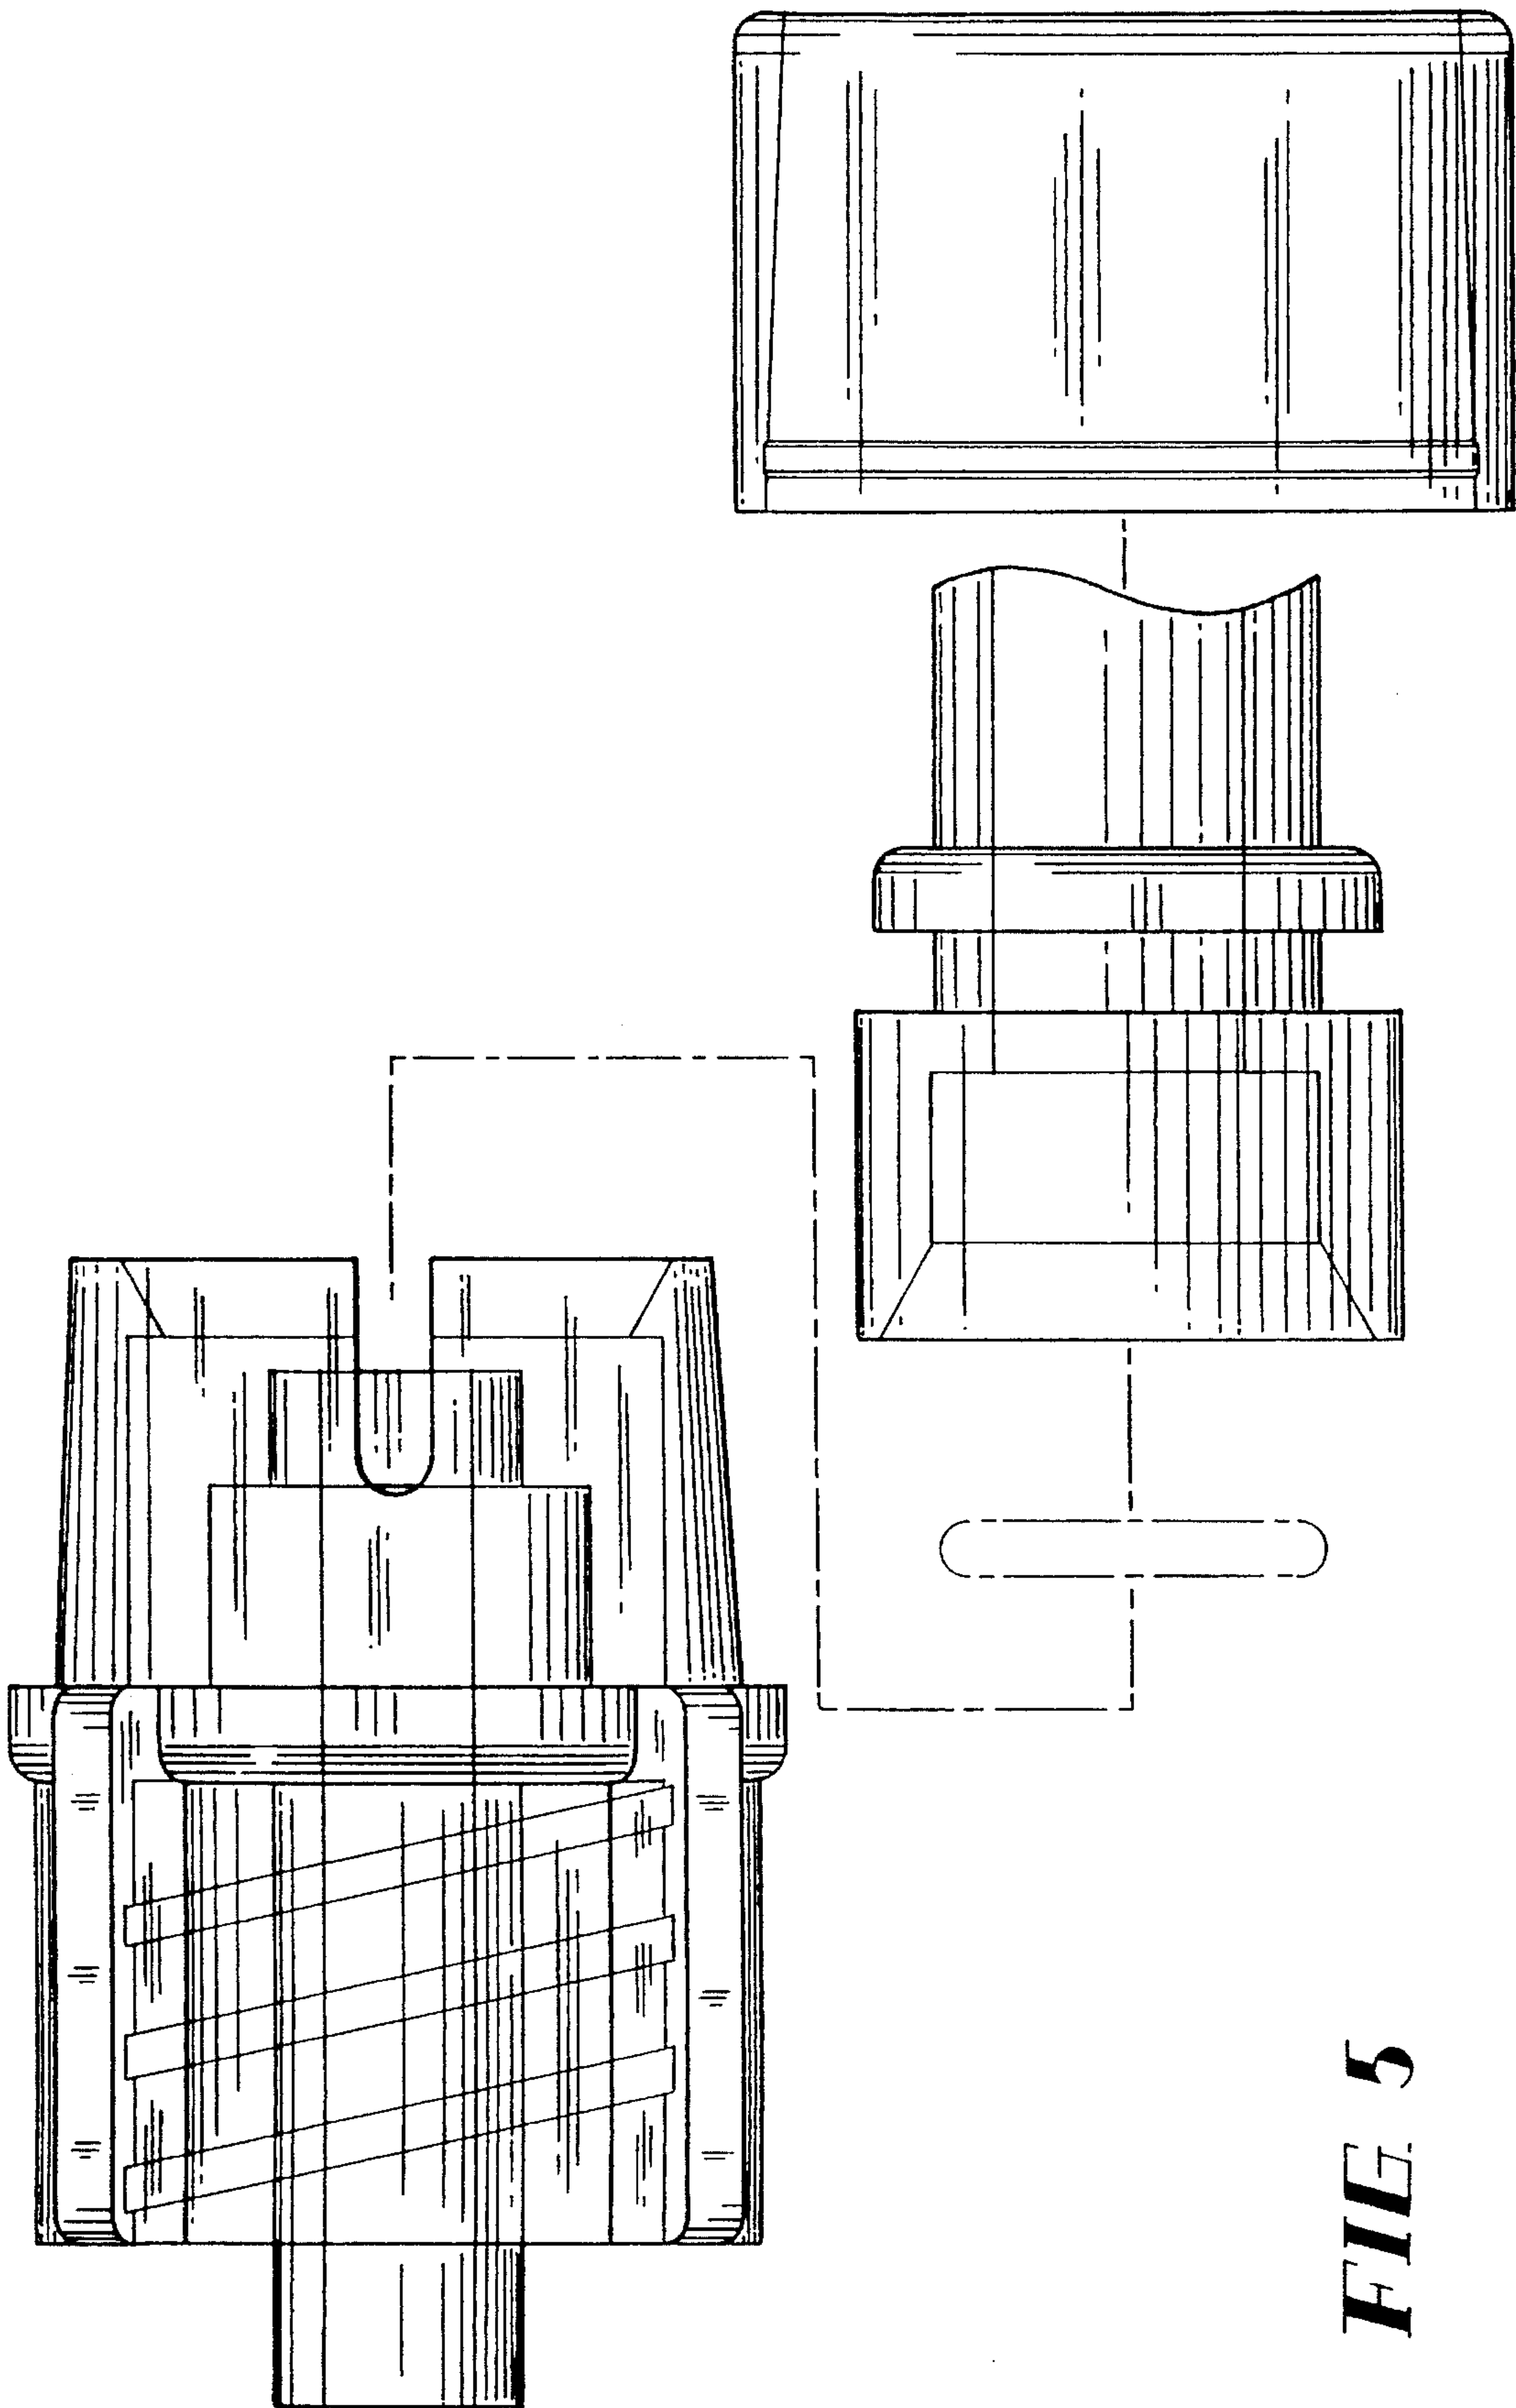


**FIG. 5**



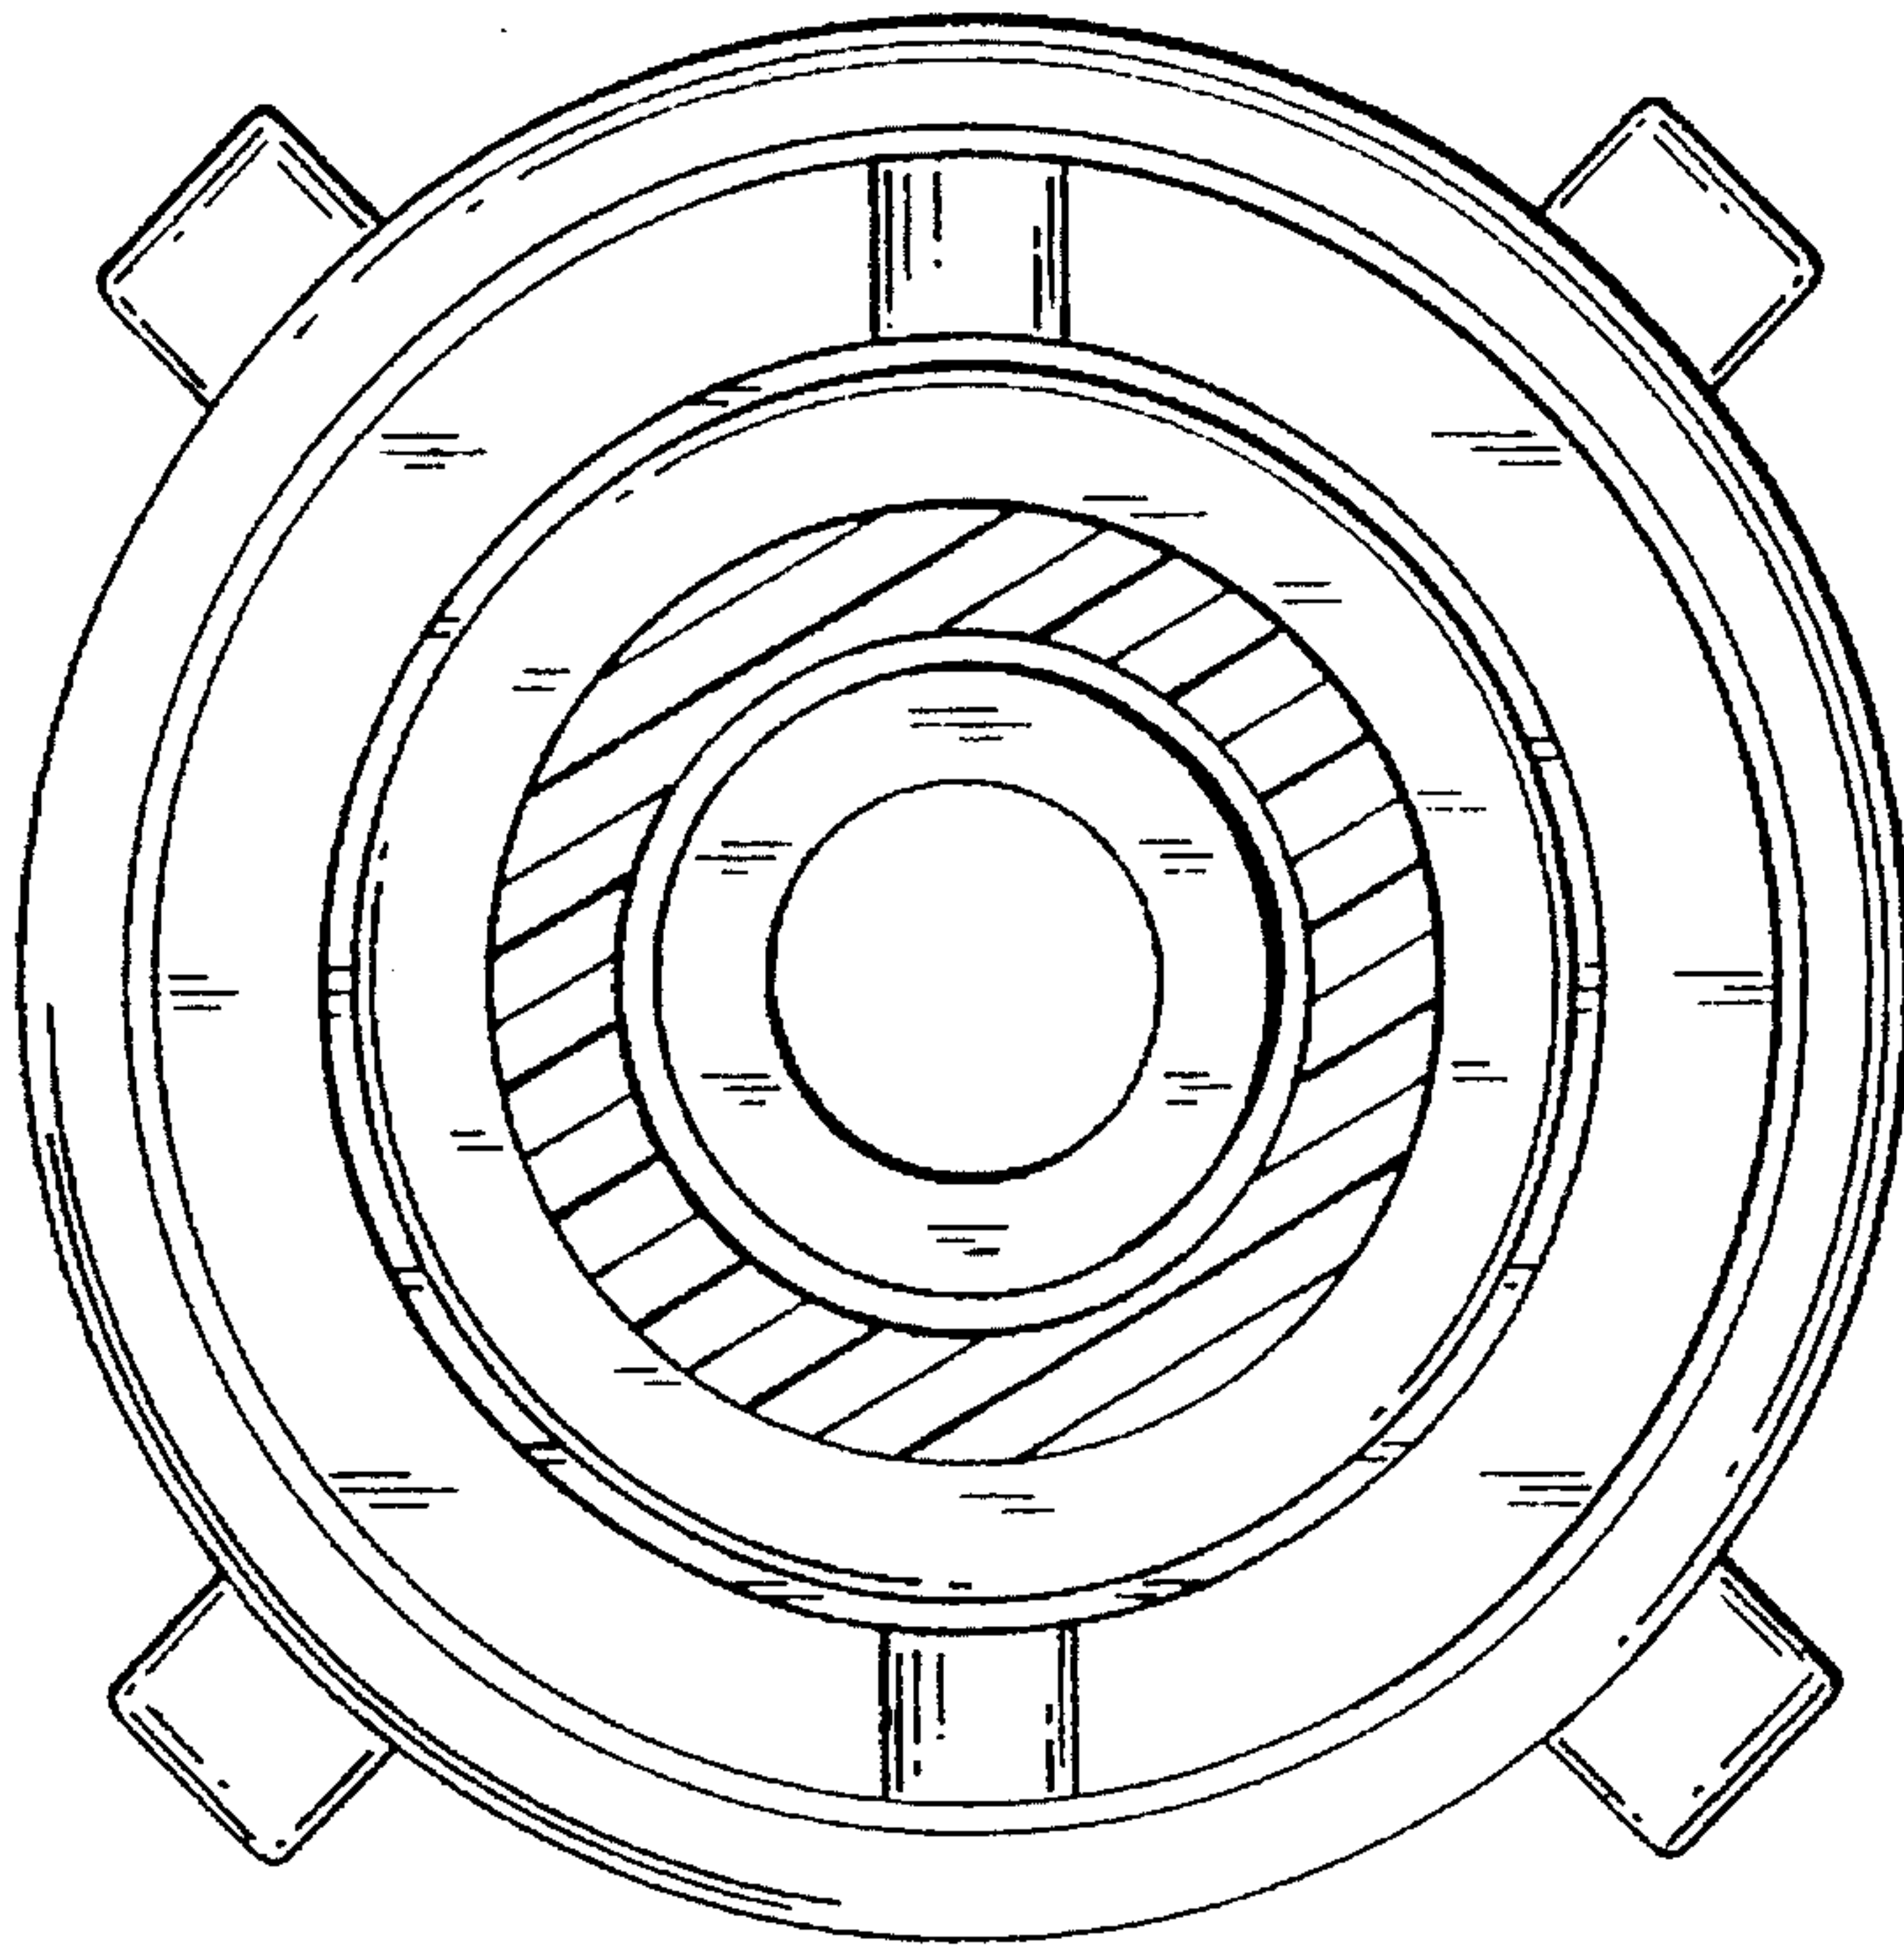

*FIG. 7*

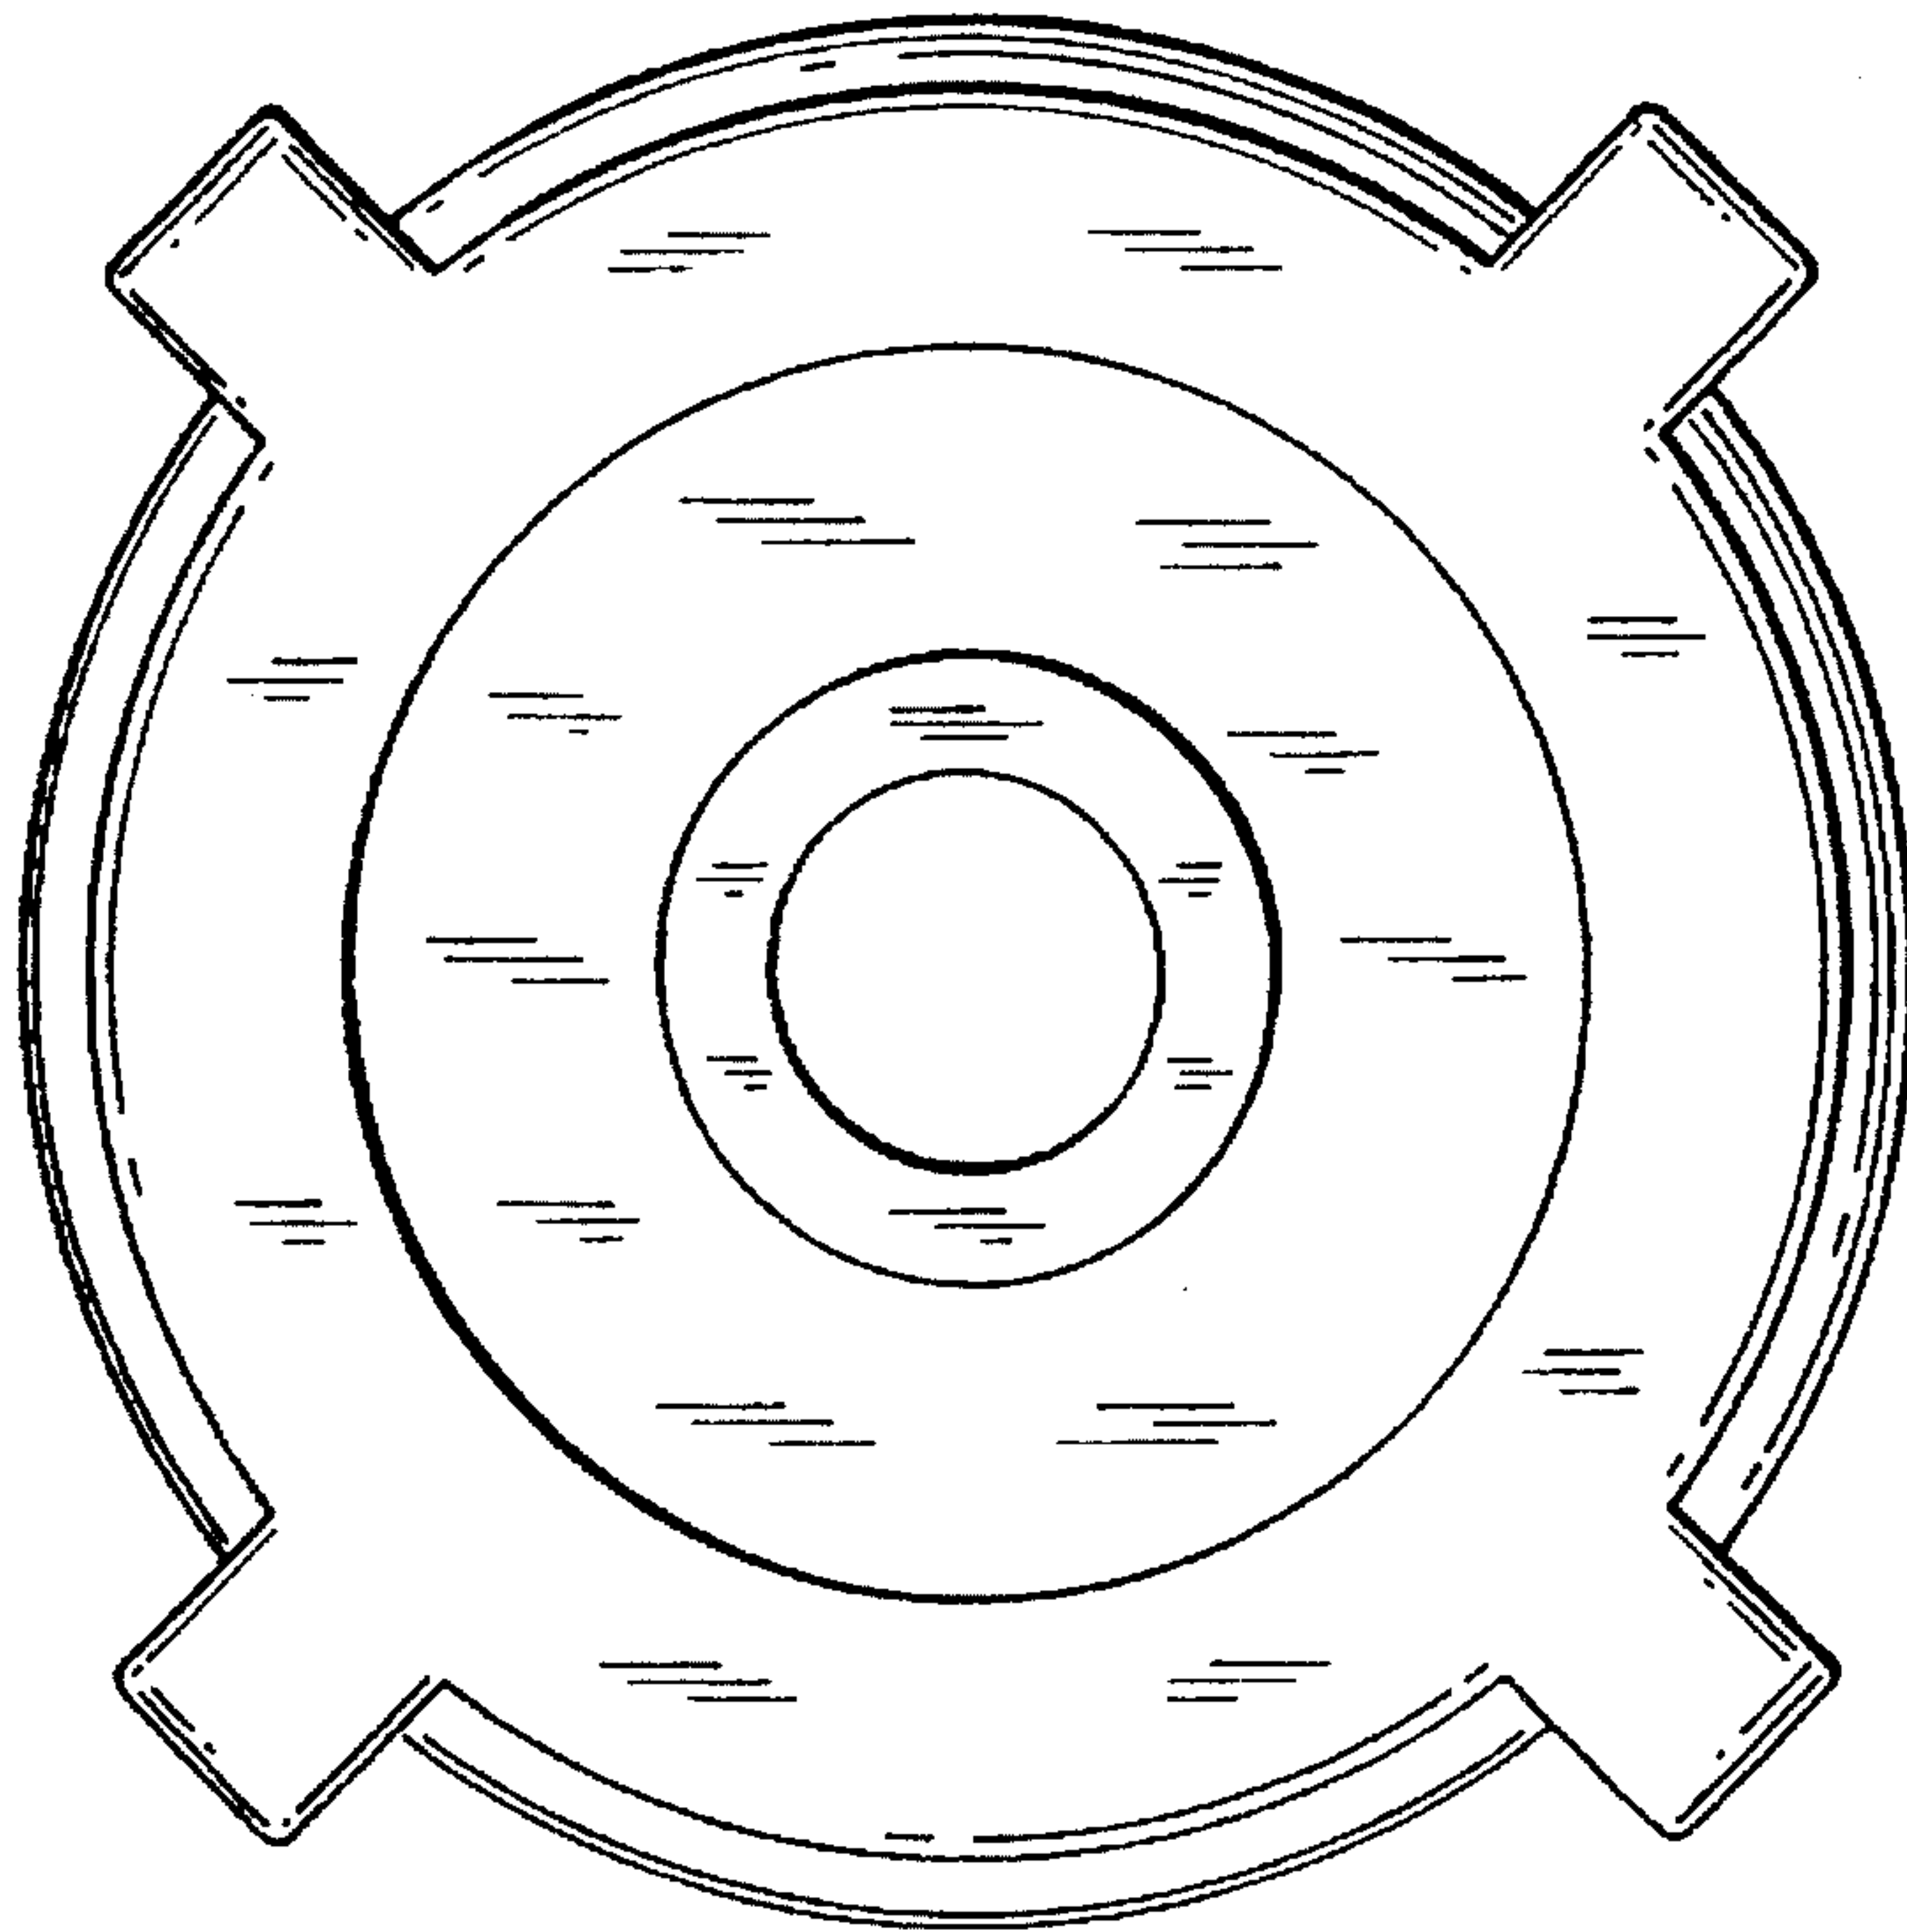

*FIG. 6*