



US00D366701S

United States Patent [19]

[11] Patent Number: **Des. 366,701**

Mazess et al.

[45] Date of Patent: ****Jan. 30, 1996**

[54] **MEDICAL IMAGING MACHINE**

Attorney, Agent, or Firm—Quarles & Brady

[75] Inventors: **Richard B. Mazess; Larry Fenske**, both of Madison, Wis.; **Bernard W. Siczek; Aldona A. Siczek**, both of Boulder, Colo.; **James G. Deluhery**, Madison; **Mike M. Tesic**, Verona, both of Wis.

[57] **CLAIM**

The ornamental design for a medical imaging machine, as shown and described.

[73] Assignee: **Lunar Corporation**, Madison, Wis.

[**] Term: **14 Years**

DESCRIPTION

[21] Appl. No.: **32,012**

[22] Filed: **Nov. 18, 1994**

FIG. 1 is a perspective view taken from the top front right side of a medical imaging machine showing our new design; FIG. 2 is a front elevational view of the medical imaging machine of FIG. 1;

FIG. 3 is a right side elevational view of the medical imaging machine of FIG. 1;

FIG. 4 is a top plan view of the medical imaging machine of FIG. 1;

FIG. 5 is a back elevational view of the medical imaging machine of FIG. 1;

FIG. 6 is a left side elevational view of the medical imaging machine of FIG. 1;

Related U.S. Application Data

[63] Continuation of Ser. No. 15,251, Nov. 12, 1993, abandoned.

[52] U.S. Cl. **D24/159**

[58] Field of Search D24/159, 158; 378/195-197, 181, 189, 208, 209, 16

FIG. 7 is a perspective view taken from the top front right side of a medical imaging table showing our new design;

FIG. 8 is a front elevational view of the medical imaging table of FIG. 7;

FIG. 9 is a right side elevational view of the medical imaging table of FIG. 7;

FIG. 10 is a top plan view of the medical imaging table of FIG. 7;

FIG. 11 is a back elevational view of the medical imaging table of FIG. 7;

FIG. 12 is a left side elevational view of the medical imaging table of FIG. 7;

FIG. 13 is a perspective view taken from the top front right side of a medical imaging C-arm and detector showing our new design;

FIG. 14 is a front elevational view of the medical imaging C-arm and detector of FIG. 13;

FIG. 15 is a right side elevational view of the medical imaging C-arm and detector of FIG. 13;

FIG. 16 is a top plan view of the medical imaging C-arm and detector of FIG. 13;

FIG. 17 is a back elevational view of the medical imaging C-arm and detector of FIG. 13; and,

FIG. 18 is a left side elevational view of the medical imaging C-arm and detector of FIG. 13.

[56] References Cited

U.S. PATENT DOCUMENTS

D. 105,507 8/1937 Werner D24/159
D. 161,717 1/1951 Stava et al. D24/159
2,818,510 12/1957 Verse 250/91

(List continued on next page.)

FOREIGN PATENT DOCUMENTS

0122849 10/1984 European Pat. Off. .
0333256 9/1989 European Pat. Off. .
3542333 11/1985 Germany .
56-155937 2/1981 Japan .

OTHER PUBLICATIONS


“Development of Dichromography Techniques” by Bertil Jacobson, M.D., admitted prior art. (1968).

“Dedicated Interventional X-Ray System With Tilt Table and Integrated C-Arm”, admitted prior art.

Integris 12000 for Interventional Radiology, admitted prior art.

Primary Examiner—Stella Reid

1 Claim, 10 Drawing Sheets

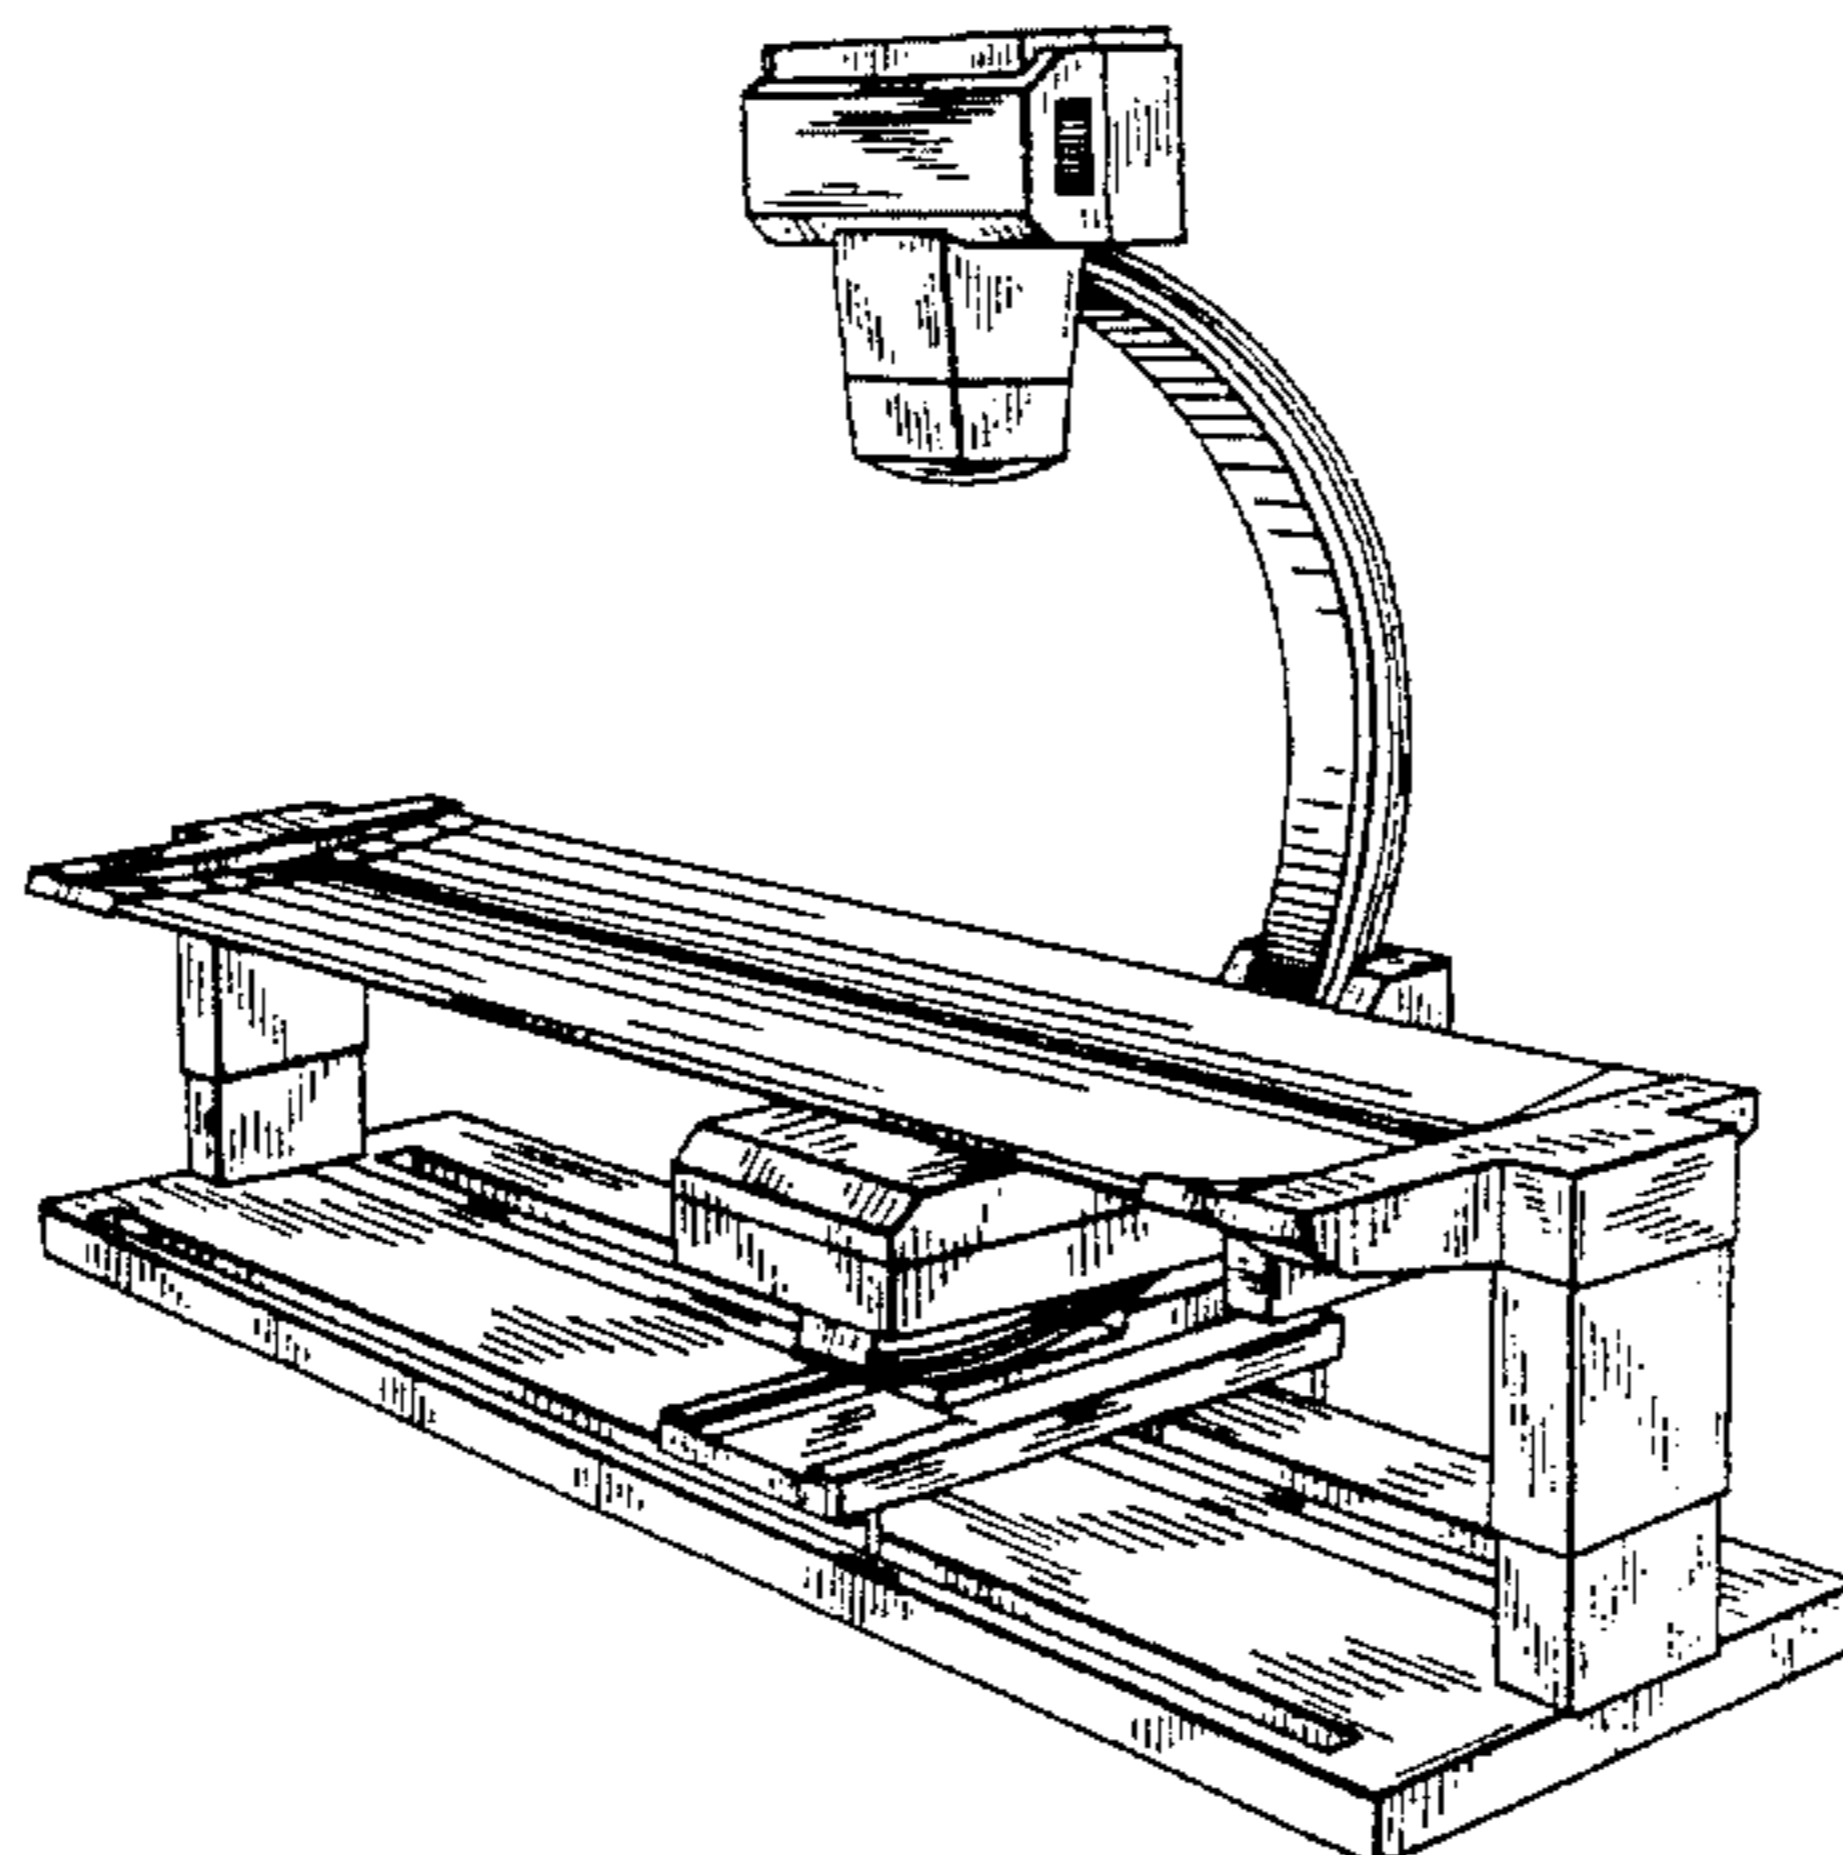

U.S. PATENT DOCUMENTS

3,281,598	10/1966	Hollstein	250/57	4,412,346	10/1983	Takenouti et al.	378/181
3,617,749	11/1971	Masslot	250/92	4,501,011	2/1985	Hauck et al.	378/196
3,670,163	6/1972	Lajus	250/50	4,541,293	9/1985	Caugant et al.	74/89.18
3,892,967	7/1975	Grady et al.	250/447	4,635,284	1/1987	Christiansen	378/197
3,967,126	6/1976	Otto, Jr.	378/195 X	4,653,083	3/1987	Rossi	378/196
4,024,403	5/1977	Bernstein et al.	250/445	4,716,581	12/1987	Barud	378/198
4,082,955	4/1978	Sell	378/196 X	4,756,016	7/1988	Grady et al.	378/197
4,150,297	4/1979	Borggren	250/490	4,987,585	1/1991	Kidd et al.	378/197
4,298,801	11/1981	Heitman	250/447	5,014,292	5/1991	Siczek et al.	378/196
4,358,856	11/1982	Stivender et al.	378/167	5,050,202	9/1991	Yanome	378/195 X
4,363,128	12/1982	Grady et al.	378/181	5,077,780	12/1991	Lee, Jr.	378/208 X

FIG. 1

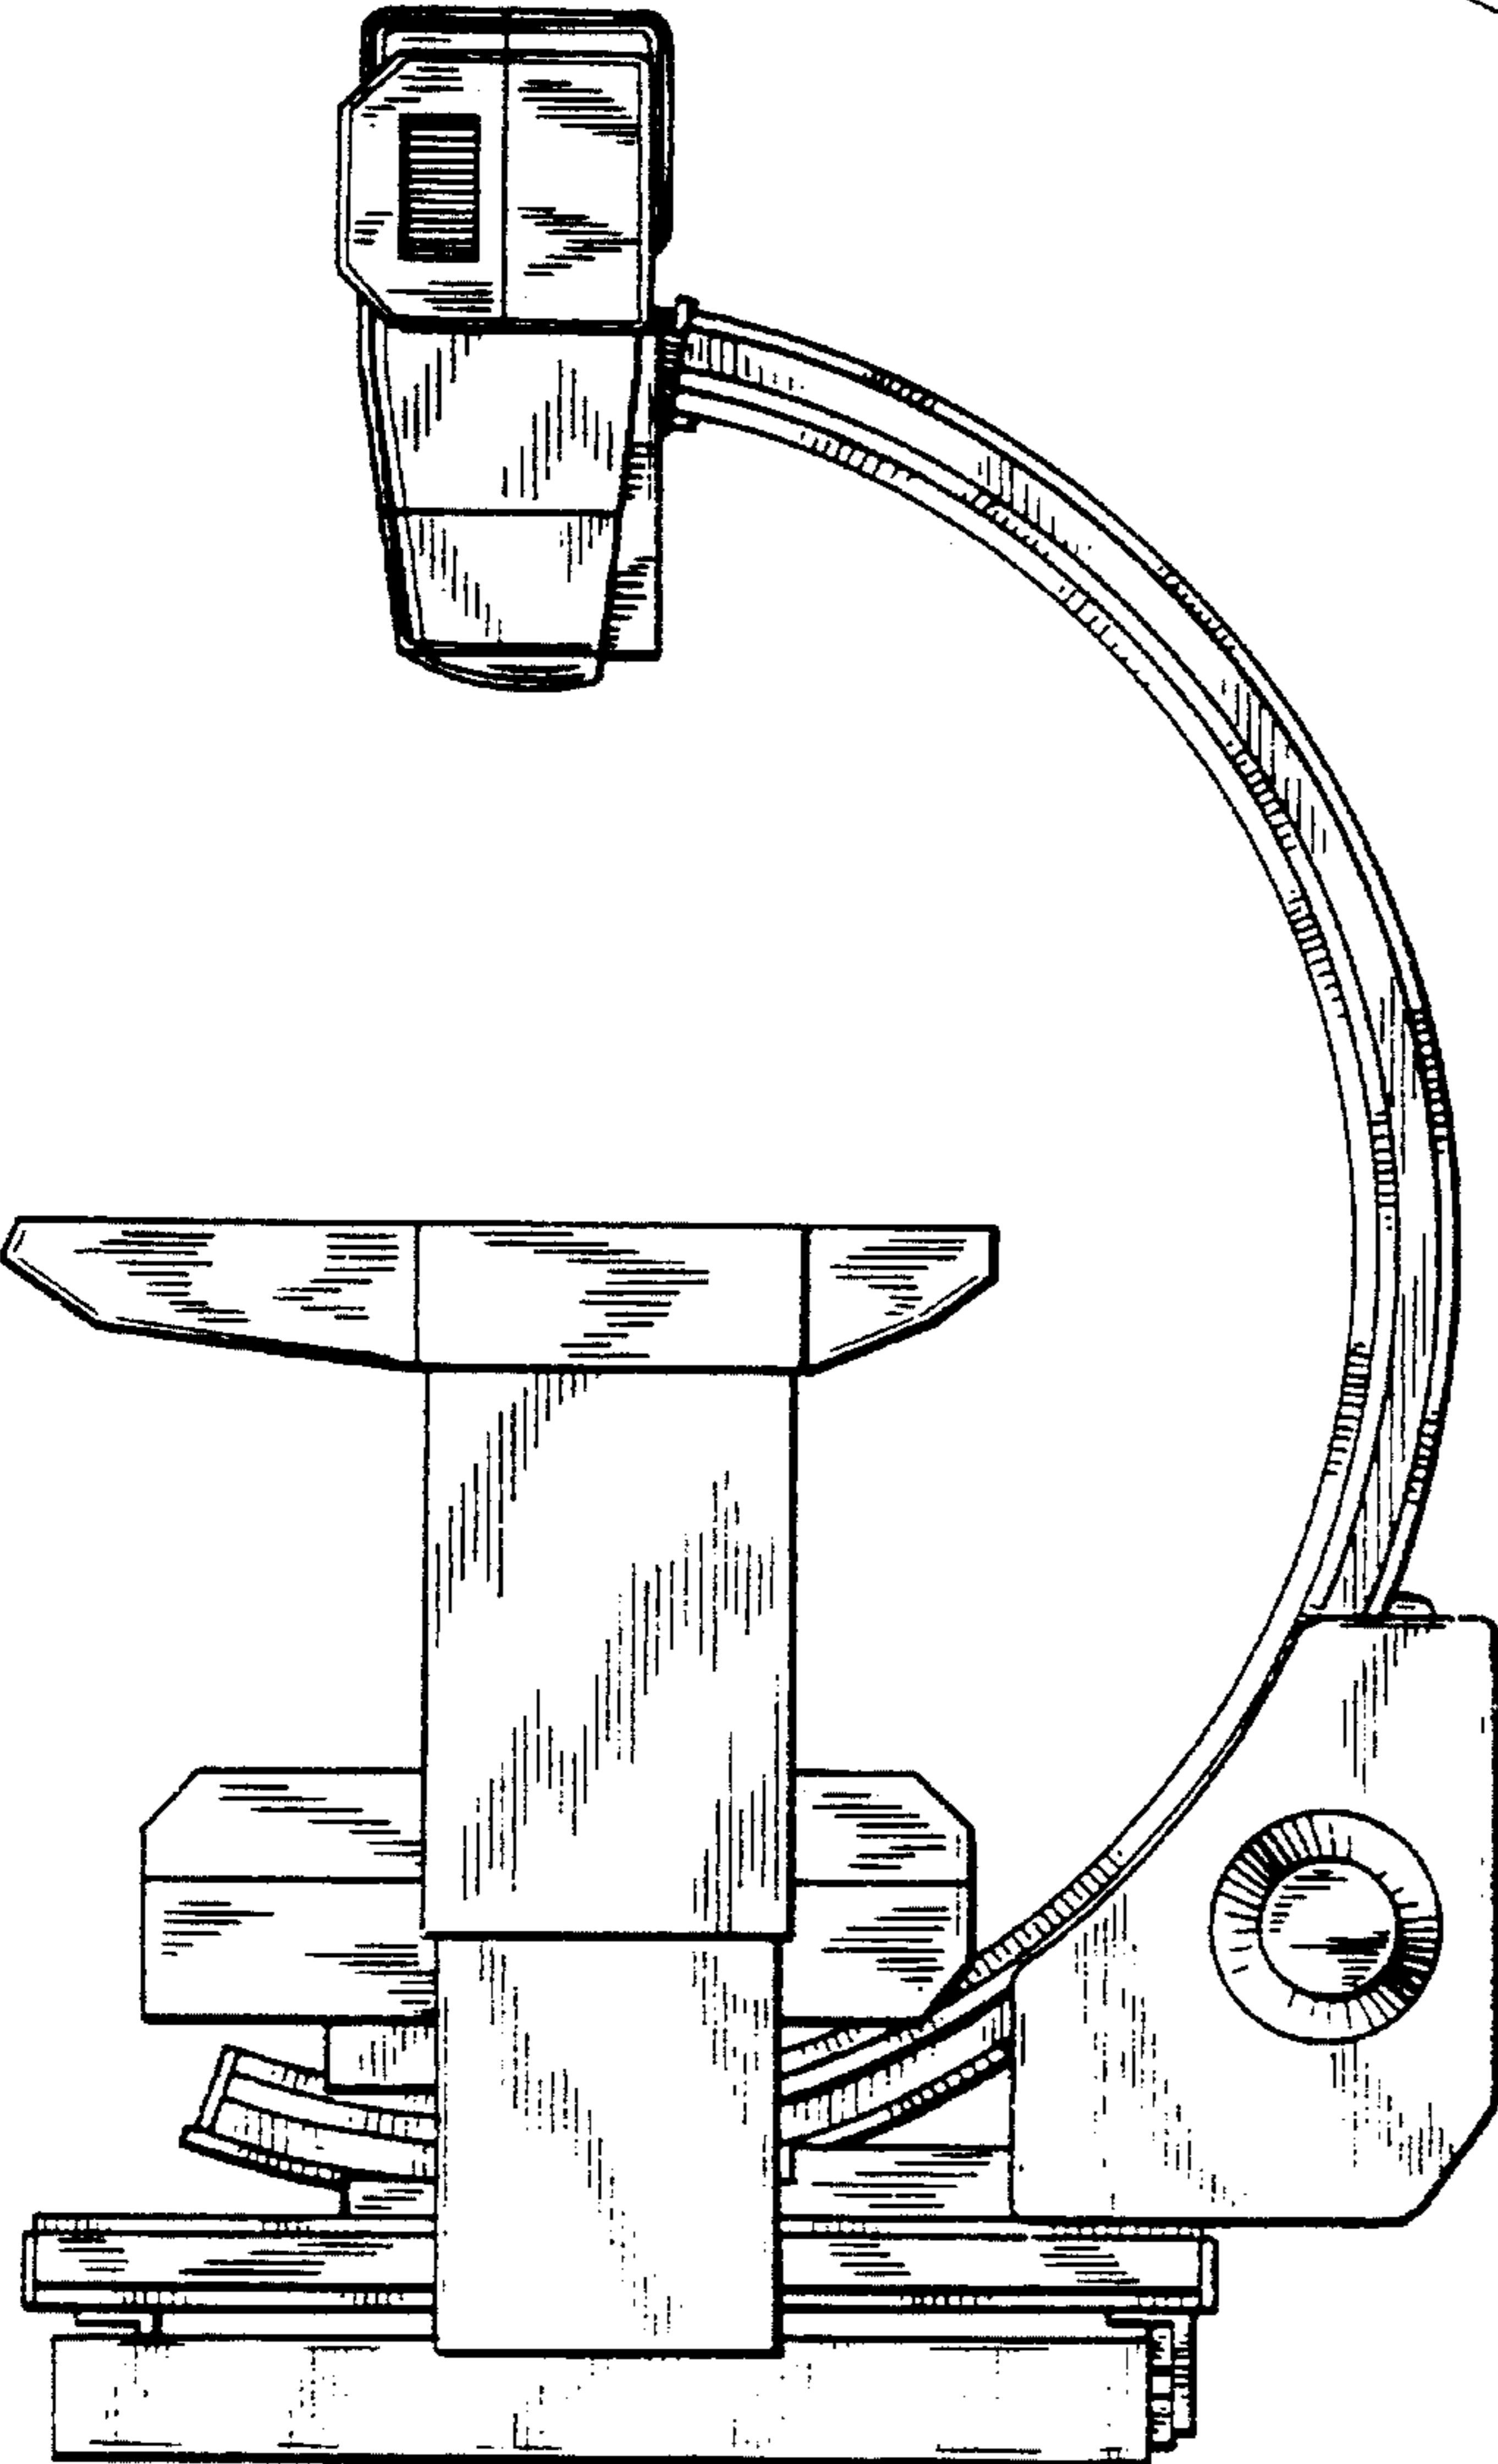
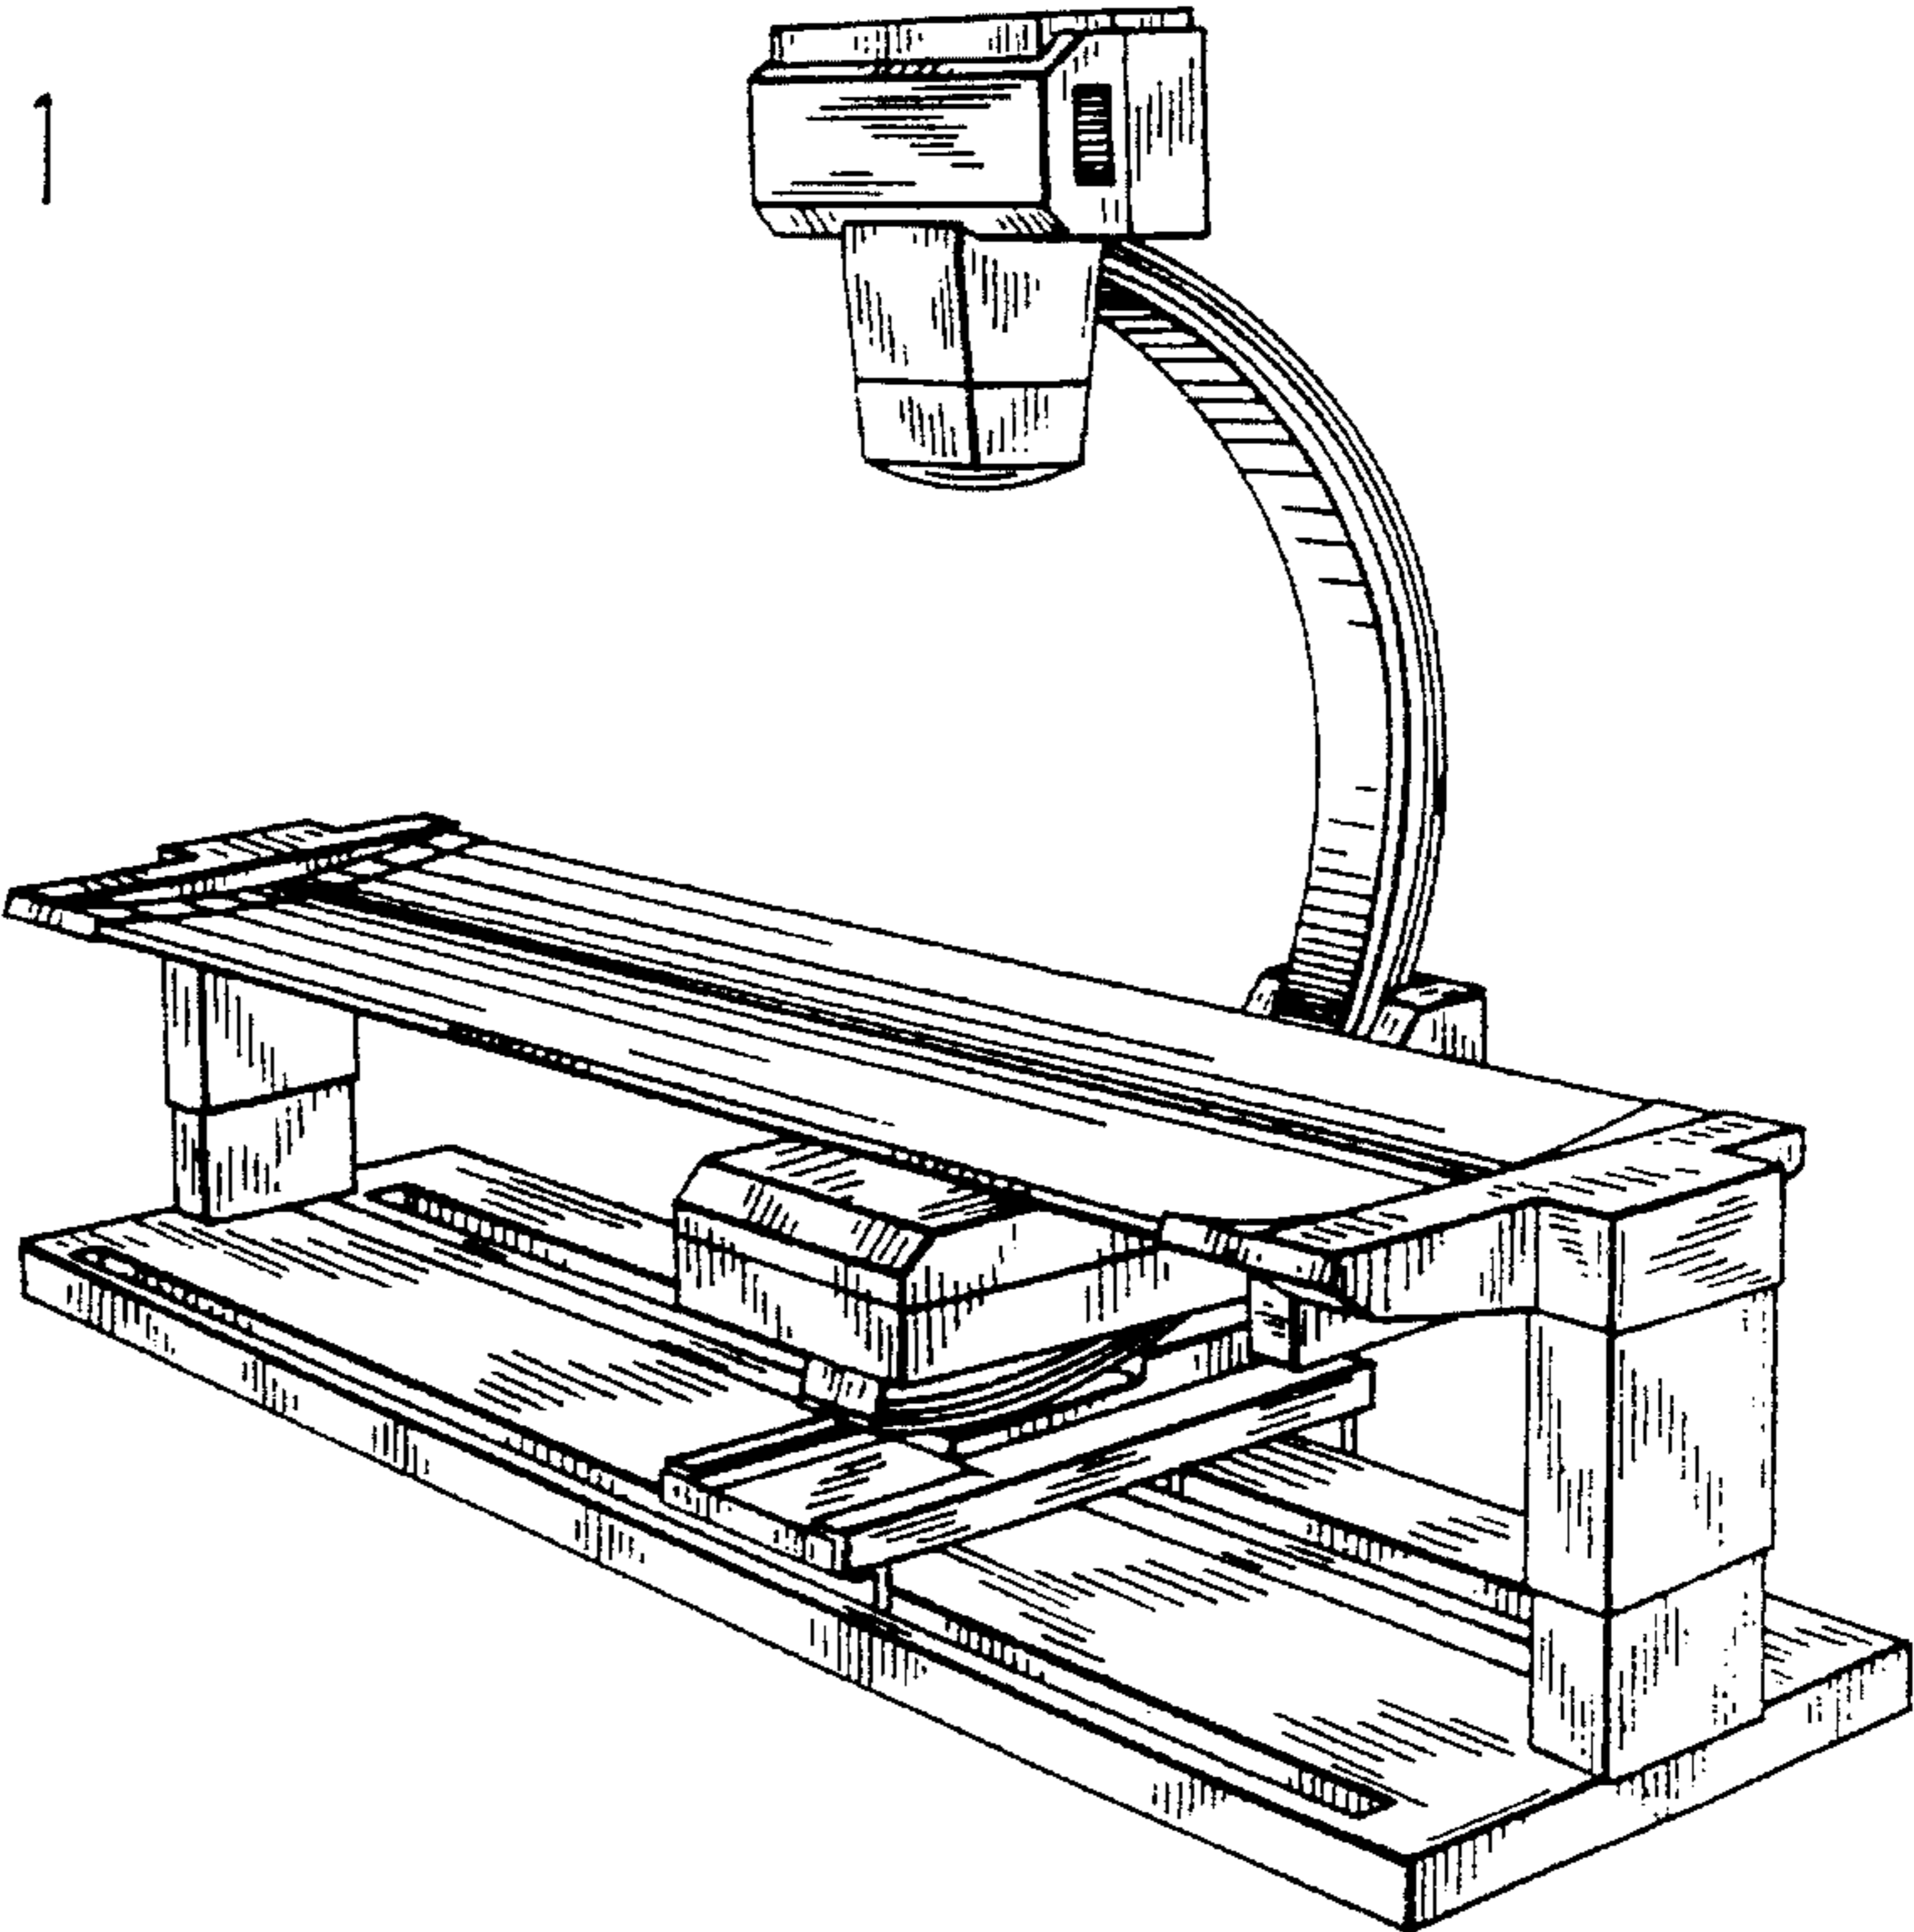


FIG. 3

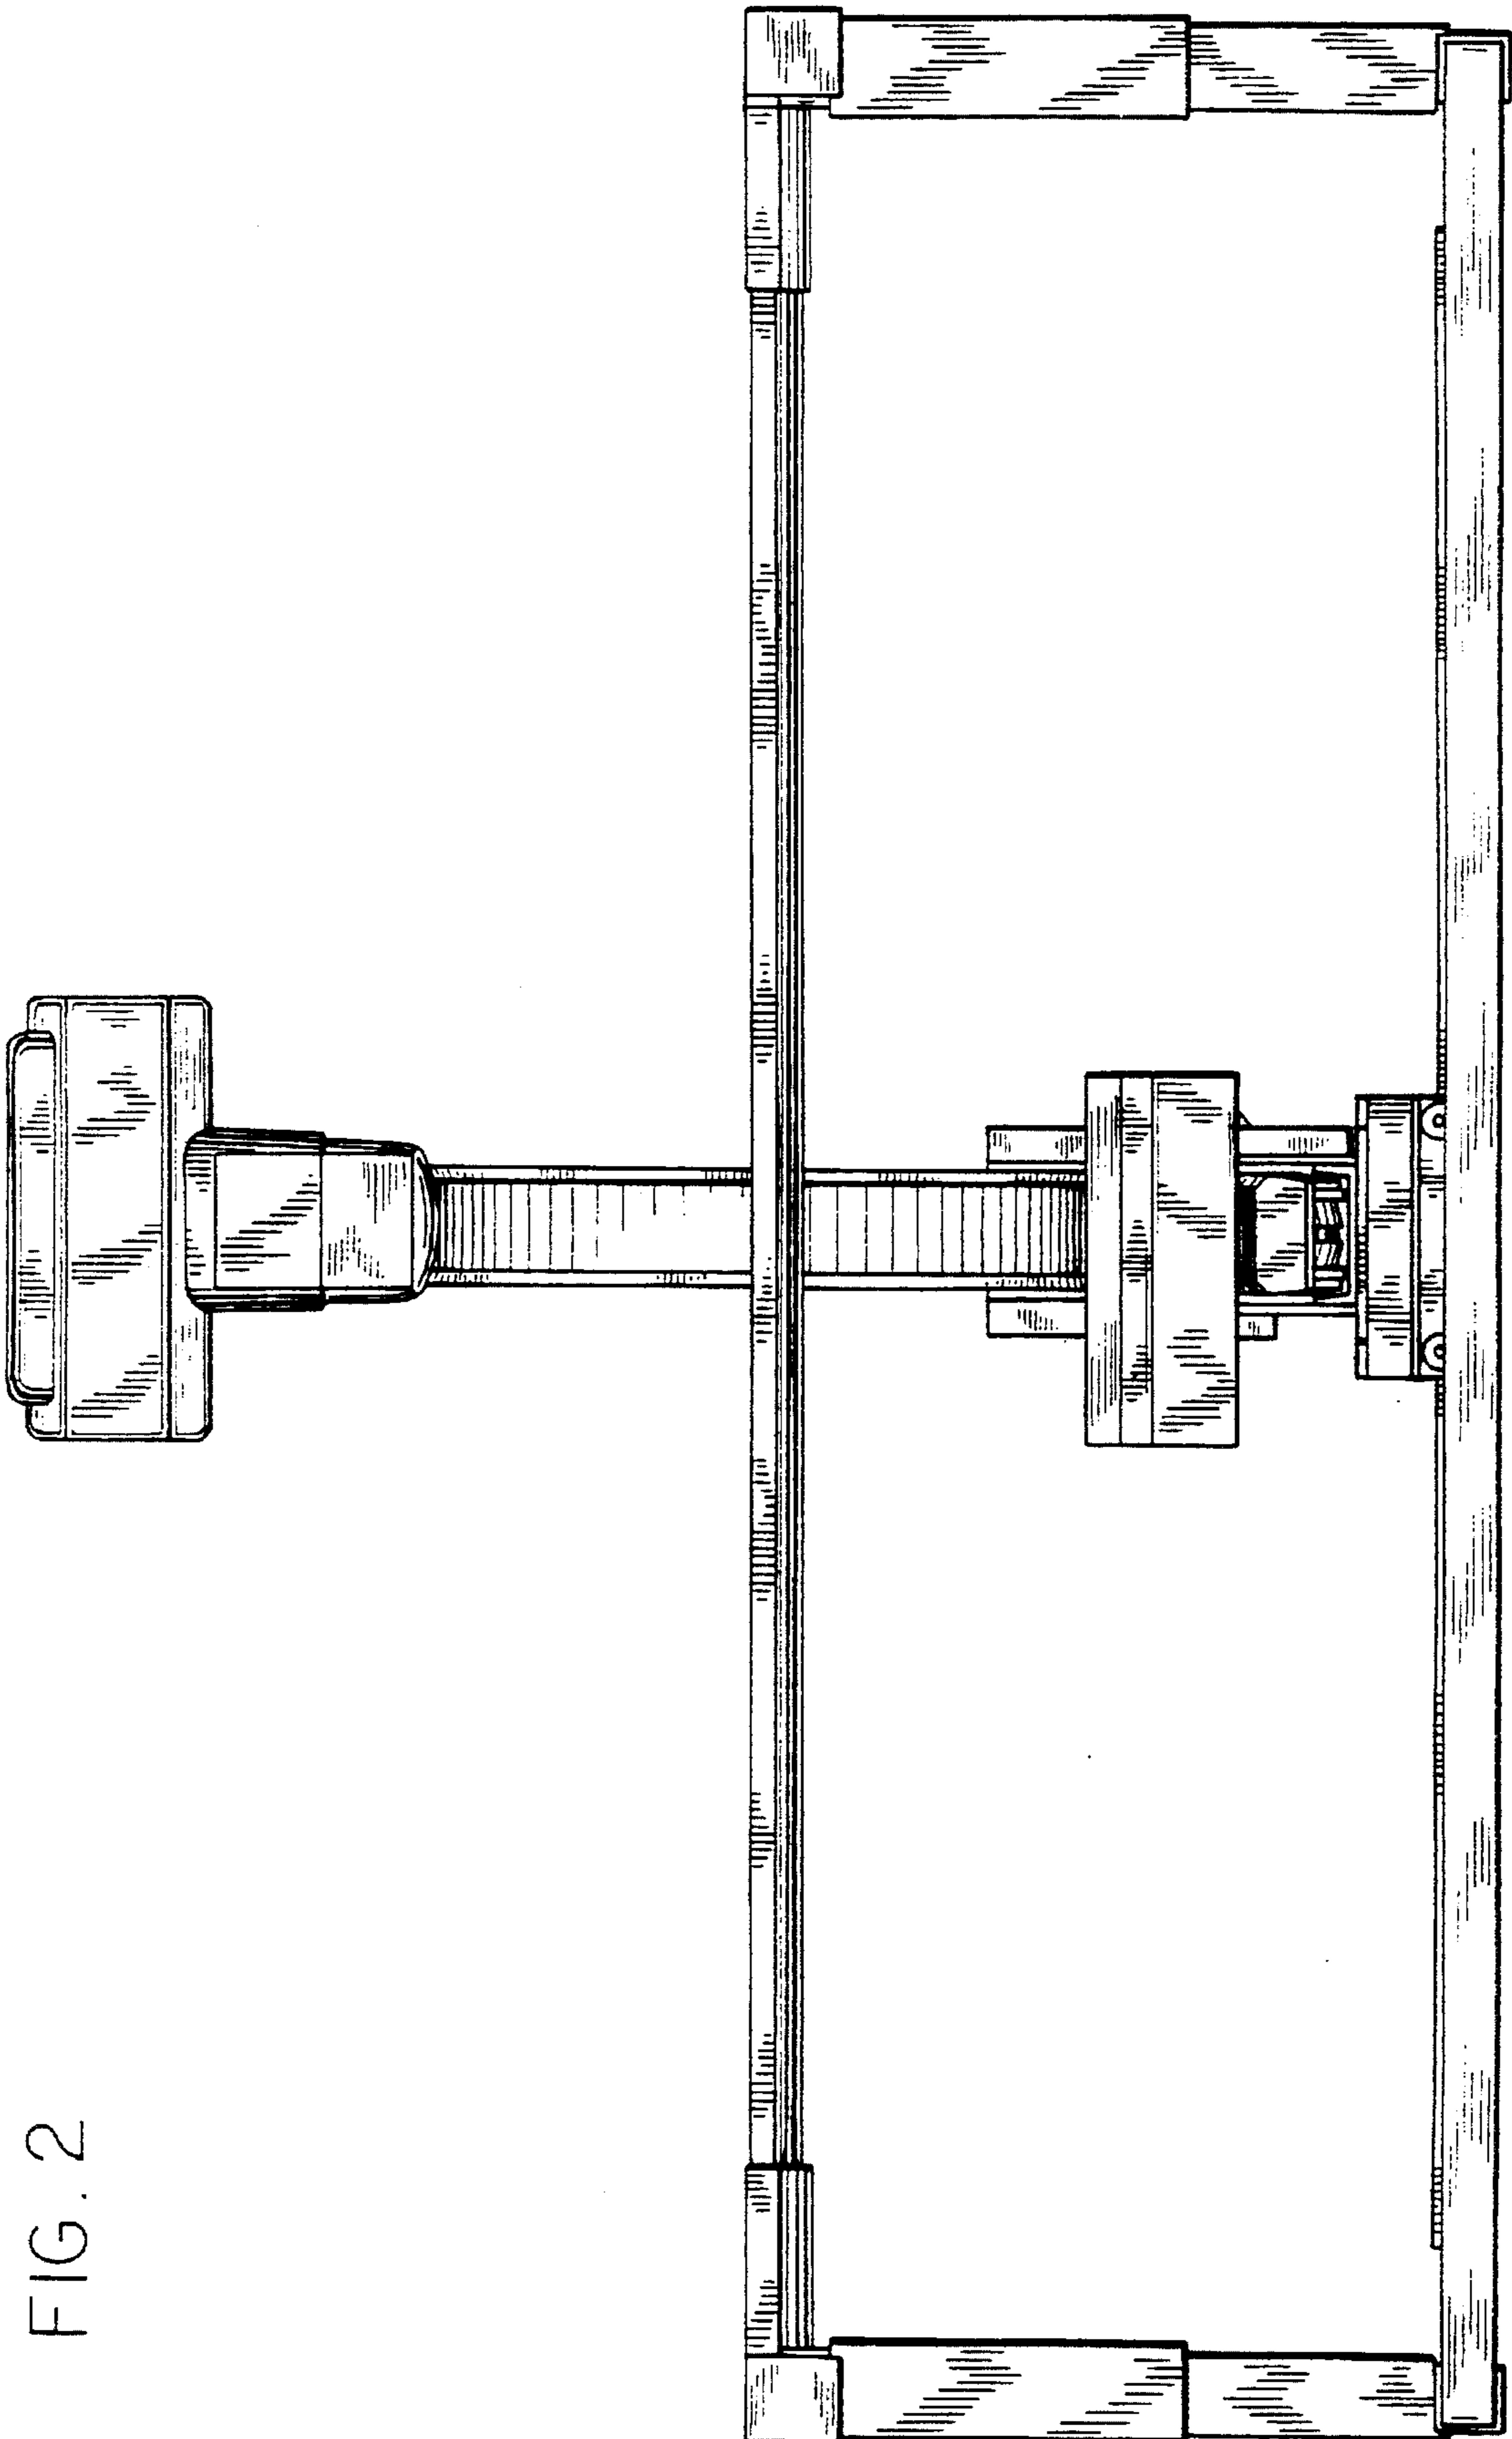


FIG. 2

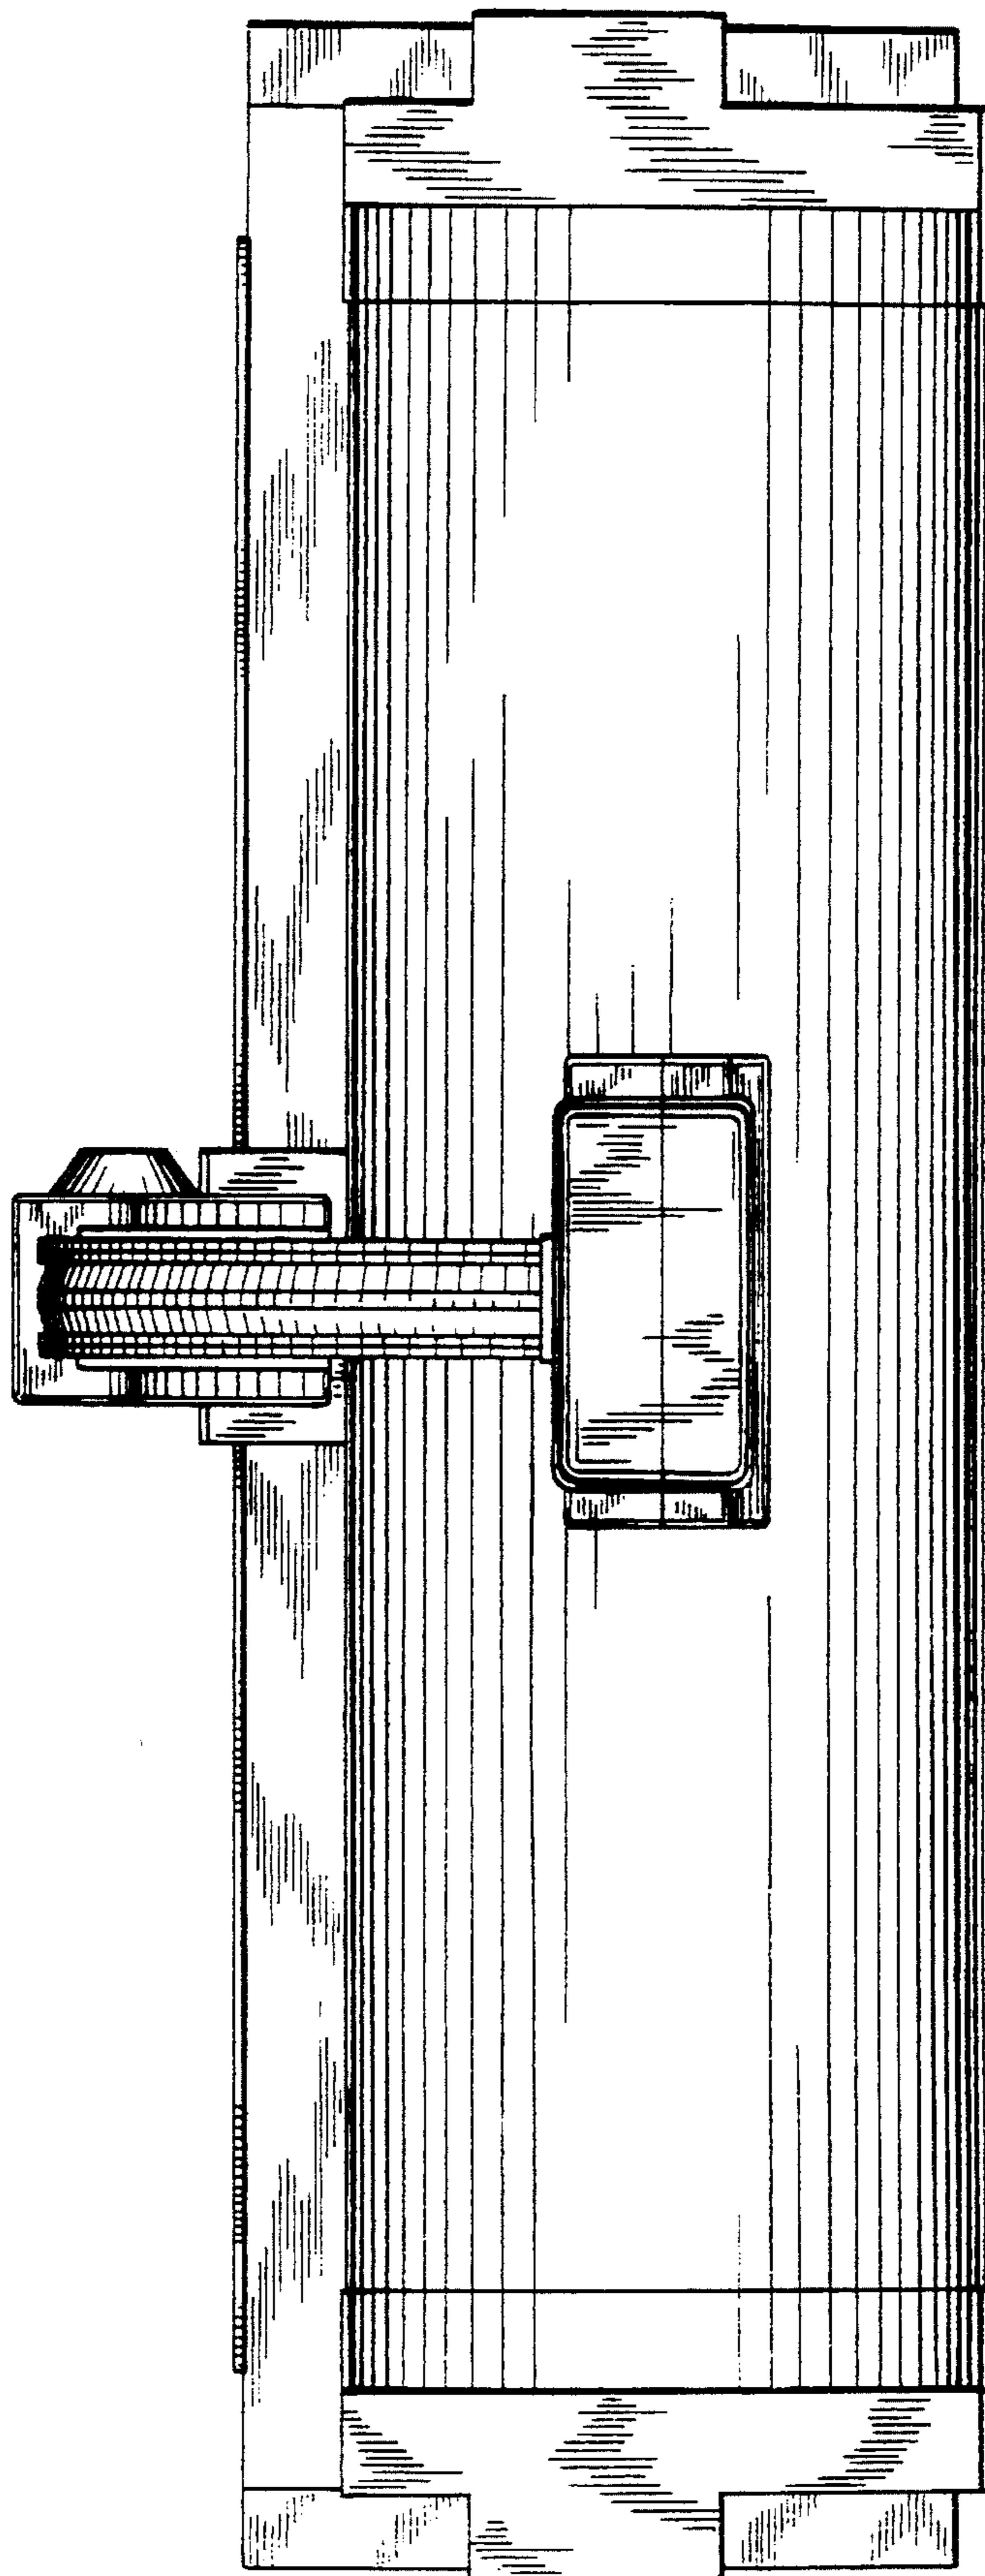


FIG. 4

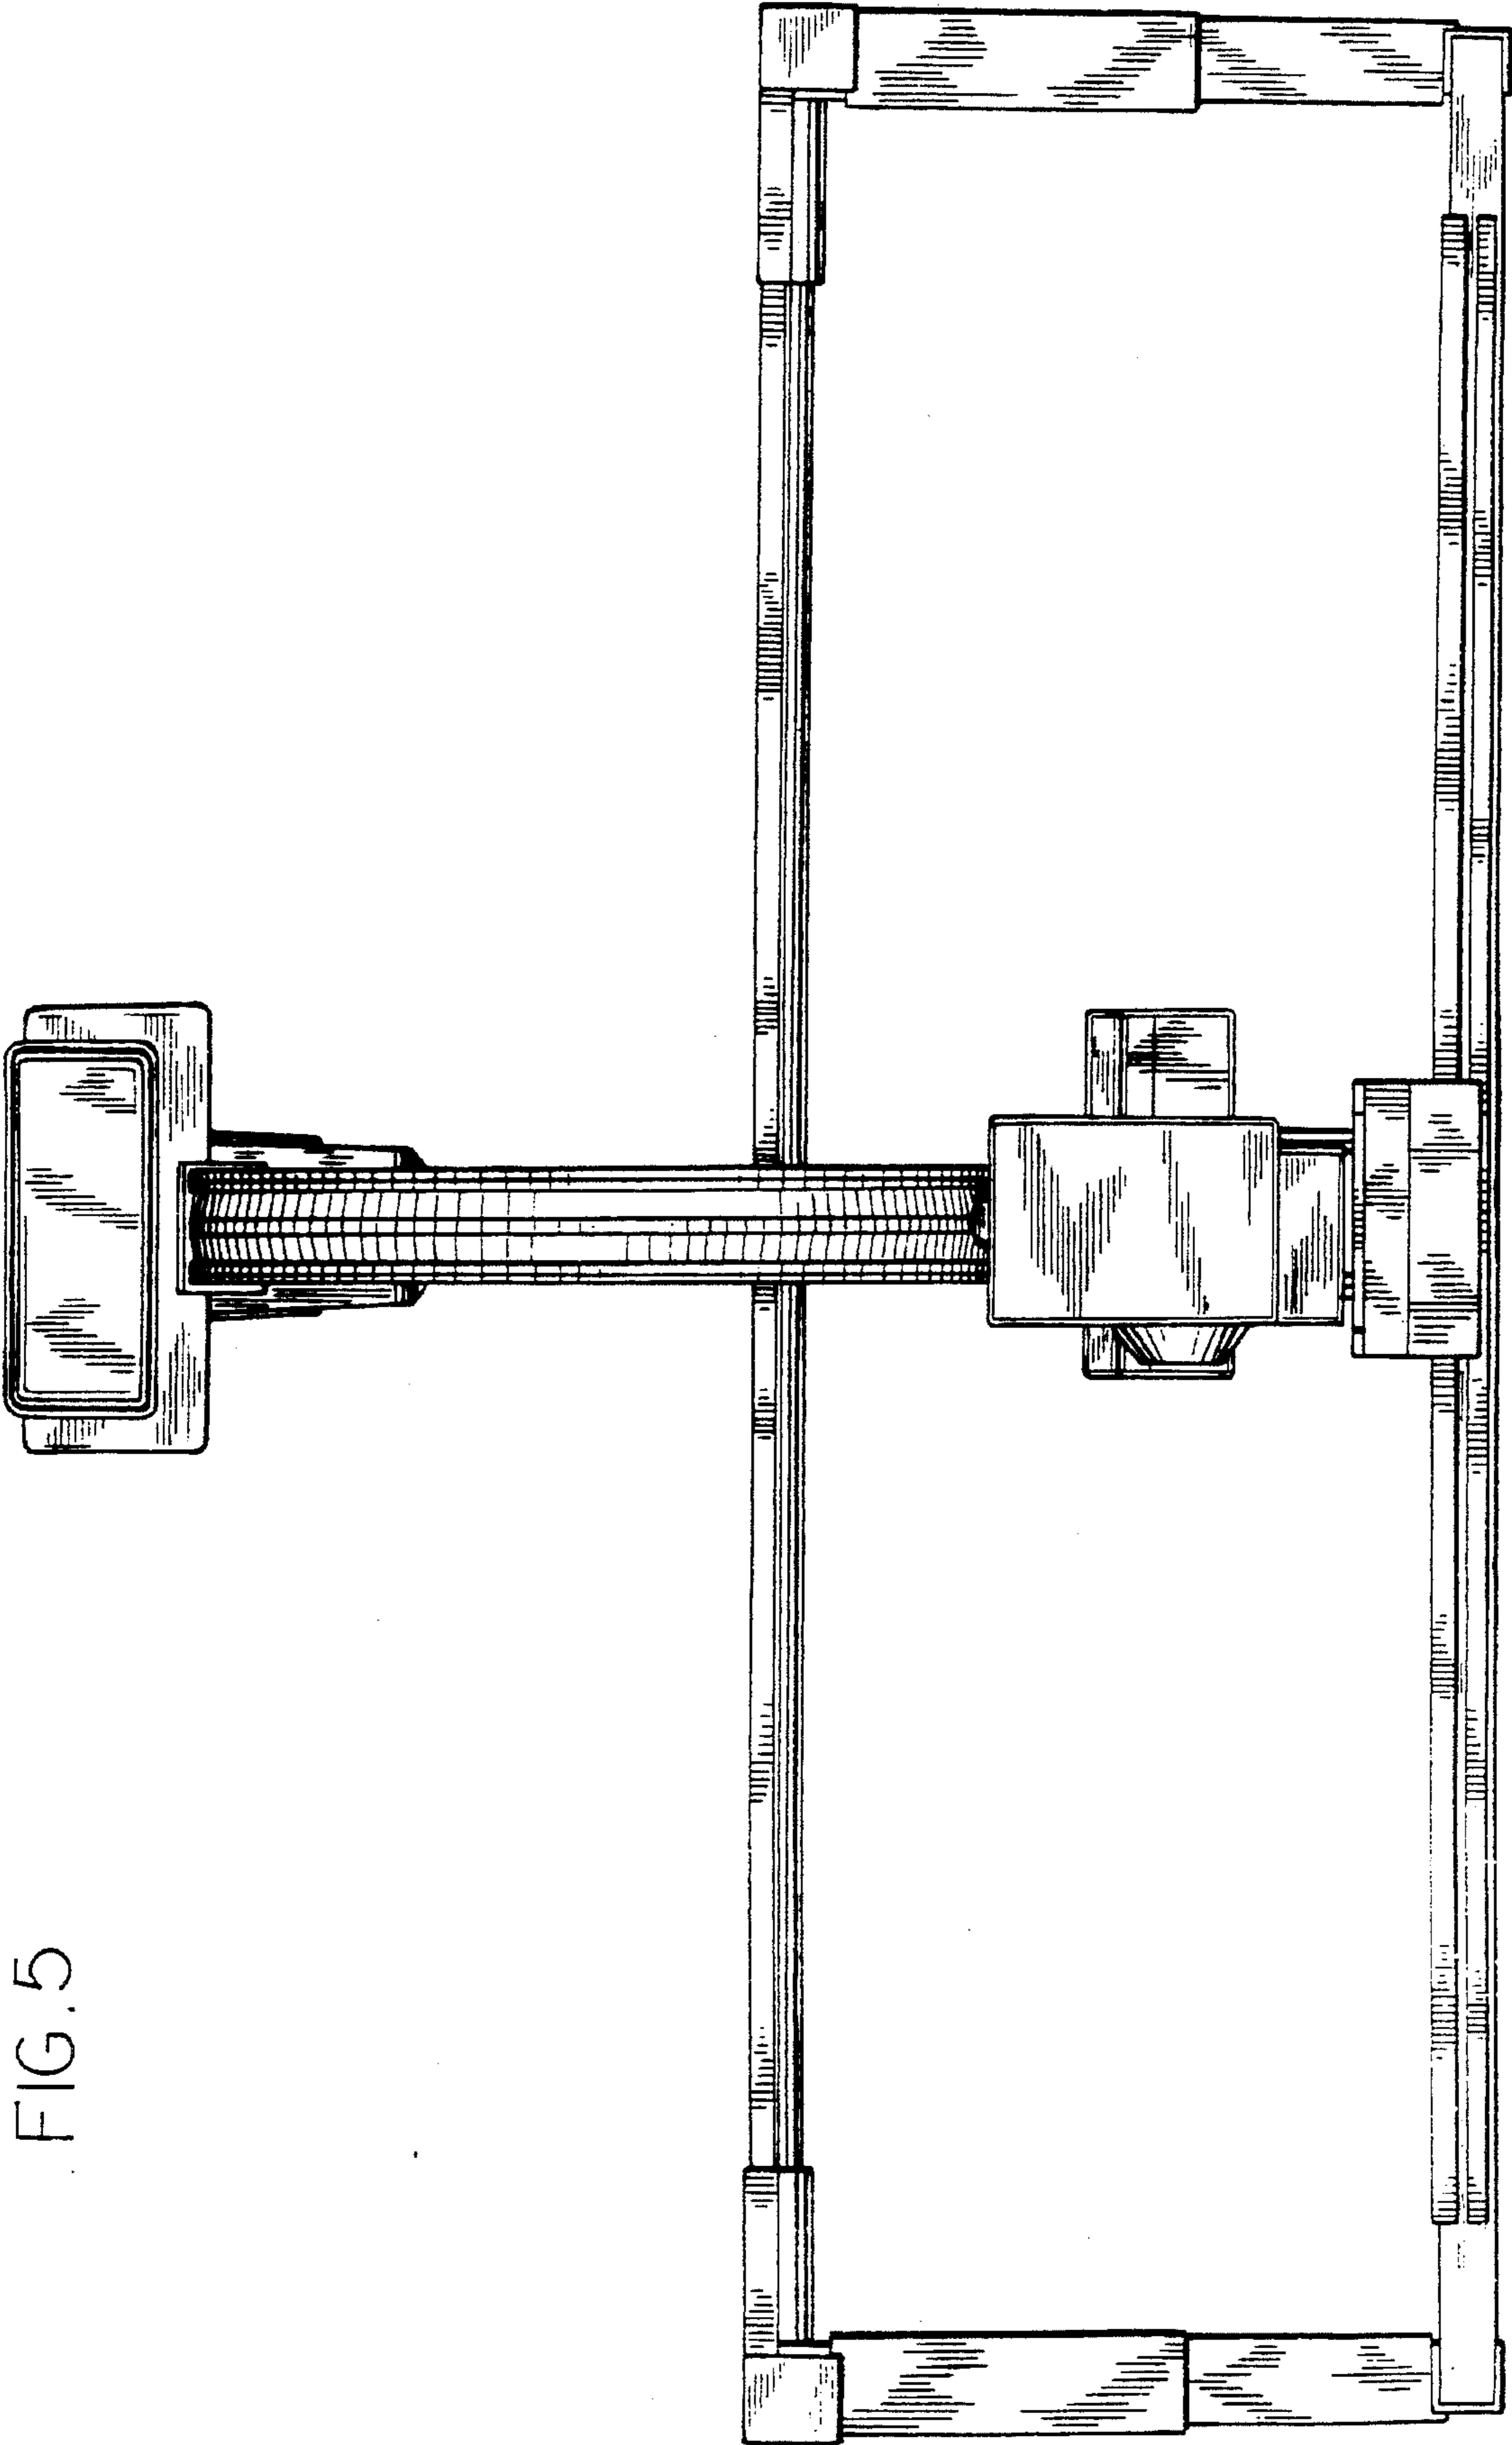


FIG. 5

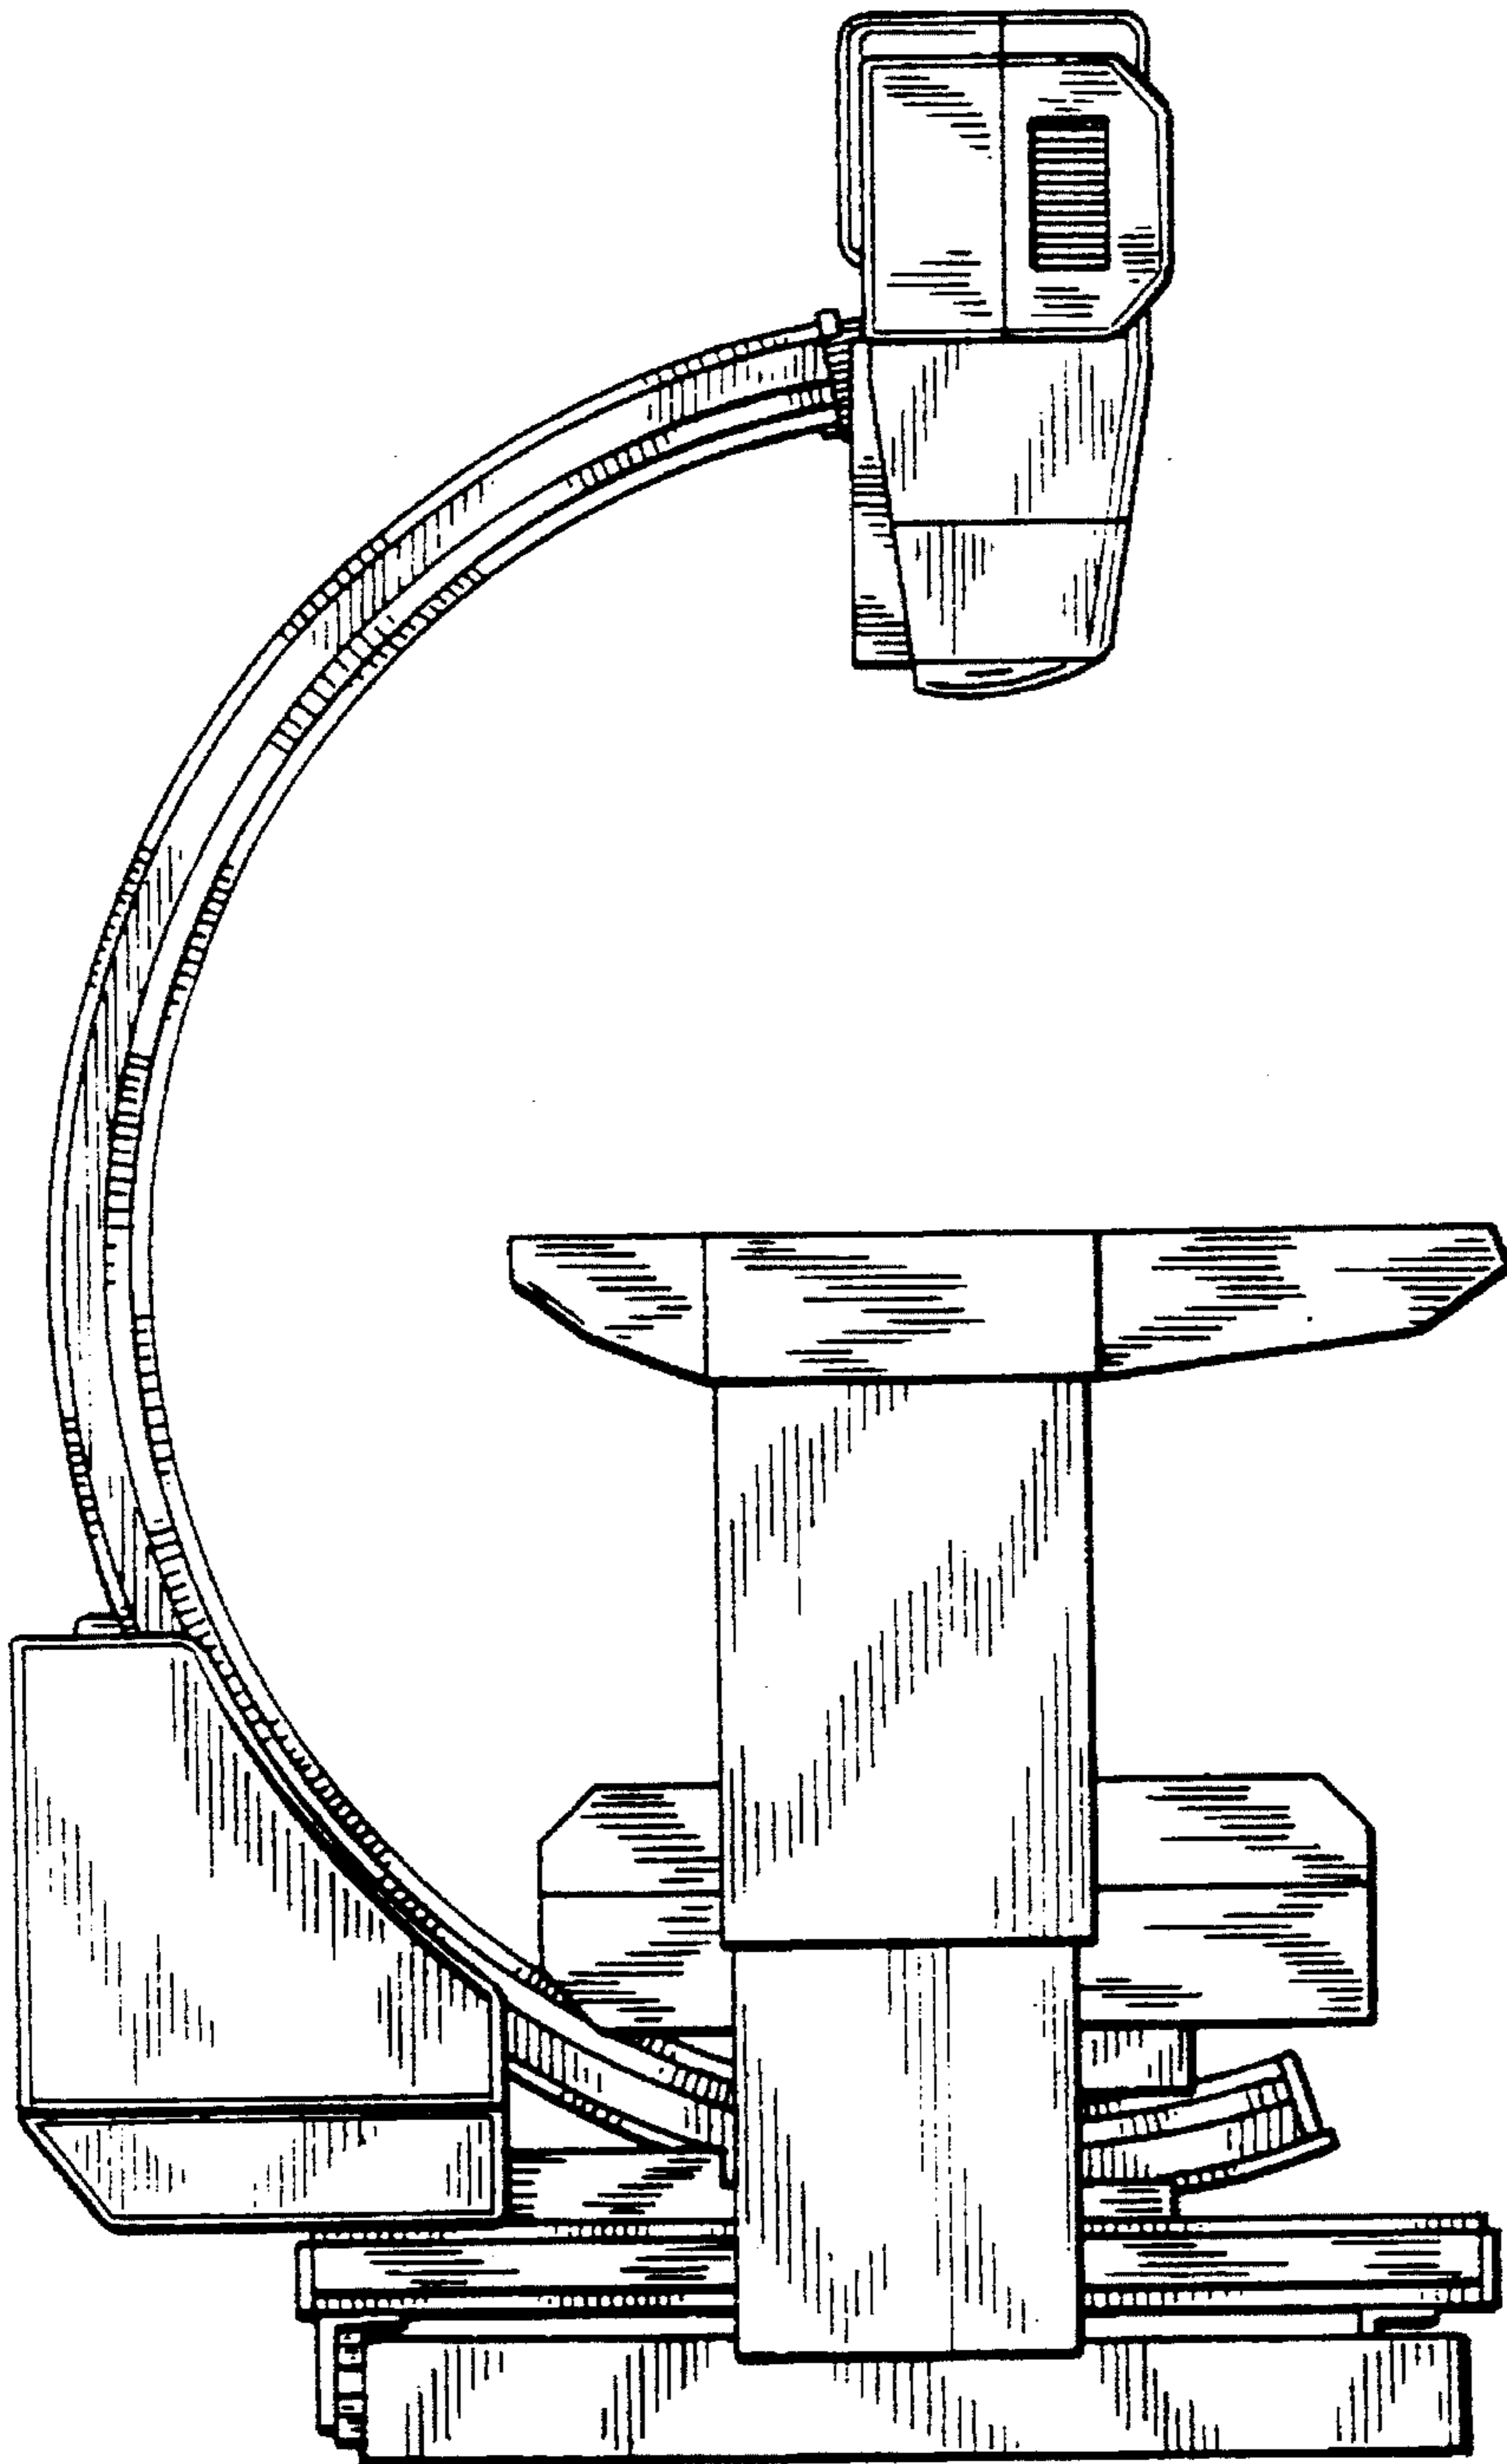


FIG. 6

FIG. 7

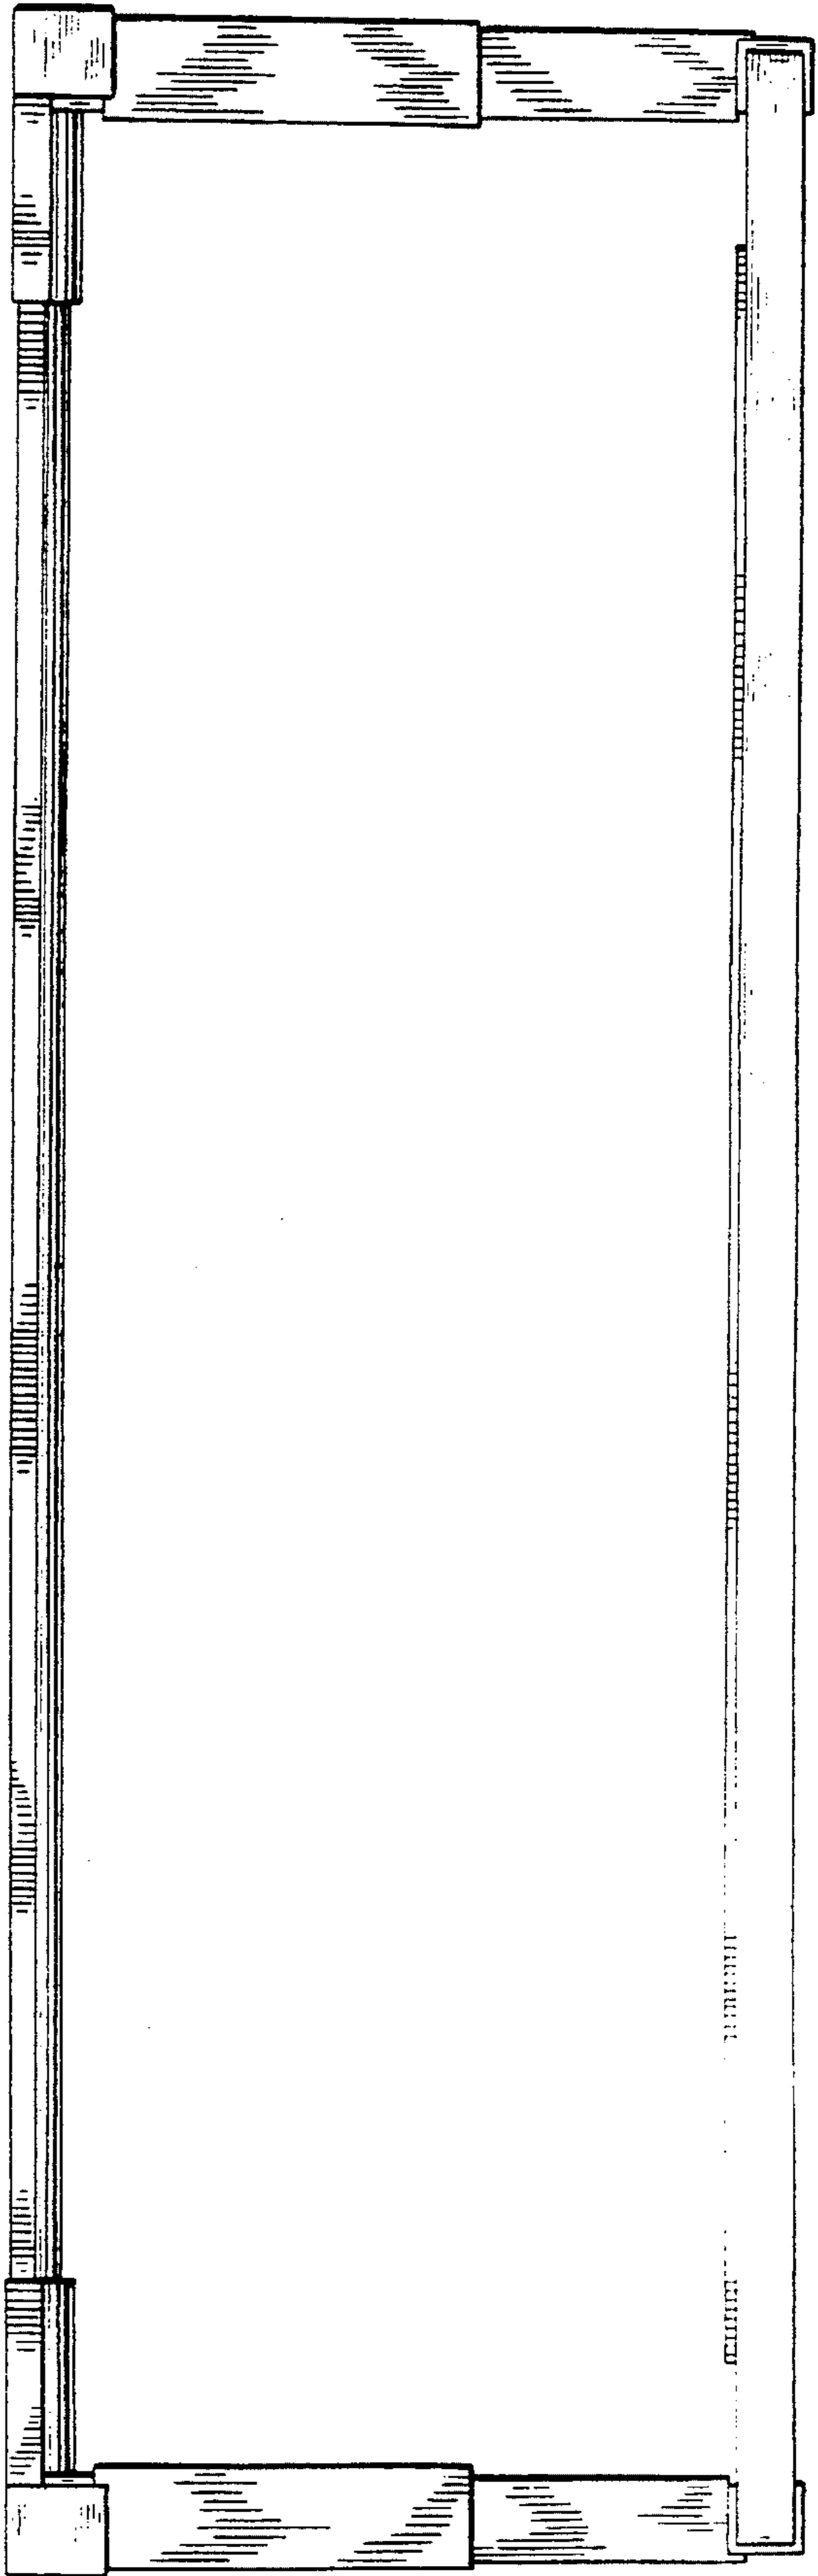
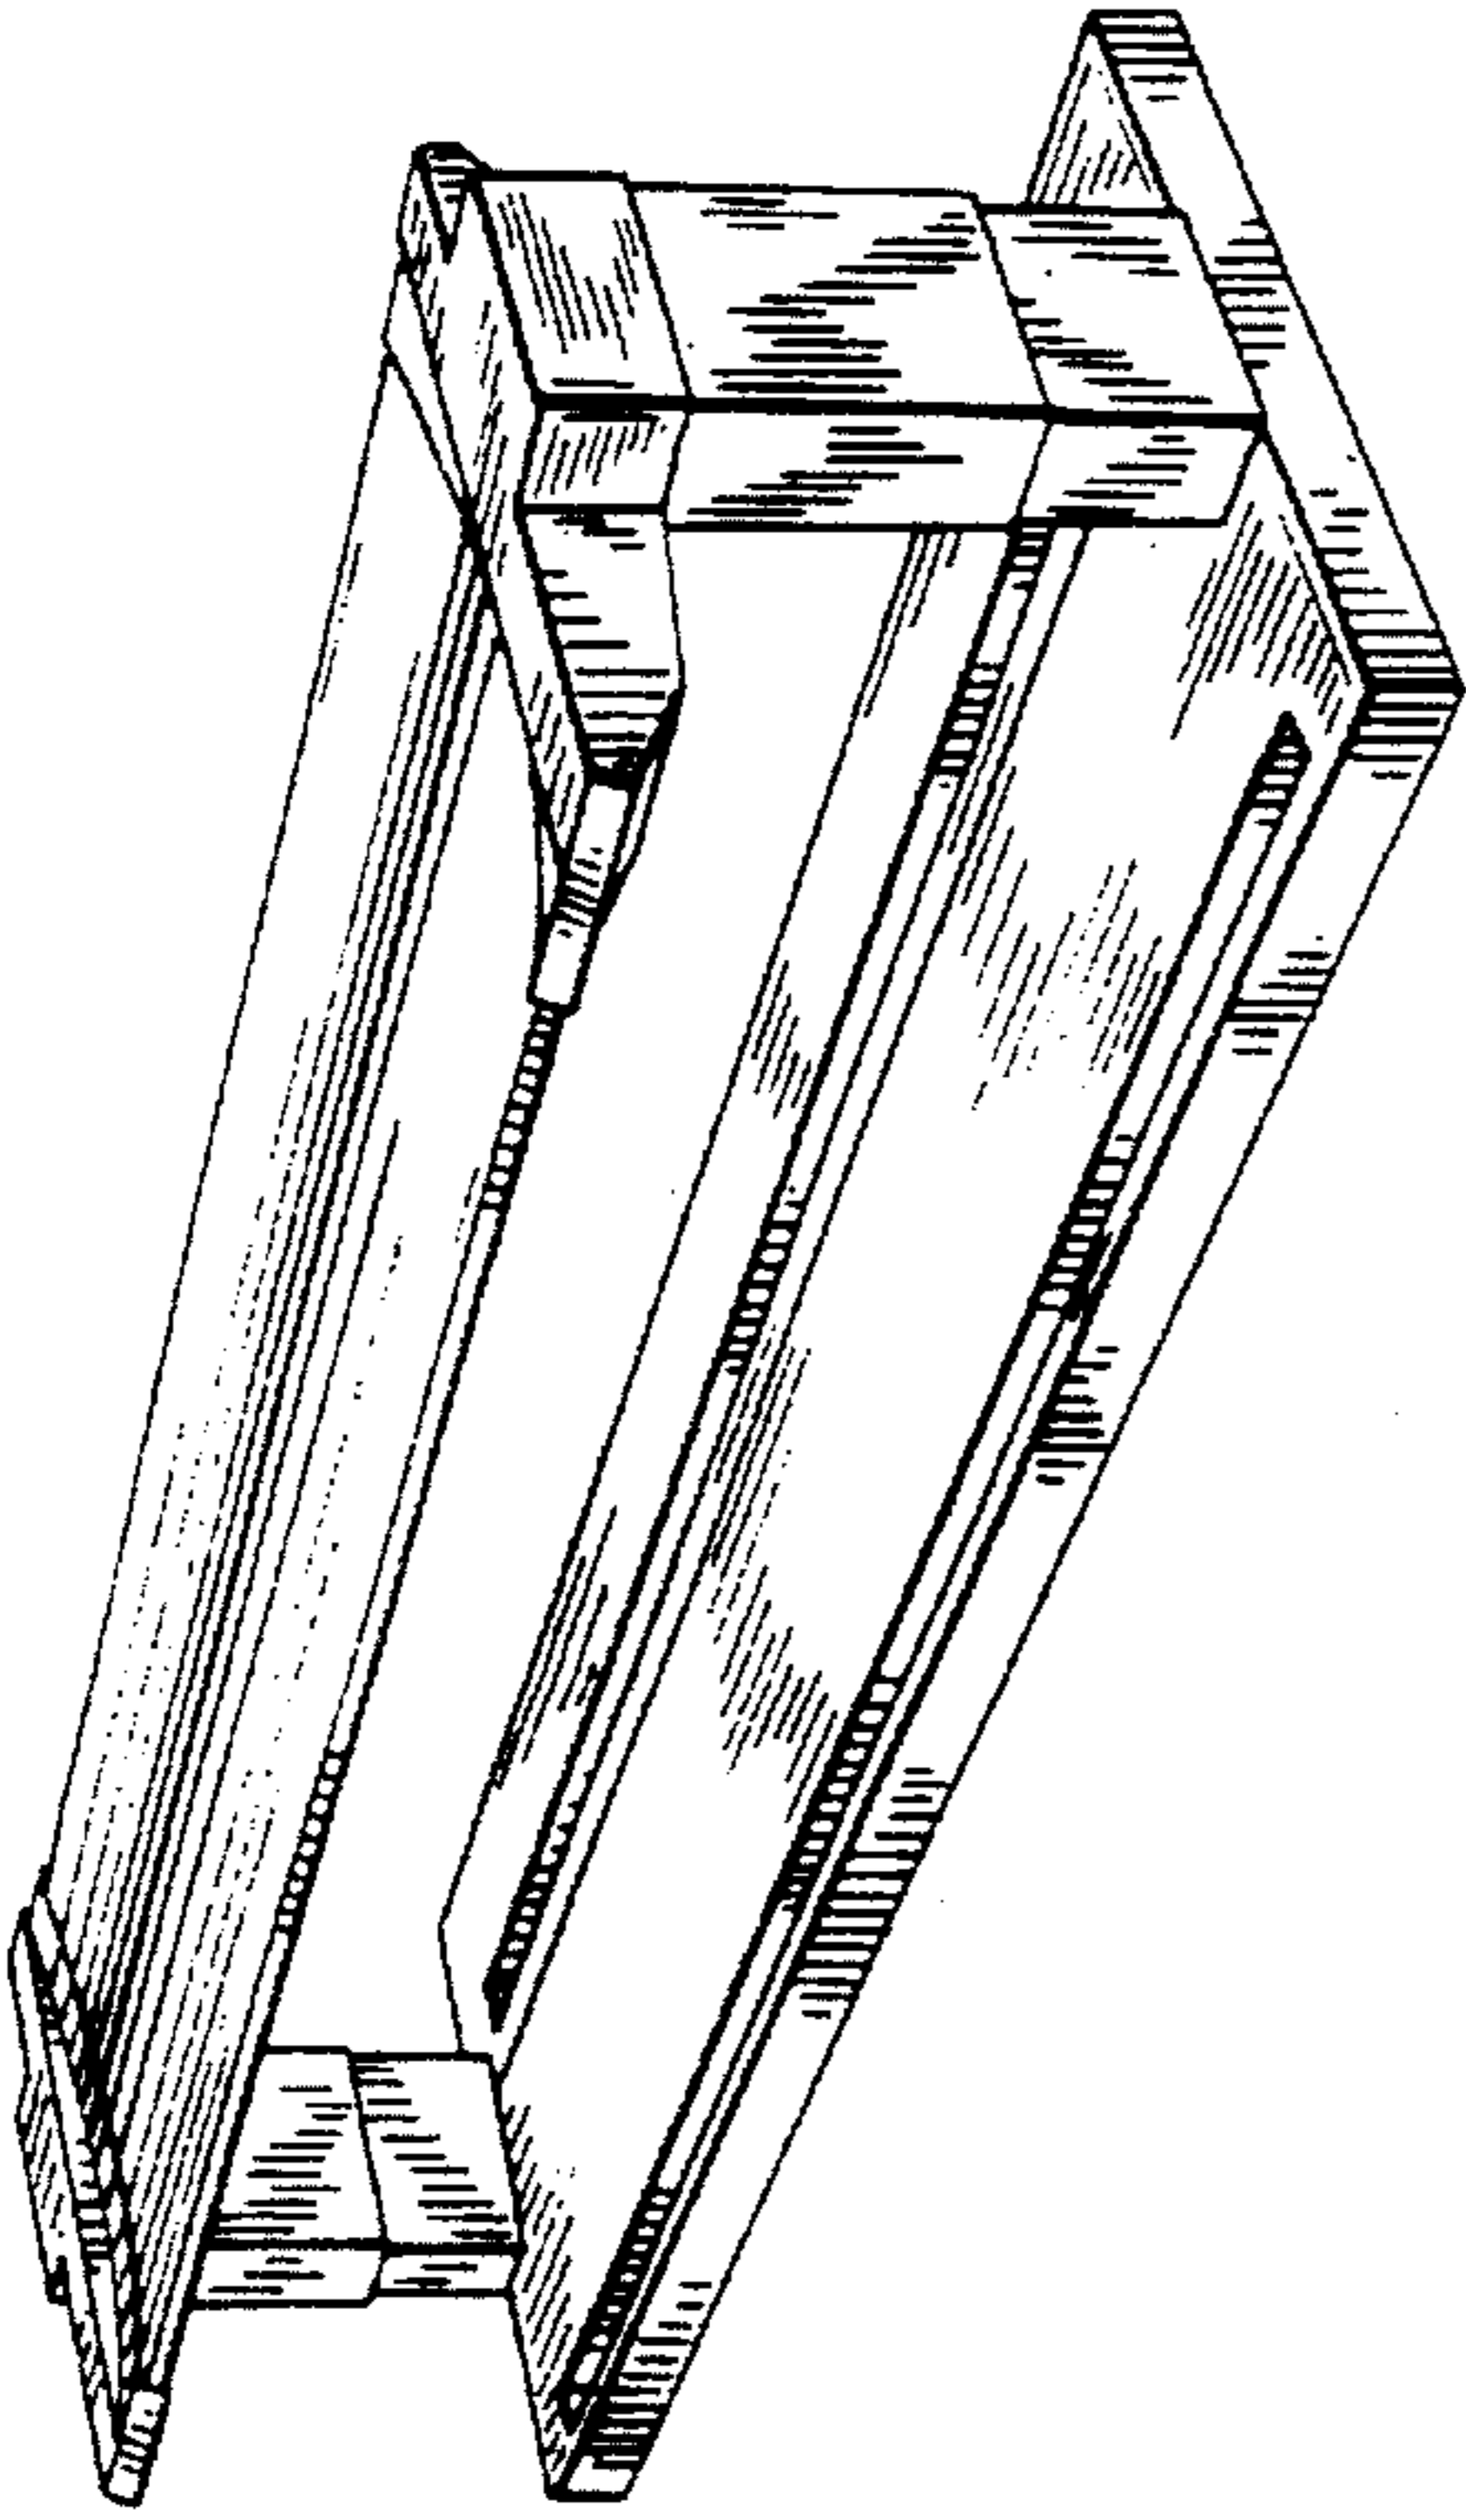


FIG. 8

FIG. 9

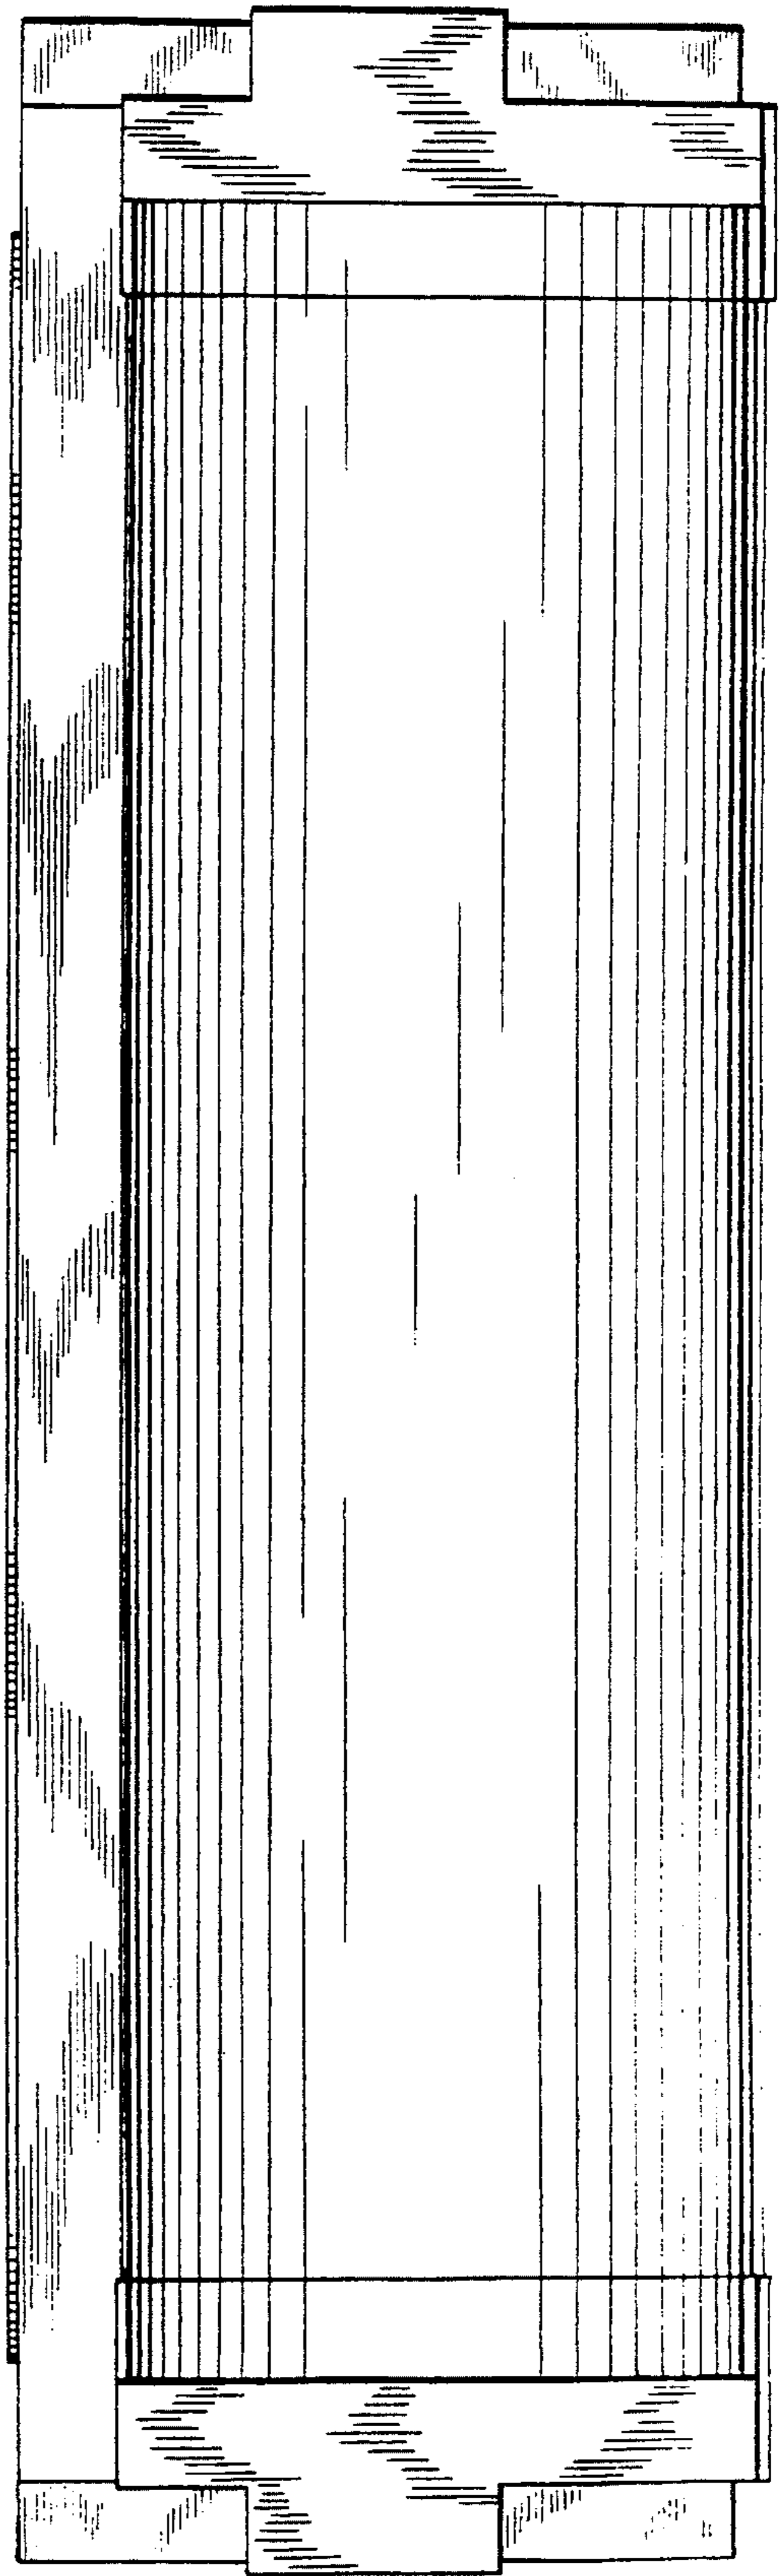
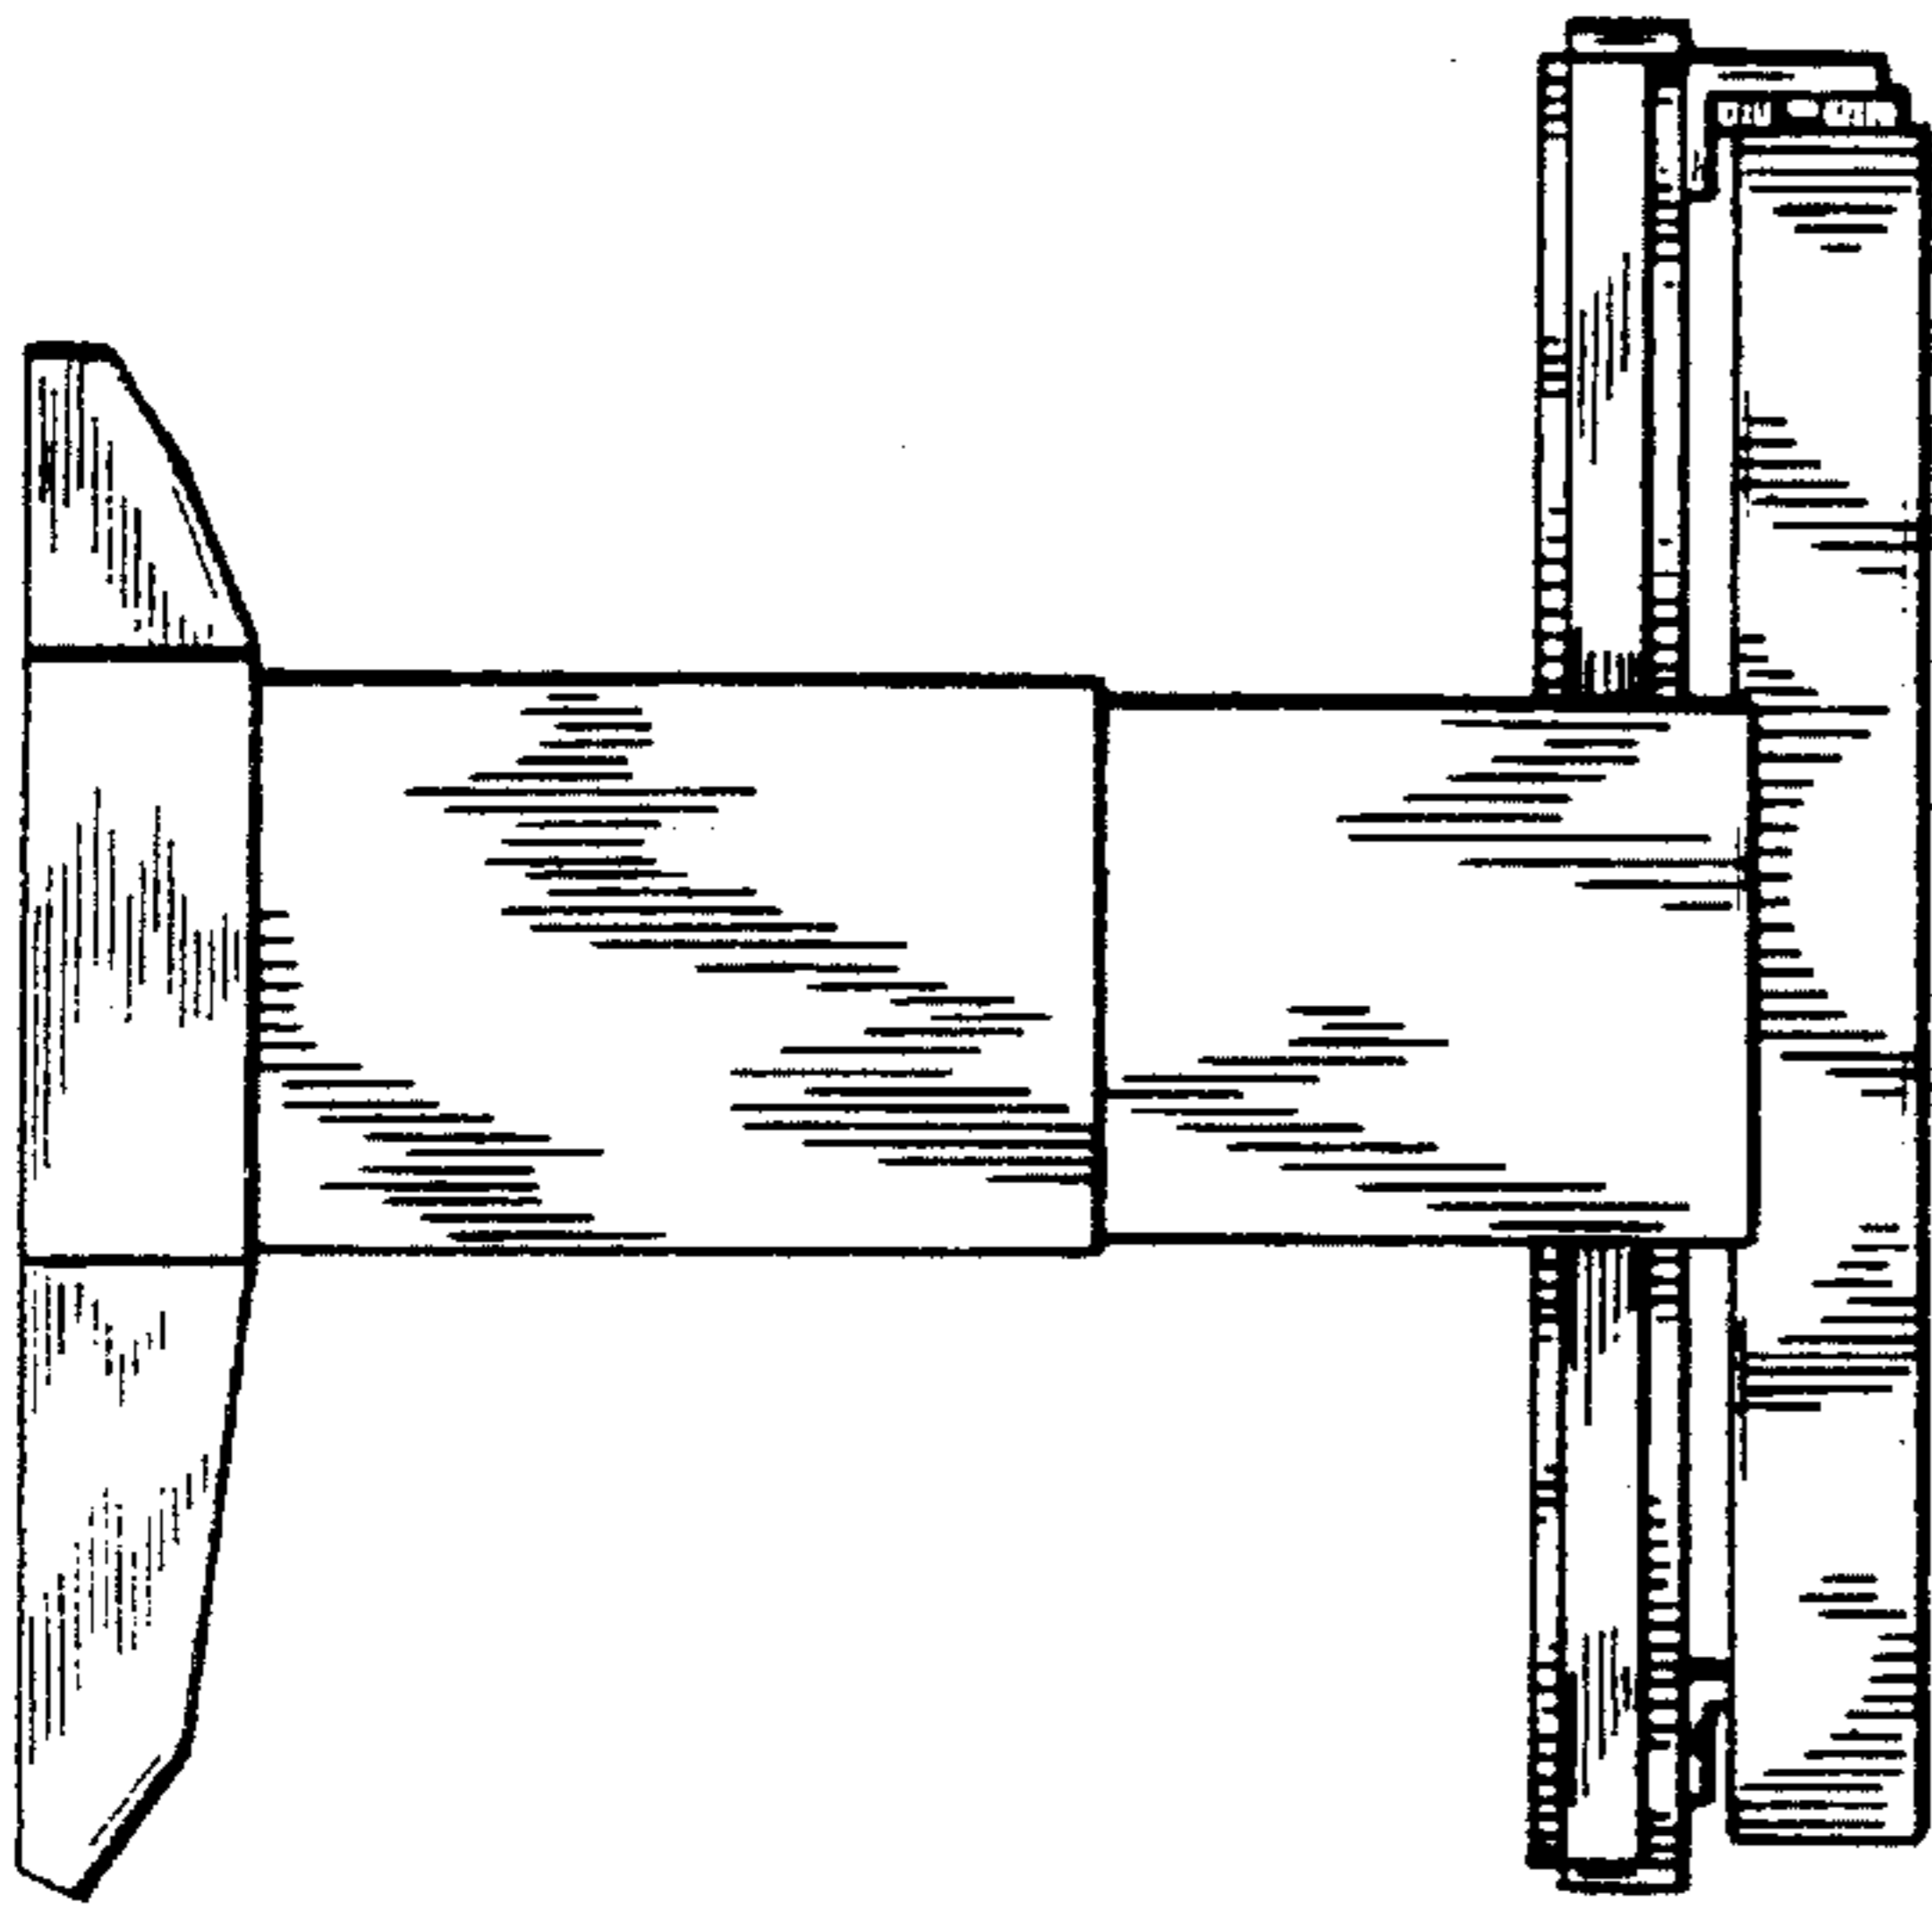


FIG. 10

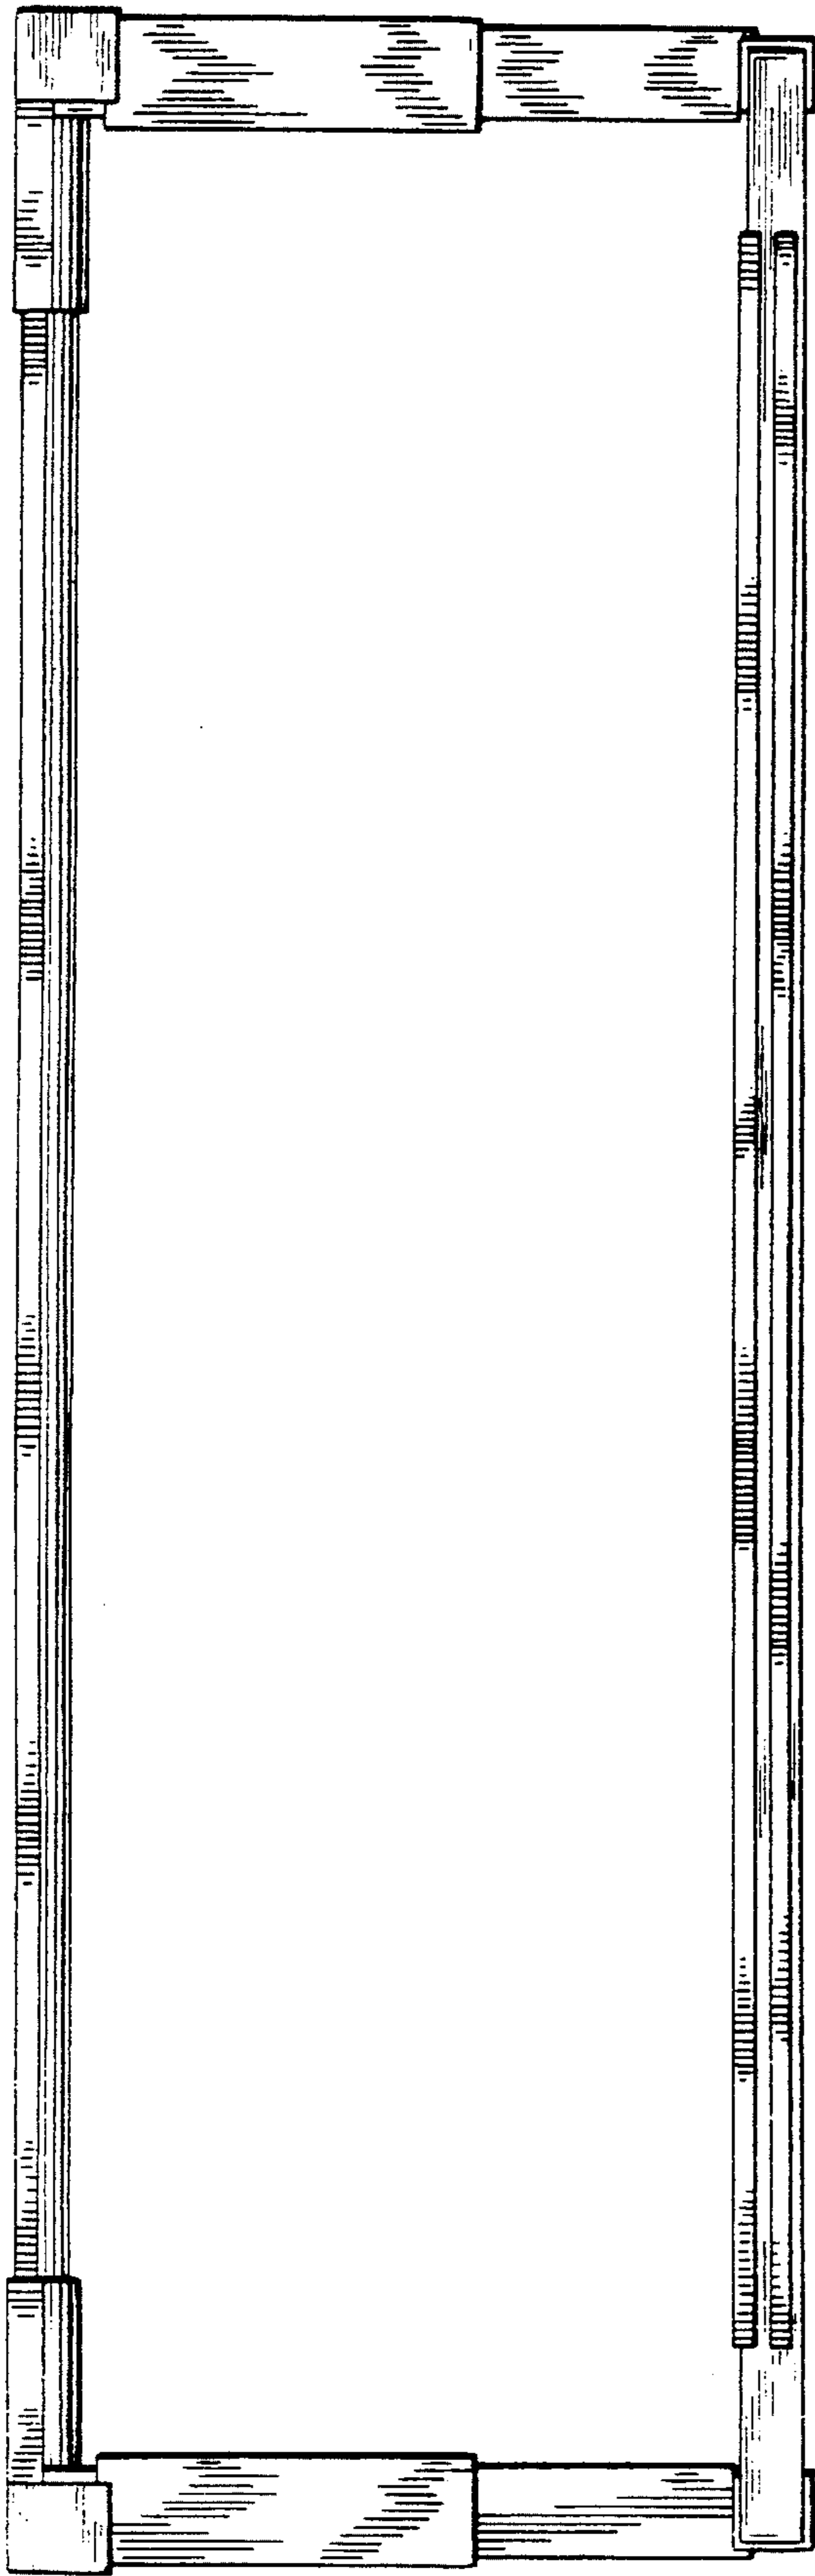


FIG. 11

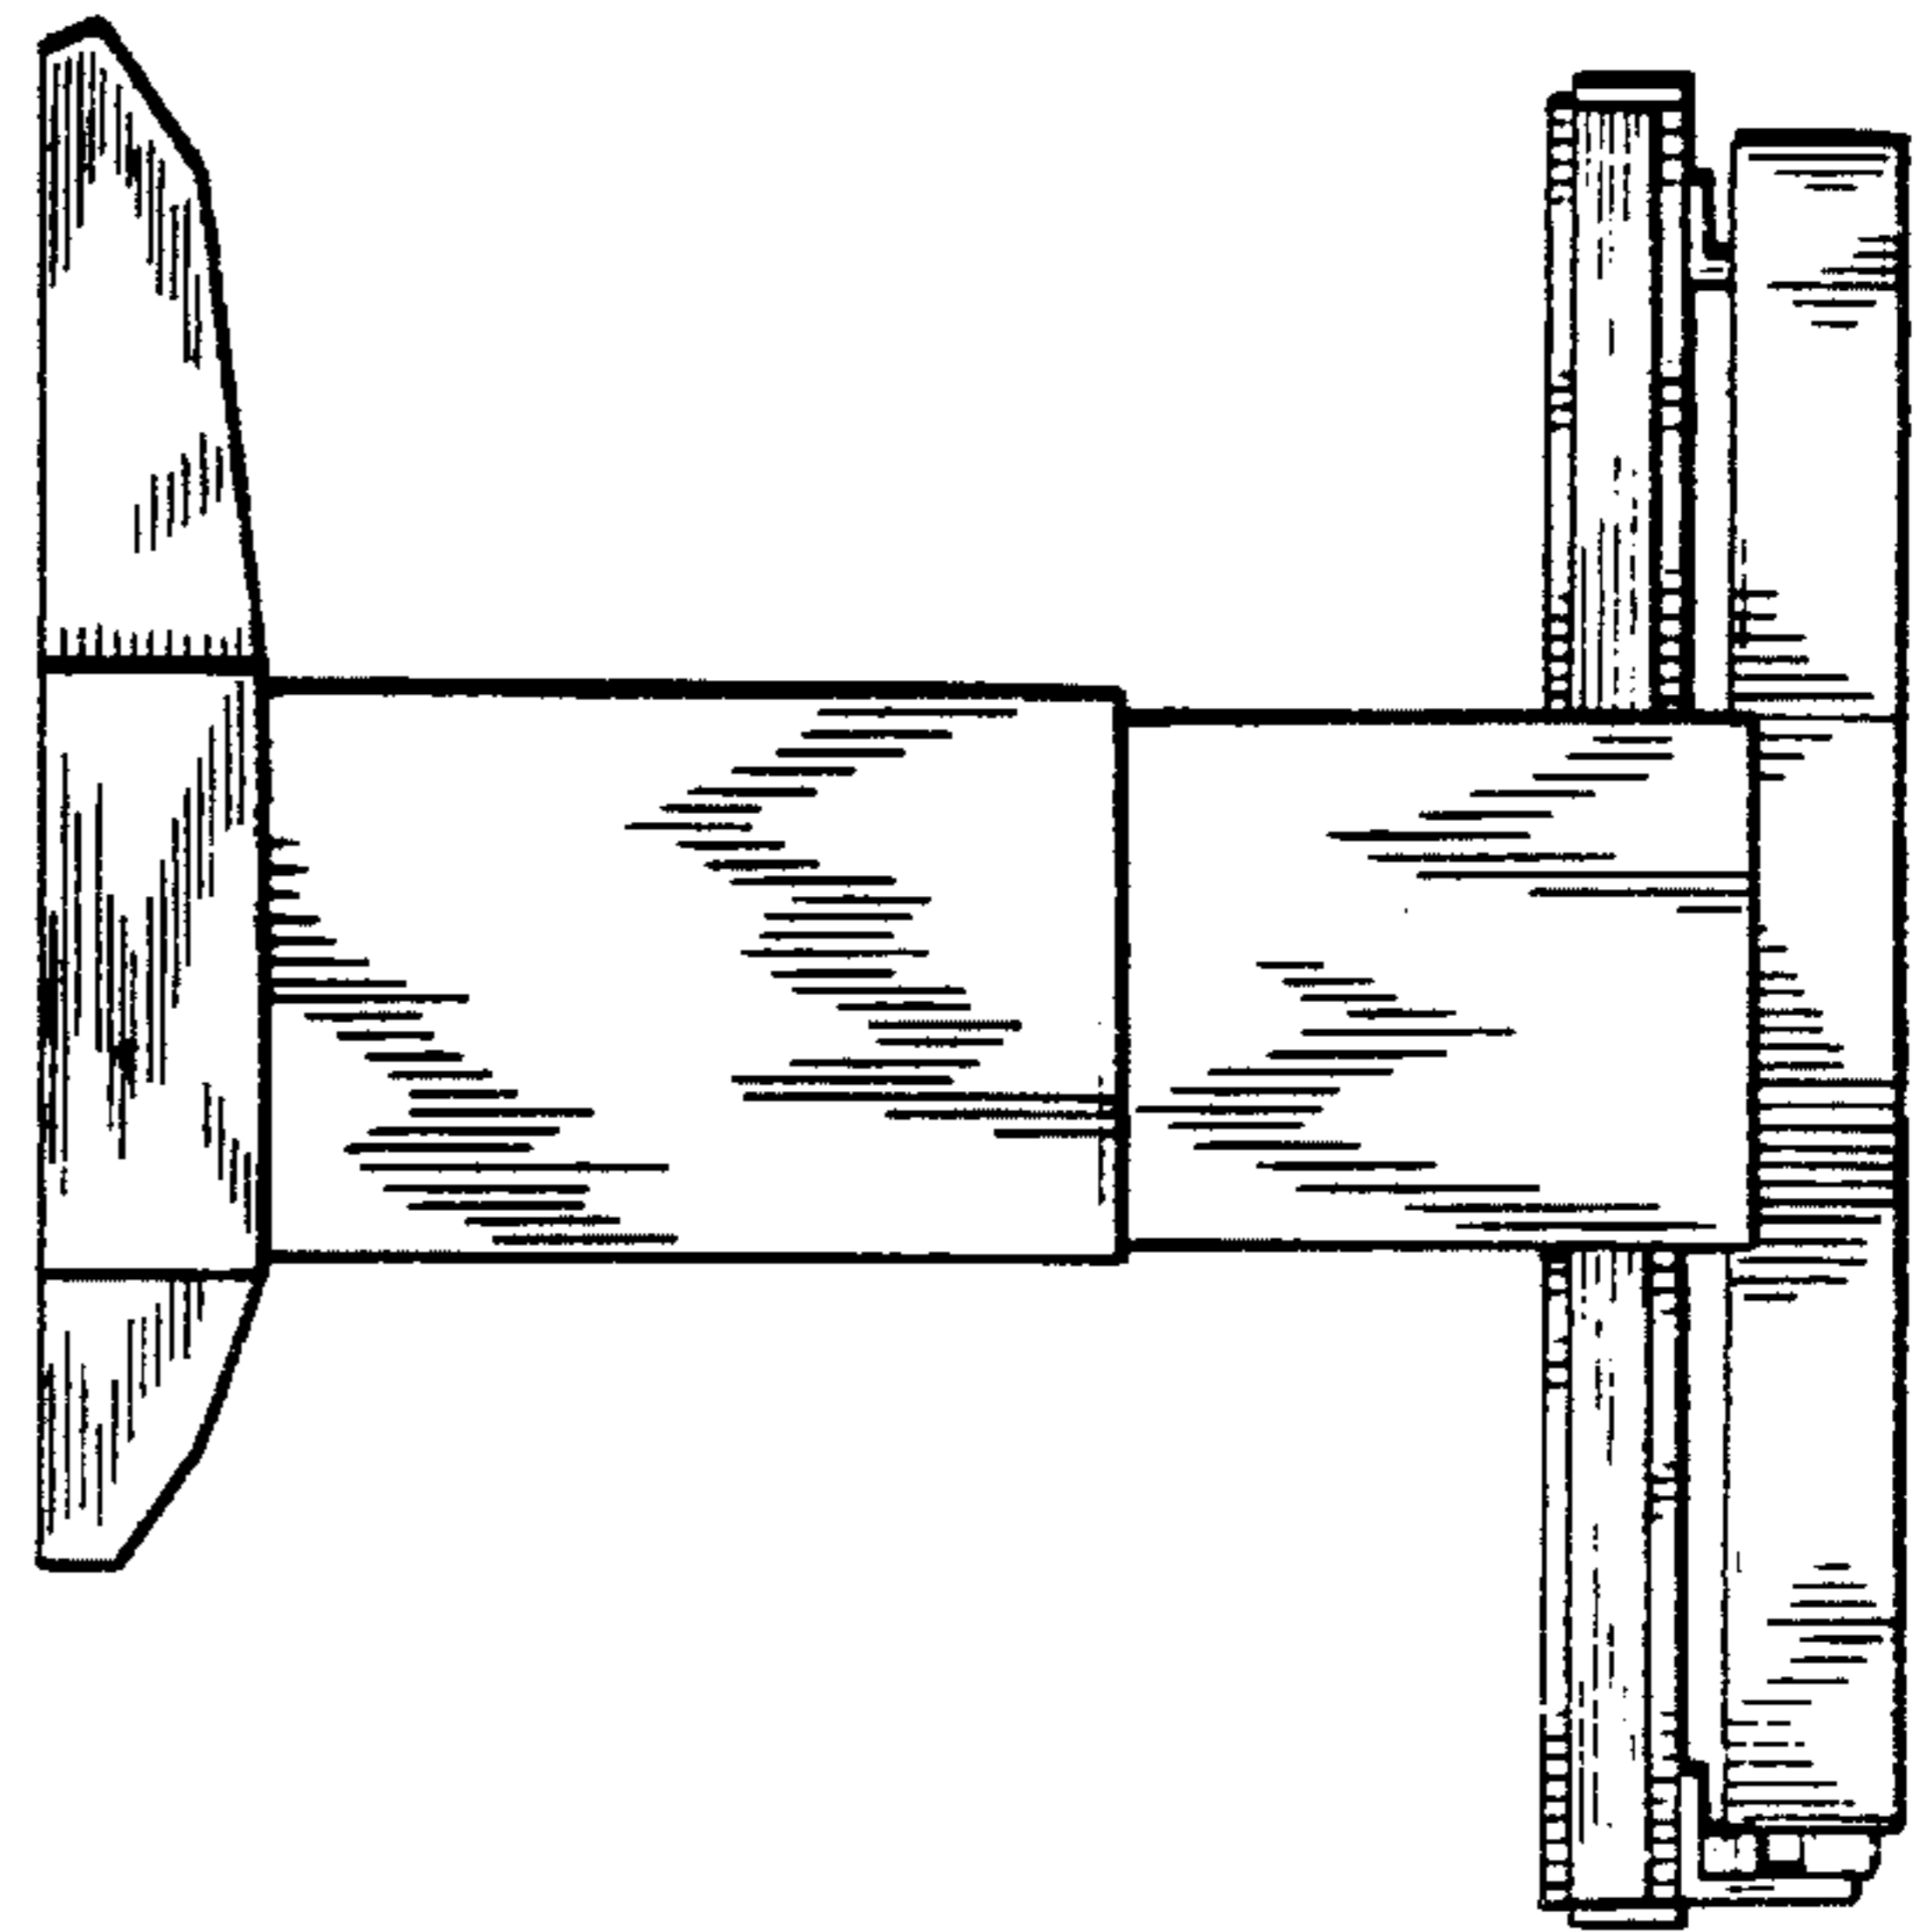


FIG. 12

FIG. 13

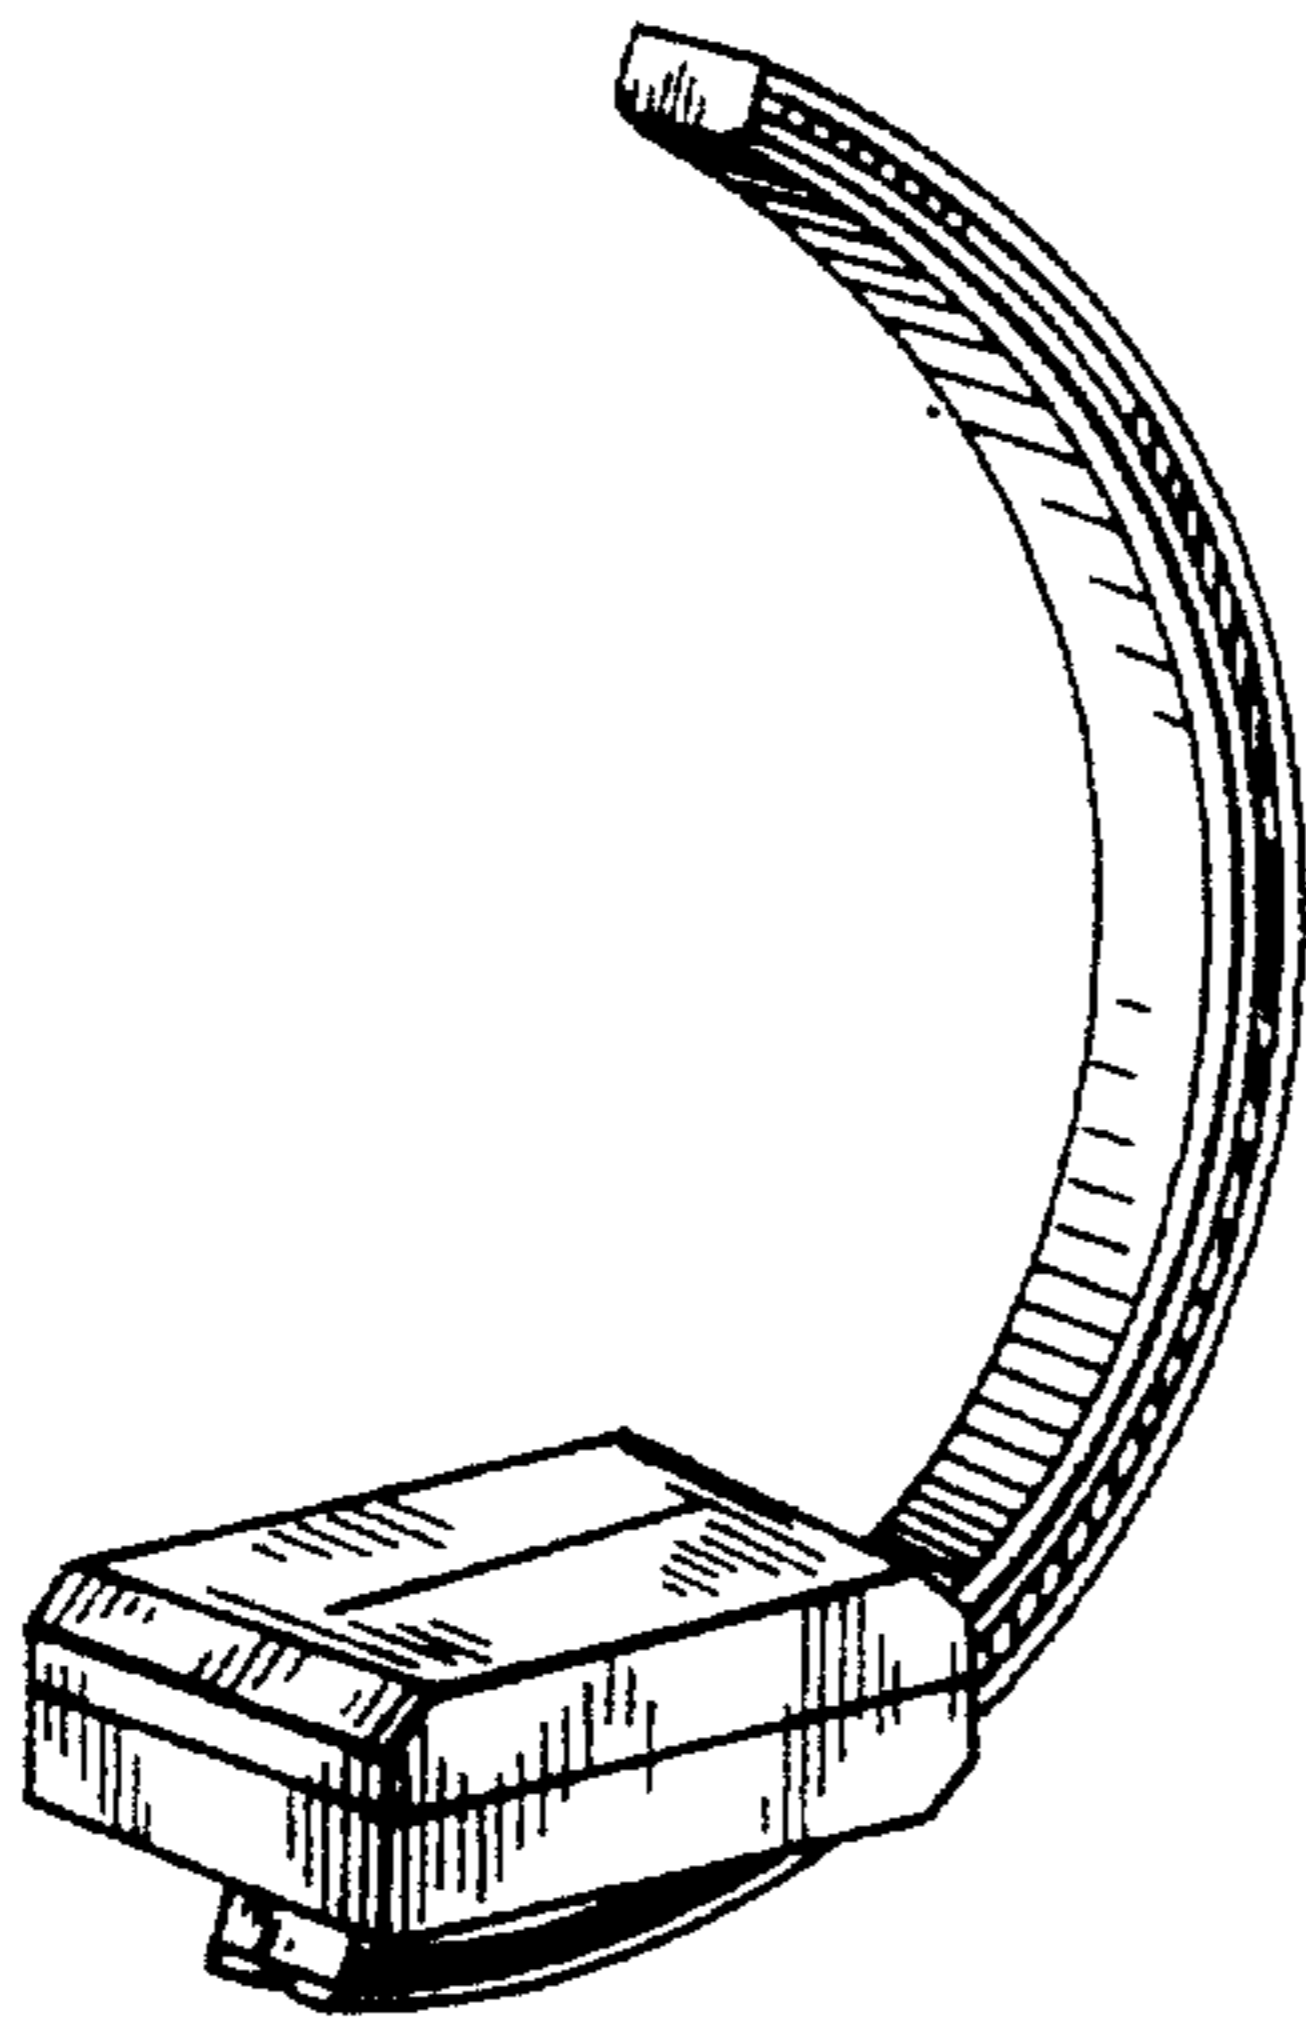


FIG. 14

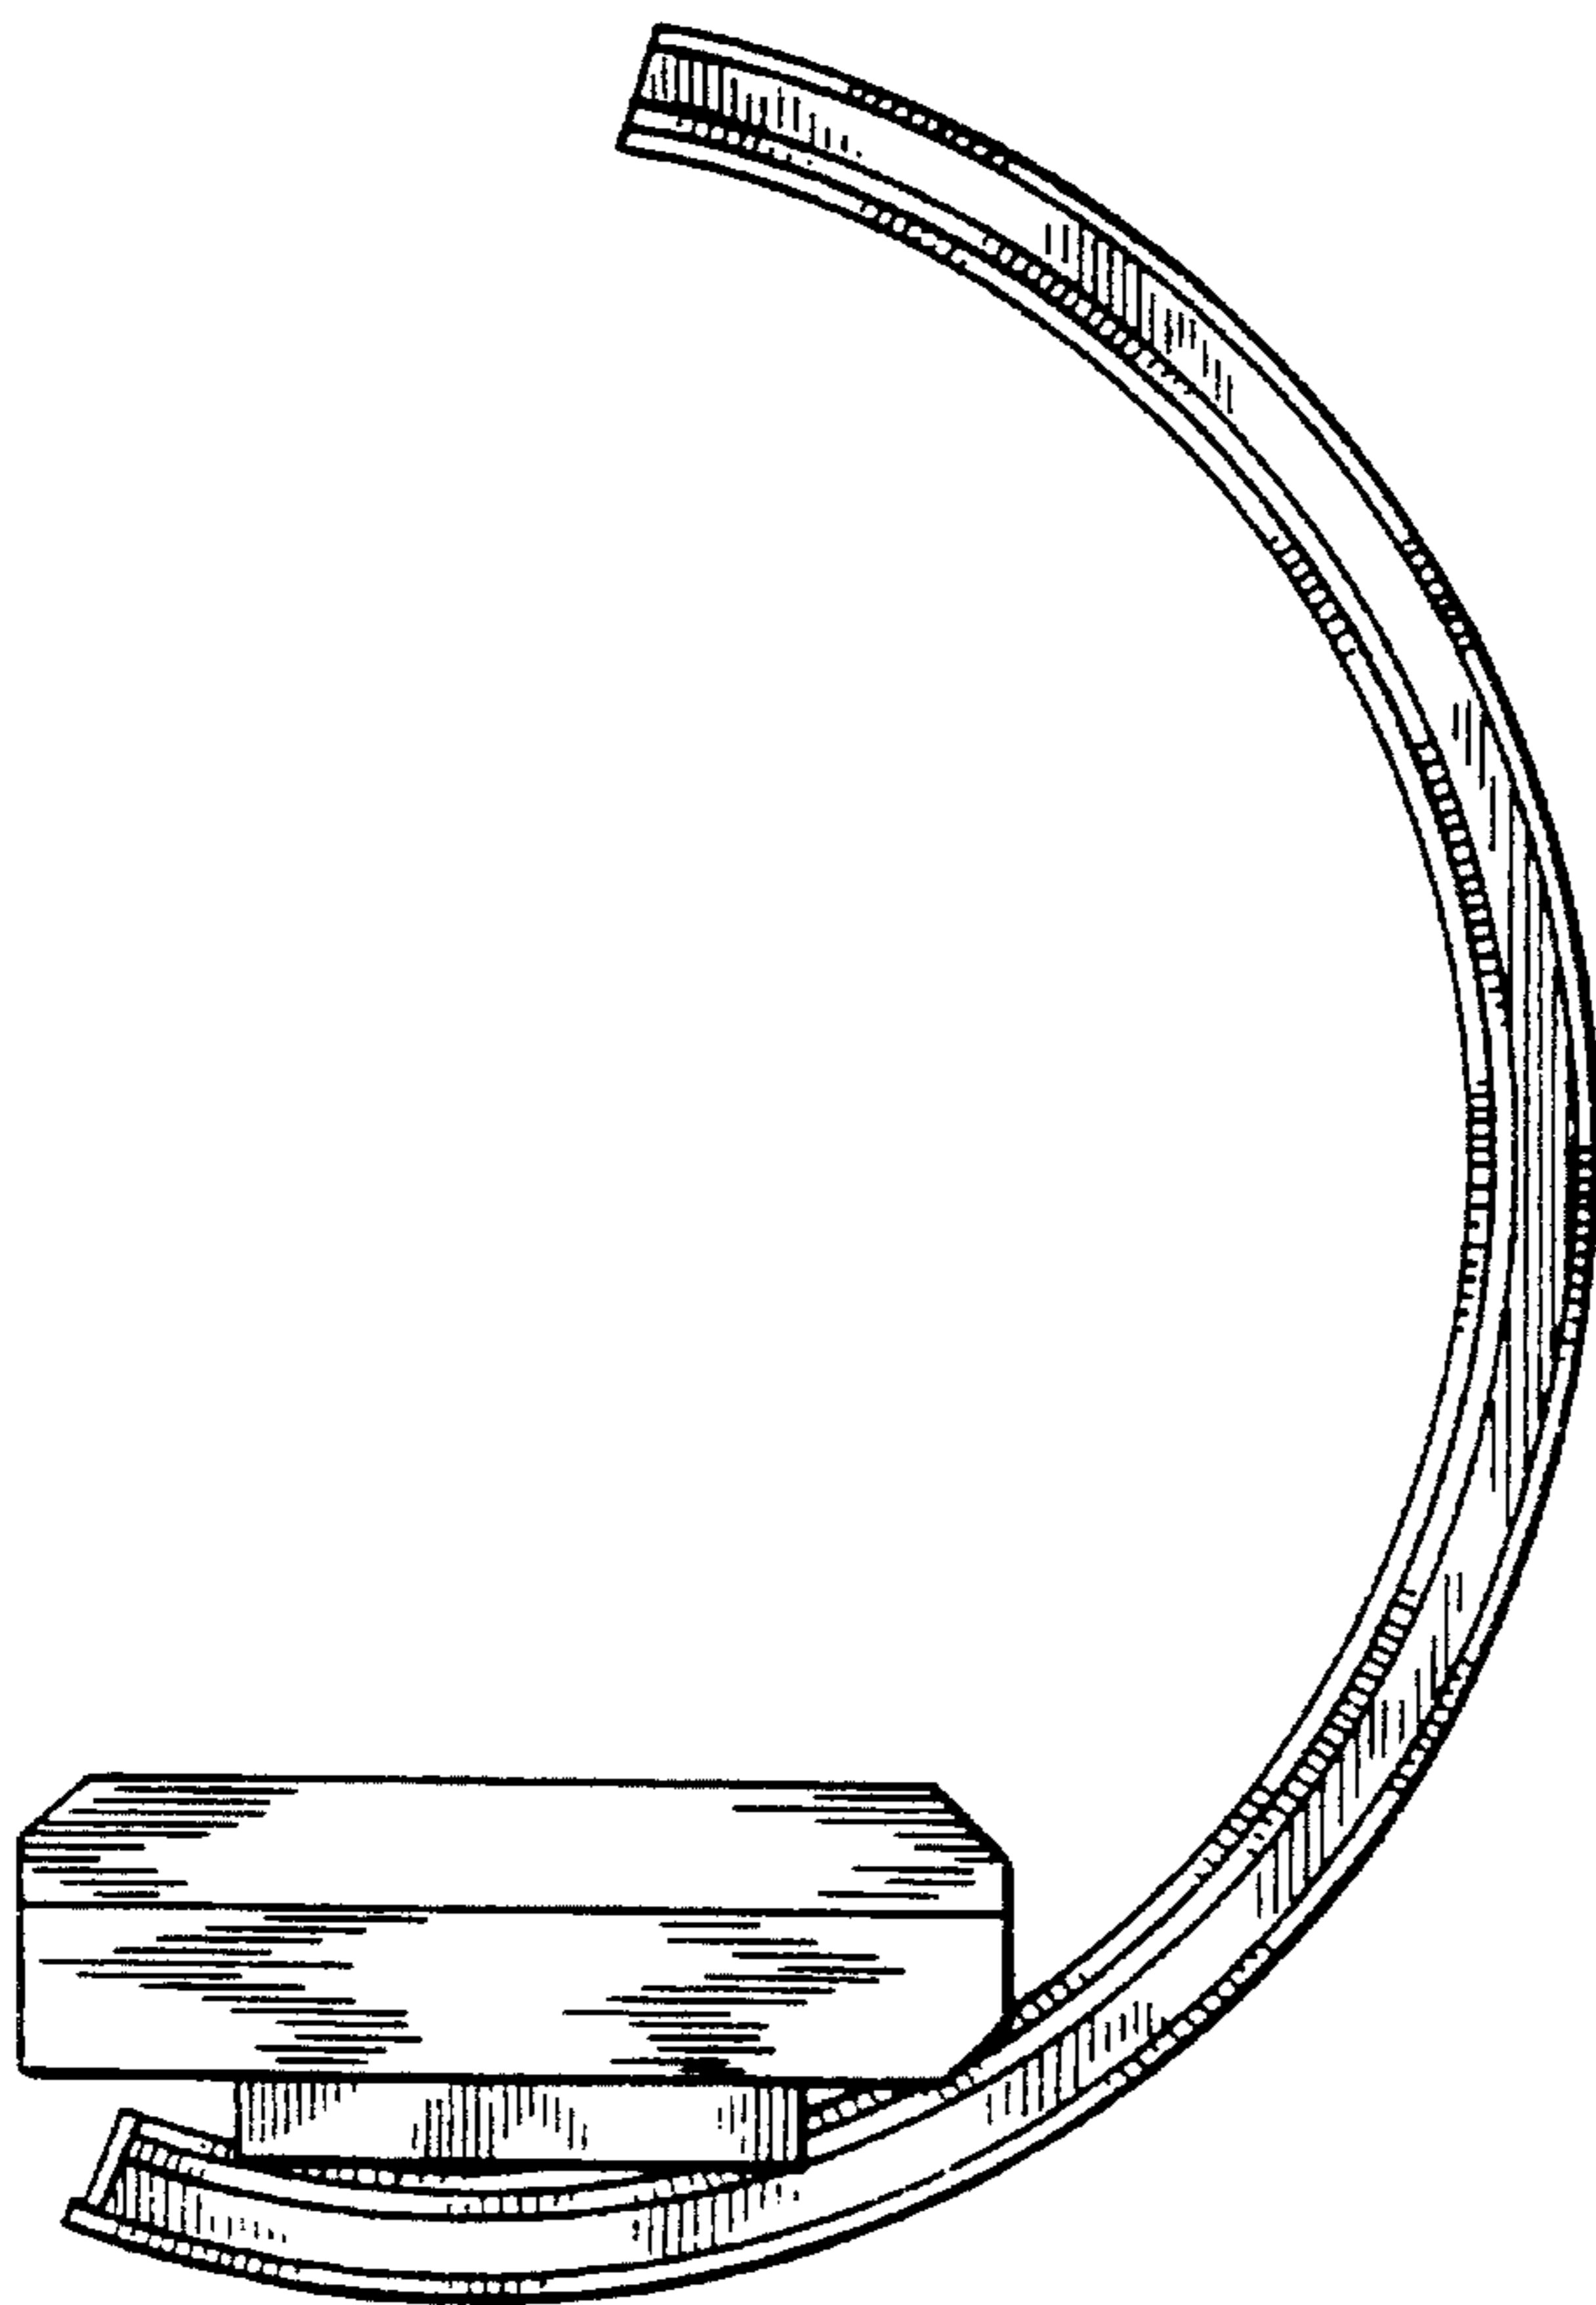
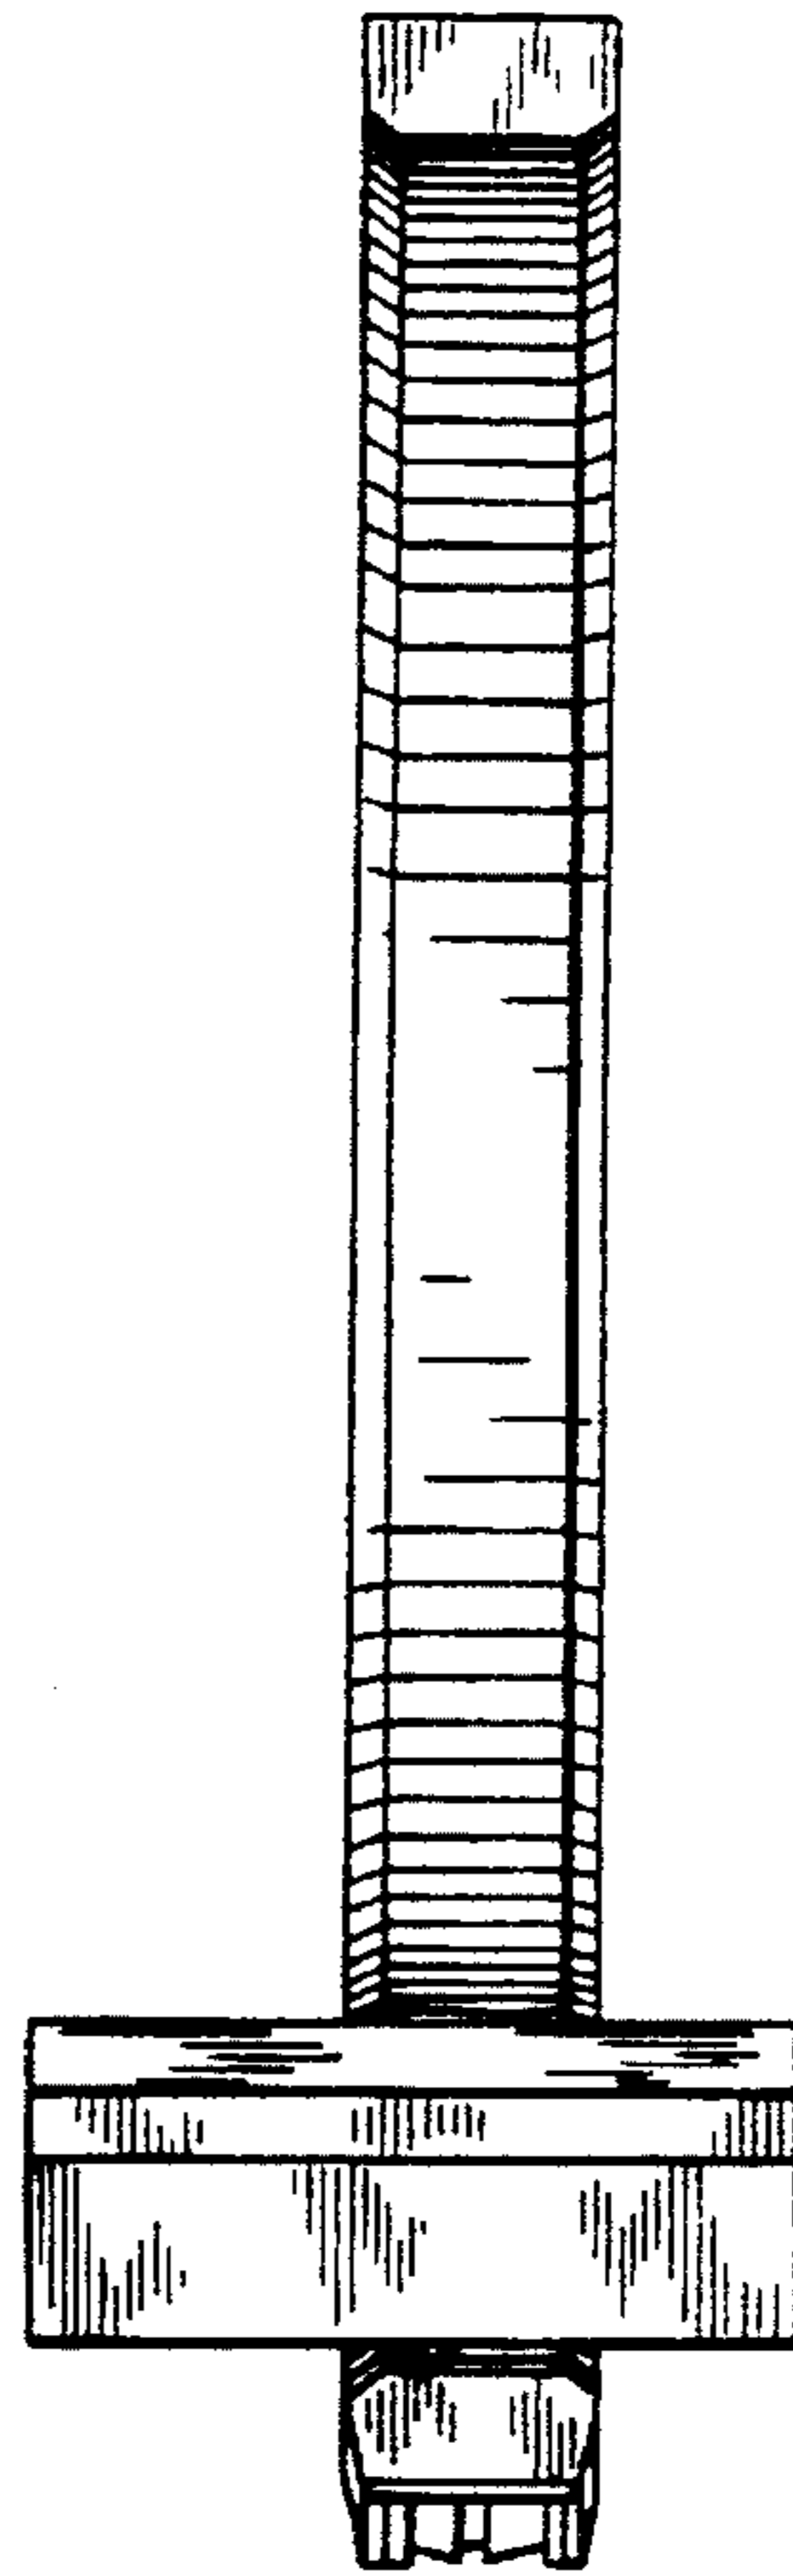


FIG. 15

FIG. 16

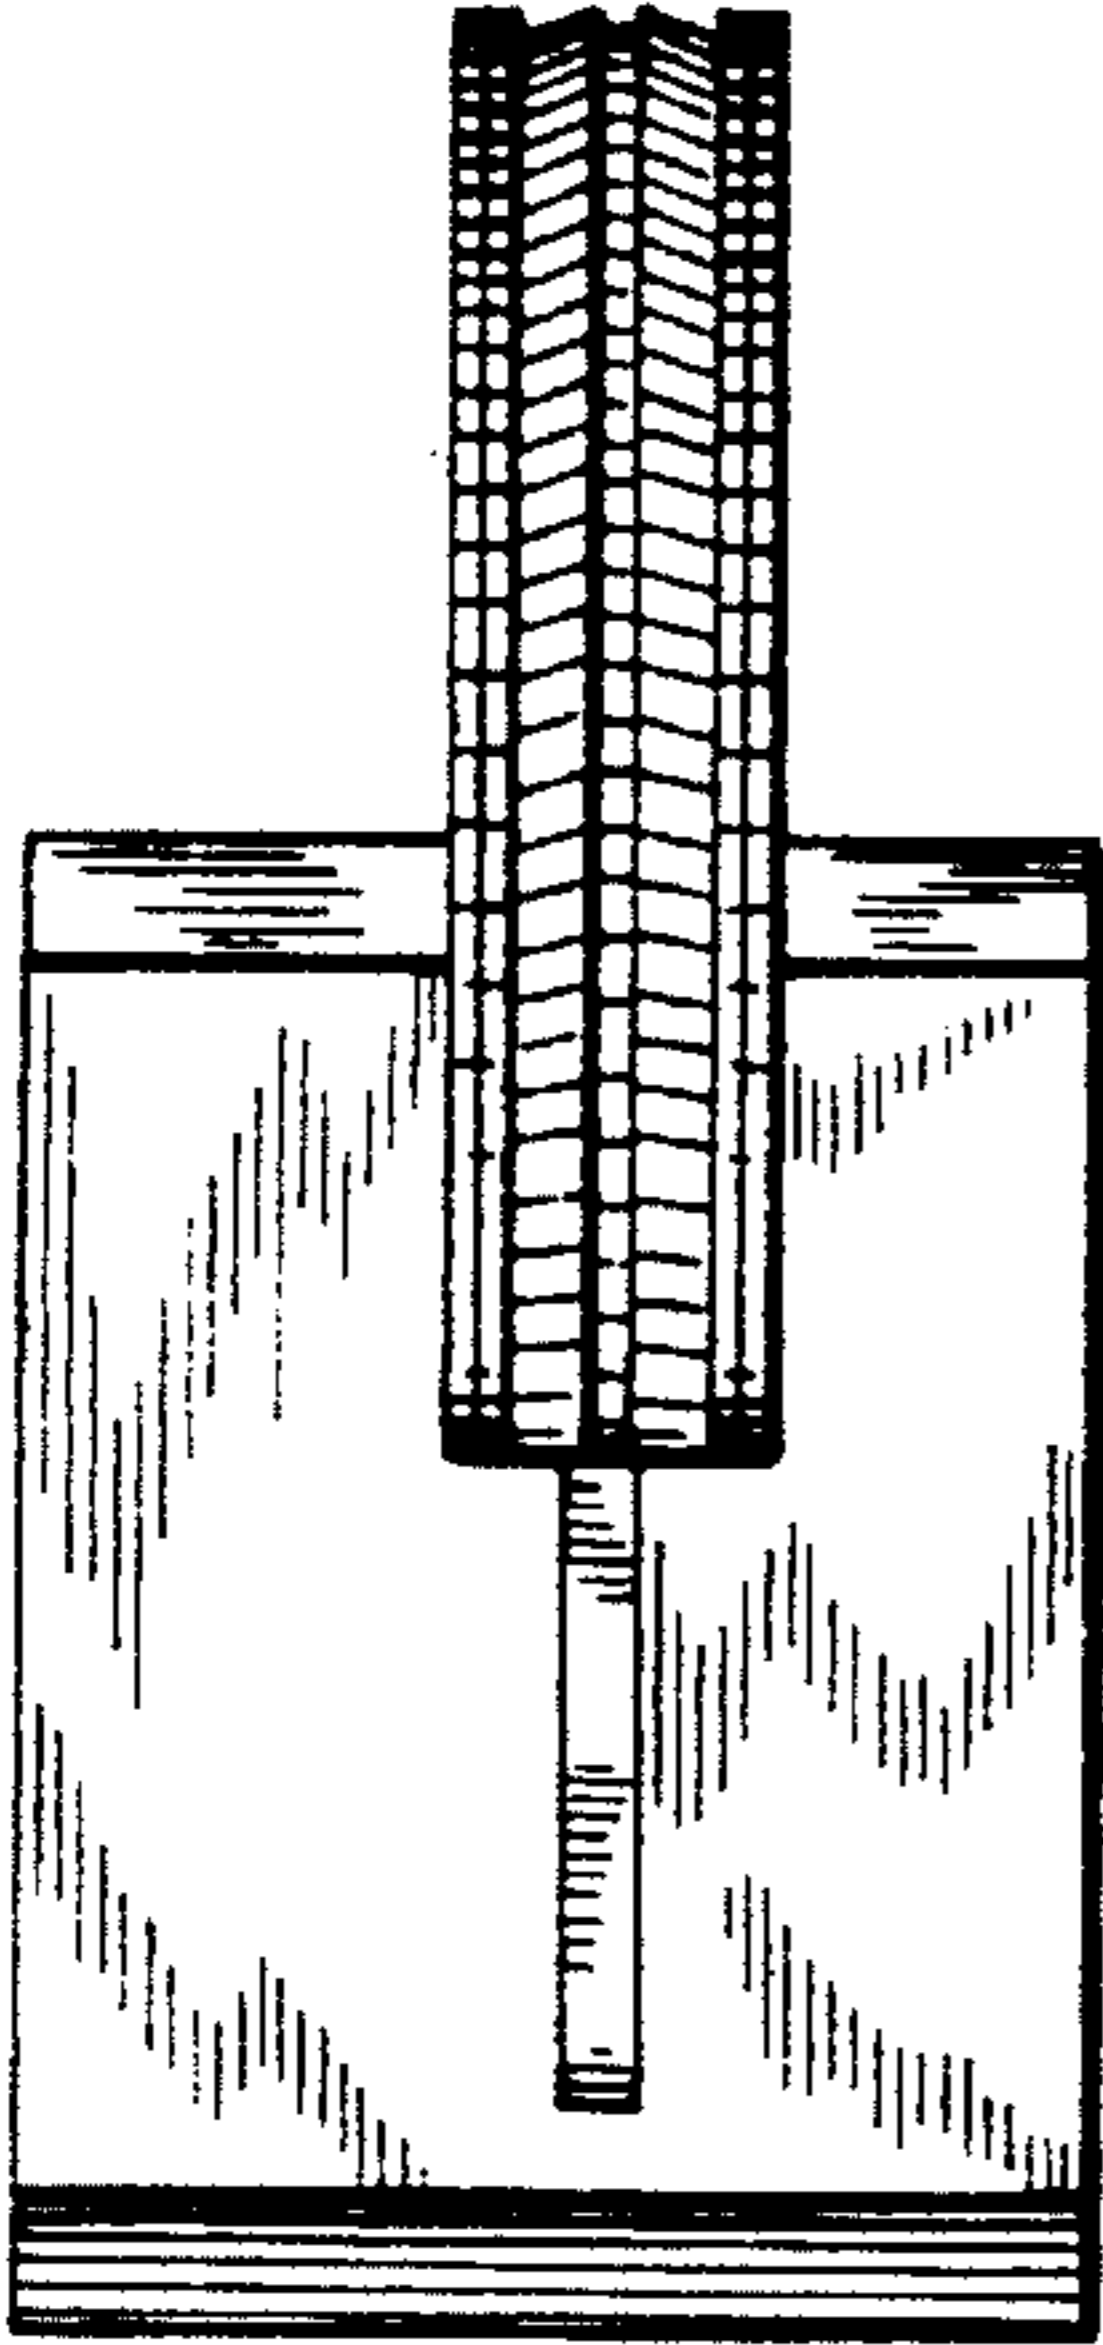


FIG. 17

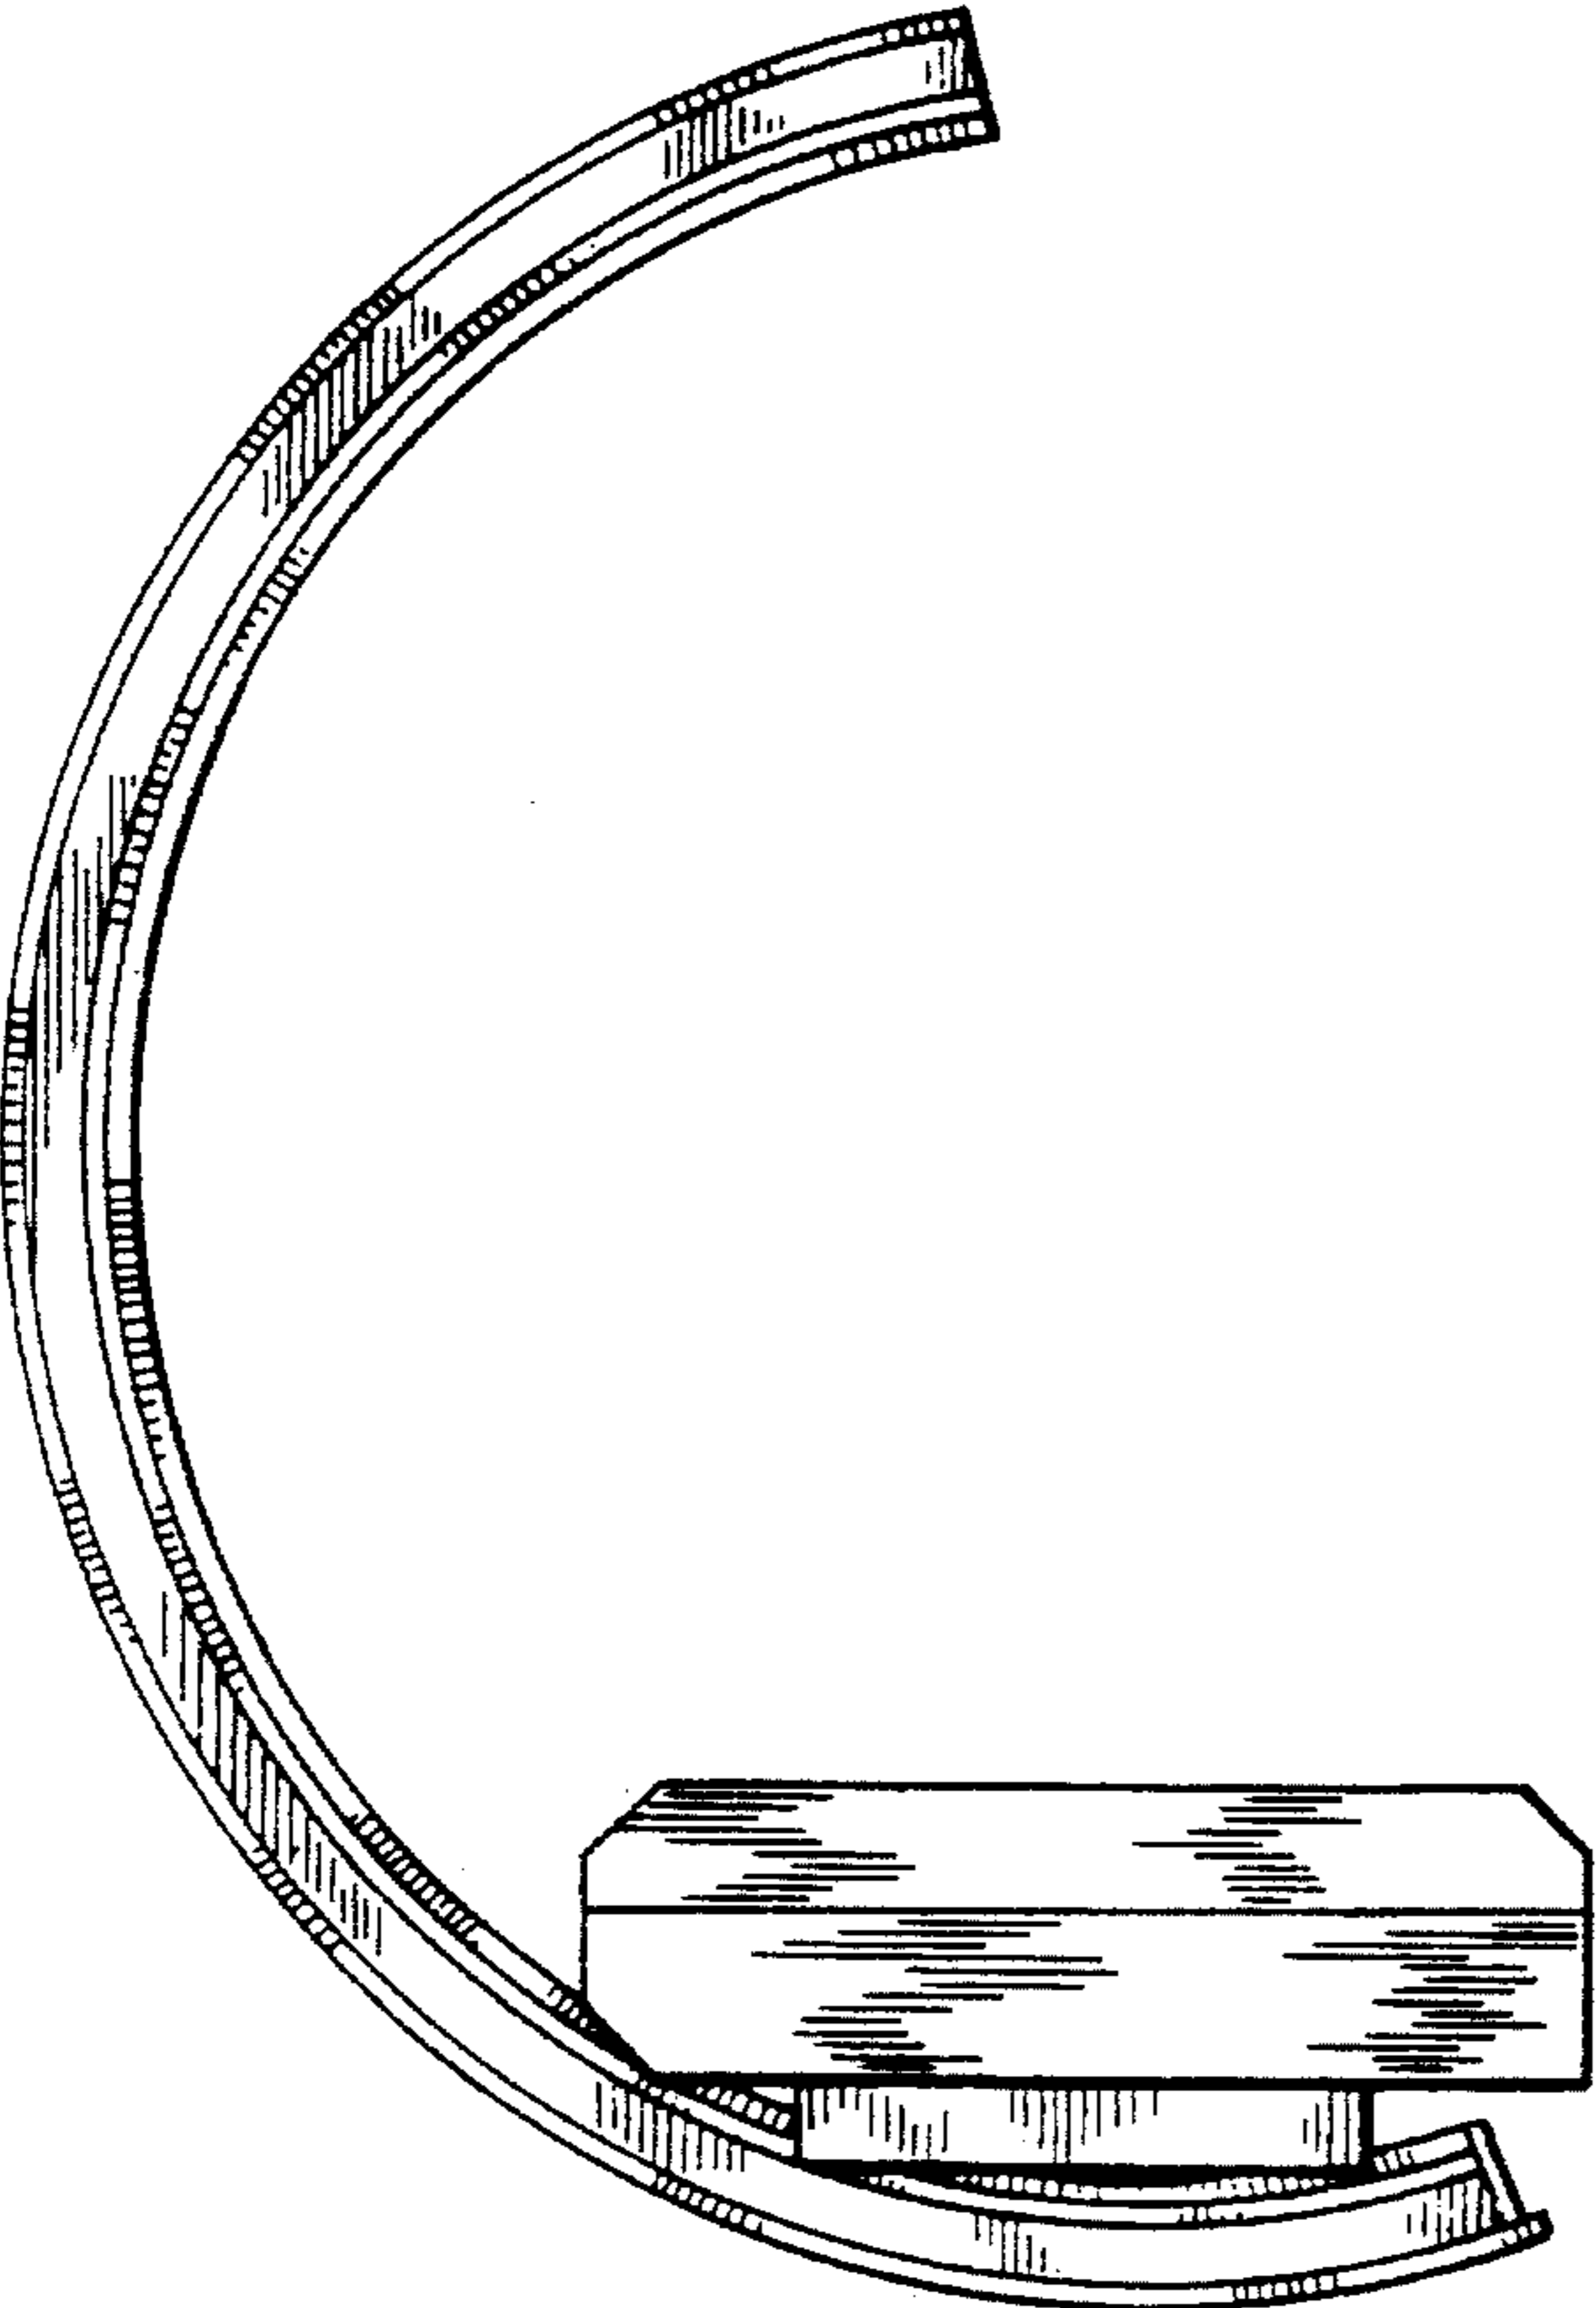
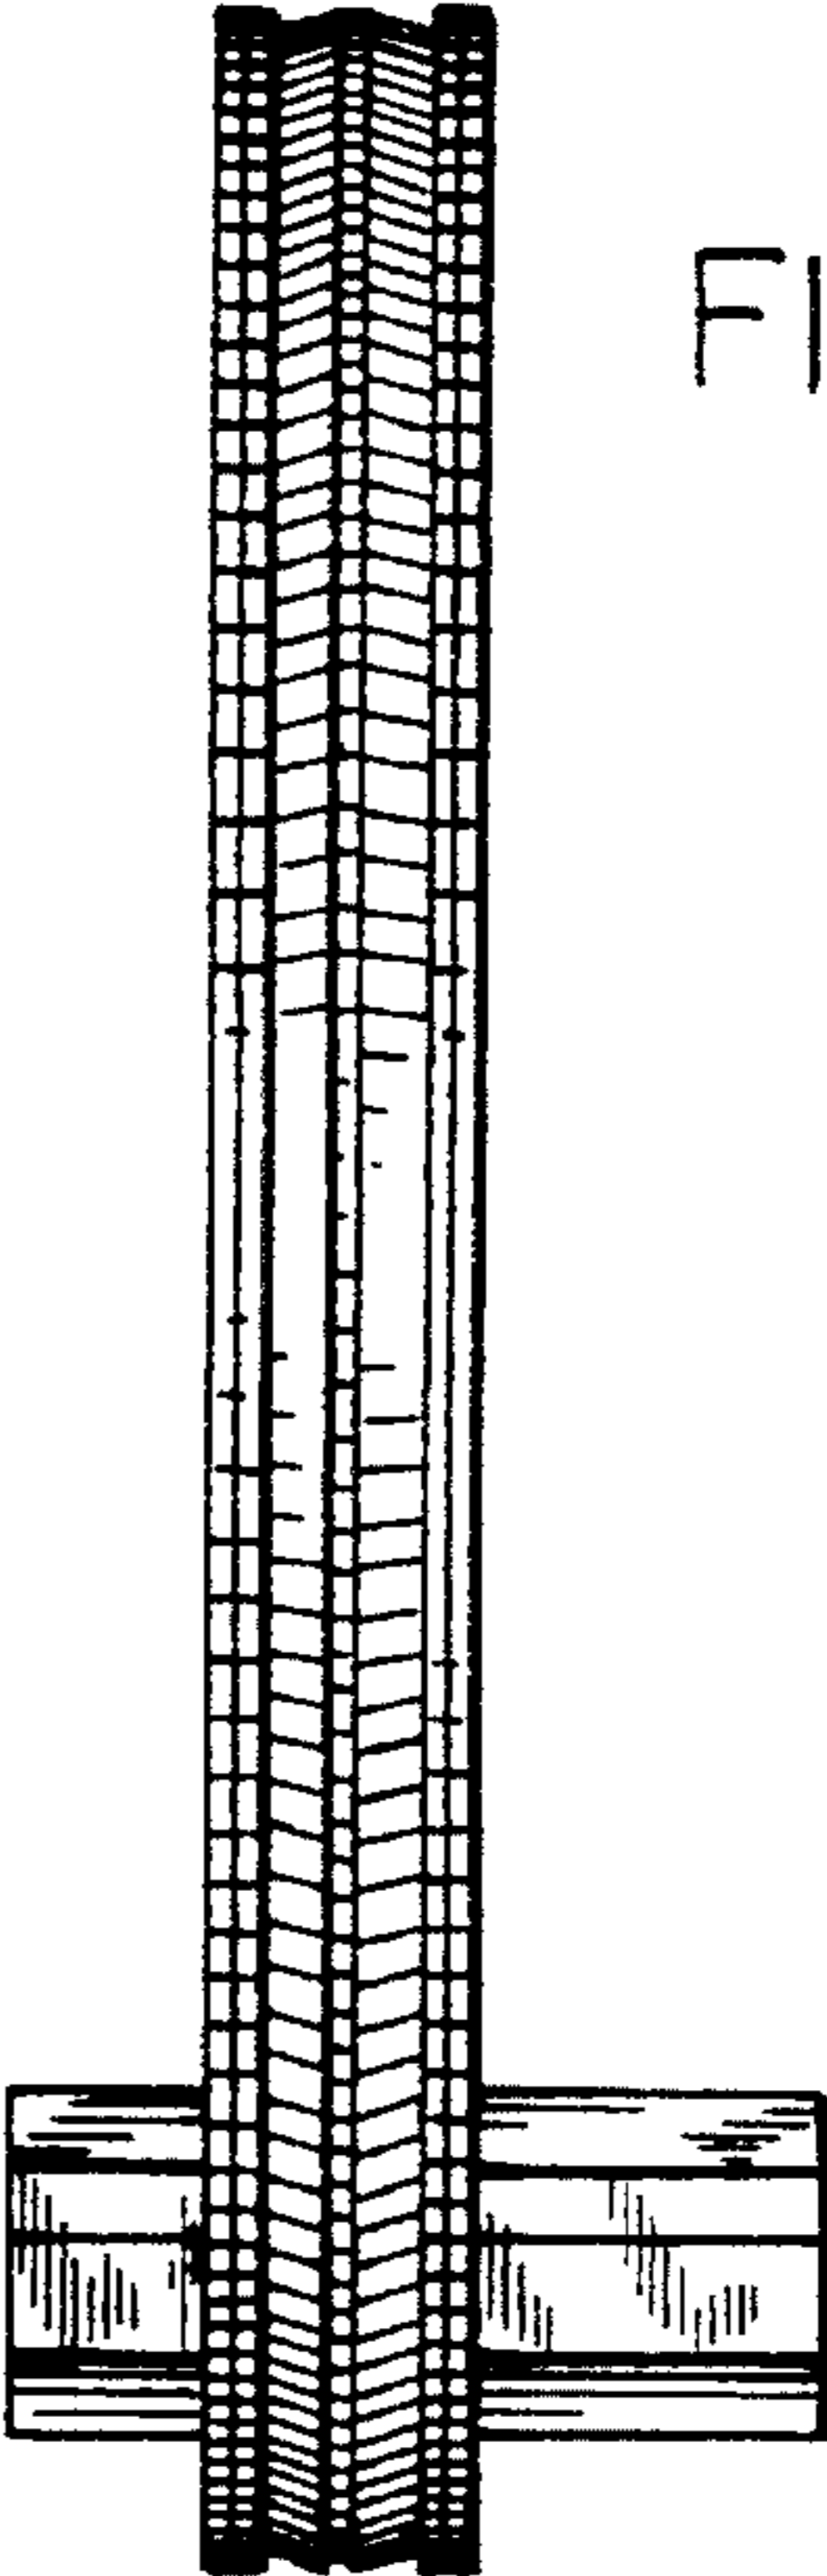


FIG. 18