



US00D369859S

**United States Patent** [19]

[11] **Patent Number: Des. 369,859**

**Ribando et al.**

[45] **Date of Patent: \*\*May 14, 1996**

[54] **MULTI-CHANNEL CONDUIT CONNECTOR FOR TREATING DEEP VEIN THROMBOSIS**

[75] Inventors: **Philip P. Ribando; Kenneth M. Bolam; Donald H. Peeler**, all of Charlotte, N.C.

[73] Assignee: **Jobst Institute, Inc.**, Charlotte, N.C.

[\*\*] Term: **14 Years**

[21] Appl. No.: **20,927**

[22] Filed: **Apr. 5, 1994**

[52] U.S. Cl. .... **D24/129**

[58] **Field of Search** ..... D24/129; 601/148, 601/149, 150, 152, 151, 153; 285/319, 26, 137.1, 317

[56] **References Cited**

**U.S. PATENT DOCUMENTS**

D. 319,312	8/1991	Schneider	.....	D24/129
D. 327,738	7/1992	Dye	.....	D24/129
D. 330,250	10/1992	Dye	.....	D24/129
4,076,279	2/1978	Klotz et al.	.....	285/26
4,253,449	3/1981	Arkans et al.	.....	128/24
4,478,436	10/1984	Hashimoto	.....	285/137.1
4,804,208	2/1989	Dye	.....	285/26
5,219,185	6/1993	Oddenino	.....	285/26
5,342,285	8/1994	Dye	.....	601/148 X

**OTHER PUBLICATIONS**

Brochure "Making Prevention Operative" from Kendall Healthcare Products Company for SCD™ Compression System, ©1991 Kendall Health Care Products Company.

Instruction Manual from Kendall Healthcare Products Company for SCD™ Therapeutic System, ©1989 Kendall Healthcare Products Company.

*Primary Examiner*—Louis S. Zarfaz  
*Assistant Examiner*—I. Simmons  
*Attorney, Agent, or Firm*—Bell, Seltzer, Park & Gibson



[57] **CLAIM**

The ornamental design for a multi-channel conduit connector for treating deep vein thrombosis, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of the multi-channel conduit connector for treating deep vein thrombosis which illustrates the new design;  
FIG. 2 is a top plan view thereof;  
FIG. 3 is a right side view thereof;  
FIG. 4 is a bottom view thereof;  
FIG. 5 is a left side view thereof;  
FIG. 6 is a back view thereof;  
FIG. 7 is a front view thereof;  
FIG. 8 is a perspective view of second embodiment of the multi-channel conduit connector for treating deep vein thrombosis which illustrates the new design;  
FIG. 9 is a top view of FIG. 8;  
FIG. 10 is a right side view of FIG. 8;  
FIG. 11 is a bottom view of FIG. 8;  
FIG. 12 is a left side view of FIG. 8;  
FIG. 13 is a back view of FIG. 8; and,  
FIG. 14 is a front view of FIG. 8.

**1 Claim, 2 Drawing Sheets**

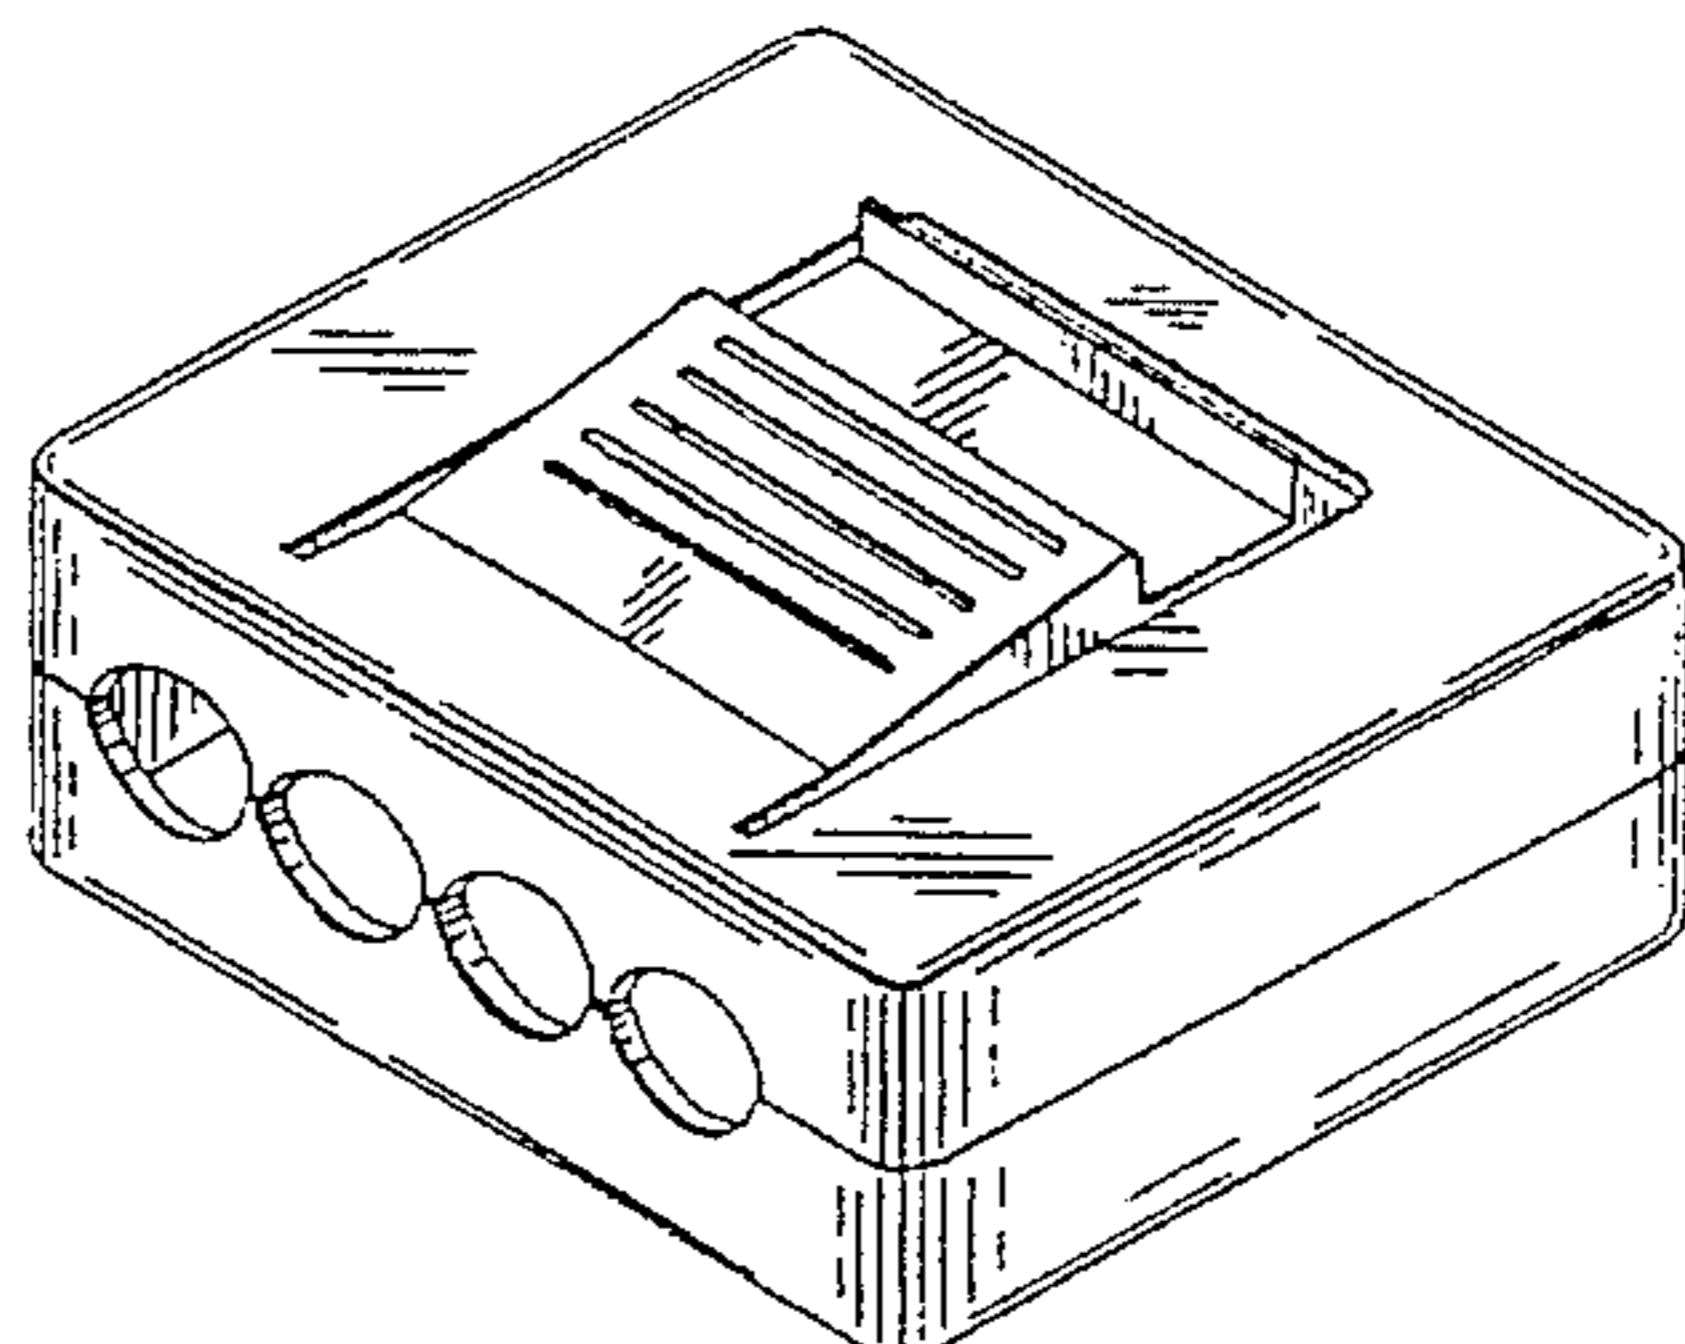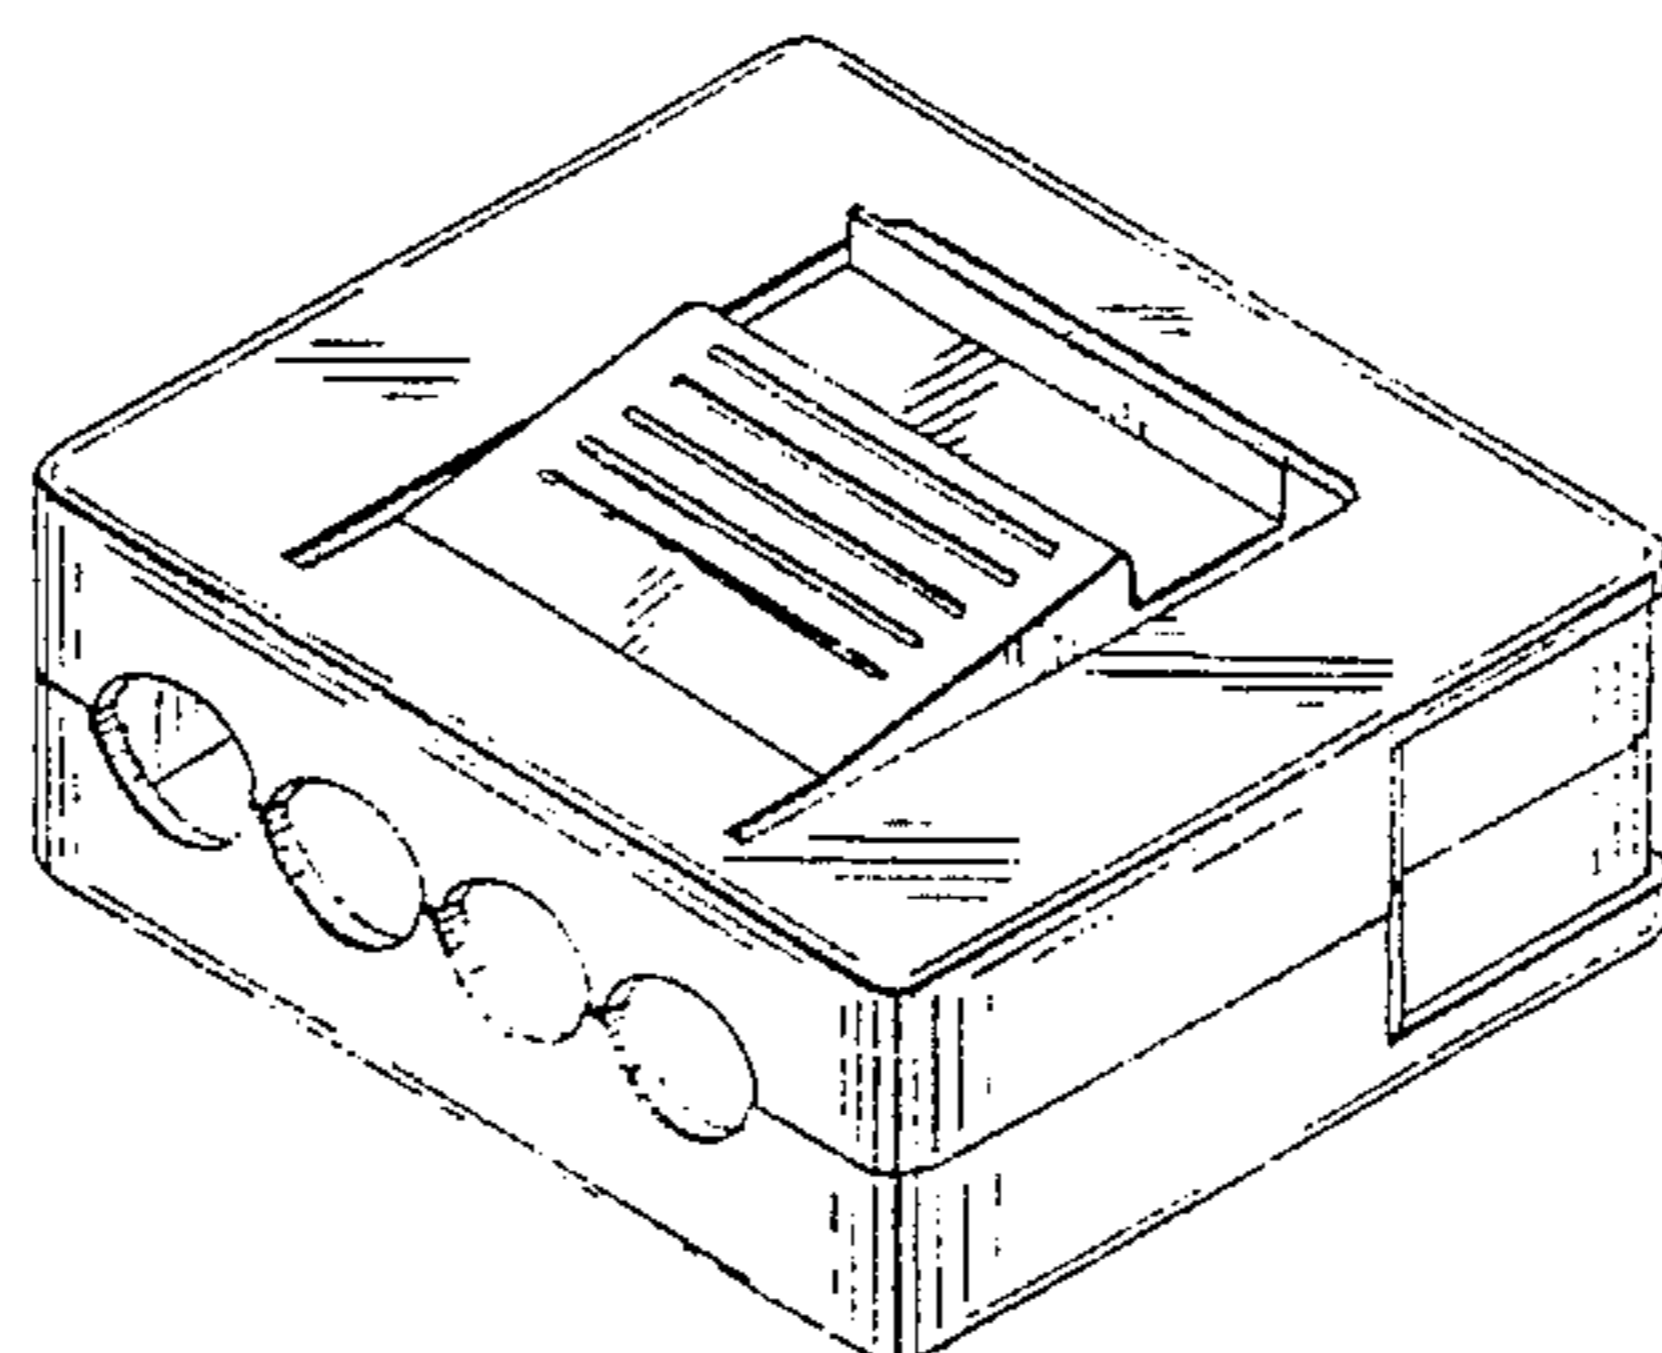

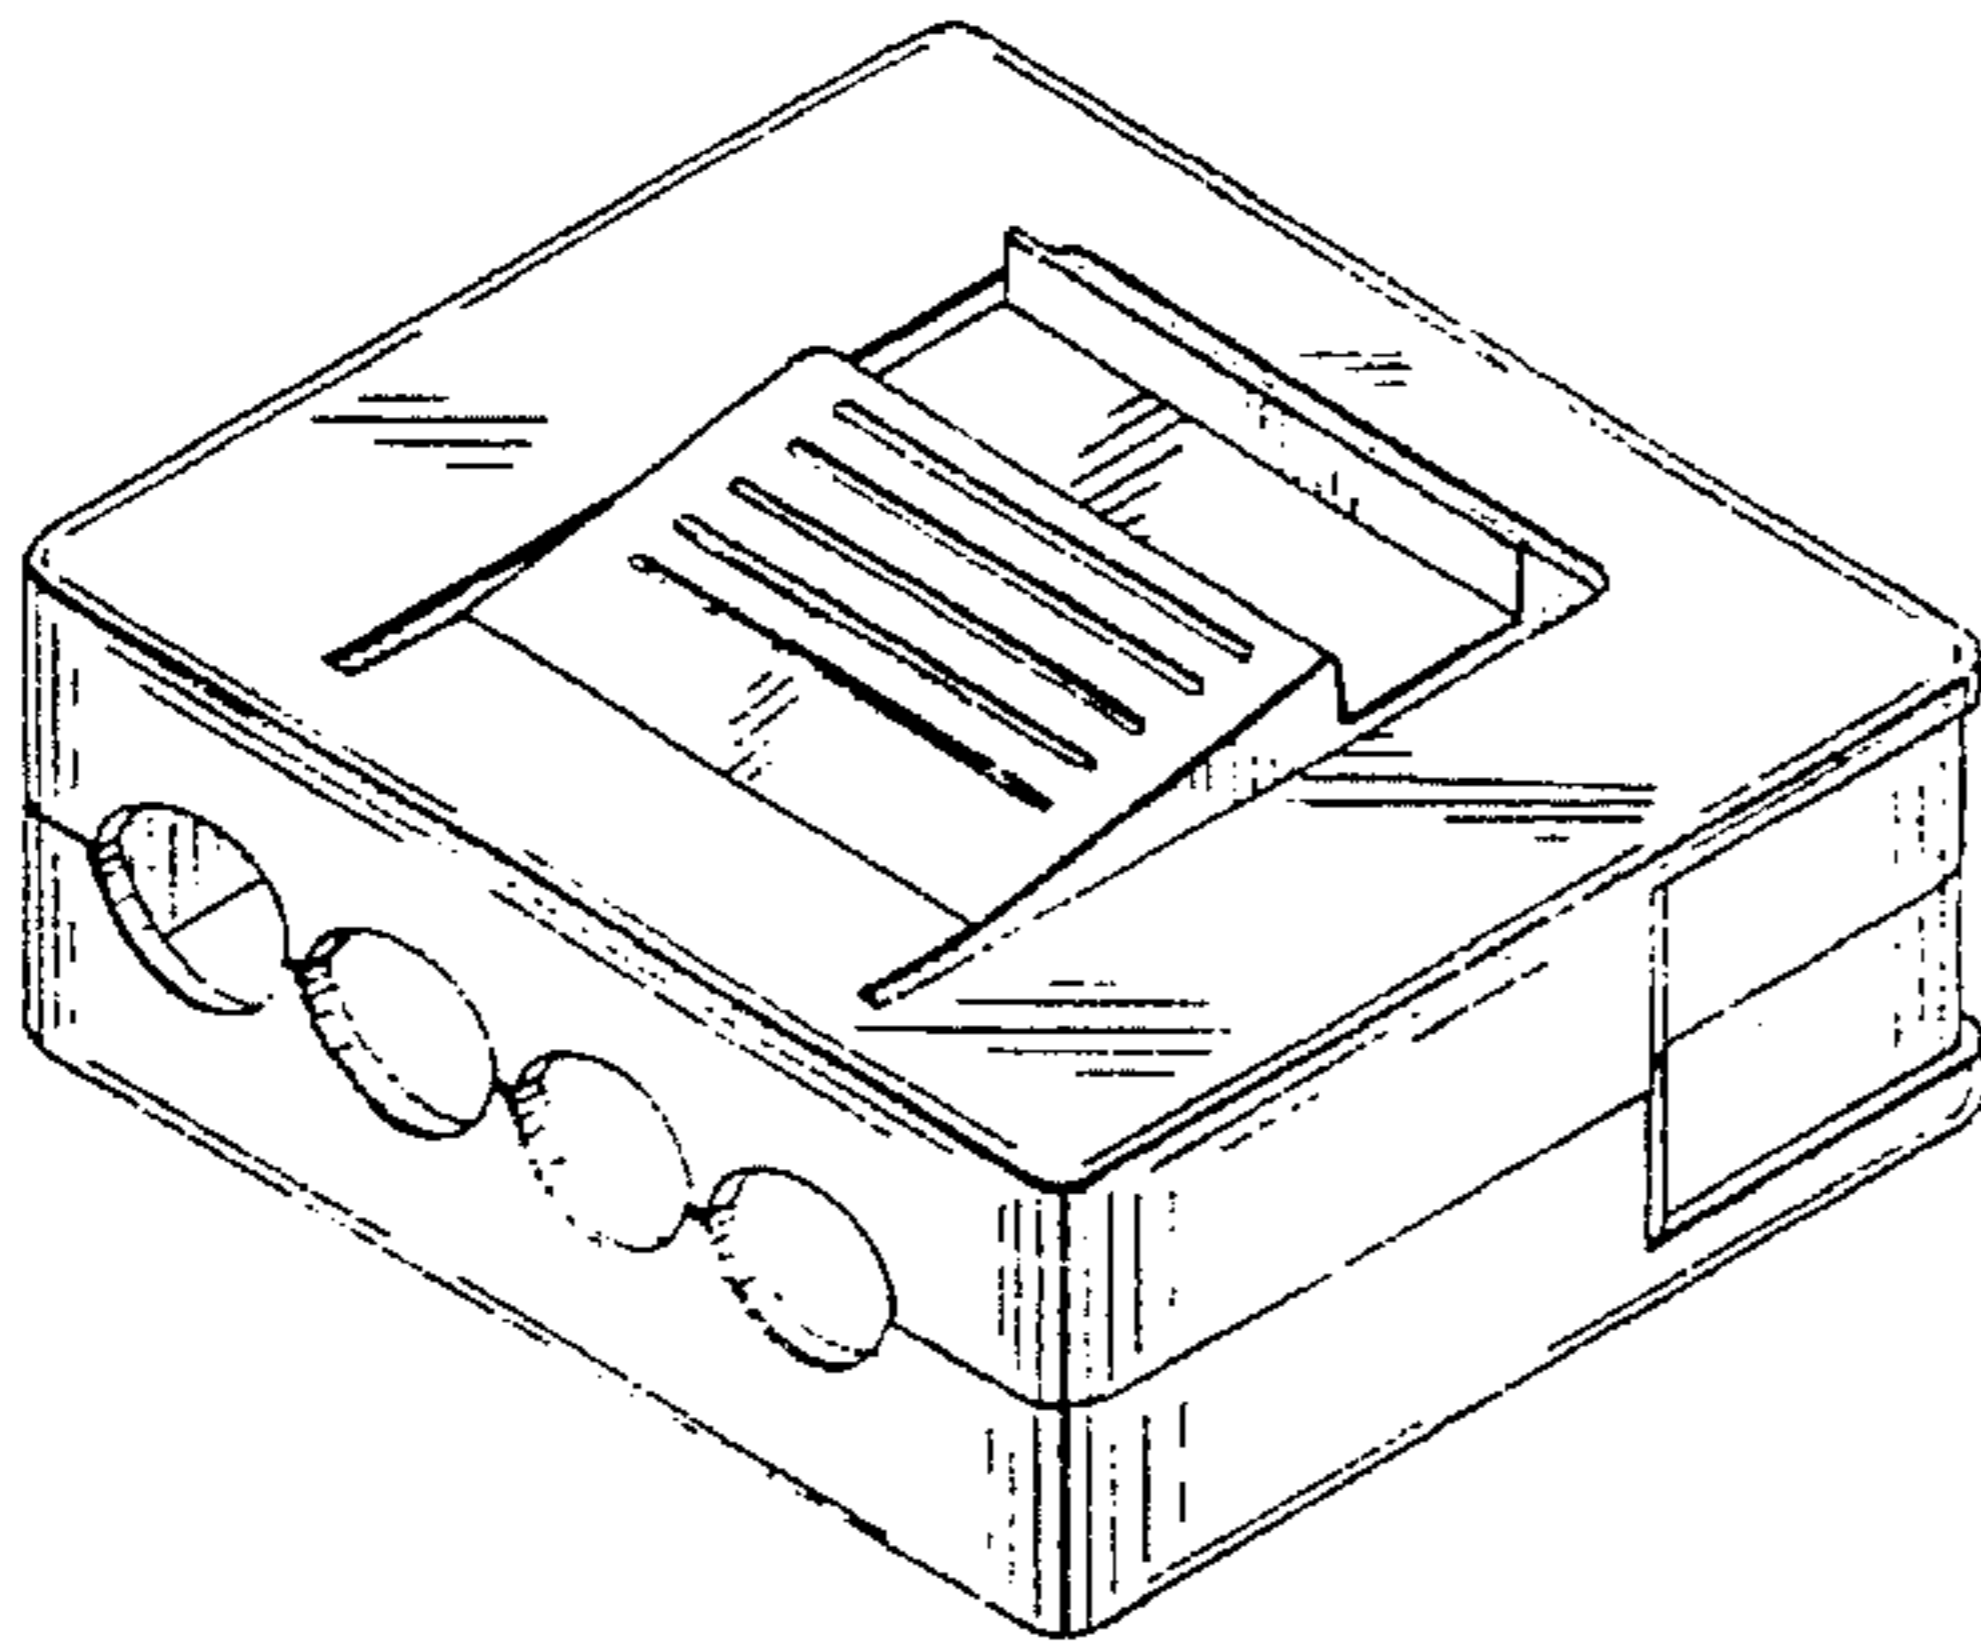


FIG. 1.

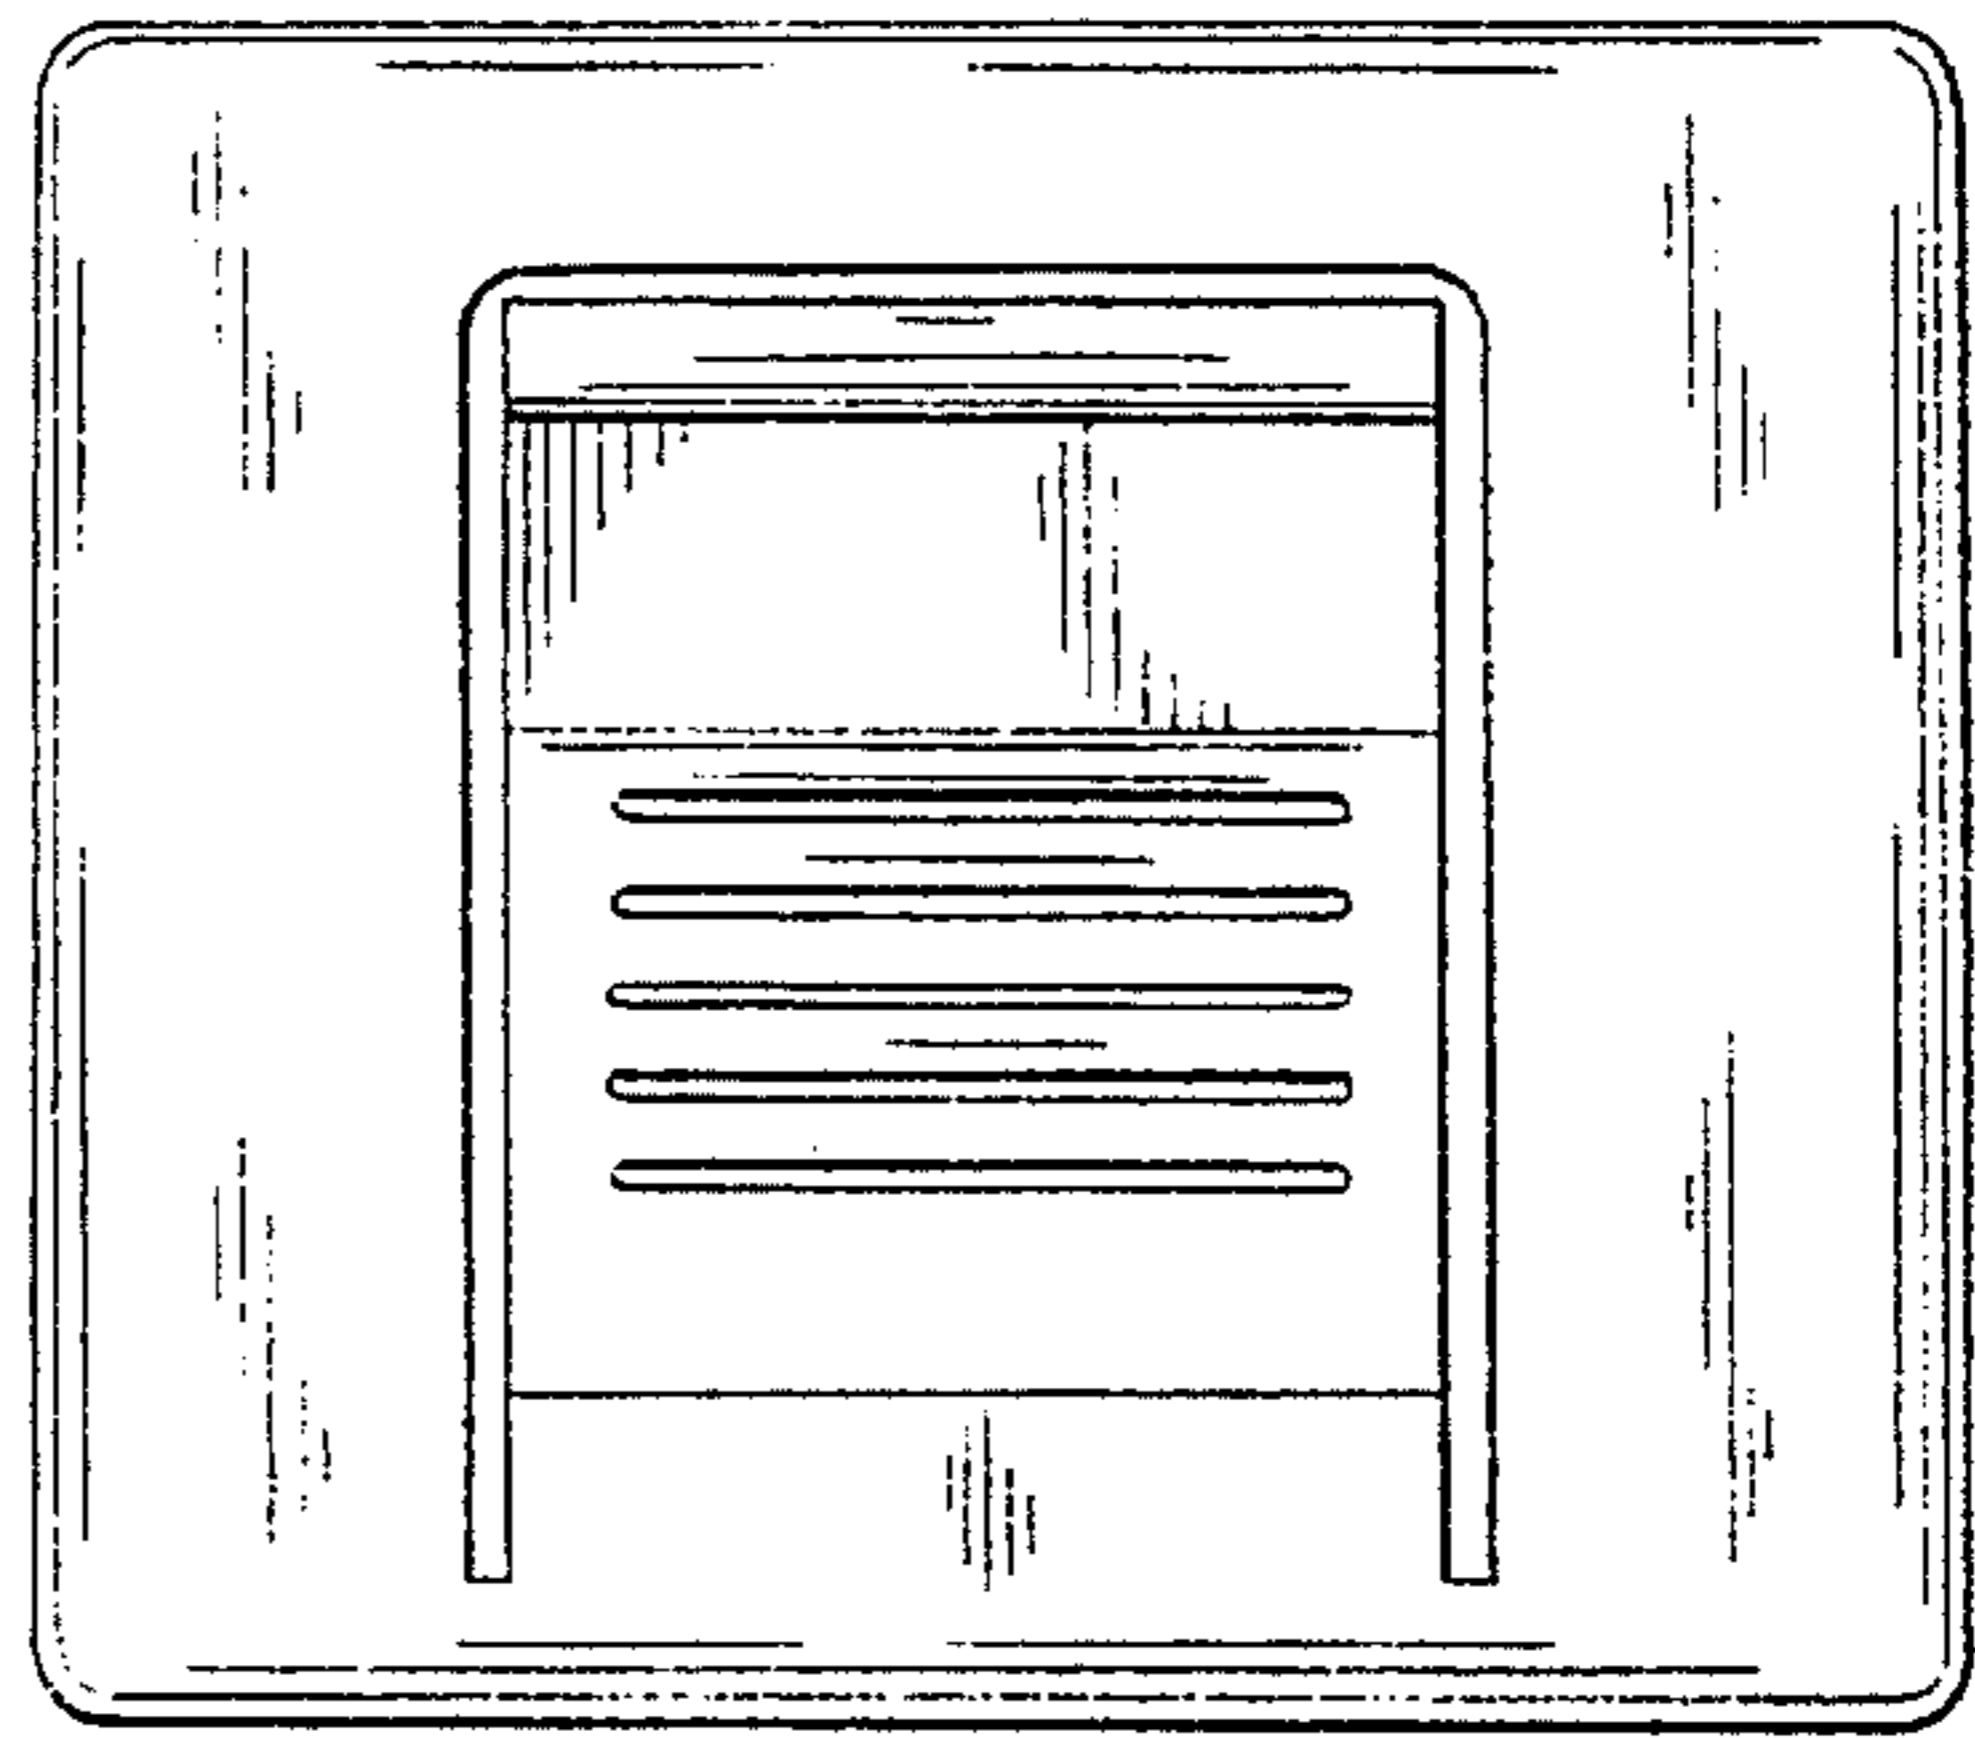


FIG. 2.

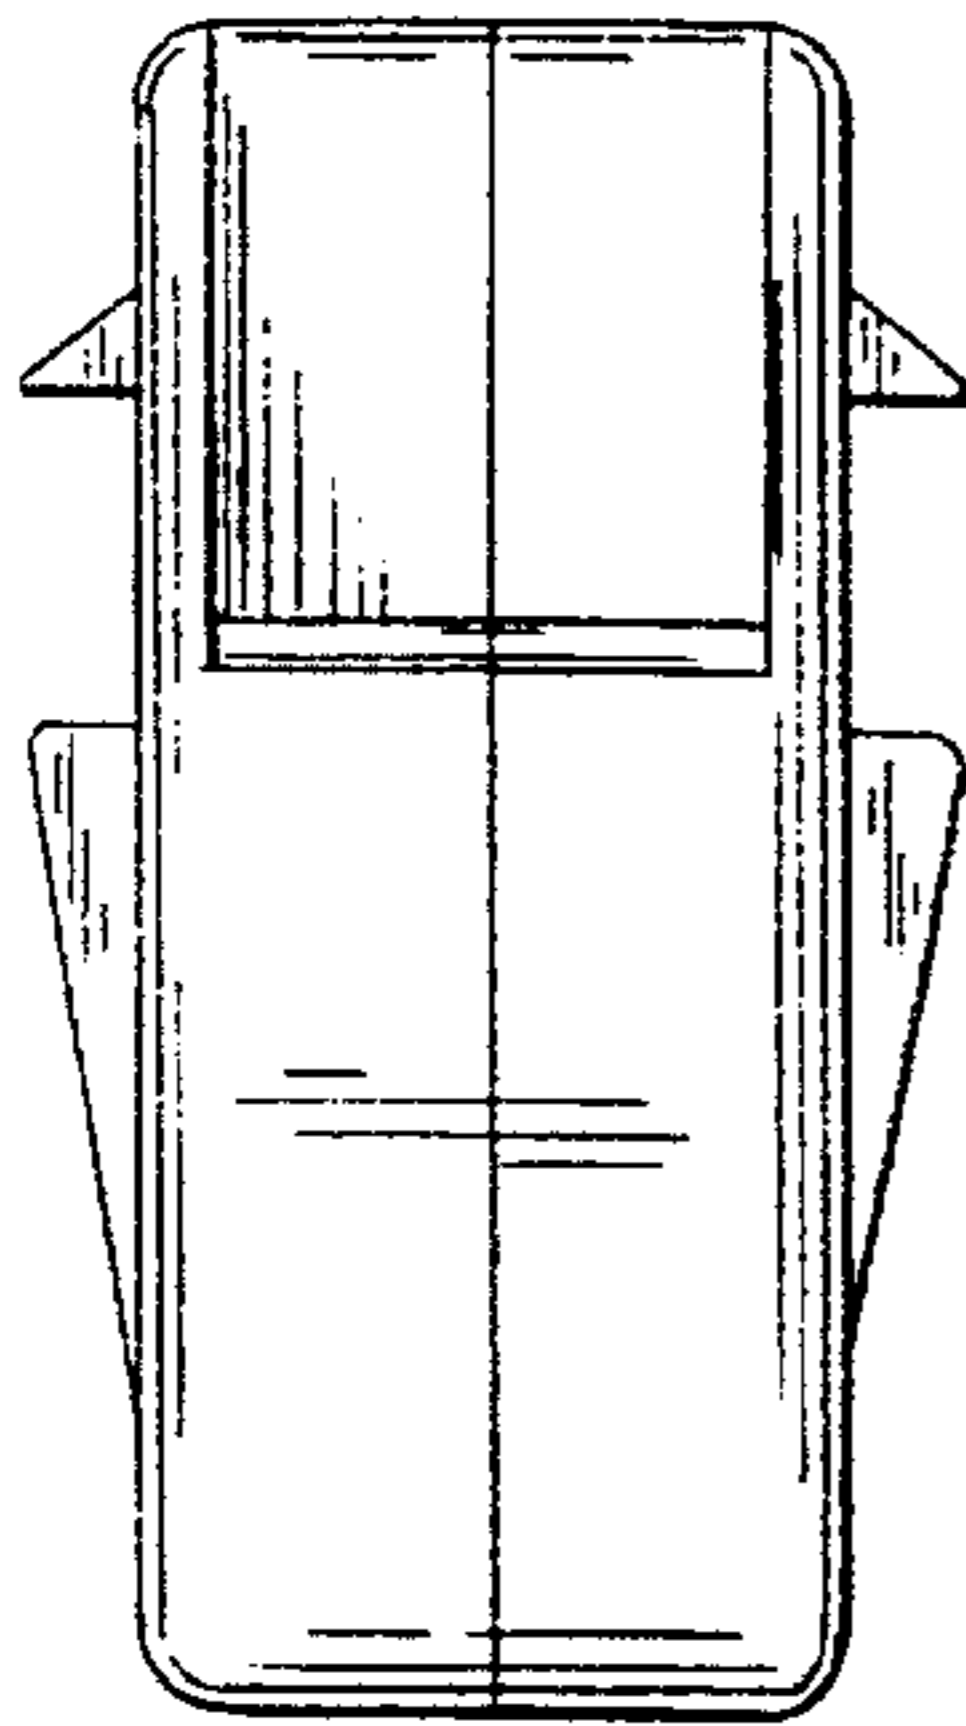


FIG. 3.

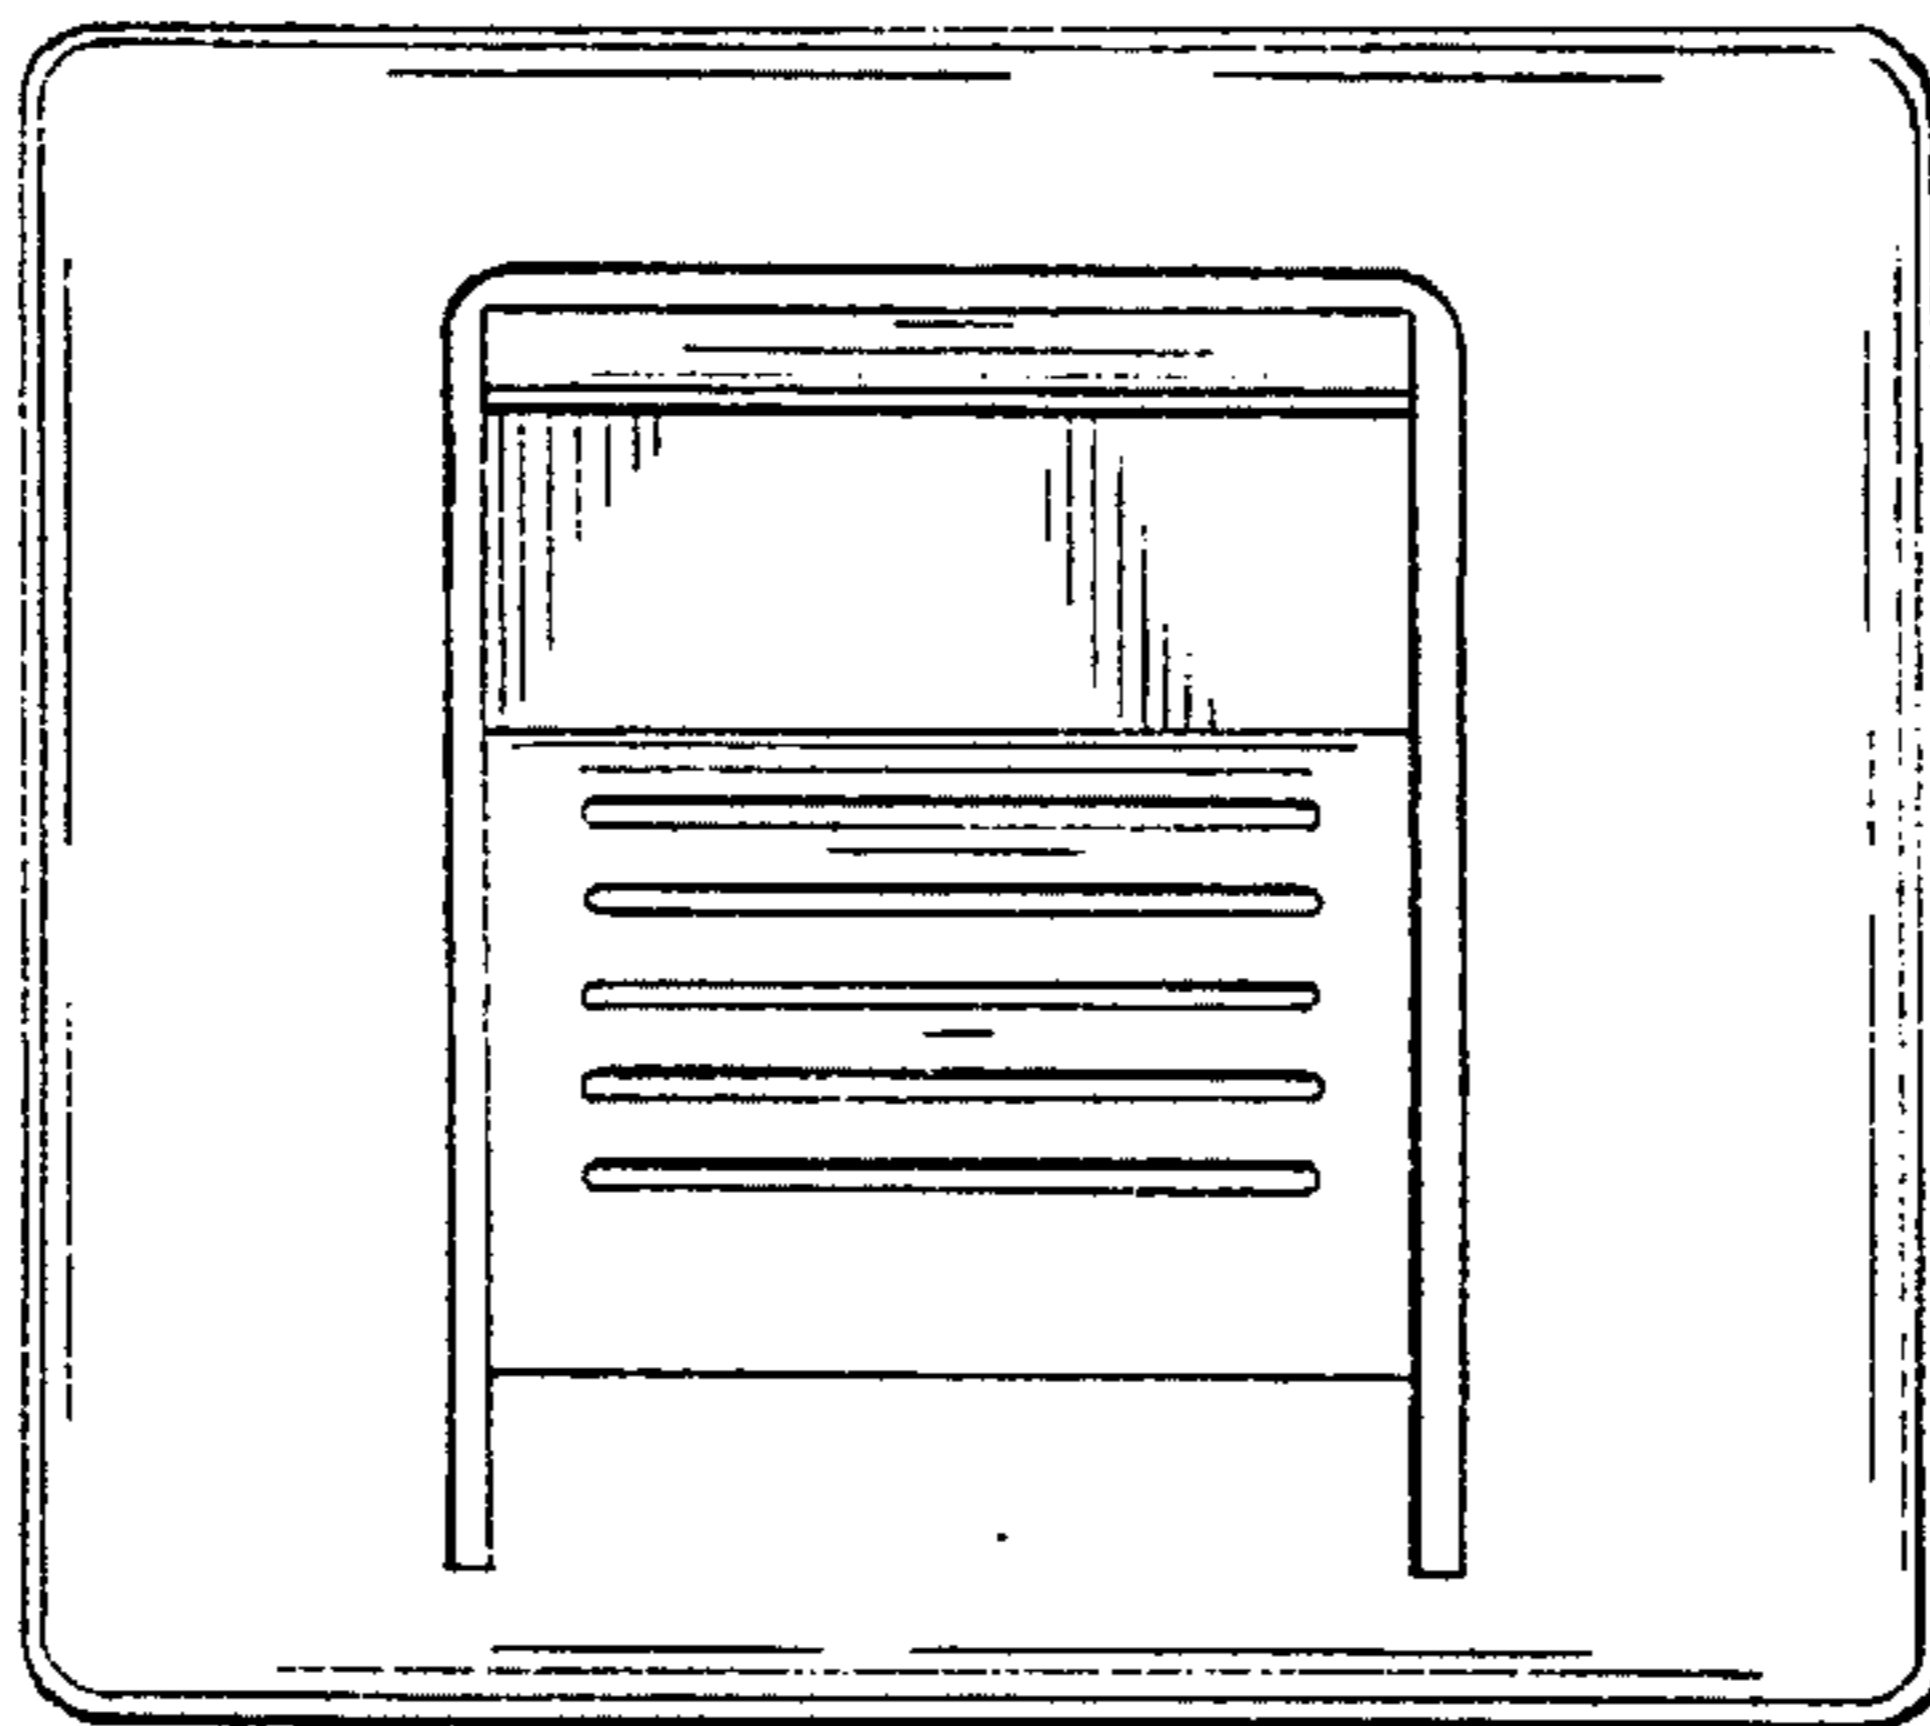


FIG. 4.

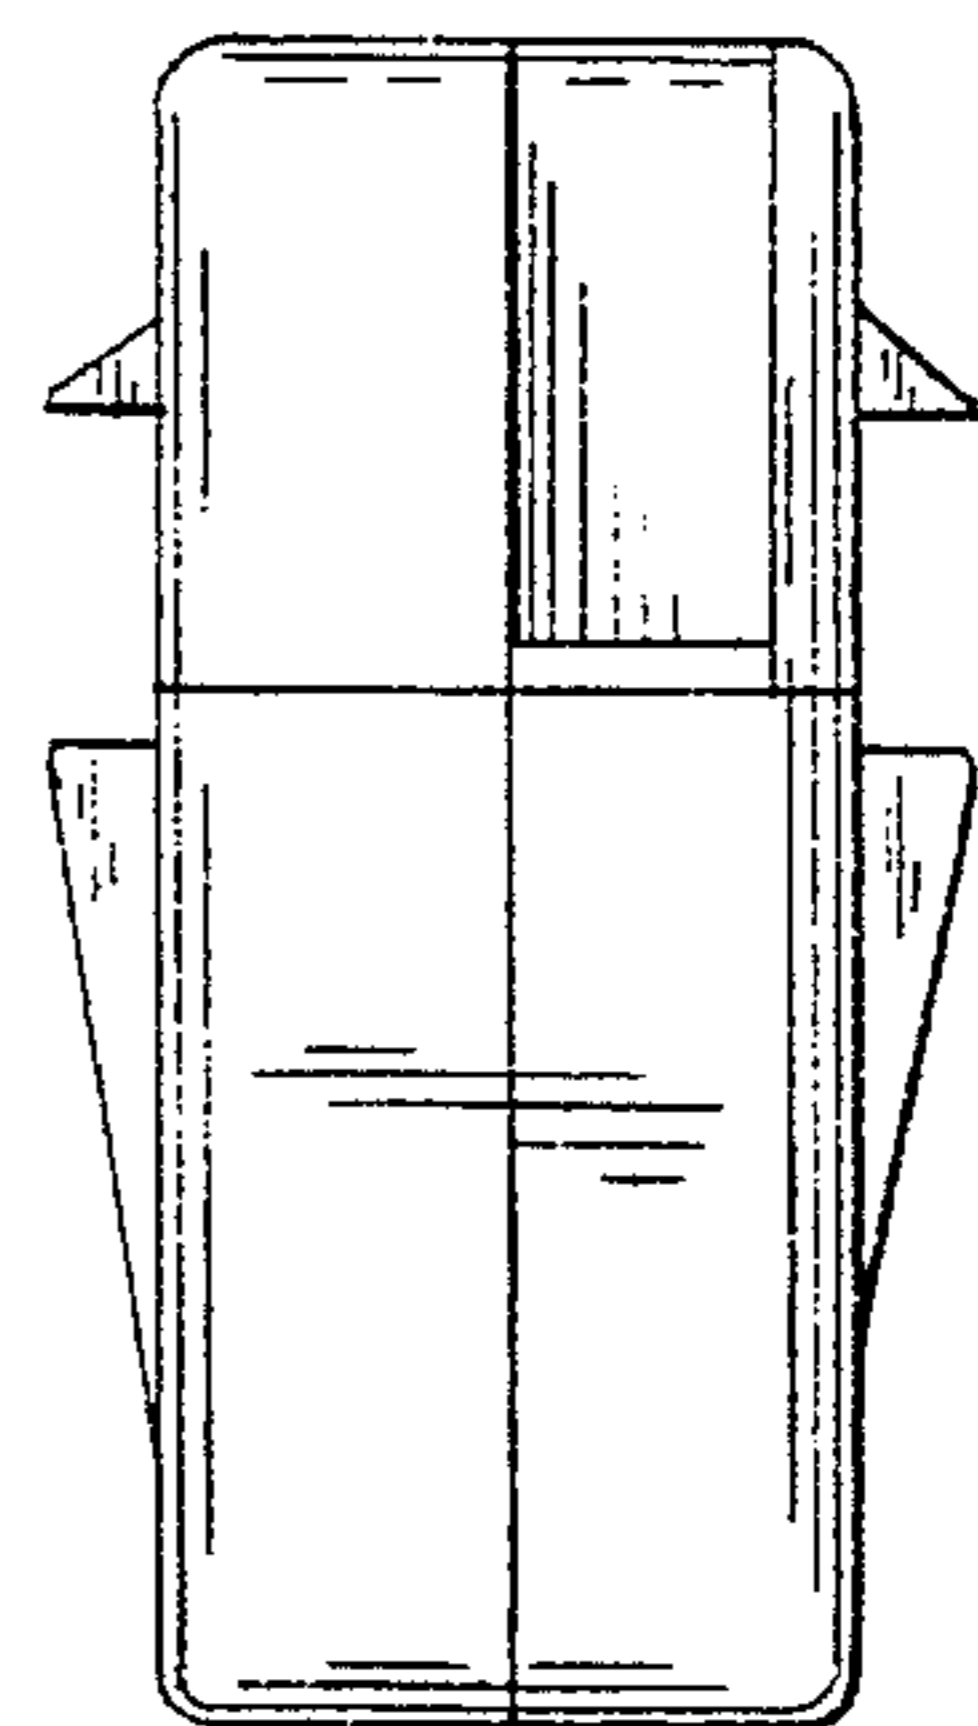


FIG. 5.

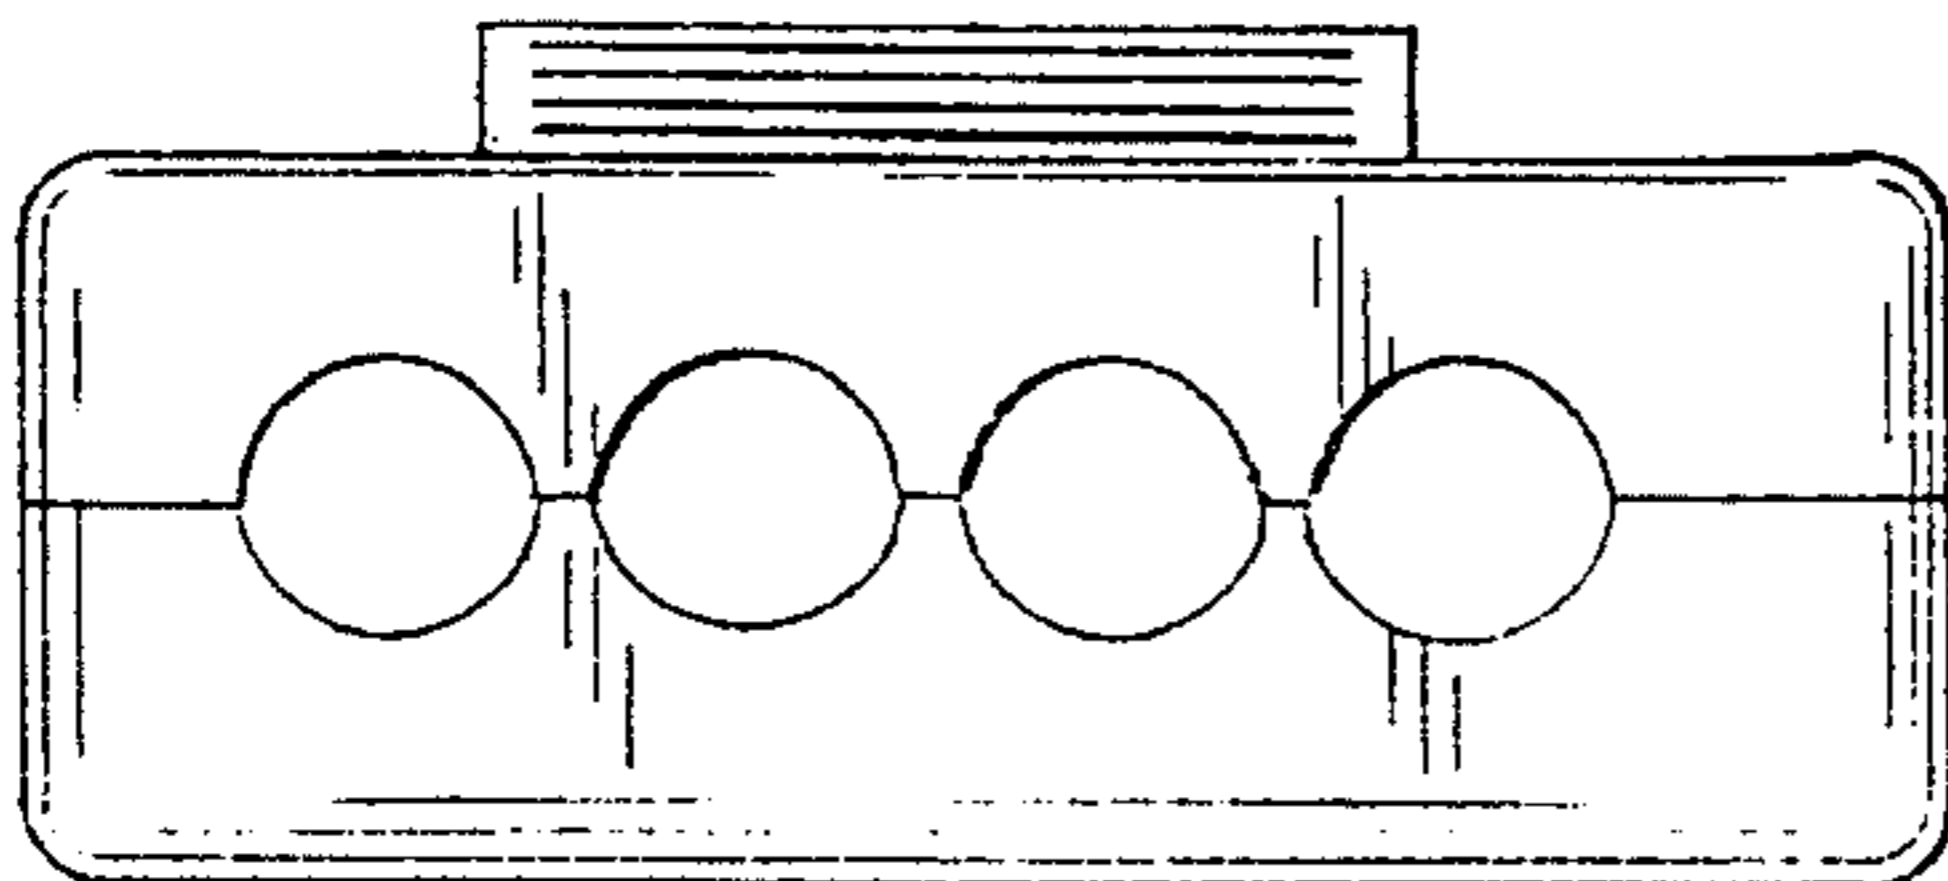


FIG. 6.

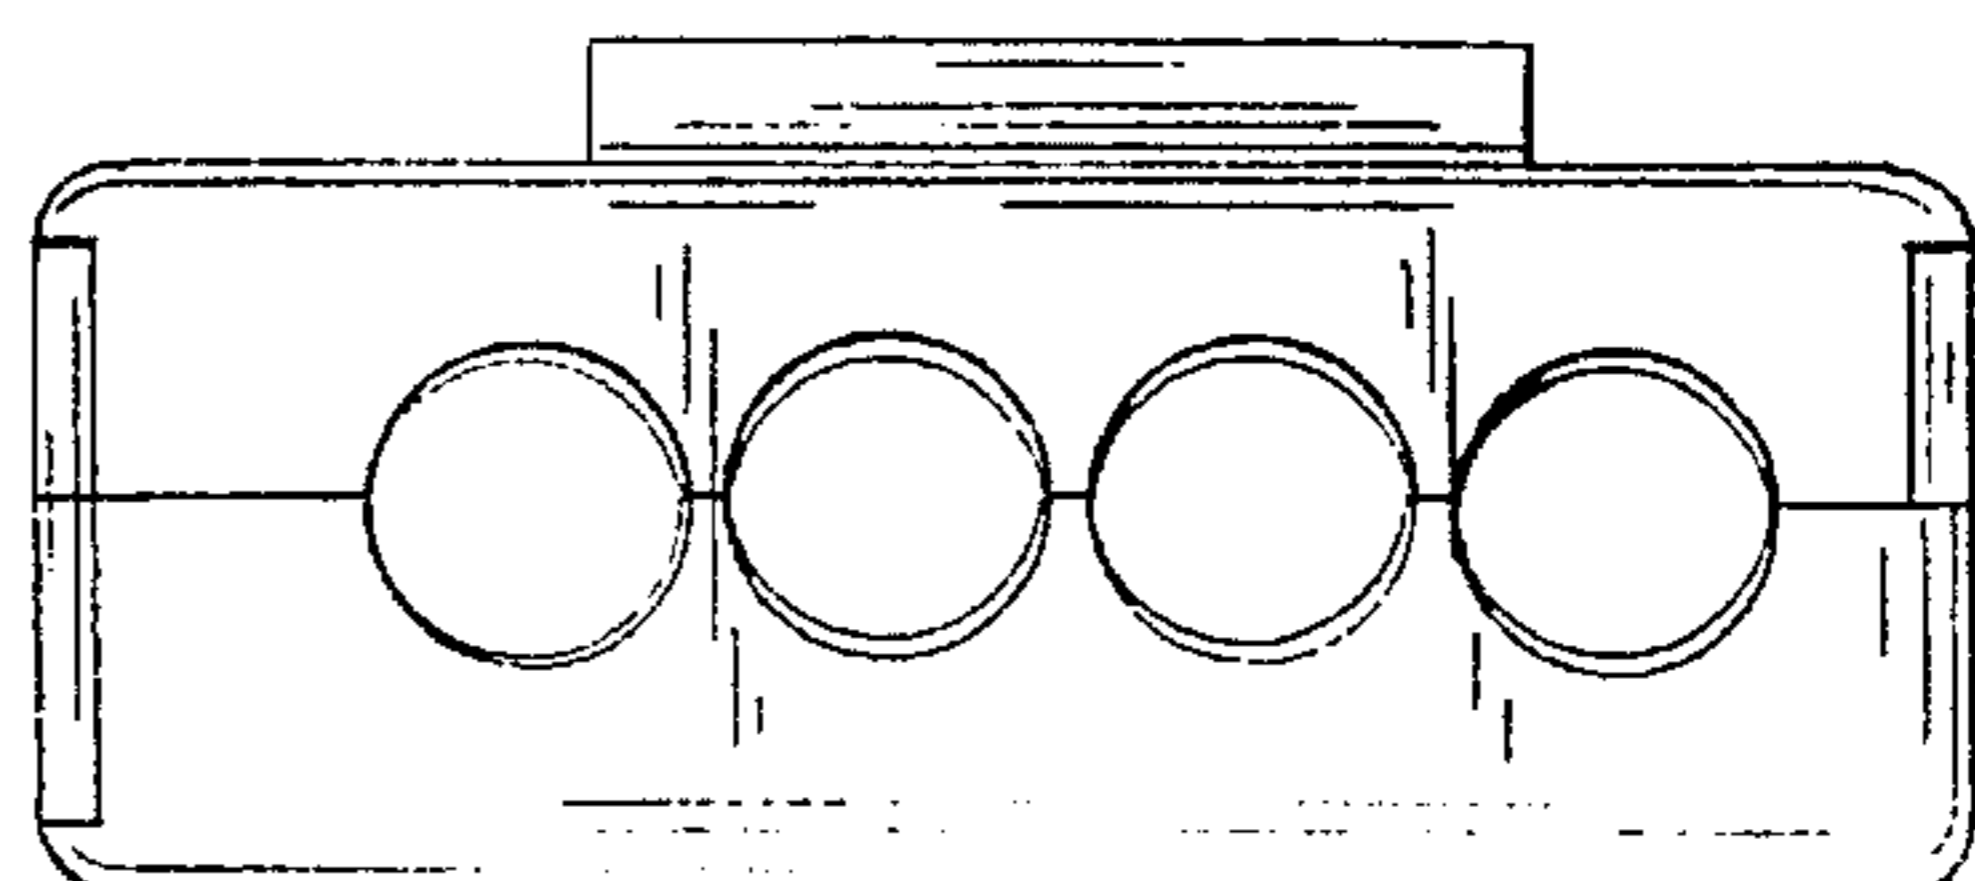


FIG. 7.

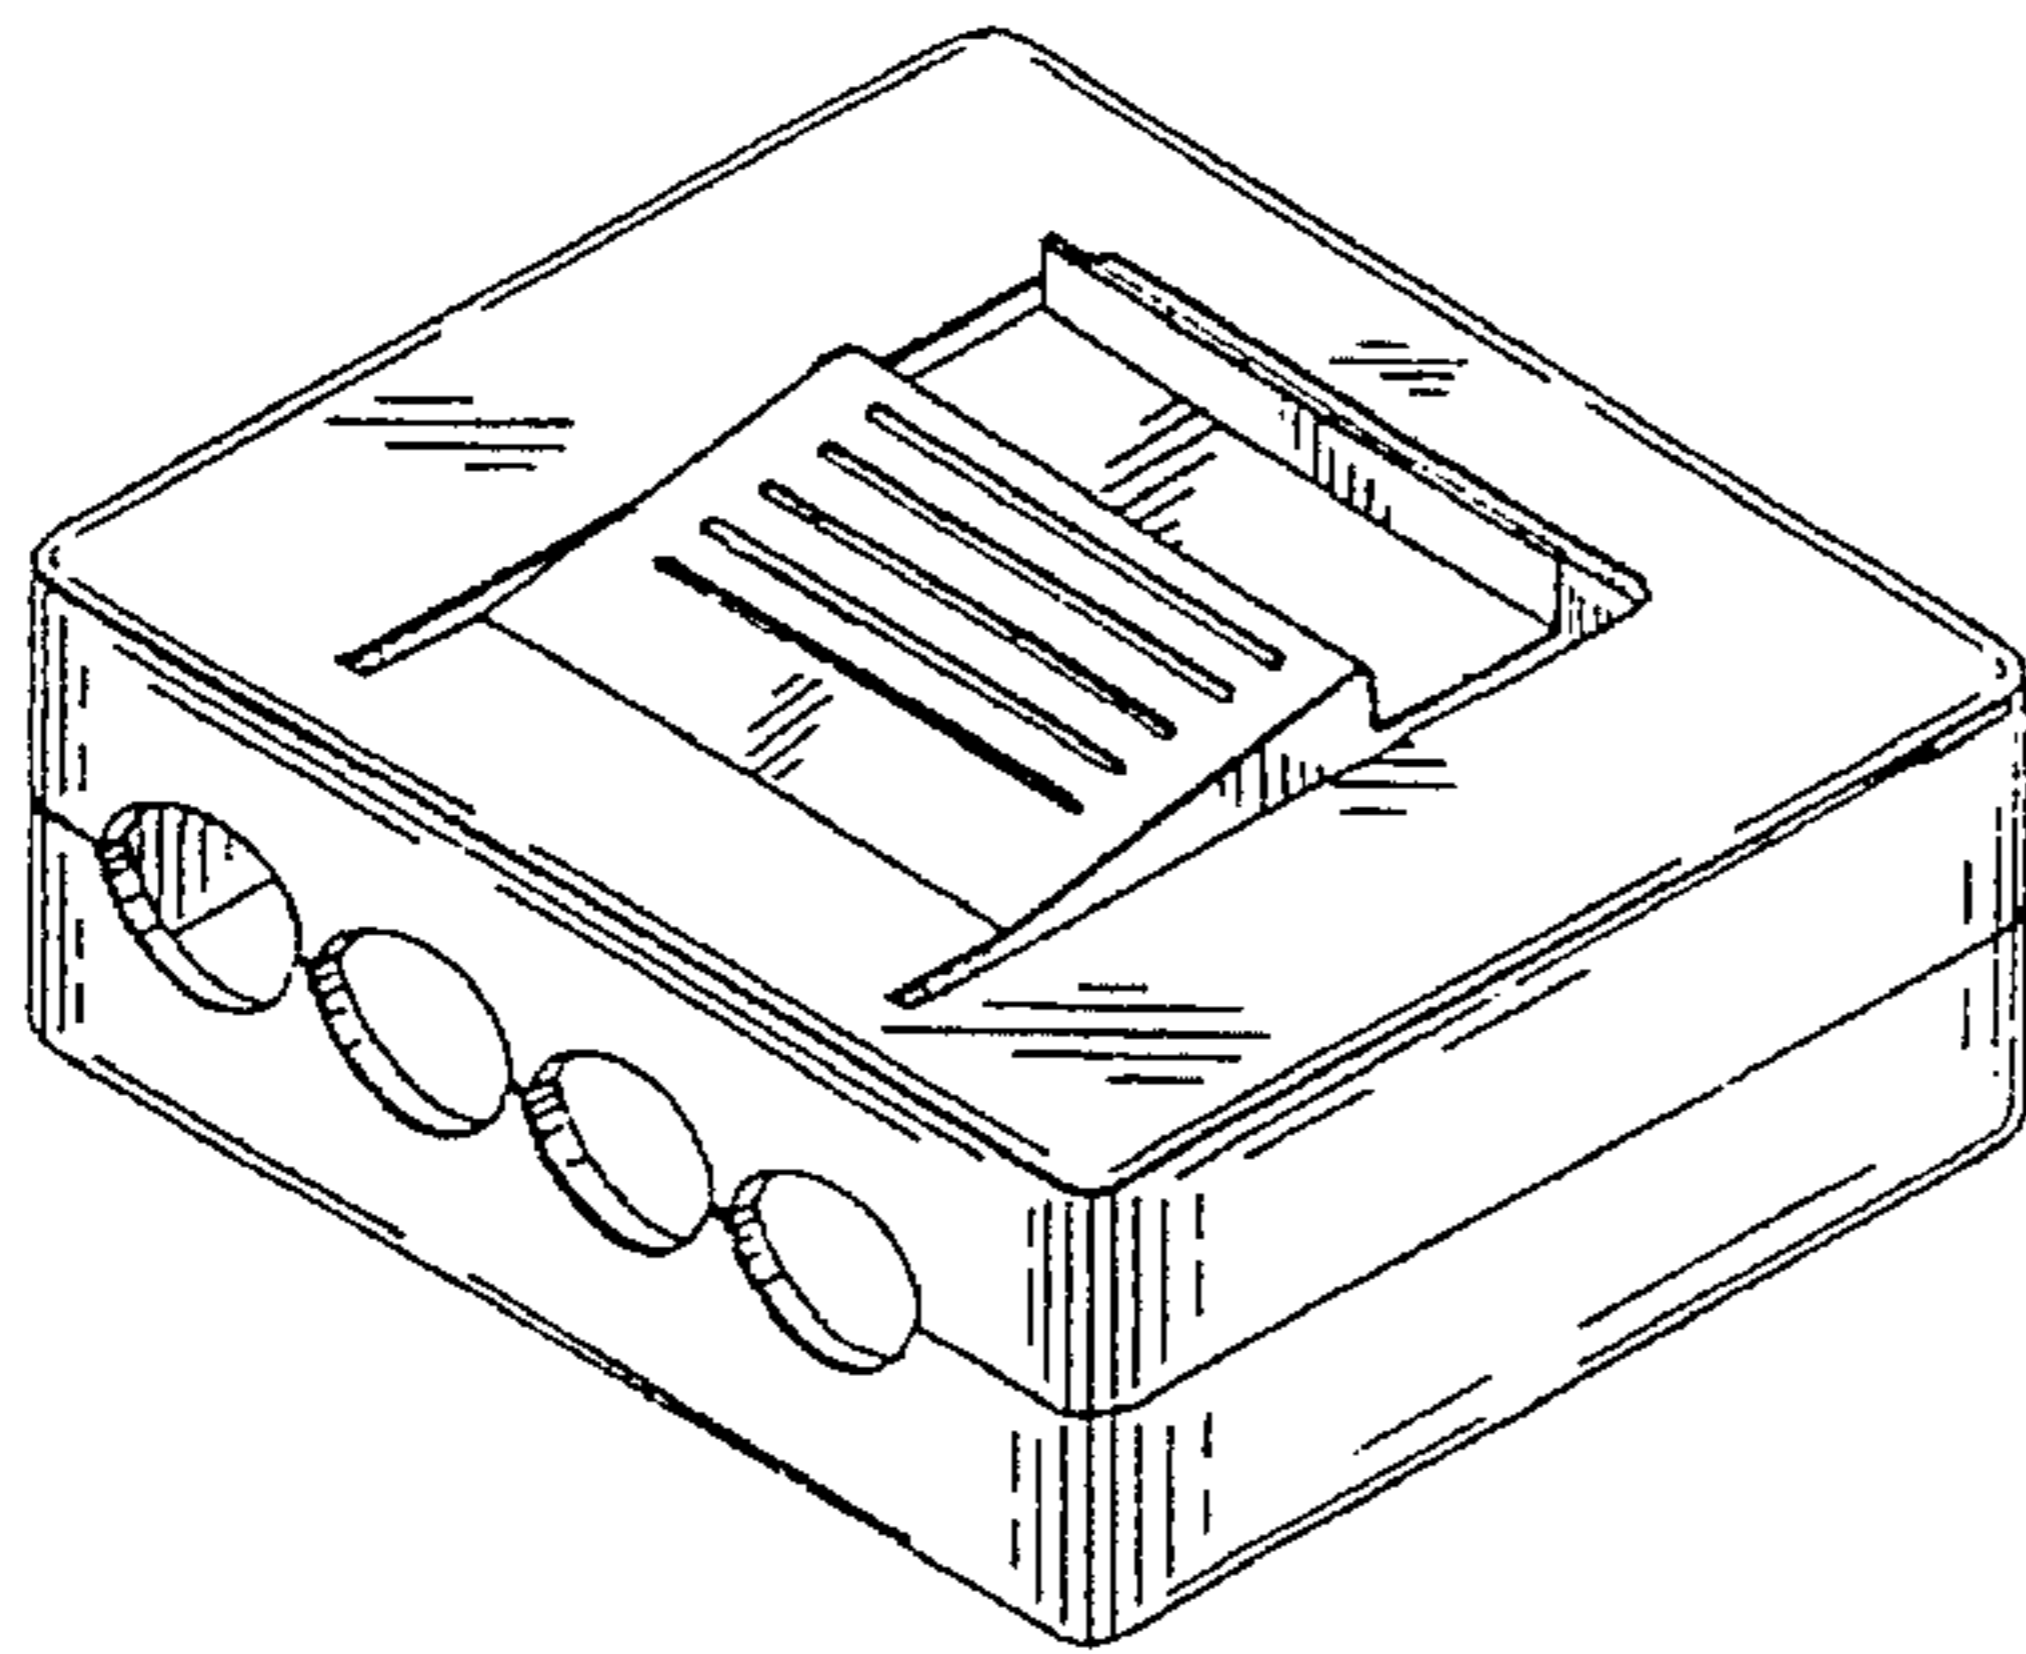


FIG. 8.

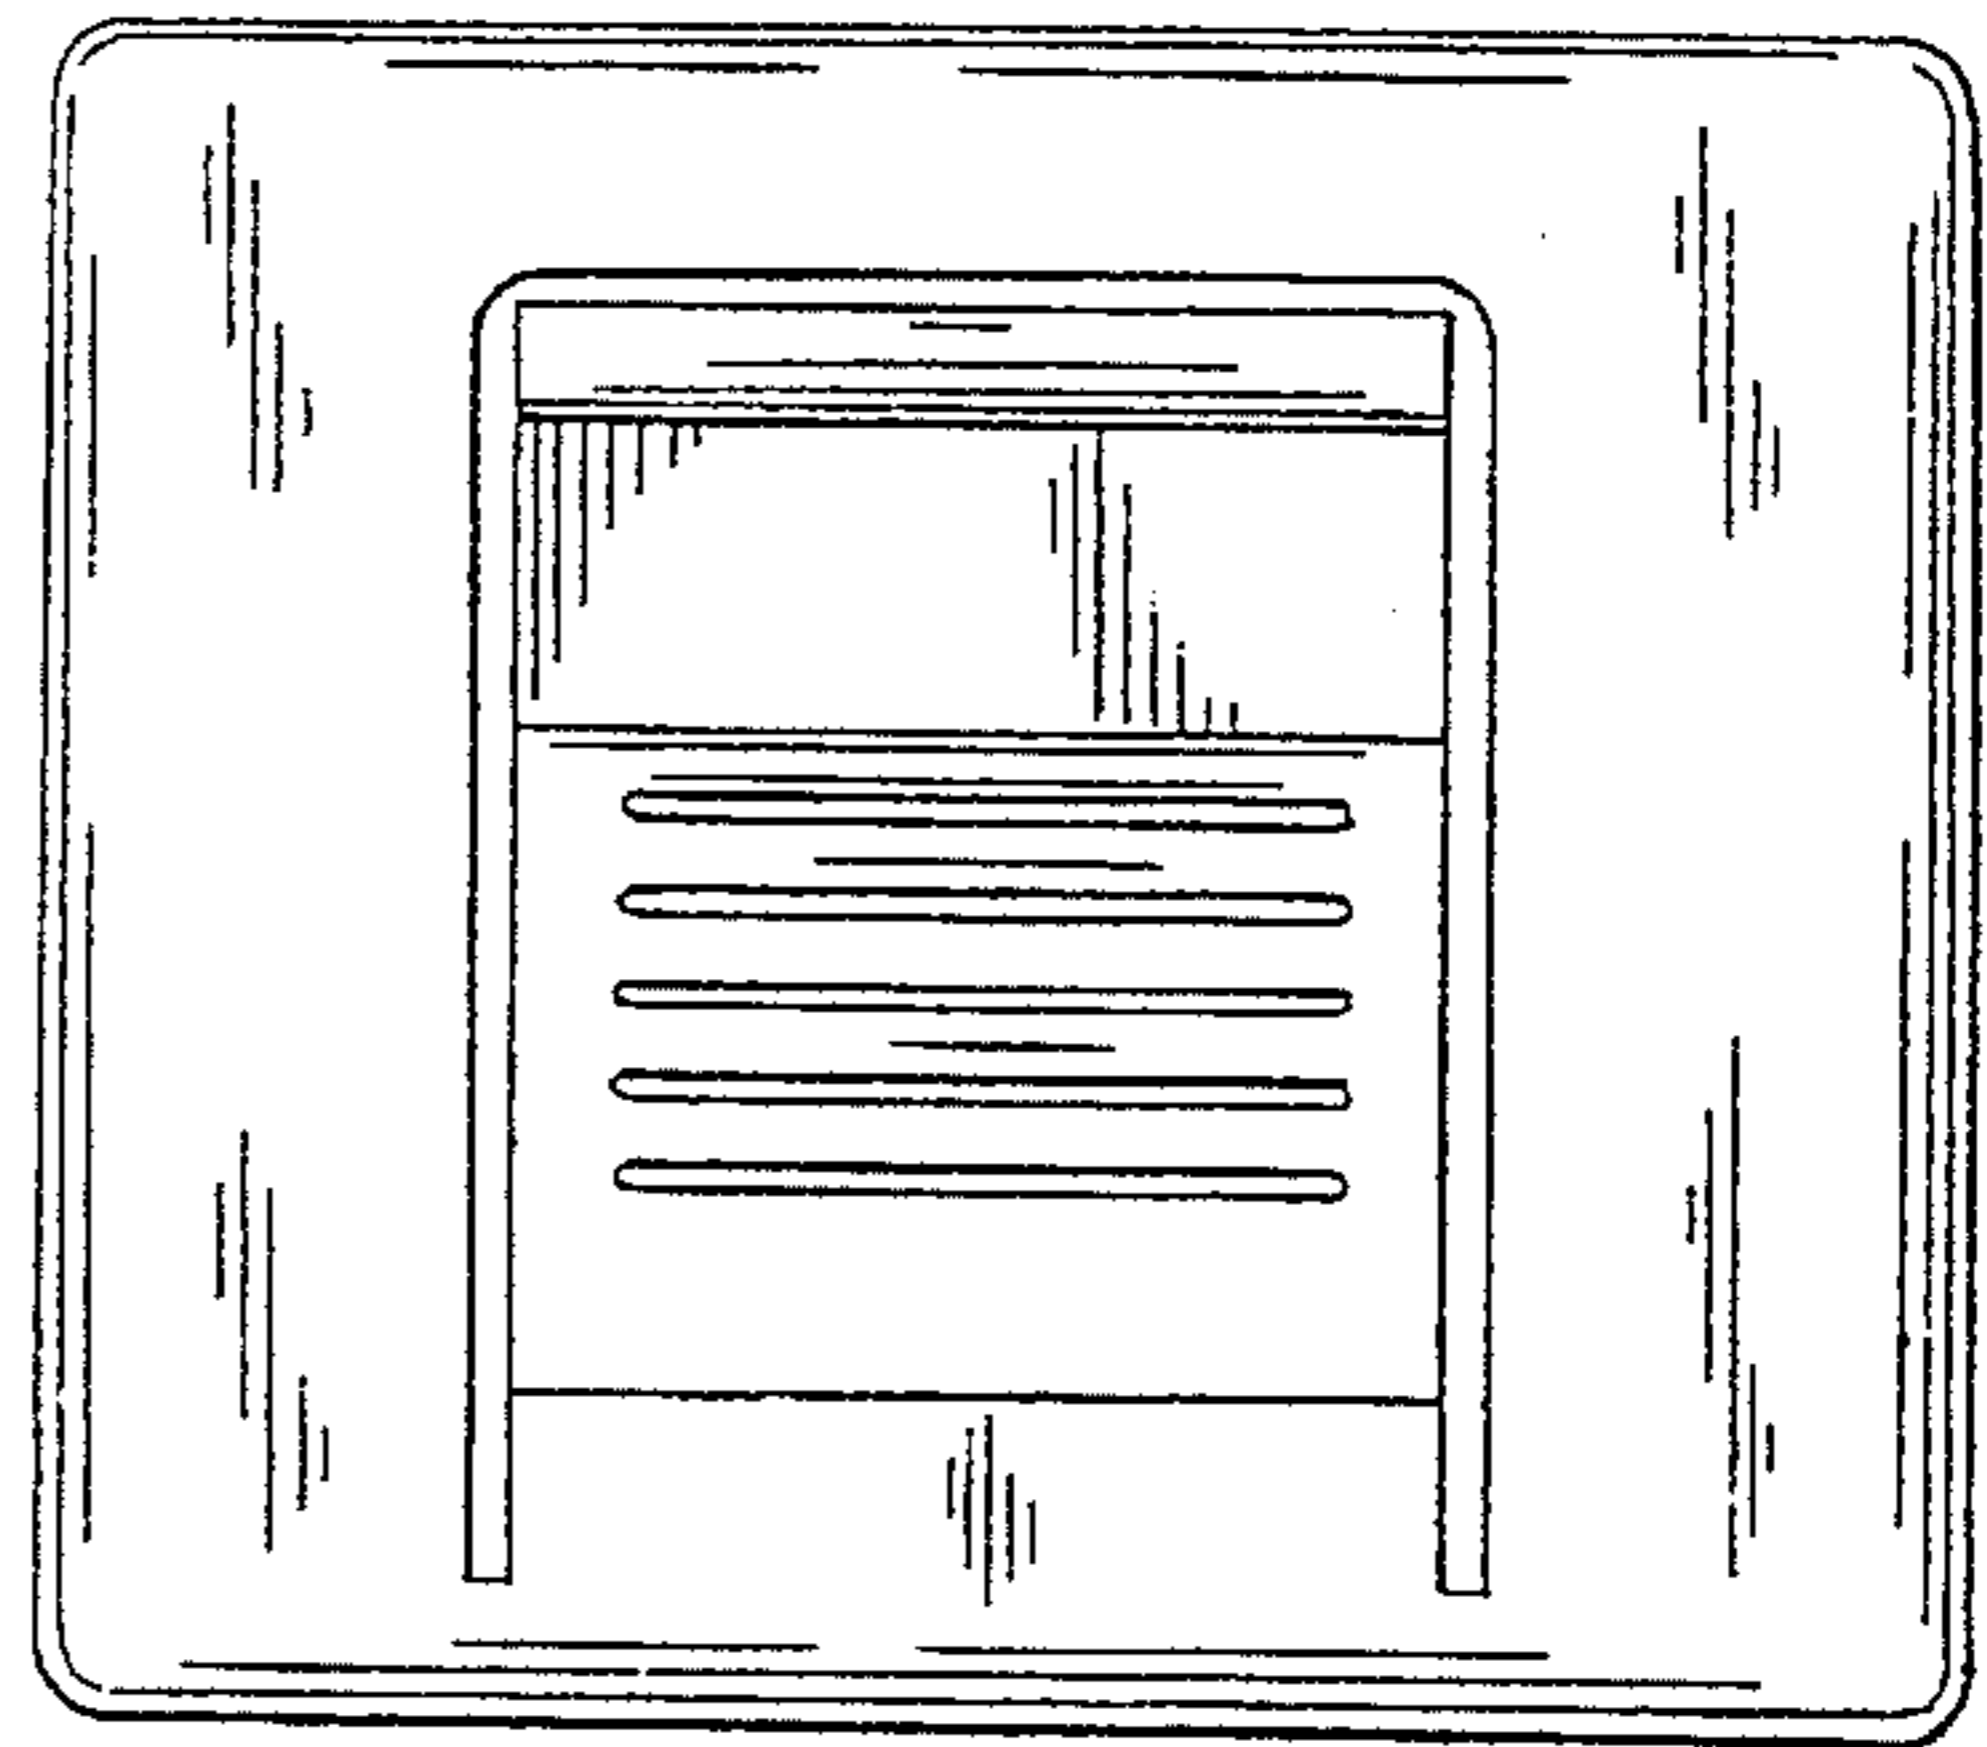


FIG. 9.

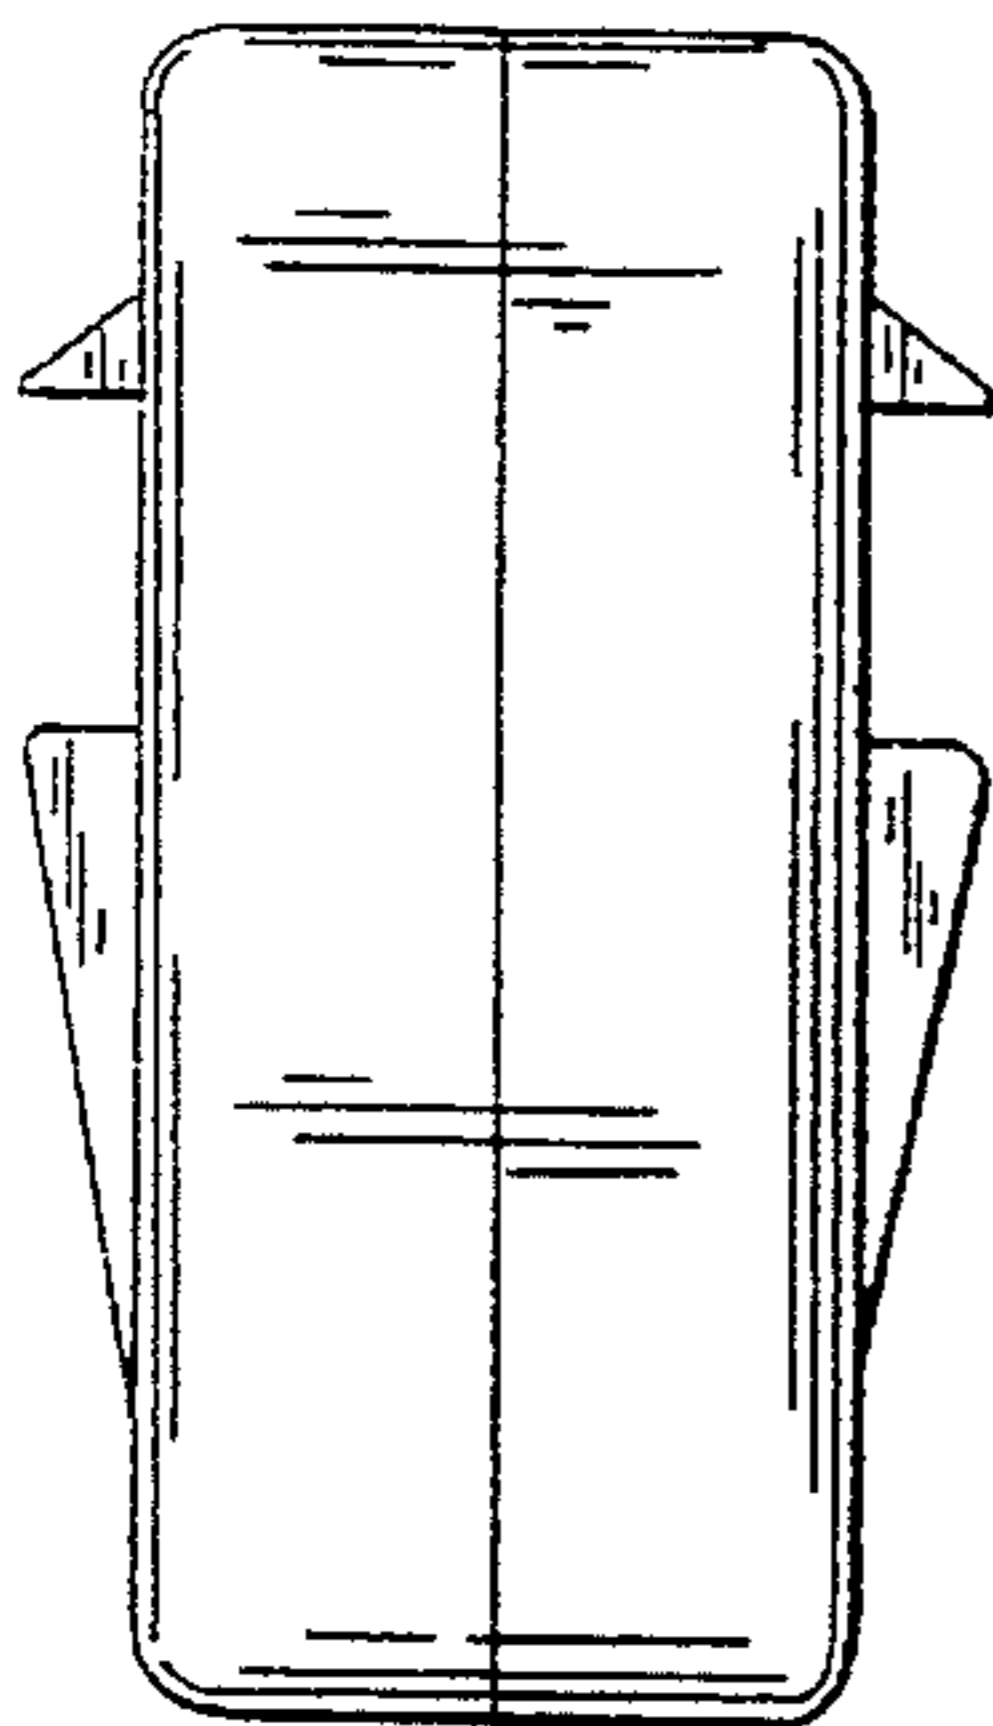


FIG. 10.

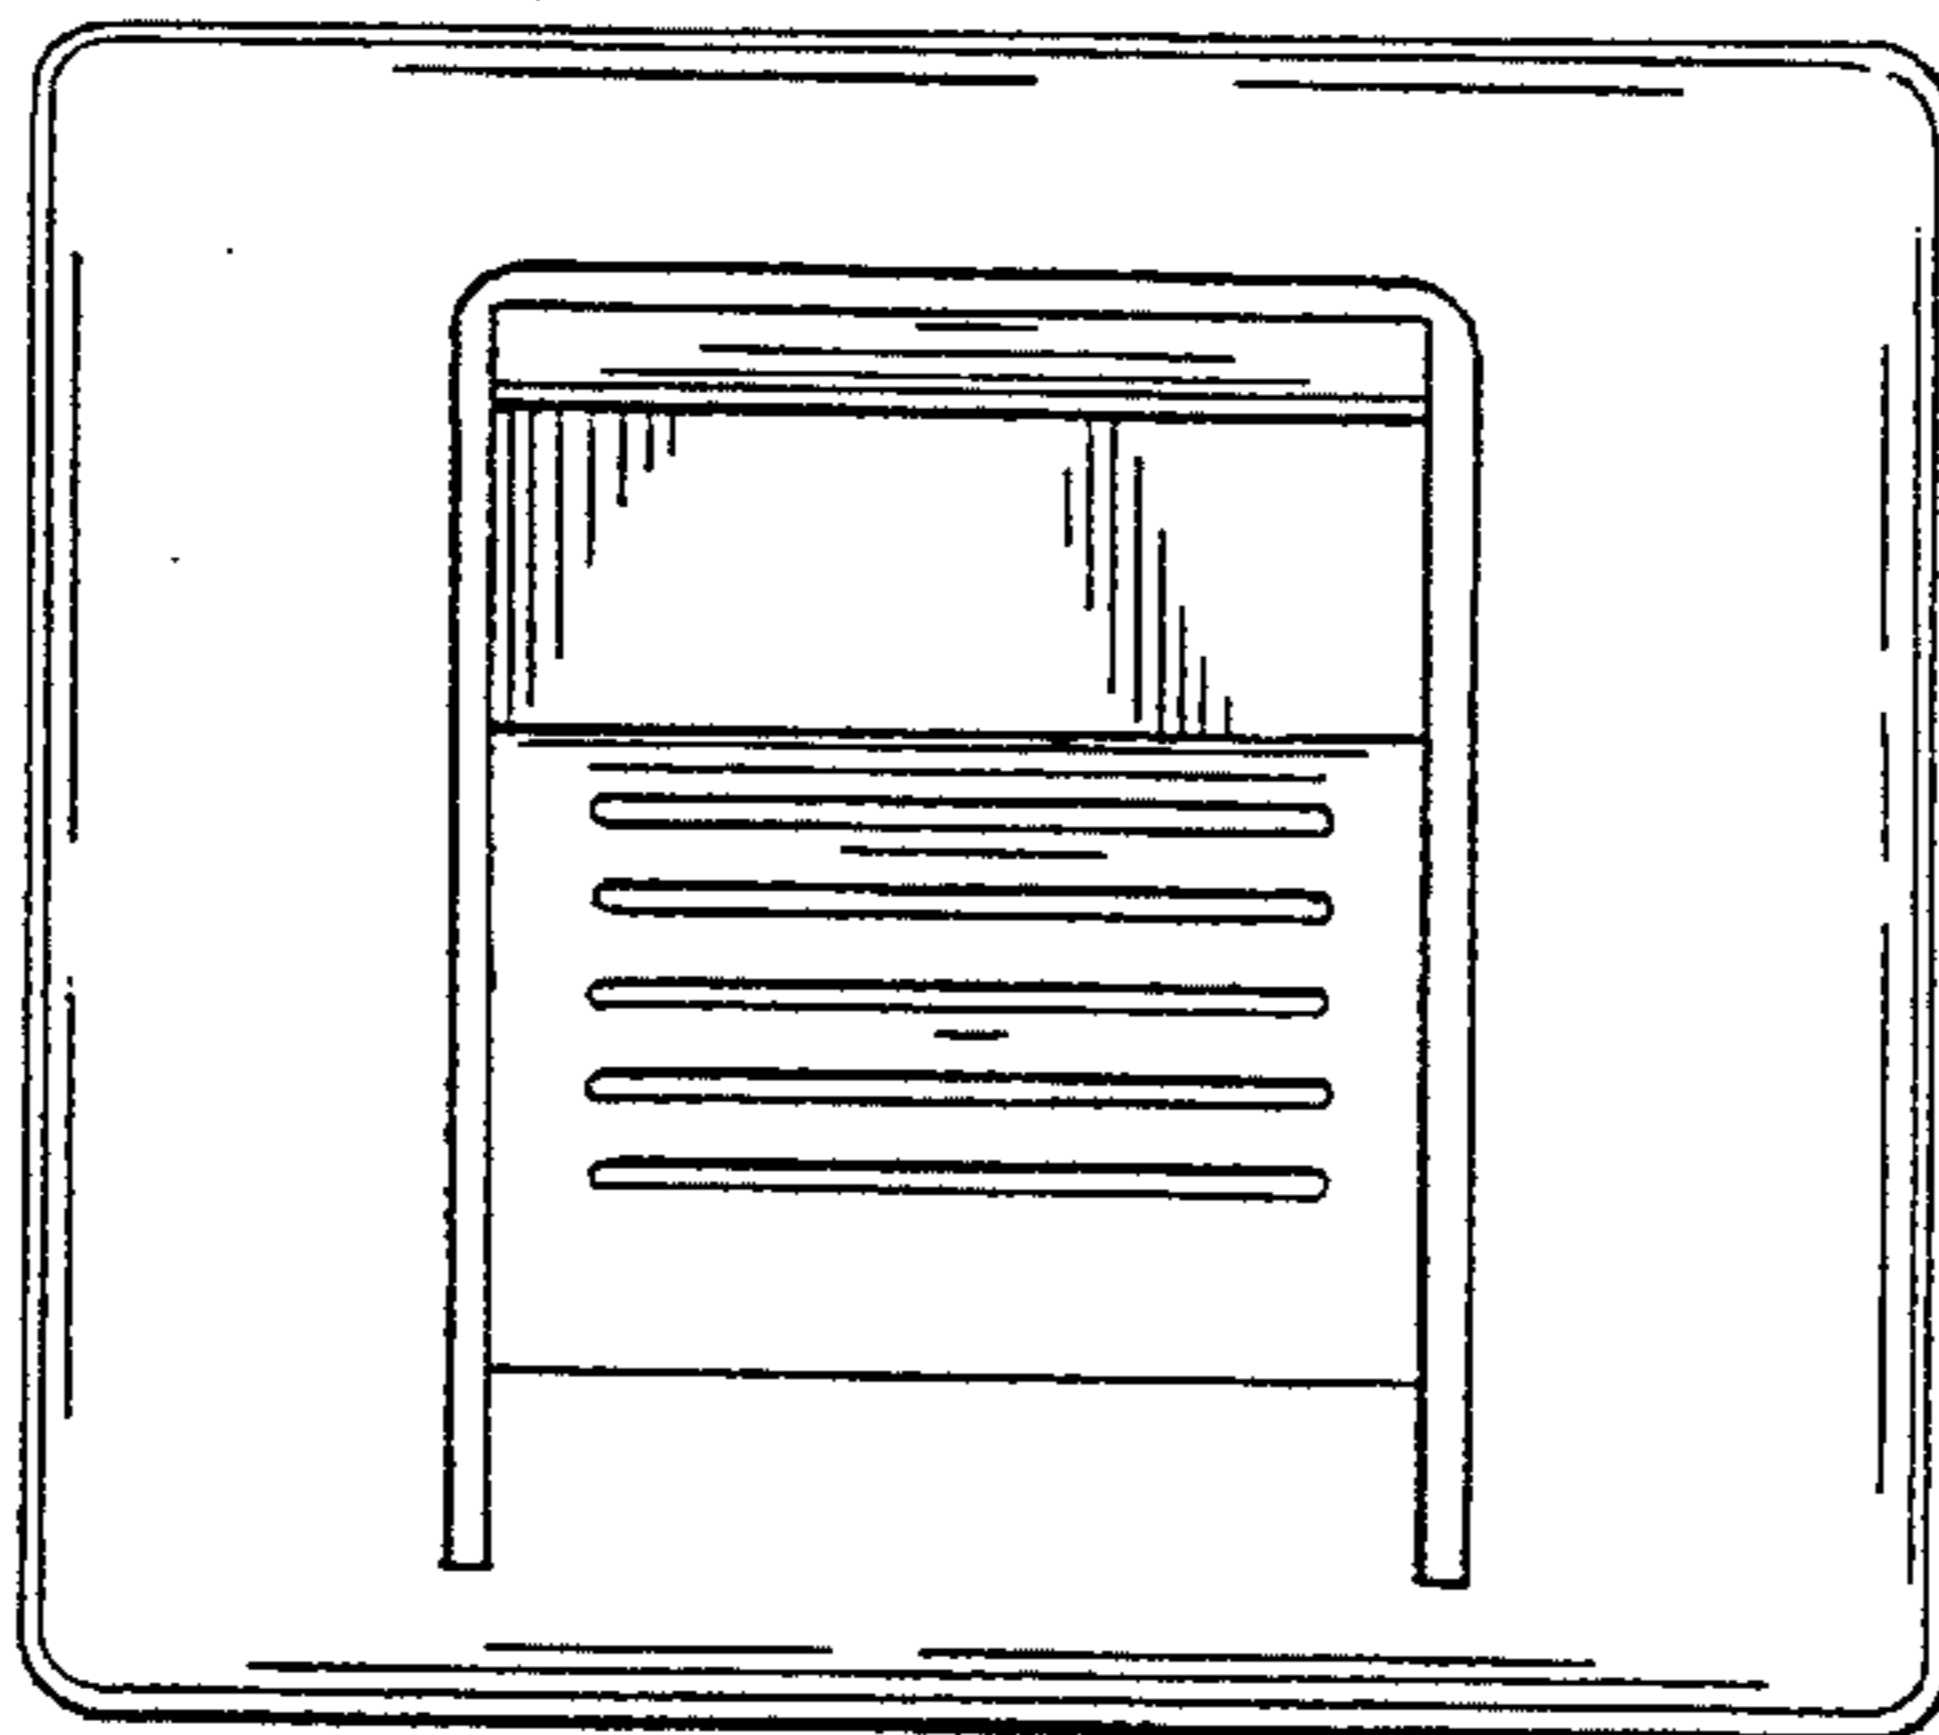


FIG. 11.

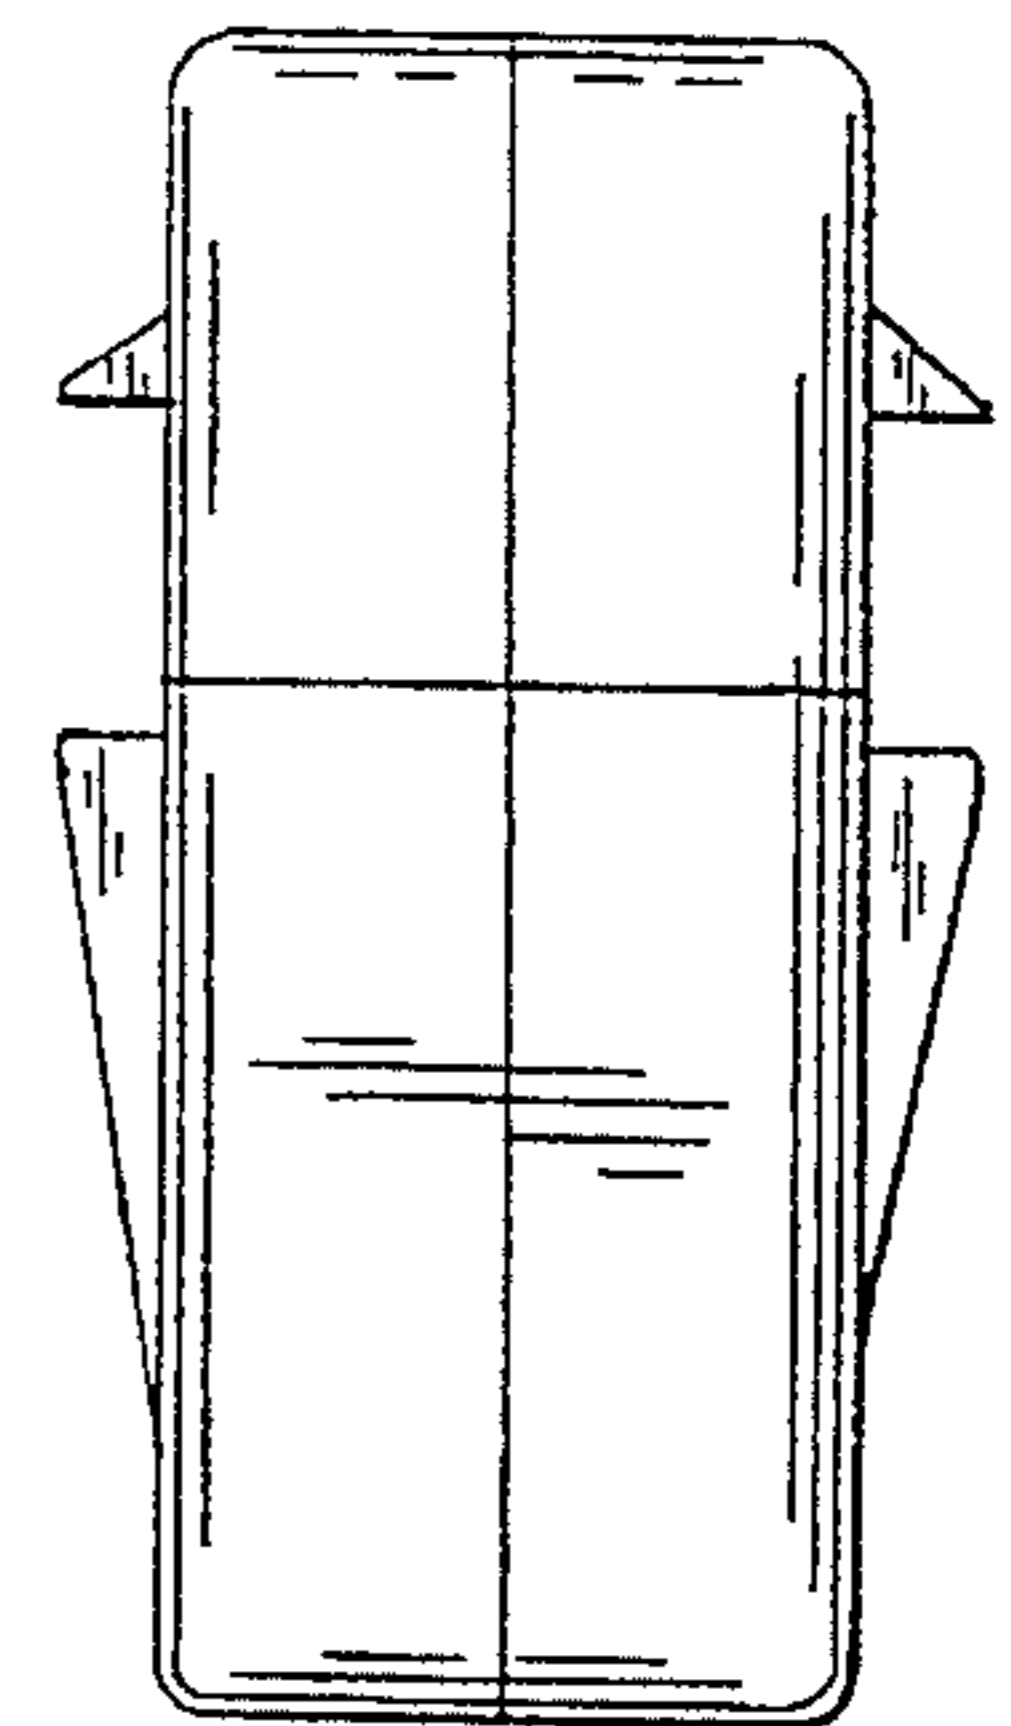


FIG. 12.

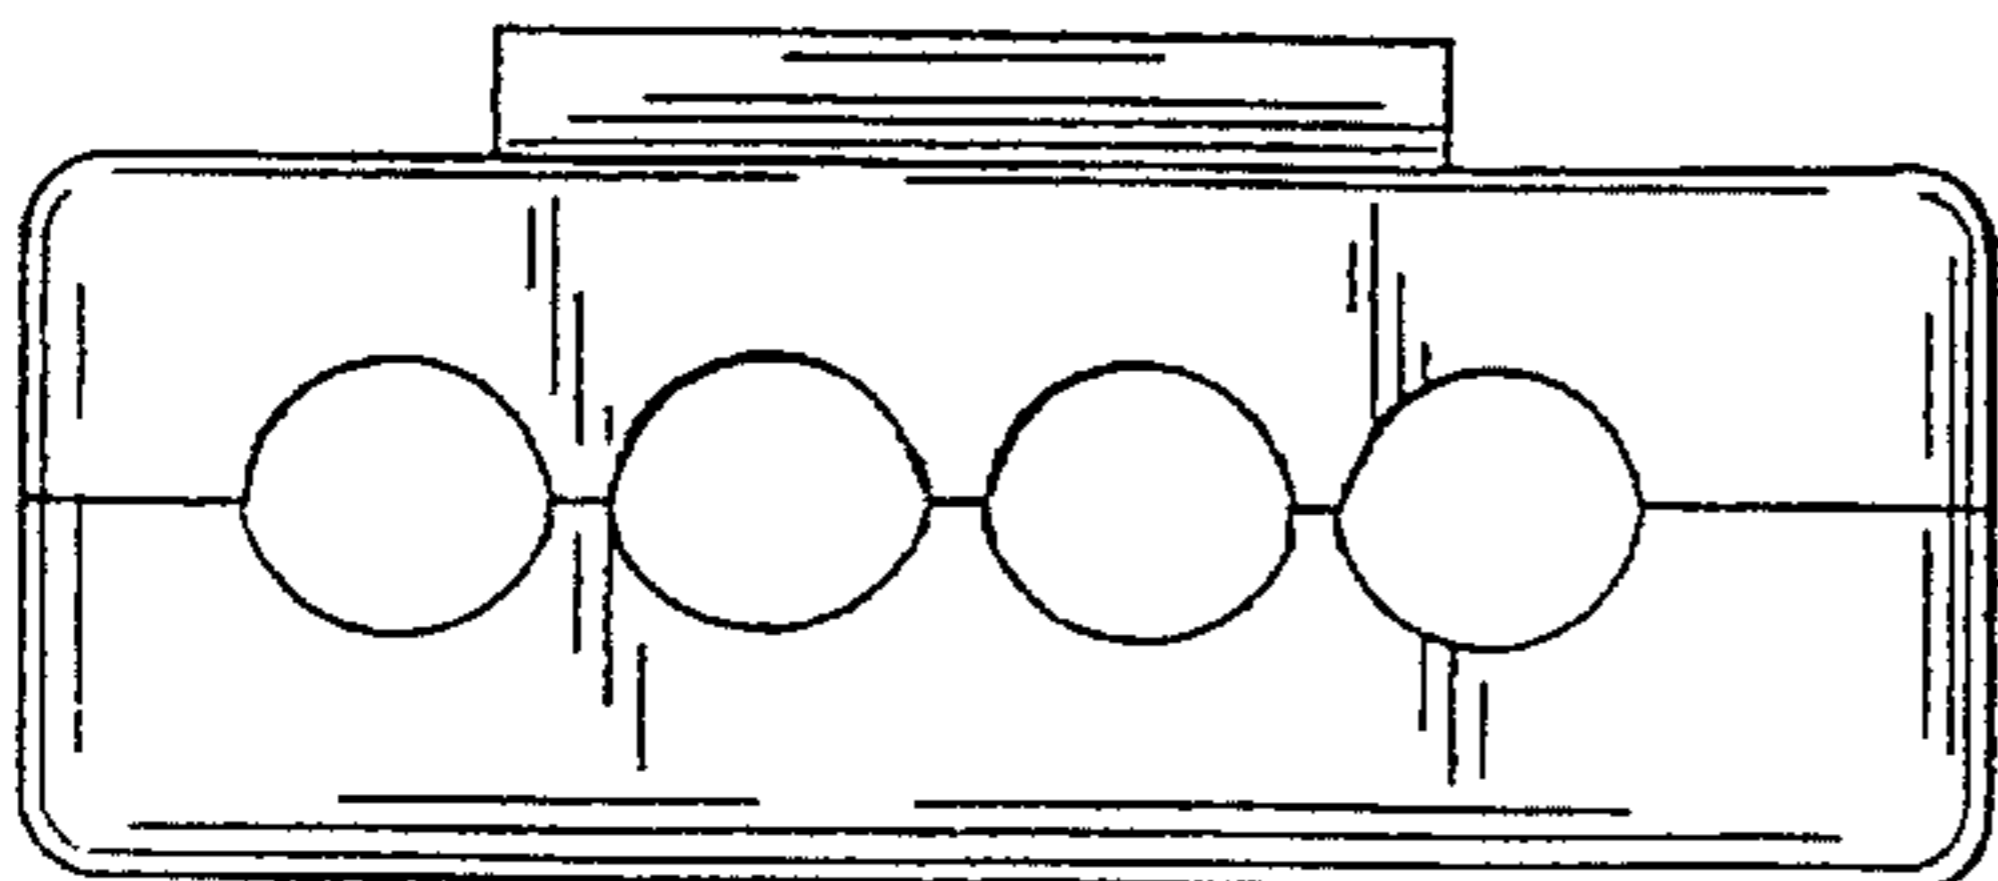


FIG. 13.

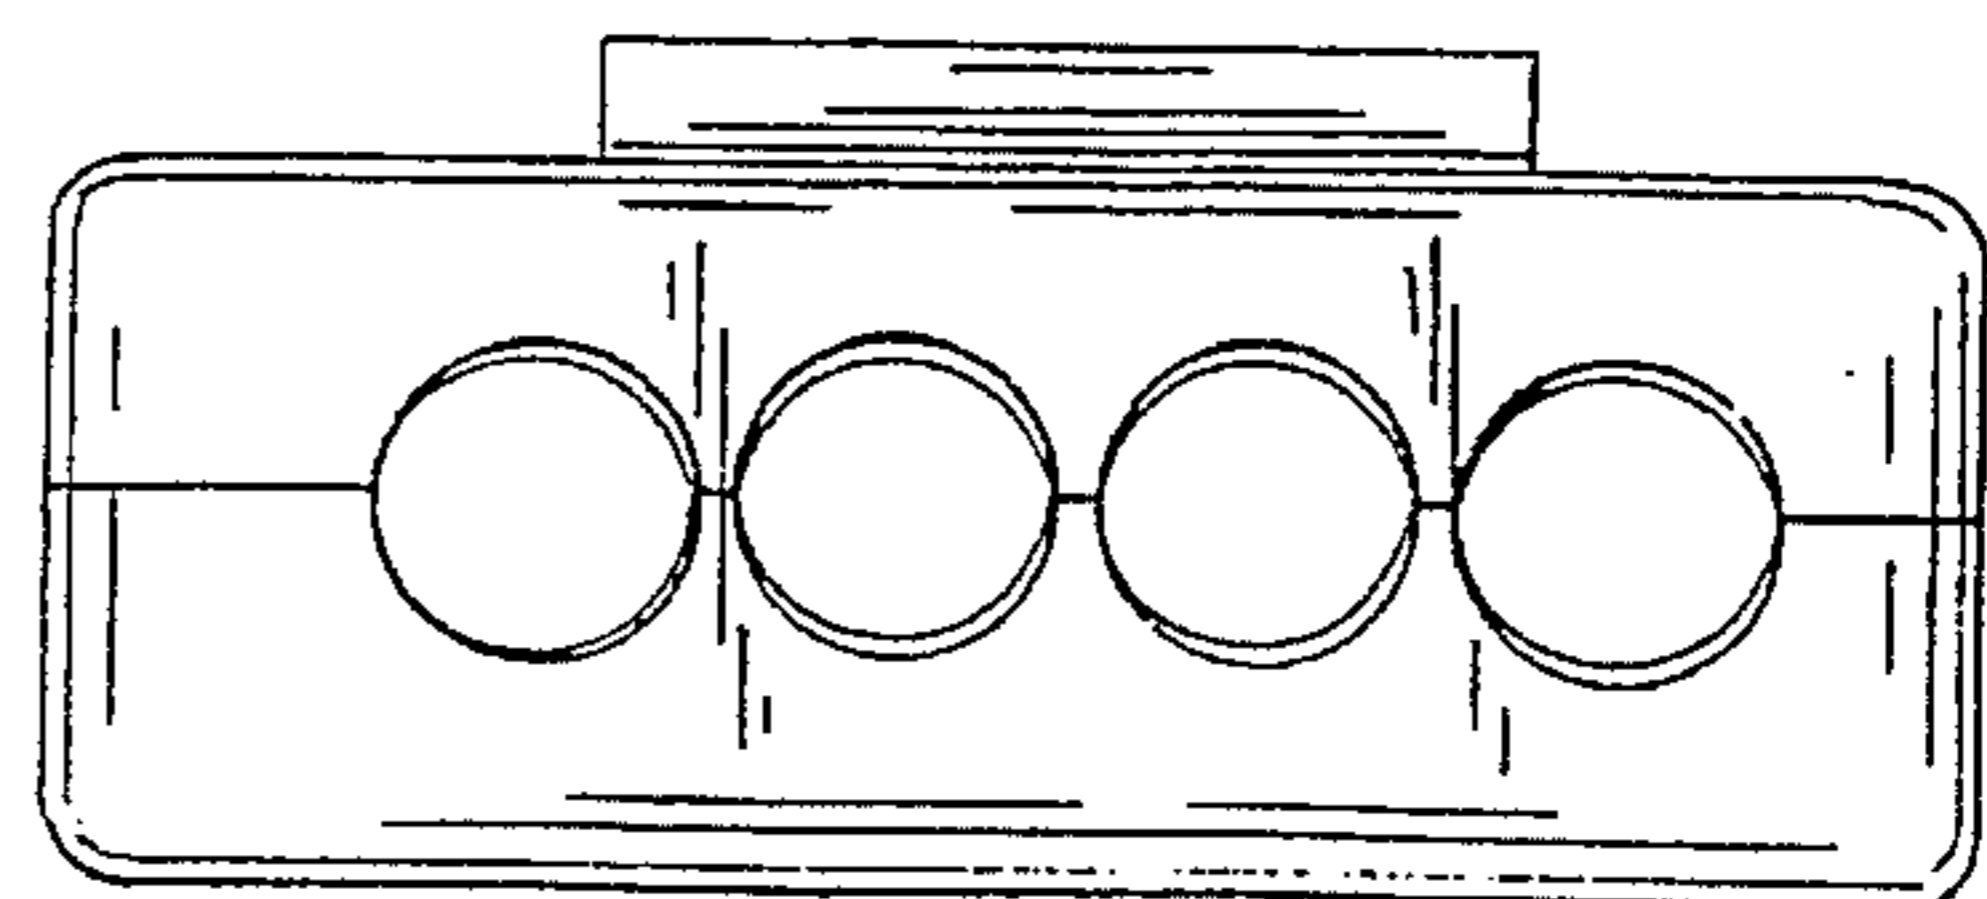


FIG. 14.

UNITED STATES PATENT AND TRADEMARK OFFICE  
**CERTIFICATE OF CORRECTION**

PATENT NO. : Des. 369,859  
DATED : May 14, 1996  
INVENTOR(S) : Philip P. Ribando, et al.

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

In the Heading insert: --[\*] Notice: The portion of the term of this patent subsequent to May 14, 2010, has been disclaimed.--

Column 2, line 2 delete "Healt-" and insert --Health-- therefor.

Column 2, in the Description of the Drawings, second line from the bottom, after "and" delete the comma (,).

**Signed and Sealed this**  
**Twenty-eighth Day of January, 1997**

*Attest:*



**BRUCE LEHMAN**

*Attesting Officer*

*Commissioner of Patents and Trademarks*