



US00D377686S

# United States Patent [19]

Waldeck et al.

[11] Patent Number: **Des. 377,686**

[45] Date of Patent: **\*\*Jan. 28, 1997**

[54] **TRAINING DEVICE FOR INHALER**

[75] Inventors: **Johan Waldeck, Södra Sandby; Nils G. Marnfeldt, Blentarp, both of Sweden**

[73] Assignee: **Astra Aktiebolag, Sodertalje, Sweden**

[\*\*] Term: **14 Years**

[21] Appl. No.: **28,911**

[22] Filed: **Sep. 26, 1994**

[30] **Foreign Application Priority Data**

Mar. 25, 1994 [SE] Sweden ..... 94-0732

[52] U.S. Cl. .... **D24/110**

[58] Field of Search ..... D24/110, 165, D24/185, 186; 128/200.14, 200.23, 203.12, 203.15, 203.21, 204.21, 204.23, 204.26, 205.23

[56] **References Cited**

**U.S. PATENT DOCUMENTS**

D. 348,928	7/1994	Ashley et al. ....	D24/110
D. 362,500	9/1995	Cook et al. ....	D24/110
4,524,769	6/1985	Wetterlin .	
4,534,345	8/1985	Wetterlin .	
4,668,218	5/1987	Virtanen .	
4,907,583	3/1990	Wetterlin et al. .	
4,984,158	1/1991	Hillsman .	
5,019,974	5/1991	Beckers .	
5,024,219	6/1991	Dietz .....	128/204.21
5,331,953	7/1994	Andersson et al. .	
5,404,871	4/1995	Goodman et al. ....	128/205.23 X
5,431,154	7/1995	Seigel et al. ....	128/200.23 X

**FOREIGN PATENT DOCUMENTS**

WO90/10470	9/1990	WIPO .
WO93/21980	11/1993	WIPO .

Primary Examiner—B. J. Bullock  
Assistant Examiner—Linda Brooks

Attorney, Agent, or Firm—Fish & Richardson P.C.

[57] **CLAIM**

The ornamental design for a training device for inhaler, as shown.

**DESCRIPTION**

FIG. 1 is a front perspective view of the training device for an inhaler, the inhaler being shown with the protective cap removed;

FIG. 2 is a view of the front of the box portion of the training device, which has been enlarged for ease of illustration;

FIG. 3 is a back view of the box portion of the training device shown in FIG. 2;

FIG. 4 is a left side view of the box portion of the training device shown in FIG. 2;

FIG. 5 is a right side view of the box portion of the training device shown in FIG. 2;

FIG. 6 is a top view of the box portion of the training device shown in FIG. 2;

FIG. 7 is a bottom view of the box portion of the training device shown in FIG. 2;

FIG. 8 is a side view of the inhaler portion of the training device shown in FIG. 1, which has been enlarged for ease of illustration;

FIG. 9 is another side view of the inhaler portion of the training device shown in FIG. 8;

FIG. 10 is another side elevational view of the inhaler portion of the training device shown in FIG. 8;


FIG. 11 is another side view of the inhaler portion of the training device shown in FIG. 8;

FIG. 12 is a top view of the inhaler portion of the training device shown in FIG. 1 with the protective cap removed, which has been enlarged for ease of illustration;

FIG. 13 is a bottom view of the inhaler portion of the training device shown in FIG. 12; and,

FIG. 14 is a side view of the protective cap shown in FIG. 1, which has been enlarged for ease of illustration.

**1 Claim, 3 Drawing Sheets**

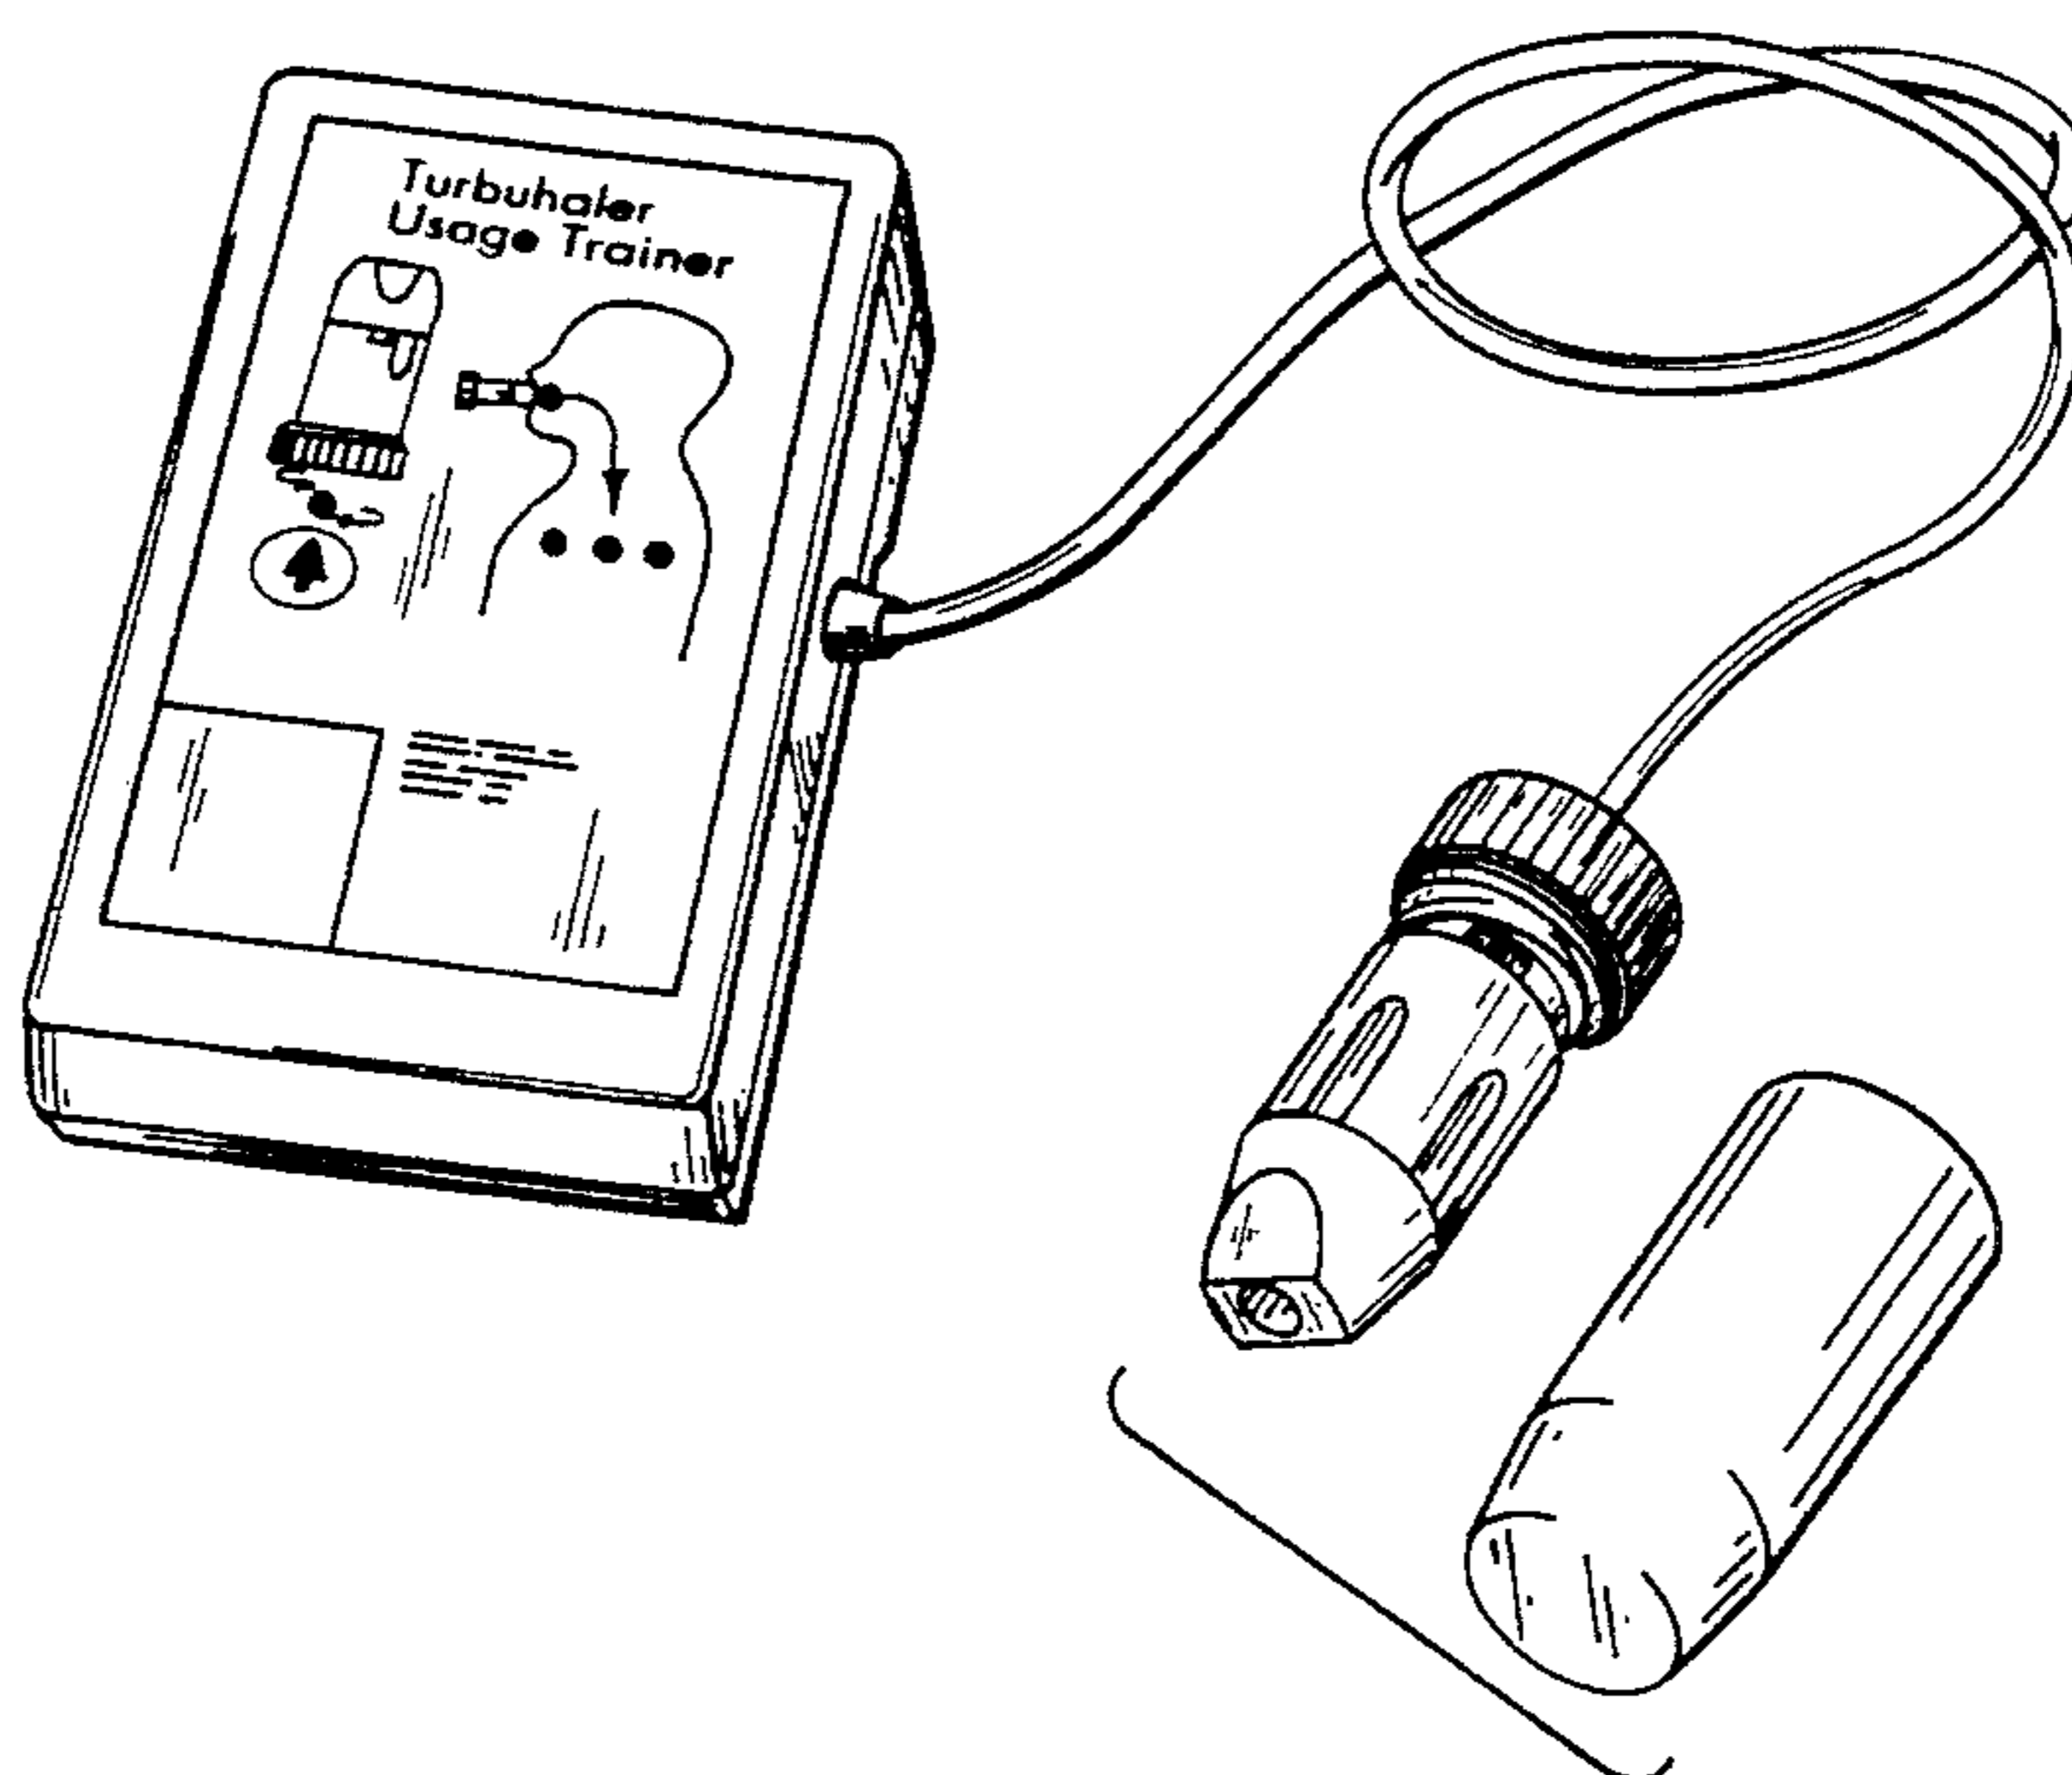

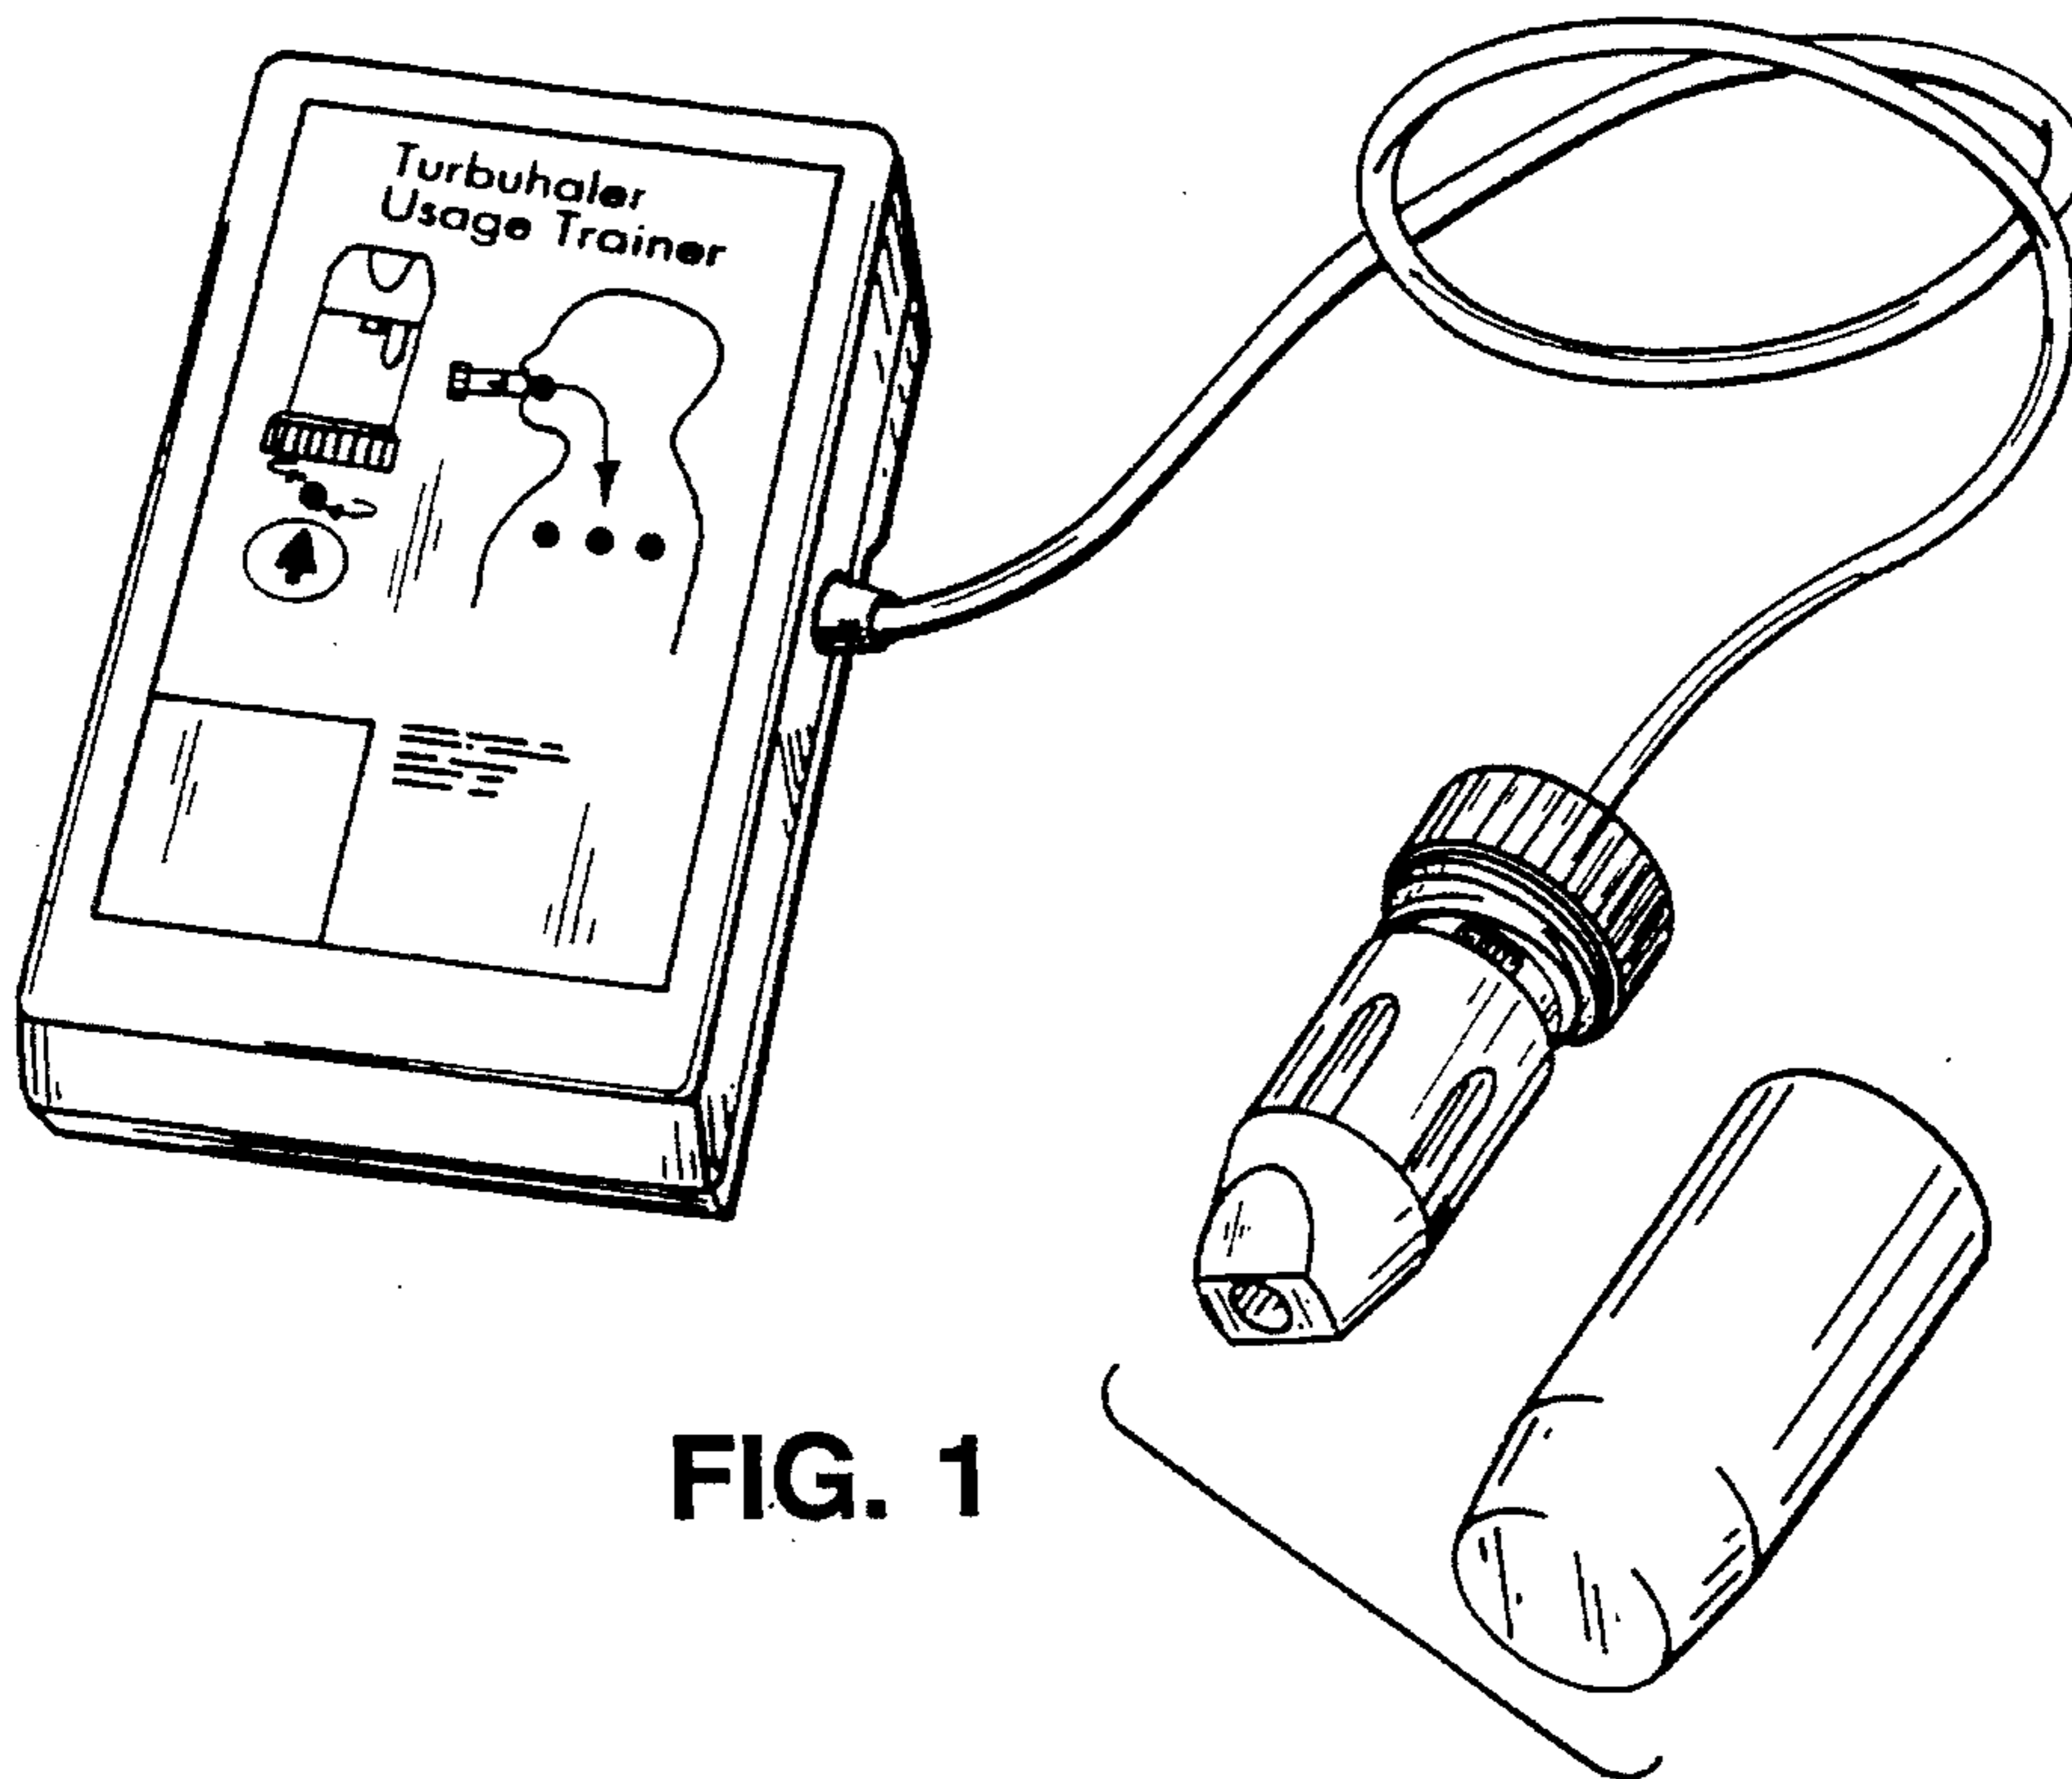


FIG. 1

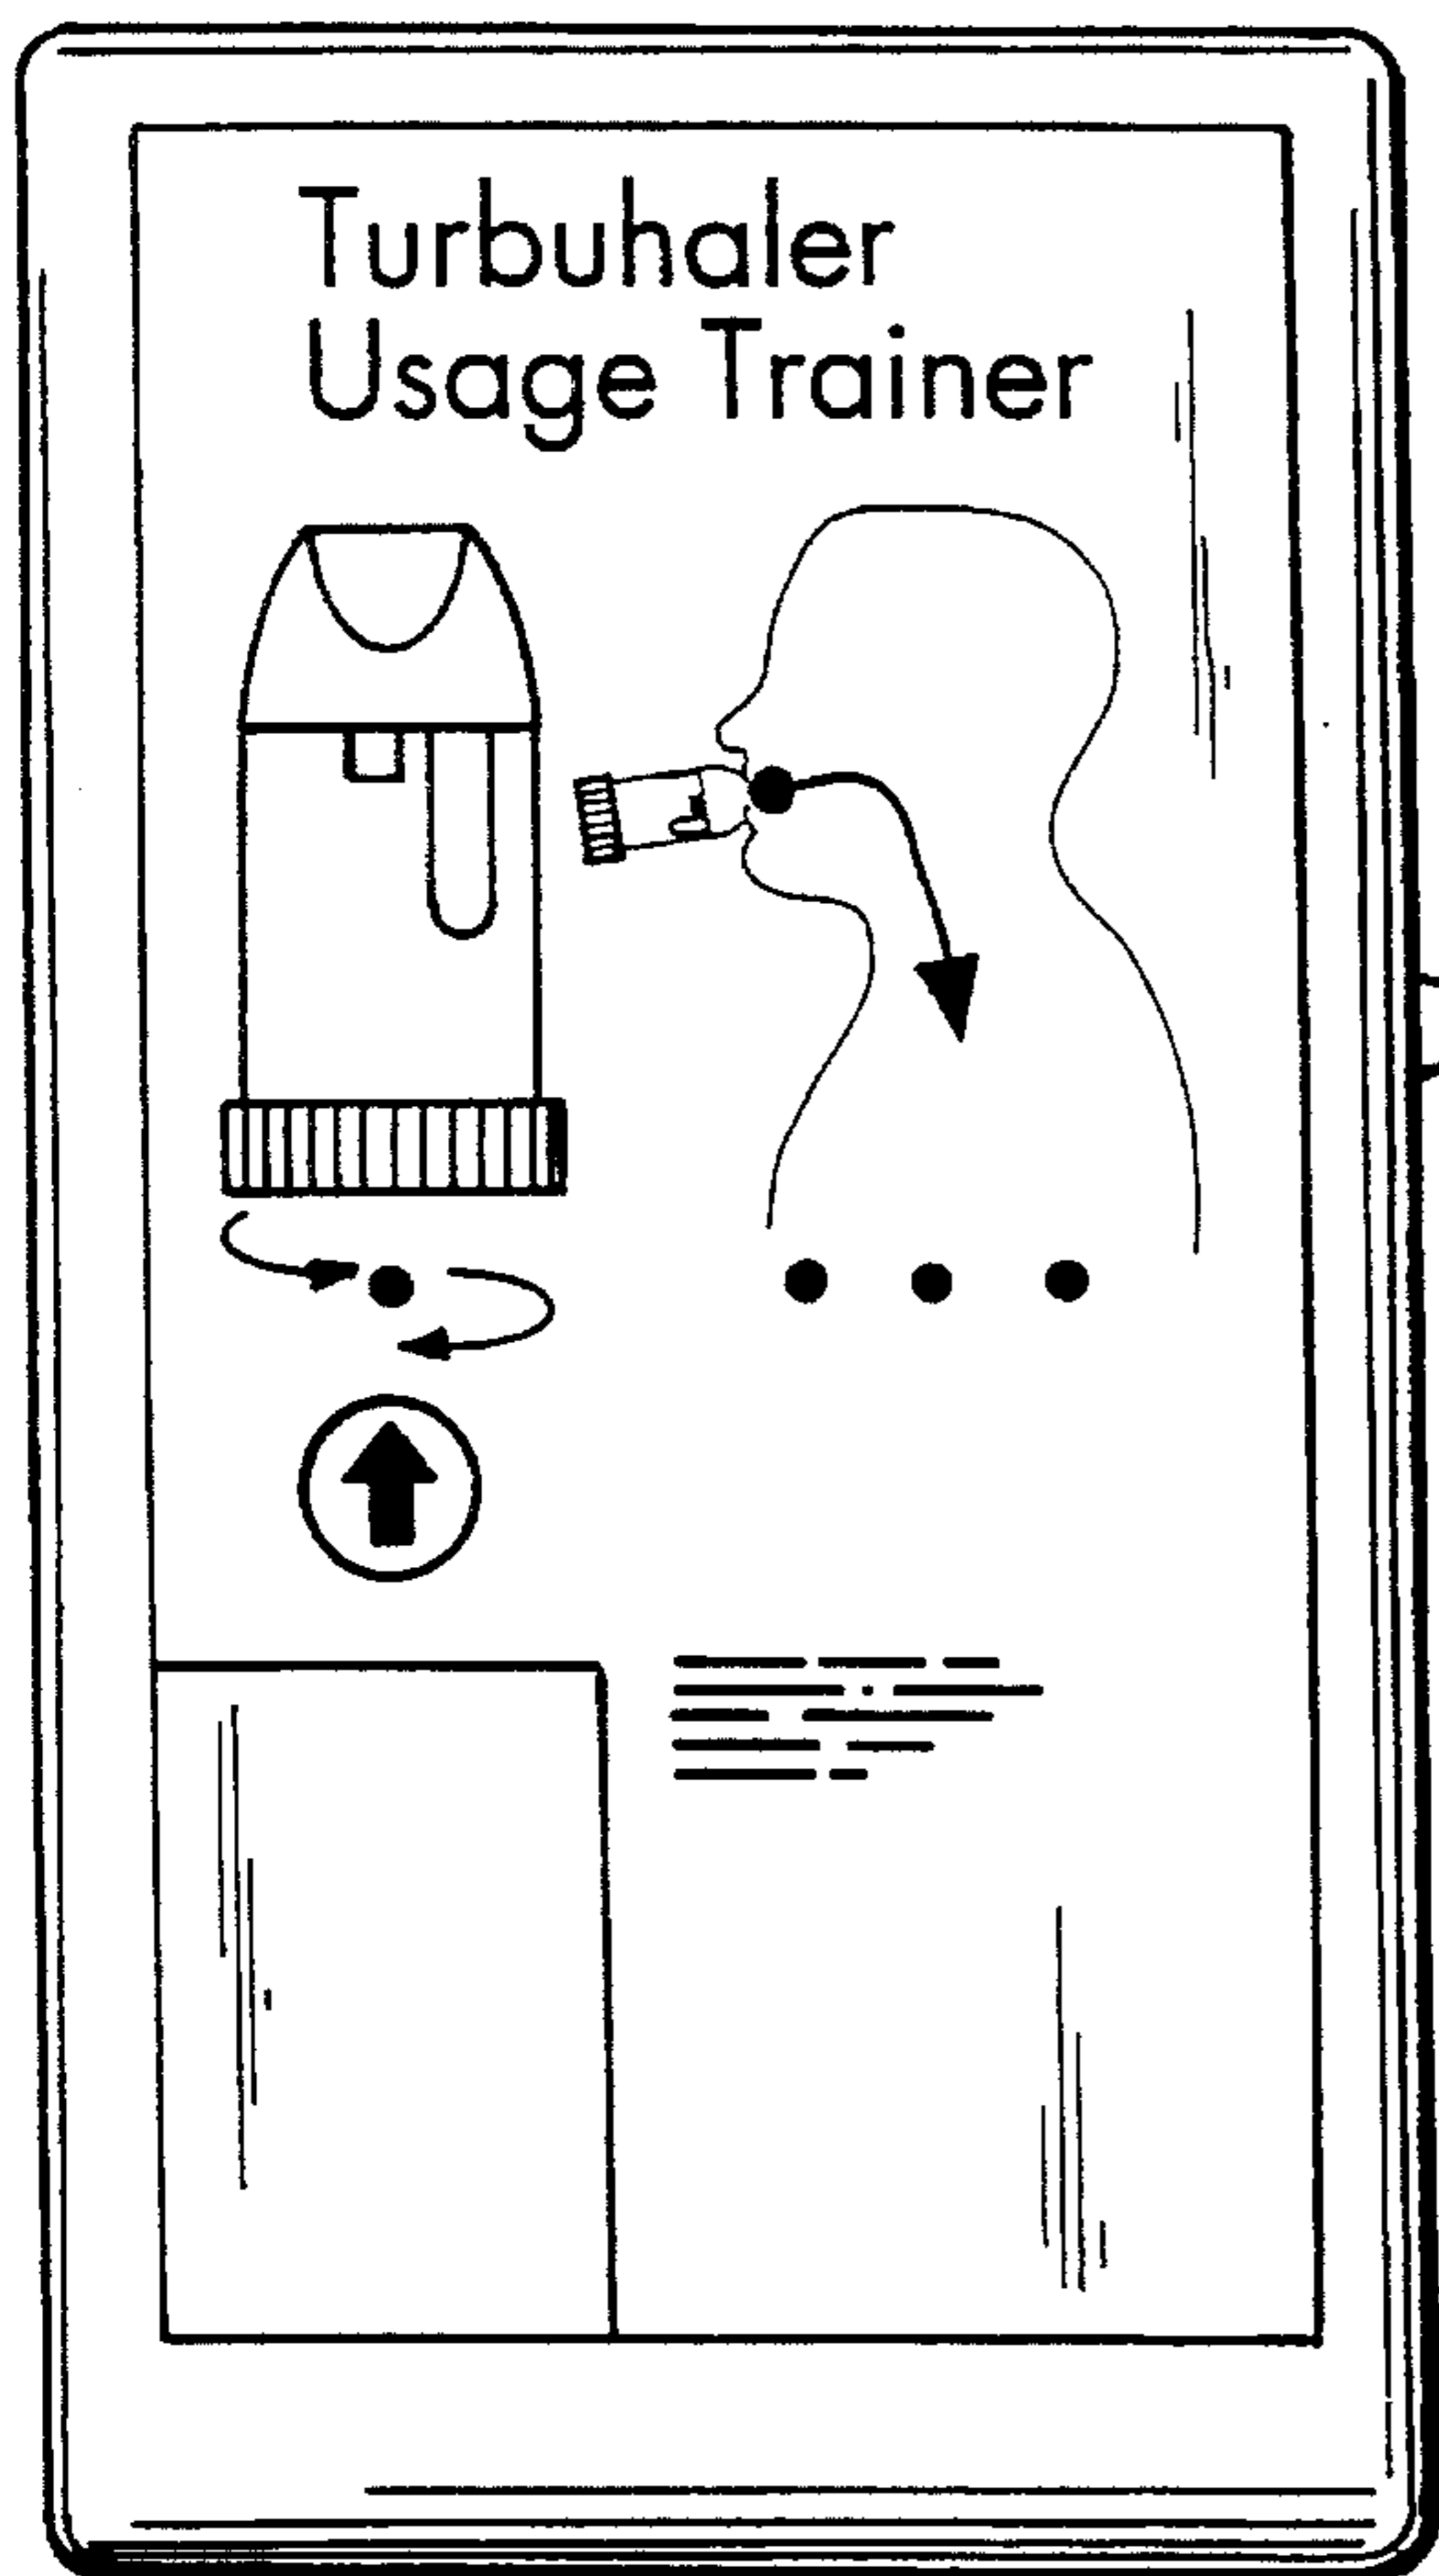


FIG. 2

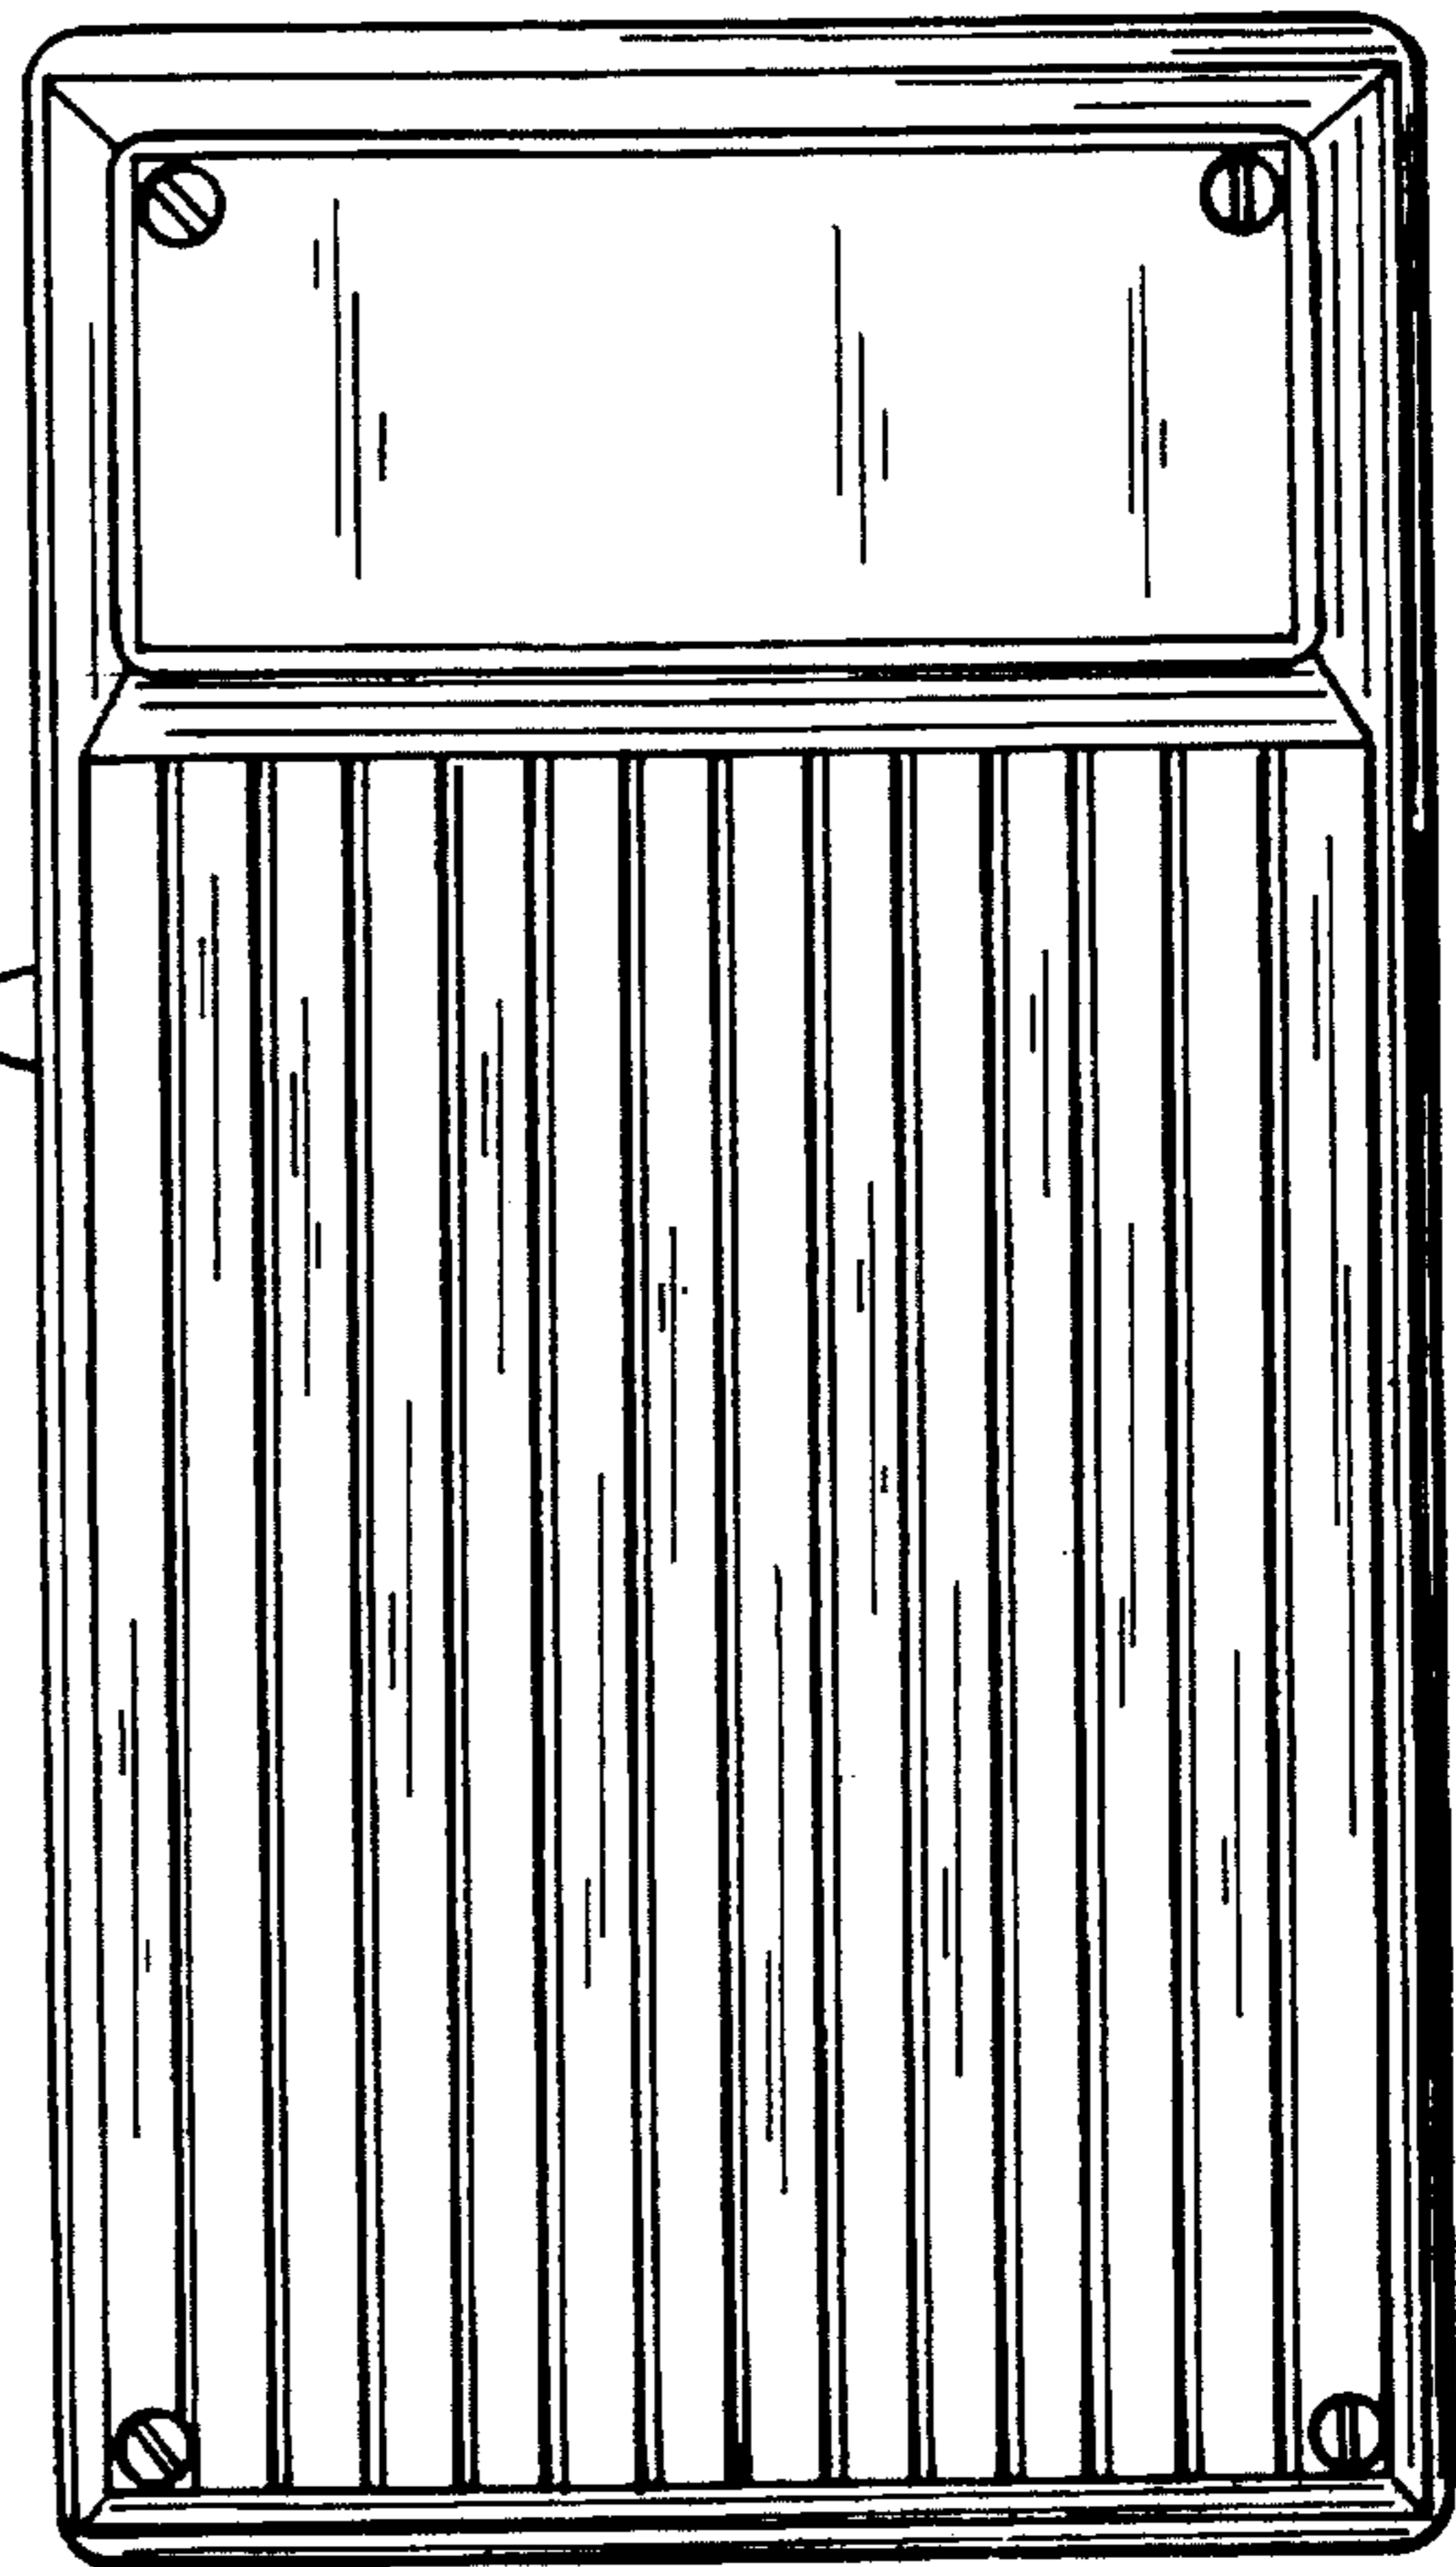


FIG. 3

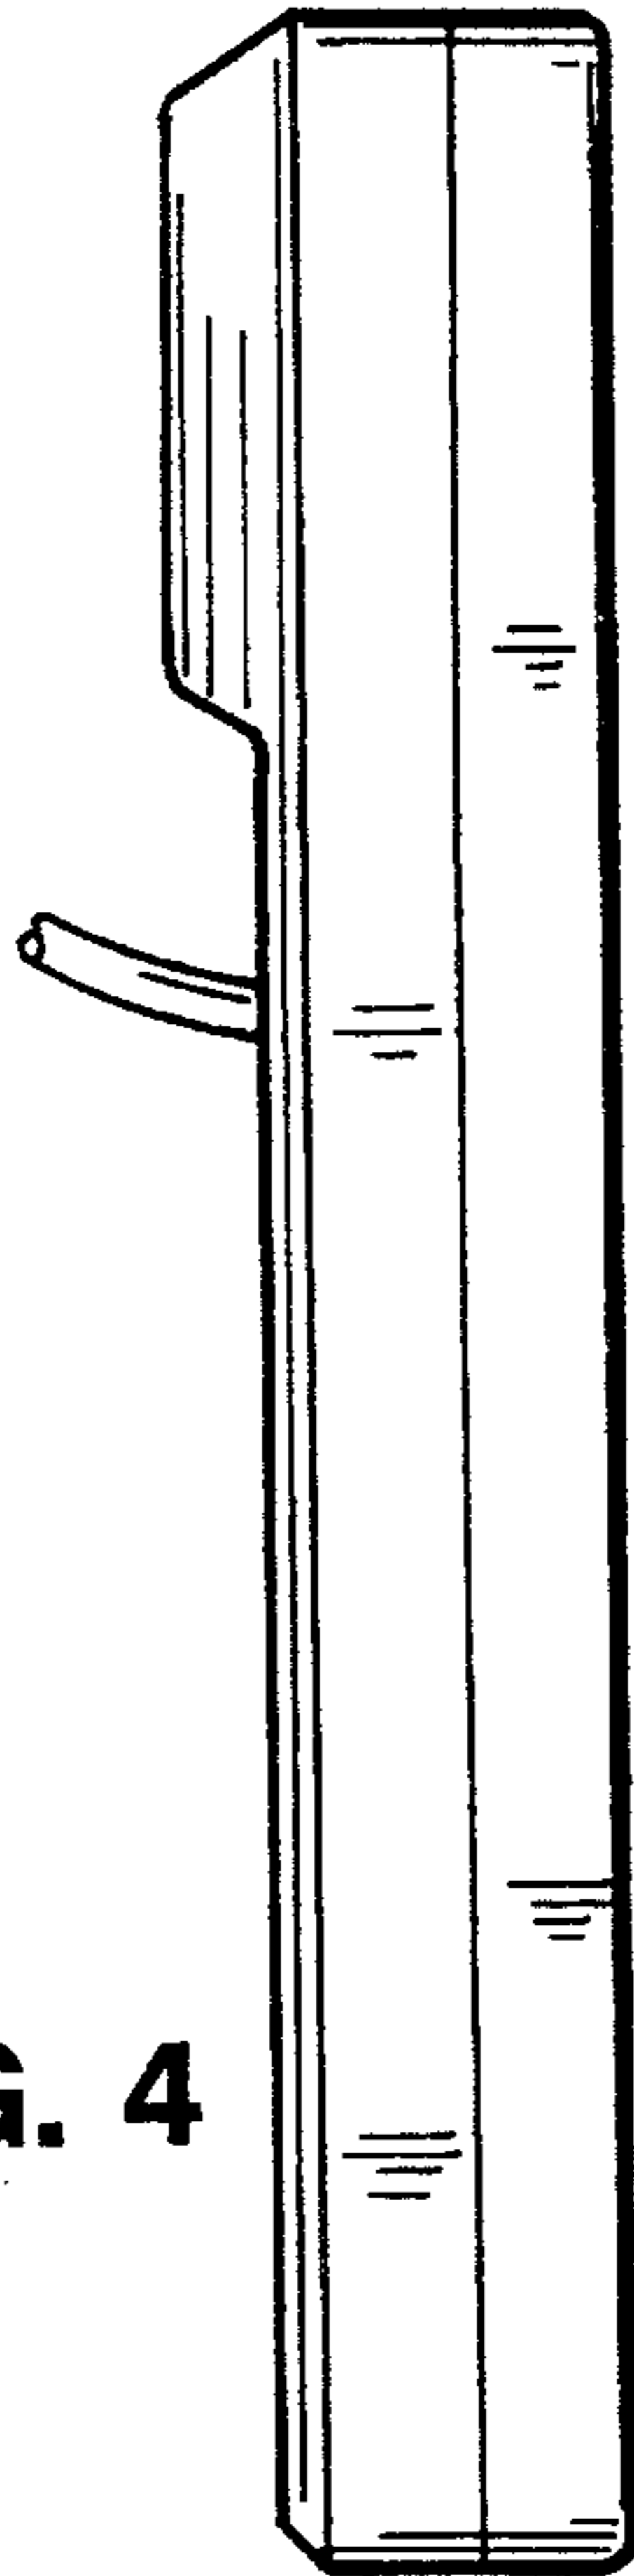


FIG. 4

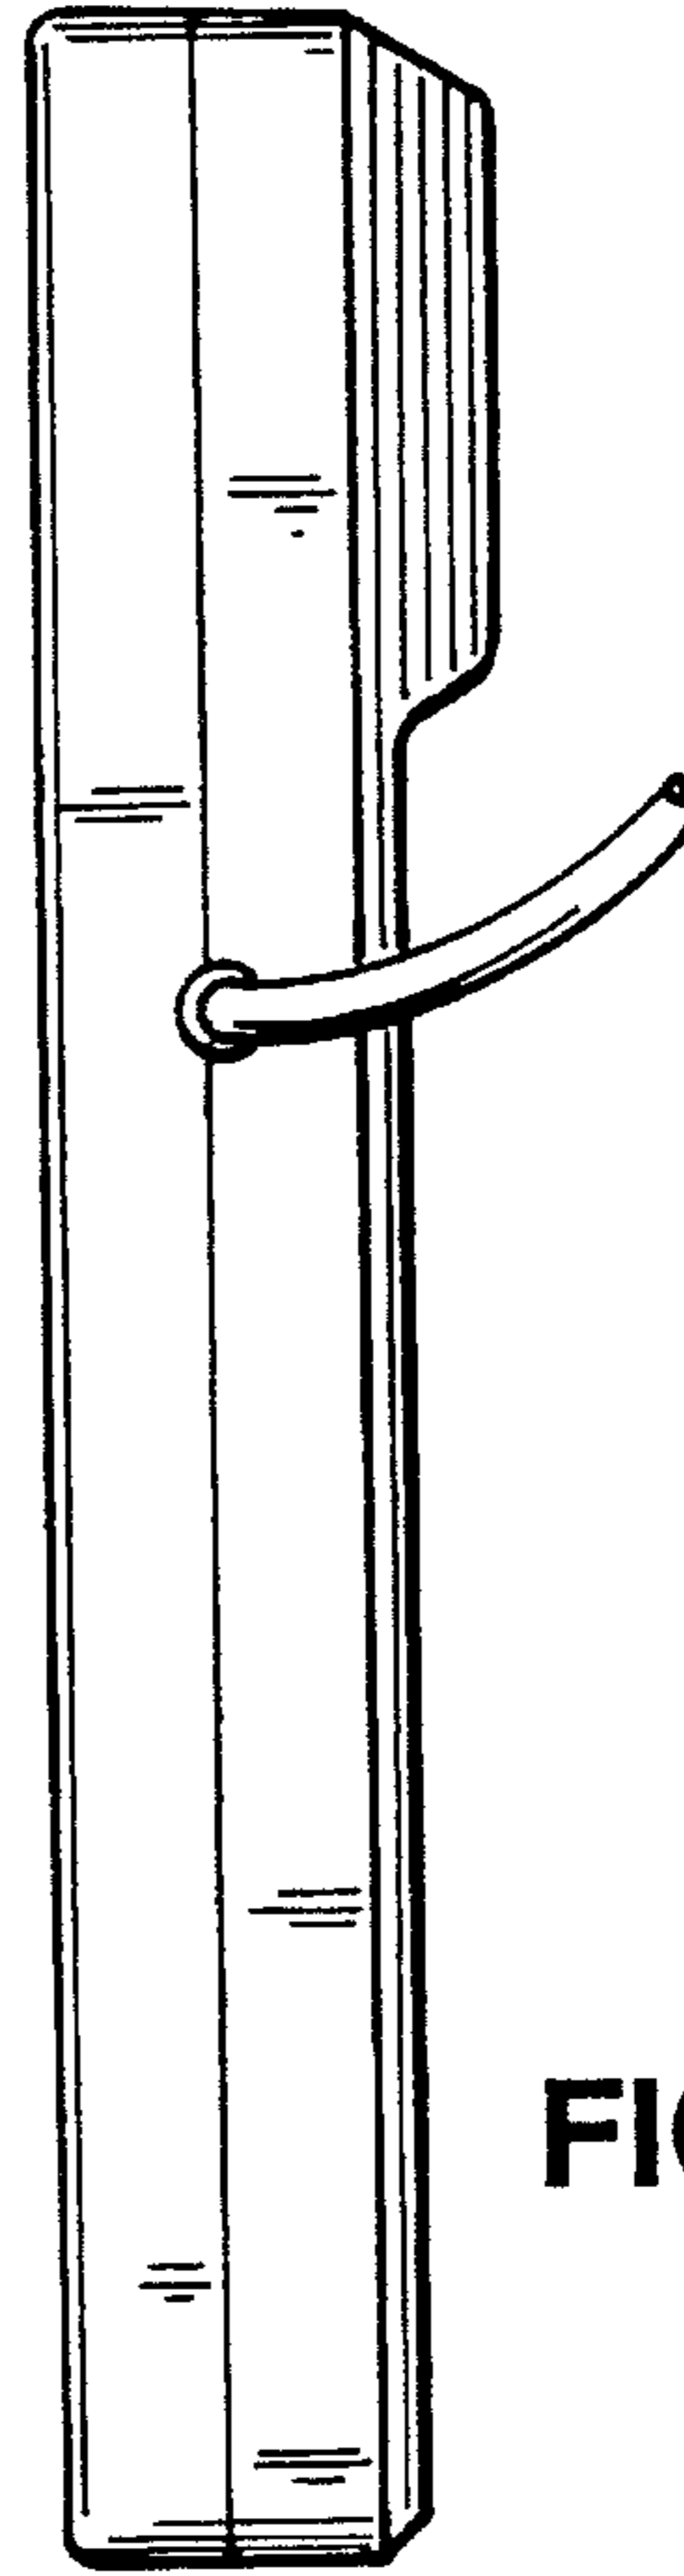


FIG. 5

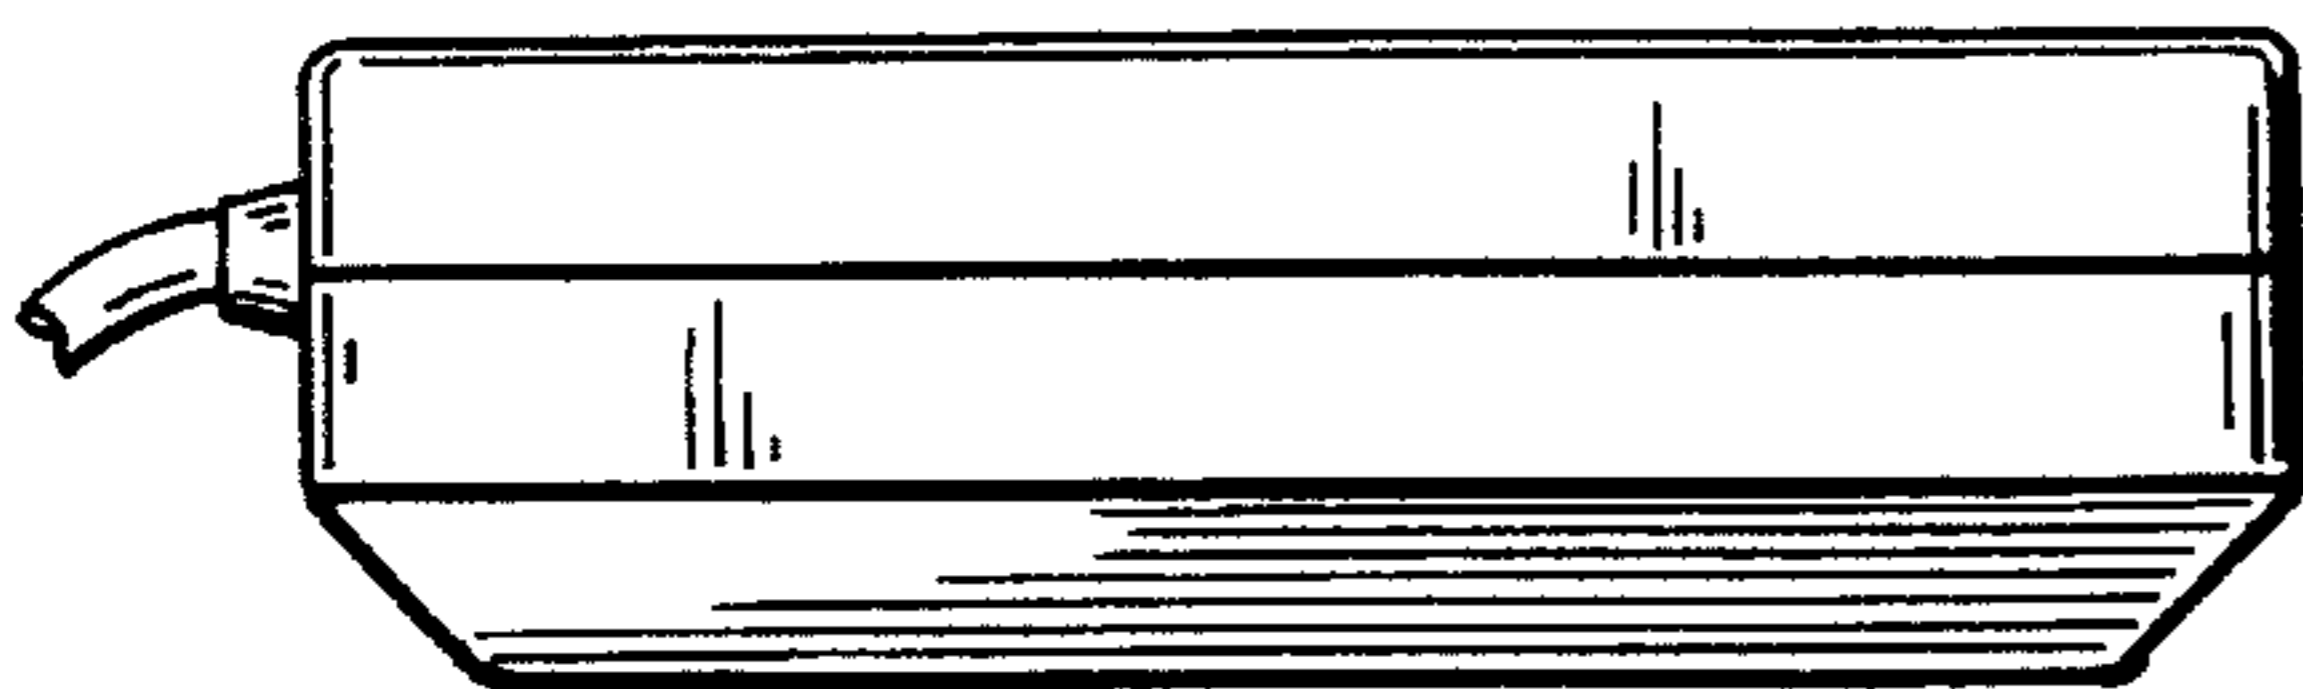


FIG. 6

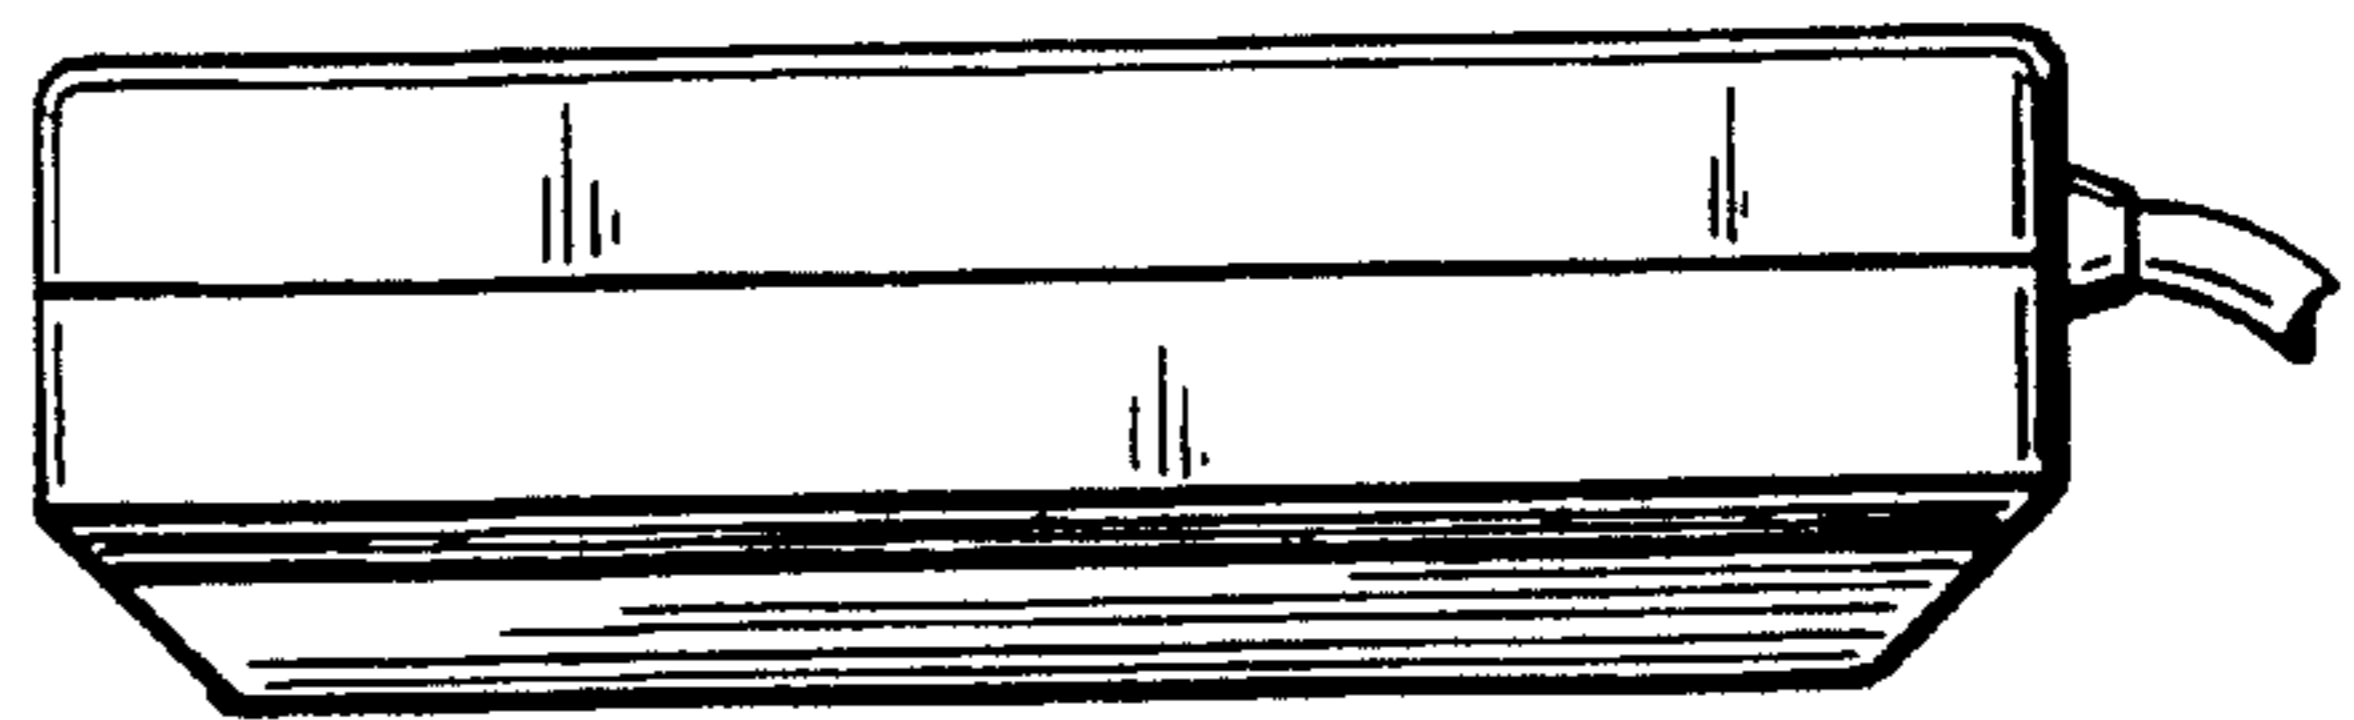


FIG. 7

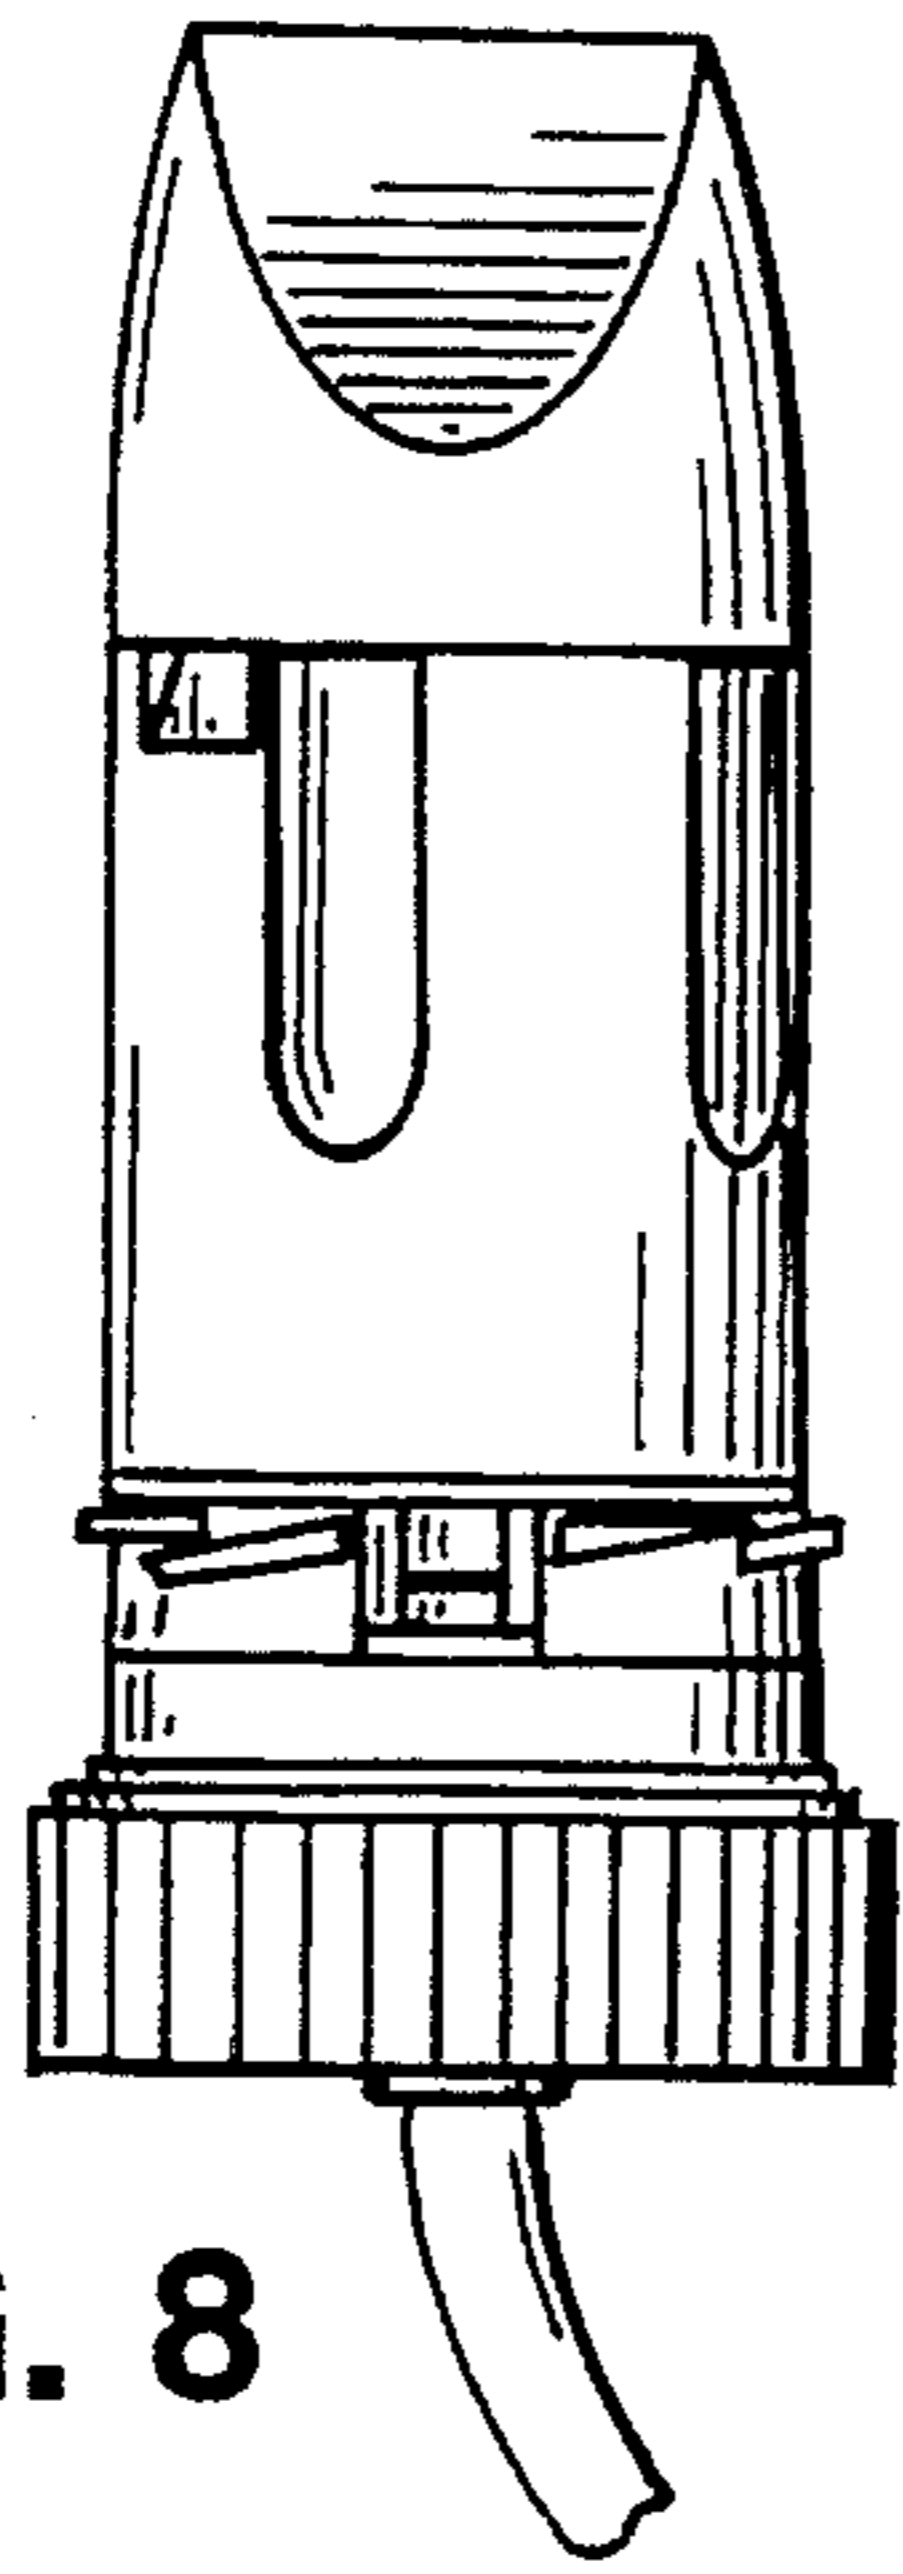


FIG. 8

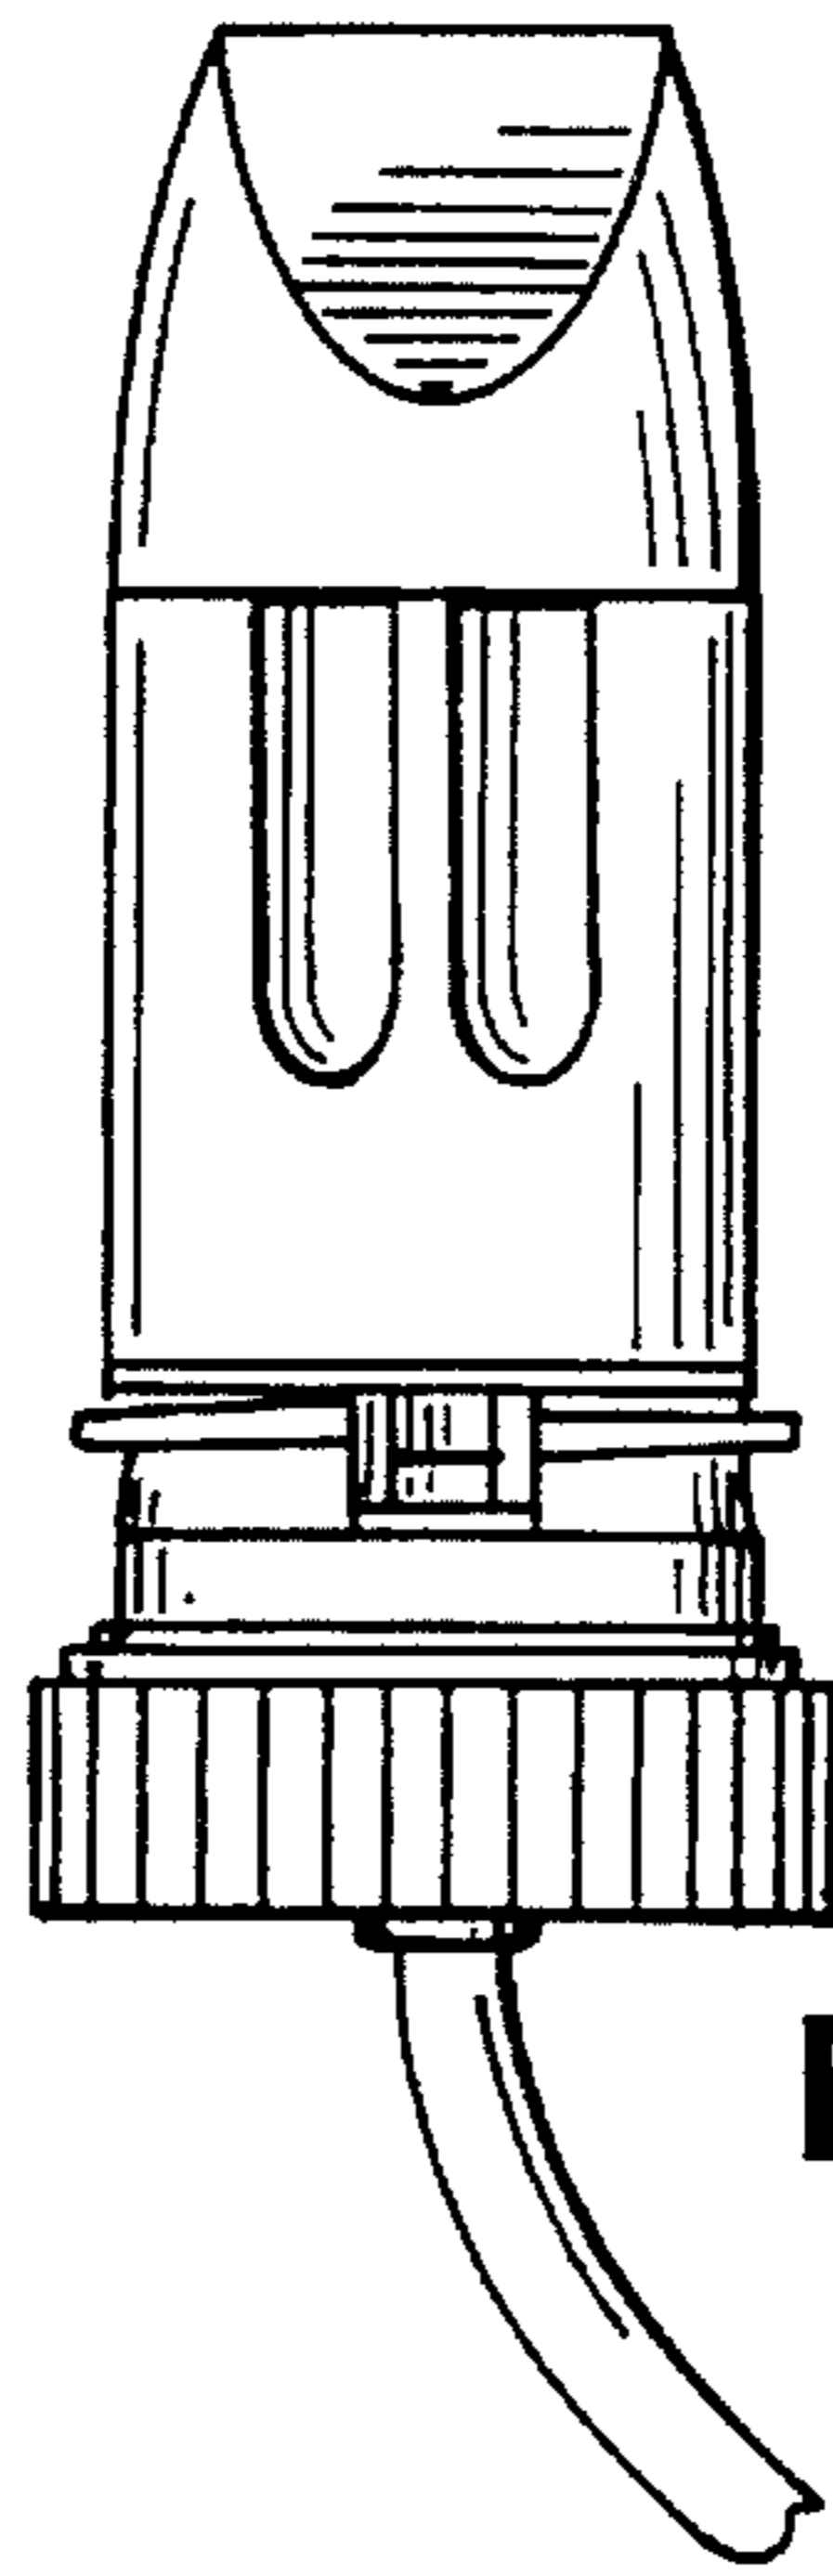


FIG. 9

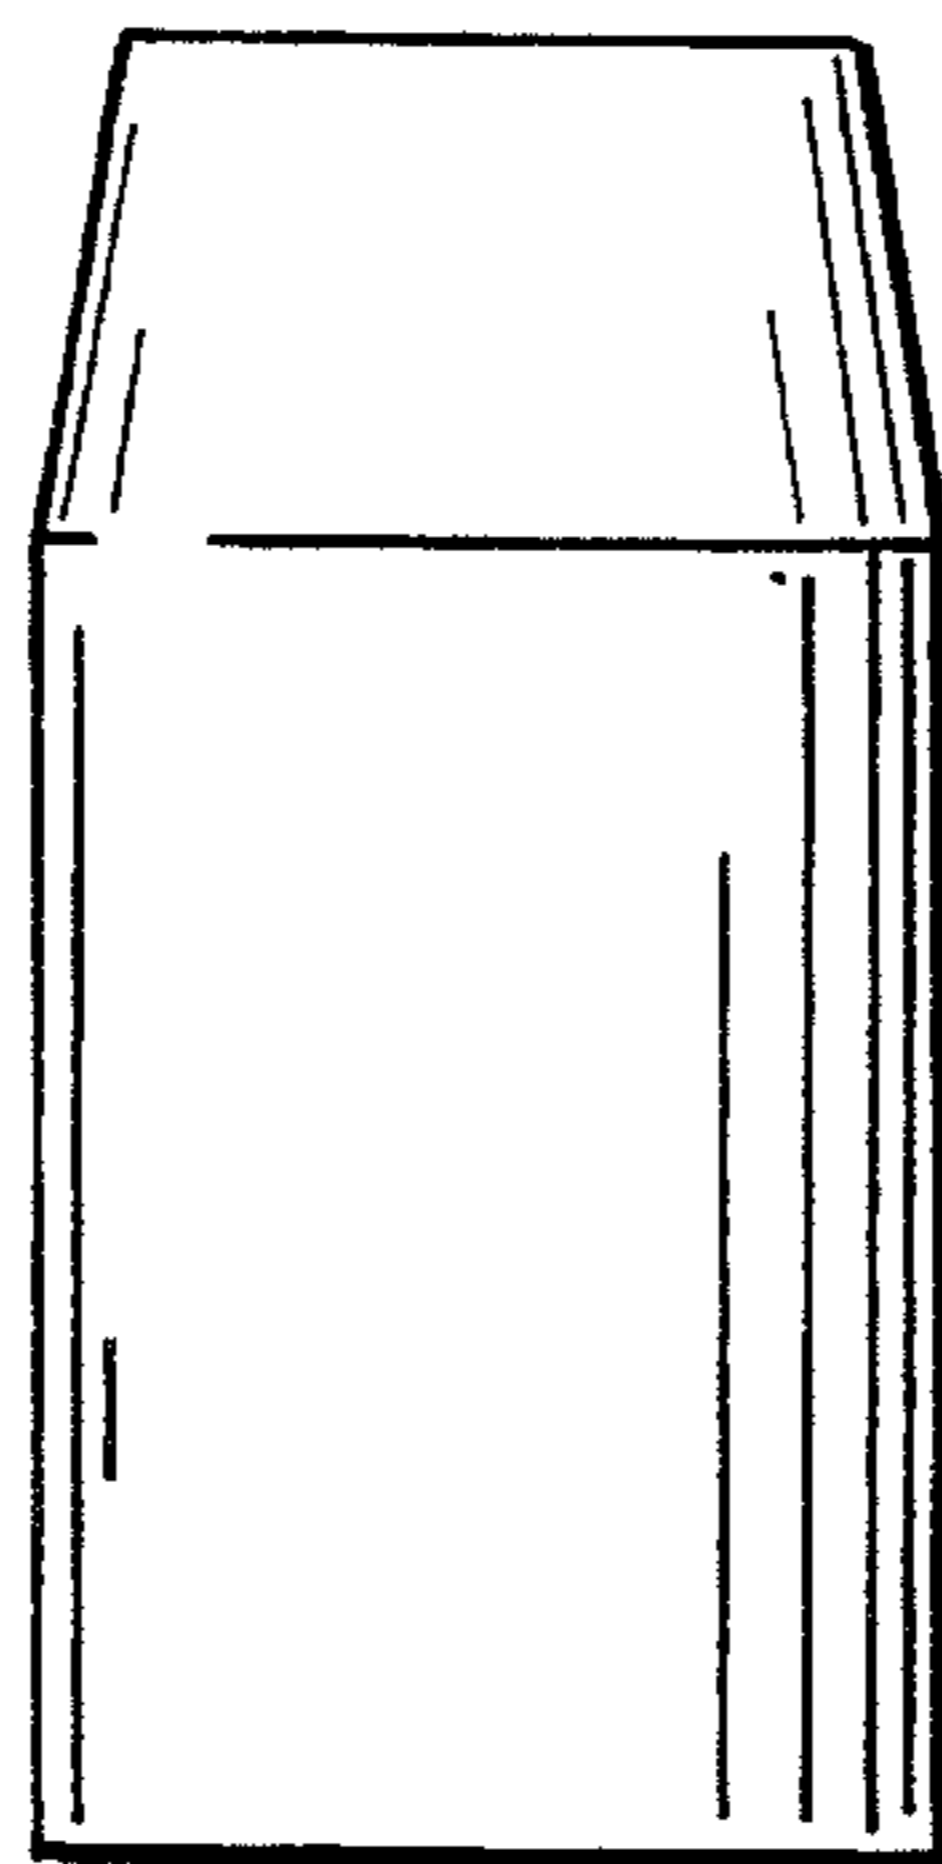


FIG. 14

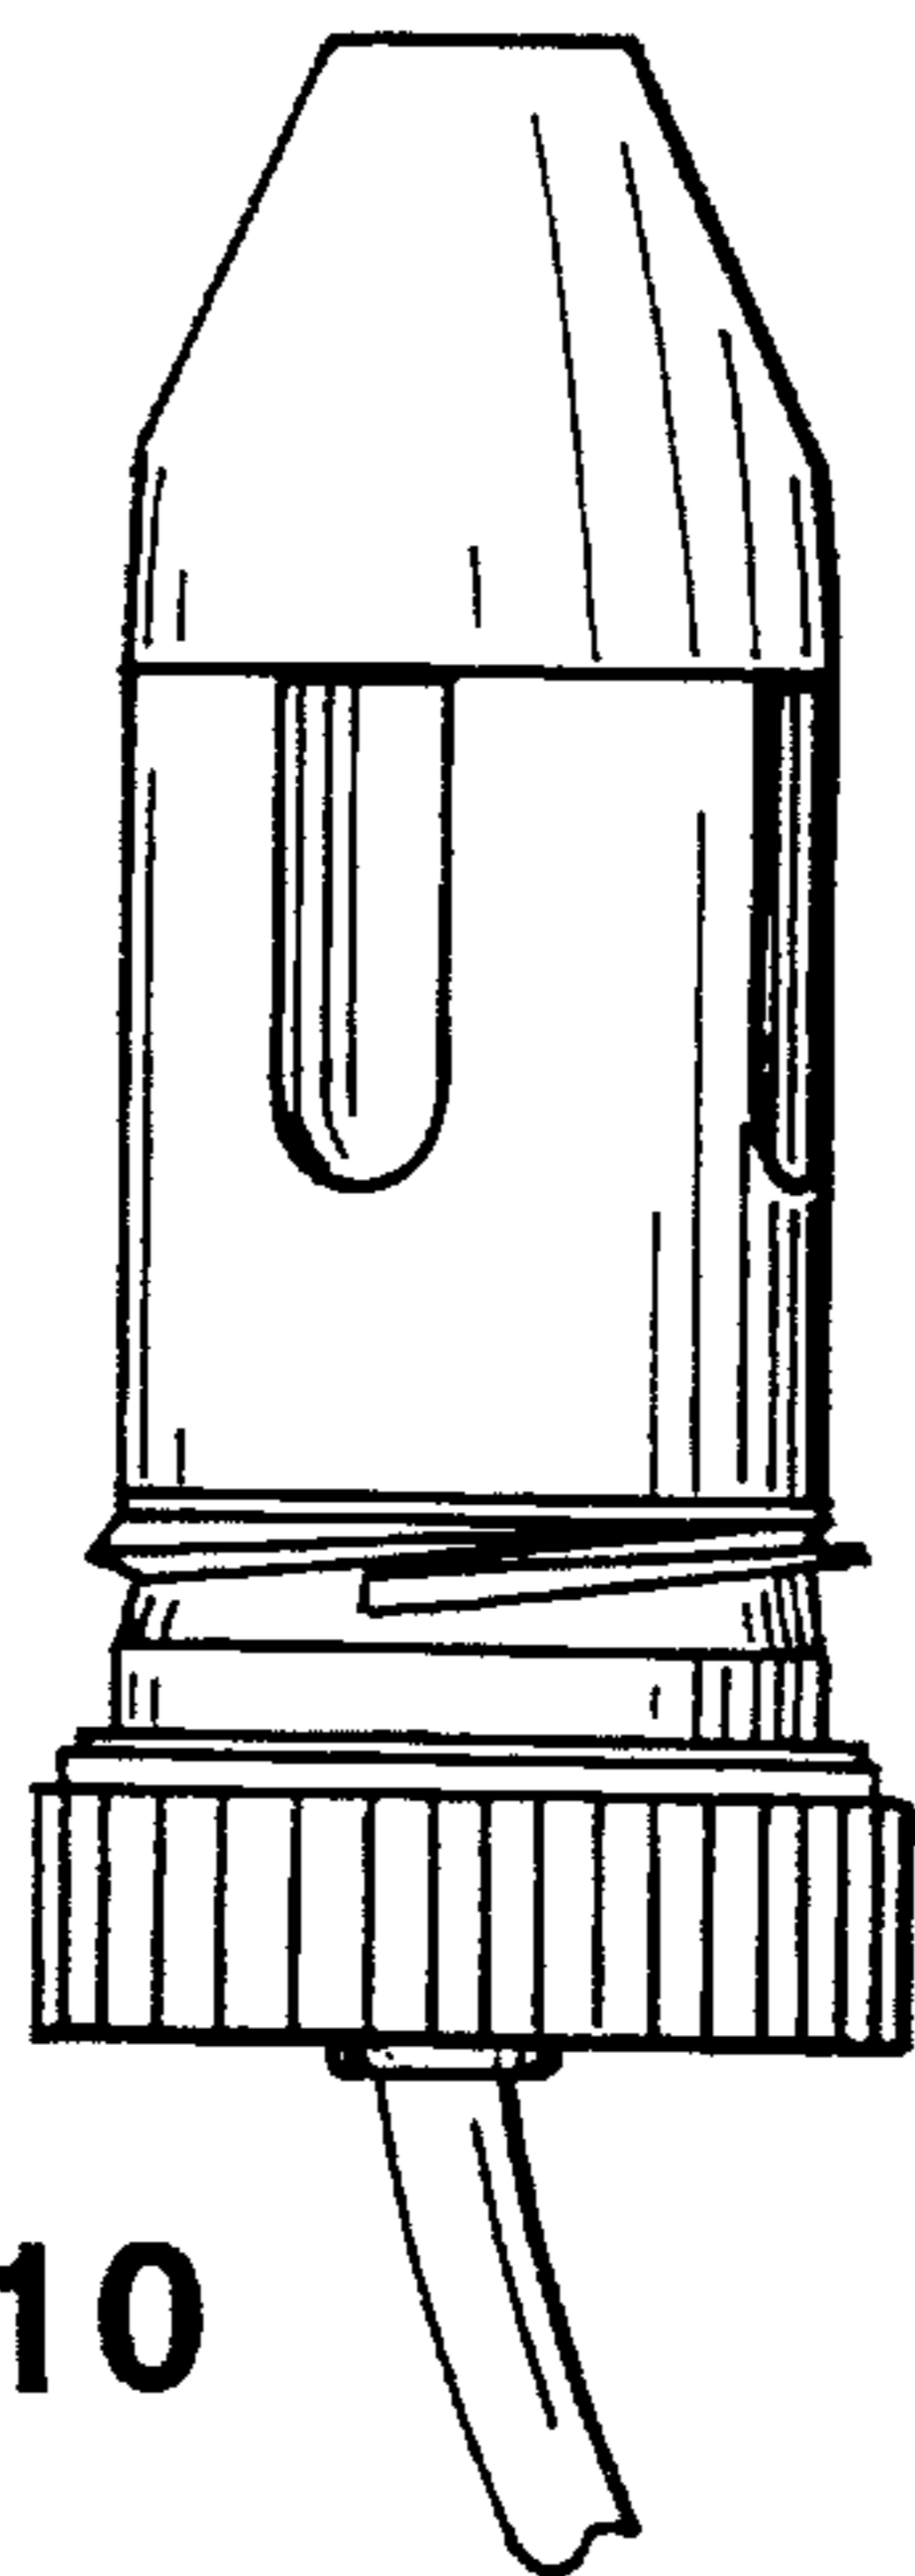


FIG. 10

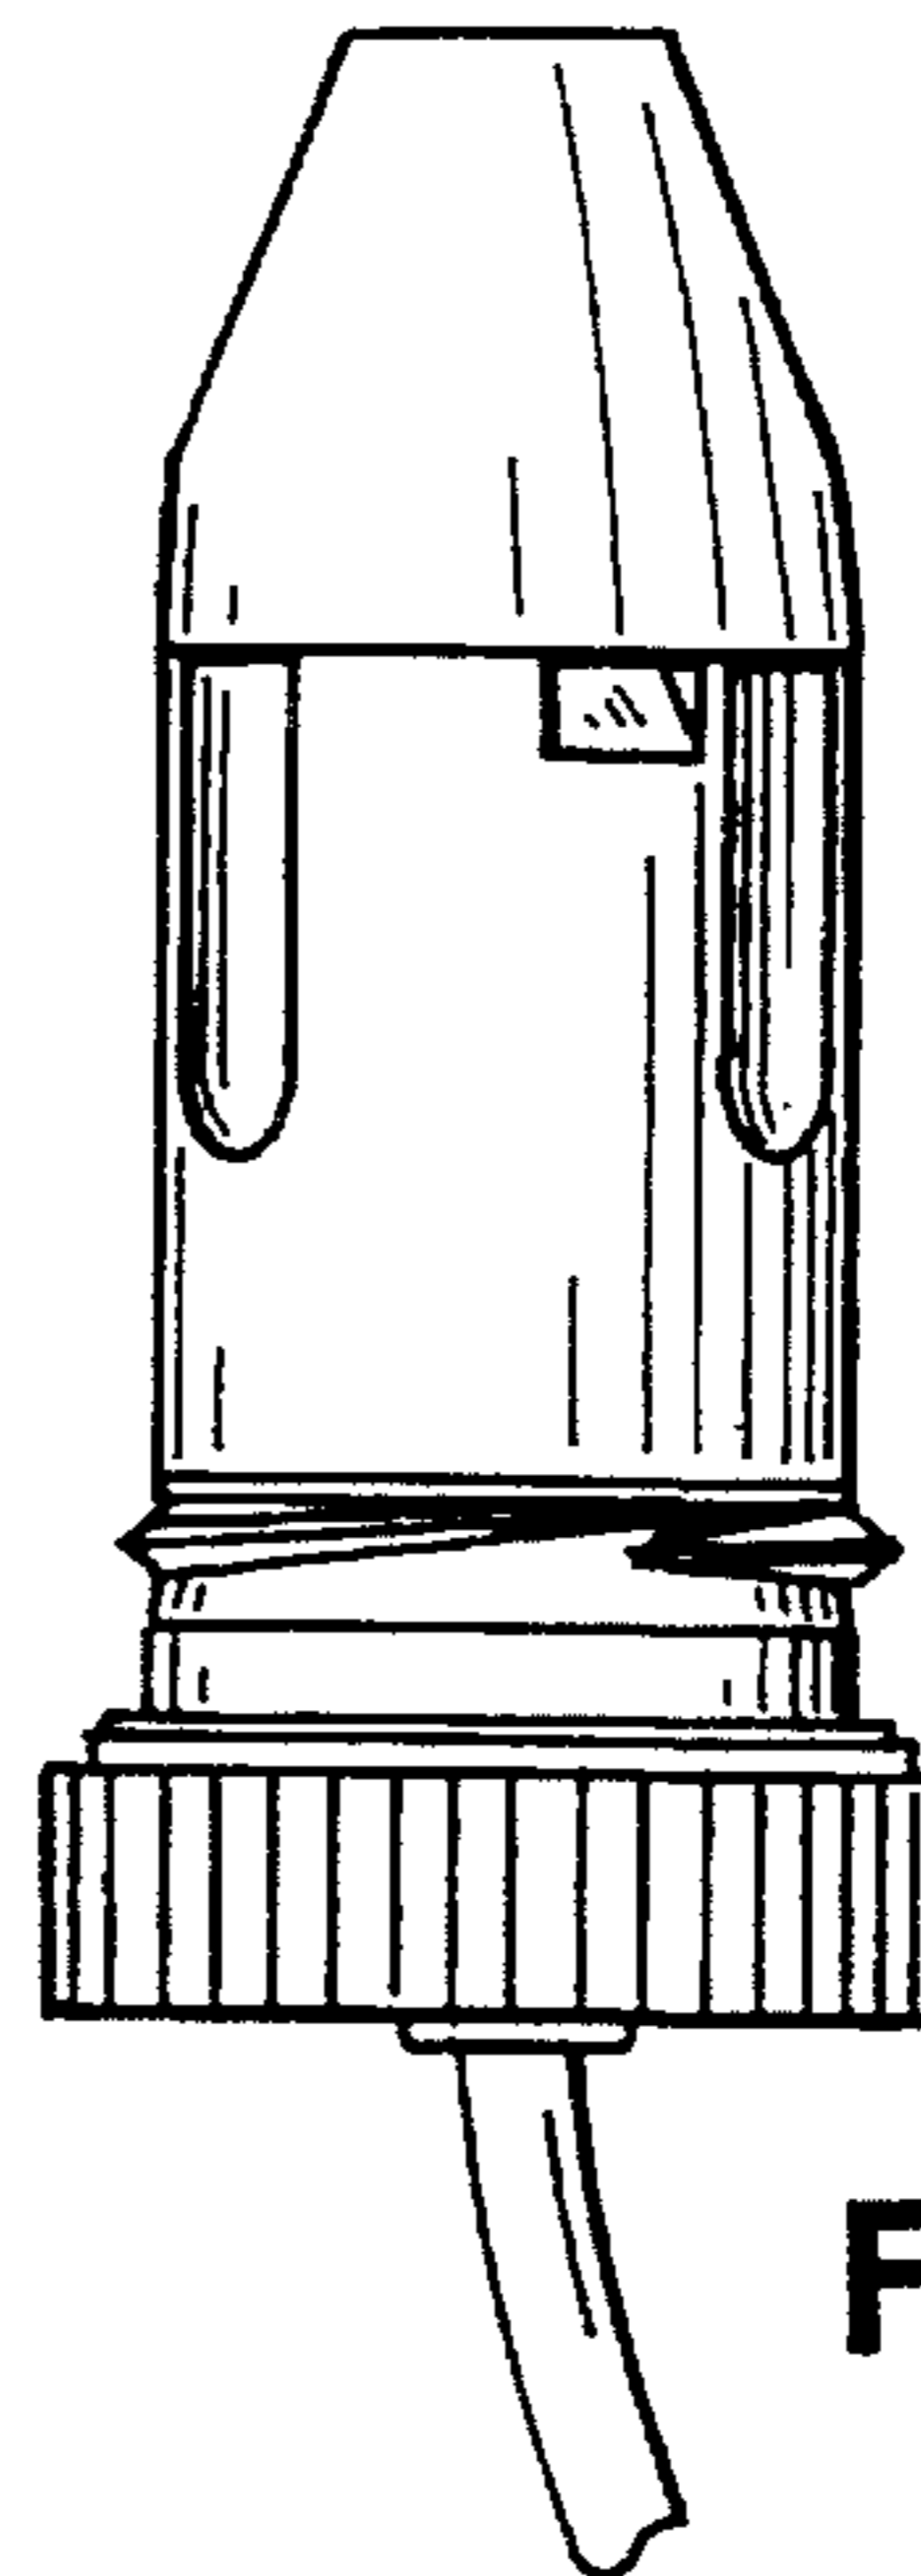


FIG. 11

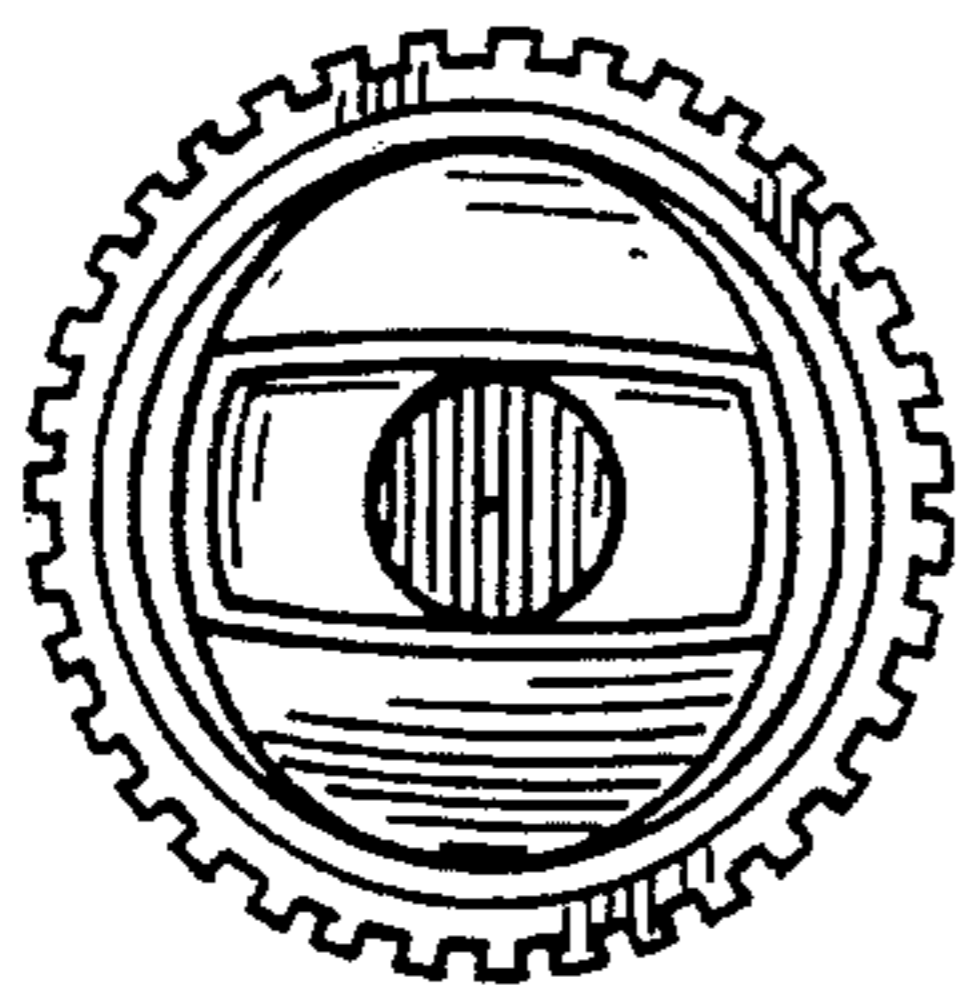


FIG. 12

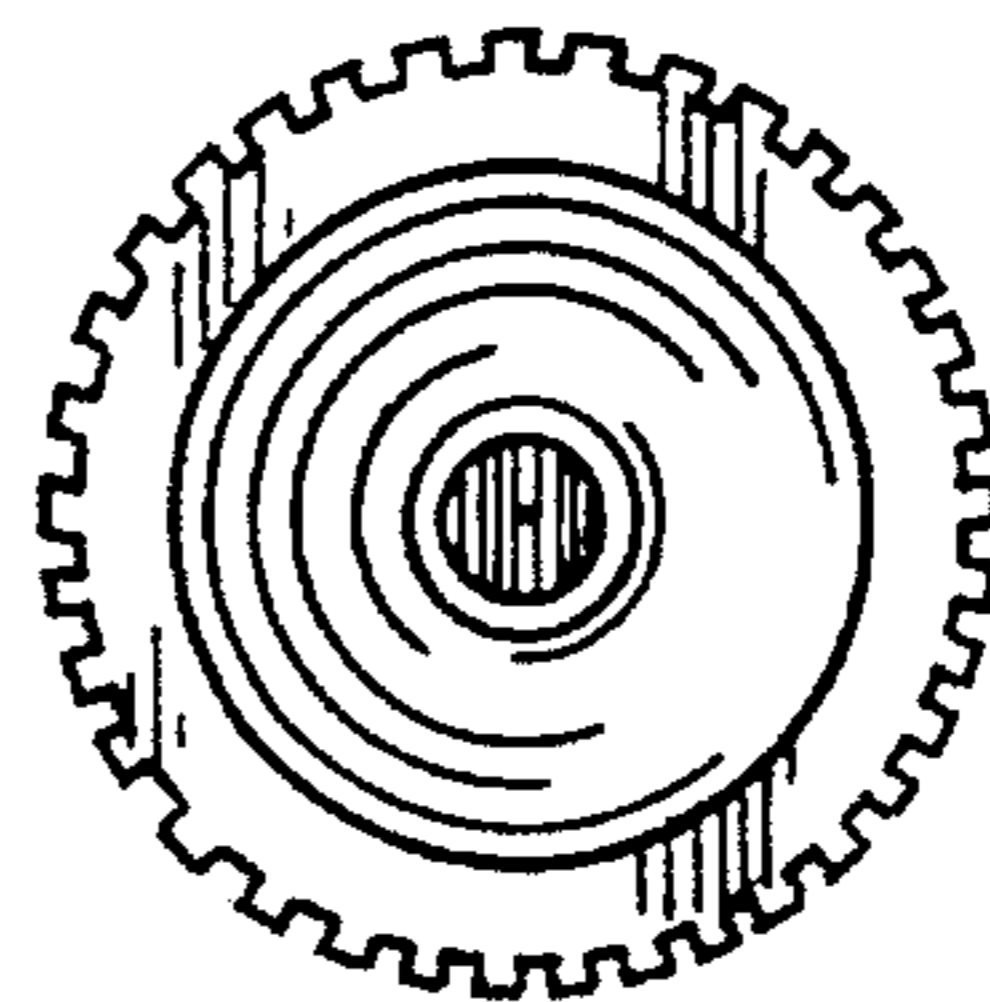


FIG. 13