



US00D379795S

**United States Patent** [19]  
**Pitzen et al.**

[11] **Patent Number:** **Des. 379,795**  
[45] **Date of Patent:** **\*\*Jun. 10, 1997**

[54] **BATTERY HOUSING FOR AN ORTHOPEDIC SURGICAL DEVICE**

[75] **Inventors:** **James F. Pitzen**, Maplewood; **Jeffrey D. Smith**, Marine on St. Croix, both of Minn.; **Charles E. Alexson**, Hayward; **Lawrence J. Fenske**, Oregon, both of Wis.

[73] **Assignee:** **Minnesota Mining and Manufacturing Company**, St. Paul, Minn.

[\*\*] **Term:** **14 Years**

[21] **Appl. No.:** **46,265**

[22] **Filed:** **Nov. 13, 1995**

**Related U.S. Application Data**

[63] Continuation-in-part of Ser. No. 33,712, Jan. 18, 1995, abandoned, which is a continuation of Ser. No. 24,242, Jun. 10, 1994, abandoned.

[51] **LOC (6) Cl.** ..... **13-02**

[52] **U.S. Cl.** ..... **D13/103**

[58] **Field of Search** ..... D13/103; 429/96-100, 429/153

[56] **References Cited**

**U.S. PATENT DOCUMENTS**

D. 207,586	5/1967	Rakocy	.....	D13/103
D. 329,634	9/1992	Mizusugi et al.	.....	D13/103
D. 346,584	5/1994	Taniguchi	.....	D13/103 X
2,261,230	11/1941	Cox et al.	.	
3,120,845	2/1964	Horner	.	
3,494,799	2/1970	Pedone, Jr.	.	
3,734,207	5/1973	Fishbein	.	
3,999,110	12/1976	Ramstrom et al.	.	
4,050,528	9/1977	Foltz et al.	.	
4,091,880	5/1978	Troutner et al.	.	
4,147,838	4/1979	Leffingwell	.....	320/2 X
4,441,563	4/1984	Walton, II	.	
4,447,749	5/1984	Reeb, Jr. et al.	.	
4,728,876	3/1988	Mongeon et al.	.	
4,736,742	4/1988	Alexson et al.	.	

4,751,452	6/1988	Kilmer et al.	.	
4,819,334	4/1989	Mongeon	.....	30/393
4,834,092	5/1989	Alexson et al.	.	
4,835,410	5/1989	Bhagwat et al.	.	
4,873,461	10/1989	Brennan et al.	.	
5,089,738	2/1992	Bergqvist et al.	.	
5,136,469	8/1992	Carusillo et al.	.	
5,207,697	5/1993	Carusillo et al.	.	
5,263,972	11/1993	Evans et al.	.	

**FOREIGN PATENT DOCUMENTS**

3 317 398 10/1985 Germany .

**OTHER PUBLICATIONS**

Product brochure entitled: "Maxion™ Cordless Powered Instrument System", by 3M HealthCare, (31 pages).

Product brochure entitled: "The K-100 Mini-Driver System, Cleaning and Lubrication", by 3M Surgical Products Division (5 pages).

Product brochure entitled: "Cordless 800 Wire Driver", by Dyonics, 1984, (2 pages).

Product brochure entitled: "Cordless 200 Reamer", by Dyonics, 1984, (2 pages).

(List continued on next page.)

*Primary Examiner*—Joel Sincavage

*Attorney, Agent, or Firm*—Gary L. Griswold; Walter N. Kirn; Jeffrey J. Hohenshell

[57] **CLAIM**

The ornamental design for a battery housing for an orthopedic surgical device, as shown and described.

**DESCRIPTION**

FIG. 1 is a perspective view of a battery housing for an orthopedic surgical device showing our new design;

FIG. 2 is a left side view thereof, the right side view being a mirror image thereof;


FIG. 3 is a front view thereof;

FIG. 4 is a rear view thereof;

FIG. 5 is a top view thereof; and,

FIG. 6 is a bottom view thereof.

**1 Claim, 2 Drawing Sheets**

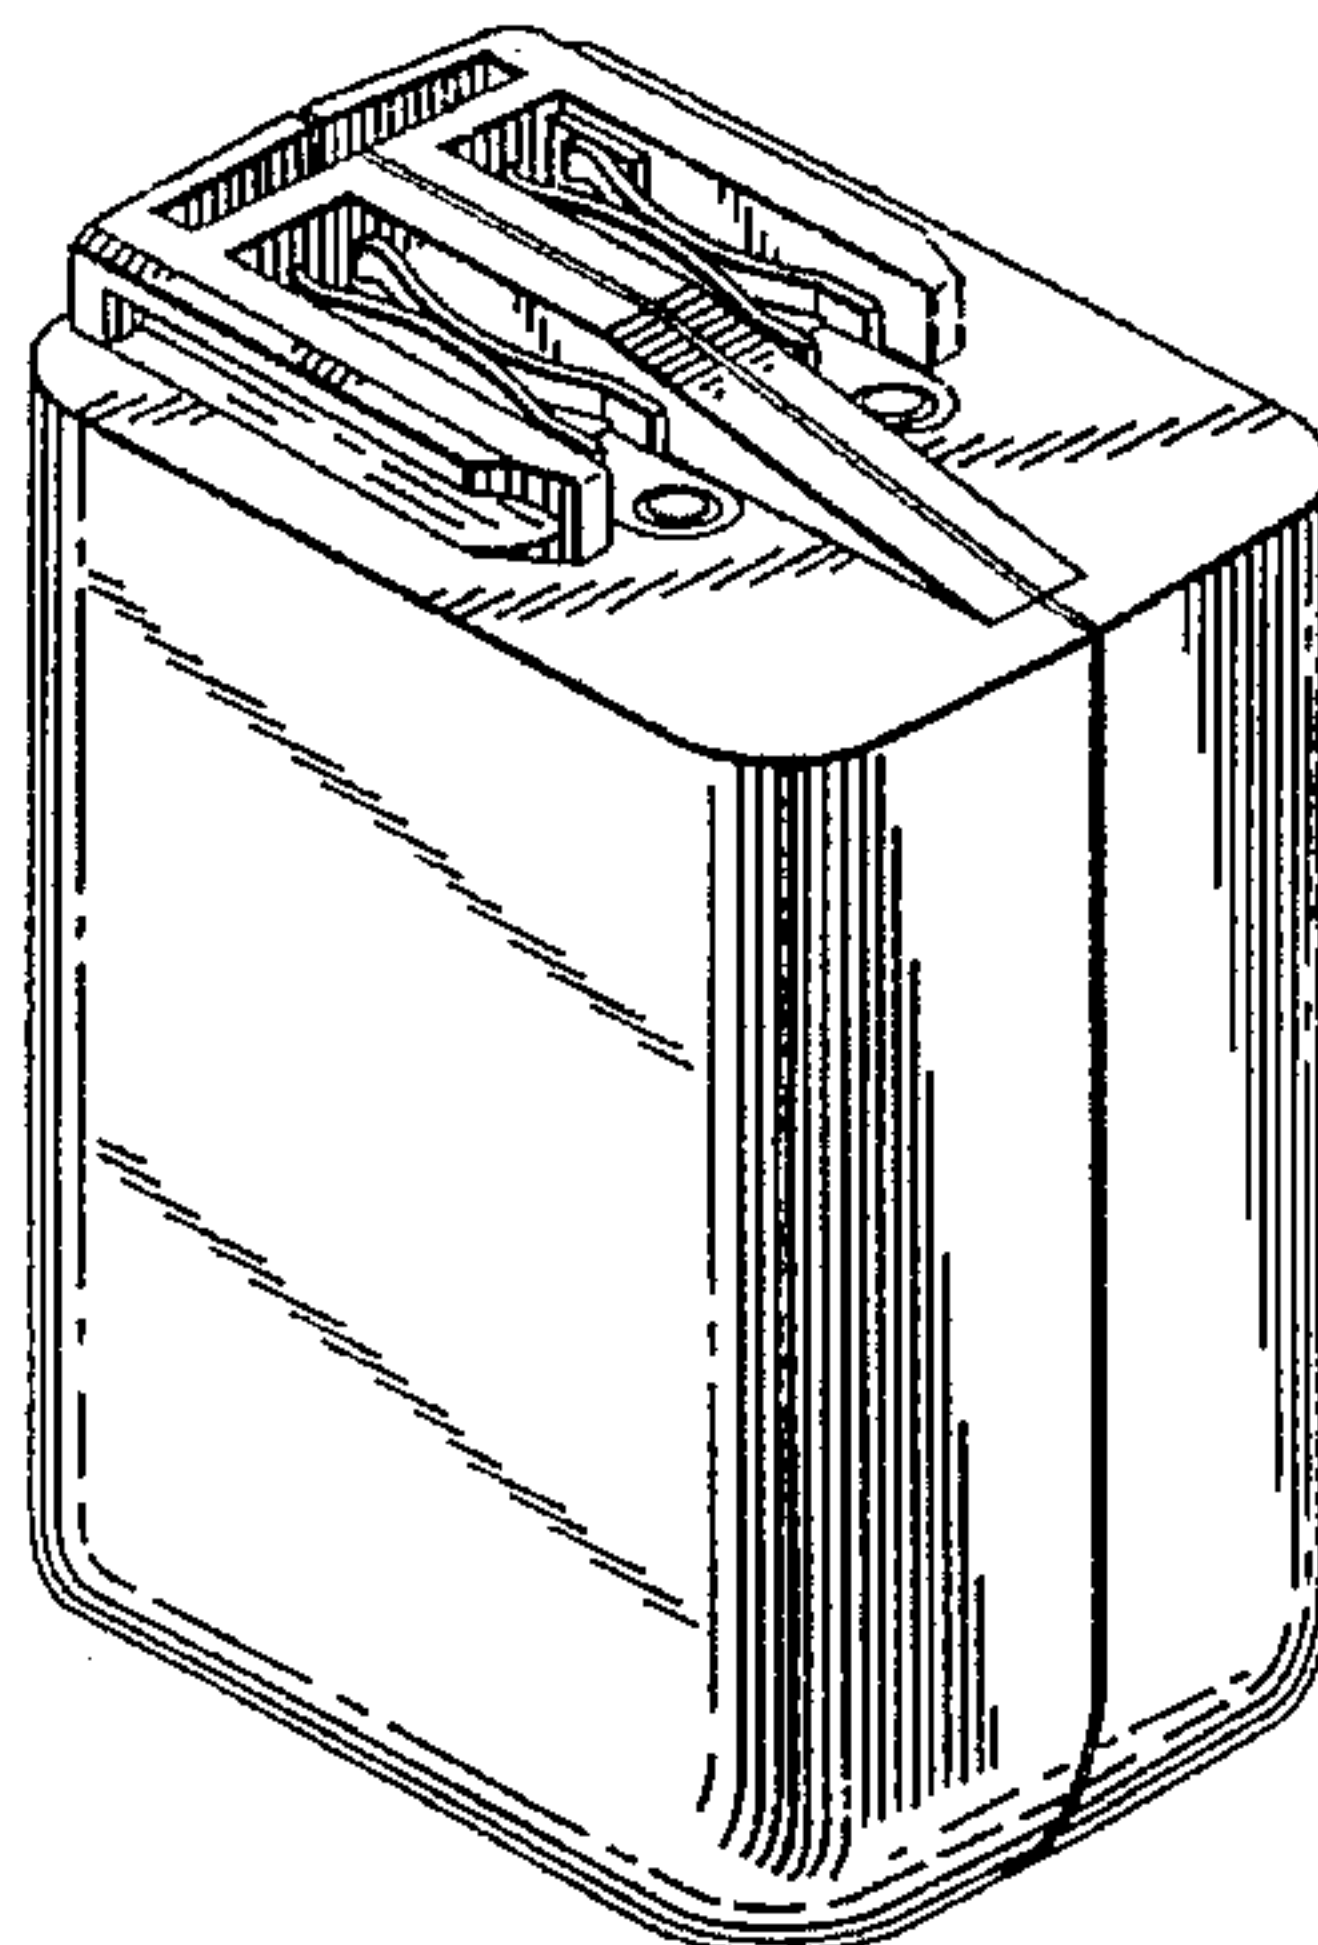

**OTHER PUBLICATIONS**

Product brochure entitled: "Cordless 450 Orthopaedic Drill", by Dyonics, 1984, (2 pages).

Product brochure entitled: "Mini-Driver™ Air Instrument System", by 3M, 1975, (4 pages).

Product brochure entitled: "Acculan", by Aesulap®, (4 pages).

Product brochure entitled: "Powered Instrumentation for Large Bone Surgery", by Stryker® (16 pages).

Product brochure entitled: "System II OrthoPower 90 Battery Powered Surgical Instruments", by Stryker®, 1986, (16 pages).

Product brochure entitled: "Sagittal Saw Attachment", by 3M, (2 pages).

Product brochure entitled: "Cordless Sagittal Saw", by Dyonics, 1984, (2 pages).

Product brochure entitled: "The Only Cordless Instrument Powerful Enough to be Stryker", by Stryker®, (4 pages).


Product brochure entitled: "System 2000 Battery Powered Instruments", by Stryker®, 1993 (18 pages).

Product brochure entitled: "System 2000 Battery Powered Instruments", by Stryker® (11 pages).


Instruction Manual entitled: "The Hall® ORTHAIR™ System" by Zimmer USA, (12 Pages).

Product brochure entitled: "Maxion™ Cordless Powered Instrument System, Assembly, Operation and Maintenance", by 3M HealthCare (6 pages).


Hall® Versipower™ Dual Power Orthopaedic Instruments, by Zimmer, 1989, (6 pages).

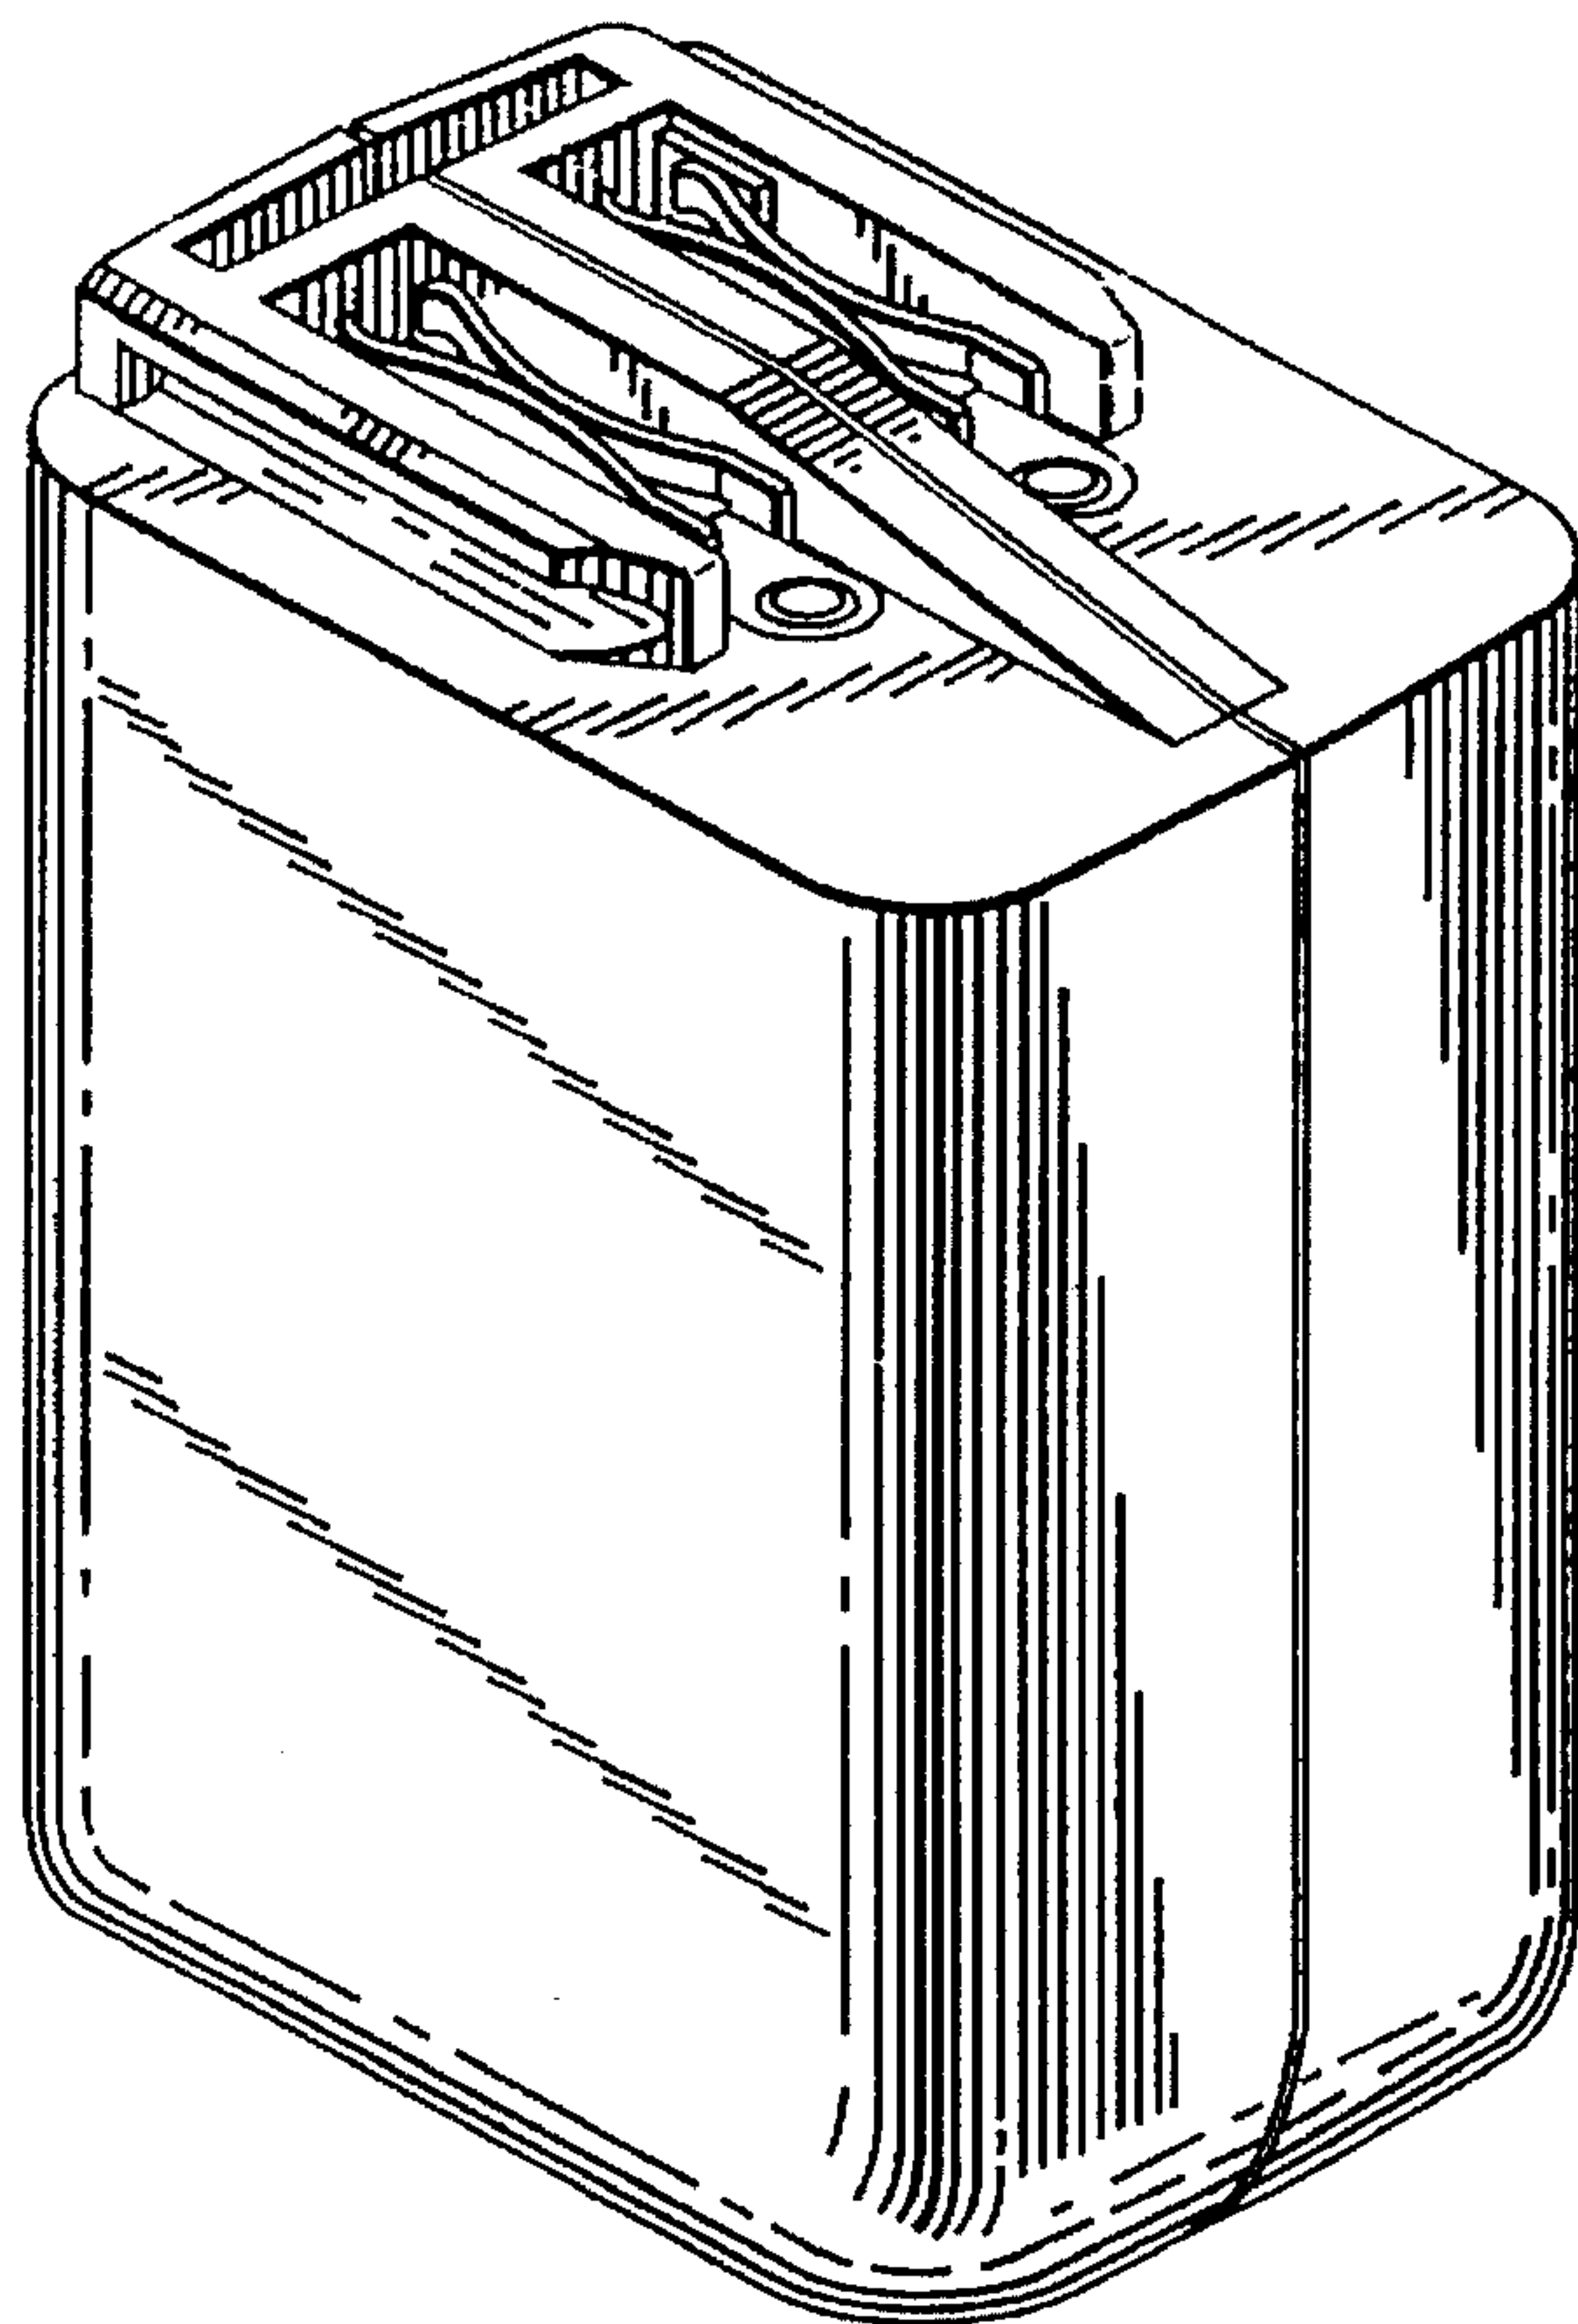

*Fig. 1*

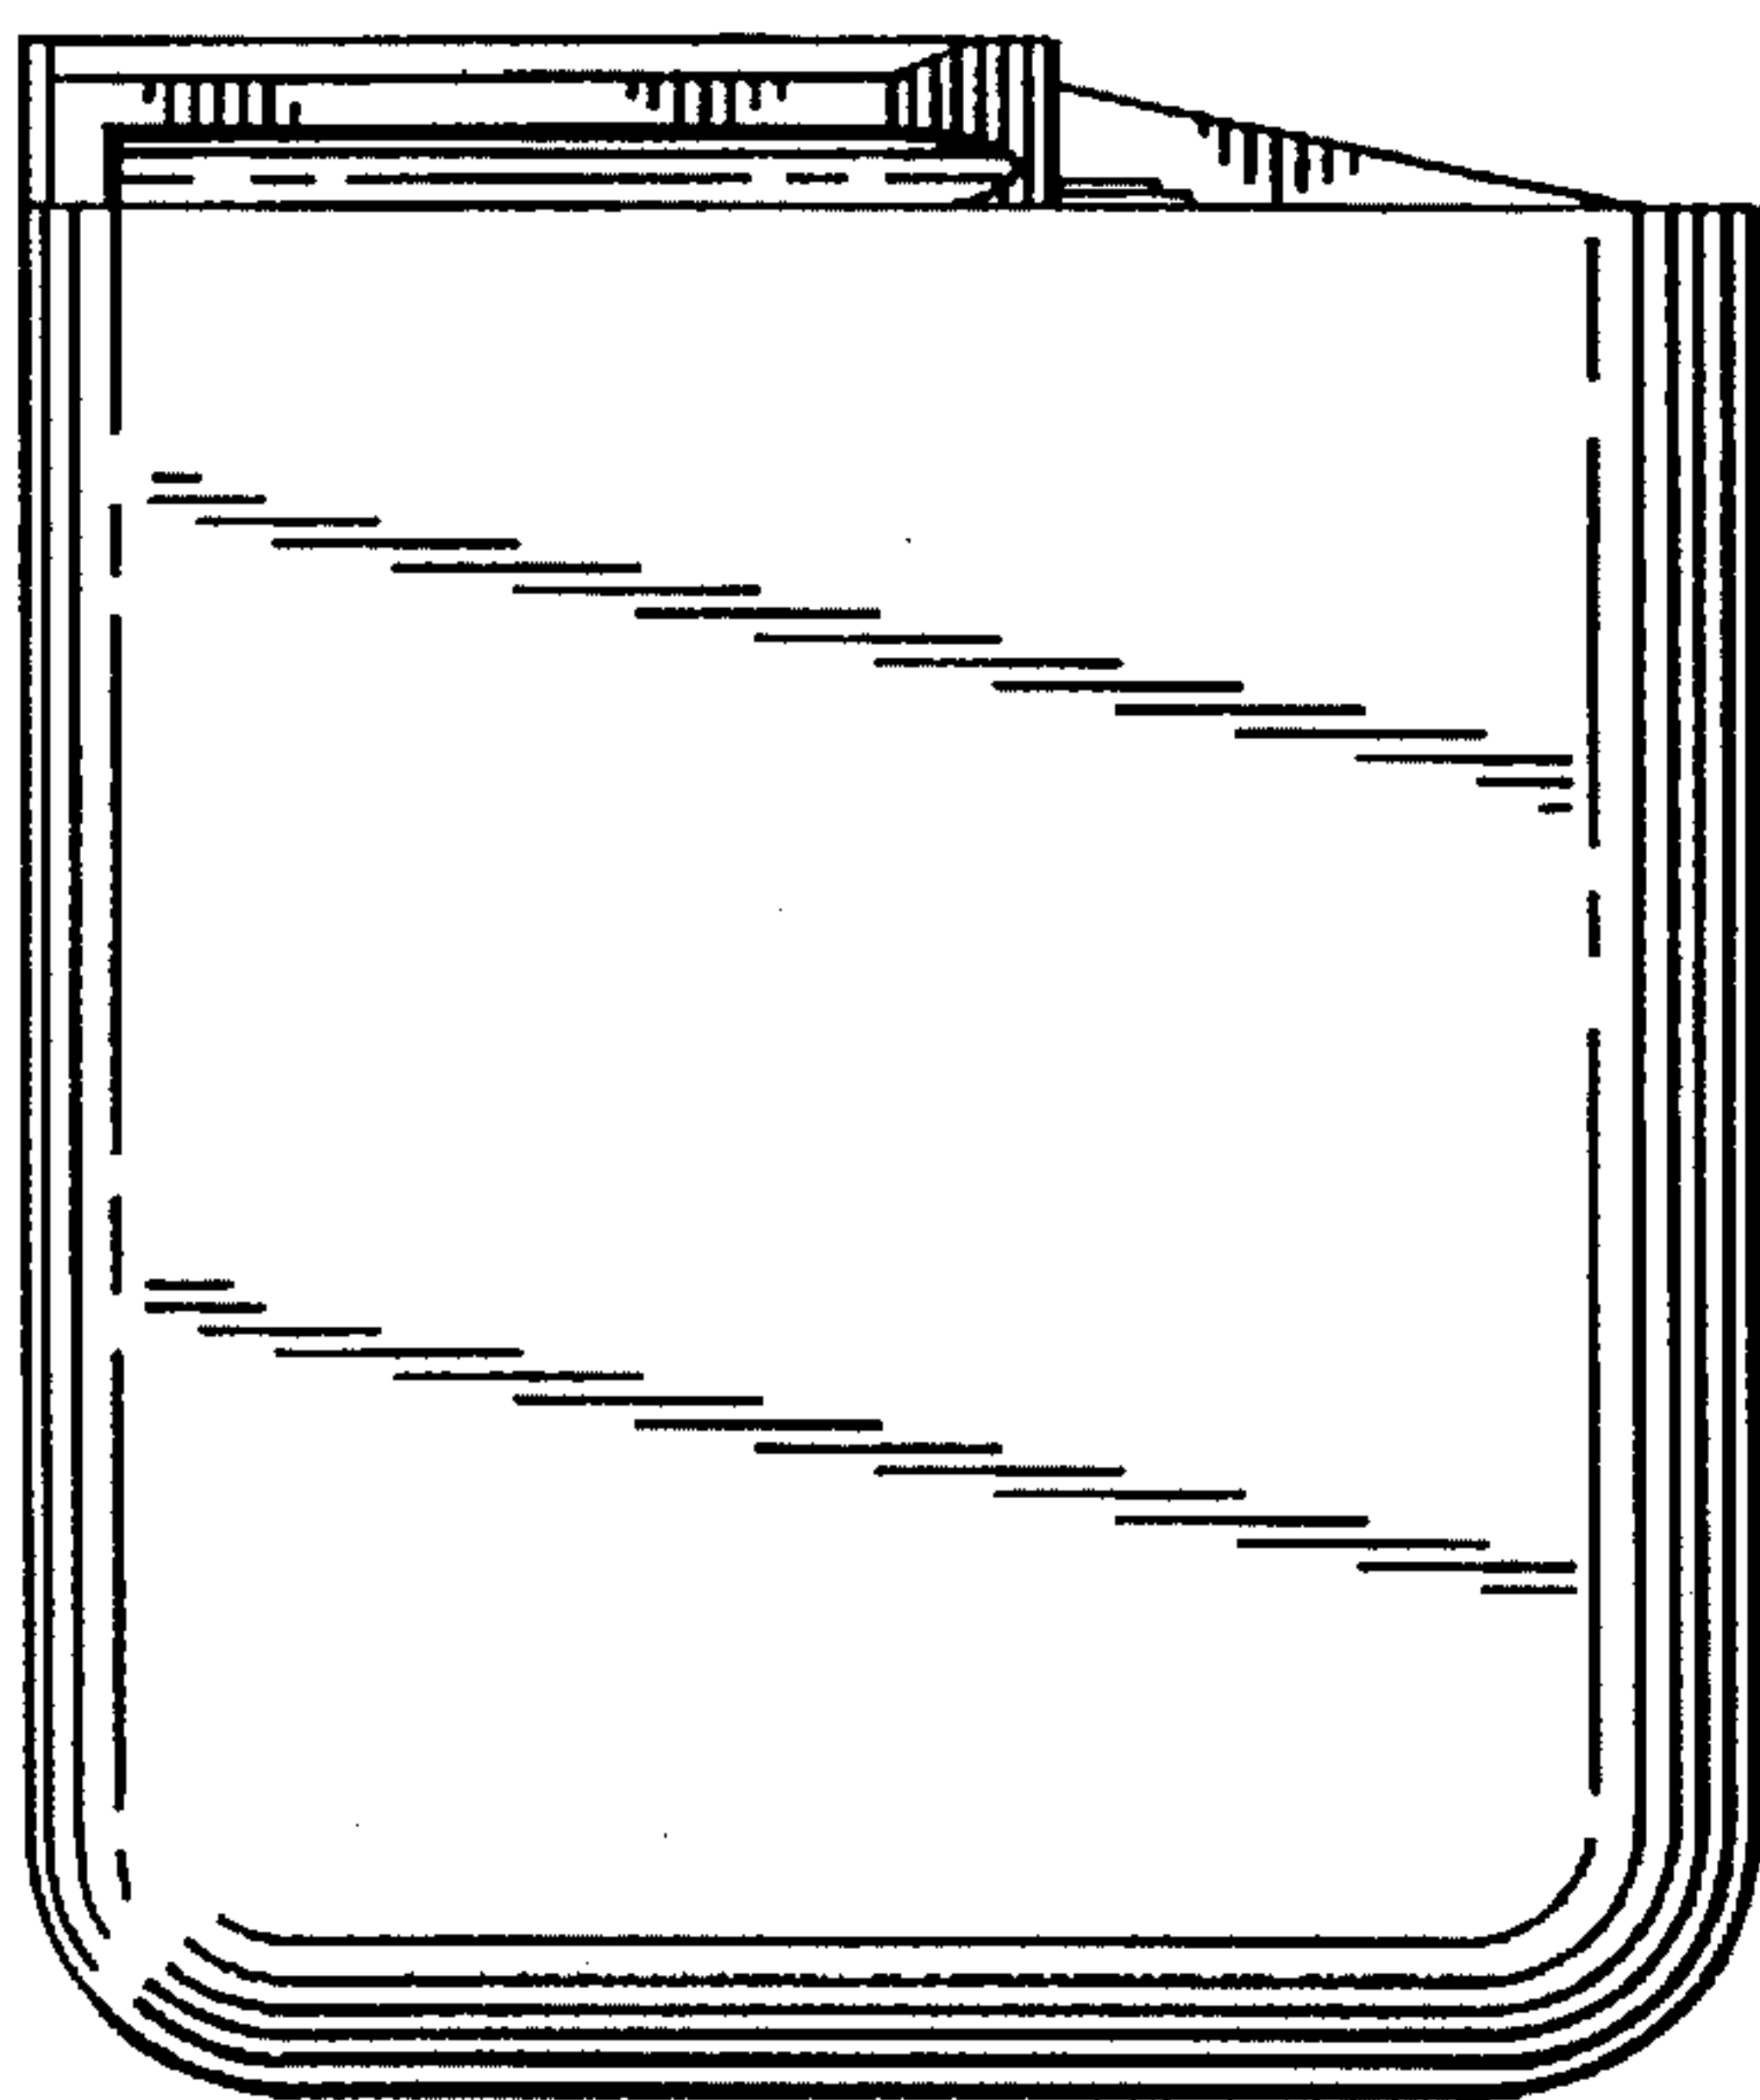


*Fig. 2*

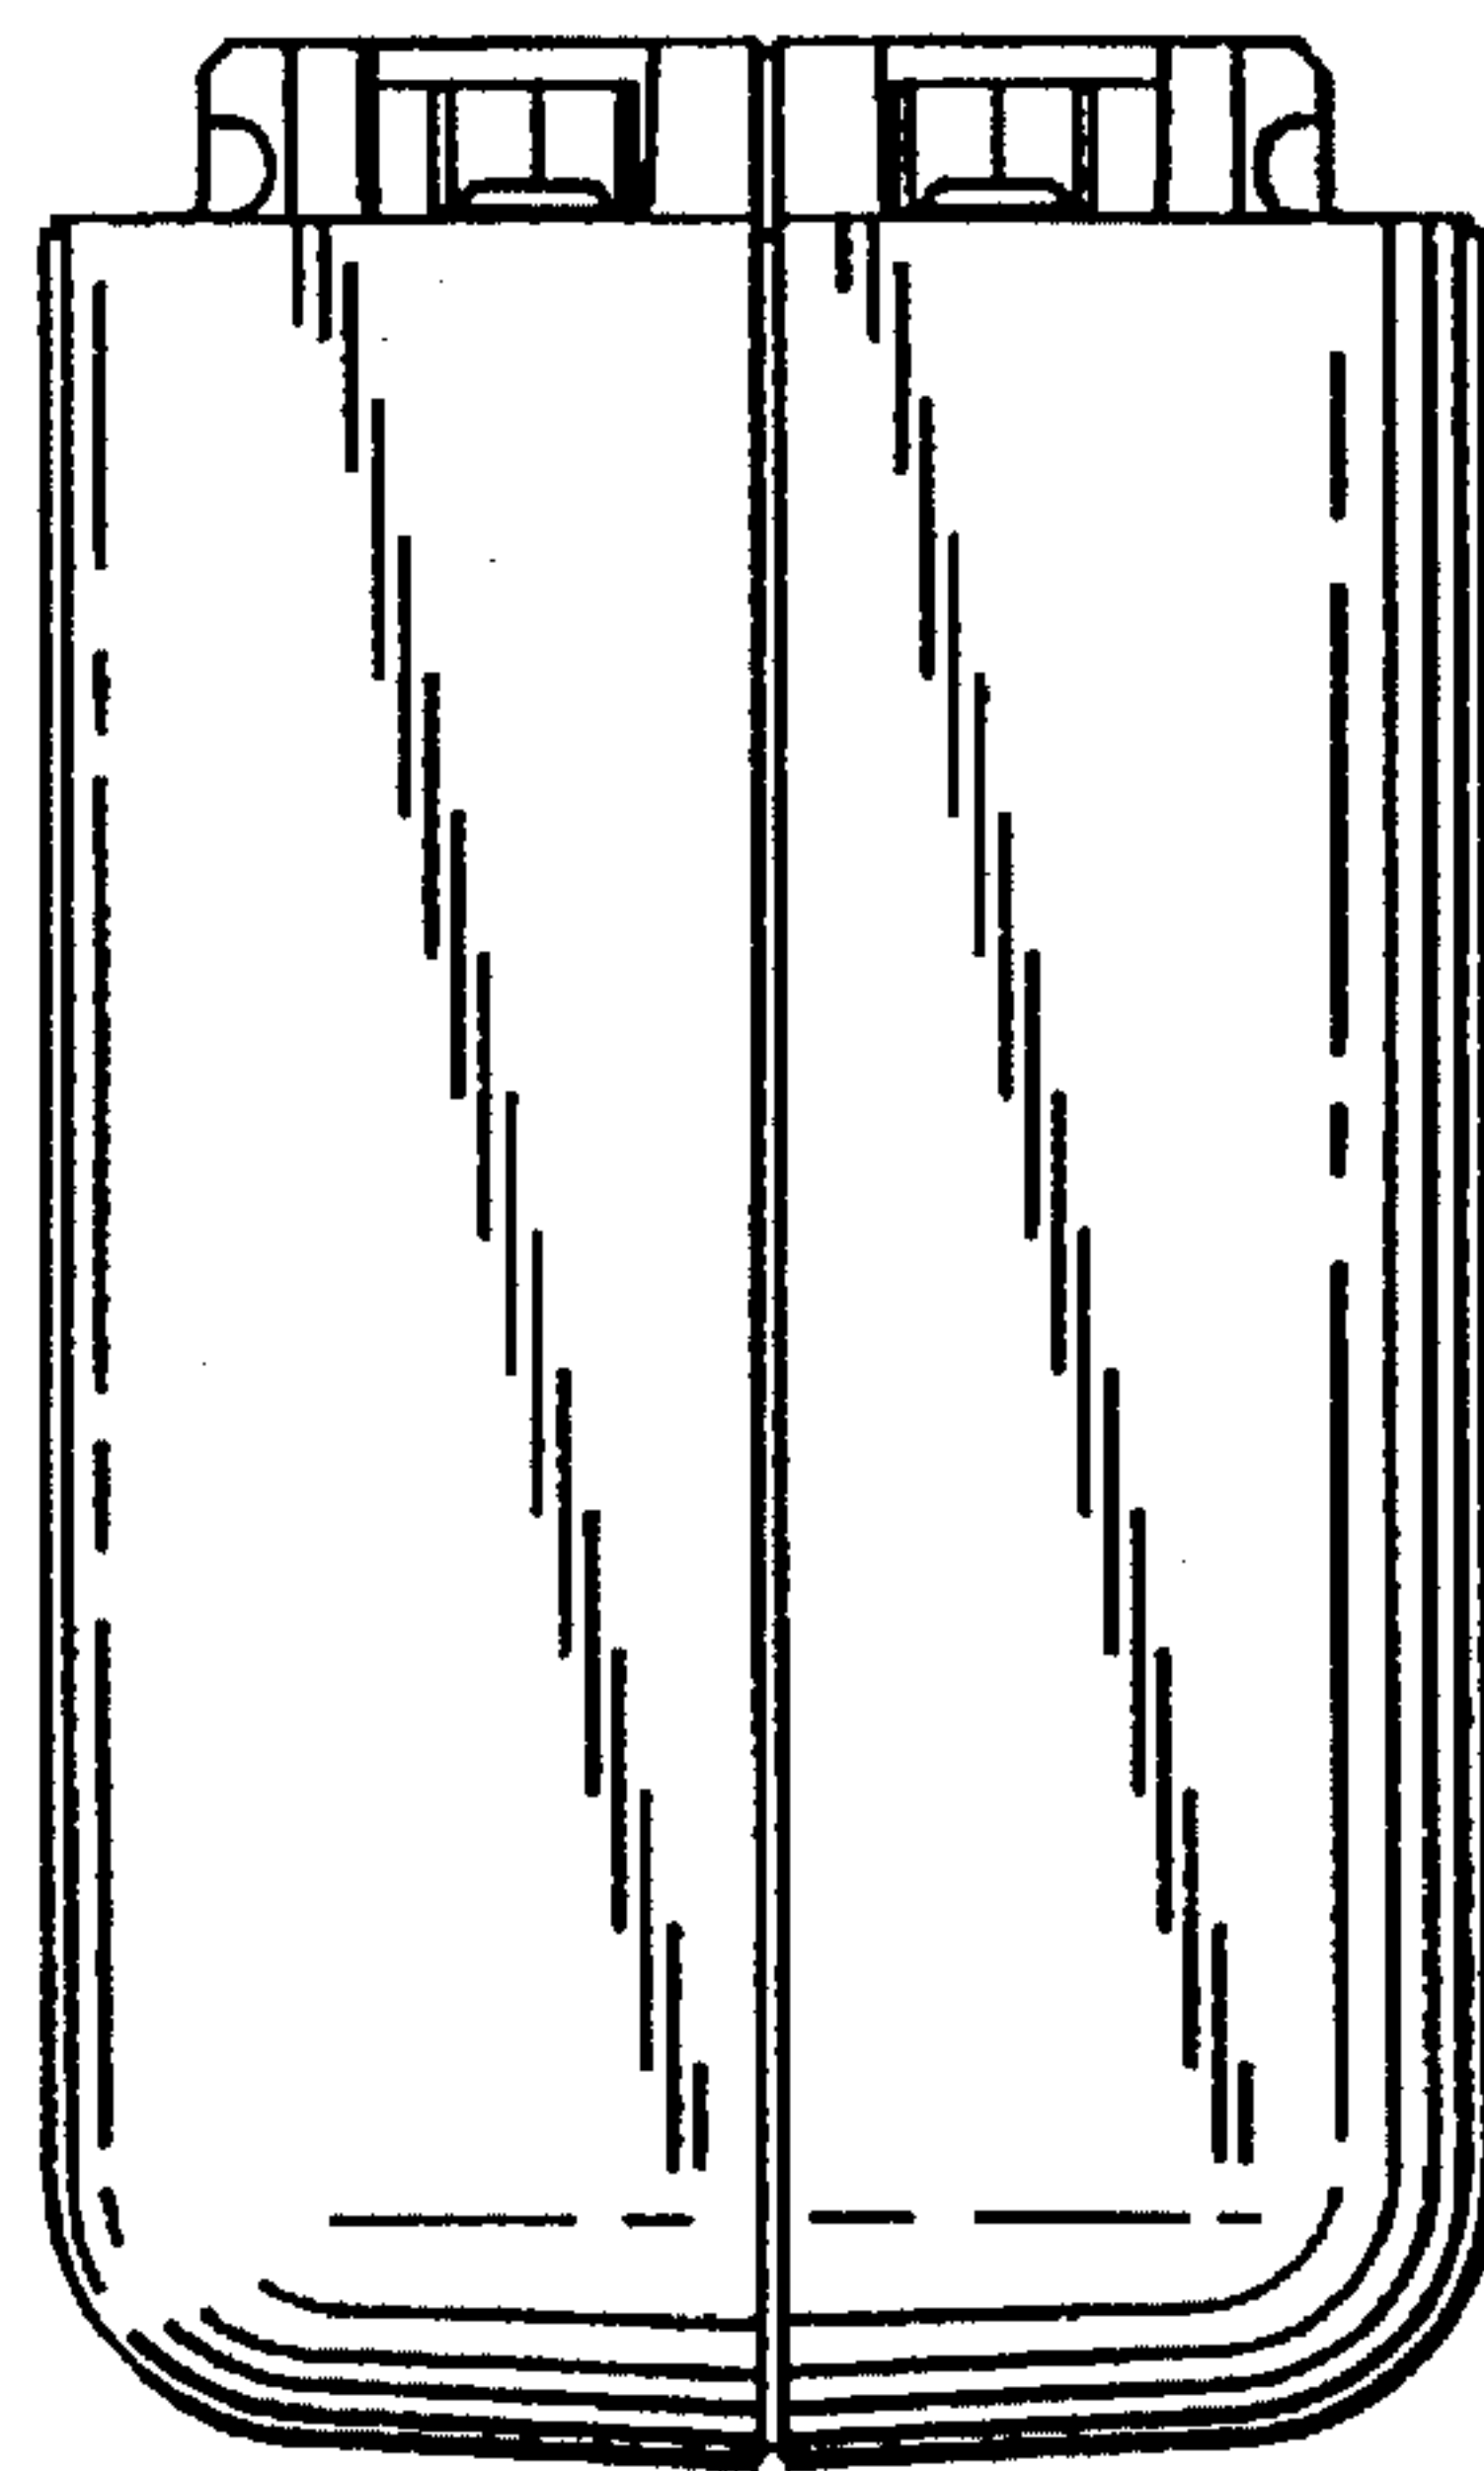


*Fig. 3*




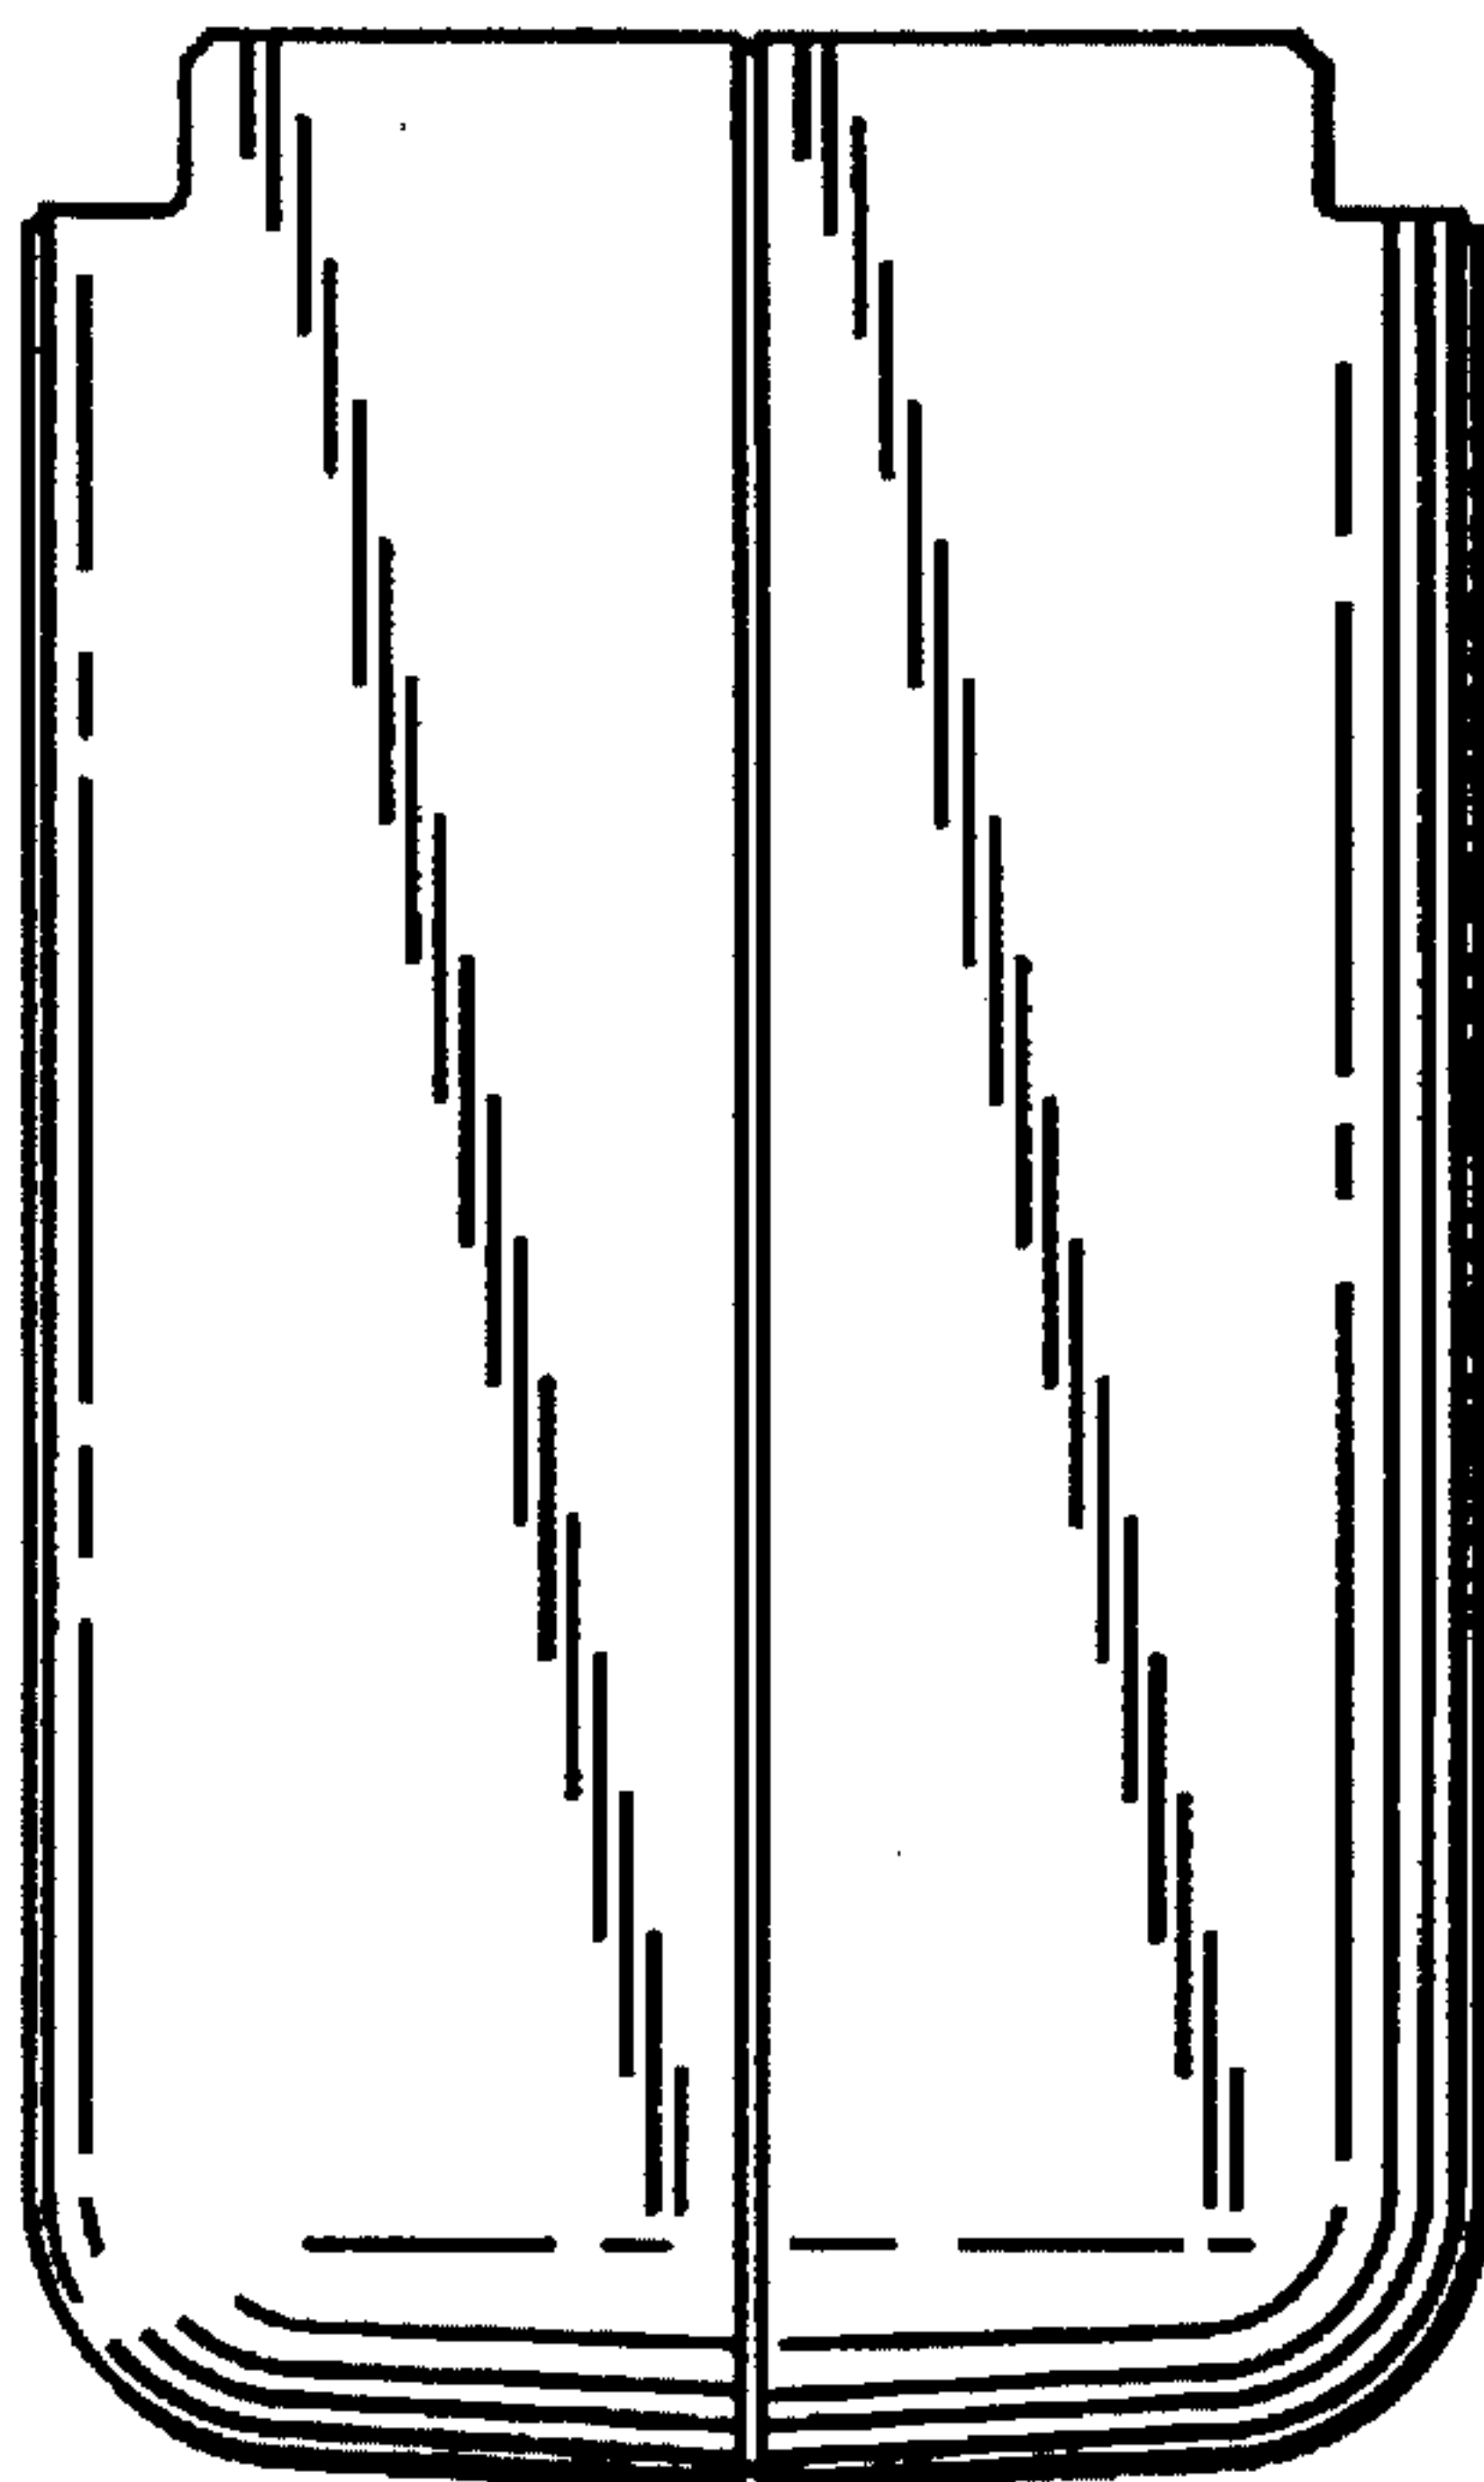

*Fig. 4*

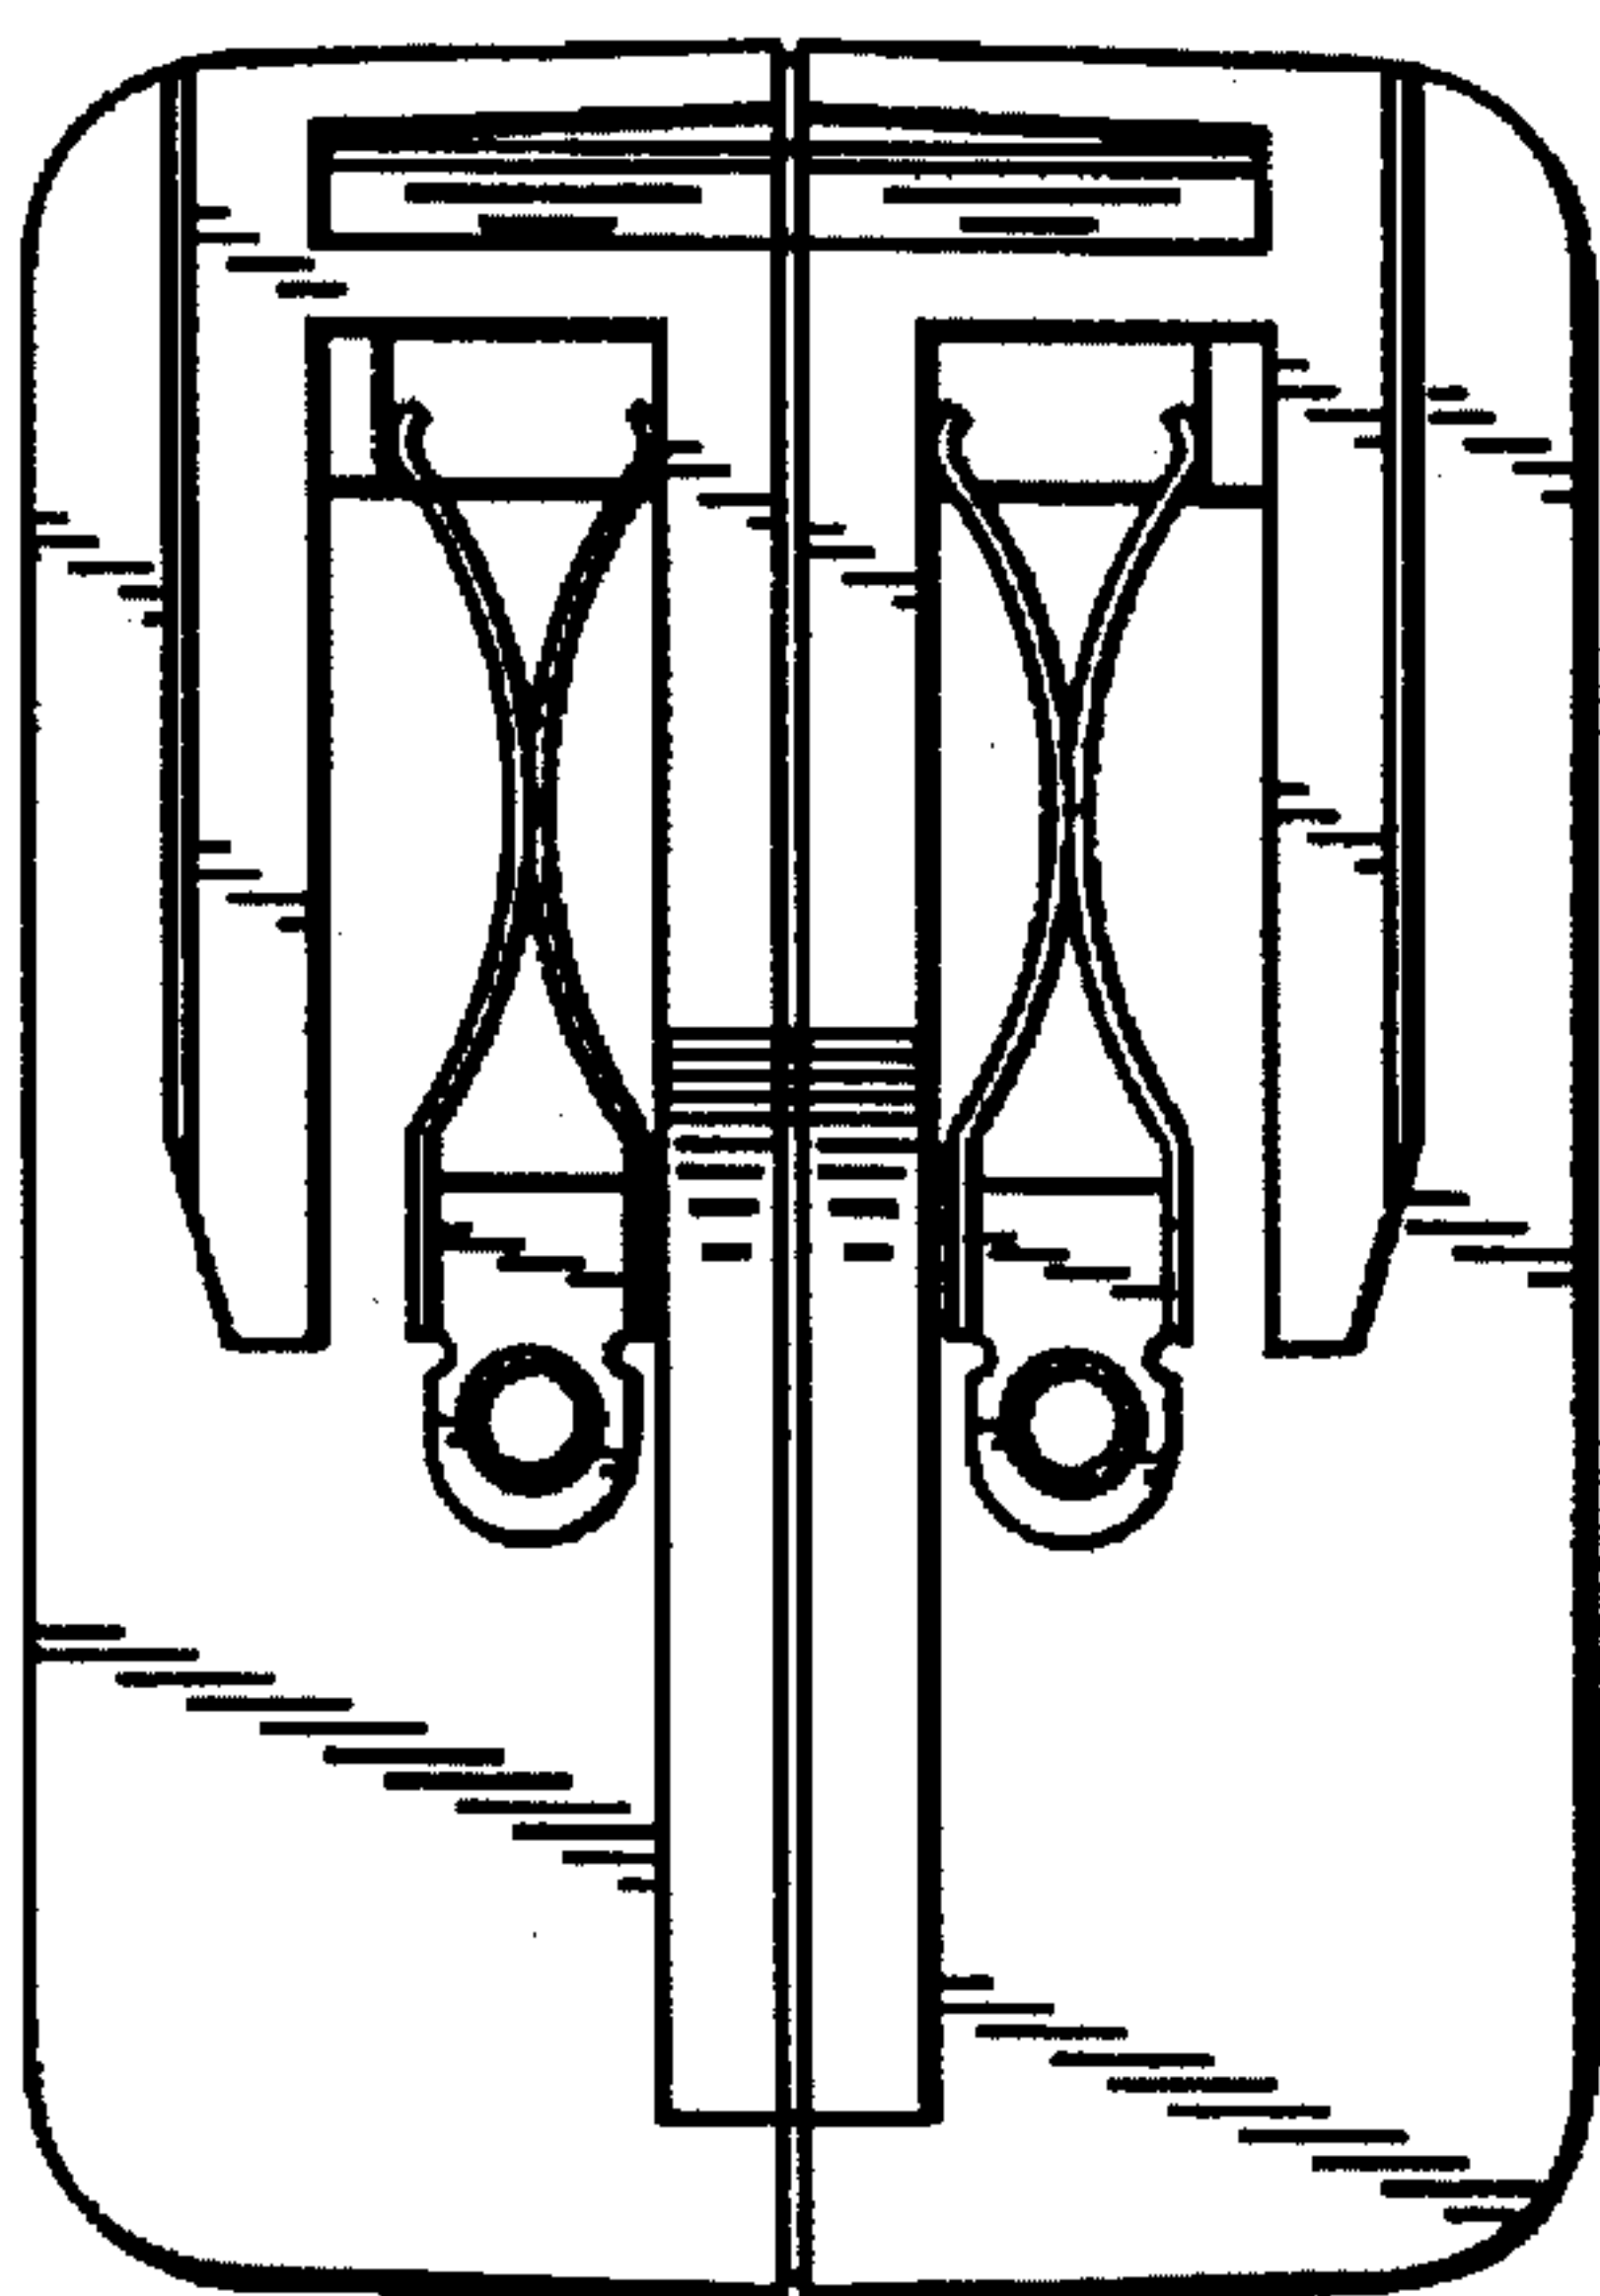

*Fig. 5*

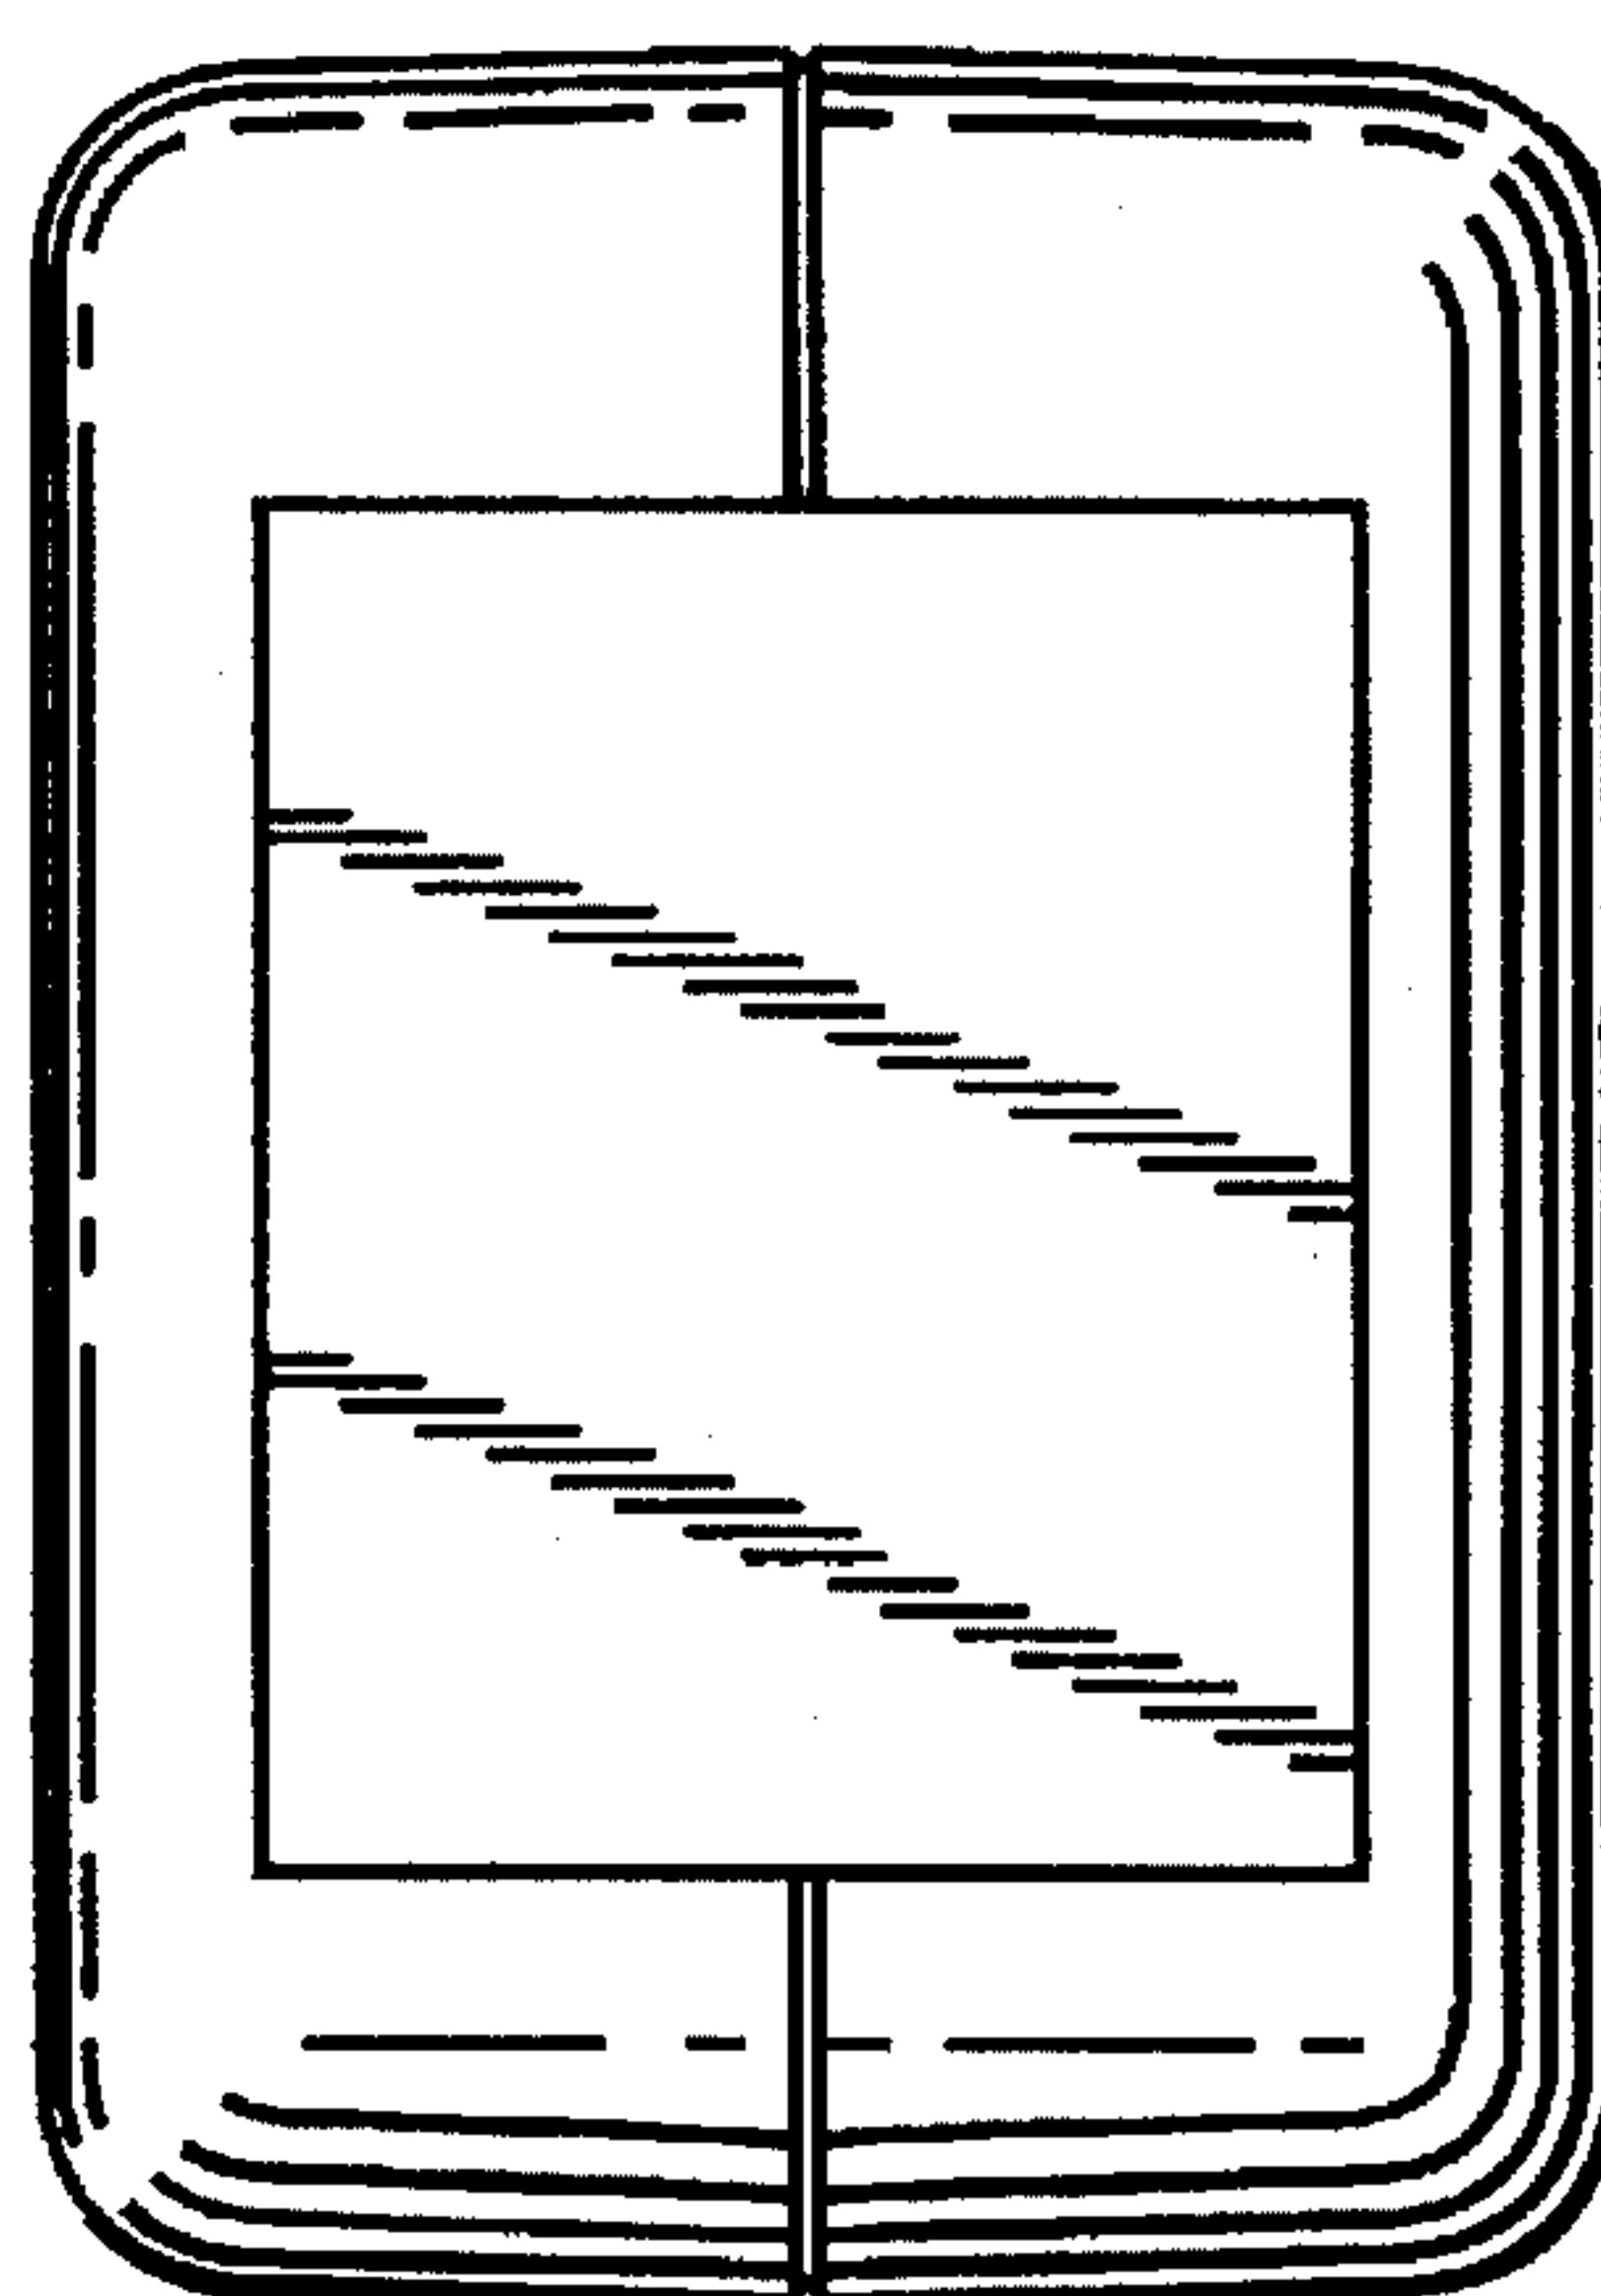

*Fig. 6*